



(12) **EUROPEAN PATENT APPLICATION**

(43) Date of publication:
14.08.2019 Bulletin 2019/33

(51) Int Cl.:
A61F 7/02 (2006.01) **A61F 7/12 (2006.01)**
A61F 7/08 (2006.01)

(21) Application number: **19163548.1**

(22) Date of filing: **11.01.2006**

(84) Designated Contracting States:
AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HU IE IS IT LI LT LU LV MC NL PL PT RO SE SI SK TR

(72) Inventors:
 • **Collins,, Kenneth, A.**
Mission Viejo, CA California 92691 (US)
 • **Worthen,, William, J.**
Coto de Caza, CA California 92679 (US)

(30) Priority: **23.05.2005 US 6418705**
18.04.2005 US 10828105

(74) Representative: **Potter Clarkson**
The Belgrave Centre
Talbot Street
Nottingham NG1 5GG (GB)

(62) Document number(s) of the earlier application(s) in accordance with Art. 76 EPC:
06718258.4 / 1 850 814

Remarks:
 This application was filed on 18.03.2019 as a divisional application to the application mentioned under INID code 62.

(71) Applicant: **Zoll Circulation, Inc.**
San Jose, CA 95131 (US)

(54) **SYSTEM AND METHOD FOR BRINGING HYPOTHERMIA RAPIDLY ONBOARD**

(57) An intravenous heat exchange catheter (12, 128) and/or an external cooling pad (18, 140, 214, 300) can be used to maintain hypothermia in, e.g., a cardiac arrest patient.

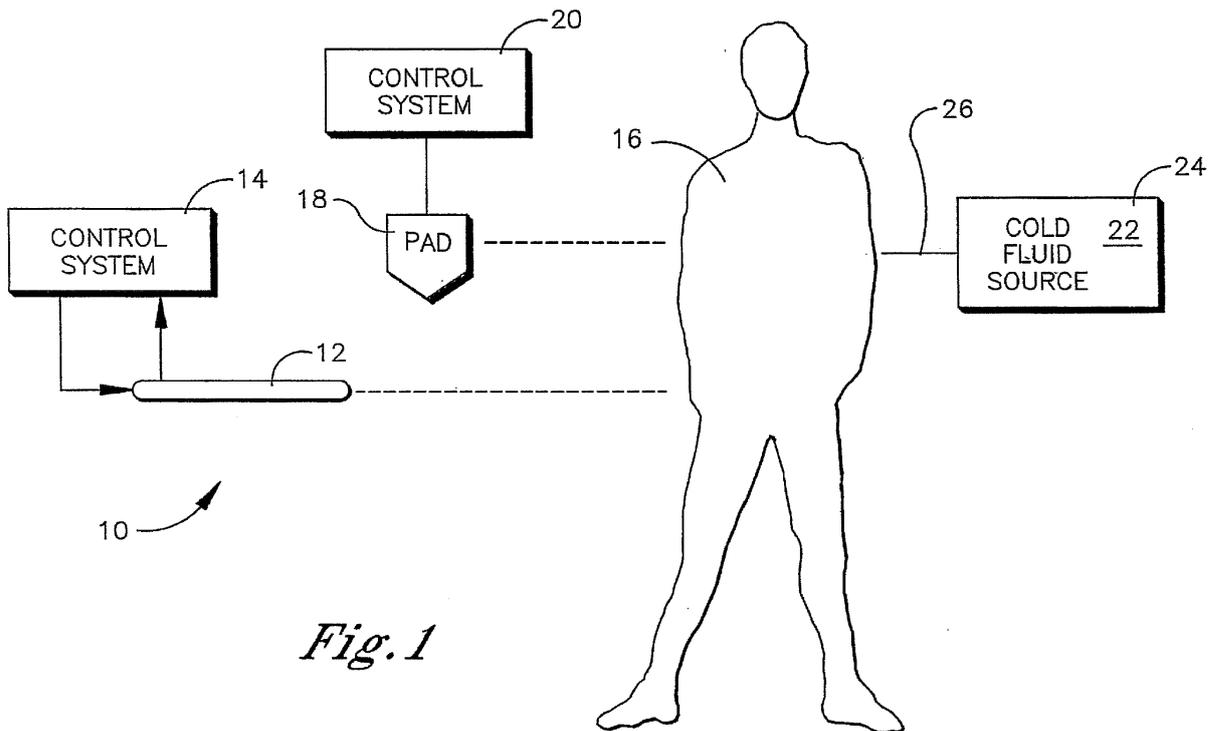


Fig. 1

Description

I. Field Of The Invention

[0001] The present invention relates generally to therapeutic hypothermia.

II. Background Of The Invention

[0002] Intravascular catheters have been introduced for controlling patient temperature. Typically, a coolant such as saline is circulated through an intravascular heat exchange catheter, which is positioned in the patient's bloodstream, to cool or heat the blood as appropriate for the patient's condition. The coolant is warmed or cooled by a computer-controlled heat exchanger that is external to the patient and that is in fluid communication with the catheter.

[0003] For example, intravascular heat exchange catheters can be used to combat potentially harmful fever in patients suffering from neurological and cardiac conditions such as stroke, subarachnoid hemorrhage, intracerebral hemorrhage, cardiac arrest, and acute myocardial infarction, or to induce therapeutic hypothermia in such patients. Further, such catheters can be used to rewarm patients after, e.g., cardiac surgery or for other reasons. Intravascular catheters afford advantages over external methods of cooling and warming, including more precise temperature control and more convenience on the part of medical personnel.

[0004] The following U.S. patents, all of which are incorporated herein by reference, disclose various intravascular catheters/systems/methods: 6,419,643, 6,416,533, 6,409,747, 6,405,090, 6,393,320, 6,368,304, 6,338,727, 6,299,599, 6,290,717, 6,287,326, 6,165,207, 6,149,670, 6,146,411, 6,126,684, 6,306,161, 6,264,679, 6,231,594, 6,149,676, 6,149,673, 6,110,168, 5,989,238, 5,879,329, 5,837,003, 6,383,210, 6,379,378, 6,364,899, 6,325,818, 6,312,452, 6,261,312, 6,254,626, 6,251,130, 6,251,129, 6,245,095, 6,238,428, 6,235,048, 6,231,595, 6,224,624, 6,149,677, 6,096,068, 6,042,559.

[0005] Surface cooling may be less optimally used. For example, externally applied cooling pads are disclosed in U.S. Patent Nos. 6,827,728, 6,818,012, 6,802,855, 6,799,063, 6,764,391, 6,692,518, 6,669,715, 6,660,027, 6,648,905, 6,645,232, 6,620,187, 6,461,379, 6,375,674, 6,197,045, and 6,188,930 (collectively, "the external pad patents"), all of which are incorporated herein by reference.

[0006] Regardless of the modality of cooling, it is believed that the sooner a patient is cooled after ischemic insult, the better the therapy. The present invention recognizes that many patients will have their first encounter with health care personnel in ambulances, prior to being afforded the opportunity for critical care such as controlled maintenance of hypothermia. Thus, it would be advantageous, as understood herein, to provide a means to bring cooling on board to patients as soon as possible.

SUMMARY OF THE INVENTION

[0007] A system for controlling patient temperature includes a closed loop heat exchange catheter configured for placement in the circulatory system of a patient to exchange heat with the blood of the patient. The system also includes a source of cold fluid, with the cold fluid being colder than normal body temperature and infusible from the source into the patient without using the catheter.

[0008] The catheter may be configured for percutaneous advancement into the central venous system of the patient. The catheter can carry coolant that is not infused into the bloodstream of the patient.

[0009] In another aspect, a method for treating a patient using hypothermia includes injecting cold saline into the venous system of the patient while the patient is located in an ambulance or in an emergency room of a hospital. Then subsequently hypothermia is maintained in the patient using an external heat exchange pad or an intravascular heat exchange catheter while the patient is in an operating room of a hospital or an intensive care unit of a hospital.

[0010] In yet another aspect, a method for treating a patient includes infusing into the patient's venous system a cold fluid having a temperature lower than a temperature of the patient to cause the fluid to mix with the blood of the patient and thereby to cool the patient. The method also includes engaging a cooling apparatus with the patient to maintain a desired hypothermic condition in the patient.

[0011] In additional embodiments, a system for controlling patient temperature includes a closed loop heat exchange catheter configured for placement in the circulatory system of a patient to exchange heat with the blood of the patient, and an external heat exchange bladder configured for exchanging heat with the skin of a patient. The system also includes a heat exchange system in a single housing and engageable with both the catheter and the bladder.

[0012] In non-limiting implementations of this last embodiment, the housing can include a sensor which detects when the heat exchange system is connected to the bladder, and potentially to the catheter as well, to provide a signal to a controller in the housing. Additionally, a controller may be in the housing and receive a patient temperature signal from a BTT sensor. Further, an IV bag can be supported on the housing for infusing cold saline directly into the bloodstream of a patient.

[0013] Continuing to summarize non-limiting implementations, the heat exchange system may include a coolant loop configured for exchanging heat with a working fluid loop associated with the catheter. The coolant loop may also be configured for direct fluid communication with the bladder. Or, the heat exchange system can include a coolant loop having a coldwell, with the catheter being associated with a catheter working fluid loop including a catheter coil disposable in the coldwell and with

the bladder being associated with a bladder working fluid loop including a bladder coil disposable in the coldwell. Both working fluid loops may be associated with respective pumps. The heat exchange system may also include an internal reservoir for priming the bladder, and may control both the catheter and bladder simultaneously. The heat exchange system can include a refrigerant loop including a compressor and one or more heat exchangers communicating with the compressor.

[0014] In another aspect, a heat exchange system includes a coolant loop, at least a first working fluid loop in thermal communication with the coolant loop and an intravascular heat exchange catheter associated with the first working fluid loop such that working fluid circulates through the heat exchange catheter without entering the patient's bloodstream when the catheter is positioned in the bloodstream. At least one external heat exchange member is configured for placement against a patient's skin to heat or cool the skin. The external heat exchange member is configured for heat transfer using the coolant loop.

[0015] In another aspect, a method for patient temperature control includes providing a heat exchange system, and engaging an intravascular heat exchange catheter with the system and with a patient to exchange heat with the patient. The method also includes engaging at least one bladder with the system and placing the bladder against the patient's skin to exchange heat with the patient.

[0016] In other aspects, a patient temperature control system includes at least one bladder through which working fluid can flow. The bladder is positionable against the skin of a patient, and a skin conditioning hydrogel can be disposed between the bladder and the skin.

[0017] In another aspect, a patient temperature control system includes at least one bladder through which working fluid can flow, with the bladder being configured as the front of a garment and having a trunk portion and two opposed limb portions that can drape over the patient.

[0018] In another aspect, a patient temperature control system includes at least one bladder through which working fluid can flow. The surface of the bladder facing away from a patient when the bladder is positioned against the skin of the patient is backed by a foam that conforms to pressure caused by the weight of the patient.

[0019] The details of the present invention, both as to its structure and operation, can best be understood in reference to the accompanying drawings, in which like reference numerals refer to like parts, and in which:

BRIEF DESCRIPTION OF THE DRAWINGS

[0020]

Figure 1 is a schematic diagram showing two modalities of controlled hypothermia maintenance in a patient, along with an apparatus for quickly reducing patient temperature;

Figure 2 is a flow chart of logic;

Figure 3 is a diagram of a single heat exchange chassis system that supports both an external cooling bladder and an intravascular temperature control catheter;

Figure 4 is a schematic diagram showing that the heat exchange system can have two heat exchangers in parallel with one compressor;

Figure 5 is a schematic diagram of an alternate system;

Figure 6 is a cross-section of a non-limiting quick disconnect feature as would be seen along the line 6-6 in Figure 5;

Figure 7 is a schematic diagram of an alternate system; and

Figure 8 is a schematic diagram of an alternate system.

DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENT

[0021] Referring initially to Figure 1, a system is shown, generally designated 10, that includes a heat exchange catheter 12 that is in fluid communication with a catheter temperature control system 14.

[0022] In accordance with present principles, the system 10 can be used to induce therapeutic hypothermia in a patient 16 using a catheter in which coolant circulates in a closed loop, such that no coolant enters the body. While certain preferred catheters are disclosed below, it is to be understood that other catheters can be used in accordance with present principles, including, without limitation, any of the catheters disclosed in the following U.S. patents, all incorporated herein by reference: USPN 5,486,208, 5,837,003, 6,110,168, 6,149,673, 6,149,676, 6,231,594, 6,264,679, 6,306,161, 6,235,048, 6,238,428, 6,245,095, 6,251,129, 6,251,130, 6,254,626, 6,261,312, 6,312,452, 6,325,818, 6,409,747, 6,368,304, 6,338,727, 6,299,599, 6,287,326, 6,126,684. The catheter 12 may be placed in the venous system, e.g., in the superior or inferior vena cava.

[0023] Instead of or in addition to the catheter 12, the system 10 may include one or more pads 18 that are positioned against the external skin of the patient 16 (only one pad 18 shown for clarity). The pad 18 may be, without limitation, any one of the pads disclosed in the external pad patents. The temperature of the pad 18 can be controlled by a pad controller 20 in accordance with principles set forth in the external pad patents to exchange heat with the patient 16, including to induce therapeutic mild or moderate hypothermia in the patient in response to the patient presenting with, e.g., cardiac arrest, myocardial infarction, stroke, high intracranial pressure, traumatic brain injury, or other malady the effects of which can be ameliorated by hypothermia.

[0024] To cool the patient while awaiting engagement of the catheter 12 and/or pad 18 with the patient, cold fluid 22 in a cold fluid source 24 may be injected into the

patient and in particular into the patient's venous system through a pathway 26. Without limitation, the pathway 26 may be an IV line, the source 24 may be an IV bag, and the fluid 22 may be chilled saline, e.g., saline at the freezing point or slightly warmer. Or, the source may be a syringe, and the saline can be injected directly into the bloodstream of the patient.

[0025] Now referring to Figure 2, at block 28 the patient presents with symptoms indicating that the application of hypothermia is appropriate. For instance, the patient may have cardiac arrest, and may be resuscitated. Or, the patient may present with myocardial infarction or stroke or other malady.

[0026] At block 30, cold saline 22 is immediately (in the case of cardiac arrest patients, immediately after resuscitation) injected into the patient's bloodstream, preferably at a venous site, using the source 24. This can occur in, e.g., an ambulance on the way to the hospital for further temperature management, and/or in the hospital emergency room. Hypothermia treatment including the establishment and maintenance of mild or moderate hypothermia subsequently is effected at block 32 using the catheter 12 and/or pad 18, typically in the operating room or intensive care unit of a hospital, although in some hospitals the step at block 32 may begin while the patient is still in the emergency room or even while the patient is still in the ambulance.

[0027] The above three modalities of cooling - intravascular closed loop catheter, external pad/bladder, and cold saline bolus infusion - may be supported by a single housing.

[0028] With greater specificity, Figure 3 shows details of one non-limiting single-chassis heat exchange system, generally designated 100, which includes a single heat exchange system housing 102 holding all or portions of three fluid loops. Specifically, a refrigerant loop 104 exists in which refrigerant flows between a compressor 106 and at least one heat exchanger 108. Exiting the heat exchanger 108, the refrigerant passes through a CP valve 110 to a condenser 112, which condenses the refrigerant. The refrigerant loop 104 may be replaced by a thermoelectric cooling loop in which the fluid is air passing over and cooling a TEC element.

[0029] In the heat exchanger 108, the refrigerant expands to cool a coolant in a coolant loop 114, which is in thermal but not fluid contact with the refrigerant loop 104. The coolant may be water, propylene glycol, a mixture thereof, or other suitable coolant. Also included in the coolant loop 114 is a heater 116 for heating the coolant to, e.g., re-warm a patient, and a coolant pump 118 to circulate the coolant through the coolant loop 114. The coolant pump may be a magnetically-coupled non-displacement pump, or a positive displacement pump.

[0030] Figure 3 shows that the coolant flows into a chamber defined by a coldwell 120, which may be the highest point in the system. A catheter fluid loop coil 122 may be disposed in the coldwell 120 in thermal but not in fluid contact with the coolant. The catheter fluid loop

coil 122 defines part of a working fluid loop 124 through which a working fluid such as saline flows. The fluid in the working fluid loop 124 circulates, under the influence of a working fluid pump 126, which can be a peristaltic pump, through an intravascular heat exchange catheter 128 without exiting the catheter into the bloodstream. The working fluid exchanges heat with the coolant in the coldwell 120. A saline bag 130 may be provided in the working fluid loop 124 for priming purposes, and an air trap 132 may also be provided to prevent any air that might exist in the working fluid loop 124 from entering the catheter 128. The entire working fluid loop 124 may be provided as a standalone catheter start-up kit, with the catheter fluid loop coil 122 disposed by medical personnel in the coldwell 120 and with the catheter 128 then being advanced into the vasculature of a patient to exchange heat with the patient. Additional details of the non-limiting system 100 may be found in the present assignee's U.S. Pat. Nos. 6,146,411, 6,581,403, and 6,529,775, all of which are incorporated herein by reference, and in U.S. patent application serial no. 10/944,544, filed September 17, 2004, also incorporated herein. The above patents further disclose non-limiting ways in which a controller/power supply 133 controls various of the components above to heat or cool the working fluid as necessary to achieve a user-set target temperature. A patient temperature sensor 133a can send a patient temperature signal to the controller 133 as shown. The sensor 133a may be any suitable sensor including, without limitation, a brain temperature tunnel (BTT) sensor to sense the temperature through thin peri-ocular skin of a sinus, which represents the temperature of the brain.

[0031] Still referring to Figure 3, in lieu of placing the catheter fluid loop coil 122 in the coldwell 120 and the catheter 128 in the patient, a bladder cooling loop coil 134, which is part of a bladder fluid loop 136, may be disposed in the coldwell 120. A bladder fluid pump 138, which can be a positive displacement pump, circulates working fluid, which could be tap water or saline or other appropriate fluid, through the loop 136. Included in the loop 136 is an externally-applied bladder 140 through which the working fluid flows to cool a patient. The bladder 140 may be any suitable cooling device such as a conformal pad or a mattress that is placed against the skin, including any of the devices referred to previously. An adhesive or non-adhesive hydrogel and/or a silver sulphur diazene cream or zinc paste may be disposed between the bladder and patient. Or, a skin conditioning hydrogel such as glycerol in sorbolene can be used. The bladder itself may be configured as the front of a shirt or trousers, i.e., with a trunk portion and two opposed limb portions that can drape over the patient. The surface of the bladder that faces away from the patient can be backed by a NASA foam that conforms to pressure caused by the weight of the patient to reduce the risk of bedsores.

[0032] A saline bag 142 may be provided in the loop 136 for priming. Also, a three-way stopcock 144 can be

provided as shown to isolate the bag 142. The loop 136 may be controlled by a separate bladder controller/power supply 146, which may communicate with the controller 133 if desired.

[0033] An IV pole 147 may be mounted on the housing 102 and may support an IV bag 148, for infusing cold saline in the IV bag directly into the bloodstream of the patient as shown. A coil 149 may be provided in communication with the IV bag. The coil 149 may be disposed in the coldwell 120 to cool saline in coil, which can circulate under the influence of a pump 149a.

[0034] Figure 4 shows that for greater heat exchange power, a compressor 150 may circulate refrigerant through two heat exchangers 152, 154, either in parallel with each other or with one of the heat exchangers isolated by means of a computer-controlled solenoid valve 156. The arrangement shown in Figure 4 could be used in lieu of the arrangements shown in the other figures herein.

[0035] Figure 5 shows the coolant loop portion 200 of an alternate system 202, which in all essential respects is identical to the system 100 shown in Figure 3 with the following exceptions. Coolant such as water may flow, under the influence of a coolant pump 204, through a heat exchanger 206 and a computer-controlled three-way valve 208, which either sends the coolant to a coldwell 210 to exchange heat with the coil of an intravascular catheter as described above, or to a bladder loop 212 that includes an external heat exchange bladder 214 as shown. A priming reservoir 216, which can be internal to the chassis of the system 202, may be provided for priming the bladder 214 with coolant, it being understood that in some embodiments the coldwell itself can be used for priming instead, in which case an additional three-way valve between the coldwell and first three-way valve 208 could be required for establishing the appropriate fluid flow control.

[0036] In any case, as shown in Figure 5 the bladder 214 is connected to a supply line 218 and a return line 220, with the lines 218, 220 terminating in respective bladder fittings 222, 224 that engage respective system fittings 226, 228 on the chassis of the system 202. Preferably, the fittings are quick disconnect fittings that provide an indication of engagement and disengagement to the controller (not shown) of the system 202 for establishing the position of the three-way valve 208 for catheter or bladder operation as appropriate. Thus, in Figure 5 the coolant loop supplies either the coldwell for exchanging heat with the working fluid circuit of the intravascular catheter, or it supplies the bladder directly.

[0037] It is undesirable that the heat exchanger freeze during, e.g., priming. Accordingly, when the system detects the bladder being connected, it can maintain system fluid temperatures above the freezing point. In any case, to avoid skin damage it is preferred that when the bladder is used the coolant temperature be maintained between four and forty two degrees Celsius.

[0038] A non-limiting example of quick disconnect fit-

tings (using 224,228 as examples) is shown in Figure 6. As shown, the bladder fitting 224 may be circumscribed by a collar 230, and as the bladder fitting 224 is advanced into the system fitting 228, the collar 230 deflects a ball 232 that is reciprocally disposed in the wall of the system fitting 228 and that is urged inwardly (toward the bladder fitting 224) as shown by a spring 234. As the ball 232 deflects, it actuates a sensing element 236 on the system fitting 228 to provide an "engaged" signal to the system controller, which can then reconfigure the user interface and/or control parameters used for establishing patient temperature. Or, the ball and spring can be omitted and the collar seat against the sensing element when the fittings are engaged, to actuate the sensing element. Other arrangements known in the art may be used. The sensing element 236 may be an electrical contact or other suitable element known in the art. It is to be understood that the catheter start-up kit shown in Figure 3 may also be connected to the system using such fittings, so that in any of the embodiments herein, the controller "knows" which device or devices, catheter and/or bladder, is connected.

[0039] Figures 7 and 8 show alternate embodiments in which a bladder 300 is part of a bladder working fluid loop 302 that includes a bladder coil 304 disposable in a bladder coldwell 306, it being understood that the catheter-related working fluid loop shown in Figure 3 with separate catheter coldwell and catheter working fluid loop pump is also provided in a system that includes the refrigerant loop and working fluid loop shown in Figure 3. In essence, in the systems of Figures 7 and 8 two separate working fluid loops are provided, one for the external cooling bladder and one for the intravascular catheter, with both loops being controlled by a common controller, e.g., the controller 303 shown in Figure 3. In any case, a bladder working fluid loop pump 308 provides the motive force for circulating the working fluid. Either an external saline bag 310 (Figure 7) can be provided for priming through a three-way stopcock 312, or a reservoir 314 (Figure 8) that is internal to the system chassis can be provided. In both cases, a supply line 316 to the coil 304 and a return line 318 from the bladder 300 (or from the stopcock 312 when one is used as shown in Figure 7) terminate in quick-disconnect fittings 320, 322 as shown, for operation as described above to alert the system controller to whether the bladder is connected. In the embodiments shown in Figures 7 and 8, since two separate working fluid loops are provided, both the catheter and the bladder can be simultaneously controlled by the controller to heat or cool a patient. Or, if simultaneous catheter/bladder use is not required, the bladder loop may not include its own coldwell and pump but rather can use a single coldwell that services either catheter and bladder.

While the particular SYSTEM AND METHOD FOR BRINGING HYPOTHERMIA RAPIDLY ONBOARD as herein shown and described in detail is fully capable of attaining the above-described objects of the invention, it is to be understood that it is the presently preferred em-

bodiment of the present invention and is thus representative of the subject matter which is broadly contemplated by the present invention, that the scope of the present invention fully encompasses other embodiments which may become obvious to those skilled in the art, and that the scope of the present invention is accordingly to be limited by nothing other than the appended claims, in which reference to an element in the singular is not intended to mean "one and only one" unless explicitly so stated, but rather "one or more". All structural and functional equivalents to the elements of the above-described preferred embodiment that are known or later come to be known to those of ordinary skill in the art are expressly incorporated herein by reference and are intended to be encompassed by the present claims. Moreover, it is not necessary for a device or method to address each and every problem sought to be solved by the present invention, for it to be encompassed by the present claims. Furthermore, no element, component, or method step in the present disclosure is intended to be dedicated to the public regardless of whether the element, component, or method step is explicitly recited in the claims. Other aspects of the invention may include any of the following.

1. A system for controlling patient temperature, comprising: a closed loop heat exchange catheter (12, 128) configured for placement in the circulatory system of a patient to exchange heat with the blood of the patient; and a source (24) of cold fluid, the cold fluid being colder than normal body temperature, the fluid being infusible from the source (24) into the patient without using the catheter (12).
2. The system of aspect 1, wherein the catheter (12, 128) is configured for percutaneous advancement into the central venous system of the patient.
3. The system of aspect 1, wherein the catheter (12, 128) carries coolant that is not infused into the bloodstream of the patient.
4. A system for controlling patient temperature, comprising: a closed loop heat exchange catheter (12, 128) configured for placement in the circulatory system of a patient to exchange heat with the blood of the patient; an external heat exchange bladder (18, 140, 214, 300) configured for exchanging heat with the skin of a patient; and a heat exchange system (100, 202) engageable with both the catheter (12, 128) and the bladder (18, 140, 214, 300).
5. The system of aspect 4, wherein the heat exchange system (100, 202) includes a housing (102) holding at least one sensor (236) sensing the fluid flow engagement of the heat exchange system with at least one of: the bladder, and the catheter, the sensor (236) providing a signal to a controller (146, 133) in the housing.
6. The system of aspect 4, comprising a controller (146, 133) receiving a patient temperature signal

from a BTT sensor (133a).

7. The system of aspect 4, wherein the heat exchange system includes at least one coolant loop (114, 200), the coolant loop configured for exchanging heat with a working fluid loop (124) associated with the catheter, the coolant loop also being configured for fluid communication with the bladder.
8. The system of aspect 4, wherein the heat exchange system includes at least one refrigerant loop (104) including a compressor (106) and at least one heat exchanger (108, 152, 154) communicating with the compressor.
9. The system of aspect 8, comprising two heat exchangers (152, 154) in fluid flow parallel with each other.
10. The system of aspect 4, wherein the heat exchange system includes at least one coolant loop having a coldwell (120, 210, 306), the catheter being associated with a catheter working fluid loop (124) including a catheter coil (122) disposable in the coldwell, the bladder being associated with a bladder working fluid loop (136) including a bladder coil (134).
11. The system of aspect 10, wherein both working fluid loops are associated with respective pumps (126, 138).
12. The system of aspect 9, wherein the heat exchange system includes an internal reservoir (314) for priming the bladder.
13. The system of aspect 4, wherein the heat exchange system controls both the catheter and bladder simultaneously.

Claims

1. A system for controlling patient temperature, comprising:
 - a closed loop heat exchange catheter (12, 128) configured for placement in the circulatory system of a patient to exchange heat with the blood of the patient;
 - an external heat exchange bladder (18, 140, 214, 300) configured for exchanging heat with the skin of a patient; and
 - a heat exchange system (100, 202) engageable with both the catheter (12, 128) and the bladder (18, 140, 214, 300).
2. A system for controlling patient temperature, comprising:
 - a heat exchange system (100, 202) having
 - a first working fluid loop (124) configured for closed loop fluid flow engagement with a heat exchange catheter (12, 128); and
 - a second working fluid loop (136, 212) config-

- ured for fluid flow engagement with an external heat exchange member or bladder (18, 140, 214, 300).
3. The system of Claim 1 or claim 2, wherein the heat exchange system (100, 202) includes a housing (102) holding at least one sensor (236) sensing the fluid flow engagement of the heat exchange system with at least one of the bladder and the catheter, the sensor (236) providing a signal to a controller (146, 133) in the housing. 5
 4. The system of Claim 1 or claim 2, comprising a controller (146, 133) receiving a patient temperature signal from a patient temperature sensor (133a). 10
 5. The system of Claim 1, wherein the heat exchange system includes at least one coolant loop (114, 200), the coolant loop configured for exchanging heat with a working fluid loop (124) associated with the catheter, the coolant loop also being configured for fluid communication with the bladder. 15
 6. The system of Claim 1, wherein the heat exchange system includes at least one refrigerant loop (104) including a compressor (106) and at least one heat exchanger (108, 152, 154) communicating with the compressor. 20
 7. The system of Claim 1, wherein the heat exchange system includes at least one coolant loop having a coldwell (120, 210, 306), the catheter being associated with a catheter working fluid loop (124) including a catheter coil (122) disposable in the coldwell, the bladder being associated with a bladder working fluid loop (136) including a bladder coil (134). 25
 8. The system of Claim 1, wherein the catheter is associated with a catheter working fluid loop (124) and the bladder is associated with a bladder working fluid loop (136), wherein both working fluid loops (124, 136) are associated with respective pumps (126, 138). 30
 9. The system of Claim 1 or claim 2, wherein the heat exchange system is configured to control both the catheter (12, 128) and bladder (18, 140, 214, 300) simultaneously. 35
 10. The system of Claim 2, wherein the first working fluid loop (124) is configured for exchanging heat with a coolant loop (114, 200). 40
 11. The system of Claim 2, wherein the heat exchange system (100, 202) includes at least one refrigerant loop (104), the refrigerant loop including a compressor (106) and at least one heat exchanger (108, 152, 154) communicating with the compressor. 45
 12. The system of Claim 10, wherein: the coolant loop (114, 200) has a coldwell (120, 210, 306); the first working fluid loop (124) includes a catheter coil (122) disposable in the coldwell; and the second working fluid loop (136) including a bladder coil (134). 50
 13. The system of Claim 2, wherein both the first working fluid loop (124) and the second working fluid loop (136, 212) are each associated with a respective pump (126, 138, 204). 55
 14. The system of Claim 2, further including the catheter (12, 128) which is configured for percutaneous advancement into the central venous system of the patient.
 15. The system of Claim 14, wherein the catheter (12, 128) carries working fluid that is not infused into the bloodstream of the patient.
 16. The system of claim 2, further including the external heat exchanger member or bladder (18, 140, 214, 300).
 17. The system of claim 16 wherein the bladder (18, 140, 214, 300) comprises a pad or a mattress or a part of a shirt or trousers or other garment.

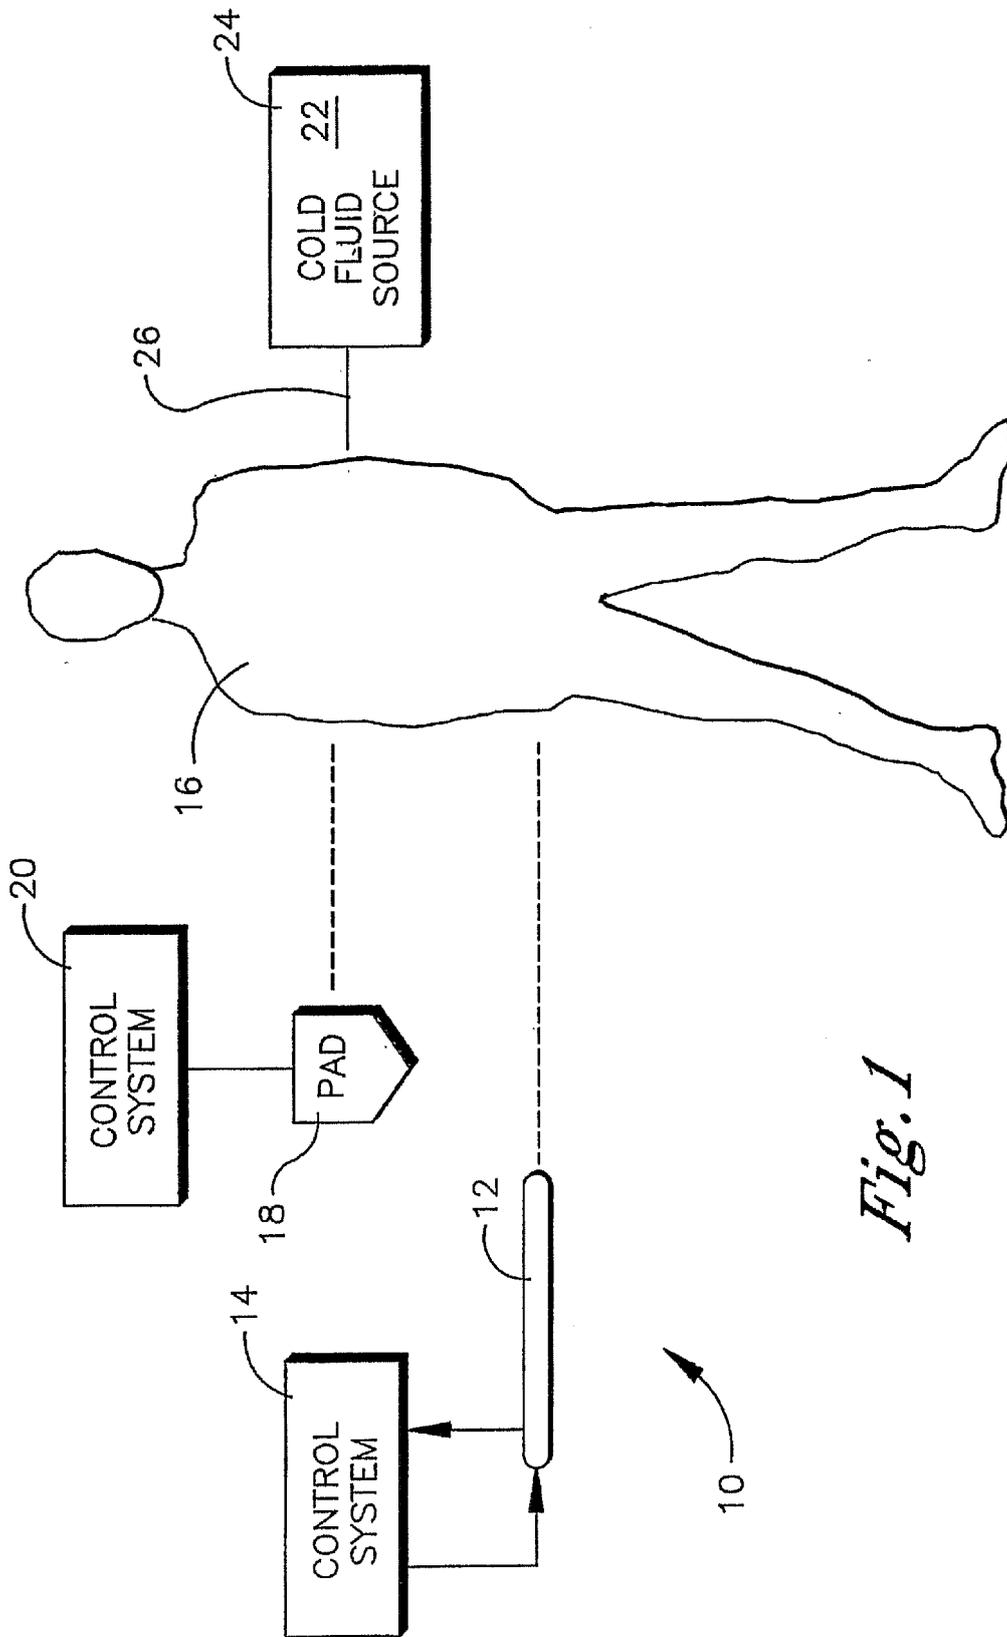


Fig. 1

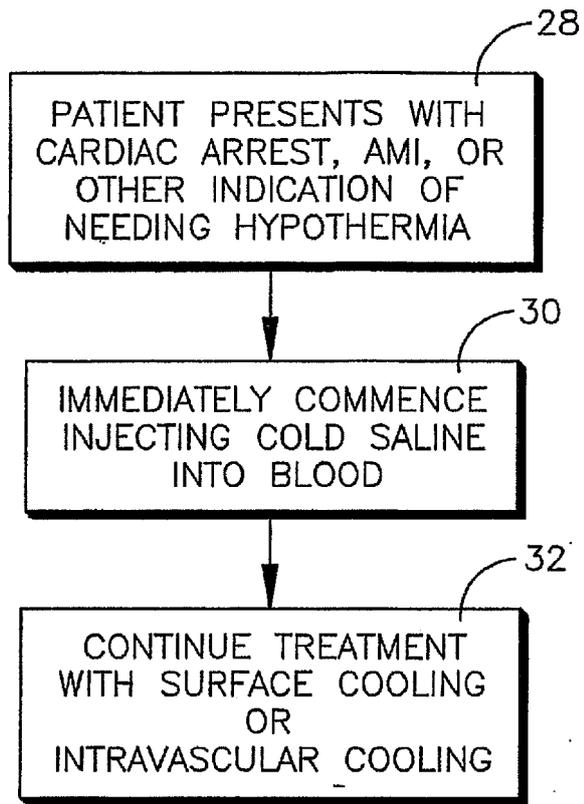


Fig. 2

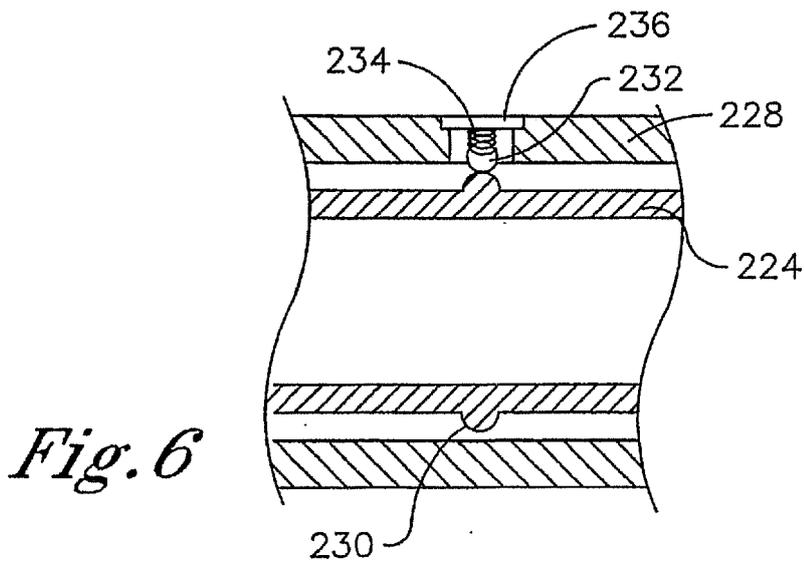


Fig. 6

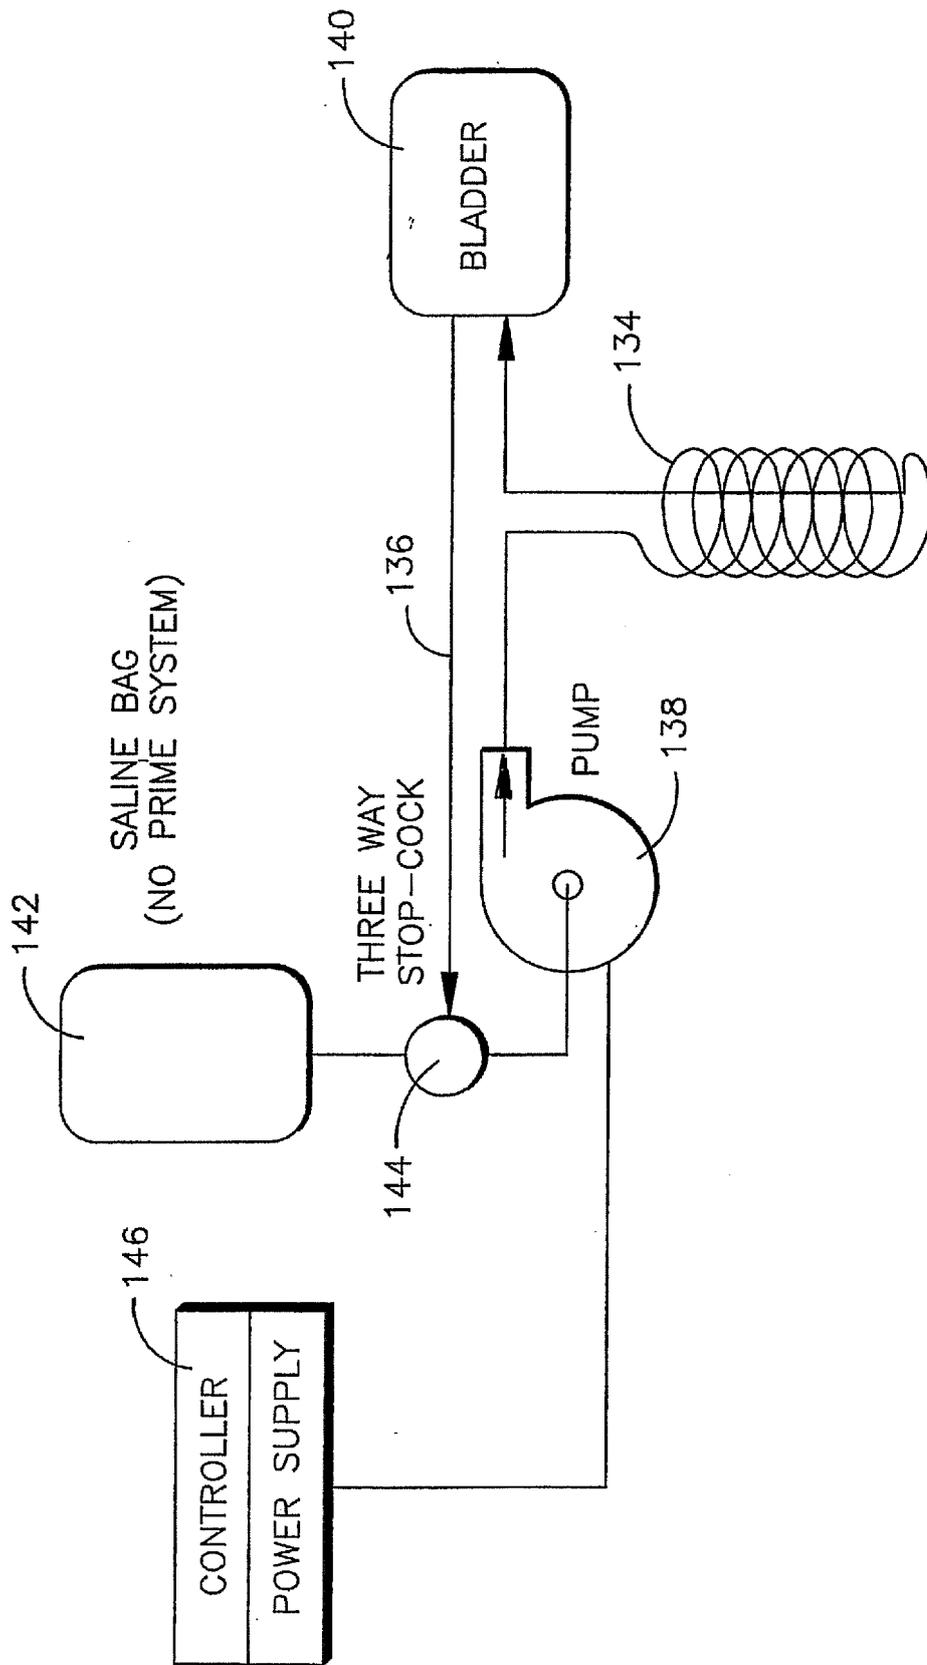


Fig. 3

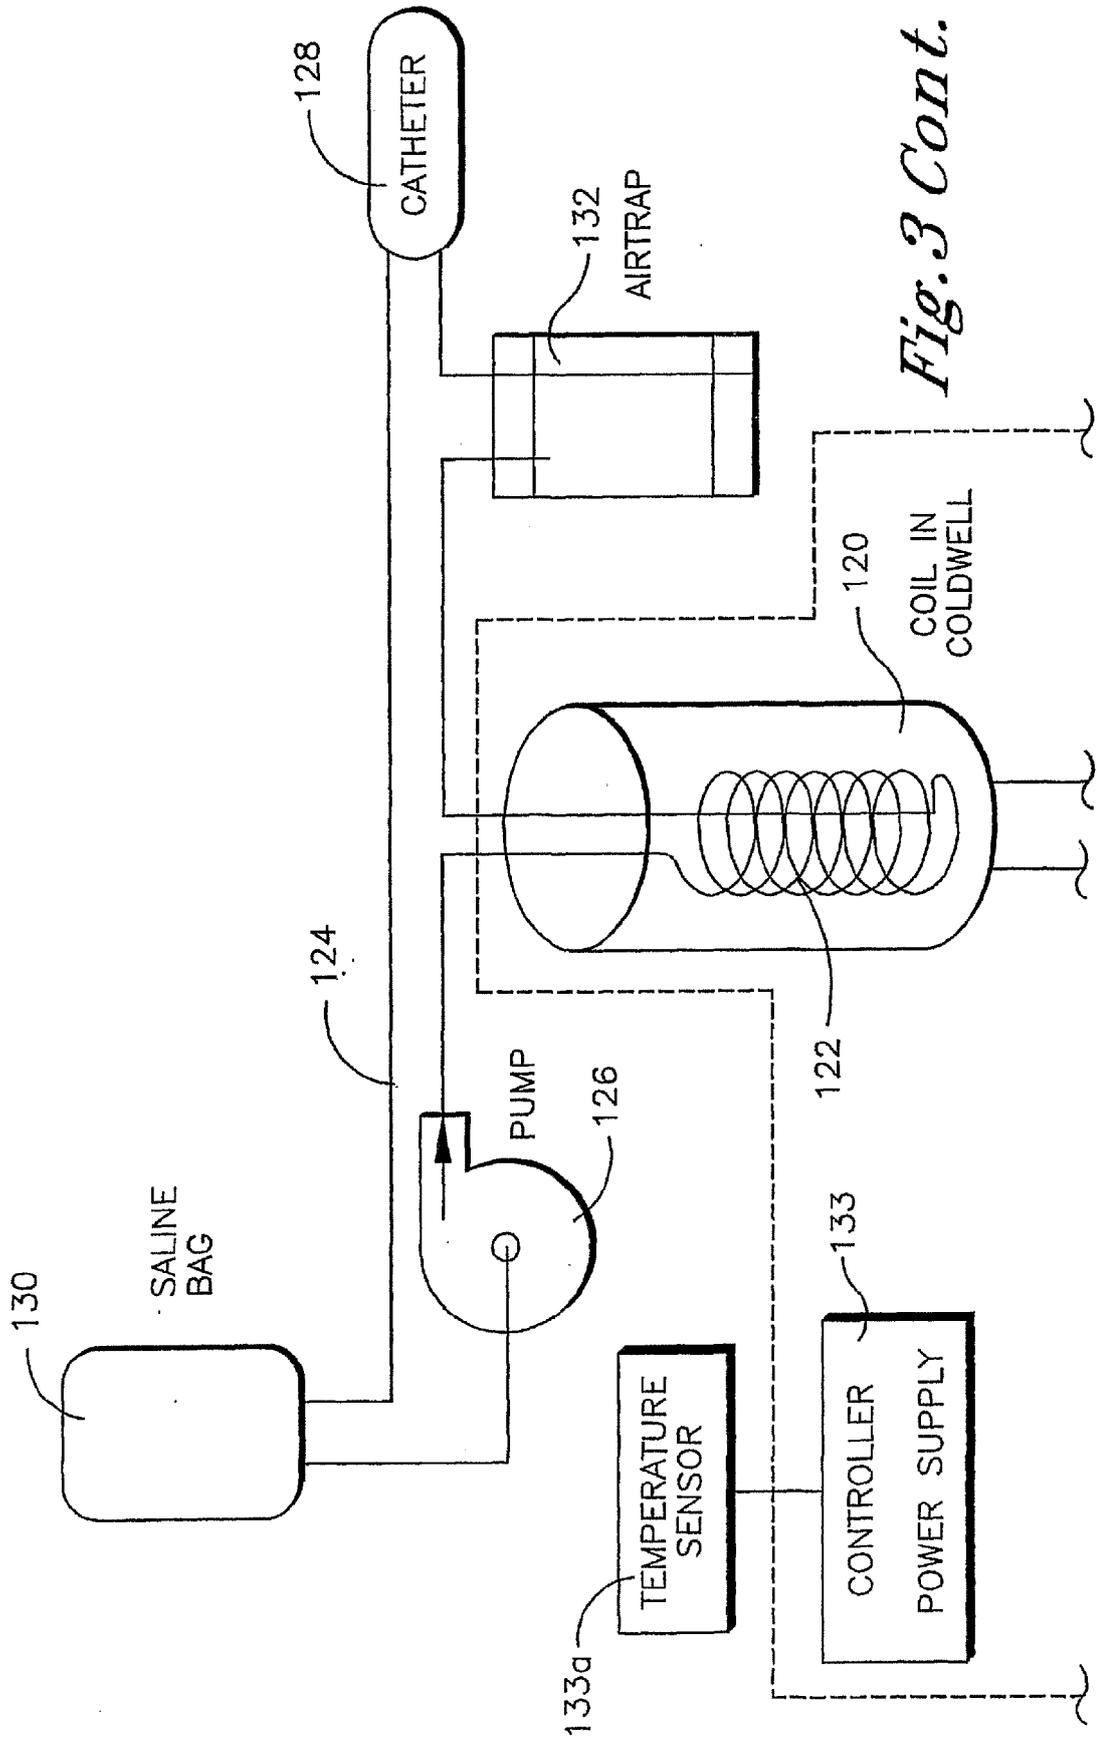


Fig. 3 Cont.

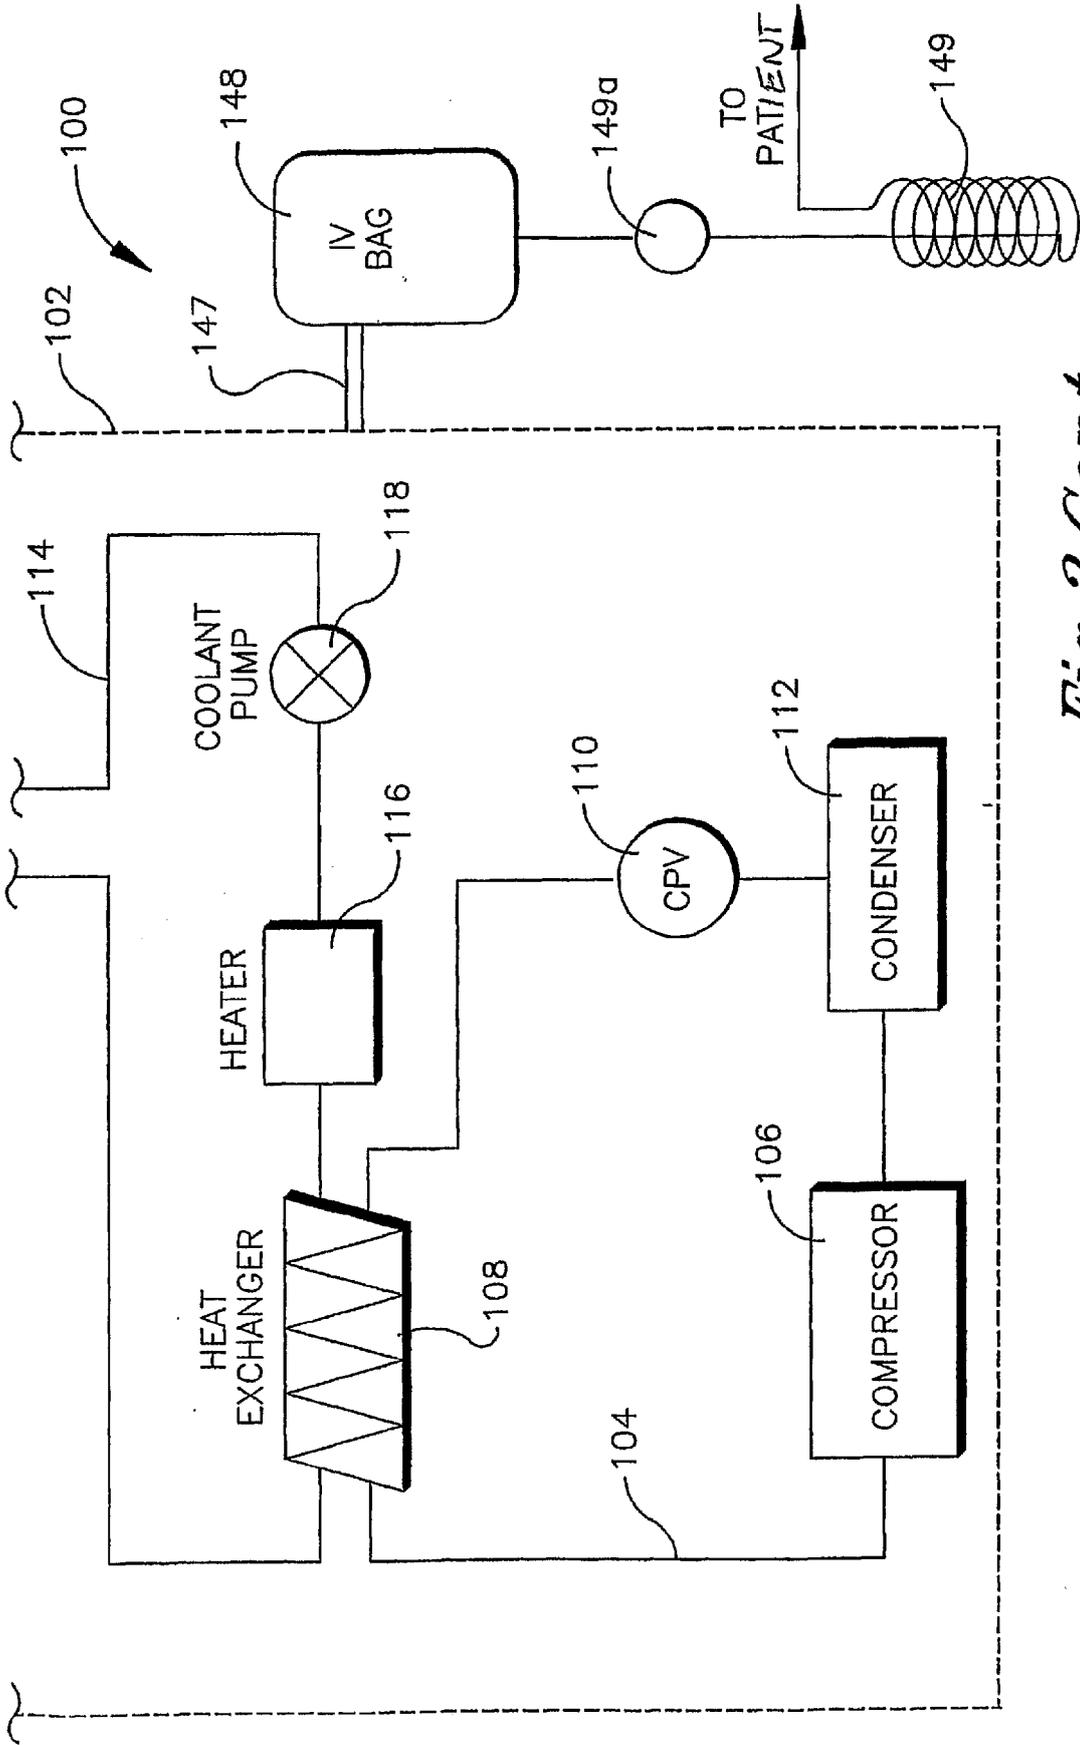


Fig. 3 Cont.

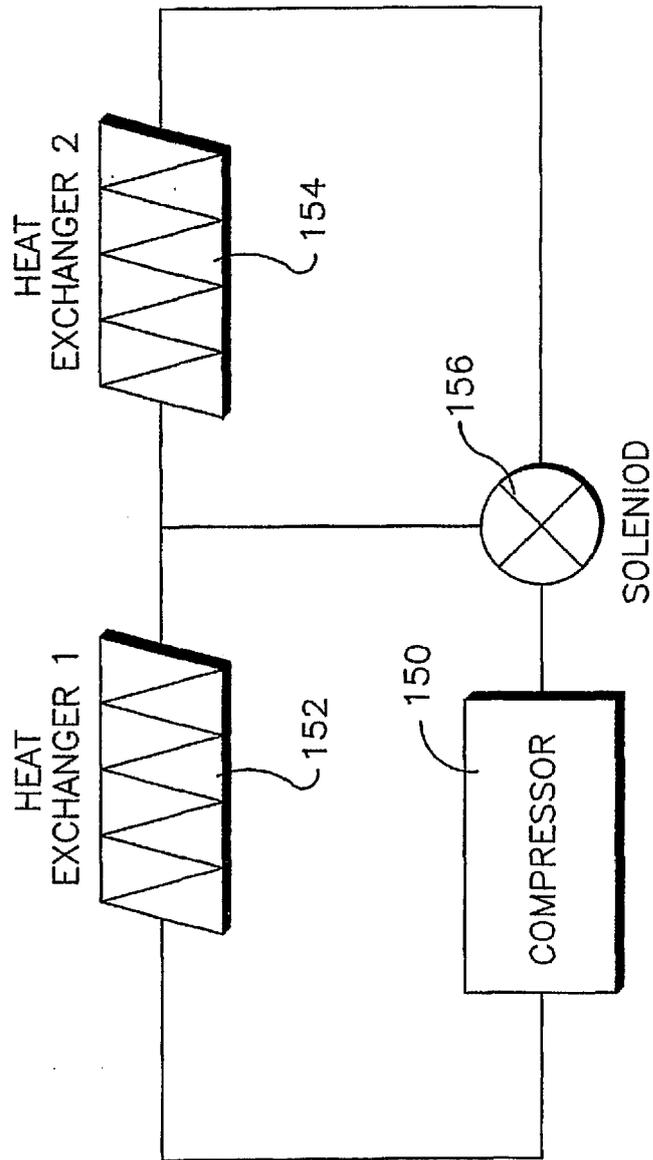


Fig. 4

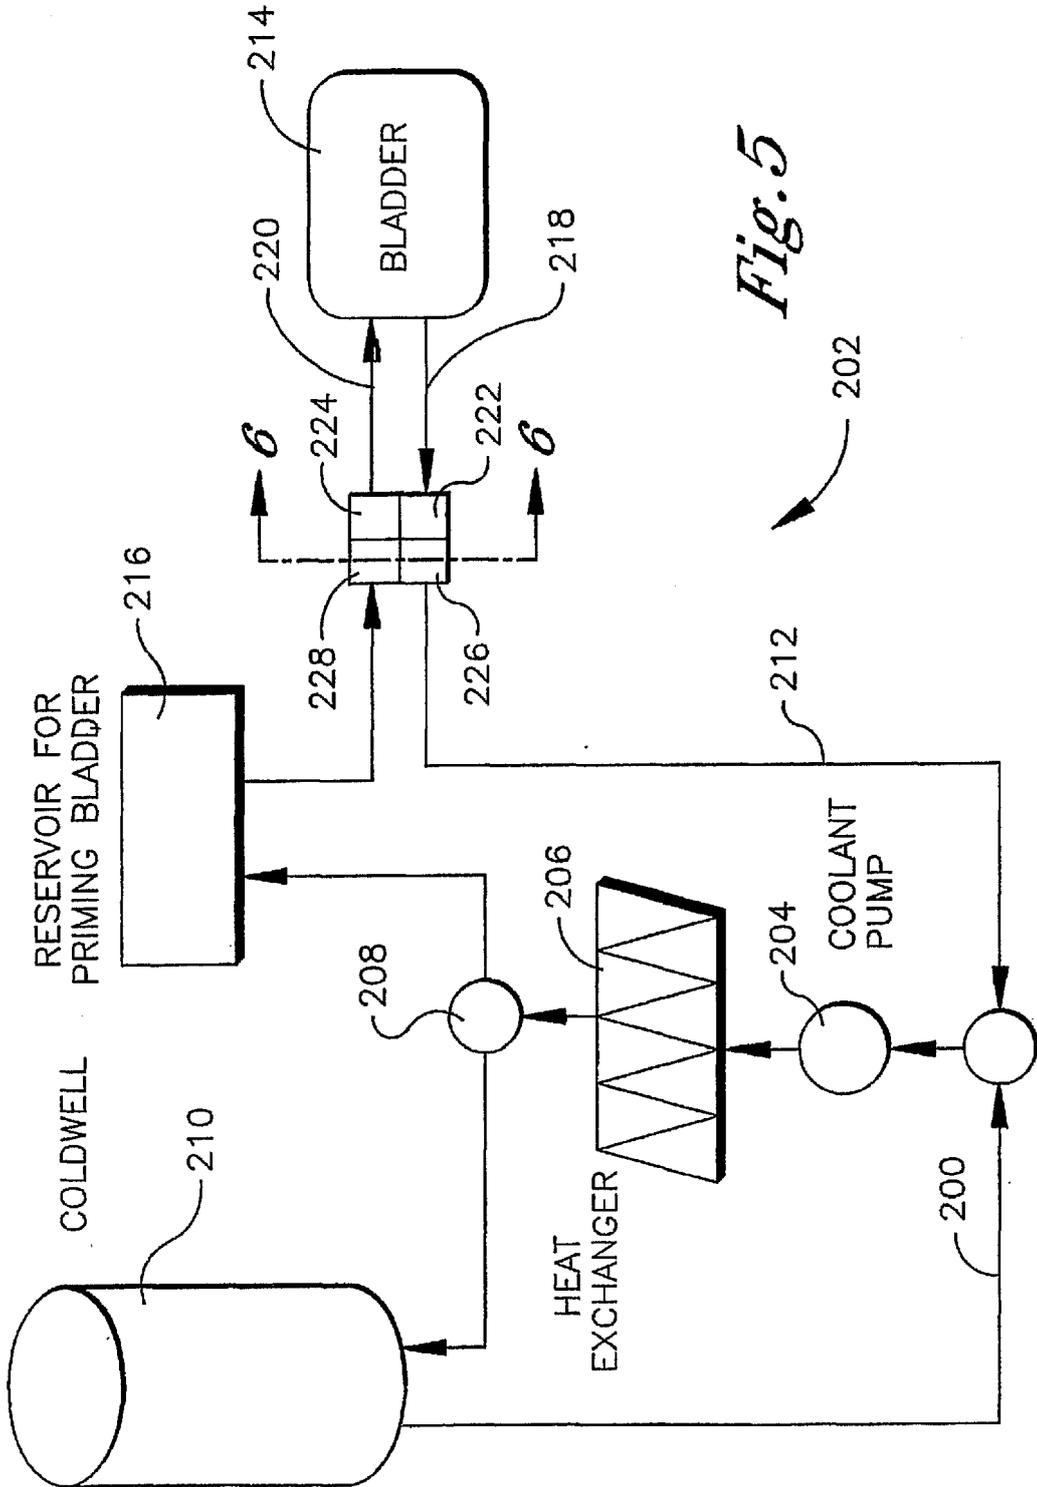


Fig. 5

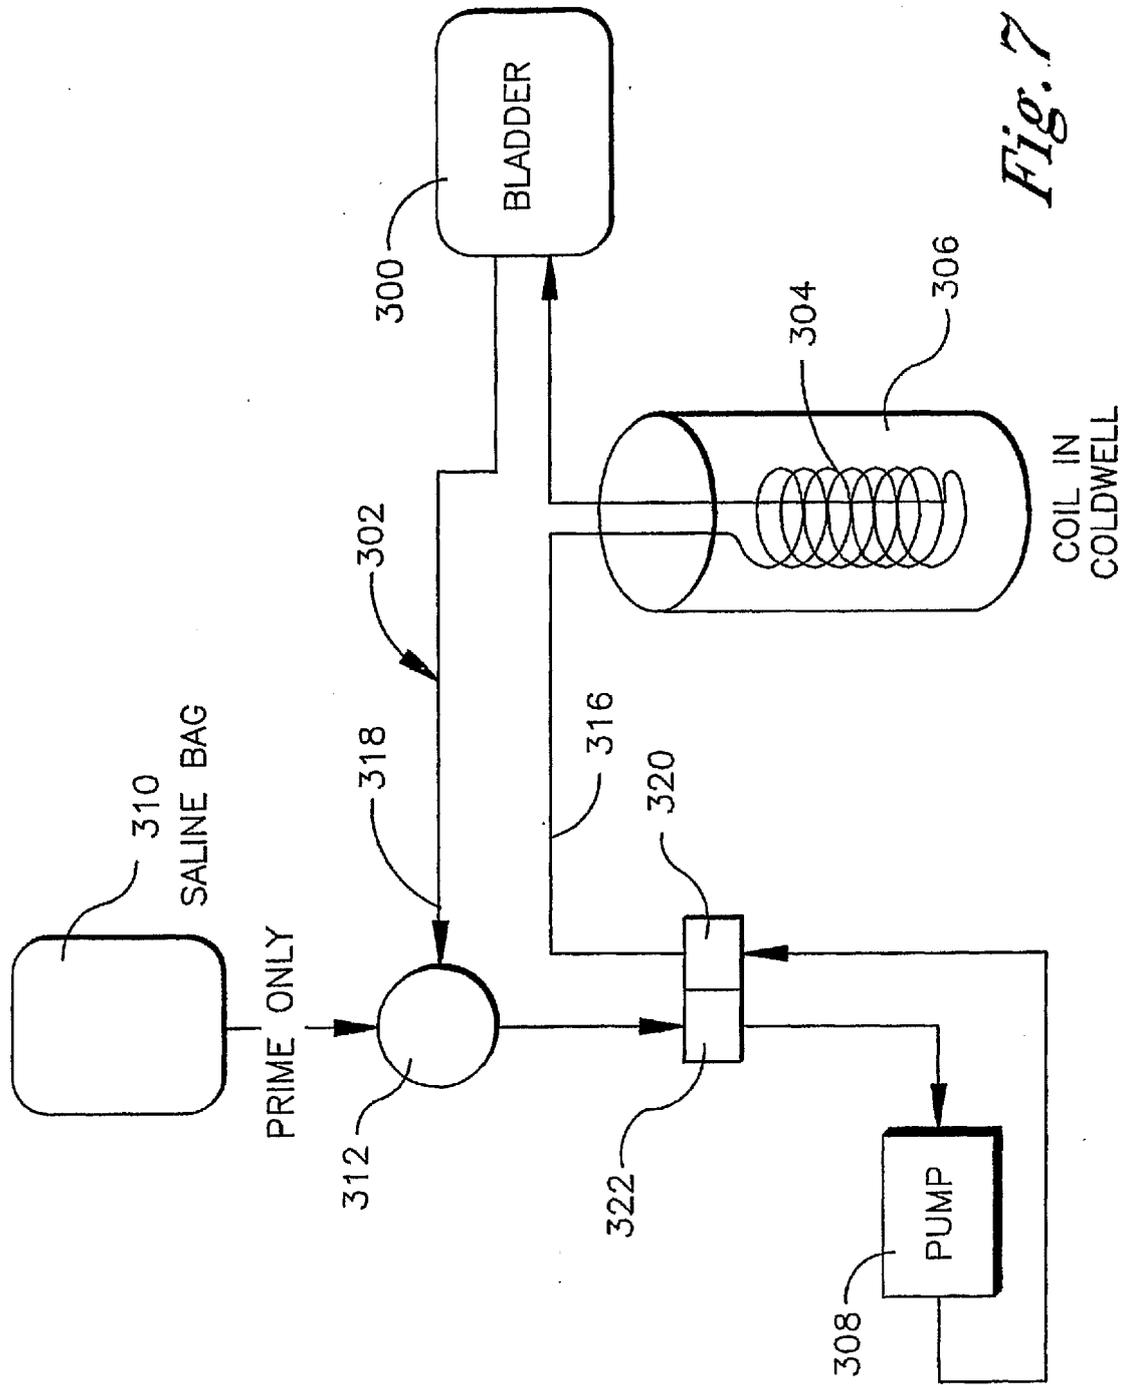


Fig. 7

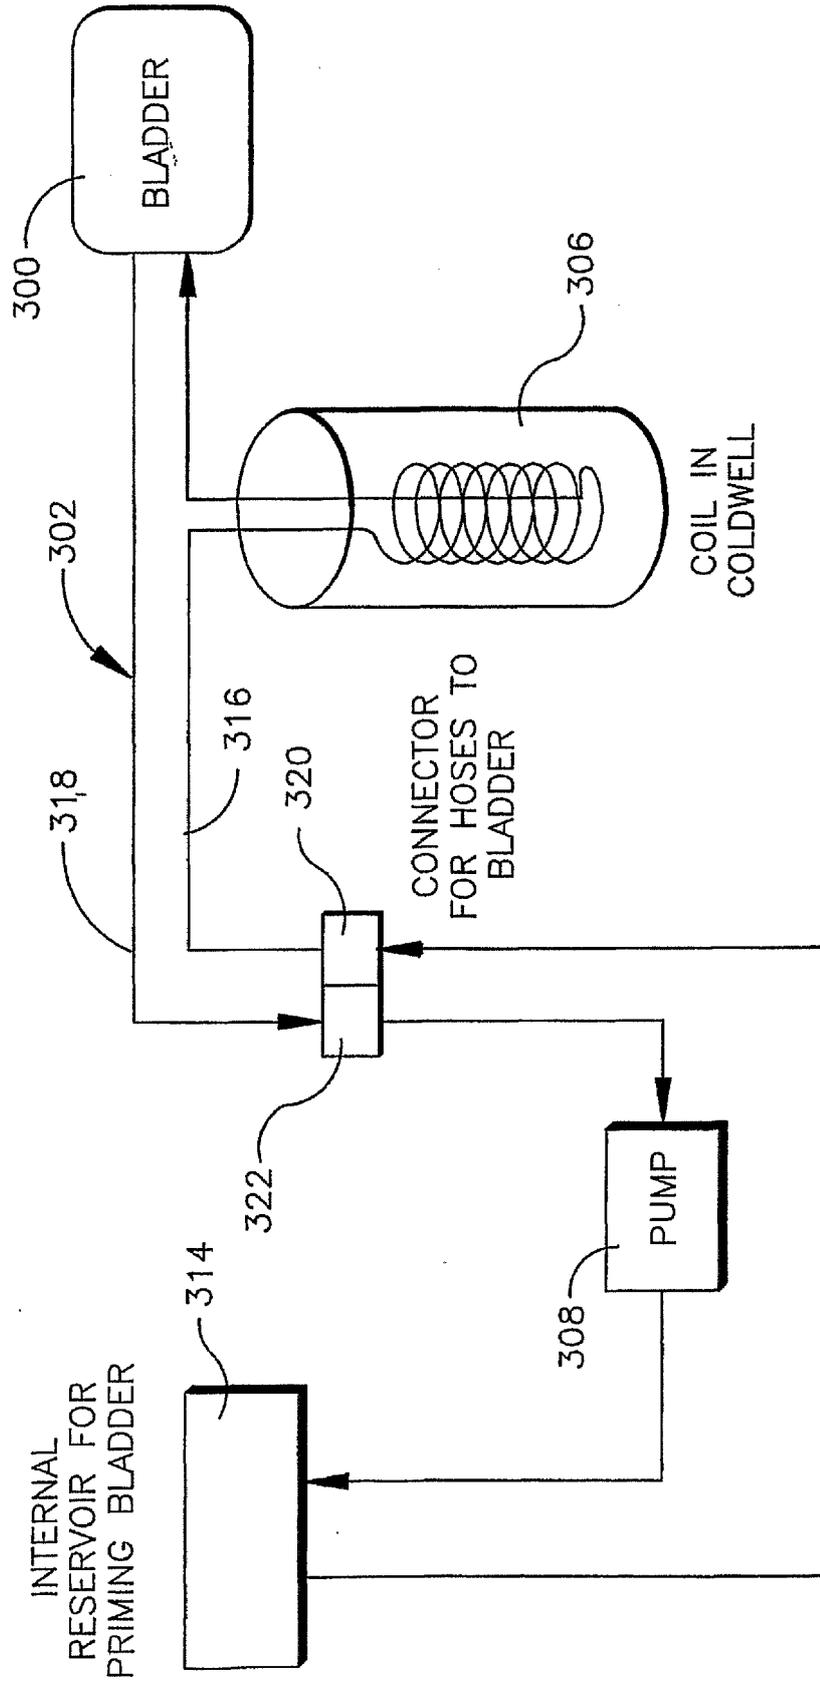


Fig. 8



EUROPEAN SEARCH REPORT

Application Number
EP 19 16 3548

5

10

15

20

25

30

35

40

45

50

55

DOCUMENTS CONSIDERED TO BE RELEVANT			
Category	Citation of document with indication, where appropriate, of relevant passages	Relevant to claim	CLASSIFICATION OF THE APPLICATION (IPC)
X	US 2001/047196 A1 (GINSBURG ROBERT [US] ET AL) 29 November 2001 (2001-11-29) * paragraph [0118] - paragraph [0119]; figure 16 * * paragraph [0002] - paragraph [0003] * * paragraph [0122] * * paragraph [0116] * * paragraph [0033] *	1,3,4,6,9-17	INV. A61F7/02 A61F7/12 A61F7/08
X	US 5 476 444 A (KEELING NORMAN G [US] ET AL) 19 December 1995 (1995-12-19) * column 9, line 31 - column 10, line 36; figure 1 * * column 4, line 63 *	2-4,10-13,16,17	
X	US 2004/158303 A1 (LENNOX CHARLES D [US] ET AL) 12 August 2004 (2004-08-12) * paragraph [0111] - paragraph [0119]; figure 11a *	2,4	
A	US 2003/130651 A1 (LENNOX CHARLES D [US]) 10 July 2003 (2003-07-10) * paragraph [0057]; figure 6 *	1-17	TECHNICAL FIELDS SEARCHED (IPC) A61F A61B
A	WO 03/059218 A1 (ALSIUS CORP [US]; EVANS SCOTT [US]; WORTHEN WILLIAM [US]) 24 July 2003 (2003-07-24) * figures 1,2 *	1-17	
The present search report has been drawn up for all claims			
Place of search The Hague		Date of completion of the search 10 July 2019	Examiner Ekstrand, Vilhelm
CATEGORY OF CITED DOCUMENTS X : particularly relevant if taken alone Y : particularly relevant if combined with another document of the same category A : technological background O : non-written disclosure P : intermediate document T : theory or principle underlying the invention E : earlier patent document, but published on, or after the filing date D : document cited in the application L : document cited for other reasons & : member of the same patent family, corresponding document			

EPO FORM 1503 03/02 (P04C01)

ANNEX TO THE EUROPEAN SEARCH REPORT
ON EUROPEAN PATENT APPLICATION NO.

EP 19 16 3548

5 This annex lists the patent family members relating to the patent documents cited in the above-mentioned European search report.
The members are as contained in the European Patent Office EDP file on
The European Patent Office is in no way liable for these particulars which are merely given for the purpose of information.

10-07-2019

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
US 2001047196 A1	29-11-2001	AT 353204 T	15-02-2007
		AT 485795 T	15-11-2010
		AU 772661 B2	06-05-2004
		AU 2004203604 A1	02-09-2004
		CA 2342107 A1	02-03-2000
		DE 69935074 T2	15-11-2007
		EP 1107714 A1	20-06-2001
		EP 1808151 A2	18-07-2007
		EP 2260802 A2	15-12-2010
		ES 2588389 T3	02-11-2016
		JP 4738595 B2	03-08-2011
		JP 5153804 B2	27-02-2013
		JP 2002523138 A	30-07-2002
		JP 2010158531 A	22-07-2010
		US 6620188 B1	16-09-2003
		US 2001005791 A1	28-06-2001
		US 2001047196 A1	29-11-2001
		US 2004147987 A1	29-07-2004
		US 2007233212 A1	04-10-2007
		US 2008228141 A1	18-09-2008
US 2011054575 A1	03-03-2011		
US 2011270368 A1	03-11-2011		
US 2011275935 A1	10-11-2011		
US 2012203201 A1	09-08-2012		
US 2012283562 A1	08-11-2012		
US 2015272777 A1	01-10-2015		
WO 0010494 A1	02-03-2000		
US 5476444 A	19-12-1995	AU 3948495 A	26-04-1996
		US 5476444 A	19-12-1995
		WO 9610437 A1	11-04-1996
US 2004158303 A1	12-08-2004	US 2004158303 A1	12-08-2004
		US 2006074469 A1	06-04-2006
US 2003130651 A1	10-07-2003	NONE	
WO 03059218 A1	24-07-2003	AU 2002243488 A1	30-07-2003
		WO 03059218 A1	24-07-2003

EPO FORM P0459

For more details about this annex : see Official Journal of the European Patent Office, No. 12/82

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- US 6419643 B [0004]
- US 6416533 B [0004]
- US 6409747 B [0004]
- US 6405090 B [0004]
- US 6393320 B [0004]
- US 6368304 B [0004]
- US 6338727 B [0004]
- US 6299599 B [0004]
- US 6290717 B [0004]
- US 6287326 B [0004]
- US 6165207 A [0004]
- US 6149670 A [0004]
- US 6146411 A [0004] [0030]
- US 6126684 A [0004]
- US 6306161 B [0004]
- US 6264679 B [0004]
- US 6231594 B [0004]
- US 6149676 A [0004]
- US 6149673 A [0004]
- US 6110168 A [0004]
- US 5989238 A [0004]
- US 5879329 A [0004]
- US 5837003 A [0004]
- US 6383210 B [0004]
- US 6379378 B [0004]
- US 6364899 B [0004]
- US 6325818 B [0004]
- US 6312452 B [0004]
- US 6261312 B [0004]
- US 6254626 B [0004]
- US 6251130 B [0004]
- US 6251129 B [0004]
- US 6245095 B [0004]
- US 6238428 B [0004]
- US 6235048 B [0004]
- US 6231595 B [0004]
- US 6224624 B [0004]
- US 6149677 A [0004]
- US 6096068 A [0004]
- US 6042559 A [0004]
- US 6827728 B [0005]
- US 6818012 B [0005]
- US 6802855 B [0005]
- US 6799063 B [0005]
- US 6764391 B [0005]
- US 6692518 B [0005]
- US 6669715 B [0005]
- US 6660027 B [0005]
- US 6648905 B [0005]
- US 6645232 B [0005]
- US 6620187 B [0005]
- US 6461379 B [0005]
- US 6375674 B [0005]
- US 6197045 B [0005]
- US 6188930 B [0005]
- US 6581403 B [0030]
- US 6529775 B [0030]
- US 94454404 A [0030]