

12

# EUROPEAN PATENT APPLICATION

21 Application number: 84104123.9

51 Int. Cl.<sup>3</sup>: H 04 R 25/00

22 Date of filing: 12.04.84

30 Priority: 28.04.83 US 489653

43 Date of publication of application:  
 14.11.84 Bulletin 84/46

64 Designated Contracting States:  
 CH DE FR GB IT LI NL

71 Applicant: Siemens Aktiengesellschaft  
 Berlin und München Wittelsbacherplatz 2  
 D-8000 München 2(DE)

72 Inventor: Ammitzboll, Knud  
 27 Osborne Avenue  
 New Providence, NJ 07974(US)

54 Resonant peak control.

57 A hearing aid having receiving means, amplifying means and means for delivering the amplified sound to a user's ear, in which an adjustable resonant peak control, such as a variable resistor, is used to tailor the frequency response to reduce feedback without substantial reduction in high frequency amplification or saturation levels.

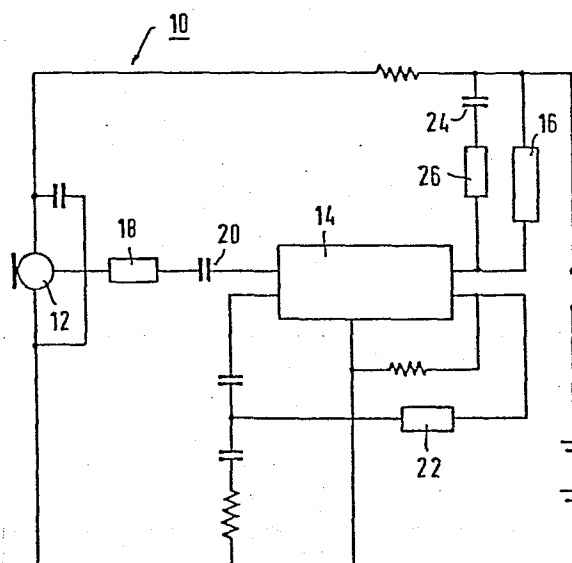


FIG 1

BACKGROUND ON THE INVENTION

This invention relates to a hearing aid in which acoustic feedback is controlled.

5

Acoustic feedback, a common problem in both in-the-ear and behind-the-ear hearing aids, can be eliminated in some users by placement of a capacitor in parallel with the hearing aid amplifier output. However, this does not allow adjustments at the time of fitting the hearing aid and therefore, feedback cannot be eliminated in all users.

10

A high frequency cutoff circuit can be used to eliminate feedback, but it also entirely eliminates the high frequency response of the hearing aid.

15

Accurate ear impressions coupled with precise duplication at the laboratory can provide a precise fit for the hearing aid which is helpful in reducing feedback. However, often the hearing aid must be returned to the laboratory for minor corrections due to inaccuracies in the original impressions or in the duplications.

20

SUMMARY OF THE INVENTION

In general, the invention features, in one aspect, a hearing aid having receiving means for receiving sound, amplifying means, connected to the receiving means, for amplifying sound, and a resonant peak control connected between the receiving and amplifying means, for reducing feedback by varying the amplifying means frequency response.

30

In a particular embodiment, the resonant peak control of the hearing aid allows the frequency response to be tailored to reduce feedback without substantial reduction in high frequency amplification by the amplifying means; the resonant peak control is an R-C circuit; the  
5 R-C circuit is a series R-C circuit having a variable resistor and a capacitor.

In another particular embodiment, the hearing aid has an adjustable vent which can be used to reduce feedback; the adjustable vent and  
10 the resonant peak control are coordinated to reduce feedback.

In another aspect, the invention features a method of reducing feedback in a hearing aid, having the steps of adjusting the volume of the hearing aid to the most comfortable level and tailoring the  
15 frequency response of the hearing aid output to reduce feedback.

In a particular embodiment, the tailoring of the frequency response is accomplished by tuning a series R-C circuit in parallel with a hearing aid output.  
20

This invention is a very significant step in the elimination of acoustic feedback in hearing aids because it allows the hearing aid to be adjusted for the elimination of feedback at the time of fitting.  
25

On the spot adjustments, obtained by varying the resonant peak control, allow the hearing aid to be customized to an individual user without the necessity of returning the aid to the factory or laboratory for adjustments or modifications. This allows accomo-  
30 dation of individual characteristics of a user's ear canal in obtaining the most comfortable level for that particular user.

- 3 -

Adjustment of the resonant peak control flattens out the frequency response and shifts the frequency response curve to a lower frequency range, resulting in almost no loss in high frequency amplification and only a minimal change in saturation levels.

5

Therefore, this hearing aid provides the advantage of being adjustable at the time of fitting without any significant sacrifice in operational characteristics.

10 Other features and advantages of the invention will be apparent from the following detailed description, and from the claims.

For a full understanding of the present invention, reference should now be made to the following detailed description and to the  
15 accompanying drawings.

BRIEF DESCRIPTION OF THE DRAWINGS

Fig. 1 is a diagrammatic view of the hearing aid circuitry.

5 Fig. 2 shows the boundaries of the frequency response curve due to adjustment of the resonant peak control.

Fig. 3 shows the boundaries of the saturation sound pressure level curve due to adjustment of the resonant peak control.

10

DETAILED DESCRIPTION

Referring to the drawings, an embodiment of the invention will now be described in detail.

15

Hearing aid 10, designed to be mounted in the user's ear, has microphone 12 for picking up external sounds, integrated circuit 14, typically an LTI 505 integrated circuit, for amplifying external sound, and receiver 16, typically a Knowles Electronics 1913 receiver for imparting the amplified sound to the user.

20

Microphone 12, is connected to integrated circuit 14 by gain control 18, which can be a potentiometer in series with capacitor 20, for adjusting the gain of the microphone.

25

Volume control 22, which can also be a potentiometer, allows variable adjustment of the amplified audio output of integrated circuit 14.

30

Receiver 16, connected in parallel with integrated circuit 14, is also connected in parallel with a series R-C circuit which includes capacitor 24 and resonant peak control (RPC) 26.

The resonant peak control is a variable potentiometer which when adjusted acts in conjunction with capacitor 24 and the inductance of receiver 16 to tailor the frequency response of the amplifier (integrated circuit 14) to reduce instability due to feedback.

5

Referring to Fig. 2, frequency response curves A and B show the two extreme conditions between which the frequency response can be tailored by adjusting the resonant peak control.

10

The adjustment of the resonant peak control varies its electrical output which tunes or tailors the frequency response resulting in shifting and flattening of the peaks of the frequency response curve which reduces feedback with only a slight reduction in high

15

frequency amplification and only a minimal change in the saturation curve.

Referring to Fig. 3, curves C and D show the limits of the change in the saturation curve due to adjustment of the resonant peak control.

20

In actual use the slight reduction in high frequency amplification is not detectable because the improved flatness of the frequency response permits a higher gain to be utilized.

25

In actual operation the hearing aid is inserted in the user's ear and volume control 22, is adjusted to the most comfortable level for the particular user. In the event feedback occurs prior to reaching the most comfortable level, resonant peak control 26 is adjusted until feedback is eliminated. Then, if required volume control 22 can be further increased to again reach the most comfortable level.

30

The sequence of maximizing the volume control to the most comfortable level followed by adjustment of the resonant peak control is repeated until the most comfortable level for the user is attained without the existence of any feedback.

-6-

Siemens Custom In-The-Ear Hearing Aid 007, sold by Siemens Hearing Instruments, Inc., 685 Liberty Avenue, Union, New Jersey, incorporates the inventive concept described in this application.

- 5 In an alternative embodiment the size of the hearing aid vent opening can be changed to effect a change in amplifier instability (integrated circuit 14) due to feedback.

- 10 This modification of the opening is especially useful when a maximum resonant peak control adjustment is reached and feedback still occurs.

- 15 There has thus been shown and described a novel method and apparatus for reducing acoustical feedback in hearing aids which fulfills all the objects and advantages sought therefor. Many changes, modifications, variations and other uses and application of the subject will, however, become apparent to those skilled in the art after considering the specification and the accompanying drawings which disclose embodiments thereof. All such changes,  
20 modifications, variations and other uses and applications which do not depart from the spirit and scope of the invention are deemed to be covered by the invention which is limited only by the claims which follow.

CLAIMS

What is Claimed is:

- 1 1. A hearing aid, comprising:
  - 2
  - 3 a) receiving means for receiving sound;
  - 4
  - 5 b) amplifying means, connected to said receiving means, for
  - 6 amplifying said sound; and
  - 7
  - 8 c) a resonant peak control connected between said receiving and
  - 9 said amplifying means, for reducing feedback by varying said
  - 10 amplifying means frequency response.
- 1 2. The hearing aid of claim 1, wherein said resonant peak control
- 2 allows said frequency response to be tailored to reduce feedback
- 3 without substantial reduction in high frequency amplification by
- 4 said amplifying means.
- 1 3. The hearing aid in claim 1, wherein said resonant peak control
- 2 comprises an R-C circuit.
- 1 4. The hearing aid of claim 3, wherein said R-C circuit is a series
- 2 R-C circuit comprising a variable resistor and a capacitor.
- 1 5. The hearing aid of claim 1, wherein an adjustable vent can be
- 2 used to reduce feedback.
- 1 6. The hearing aid of claim 5, wherein said adjustable vent and
- 2 said resonant peak control are coordinated to reduce feedback.

1 7. The method of reducing feedback in a hearing aid, comprising the  
2 steps of:

3

4 a) adjusting the volume of said hearing aid to a most  
5 comfortable level; and

6

7 b) tailoring the frequency response of said hearing aid output  
8 to reduce feedback.

1 8. The method of claim 7, wherein said tailoring is accomplished by  
2 tuning a series R-C circuit in parallel with said hearing aid output.

1/1

83 P 7413

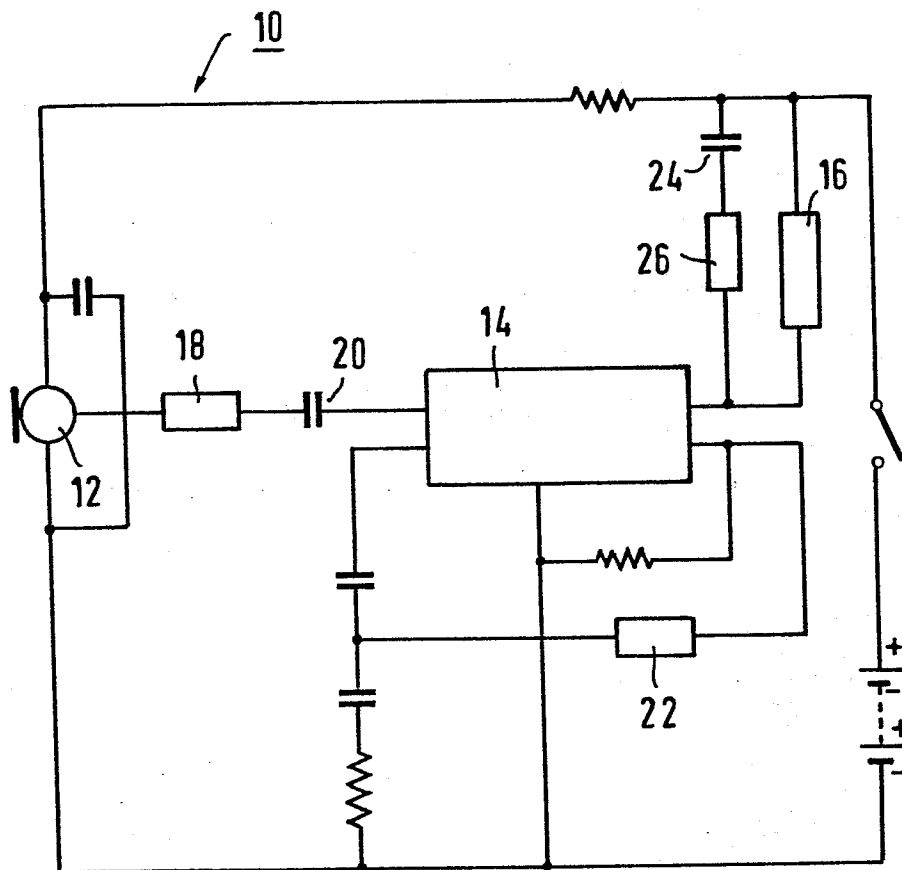


FIG 1

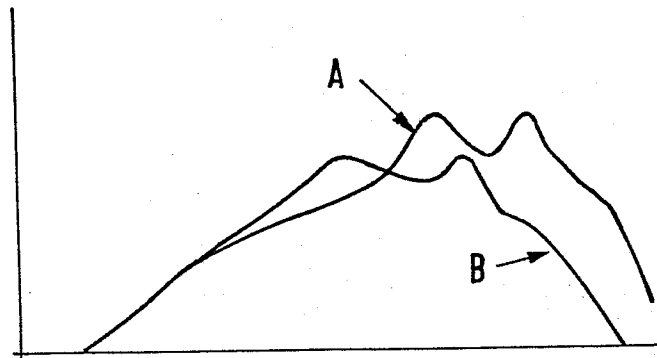


FIG 2

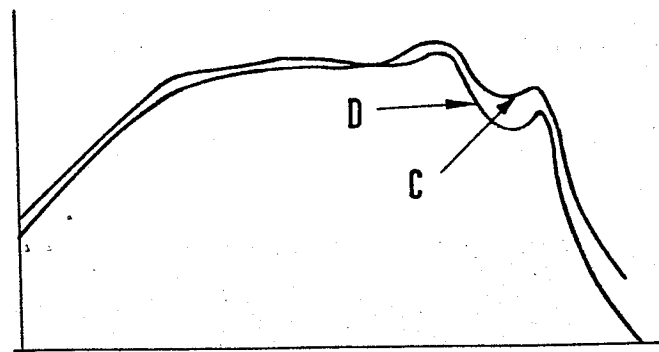


FIG 3



DOCUMENTS CONSIDERED TO BE RELEVANT			
Category	Citation of document with indication, where appropriate, of relevant passages	Relevant to claim	CLASSIFICATION OF THE APPLICATION (Int. Cl. 3)
X	CH-A- 474 200 (A.G. FÜR ELEKTROAKUSTIK) * Column 1, lines 1-22; column 3, lines 1-28 *	1-4	H 04 R 25/00
Y		5-8	
Y	US-A-3 368 644 (HENDERSON) * Column 1, lines 15-31; column 2, line 15 - column 3, line 15 *	5-8	
			TECHNICAL FIELDS SEARCHED (Int. Cl. 3)
			H 04 R
The present search report has been drawn up for all claims			
Place of search THE HAGUE		Date of completion of the search 20-07-1984	Examiner GERLING J.C.J.
<b>CATEGORY OF CITED DOCUMENTS</b>			
X : particularly relevant if taken alone Y : particularly relevant if combined with another document of the same category A : technological background O : non-written disclosure P : intermediate document		T : theory or principle underlying the invention E : earlier patent document, but published on, or after the filing date D : document cited in the application L : document cited for other reasons & : member of the same patent family, corresponding document	