



(11) **EP 1 185 215 B9**

(12) **CORRECTED EUROPEAN PATENT SPECIFICATION**

Note: Bibliography reflects the latest situation

(15) Correction information:
Corrected version no 1 (W1 B1)
Corrections, see page(s) 18

(48) Corrigendum issued on:
13.06.2007 Bulletin 2007/24

(45) Date of publication and mention
of the grant of the patent:
04.04.2007 Bulletin 2007/14

(21) Application number: **00932419.5**

(22) Date of filing: **12.05.2000**

(51) Int Cl.:
A61F 2/06 (2006.01)

(86) International application number:
PCT/US2000/013244

(87) International publication number:
WO 2000/071054 (30.11.2000 Gazette 2000/48)

(54) **EXPANDABLE MEDICAL STENT WITH DUCTILE HINGES**

AUSWEITBARER MEDIZINISCHER STENT MIT DUKTILEN GELENKEN

STENT EXTENSIBLE ARTICULATIONS DUCTILES

(84) Designated Contracting States:
**AT BE CH CY DE DK ES FI FR GB GR IE IT LI LU
MC NL PT SE**

(30) Priority: **20.05.1999 US 315892**

(43) Date of publication of application:
13.03.2002 Bulletin 2002/11

(60) Divisional application:
07006868.9
07006999.2

(73) Proprietors:
• **Conor Medsystems, Inc.**
Menlo Park, CA 94025 (US)
• **Shanley, John F.**
Redwood City CA 94061 (US)

(72) Inventor: **SHANLEY, John, F.**
Redwood City, CA 94061 (US)

(74) Representative: **Diehl, Hermann O. Th. et al**
Diehl & Partner
Augustenstrasse 46
80333 München (DE)

(56) References cited:
WO-A-96/29028 **WO-A-99/15108**
WO-A-99/49928 **FR-A- 2 764 794**

Note: Within nine months from the publication of the mention of the grant of the European patent, any person may give notice to the European Patent Office of opposition to the European patent granted. Notice of opposition shall be filed in a written reasoned statement. It shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

EP 1 185 215 B9

Description**BACKGROUND OF THE INVENTION****1. Field of the Invention**

[0001] The present invention relates to tissue-supporting medical devices, and more particularly to expandable, non-removable devices that are implanted within a bodily lumen of a living animal or human to support the organ and maintain patency.

2. Summary of the Related Art

[0002] In the past, permanent or biodegradable devices have been developed for implantation within a body passageway to maintain patency of the passageway. These devices are typically introduced percutaneously, and transported transluminally until positioned at a desired location. These devices are then expanded either mechanically, such as by the expansion of a mandrel or balloon positioned inside the device, or expand themselves by releasing stored energy upon actuation within the body. Once expanded within the lumen, these devices, called stents, become encapsulated within the body tissue and remain a permanent implant.

[0003] Known stent designs include monofilament wire coil stents (U.S. Pat. No. 4,969,458); welded metal cages (U.S. Pat. Nos. 4,733,665 and 4,776,337); and, most prominently, thin-walled metal cylinders with axial slots formed around the circumference (U.S. Pat. Nos. 4,733,665, 4,739,762, and 4,776,337). Known construction materials for use in stents include polymers, organic fabrics and biocompatible metals, such as, stainless steel, gold, silver, tantalum, titanium, and shape memory alloys such as Nitinol.

[0004] U.S. Pat. Nos. 4,733,665, 4,739,762, and 4,776,337 disclose expandable and deformable interluminal vascular grafts in the form of thin-walled tubular members with axial slots allowing the members to be expanded radially outwardly into contact with a body passageway. After insertion, the tubular members are mechanically expanded beyond their elastic limit and thus permanently fixed within the body. The force required to expand these tubular stents is proportional to the thickness of the wall material in a radial direction. To keep expansion forces within acceptable levels for use within the body (e.g., 5 - 10 atm), these designs must use very thin-walled materials (e.g., stainless steel tubing with 0.0025 inch thick walls). However, materials this thin are not visible on conventional fluoroscopic and x-ray equipment and it is therefore difficult to place the stents accurately or to find and retrieve stents that subsequently become dislodged and lost in the circulatory system.

[0005] Further, many of these thin-walled tubular stent designs employ networks of long, slender struts whose width in a circumferential direction is two or more times greater than their thickness in a radial direction. When expanded, these struts are frequently unstable, that is, they display a tendency to buckle, with individual struts twisting out of plane. Excessive protrusion of these twisted struts into the bloodstream has been observed to increase turbulence, and thus encourage thrombosis. Additional procedures have often been required to attempt to correct this problem of buckled struts. For example, after initial stent implantation is determined to have caused buckling of struts, a second, high-pressure balloon (e.g., 12 to 18 atm) would be used to attempt to drive the twisted struts further into the lumen wall. These secondary procedures can be dangerous to the patient due to the risk of collateral damage to the lumen wall.

[0006] Many of the known stents display a large elastic recovery, known in the field as "recoil," after expansion inside a lumen. Large recoil necessitates over-expansion of the stent during implantation to achieve the desired final diameter. Over-expansion is potentially destructive to the lumen tissue. Known stents of the type described above experience recoil of up to about 6 to 12 % from maximum expansion.

[0007] Large recoil also makes it very difficult to securely crimp most known stents onto delivery catheter balloons. As a result, slippage of stents on balloons during interluminal transportation, final positioning, and implantation has been an ongoing problem. Many ancillary stent securing devices and techniques have been advanced to attempt to compensate for this basic design problem. Some of the stent securing devices include collars and sleeves used to secure the stent onto the balloon.

[0008] Another problem with known stent designs is non-uniformity in the geometry of the expanded stent. Non-uniform expansion can lead to non-uniform coverage of the lumen wall creating gaps in coverage and inadequate lumen support. Further, over expansion in some regions or cells of the stent can lead to excessive material strain and even failure of stent features. This problem is potentially worse in low expansion force stents having smaller feature widths and thicknesses in which manufacturing variations become proportionately more significant. In addition, a typical delivery catheter for use in expanding a stent includes a balloon folded into a compact shape for catheter insertion. The balloon is expanded by fluid pressure to unfold the balloon and deploy the stent. This process of unfolding the balloon causes uneven stresses to be applied to the stent during expansion of the balloon due to the folds causing the problem non-uniform stent expansion.

[0009] U.S. Pat. No. 5,545,210 discloses a thin-walled tubular stent geometrically similar to those discussed above,

but constructed of a nickel-titanium shape memory alloy ("Nitinol"). This design permits the use of cylinders with thicker walls by making use of the lower yield stress and lower elastic modulus of martensitic phase Nitinol alloys. The expansion force required to expand a Nitinol stent is less than that of comparable thickness stainless steel stents of a conventional design. However, the "recoil" problem after expansion is significantly greater with Nitinol than with other materials. For example, recoil of a typical design Nitinol stent is about 9%. Nitinol is also more expensive, and more difficult to fabricate and machine than other stent materials, such as stainless steel.

[0010] All of the above stents share a critical design property: in each design, the features that undergo permanent deformation during stent expansion are prismatic, i.e., the cross sections of these features remain constant or change very gradually along their entire active length. To a first approximation, such features deform under transverse stress as simple beams with fixed or guided ends: essentially, the features act as a leaf springs. These leaf spring like structures are ideally suited to providing large amounts of elastic deformation before permanent deformation commences. This is exactly the opposite of ideal stent behavior. Further, the force required to deflect prismatic stent struts in the circumferential direction during stent expansion is proportional to the square of the width of the strut in the circumferential direction. Expansion forces thus increase rapidly with strut width in the above stent designs. Typical expansion pressures required to expand known stents are between about 5 and 10 atmospheres. These forces can cause substantial damage to tissue if misapplied.

[0011] FIG. 1 shows a typical prior art "expanding cage" stent design. The stent 10 includes a series of axial slots 12 formed in a cylindrical tube 14. Each axial row of slots 12 is displaced axially from the adjacent row by approximately half the slot length providing a staggered slot arrangement. The material between the slots 12 forms a network of axial struts 16 joined by short circumferential links 18. The cross section of each strut 16 remains constant or varies gradually along the entire length of the strut and thus the rectangular moment of inertia and the elastic and plastic section moduli of the cross section also remain constant or vary gradually along the length of the strut. Such a strut 16 is commonly referred to as a prismatic beam. Struts 16 in this type of design are typically 0.127-0.1524 mm (0.005 to 0.006 inches) wide in the circumferential direction. Strut thicknesses in the radial direction are typically about 0.0635 mm (0.0025 inches) or less to keep expansion forces within acceptable levels. However, most stent materials must be approximately 0.127 mm (0.005 inches) thick for good visibility on conventional fluoroscopic equipment. This high ratio of strut width to thickness, combined with the relatively high strut length and the initial curvature of the stent tubing combine to cause the instability and buckling often seen in this type of stent design. When expanded, the stent structure of FIG. 1 assumes the roughly diamond pattern commonly seen in expanded sheet metal.

[0012] Another stent described in PCT publication number WO 96/29028 uses struts with relatively weak portions of locally-reduced cross sections which on expansion of the stent act to concentrate deformation at these areas. However, as discussed above non-uniform expansion is even more of a problem when smaller feature widths and thicknesses are involved because manufacturing variations become proportionately more significant. The locally-reduced cross section portions described in this document are formed by pairs of circular holes. The shape of the locally-reduced cross section portions undesirably concentrates the plastic strain at the narrowest portion. This concentration of plastic strain without any provision for controlling the level of plastic strain makes the stent highly vulnerable to failure.

[0013] In view of the drawbacks of the prior art stents, it would be advantageous to be able to expand a stent with an expansion force at a low level independent of choice of stent materials, material thickness, or strut dimensions.

[0014] It would further be advantageous to have a tissue-supporting device that permits a choice of material thickness that could be viewed easily on conventional fluoroscopic equipment for any material.

[0015] It would also be advantageous to have a tissue-supporting device that is inherently stable during expansion, thus eliminating buckling and twisting of structural features during stent deployment.

[0016] It would also be desirable to control strain to a desired level which takes advantage of work hardening without approaching a level of plastic strain at which failure may occur.

[0017] In addition, it would be advantageous to have a tissue-supporting device with minimal elastic recovery, or "recoil" of the device after expansion.

[0018] It would be advantageous to have a tissue supporting device that can be securely crimped to the delivery catheter without requiring special tools, techniques, or ancillary clamping features.

[0019] It would further be advantageous to have a tissue-supporting device that has improved resistance to compressive forces (improved crush strength) after expansion.

[0020] It would also be advantageous to have a tissue-supporting device that achieves all the above improvements with minimal foreshortening of the overall stent length during expansion.

[0021] Finally, it would also be advantageous to provide a tissue-supporting device which is differentially expandable and/or which has framed hole features for accommodating bifurcations.

SUMMARY OF THE INVENTION

[0022] The present invention addresses several important problems in expandable medical device design including:

high expansion force requirements; lack of radio-opacity in thin-walled stents; buckling and twisting of stent features during expansion; poor crimping properties; and excessive elastic recovery ("recoil") after implantation. The invention also provides benefits of improved resistance to compressive forces after expansion, control of the level of plastic strain, and low axial shortening during expansion. Some embodiments of the invention also provide improved uniformity of expansion by limiting a maximum geometric deflection between struts. Other embodiments of the invention include segments of the expandable device which may be expanded in a specified sequence and/or framed hole features for accommodating bifurcations.

[0023] The invention involves the incorporation of stress/strain concentration features or "ductile hinges" at selected points in the body of an expandable cylindrical medical device. When expansion forces are applied to the device as a whole, these ductile hinges concentrate expansion stresses and strains in small, well-defined areas while limiting strut deflection and plastic strain to specified levels.

[0024] In accordance with one aspect of the present invention, an expandable medical device includes a plurality of elongated beams and a plurality of ductile hinges connecting the plurality of beams together in a radially expandable substantially cylindrical device. The plurality of elongated beams have a beam width in a circumferential direction. The ductile hinges have a width in a circumferential direction along a portion of a hinge length which is smaller than the beam width such that as the device is expanded the ductile hinges experience plastic deformation while the beams are not plastically deformed. A first section of the substantially cylindrical device includes ductile hinges having a first width and a second section of the substantially cylindrical device includes ductile hinges having a second width different from the first width such that the first section expands before the second section.

[0025] In accordance with a further aspect of the invention, an expandable medical device includes a plurality of elongated beams and a plurality of ductile hinges connecting the plurality of beams together in a radially expandable substantially cylindrical device. The plurality of elongated beams are joined together in a regular pattern to form the substantially cylindrical device. The plurality of elongated beams have a beam width in a circumferential direction and the ductile hinges have a width in a circumferential direction along a portion of a hinge length which is smaller than the beam width such that as the device is expanded the ductile hinges experience plastic deformation while the beams are not plastically deformed. A hole feature interrupts the regular pattern of the plurality of beams, the hole feature accommodating a bifurcation in a vessel.

[0026] In accordance with another aspect of the present invention, a method of expanding a medical device includes the steps of:

providing a substantially cylindrical expandable medical device having a first section with ductile hinges of a first configuration and a second section with ductile hinges of a second configuration which requires a different force for expansion than the first configuration; and
expanding the device in a controlled expansion sequence with an expandable member.

BRIEF DESCRIPTION OF THE DRAWINGS

[0027] The invention will now be described in greater detail with reference to the preferred embodiments illustrated in the accompanying drawings, in which like elements bear like reference numerals, and wherein:

FIG. 1 is an isometric view of a prior art tissue-supporting device;
FIG. 2 is an isometric view of a tissue-supporting device in accordance with one embodiment of the invention;
FIGS. 3a-d are perspective views of ductile hinges according to several variations of the invention;
FIG. 3e is a side view of another embodiment of a ductile hinge;
FIGS. 4a and 4b are an isometric view and an enlarged side view of a tissue-supporting device in accordance with an alternative embodiment of the invention;
FIGS. 5a-5c are perspective, side, and cross-sectional views of an idealized ductile hinge for purposes of analysis;
FIG. 5d is a stress/strain curve for the idealized ductile hinge;
FIGS. 6 is a perspective view of a simple beam for purposes of calculation;
FIG. 7 is a moment verses curvature graph for a rectangular beam;
FIG. 8 is an enlarged side view of a bent ductile hinge;
FIGS. 9a and 9b are enlarged side views of ductile hinges in initial and expanded positions with shortened struts to illustrate axial contraction relationships; and
FIG. 10 is a side view of a portion of an alternative embodiment of a tissue supporting device having a high-crush-strength and low-recoil;
FIGS. 11a-11c are schematic side views of unexpanded, partially expanded, and fully expanded views of a differentially expanding tissue supporting device;
FIG. 12a is an unexpanded side view of a cylindrical tissue supporting device with a side hole feature, which has

been laid flat for ease of illustration; and

FIGS. 12b and 12c are unexpanded and expanded schematic side views of the tissue supporting device of FIG. 12a.

DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENTS

[0028] FIG. 2 shows one embodiment of an expandable tissue supporting device 20 in accordance with the present invention. The tissue supporting device 20 includes a series of axial slots 22 formed in a cylindrical tube 24. Each axial slot 22 is displaced axially from the slots in adjacent rows of slots by approximately half the slot length resulting in a staggered slot arrangement. The offset between adjacent rows of slots results in alternate rows of slots which extend to the ends of the cylindrical tube 24. At each interior end of each of the axial slots 22 a circumferential slot 26 is formed. The material between the slots 22 forms a network of axial struts 28 extending substantially parallel to an axis of the tube 24. The axial struts 28 are joined by short circumferential links 30. The circumferential links 30 are positioned at both the interior of the cylindrical tube and at the ends of the cylindrical tube. The cross section (and rectangular moment of inertia) of each of the struts 28 is not constant along the length of the strut. Rather, the strut cross section changes abruptly at both ends of each strut 28 at the location of the circumferential slots 26. The struts 28 are thus not prismatic. Each individual strut 28 is linked to the rest of the structure through a pair of reduced sections 32, one at each end, which act as stress/strain concentration features. The reduced sections 32 of the struts function as hinges in the cylindrical structure. Since the stress/strain concentration features 32 are designed to operate into the plastic deformation range of generally ductile materials, they are referred to as ductile hinges. Such features are also commonly referred to as "Notch Hinges" or "Notch Springs" in ultra-precision mechanism design, where they are used exclusively in the elastic range.

[0029] With reference to the drawings and the discussion, the *width* of any feature is defined as its dimension in the circumferential direction of the cylinder. The *length* of any feature is defined as its dimension in the axial direction of the cylinder. The *thickness* of any feature is defined as the wall thickness of the cylinder.

[0030] The presence of the ductile hinges 32 allows all of the remaining features in the tissue supporting device to be increased in width or the circumferentially oriented component of their respective rectangular moments of inertia - thus greatly increasing the strength and rigidity of these features. The net result is that elastic, and then plastic deformation commence and propagate in the ductile hinges 32 before other structural elements of the device undergo any significant elastic deformation. The force required to expand the tissue supporting device 20 becomes a function of the geometry of the ductile hinges 32, rather than the device structure as a whole, and arbitrarily small expansion forces can be specified by changing hinge geometry for virtually any material wall thickness. In particular, wall thicknesses great enough to be visible on a fluoroscope can be chosen for any material of interest.

[0031] In order to get minimum recoil, the ductile hinges 32 should be designed to operate well into the plastic range of the material, and relatively high local strain-curvatures are developed. When these conditions apply, elastic curvature is a very small fraction of plastic or total curvature, and thus when expansion forces are relaxed, the percent change in hinge curvature is very small. When incorporated into a strut network designed to take maximum advantage of this effect, the elastic springback, or "recoil," of the overall stent structure is minimized.

[0032] In the embodiment of FIG. 2, it is desirable to increase the width of the individual struts 28 between the ductile hinges 32 to the maximum width that is geometrically possible for a given diameter and a given number of struts arrayed around that diameter. The only geometric limitation on strut width is the minimum practical width of the slots 22 which is about 0.0508 mm (0.002 inches) for laser machining. Lateral stiffness of the struts 28 increases as the cube of strut width, so that relatively small increases in strut width significantly increase strut stiffness. The net result of inserting ductile hinges 32 and increasing strut width is that the struts 28 no longer act as flexible leaf springs, but act as essentially rigid beams between the ductile hinges. All radial expansion or compression of the cylindrical tissue supporting device 20 is accommodated by mechanical strain in the hinge features 32, and yield in the hinge commences at very small overall radial expansion or compression.

[0033] Yield in ductile hinges at very low gross radial deflections also provides the superior crimping properties displayed by the ductile hinge-based designs. When a tissue supporting device is crimped onto a folded catheter balloon, very little radial compression of the device is possible since the initial fit between balloon and device is already snug. Most stents simply rebound elastically after such compression, resulting in very low clamping forces and the attendant tendency for the stent to slip on the balloon. Ductile hinges, however, sustain significant plastic deformation even at the low deflections occurring during crimping onto the balloon, and therefore a device employing ductile hinges displays much higher clamping forces. The ductile hinge designs according to the present invention may be securely crimped onto a balloon of a delivery catheter by hand or by machine without the need for auxiliary retaining devices commonly used to hold known stents in place.

[0034] The geometric details of the stress/strain concentration features or ductile hinges 32 can be varied greatly to tailor the exact mechanical expansion properties to those required in a specific application. The most obvious and straightforward ductile hinges are formed by slots or notches with rounded roots, as in FIGS. 3a and 3c. Since the laser

beams often used to fabricate these features are themselves round, slots or notches with circular roots are also among the easiest to fabricate.

[0035] FIG. 3a shows a ductile hinge 36 formed by a pair of opposed circular grooves 38, 40. According to this embodiment the circumferential slot 26 has semicircular ends 38 having a radius of curvature r . Outer semicircular grooves 40 opposed the semicircular ends 38 and also have a radius of curvature r . FIG. 3c shows another ductile hinge 54 formed by a parabolic groove 56.

[0036] Generally, the ductile hinges 36 of the embodiment of FIG. 3a formed between pairs of concave curves 38, 40 have a minimum width along a line connecting their respective centers of curvature. When the struts connected by the ductile hinge are moved apart or together, plastic deformation is highly concentrated in a region immediately adjacent to the plane that bisects the hinge at this narrow point.

[0037] For smaller deflection, this very high strain concentration at the bisecting plane is acceptable, and in some cases, useful. For stent crimping purposed, for example, it is desirable to generate relatively large plastic deformations at very small deflection angles.

[0038] As a practical matter, however, strut deflection angles for device *expansion* are often in the 25° to 45° range. At these angles, strain at the root or bisecting plane of concave ductile hinge features can easily exceed the 50 to 60% elongation-to-failure of 316L stainless steel, one of the most ductile stent materials. Deflection limiting features which will be described further below limit the *geometric* deflection of struts, but these features do not in themselves affect the propagation pattern of plastic deformation in a given ductile hinge design. For concave ductile hinges at large bend angles, very high strain concentrations remain. Scanning electron micrographs have confirmed this analysis.

[0039] In many engineering applications, it is desirable to limit the amount of strain, or "cold-work," in a material to a specified level in order to optimize material properties and to assure safe operation. For example, in medical applications it is desirable to limit the amount of cold-work in 316L stainless steel to about 30%. At this level, the strength of the material is increased, while the material strain is still well below the failure range. Ideally, therefore, a safe and effective ductile hinge should not simply limit gross deflection, but reliably limit *material strain* to a specified level.

[0040] FIG. 3b shows a simple ductile hinge design that allows material strain to be limited to some specified level. The ductile hinge of FIG. 3b is formed by a rectangular circumferential groove 46 with filleted corners 48 on one side of a strut, the opposite side 50 of the strut remaining straight. The ductile hinges 44 are substantially rectangular sections between the ends of the groove 46 and the side walls 50.

[0041] One of the key concepts in FIG. 3b is that the ductile hinge 44 has a constant or substantially constant width along at least a portion of its total length. In this configuration, there is no local minimum width along the ductile hinge axis, as there is with pairs of concave roots. There is therefore no point concentration of stresses and strains along the length of the ductile hinge beam during stent expansion. In particular, maximum tensile and compressive strains will be distributed evenly along the upper and lower surfaces of the hinge 44 during stent expansion. With the gross bend angle limited by mechanical stops, which are described below in detail, the maximum *material strain* (at the hinge surfaces) can therefore be reliably limited by adjusting the initial length of the ductile hinge over which the total elongation is distributed.

[0042] FIG. 3d shows a ductile hinge 60 in a cylindrical wire 62 for incorporating into a wire-form tissue-supporting device. The ductile hinge 60 is formed by a reduced diameter portion of the wire 62. Again, it is important that the ductile hinge have a substantially constant width over a portion of its length in order to provide strain control. Preferably, the ductile hinge is prismatic over a portion of its length. Maximum material strain can be varied by adjusting the hinge length. The ductile hinges of the present invention have a constant or substantially constant width over at least 1/3 of the ductile hinge length, and preferably over at least 1/2 of the ductile hinge length.

[0043] FIG. 3e shows an asymmetric ductile hinge 63 that produces different strain versus deflection-angle functions in expansion and compression. Each of the ductile hinges 64 is formed between a convex surface 68 and a concave surface 69. The ductile hinge 64 according to a preferred embodiment essentially takes the form of a small, prismatic curved beam having a substantially constant cross section. However, a thickness of the curved ductile hinge 64 may vary somewhat as long as the ductile hinge width remains constant along a portion of the hinge length. The width of the curved beam is measured along the radius of curvature of the beam. This small curved beam is oriented such that the smaller *concave* surface 69 is placed in tension in the device *crimping* direction, while the larger *convex* surface 68 of the ductile hinges is placed in tension in the device *expansion* direction. Again, there is no local minimum width of the ductile hinge 64 along the (curved) ductile hinge axis, and no concentration of material strain. During device expansion tensile strain will be distributed along the convex surface 68 of the hinge 64 and maximum expansion will be limited by the angle of the walls of the concave notch 69 which provide a geometric deflection limiting feature. Maximum tensile strain can therefore be reliably limited by adjusting the initial length of the convex arc shaped ductile hinge 64 over which the total elongation is distributed.

[0044] The ductile hinges illustrated in FIGS. 3a-e are examples of different structures that will function as a stress/strain concentrator. Many other stress/strain concentrator configurations may also be used as the ductile hinges in the present invention. The ductile hinges according to the present invention generally include an abrupt change in width of

a strut that functions to concentrate stresses and strains in the narrower section of the strut. These ductile hinges also generally include features to limit mechanical deflection of attached struts and features to control material strain during large strut deflections. Although the ductile hinges have been illustrated in FIG. 2 as positioned at the ends of each of the axial slots 22, they may also be positioned at other locations in other designs without departing from the present invention.

[0045] An alternative embodiment of a tissue supporting device 80 is illustrated in FIG. 4a. and in the enlarged side view of FIG. 4b. The tissue supporting device 80 includes a plurality of cylindrical tubes 82 connected by S-shaped bridging elements 84. The bridging elements 84 allow the tissue supporting device to bend axially when passing through the tortuous path of the vasculature to the deployment site and allow the device to bend when necessary to match the curvature of a lumen to be supported. The S-shaped bridging elements 84 provide improved axial flexibility over prior art devices due to the thickness of the elements in the radial direction which allows the width of the elements to be relatively small without sacrificing radial strength. For example, the width of the bridging elements 84 may be about 0.0305 - 0.0330 mm (0.0012 - 0.00013 inches). Each of the cylindrical tubes 82 has a plurality of axial slots 86 extending from an end surface of the cylindrical tube toward an opposite end surface. A plurality of axial struts 88 having ductile hinges 90 are formed between the axial slots 86. The ductile hinges 90 are formed by circumferential slots 92 formed at the interior ends of the axial slots 86 and opposed notches 94.

[0046] The notches 94 each have two opposed angled walls 96 which function as a stop to limit geometric deflection of the ductile hinge, and thus limit maximum device expansion. As the cylindrical tubes 82 are expanded and bending occurs at the ductile hinges 90, the angled side walls 96 of the notches 94 move toward each other. Once the opposite side walls 96 of a notch come into contact with each other, they resist further expansion of the particular ductile hinge causing further expansion to occur at other sections of the tissue supporting device. This geometric deflection limiting feature is particularly useful where uneven expansion is caused by either variations in the tissue supporting device 80 due to manufacturing tolerances or uneven balloon expansion.

[0047] The tissue supporting device 20, 80 according to the present invention may be formed of any ductile material, such as steel, gold, silver, tantalum, titanium, Nitinol, other shape memory alloys, other metals, or even some plastics. One preferred method for making the tissue supporting device 20, 80 involves forming a cylindrical tube and then laser cutting the slots 22, 26, 86, 92 and notches 94 into the tube. Alternatively, the tissue supporting device may be formed by electromachining, chemical etching followed by rolling and welding, or any other known method.

[0048] The design and analysis of stress/strain concentration for ductile hinges, and stress/strain concentration features in general, is complex. For example, the stress concentration factor for the simplified ductile hinge geometry of FIG. 3a can be calculated and is given by the following expression where D is the width of the struts 28, h is the height of the circular grooves 38, 40, and r is the radius of curvature of the grooves. For purposes of this example the ratio of h/r is taken to be 4. However, other ratios of h/r can also be implemented successfully.

$$K = 4.935 - 7.586 \left(\frac{2h}{D} \right) + 0.515 \left(\frac{2h}{D} \right)^2 + 0.432 \left(\frac{2h}{D} \right)^3$$

[0049] The stress concentration factors are generally useful only in the linear elastic range. Stress concentration patterns for a number of other geometries can be determined through photoelastic measurements and other experimental methods. Stent designs based on the use of stress/strain concentration features, or ductile hinges, generally involve more complex hinge geometries and operate in the non-linear elastic and plastic deformation regimes.

[0050] The general nature of the relationship among applied forces, material properties, and ductile hinge geometry can be more easily understood through analysis of an idealized hinge 66 as shown in FIGS. 5a-5c. The hinge 66 is a simple beam of rectangular cross section having a width h, length L and thickness b. The idealized hinge 66 has elastic-ideally-plastic material properties which are characterized by the ideal stress/strain curve of FIG. 5d. It can be shown that the "plastic" or "ultimate bending moment" for such a beam is given by the expression:

$$M_p \equiv M_{ult} = \delta_{yp} \frac{bh^2}{4}$$

Where b corresponds to the cylindrical tube wall thickness, h is the circumferential width of the ductile hinge, and δ_{yp} is the yield stress of the hinge material. Assuming only that expansion pressure is proportional to the plastic moment, it can be seen that the required expansion pressure to expand the tissue supporting device increases *linearly* with wall thickness b and as the *square* of ductile hinge width h . It is thus possible to compensate for relatively large changes in wall thickness b with relatively small changes in hinge width h . While the above idealized case is only approximate, empirical measurements of expansion forces for different hinge widths in several different ductile hinge geometries have confirmed the general form of this relationship. Accordingly, for different ductile hinge geometries it is possible to increase the thickness of the tissue supporting device to achieve radiopacity while compensating for the increased thickness with a much smaller decrease in hinge width.

[0051] Ideally, the stent wall thickness b should be as thin as possible while still providing good visibility on a fluoroscope. For most stent materials, including stainless steel, this would suggest a thickness of about 0.127 - 0.178 mm (0.005 - 0.007 inches) or greater. The inclusion of ductile hinges in a stent design can lower expansion forces/pressures to very low levels for any material thickness of interest. Thus ductile hinges allow the construction of optimal wall thickness tissue supporting devices at expansion force levels significantly lower than current non-visible designs.

[0052] The expansion forces required to expand the tissue supporting device 20 according to the present invention from an initial condition illustrated in FIG. 2 to an expanded condition is between 1 and 5 atmospheres, preferably between 2 and 3 atmospheres. The expansion may be performed in a known manner, such as by inflation of a balloon or by a mandrel. The tissue supporting device 20 in the expanded condition has a diameter which is preferably up to three times the diameter of the device in the initial unexpanded condition.

[0053] Many tissue supporting devices fashioned from cylindrical tubes comprise networks of long, narrow, prismatic beams of essentially rectangular cross section as shown in FIG. 6. These beams which make up the known tissue supporting devices may be straight or curved, depending on the particular design. Known expandable tissue supporting devices have a typical wall thickness b of 0.0635 mm (0.0025 inches) and a typical strut width h of 0.127 - 0.1524 mm (0.005 to 0.006 inches). The ratio of $b:h$ for most known designs is 1:2 or lower. As b decreases and as the beam length L increases, the beam is increasingly likely to respond to an applied bending moment M by buckling, and many designs of the prior art have displayed this behavior. This can be seen in the following expression for the "critical buckling moment" for the beam of FIG. 6.

$$M_{crit} = \frac{\pi b^3 h \sqrt{EG(1 - 0.63 \frac{b}{h})}}{6L}$$

Where:

E = Modulus of Elasticity

G = Shear Modulus

[0054] By contrast, in a ductile hinge based design according to the present invention, only the hinge itself deforms during expansion. The typical ductile hinge 32 is not a long narrow beam as are the struts in the known stents. Wall thickness of the present invention may be increased to 0.127 mm (0.005 inches) or greater, while hinge width is typically 0.0508-0.0762 mm (0.002-0.003 inches), preferably 0.0635 mm (0.0025 inches) or less. Typical hinge length, at 0.0508-0.0127 mm (0.002 to 0.005 inches), is more than an order of magnitude less than typical strut length. Thus, the ratio of $b:h$ in a typical ductile hinge 32 is 2:1 or greater. This is an inherently stable ratio, meaning that the plastic moment for such a ductile hinge beam is much lower than the critical buckling moment M_{crit} , and the ductile hinge beam deforms through normal strain-curvature. Ductile hinges 32 are thus not vulnerable to buckling when subjected to bending moments during expansion of the tissue supporting device 20.

[0055] To provide optimal recoil and crush-strength properties, it is desirable to design the ductile hinges so that relatively large strains, and thus large curvatures, are imparted to the hinge during expansion of the tissue supporting device. Curvature is defined as the reciprocal of the radius of curvature of the neutral axis of a beam in pure bending. A larger curvature during expansion results in the elastic curvature of the hinge being a small fraction of the total hinge curvature. Thus, the gross elastic recoil of the tissue supporting device is a small fraction of the total change in circumference. It is generally possible to do this because common stent materials, such as 316L Stainless Steel have very large elongations-to-failure (i.e., they are very ductile).

[0056] It is not practical to derive exact expressions for residual curvatures for complex hinge geometries and real materials (i.e., materials with non-idealized stress/strain curves). The general nature of residual curvatures and recoil of a ductile hinge may be understood by examining the moment-curvature relationship for the elastic-ideally-plastic rectangular hinge 66 shown in FIGS. 5a-c. It may be shown that the relationship between the applied moment and the

resulting beam curvature is:

$$M = M_p \left[1 - \frac{1}{3} \left(\frac{y_o}{h/2} \right)^2 \right] = \frac{3}{2} M_{yp} \left[1 - \frac{1}{3} \left(\frac{\kappa_{yp}}{\kappa} \right)^2 \right]$$

This function is plotted in FIG. 7. It may be seen in this plot that the applied moment M asymptotically approaches a limiting value M_p , called the plastic or ultimate moment. Beyond $^{11}/_{12} M_p$ large plastic deformations occur with little additional increase in applied moment. When the applied moment is removed, the beam rebounds elastically along a line such as a-b. Thus, the elastic portion of the total curvature approaches a limit of $3/2$ the curvature at the yield point. These relations may be expressed as follows:

$$M_p = \frac{3}{2} M_{yp} \Rightarrow \kappa_{rebound} = \frac{3}{2} \kappa_{yp}$$

[0057] Imparting additional curvature in the plastic zone cannot further increase the elastic curvature, but *will* decrease the ratio of elastic to plastic curvature. Thus, additional curvature or larger expansion of the tissue supporting device will reduce the percentage recoil of the overall stent structure.

[0058] As shown in FIG. 8, when a rigid strut 28 is linked to the ductile hinge 66 described above, the strut 28 forms an angle θ with the horizontal that is a function of hinge curvature. A change in hinge curvature results in a corresponding change in this angle θ . The angular elastic rebound of the hinge is the change in angle $\Delta \theta$ that results from the rebound in elastic curvature described above, and thus angular rebound also approaches a limiting value as plastic deformation proceeds. The following expression gives the limiting value of angular elastic rebound for the idealized hinge of FIG. 8.

$$\theta_{rebound} = 3\epsilon_{yp} \frac{L}{h}$$

Where strain at the yield point is an independent material property (yield stress divided by elastic modulus); L is the length of the ductile hinge; and h is the width of the hinge. For non-idealized ductile hinges made of real materials, the constant 3 in the above expression is replaced by a slowly rising function of total strain, but the effect of geometry would remain the same. Specifically, the elastic rebound angle of a ductile hinge decreases as the hinge width h increases, and increases as the hinge length L increases. To minimize recoil, therefore, hinge width h should be increased and length L should be decreased.

[0059] Ductile hinge width h will generally be determined by expansion force criteria, so it is important to reduce hinge length to a practical minimum in order to minimize elastic rebound. Empirical data on recoil for ductile hinges of different lengths show significantly lower recoil for shorter hinge lengths, in good agreement with the above analysis.

[0060] The ductile hinges 32 of the tissue supporting device 20 provide a second important advantage in minimizing device recoil. The embodiment of FIG. 2 shows a network of struts joined together through ductile hinges to form a cylinder. In this design, the struts 28 are initially parallel to an axis of the device. As the device is expanded, curvature is imparted to the hinges 32, and the struts 28 assume an angle θ with respect to their original orientation, as shown in FIG. 8. The total circumferential expansion of the tissue supporting device structure is a function of hinge curvature (strut angle) and strut length. Moreover, the incremental contribution to stent expansion (or recoil) for an individual strut depends on the instantaneous strut angle. Specifically, for an incremental change in strut angle $\Delta \theta$, the incremental change in circumference ΔC will depend on the strut length R and the cosine of the strut angle θ .

$$\Delta C = R \Delta \theta \cos \theta$$

[0061] Since elastic rebound of hinge curvature is nearly constant at any gross curvature, the net contribution to circumferential recoil ΔC is lower at higher strut angles θ . The final device circumference is usually specified as some fixed value, so decreasing overall strut length can increase the final strut angle θ . Total stent recoil can thus be minimized with ductile hinges by using shorter struts and higher hinge curvatures when expanded.

[0062] Empirical measurements have shown that tissue supporting device designs based on ductile hinges, such as the embodiment of FIG. 2, display superior resistance to compressive forces once expanded despite their very low expansion force. This asymmetry between compressive and expansion forces may be due to a combination of factors including the geometry of the ductile hinge, the increased wall thickness, and increased work hardening due to higher strain levels.

[0063] According to one example of the tissue supporting device of the invention, the device can be expanded by application of an internal pressure of about 2 bar (2 atmospheres) or less, and once expanded to a diameter between

2 and 3 times the initial diameter can withstand a compressive force of about 157 to 196 $\frac{\text{N}}{\text{m}}$ (16 to 20 gf/mm) or greater.

Examples of typical compression force values for prior art devices are 37 to 39 $\frac{\text{N}}{\text{m}}$ (3.8 to 4.0 gf/mm).

[0064] While both recoil and crush strength properties of tissue supporting devices can be improved by use of ductile hinges with large curvatures in the expanded configuration, care must be taken not to exceed an acceptable maximum strain level for the material being used. For the ductile hinge 44 of FIG. 3b, for example, it may be shown that the maximum material strain for a given bend angle is given by the expression:

$$\epsilon_{\max} = \frac{h}{L} \frac{\theta}{2}$$

[0065] Where ϵ_{\max} is maximum strain, h is ductile hinge width, L is ductile hinge length and θ is bend angle in radians. When strain, hinge width and bend angle are determined through other criteria, this expression can be evaluated to determine the correct ductile hinge length L .

[0066] For example, suppose the ductile hinge 44 of FIG. 3b was to be fabricated of 316L stainless steel with a maximum strain of 30%; ductile hinge width h is set at 0.0635 mm (0.0025 inch) by expansion force criteria; and the bend angle θ is mechanically limited to 0.5 radians ($\approx 30^\circ$) at full stent expansion. Solving the above expression for L gives the required ductile hinge length of at least about 0.0838 mm (0.0033 inches).

[0067] Similar expressions may be developed to determine required lengths for more complicated ductile hinge geometries, such as shown in FIG. 3e. Typical values for the prismatic portions of these curved ductile hinges range 0.051 - 0.089 mm from about 0.002 to about 0.0035 inches) in hinge width and 0.051 - 0.152 mm (about 0.002 to about 0.006 inches) in hinge length. The tissue supporting device design of FIGS. 4a and 4b include a stop which limits the maximum geometric deflection at the ductile hinges by the design of the angled walls 96 of the notches 94.

[0068] In many designs of the prior art, circumferential expansion was accompanied by a significant contraction of the axial length of the stent which may be up to 15 % of the initial device length. Excessive axial contraction can cause a number of problems in device deployment and performance including difficulty in proper placement and tissue damage. Designs based on ductile hinges 32 can minimize the axial contraction, or foreshortening, of a tissue supporting device during expansion as follows.

[0069] FIGS. 9a and 9b illustrate an exaggerated ductile hinge 32 and shortened struts 28 in initial and expanded conditions. Each strut 28 is attached to two ductile hinges 32 at opposite ends. Each ductile hinge 32 has an instant center of rotation C_1 , C_2 that is an effective pivot point for the attached strut 28. Initially, during expansion the pivot point C_1 is displaced vertically by a distance d until C_1 is positioned even with C_2 as shown in FIG. 9b. When the array is expanded vertically, the axial struts 28 move in a circular arc with respect to the pivot points, as shown in FIG. 9b. It can

be seen that the horizontal distance e between pivot points C_1 and C_2 actually increases initially, reaching a maximum e_{\max} when the two points are on the same horizontal axis as shown in FIG. 9b. As the vertical expansion continues, the device compresses axially back to its original length. Only when vertical expansion of the array continues beyond the point where the horizontal distance e between C_1 and C_2 is the same as the original horizontal distance e does the overall length of the array actually begin to contract. For the stent shown in FIG. 2, for example, approximately 1/3 of the total circumferential expansion has been accomplished by the time the configuration of FIG. 9b is reached, and the stent exhibits very low axial contraction.

[0070] This ability to control axial contraction based on hinge and strut design provides great design flexibility when using ductile hinges. For example, a stent could be designed with zero axial contraction.

[0071] An alternative embodiment that illustrates the trade off between crush strength and axial contraction is shown in FIG. 10. FIG. 10 shows a portion of a tissue supporting device 70 having an array of struts 72 and ductile hinges 74 in the unexpanded state. The struts 72 are positioned initially at an angle θ_1 with respect to a longitudinal axis X of the device. As the device is expanded radially from the unexpanded state illustrated in FIG. 10, the angle θ_1 increases. In this case the device contracts axially from the onset of vertical expansion throughout the expansion. Once the device has been completely expanded the final angle θ_1 made by the strut 72 with the horizontal will be much greater than the angle θ in the device of FIG. 8a and 8b. As shown previously, a higher final strut angle θ_1 , can significantly increase crush strength and decrease circumferential recoil of the stent structure. However, there is a trade off between increased crush strength and increase in axial contraction.

[0072] According to one example of the present invention, the struts 72 are positioned initially at an angle of about 0° to 45° with respect to a longitudinal axis of the device. As the device is expanded radially from the unexpanded state illustrated in FIG. 10a, the strut angle increases to about 20° to 80° .

[0073] Tissue supporting devices including ductile hinges as described above can be used to create many useful device configurations in addition to the substantially cylindrical devices described above. For example, tissue supporting devices having ductile hinges may be designed in which various sections or areas of the device open at differential expansion pressures by varying the hinge configuration. This feature makes it possible to control the expansion sequence of different features and areas of the device. Another tissue supporting device design variation allows the creation of specially shaped side-access holes in the device which open up as the device expands and can be used accommodate vessel bifurcations.

[0074] Ductile hinges are especially useful in creating tissue supporting devices that expand in a specified sequence. By varying the width of specific ductile hinges in different areas of the tissue supporting device, the expansion pressure of each of the different areas of the device can be adjusted independently. As the device is expanded, such as by increasing pressure within a balloon, areas with the smallest hinge width open first, followed by expansion of areas with progressively wider hinge widths. A method of delivering an expandable medical device employing controlled expansion of the device is described in U.S. Patent Application Serial No.09/315,885, filed on May 20, 1999.

[0075] FIGS. 11a-11c show the sequence of expansion of a differentially expanding tissue supporting device 100 according to one embodiment of the invention. FIG. 11a shows an unexpanded tissue supporting device 100 in which a left portion 102 of the device has ductile hinges with larger hinge widths than a right portion 104 of the device. For example, the two left rows of struts of the device may have larger hinge widths than the two right rows of struts on the same device. Although the hinges in different sections 102, 104 of the device 100 have been described as having differing widths for achieving the desired differential expansion, the hinge geometry may alternatively be modified in other ways to achieve differential expansion.

[0076] To expand the device 100, a balloon or other expansion device is inserted into the central lumen of the device and the balloon is inflated. As the inflation pressure of the balloon is increased, the right side 104 of the device expands as shown in FIG. 11b. At this point, expansion can be halted with one half of the device expanded and the other unexpanded. The expansion may be halted to perform some other task such as removal of a locating device or for other reasons. Pressurization of the balloon is then continued to complete deployment of the left side 102 of the device as shown in FIG. 11c. Many more complex sequences of expansion are possible and potentially useful. For example, three or more segments of the device may be expanded at different times. Alternatively, the sections of the device which are differentially expanded may be cylindrical sections, longitudinal sections, rectangular sections, or sections of any other shape. Differential expansion is very useful in special deployment situations, such as treatment of bifurcations, and in creating special tissue supporting device features, such as side access holes as shown in FIGS. 12a-12c.

[0077] A framed hole feature, such as the feature shown in FIGS. 12a-12c, is capable of providing strong, uniform support to the tissue at a bifurcation in an artery. Known techniques for treating bifurcations generally deliver a mesh tissue supporting device into the artery and position the device over the bifurcation. According to the known methods, a surgeon then attempts to create one or more branch lumen access holes by inserting a balloon through the sidewall of the mesh device, and then inflating the balloon to simply push the local features of the mesh aside. These techniques are inherently random in nature: the exact point of expansion in the device lattice cannot be predicted, and the device may or may not expand satisfactorily at that point. Tissue support provided by these known techniques for treating

bifurcated arteries is similarly unpredictable.

[0078] FIG. 12a shows an unexpanded tissue support device 110 in which a rectangular hole 112 has been formed in the center. Ductile hinges 116 connect all the struts 118 and links 120 of the device as described above with respect to the previous embodiments. The ends of the device 110 have a regular pattern of struts 118 and ductile hinges 116. The hole 112 is formed by removing several axial struts and connecting their respective side links into two longer circumferential side links 114, which provide a vertical frame for the hole 112. The struts 122 which frame the hole 112 and connect the side links 114 may be straight, as shown, rounded, or contoured in some other way, depending on the desired final shape of the expanded hole feature.

[0079] According to one alternative embodiment of the invention, the ductile hinges 116 connecting the frame struts 122 and the side links 114 will be designed to open at a somewhat lower inflation pressure than the remainder of the ductile hinges around the rest of the circumference of the device. Thus, when the device 110 is expanded the struts 122 and side links 114 that frame the hole feature 112 will open first. When these struts 122 reach their maximum angle, defined by the hinge angles, the frame surrounding the hole 112 "locks" in its desired shape. The remaining struts 118 around the circumference of the device then expand in a normal fashion, providing full strength and support to the lumen opposite the hole 112. FIGS. 12b and 12c show schematic representations of the device of FIG. 12a in unexpanded and expanded configurations. As shown in FIG. 12c, the rectangular unexpanded hole feature 112 expands into an octagon shape.

[0080] A second property of ductile hinges is important in the creation of the side hole features 112. In applications requiring larger side holes, the expanded side hole may span less of the circumference of the expanded stent than the struts that were removed to create the hole. For this reason, the remaining struts in the rows containing the hole feature must span a larger portion of the circumference of the device. To do this, they must assume a greater bend angle, often as high as 60 degrees. This is easily accomplished with ductile hinges such as the one shown in FIG. 3e by increasing the arc length of the hinge.

[0081] The hole features according to the present invention may take on different shapes and sizes depending on the application. The framed-hole features can also be designed to take advantage of the superior crimping properties of ductile hinges. For example, ancillary devices can be crimped into a stent catheter assembly in specially designed holes.

[0082] According to one alternative embodiment of the present invention, the expandable tissue supporting device can also be used as a delivery device for certain beneficial agents including drugs, chemotherapy, or other agents. Due to the structure of the tissue supporting device incorporating ductile hinges, the widths of the struts can be substantially larger than the struts of the prior art devices. The struts due to their large size can be used for beneficial agent delivery by providing beneficial agent on the struts or within the struts. Examples of beneficial agent delivery mechanisms include coatings on the struts, such as polymer coatings containing beneficial agents, laser drilled holes in the struts containing beneficial agent, and the like.

[0083] While the invention has been described in detail with reference to the preferred embodiments thereof, it will be apparent to one skilled in the art that various changes and modifications can be made and equivalents employed, without departing from the present invention.

Claims

1. An expandable medical device (100;110) comprising:

a plurality of elongated beams (118), the plurality of elongated beams (118) joined together to form a substantially cylindrical device (100;110) which is radially expandable, the plurality of elongated beams (118) having a beam width; and

a plurality of ductile hinges (116) connecting the plurality of beams (118) together in the substantially cylindrical device (100;110), a first section (104) of the substantially cylindrical device (100;110) including ductile hinges (116) having a first width and a second section (102) of the substantially cylindrical device (100;110) including ductile hinges (116) having a second width;

characterised in that

the ductile hinges (116) have a width along a portion of a hinge length which is smaller than the beam width such that as the device (100;110) is expanded the ductile hinges (116) experience plastic deformation while the beams (118) are not plastically deformed, and in that

the second width is different from the first width, such that the first section (104) expands before the second section (102).

2. The expandable medical device (100) according to Claim 1, wherein the first section (104) is a substantially cylindrical

section at a first end of the device (100;110) and the second section (102) is a substantially cylindrical section at a second end of the device (100).

3. The expandable medical device (100;110) according to Claims 1 or 2, wherein the first width and the second width are selected such that the entire first section (102) expands prior to expansion of the second section (104).
4. The expandable medical device (100;110) according to one of Claims 1 to 3, further comprising a balloon for expanding the device (100;110) from a first diameter to a second diameter.
5. The expandable medical device (100;110) according to Claims 1 to 4, wherein the plurality of elongated beams (28) extend substantially axially and a plurality of circumferential beams (24) are each connected at first and second ends to one of the axial beams (28) by a ductile hinge (32).
6. The expandable medical device (110) according to one of Claims 1 to 5, further comprising a side access hole (112) formed in the device (110) in an unexpanded state which accommodates a vessel bifurcation when the device (110) is expanded.

Patentansprüche

1. Expandierbare medizinische Vorrichtung (100, 110), umfassend:

mehrere längliche Streben (118), wobei die mehreren länglichen Streben (118) miteinander verbunden sind, um eine im Wesentlichen zylindrische Vorrichtung (100, 110) zu bilden, welche radial expandierbar ist, wobei die mehreren länglichen Streben (118) eine Strebenbreite aufweisen; und mehrere duktile Gelenke (116), welche die mehreren Streben (118) zusammen zu der im Wesentlichen zylindrischen Vorrichtung (100, 110) verbinden, wobei ein erster Abschnitt (104) der im Wesentlichen zylindrischen Vorrichtung (100, 110) duktile Gelenke (116) einer ersten Breite umfasst und ein zweiter Abschnitt (102) der im Wesentlichen zylindrischen Vorrichtung (100, 110) duktile Gelenke (116) einer zweiten Breite umfasst;

dadurch gekennzeichnet, dass

die duktilen Gelenke (116) entlang eines Abschnitts einer Gelenklänge eine Breite aufweisen, die kleiner ist als die Strebenbreite, so dass bei Expansion der Vorrichtung (100, 110) die duktilen Gelenke (116) plastische Verformung erfahren, während die Streben (118) nicht plastisch verformt werden, und **dadurch** dass die zweite Breite verschieden ist von der ersten Breite, so dass der erste Abschnitt (104) vor dem zweiten Abschnitt (102) expandiert.

2. Expandierbare medizinische Vorrichtung (100) nach Anspruch 1, wobei der erste Abschnitt (104) ein im Wesentlichen zylindrischer Abschnitt an einem ersten Ende der Vorrichtung (100, 110) ist und der zweite Abschnitt (102) ein im Wesentlichen zylindrischer Abschnitt an einem zweiten Ende der Vorrichtung (100) ist.
3. Expandierbare medizinische Vorrichtung (100, 110) nach Anspruch 1 oder 2, wobei die erste Breite und die zweite Breite derart ausgewählt sind, dass der gesamte erste Abschnitt (102) vor dem zweiten Abschnitt (104) expandiert.
4. Expandierbare medizinische Vorrichtung (100, 110) nach einem der Ansprüche 1 bis 3, ferner umfassend einen Ballon zum Expandieren der Vorrichtung (100, 110) von einem ersten Durchmesser auf einen zweiten Durchmesser.
5. Expandierbare medizinische Vorrichtung (100, 110) nach einem der Ansprüche 1 bis 4, wobei sich die mehreren länglichen Streben (28) im Wesentlichen axial erstrecken und mehrere Umfangsstreben (24) jeweils mittels eines duktilen Gelenkes (32) an dem ersten und dem zweiten Ende einer der axialen Streben (28) verbunden sind.
6. Expandierbare medizinische Vorrichtung (110) nach einem der Ansprüche 1 bis 5, ferner umfassend eine Seitenzugangsöffnung (112), welche in der Vorrichtung (110) in einem nicht expandierten Zustand gebildet ist und angepasst ist an eine Gefäßverzweigung, wenn die Vorrichtung (110) expandiert ist.

Revendications**1.** Dispositif médical expansible (100; 110) comprenant :

une pluralité de traverses allongées (118), la pluralité de traverses allongées (118) étant assemblée pour former un dispositif sensiblement cylindrique (100; 110) qui est radialement expansible, la pluralité de traverses allongées (118) ayant une largeur de traverse ; et
 une pluralité d'articulations ductiles (116) raccordant la pluralité de traverses (118) ensemble dans le dispositif sensiblement cylindrique (100; 110), une première section (104) du dispositif sensiblement cylindrique (100; 110) comprenant des articulations ductiles (116) ayant une première largeur et une seconde section (102) du dispositif sensiblement cylindrique (100; 110) comprenant des articulations ductiles (116) ayant une seconde largeur ;

caractérisé en ce que :

les articulations ductiles (116) ayant une largeur le long d'une partie d'une longueur d'articulation qui est inférieure à la largeur de traverse de sorte que lorsque le dispositif (100; 110) est dilaté, les articulations ductiles (116) subissent une déformation plastique alors que les traverses (118) ne sont pas déformées plastiquement, et **en ce que :**

la seconde largeur est différente de la première largeur, de sorte que la première section (104) se dilate avant la seconde section (102).

2. Dispositif médical expansible (100) selon la revendication 1, dans lequel la première section (104) est une section sensiblement cylindrique au niveau de la première extrémité du dispositif (100; 110) et la seconde section (102) est une section sensiblement cylindrique au niveau d'une seconde extrémité du dispositif (100).

3. Dispositif médical expansible (100; 110) selon les revendications 1 ou 2, dans lequel la première largeur et la seconde largeur sont sélectionnées de sorte que toute la première section (102) se dilate avant l'expansion de la seconde section (104).

4. Dispositif médical expansible (100; 110) selon l'une des revendications 1 à 3, comprenant en outre un ballonnet pour dilater le dispositif (100; 110) d'un premier diamètre à un second diamètre.

5. Dispositif médical expansible (100; 110) selon les revendications 1 à 4, dans lequel la pluralité de traverses allongées (28) s'étend sensiblement de manière axiale et une pluralité de traverses circonférentielles (24) sont chacune raccordées au niveau des première et seconde extrémités à l'une des traverses axiales (28) par une articulation ductile (32).

6. Dispositif médical expansible (110) selon une des revendications 1 à 5, comprenant en outre un trou d'accès latéral (112) formé dans le dispositif (110) dans un état non dilaté qui loge une bifurcation de vaisseau lorsque le dispositif (110) est dilaté.

FIG. 1
PRIOR ART

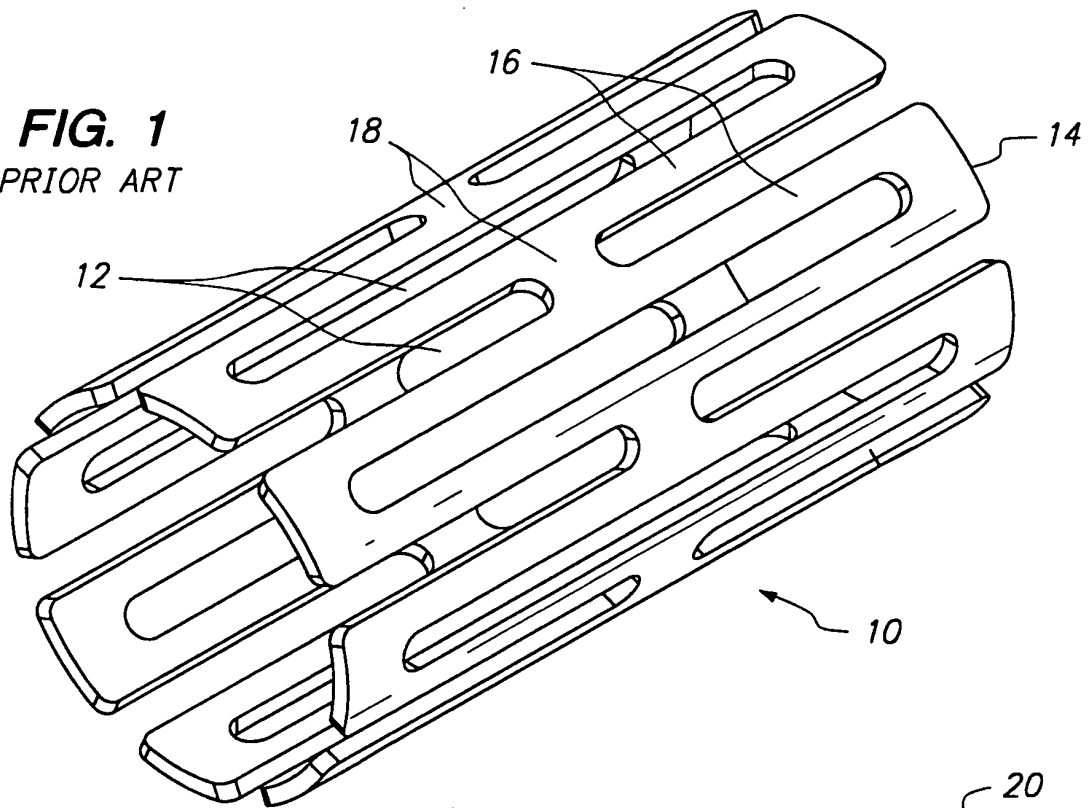
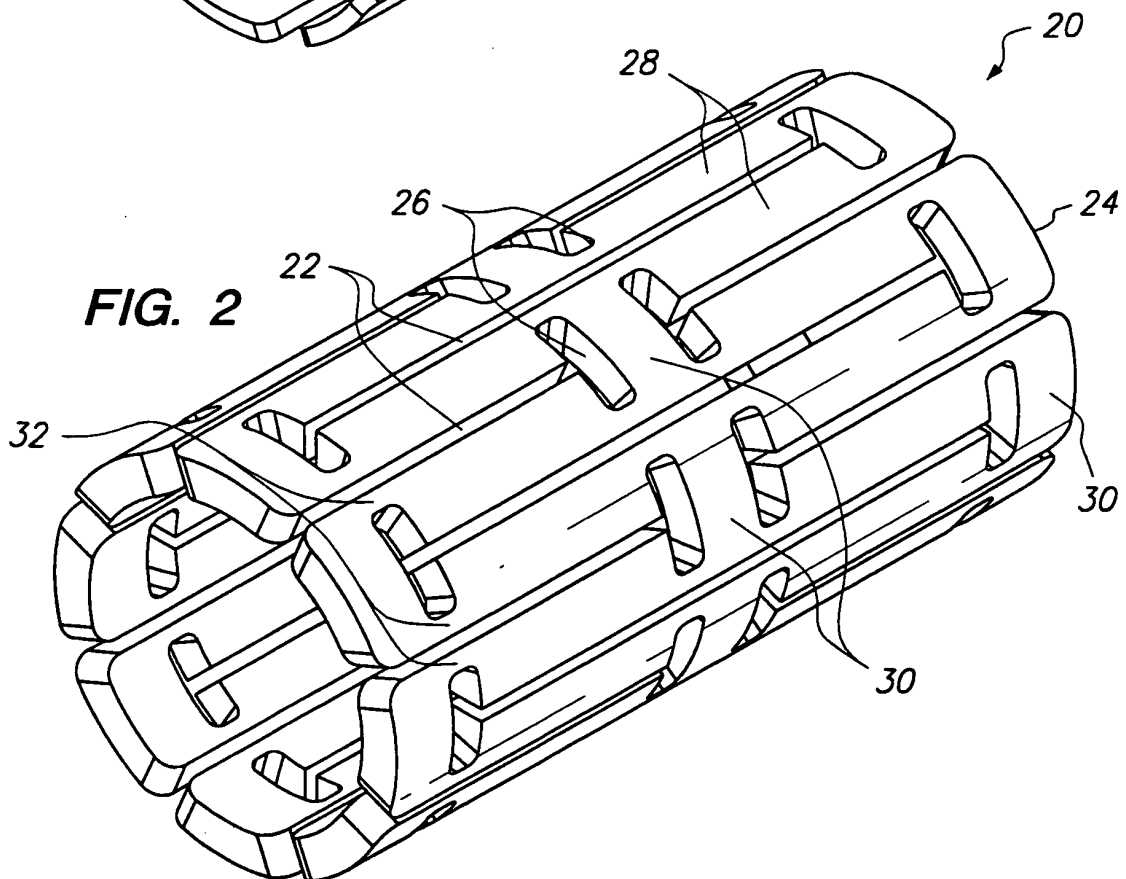


FIG. 2



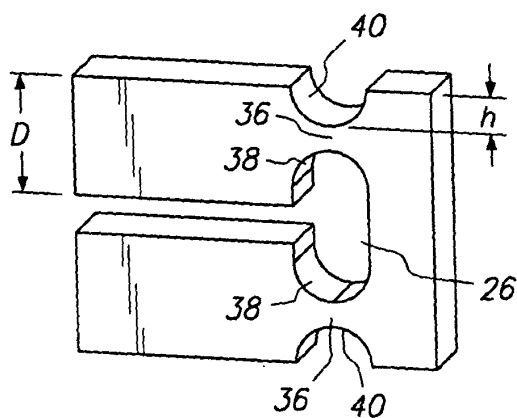


FIG. 3a

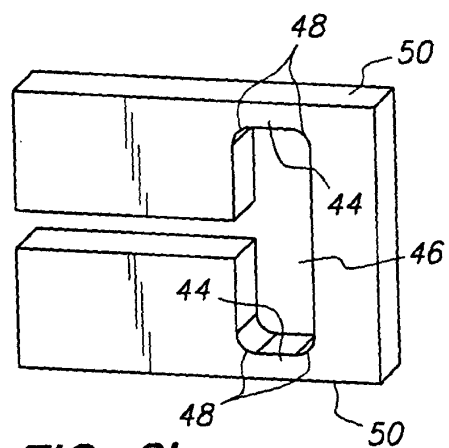


FIG. 3b

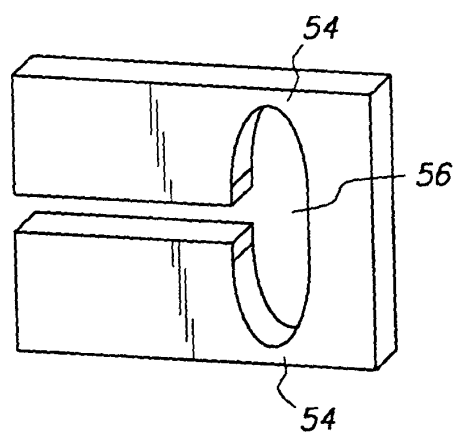


FIG. 3c

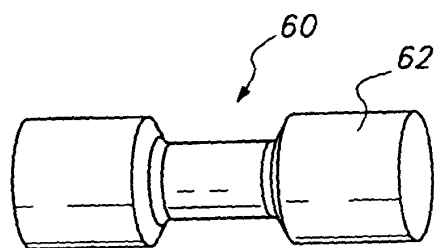


FIG. 3d

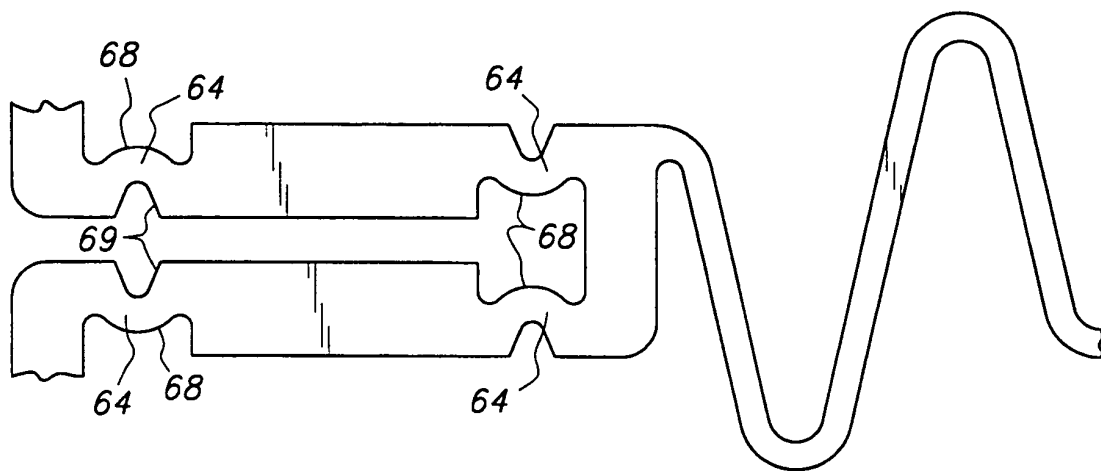


FIG. 3e

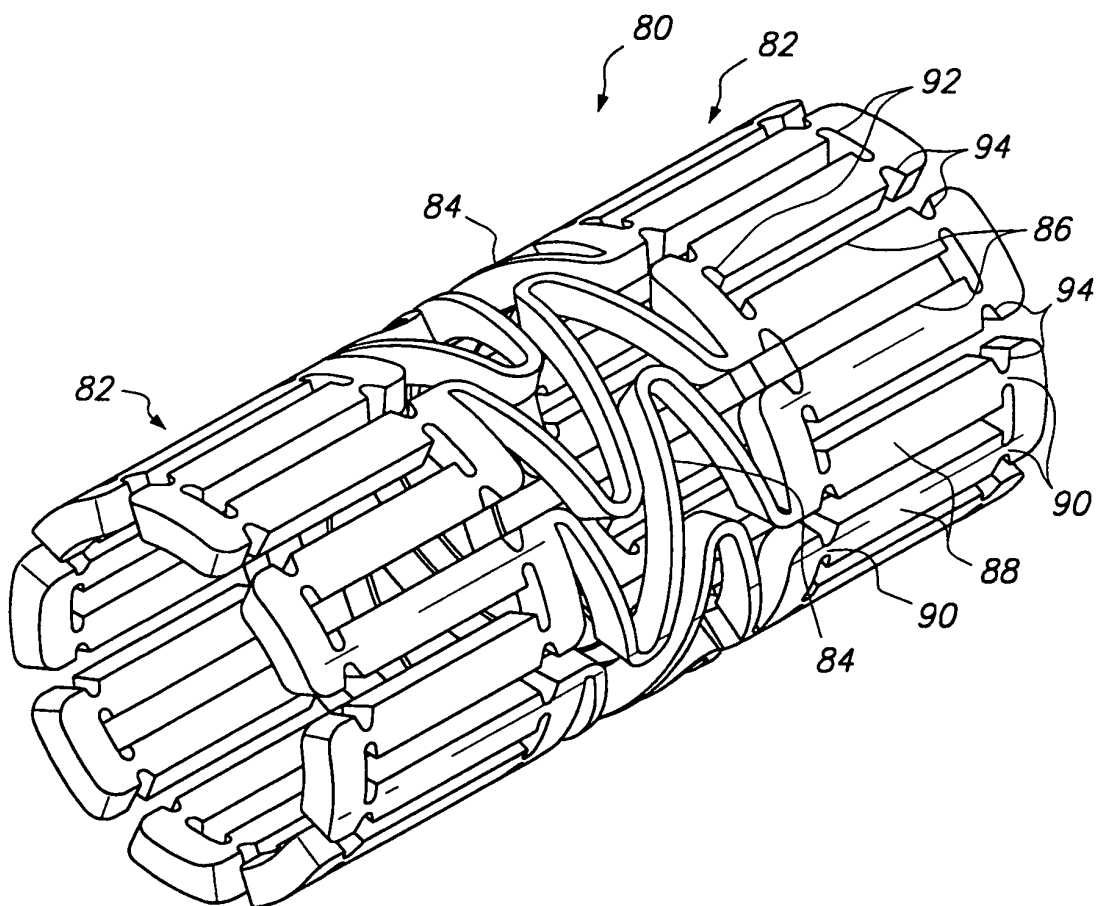


FIG. 4a

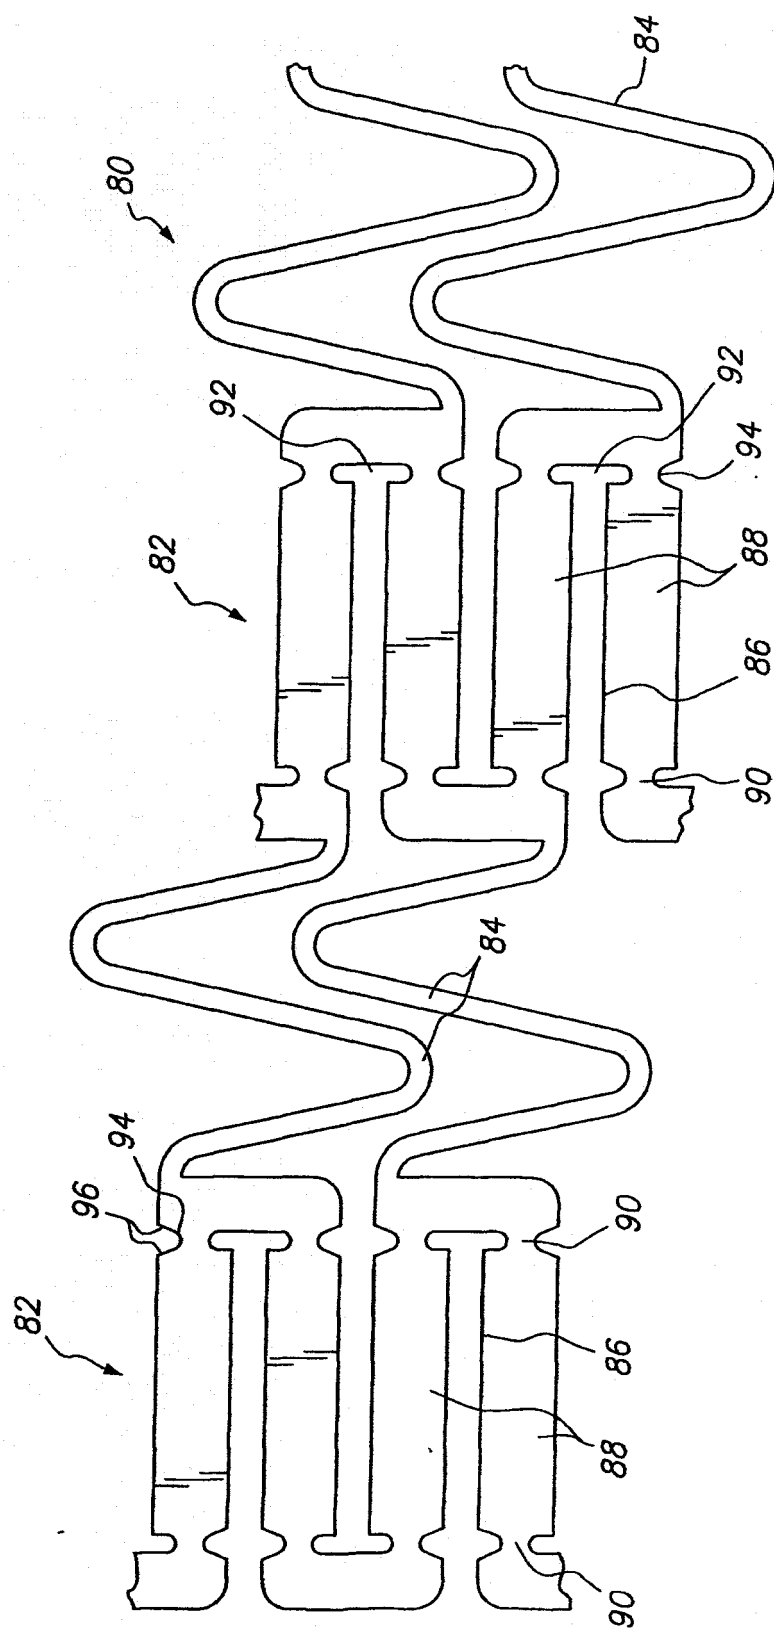


FIG. 4b

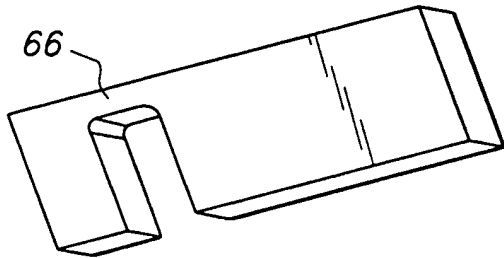


FIG. 5a

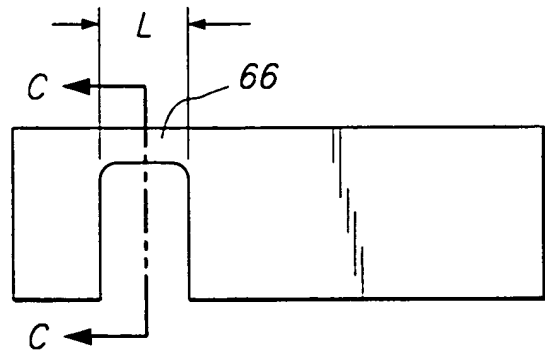


FIG. 5b

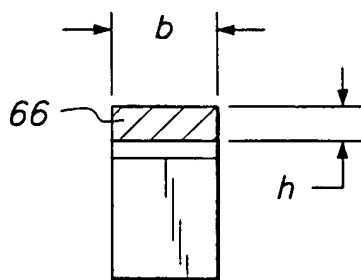


FIG. 5c

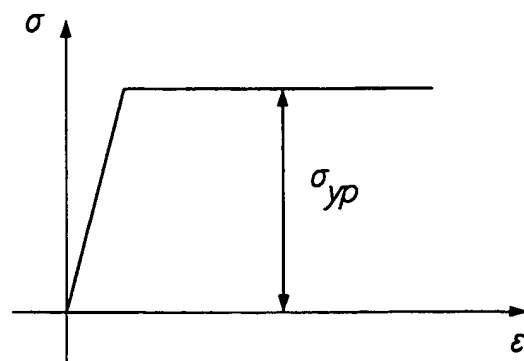
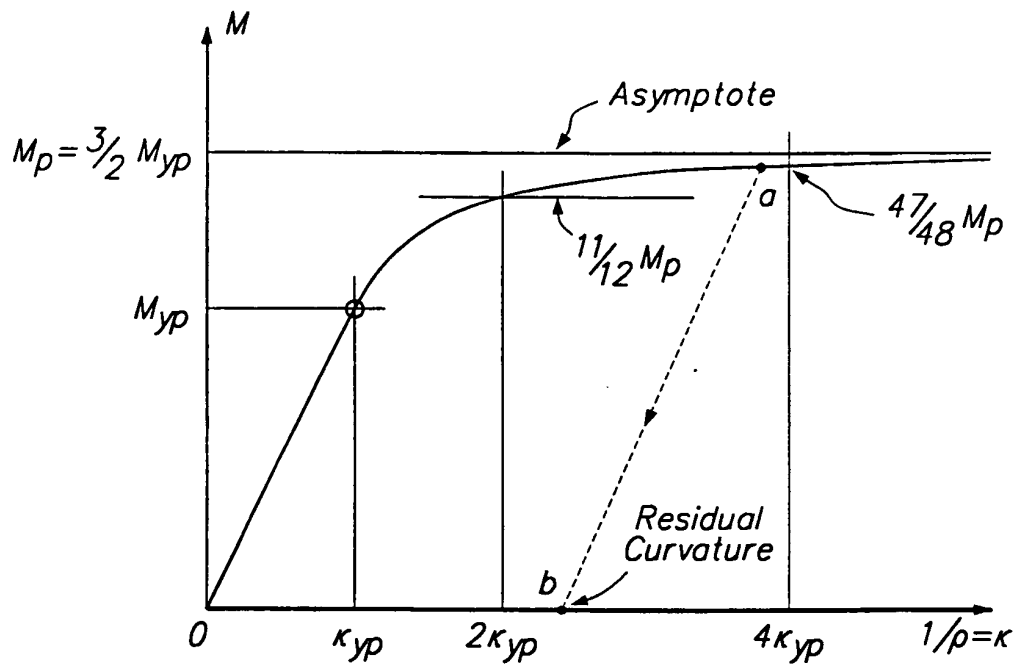
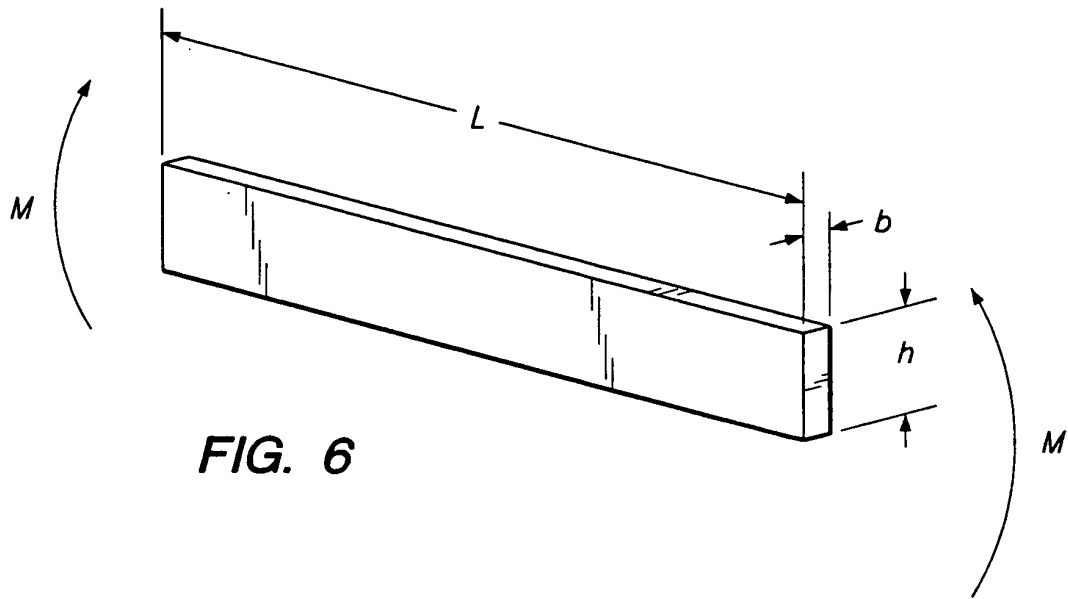
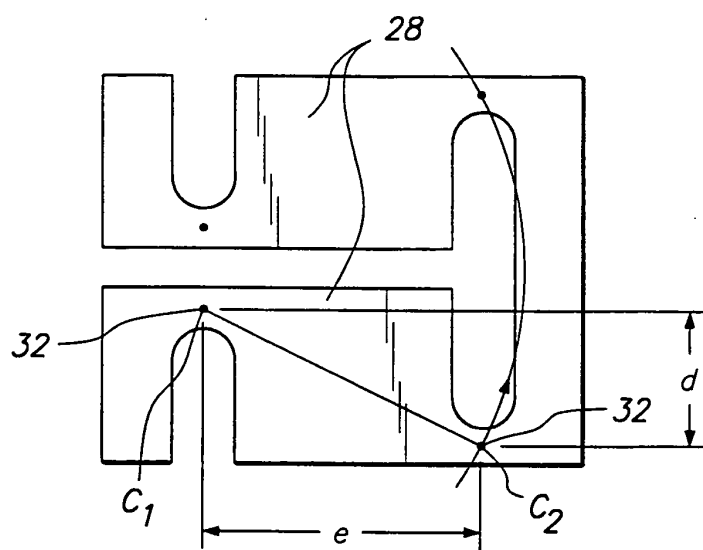
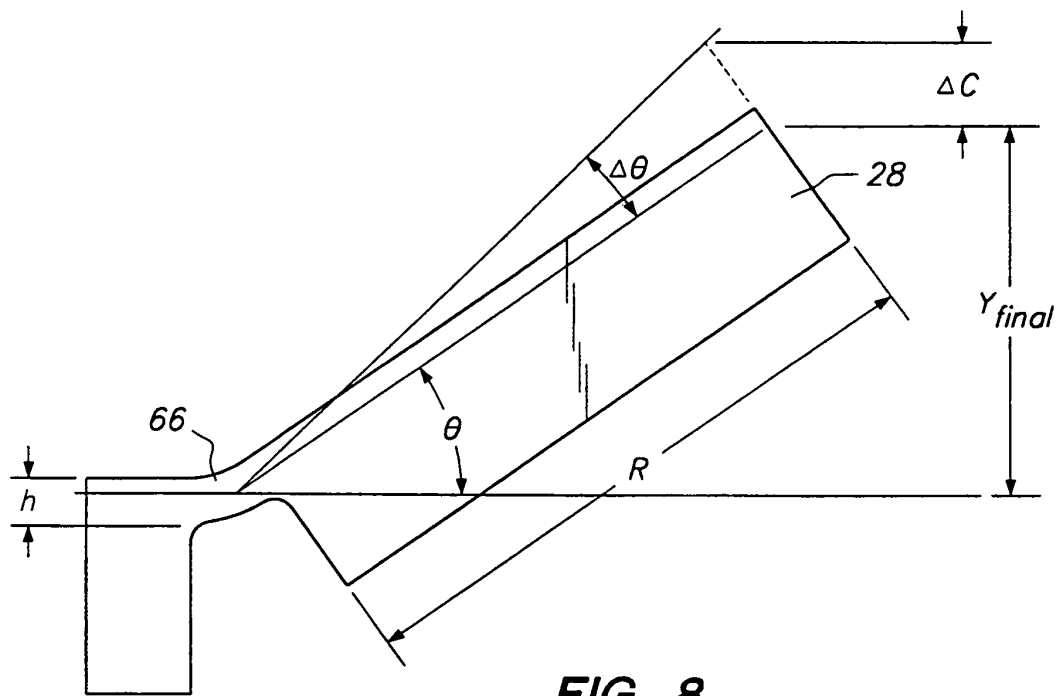


FIG. 5d





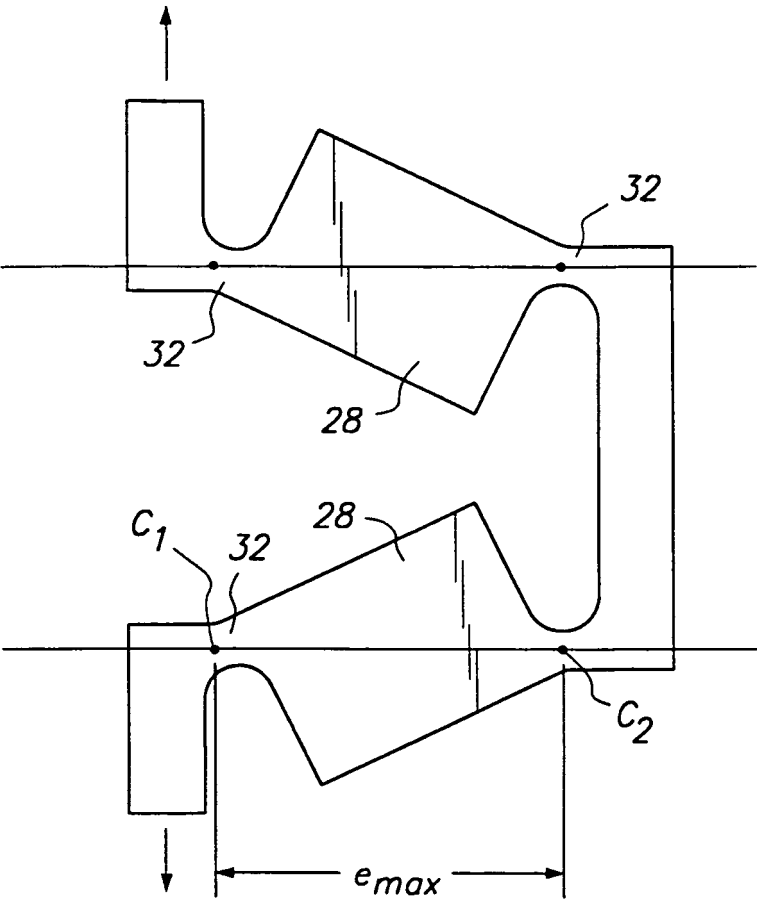


FIG. 9b

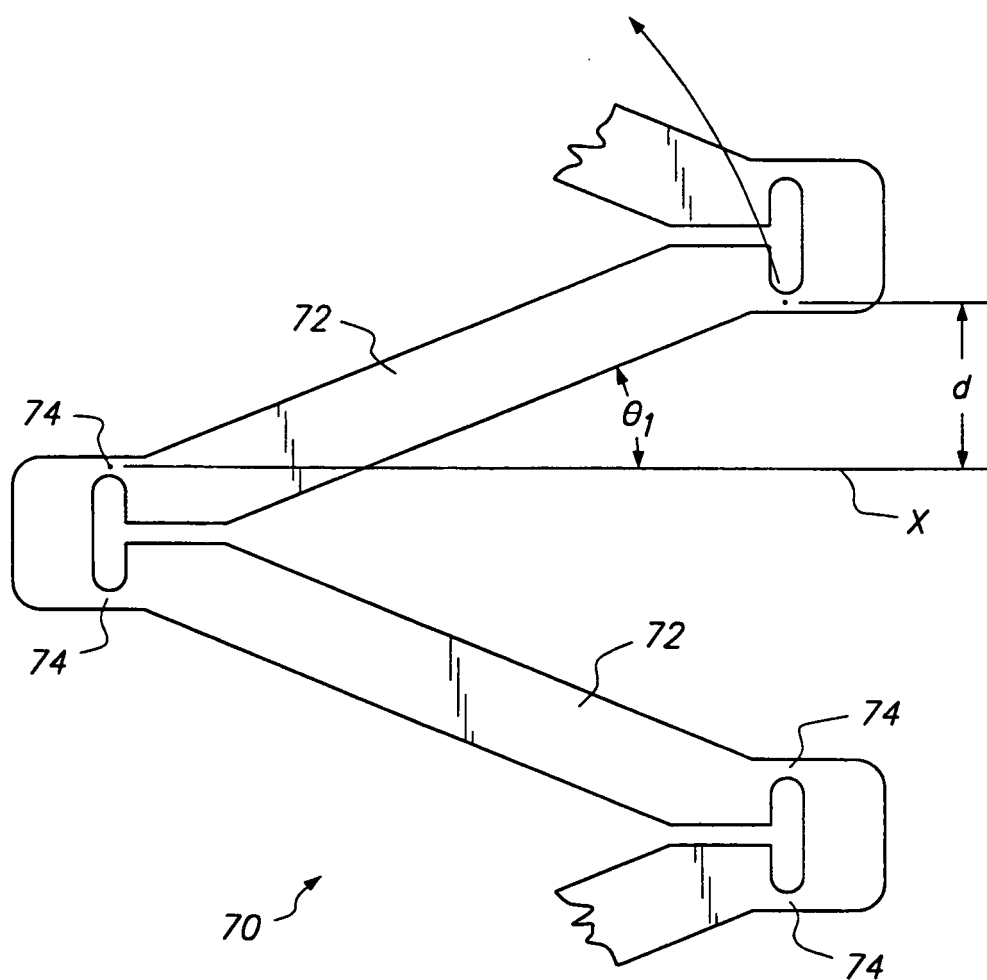


FIG. 10

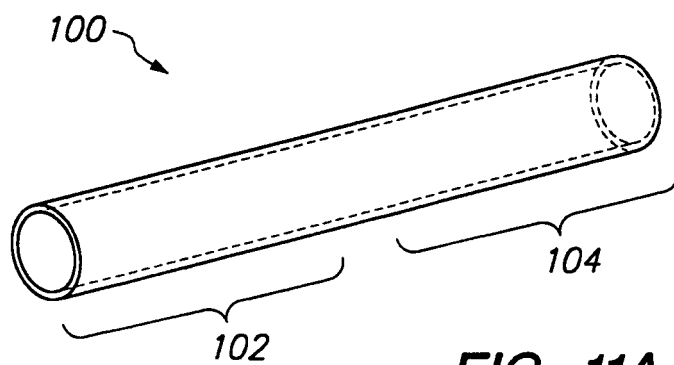


FIG. 11A

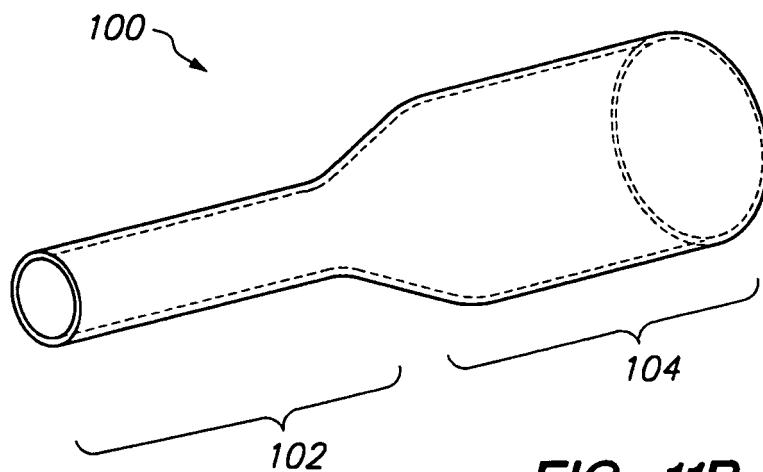


FIG. 11B

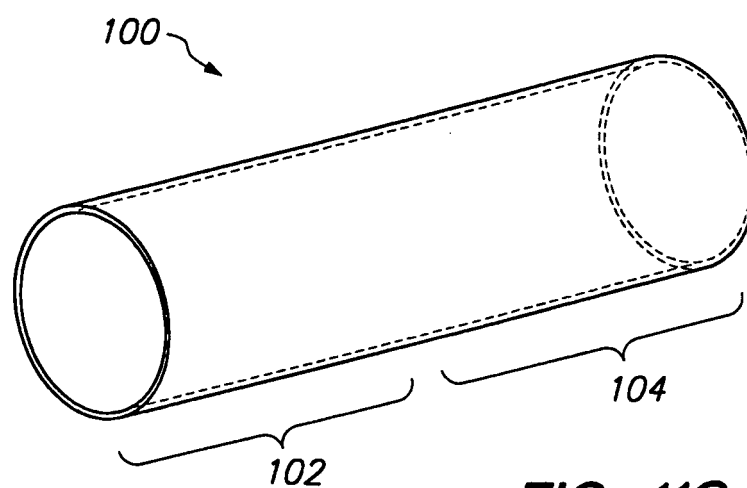


FIG. 11C

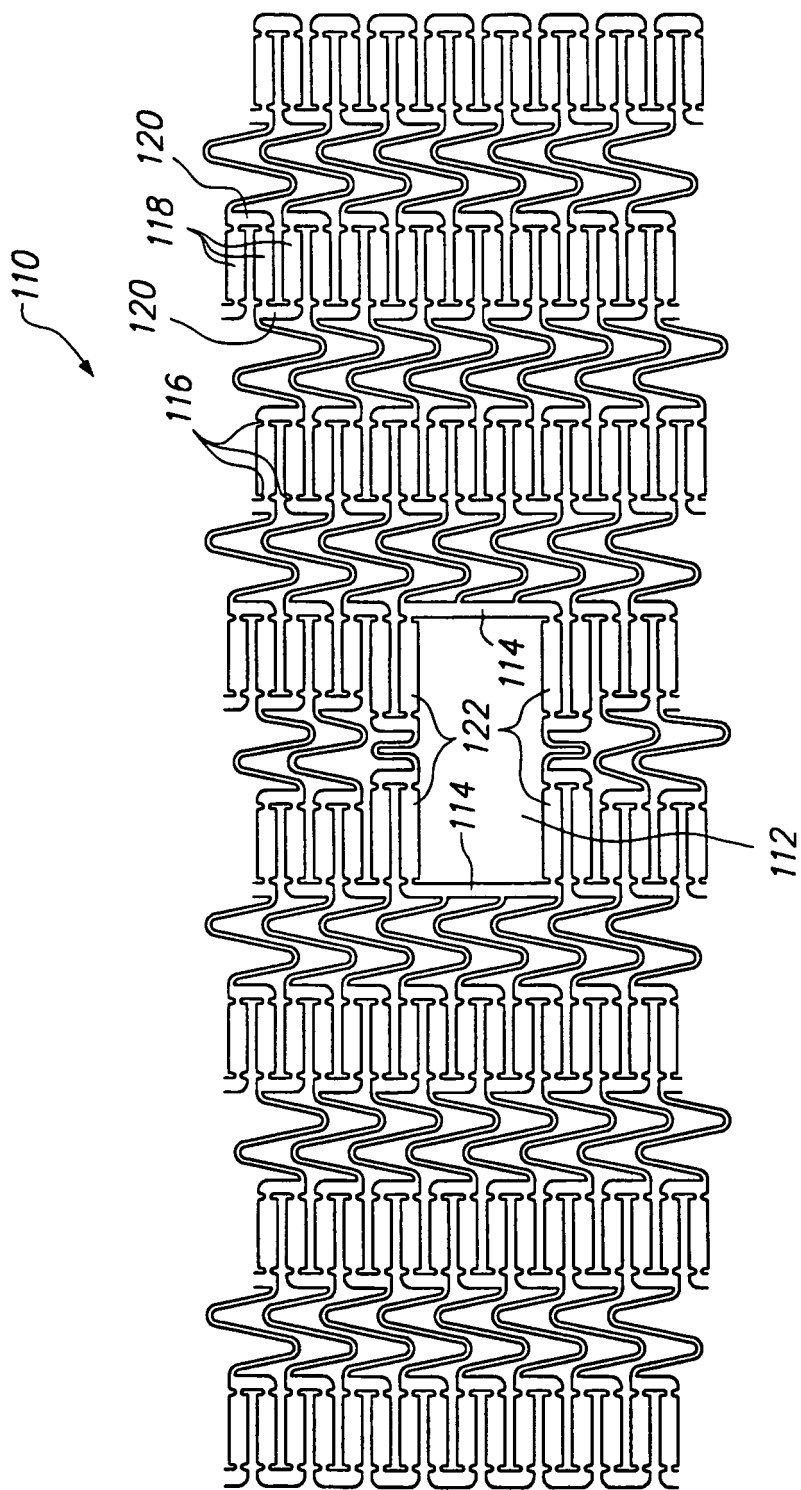


FIG. 12A

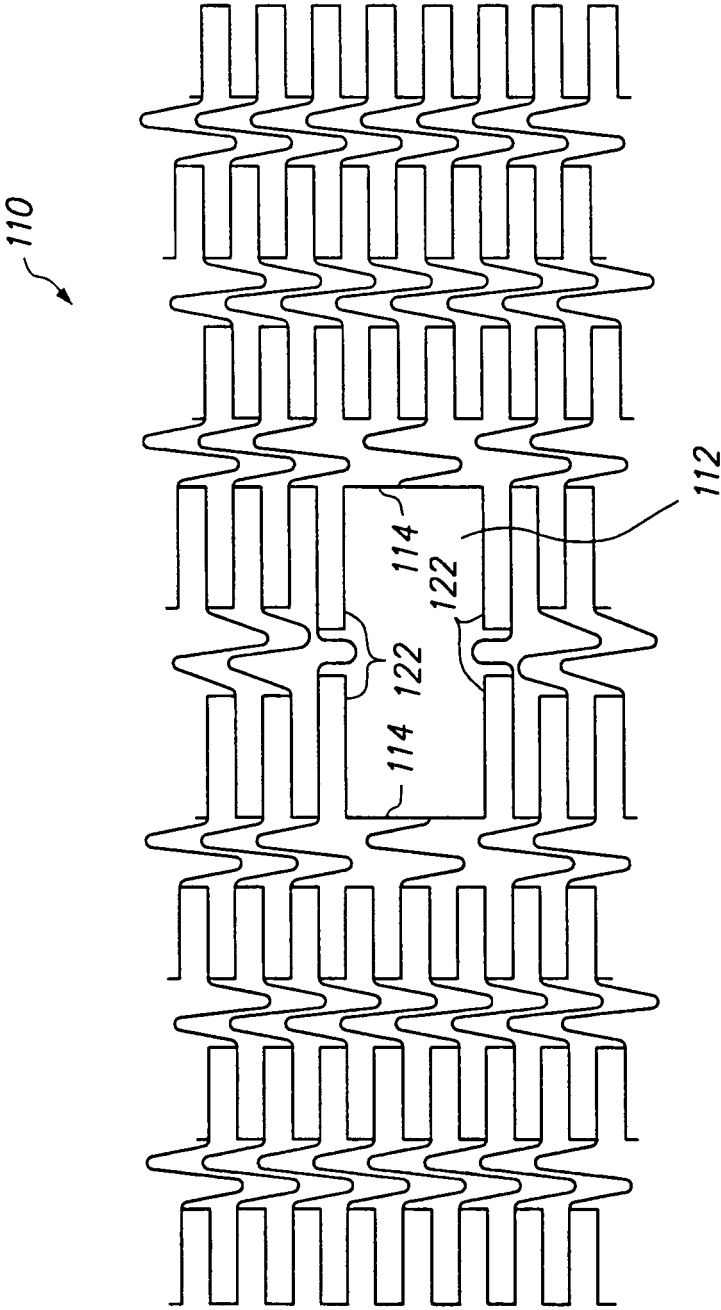


FIG. 12B

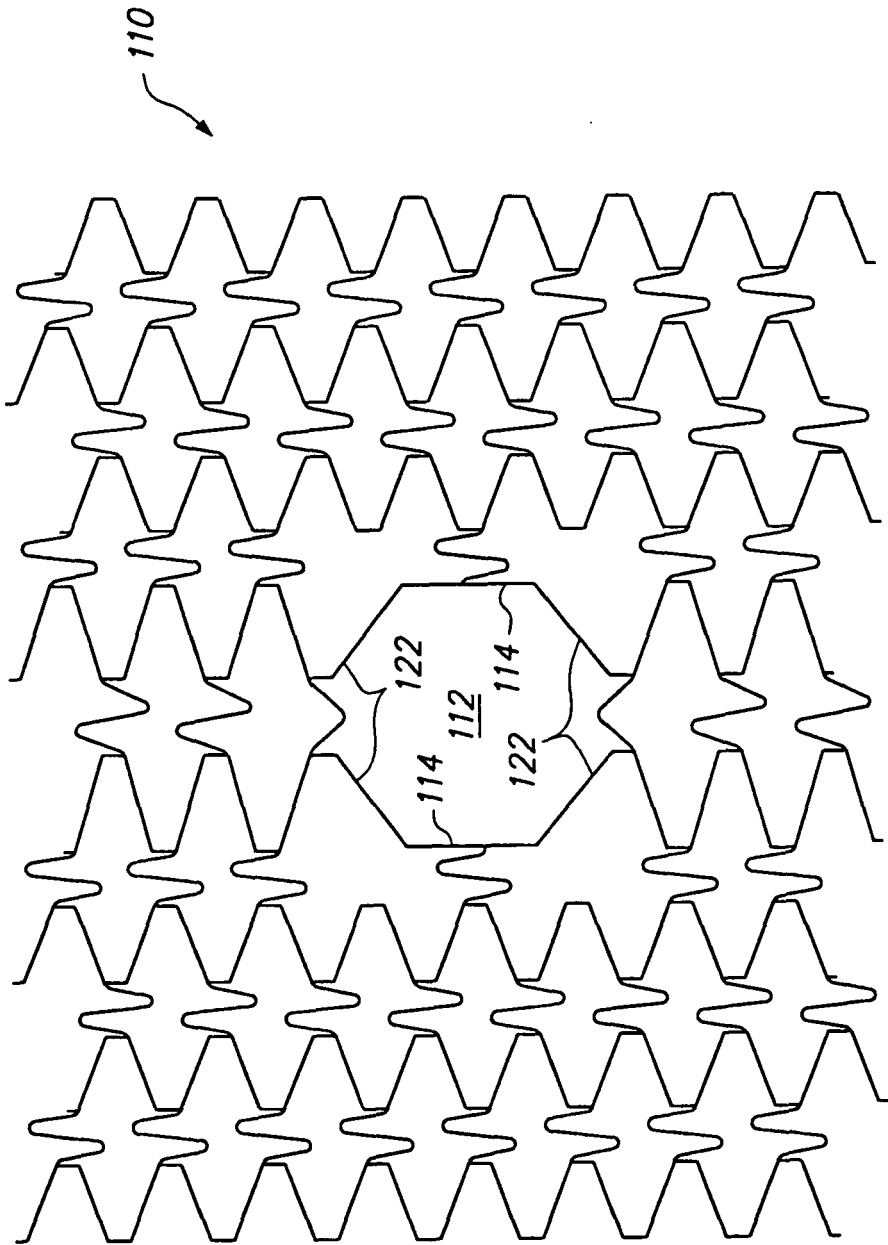


FIG. 12C

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- US 4969458 A [0003]
- US 4733665 A [0003] [0003] [0004]
- US 4776337 A [0003] [0003] [0004]
- US 4739762 A [0003] [0004]
- US 5545210 A [0009]
- WO 9629028 A [0012]
- US 315885 A [0074]