

(19)



(11)

EP 1 280 428 B1

(12)

EUROPEAN PATENT SPECIFICATION

(45) Date of publication and mention
of the grant of the patent:

06.08.2014 Bulletin 2014/32

(51) Int Cl.:

A61G 13/12 (2006.01)

(86) International application number:

PCT/US2000/009529

(21) Application number: **00921996.5**

(22) Date of filing: **09.04.2000**

(87) International publication number:

WO 2001/076403 (18.10.2001 Gazette 2001/42)

(54) **Protective cushion and cooperatively engageable helmet casing for anesthetized patient**

Schutzkissen und in Wirkungseingriff bringbare Helmschale für einen narkotisierten Patient

Coussin de protection et boîtier de casque joignable de façon coopérative destinés a un patient anesthésié

(84) Designated Contracting States:

**AT BE CH CY DE DK ES FI FR GB GR IE IT LI LU
MC NL PT SE**

• **VU, An**

Fallbrook CA 92028 (US)

(43) Date of publication of application:

05.02.2003 Bulletin 2003/06

(74) Representative: **Gray, James et al**

Withers & Rogers LLP

4 More London Riverside

London

SE1 2AU (GB)

(73) Proprietor: **Dupaco, Inc.**

Oceanside, CA 92056 (US)

(72) Inventors:

• **JORDAN, Gregory**

Carlsbad, CA 92008 (US)

(56) References cited:

US-A- 3 337 883 US-A- 4 504 050

US-A- 4 752 064 US-A- 5 220 699

US-A- 5 771 514 US-A- 6 112 333

EP 1 280 428 B1

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

Description

BACKGROUND OF THE INVENTION

1. Field of the Invention

[0001] The present invention relates to a safety helmet for cranial protection. More particularly it relates to a modular helmet apparatus constructed of interchanging co-operative components of differing sizes which provide a prophylactic cushion and helmet to be worn by patients undergoing general anesthesia to prevent eye, skin, or other nerve damage from prolonged pressure upon areas of the head as well as to provide a safer manner for cranial manipulation during surgery.

2. Prior Art

[0002] Surgeries upon patients in the prone position present a number of patient care challenges to the anesthesiologist and surgical staff. Once a patient undergoing a surgery requiring general anesthesia is anesthetized, that patient is essentially in a coma like state. In such a state, noxious stimuli to the patient's body and skin, such as pressure or pain, which would normally cause an awake patient to move to relieve the stimulus, no longer causes such a reaction. Consequently, patients under general anesthesia are especially threatened by a number of factors, other than the surgery itself, which arise during such surgical procedures.

[0003] One hazard which requires constant vigilance by the surgical staff to protect against injury is the threat of eye damage. Inadvertent pressure upon the ocular structures of a patient for just a matter of minutes can cause extreme damage or blindness to the eye. As noted above, because the anesthetized patient is in a coma like state, the discomfort of facial compression upon the eye, which would normally cause an awake patient to move and relieve that pressure, fails to alert the anesthetized patient. Care must be taken by an ever alert surgical staff to inspect for possible pressure points about the ocular structures of the patient and to move the patient's face to prevent eye damage.

[0004] Other compression injuries can occur to the anesthetized patient's forehead and chin areas. Here again, the constant pressure upon those areas, caused by the weight of the patient's own head, if not relieved by movement of the face to allow blood flow thereto, can cause localized ischemia to the chin and forehead area. Since the anesthetized patient does not react to the body's cues of discomfort preceding injury, the risk of harm in a matter of minutes to these areas is great.

[0005] An additional concern during surgical procedures of the anesthetized patient is the decrease in body temperature that can occur during surgery. Currently bulky warmed towels and electric blankets are used in an attempt to warm the patient. Such endeavors crowd the operating field and are not easily controlled for tem-

perature.

[0006] Currently, there are a number of conventional methods to support the head and protect the eyes and face of a patient from compression injuries during surgery which require the patient to be placed in a prone, face down, position for the long periods of time involved in surgery. One method conventionally used is placement of the patient's head and face in a horseshoe shaped frame supporting a foam pillow which holds the patient's face off of the operating table in a supported manner. The patient's eyes are generally taped shut when such a structure is used to keep them from contact with the foam and to prevent eye fluid drainage. This frame and pillow support however has inherent hazards of its own in that it cannot distribute pressure maximally over the surface of the head. Further, great care must be taken by the anesthesiologist and staff to make sure that any anesthetic equipment, such as endotracheal tubes, esophageal stethoscopes, or electronic sensing devices, are not dislodged or disrupted by gravity or patient positioning during the term of the surgical procedure. Such disruption or dislodgement of surgical equipment can cut off the air supply to the patient or lead to inaccurate readings by monitoring equipment.

[0007] Another method is simply to place the patient's face sideways on a pillow or towel located upon the surgical table. However, this method suffers from the danger of tubing collapse due to the patient's head weight, and even a face or eye supported by a foam pillow may be damaged if the pressure is uneven and remains on one area too long. Further, the placement of the patient's face on a towel requires the head to be turned one way or the other, placing pressure on one side of the face which, as noted earlier, subjects the patient to the potential of injury. Additionally, blood flow through the veins and arteries of the neck may be impaired by this twisted fashion of head support. Hazards to the patient increase if the surgery requires a face down posture because the danger of tube collapse from pressure or bending increases with the tubes entering the patient's body through the mouth or nose being compressed between the patient's face and the operating table. With the entry points to the head out of view, such constrictions of the tubes also remain out of sight.

[0008] A further challenge facing surgical teams during surgery on anesthetized patients is the seemingly simple task of rolling the patient over from a supine position to a prone position on the operating table or from a cart onto the operating table. Generally, the patient at this point in the surgical procedure is already intubated, asleep, and basically "dead weight." In this physical state, the patient is at great risk of injury during the roll over procedure, especially to the neck area. Additionally vexing to the surgical staff is the fact that the patient, with tubes exiting the mouth and/or nose, must be rolled over, without disturbing the tubes and without injuring the neck. Concurrently during the roll over procedure, the surgical staff must plan ahead so that when the patient is placed face

down on an operating table, the face is properly aligned with, and inserted upon or into the pillow, already located upon the table. This insertion of the face into the pillow is conventionally done without the benefit of a pre surgery fit to make sure the face and pillow and frame mate in a manner that will accommodate the patient for the term of the surgery and protect the face from compression injury. Heads and faces being quite different amongst people in general, an optimum fit between face and pillow is achieved only a small percentage of the time. Once in this prone position, the danger of injury remains constant and continued and consistent vigilance by the surgical staff is required to ascertain, that in fact, the patient's airways are open, the eyes are not compressed, and the face is not being subjected to pressure at any point for a duration sufficient to cause nerve damage.

[0009] Finally, when the operation is over, the patient must again be moved off of the operating table and is generally rolled over onto a gurney in a reverse roll over procedure. Still anesthetized, the patient is at great risk of injury to the neck if the head is not adequately supported and manipulated during this roll over process.

[0010] Still further, if an emergency develops while the patient is in the face down prone position, requiring the patient to be rolled to the supine position, valuable life saving time can be lost trying to upright the patient without injury to the neck, and without crimping the airway supply tubing and monitoring equipment communicating through the nose and mouth of the patient.

[0011] Further, patient size is also a factor in the fitting of facial and head support. A child may have a very small face and head and an adult a large one. Conversely, a large child may have a head and face requiring support in areas much different from a small stature adult.

[0012] U.S. Patent 5,220,699 (Farris) teaches an inflatable pillow mounted inside a mask for variable support of differing sized patients. However Farris requires the use of an inflatable chamber which as taught is inflated once the patient has already been rolled to the prone position. It requires an air inflation device to function and lacks the ability for an easy installation prior to surgery and will not function without compressed air.

[0013] U.S. Patent 4,400,820 (O'Dell) teaches an apparatus using pads and having a "T" shaped void which may be used in combination with a support structure to hold the patient's head. However, O'Dell does not allow for pre-fitting and pre-installing the protective device prior to surgery and does not aid in protecting the patient during roll over on and off the table.

[0014] U.S. Patent 5,214,815 (Agbodoe) teaches a surgical headrest with a removable foam pad; however, Agbodoe does not provide any manner to pre-fit and install the device on the patient prior to being asleep and it mounts to the table and is intended for use after roll over thereon.

[0015] U.S. Patent 4,757,983 (Ray) features a pair of cushions attached to a horseshoe-shaped frame for surgical head support. However Ray also suffers from an

inability to pre-fit and install the device on patients prior to surgery while they are awake as well as lacking any protective ability during dangerous roll over onto the table and like the aforementioned prior art, lacks the ability to see the patient's eyes and face from the side or from above.

[0016] US-A-4,504,050 discloses a head support for examination of a subject who is oriented in a prone position on a platform which includes a base positioned on the platform, at least one flange extending from the base, a faceplate connected to the flange defining a support for cooperating with the face of the subject such that a forehead portion of the subject is supported at a first end portion of the faceplate and a chin portion of the subject is supported at a second end portion of the faceplate while the subject is supported at a second end portion of the faceplate while the subject is in the prone position and a mechanism for adjusting the position of the faceplate with respect to the flange and for controlling the degree of extension of the subject which is necessary for performing the examination of the subject.

[0017] As such, there exists a need for a support device that is easily modified to fit a variety of patients of differing size, and that may be pre-fit to the patient prior to surgery while the patient is alert and able to ascertain the comfort or discomfort level of the device. Further such a device should provide an additional manner to support the head and maximally diffuse pressure over a large area while helping prevent patient thermal heat loss during surgery, as well as during the hazardous movement of the patient prior to and after surgery. Such a device should also provide for easy viewing of the patient's eyes and nose from a side and top view during the operative procedure so that the patient may be continually monitored by the staff.

[0018] A further need exists for such a device that may be cooperatively engaged with a positionable mount or used by itself if needed yet still provide a view of the eyes and ocular area of the patient from looking inward from the side.

SUMMARY OF THE INVENTION

[0019] According to one aspect of the present invention, there is provided a protective helmet apparatus having the features of claim 1. According to a further aspect of the present invention, there is provided a method having the features of claim 7.

[0020] The present invention relates to a new and improved protective helmet apparatus which provided functionally through the ability to vary the configuration for the physical characteristics of patients undergoing general anesthesia during surgery, and provide optimum cranial support to the patient using differing configurations of the various parts of the device. Concurrently, the device, when using a substantially transparent helmet casing and operatively placed apertures provides the medical professionals operating on the patient, easy viewing of the patients facial features and easy access to the

nasal and oral passages of the patient in either the prone or supine position. The device is best made of modular construction allowing for the substantially transparent helmet casing to fit a variety of different sized patients. Interchangeable and replaceable cushions of variable dimensions on one surface to accommodate different patient facial structures are positionaable in a plurality of interchangeable light weight helmet casings. The cushions on their exterior surface are dimensioned for a registered fit with the helmet casing surface and apertures in the cushion register with apertures in the helmet casing. The cushions can also be color coded to designate different sizes to accommodate different sized patients. If desired, while not the best mode for maximum support and positioning, the cushions themselves can be used without the helmet casing, yet still provide a side view of the patient's eyes and temple area during the procedure through an aperture communicating through a sidewall to the face of the patient. Such might be the case in emergencies when sufficient helmet casings are not available or when a low mount of the patient's head is desirable.

[0021] The device is especially useful in that it allows for pre-fitting of the patient while the patient is awake and alert using modular pads of differing facial dimensions and having a rear or mask side dimension configured to fit into a registered position in the helmet casing. While the current best mode combines the proper sized cushion with the appropriate helmet casing for a mount on the table surface, even using the facial cushion by itself, if desired, yields a substantial increase in utility over prior art due to the viewing of the patient's eyes and temple area from the side afforded by the apertures therefor. The device having the pre-fitted cushions or pads mounted into the helmet casing, and featuring appropriate indentations on the facial contact surface, evenly diffuses pressures on the face of the wearer and may be worn into surgery such that the surgical team need not worry about trying to fit the patient with pillows or pads in a table mounted frames after the patient is asleep.

[0022] For use in a variety of patients in prone or supine positions during surgery the various embodiments of the device offer a plurality of ways in which to support the patient's head. One embodiment features a hinged or optionally removable lower chin support which is moveable from a first position in operable contact with the helmet casing to a second position out of such contact, thus allowing the surgical team easy access to the entire face and mouth area for insertion of required tubing into the patients mouth and/or nose. The chin support is thereafter reinstalled to provide lower chin support with the entire helmet being worn by the patient for the rollover procedure on and off the table to protect the patient from injury during the course of the surgical procedure. Or, the chin support may be provided by the cushion itself with the cushion and the helmet casing extending below the mouth area of the patient thus eliminating the detachable chin support.

[0023] As the device may be pre-fitted for optimal

weight diffusion and comfort and can be worn during the movement of the patient on and off the operating table, the surgical team is relieved on concerns of whether the device to hold the face and head actually fits the patient.

Further, an optional rotating handle upon the top of the helmet provides a handy gripping point for the head for the surgical team to help prevent neck injury during roll over of the patient on and off the table. By placement of a hand on the face of the mask and another on the rotating handle, smooth and continual support may be provided to the neck and head area when the patient is being rolled over on or off of the operating table.

[0024] Another embodiment of the device features a helmet casing, which is best made of substantially transparent material, having an interior cavity that is formed to register with a cooperatively engageable cushion. The cushion is made from foam or other soft resilient material and is dimensioned on one surface to accommodate the patient's face, and on the other opposite or exterior surface, to register with the interior cavity of the helmet casing. A raised border about the exterior surface perimeter of the cushion could be formed during manufacture to provide an additional means to register and align the cushion with the openings in the helmet casing. Optionally, the cushions may be color coded for patient facial sizing. One or a plurality of apertures communicating through the helmet casing register with appropriately configured apertures communicating between the two surfaces of the cushion and provide an in line cavity from the patient's face through the casing. This in-line cavity provides access to the patient's mouth, nose, and eyes. By dimensioning the cavity to extend around the patients face at eye level, easy viewing of the patient's eyes and nose is provided to the operating room staff.

[0025] An additional embodiment of the device would feature a plurality of legs on the exterior surface of the helmet casing to provide a raised mount above the operating table. The legs can be adjustable for height above the operating table to provide comfortable posture to the patient while affording the best access and view of the face of the patient to the staff of the operating room.

[0026] In the current best mode, an optional base may also be provided which provides a releasable but solid mount for the helmet casing using cooperating fasteners located on the mount and the exterior of the helmet casing. The mount acts as a positioner by providing a stable mount for the helmet casing and optionally may provide additional utility in the best mode with a surface mounted mirror for providing a reflective view of the patient's eyes and nose to the staff of the operating room while the patient is face down and the staff is substantially in an upright position. This eliminates the constant need for members of the operating team to bend over to inspect the face and eyes of the patient during surgery in providing a continuous view of the eyes and face of the face-down patient. Additional utility is provided by an optional light means positioned on the upper surface of the mount adjacent to the mirror by illuminating the patient's face

through the in-line cavity and enlightening the reflection on the mirror for the staff to more easily view it from a distance.

[0027] An object of this invention is to provide a helmet which prevents injury due to ocular compression during surgery by minimizing ischemic damages through maximal diffusion of pressure about the patient's head.

[0028] Another object of this invention is the provision of a protective device for use during surgery which allows for pre-fit of the patient prior to surgery while the patient may comment on the comfort or discomfort level of the device.

[0029] A further object of this invention is to provide a protective helmet for surgery which provides a facial and chin support to the patient which is easily removable by the surgical team for insertion of required devices into the mouth and nose of patient and thereafter easily re-installed.

[0030] An additional object of this invention is the allowance of easy access to and viewing of, the patients eyes and temple area through apertures in the device positioned to accommodate such access and viewing.

[0031] Another object of this invention is the provision of a protective surgical helmet of modular construction which allows for positioning of different sized facial cushions and components into the helmet casing to accommodate the head different sized patients.

[0032] An additional object of this invention is providing an easily sterilized protective helmet through the use of easily sterilized cushions or inexpensive throw away insertable cushions removably mountable inside an easily sterilized or cleaned helmet shell.

[0033] A still further object of this invention is to concurrently provide easy viewing of the eyes and mouth area of the patient while the device is mounted upon the patient.

[0034] A still further object of the invention is the provision of the ability to control and alter the temperature of the device to aid in temperature control of the patient during surgery.

[0035] An additional object of this invention is to provide easy viewing of the patients facial features to the operating staff using while concurrently allows the staff members to remain substantially upright through the provision of a reflective means of the face of the patient.

[0036] Further objects of the invention will be brought out in the following part of the specification, wherein detailed description is for the purpose of fully disclosing the invention without placing limitations thereon.

BRIEF DESCRIPTION OF DRAWING FIGURES

[0037]

Figure 1 is a perspective frontal view of the protective helmet device showing the chin support in a mounted position.

Figure 2 is a frontal view of the device featuring the

hinged repositionable chin support.

Figure 3 is a rear exploded view of the protective helmet device showing the modular pads for the ocular area and chin support.

Figure 4 shows the helmet with detachable and repositionable chin support portion.

Figure 5 depicts the helmet with detachable and repositionable chin support slidably mountable to the helmet.

Figure 6 depicts a side view of the apparatus showing the optional handle side grip and the flat face for secure positioning on the surgery table.

Figure 7 depicts another embodiment of the device featuring an exploded view a helmet casing of unitary construction with insertable modular pad providing facial and chin support in a single combined unit.

Figure 8 depicts the helmet casing of figure 7 in a registered position removably or otherwise attached to a mount with optionally mirrored surface for reflection of the patient's face therein.

Figure 9 is a top perspective view of the facial cushion showing the facial indentation and apertures therethrough.

Figure 10 depicts and end cut away view of the facial cushion for removable mounting to the helmet casing showing the facial indentation formed to accommodate patient facial structures therein, and the lip for registration with the casing edge.

Figure 11 depicts a bottom perspective view of the helmet casing showing the unitary construction and the legs affixed to the exterior which provide an elevated mount along with the communicating aperture through the casing.

Figure 12 depicts a top view of the mounting base for the helmet casing with a surface mounted mirror and light source.

Figure 13 depicts a side view of the mounting plate with a mirror and cooperatively engageable mounts on the upper surface.

Figure 14 is a top view of the upper surface of the mounting plate showing the mirror and mounts.

Figure 15 is a tope view of the removably attachable heating blanket with temperature control and clip.

DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENTS OF THE INVENTION

[0038] Referring now to the drawings, Figure 1 depicts a preferred embodiment of the modularly assembled protective surgical helmet apparatus **10** featuring the helmet casing **12** which is best made from a substantially rigid but easily molded material such as plastic. The plastic casing should also be resistant to the heat or chemicals sufficient to allow for sterilization between uses. The modular version of the helmet casing **12** mates with a chin support **14** using conventional registering mating positioners such as registration pins **16** which correspond to apertures **18** upon the helmet casing **12**. Of course

the registration pins **16** and apertures **18** might be reversed in positioning or other conventional means of registration and dismountable attachment may be used to achieve a properly aligned mounting of the chin support **14** to the helmet casing **12**. Alternatively, the chin support **14** can be slidably mounted to the helmet casing **12** using a cooperating pair of slide mounts **53** and **51** depicted in figure 5 wherein the chin support **14** with one half of the fastener slid mount **53** would be lined up with the helmet casing **12** and cooperating slide mounts **51** and **53** and thereupon the chin support **14** would slide onto the helmet casing **12** by pushing it into position and interfacing the cooperating slide mounts **51** and **53**. Cooperating fasteners **20** and **22** in the two-piece embodiment, such as hook and loop fabric, are used to maintain the chin support **14** in operative contact in a first position wherein it is in a removably fixed position upon the helmet casing **12**, however, other conventional mating fasteners such as plastic or metal releasable locking fasteners can also be used and are anticipated. Cooperating fasteners **20** and **22** would also be used to maintain the hinged chin support **14** and slidable chin support **14** in the first position of operable and registered contact with the helmet casing **12** although in the case of the slidable version friction alone in the cooperating slides may be sufficient to releasably hold the chin support **14** in proper contact with the helmet casing **12**.

[0039] The dismountable chin support **14** may also be attached to the helmet casing **12** at one end using a conventional metal or plastic hinge fastener **34** such that the chin support **14** will swing away from its first position in operative contact in a registered mounting with the helmet casing **12**. This embodiment allows for easy access to the patient's facial area during surgery or emergencies while maintaining the chin support attached to the helmet casing **12** when swung to the second position out of operative contact with the helmet casing so as to avoid loss of the chin support **14**.

[0040] Straps **24** having cooperating fasteners **25** at their distal ends securable to mating cooperating fasteners **25a** upon the helmet casing **12** may be optionally used to secure the helmet casing **12** upon the face of the patient once the properly sized ocular cushion **26** has been removably mounted into the helmet casing **12**.

[0041] In certain instances the helmet casing and chin support might also be formed as one piece for surgeries where a removal of the chin support **14** is not a major consideration and for ease of use and reduction in parts to inventory. In such a one piece embodiment the support to the face of the patient provided by the ocular cushion **26** and chin cushion **28** would be provided by a single once piece facial cushion **31** which is configured to removably mount into a one piece embodiment of the helmet casing **12** in a registered position, therein thereby providing stable even support the entire face of the patient from forehead to chin. In the one piece version of the helmet casing **12** the front surface would be extended to a point below the chin and thereby accommodate a

once piece facial cushion **31** and apply complete support to the head of a patient.

[0042] The ocular cushion **26** and chin cushion **28**, or one piece facial cushion **31**, if reusable, are best made of a closed cell foam material or other cushioning material which does not absorb fluid easily to allow the cushions to be sterilized in the conventional fashion for reuse. In many instances sterilization may not be necessary and a simple washing may provide the required level of cleanliness. In such cases the material used will be durable for reuse and resistant to cleaning to allow multiple uses of the cushions **26**, **28**, or **31**. However, for ease of use and to maintain a highly sterile field about the patient, disposable ocular cushions **26**, chin cushions **28**, and one piece facial cushions **31** may be more desirable since they could be used once and replaced after each operation to maintain a highly sterile or sufficiently clean field. The best mode as to disposable or reusable is best determined by the criteria of the hospital or surgery center involved and their individual criteria.

[0043] Optionally, for an even more custom fit to individual patients is desirable, the ocular cushion **26** and chin cushion **28** or the once piece facial cushion **31** may also be made inflatable with gas or fluid or silicone or other gel such that they may be adjusted in size and flexibility by filling them with a gas or liquid into the cushions through a sealable orifice communicating through the wall of the cushion.

[0044] The ocular cushion **26** may be made in a set of multiple ocular cushions **26** varied in dimensions of both thickness and width and have variable sized and located ocular apertures **27** therein to best accommodate the size and facial structure of a variety of differing sized individuals using the same helmet casing **12**. The chin cushions **28** may also be from a set of such chin cushions **28** varied in dimensions of both thickness and width to achieve optimum fit on individual patients. The one piece facial cushion **31** used with the one piece embodiment of the helmet casing **12** provides the same adjustable utility and can be varied in the same fashion by providing multiple facial cushions **31** for use as a kit to be combined with one piece helmet casing **12**. The facial cushion **31** has a facial indentation **59** formed on a first side of the facial cushion **31** sized to accommodate the face size of the intended patient. The opposite side or exterior surface **38** of the facial cushion **31** would be dimensioned for cooperative engagement with the interior surface **35** of the one piece embodiment of the casing **12**. By varying the dimensions of the cushions **26** and **28** or **31**, and the size and location of the apertures therein, and matching them to the properly sized one or two piece helmet casing **12**, virtually any adult or child may be fitted to wear the resulting assembled device **10** comfortably with optimal support of the facial structure of the cranium and maximal diffusion of pressure and weight about the face and sides of the patient's head to obviate injury to the eyes and face and nerves.

[0045] In the two-piece embodiment, the ocular cush-

ion **26** and the chin cushion **28** are attached to the helmet casing **12** and repositionable chin support **14** respectively, using a means of attachment such as corresponding mounts **32** formed of hook and loop fabric or adhesive pad fasteners mounted on the cushions **26** and **28** in positions to contact corresponding cooperating mounts **33** on the respective interior surfaces **35** and **36** of the helmet casing **12** and chin support **14**. However, adhesive mounting does not require using cooperating mounts **32** and **33**. In this manner using adhesion, adhesive, two-sided tape, adhesive pads, adhesive covered by an easily removable paper, or similar conventional adhesive attachments can be placed between the cushions **26** and **28** and the inside faces of the helmet casing **12** and chin support **14**. A frictional engagement between the facial cushion **31** and interior surface **35** of the one piece embodiment of the helmet casing **12** would also provide a means of attachment therein using the weight of the patient's head to maintain registration of the facial cushion **31** in the casing **12** and in such a use of components optional retaining tabs **43** could be provided as an additional means of attachment of the facial cushion **31** to the helmet casing **12** to insure that it stays registered therein.

[0046] When using a disposable form of cushions **26** and **28**, and **31** adhesive or other means for a removable attachment can be placed upon the helmet side of the respective cushion surface for an easy mount of the cushions into the helmet casing **12** and/or repositionable chin support **14**. Such a disposable form of cushions **26**, **28**, and **31**, would be kept sterile inside a sealed wrapper in the conventional manner and removed and mounted to the inside face or interior surfaces **35** and **36** of the helmet casing **12** and chin support **14** respectively as necessary in the configuration decided upon, using conventional peel and stick adhesive pads positioned upon the surface of the cushions to attach them to the helmet interior surface **35**.

[0047] The device **10** offers great utility to the user since it is capable of using either disposable or reusable cushions for cushions **26**, **28**, or **31**, or combinations thereof at the discretion of the professional using the device. Where disposable cushions are desirable due to their ease of use and lack of the need for sterilization, just the helmet casing **12** and chin support **14**, if used, need be sterilized. Or, in the case of the once piece casing just the casing need be sterilized if required. However, a reusable form of cushions **26**, **28** and **31** may also be used in the device **10** where the cushions can be sterilized between use, or, in instances where sterilization is determined not to be needed they need only be washed. Or, a combination of reusable and disposable cushions **26**, **28** and **31** may be used should such be desired or required if a reusable cushion is lost or damaged.

[0048] In use, with the two-piece embodiment, the patient would be measured for the optimum helmet casing **12** size which would be chosen from a plurality of available interchangeable helmet casings available, and, a

chin support **14** of proper size which would be chosen from a plurality of interchangeable chin supports capable of attachment to said casing **12**. Also chosen to accommodate differing facial and head dimensions would be the properly dimensioned cushions **26** and **28**, from a set of interchangeable cushions, to allow the patient maximum comfort and diffusion of pressure about the surface of the face and side of the head. The patient could be given samples of the different sizes of cushions **26** and **28** from a set of variable dimensioned cushions **26** and **28** to which the patient would give input as to the best possible fit or a medical technician might also help determine the optimum casing and cushion dimensions with or without the patient's input. This availability of an assortment of cushions and assembled helmet sizes allows for a modular system of helmet casings **12** and attachable chin supports **14** assembled to the helmet, to be used in conjunction with the desired dimension of cushions **26** and **28**, also from a set of such cushions of differing dimensions, to achieve the optimum fit on a variety of sizes of patient heads.

[0049] Once the optimum dimensions of the cushions **26** and **28** are determined, yielding a comfortable fit and maximal pressure distribution about the face and sides of the head, the cushions **26** and **28** are removably mounted into the interior of both the helmet casing **12** and chin support **14** using the aforementioned adhesive or fastener cooperating mounts **32** located upon the cushions which attach to cooperating mounts **33** which are positioned upon the helmet casing **12** and chin support **14** respectively. This is accomplished in a manner to allow for the mounting the cushions **26** and **28** into the cooperatively configured interior surfaces **35** and **36** of the helmet casing **12** and chin support **14** respectively.

[0050] The inside surface **35** of the helmet casing **12** features a casing ocular aperture **37** and the chin support **14** has a chin support aperture **39**. When properly positioned in the cooperating inside faces of the helmet casing **12**, the aperture **27** in the ocular cushion **26** will be relatively in line with the casing ocular aperture **37** such that the eyes and nose and some surrounding portions of the patient's face, or the ocular area of a patient's face, may be easily viewed through the ocular aperture **37** when the device **10** is being used during surgery after being positioned upon the patient's face. The ocular aperture **27** might best be made slightly larger than the casing ocular aperture **37** to allow for easy mounting of the ocular cushion **26** into the helmet casing **12** to allow for the patient's eyes and surrounding skin area to be viewed through the casing ocular aperture **37** and relatively in-line cushion ocular aperture **27**. Where the casing ocular aperture **37** wraps around to the side of the helmet casing **12**, the in-line ocular cushion aperture **27** would also wrap around in a relatively in-line position with the casing ocular aperture **37**. This in line relationship of apertures creates a viewing passage communicating through the helmet casing **12** and apertures **37** and **27** thus revealing the patient's temple area of the head in addition to the

ocular area of the face and the nose. This in line relationship of the apertures of the cushions **26** and **28** with the casing apertures **37** and **29** also allow for the passage of conventionally used tubes through the in line apertures into the patient's nose and/or mouth for providing life support during the operation. Further, the cavity formed by the in line cushions **26** and **28** attached to the helmet casing **12** and chin support **14** gives protection to these tubes at the critical entry and exit positions on the patient at the nose and mouth such that the tubes, inside the cavity, will not bend to a point where flow therethrough is interrupted with possible life threatening consequences to the patient. For additional utility, optional tube passages **44** communicating a tubular passageway from the interior of the device **10** to the exterior, can provide for communication of tubes or sensing device wires there-through to the patient. Exterior mounted optional tube positioners **46**, of hook and loop fabric or other type of fastener suited to the job, can be optionally mounted upon the exterior of the device **10** to hold tubing and/or wires for monitoring the patient operatively therein during surgery. Snap on fasteners may also be optionally attached at the exterior of the device **10** to hold tubing and the like. By providing optional strategically placed snap mounts **48** the snap on fasteners may be placed in differing positions about the exterior to hold the tubing and/or wiring required for certain surgical procedures in place and out of harms way.

[0051] The chin support aperture **39** of the two-piece embodiment lines up with the bottom of the casing ocular aperture **37** when the dismountable chin support **14** is operably mounted to the helmet casing **12**. The chin support aperture **39** allows for viewing and access to the lower mouth area of the face of the patient with the chin of the patient being supported by the chin aperture **39** in chin cushion **28** removably attached to the interior surface **36** of the chin support **14**.

[0052] Added utility is provided by the device **10** operably mounted to the face of the patient using attributes of the frontal surface **41** of the device **10**. This frontal surface **41** if made flat like that of the upper table surface **64** of a conventional operating table, allows for a stable support of the patients face inside the properly mounted device **10** when the frontal surface **41** is placed upon the operating table without a mount if such a positioning is desired. For especially stable maintenance of the patient's head when in a sideways position a second side flat surface area on the sidewall **47** area may be located on one or both sidewalls **47** of the device **10**.

[0053] Or, as depicted as the one-piece embodiment of the device in figure 7, legs **60** attached to the casing exterior surface **49** can provide both a means for elevation of the helmet casing **12** above the couplings **62** on the mounting plate **66** and underlying table surface **64** and if desired, registration using at least two of the couplings **62**. The couplings **62** as depicted, are dimensioned to cooperatively engage the distal ends of the legs **60** and can be mounted directly to the operating table sur-

face **64** using a means for attachment to the operating table surface **64** such as adhesive **65**, frictional engagement, or other means of attachment to the table surface **64**. Or in the current best mode a mounting plate **66** would have the couplings **62** mounted thereon positioned to provide a registerable mount through cooperative engagement with an axial leg aperture **63** in the distal end of the legs **60**. Insertable leg extensions **61**, made of differing lengths to achieve the desired elevation, provide an adjustable means for elevation would fit between the leg apertures **63** and onto the couplings **62** providing a means for height adjustment of the helmet casing **12** above the underlying table surface **64** to accommodate various posture positions for the patient's head and neck.

[0054] The single piece embodiment of the helmet casing **12** features a front wall surface **41** which extends laterally and then curves to a pair of side walls **47** both of which begin at one side with their communication with the front wall surface **41** and extend vertically at an acute angle from the front wall surface **41** to form the two substantially parallel sidewalls **47**. In this embodiment the casing ocular aperture **37** in the current best mode, is enlarged and extended around and through the front wall surface **41** and upward onto and through at least one side surface **47** of the helmet casing **12** providing a clear view of the patients eye, and face in the temple area, as well as the area in front of the nose, from one or both sides of the device **10**. Extending the casing ocular aperture **37** and the cushion ocular aperture **27** up at least one sidewall **47**, whether they are used in combination or when the cushion might be used by itself, thus provides a means to view the eye socket and surrounding area through the sidewalls **47** of the device of the patients who might use the device. In the current best mode, the ocular apertures of both the once piece helmet casing **12** and the facial cushion **31** extend up both sidewalls **47** to provide a viewing passage **82** of both eyes and the surrounding temple area of the head of the patient through the sidewalls **47**. Viewing of the temple area is also achieved through the transparent material making up the helmet casing **12** and would allow for a larger ocular cushion aperture **27** to provide more of a view of this area thus allowing even greater viewing of the patients eye area much like a window.

[0055] During times of moving of the patient for roll over or off of the surgical table and onto a gurney, an optional top handle **40** attached to the top area of the helmet casing **12** portion of the assembled device **10** allows medical personnel a solid gripping point for providing head and neck support to the patient while being rolled over or otherwise moved. By holding the patient's neck with one hand and the handle **40** in the other, essential support can be provided to avoid injury to the anesthetized patient. A roller or ball or other conventional bearing **42** can also be placed at the base of the handle **40** should easy rotation of the handle **40** be desired during use. Such a rotation of the handle **40** on the bearing **42** allows for a smooth roll over of the patient with the pa-

tient's neck concurrently supported, thus minimizing possible neck injuries during roll over and other hazardous patient relocation procedures.

[0056] Additional utility in the disclosed apparatus herein is provided by the insulating factor provided to the patient wearing the surgical helmet **10** and cushions **26**, **28**, and **31**, when mounted upon the face of the patient during a surgical procedure. Operating rooms are conventionally kept quite cold to keep medical personnel and surgeons cool and alert during surgical procedures. The patient however is generally unclothed during such procedures and can suffer discomfort from the overly cool environment of the room. The cushions **26**, **28** and **31**, form to the face of the patient and are mounted upon the interior surface **35** of the device **10**, and thereby encompass the face and part of the sides and top of the head of the patient. The result being that the face, sides, and top of the patient's head are insulated from the cool room temperature, helping to keep the patient warmer in the unnaturally cool environment of the operating room.

[0057] Further utility is also provided by this surgical helmet device **10** through the use of optional slot passages **45** located in the face of the device for positioning of tubes therein. During a surgery requiring the patient to lay face down, tubes providing breathing supplies to the patient may be positioned in a slot configured to allow the tube to recess therein such that the tube will not collapse when the patient is face down and the tube is between the table and casing exterior surface **49** of the device **10**. Such a slot passage or multiple slot passages **45** may be positioned about the face of the helmet in other locations than shown.

[0058] Figure 7 depicts a preferred embodiment of the device **10** featuring an exploded view showing the helmet casing **12** of a one piece or unitary construction. In this embodiment, the casing walls are best constructed of rigid substantially transparent material such as plastic in a unitary construction. This embodiment provides the same desired support for the chin and face provided by the two-piece embodiment accomplishing this support with a cooperatively engageable once piece facial cushion **31**. This one piece embodiment continues to provide proper chin and face support by slightly elongating the helmet casing **12** in a one piece design and combining the ocular cushion **26** and chin cushion **28** into a one piece facial cushion **31** which is dimensioned on the exterior surface **70** of the facial cushion **31** for cooperative engagement with the interior surface **35** of the helmet casing **12**. The facial cushion **31** is dimensioned on the interior surface **69** to provide a comfortable fit to the face of the patient for which it is to be used. In use, in essentially the same manner as the two-piece embodiment, the intended patient would be measured for the optimum facial cushion size **31** which would be chosen from a plurality of available interchangeable facial cushions **31** available for registered cooperative engagement with the one piece helmet casing **12**.

[0059] In many cases only one or two different sized

helmet casings **12** would be needed in inventory to be mated with cushions to accommodate a very large number of differently dimensioned facial cushions **31** since the size, thickness, and exterior and interior dimensions of the facial cushion **31** may be varied to accommodate the different facial dimensions of different patients. This is accomplished by the variance of the dimensions of the indentations **68** formed on the interior surface **69** of the facial cushion **31** which are used to accommodate the facial dimensions of the intended patient. The exterior surface **70** of the facial cushion **31** would be dimensioned for operative cooperative engagement with the shape and dimensions of the interior surface **35** of the helmet casing **12** in the aforementioned registered and cooperative engagement therein.

[0060] The registration and cooperative operative engagement between the cushion **31** and helmet casing **12** would be maintained using a means for registered engagement of the facial cushion **31** with the helmet casing **12** which includes one, or a combination, of registration means, from a group of such registration means consisting of frictional engagement between the interior surface **35** of the helmet casing **12** and exterior surface **70** of the facial cushion **31**, adhesive **65**, a lip **71** located about the upper exterior surface **70** of the facial cushion **31** in a position to cooperatively engage the upper edge **75** of the sidewalls **47** of the helmet casing **12**, or, registration pins **73** attached to the body of the facial cushion **31** in positions to cooperatively engage registration apertures in the casing, in this case axial passages **77** formed into the legs **60** and sized to accept the registration pins **73** in a removable cooperative engagement. Since the registration pins **73** would in the current best mode be molded of the same flexible foam as the facial cushion **31** they offer the current best mode of registration since the registration pins **73** will compress during insertion into the axial passages **77** and then naturally bias against such compression into removable biased frictional engagement with the interior of the axial passages **77**. While the aforementioned are the current best mode of a registration means between the facial cushion **31** and the helmet casing **12**, those skilled in the art may devise other such means of registered engagement and such are anticipated.

[0061] In fitting the patient for maximum comfort and support, the patient could be given samples of the differently dimensioned facial cushions **31** from an available plurality or set of variably dimensioned facial cushions **31** to which the patient would give input as to which formed indentations **68** provide the best possible fit to the facial dimension of the patient. Or, a medical technician might also help determine the optimum helmet casing **12** and facial cushion **31** dimensions with or without the patient's input. This availability of an assortment of differently dimensioned facial cushions **31** to cooperatively and operatively engage one or a plurality of helmet casings **12**, allows for a kit or modular system of helmet casings **12** and attachable to facial cushions **31** to

achieve the optimum fit on a variety of sizes of patient heads. For easy identification of size the facial cushions **31** would be marked with appropriate indicia **30** in writing showing a size designation or in the best current mode with indicia in the form of color coding for easy identification. The color coding or written indicia **30** to identify size could be imparted by extruding it in the color of the foam making up the facial cushion **31** or silkscreened or otherwise applied on the surface of the cushions **26**, **28**, and **31**. Once the optimum dimensions of the facial cushion **31** are determined, yielding a comfortable fit and maximal pressure distribution about the face and sides of the patient's head, the facial cushion **31** is removably mounted to the interior of the helmet casing **12** using the aforementioned means for registered engagement of the facial cushion **31** with the helmet casing **12**.

[0062] The one piece facial cushion **31** offers an additional benefit in that in some cases it might be used without the helmet casing **12**. Use without the casing might occur when an especially low mount of the patient's head is desired for posture or for the surgical procedure, or, in an emergency or other situation where the additional support and utility of the in-line helmet casing **12** is not required. Use of the facial cushion **31** by itself, while not offering the full utility of the best mode in combination with the helmet casing **12**, does provide the easy side viewing of the patients eyes through the elongated ocular cushion aperture **27** and still provides improved support and padding to the patient's head during surgery. Consequently, it is anticipated that the cushion might be used alone without the casing **12**, and while not providing all of the utility of the device featuring the combination of the facial cushion **31** with the helmet casing **12**, using the cushion alone would still provide much better support to the patient's face, a clear view of the eyes through the elongated cushion ocular aperture **27** and a solid support to the patient's head on the table through frictional engagement therewith.

[0063] Or, in some cases, where reuse of the cushion may not be advisable due to the patient, the helmet casing **12** might also be formed into the exterior of the facial cushion **31** itself. This could be done if a substantially rigid shell **80** were formed about the exterior surface **70** of the facial cushion **31** by either lamination thereto or in the molding process and would provide rigid support to the facial cushion **31**. However this configuration with the helmet casing **12** as attached to the facial cushion **31** as a laminated or permanent shell yields less utility in that different facial cushions **31** for different sized patients could not be matched to a single helmet casing **12** thus requiring more stock of product. But, differing user criteria and requirements may call for the facial cushion **31** to be thus used and manufactured with a casing formed by the rigid shell **80** formed on the outside surface for use without the additional advantages afforded by mating with the helmet casing **12** and such is anticipated. While the current best mode of the device, affording the most utility, is the registered engagement of a properly sized facial

cushion **31** with the helmet casing **12**, the cushion-only embodiments offer the operating staff the option to use the facial cushion **31** without the helmet casing **12** and still achieve much better support of the patient's head, thermal insulation and view of the patient's eye and surrounding temple area **74** which is a marked improvement to the current practice of placing the head on a towel. The very nature of the exterior surface **70** of the soft foam facial cushion **31** would provide a good frictional mount to the surface of the table surface **64** and good side and frontal support to the head of the patient with a concurrent view through the elongated casing ocular aperture **37** reaching around the side to allow a view of the patient's eye socket from an operative distance. Use of the facial cushion **31** could also occur if there were a shortage of helmet casings **12** for the number of patients requiring surgery during an emergency situation. Consequently it is anticipated that the facial cushion **31** could be used by itself in certain instances and would still be a substantial improvement for a mount and support of the patient's head than the present art.

[0064] To provide an excellent view of the patient's facial features, as with the two piece embodiment, the interior surface **35** of helmet casing **12** features a casing ocular aperture **37** communicating through the casing front wall **41** surface and side walls **47** and the chin support aperture **39** formed into the front wall **41** surface and communicating therethrough. The one piece embodiment the helmet casing **12** as noted also features an elongated casing ocular aperture **37** which wraps around the helmet casing **12** to determined termination points in one or both substantially parallel side walls **47**, and thus allow for easy viewing of the eye area of the patient during use by looking through the in line casing ocular aperture **37** and cushion ocular aperture **27**. In the one piece embodiment this casing ocular aperture **37** communicates with the chin support aperture **29** to yield a somewhat figure eight shaped aperture when the casing is viewed from the bottom. The in line ocular cushion ocular aperture **27** where it intersects the cushion chin support aperture **39**, yield a nose cavity **57** the area of which is defined by the thickness of the wall surface of the facial cushion **31** and the perimeter of the intersecting chin support aperture **39** and the cushion ocular aperture **27**. Along with providing a passageway for tubes to the patient, the nose cavity **57** also yields a good view of the nose and facial area around the nose when the patient is in the prone position, providing additional utility to the device.

[0065] When properly positioned, the cooperating engagement of the facial cushion **31** and helmet casing **12**, will place the cushion ocular aperture **27** substantially in line in a registered position in relation to the casing ocular aperture **37**. The ocular cushion ocular aperture **27** might best be made slightly larger than the helmet casing ocular aperture **37**. This slight increase in size provides for easy mounting of the facial cushion **31** into the helmet casing **12** to a position to allow the patient's eyes and surround-

ing skin area to be viewed through the wrap around casing ocular aperture **37** and relatively in-line cushion ocular aperture **27**. When the helmet casing **12** is substantially transparent material, as in the current best mode, the increased size of the apertures of the facial cushion **31** also increase the area around the eyes and nose of the patient that can easily be viewed since these areas may be viewed through the helmet casing **12** itself.

[0066] As noted, in the current best mode, the casing ocular aperture **37** wraps around from the front to both sides of the helmet casing **12**. The ocular cushion aperture **27** would also wrap around substantially the same such that when mounted it would engage the casing ocular aperture **37** in a relatively in-line position, registered with the ocular casing aperture **37**. A viewing passage **82** provides a means to view the eyes and nose and some surrounding portions of the patient's face through the sidewall **47** is thus defined and provided by the in-line relationship of the wrap around facial cushion ocular aperture **27** and the casing ocular aperture **37** and the cushion chin support aperture **39** and the casing chin aperture **29** thus forming the viewing passage communicating through the helmet casing **12** and the apertures in the facial cushion **31** providing an excellent view of the patient's temple area of the head in addition to the ocular area of the face and a nose cavity **57** for accommodating and viewing the nose from both sides of the device and well as from below the device when mounted on the operating table. This in-line relationship of the cushion apertures **27** and **39** with the casing apertures **37** and **29** also allows for the passage of conventionally used tubes through the in line apertures into the patient's nose and/or mouth for providing life support during the operation.

[0067] Figure 8 depicts the facial cushion **31** inserted and registered in position with the helmet casing **12** which is in a registered position removably attached to an optional mount plate **66** using couplings **62** configured to cooperatively engage the distal ends of the legs **60** which are attached to the helmet casing **12** at their opposite ends. The couplings **62** are depicted as pins that insert into indents in the legs **60** but this arrangement could be reversed with the legs positionable into indents in the mounting plate **66** or other means for attachment of the legs **60** to the couplings **62** could be used and are anticipated. If needed to adjust the height of the helmet casing **12**, and thus the height of the head of the patient for comfort or function, one or a plurality of leg extensions **61** may be used to adjust the height as desired. The leg extensions **61** would of course be configured to operatively engage in a fit between the legs **60** and the couplings **62**.

[0068] The couplings **62** alone using adhesive or other manner of attachment could be pre-installed to the operating table surface **64** in cases where the optional mounting plate **66** is not desired, however in the current best mode, the mounting plate **66** positioned on the operating table surface **64** would provide the couplings **62** attached in positions to cooperatively engage the distal

end of the legs **60** to thereby provide a stable means of elevated attachment of the helmet casing **12** above the table surface **64** in registered engagement with the mounting plate **66**.

[0069] By the provision of a means for elevation, through the provision of legs **60** to slightly elevate the helmet casing **12** above the operating table surface **64**, and the means for elevation adjustment using the leg extensions **61**, or other manner of extending the length of the legs **60** such as telescopic legs, or legs extending with pins to hold the elongation of the legs, better patient posture is achieved by keeping the patient's neck in line. Elevating the helmet casing **12** and patient therein also elevates the casing ocular aperture **37** and casing chin aperture **29** thereby allowing better views therethrough of the patient for direct viewing by the staff. The casing ocular aperture **37** being extended around the frontal area and communicating between the casing interior surface **35** and casing exterior surface **49** and extending to the side area of the helmet casing **12**, provides an easy and clear view of the patients eye and temple area **74**. For additional utility, the aforementioned optional tube passages **44** could be operatively positioned in the once piece embodiment of the helmet casing **12** to provide a tubular passageway from the interior of the device **10** to the exterior for the various devices requiring such.

[0070] While elevating the helmet casing **12** provides extra room between the table and the in-line apertures to allow better viewing of the patient from the side and below, in the current best mode, the placement of a mirrored surface **72** on the upper surface **67** of the mounting plate **66** provides additional utility through the provision of a means for the upright operating staff to view of the patients eyes and temple area around the eye, through the in line ocular and chin apertures **29** and **37**. Normally the doctor or staff member wishing to view the patient's eyes area adjacent to the eye temple area **74** or face would have to stoop to an angle wherein they can be seen through the in line apertures in the helmet casing **12** from the side, or in some cases from below the operating table. However, with the provision of a mirrored surface **72**, operatively placed on the upper surface **67** of the mounting plate **66**, the doctors and staff are afforded a means for a continuous real time view while standing, of the patient's eyes and mouth through the apertures **37** and **29** in the helmet casing **12**. Should even more adjustability of the reflection be desired so that certain staff in certain positions can see the patient's eyes and mouth, a means for angular adjustment of the mirrored surface **72** could be attached between the mounting plate **66** and the mirrored surface **72** such as a ratchet **78** or other conventional means for angular adjustment that will provide the user with the ability to adjust the angle of the mirrored surface **72** from substantially parallel to the mounting plate **66** toward a position normal to the mounting plate **66**. The mirrored surface **72** with the means for angular adjustment thus may be positioned to an infinite number of angles between positions parallel and normal

to the mounting plate **66**. Such adjustment provides substantial utility to the operating room staff and doctors by allowing them to adjust the mirrored surface **72** to obtain the best possible view of the patient through the in line apertures of the facial cushion **31** and helmet casing **12**.

[0071] Should additional enhancement of patient viewing be desired, the addition of the optional illumination means in the current best mode in the form of light **76** which further enhances the reflected view in the mirrored surface **72** by illumination of the patient's facial features which reflect in the mirrored surface **72**. The illumination means could be a conventional light bulb, a light emitting diode, or other similar light sources and can be powered by conventional AC or battery power that is readily available in the operating arena.

[0072] Construction of the one piece embodiment of the facial cushion **31** and the various options thereto, is best depicted in figure 9 and Figure 10. As shown from the top perspective view of figure 9, the indentations **68** to accommodate various sized faces and facial structures are operatively positioned and provide excellent head support in the form of a forehead support **54**, cheek supports **55** and chin support **56**. The registration pins **73** protrude from the exterior surface **70** in positions to register the facial cushion **31** in operative engagement with the leg axial passages **77** extending axially through the legs **60** of the one piece embodiment of the helmet casing **12**. Registered insertion of the facial cushion **31** into the helmet casing **12** is thus easily achieved by the in line cooperative engagement of the registration pins **73** with the axial passages **77** in the legs **60**. Of course the other aforementioned means of registration of the facial cushion **31** with the helmet casing **12** might also be used including the lip **71**, adhesive **65**, or frictional engagement of the exterior surface **70** of the facial cushion **31** with the interior surface of the helmet casing **12**. In cases where the additional utility of the helmet casing **12** encompassing the facial cushion **31** is not required the facial cushion **31** could be used alone in a frictional engagement with the surface of the table surface **64**.

[0073] Figures 11 and 12 provides a bottom perspective view and a top perspective view respectively, of the one piece embodiment of the helmet casing **12**. As shown, the legs **60** contain the axial passageway **77** therein communicating with an leg aperture **63** at each end for registered engagement of the molded registration pins **73**. The elongated casing ocular aperture **37** in the one piece casing extends across the bottom and up both sides of the one piece helmet casing **12**, and communicates with the chin aperture **29** to form a single large "I" or figure eight shaped aperture which registers in an in-line relationship with a similar shaped and slightly larger aperture in the one piece facial cushion **31**. Also depicted are a pair of optional tube passageways **50** providing communication to the interior of the helmet casing **12** through axial tube passages **52** therein.

[0074] A preferred embodiment of the mounting plate **66** component is depicted in figures 13 and 14. The

mounting plate **66** in the current best embodiment is constructed of rigid plastic such as polycarbonate which is substantially transparent. A plurality of couplings **62** are attached to the upper surface **67** of the mounting plate **66** to provide the registered mount for the legs **60** of the helmet casing **12**. In this embodiment, rather than having the mirrored surface **72** on the upper surface **67** of the mounting plate **66** the mirrored surface **72** is adhered to the bottom surface **83** of the mounting plate **66**. Adhering the mirrored surface **72** to the mounting plate bottom surface **83** facing upward toward the tope surface, allows the mirrored surface **72** to provide the desired reflection of the patients face through the substantially transparent plastic material of the mounting plate **66** while concurrently protecting the mirrored surface **72** from scratching. In this embodiment the mirrored surface **72** may be adhered to the bottom of the mounting plate **66** by using mirror attached into an indent in the bottom surface **83** or by applique of a metalized or reflective surface to the bottom surface **83** such that when viewed through the substantially transparent material making up the mounting plate **66** from the upper surface **67** a reflection is provided. The depicted optional outwardly biased conventional plunger ball **85** would provide additional stability to the couplings **62** in their cooperating engagement with the legs **60**.

[0075] Additional utility during procedures where the temperature of the patient is a concern is provided by the optional removably attachable means for heating the head of the patient. In the current best embodiment the means for heating the head of the patient is provided by a removably attachable heating blanket **87** as depicted in figure 15. The heating blanket is removably attachable to the helmet casing **12** using biased clip **90** which is spring loaded and attaches to an upper edge of the helmet casing **12**. The heating blanket **87** provides heat using a resistive element **92** which heats the blanket body **93** when power from an electrical power source **94** is communicated thereto through conventional wires **96**. The heat is distributed evenly by the serpentine arrangement of the resistive element **92** thus avoiding hot spots. Control of the amount and duration of heat would be provided by a conventional thermostat **98** engagement with the resistive element **92** to break the circuit when the desired temperature is obtained. The wires **96** might also be a flat strip style wire that is applied to the exterior surface **70** of the helmet casing **12** and an interface on the clip **90** such that attaching the clip **90** to the helmet casing **12** would also provide power to the blanket **87** through the interface in the clip **90**. Alternatively, in some cases it may be more advantageous to attach the resistive element **92** by affixing it or appliqueing it to the interior surface of the helmet casing **12** in between the facial cushion **31** and the helmet casing **12** where it would work in the aforementioned fashion but provide heat to the face of a prone patient or the back of the head of a supine patient using the disclosed device.

[0076] While all of the fundamental characteristics and

features of the protective cushion and cooperatively engageable helmet casing for anesthetized patient have been shown and described, it should be understood that various substitutions, modifications, and variations may be made by those skilled in the art without departing from the spirit or scope of the invention. Consequently, all such modifications and variations are included within the scope of the invention as defined by the following claims.

Claims

1. A protective helmet apparatus (10) comprising: a facial cushion (26,28,31) for providing stable patient cranial support during surgery for an anesthetized patient in a prone position, said facial cushion (26,28,31) having a front portion, an interior surface and an exterior surface; said interior surface of said cushion dimensioned to accommodate the facial structure of a human being; at least one cushion ocular aperture (27) in said cushion communicating laterally across said front portion, said ocular aperture providing communication between said interior surface and said exterior surface; **characterised in that** said facial cushion (26,28,31) has two cushion sidewalls extending upward from said front portion, said cushion ocular aperture (27) forms a viewing passage (82) continuing up both of said cushion sidewalls and providing a view through said cushion sidewalls, wherein one of the two eyes of a patient wearing said cushion while in the prone position, may be seen through said viewing passage from a position adjacent to either said two cushion sidewalls, thereby allowing both of said patient's eyes to be viewed through said viewing passage.

2. The protective helmet apparatus as defined in claim 1 wherein said exterior surface of said cushion (31) is dimensioned for cooperative engagement with the interior of a helmet casing (12) wherein said cushion (31) is interchangeably positionable to either one of a first position cooperatively engaged with a helmet casing (12) or a second position with said exterior surface of said cushion (31) supported on a mounting plate (66), whereby said cushion (31) may be used either in said first position or said second position to provide support to the head of a patient undergoing surgery.

3. The protective helmet apparatus (10) as defined in claim 1 or 2 further comprising:

a helmet casing (12) for use in combination with said cushion (26,28,31), said helmet casing (12) having a casing front wall and two casing sidewalls (47), each of said casing sidewalls attached at a first edge to said casing front wall and extending generally vertically therefrom to

an upper edge of said sidewalls, said helmet casing (12) having a casing interior surface and a casing exterior surface;

at least one casing ocular aperture (37) in said helmet casing (12) communicating between said casing interior surface and said casing exterior surface, said casing ocular aperture (37) shaped substantially similar to said cushion ocular aperture (27), and positioned in said helmet casing (12) to substantially align with said cushion ocular aperture (27) when said cushion (26,28,31) is in registered cooperative engagement with said helmet casing (12), whereby either of said eyes of a patient wearing said cushion (26,28,31) may be seen through the respective adjacent casing sidewall (47) of said helmet casing (12) when said cushion (26,28,31) is in said registered cooperative engagement with said helmet casing (12).

4. The protective helmet apparatus (10) as defined in claim 2 or claim 3 when dependent upon claim 2 said helmet apparatus being in combination with a mirrored surface (72) on said mounting plate (66) that supports said exterior surface of said cushion (31), wherein said mirrored surface provides a means for upright individuals standing adjacent to said protective head apparatus (10) to view the ocular area of the patient's face reflected in the mirrored surface by looking downward at said mirrored surface (72), while the patient wearing said cushion (31) is in the prone position.

5. The protective helmet apparatus (10) as defined in claim 4 additionally comprising:

means for height adjustment of said helmet casing above said mirrored surface (72).

6. The protective helmet apparatus as defined in claim 1 or claim 3 when dependent upon claim 1, wherein said facial cushion (26,28) is assembled from a plurality of cooperatively engageable components of differing dimensions for achieving optimum fit and pressure diffusion on the face of the intended helmet wearer.

7. A method, comprising the steps of:

(a) providing stable cranial support during surgery for an anesthetized patient in a prone position by fitting the patient with a protective helmet apparatus, the facial helmet apparatus comprising: a facial cushion (26, 28, 31) having a front portion, an interior surface and an exterior surface; said interior surface of said facial cushion being dimensioned to accommodate the facial structure of a human being; at least one

cushion ocular aperture (27) in said facial cushion communicating laterally across said front portion, said ocular aperture providing communication between said interior surface and said exterior surface; and

(b) supporting said exterior surface of said facial cushion on a mounting surface; said method being **characterised by** step (a) comprising the step of:

(c) fitting the patient with a said facial cushion wherein said facial cushion (26,28,31) has two cushion sidewalls extending upward from said front portion, and said cushion ocular aperture forms a viewing passage (82) continuing up both of said two cushion sidewalls and providing a view through said cushion sidewalls, wherein one of the two eyes of a patient wearing said cushion while in the prone position, may be seen through said viewing passage from a position adjacent to either of said two cushion sidewalls, thereby allowing both of said patients eyes to be viewed through said viewing passage.

8. The method as defined in claim 7 **characterised by** step (a) comprising the step of:

(d) fitting the patient with a said facial cushion wherein said exterior surface of said cushion (31) is dimensioned for cooperative engagement with the interior of a helmet casing (12) wherein said cushion is interchangeably positionable to either one of a first position cooperatively engaged with a helmet casing or a second position with said exterior surface of said cushion supported on a mounting plate (66), whereby said cushion may be used either in said first position or said second position to provide support to the head of a patient undergoing surgery.

9. The method as defined in claim 7 or 8 **characterised by** step (a) further comprising the step of:

(e) fitting the patient with a said protective helmet apparatus that further comprises:

a helmet casing (12) for use in combination with said cushion (26, 28, 31), said helmet casing having a casing front wall and two casing sidewalls (47), each of said casing sidewalls attached at a first edge to said casing front wall and extending generally vertically therefrom to an upper edge of said sidewalls, said helmet casing having a casing interior surface and a casing exterior surface; at least one casing ocular aperture (37) in said helmet casing communicating between said casing interior surface and

said casing exterior surface, said casing ocular aperture shaped substantially similar to said cushion ocular aperture (27), and positioned in said helmet casing to substantially align with said cushion ocular aperture when said facial cushion is in cooperative engagement with said helmet casing, whereby either of said eyes of a patient wearing said cushion may be seen through the respective adjacent casing sidewall of said helmet casing when said facial cushion is in said cooperative engagement with said helmet casing.

10. The method as defined in claim 8 or claim 9 when dependent upon claim 8 **characterised by** further comprising the step of:

(e) providing a mirrored surface (72) on the mounting plate (66) to provide a means for upright individuals standing adjacent to said protective helmet apparatus to view the ocular area of the patients face reflected in the mirrored surface by looking downward at said mirrored surface while the patient wearing said cushion is in the prone position.

11. The method as defined in claim 10 **characterised by** further comprising the step of:

(f) adjusting the height of said protective helmet apparatus above said mirrored surface (72).

12. The method as defined in claim 7 or claim 9 when dependent upon claim 7, wherein said facial cushion (26, 28) is assembled from a plurality of co-operatively engageable components of differing dimensions for achieving optimum fit and pressure diffusion on the face of the intended helmet wearer.

Patentansprüche

1. Schutzhelmvorrichtung (10) aufweisend: Ein Gesichtskissen (26, 28, 31) zum Bereitstellen einer stabilen Patientenschädelstütze während einer Operation für einen betäubten Patienten in Bauchlage, wobei das Gesichtskissen (26, 28, 31) einen Vorderteil, eine innere Oberfläche und eine äußere Oberfläche hat, wobei die innere Oberfläche des Kissens dimensioniert ist, um die Gesichtsstruktur eines Menschen aufzunehmen; mindestens eine Kissensichtöffnung (27) in dem Kissen, die sich lateral über den Vorderteil erstreckt, wobei die Sichtöffnung eine Verbindung zwischen der inneren Oberfläche und der äußeren Oberfläche schafft; dadurch charakterisiert, dass das Gesichtskissen (26, 28, 31) zwei Kissenseiten-

wände hat, die sich von dem ersten Teil nach oben erstrecken, wobei die Kissensichtöffnung (27) einen Sichtkorridor (82) bildet, der nach oben entlang beider Kissenseitenwände weiterführt und eine Sicht durch die Kissenseitenwände bereitstellt, wobei eines der beiden Augen eines Patienten, der das Kissen trägt, während er in Bauchlage ist, durch den Sichtkorridor von einer Position neben einer der beiden Kissenseitenwände gesehen werden kann, so dass es ermöglicht wird, dass beide der Augen des Patienten durch den Sichtkorridor gesehen werden.

2. Schutzhelmvorrichtung gemäß Anspruch 1, wobei die äußere Oberfläche des Kissens (31) dimensioniert ist für ein kooperatives Ineinandergreifen mit dem Inneren einer Helmschale (12), wobei das Kissen (31) austauschbar in entweder eine erste Position, die kooperativ mit einer Helmschale (12) ineinandergreift, oder eine zweite Position, bei der die äußere Oberfläche des Kissens (31) von einer Befestigungsplatte (66) gestützt wird, positionierbar ist, wobei das Kissen (31) entweder in der ersten Position oder in der zweiten Position verwendet werden kann, um den Kopf eines Patienten, der operiert wird, zu stützen.
3. Schutzhelmvorrichtung (10) gemäß Anspruch 1 oder 2, ferner aufweisend:

eine Helmschale (12) zur Verwendung in Kombination mit dem Kissen (26, 28, 31), wobei die Helmschale (12) eine Schalenvorderwand und zwei Schalenseitenwände (47) aufweist, wobei jede der Schalenseitenwände an einer ersten Kante an der Schalenvorderwand befestigt ist und sich hauptsächlich vertikal davon zu einer oberen Kante der Seitenwände erstreckt, wobei die Helmschale (12) eine innere Schalenoberfläche und eine äußere Schalenoberfläche hat; mindestens eine Schalensichtöffnung (37) in der Helmschale (12), die sich zwischen der inneren Schalenoberfläche und der äußeren Schalenoberfläche erstreckt, wobei die Schalensichtöffnung (37) im Wesentlichen gleich wie die Kissensichtöffnung (27) geformt ist und in der Helmschale (12) positioniert ist, so dass sie im Wesentlichen auf die Kissensichtöffnung (27) ausgerichtet ist, wenn das Kissen (26, 28, 31) mit der Helmschale (12) eingerastet kooperativ ineinandergreift, wobei eines der Augen eines Patienten, der das Kissen (26, 28, 31) trägt, durch die jeweilige angrenzende Schalenseitenwand (47) der Helmschale (12) gesehen werden kann, wenn das Kissen (26, 28, 31) mit der Helmschale (12) eingerastet kooperativ ineinandergreift.

4. Schutzhelmvorrichtung (10) gemäß Anspruch 2 oder

Anspruch 3, wenn er von Anspruch 2 abhängt, wobei die Helmvorrichtung in Kombination mit einer verspiegelten Oberfläche (72) auf der Befestigungsplatte (66), die die äußere Oberfläche des Kissens (31) stützt, ist, wobei die verspiegelte Oberfläche ein Mittel für Individuen, die aufrecht neben der Schutzhelmvorrichtung (10) stehen, schafft, zum Sehen des Augenbereichs des Gesichts des Patienten, der von der verspiegelten Oberfläche reflektiert wird, durch Herunterschauen auf die verspiegelte Oberfläche (72), während der Patient, der das Kissen (31) trägt, in der Bauchlage ist.

5. Schutzhelmvorrichtung (10) gemäß Anspruch 4, ferner aufweisend:

Mittel für die Höheneinstellung der Helmschale über der verspiegelten Oberfläche (72).

6. Schutzhelmvorrichtung gemäß Anspruch 1 oder Anspruch 3, wenn er von Anspruch 1 abhängt, wobei das Gesichtskissen (26, 28) aus einer Mehrzahl von Komponenten unterschiedlicher Größen, die kooperativ ineinandergreifen können, zusammengesetzt ist, so dass eine optimale Passform und Druckverteilung auf dem Gesicht des vorgesehenen Helmträgers erreicht wird.

7. Verfahren, aufweisend die Schritte:

(a) Bereitstellen einer stabilen Patientenschädelstütze während einer Operation für einen betäubten Patienten in Bauchlage durch Ausstatten des Patienten mit einer Schutzhelmvorrichtung, wobei die Schutzhelmvorrichtung aufweist: Ein Gesichtskissen (26, 28, 31) mit einem Vorderteil, einer inneren Oberfläche und einer äußeren Oberfläche, wobei die innere Oberfläche des Kissens dimensioniert ist, um die Gesichtsstruktur eines Menschen aufzunehmen; mindestens eine Kissensichtöffnung (27) in dem Kissen, die sich lateral über den Vorderteil erstreckt, wobei die Sichtöffnung eine Verbindung zwischen der inneren Oberfläche und der äußeren Oberfläche schafft; und

(b) Stützen der äußeren Oberfläche des Gesichtskissens durch eine Befestigungsfläche; wobei das Verfahren dadurch charakterisiert ist, dass der Schritt (a) den Schritt aufweist:

(c) Ausstatten des Patienten mit dem Gesichtskissen, wobei das Gesichtskissen (26, 28, 31) zwei Kissenseitenwände hat, die sich von dem ersten Teil nach oben erstrecken und die Kissensichtöffnung (27) einen Sichtkorridor (82) bildet, der nach oben entlang beider Kissenseitenwände weiterführt und eine Sicht durch die Kissenseitenwände bereitstellt, wobei eines der beiden Augen eines Patienten, der das Kissen

trägt, während er in Bauchlage ist, durch den Sichtkorridor von einer Position neben einer der beiden Kissenseitenwände gesehen werden kann, so dass es ermöglicht wird, dass beide der Augen des Patienten durch den Sichtkorridor gesehen werden.

8. Verfahren gemäß Anspruch 7, dadurch charakterisiert, dass der Schritt (a) den Schritt aufweist:

(d) Ausstatten des Patienten mit dem Gesichtskissen, wobei die äußere Oberfläche des Kissens (31) dimensioniert ist für ein kooperatives Ineinandergreifen mit dem Inneren einer Helmschale (12), wobei das Kissen (31) austauschbar in entweder eine erste Position, die kooperativ mit einer Helmschale ineinandergreift, oder eine zweite Position, bei der die äußere Oberfläche des Kissens (31) von einer Befestigungsplatte (66) gestützt wird, positionierbar ist, wobei das Kissen entweder in der ersten Position oder in der zweiten Position verwendet werden kann, um den Kopf eines Patienten, der operiert wird, zu stützen.

9. Verfahren gemäß Anspruch 7 oder 8, dadurch charakterisiert, dass der Schritt (a) ferner den Schritt aufweist:

(e) Ausstatten des Patienten mit der Schutzhelmvorrichtung, die ferner aufweist:

eine Helmschale (12) zur Verwendung in Kombination mit dem Kissen (26, 28, 31), wobei die Helmschale (12) eine Schalen-vorderwand und zwei Schalenseitenwände (47) aufweist, wobei jede der Schalenseitenwände an einer ersten Kante an der Schalen-vorderwand befestigt ist und sich hauptsächlich vertikal davon zu einer oberen Kante der Seitenwände erstreckt, wobei die Helmschale eine innere Schalenoberfläche und eine äußere Schalenoberfläche hat; mindestens eine Schalensichtöffnung (37) in der Helmschale, die sich zwischen der inneren Schalenoberfläche und der äußeren Schalenoberfläche erstreckt, wobei die Schalensichtöffnung im Wesentlichen gleich wie die Kissensichtöffnung (27) geformt ist und in der Helmschale positioniert ist, so dass sie im Wesentlichen auf die Kissensichtöffnung ausgerichtet ist, wenn das Gesichtskissen mit der Helmschale kooperativ ineinandergreift, wobei eines der Augen eines Patienten, der das Kissen trägt, durch die jeweilige angrenzende Schalenseitenwand der Helmschale gesehen werden kann, wenn das Kissen mit der Helm-

schale eingerastet kooperativ ineinandergreift.

10. Verfahren gemäß Anspruch 8 oder Anspruch 9, wenn er von Anspruch 8 abhängt, dadurch charakterisiert, dass es ferner den Schritt aufweist:

(e) Bereitstellen einer verspiegelten Oberfläche (72) auf der Befestigungsplatte (66) zum Schaffen eines Mittels für Individuen, die aufrecht neben der Schutzhelmvorrichtung stehen, zum Sehen des Augenbereichs des Gesichts des Patienten, der von der verspiegelten Oberfläche reflektiert wird, durch Herunterschauen auf die verspiegelte Oberfläche, während der Patient, der das Kissen trägt, in der Bauchlage ist.

11. Verfahren gemäß Anspruch 10, dadurch charakterisiert, dass es ferner den Schritt aufweist:

(f) Einstellen der Höhe der Schutzhelmvorrichtung über der verspiegelten Oberfläche (72).

12. Verfahren gemäß Anspruch 7 oder 9, wenn er von Anspruch 7 abhängt, wobei das Gesichtskissen (26, 28) aus einer Mehrzahl von Komponenten unterschiedlicher Größen, die kooperativ ineinandergreifen können, zusammengesetzt ist, so dass eine optimale Passform und Druckverteilung auf dem Gesicht des vorgesehenen Helmträgers erreicht wird.

Revendications

1. Appareil formant casque de protection (10) comprenant : un coussin facial (26, 28, 31) pour offrir un support crânien stable, pendant une opération, à un patient anesthésié qui se trouve dans une position ventrale, le coussin facial (26, 28, 31) ayant une partie frontale, une surface intérieure et une surface extérieure ; la surface intérieure du coussin étant dimensionnée pour recevoir la structure faciale d'un être humain ; au moins une ouverture oculaire de coussin (27), dans le coussin, offrant une communication latéralement sur la partie frontale, laquelle ouverture oculaire offre une communication entre la surface intérieure et la surface extérieure ; **caractérisé en ce que** le coussin facial (26, 28, 31) présente deux parois latérales de coussin qui s'étendent vers le haut à partir de la première partie, l'ouverture oculaire de coussin (27) forme un passage de vue (82) qui se poursuit vers le haut sur les deux parois latérales de coussin et qui offre une vue à travers celles-ci, étant précisé que l'un des deux yeux d'un patient qui porte le coussin alors qu'il se trouve en position ventrale peut être vu à travers le passage de vue, à partir d'une position voisine de l'une ou l'autre des parois

latérales de coussin, permettant ainsi de voir les deux yeux du patient à travers le passage de vue.

2. Appareil formant casque de protection tel qu'il est défini dans la revendication 1, étant précisé que la surface extérieure du coussin (31) est dimensionnée pour un emboîtement coopérant avec l'intérieur d'une enveloppe de casque (12) dans laquelle ledit coussin (31) est positionnable de manière interchangeable au niveau d'une première position emboîtée de manière coopérante avec une enveloppe de casque (12), ou d'une seconde position avec la surface extérieure du coussin (31) supportée sur une plaque de montage (66), moyennant quoi le coussin (31) peut être utilisé soit dans la première position, soit dans la seconde position afin d'offrir un support à la tête d'un patient qui subit une opération.

3. Appareil formant casque de protection (10) tel qu'il est défini dans la revendication 1 ou 2, comprenant par ailleurs :

une enveloppe de casque (12) à utiliser en combinaison avec le coussin (26, 28, 31), ladite enveloppe de casque (12) présentant une paroi frontale d'enveloppe et deux parois latérales d'enveloppe (47), chacune des parois latérales d'enveloppe étant fixée, sur un premier bord, à la paroi frontale d'enveloppe et s'étendant globalement à la verticale à partir de celle-ci jusqu'à un bord supérieur desdites parois latérales, l'enveloppe de casque (12) ayant une surface intérieure d'enveloppe et une surface extérieure d'enveloppe ;

au moins une ouverture oculaire d'enveloppe (37) dans l'enveloppe de casque (12), qui offre une communication entre la surface intérieure d'enveloppe et la surface extérieure d'enveloppe, ladite ouverture oculaire (37) ayant une forme similaire à celle de l'ouverture oculaire de coussin (27) et étant positionnée dans l'enveloppe de casque (12) de manière à être globalement dans l'alignement de ladite ouverture oculaire de coussin (27) quand le coussin (26, 28, 31) est emboîté de manière coopérante et coïncidente avec l'enveloppe de casque (12), moyennant quoi les yeux d'un patient qui porte le coussin (26, 28, 31) peuvent être vus à travers les parois d'enveloppe voisines respectives (47) de l'enveloppe de casque (12) quand ledit coussin (26, 28, 31) est emboîté de manière coopérante et coïncidente avec l'enveloppe de casque (12).

4. Appareil formant casque de protection (10) tel qu'il est défini dans la revendication 2 ou la revendication 3 lorsqu'elle est dépendante de la revendication 2, ledit appareil formant casque étant combiné avec

une surface réfléchissante (72), sur la plaque de montage (66) qui supporte la surface extérieure du coussin (31), étant précisé que ladite surface réfléchissante offre un moyen, pour des personnes qui sont debout près de l'appareil formant casque de protection (10), de voir la zone oculaire du visage du patient qui est réfléchi dans ladite surface réfléchissante, en baissant les yeux pour regarder la surface réfléchissante (72), alors que le patient qui porte le coussin (31) est en position ventrale.

5. Appareil formant casque de protection (10) tel qu'il est défini dans la revendication 4, comprenant en supplément :

des moyens pour régler en hauteur l'enveloppe de casque au-dessus de la surface réfléchissante (72).

6. Appareil formant casque de protection tel qu'il est défini dans la revendication 1 ou la revendication 3 lorsqu'elle est dépendante de la revendication 1, étant précisé que le coussin facial (26, 28) est assemblé à partir de plusieurs éléments qui sont emboîtables de manière coopérante et qui ont des dimensions différentes, pour obtenir un ajustement optimal et une diffusion de pression optimale sur le visage du porteur du casque.

7. Procédé comprenant les étapes qui consistent :

(a) à offrir un support crânien stable, pendant une opération, à un patient anesthésié qui se trouve dans une position ventrale, en équipant le patient d'un appareil formant casque de protection, l'appareil formant casque facial comprenant : un coussin facial (26, 28, 31) qui présente une partie frontale, une surface intérieure et une surface extérieure ; la surface intérieure du coussin facial étant dimensionnée pour recevoir la structure faciale d'un être humain ; au moins une ouverture oculaire de coussin (27), dans le coussin facial, offrant une communication latéralement sur la partie frontale, laquelle ouverture oculaire offre une communication entre la surface intérieure et la surface extérieure ; et

(b) à supporter ladite surface extérieure du coussin facial sur une surface de montage ; le procédé étant **caractérisé en ce que** l'étape (a) comprend l'étape qui consiste :

(c) à équiper le patient d'un coussin facial, étant précisé que le coussin facial (26, 28, 31) présente deux parois latérales de coussin qui s'étendent vers le haut à partir de la partie frontale, et que l'ouverture oculaire de coussin forme un passage de vue (82) qui se poursuit vers le haut sur les deux parois latérales de coussin et

qui offre une vue à travers celles-ci, étant précisé que l'un des deux yeux d'un patient qui porte le coussin alors qu'il se trouve en position ventrale peut être vu à travers le passage de vue, à partir d'une position voisine de l'une ou l'autre des parois latérales de coussin, permettant ainsi de voir les deux yeux du patient à travers le passage de vue.

8. Procédé tel qu'il est défini dans la revendication 7, **caractérisé en ce que** l'étape (a) comprend également l'étape qui consiste :

(d) à équiper le patient du coussin facial, étant précisé que la surface extérieure du coussin (31) est dimensionnée pour un emboîtement coopérant avec l'intérieur d'une enveloppe de casque (12) dans laquelle ledit coussin est positionnable de manière interchangeable au niveau d'une première position emboîtée de manière coopérante avec une enveloppe de casque, ou d'une seconde position avec la surface extérieure du coussin supportée sur une plaque de montage (66), moyennant quoi le coussin peut être utilisé soit dans la première position, soit dans la seconde position afin d'offrir un support à la tête d'un patient qui subit une opération.

9. Procédé tel qu'il est défini dans la revendication 7 ou 8, **caractérisé en ce que** l'étape (a) comprend également l'étape qui consiste :

(e) à équiper le patient d'un appareil formant casque de protection qui comprend par ailleurs :

une enveloppe de casque (12) à utiliser en combinaison avec le coussin (26, 28, 31), ladite enveloppe de casque présentant une paroi frontale d'enveloppe et deux parois latérales d'enveloppe (47), chacune des parois latérales d'enveloppe étant fixée, sur un premier bord, à la paroi frontale d'enveloppe et s'étendant globalement à la verticale à partir de celle-ci jusqu'à un bord supérieur desdites parois latérales, l'enveloppe de casque ayant une surface intérieure d'enveloppe et une surface extérieure d'enveloppe ; au moins une ouverture oculaire d'enveloppe (37) dans l'enveloppe de casque, qui offre une communication entre la surface intérieure d'enveloppe et la surface extérieure d'enveloppe, ladite ouverture oculaire ayant une forme similaire à celle de l'ouverture oculaire de coussin (27) et étant positionnée dans l'enveloppe de casque de manière à être globalement dans l'alignement de ladite ouverture oculaire de coussin quand le coussin facial est emboîté

de manière coopérante avec l'enveloppe de casque, moyennant quoi les yeux d'un patient qui porte le coussin peuvent être vus à travers les parois d'enveloppe voisines respectives de l'enveloppe de casque quand ledit coussin facial est emboîté de manière coopérante avec l'enveloppe de casque.




10. Procédé tel qu'il est défini dans la revendication 8 ou la revendication 9 quand elle est dépendante de la revendication 8, **caractérisé en ce qu'il** comprend également l'étape qui consiste :

(e) à prévoir une surface réfléchissante (72) sur la plaque de montage (66), pour offrir un moyen, pour des personnes qui sont debout près de l'appareil formant casque de protection, de voir la zone oculaire du visage du patient qui est réfléchi dans ladite surface réfléchissante, en baissant les yeux pour regarder la surface réfléchissante, alors que le patient qui porte le coussin est en position ventrale.

11. Procédé tel qu'il est défini dans la revendication 10, **caractérisé en ce qu'il** comprend également l'étape qui consiste :

(f) à régler la hauteur de l'appareil formant casque de protection au-dessus de la surface réfléchissante (72).

12. Procédé tel qu'il est défini dans la revendication 7 ou la revendication 9 quand elle est dépendante de la revendication 7, étant précisé que le coussin facial (26, 28) est assemblé à partir de plusieurs éléments qui sont emboîtables de manière coopérante et qui ont des dimensions différentes, pour obtenir un ajustement optimal et une diffusion de pression optimale sur le visage du porteur du casque.

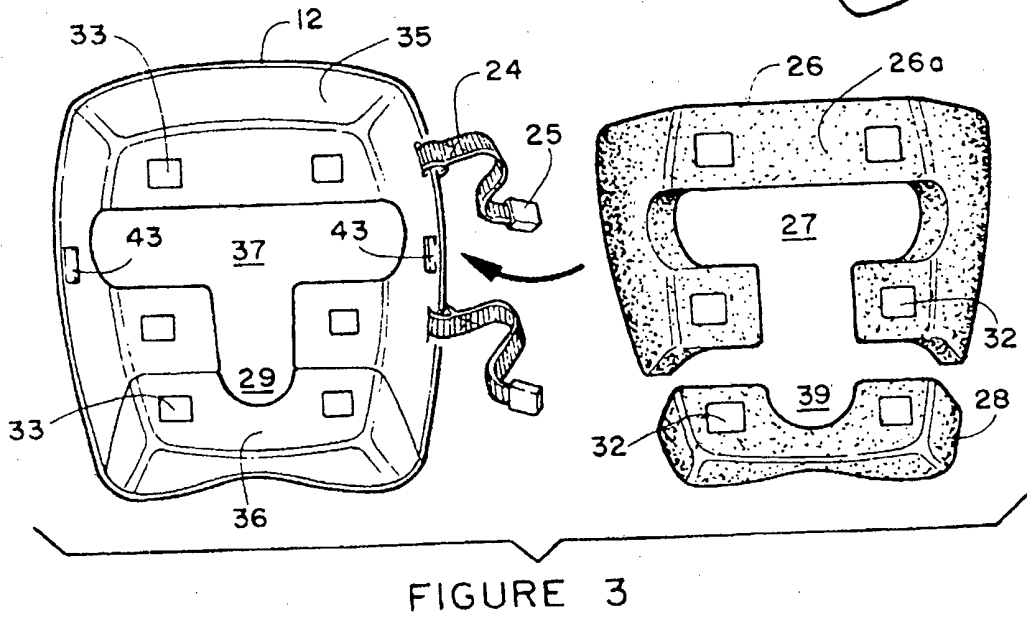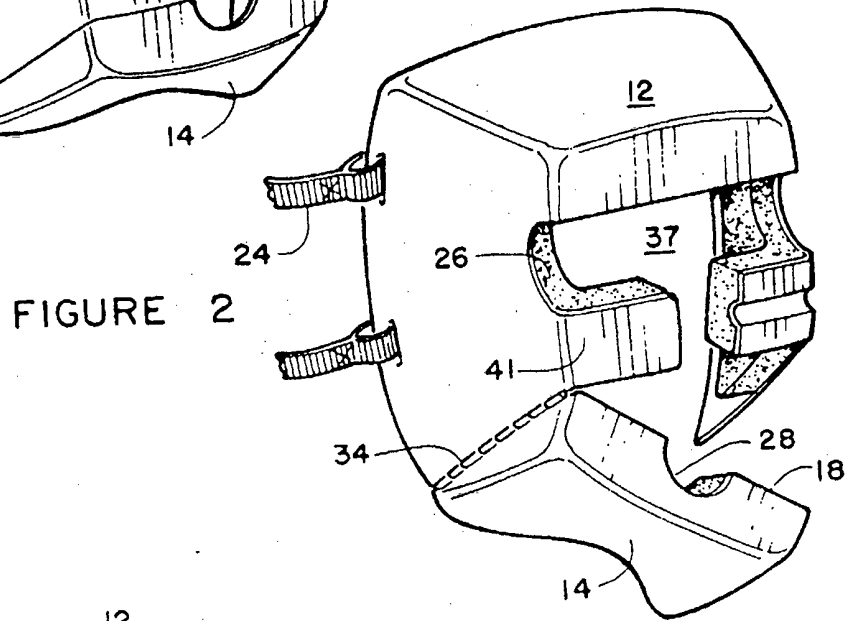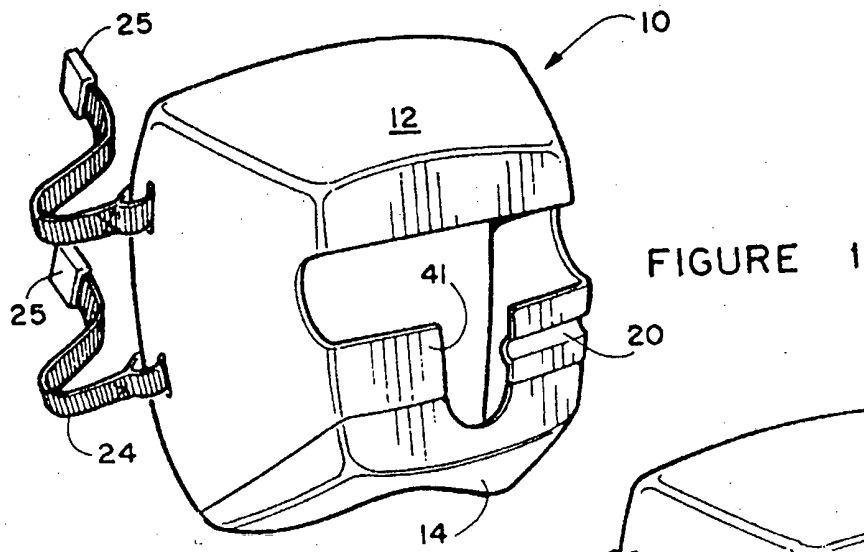

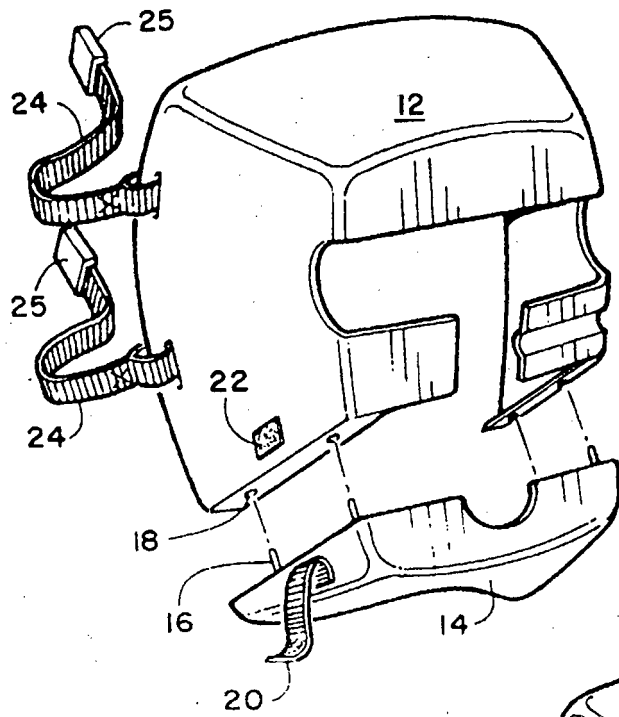
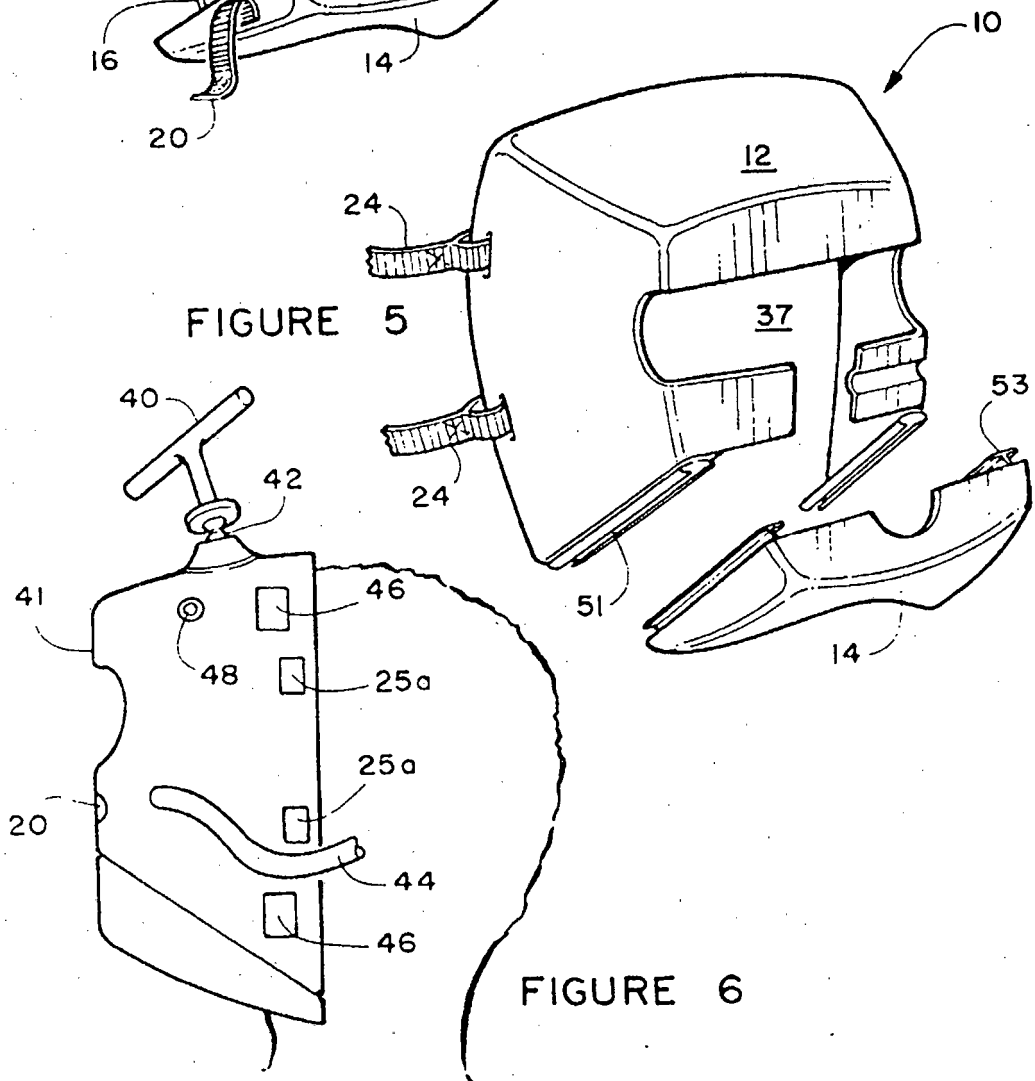


FIGURE 4



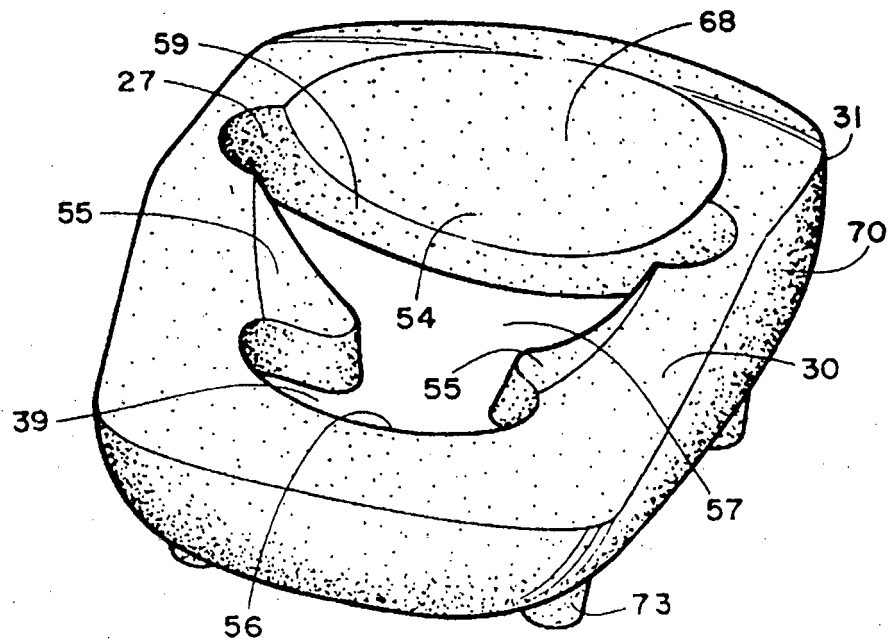


FIGURE 9

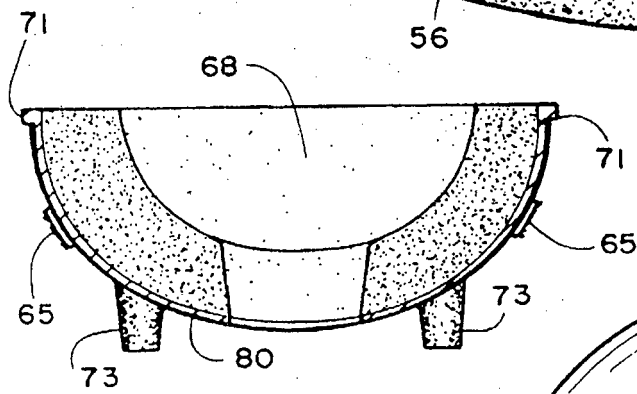


FIGURE 10

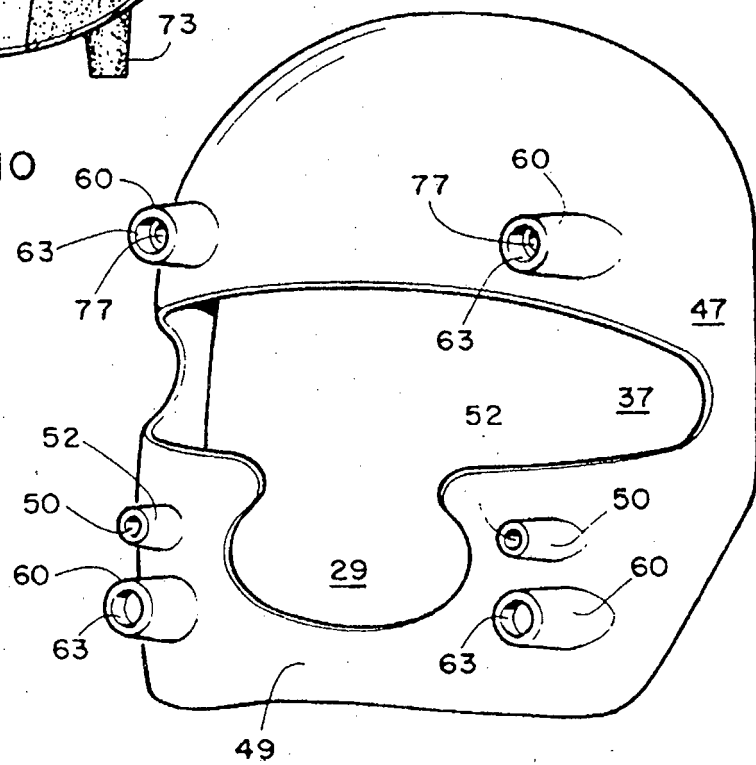


FIGURE 11

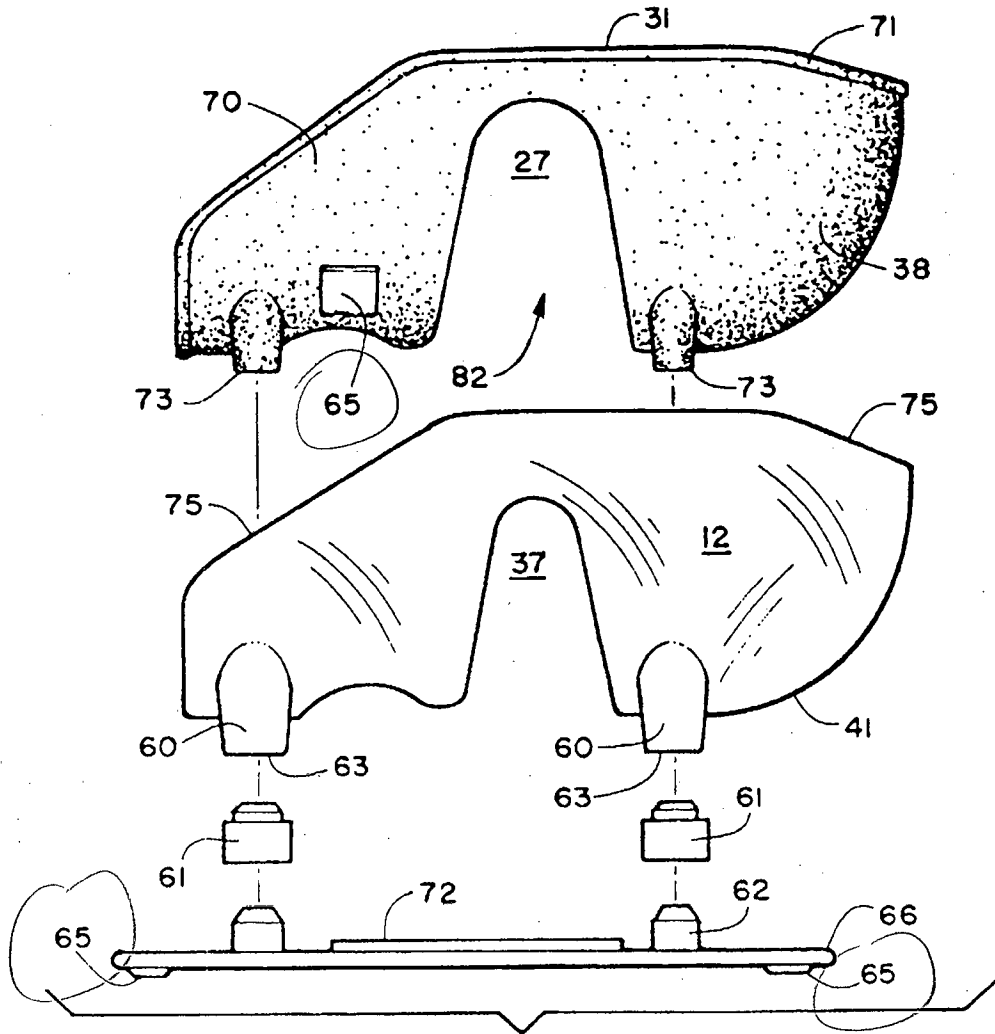


FIGURE 7

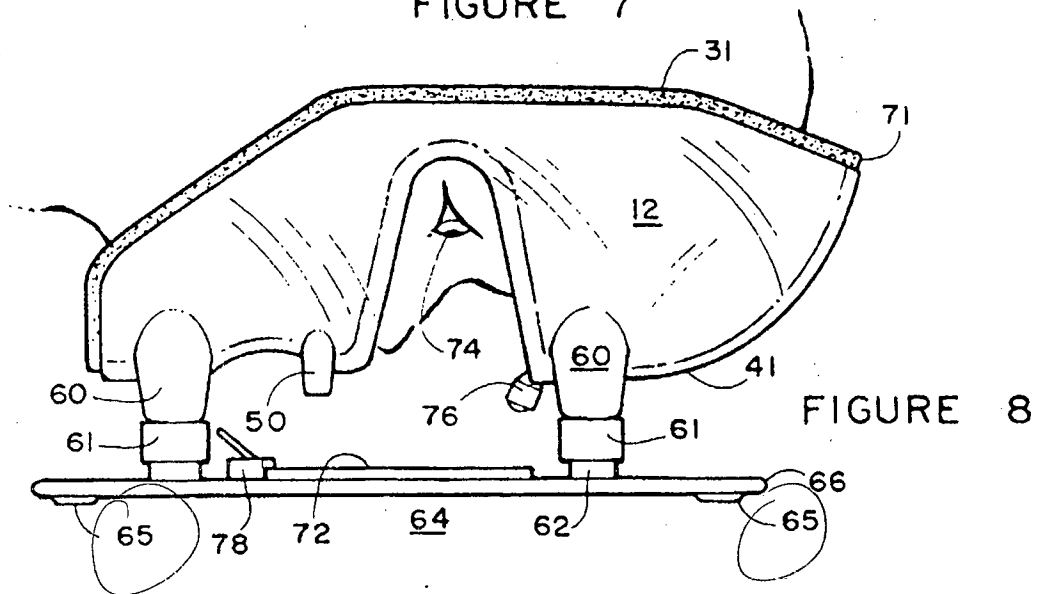


FIGURE 8

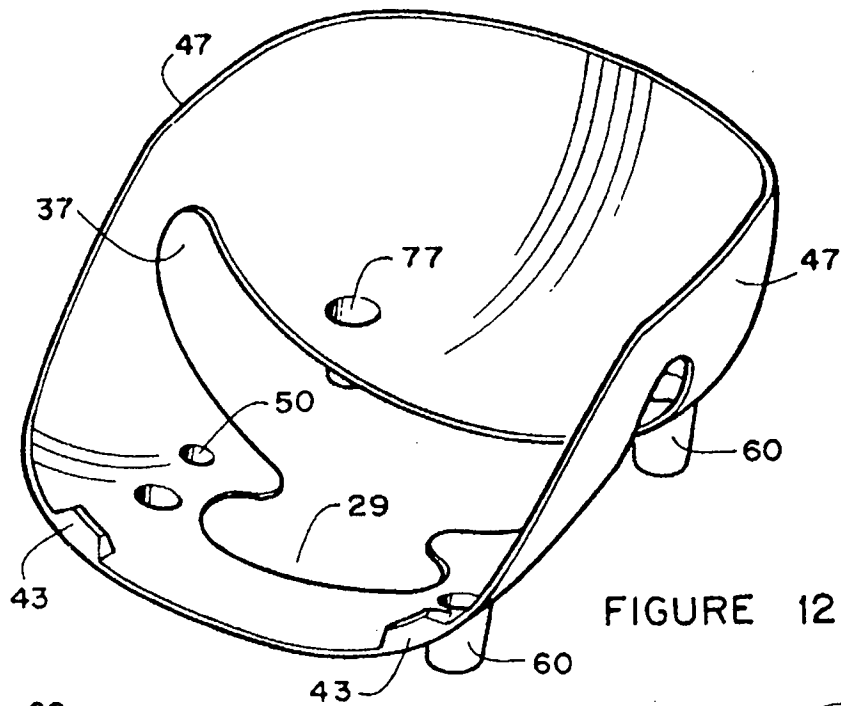


FIGURE 12

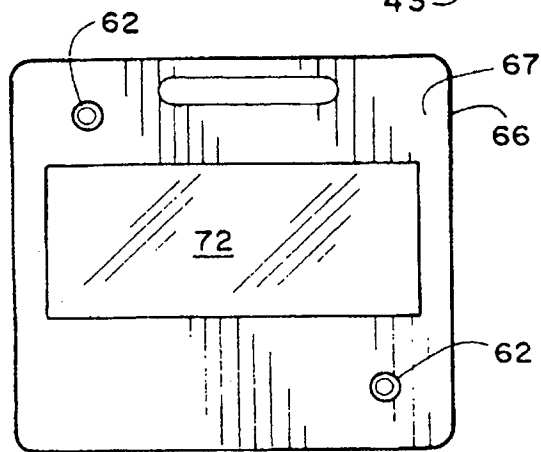


FIGURE 14

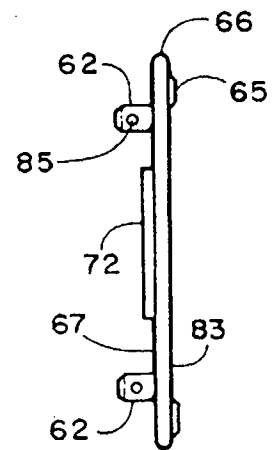


FIGURE 13

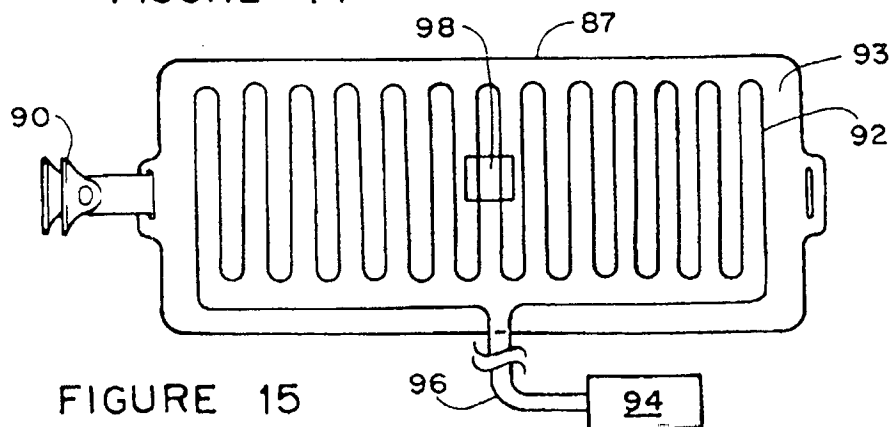


FIGURE 15

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- US 5220699 A, Farris **[0012]**
- US 4400820 O, O'Dell **[0013]**
- US 5214815 A, Agbodoe **[0014]**
- US 4757983 A, Ray **[0015]**
- US 4504050 A **[0016]**