



Europäisches Patentamt
European Patent Office
Office européen des brevets



(11) **EP 1 422 557 A1**

(12) **EUROPEAN PATENT APPLICATION**

(43) Date of publication:
26.05.2004 Bulletin 2004/22

(51) Int Cl.7: **G03C 5/16, G03C 5/17**

(21) Application number: **03078511.7**

(22) Date of filing: **07.11.2003**

(84) Designated Contracting States:
**AT BE BG CH CY CZ DE DK EE ES FI FR GB GR
HU IE IT LI LU MC NL PT RO SE SI SK TR**
Designated Extension States:
AL LT LV MK

(30) Priority: **19.11.2002 US 299765
19.11.2002 US 299941
19.11.2002 US 299759**

(71) Applicant: **EASTMAN KODAK COMPANY
Rochester, New York 14650 (US)**

(72) Inventors:
• **Dickerson, Robert E. Eastman Kodak Company
Rochester New York 14650-2201 (US)**
• **Moore, William E. Eastman Kodak Company
Rochester New York 14650-2201 (US)**
• **Steklenski, David J. Eastman Kodak Company
Rochester New York 14650-2201 (US)**

(74) Representative: **Haile, Helen Cynthia et al
Kodak Limited,
Patents Department (W92-3A),
Headstone Drive
Harrow, Middlesex HA1 4TY (GB)**

(54) **Mammography film and imaging assembly for use with rhodium or tungsten anodes**

(57) A radiographic silver halide film comprises a cubic grain silver halide emulsion layer on one side of the support and a tabular grain silver halide emulsion layer on the other side. The cubic grain silver halide emulsion layer comprises a combination of first and second spectral sensitizing dyes that provides a combined maximum J-aggregate absorption on the cubic silver halide grains of from 540 to 560 nm. The first spectral sensitizing dye is an anionic benzimidazole-benzoxazole carbocyanine, the second spectral sensitizing dye is an anionic oxycarbocyanine. The cubic grain silver halide emulsion layer also includes a mixture of gelatin or a gelatin de-

rivative and a second hydrophilic binder other than gelatin or a gelatin derivative at a weight ratio of first to second hydrophilic binder of from 2:1 to 5: 1. The cubic silver halide grains comprise from 1 to 20 mol % chloride and from 0.25 to 1.5 mol % iodide, which cubic silver halide grains have an average ECD of from 0.65 to 0.8 μm . Moreover, the cubic silver halide grains are doped with a hexacoordination complex compound within part or all of the innermost 95% of the grains. These films can be exposed to provide a black-and-white image having a $d(\gamma)/d(\log E)$ value greater than 5 and are particularly useful when imaged using X-radiation generating devices comprising rhodium or tungsten anodes.

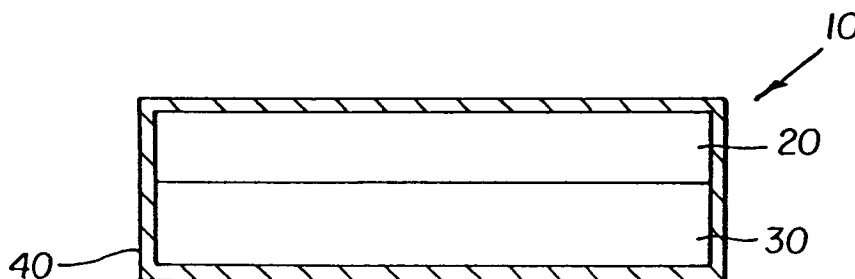


FIG. 1

EP 1 422 557 A1

Description

[0001] This invention is directed to radiography. In particular, it is directed to a radiographic silver halide film and imaging assembly that are useful for providing medical diagnostic images of soft tissues such as in mammography. These films provide advantages when exposed to X-radiation generated using rhodium or tungsten anodes.

[0002] The use of radiation-sensitive silver halide emulsions for medical diagnostic imaging can be traced to Roentgen's discovery of X-radiation by the inadvertent exposure of a silver halide film. Eastman Kodak Company then introduced its first product specifically that was intended to be exposed by X-radiation in 1913.

[0003] In conventional medical diagnostic imaging the object is to obtain an image of a patient's internal anatomy with as little X-radiation exposure as possible. The fastest imaging speeds are realized by mounting a dual-coated radiographic element between a pair of fluorescent intensifying screens for imagewise exposure. 5% or less of the exposing X-radiation passing through the patient is adsorbed directly by the latent image forming silver halide emulsion layers within the dual-coated radiographic element. Most of the X-radiation that participates in image formation is absorbed by phosphor particles within the fluorescent screens. This stimulates light emission that is more readily absorbed by the silver halide emulsion layers of the radiographic element.

[0004] Examples of radiographic element constructions for medical diagnostic purposes are provided by U. S. Patent 4,425,425 (Abbott et al.) and U.S. Patent 4,425,426 (Abbott et al.), U.S. Patent 4,414,310 (Dickerson), U.S. Patent 4,803,150 (Kelly et al.), U.S. Patent 4,900,652 (Kelly et al.), U.S. Patent 5,252,442 (Tsaur et al.), and *Research Disclosure*, Vol. 184, August 1979, Item 18431.

[0005] While the necessity of limiting patient exposure to high levels of X-radiation was quickly appreciated, the question of patient exposure to even low levels of X-radiation emerged gradually. The separate development of soft tissue radiography, which requires much lower levels of X-radiation, can be illustrated by mammography. The first intensifying screen-film combination (imaging assembly) for mammography was introduced to the public in the early 1970's. Mammography film generally contains a single silver halide emulsion layer and is exposed by a single intensifying screen, usually interposed between the film and the source of X-radiation. Mammography utilizes low energy X-radiation, that is, radiation that is predominantly of an energy level less than 40 keV.

[0006] U.S. Patent 6,033,840 (Dickerson) and U.S. Patent 6,037,112 (Dickerson) describe asymmetric imaging elements and processing methods for imaging soft tissue.

Problem to be Solved

[0007] In mammography, as in many forms of soft tissue radiography, pathological features that are to be identified are often quite small and not much different in density than surrounding healthy tissue. Thus, the use of films with relatively high average contrast (in the range of from 2.5 to 3.5) over a density range of from 0.25 to 2.0 is typical. Limiting the amount of X-radiation requires higher absorption of the X-radiation by the intensifying screen and lower X-radiation exposure of the film. This can contribute to loss of image sharpness and contrast. Thus mammography is a very difficult task in medical radiography.

[0008] Radiographic imaging of soft tissue as in mammography is usually carried out using X-ray imaging equipment that includes an X-ray tube with a rotating anode. The anode is the "source" of the X-radiation that is created when electrons interact with the electrons or nuclei of the metallic atoms in the anode. To maximize image quality, molybdenum anodes are generally used in such equipment. Rhodium anodes are also known in the art for lowering patient exposure to radiation, but in the case of mammography, poorer image quality is usually the result when they are used.

[0009] There remains a need in mammography for a way to minimize patient exposure to radiation while providing optimal radiographic image quality such as image contrast.

[0010] The present invention provides an advance in the art with a radiographic silver halide film that comprises a support having first and second major surfaces and that is capable of transmitting X-radiation,

the radiographic silver halide film having disposed on the first major support surface, one or more hydrophilic colloid layers including at least one cubic grain silver halide emulsion layer, and having disposed on the second major support surface, one or more hydrophilic colloid layers including at least one tabular grain silver halide emulsion layer,
the film characterized wherein it can be exposed to provide a black-and-white image having a $d(\gamma)/d(\log E)$ value greater than 5.

[0011] The invention also provides a radiographic silver halide film that comprises a support having first and second major surfaces and that is capable of transmitting X-radiation,

the radiographic silver halide film having disposed on the first major support surface, one or more hydrophilic

colloid layers including at least one cubic grain silver halide emulsion layer, and having disposed on the second major support surface, one or more hydrophilic colloid layers including at least one tabular grain silver halide emulsion layer,
the film characterized wherein the cubic grain silver halide emulsion layer comprises:

1) a combination of first and second spectral sensitizing dyes that provides a combined maximum J-aggregate absorption on the cubic silver halide grains of from 540 to 560 nm, and

wherein the first spectral sensitizing dye is an anionic benzimidazole-benzoxazole carbocyanine, the second spectral sensitizing dye is an anionic oxycarbocyanine, and the first and second spectral sensitizing dyes are present in a molar ratio of from 0.25:1 to 4:1,

2) a mixture of a first hydrophilic binder that is gelatin or a gelatin derivative and a second hydrophilic binder other than gelatin or a gelatin derivative, wherein the weight ratio of the first hydrophilic binder to the second hydrophilic binder is from 2:1 to 5:1, and the level of hardener in the cubic grain silver halide emulsion layer is from 0.4 to 1.5 weight % based on the total weight of the first hydrophilic binder in the cubic grain silver halide emulsion layer,

3) cubic silver halide grains comprising from 1 to 20 mol % chloride and from 0.25 to 1.5 mol % iodide, both based on total silver in the cubic grain emulsion layer, which cubic silver halide grains have an average ECD of from 0.65 to 0.8 μm , and

4) cubic silver halide grains that are doped with a hexacoordination complex compound within part or all of 95% of the innermost volume from the center of the cubic silver halide grains.

[0012] Preferred embodiments of the present invention include a radiographic silver halide film having a photographic speed of at least 100 and comprising a transparent film support having first and second major surfaces and that is capable of transmitting X-radiation,


the radiographic silver halide film having disposed on the first major support surface, one or more hydrophilic colloid layers including at least one silver halide emulsion layer, and having disposed on the second major support surface, one or more hydrophilic colloid layers including at least one tabular grain silver halide emulsion layer,


the film also comprising a protective overcoat layer disposed on both sides of the support,

the film characterized wherein the cubic grain silver halide emulsion layer comprises:

1) a combination of first and second spectral sensitizing dyes that provides a combined maximum J-aggregate absorption of from 545 to 555 nm when the dyes are absorbed on the surface of the cubic silver halide grains,

wherein the first spectral sensitizing dye is the following Dye A-2, and wherein the second spectral sensitizing dye is following Dye B-1, the first and second spectral sensitizing dyes being present in a molar ratio of from 0.5:1 to 1.5:1, and the total spectral sensitizing dyes in the film is from 0.25 to 0.75 mg/mole of silver,

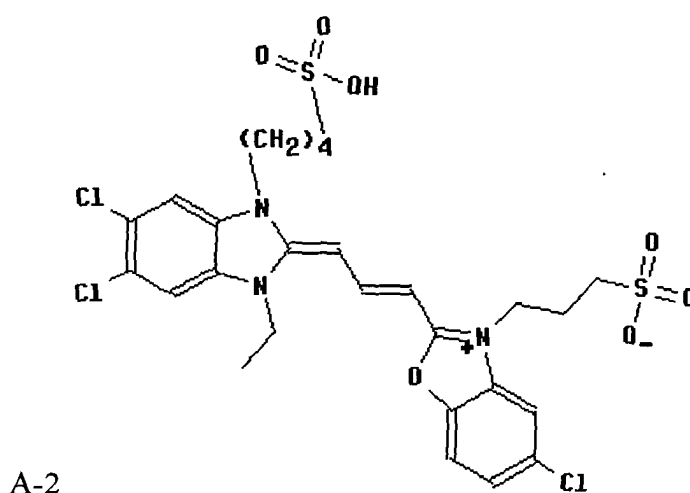

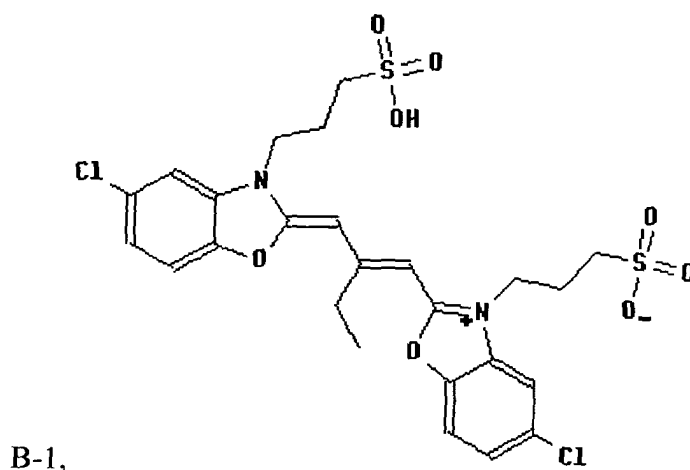

20 2) a mixture of a first hydrophilic binder that is gelatin or a gelatin derivative and a second hydrophilic binder that is a dextran or polyacrylamide, wherein the weight ratio of the first hydrophilic binder to the second hydrophilic binder is from 2.5:1 to 3.5:1 and the level of hardener in the cubic grain silver halide emulsion is from 0.5 to 1.5 weight % based on the total weight of the first hydrophilic binder in the cubic grain silver halide emulsion layer,

25 3) cubic silver halide grains comprising from 10 to 20 mol % chloride and from 0.5 to 1 mol % iodide, both based on total silver in the cubic grain silver halide emulsion layer, which cubic silver halide grains have an average ECD of from 0.72 to 0.76 μ m, and

30 4) cubic silver halide grains that are doped with a hexacoordination complex compound within 75 to 80% of the innermost volume from the center of the cubic silver halide grains, wherein the hexacoordination complex compound is represented by the following Structure I:



35 wherein M is Fe⁺², Ru⁺², OS⁺², Co⁺³, Rh⁺³, Ir⁺³, Pd⁺³, or Pt⁺⁴, L represents six coordination complex ligands that can be the same or different provided that at least three of the ligands are cyanide ions, and n is -2, -3, or -4.

[0013] This invention also provides a radiographic imaging assembly comprising:

40 A) the radiographic silver halide film of the present invention, and

B) a fluorescent intensifying screen that comprises an inorganic phosphor capable of absorbing X-rays and emitting electromagnetic radiation having a wavelength greater than 300 nm.

[0014] Preferably, the radiographic imaging assembly of this invention comprises a single fluorescent intensifying screen that comprises an inorganic phosphor coated in admixture with a polymeric binder in a phosphor layer onto a flexible support and has a protective overcoat disposed over the phosphor layer.

45 **[0015]** In addition, a method of providing a black-and-white image comprises exposing the radiographic imaging assembly of the present invention to X-radiation generated using rhodium or tungsten anodes in an X-radiation generating device, and processing the radiographic silver halide film, sequentially, with a black-and-white developing composition and a fixing composition, the processing being carried out within 90 seconds, dry-to-dry.

50 **[0016]** Still further, a method of providing a black-and-white image comprises exposing the radiographic imaging assembly of the present invention to X-radiation at a peak voltage greater than 28 kVp, and processing the radiographic silver halide film, sequentially, with a black-and-white developing composition and a fixing composition, the processing being carried out within 90 seconds, dry-to-dry.

55 **[0017]** The present invention provides a means for providing radiographic images for mammography unexpectedly exhibiting improved image quality while minimizing radiation dosage to which patients are exposed. In particular, image quality can be improved with the present invention by increasing image contrast, decreasing "noise" (for example, film granularity), or both. These advantages are possible with the unique radiographic film and imaging assembly of this invention and thereby allow patient imaging to be carried out using imaging equipment containing rhodium or tungsten anodes without sacrificing image quality such as image contrast.

[0018] In particular, it has been found that the radiographic silver halide films of the present invention provide images that exhibit desired contrast in the mid-scale region. This contrast can be evaluated by calculating the derivative (or slope) of a gamma vs. log E curve to obtain a term " $d(\gamma)/d(\log E)$ " that is defined in more detail below. In the present invention, the films exhibit a $d(\gamma)/d(\log E)$ greater than 5 and preferably greater than 5.5.

[0019] In addition, all other desirable sensitometric properties are maintained and the radiographic film can be rapidly processed in the same conventional processing equipment and compositions.

[0020] In most preferred embodiments, patients are exposed at a peak voltage greater than 28 kVp using rhodium or tungsten anodes in an X-radiation generating device, whereby patient dosage is reduced without sacrificing image quality such as image contrast.

BRIEF DESCRIPTION OF THE DRAWING

[0021]

FIG. 1 is a schematic cross-sectional illustration of an embodiment of this invention comprising a radiographic silver halide film and a single fluorescent intensifying screen in a cassette holder.

Definition of Terms:

[0022] The term "contrast" as herein employed indicates the average contrast derived from a characteristic curve of a radiographic film using as a first reference point (1) a density (D_1) of 0.25 above minimum density and as a second reference point (2) a density (D_2) of 2.0 above minimum density, where contrast is ΔD (i.e. 1.75) $\div \Delta \log E$ ($\log E_2 - \log E_1$), E_1 and E_2 being the exposure levels at the reference points (1) and (2).

[0023] "Gamma" is described as the instantaneous rate of change of a D vs. log E sensitometric curve or the instantaneous contrast at any log E value.

[0024] "Photographic speed" for the radiographic films refers to the exposure necessary to obtain a density of at least 1.0 plus D_{min} .

[0025] "Photographic speed" for the fluorescent intensifying screens refers to the percentage of photicity relative to a conventional KODAK MinR fluorescent intensifying screen.

[0026] "Photicity" is the integral from the minimum wavelength of the light emitted by the screen to the maximum wavelength of the intensity of light emitted by the screen divided by the sensitivity of the recording medium (film). This is shown by the following equation where $I(\lambda)$ is the intensity of the light emitted by the screen at wavelength λ and $S(\lambda)$ is the sensitivity of the film at wavelength λ . $S(\lambda)$ is in units of ergs/cm² required to reach a density of 1.0 above base plus fog.

$$Photicity = \int_{\lambda_{min}}^{\lambda_{max}} \frac{I(\lambda)}{S(\lambda)} d\lambda$$

[0027] Image tone can be evaluated using conventional CIELAB (Commission Internationale de l'Eclairage) a^* and b^* values that can be evaluated using the techniques described by Billmeyer et al., Principles of Color Technology, 2nd Edition, Wiley & Sons, New York, 1981, Chapter 3. The a^* value is a measure of reddish tone (positive a^*) or greenish tone (negative a^*). The b^* value is a measure of bluish tone (negative b^*) or yellowish tone (positive b^*).

[0028] The term " $d(\gamma)/d(\log E)$ " refers to a mathematical derivative or the slope of a gamma vs. log E sensitometric curve. This term can be obtained by providing a conventional D(density) vs. log E curve, mathematically differentiating that curve to provide a γ (gamma) vs. log E sensitometric curve, and then determining the slope of the "leading edge" (or rising side) of that curve.

[0029] Exposure latitude refers to the width (in logE terms) of the γ vs. log E sensitometric curve when measured at a specific gamma value. The curve width is measured in log E terms and upon conversion to the appropriate "antilog" provides a ratio of a specific number to 1.

[0030] The term "fully forehardened" is employed to indicate the forehardening of hydrophilic colloid layers to a level that limits the weight gain of a radiographic film to less than 120% of its original (dry) weight in the course of wet processing. The weight gain is almost entirely attributable to the ingestion of water during such processing.

[0031] The term "rapid access processing" is employed to indicate dry-to-dry processing of a radiographic film in 45 seconds or less. That is, 45 seconds or less elapse from the time a dry imagewise exposed radiographic film enters a wet processor until it emerges as a dry fully processed film.

[0032] In referring to grains and silver halide emulsions containing two or more halides, the halides are named in

order of ascending molar concentrations.

[0033] The term "equivalent circular diameter" (ECD) is used to define the diameter of a circle having the same projected area as a silver halide grain.

[0034] The term "aspect ratio" is used to define the ratio of grain ECD to grain thickness.

[0035] The term "coefficient of variation" (COV) is defined as 100 times the standard deviation (σ) of grain ECD divided by the mean grain ECD.

[0036] The term "covering power" is used to indicate 100 times the ratio of maximum density to developed silver measured in mg/dm^2 .

[0037] The term "dual-coated" is used to define a radiographic film having silver halide emulsion layers disposed on both the front- and backsides of the support. The radiographic silver halide films used in the present invention are "dual-coated."

[0038] The term "dynamic range" refers to the range of exposures over which useful images can be obtained (usually having a gamma greater than 2).

[0039] The units "kVp" and "MVp" stand for peak voltage applied to an X-ray tube times 10^3 and 10^6 , respectively.

[0040] The term "fluorescent intensifying screen" refers to a screen that absorbs X-radiation and emits light. A "prompt" emitting fluorescent intensifying screen will emit light immediately upon exposure to radiation while a "storage" fluorescent screen can "store" the exposing X-radiation for emission at a later time when the screen is irradiated with other radiation (usually visible light). The screens useful in the practice of the present invention are "prompt" emitting fluorescent intensifying screens.

[0041] The terms "front" and "back" refer to layers, films, or fluorescent intensifying screens nearer to and farther from, respectively, the source of X-radiation.

[0042] The term "rare earth" is used to indicate chemical elements having an atomic number of 39 or 57 through 71.

[0043] The radiographic silver halide films useful in this invention include a flexible support having disposed on both sides thereof, one or more photographic silver halide emulsion layers and optionally one or more non-radiation sensitive hydrophilic layer(s).

[0044] In preferred embodiments, the photographic silver halide film has a protective overcoat (described below) over all of the layers on each side of the support.

[0045] The support can take the form of any conventional radiographic film support that is X-radiation and light transmissive. Useful supports for the films of this invention can be chosen from among those described in *Research Disclosure*, September 1996, Item 38957 XV. Supports and *Research Disclosure*, Vol. 184, August 1979, Item 18431, XII. Film Supports.

[0046] The support is preferably a transparent film support. In its simplest possible form the transparent film support consists of a transparent film chosen to allow direct adhesion of the hydrophilic silver halide emulsion layers or other hydrophilic layers. More commonly, the transparent film is itself hydrophobic and subbing layers are coated on the film to facilitate adhesion of the hydrophilic silver halide emulsion layers. Typically the film support is either colorless or blue tinted (tinting dye being present in one or both of the support film and the subbing layers). Referring to *Research Disclosure*, Item 38957, Section XV Supports, cited above, attention is directed particularly to paragraph (2) that describes subbing layers, and paragraph (7) that describes preferred polyester film supports.

[0047] Polyethylene terephthalate and polyethylene naphthalate are the preferred transparent film support materials.

[0048] In the more preferred embodiments, at least one non-light sensitive hydrophilic layer is included with the one or more silver halide emulsion layers on each side of the film support. This layer may be called an interlayer or overcoat, or both.

[0049] The "frontside" of the support comprises one or more silver halide emulsion layers, at least one of which contains predominantly cubic grains (that is, more than 50 weight % of all grains). These cubic silver halide grains include predominantly (at least 78.5 mol %) bromide, and up to 98.75 mol % bromide, based on total silver in the cubic grain silver halide emulsion layer. In addition, these cubic grains must have from 1 to 20 mol % chloride (preferably from 10 to 20 mol % chloride) and from 0.25 to 1.5 mol % iodide (preferably from 0.5 to 1 mol % iodide), based on total silver in this cubic grain emulsion layer. The cubic silver halide grains in each silver halide emulsion unit (or silver halide emulsion layers) can be the same or different.

[0050] The amount of chloride in the cubic silver halide grains is critical to provide desired processability and image tone while the amount of iodide is critical to provide desired photographic speed. Too much chloride results in poor absorption of spectral sensitizing dyes to the grains.

[0051] The average silver halide grain size can vary within each radiographic silver halide film, and within each emulsion layer within that film. For example, the average grain size in each cubic grain silver halide emulsion layer is generally from 0.65 to 0.8 μm (preferably from 0.72 to 0.76 μm), but the average grain size can be different in the various other emulsion layers.

[0052] The non-cubic silver halide grains (if present) in the cubic grain emulsion layers can have any desirable morphology including, but not limited to, octahedral, tetradecahedral, rounded, spherical or other non-tabular morphologies,


or be comprised of a mixture of two or more of such morphologies.

[0053] As noted above, it is essential that at least one of the cubic grain silver halide emulsion layers comprise a combination of one or more first spectral sensitizing dyes and one or more second spectral sensitizing dyes that provide a combined J-aggregate absorption within the range of from 540 to 560 nm (preferably from 545 to 555 nm) when absorbed on the cubic silver halide grains. The one or more first spectral sensitizing dyes are anionic benzimidazole-benzoxazole carbocyanines and the one or more second spectral sensitizing dyes are anionic oxycarbocyanines.


[0054] Preferably, all cubic grain silver halide emulsions in the film contain one or more of these combinations of spectral sensitizing dyes. The combinations of dyes can be the same or different in each cubic grain silver halide emulsion layer. A most preferred combination of spectral sensitizing dyes A-2 and B-1 identified below has a combined J-aggregate absorption λ_{max} of 552 nm when absorbed to cubic silver halide grains.

[0055] The first and second spectral sensitizing dyes are provided on the cubic silver halide grains in a molar ratio of one or more first spectral sensitizing dyes to one or more second spectral sensitizing dyes of from 0.25:1 to 4:1, preferably at a molar ratio of from 0.5: 1 to 1.5: 1, and more preferably at a molar ratio of from 0.75:1 to 1.25:1. A most preferred combination of spectral sensitizing dyes A-2 and B-1 identified below is a molar ratio of 1:1. The useful total amounts of the first and second dyes in a given cubic grain silver halide emulsion layer are generally and independently within the range of from 0.1 to 1 mmol/mole of silver in the emulsion layer. Optimum amounts will vary with the particular dyes used and a skilled worker in the art would understand how to achieve optimal benefit with the combination of dyes in appropriate amounts. The total amount of both dyes is generally from 0.25 to 0.75 mmol/mole of silver.

[0056] Preferred "first" spectral sensitizing dyes can be represented by the following Structure I, and preferred "second" spectral sensitizing dyes can be represented by the following Structure II.

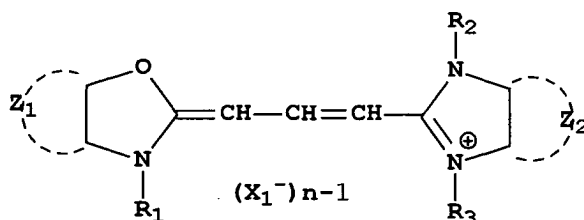

I

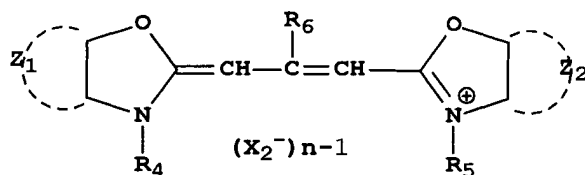

II

[0057] In both Structure I and II, Z_1 and Z_2 are independently the carbon atoms that are necessary to form a substituted or unsubstituted benzene or naphthalene ring. Preferably, each of Z_1 and Z_2 independently represent the carbon atoms necessary to form a substituted or unsubstituted benzene ring.

[0058] X_1^- and X_2^- are independently anions such as halides, thiocyanate, sulfate, perchlorate, *p*-toluene sulfonate, ethyl sulfate, and other anions readily apparent to one skilled in the art. In addition, "n" is 1 or 2, and it is 1 when the compound is an intermolecular salt.

[0059] In Structure I, R_1 , R_2 , and R_3 are independently alkyl groups having 1 to 10 carbon atoms, alkoxy groups having 1 to 10 carbon atoms, aryl groups having 6 to 10 carbon atoms in the aromatic ring, alkenyl groups having 2 to 8 carbon atoms, and other substituents that would be readily apparent to one skilled in the art. Such groups can be substituted with one or more hydroxy, alkyl, carboxy, sulfo, halo, and alkoxy groups. Preferably, at least one of the R_1 , R_2 , and R_3 groups comprises at least one sulfo or carboxy group.


[0060] Preferably, R_1 , R_2 , and R_3 are independently alkyl groups having 1 to 4 carbon atoms, phenyl groups, alkoxy groups having 1 to 4 carbon atoms, or alkenyl groups having 2 to 4 carbon atoms. All of these groups can be substituted

as described above, and in particular, they can be substituted with a sulfo or carboxy group.


[0061] In Structure II, R_4 and R_5 are independently defined as noted above for R_1 , R_2 , and R_3 . R_6 is hydrogen, an alkyl group having 1 to 4 carbon atoms, or a phenyl group, each of which groups can be substituted as described above for the other radicals.

[0062] Further details of such spectral sensitizing dyes are provided in U.S. Patent 4,659,654 (Metoki et al.). These dyes can be readily prepared using known synthetic methods, as described for example in Hamer, Cyanine Dyes and Related Compounds, John Wiley & Sons, 1964.


[0063] Representative "first" spectral sensitizing dyes useful in the practice of this invention include the following Compounds A-1 to A-7:

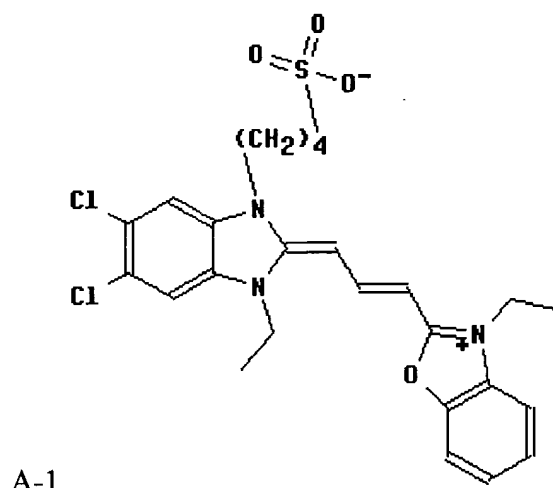


A-1

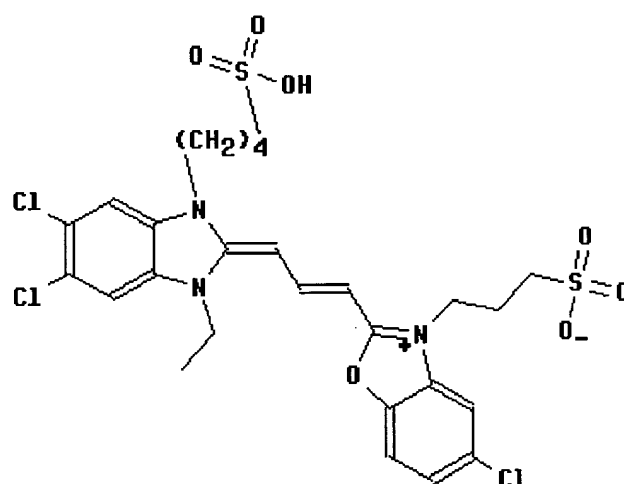


A-2

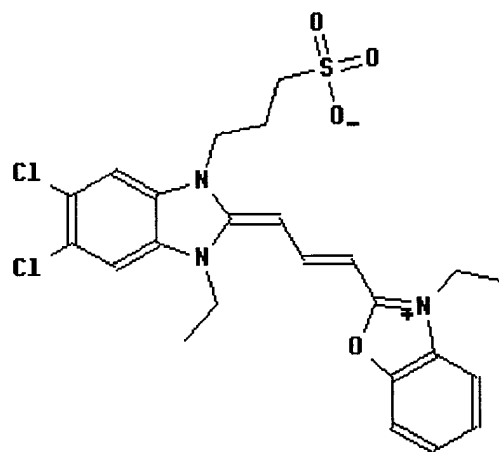


A-3

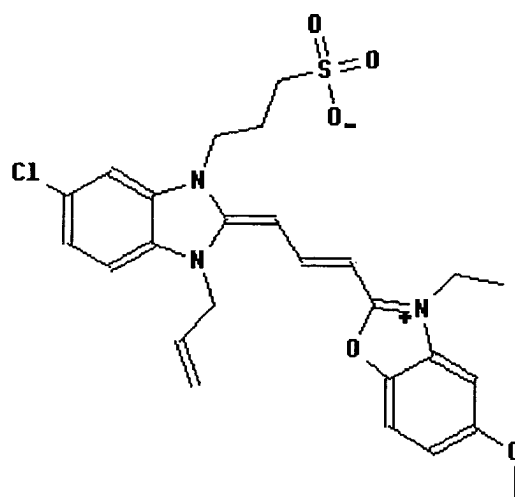


A-4

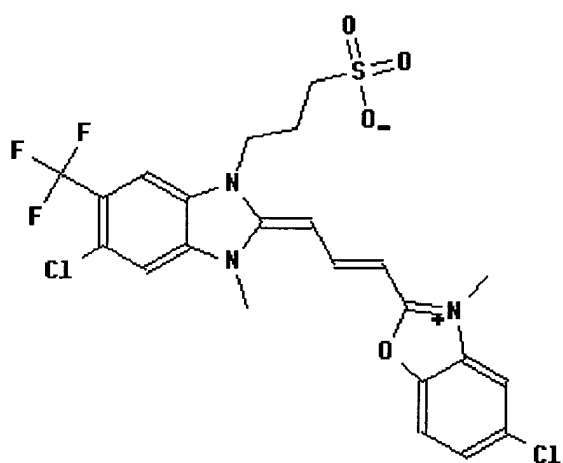

A-5

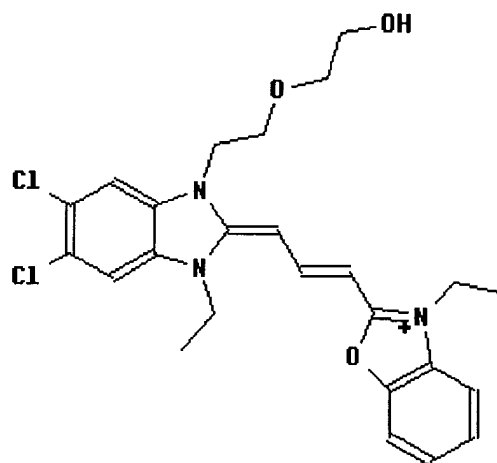


A-6

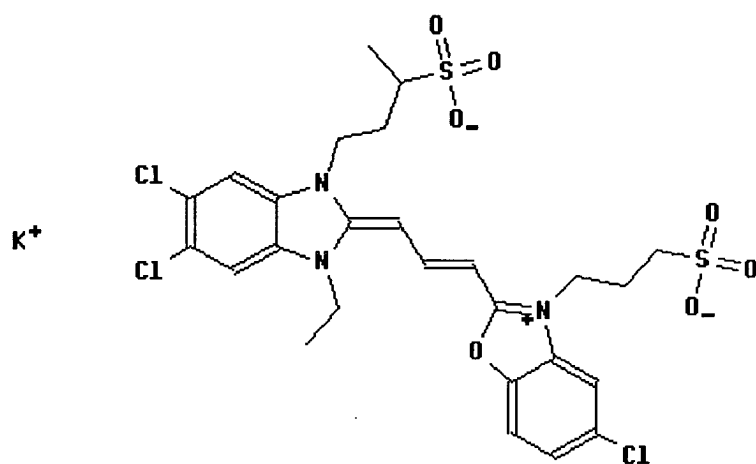


A-7




[0064] Representative "second" spectral sensitizing dyes useful in the practice of this invention include the following Compounds B-1 to B-5:

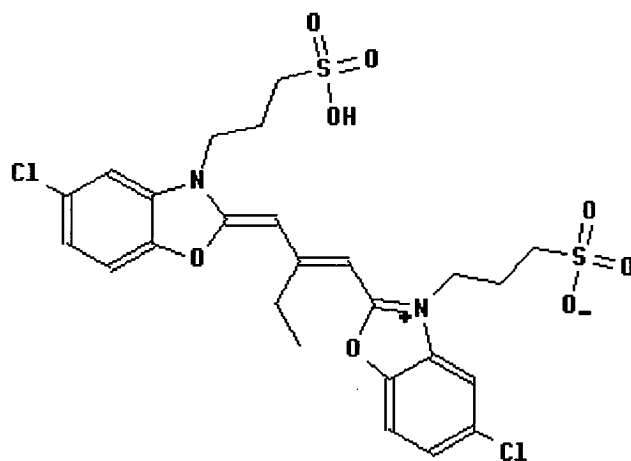

B-1

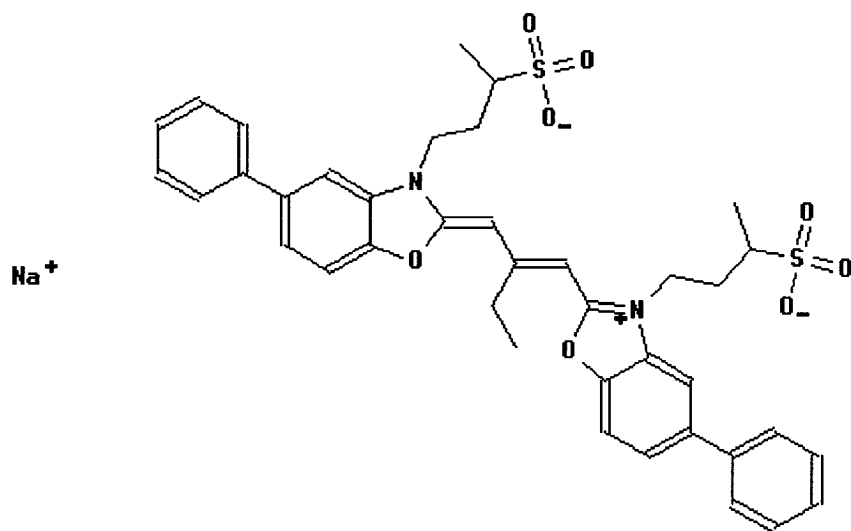

B-2

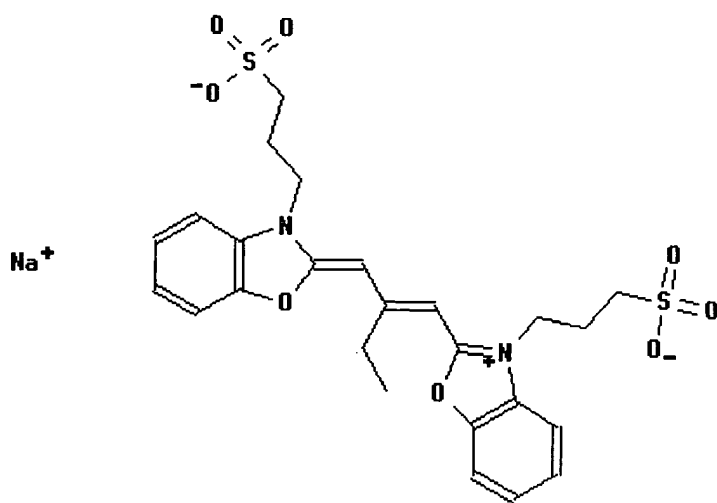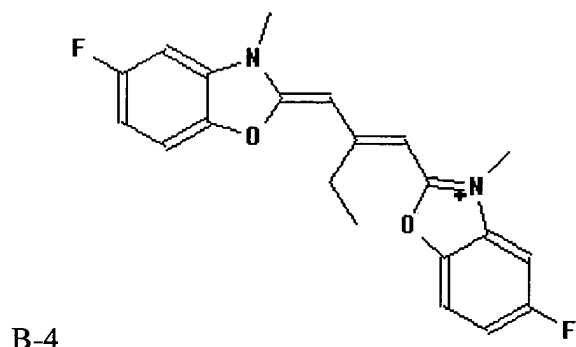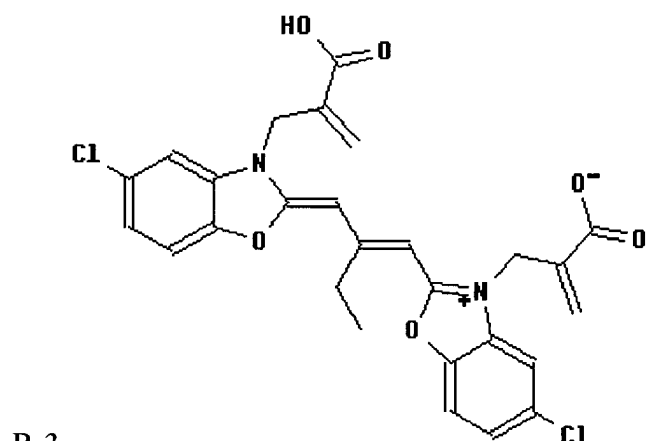

[0065] Another important feature of the radiographic film of this invention is the presence of one or more hexacoordination complex compounds as silver halide dopants in the cubic silver halide grains of one or more cubic grain emulsions. Preferably, only the cubic grains on the frontside of the film are doped with hexacoordination complex compounds. The term "dopant" is well known in photographic chemistry and generally refers to a compound that includes a metal ion that displaces silver in the crystal lattice of the silver halide grain, exhibits a positive valence of from 2 to 5, and has its highest energy electron occupied molecular orbital filled and its lowest energy unoccupied molecular orbital at an energy level higher than the lowest energy conduction band of the silver halide crystal lattice forming the protrusions.

[0066] The hexacoordination complex compounds particularly useful in the practice of this invention are represented by the following Structure I:



wherein M is a Group VIII polyvalent transition metal ion, L represents six coordination complex ligands that can be the same or different provided that at least four of the ligands are anionic ligands and at least one (preferably at least 3) of the ligands is more electronegative than any halide ligand, and n is -2, -3, or -4. Preferably, n is -3 or -4.

[0067] Examples of M include but are not limited to, Fe⁺², Ru⁺², Os⁺², Co⁺³, Rh⁺³, Ir⁺³, Pd⁺³, and Pt⁺⁴, and preferably M is Ru⁺². Examples of useful coordination complex ligands include but are not limited to, cyanide, pyrazine, chloride, iodide, bromide, oxycyanide, water, oxalate, thiocyanide, and carbon monoxide. Cyanide is a preferred coordination complex ligand.

[0068] Particularly useful dopants are ruthenium coordination complexes comprising at least 4 and more preferably 6 cyanide coordination complex ligands.

[0069] Mixtures of dopants described above can also be used.

[0070] The metal dopants can be introduced during emulsion precipitation using procedures well known in the art. They can be present in the dispersing medium present in the reaction vessel before grain nucleation. More typically, the metal coordination complexes are introduced at least in part during precipitation through one of the halide ion or silver ion jets or through a separate jet. Such procedures are described in U.S. Patent 4,933,272 (McDugle et al.) and U.S. Patent 5,360,712 (Olm et al.), cited therein.

[0071] While some dopants in the art are distributed uniformly throughout 100% of the volume of the silver halide grains, it is desired in the practice of this invention to provide the dopant in only a part of the grain volume, generally within 95% and preferably within 90% of the innermost volume from the center of the cubic silver halide grains. Methods for doing this are known in the art, for example is described in U.S. Patent 4,933,272 and U.S. Patent 5,360,712 (both noted above).

[0072] In other embodiments, the dopants are uniformly distributed in "bands" of the silver halide grains, for example, within a band that is from 50 to 80 innermost volume % (preferably from 75 to 80 innermost volume % for ruthenium hexacoordinating complex compounds) from the center or core of the cubic silver halide grains. One skilled in the art would readily know how to achieve these results by planned addition of the doping compounds during only a portion of the process used to prepare the silver halide.

[0073] It is also desired that the one or more dopants be present within the cubic grains in an amount of at least 1 x 10⁻⁶ mole, preferably from 1 x 10⁻⁶ to 5 x 10⁻⁴ mole, and more preferably from 1 x 10⁻⁵ to 5 x 10⁻⁴ mole, per mole of silver in the cubic grain emulsion layer.

[0074] The backside of the support also includes one or more silver halide emulsion layers, preferably at least one of which comprises tabular silver halide grains. Generally, at least 50% (and preferably at least 80%) of the silver halide grain projected area in this silver halide emulsion layer is provided by tabular grains having an average aspect ratio greater than 5, and more preferably greater than 10. The remainder of the silver halide projected area is provided by silver halide grains having one or more non-tabular morphologies. In addition, the tabular grains are predominantly (at least 90 mol %) bromide based on the total silver in the emulsion layer and can include up to 1 mol % iodide. Preferably, the tabular grains are pure silver bromide.


[0075] Tabular grain emulsions that have the desired composition and sizes are described in greater detail in the following patents:

[0076] U. S. Patent 4,414,310 (Dickerson), U.S. Patent 4,425,425 (Abbott et al.), U.S. Patent 4,425,426 (Abbott et al.), U.S. Patent 4,439,520 (Kofron et al.), U.S. Patent 4,434,226 (Wilgus et al.), U.S. Patent 4,435,501 (Maskasky), U.S. Patent 4,713,320 (Maskasky), U.S. Patent 4,803,150 (Dickerson et al.), U.S. Patent 4,900,355 (Dickerson et al.), U.S. Patent 4,994,355 (Dickerson et al.), U.S. Patent 4,997,750 (Dickerson et al.), U.S. Patent 5,021,327 (Bunch et al.), U.S. Patent 5,147,771 (Tsaur et al.), U.S. Patent 5,147,772 (Tsaur et al.), U.S. Patent 5,147,773 (Tsaur et al.), U.S. Patent 5,171,659 (Tsaur et al.), U.S. Patent 5,252,442 (Dickerson et al.), U.S. Patent 5,370,977 (Zietlow), U.S. Patent 5,391,469 (Dickerson), U.S. Patent 5,399,470 (Dickerson et al.), U.S. Patent 5,411,853 (Maskasky), U.S. Patent 5,418,125 (Maskasky), U.S. Patent 5,494,789 (Daubendiek et al.), U.S. Patent 5,503,970 (Olm et al.), U.S. Patent 5,536,632 (Wen et al.), U.S. Patent 5,518,872 (King et al.), U.S. Patent 5,567,580 (Fenton et al.), U.S. Patent 5,573,902 (Daubendiek et al.), U.S. Patent 5,576,156 (Dickerson), U.S. Patent 5,576,168 (Daubendiek et al.), U.S. Patent 5,576,171 (Olm et al.), and U.S. Patent 5,582,965 (Deaton et al.). The patents to Abbott et al., Fenton et al., Dickerson, and Dickerson et al. are also cited to show conventional radiographic film features in addition to gelatino-vehicle, high bromide (≥ 80 mol % bromide based on total silver) tabular grain emulsions and other features useful in the present invention.

[0077] The backside ("second major support surface") of the radiographic silver halide film also preferably includes an antihalation layer disposed over the silver halide emulsion layer(s). This layer comprises one or more antihalation dyes or pigments dispersed on a suitable hydrophilic binder (described below). In general, such antihalation dyes or pigments are chosen to absorb whatever radiation the film is likely to be exposed to from a fluorescent intensifying

screen. For example, pigments and dyes that can be used as antihalation pigments or dyes include various water-soluble, liquid crystalline, or particulate magenta or yellow filter dyes or pigments including those described for example in U.S. Patent 4,803,150 (Dickerson et al.), U.S. Patent 5,213,956 (Diehl et al.), U.S. Patent 5,399,690 (Diehl et al.), U.S. Patent 5,922,523 (Helber et al.), U.S. Patent 6,214,499 (Helber et al.), and Japanese Kokai 2-123349, all of which cited for pigments and dyes useful in the practice of this invention. One useful class of particulate antihalation dyes includes nonionic polymethine dyes such as merocyanine, oxonol, hemioxonol, styryl, and arylidene dyes as described in U.S. Patent 4,803,150 (noted above) that is cited for the definitions of those dyes. The magenta merocyanine and oxonol dyes are preferred and the oxonol dyes are most preferred.

[0078] The amounts of such dyes or pigments in the antihalation layer are generally from 1 to 2 mg/dm². A particularly useful antihalation dye is the magenta filter dye M-1 identified as follows:

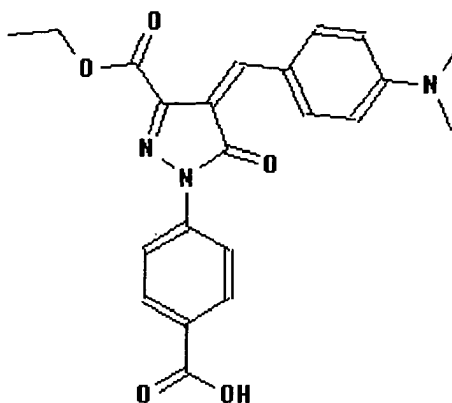

M-1.

[0079] A general summary of silver halide emulsions and their preparation is provided by *Research Disclosure*, Item 38957, cited above, Section I. Emulsion grains and their preparation. After precipitation and before chemical sensitization the emulsions can be washed by any convenient conventional technique using techniques disclosed by *Research Disclosure*, Item 38957, cited above, Section III. Emulsion washing.

[0080] The emulsions can be chemically sensitized by any convenient conventional technique as illustrated by *Research Disclosure*, Item 38957, Section IV. Chemical Sensitization: Sulfur, selenium or gold sensitization (or any combination thereof) are specifically contemplated. Sulfur sensitization is preferred, and can be carried out using for example, thiosulfates, thiosulfonates, thiocyanates, isothiocyanates, thioethers, thioureas, cysteine or rhodanine. A combination of gold and sulfur sensitization is most preferred.

[0081] Instability that increases minimum density in negative-type emulsion coatings (that is fog) can be protected against by incorporation of stabilizers, antifoggants, antikinking agents, latent-image stabilizers and similar addenda in the emulsion and contiguous layers prior to coating. Such addenda are illustrated by *Research Disclosure*, Item 38957, Section VII. Antifoggants and stabilizers, and Item 18431, Section II: Emulsion Stabilizers, Antifoggants and Antikinking Agents.

[0082] It may also be desirable that one or more silver halide emulsion layers include one or more covering power enhancing compounds adsorbed to surfaces of the silver halide grains. A number of such materials are known in the art, but preferred covering power enhancing compounds contain at least one divalent sulfur atom that can take the form of a -S- or =S moiety. Such compounds include, but are not limited to, 5-mercapotetrazoles, dithioxotriazoles, mercapto-substituted tetraazaindenes, and others described in U.S. Patent 5,800,976 (Dickerson et al.) that is cited for the teaching of the sulfur-containing covering power enhancing compounds.

[0083] The silver halide emulsion layers and other hydrophilic layers on both sides of the support of the radiographic films generally contain conventional polymer vehicles (peptizers and binders) that include both synthetically prepared and naturally occurring colloids or polymers. The most preferred polymer vehicles include gelatin or gelatin derivatives alone or in combination with other vehicles. Conventional gelatino-vehicles and related layer features are disclosed in *Research Disclosure*, Item 38957, Section II. Vehicles, vehicle extenders, vehicle-like addenda and vehicle related addenda. The emulsions themselves can contain peptizers of the type set out in Section II, paragraph A. Gelatin and hydrophilic colloid peptizers. The hydrophilic colloid peptizers are also useful as binders and hence are commonly present in much higher concentrations than required to perform the peptizing function alone. The preferred gelatin

vehicles include alkali-treated gelatin, acid-treated gelatin or gelatin derivatives (such as acetylated gelatin, deionized gelatin, oxidized gelatin and phthalated gelatin). Cationic starch used as a peptizer for tabular grains is described in U.S. Patent 5,620,840 (Maskasky) and U.S. Patent 5,667,955 (Maskasky). Both hydrophobic and hydrophilic synthetic polymeric vehicles can be used also. Such materials include, but are not limited to, polyacrylates (including polymethacrylates), polystyrenes and polyacrylamides (including polymethacrylamides). Dextrans can also be used. Examples of such materials are described for example in U.S. Patent 5,876,913 (Dickerson et al.).

[0084] The silver halide emulsion layers (and other hydrophilic layers) in the radiographic films are generally fully hardened using one or more conventional hardeners. Thus, the amount of hardener in each silver halide emulsion and other hydrophilic layer is generally at least 2% and preferably at least 2.5%, based on the total dry weight of the polymer vehicle in each layer (unless otherwise stated herein).

[0085] Conventional hardeners can be used for this purpose, including but not limited to formaldehyde and free dialdehydes such as succinaldehyde and glutaraldehyde, blocked dialdehydes, α -diketones, active esters, sulfonate esters, active halogen compounds, s-triazines and diazines, epoxides, aziridines, active olefins having two or more active bonds, blocked active olefins, carbodiimides, isoxazolium salts unsubstituted in the 3-position, esters of 2-alkoxy-N-carboxy-dihydroquinoline, N-carbamoyl pyridinium salts, carbamoyl oxypyridinium salts, bis(amidino) ether salts, particularly bis(amidino) ether salts, surface-applied carboxyl-activating hardeners in combination with complex-forming salts, carbamoylonium, carbamoyl pyridinium and carbamoyl oxypyridinium salts in combination with certain aldehyde scavengers, dication ethers, hydroxylamine esters of imidic acid salts and chloroformamidinium salts, hardeners of mixed function such as halogen-substituted aldehyde acids (for example, mucochloric and mucobromic acids), onium-substituted acroleins, vinyl sulfones containing other hardening functional groups, polymeric hardeners such as dialdehyde starches, and poly(acrolein-co-methacrylic acid).

[0086] An important feature of this invention is the presence of a mixture of hydrophilic binders in at least one of the cubic silver halide grain emulsions on the frontside of the films of this invention. This mixture of hydrophilic binders includes gelatin or a gelatin derivative (as defined above) as a "first" binder (or a mixture of gelatin and gelatin derivatives), and a "second" hydrophilic binder (or mixture thereof) that is not gelatin or a gelatin derivative. Preferably, this mixture of binders is present in the frontside cubic grain silver halide emulsion layer that also includes the mixture of first and second spectral sensitizing dyes, the hexacoordination complex compounds as dopants, and the unique combination of silver bromide, silver iodide, and silver chloride in the cubic grains described above.

[0087] Useful "second" hydrophilic binders include, but are not limited to, polyacrylates (including polymethacrylates), polystyrenes and polyacrylamides (including polymethacrylamides), dextrans, and various polysaccharides. Examples of such materials are described for example in U.S. Patent 5,876,913 (Dickerson et al.). The dextrans are preferred.

[0088] The weight ratio of first hydrophilic binder (or mixture thereof) to second hydrophilic binder (or mixture thereof) in the cubic grain silver halide emulsion layer is from 2:1 to 5:1. Preferably, this weight ratio is from 2.5:1 to 3.5:1. A most preferred weight ratio is 3:1.

[0089] The cubic grain silver halide emulsion layers in the radiographic films are generally hardened to various degrees using one or more conventional hardeners. Conventional hardeners can be used for this purpose, including but not limited to those described above.

[0090] The cubic grain silver halide emulsion layer comprising the mixture of first and second binders includes a critical amount of one or more hardeners that is at least 0.4 weight % based on the total binder weight in that emulsion layer. Preferably, the amount of hardener in that emulsion layer is from 0.5 to 1.5 weight % and a most preferred amount is 1 weight %. While any of the noted conventional hardeners can be used, the preferred hardeners include bisvinyl-sulfonylmethylether and bisvinylsulfonylmethane.

[0091] The levels of silver and polymer vehicle in the radiographic silver halide film used in the present invention are not critical. In general, the total amount of silver on each side of each film is at least 10 and no more than 55 mg/dm² in one or more emulsion layers. In addition, the total amount of polymer vehicle on each side of each film is generally at least 35 and no more than 45 mg/dm² in one or more hydrophilic layers. The amounts of silver and polymer vehicle on the two sides of the support in the radiographic silver halide film can be the same or different. Preferably, the amounts are different. These amounts refer to dry weights.

[0092] The radiographic silver halide films useful in this invention generally include a surface protective overcoat on each side of the support that typically provides physical protection of the emulsion and other hydrophilic layers. Each protective overcoat can be sub-divided into two or more individual layers. For example, protective overcoats can be sub-divided into surface overcoats and interlayers (between the overcoat and silver halide emulsion layers). In addition to vehicle features discussed above the protective overcoats can contain various addenda to modify the physical properties of the overcoats. Such addenda are illustrated by *Research Disclosure*, Item 38957, Section IX. Coating physical property modifying addenda, A. Coating aids, B. Plasticizers and lubricants, C. Antistats, and D. Matting agents. Interlayers that are typically thin hydrophilic colloid layers can be used to provide a separation between the emulsion layers and the surface overcoats. The overcoat on at least one side of the support can also include a blue toning dye or a tetraazaindene (such as 4-hydroxy-6-methyl-1,3,3a,7-tetraazaindene) if desired.

[0093] The protective overcoat is generally comprised of one or more hydrophilic colloid vehicles, chosen from among the same types disclosed above in connection with the emulsion layers. Protective overcoats are provided to perform two basic functions. They provide a layer between the emulsion layers and the surface of the film for physical protection of the emulsion layer during handling and processing. Secondly, they provide a convenient location for the placement of addenda, particularly those that are intended to modify the physical properties of the radiographic film. The protective overcoats of the films of this invention can perform both these basic functions.

[0094] The various coated layers of radiographic silver halide films used in this invention can also contain tinting dyes to modify the image tone to transmitted or reflected light. These dyes are not decolorized during processing and may be homogeneously or heterogeneously dispersed in the various layers. Preferably, such non-bleachable tinting dyes are in a silver halide emulsion layer.

[0095] The radiographic imaging assemblies of the present invention are composed of one radiographic silver halide film as described herein and one or more fluorescent intensifying screens. Preferably, the imaging assembly includes a single fluorescent intensifying screen. Fluorescent intensifying screens are typically designed to absorb X-rays and to emit electromagnetic radiation having a wavelength greater than 300 nm. These screens can take any convenient form providing they meet all of the usual requirements for use in radiographic imaging. Examples of conventional, useful fluorescent intensifying screens and methods of making them are provided by *Research Disclosure*, Item 18431, cited above, Section IX. X-Ray Screens/Phosphors, and U.S. Patent 5,021,327 (Bunch et al.), U.S. Patent 4,994,355 (Dickerson et al.), U.S. Patent 4,997,750 (Dickerson et al.), and U.S. Patent 5,108,881 (Dickerson et al.). The fluorescent layer contains phosphor particles and a binder, optimally additionally containing a light scattering material, such as titania or light absorbing materials such as particulate carbon, dyes or pigments. Any conventional binder (or mixture thereof) can be used but preferably the binder is an aliphatic polyurethane elastomer or another highly transparent elastomeric polymer.

[0096] Any conventional or useful phosphor can be used, singly or in mixtures, in the intensifying screens used in the practice of this invention. For example, useful phosphors are described in numerous references relating to fluorescent intensifying screens, including but not limited to, *Research Disclosure*, Vol. 184, August 1979, Item 18431, Section IX, X-ray Screens/Phosphors, and U.S. Patent 2,303,942 (Wynd et al.), U.S. Patent 3,778,615 (Luckey), U.S. Patent 4,032,471 (Luckey), U.S. Patent 4,225,653 (Brixner et al.), U.S. Patent 3,418,246 (Royce), U.S. Patent 3,428,247 (Yocon), U.S. Patent 3,725,704 (Buchanan et al.), U.S. Patent 2,725,704 (Swindells), U.S. Patent 3,617,743 (Rabatin), U.S. Patent 3,974,389 (Ferri et al.), U.S. Patent 3,591,516 (Rabatin), U.S. Patent 3,607,770 (Rabatin), U.S. Patent 3,666,676 (Rabatin), U.S. Patent 3,795,814 (Rabatin), U.S. Patent 4,405,691 (Yale), U.S. Patent 4,311,487 (Luckey et al.), U.S. Patent 4,387,141 (Patten), U.S. Patent 5,021,327 (Bunch et al.), U.S. Patent 4,865,944 (Roberts et al.), U.S. Patent 4,994,355 (Dickerson et al.), U.S. Patent 4,997,750 (Dickerson et al.), U.S. Patent 5,064,729 (Zegarski), U.S. Patent 5,108,881 (Dickerson et al.), U.S. Patent 5,250,366 (Nakajima et al.), U.S. Patent 5,871,892 (Dickerson et al.), EP-A-0 491,116 (Benzo et al.), the disclosures of all of which are cited with respect to the phosphors.

[0097] Useful classes of phosphors include, but are not limited to, calcium tungstate (CaWO_4) activated or unactivated lithium stannates, niobium and/or rare earth activated or unactivated yttrium, lutetium, or gadolinium tantalates, rare earth (such as terbium, lanthanum, gadolinium, cerium, and lutetium)-activated or unactivated middle chalcogen phosphors such as rare earth oxychalcogenides and oxyhalides, and terbium-activated or unactivated lanthanum and lutetium middle chalcogen phosphors.

[0098] Still other useful phosphors are those containing hafnium as described for example in U.S. Patent 4,988,880 (Bryan et al.), U.S. Patent 4,988,881 (Bryan et al.), U.S. Patent 4,994,205 (Bryan et al.), U.S. Patent 5,095,218 (Bryan et al.), U.S. Patent 5,112,700 (Lambert et al.), U.S. Patent 5,124,072 (Dole et al.), and U.S. Patent 5,336,893 (Smith et al.).

[0099] Some preferred rare earth oxychalcogenide and oxyhalide phosphors are represented by the following formula (1):



wherein M' is at least one of the metals yttrium (Y), lanthanum (La), gadolinium (Gd), or lutetium (Lu), M'' is at least one of the rare earth metals, preferably dysprosium (Dy), erbium (Er), europium (Eu), holmium (Ho), neodymium (Nd), praseodymium (Pr), samarium (Sm), tantalum (Ta), terbium (Tb), thulium (Tm), or ytterbium (Yb), X' is a middle chalcogen (S, Se, or Te) or halogen, n is 0.002 to 0.2, and w is 1 when X' is halogen or 2 when X' is a middle chalcogen. These include rare earth-activated lanthanum oxybromides, and terbium-activated or thulium-activated gadolinium oxides such as $\text{Gd}_2\text{O}_2\text{S:Tb}$.

[0100] Other suitable phosphors are described in U.S. Patent 4,835,397 (Arakawa et al.) and U.S. Patent 5,381,015 (Dooms), including for example divalent europium and other rare earth activated alkaline earth metal halide phosphors

and rare earth element activated rare earth oxyhalide phosphors. Of these types of phosphors, the more preferred phosphors include alkaline earth metal fluorohalide prompt emitting and/or storage phosphors [particularly those containing iodide such as alkaline earth metal fluorobromiodide storage phosphors as described in U.S. Patent 5,464,568 (Bringley et al.)].

[0101] Another class of useful phosphors includes rare earth hosts such as rare earth activated mixed alkaline earth metal sulfates such as europium-activated barium strontium sulfate.

[0102] Particularly useful phosphors are those containing doped or undoped tantalum such as YTaO_4 , $\text{YTaO}_4\text{:Nb}$, Y(Sr)TaO_4 , and $\text{Y(Sr)TaO}_4\text{:Nb}$. These phosphors are described in U.S. Patent 4,226,653 (Brixner), U.S. Patent 5,064,729 (Zegarski), U.S. Patent 5,250,366 (Nakajima et al.), and U.S. Patent 5,626,957 (Benso et al.).

[0103] Other useful phosphors are alkaline earth metal phosphors that can be the products of firing starting materials comprising optional oxide and a combination of species characterized by the following formula (2):



wherein "M" is magnesium (Mg), calcium (Ca), strontium (Sr), or barium (Ba), "F" is fluoride, "X" is chloride (Cl) or bromide (Br), "I" is iodide, M^a is sodium (Na), potassium (K), rubidium (Rb), or cesium (Cs), X^a is fluoride (F), chloride (Cl), bromide (Br), or iodide (I), "A" is europium (Eu), cerium (Ce), samarium (Sm), or terbium (Tb), "Q" is BeO, MgO, CaO, SrO, BaO, ZnO, Al_2O_3 , La_2O_3 , In_2O_3 , SiO_2 , TiO_2 , ZrO_2 , GeO_2 , SnO_2 , Nb_2O_5 , Ta_2O_5 , or ThO_2 , "D" is vanadium (V), chromium (Cr), manganese (Mn), iron (Fe), cobalt (Co), or nickel (Ni). The numbers in the noted formula are the following: "z" is 0 to 1, "u" is from 0 to 1, "y" is from 1×10^{-4} to 0.1, "e" is from 0 to 1, and "t" is from 0 to 0.01. These definitions apply wherever they are found in this application unless specifically stated to the contrary. It is also contemplated that "M", "X", "A", and "D" represent multiple elements in the groups identified above.

[0104] Some fluorescent intensifying screens useful in the present invention have as the preferred phosphor, a gadolinium oxysulfide:terbium phosphor. Moreover, the particle size distribution of the phosphor particles is an important factor in determining the speed and sharpness of the screen. For example, at least 50% of the particles have a size of less than 3 μm and 85% of the particles have a size of less than 5.5 μm . In addition, the coverage of phosphor in the dried layer is from 260 to 380 g/m^2 , and preferably from 290 to 350 g/m^2 .

[0105] Flexible support materials for radiographic screens in accordance with the present invention include cardboard, plastic films such as films of cellulose acetate, polyvinyl chloride, polyvinyl acetate, polyacrylonitrile, polystyrene, polyester, polyethylene terephthalate, polyamide, polyimide, cellulose triacetate and polycarbonate, metal sheets such as aluminum foil and aluminum alloy foil, ordinary papers, baryta paper, resin-coated papers, pigmented papers containing titanium dioxide or the like, and papers sized with polyvinyl alcohol or the like. A plastic film is preferably employed as the support material.

[0106] The plastic film may contain a light-absorbing material such as carbon black, or may contain a light-reflecting material such as titanium dioxide or barium sulfate. The former is appropriate for preparing a high-resolution type radiographic screen, while the latter is appropriate for preparing a high-sensitivity type radiographic screen. For use in this invention it is highly preferred that the support absorb substantially all of the radiation emitted by the phosphor. Examples of particularly preferred supports include polyethylene terephthalate, blue colored or black colored (for example, LUMIRROR C, type X30 supplied by Toray Industries, Tokyo, Japan).

[0107] These supports may have thickness that is generally between 60 and 1000 μm , more preferably between 80 and 500 μm .

[0108] A representative fluorescent intensifying screen useful in the present invention is described in the example below.

[0109] An embodiment of the present invention is illustrated in FIG. 1. In reference to the imaging assembly **10** shown in FIG. 1, fluorescent intensifying screen **20** is arranged in association with radiographic silver halide film **30** in cassette holder **40**.

[0110] Exposure and processing of the radiographic silver halide films can be undertaken in any convenient conventional manner. The exposure and processing techniques of U.S. Patent 5,021,327 and U.S. Patent 5,576,156 (both noted above) are typical for processing radiographic films. Other processing compositions (both developing and fixing compositions) are described in U.S. Patent 5,738,979 (Fitterman et al.), U.S. Patent 5,866,309 (Fitterman et al.), U.S. Patent 5,871,890 (Fitterman et al.), U.S. Patent 5,935,770 (Fitterman et al.), U.S. Patent 5,942,378 (Fitterman et al.). The processing compositions can be supplied as single- or multi-part formulations, and in concentrated form or as more diluted working strength solutions.

[0111] Exposing X-radiation is generally directed through a fluorescent intensifying screen before it passes through the radiographic silver halide film for imaging soft tissue such as breast tissue. X-radiation can be generated at 28 kVp or less using conventional equipment that comprises rhodium or tungsten anodes. In other embodiments the x-radiation

is generated at greater than 28 kVp. Preferably, the peak voltage is 30 kVp or more in such embodiments.

[0112] It is particularly desirable that the radiographic silver halide films be processed within 90 seconds ("dry-to-dry") and preferably within 60 seconds and at least 20 seconds, for the developing, fixing, any washing (or rinsing) steps, and drying. Such processing can be carried out in any suitable processing equipment including but not limited to, a Kodak X-OMAT™ RA 480 processor that can utilize Kodak Rapid Access processing chemistry. Other "rapid access processors" are described for example in U.S. Patent 3,545,971 (Barnes et al.) and EP 0 248,390A1 (Akio et al.). Preferably, the black-and-white developing compositions used during processing are free of any gelatin hardeners, such as glutaraldehyde.

[0113] Since rapid access processors employed in the industry vary in their specific processing cycles and selections of processing compositions, the preferred radiographic films satisfying the requirements of the present invention are specifically identified as those that are capable of dry-to-dye processing according to the following reference conditions:

Development	11.1 seconds at 35°C,
Fixing	9.4 seconds at 35°C,
Washing	7.6 seconds at 35°C,
Drying	12.2 seconds at 55-65°C.

Any additional time is taken up in transport between processing steps. Typical black-and-white developing and fixing compositions are described in the Example below.


[0114] Radiographic kits can include a radiographic imaging assembly of this invention, one or more additional fluorescent intensifying screens and/or metal screens, and/or one or more suitable processing compositions (for example black-and-white developing and fixing compositions).

[0115] The following example is presented for illustration and the invention is not to be interpreted as limited thereby.

Example 1:

Radiographic Film A (Control):

[0116] Radiographic Film A was a single-coated film having the a silver halide emulsion on one side of a blue-tinted 170 µm transparent poly(ethylene terephthalate) film support and a pelloid layer on the opposite side. The emulsion was chemically sensitized with sulfur and gold and spectrally sensitized with the following dye A-1:

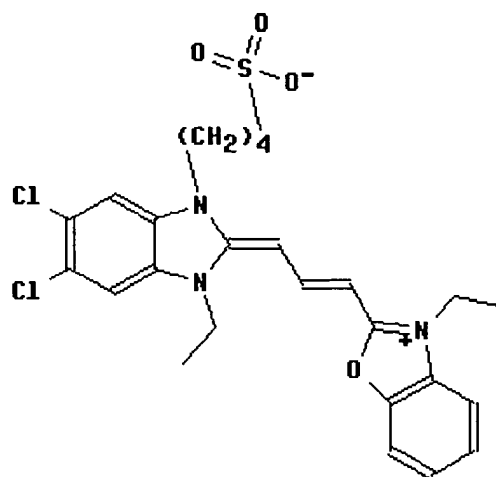

A-1.

[0117] Radiographic Film A had the following layer arrangement:

Overcoat
Interlayer
Emulsion Layer
Support

Peloid Layer
Overcoat



[0118] The noted layers were prepared from the following formulations.



Overcoat Formulation	Coverage (mg/dm ²)
Gelatin vehicle	4.4
Methyl methacrylate matte beads	0.35
Carboxymethyl casein	0.73
Colloidal silica (LUDOX AM)	1.1
Polyacrylamide	0.85
Chrome alum	0.032
Resorcinol	0.073
Dow Corning Silicone	0.153
TRITON X-200 surfactant (Union Carbide)	0.26
LODYNE S-100 surfactant (Ciba Specialty Chem.)	0.0097

Interlayer Formulation	Coverage (mg/dm ²)
Gelatin vehicle	4.4

Emulsion Layer Formulation	Coverage (mg/dm ²)
Cubic grain emulsion [AgBr 0.85 μ m average size]	51.1
Gelatin vehicle	34.9
Spectral sensitizing dye A-1	250 mg/Ag mole
4-Hydroxy-6-methyl-1,3, 3 a,7-tetraazaindene	1 g/Ag mole
Maleic acid hydrazide	0.0075
Catechol disulfonate	0.42
Glycerin	0.22
Potassium bromide	0.14
Resorcinol	2.12
Bisvinylsulfonylmethylether	0.4% based on total gelatin in all layers on that side

Peloid Layer	Coverage (mg/dm ²)
Gelatin	43
Dye C-1 noted below	0.31
Dye C-2 noted below	0.11
Dye C-3 noted below	0.13
Dye C-4 note below	0.12
Bisvinylsulfonylmethylether	0.4% based on total gelatin in all layers on that side

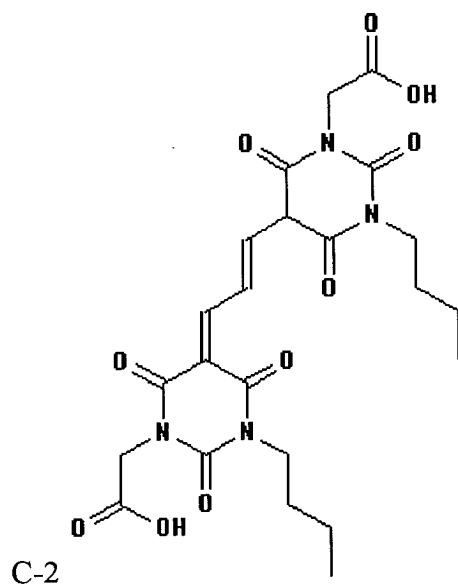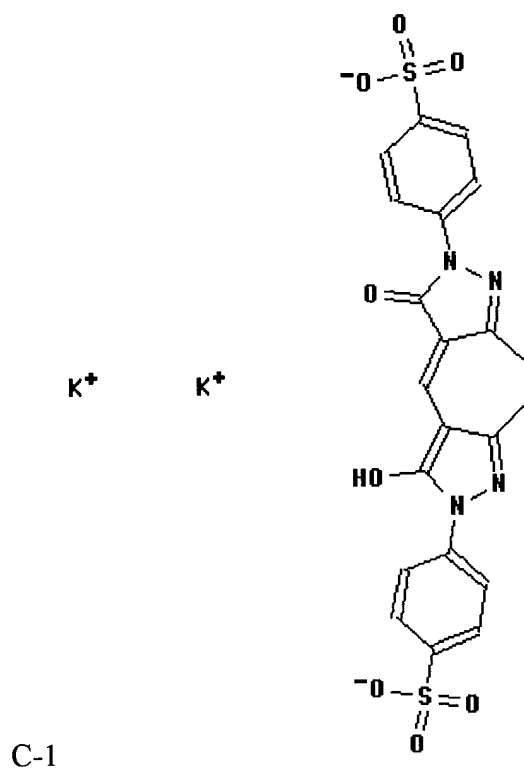

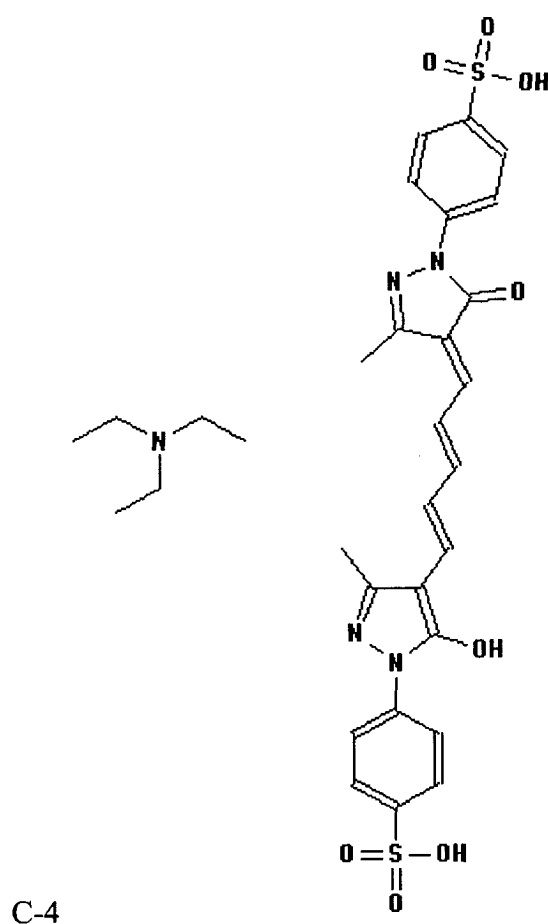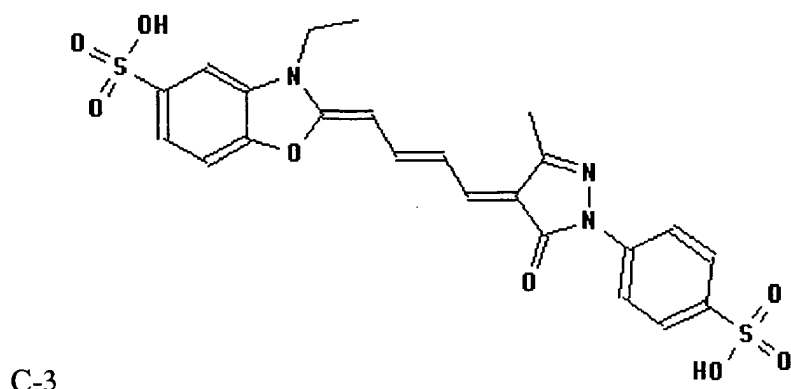

50

Radiographic Film B (Invention):

55

[0119] Radiographic Film B was a dual-coated radiographic film with 2/3 of the silver and gelatin coated on one side of the support and the remainder coated on the opposite side of the support. It also included a halation control layer containing solid particle dyes to provide improved sharpness. The film contained a green-sensitive, high aspect ratio tabular silver bromide grain emulsion on both sides of the support. Thus, at least 50% of the total grain projected area is accounted for by tabular grains having a thickness of less than 0.3 μm and having an average aspect ratio greater than 8:1. The emulsion average grain diameter was 2.0 μm and the average grain thickness was 0.10 μm . It was polydisperse in distribution and had a coefficient of variation of 38. The emulsion was spectrally sensitized with anhydro-5,5-dichloro-9-ethyl-3,3'-bis(3-sulfopropyl)oxacarbo-cyanine hydroxide (680 mg/Ag mole), followed by potassium io-

EP 1 422 557 A1

dide (300 mg/Ag mole). The frontside cubic grain silver halide emulsion comprised cubic grains spectrally sensitized with a 1:1 molar ratio of dyes A-2 and B-1 (noted above). The cubic grains were doped with ruthenium hexacyanide (50 mg/Ag mole). Film B had the following layer arrangement and formulations on the film support:

- 5 Overcoat 1
- Interlayer
- Emulsion Layer 1
- Support
- Emulsion Layer 2
- 10 Halation Control Layer
- Overcoat 2

15

20

25

Overcoat 1 Formulation	Coverage (mg/dm ²)
Gelatin vehicle	4.4
Methyl methacrylate matte beads	0.35
Carboxymethyl casein	0.73
Colloidal silica (LUDOX AM)	1.1
Polyacrylamide	0.85
Chrome alum	0.032
Resorcinol	0.73
Dow Corning Silicone	0.153
TRITON X-200 surfactant	0.26
LODYNE S-100 surfactant	0.0097

30

Interlayer Formulation	Coverage (mg/dm ²)
Gelatin vehicle	4.4

35

40

45

Emulsion Layer 1 Formulation	Coverage (mg/dm ²)
Cubic grain emulsion [AgIClBr 5:15:84.5 halide molar ratio 0.73 µm average size]	40.3
Gelatin vehicle	22.6
Dextran	8.1
4-Hydroxy-6-methyl-1,3,3a,7-tetraazaindene	1 g/Ag mole
1-(3-Acetamidophenyl)-5-mercaptotetrazole	0.026
Maleic acid hydrazide	0.0076
Catechol disulfonate	0.2
Glycerin	0.22
Potassium bromide	0.13
Resorcinol	2.12
Bisvinylsulfonylmethane	0.8 % based on total gelatin in all layers on that side

50

55

Emulsion Layer 2 Formulation	Coverage (mg/dm ²)
Tabular grain emulsion [AgBr 2.9 x 0.10 µm average size]	10.7
Gelatin vehicle	16.1
4-Hydroxy-6-methyl-1,3,3a,7-tetraazaindene	2.1 g/Ag mole
1-(3-Acetamidophenyl)-5-mercaptotetrazole	0.013
Maleic acid hydrazide	0.0032
Catechol disulfonate	0.2

(continued)

Emulsion Layer 2 Formulation	Coverage (mg/dm ²)
Glycerin	0.11
Potassium bromide	0.06
Resorcinol	1.0
Bisvinylsulfonylmethane	2 % based on total gelatin in all layers on that side

Halation Control Layer	Coverage (mg/dm ²)
Magenta filter dye M-1 (noted above)	2.2
Gelatin	10.8

Overcoat 2 Formulation	Coverage (mg/dm ²)
Gelatin vehicle	8.8
Methyl methacrylate matte beads	0.14
Carboxymethyl casein	1.25
Colloidal silica (LUDOX AM)	2.19
Polyacrylamide	1.71
Chrome alum	0.066
Resorcinol	0.15
Dow Corning Silicone	0.16
TRITON X-200 surfactant	0.26
LODYNE S-100 surfactant	0.01

[0120] The cassettes used in the practice of this invention were those commonly used in mammography.

[0121] Fluorescent intensifying screen "X" had the same composition and structure as commercially available KODAK Min-R 2000 Screen. It comprised a terbium activated gadolinium oxysulfide phosphor (median particle size of about 4.0 μm) dispersed in a Permuthane TM polyurethane binder on a blue-tinted poly(ethylene terephthalate) film support. The total phosphor coverage was 315 g/m² and the phosphor to binder weight ratio was 21:1.

[0122] In the practice of this invention, a single screen X was placed in back of the film to form a radiographic imaging assembly.

[0123] Samples of the films in the imaging assemblies were imaged using a commercially available GE DMR Mammographic X-ray unit equipped with both molybdenum and rhodium anodes. It was capable of accelerating voltages of 25,000-40,000 volts. Images were made using an RMI 156 phantom (available from Gammex-RMI, Middleton, Wisconsin), and RMI phantom 165, and a Kodak-Pathe "Indicateur de Technique Operatoire" phantom.

[0124] The film samples were processed using a processor commercially available under the trademark KODAK RP X-OMAT® film Processor M6A-N, M6B, or M35A. Development was carried out using the following black-and-white developing composition:

Hydroquinone	30 g
Phenidone	1.5 g
Potassium hydroxide	21 g
NaHCO ₃	7.5 g
K ₂ SO ₃	44.2 g
Na ₂ S ₂ O ₅	12.6 g
Sodium bromide	35 g
5-Methylbenzotriazole	0.06 g
Glutaraldehyde	4.9 g
Water to 1 liter, pH 10	

[0125] The film samples were processed in each instance for less than 90 seconds (dry-to-dry). Fixing was carried

out using KODAK RP X-OMAT® LO Fixer and Replenisher fixing composition (Eastman Kodak Company).

[0126] Optical densities are expressed below in terms of diffuse density as measured by a conventional X-rite Model 310TM densitometer that was calibrated to ANSI standard PH 2.19 and was traceable to a National Bureau of Standards calibration step tablet. The characteristic D vs. log E curve was plotted for each radiographic film that was imaged and processed. Speed was measured at a density of $1.4 + D_{\min}$. Gamma (contrast) is the slope (derivative) of the noted curves.

[0127] "Entrance Exposure" (mR) refers to the amount of X-radiation exposure (measured in milliRoentgens) that impinges on the surface of the phantom (or patient) closest to the X-radiation source.

[0128] The " Δ Density" refers to the difference in diffuse optical density between two specified parts of the phantom (or patient).

[0129] "Image noise" was determined by a visual comparison of the resulting image to an image obtained using the conventional KODAK Min-R 2000 Mammography film and KODAK Min-R 2000 intensifying screen. The resulting images were rated by an experienced observer on a scale of from 1 to 6 where a rating of "1" represents the lowest noise and a rating of "6" represents the highest noise.

[0130] "Image resolution" refers to the ability of an experienced observer to discern discrete lines in a low contrast resolution test pattern. Resolution was measured in a line pair per millimeter. The resulting images were rated by a very experienced observer on a scale of from 1 to 6 where a rating of "1" represents the highest resolution and a rating of "6" represents the lowest resolution.

[0131] "Image quality" refers to the ability of a human observer easily and clearly to discern low contrast objects and fine details in the phantoms (or patients). The resulting images were rated by an experienced observer on a scale of from 1 to 6 where a rating of "1" represents the best image quality and a rating of "6" represents the poorest image quality.

[0132] The term " $d(\gamma)/d(\log E)$ " was determined as described above.

[0133] The following TABLES I and II show the results of imaging and processing of Films A and B. It is apparent from the data that using the rhodium anodes in the imaging equipment with the Control radiographic film allowed for a reduction in patient X-radiation dose but the resulting images were poorer in quality. For the radiographic film of the present invention, however, the use of the rhodium anodes provided a patient X-radiation dose reduction and improved image quality relative to the Control film.

[0134] In addition, the film of the present invention (Film B) provided increased contrast in the mid-scale region as indicated by the increase in the " $d(\gamma)/d(\log E)$ " value.

TABLE I

Film	kVp	Screen	Target/- Filter*	Entrance Exposure (mR)	Δ Density	Image Resolution	Image Noise	Image Quality
A (Control)	28	X	Mo/Mo	1x	1x	2	2	4
A (Control)	28	X	Rh/Rh	0.52x	0.85x	3	3	6
B (Invention)	28	X	Mo/Mo	1x	1.19x	1	1	2
B (Invention)	28	X	Rh/Rh	0.53x	1.15x	1	2	3

* "Mo" refers to molybdenum anodes and "Rh" refers to rhodium anodes.

TABLE II

Film	kVp	Screen	Target/-Filter*	$d(\gamma)/d(\log E)$
A (Control)	28	X	Mo/Mo	4.25
A (Control)	28	X	Rh/Rh	4.25
B (Invention)	28	X	Mo/Mo	6.25
B (Invention)	28	X	Rh/Rh	6.25

Example 2:

[0135] Films A and B were imaged and processed as described in Example 1. The following TABLE III shows the results of imaging and processing of Films A and B. It is apparent from the data that image quality is degraded in Film A when the imaging peak voltage was increased from 28 to 32 kVp. However, when the peak voltage was similar increased using Film B, image quality was restored at the lower patient dosage. Film B was a radiographic film having the characteristics required for the present invention.

TABLE III

Film	kVp	Screen	Target/- Filter*	Entrance Exposure (mR)	Δ Density	Image Resolution	Image Noise	Image Quality
A(Control)	28	X	Mo/Mo	1x	1x	2	2	4
A (Control)	30	X	Mo/Mo	0.85x	0.93x	2.5	2	4.5
A (Control)	32	X	Mo/Mo	0.74x	0.94x	3	3	6
B (Control)	28	X	Mo/Mo	1x	1.19x	1	1	2
B (Invention)	30	X	Mo/Mo	0.86x	1.15x	1.5	1	2.5
B (Invention)	32	X	Mo/Mo	0.73x	1.10x	2	2	4

* "Mo" refers to molybdenum anodes.

Example 3:

[0136] Films A and B were imaged and processed as described in Example 1 using preferred patient imaging conditions. The following TABLE IV shows the results of imaging and processing of Films A and B. Film A was imaged using a conventional dose (28 kVp) and conventional molybdenum anodes. The present invention, using Film B, was practiced using higher kVp and rhodium anodes to provide acceptable image quality but with significantly lower patient dosage.

5

10

15

20

25

30

35

40

45

50

55

TABLE IV

Film	kVp	Screen	Target/- Filter*	Entrance Exposure (mR)	Δ Density	Image Resolution	Image Noise	Image Quality
A(Control)	28	X	Mo/Mo	1x	1x	2	2	4
A (Control)	30	X	Rh/Rh	0.45x	0.85x	3.5	3	6.5
B (Invention)	30	X	Rh/Rh	0.45x	0.98x	2	2	4

* "Mo" refers to molybdenum anodes, and "Rh" refers to rhodium anodes.

Claims

1. A radiographic silver halide film that comprises a support having first and second major surfaces and that is capable of transmitting X-radiation,

the radiographic silver halide film having disposed on the first major support surface, one or more hydrophilic colloid layers including at least one cubic grain silver halide emulsion layer, and having disposed on the second major support surface, one or more hydrophilic colloid layers including at least one tabular grain silver halide emulsion layer,
the film **characterized** wherein it can be exposed to provide a black-and-white image having a $d(\gamma)/d(\log E)$ value greater than 5.

2. The radiographic silver halide film of claim 1 wherein the cubic grain silver halide emulsion layer comprises:

1) a combination of first and second spectral sensitizing dyes that provides a combined maximum J-aggregate absorption on the cubic silver halide grains of from 540 to 560 nm, and


wherein the first spectral sensitizing dye is an anionic benzimidazole-benzoxazole carbocyanine, the second spectral sensitizing dye is an anionic oxycarbocyanine, and the first and second spectral sensitizing dyes are present in a molar ratio of from 0.25:1 to 4:1,

2) a mixture of a first hydrophilic binder that is gelatin or a gelatin derivative and a second hydrophilic binder other than gelatin or a gelatin derivative, wherein the weight ratio of the first hydrophilic binder to the second hydrophilic binder is from 2:1 to 5:1, and the level of hardener in the cubic grain silver halide emulsion layer is from 0.4 to 1.5 weight % based on the total weight of the first hydrophilic binder in the cubic grain silver halide emulsion layer,


3) cubic silver halide grains comprising from 1 to 20 mol % chloride and from 0.25 to 1.5 mol % iodide, both based on total silver in the cubic grain emulsion layer, which cubic silver halide grains have an average ECD of from 0.65 to 0.8 μm , and

4) cubic silver halide grains that are doped with a hexacoordination complex compound within part or all of 95% of the innermost volume from the center of the cubic silver halide grains.

3. The radiographic silver halide film of claim 2 wherein the first spectral sensitizing dye is represented by the following Structure I:

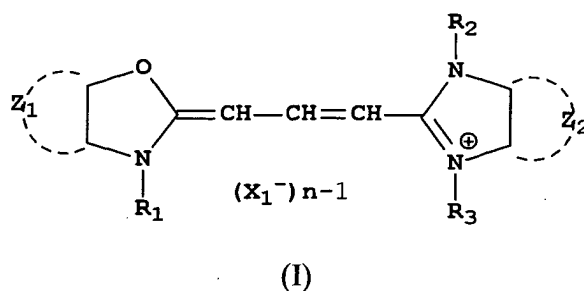





wherein Z_1 and Z_2 represent the carbon atoms necessary to form a substituted or unsubstituted benzene or naphthalene ring, R_1 , R_2 , and R_3 are independently substituted or unsubstituted alkyl, alkoxy, aryl, or alkenyl groups, X_1^- is an anion, and n is 1 or 2, and the second spectral sensitizing dye is represented by the following Structure II:

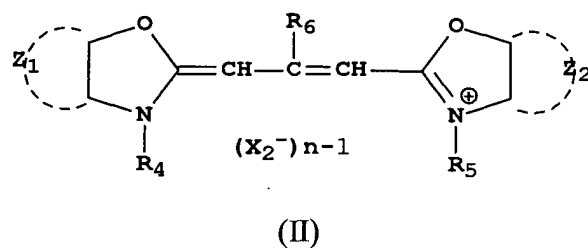


wherein Z_1 and Z_2 represent the carbon atoms necessary to form a substituted or unsubstituted benzene or naphthalene ring, R_4 and R_5 are independently substituted or unsubstituted alkyl, alkoxy, aryl, or alkenyl groups, R_6 is hydrogen or a substituted or unsubstituted alkyl or phenyl group, X_2^- is an anion, and n is 1 or 2.


4. The radiographic silver halide film of claim 2 or 3 wherein the total amount of the combination of the first and second spectral sensitizing dyes is from 0.25 to 0.75 mol/mole of silver, and the first and second spectral sensitizing dyes are present in a molar ratio of from 0.5:1 to 1.5:1.
5. The radiographic silver halide film of any of claims 2 to 4 wherein the combination of the first and second spectral sensitizing dyes provide a combined J-aggregate absorption of from 545 to 555 nm when the dyes are absorbed on the cubic silver halide grains.
6. The radiographic silver halide film of any of claims 2 to 5 wherein the first spectral sensitizing dye is selected from the following Compounds A-1 to A-7, and the second spectral sensitizing dye is selected from the following Compounds B-1 to B-5:

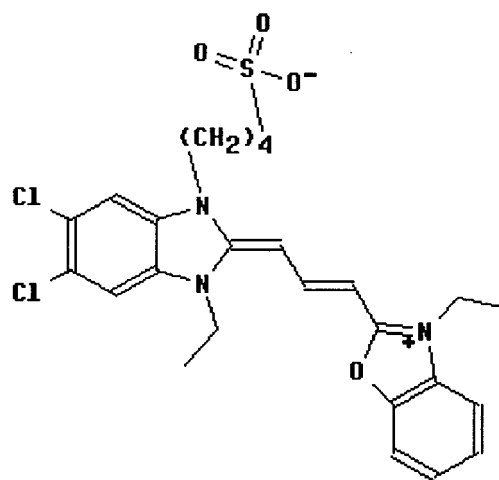

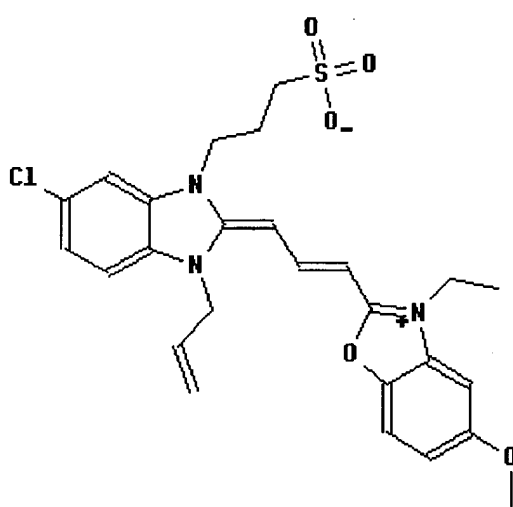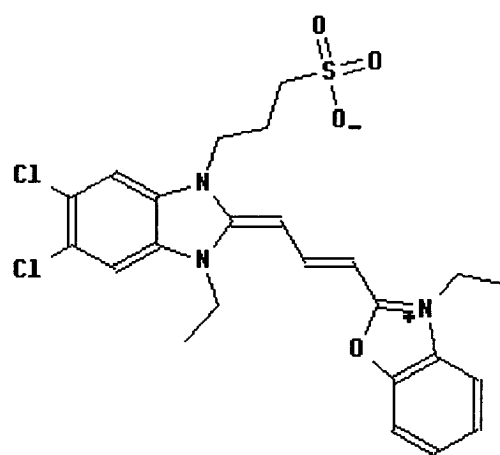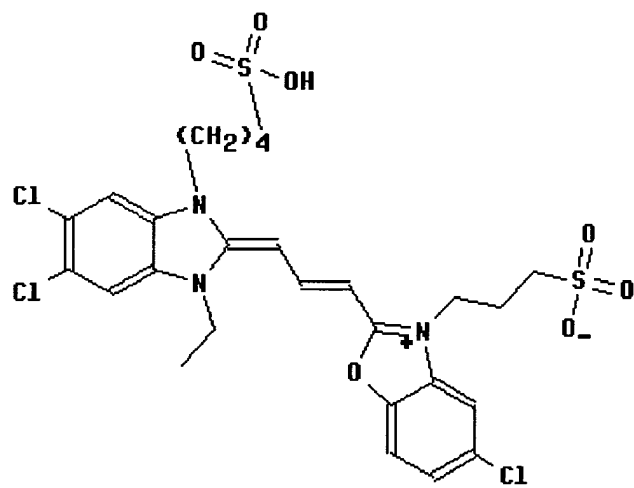


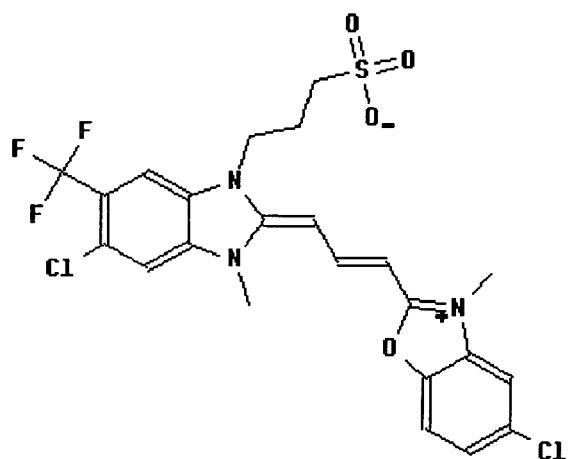




A-5


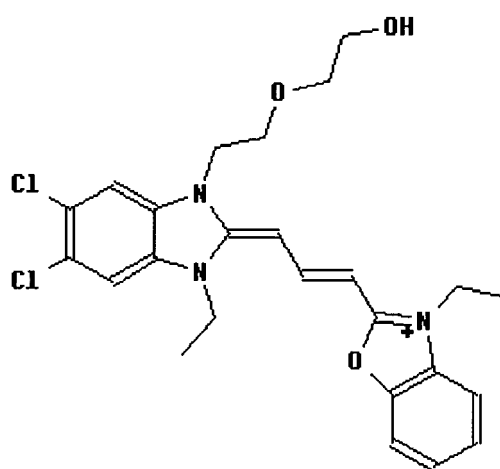


A-6

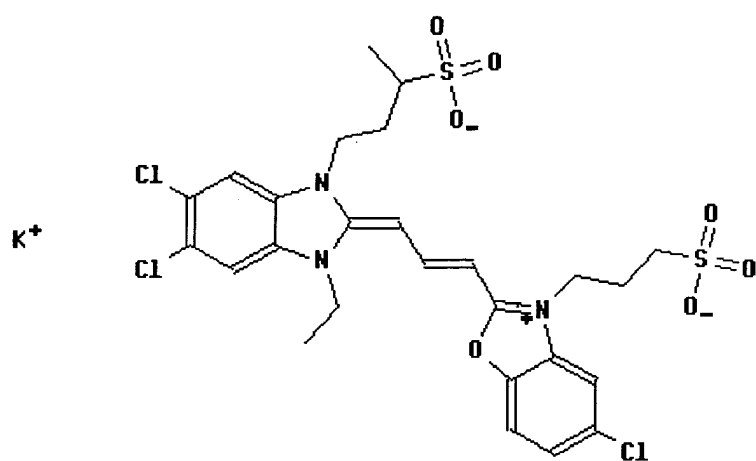

A-7

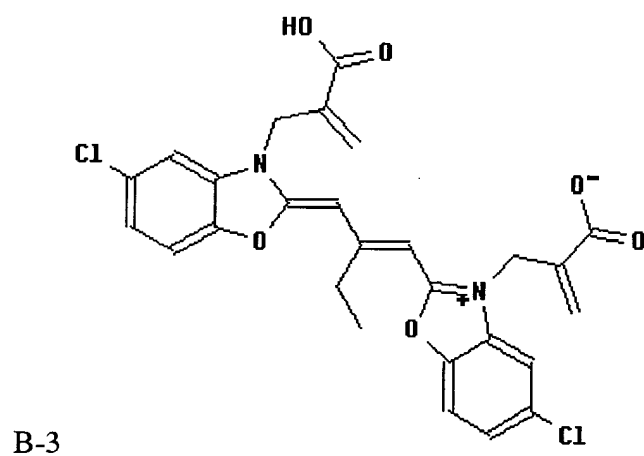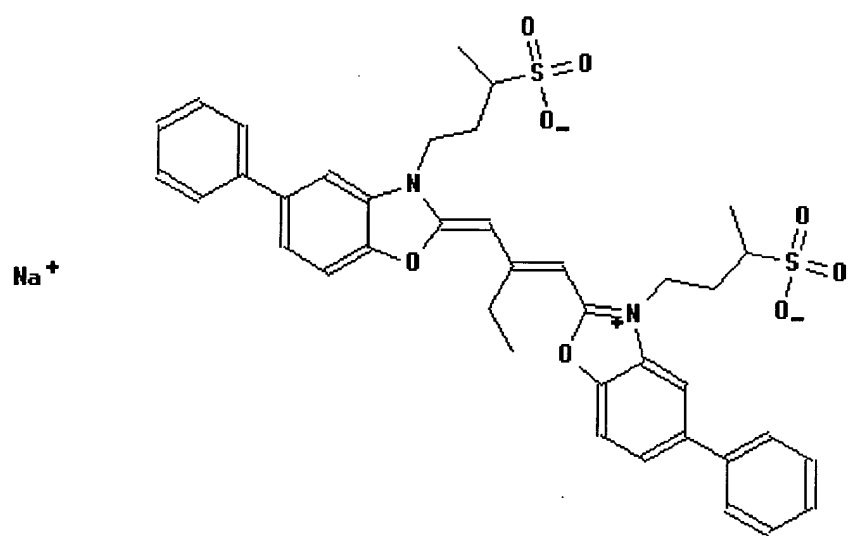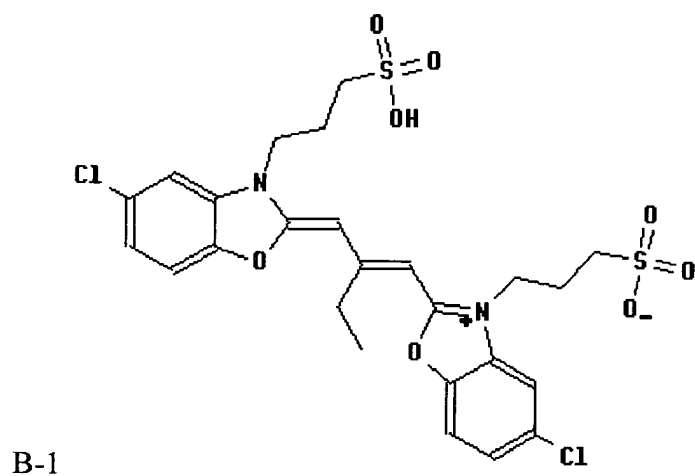

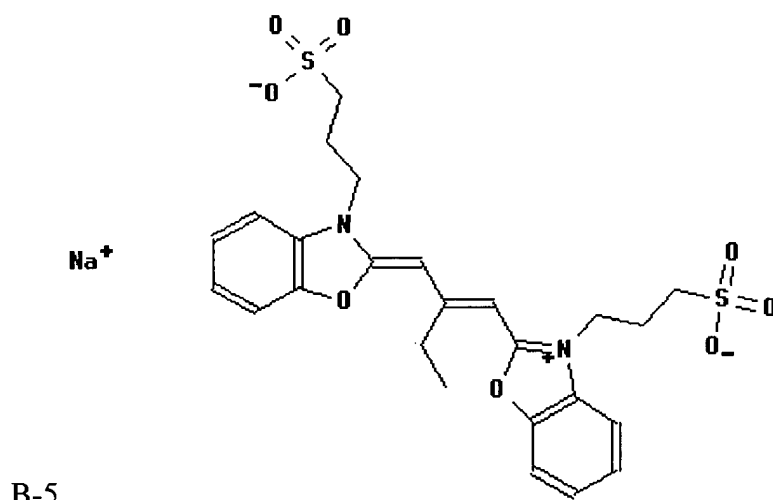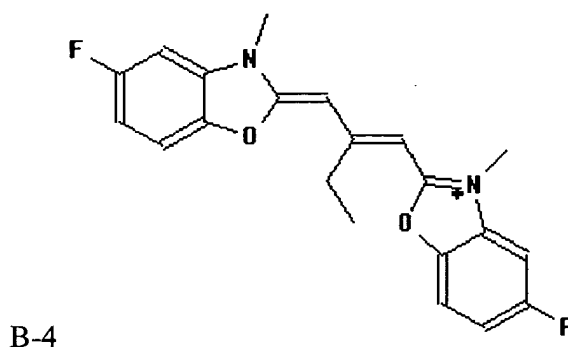

- 35 7. The radiographic silver halide film of any of claims 2 to 6 wherein the hexacoordination complex compound is present in an amount of from 1×10^{-6} to 5×10^{-4} mole per mole of silver in the silver halide emulsion layer in which it is present.
- 40 8. The radiographic silver halide film of any of claims 2 to 7 wherein the hexacoordination complex compound is present within the innermost 90% of the volume of the cubic silver halide grains.
- 45 9. The radiographic silver halide film of any of claims 2 to 8 wherein the hexacoordination complex compound is represented by the following Structure I:



50 wherein M is a Group 8 polyvalent transition metal ion, L represents six coordination complex ligands that can be the same or different provided that at least four of the ligands are anionic ligands and at least one of the ligands is more electronegative than any halide ligand, and n is -2, -3, or -4.

- 55 10. The radiographic silver halide film of any of claims 2 to 9 wherein the cubic silver halide grains are composed of from 10 to 20 mol % chloride, based on total silver in the emulsion layer, and from 0.5 to 1 mol % iodide, based on total silver in the cubic grain silver halide emulsion layer.
11. The radiographic silver halide film of any of claims 2 to 10 wherein the weight ratio of the first hydrophilic binder to the second hydrophilic binder is from 2.5: 1 to 3.5: 1, and

the level of the hardener is from 0.5 to 1.5 weight % based on the total weight of the first hydrophilic binder in the cubic grain silver halide emulsion layer.

12. The radiographic silver halide film of any of claims 2 to 11
wherein the second hydrophilic binder is a dextran or polyacrylamide.

13. A radiographic silver halide film having a photographic speed of at least 100 and comprising a transparent film support having first and second major surfaces and that is capable of transmitting X-radiation,


the radiographic silver halide film having disposed on the first major support surface, one or more hydrophilic colloid layers including at least one silver halide emulsion layer, and having disposed on the second major support surface, one or more hydrophilic colloid layers including at least one tabular grain silver halide emulsion layer,


the film also comprising a protective overcoat layer disposed on both sides of the support,

the film **characterized** wherein the cubic grain silver halide emulsion layer comprises:

- 1) a combination of first and second spectral sensitizing dyes that provides a combined maximum J-aggregate absorption of from 545 to 555 nm when the dyes are absorbed on the surface of the cubic silver halide grains,

wherein the first spectral sensitizing dye is the following Dye A-2, and wherein the second spectral sensitizing dye is following Dye B-1, the first and second spectral sensitizing dyes being present in a molar ratio of from 0.5:1 to 1.5: 1, and the total spectral sensitizing dyes in the film is from 0.25 to 0.75 mg/mole of silver,

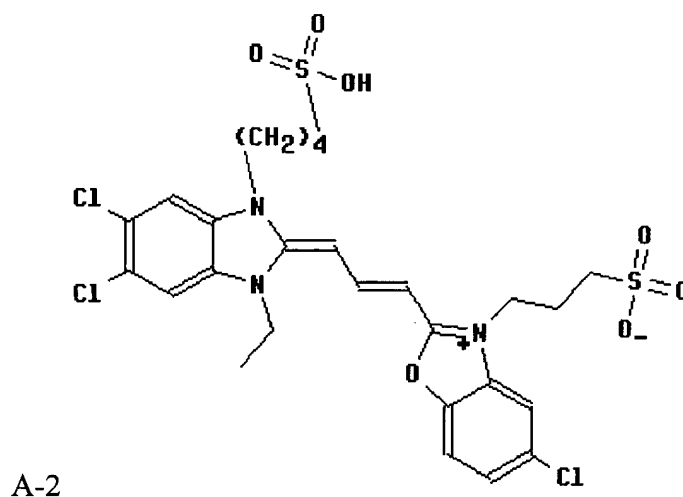

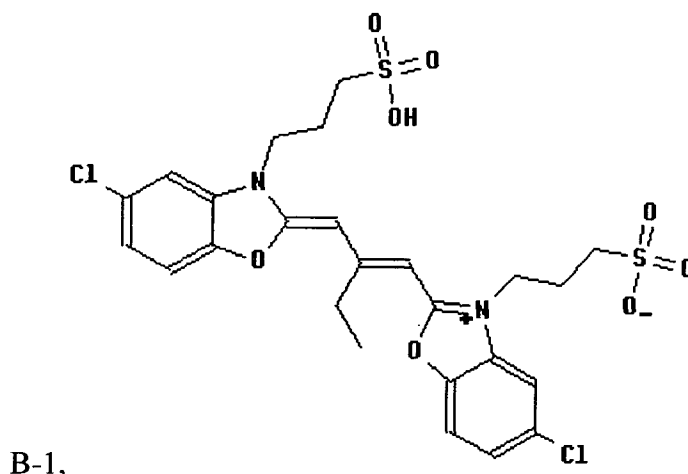

20 2) a mixture of a first hydrophilic binder that is gelatin or a gelatin derivative and a second hydrophilic binder that is a dextran or polyacrylamide, wherein the weight ratio of the first hydrophilic binder to the second hydrophilic binder is from 2.5:1 to 3.5:1 and the level of hardener in the cubic grain silver halide emulsion is from 0.5 to 1.5 weight % based on the total weight of the first hydrophilic binder in the cubic grain silver halide emulsion layer,

25 3) cubic silver halide grains comprising from 10 to 20 mol % chloride and from 0.5 to 1 mol % iodide, both based on total silver in the cubic grain silver halide emulsion layer, which cubic silver halide grains have an average ECD of from 0.72 to 0.76 μm , and

30 4) cubic silver halide grains that are doped with a hexacoordination complex compound within 75 to 80% of the innermost volume from the center of the cubic silver halide grains, wherein the hexacoordination complex compound is represented by the following Structure I:



35 wherein M is Fe^{+2} , Ru^{+2} , Os^{+2} , Co^{+3} , Rh^{+3} , Ir^{+3} , Pd^{+3} , or Pt^{+4} , L represents six coordination complex ligands that can be the same or different provided that at least three of the ligands are cyanide ions, and n is -2, -3, or -4.

14. A radiographic imaging assembly comprising:

- 40 A) the radiographic silver halide film of any of claims 1 to 13, and
B) a fluorescent intensifying screen that comprises an inorganic phosphor capable of absorbing X-rays and emitting electromagnetic radiation having a wavelength greater than 300 nm.

15. The radiographic imaging assembly of claim 14 wherein the inorganic phosphor is present as particles wherein at least 50% of the particles have a size of less than 3 μm and at least 85% of the particles have a size of less than 5.5 μm , and the coverage of the inorganic phosphor in the phosphor layer is from 260 to 380g/m².

16. A method of providing a black-and-white image comprising exposing the radiographic imaging assembly of claim 14 or 15 to X-radiation generated using rhodium or tungsten anodes in an X-radiation generating device, and processing the radiographic silver halide film, sequentially, with a black-and-white developing composition and a fixing composition, the processing being carried out within 90 seconds, dry-to-dry.

17. A method of imaging for mammography comprising exposing a patient to X-radiation using an X-radiation generating device comprising rhodium or tungsten anodes, and providing a black-and-white image of the exposed patient using an imaging assembly comprising:

- 55 A) a radiographic silver halide film that has a photographic speed of at least 100 and comprises a support having first and second major surfaces and that is capable of transmitting X-radiation,
the radiographic silver halide film having disposed on the first major support surface, one or more hy-

drophilic colloid layers including at least one cubic grain silver halide emulsion layer, and having disposed on the second major support surface, one or more hydrophilic colloid layers including at least one tabular grain silver halide emulsion layer,

wherein the cubic grain silver halide emulsion layer comprises:

1) a combination of first and second spectral sensitizing dyes that provides a combined maximum J-aggregate absorption on the cubic silver halide grains of from 540 to 560 nm, and

wherein the first spectral sensitizing dye is an anionic benzimidazole-benzoxazole carbocyanine, the second spectral sensitizing dye is an anionic oxycarbocyanine, and the first and second spectral sensitizing dyes are present in a molar ratio of from 0.25:1 to 4:1,

2) a mixture of a first hydrophilic binder that is gelatin or a gelatin derivative and a second hydrophilic binder other than gelatin or a gelatin derivative, wherein the weight ratio of the first hydrophilic binder to the second hydrophilic binder is from 2:1 to 5:1, and the level of hardener in the cubic grain silver halide emulsion layer is from 0.4 to 1.5 weight % based on the total weight of the first hydrophilic binder in the cubic grain silver halide emulsion layer,

3) cubic silver halide grains comprising from 1 to 20 mol % chloride and from 0.25 to 1.5 mol % iodide, both based on total silver in the cubic grain emulsion layer, which cubic silver halide grains have an average ECD of from 0.65 to 0.8 μm , and

4) cubic silver halide grains that are doped with a hexacoordination complex compound within part or all of 95% of the innermost volume from the center of the cubic silver halide grains, and

B) a fluorescent intensifying screen that comprises an inorganic phosphor capable of absorbing X-rays and emitting electromagnetic radiation having a wavelength greater than 300 nm.

18. The method of claim 17 wherein the patient is exposed to X-radiation at a peak voltage greater than 28 kVp.

19. A method of providing a black-and-white image comprising exposing the radiographic imaging assembly of claim 14 or 15 to X-radiation at a peak voltage greater than 28 kVp, and processing the radiographic silver halide film, sequentially, with a black-and-white developing composition and a fixing composition, the processing being carried out within 90 seconds, dry-to-dry.

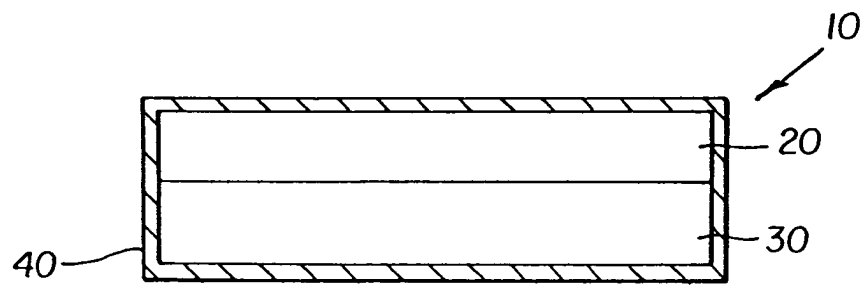


FIG. 1



European Patent
Office

PARTIAL EUROPEAN SEARCH REPORT

Application Number

which under Rule 45 of the European Patent Convention shall be considered, for the purposes of subsequent proceedings, as the European search report

EP 03 07 8511

DOCUMENTS CONSIDERED TO BE RELEVANT			
Category	Citation of document with indication, where appropriate, of relevant passages	Relevant to claim	CLASSIFICATION OF THE APPLICATION (Int.Cl.7)
D, X	US 6 033 840 A (DICKERSON) 7 March 2000 (2000-03-07)	1, 14, 16, 19	G03C5/16 G03C5/17
Y	* column 2, line 58 - line 63 * * column 8, line 40 - line 46 * * column 9, line 34 - line 35 * * column 10, line 48 - line 52 * * column 13, line 67 - column 14, line 2 * * column 17, line 42 - line 43 * * column 21, line 30 - column 22, line 24 * * column 22, line 42 - line 45; claim 7 * --- -/--	2-13, 15, 17, 18	
			TECHNICAL FIELDS SEARCHED (Int.Cl.7)
			G03C
INCOMPLETE SEARCH			
The Search Division considers that the present application, or one or more of its claims, does/do not comply with the EPC to such an extent that a meaningful search into the state of the art cannot be carried out, or can only be carried out partially, for these claims. Claims searched completely : Claims searched incompletely : Claims not searched : Reason for the limitation of the search: see sheet C			
Place of search		Date of completion of the search	Examiner
THE HAGUE		29 January 2004	Magrizos, S
CATEGORY OF CITED DOCUMENTS		T : theory or principle underlying the invention E : earlier patent document, but published on, or after the filing date D : document cited in the application L : document cited for other reasons & : member of the same patent family, corresponding document	
X : particularly relevant if taken alone Y : particularly relevant if combined with another document of the same category A : technological background O : non-written disclosure P : intermediate document			

EPO FORM 1503 03.82 (P04C07)



European Patent
Office

INCOMPLETE SEARCH
SHEET C

Application Number
EP 03 07 8511

Claim(s) searched completely:
2-13,15,17,18

Claim(s) searched incompletely:
1,14,16,19

Reason for the limitation of the search:

Present claims 1, 14, 16, 19 relate to a product and process defined by reference to a desirable characteristic or property, namely a $d\gamma/d\log E$ value greater than 5. The claims cover all products and processes having this characteristic or property, whereas the application provides support within the meaning of Article 84 EPC and/or disclosure within the meaning of Article 83 EPC for only a very limited number of such products and processes. In the present case, the claims so lack support, and the application so lacks disclosure, that a meaningful search over the whole of the claimed scope is impossible. Independent of the above reasoning, the claims also lack clarity (Article 84 EPC). An attempt is made to define the product by reference to a result to be achieved. Again, this lack of clarity in the present case is such as to render a meaningful search over the whole of the claimed scope impossible. Consequently, the search has been carried out for those parts of the claims which appear to be clear, supported and disclosed, namely those parts relating to the products and processes mentioned in the claims 2-13.



European Patent
Office

PARTIAL EUROPEAN SEARCH REPORT

Application Number
EP 03 07 8511

DOCUMENTS CONSIDERED TO BE RELEVANT			CLASSIFICATION OF THE APPLICATION (Int.Cl.7)
Category	Citation of document with indication, where appropriate, of relevant passages	Relevant to claim	
Y	EP 0 862 083 A (AGFA-GEVAERT) 2 September 1998 (1998-09-02) * page 2, line 5 - line 6 * * page 3, line 7 - line 40 * * page 4, line 32 - line 39 * * page 4, line 50 - line 55 * * page 5, line 46 - line 49 * * page 7, line 17 - line 20 * * page 7, line 44 - line 54 * * page 8, line 39 - line 41 * * page 8, line 53 - line 56 * * page 9, line 57 - page 10, line 1 * * page 12, line 22 - line 25 * * page 14, line 25 - page 17, line 9; claims 1-3,5,9 *	2-13,15, 17,18	
	---		TECHNICAL FIELDS SEARCHED (Int.Cl.7)
Y	EP 0 212 968 A (KONISHIROKU) 4 March 1987 (1987-03-04) * page 1, line 3 - page 2, line 2 * * page 5, line 13 - page 6, line 10 * * page 10, line 6 - line 8 * * page 20, line 8 - line 20 * * page 22, line 5 - line 12 * * page 24, line 7 - line 14 * * page 32; example 8 * * page 42; example 43 * * page 51, line 1 - line 8 * * page 67, line 14 - page 68, line 4 * * page 70, line 23 - page 71, line 3 * * page 76, line 19 - line 24 * * page 77; examples 1,2 * * page 79; table 2 *	2-13,15, 17,18	

	-/--		

PARTIAL EUROPEAN SEARCH REPORT

Application Number
EP 03 07 8511

DOCUMENTS CONSIDERED TO BE RELEVANT			CLASSIFICATION OF THE APPLICATION (Int.Cl.7)
Category	Citation of document with indication, where appropriate, of relevant passages	Relevant to claim	
D,Y	US 5 800 976 A (DICKERSON ET AL.) 1 September 1998 (1998-09-01) * column 3, line 57 - column 4, line 34 * * column 5, line 23 - line 32 * * column 8, line 3 - line 22 * * column 13, line 1 - line 51 * ---	2-13, 15, 17, 18	
Y	EP 0 407 890 A (3M) 16 January 1991 (1991-01-16) * page 8, line 8 - line 21 * * page 9, line 1 - line 5 * * page 13, line 12 - line 18 * * page 13, line 41 - line 55 * * page 14, line 46 - line 47 * -----	15, 17	TECHNICAL FIELDS SEARCHED (Int.Cl.7)

**ANNEX TO THE EUROPEAN SEARCH REPORT
ON EUROPEAN PATENT APPLICATION NO.**

EP 03 07 8511

This annex lists the patent family members relating to the patent documents cited in the above-mentioned European search report. The members are as contained in the European Patent Office EDP file on
The European Patent Office is in no way liable for these particulars which are merely given for the purpose of information.

29-01-2004

Patent document cited in search report		Publication date	Patent family member(s)	Publication date
US 6033840	A	07-03-2000	NONE	
EP 862083	A	02-09-1998	EP 0862083 A1	02-09-1998
			JP 10274828 A	13-10-1998
			US 5998083 A	07-12-1999
EP 212968	A	04-03-1987	JP 1797035 C	28-10-1993
			JP 5004655 B	20-01-1993
			JP 62042146 A	24-02-1987
			JP 1826183 C	28-02-1994
			JP 5035850 B	27-05-1993
			JP 62056950 A	12-03-1987
			EP 0212968 A2	04-03-1987
			US 4801526 A	31-01-1989
US 5800976	A	01-09-1998	NONE	
EP 407890	A	16-01-1991	IT 1230335 B	18-10-1991
			DE 69028663 D1	31-10-1996
			DE 69028663 T2	22-05-1997
			EP 0407890 A2	16-01-1991
			JP 2778810 B2	23-07-1998
			JP 3046649 A	27-02-1991
			US 5070248 A	03-12-1991

EPO FORM P0459

For more details about this annex : see Official Journal of the European Patent Office, No. 12/82