

(19)



(11)

EP 2 611 215 B1

(12)

EUROPEAN PATENT SPECIFICATION

(45) Date of publication and mention
of the grant of the patent:
20.04.2016 Bulletin 2016/16

(51) Int Cl.:
H04R 25/00 (2006.01)

(21) Application number: **11196247.8**

(22) Date of filing: **30.12.2011**

(54) **A hearing aid with signal enhancement**

Hörgerät mit Signalverbesserung

Aide auditive dotée d'un meilleur signal

(84) Designated Contracting States:
**AL AT BE BG CH CY CZ DE DK EE ES FI FR GB
GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO
PL PT RO RS SE SI SK SM TR**

(43) Date of publication of application:
03.07.2013 Bulletin 2013/27

(73) Proprietor: **GN ReSound A/S
2750 Ballerup (DK)**

(72) Inventors:
• **Gran, Karl-Fredrik Johan
SE-216 11 Limhamn (SE)**
• **Dittberner, Andrew Burke
Andover, MN Minnesota 55304 (US)**

(74) Representative: **Guardian
IP Consulting I/S
Diplomvej, Building 381
2800 Kgs. Lyngby (DK)**

(56) References cited:
EP-A2- 1 879 426 WO-A2-02/03749

- **MEISTER H ET AL: "A measurement system for assessing binaural masking level difference (BMLD) in children", HNO ; DEUTSCHE GESELLSCHAFT FÜR HALS-NASEN-OHREN-HEILKUNDE, KOPFUND HALS-CHIRURGIE, SPRINGER, BERLIN, DE, vol. 53, no. 8, 1 August 2005 (2005-08-01) , pages 695-700, XP019319798, ISSN: 1433-0458, DOI: 10.1007/S00106-004-1199-5**

EP 2 611 215 B1

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

Description

FIELD OF THE INVENTION

[0001] A new binaural hearing aid system is provided that compensates for a hearing impaired user's loss of ability to understand speech in noise.

BACKGROUND OF THE INVENTION

[0002] Hearing impaired individuals often experience at least two distinct problems: a hearing loss, which is an increase in hearing threshold level, and a loss of ability to understand high level speech in noise in comparison with normal hearing individuals. For most hearing impaired patients, the performance in speech-in-noise intelligibility tests is worse than for normal hearing people, even if the audibility of the incoming sounds is restored by amplification. An individual's speech reception threshold (SRT) is the signal-to-noise ratio required in a presented signal to achieve 50 percent correct word recognition in a hearing in noise test.

[0003] Today's digital hearing aids that use multi-channel amplification and compression signal processing can readily restore audibility of amplified sound for a hearing impaired individual. The patient's hearing ability can thus be improved by making previously inaudible speech cues audible.

[0004] Loss of capability to understand speech in noise is accordingly the most significant problem of most hearing aid users today. The traditional way of increasing SRT in hearing instruments, is to apply either beamforming or spectral subtraction techniques. In the first case, at least one microphone in combination with a number of filters, fixed or adaptive, is used to enhance a signal from the presumed target direction and at the same time suppress all other signals.

[0005] In spectral subtraction techniques, the goal is to create an estimate of the long term noise spectrum and turn down gain in frequency bands where the instantaneous target signal power is lower than the long term noise power. Even though the methods are very different from a technological standpoint, they still have the common goal; enhance the target signal and remove the noise disturbance.

[0006] The article "A measurement system for assessing binaural masking level difference (BMLD) in children" (H. Meister and H. Klüser et al.) is concerned with provision of a method of assessing BMLD for children which is intended to facilitate further clinical treatment.

[0007] The methods cannot take listener intent into account and they may remove parts of the audio signal which the listener is trying to focus on.

SUMMARY OF THE INVENTION

[0008] Below, a new method of enhancement of a desired signal is disclosed. The new method makes use of

the human auditory system's capability of concentrating on a desired signal. A new binaural hearing aid system using the new method is also disclosed.

[0009] Listening in complex sound fields is to a large extent facilitated by binaural processing in the auditory system. Due to diffraction effects by the pinna, concha, head and torso and due to reflection effects in reverberant environments, cues are imparted to the sound field, which are highly individual for the given subject.

[0010] The most important cues in binaural processing are the interaural time differences (ITD) and the interaural level differences (ILD). The ITD results from the difference in distance from the source to the two ears. This cue is primarily useful up till approximately 1.5 kHz and above this frequency the auditory system can no longer resolve the ITD cue.

[0011] The level difference is a result of diffraction and is determined by the relative position of the ears compared to the source. This cue is dominant above 2 kHz but the auditory system is equally sensitive to changes in ILD over the entire spectrum.

[0012] It has been argued that hearing impaired subjects benefit the most from the ITD cue as the hearing loss tends to be less severe in the lower frequencies.

[0013] It has been shown that manipulating the relative interaural phase and level of a target signal, i.e. a signal a listener desires to listen to, and of a noise signal, i.e. a signal the listener perceives as disturbing, can improve speech intelligibility significantly. It seems as if the auditory system is indeed adapted to separate signals with different ITD and ILD encoding to perform a natural type of noise reduction to facilitate focusing on the target signal.

[0014] It has been found that if the target signal is presented in anti-phase, i.e. phase shifted 180°, and the noise in-phase in the two ears, an increase of the Binaural Masking Level Difference (BMLD) of 13 dB can be achieved compared to when both signals are presented in-phase in the two ears. Depending on the type of noise, an improvement of 20 dB of the BMLD is achievable.

[0015] The reverse situation where noise is presented out of phase and the target is presented in phase yields a slightly lower performance.

[0016] In the new method, at least one of the target signal and the noise signal is estimated, and the at least one estimate is presented to the user of the binaural hearing aid system in such a way that a user's capability of understanding speech in noise is improved.

[0017] For example, a listener may listen to sound with a signal S that the listener desires to listen to and noise N that the listener finds disturbing, i.e. the sound signal is S+N. Based on the sound signal S+N, the desired signal S may be estimated. The estimate is denoted ES. Subtracting two times the estimate ES from the sound signal S+N results in a modified signal: S+N-ES-ES, and since ES is approximately equal to S, modified signal is: N-ES which is approximately equal to -S+N, i.e. the original sound signal wherein the desired signal S has been

substantially substituted with signal S phase shifted by 180°. Now, the original signal S+N may be presented to one ear of a user, and the phase shifted signal N-ES, or more accurately S+N-2ES, may be presented to the other ear for improved BMLD and SRT.

[0018] Alternatively, both the desired signal S and the noise N may be estimated and the sum of the estimates ES+EN may be presented to one ear of the user, and the phase shifted sum -ES+EN may be presented to the other ear for improved BMLD and SRT.

[0019] The desired signal S and the noise may be swapped so that the noise estimated is phase shifted instead of the desired signal for improved BMLD and SRT; however with decreased performance compared to phase shifting the desired signal S.

[0020] Noise can be background speech, restaurant clatter, music (when speech is the desired signal), traffic noise, etc.

[0021] The purpose for the method is not to remove any part of the signal but instead present the signals so that the auditory system can perform natural noise reduction and separate the target signal from the noise signal.

[0022] In this way, if for some reason (e.g. the presumed target direction is wrong, or the unit is not able to achieve sufficient target/noise separation, the target signal and the noise signal are swapped; enhancement of the target signal is still obtained, although with slightly decreased performance.

[0023] This would not be possible with traditional noise reduction techniques, since the target signal, which in this case would be assumed to be the noise would be suppressed.

[0024] Thus, a new binaural hearing aid system is provided, comprising

at least one microphone for provision of respective at least one microphone audio signal in response to sound received at the at least one microphone,

a signal separation unit configured to provide an estimate of one of a target signal and a noise signal based on the at least one microphone audio signal,

a phase shift circuit configured to phase shift the estimate of one of the target signal and the noise signal, and

a phase shift adder connected to provide a phase shifted signal representing sound received at the at least one microphone in which the estimate of one of the target signal and the noise signal has substantially substituted the respective original one of the target signal and the noise signal, and

a first receiver for conversion of a receiver input signal into an acoustic signal for transmission towards one of the eardrums of a user of the binaural hearing aid system, and

a second receiver for conversion of a receiver input signal into an acoustic signal for transmission towards the other one of the eardrums of the user, and wherein the receiver input of one of the first and second receivers is connected to a signal representing the phase shifted signal, and

the receiver input of the other one of the first and second receivers is connected to a signal representing sound received at the at least one microphone.

[0025] Further, a new method is provided of binaural signal enhancement in a binaural hearing aid system, the method comprising the steps of
5 providing at least one microphone audio signal in response to sound, and providing an estimate of one of a target signal and a noise signal based on the at least one audio signal,

10 phase shifting the estimate of one of the target signal and the noise signal, and providing a phase shifted signal representing the at least one microphone audio signal in which the phase shifted estimate of one of the target signal and the noise signal has substantially substituted the respective original one of the target signal and the noise signal, and

15 transmitting a signal representing the phase shifted signal towards one of the eardrums of a user of the binaural hearing aid system, and

20 transmitting a signal representing the at least one microphone audio signal towards the other one of the eardrums of the user.

[0026] In the event that the estimate of one of the target signal and the noise signal is equal to the corresponding original one of the target signal and the noise signal, the phase shifted estimate can exactly substitute the respective original signal; however typically, the estimate of a signal will deviate from the original signal and substitution of the original signal with its estimate will typically not lead to substitution of the deviation, and thus the estimate is said to substantially substitute the original signal.

[0027] Throughout the present disclosure, one signal is said to represent another signal when the one signal is a function of the other signal, for example the one signal may be formed by analogue-to-digital conversion, or digital-to analogue conversion of the other signal; or, the one signal may be formed by conversion from another acoustic signal to an electronic signal or vice versa; or the one signal may be formed by analogue or digital filtering or mixing of the other signal; or the one signal may be formed by transformation, such as frequency transformation, etc, of the other signal; etc.

[0028] Further, signals that are processed by specific circuitry, e.g. in a signal processor, may be identified by a name that may be used to identify any analogue or digital signal forming part of the signal path from the source of the signal in question to an input of the circuitry, e.g. signal processor, in question. For example an output signal of a microphone, i.e. the microphone audio signal, may be used to identify any analogue or digital signal forming part of the signal path from the output of the microphone to its input to the signal processor, including pre-processed microphone audio signals.

[0029] The at least one microphone may contain a single microphone; however preferably, the at least one microphone has two microphones. Further, the at least one microphone may have more than two microphones for

improved separation of the target signal and the noise signal.

[0030] For improved signal enhancement, the second hearing aid may also comprise at least one microphone for provision of microphone audio signals in response to sound received at the respective microphones. In this case, the transceiver of the first hearing aid is connected for reception of signals representing the microphone audio signals of the second hearing aid, and the signal separation unit is configured to provide the estimate of the target signal and the estimate of the noise signal based on the audio signals of the first and second hearing aids.

[0031] Preferably, the phase shift circuit phase shifts the estimate of the target signal, and preferably, the phase shift ranges from 150° to 210°, more preferred the phase shift is approximately equal to 180°, and most preferred equal to 180°.

[0032] The signal separation unit may be configured to provide the estimates based on spectral characteristics of the audio signals as is well-known in the art of noise reduction. However, according to the new method, the noise estimate is not suppressed in the output presented to the user; rather the target estimate and the noise estimate is presented to the user in a way that improves the user's SRT.

[0033] The signal separation unit may be configured to provide the estimates based on statistical characteristics of the audio signals as is well-known in the art of noise reduction. However, according to the new method, the noise estimate is not suppressed in the output presented to the user; rather the target estimate and the noise estimate is presented to the user in a way that improves the user's SRT.

[0034] The signal separation unit may comprise a beamformer, and the beam former may be configured to provide the estimates based on microphone audio signals of the first and second hearing aids. The beamformer of the signal separation unit is different from conventional beamformers in that the noise estimate is not suppressed in the output presented to the user; rather the target estimate and the noise estimate is presented to the user in a way that improves the user's SRT.

[0035] The beamformer combines the microphone audio signals output by a plurality of microphones of the at least one microphone into a target signal with varying sensitivity to sound sources in different directions in relation to the plurality of microphones. Throughout the present disclosure, a plot of the varying sensitivity as a function of the direction is denoted the directivity pattern. Typically, a directivity pattern has at least one direction wherein the microphone signals substantially cancel each other. Throughout the present disclosure, such a direction is denoted a null direction. A directivity pattern may comprise several null directions depending on the number of microphones in the plurality of microphones and depending on the signal processing.

[0036] The beamformer may be a fixed beamformer with a directional pattern that is fixed with relation to the

head of the user. The beamformer may for example be based on at least two microphones, with a directional pattern that has a maximum in the front direction of the user, i.e. the forward looking direction of the user, and a null in the opposite direction, i.e. the rear direction of the user.

[0037] The beamformer may be based on more than two microphones, and may include microphones of both hearing aids using wireless or wired communication techniques. The increased distance between the microphones may be utilized to form a directional pattern with a narrow beam providing improved spatial separation of the target estimate from the noise estimate. The conventional output of the beamformer may be used as the target estimate, and the noise estimate may be provided by subtraction of the target estimate from the microphone audio signal of one of the microphones of the plurality of microphones.

[0038] When microphones of both hearing aids of the binaural hearing aid system cooperate with the beamformer, the respective microphone signals must be sampled substantially synchronously. Time shifts as small as 20 -30 μS between sampling instants of the respective microphone signals in the two hearing aids may lead to a perceivable shift in the beam direction. Furthermore, a slowly time varying time shift between the sampling instants of the respective microphone signals, which inevitably will occur if the hearing aids are operated asynchronously, will result in an acoustic beam that appears to drift and focus in alternating directions.

[0039] Thus, the hearing aids of the binaural hearing aid system may be synchronized as for example discloses in more detail in WO 02/07479.

[0040] The beamformer may comprise adaptive filters configured to filter respective microphone audio signals and to adapt the respective filter coefficients for adaptive beamforming towards a sound source. For example, the beamformer may adapt to optimize the signal to noise ratio.

[0041] An adaptable beamformer makes it possible to focus on a moving sound source or to focus on a non-moving sound source, while the user of the hearing aid system is moving. Furthermore, the adaptable beamformer is capable of adapting to changes in the sound environment, such as appearance of a new sound source, disappearance of a noise source or movement of noise sources relative to the user of the hearing aid system.

[0042] An adaptive beamformer may be designed under the assumption that the signals received at the at least one microphone can be modelled as a combination of a target signal from a pre-determined target direction plus noise:

$$y_i(n) = h_i(n) * s(n) + v_i(n)$$

where $h_i(n)$ is the impulse response of sound propagation from the source emitting the signal $s(n)$ to the i^{th} microphone and $v_i(n)$ is the noise signal at the same microphone.

[0043] The noise can consist of both directional noise and other types of noise such as diffuse noise or babble noise.

[0044] The filter coefficients may adaptively be determined by solving the following optimization problem:

$$\{a_i(n)\}_{i=1}^4 = \arg \min_{\{a_i(n)\}_{i=1}^4} \|z(n)\|^2$$

$$\text{subject to } \sum_{i=1}^4 a_i(n) * h_i(n) = h_1(n)$$

[0045] Finding a solution to this optimization could be done adaptively using least mean square, recursive least square, steepest descent or other types of numerical optimization algorithms.

[0046] Once the target and noise estimate has been determined, the signals are presented to the user in such a way that the SRT of the user is improved.

[0047] Preferably, the target estimate is presented in opposite phase, i.e. 180° phase shifted with relation to each other, at the two ears of the user, while the noise estimate is presented in phase at the two ears of the user. Thus, in the first hearing aid, a first adder may be connected to the signal separation unit, and output a sum of the target estimate and the noise estimate provided by the signal separation unit, and the output of the first adder may be connected to a signal processor for further processing, such as hearing loss compensation, and the output of the signal processor may be connected to an output transducer that outputs a corresponding output to one ear of the user, or the output of the first adder may be connected directly to the output transducer. A second adder may be connected to the signal separation unit, and output a sum of the reverse phases target estimate and the noise estimate provided by the signal separation unit, and the output of the second adder is connected to a transceiver that transmits the output of the second adder to the other hearing aid having a transceiver for reception of the output of the second adder. The output of the transceiver may be connected to a signal processor for further processing, such as hearing loss compensation, and the output of the signal processor may be connected to an output transducer that outputs a corresponding output to another ear of the user, or the output of the transceiver may be connected directly to the output transducer.

[0048] Instead, with somewhat reduced performance in improved SRT of the user, the noise signal may be presented in opposite phase, i.e. 180° phase shifted with relation to each other, at the two ears of the user, while

the target estimate is presented in phase at the two ears of the user.

[0049] Preferably, the first hearing aid includes a delay between the adder and the output transducer so that the relative phase of the signals output by the respective output transducers of the first and second hearing aids is maintained.

[0050] The improvement of SRT as a function of the phase shift has a maximum at 180°; however the function is sine-shape with a flat maximum so that the improvement obtained by a phase shift ranging from 150° to 210° is close to the maximum improvement. Thus, the phase shift need not be exactly 180°, but preferably has a value within the range from 135° to 225°, more preferred from 150° to 210°.

[0051] The new binaural hearing aid system may comprise a multi-channel first hearing aid in which the microphone audio signals are divided into a plurality of frequency channels.

[0052] Correspondingly, individual target signal estimates and noise estimates may be provided in each frequency channel of the plurality of frequency channels, or may be provided in one or more selected frequency channels of the plurality of frequency channels, or one or more target signal estimates and noise estimates may be provided for one or more respective groups of selected frequency channels of the plurality of frequency channels, or one target signal estimate and noise estimate may be provided based on all the frequency channels of the plurality of frequency channels.

[0053] The plurality of frequency channels may include warped frequency channels, for example all of the frequency channels may be warped frequency channels.

[0054] The new binaural hearing aid system may additionally provide circuitry used in accordance with other conventional methods of hearing loss compensation so that the new circuitry or other conventional circuitry can be selected for operation as appropriate in different types of sound environment. The different sound environments may include speech, babble speech, restaurant clatter, music, traffic noise, etc.

[0055] The new binaural hearing aid system may for example comprise a Digital Signal

[0056] Processor (DSP), the processing of which is controlled by selectable signal processing algorithms, each of which having various parameters for adjustment of the actual signal processing performed. The gains in each of the frequency channels of a multi-channel hearing aid are examples of such parameters.

[0057] One of the selectable signal processing algorithms operates in accordance with the new method.

[0058] For example, various algorithms may be provided for conventional noise suppression, i.e. attenuation of undesired signals and amplification of desired signals.

[0059] Microphone audio signals obtained from different sound environments may possess very different characteristics, e.g. average and maximum sound pressure levels (SPLs) and/or frequency content. Therefore, each

type of sound environment may be associated with a particular program wherein a particular setting of algorithm parameters of a signal processing algorithm provides processed sound of optimum signal quality in a specific sound environment. A set of such parameters may typically include parameters related to broadband gain, corner frequencies or slopes of frequency-selective filter algorithms and parameters controlling e.g. knee-points and compression ratios of Automatic Gain Control (AGC) algorithms.

[0060] Signal processing characteristics of each of the algorithms may be determined during an initial fitting session in a dispenser's office and programmed into the new binaural hearing aid system in a non-volatile memory area.

[0061] The new binaural hearing aid system may have a user interface, e.g. buttons, toggle switches, etc, of the hearing aid housings, or a remote control, so that the user of the new binaural hearing aid system can select one of the available signal processing algorithms to obtain the desired hearing loss compensation in the sound environment in question.

[0062] The new binaural hearing aid system may be capable of automatically classifying the user's sound environment into one of a number of sound environment categories, such as speech, babble speech, restaurant clatter, music, traffic noise, etc, and may automatically select the appropriate signal processing algorithm accordingly as known in the art.

BRIEF DESCRIPTION OF THE DRAWINGS

[0063] In the following, preferred embodiments of the invention is explained in more detail with reference to the drawing, wherein

- Fig. 1 schematically illustrates an exemplary new binaural hearing aid system,
- Fig. 2 schematically illustrates an exemplary new binaural hearing aid system,
- Fig. 3 schematically illustrates an exemplary new binaural hearing aid system,
- Fig. 4 schematically illustrates an exemplary new binaural hearing aid system,
- Fig. 5 schematically illustrates a signal separation unit with an adaptive beamformer based on two microphones,
- Fig. 6 schematically illustrates a signal separation unit based on four microphones, and
- Fig. 7 schematically illustrates an exemplary new binaural hearing aid system.

[0064] The present invention will now be described more fully hereinafter with reference to the accompanying drawings, in which exemplary embodiments of the invention are shown. The invention may, however, be embodied in different forms and should not be construed as limited to the embodiments set forth herein. Rather,

these embodiments are provided so that this disclosure will be thorough and complete, and will fully convey the scope of the invention to those skilled in the art. Like reference numerals refer to like elements throughout. Like elements will, thus, not be described in detail with respect to the description of each figure.

DESCRIPTION OF PREFERRED EMBODIMENTS

[0065] Fig. 1 schematically illustrates an example of the new binaural hearing aid system 10.

[0066] The new binaural hearing aid system 10 has first and second hearing aids 10A, 10B. The second hearing aid 10B has a receiver 48B and a transceiver (not shown) for reception of the input signal to the receiver 48B from the first hearing aid 10A by wired or wireless transmission. Thus, in the illustrated example, the acoustic output signal emitted by the second hearing aid 10B is controlled by the first hearing aid 10A.

[0067] The first hearing aid 10A comprises one microphone 14 for provision of microphone audio signal 18 in response to sound received at the microphone 14. The microphone audio signal 18 may be pre-filtered in respective pre-filters (not shown) well-known in the art, and input to the signal separation unit 12. The signal separation unit 12 estimates the target signal and subtracts two times the estimated target signal from the microphone audio signal 18 to obtain a signal, in the following denoted "the phase shifted signal", representing the microphone audio signal 18; however, wherein the original target signal has been replaced by the estimate of the target signal phase shifted by 180°. The phase shifted signal is output to a transceiver (not shown) in the first hearing aid 10A for transmission to the second hearing aid 10B. A receiver 48 of the first hearing aid 10A converts the microphone audio signal 18 into an acoustic signal for transmission towards the eardrum of one ear of the user, and the receiver 48B of the second hearing aid 10B converts the phase shifted signal into an acoustic signal for transmission towards the eardrum of the other ear of the user thereby improving BMLD and SRT. The signal separation unit 12 may be configured to provide the estimate based on time-domain, spectral, and/or statistical characteristics of the microphone audio signal as is well-known in the art of noise reduction. Optionally, further processing may be applied to the respective signals before input to the respective receivers 48, 48B, e.g. for hearing loss compensation of the respective signals.

[0068] The new binaural hearing aid system (10) shown in Fig. 2 is similar to the hearing aid system shown in Fig. 1 except for the fact that the signal separation unit 12 shown in Fig. 2 is configured to provide both an estimate of the target signal 26 and an estimate of the noise signal 30 based on the possibly pre-filtered microphone audio signal 18.

[0069] The estimate of the target signal 26 is added to the estimate of the noise signal 30 in a first adder 42 and the output sum of the estimate of the target signal 26 and

the estimate of the noise signal 30 is input to an output transducer 48 that converts the output of first adder 42 into an acoustic output signal that is transmitted towards the eardrum of the user wearing the binaural hearing aid system 10.

[0070] Further, the estimate of the target signal 26 is subtracted; corresponding to a phase shift of 180° , from the estimate of the noise signal 30 in a second adder 50, and the output of the second adder 50 is transmitted output transducer 48B for conversion into an acoustic output signal that is transmitted towards the other eardrum of the user wearing the binaural hearing aid system 10. In this way, the BMLD and SRT are improved.

[0071] The estimate of the target signal 26 and the estimate of the noise signal 30 may be swapped so that the estimate of the noise signal 20 is phase shifted 180° before presentation to one of the eardrums of the user instead of phase shifting the estimate of the target signal 26. The improvement in BMLD and SRT obtained in this way is smaller than the improvement obtained by phase shift of the estimate of the target signal 26.

[0072] The new binaural hearing aid system (10) shown in Fig. 3 is similar to the hearing aid system shown in Fig. 1 except for the fact that a microphone audio signal 188 output by a microphone 148 in the second hearing aid 108 is transmitted by wired or wireless transmission to the first hearing aid 10A and input to the signal separation unit 12 so that the signal separation unit 12 can base the estimate of the target signal on both microphone audio signals 18, 188, e.g. by beamforming as explained further below. The relatively large distance between the microphones 14, 148, when a user wears the first and second hearing aids 10A, 10B in their intended positions at the respective ears of the user, makes it possible to form a narrow beam and therefore allow a good spatial separation of the target signal from the noise signal.

[0073] The new binaural hearing aid system (10) shown in Fig. 4 is similar to the hearing aid system shown in Fig. 3 except for the fact that the signal separation unit 12 shown in Fig. 4, like the signal separation unit shown in Fig. 2, is configured to provide both an estimate of the target signal 26 and an estimate of the noise signal 30 based on the possibly pre-filtered microphone audio signal 18.

[0074] The estimate of the target signal 26 is added to the estimate of the noise signal 30 in a first adder 42 and the output sum of the estimate of the target signal 26 and the estimate of the noise signal 30 is input to an output transducer 48 that converts the output of first adder 42 into an acoustic output signal that is transmitted towards the eardrum of the user wearing the binaural hearing aid system 10.

[0075] Further, the estimate of the target signal 26 is subtracted; corresponding to a phase shift of 180° , from the estimate of the noise signal 30 in a second adder 50, and the output of the second adder 50 is transmitted output transducer 48B for conversion into an acoustic output signal that is transmitted towards the other eardrum of

the user wearing the binaural hearing aid system 10. In this way, the BMLD and SRT are improved.

[0076] Fig. 5 schematically illustrates a digital signal separation unit 12 including an adaptive beamformer 10 with two microphones 14, 16.

[0077] The microphone audio signals 18, 20 are pre-filtered in conventional pre-filters 22, 24 before beamforming. The microphone audio signals 18, 20 may be digitized before or after the pre-filters 22, 24 by A/D converters (not shown). Signals before and after prefiltering and before and after analogue-digital conversion are all termed microphone audio signals.

[0078] The output 26 of first subtracter 28 generates the estimate of the target signal from the assumed target direction using adaptive beamforming. The estimate of the target signal 26 is subsequently presented to one of the two ears of the user and in opposite phase to the other of the two ears of the user. The output 30 of the adaptive filter 32 filtering the output of second subtracter 34 generates the noise estimate for subsequent presentation to both ears of the user.

[0079] The input $x_1(n)$ to the first microphone 14 is given by:

$$x_1(n) = h_1(n) * s(n) + g_1(n) * q(n)$$

where $h_1(n)$ is the impulse response of sound propagation from the source emitting the signal $s(n)$ to the first microphone 14 and $g_1(n)$ is the impulse response of sound propagation from the noise source emitting the signal $q(n)$ to the first microphone 14.

[0080] The input $x_2(n)$ to the second microphone 16 is given by:

$$x_2(n) = h_2(n) * s(n) + g_2(n) * q(n)$$

where $h_2(n)$ is the impulse response of sound propagation from the source emitting the signal $s(n)$ to the second microphone 16 and $g_2(n)$ is the impulse response of sound propagation from the noise source emitting the signal $q(n)$ to the second microphone 16.

[0081] Then, the output 26 of the target signal is equal to $h_1(n) * s(n)$, and the output 30 of the noise estimate is equal to $g_1(n) * q(n)$.

[0082] Fig. 6 schematically illustrates a signal separation unit 12 based on four microphones 22, 24, 22B, 24B, two of which 22, 24 are located in the first hearing aid 10A and other two of which 22B, 24B are located in the second hearing aid 10B.

[0083] The increased distance between the microphones may be utilized to form a directional pattern with a narrow beam providing improved spatial separation of the target estimate from the noise estimate. The conventional output of the beamformer may be used as the target estimate, and the noise estimate may be provided by

subtraction of the target estimate from the microphone audio signal of one of the microphones in the plurality of microphones.

[0084] The microphone audio signals 18, 20 of the two microphones 22, 24 of the first hearing aid 10 are pre-filtered in respective pre-filters 22, 24 well-known in the art, into microphone audio signals $y_1(n)$, $y_2(n)$ and input to respective adaptive filters $a_1(n)$, $a_2(n)$.

[0085] The pre-filtered microphone audio signals of the two microphones 22B, 24B of the second hearing aid 10B are encoded for transmission in the second hearing aid 10B and transmitted to the first hearing aid 10A using wireless or wired data transmission. The transmitted data representing the microphone audio signals of the two microphones 22B, 24B of the second hearing aid 10B are received by the transceiver 36 of the first hearing aid 10A and decoded in decoder 38 into two microphone audio signals $y_3(n)$, $y_4(n)$ and input to respective adaptive filters $a_3(n)$, $a_4(n)$.

[0086] The adaptive filters $a_1(n)$, $a_2(n)$, $a_3(n)$, $a_4(n)$ are configured to filter the respective microphone audio signals $y_1(n)$, $y_2(n)$, $y_3(n)$, $y_4(n)$ and to adapt the respective filter coefficients for adaptive beamforming towards a sound source.

[0087] The adaptable filters $a_1(n)$, $a_2(n)$, $a_3(n)$, $a_4(n)$ make it possible to focus on a moving sound source or to focus on a non-moving sound source, while the user of the hearing aid system is moving. Furthermore, the adaptable filters $a_1(n)$, $a_2(n)$, $a_3(n)$, $a_4(n)$ are capable of adapting to changes in the sound environment, such as appearance of a new sound source, disappearance of a noise source or movement of noise sources relative to the user of the hearing aid system.

[0088] The adaptive beamformer filters $a_1(n)$, $a_2(n)$, $a_3(n)$, $a_4(n)$ are designed under the assumption that the signals received at the at least one microphone 14, 16, 14B, 16B can be modelled as a combination of a target signal from a pre-determined target direction plus noise:

$$y_i(n) = h_i(n) * s(n) + v_i(n)$$

where $h_i(n)$ is the impulse response of sound propagation from the source emitting the signal $s(n)$ to the i^{th} microphone and $v_i(n)$ is the noise signal at the same microphone. The noise can consist of both directional noise and other types of noise such as diffuse noise or babble noise.

[0089] The filter coefficients are adaptively determined by solving the following optimization problem:

$$\{a_i(n)\}_{i=1}^4 = \arg \min_{\{a_i(n)\}_{i=1}^4} \|z(n)\|^2$$

$$\text{subject to } \sum_{i=1}^4 a_i(n) * h_i(n) = h_1(n)$$

[0090] Filter adaptation is preferably performed using the least mean square (LMS) algorithm, more preferred the normalized least means square (NLMS) algorithm; however other algorithms may also be used, such as recursive least square, steepest descent or other types of numerical optimization algorithms.

[0091] The outputs of the adaptive filters $a_1(n)$, $a_2(n)$, $a_3(n)$, $a_4(n)$ are added in adder 34, and the output 26 of adder 34 constitutes the estimate of the target signal $z(n)$ = $\widehat{h_1(n)} * s(n)$.

[0092] Subtractor 28 outputs an estimate of the noise: $\widehat{v_1(n)} = y_1(n) - z(n)$.

[0093] Once the target and noise estimate has been determined, the signals are presented to the user in such a way that the SRT of the user is improved as schematically illustrated in Fig. 7.

[0094] Fig. 7 shows an example of the new binaural hearing aid system 10.

[0095] The new binaural hearing aid system 10 has first and second hearing aids 10A, 10B with transceivers 36, 36B for data communication between the two hearing aids 10A, 10B. The first hearing aid 10A comprises at least one microphone with two microphones 14, 16 for provision of microphone audio signals 18, 20 in response to sound received at the respective microphones 14, 16. The microphone audio signals 18, 20 are pre-filtered in respective pre-filters 22, 24 well-known in the art, into microphone audio signals and input to the signal separation unit 12. The signal separation unit 12 is shown in more detail in Fig. 6 and explained above with reference to Fig. 6.

[0096] The second hearing aid 10B also comprises at least one microphone with two microphones 14B, 16B for provision of microphone audio signals 18B, 20B in response to sound received at the respective microphones 14B, 16B. The microphone audio signals 18B, 20B are pre-filtered by pre-filters 22B, 24B as is well-known in the art. Then the pre-filtered microphone audio signals of the two microphones 22B, 24B are encoded in Codec 40B for transmission to the first hearing aid 10A using wireless data transmission. The transmitted data representing the microphone audio signals of the second hearing aid 10B are received by the transceiver 36 of the first hearing aid 10A and decoded in decoder 38 into two microphone audio signals that are input to the signal separation unit 12 as explained above with reference to Fig. 6.

[0097] The signal separation unit 12 is configured to provide the estimate of the target signal 26 and the estimate of the noise signal 30 based on the pre-filtered microphone audio signals of the first and second hearing

aids 10A, 10B.

[0098] The relatively large distance between the microphones of the individual hearing aids 10A, 10B as compared to the distance between microphones of a single hearing aid, makes it possible to configure the beamformer of the signal separation unit 12, see Fig. 6, with a narrow beam directional pattern providing improved spatial separation of the estimate of the target signal 26 from the estimate of the noise signal 30. The conventional output of the beamformer is used as the estimate of the target signal 26, and the estimate of the noise signal 30 is provided by subtraction of the estimate of the target signal 26 from the pre-filtered microphone audio signal of one of the microphones in the plurality of four microphones 14, 16, 14B, 16B.

[0099] Once the target and noise estimate has been determined, the signals are presented to the user in such a way that the SRT of the user is improved: The estimate of the target signal 26 is added to the estimate of the noise signal 30 in a first adder 42 and the output sum of the estimate of the target signal 26 and the estimate of the noise signal 30 is delayed in delay 44 and input to a signal processor 46 for hearing loss compensation. The delay 44 maintains the desired relative phase of the signals output by the first and second hearing aids 10A, 10B, respectively.

[0100] An output transducer 48, in the illustrated example a receiver 48, converts the output of the signal processor 46 into an acoustic output signal that is transmitted towards the eardrum of the user wearing the binaural hearing aid system 10.

[0101] Further, the estimate of the target signal 26 is subtracted; corresponding to a phase shift of 180° , from the estimate of the noise signal 30 in a second adder 50, and the output of the second adder 50 is encoded in Codec 40 for transmission by transceiver 36 to the second hearing aid 10B. In the second hearing aid 10B the transmitted sum is received by the transceiver 36B and decoded by decoder 38B and input to signal processor 46B for hearing loss compensation. An output transducer 48B, in the illustrated example a receiver 48B, converts the output of the signal processor 46B into an acoustic output signal that is transmitted towards the eardrum of the user wearing the binaural hearing aid system 10. In this way, the SRT of the user may be improved up to 20 dB depending on the sound environment.

[0102] The estimate of the target signal 26 and the estimate of the noise signal 30 may be swapped so that the estimate of the noise signal 20 is phase shifted 180° before presentation to one of the eardrums of the user instead of phase shifting the estimate of the target signal 26. The improvement in SRT obtained in this way is smaller than the improvement obtained by phase shift of the estimate of the target signal 26.

Claims

1. A binaural hearing aid system (10) comprising at least one microphone (14, 16, 14B, 16B) for provision of respective at least one microphone audio signal (18, 20, 18B, 20B) in response to sound received at the at least one microphone (14, 16, 14B, 16B),
a signal separation unit (12) configured to provide an estimate of one of a target signal (26) and a noise signal (30) based on the at least one microphone audio signal (18, 20, 18B, 20B),
a phase shift circuit configured to phase shift the estimate of one of the target signal (26) and the noise signal (30) wherein the phase shift ranges from 135° to 225° , and
a phase shift adder (50) connected to provide a phase shifted signal representing sound received at the at least one microphone (14, 16, 14B, 16B) in which the phase shift of the estimate of one of the target signal (26) and the noise signal (30) has substantially substituted the respective original one of the target signal (26) and the noise signal (30), and
a first receiver (48) for conversion of a receiver input signal into an acoustic signal for transmission towards one of the eardrums of a user of the binaural hearing aid system (10), and
a second receiver (48B) for conversion of a receiver input signal into an acoustic signal for transmission towards the other one of the eardrums of the user, and wherein the receiver input of one of the first and second receivers (48, 48B) is connected to a signal representing the phase shifted signal, and
the receiver input of the other one of the first and second receivers (48B, 48) is connected to a signal representing sound received at the at least one microphone (14, 16, 14B, 16B).
2. A binaural hearing aid system (10) according to claim 1, comprising a first hearing aid (10A) comprising at least one microphone (14, 16) for provision of respective at least one microphone audio signal (18, 20) in response to sound received at the at least one microphone (14, 16), and
a second hearing aid (10B) comprising at least one microphone (14B, 16B) for provision of respective at least one microphone audio signal (18B, 20B) in response to sound received at the at least one microphone (14B, 16B), and wherein
a transceiver (36B) in the second hearing aid (10B) is connected for transmission of signals representing the at least one microphone audio signal (18B, 20B) to the first hearing aid (10A), and wherein
a transceiver (36) in the first hearing aid (10A) is connected for reception of the signals representing the at least one microphone audio signal (18B, 20B) of the second hearing aid (10B), and wherein
the signal separation unit (12) is configured to pro-

vide the estimate of one of the target signal (26) and the noise signal (30) based on the at least one microphone audio signals (18, 20, 18B, 20B) of the first and second hearing aids (10A, 10B).

3. A binaural hearing aid system (10) according to claim 1 or 2, wherein the phase shift circuit phase shifts the estimate of the target signal (26).
4. A binaural hearing aid system (10) according to any of the preceding claims, comprising an in-phase adder (42) connected to provide an in-phase sum of the estimate of the target signal (26) and the estimate of the noise signal (30), and wherein the signal representing sound received at the at least one microphone (14, 16, 14B, 16B) is a signal representing the output of the in-phase adder (42).
5. A binaural hearing aid system (10) according to any of the preceding claims, wherein the signal separation unit (12) is configured to provide the estimate based on spectral characteristics of the audio signals.
6. A binaural hearing aid system (10) according to any of the preceding claims, wherein the signal separation unit (12) is configured to provide the estimate based on statistical characteristics of the audio signals.
7. A binaural hearing aid system (10) according to any of the preceding claims, wherein the signal separation unit (12) comprises a beamformer.
8. A binaural hearing aid system (10) according to claim 7 as dependent on claim 2, wherein the beam former is configured to provide the estimate based on microphone audio signals (18, 20, 18B, 20B) of the first and second hearing aids (10A, 10B).
9. A binaural hearing aid system (10) according to claim 7 or 8, wherein the beam former comprises adaptive filters configured to filter respective microphone audio signals and to adapt the respective filter coefficients to minimize the sum of the output signals of the filters.
10. A binaural hearing aid system (10) according to any of the preceding claims, wherein the phase shift ranges from 150° to 210°.
11. A method of binaural signal enhancement in a binaural hearing aid system (10), the method comprising the steps of,
 - providing at least one microphone audio signal (18, 20) in response to sound, and providing an estimate of one of a target signal and a noise signal (30) based on the at least one audio signal,

phase shifting the estimate of one of the target signal (26) and the noise signal (30) wherein the phase shift ranges from 135° to 225°, and
 providing a phase shifted signal representing the at least one microphone audio signal in which the phase shifted estimate of one of the target signal (26) and the noise signal (30) has substantially substituted the respective original one of the target signal (26) and the noise signal (30), and
 transmitting a signal representing the phase shifted signal towards one of the eardrums of a user of the binaural hearing aid system (10), and
 transmitting a signal representing the at least one microphone audio signal towards the other one of the eardrums of the user.

12. A method of binaural signal enhancement according to claim 11, comprising the steps of:

- providing at least one microphone audio signal (18, 20, 18B, 20B) at both ears of the user in response to sound received at both ears, and
 providing the estimate of one of the target signal (26) and the noise signal (30) based on the microphone audio signals (18, 20, 18B, 20B) at both ears.

13. A method of binaural signal enhancement according to claim 11 or 12, wherein the target signal (26) is estimated and phase shifted.

14. A method of binaural signal enhancement according to any of claims 11 - 13, comprising the step of beamforming based on the microphone audio signals.

15. A method of binaural signal enhancement according to claim 14, comprising the step of adaptive filtering of the microphone audio signals by adapting the respective filter coefficients to minimize the sum of the adaptively filtered output signals.

16. A method of binaural signal enhancement according to any of claims 11 - 15, wherein the phase shift ranges from 150° to 210°.

Patentansprüche

1. Binaurales Hörhilfesystem (10), Folgendes umfassend:

- mindestens ein Mikrofon (14, 16, 14B, 16B) zum Bereitstellen mindestens eines Mikrofonaudio-signals (18, 20, 18B, 20B) in Reaktion auf ein Geräusch, das von dem mindestens einen Mikrofon (14, 16, 14B, 16B) empfangen wurde, eine Signaltrennungseinheit (12), die dafür konfiguriert ist, basierend auf dem mindestens ei-

nen Mikrofonaudiosignal (18, 20, 18B, 20B) eine Schätzung eines Sollsignals (26) und/oder eines Rauschsignals (30) bereitzustellen, eine Phasenverschiebungsschaltung, die dafür konfiguriert ist, die Schätzung des Sollsignals (26) und/oder Rauschsignals (30) phasenzuverschieben, wobei die Phasenverschiebung im Bereich von 135 bis 225° liegt, und einen Phasenverschiebungsaddierer (50), der angeschlossen ist, um ein phasenverschobenes Signal bereitzustellen, welches das von dem mindestens einen Mikrofon (14, 16, 14B, 16B) empfangene Geräusch darstellt und bei dem die Phasenverschiebung der Schätzung des Sollsignals (26) und/oder Rauschsignals (30) im Wesentlichen das ursprüngliche Sollsignal (26) beziehungsweise Rauschsignal (30) ersetzt hat, und einen ersten Empfänger (48) zum Umwandeln eines Empfängereingangssignals in ein akustisches Signal für eine Übertragung zu einem der Trommelfelle eines Benutzers des binauralen Hörhilfesystems (10) und einen zweiten Empfänger (48B) zum Umwandeln eines Empfängereingangssignals in ein akustisches Signal für eine Übertragung zu dem anderen der Trommelfelle des Benutzers, wobei der Empfängereingang vom ersten oder zweiten Empfänger (48, 48B) mit einem Signal verbunden ist, welches das phasenverschobene Signal darstellt, und der Empfängereingang des anderen des ersten und zweiten Empfängers (48B, 48) mit einem Signal verbunden ist, welches ein Geräusch darstellt, das von dem mindestens einen Mikrofon (14, 16, 14B, 16B) empfangen wurde.

2. Binaurales Hörhilfesystem (10) nach Anspruch 1, Folgendes umfassend:

eine erste Hörhilfe (10A), die mindestens ein Mikrofon (14, 16) zum Bereitstellen jeweils mindestens eines Mikrofonaudiosignals (18, 20) in Reaktion auf ein Geräusch umfasst, das von dem mindestens einen Mikrofon (14, 16) empfangen wurde, und eine zweite Hörhilfe (10B), die mindestens ein Mikrofon (14B, 16B) zum Bereitstellen jeweils mindestens eines Mikrofonaudiosignals (18B, 20B) in Reaktion auf ein Geräusch umfasst, das von dem mindestens einen Mikrofon (14B, 16B) empfangen wurde, und wobei ein Sendeempfänger (36B) in der zweiten Hörhilfe (10B) angeschlossen ist, um Signale, die das mindestens eine Mikrofonaudiosignal (18B, 20B) darstellen, zur ersten Hörhilfe (10A) zu übertragen, und wobei ein Sendeempfänger (36) in der ersten Hörhilfe

(10A) angeschlossen ist, um die Signale, die das mindestens eine Mikrofonaudiosignal (18B, 20B) der zweiten Hörhilfe (10B) darstellen, zu empfangen, und wobei die Signaltrennungseinheit (12) dafür konfiguriert ist, die Schätzung des Sollsignals (26) oder des Rauschsignals (30) basierend auf den mindestens einen Mikrofonaudiosignalen (18, 20, 18B, 20B) der ersten und der zweiten Hörhilfe (10A, 10B) bereitzustellen.

3. Binaurales Hörhilfesystem (10) nach Anspruch 1 oder 2, wobei die Phasenverschiebungsschaltung die Schätzung des Sollsignals (26) phasenverschiebt.
4. Binaurales Hörhilfesystem (10) nach einem der vorhergehenden Ansprüche, einen gleichphasigen Addierer (42) umfassend, der dafür angeschlossen ist, eine gleichphasige Summe der Schätzung des Sollsignals (26) und der Schätzung des Rauschsignals (30) bereitzustellen, und wobei das Signal, welches das an dem mindestens einen Mikrofon (14, 16, 14B, 16B) empfangene Geräusch darstellt, ein Signal ist, das die Ausgabe des gleichphasigen Addierers (42) darstellt.
5. Binaurales Hörhilfesystem (10) nach einem der vorhergehenden Ansprüche, wobei die Signaltrennungseinheit (12) dafür konfiguriert ist, die Schätzung basierend auf Spektraleigenschaften des Audiosignals bereitzustellen.
6. Binaurales Hörhilfesystem (10) nach einem der vorhergehenden Ansprüche, wobei die Signaltrennungseinheit (12) dafür konfiguriert ist, die Schätzung basierend auf statistischen Eigenschaften des Audiosignals bereitzustellen.
7. Binaurales Hörhilfesystem (10) nach einem der vorhergehenden Ansprüche, wobei die Signaltrennungseinheit (12) einen Strahlformer umfasst.
8. Binaurales Hörhilfesystem (10) nach Anspruch 7, soweit abhängig von Anspruch 2, wobei der Strahlformer dafür konfiguriert ist, basierend auf Mikrofonaudiosignalen (18, 20, 18B, 20B) der ersten und der zweiten Hörhilfe (10A, 10B) die Schätzung bereitzustellen.
9. Binaurales Hörhilfesystem (10) nach Anspruch 7 oder 8, wobei der Strahlformer adaptive Filter umfasst, die dafür konfiguriert sind, entsprechende Mikrofonaudiosignale zu filtern und die entsprechenden Filterkoeffizienten anzupassen, um die Summe der Ausgabesignale der Filter zu minimieren.
10. Binaurales Hörhilfesystem (10) nach einem der vor-

hergehenden Ansprüche, wobei die Phasenverschiebung im Bereich von 150 bis 210° liegt.

11. Verfahren zur binauralen Signalverstärkung in einem binauralen Hörhilfesystem (10), wobei das Verfahren folgende Schritte umfasst:

Bereitstellen mindestens eines Mikrofonaudiosignals (18, 20) in Reaktion auf ein Geräusch und
Bereitstellen einer Schätzung eines Sollsignals oder eines Rauschsignals (30) basierend auf dem mindestens einen Audiosignal, Phasenverschieben der Schätzung des Sollsignals (26) oder des Rauschsignals (30), wobei die Phasenverschiebung im Bereich von 135 bis 225° liegt, und
Bereitstellen eines phasenverschobenen Signals, welches das mindestens eine Mikrofonaudiosignal darstellt, bei dem die phasenverschobene Schätzung des Sollsignals (26) oder des Rauschsignals (30) im Wesentlichen das entsprechende ursprüngliche Sollsignal (26) oder Rauschsignal (30) ersetzt hat, und
Übertragen eines Signals, welches das phasenverschobene Signal darstellt, zu einem der Trommelfelle eines Benutzers des binauralen Hörhilfesystems (10) und
Übertragen eines Signals, welches das mindestens eine Mikrofonaudiosignal darstellt, zu dem anderen der Trommelfelle des Benutzers.

12. Verfahren zur binauralen Signalverstärkung nach Anspruch 11, folgende Schritte umfassend:

Bereitstellen mindestens eines Mikrofonaudiosignals (18, 20, 18B, 20B) an beiden Ohren des Benutzers in Reaktion auf an beiden Ohren empfangene Geräusche und
Bereitstellen der Schätzung des Sollsignals (26) oder des Rauschsignals (30) basierend auf dem Mikrofonaudiosignal (18, 20, 18B, 20B) an beiden Ohren.

13. Verfahren zur binauralen Signalverstärkung nach Anspruch 11 oder 12, wobei das Sollsignal (26) geschätzt und phasenverschoben wird.

14. Verfahren zur binauralen Signalverstärkung nach einem der Ansprüche 11 - 13, umfassend den Schritt der Strahlbildung basierend auf den Mikrofonaudiosignalen.

15. Verfahren zur binauralen Signalverstärkung nach Anspruch 14, den Schritt des adaptiven Filterns der Mikrofonaudiosignale durch Anpassen des entsprechenden Filterkoeffizienten umfassend, um die Summe der adaptiv gefilterten Ausgabesignale zu

minimieren.

16. Verfahren zur binauralen Signalverstärkung nach einem der Ansprüche 11 - 15, wobei die Phasenverschiebung im Bereich von 150 bis 210° liegt.

Revendications

1. Système de prothèse auditive stéréophonique (10) comprenant :

au moins un microphone (14, 16, 14B, 16B) pour fournir respectivement au moins un signal audio de microphone (18, 20, 18B, 20B) en réponse à un son reçu sur le au moins un microphone (14, 16, 14B, 16B),
une unité de séparation de signal (12) configurée pour fournir une estimation de l'un ou l'autre d'un signal cible (26) et d'un signal de bruit (30) sur la base du au moins un signal audio de microphone (18, 20, 18B, 20B),
un circuit de déphasage configuré pour déphaser l'estimation de l'un ou l'autre du signal cible (26) et du signal de bruit (30), dans lequel le déphasage se situe dans une plage de 135° à 225° et
un additionneur de déphasage (50) raccordé pour fournir un signal déphasé représentant un son reçu sur le au moins un microphone (14, 16, 14B, 16B), dans lequel le déphasage de l'estimation de l'un ou l'autre du signal cible (26) et du signal de bruit (30) a sensiblement remplacé le signal original respectif entre le signal cible (26) et le signal de bruit (30), et
un premier récepteur (48) pour la conversion d'un signal d'entrée de récepteur en un signal acoustique pour transmission vers l'une des caisses de tympan d'un utilisateur du système de prothèse auditive stéréophonique (10) et
un second récepteur (48B) pour la conversion d'un signal d'entrée de récepteur en un signal acoustique pour la transmission vers l'autre des caisses de tympan de l'utilisateur et dans lequel l'entrée de l'un ou l'autre du premier et du second récepteur (48, 48B) est raccordée à un signal représentant le signal déphasé et
l'entrée de l'autre des premier et second récepteurs (48B, 48) est raccordée à un signal représentant le son reçu sur le au moins un microphone (14, 16, 14B, 16B).

2. Système de prothèse auditive stéréophonique (10) selon la revendication 1, comprenant :

une première prothèse auditive (10A) comprenant au moins un microphone (14, 16) pour fournir respectivement au moins un signal audio de

- microphone (18, 20) en réponse au son reçu sur le au moins un microphone (14, 16) et une seconde prothèse auditive (10B) comprenant au moins un microphone (14B, 16B) pour fournir respectivement au moins un signal audio de microphone (18B, 20B) en réponse au son reçu sur le au moins un microphone (14B, 16B), et dans lequel :
- un émetteur-récepteur (36B) dans la seconde prothèse auditive (10B) est raccordé pour transmettre des signaux représentant le au moins un signal audio de microphone (18B, 20B) à la première prothèse auditive (10A), et dans lequel :
- un émetteur-récepteur (36) dans la première prothèse auditive (10A) est raccordé pour recevoir des signaux représentant le au moins un signal audio de microphone (18B, 20B) de la seconde prothèse auditive (10B), et dans lequel :
- l'unité de séparation de signal (12) est configurée pour fournir l'estimation de l'un ou l'autre du signal cible (26) et du signal de bruit (30) sur la base du au moins un signal audio de microphone (18, 20, 18B, 20B) des première et seconde prothèses auditives (10A, 10B).
3. Système de prothèse auditive stéréophonique (10) selon la revendication 1 ou la revendication 2, dans lequel le circuit de déphasage déphase l'estimation du signal cible (26).
 4. Système de prothèse auditive stéréophonique (10) selon l'une quelconque des revendications précédentes, comprenant un additionneur en phase (42) raccordé pour fournir une somme en phase de l'estimation du signal cible (26) et de l'estimation du signal de bruit (30) et dans lequel le signal représentant le son reçu sur le au moins un microphone (14, 16, 14B, 16B) est un signal représentant la sortie de l'additionneur en phase (42).
 5. Système de prothèse auditive stéréophonique (10) selon l'une quelconque des revendications précédentes, dans lequel l'unité de séparation de signal (12) est configurée pour fournir l'estimation basée sur les caractéristiques spectrales des signaux audio.
 6. Système de prothèse auditive stéréophonique (10) selon l'une quelconque des revendications précédentes, dans lequel l'unité de séparation de signal (12) est configurée pour fournir l'estimation basée sur les caractéristiques statistiques des signaux audio.
 7. Système de prothèse auditive stéréophonique (10) selon l'une quelconque des revendications précédentes, dans lequel l'unité de séparation du signal (12) comprend un formateur de faisceau.
 8. Système de prothèse auditive stéréophonique (10) selon la revendication 7 dans la mesure où elle dépend de la revendication 2, dans lequel le formateur de faisceau est configuré pour fournir l'estimation basée sur les signaux audio de microphone (18, 20, 18B, 20B) de la première et de la seconde prothèse auditive (10A, 10B).
 9. Système de prothèse auditive stéréophonique (10) selon la revendication 7 ou la revendication 8, dans lequel le formateur de faisceau comprend des filtres adaptatifs configurés pour filtrer des signaux audio de microphone respectifs et pour adapter les coefficients de filtres respectifs afin de minimiser la somme des signaux de sortie des filtres.
 10. Système de prothèse auditive stéréophonique (10) selon l'une quelconque des revendications précédentes, dans lequel le décalage de phase se situe dans une plage de 150° à 210°.
 11. Procédé de renforcement du signal stéréophonique dans un système de prothèse auditive stéréophonique (10), le procédé comprenant les étapes consistant à :

fournir au moins un signal audio de microphone (18, 20) en réponse à un son et

fournir une estimation de l'un ou l'autre d'un signal cible et d'un signal de bruit (30) sur la base du au moins un signal audio,

déphaser l'estimation de l'un ou l'autre du signal cible (26) et du signal de bruit (30), dans lequel le déphasage se situe dans une plage de 135° à 225° et

fournir un signal déphasé représentant le au moins signal audio de microphone, dans lequel l'estimation déphasée de l'un ou l'autre du signal cible (26) et du signal de bruit (30) a sensiblement remplacé le signal original respectif entre le signal cible (26) et le signal de bruit (30), et

transmettre un signal représentant le signal déphasé vers l'une des caisses de tympan d'un utilisateur d'un système de prothèse auditive stéréophonique (10) et

transmettre un signal représentant le au moins un signal audio de microphone vers l'autre des caisses de tympan de l'utilisateur.
 12. Procédé de renforcement du signal stéréophonique selon la revendication 11, comprenant les étapes consistant à :

fournir au moins un signal audio de microphone (18, 20, 18B, 20B) aux deux oreilles de l'utilisateur en réponse à un son reçu aux deux oreilles et

fournir l'estimation de l'un ou l'autre du signal cible (26) et du signal de bruit (30) sur la base des signaux audio de microphone (18, 20, 18B, 20B) au niveau des deux oreilles. 5

13. Procédé de renforcement du signal stéréophonique selon la revendication 11 ou la revendication 12, dans lequel le signal cible (26) est estimé et déphasé. 10

14. Procédé de renforcement du signal stéréophonique selon l'une quelconque des revendications 11 à 13, comprenant l'étape de formation d'un faisceau sur la base des signaux audio de microphone. 15

15. Procédé de renforcement du signal stéréophonique selon la revendication 14, comprenant l'étape de filtration adaptative des signaux audio de microphone par adaptation des coefficients de filtres respectifs afin de minimiser la somme des signaux de sortie filtrés de manière adaptative. 20

16. Procédé de renforcement du signal stéréophonique selon l'une quelconque des revendications 11 à 15, dans lequel le déphasage se situe dans une plage de 150° à 210°. 25

30

35

40

45

50

55

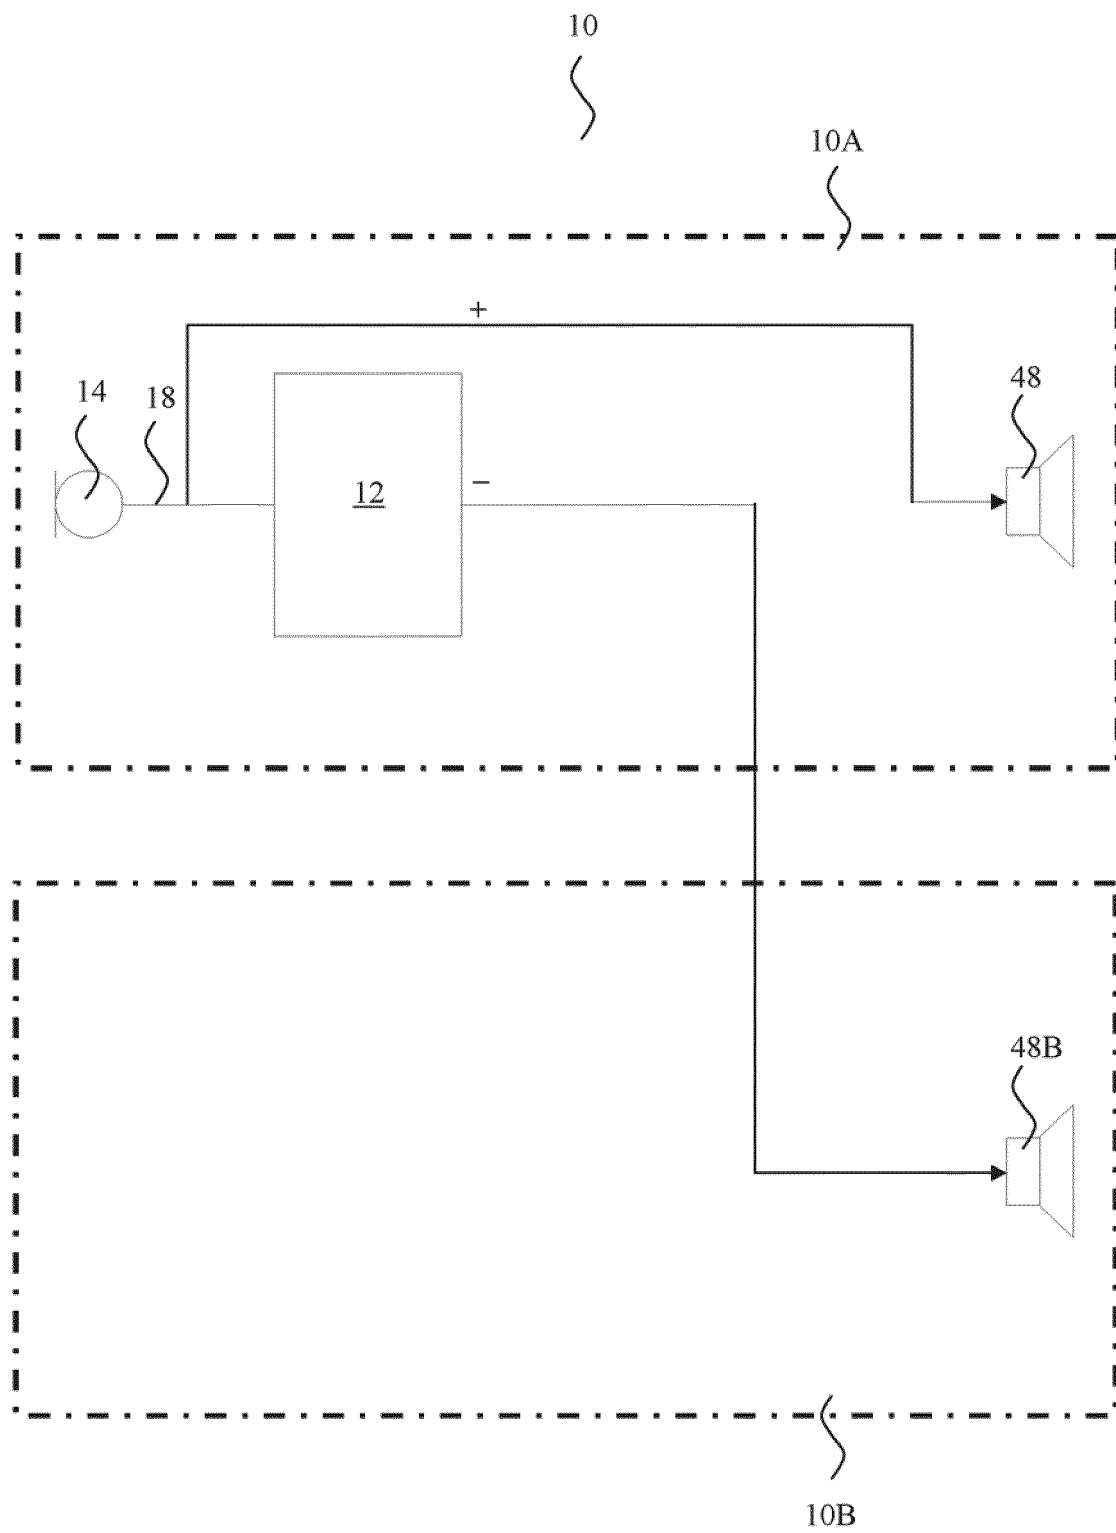


Fig. 1

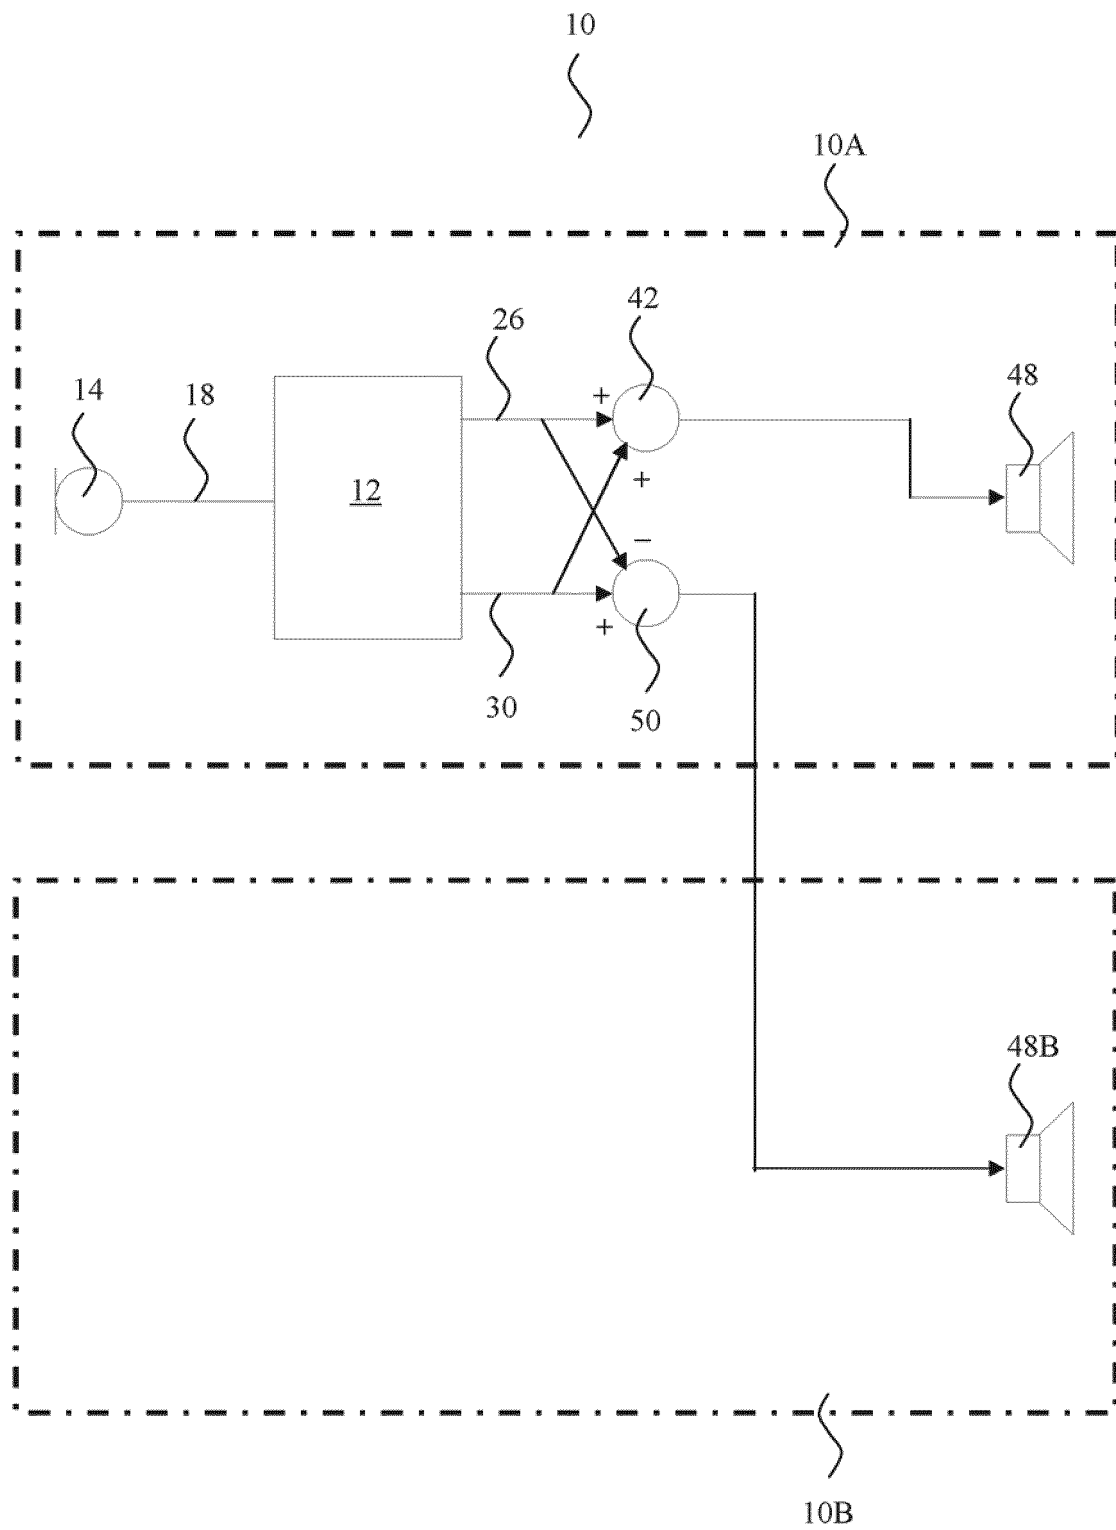


Fig. 2

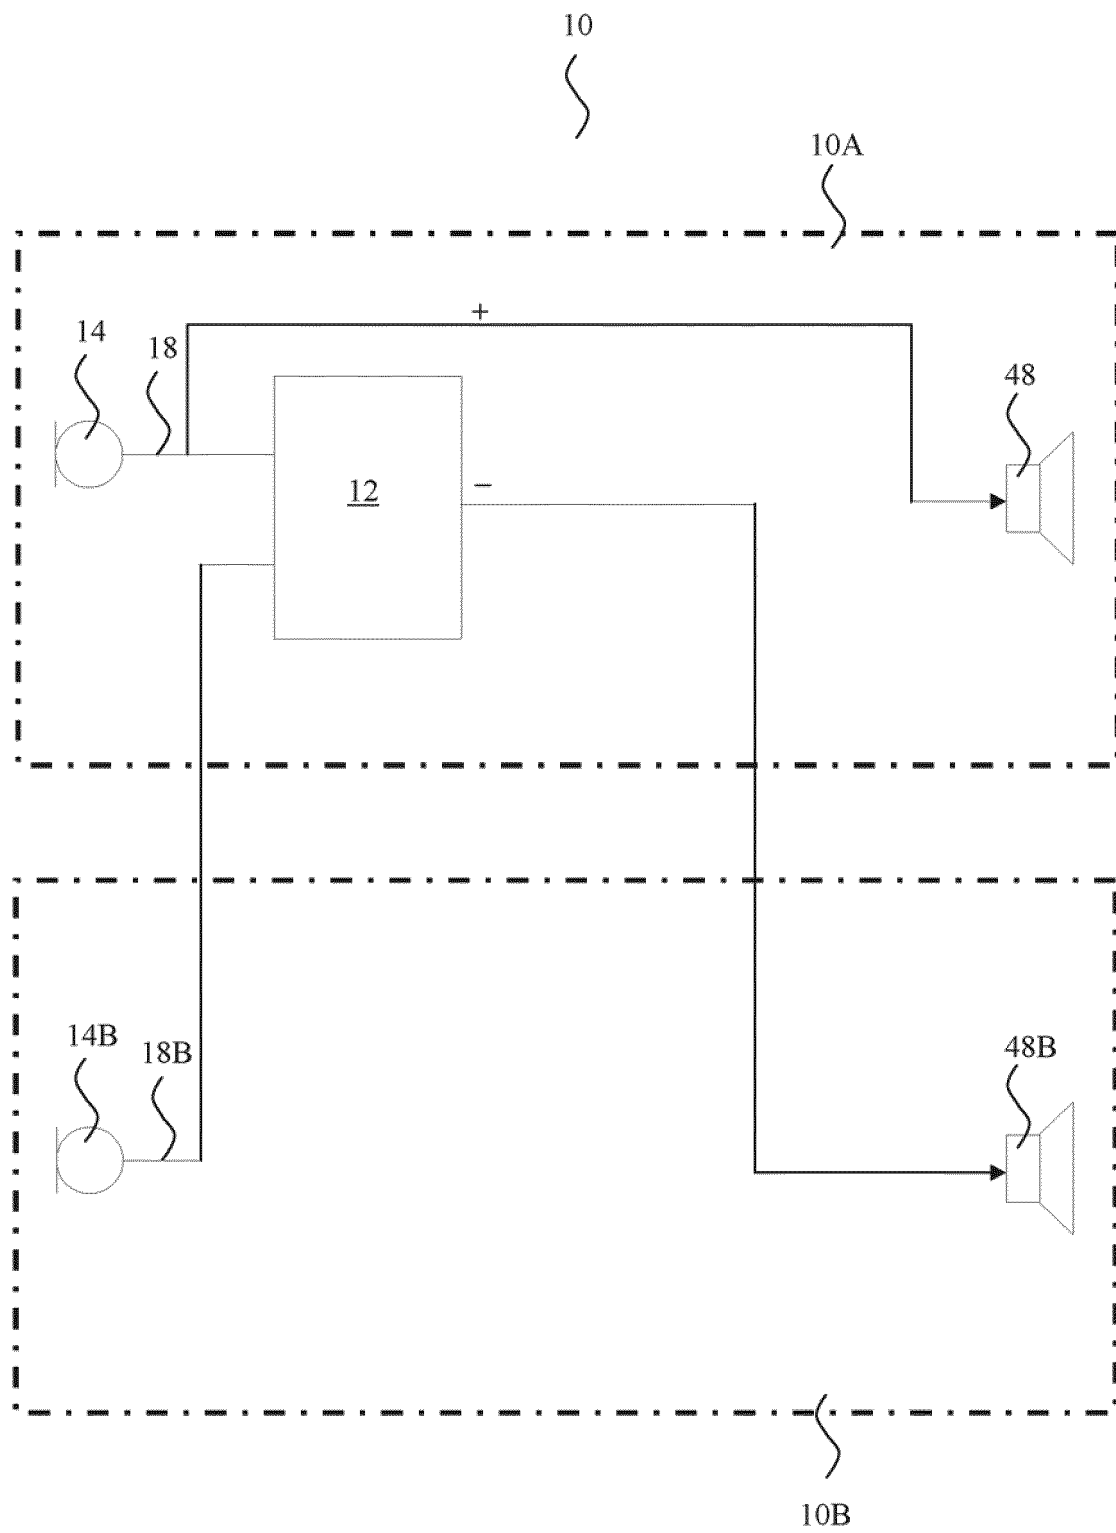


Fig. 3

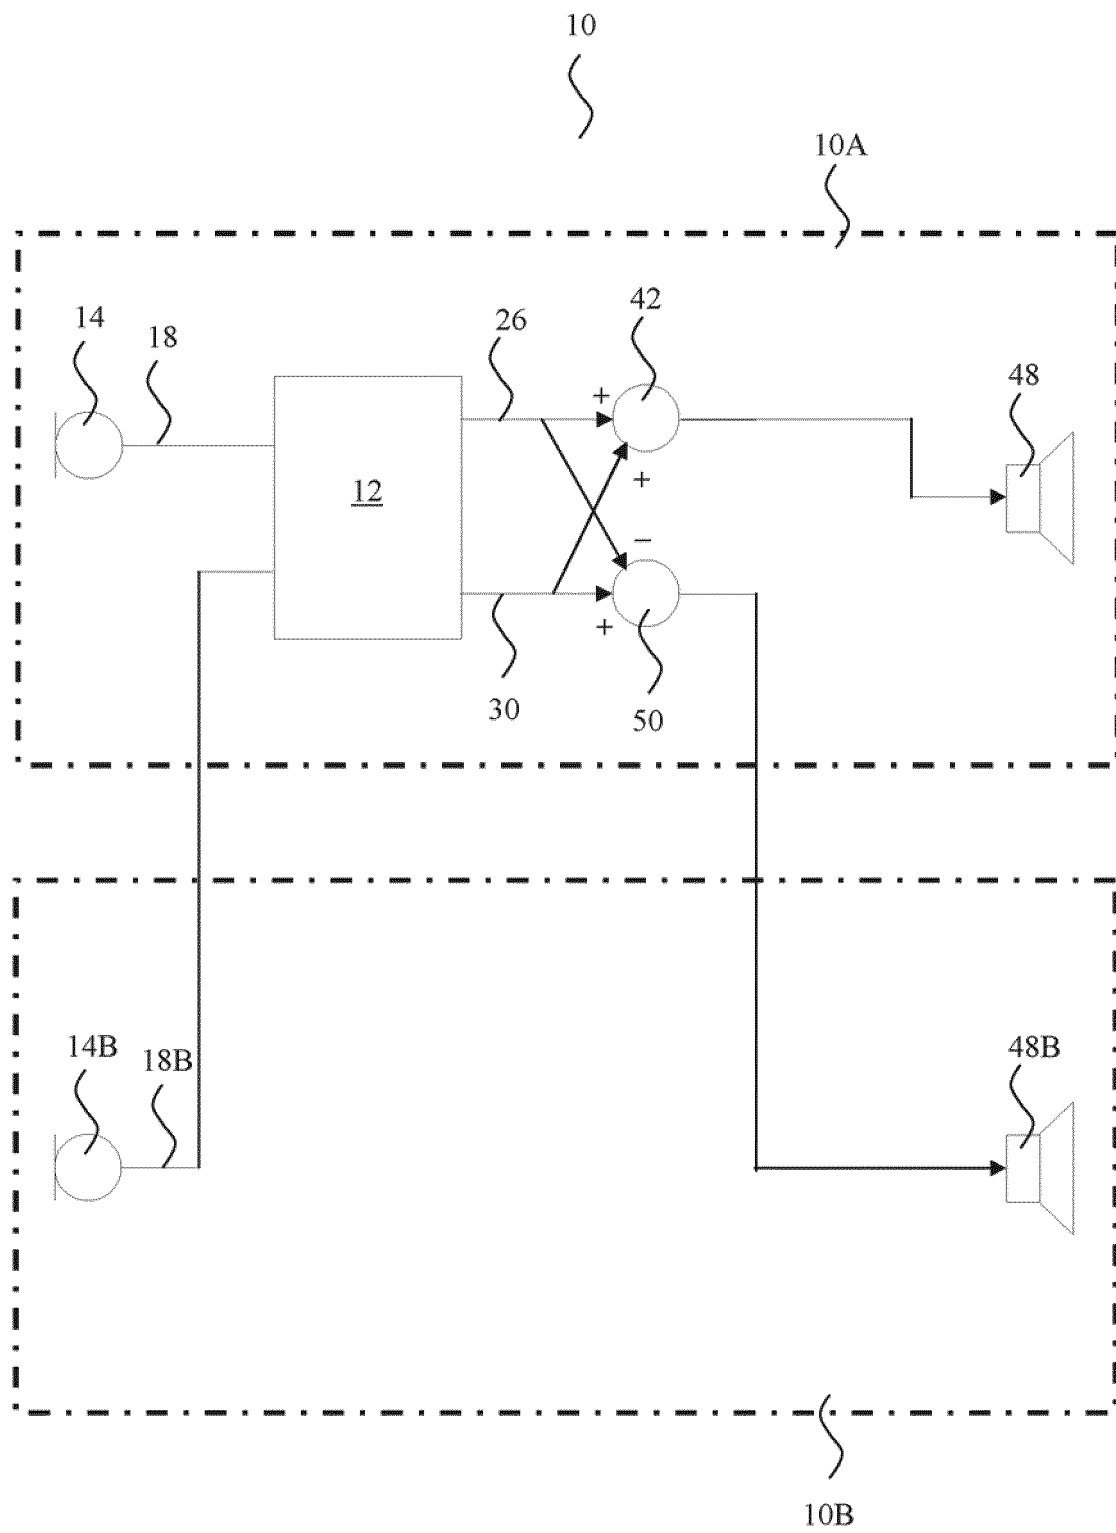


Fig. 4

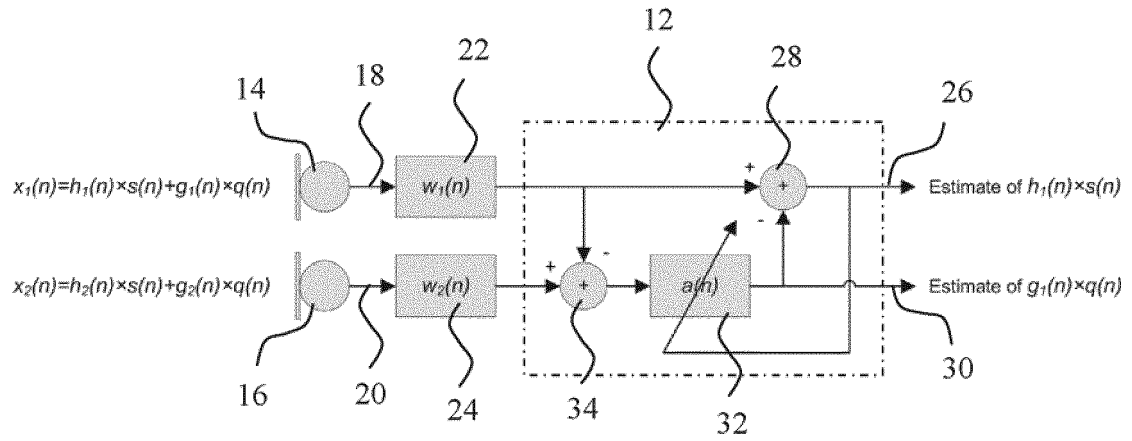


Fig. 5

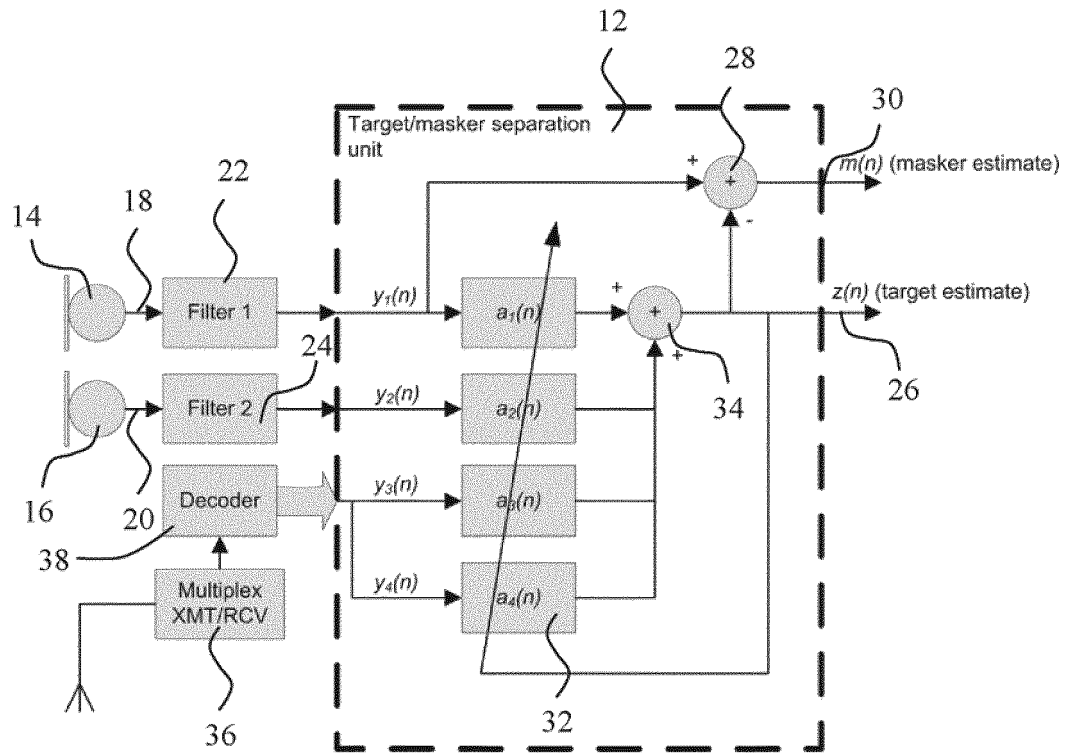


Fig. 6

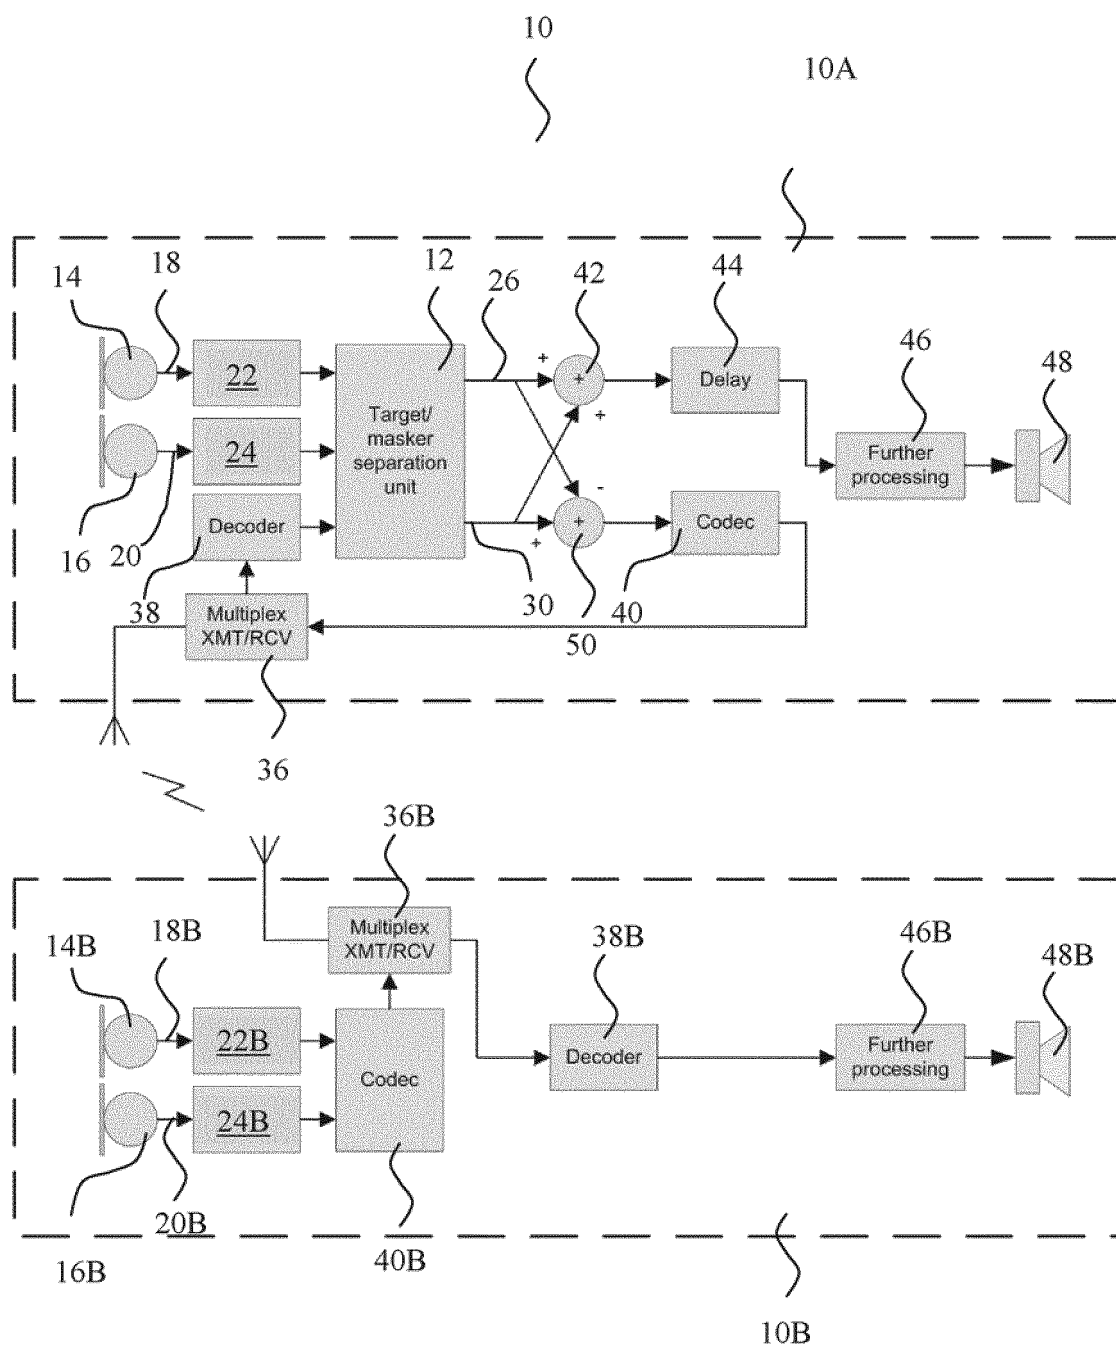


Fig. 7

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- WO 0207479 A [0039]