



(12) **EUROPEAN PATENT APPLICATION**

(43) Date of publication:
11.11.2015 Bulletin 2015/46

(51) Int Cl.:
A61N 1/36 (2006.01)

(21) Application number: **15170882.3**

(22) Date of filing: **10.04.2012**

(84) Designated Contracting States:
**AL AT BE BG CH CY CZ DE DK EE ES FI FR GB
GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO
PL PT RO RS SE SI SK SM TR**

- **Weisgarber, Jeffrey A.**
Jewett, OH Ohio 43986 (US)
- **Polefko, Richard J.**
Parma, OH Ohio 44130 (US)

(30) Priority: **07.04.2011 US 201113082097**

(74) Representative: **Lecomte & Partners**
P.O. Box 1623
1016 Luxembourg (LU)

(62) Document number(s) of the earlier application(s) in
accordance with Art. 76 EPC:
12163520.5 / 2 508 226

(71) Applicant: **Greatbatch Ltd.**
Clarence, NY 14031 (US)

Remarks:

This application was filed on 05-06-2015 as a
divisional application to the application mentioned
under INID code 62.

(72) Inventors:
• **Trier, Stephen**
Mayfield Heights, OH Ohio 44124 (US)

(54) **ARBITRARY WAVEFORM GENERATOR AND NEURAL STIMULATION APPLICATOR WITH
SCALABLE WAVEFORM FEATURE**

(57) A device and/or system for generating arbitrary
scalable waveforms of a desired shape that can be used
for generating a stimulation pulse for medical purposes
such as for spinal cord stimulation therapy, where scaling

function(s) can be used to scale arbitrary waveforms for
increased flexibility and which can also be used for
charge balancing purposes as well.

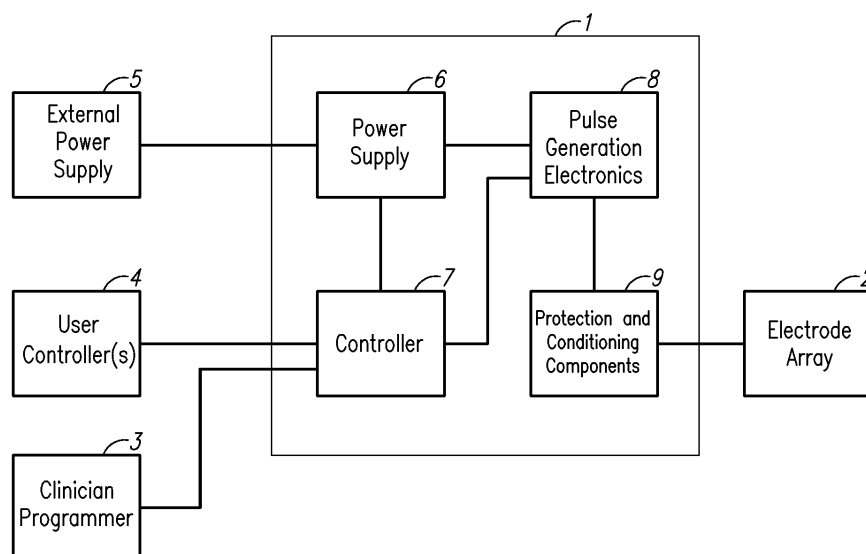


FIG. 1

Description

FIELD OF THE INVENTION

[0001] This application relates generally to a device for generating waveforms, and more specifically, this application relates to an implantable medical device for generating waveforms for spinal cord stimulation.

BACKGROUND OF THE INVENTION

[0002] Programmable pulse generating systems are used to treat chronic pain by providing electrical stimulation pulses from an electrode array placed in or near a patient's spine. Such Spinal Cord Stimulation (SCS) is useful for reducing pain in certain populations of patients. SCS systems typically include one or more electrodes connected to an External Pulse Generator (EPG) or an Implanted Pulse Generator (IPG) via lead wires. In the case of an EPG, the lead wires must be connected to the EPG via an exit from the body. The pulse generator, whether implanted or external, generates electrical pulses that are typically delivered to the dorsal column fibers within the spinal cord through the electrodes which are implanted along or near the epidural space of the spinal cord. In a typical situation, the attached lead wires exit the spinal cord and are tunneled within the torso of the patient to a sub-cutaneous pocket where the IPG is implanted, or the wires exit the patient for connection to the EPG.

[0003] Neural stimulators for SCS to date have been limited to waveform shapes dictated by their circuitry. Most emit relatively simple rectangular or trapezoidal stimulation phases with exponential, clamped-exponential, or rectangular charge recovery phases. Similar waveform limitations typically exist for stimulators used in other medical applications such as cardiac implants, cochlear implants, etc. Nevertheless, it is desirable that other waveform shapes be available, as such shapes may be useful in controlling which nerve fibers respond to a stimulation pulse. By selecting particular fibers for response, the therapeutic benefit of neural stimulation can be increased and side-effects decreased. Additionally, other waveform shapes may achieve effective stimulation results while requiring less energy than traditional waveforms, thereby extending the battery life of the stimulator.

[0004] Currently, the principal way to select a stimulation waveform was to design a stimulator that emitted that waveform as its only form, or as one of a handful of parameter-driven options. For example, a stimulator may be provided that adjusts the charge recovery phase to either an exponential or a rectangular shape based on the pulse rate selected by the user. The stimulation phase is typically provided with only a fixed rectangular shape. In contrast, it would be useful to allow the use of an arbitrary waveform shape for the either the stimulation phase, charge recovery phase, or both, rather than being

limited to a simple waveform shape designed into the circuitry.

[0005] Desired is a capability of producing complex waveform shapes, whether or not they are inherently piecewise-linear, in particular with an ability to adjust amplitudes and pulsewidths simply and efficiently, such as, for example, by providing an ability to rescale portions of a waveform in time, thus adjusting pulsewidths on the fly without having to re-compute the waveform samples.

[0006] An additional problem with existing neural stimulators is that they include DC blocking capacitors to balance charges and prevent the flow of direct current to the body tissue. Balancing such charges and blocking dc current flow is considered desirable for safety reasons. Desired is an approach that removes or reduces the need for such blocking capacitors or their size by inherently balancing the stimulation waveform charges and preventing the flow of direct current.

[0007] Finally, it would be useful to scale an arbitrary waveform in time and amplitude in a manner that preserves the overall charge that is provided by the waveform when used in a stimulation pulse.

SUMMARY OF THE INVENTION

[0008] Disclosed herein is a device/system capable of producing complex waveform shapes, whether or not they are inherently piecewise-linear. It is also capable of adjusting amplitudes and pulsewidths simply and efficiently.

[0009] Further disclosed herein is a device/system that can rescale portions of a waveform in time, thus adjusting pulsewidths, directly without having to recompute the waveform samples. Such a device/system can also generate the waveform, for example by using data from one or more small template waveshapes stored in a small memory, permitting it to use much less memory for complex waveforms.

[0010] Provided are a plurality of embodiments of the invention, including, but not limited to, a method for providing a therapy to a patient, the method comprising the steps of:

providing a waveform generating circuit for generating a waveform of a desired shape having an amplitude and a duration;

defining a scaling factor;

using the scaling factor for scaling the waveform generated by the waveform generating circuit, such that both the amplitude and the duration of the waveform is adjusted using the scaling factor; and

providing a stimulation pulse including at least a substantial portion that is based on the scaled waveform having shape resembling the desired shape of the waveform for stimulating a stimulation region of the

patient.

[0011] Also provided is a method for providing a therapy to a patient, with the method comprising the steps of:

generating a first waveform of a desired shape using a waveform generator;

providing a first portion of a stimulation pulse substantially resembling the first waveform, the stimulation pulse for stimulating a stimulation region of the patient;

defining a scaling factor;

using the scaling factor for generating a second waveform using the waveform generator, the second waveform being a scaled version of the first waveform; and

providing a second portion of the stimulation pulse substantially resembling the second waveform, the second portion of the stimulation pulse for stimulating the stimulation region of the patient.

[0012] Further provided is a method for providing a therapy to a patient, with the method comprising the steps of:

determining a first waveform of a desired shape using a waveform generator, the desired shape including at least a portion of a shape other than a square wave;

defining a scaling factor;

using the scaling factor for generating a second waveform using the waveform generator, the second waveform being a scaled version of the first waveform such that the second waveform is scaled in time and/or amplitude based on the scaling factor; and

providing a stimulation pulse including a portion substantially resembling the second waveform, the stimulation pulse for stimulating a stimulation region of the patient.

[0013] Also provided is a stimulation device for stimulating a stimulation region within a patient comprising a waveform generation circuit for generating a waveform part having a shape based on a desired waveform other than a square wave; a time scaling circuit for input to the waveform generation circuit, wherein the waveform part generated by the waveform generation circuit resembles the desired waveform scaled in time based on a value of a scaling factor; and a stimulation pulse generating circuit for generating a stimulation pulse including a portion based on the scaled waveform part, wherein the stimu-

lation pulse is provided to a stimulation region of the patient.

[0014] Also provided is a stimulation device for stimulating a stimulation region within a patient comprising: a waveform generation circuit for generating a first waveform and a second waveform; a time scaling circuit for input to the waveform generation circuit; a scaling circuit connected to the waveform generation circuit for scaling the second waveform based on the first waveform scaled in time by a scaling factor; an amplitude scaling circuit for further scaling the second waveform in amplitude based on the scaling factor; and a stimulation pulse generating circuit for generating a stimulation pulse including a portion based on the second waveform such that the portion of the stimulation pulse resembles the first waveform scaled both in time and in amplitude based on the scaling factor, and for providing the stimulation pulse to a stimulation region of the patient.

[0015] Further provided is a stimulation device for stimulating a stimulation region within a patient comprising: a first waveform generation circuit for generating a first waveform part/phase based on a first waveform; a second waveform generation circuit for generating a second waveform part based on a second waveform; a scaling circuit for input to the first waveform generation circuit and the second waveform generation circuit; a scaling register for storing, or an input for inputting, one or more variable scaling values for input to the scaling circuit, wherein the first waveform part/phase generated by the first waveform generation circuit is based on the first waveform scaled based on a value one of the one or more scaling values and wherein the second waveform part generated by the second waveform generation circuit is based on the second waveform scaled based on a value of one of the one or more scaling values, such that the stimulation device is adapted such that different scaling values can be used for respectively generating the first part/phase and the second part/phase; a stimulation pulse generating circuit for generating a stimulation pulse comprised of a first pulse phase generated from the first waveform part/phase and a second pulse phase generated from the second waveform part/phase, wherein the stimulation pulse is provided to a stimulation region of the patient.

[0016] Also provided is a stimulation device for stimulating a stimulation region within a patient comprising: a first waveform generation circuit for generating a first waveform part based on a first waveform; a second waveform generation circuit for generating a second waveform part based on a second waveform; a time scaling circuit for input to the first waveform generation circuit and the second waveform generation circuit; a scaling register for storing, or an input for inputting, one or more variable scaling values for input to the time scaling circuit, wherein the first waveform part generated by the first waveform generation circuit is based on the first waveform scaled in time based on a value of one of the one or more scaling values and wherein the second waveform part generated

by the second waveform generation circuit is based on the second waveform scaled in time based on the value of the one, or another one, of the one or more scaling values; an amplitude scaling circuit for inputting the one or more variable scaling values for further scaling an amplitude the first waveform part in amplitude based on the value of the one of the one or more scaling values, the amplitude scaling circuit also for inputting the value of the one, or the another one, of the one or more scaling values for further scaling an amplitude the second waveform part in amplitude based on the value of the one, or the another one, of the one or more scaling values; and a stimulation pulse generating circuit for generating a stimulation pulse comprised of a first pulse phase generated from the first waveform part and a second pulse phase generated from the second waveform part as scaled by the amplitude scaling circuit and the time scaling circuit, wherein the stimulation pulse is provided to a stimulation region of the patient.

[0017] For the above device, the pulse can be adapted such that a charge induced on the stimulation region of the patient by the first part of the stimulation pulse is substantially canceled by the second part of the stimulation pulse

[0018] Also provided is a stimulation device for stimulating a stimulation region within a patient comprising: a waveform generation circuit for generating a waveform; a time scaling circuit for input to the waveform generation circuit for providing a programmable time scale to the waveform generation circuit; a scaling register for storing, or an input for inputting a programmable scaling value for input to the time scaling circuit, wherein the waveform generated by the waveform generation circuit is scalable in time based the scaling value such that different values of the scaling value can be used to expand and/or compress the waveform in time; and a stimulation pulse generating circuit for generating a stimulation pulse comprised of the waveform, wherein the stimulation pulse is provided to a stimulation region of the patient.

[0019] Further provided is a system using any of the above devices and/or methods.

[0020] Also provided is a system for stimulating a stimulation region of the spine within a patient comprising: an implantable pulse generation device (IPG) adapted to be implanted in the patient, one or more electrodes connected to the IPG and adapted to be provided near the stimulation region for providing the stimulation pulse to the stimulation region; an external device for wirelessly connecting to the IPG for controlling an operation of the IPG; and an external energy transmitter for wirelessly providing electrical energy to an energy storage device inside the IPG.

[0021] The IPG of the above system includes: a rechargeable battery for providing power to the IPG, a first waveform generation circuit for generating a first waveform part, a second waveform generation circuit for generating a second waveform part, a time scaling circuit for input to the first waveform generation circuit and the sec-

ond waveform generation circuit, a scaling register for storing one or more variable scaling values for input to the time scaling circuit, wherein the first waveform part generated by the first waveform generation circuit is scaled in time based on a value of one of the one or more scaling values and wherein the second waveform part generated by the second waveform generation circuit is scaled in time based on the value of the one, or another one, of the one or more scaling values, an amplitude scaling circuit for inputting the one or more variable scaling values for further scaling the first waveform part in amplitude based on the value of the one of the one or more scaling values, the amplitude scaling circuit also for inputting the value of the one, or the another one, of the one or more scaling values for further scaling the second waveform part in amplitude based on the value of the one, or the another one, of the one or more scaling values, and a stimulation pulse generating circuit for generating a stimulation pulse comprised of a first pulse phase generated from the first waveform part and a second pulse phase generated from the second waveform part as scaled by the amplitude scaling circuit and the time scaling circuit.

[0022] The stimulation system also comprising one or more electrodes connected to the IPG and adapted to be provided near the stimulation region for providing the stimulation pulse to the stimulation region; an external device for wirelessly connecting to the IPG for controlling an operation of the IPG; and an external energy transmitter for wirelessly providing electrical energy to the energy storage device.

[0023] Further, the present invention may also be directed to one or more features according to the following sections. All features of these sections, but also all features of the entire specification, may be combined with one another.

1. A method for providing a therapy to a patient, said method comprising the steps of:

providing a waveform generating circuit for generating a waveform of a desired shape having an amplitude and a duration;
defining a scaling factor;
using said scaling factor for scaling the waveform generated by said waveform generating circuit, such that both the amplitude and the duration of the waveform is adjusted using said scaling factor; and
providing a stimulation pulse including at least a substantial portion that is based on said scaled waveform having shape resembling the desired shape of the waveform for stimulating a stimulation region of the patient.

2. The method according to section 1, wherein said portion of the stimulation pulse based on said scaled waveform is used to substantially cancel a charge

induced in the stimulation region by a different portion of the stimulation pulse.

3. The method according to section 1 or 2, wherein said scaled portion of the stimulation pulse is based on the waveform of the desired shape not scaled, or scaled using a different scaling factor. 5

4. The method according to one of the preceding sections, wherein said waveform is generated by retrieving stored waveform samples from a memory. 10

5. The method according to one of the preceding sections, where said waveform is generated using a mathematical function generated by a waveform function generator. 15

6. A method for providing a therapy to a patient, said method comprising the steps of: 20

generating a first waveform of a desired shape using a waveform generator;
providing a first portion of a stimulation pulse substantially resembling said first waveform, said stimulation pulse for stimulating a stimulation region of the patient; 25
defining a scaling factor;
using said scaling factor for generating a second waveform using the waveform generator, said second waveform being a scaled version of the first waveform; and 30
providing a second portion of the stimulation pulse substantially resembling said second waveform, said second portion of the stimulation pulse for stimulating the stimulation region of the patient. 35

7. The method according to section 6, wherein said second portion of the stimulation pulse substantially cancels a charge provided to the stimulation region by the first portion of the stimulation pulse. 40

8. The method according to one of the preceding sections, wherein said first waveform is generated by retrieving stored waveform samples from a memory. 45

9. The method according to one of the preceding sections, wherein said desired shape includes at least a portion of a shape other than a square wave, and further wherein said first waveform is generated using a mathematical function generated by a waveform function generator. 50

11. The method according to one of the preceding sections, wherein said second waveform is scaled in time based on the scaling factor. 55

12. The method according to one of the preceding sections, wherein said second waveform is scaled in both time and amplitude based on the scaling factor such that the total charge delivered during the first waveform is equal but inverse to the total charge delivered during the second waveform.

13. A method for providing a therapy to a patient, said method comprising the steps of:

determining a first waveform of a desired shape using a waveform generator, said desired shape including at least a portion of a shape other than a square wave;
defining a scaling factor;
using said scaling factor for generating a second waveform using the waveform generator, said second waveform being a scaled version the first waveform such that said second waveform is scaled in time and/or amplitude based on the scaling factor; and
providing a stimulation pulse including a portion substantially resembling said second waveform, said stimulation pulse for stimulating a stimulation region of the patient.

14. The method according to section 13, wherein both time and amplitude are scaled based on the scaling factor.

15. The method according to section 13 or 14, further comprising the step of providing a first portion of a stimulation pulse, substantially resembling said first waveform, for stimulating the stimulation region of the patient, wherein a second portion of the stimulation pulse is for substantially canceling a charge provided to the stimulation region during the first portion of the stimulation pulse.

16. A stimulation device for stimulating a stimulation region within a patient comprising:

a waveform generation circuit for generating a waveform part having a shape based on a desired waveform other than a square wave;
a time scaling circuit for input to said waveform generation circuit, wherein said waveform part generated by said waveform generation circuit resembles said desired waveform scaled in time based on a value of a scaling factor; and
a stimulation pulse generating circuit for generating a stimulation pulse including a portion based on said scaled waveform part. Preferably, said stimulation pulse is provided to a stimulation region of the patient.

17. The stimulation device according to section 16, further comprising an amplitude scaling circuit,

wherein at least a portion of said stimulation pulse generated by said stimulation pulse generating circuit is scaled in amplitude by said amplitude scaling circuit based on said scaling factor.

18. The device according to section 16 or 17, wherein said waveform generation circuit is comprised of a memory storing a plurality of samples of a desired waveform.

19. The device according to one of sections 16-18, wherein said stimulation device is further comprised of:

a register for storing a step size; and
an offset register for storing an offset value, wherein
at least a subset of said plurality of samples is retrieved from the memory based on both said step size and said offset value for generating said waveform part.

20. The device according to one of sections 16-19, wherein said waveform generation circuit is a circuit for generating a waveform based on a mathematical equation.

21. A stimulation device for stimulating a stimulation region within a patient comprising:

a waveform generation circuit for generating a first waveform and a second waveform;
a time scaling circuit for input to said waveform generation circuit;
a scaling circuit connected to said waveform generation circuit for scaling said second waveform based on said first waveform scaled in time by a scaling factor;
an amplitude scaling circuit for further scaling said second waveform in amplitude based on said scaling factor; and
a stimulation pulse generating circuit for generating a stimulation pulse including a portion based on said second waveform such that said portion of said stimulation pulse resembles said first waveform scaled both in time and in amplitude based on said scaling factor, and preferably for providing said stimulation pulse to a stimulation region of the patient.

22. The stimulation device according to section 21, wherein said stimulation pulse generating circuit also generates a portion of a stimulation pulse using said first waveform for providing to the stimulation region or another stimulation region of the patient.

23. The stimulation device according to section 21 or 22, wherein said stimulation pulse generating circuit

also generates a stimulation pulse using said first waveform for providing to the stimulation region of the patient, wherein charges delivered to the stimulation region by the stimulation pulse based on the first waveform and the second waveform substantially cancel each other.

24. The stimulation device according to one of sections 21-23, further comprising a passive charge recovery circuit for dissipating a residual charge at said stimulation region subsequent to providing the stimulation pulse.

25. The device according to one of sections 21-24, wherein said waveform generation circuit is comprised of a memory storing a plurality of samples of a desired waveform.

26. The device according to one of sections 21-25, wherein said stimulation device is further comprised of:

a register for storing a step size; and
an offset register for storing an offset value, wherein
at least a subset of said plurality of samples is retrieved from the memory based on both said step size and said offset value for generating said waveform part.

27. The device according to one of sections 21-26 wherein said waveform generation circuit is a circuit for generating a waveform based on a mathematical equation.

28. A stimulation device for stimulating a stimulation region within a patient comprising:

a first waveform generation circuit for generating a first waveform part based on a first waveform;
a second waveform generation circuit for generating a second waveform part based on a second waveform;
a scaling circuit for input to said first waveform generation circuit and said second waveform generation circuit;
a scaling register for storing, or an input for inputting, one or more variable scaling values for input to said scaling circuit, wherein said first waveform part generated by said first waveform generation circuit is based on said first waveform scaled based on a value one of said one or more scaling values and wherein said second waveform part generated by said second waveform generation circuit is based on said second waveform scaled based on a value of one of said one or more scaling values, such that said stimulation device is adapted such that different scaling

values can be used for respectively generating said first part and said second part; a stimulation pulse generating circuit for generating a stimulation pulse comprised of a first pulse phase generated from said first waveform part and a second pulse phase generated from said second waveform part, wherein said stimulation pulse is preferably provided to a stimulation region of the patient.

29. The stimulation device according to section 28, wherein said first pulse phase and said second pulse phase provided in series.

30. The stimulation according to one of sections 28-29, wherein said scaling circuit is a time scaling circuit for scaling waveforms in time.

31. The stimulation device according to one of sections 28-30, wherein said scaling circuit is an amplitude scaling circuit for scaling waveforms in amplitude.

32. The stimulation device according to section 31, wherein said amplitude is scaled by using a division operation.

33. The stimulation device according to one of sections 28-32, wherein said scaling circuit includes a time scaling circuit for scaling waveforms in time, and an amplitude scaling circuit for scaling waveforms in amplitude.

34. The device according to one of sections 28-33, wherein said first waveform generation circuit is comprised of a first memory storing a plurality of samples of a desired waveform, and wherein said stimulation device is further comprised of:

a register for storing a step size; and an offset register for storing an offset value, wherein at least a subset of said plurality of samples is retrieved from the memory based on both said step size and said offset value for generating said first waveform part.

35. The device according to one of sections 28-34, wherein said second waveform generation circuit is comprised of a second memory or another area of said first memory for storing a plurality of additional samples of another desired waveform, wherein at least a subset of said plurality of additional samples is retrieved from said second memory or said another area of said first memory based on both a step size and an offset for generating said second waveform part.

36. A stimulation device for stimulating a stimulation region within a patient comprising:

a first waveform generation circuit for generating a first waveform part based on a first waveform; a second waveform generation circuit for generating a second waveform part based on a second waveform; a time scaling circuit for input to said first waveform generation circuit and said second waveform generation circuit; a scaling register for storing, or an input for inputting, one or more variable scaling values for input to said time scaling circuit, wherein said first waveform part generated by said first waveform generation circuit is based on said first waveform scaled in time based on a value of one of said one or more scaling values and wherein said second waveform part generated by said second waveform generation circuit is based on said second waveform scaled in time based on the value of said one, or another one, of said one or more scaling values; an amplitude scaling circuit for inputting said one or more variable scaling values for further scaling in amplitude said first waveform part in amplitude based on said value of said one of said one or more scaling values, said amplitude scaling circuit also for inputting said value of said one, or said another one, of said one or more scaling values for further scaling in amplitude said second waveform part in amplitude based on said value of said one, or said another one, of said one or more scaling values; and a stimulation pulse generating circuit for generating a stimulation pulse comprised of a first pulse phase generated from said first waveform part and a second pulse phase generated from said second waveform part as scaled by said amplitude scaling circuit and said time scaling circuit, wherein said stimulation pulse is preferably provided to a stimulation region of the patient.

37. The stimulation device according to section 36, wherein a stimulation pulse is provided to said stimulation region based on said first waveform and said second waveform, such that the charge delivered to said stimulation region of the patient is substantially canceled by said waveforms.

38. The stimulation device according to section 36 or 37, further comprising a passive charge recovery circuit for dissipating a residual charge at said stimulation region subsequent to providing said stimulation pulse.

39. A stimulation device for stimulating a stimulation

region within a patient comprising:

a register for storing a step size;
 an offset register for storing an offset value;
 a first waveform generation circuit for generating
 a first waveform part based on a first waveform,
 said first waveform generation circuit comprising
 a first memory storing a plurality of samples of
 a desired waveform, wherein at least a subset
 of said plurality of samples is retrieved from the
 memory based on both said step size and said
 offset value for generating said first waveform
 part;
 a second waveform generation circuit for gener-
 ating a second waveform part based on a sec-
 ond waveform,
 a time scaling circuit for input to said first wave-
 form generation circuit and said second wave-
 form generation circuit,
 a scaling register for storing one or more variable
 scaling values for input to said time scaling cir-
 cuit, wherein said first waveform part generated
 by said first waveform generation circuit is based
 on said first waveform scaled in time based on
 a value of one of said one or more scaling values
 and wherein said second waveform part gener-
 ated by said second waveform generation circuit
 is based on said second waveform scaled in time
 based on the value of said one, or another one,
 of said one or more scaling values,
 an amplitude scaling circuit for inputting said one
 or more variable scaling values for further scal-
 ing said first waveform part in amplitude based
 on said value of said one of said one or more
 scaling values, said amplitude scaling circuit al-
 so for inputting said value of said one, or said
 another one, of said one or more scaling values
 for scaling said second waveform part in ampli-
 tude based on said value of said one, or said
 another one, of said one or more scaling values,
 and
 a stimulation pulse generating circuit for gener-
 ating a stimulation pulse comprised of a first
 pulse phase generated from said first waveform
 part and a second pulse phase generated from
 said second waveform part as scaled by said
 amplitude scaling circuit and said time scaling
 circuit, wherein
 said stimulation pulse may be provided to a stim-
 ulation region of the patient, and wherein
 a charge induced on said stimulation region of
 the patient by said first part of said stimulation
 pulse is substantially canceled by said second
 part of said stimulation pulse.

40. A system for stimulating a stimulation region of the spine within a patient comprising:

an implantable pulse generation device (IPG) adapted to be implanted in the patient, said IPG including:

a rechargeable battery for providing power to said IPG,
 a first waveform generation circuit for gener-
 ating a first waveform part,
 a second waveform generation circuit for gener-
 ating a second waveform part,
 a time scaling circuit for input to said first
 waveform generation circuit and said sec-
 ond waveform generation circuit,
 a scaling register for storing one or more
 variable scaling values for input to said time
 scaling circuit, wherein said first waveform
 part generated by said first waveform gen-
 eration circuit is scaled in time based on a
 value of one of said one or more scaling
 values and wherein said second waveform
 part generated by said second waveform
 generation circuit is scaled in time based on
 the value of said one, or another one, of said
 one or more scaling values,
 an amplitude scaling circuit for inputting
 said one or more variable scaling values for
 further scaling an amplitude said first wave-
 form part in amplitude based on said value
 of said one of said one or more scaling val-
 ues, said amplitude scaling circuit also for
 inputting said value of said one, or said an-
 other one, of said one or more scaling val-
 ues for further scaling an amplitude said
 second waveform part in amplitude based
 on said value of said one, or said another
 one, of said one or more scaling values, and
 a stimulation pulse generating circuit for
 generating a stimulation pulse comprised of
 a first pulse phase generated from said first
 waveform part and a second pulse phase
 generated from said second waveform part
 as scaled by said amplitude scaling circuit
 and said time scaling circuit;

an electrode connected to said IPG and adapted to be provided near the stimulation region for providing the stimulation pulse to the stimulation region;

an external device for wirelessly connecting to said IPG for controlling an operation of said IPG; and

an external energy transmitter for wirelessly providing electrical energy to said energy storage device.

41. The system of section 40, wherein said IPG further comprises a circuit for inserting a variable delay between said first pulse phase and said second

pulse phase, wherein said delay is controllable;

42. The stimulation device of section 40 or 41, wherein said first stimulation pulse phase is provided to said stimulation region based on said first waveform and said second stimulation pulse phase is provided to said stimulation region based on said second waveform, such that a charge delivered to said stimulation region of the patient is substantially canceled by said stimulation pulse phases.

43. The stimulation device according to one of sections 40-42, further comprising a passive charge recovery circuit for dissipating a residual charge at said stimulation region subsequent to providing said stimulation pulse.

44. A system for stimulating a stimulation region of the spine within a patient comprising:

an implantable pulse generation device (IPG) adapted to be implanted in the patient, said IPG including:

a rechargeable battery for providing power to said IPG,
 a register for storing a step size;
 an offset register for storing an offset value;
 a first waveform generation circuit for generating a first waveform part based on a first waveform, said first waveform generation circuit comprising a first memory storing a plurality of samples of a desired waveform, wherein at least a subset of said plurality of samples is retrieved from the memory based on both said step size and said offset value for generating said first waveform part;
 a second waveform generation circuit for generating a second waveform part based on a second waveform,
 a time scaling circuit for input to said first waveform generation circuit and said second waveform generation circuit,
 a scaling register for storing one or more variable scaling values for input to said time scaling circuit, wherein said first waveform part generated by said first waveform generation circuit is based on said first waveform scaled in time based on a value of one of said one or more scaling values and wherein said second waveform part generated by said second waveform generation circuit is based on said second waveform scaled in time based on the value of said one, or another one, of said one or more scaling values,
 an amplitude scaling circuit for inputting

said one or more variable scaling values for further scaling said first waveform part in amplitude based on said value of said one of said one or more scaling values, said amplitude scaling circuit also for inputting said value of said one, or said another one, of said one or more scaling values for scaling said second waveform part in amplitude based on said value of said one, or said another one, of said one or more scaling values, and

a stimulation pulse generating circuit for generating a stimulation pulse comprised of a first pulse phase generated from said first waveform part and a second pulse phase generated from said second waveform part as scaled by said amplitude scaling circuit and said time scaling circuit;

an electrode connected to said IPG and adapted to be provided near the stimulation region for providing the stimulation pulse to the stimulation region;

an external device for wirelessly connecting to said IPG for controlling an operation of said IPG; and

an external energy transmitter for wirelessly providing electrical energy to said energy storage device, wherein

said stimulation pulse is provided to said stimulation region based on said first waveform and said second waveform, such that a charge induced on said stimulation region of the patient by one portion of the stimulation pulse is substantially canceled by another portion of said stimulation pulse.

45. A stimulation device for stimulating a stimulation region within a patient comprising:

a waveform generation circuit for generating a waveform;
 a time scaling circuit for input to said waveform generation circuit for providing a programmable time scale to said waveform generation circuit;
 a scaling register for storing, or an input for inputting a programmable scaling value for input to said time scaling circuit, wherein said waveform generated by said first waveform generation circuit is scalable in time based said scaling value such that different values of said scaling value can be used to expand and/or compress said waveform in time; and
 a stimulation pulse generating circuit for generating a stimulation pulse comprised of said waveform, wherein said stimulation pulse is provided to a stimulation region of the patient.

[0024] Also provided are additional embodiments of the invention, some, but not all of which, are described hereinbelow in more detail.

BRIEF DESCRIPTION OF THE DRAWINGS

[0025] The features and advantages of the examples of the present invention described herein will become apparent to those skilled in the art to which the present invention relates upon reading the following description, with reference to the accompanying drawings, in which:

Figure 1 is a block diagram showing a high-level structure of an example embodiment;

Figure 2 is a block diagram showing a more detailed structure of a possible construction of the example embodiment used as an implantable pulse generator;

Figure 3 is a block diagram showing an example system used as an external pulse generator;

Figure 4 is a schematic of one example implementation of part of a pulse generator circuit and supporting components in an example system;

Figure 5 is a schematic of another example implementation of part of a pulse generator circuit and supporting components in another example system;

Figure 6 is a schematic of an example implementation of a waveform generation circuit and supporting components in an example system;

Figure 7 is an example output waveform construction result of an example waveform generation circuit;

Figure 8 is another example output waveform construction result of an example waveform generation circuit;

Figure 9 is another example output waveform construction result of the example waveform generation circuit;

Figure 10 is another example output waveform construction result of the example waveform generation circuit;

Figure 11 is a circuit diagram of an example amplitude dividing circuit;

Figure 12 is a circuit diagram of an example amplitude multiplier circuit;

Figure 13 is a diagram illustrating time scaling;

Figure 14 is an example output waveform construction result of the example waveform generation circuit using scaling features;

Figure 15 is an example complex output waveform construction result of the example waveform generation circuit;

Figure 16 is a diagram illustrating an example implantable pulse generation device;

Figure 17 is a diagram illustrating a medical application of some of the example devices;

Figure 18 is another example complex output waveform construction result of the example waveform generation circuit; and

Figure 19 is a diagram illustrating a two-phase stimulation pulse with charge balancing.

DETAILED DESCRIPTION OF THE EXAMPLE EMBODIMENTS

[0026] Disclosed is a device, or system of devices cooperating with each other, for providing a flexible and highly adaptable stimulation waveform, such as might be used for medical purposes such as spinal stimulation (such as for pain reduction, for example). This system includes a neurostimulation pulse generator that uses digital waveform synthesis techniques to generate stimulation pulses with programmable waveshapes.

[0027] Figure 1 is a generic diagram of an example stimulation system. Such a system includes a Pulse Generator (PG) component **1**, a set of two or more electrodes (which may include the PG's enclosure) **2**, external programming and user controlling devices **3**, **4**, and a connection to an external power supply **5**. The Pulse Generator **1** is typically generally comprised of an internal power supply **6**, a controller **7**, pulse generation electronics **8**, and a protection circuit **9**.

[0028] Figure 2 shows a more specific example system where most of the components for generating the stimulation waveform are implanted in a patient for providing medical therapy by utilizing an implantable PG (IPG) **101** that could utilize the disclosed features. This system is comprised of the IPG **101** that includes a stimulation ASIC **108** and protection components **109**. The IPG **101** is further comprised of a microcontroller **107** for controlling the functions of the IPG via the control bus **12**, and a power ASIC **106** for powering the components via a power bus **11**. Because this implantable system avoids the need for any components or wires that exit the body of the patient **120**, the IPG **101** includes an RF transceiver (transmitter/receiver) **14** with an antenna **16** for allowing the IPG to communicate with devices external to the patient's body, such as a clinician programmer **103** and user controller(s) **104**, which also have antennas **18** and

19, respectively, to communicate with the transceiver 14 via a wireless protocol. Furthermore, the IPG also includes an embedded power supply including a power ASIC 106 for conditioning the device power, a (long life) rechargeable battery 13, and a secondary inductive coil 15 (or some other means) for receiving power from an external source outside the body of the patient 120. A corresponding external power supply 105 would typically require a corresponding primary charging coil 17 to complete the power connection to the embedded power supply to charge the battery 13. The IPG 101 is connected to one or more electrode arrays 102 including a plurality of electrodes via a header (not shown) connected via feedthroughs (not shown) to the protection components 109. The IPG 101 is provided in a hermetically sealed case made of, or coated by, human implantable compatible materials, and requiring only that the contacts attached to the lead body of the electrode array(s) be electrically connectable to the IPG through the header. The electrode leads and electrodes themselves, along with portions of the header that are exposed to the patient, must all be made of, or coated by, materials that are compatible with implantation in the human body.

[0029] Figure 3 shows an example system that can be provided with similar capabilities, but without requiring an implantable PG. Instead, the system of Figure 3 uses an external PG (EPG) 201 that is provided outside of the body of the patient 220. The EPG 201 can be comprised of similar components as that of the IPG 101, except that it need not be made of implantable materials. Instead, the EPG 201 is connected to the electrode array 202 via a percutaneous lead 22 that must exit the body. The lead 22 is then connected to the EPG 201 via a connector 23. The EPG 201 can be directly connected to the corresponding clinician programmer 203 and user controller(s) 204, or a wireless connection similar to that of the IPG 101 could also be used. The EPG can be powered via an internal battery or connected to an external power source, as desired.

[0030] One end of the percutaneous lead 22 is typically surgically implanted in or near the tissue to be stimulated. The other end is brought through a wound in the skin, and can be connected to the EPG when electrical stimulation is needed. The implanted end of the Percutaneous Lead typically includes electrode surfaces similar to those on the implanted lead(s). The EPG may be designed to be mobile, such that it can be carried by the patient, such as by mounting on a belt. In such a case, a battery would prove useful to increase mobility.

[0031] An Implantable Pulse Generator is surgically placed inside the body along with one or more implanted leads (as shown by example in Fig. 2 and discussed above). One end of each implanted lead (often called the "proximal" end) is electrically and physically connected to the IPG via the header, while the other end (often called the "distal" end) is placed in or near the tissue to be electrically stimulated. The distal end includes one or more exposed electrode surfaces, electrically connected to the

IPG, that transfer the electrical stimulation pulses to the tissue.

[0032] Outside the body, the external power supply is used to transfer power to the IPG, either for charging a battery or capacitor inside the IPG or providing direct power for the IPG's electronics. This is done via the charging coil, which is placed over or near the area where the IPG is implanted, and forms the primary coil of a transformer with the secondary coil inside the IPG, although a separate coil electrically connected to the IPG but somewhat remote from the IPG could be used. The two coils, coupled inductively, provide power transfer through the skin. The external power supply itself can be powered by a battery to allow for patient mobility, or it may also draw power from a mains power source.

[0033] Also outside the body, the Clinician Programmer is used to program the IPG, configuring it for the particular patient and defining the electrical stimulation therapy to be delivered to the target tissue. The clinician programmer is typically highly functional, allowing IPG programs to be substantially modified by updating programs and/or data stored in memory in the IPG, to allow great flexibility in programming the IPG.

[0034] The User Controller is used to control the operation of the IPG in a manner limited by its programming. Thus, the user controller is typically less functional than the clinician programmer. The user controller can alter one or more parameters of the electrical stimulation therapy to adjust the therapy to the liking of the patient, depending on the IPG's program and configuration as set with the Clinician Programmer.

[0035] The operation of an EPG (as shown by example in Fig. 3 and discussed above) is similar, with the exception that there is typically no need for inductive transfer of power as direct cable connections can be used to recharge any battery, for example, and the electrode leads must pass through the body to connect to the EPG.

[0036] Pulse generators (PGs), whether implanted pulse generators (IPGs) or external pulse generators (EPGs), have, to date, used waveforms that are generally rectangular for the stimulation phase of the waveform and either rectangular or exponential for the charge recovery phase. However, waveform shapes other than these basic choices may be effective in selecting which nerve fibers are activated by an EPG or IPG. For example, one waveform shape may be preferable for selecting large-diameter fibers, while another shape may be preferable for small-diameter fibers. Because the fiber diameter in a given nerve is related to the function of that fiber, improved selectivity of one nerve fiber over another can improve the likelihood of achieving the desired results of neural stimulation, such as pain relief, with less occurrence of undesirable side-effects such as pain or muscle spasms.

[0037] For safety reasons, most PGs use charge-balanced waveforms. A charge-balanced waveform is one in which the effective DC current is zero or nearly zero. For example, various national and international stand-

ards limit the net DC current to 10 μ A (AAMI/ANSI NS-14, incorporated by reference), or 0.1 μ A (ISO 45502-2-1, incorporated by reference), depending on the intended use of the PG. A charge-balanced pulse is made up of at least two phases of stimulation current, each phase having a single polarity, such that the integral of the current over time of all the phases, representing accumulated electrical charge, equals zero. Typically, there are two phases, the first phase being intended to create the desired effect in the tissue, and the second phase, of opposite polarity, used to bring the waveform into charge balance.

[0038] To prevent tissue damage and/or electrode corrosion, charge delivered on one electrode is usually recovered on the same electrode, because any residual charge can change the chemical composition of the tissue near the electrode. It doesn't take much imbalance to get significant electrode corrosion, which would be particularly problematic in implanted devices.

[0039] Typically, charge-balancing is done with the aid of DC blocking capacitors that are provided in the conditioning/protection circuit, which serve the function of integrating the charge transferred in the stimulation phases up to a given time. By bringing the voltage on the capacitor to its original value during the charge recovery phase of the pulse, the integral of the current is brought to zero, assuring charge balance. These DC blocking capacitors are bulky, which runs counter to the goal of making a PG as small as possible (in particular, for an IPG). DC blocking capacitors have other drawbacks as well, as in some designs, the DC leakage of the capacitors results in a DC current through the tissue, the opposite of the intended reason for including the capacitors.

[0040] Thus, provisions for charge balancing without requiring DC blocking capacitors are discussed herein as well. This feature permits the construction of smaller PGs and eliminates the risk of DC leakage through the capacitors.

[0041] Although a rudimentary device allowing waveforms stored in memory is discussed in U.S. Pat. No. 7,715,912, which is incorporated herein by reference, such an approach as disclosed in that reference has a number of shortcomings that can be overcome by the approach disclosed herein

[0042] The waveform generation core is the primary component that is modified by this disclosure, and can be comprised of waveform generation circuitry including any or all of the following components: one or more memories to store waveshape templates, a phase accumulator, a step-size register, one or more waveshape calculation logic circuits, and a clock source. Which of these devices are utilized depends on the desired implementation, any of which may be omitted where not needed, and any of which can be replicated as desired. An example operation of a device comprising at least one of all of these components can be generally described, along with at least one medical application.

[0043] One of the most flexible approaches disclosed

herein is the utilization of a waveform shape stored in memory and used as a template for generating shaped stimulation pulses. These templates can be programmed via the clinician programmer, which may have a selection of available shape templates for the clinician to choose from, or the templates may be programmed into the device during manufacture. The memory is structured such that each memory location represents a time step, and the value stored in each memory location represents the amplitude at that time step. Basically, the waveform is generated by addressing a memory to retrieve some number of waveform samples stored in a memory for any of the desired waveform shapes, in the following manner: A waveform is to be constructed using one or more phases for creating portions of the stimulation pulse waveform, including both the stimulation phase and the charge recovery phase. At the start of each phase of the stimulation pulse, a phase accumulator is set to a programmed offset value as a start address used to retrieve a waveform sample value from memory. This offset value sets the sample, from the waveshape template stored in memory, that will start the pulse.

[0044] As the phase continues, at each sample time the phase accumulator is incremented by a step size stored in a step-size register to calculate the next address value. This next address value is used to select an additional sample from the stored waveshape template, and the process is iterated again to retrieve additional amplitude samples from the waveshape template that make up the current phase of the pulse. The step size in the example is a fixed-point number that can have both integer and fractional components, if desired. By permitting fractional increments in the step size, it is possible to generate waveshape durations of any integer length, not just those that divide evenly into the number of samples in the waveshape template. Also, if the fixed-point step size is less than one, the pulse width will be made longer than the number of samples in the template; samples can then be automatically be duplicated, as necessary, to extend the pulse. This allows the memory size required for reasonable fidelity to be optimized for the typical pulse width used by the therapy, while still allowing very short or very long pulse widths to be possible.

[0045] The output from the phase accumulator is used as an index into a programmably selected waveform memory as described above, or it can be used to index a shape-generating logic circuit, depending on the current implementation and/or desired output waveform. A waveform memory would be used to look up a waveform sample that was stored in advance at the indexed location of the memory and output the desired waveform shape, which allows a great flexibility in the shapes of waveforms. A single register, in contrast, which outputs the same (constant) programmed value regardless of the index could be used to generate rectangular waveforms. A shape logic circuit, in contrast, computes a fixed mathematical function based on the input index (or based some other input or internal function) and outputs the

result as a waveform shape, which may be particularly useful for situations where waveforms that are provided by simple mathematical equations are desired (such as exponentials, ramps, sine waves, etc.).

[0046] The output from the waveform memory or waveform calculation logic (whichever was chosen) then drives a digital-to-analog converter (DAC), called a "waveform DAC", which creates a reference current (or voltage). This reference current (or voltage) is in turn used as the input of several multiplying digital-to-analog converters, called "amplitude multipliers". The data input of the converters comes from programmable amplitude registers for that phase of the stimulation waveform. The result of the multiplication is a current (though a voltage could also be generated), positive or negative (or equivalently, sink or source), which is output to the electrodes in contact with body tissue. By adjusting the values in the amplitude registers, the amount and polarity of current (or voltage) output to each electrode can be adjusted, thus shaping the electric field generated by the phase. Although the examples provided herein focus on the use of a single waveform generation circuit that can drive a plurality of electrodes by driving the output into a number of amplitude-multiplying DACs, replication of the waveform generation circuit can be used to provide additional flexibility to the output, if desired, such that any given waveform generation circuit may independently drive a subset of one or more electrodes. In such a situation, the circuits could be modified to share memories of waveform shape templates to reduce unnecessary replication.

[0047] The stimulation waveform is divided into a series of pulses, each of which is divided into a series of unipolar phases. Each phase has a programmable repetition count (to repeat the phase a number of times, if desired) and a programmable delay before the next phase. Circuitry in the stimulator automatically sequences the phases and their repetitions, and hence, the pulses that are made up from the phases. This allows a single stimulation pulse to have more than two phases defined for it. This structure allows for "n-lets", or pulses that have repeated stimulation phases, as well as one or more "pre-pulses", where one or more additional phases are added prior to the stimulation phase to provide pre-polarization.

[0048] Programmable dividers for amplitude (each called a "current divider") and time (each called a "clock divider") can be used to scale a waveform simultaneously in time and amplitude in such a way that permits charge balancing in cases where the same shape is used for both the stimulus and charge recovery phases. The current divider and clock divider registers could be programmed appropriately to provide charge balancing.

[0049] The pulse generator typically includes amplitude multipliers for every channel on the device.

PULSE GENERATOR ARCHITECTURE

[0050] The improvements discussed herein can be used with an Implantable Pulse Generator (IPG) as

shown in Fig. 2 (discussed above) or an External Pulse Generator (EPG) as shown in Fig. 3 (also discussed above). The description below will focus on example implementations using the IPG based system, but an EPG system could be easily adapted in a similar manner.

[0051] As described above, a block diagram of the internal functions of an example IPG system is shown in Figure 2.

[0052] The microcontroller **107**, which is implemented using a programmable controller as is known in the art, controls at least the embedded components of the system, stores stimulation program information, and performs other control and management functions, some of which are disclosed herein. The RF Transceiver **14** implements bidirectional digital communications at radio frequencies in the IPG with external devices as desired. The attached antenna **16** is used to transmit and receive these radio signals, by which the IPG communicates with such components as the User Controller **104**, Clinician Programmer **103**, and/or External Power source **105**, among other possible devices.

[0053] The Power ASIC **106** is connected to the Battery **13**, which provides electrical power to the powered internal components. The Power ASIC **106** is also connected to the secondary coil **15**, by which it receives electrical energy inductively coupled through the patient's body from the primary charging coil **17**. The Battery **13** may be either primary or rechargeable, or may be omitted in lieu of some other power source. If the battery **13** is a primary battery, the external power unit **105**, the charging coil **17** and secondary coil **15** may be omitted. Typically, a secondary battery that is rechargeable is desirable to lengthen the useful life of the battery and avoid additional surgeries to replace the pulse generator or its components. Other power supplies in the future may prove useful to replace the battery implementation.

[0054] The Stimulation ASIC **108** includes the stimulation pulse waveform generation circuitry. This ASIC **108** is controlled by the microcontroller **107** and has power supplied by the Battery and/or Secondary Coil via the Power ASIC.

[0055] The Protection Components **109**, if used, may include DC blocking capacitors and electrical transient suppression components, among other components. Together, these components protect the tissue from unwanted electrical signals and DC currents, and protect the PG from external electrical events such as electrostatic discharge, defibrillation, or electrocautery. In some embodiments, particularly those discussed in a related application, some of these components might be reduced (in size and/or quantity) or eliminated through the use of active charge balancing techniques. Thus, for at least some embodiments (in particular embodiments exclusively using active charge balancing), the waveform generation core may consist of only the stimulation ASIC, along with any supporting components, if necessary.

WAVEFORM GENERATION CORE

[0056] Figures 4 and 5 show generalized embodiments of potential waveform generation core designs for use in providing the improved waveform generation capabilities. In general, power and control connections are not shown in these figures, as their use is within the skill of the art based on this discussion.

[0057] Figure 4 shows a simplified block diagram of a generic waveform generation core of a stimulator system incorporating the waveform generation improvements. A reference generator "Iref" **41** that is a reference current source sets the over-all amplitude scaling of the system. A clock signal CLK **42**, sets the over-all time scaling of the system, and the Clock Divider **43** scales the clock by a configurable division factor. The Waveform Generator **40**, representing the core of the waveform generation function, outputs the shape of each phase of the pulse, creating the "normalized waveform" that basically forms the stimulation waveform into its desired shape. The Current Divider **44** scales the output of the Waveform Generator **40** by performing a division operation, creating the "scaled waveform". Finally, the Amplitude Multipliers **45a~45n** (typically one per channel) multiply the scaled waveform by a configurable amplitude and polarity for each individual channel CH1~CHn in the electrode array **49**. The peak amplitude and polarity for each channel do not vary during a given phase of a pulse, but do change from one phase to the next. Each Amplitude Multiplier **45** has an independent current output, each of which can be used to drive a subset of one or more of the stimulation electrodes. Furthermore, multiple current outputs can be used to drive a single electrode.

[0058] Figure 5 shows a simplified block diagram of a stimulator similar to that of Fig. 4 with the addition of DC blocking capacitors **47a~47n** and passive-recovery switches **46a~46n**. The addition of the blocking capacitors and passive-recovery switches allows charge balancing to be achieved in a passive manner by selectively closing the switches and connecting the capacitors to a common node. Thus, the embodiment of Fig. 5 would be more likely utilized where an active charge balance function is either not utilized, or not sufficient to completely balance the charges produced by the device, whereas the embodiment of Fig. 4 could be utilized where an effective charge balancing procedure is used.

[0059] Although not shown, the waveform generation circuitry could be replicated and provided with a multiplexor or set of switches connected to the inputs of the amplitude-multiplying DACs in order to allow different waveforms to drive various subsets of the electrodes. However, in the example, one waveform generation circuit is provided, and deemed satisfactory for many purposes.

WAVEFORM GENERATOR

[0060] The internal structure of an example embodi-

ment of the Waveform Generator **40** is shown in Figure 6. Again, the power connections are not shown, and only some of the control inputs most applicable to this discussion are shown in this figure.

[0061] Generally, this example waveform generator is comprised of, for example, a 24 bit input bus **601** for inputting a desired step size. A summer **602** is used to increment an address value based on the step size as the device iterates over each phase. An offset register or input **613** can be used to correct for waveform distortions that may occur for certain step sizes by being preloaded in the preload, as described below. A digital preload multiplexer **604** is used to switch between the offset at the start of the phase or the sum value to continue the phase.

[0062] The output of the preload multiplexer **604** is carried by the address bus **612** and contains the address value that is input into the delay **603** for a step delay for input into the summer **602** to increment the address by one step size. For the example embodiment, only the highest 8 bits of the address are input into the waveform generating circuit **600**. Other embodiments might use the entire address, however, or may also use more or fewer bits depending on the shape fidelity required for the therapeutic application.

[0063] The waveform generating circuit **600** outputs digital values representing the desired amplitude values at each time step of the waveform, and is comprised of those shape components that will generate the desired waveform shapes. Such shape components can include one or more RECT registers **607** which generate constant values regardless of input address for generating square wave pulses. Such shape components can also include one or more shape logic circuits **605a, 605b...** for generating waveforms based on mathematical functions, for example. Furthermore, the waveform generating circuit **600** can also be comprised of one or more memory circuits **606a, 606b...** that contain values representing programmed shape templates of desired waveforms.

[0064] A shape multiplexor **608** is used for choosing which shape component output is desired, based on a shape control input from the microcontroller (not shown), for example. The shape multiplexor **608** output **614** is connected to a carry multiplexor **609** that is used to zero the value at the start/end of the phase (when the summer overflows, for example). A Digital to Analog converter **610** converts the 8 bit shape data value into an analog value **611** of a current or, in some embodiments, a voltage, which is then connected to dividers and/or multipliers, as desired, to scale the shape into the desired amplitude.

[0065] Example operations of the example Waveform Generator described above can now be provided. In the first cycle of waveform generation in this example, the preload input of the preload multiplexer **604** has a value of "1". This causes the initial 24-bit output on the address bus **612** to be the 24-bit value OFFSET:\$00:\$00. That is

to say, it is a 24-bit value with an OFFSET value in the most significant eight bits, and the least significant sixteen bits all zero. In subsequent cycles the preload input to the multiplexer **604** is "0", and as a result, the 24-bit digital word "STEP" input **601** is added in the summer **602** (Σ) to the output of the unit delay **603** (z^{-1}) block, making a new 24-bit sum and one bit of carry. Tracing the path of the sum, one can see that it then becomes the input to the unit delay **603** (z^{-1}) block. Thus, with each clock cycle, the sum on the address bus **612** increases by the amount "STEP".

[0066] In the Example shown in Fig. 6, the most significant eight bits of the sum are used as the address into two memories, Memory 1 **606a** and Memory 2 **606b**, which may be any kind of digital memory such as RAM, ROM, EEPROM, Flash, or other types. The memories **606a** and **606b** each store a different wave shape template of a desired waveform to be generated. The address indexes the desired entry of the template for the particular clock cycle. Note that the address does not necessarily increment by one in every clock cycle. Depending on the value of STEP, it could also increment by less than one, resulting in multiple samples of a given entry in the template being used, or it could increment by more than one, resulting in only some, but not all, samples being used. Thus, an output waveform of arbitrary duration is synthesized from a wave shape template of fixed duration.

[0067] In the special case of rectangular waveforms, every element of the memory would be set to the same value. Thus, to avoid this inefficient use of memory space, the device can provide a number of rectangle registers, numbered RECT1-RECTn. In the Example of Fig. 6, four such RECT1-RECT4 registers **607** are used. Since rectangular waveforms have the same amplitude value for all addresses, it is not necessary to actually address these registers.

[0068] Similarly, it is possible to use digital logic circuits in place of a memory to generate useful waveforms. Two such logic circuits are shown in Figure 6 as blocks Shape Logic 1 **605a** and Shape Logic 2 **605b**. For example, a rising ramp waveform may be generated by connecting the top 8 bits of the sum directly to one of the multiplexer **608** inputs (in lieu of a memory), or a falling ramp may be generated by connecting the logical inverses (using a NOT operation) of the top 8 bits to the multiplexer input. Other variations are possible, such as providing exponential generators, sine wave generators, parabolic generators, etc. Such circuits might utilize the address inputs as part of the mathematical function or not, depending on the desired application.

[0069] The outputs of the memories **606a**, **606b**, rectangle registers **607**, and shape logic circuits **605a**, **605b** pass to the shape multiplexer **608**, which is controlled by the SHAPE input. This input is configured to select the desired waveform for a given phase, and is typically held constant for the entire phase. By setting SHAPE to the binary code 0111, for example, the waveform generated will use the template contained in Memory 2 **606b**. This

embodiment shows a data bus width of 8 bits as the output of the shape multiplexer, though more or fewer bits may be used to achieve the shape fidelity required for the therapeutic application.

[0070] The output of the shape multiplexer **608** passes into the carry multiplexer **609**, which is controlled by the carry output from the sum (Σ) block **602**. The carry multiplexer **609** sets the output of the waveform generator to zero when the sum overflows its 24 bits, for example.

[0071] Finally, the output of the carry multiplexer **609** drives a digital-to-analog converter **610** (DAC), which emits the normalized waveform output **611** from the Waveform Generator.

[0072] It can be seen that with each clock cycle, the sum, and hence the address, is incremented by the amount "STEP". Hence, "STEP" is called the "step size" and sets the rate at which elements of the wave shape template are used to create the waveform. It also implicitly sets the pulse width, since after enough steps of that size, the sum operation will generate a carry, which signals that the waveform generation is complete for the current phase.

[0073] The waveform generator constructs stimulation pulses via control from a microcontroller and/or state machine (e.g., a sequencer) that programs the desired shape, step size, and offset required for each phase of the pulse. The microcontroller and/or state machine also control the delays between pulse phases and provide the clock source to the waveform generator.

[0074] When memory devices are to be used for waveform generation using stored shape templates, it is often desirable to ensure that a particular point in the template is reached, such as guaranteeing that the peak point of a sine wave is emitted, for example. If the sum were to always start at zero, this may not be possible for some step sizes on some shape samples as the peak could be bypassed in some of those cases. By configuring the OFFSET input appropriately, one can ensure that any selected single sample in the template waveform will be emitted in the synthesized waveform by shifting the chosen samples of the waveform. Thus, depending on the type of waveform, or the scaling of a particular waveform, or both, an appropriate OFFSET value is calculated by the microcontroller for each phase to ensure that the desired particular point in each phase is provided in the output waveform.

[0075] As a possible example of the operation of the example waveform generator of Fig. 6, consider the generation of a six-sample half-sine-wave pulse. Assume the waveform memory is configured with a template waveform of a half sine wave pulse, a portion of the data for an example sampled waveform which is shown in TABLE 1. Further suppose the STEP is set to \$2AAAAB and the OFFSET is set to \$00. When the waveform generator is started, the phase accumulator will take the values, in successive cycles, \$000000, \$2AAAAB, \$555556, \$800001, \$AAAAAC, and \$D55557 before the sum overflows 24 bits and the waveform stops. The top

eight bits of these values are taken to compute the sequence \$00, \$2A, \$55, \$80, \$AA, \$D5, which becomes the addresses into the shape memory. The memory then reads out the values \$02, \$7F, \$DD, \$FF, \$DD, \$7F. Figure 7 shows these values as the bars, demonstrating the example waveform, while the dashed line illustrates the continuous-time half-sine pulse that these data points approximate. Although the data points are numerically correct, in that they do lie on the sine waveform, there is an asymmetry posed by the first chosen sample amplitude being \$02 without a corresponding sample of \$02 at the finish, thereby skewing the sine wave to the right. Thus, the overall shape of the pulse might not have the desired fidelity to a sine wave.

TABLE 1

Address	Data
00	02
01	05
02	08
03	0B
...	...
15	43
...	...
2A	7F
...	...
3F	B3
...	...
55	DD
...	...
6A	F6
...	...
80	FF
...	...
95	F6
...	...
AA	DD
...	...
BF	B5
...	...
D5	7F
...	...
EA	43
...	...
FF	02

[0076] This asymmetry can be corrected by using an appropriate OFFSET input. Again consider the generation of a six-step half-sine-wave pulse, with the waveform memory configured with the data shown in TABLE 1 and the STEP set to \$2AAAAB. This time, however, suppose the OFFSET is set to \$15. Now, when the waveform generator is started, the phase accumulator will take the values, in successive cycles, \$150000, \$3FAAAB, \$6A5556, \$950001, \$BFAAAC, and \$EA5557, which will result in the sequence of truncated addresses \$15, \$3F, \$6A, \$95, \$BF, \$EA. For these addresses, the shape memory returns the data sequence \$43, \$B3, \$F6, \$F6, \$B5, \$43. Figure 8 shows these data points as bars, with the continuous-time half sine wave pulse approximated by these pulses drawn as a dashed line. It can easily be seen that the data points both fit the sine wave curve well and have good symmetry. Thus, the OFFSET input can be used as illustrated to adjust the shape of the output waveform.

[0077] As a second example, consider the creation of an eight-sample rising exponential pulse. The data loaded into the memory for an example of such a sampled waveform are shown in part in TABLE 2. The STEP input is set to \$200000 and the OFFSET to \$00. The phase accumulator values are the sequence \$000000, \$200000, \$400000, \$600000, \$800000, \$A00000, \$C00000, \$E00000, and the addresses are \$00, \$20, \$40, \$60, \$80, \$A0, \$C0, \$E0. The resulting data sequence is \$01, \$02, \$04, \$08, \$10, \$20, \$41, \$82. These data are plotted as the bars in Figure 9, with the continuous-time exponential pulse these points approximate drawn as a dashed line. Although the data fit the ideal exponential pulse, they never reach the maximum amplitude of \$FF, which may be considered undesirable. In this situation, an OFFSET may be desirable.

TABLE 2

Address	Data
00	01
01	01
02	01
03	01
...	...
1F	02
20	02
...	...
...	...
3F	04
40	04
...	...
7F	10

(continued)

Address	Data
80	10
...	...
9F	20
A0	20
...	...
BF	3F
C0	41
...	...
DF	7F
E0	82
...	...
FF	FF

[0078] Accordingly, the exponential pulse can be configured to reach its peak value by setting the OFFSET input to \$1F. Now, the phase accumulator values are \$1F0000, \$3F0000, \$5F0000, \$7F0000, \$9F0000, \$BF0000, \$DF0000, \$FF0000, and the resulting addresses are \$1F, \$3F, \$5F, \$7F, \$9F, \$BF, \$DF, \$FF. The resulting data sequence is \$02, \$04, \$08, \$10, \$20, \$3F, \$7F, \$FF. These data are plotted as the bars in Figure 10, with the continuous-time exponential they approximate plotted as a dashed line. It can be seen that the points fit the continuous-time exponential well, and they reach the maximum amplitude. Thus, the OFFSET input provides sufficient control to ensure that a particular sample in the template waveform—in this case the last and peak sample—is reached when the waveform is generated.

[0079] Although both of the previous examples were of waveforms shorter than the template waveform, the waveform generator can also be used to create waveforms that are longer than the template waveform. Consider what happens if the STEP input is \$00418A and the OFFSET is \$00. The phase accumulator values are \$000000, \$00418A, \$008314, \$00C49E, \$010628, \$0147B2, ..., \$FEFCE8, \$FF3E72, \$FF7FFC, \$FFC186. With this STEP size, the waveform generator will make 1000 steps before the accumulator overflows 24 bits and waveform generation stops. These phase accumulator values result in the sequence of addresses \$00, \$00, \$00, \$00, \$01, \$01, ... \$FE, \$FF, \$FF, \$FF. It can be seen that when the STEP input is sufficiently small (less than \$010000 in this example), the waveform generator will repeat samples from the template waveform to create a pulse of the desired width by stretching the waveform.

[0080] It is worth noting that there are trivial variations on this design that are basically equivalent. For example, the memories could be combined into a single larger

memory, using one or more additional address lines to select between multiple wave shape templates. Similarly, enable inputs to the memories, rectangle registers, and/or shape logic could achieve a selection function equivalent to part or all of the shape multiplexer. Thus, there are a number of variations that can be used to implement the features of the waveform generator using different alternatives.

[0081] There are also several ways for the waveform generation circuitry components to be realized in hardware. First, it is possible to implement all of this circuitry in a single ASIC, either combined on-chip with the microcontroller or separate from it. Second, it is possible to combine some elements of this circuit on an ASIC with various separate components, for example by building most of the waveform generator in the ASIC and interfacing it to separate memories that are not part of the ASIC. Finally, it is also possible to build the waveform generator using discrete components.

[0082] Depending on the complexity of the waveforms to be generated and the therapeutic needs of the application, there are many ways to structure the architecture to achieve the features described above. A low-power microcontroller with dedicated programming stored in ROM could be utilized. Or, rather than using a low-power microcontroller, a device such as a more powerful central processing unit or a digital signal processor with appropriate programming stored in a computer readable medium, such as a memory device, could be used to directly synthesize the waveforms. In addition, field-programmable gate arrays could be programmed as a control source, state machine, and/or waveform generator. In this embodiment the preferred memory type for waveform template storage is RAM, though it could be equally effective to use flash memory, EEPROM, or some other form of ROM memory as is known in the art.

CURRENT DIVIDER FOR AMPLITUDE SCALING

[0083] In an example embodiment, the output from the waveform generator is provided to a Current Divider to help provide relatively precise control over the normalized waveform amplitude. The Current Divider performs a division operation for scaling the waveform. As an example, such a scaling factor can scale the waveform by a division factor ranging from 1/1, 1/2, 1/3, and so on to 1/16.

[0084] With a current output from the example waveform generator described above, an example current divider can be implemented as shown in Figure 11. Note that in Figure 11, the notation "M=n" is used, where n is some number that indicates that the corresponding FET is replicated n times. Each of the n copies of that FET have the same gate, drain, and source connection shown in the diagram.

[0085] The circuit in Figure 11 adapts current mirror techniques to perform current division on the normalized waveform. In the example, a digital 4-bit divisor word en-

ters on the D bus **32**, and the analog waveform to be divided enters on the I wire **31**. To describe its operation, it is first assumed that all of the FETs in the top row (**Q7-Q12**) are functioning as switches and all are initially turned "on". A portion of the waveform current coming in the I input **31** passes through FET **Q7** and then FET **Q1**. FET **Q1**, having its gate tied to its drain, sets the gate voltage for all of the rest of the bottom-row FETs (**Q2-Q6**) to the exact value that is needed for it to carry the current flowing through it. Thus, each individual FET in the bottom row is biased to carry the same current value. However, many of the FETs are replicated according to the M factor—for those FETs, each replica is biased to carry that same current. Thus, if all four of **Q2-Q5** are carrying current, they will carry a total of 15 ($8+4+2+1=15$) times the current through **Q1**, and the current through **Q1** will be $1/16$ of the current through the I input.

[0086] Now, consider the function of the D input **32**, which is a 4-bit value controlling **Q8-Q11** as switches. When D has the binary value 0000, all four switches (**Q8-Q11**) are turned off, and the full current of the I input **31** (which is based on the output of the DAC in the Waveform Generator) will flow through **Q1**. When D has the binary value 0001, **Q11** will be turned on, so half the current from I will flow through **Q1** and half will flow through **Q5**. When D has the binary value 0100, **Q9** will be turned on, enabling the corresponding $M=4$ FET (**Q3**). The result is that $1/5$ of the input current I will flow through the **Q1** and $4/5$ will flow through **Q3**. Thus, the binary value of the D input acts as a divisor, controlling how much of the input current I flows through **Q1**.

[0087] The output from the current divider is created by **Q6**. Its gate voltage is set by **Q1**, causing the current through it to be the same as that flowing through **Q1**. Thus, as the D and I inputs are varied, the current sunk at the output is equal to the current sunk by the I input, divided by $(D+1)$, thereby providing a current sink **33** that is a value of $I/(D+1)$.

[0088] **Q7** and **Q12** are configured as switches that are permanently turned on. Their purpose is to match the electrical environment of **Q1** and **Q6** to that of **Q2-Q5**, so that all of the bottom-row FETs see similar voltage, resistance, and capacitance in their connected components. This matching improves the accuracy of the division operation.

[0089] An alternative implementation could be provided using complimentary circuitry to provide a controlled voltage output when the DAC converter outputs a voltage rather than a current. It is also possible to bypass or eliminate the current divider for applications where its use is not necessary.

[0090] This amplitude scaling function can be utilized in conjunction with the time scaling function described below in order to perform charge balancing functions using a single scaling factor for scaling both time and amplitude to generate a charge balancing portion of the stimulation pulse.

AMPLITUDE MULTIPLIER

[0091] The output from the waveform generation circuitry is passed to the amplitude multipliers that are associated with corresponding channels. The output from the waveform generation circuitry is replicated in a current mirror, creating one copy of the current per amplitude multiplier. Those copies of the current are passed to the amplitude multipliers that are associated with corresponding channels. Each amplitude multiplier is comprised of two sets of switched current mirrors, one using p-channel FETs (pFETs) and one using n-channel FETs (nFETs). A schematic of one amplitude multiplier (for a single one of the channels) is shown in Figure 12. The PG contains multiple amplitude multipliers, one for each stimulation channel. In this diagram, the notation " $M=n$ " is again used, where n is some number that indicates that the corresponding FET on the diagram is replicated n times in practice.

[0092] To understand the amplitude multiplier, first consider just the pFET side, FETs **Q100-Q270** in Figure 12. The top row, FETs **Q100-Q170**, forms a current mirror that multiplies the current from FET **Q101**, which is driven by the current divider output **33**. The gate voltage developed by FET **Q101** then controls the current through the replicated FETs **Q100-Q170**. Thus, FETs **Q170**, marked $M=128$ (and thus representing a FET replicated 128 times), attempts to output 128 times the current through **Q101**, whereas the FET marked $M=64$, **Q160**, attempts to output 64 times the current through **Q101**, and so on.

[0093] The second row of FETs, **Q200-Q270**, function as switches that controllably connect the FETs of the first row to the output, CHn **39** representing one channel. To determine how much current is to be supplied on CHn, the suitable switches are turned on. For example, a binary code of 1100 0000 on the bus **34** (AMP_n) turns on **Q270** and **Q260**, permitting $(128+64)=192$ times the current through **Q101** to flow to the output CHn.

[0094] The bottom two rows of nFETs behave similarly. The bottom row of nFETs, **Q400-Q470**, form a current mirror that multiplies the current from **Q102**. nFETs **Q300-Q370** serve as a set of switches that controllably connect **Q400-Q470** to the output CHn **39**. As with the pFETs, the binary code controlling the **Q300-Q370** switches sets the current that flows to the output CHn.

[0095] The binary codes controlling the pFET and nFET switches are developed by the digital logic on the left side of Figure 12. The AMP_n signal **34** is an 8-bit binary bus that sets the multiplication factor, and the POL input **35** sets the polarity. The POL input **35** controls two multiplexers, **36**, **37** that switch the AMP_n multiplication factor to either the pFET or nFET switches, respectively, and switch \$00, meaning all switches open, to the other set of switches. The output from the multiplexer **36** passes through an inverting level-shift operation **38**, before connecting to the pFETs **Q200-Q270**. The output from the multiplexer **37** drives the nFETs **Q300-Q370** directly.

While this embodiment shows an 8-bit bus for selecting the multiplication factor, any number of bits may be used to achieve the amplitude resolution desired.

[0096] Thus, the current from the current divider is multiplied by the AMPn **34** amplitude value and assigned a polarity set by the POL **35** bit. The resulting current is then output on CHn **39**. The CHn output channel **39** is either connected through a detachable lead and an electrode contact to the tissue to be stimulated, or through protection circuitry to the lead and electrode contact, if protection circuitry is utilized.

[0097] It must be noted here that variations of the amplitude multiplier circuitry discussed herein may be included to achieve better accuracy or to meet timing or power requirements. This embodiment of the amplitude multiplier is only one of many configurations that can be used to transfer the output of the waveform generator into an output signal that is provided at the desired electrodes.

CLOCK DIVIDER FOR TIME SCALING

[0098] The clock divider **43** (see Figs. 4, 5) uses standard digital logic techniques to perform frequency division on the CLK input **42**. The division factor is configurable and must be an integer. That is to say, if the division factor is 3, then the clock divider outputs one clock cycle for every three cycles of the CLK input. If the division factor is 5, the clock divider outputs one clock cycle for every five cycles of the CLK input. Thus, the CLK frequency should be chosen sufficiently high to satisfy the shortest pulse width that would be expected, and must be high enough to consider the maximum number of samples that are to be used in any given pulse width (or "phase" as that term is used below).

[0099] Accordingly, with the application of both time dividing and current dividing, the example PG is capable of performing true division on the output current, without being constrained to integer quotients, and to similarly divide the clock signal to cover a longer period of time. (Note that division of a clock signal results in multiplication of time).

WAVEFORM SCALING FOR CHARGE BALANCING

[0100] Desired is a means to control the aspect ratio of the charge recovery phase as a function of the amplitude and pulse width of the stimulation phase. Consider Figure 19, which shows a two-phase stimulation pulse. The first phase **61**, the stimulation phase, has a negative polarity, an amplitude of n_p and a pulse width of t_p . The second phase **62**, the recovery phase, has a positive polarity, an amplitude of n_r and a pulse width of t_r . Both amplitudes n_p and n_r have units of digital-to-analog converter (DAC) current or voltage units and are nonnegative integers. Both pulse widths t_p and t_r have units of clock cycles and are nonnegative integers. The net charge of the pulse is $(n_r \cdot t_r - n_p \cdot t_p)$. If the aspect ratio of the recovery

phase is defined by a scaling factor k , such that the amplitude is scaled by $(n_r = n_p/k)$ and the pulse width is scaled by $(t_r = k \cdot t_p)$, the charge delivered during the recovery phase is equal to the charge delivered during the stimulation phase.

[0101] Figure 13 illustrates a simple example of how this division in the dimension of current and multiplication in the dimension of time can be utilized, showing the use of scaling factor k being used to divide the clock (so that only every k clock cycles are utilized) thereby stretching the wave in time, and a divisor k in amplitude, thereby preserving the overall areas of the waveform pulse **150** and pulse **251**. Such a division results in the same amount of charge transferred by each of the two curves, as their areas are basically equal, but because their polarity is opposite, the charges cancel out. Thus, Figure 13 shows how a pulse can be modified while preserving the charge using these two division operations.

[0102] Figure 14 shows this feature being applied to a half-sine wave shape. In this figure, both the stimulation **52** and charge recovery **53** phases are half-sine-waves using five samples each based on the same sample stored in memory. The recovery phase is scaled by two ($k=2$) using that value as both the current and clock dividers. Thus, the recovery phase has half the amplitude and twice the duration of the stimulation phase, the net DC charge is zero, and the pulse is charge-balanced, except for possible effects of residual inaccuracies in the system. Because the division is done in analog instead of by changing the amplitude multiplier DAC values, the relationship is truly independent of the amplitude value chosen.

[0103] Some residual inaccuracies in the pulse generator circuitry may cause the pulse to have a slightly non-zero net DC current. If this residual current is unacceptable, a solution is to include DC blocking capacitors and passive recovery switches that connect all of the stimulation outputs to a common point, restoring charge balance, as is shown in Figure 5.

[0104] Furthermore, when a pulse consists of phases of different shapes, it may not be possible to generate a completely charge-balanced waveform while maintaining the intended shapes. In such situations, an additional subtherapeutic phase may be added to transfer enough charge to provide balance, or DC blocking capacitors and passive recovery switches may be used.

[0105] Accordingly, by utilizing the time clock and current division functions, such balancing operations and scaling of waveform shapes is accommodated.

ARBITRARY WAVEFORM CREATION

[0106] The hardware discussed above is primarily intended to be utilized to generate a waveform of an arbitrary shape to be used for such purposes as spinal stimulation, such as for pain control, for example, for implementation in systems such as those described in Figs. 1-3. Some examples of waveforms that can be generated

by this arrangement are described below, although it must be emphasized that one of the primary benefits of this approach is that waveforms of almost any desired arbitrary shape (scaled in amplitude and time) can be provided using these techniques.

[0107] By adding further modifications to the example embodiments, even more flexibility in generating waveform shapes can be provided. For example, utilizing the entire address bus (or even increasing its size) to address much more memory to access many different waveform samples could be utilized. Additional RECT registers can be added to increase the options for rectangular pulses, and/or any number of shape logic circuits could be utilized to provide complex mathematical shapes. As discussed above, the waveform generation circuitry could be replicated to provide additional flexibility in generating output waveforms to the electrodes. Thus, these concepts offer nearly infinite possibilities in generating waveform shapes, as desired, by providing the appropriate adaptations.

[0108] As an example of the flexibility of waveform generation, a pulse using these techniques can be divided into two or more phases of stimulation, an example of which is illustrated in Figure 15, where three different phases are shown, one used twice. For any given channel, each phase has a single polarity and amplitude defined. Each phase has associated with it a clock divider value, a current divider value, a repetition count, a delay value, a waveform step size, a waveform offset value, and a waveform shape. Before generating a pulse, the external microcontroller loads registers in the stimulation ASIC with values representing the phases of the pulse.

[0109] To generate the example waveform of Fig. 15, when the microcontroller commands the ASIC to start the pulse, the ASIC then generates the phases in sequence. As each phase begins, the amplitude multipliers are loaded with the amplitude values and the polarities of each channel. The waveform generator is configured for the selected waveform for the phase, the current divider is loaded with the current division factor for the phase, and the clock divider is loaded with the clock division factor for the phase. The waveform generator then generates the waveform for the phase, after which the ASIC inserts a pre-programmed delay before starting the next phase. Phases can be repeated if the phase repetition count is set to a value greater than zero. Once the repetitions, if any, are completed, the ASIC then proceeds to generate the next phase of the pulse.

[0110] Thus, in the example of Fig. 15, a first phase 1 **54** is generated consisting of a rectangular pulse **54'** and a delay **54''**, a repeat of phase 1 **55**, a phase 2 **56** consisting of a half-sine pulse **56'** and a delay **56''**, and phase 3 pulse **57** consisting of a dying exponential curve **57'** and a delay **57''**.

[0111] In the additional example of Fig. 18, another waveform is generated including a first phase 1 **74** consisting of a rectangular pulse **74'** with negative polarity and a delay **74''**, a phase 2 **75** consisting of a rising ex-

ponential pulse **75'** with negative polarity and a delay **75''**, and phase 3 **76** consisting of a quarter-sine pulse **76'** with positive polarity and a delay **76''**.

[0112] By the above example architectures, the rectangular pulse could be generated using a RECT register, while the dying exponential, rising exponential, half-sine and quarter-sine pulses could be generated either by sampling respective normalized sine and exponential curves stored in memories, or by using a sine or exponential generator shape logic function, or some combination thereof.

[0113] At the microcontroller's command, charge balancing may be achieved by closing the switches that connect all of the DC blocking capacitors (if present) to a common node to passively balance the charge, or by generating an inverse of the curve of Fig. 15 (or a new curve of equal but inverse area) to actively balance the charge, or some combination of the two or by using the scaling procedure discussed hereinabove on the curve, but changing its scale at an equal inverse charge. Note that because phases 1 and 2 of Fig. 15 are negative pulses, but phase 3 is a positive pulse, by ensuring that the area of phase three is equal to the sum of the areas of phase 1 times 2 plus phase 2 (or adding an additional phase to counter any residual charge), active charge balancing is possible for at least some circumstances. It is also possible to use a combination of active and passive charge balancing, if desired.

[0114] Figure 16 shows an example IPG implementation useful for spinal pain management using an implanted PG that can utilize the features described above in more detail.

[0115] The microcontroller **307** will run the software and control the IPG's output. The microcontroller **307** will interface to other functional blocks to monitor IPG status, to send and receive communications, and to drive the channel configuration and output waveforms.

[0116] The RF transceiver **314** and matching network **340** and antenna **316** will provide a wireless communications interface to several external devices. The transceiver **314** will send and receive data while automatically handling data flow, RF channel control, error correction, and wakeup detection. The matching network **340** will provide the interface to the IPG's antenna **316**, which will be located in the header of the device.

[0117] The power architecture consists of the rechargeable battery **313**, the Power ASIC **306**, recharge coil **315**, along with a rectifier **330** and data modulation circuitry **331**. The rechargeable battery **313** will provide raw power to the IPG. The recharge coil **315** and rectifier **330** will accept power from a transcutaneous power link and convert it to a DC voltage, while the data modulation circuit **331** will use this link to transfer data to and from the external charger. The Power ASIC **306** will provide control of the recharge process, battery protection, and power for the digital, analog, and high-voltage components of the system.

[0118] The Stimulation ASIC **308** will produce the

waveforms for stimulation, for example using one of the techniques identified hereinabove. It will provide pulse shaping in arbitrary waveforms to allow complete control of nerve fiber recruitment.

[0119] The protection circuitry **309** will enhance safety for both the patient and the IPG itself. The protection circuitry **309** will include protection from electrostatic discharge (ESD) and over-voltage conditions (from defibrillation pulses and electrocautery). The protection circuitry **309** will also include EMI filters. Ultimately, the pulses are delivered to the desired site within the patient by a series of electrodes **302**.

[0120] Figure 17 shows an example application of the stimulator system for providing spinal stimulation. In that figure, the IPG **1** (or IPG **101** in Figure 2) is shown implanted in a patient. Also shown is the human spine comprising the C1-C7 cervical vertebrae **65**, the T1-T12 thoracic vertebrae **66**, the L1-L5 lumbar vertebrae **67**, and the S1-S5 sacral vertebrae **68**. Electrodes **63** are shown disposed near and along the spine and are positioned near the thoracic vertebrae **66**. The Electrodes **63** are attached to the IPG **1** via electrode leads **64**.

[0121] The leads and electrodes may be positioned anywhere along the spine to achieve the intended therapeutic effects of spinal cord stimulation. The distal end of the lead with its accompanying electrodes may be located along the epidural space and adjacent a desired portion of the spinal cord using well-established and known techniques for implanting and positioning SCS leads and electrodes, and the IPG **1** may be programmed using a clinician programmer, patient programmer, or other type of programming device **3**, **4** (or **103**, **104**), as desired (and further described above).

[0122] With respect to the Waveform Generator inside the Stimulation ASIC, the provided reference output to the Amplitude Multipliers could be a current, a voltage, or a digital value; all three forms are basically equivalent, and thus only the current output embodiments are shown. Similarly, the output from the Current Divider could be a current, a voltage, or a digital value. The output of the Iref generator could be either a current or a voltage, or the Iref generator could be omitted if the Waveform Generator outputs a digital value. Thus, using the techniques described herein modified according to the particular output needs can be used to apply these concepts to a great number of different applications.

[0123] Furthermore, the Current Divider could be connected between the Iref and the Waveform Generator, or it could be connected between the Waveform Generator and the Amplitude Multipliers. The Current Divider could also be bypassed or omitted. The outputs from the Amplitude Multipliers could be voltages instead of currents.

[0124] The terminology of current "flowing to" and "flowing from", or "sink" and "source", can vary depending on whether one uses the convention of current flowing from positive to negative or from negative to positive. Whichever convention one uses isn't important to prac-

ticating the invention.

[0125] The current divider and waveform multiplier could be built with thermometer encoding instead of binary weighting.

[0126] The current divider and waveform multiplier could have built-in fixed scaling factors ($\times 2$, $\times 4$, $\times \frac{1}{2}$, $\times \frac{1}{4}$, etc.).

[0127] The operation of truncating the phase accumulator to generate the address could be replaced by a round-to-nearest or ceiling (round-upwards) operation. If a large memory is available, truncation or rounding could be skipped and the entire phase accumulator used as the address.

[0128] Many other example embodiments of the invention can be provided through various combinations of the above described features. Although the invention has been described hereinabove using specific examples and embodiments, it will be understood by those skilled in the art that various alternatives may be used and equivalents may be substituted for elements and/or steps described herein, without necessarily deviating from the intended scope of the invention. Modifications may be necessary to adapt the invention to a particular situation or to particular needs without departing from the intended scope of the invention. It is intended that the invention not be limited to the particular implementations and embodiments described herein, but that the claims be given their broadest reasonable interpretation to cover all novel and non-obvious embodiments, literal or equivalent, disclosed or not, covered thereby.

Claims

1. A method for generating a stimulation pulse, said method comprising the steps of:

generating a first waveform of a desired shape different than a square wave using a waveform generator;
providing a first portion of the stimulation pulse substantially resembling said first waveform;
defining a scaling factor;
using said scaling factor for generating a second waveform using the waveform generator, said second waveform being a scaled version of the first waveform; and
providing a second portion of the stimulation pulse substantially resembling said second waveform, said second portion of the stimulation pulse for stimulating the stimulation region of the patient.

2. The method of claim 1, wherein said second portion of the stimulation pulse substantially cancels a charge provided to the stimulation region by the first portion of the stimulation pulse.

3. The method of any of the above claims, wherein said first waveform is generated by retrieving stored waveform samples from a memory.
4. The method of any of the above claims, wherein said first waveform is generated using a mathematical function generated by a waveform function generator.
5. The method of any of the above claims, wherein said second waveform is scaled in time based on the scaling factor.
6. The method of any of the above claims, wherein said second waveform is scaled in both time and amplitude based on the scaling factor such that the total charge delivered during the first waveform is substantially equal but inverse to the total charge delivered during the second waveform.
7. The method of any of the above claims, wherein in the stimulation pulse, the second waveform portion is provided following the first waveform portion.
8. A device for providing a therapy to a patient, said device comprising:
 - a waveform generator for generating a first waveform portion having a desired shape, wherein said desired shape includes at least a substantial portion of a shape other than a square wave, wherein said waveform generator has an input for receiving a scaling factor; said waveform generator being configured to use said scaling factor for generating a second waveform portion being a scaled version of the first waveform portion, wherein said device outputs a stimulation pulse comprising both said first waveform portion and said second waveform portion for stimulating a stimulation region of the patient.
9. The device of claim 8, wherein said second portion of the stimulation pulse substantially cancels a charge provided to the stimulation region by the first portion of the stimulation pulse.
10. The device of any of claims 8-9, wherein said second waveform portion is based on said first waveform portion scaled in both amplitude and time
11. The device of any of claims 8-10, wherein said waveform generator determines said desired shape by retrieving a stored waveform samples from a memory.
12. The device of any of claims 8-10, wherein said waveform generator determines said desired shape using a mathematical function generated by a waveform function generator.
13. The device of any of claims 8-12, further comprising a time scaling circuit for inputting at least part of said scaling factor into said waveform generator for scaling a time width of said first waveform portion for generating said second waveform portion.
14. The device of any of claims 8-13, further comprising an amplitude scaling circuit for inputting at least part of said scaling factor into said waveform generator for scaling an amplitude of said first waveform portion for generating said second waveform portion.

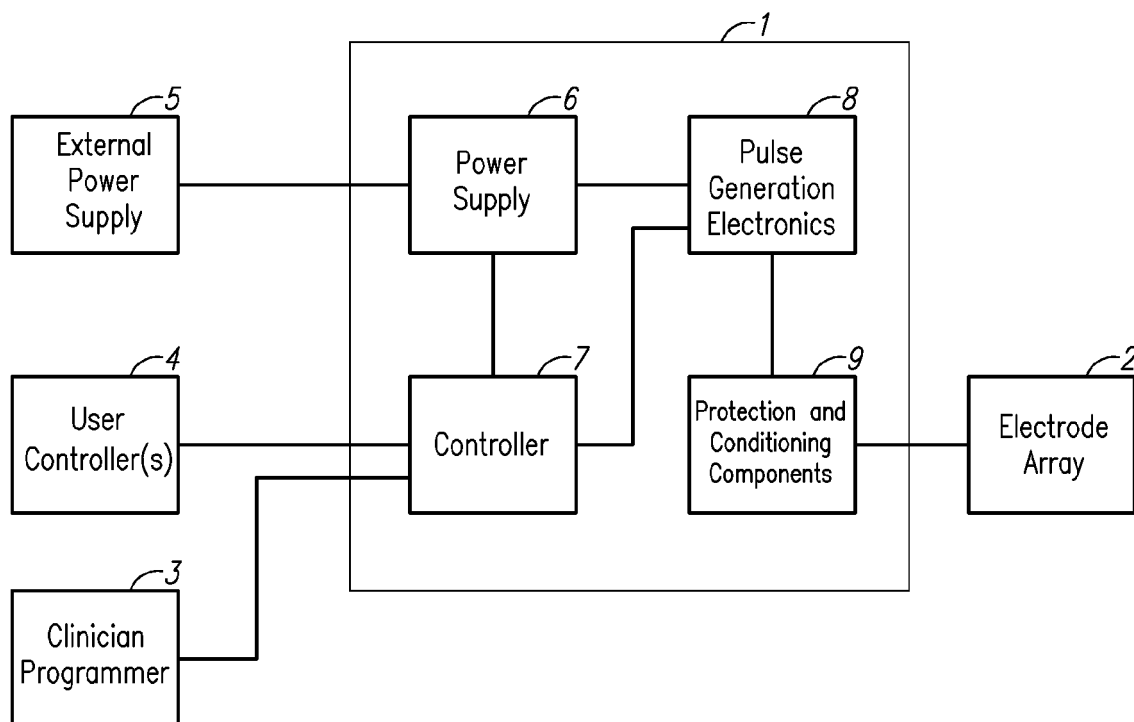


FIG. 1

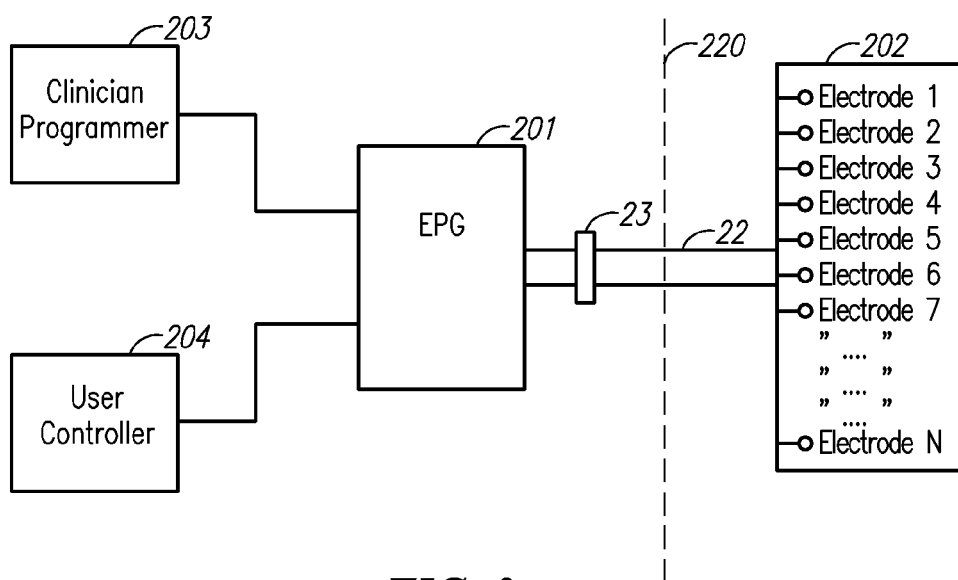


FIG. 3

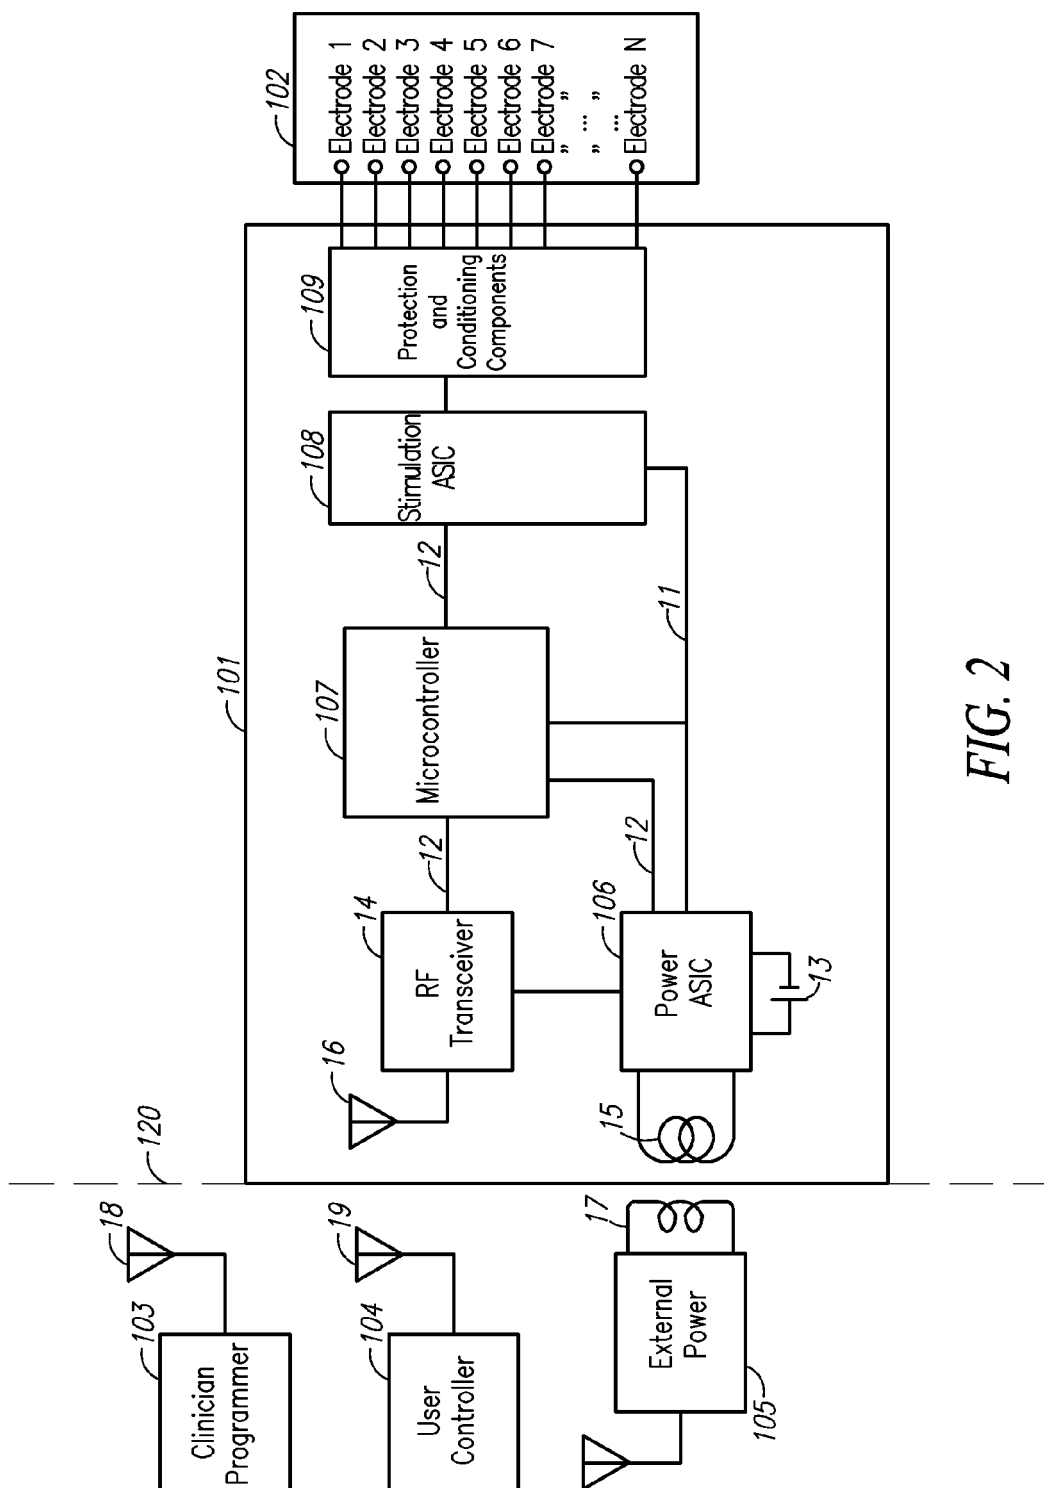


FIG. 2

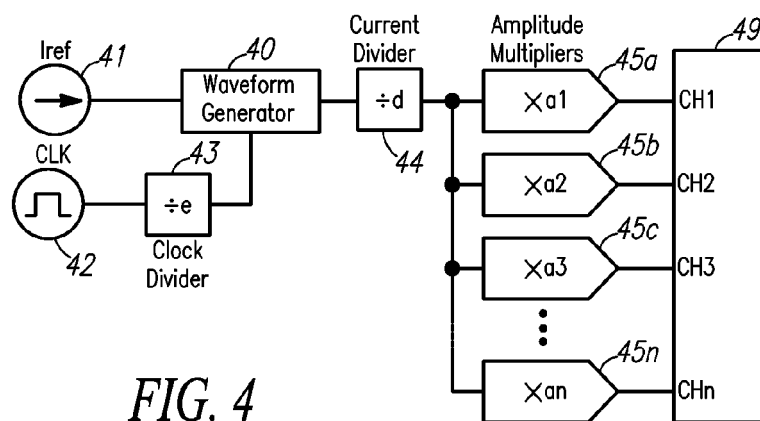


FIG. 4

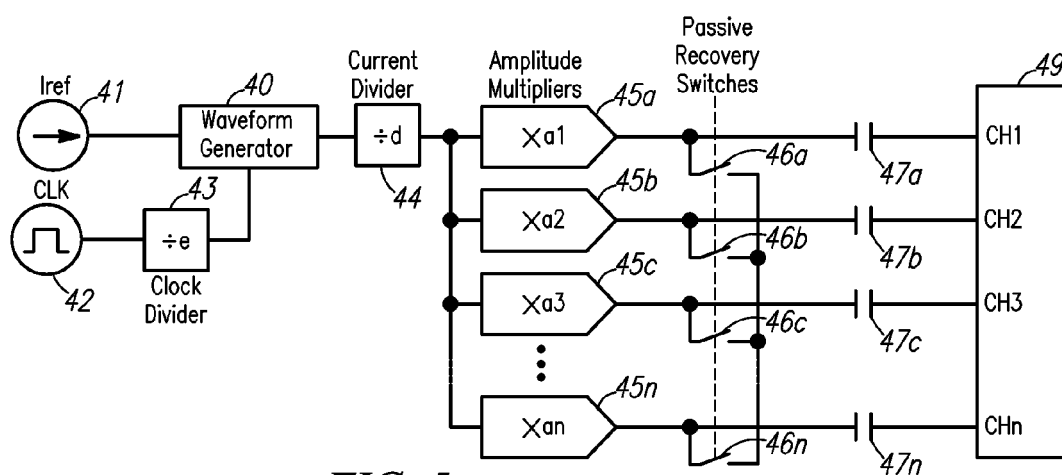


FIG. 5

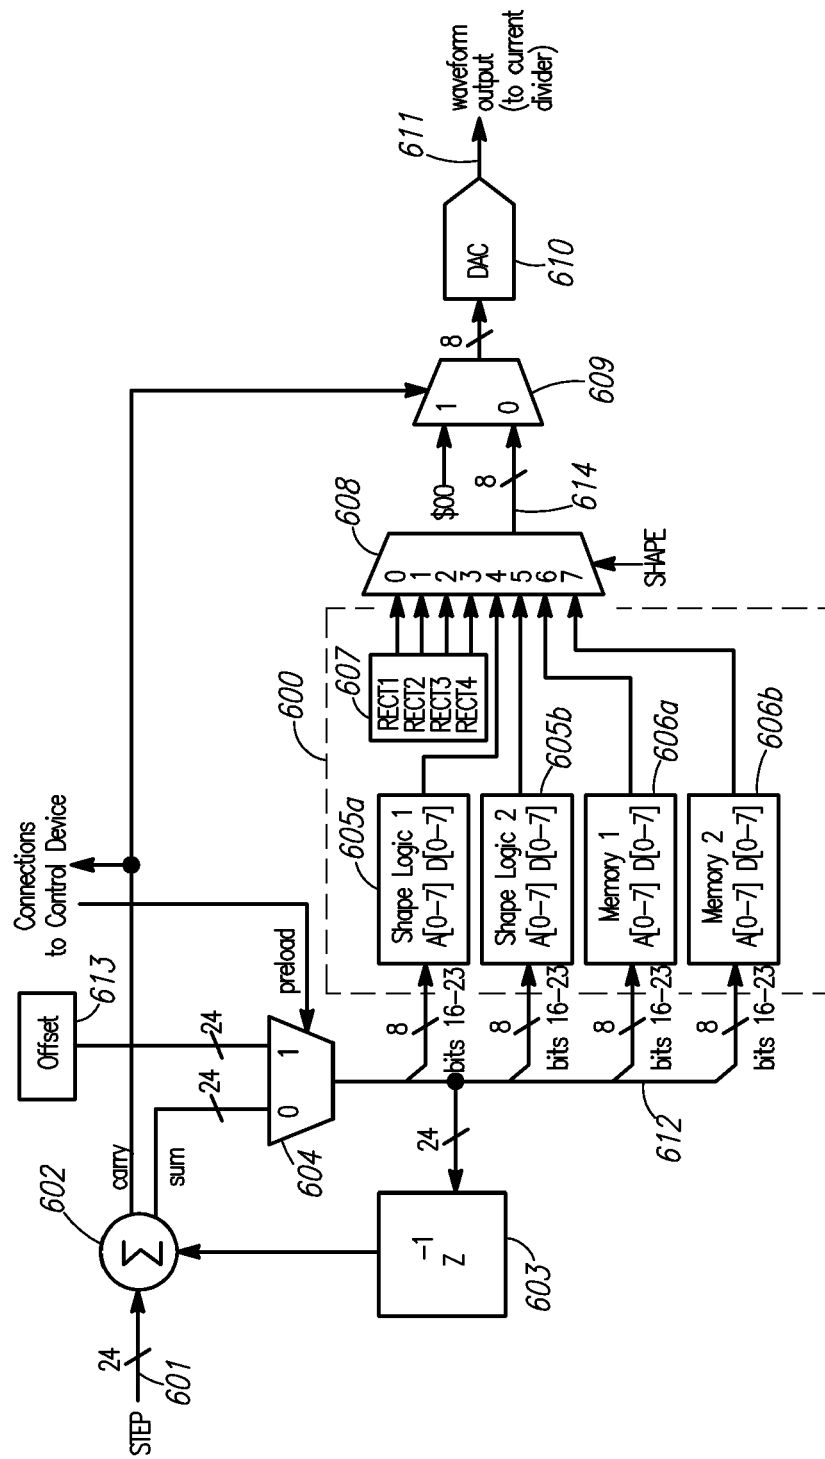


FIG. 6

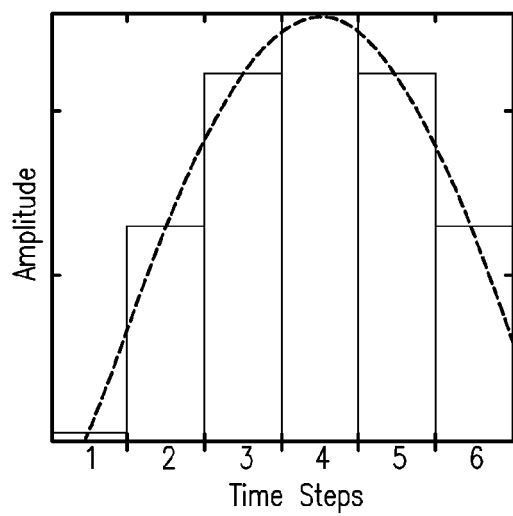


FIG. 7

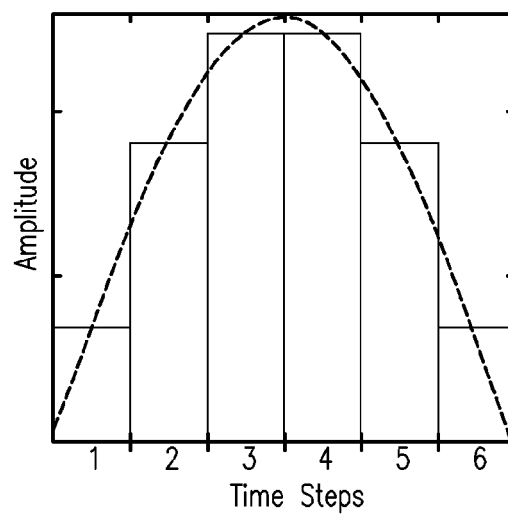


FIG. 8

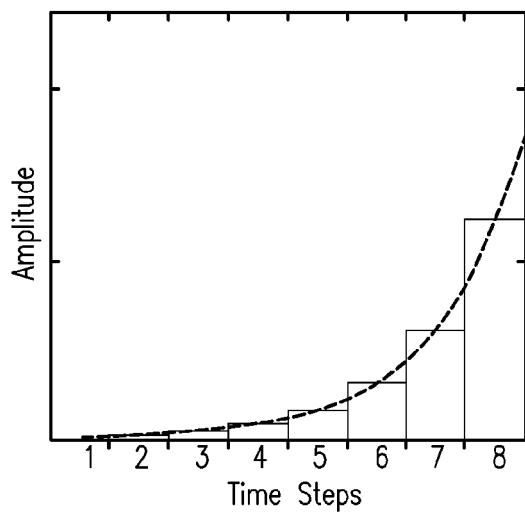


FIG. 9

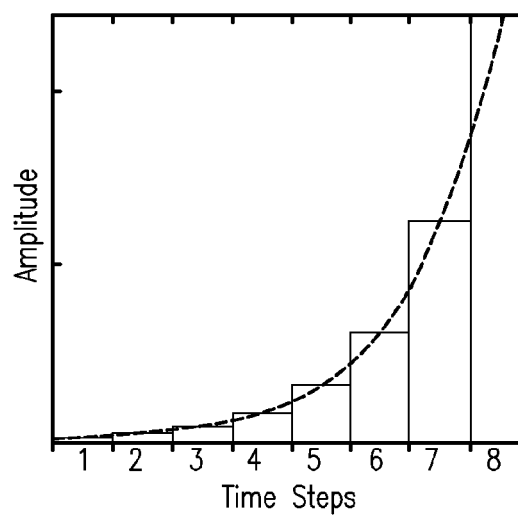


FIG. 10

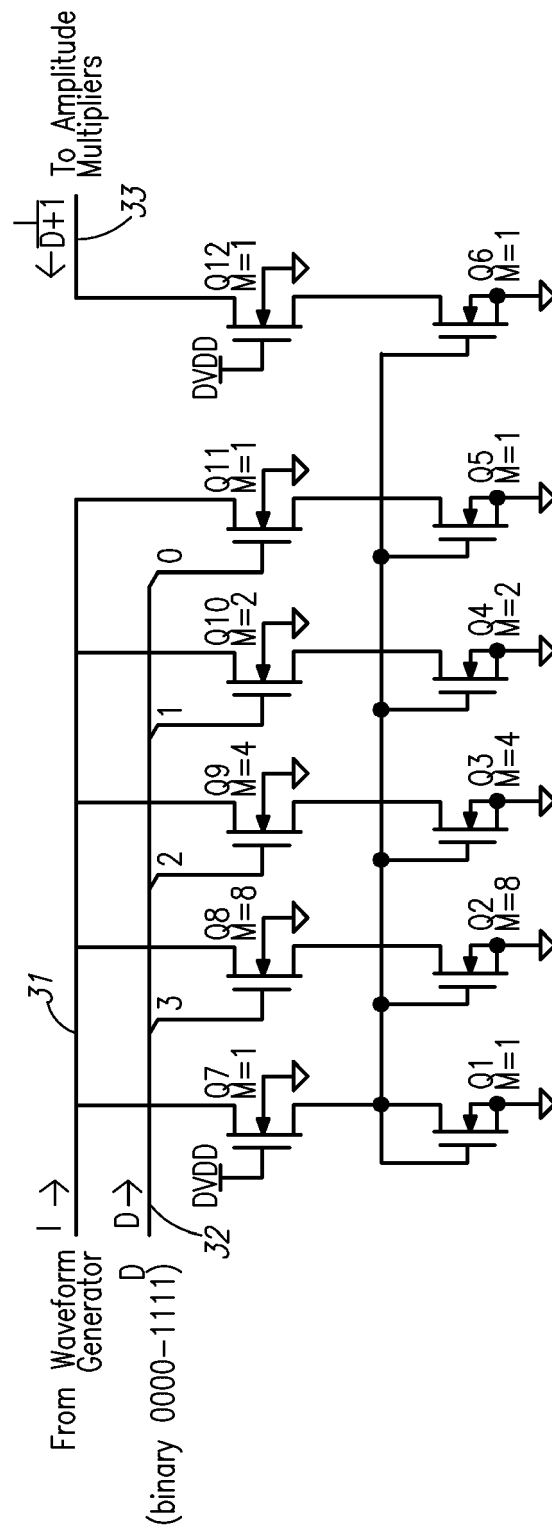
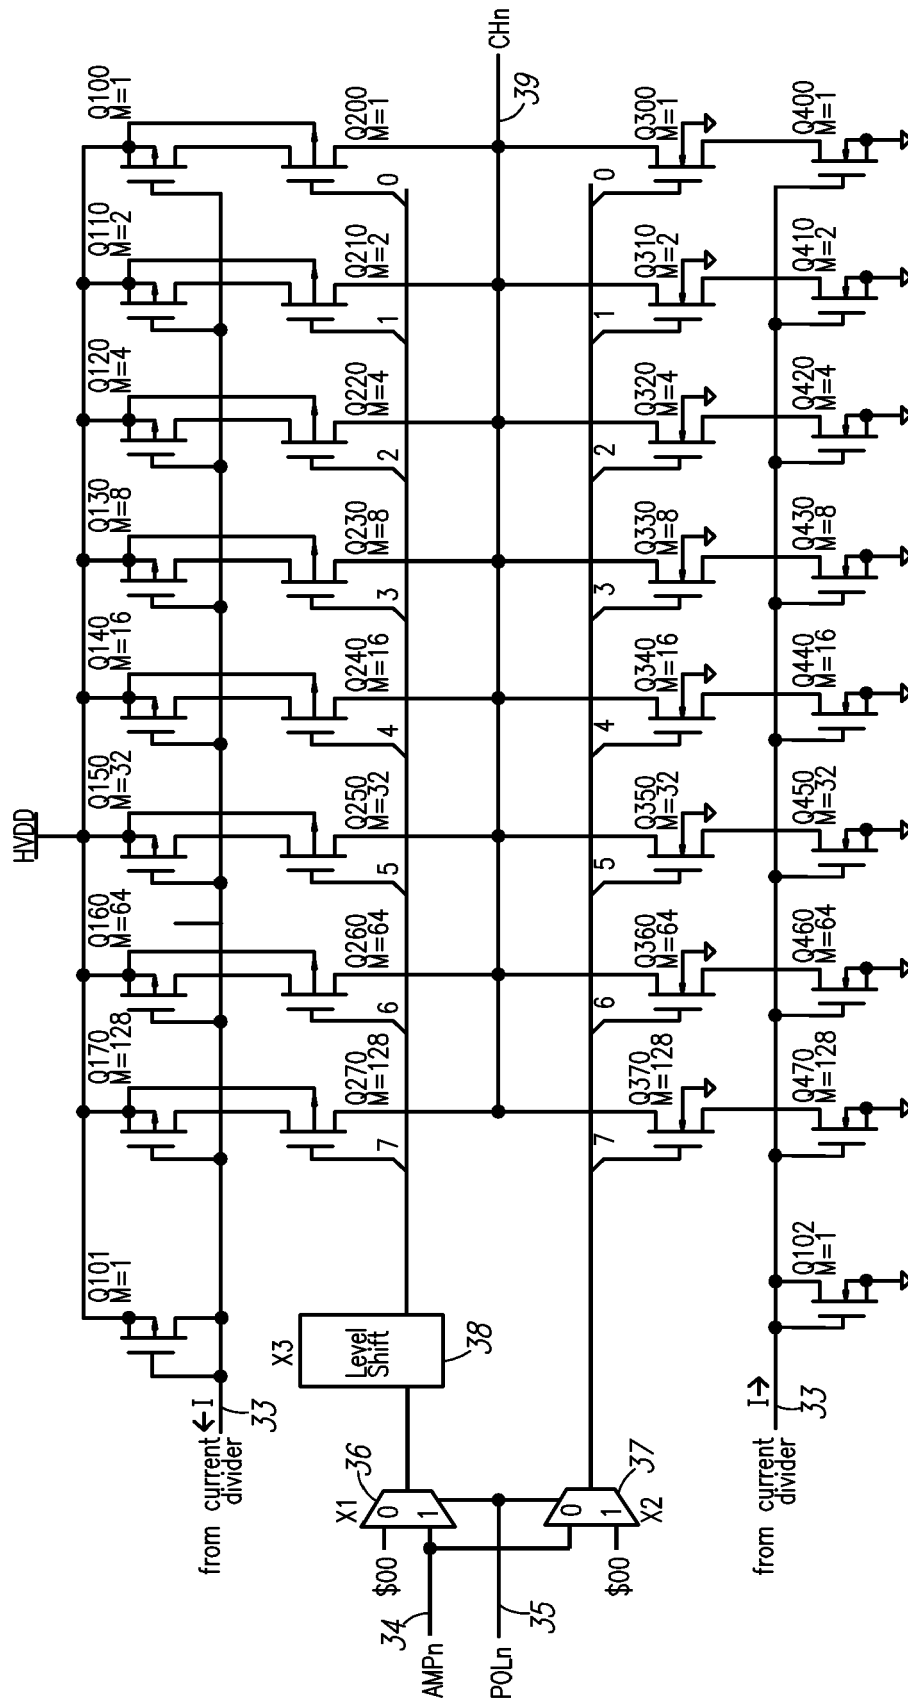


FIG. 11



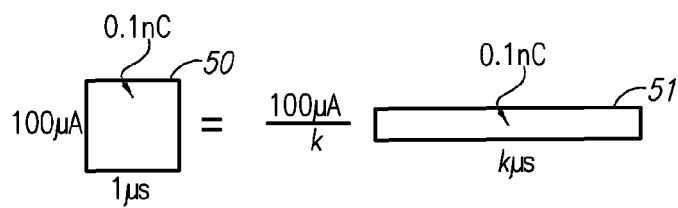


FIG. 13

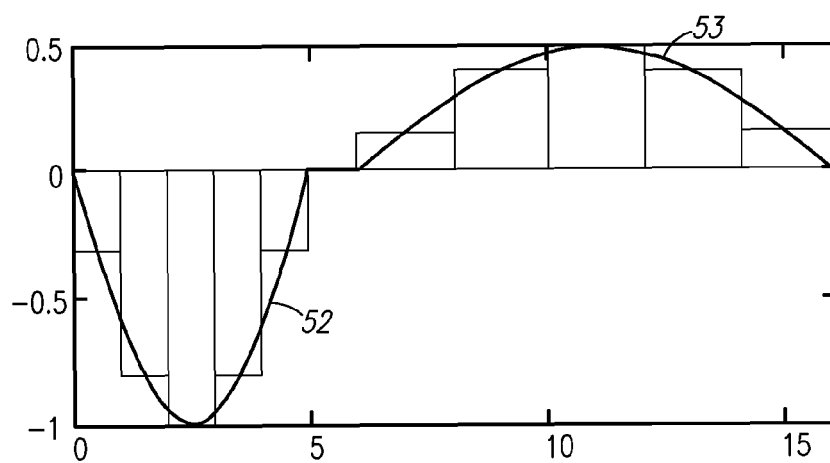


FIG. 14

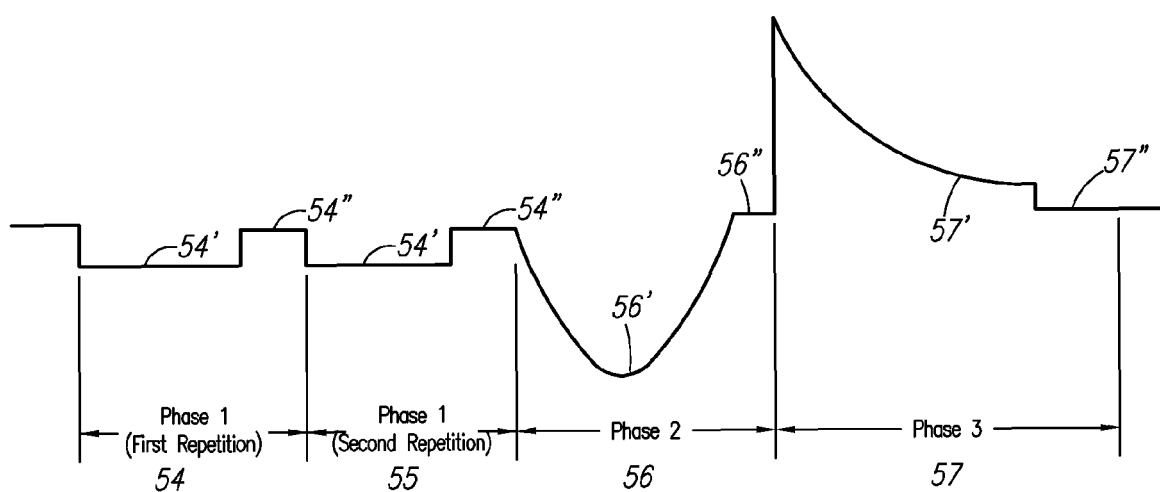


FIG. 15

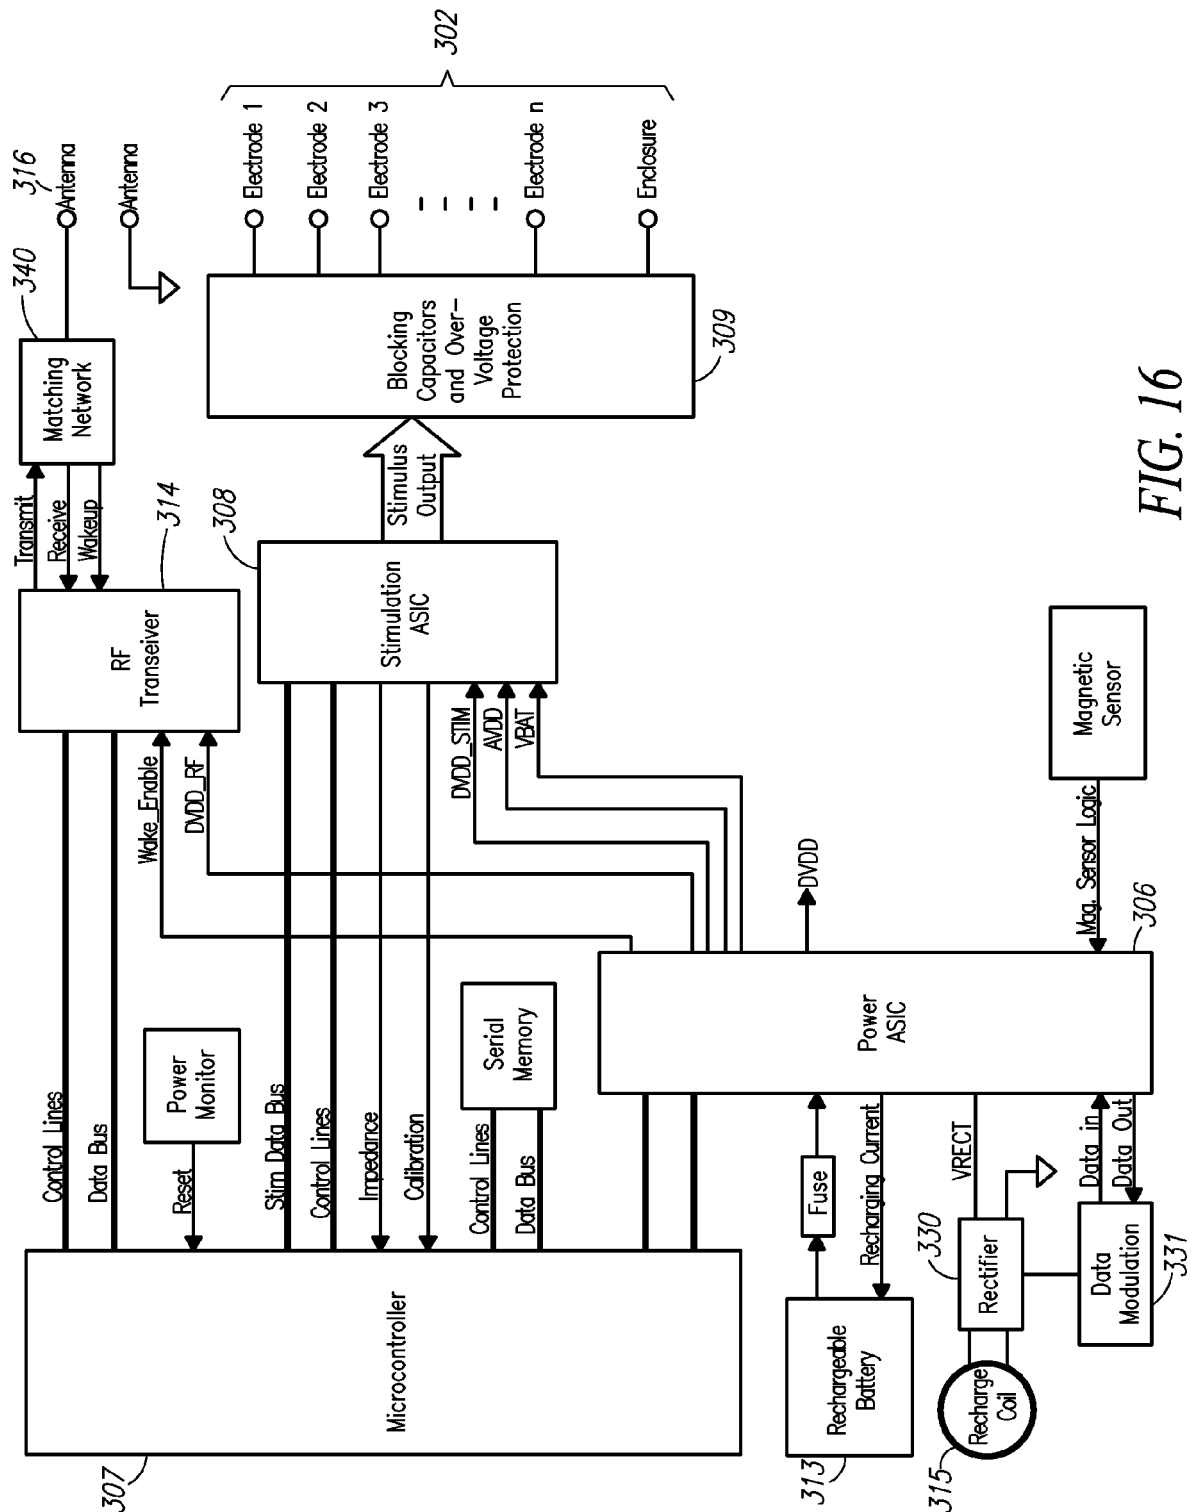


FIG. 16

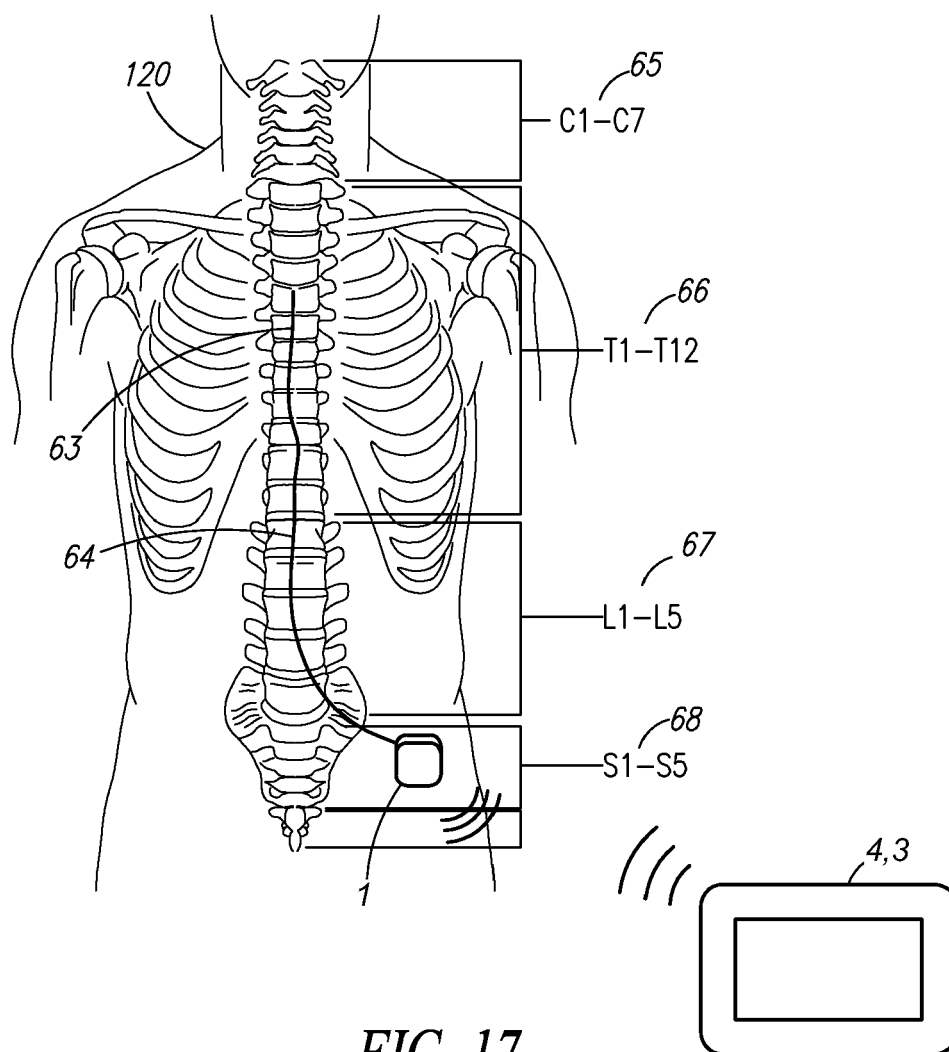


FIG. 17


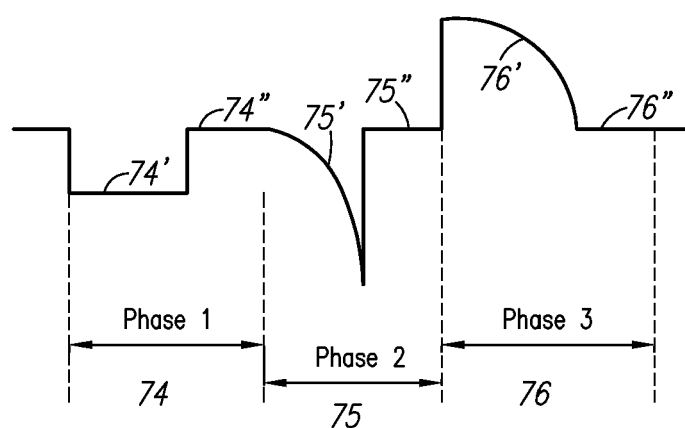


FIG. 18



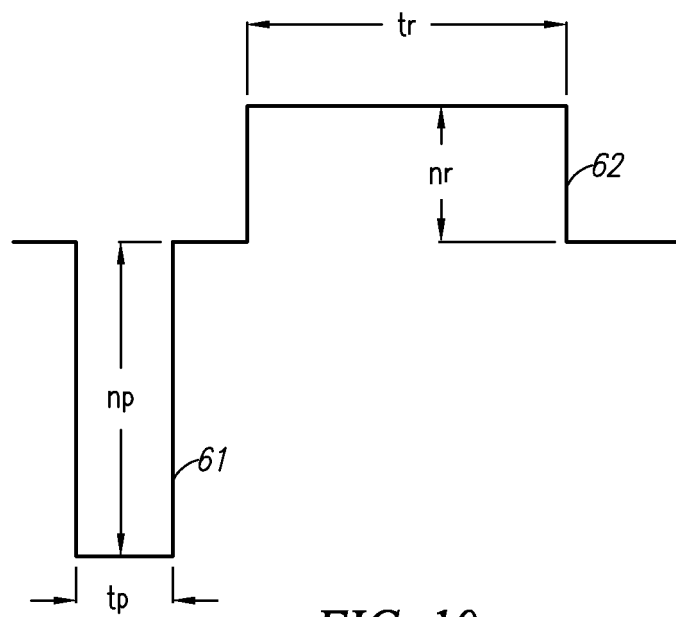

EUROPEAN SEARCH REPORT

Application Number
EP 15 17 0882

5

10

15

20

25

30

35

40

45

50

55

DOCUMENTS CONSIDERED TO BE RELEVANT			
Category	Citation of document with indication, where appropriate, of relevant passages	Relevant to claim	CLASSIFICATION OF THE APPLICATION (IPC)
Y	US 2011/029040 A1 (WALKER ANDRE B [US] ET AL) 3 February 2011 (2011-02-03) * abstract; figures 1a,2 * * paragraphs [0019], [0030] - [0034] * -----	1-14	INV. A61N1/36
Y	US 2010/274318 A1 (WALKER ANDRE B [US] ET AL) 28 October 2010 (2010-10-28) * abstract; figure 9 * * paragraph [0082] * -----	1-14	
A,D	US 7 715 912 B2 (REZAI ALI R [US] ET AL) 11 May 2010 (2010-05-11) * the whole document * -----	1-14	
A	US 2009/326624 A1 (MELSE ABRAHAM LODEWIJK [NL]) 31 December 2009 (2009-12-31) * the whole document * -----	1-14	
A	US 7 242 985 B1 (FRIDMAN GENE Y [US] ET AL) 10 July 2007 (2007-07-10) * the whole document * -----	1-14	
A	US 6 728 578 B1 (VOELKEL ANDREW W [US]) 27 April 2004 (2004-04-27) * the whole document * -----	1-14	TECHNICAL FIELDS SEARCHED (IPC) A61N
A	US 6 393 316 B1 (GILLBERG JEFFREY J [US] ET AL) 21 May 2002 (2002-05-21) * the whole document * -----	1-14	
A	US 6 289 247 B1 (FALTYS MICHAEL A [US] ET AL) 11 September 2001 (2001-09-11) * the whole document * -----	1-14	
A	US 5 690 688 A (NOREN KJELL [SE] ET AL) 25 November 1997 (1997-11-25) * the whole document * -----	1-14	
The present search report has been drawn up for all claims			
Place of search Munich		Date of completion of the search 27 August 2015	Examiner Pereda Cubián, David
CATEGORY OF CITED DOCUMENTS X : particularly relevant if taken alone Y : particularly relevant if combined with another document of the same category A : technological background O : non-written disclosure P : intermediate document		T : theory or principle underlying the invention E : earlier patent document, but published on, or after the filing date D : document cited in the application L : document cited for other reasons & : member of the same patent family, corresponding document	

EPO FORM 1503 03.02 (P04C01)

**ANNEX TO THE EUROPEAN SEARCH REPORT
ON EUROPEAN PATENT APPLICATION NO.**

EP 15 17 0882

This annex lists the patent family members relating to the patent documents cited in the above-mentioned European search report.
The members are as contained in the European Patent Office EDP file on
The European Patent Office is in no way liable for these particulars which are merely given for the purpose of information.

27-08-2015

Patent document cited in search report		Publication date	Patent family member(s)	Publication date
US 2011029040 A1	03-02-2011	AU	2010279054 A1	16-02-2012
		CA	2769384 A1	03-02-2011
		EP	2459271 A1	06-06-2012
		JP	5676609 B2	25-02-2015
		JP	2013500779 A	10-01-2013
		US	2011029040 A1	03-02-2011
		US	2014031893 A1	30-01-2014
		US	2014330338 A1	06-11-2014
		US	2015217113 A1	06-08-2015
		WO	2011014570 A1	03-02-2011

US 2010274318 A1	28-10-2010	AU	2010238763 A1	10-11-2011
		AU	2010238768 A1	10-11-2011
		CA	2758975 A1	28-10-2010
		CA	2759018 A1	28-10-2010
		CN	102458568 A	16-05-2012
		CN	102458569 A	16-05-2012
		DE	202010018211 U1	29-09-2014
		EP	2243510 A2	27-10-2010
		EP	2243511 A2	27-10-2010
		EP	2586488 A1	01-05-2013
		JP	5734279 B2	17-06-2015
		JP	2012524629 A	18-10-2012
		JP	2012524630 A	18-10-2012
		KR	20120024623 A	14-03-2012
		KR	20120028307 A	22-03-2012
		US	2010274314 A1	28-10-2010
		US	2010274315 A1	28-10-2010
		US	2010274316 A1	28-10-2010
		US	2010274317 A1	28-10-2010
		US	2010274318 A1	28-10-2010
		US	2010274326 A1	28-10-2010
		US	2012016437 A1	19-01-2012
		US	2012016438 A1	19-01-2012
		US	2012016439 A1	19-01-2012
		US	2012158093 A1	21-06-2012
		US	2012197369 A1	02-08-2012
		US	2012203303 A1	09-08-2012
		US	2012203304 A1	09-08-2012
		US	2012203319 A1	09-08-2012
		US	2012209349 A1	16-08-2012
		US	2013110196 A1	02-05-2013
		US	2013123879 A1	16-05-2013
		US	2013172955 A1	04-07-2013
		US	2013204320 A1	08-08-2013
		US	2013204321 A1	08-08-2013

EPO FORM P0459

For more details about this annex : see Official Journal of the European Patent Office, No. 12/82

**ANNEX TO THE EUROPEAN SEARCH REPORT
ON EUROPEAN PATENT APPLICATION NO.**

EP 15 17 0882

This annex lists the patent family members relating to the patent documents cited in the above-mentioned European search report.
The members are as contained in the European Patent Office EDP file on
The European Patent Office is in no way liable for these particulars which are merely given for the purpose of information.

27-08-2015

Patent document cited in search report	Publication date	Patent family member(s)	Publication date	
		US 2013204322 A1	08-08-2013	
		US 2013204338 A1	08-08-2013	
		US 2014025134 A1	23-01-2014	
		US 2014025146 A1	23-01-2014	
		US 2014031896 A1	30-01-2014	
		US 2014142656 A1	22-05-2014	
		US 2014142657 A1	22-05-2014	
		US 2014142658 A1	22-05-2014	
		US 2014142659 A1	22-05-2014	
		US 2014142673 A1	22-05-2014	
		US 2014188187 A1	03-07-2014	
		US 2014343622 A1	20-11-2014	
		US 2014379044 A1	25-12-2014	
		US 2015018896 A1	15-01-2015	
		US 2015032182 A1	29-01-2015	
		US 2015032183 A1	29-01-2015	
		US 2015039049 A1	05-02-2015	
		US 2015039050 A1	05-02-2015	
		US 2015045853 A1	12-02-2015	
		US 2015045854 A1	12-02-2015	
		US 2015051664 A1	19-02-2015	
		US 2015142076 A1	21-05-2015	
		WO 2010124139 A1	28-10-2010	
		WO 2010124144 A1	28-10-2010	

US 7715912	B2	11-05-2010	EP 1900335 A1	19-03-2008
			US 2007078498 A1	05-04-2007

US 2009326624	A1	31-12-2009	NONE	

US 7242985	B1	10-07-2007	US 7242985 B1	10-07-2007
			US 2010179616 A1	15-07-2010

US 6728578	B1	27-04-2004	US 6728578 B1	27-04-2004
			US 6996438 B1	07-02-2006
			US 7542806 B1	02-06-2009
			US 7937155 B1	03-05-2011

US 6393316	B1	21-05-2002	DE 60029776 T2	02-08-2007
			EP 1178855 A1	13-02-2002
			US 6393316 B1	21-05-2002
			WO 0069517 A1	23-11-2000

US 6289247	B1	11-09-2001	NONE	

US 5690688	A	25-11-1997	DE 69733531 D1	21-07-2005

EPO FORM P0459

For more details about this annex : see Official Journal of the European Patent Office, No. 12/82

10

15

20

25

30

35

40

45

50

55

EPO FORM P0459

37

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- US 7715912 B [0041]