



(12) **EUROPEAN PATENT APPLICATION**

(43) Date of publication:
16.12.2015 Bulletin 2015/51

(51) Int Cl.:
A61G 7/002 (2006.01) **A61G 7/015 (2006.01)**
A61G 7/018 (2006.01)

(21) Application number: **15170984.7**

(22) Date of filing: **08.06.2015**

(84) Designated Contracting States:
AL AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO PL PT RO RS SE SI SK SM TR
Designated Extension States:
BA ME
Designated Validation States:
MA

(30) Priority: **13.06.2014 PCT/US2014/042342**
20.11.2014 US 201414548647

(71) Applicant: **Hill-Rom Services, Inc.**
Batesville, IN 47006-9167 (US)

(72) Inventors:
• **HUTCHISON, Stephen, E.**
Batesville, IN Indiana 47006 (US)
• **RUSCHKE, Jeffrey A.**
Lawrenceburg, IN Indiana 47025 (US)

- **CHRISTIE, John D.**
Batesville, IN Indiana 47006 (US)
- **GUTHRIE, Brian**
Greensburg, IN Indiana 47240 (US)
- **LANNING, Mark E.**
Mt. Pleasant, SC South Carolina 29466 (US)
- **ERNST, Joseph A.**
Cincinnati, OH Ohio 45247 (US)
- **TURNER, Jonathan D.**
Dillsboro, IN Indiana 47018 (US)
- **BOSSINGHAM, Robert A.**
Rushville, IN Indiana 46173 (US)
- **RIGSBY, Mark Tyler**
Dayton, OH Ohio 45420 (US)
- **LATTIMORE, James D.**
Fairport, IN 14450 (US)

(74) Representative: **Findlay, Alice Rosemary**
Reddie & Grose LLP
16 Theobalds Road
London WC1X 8PL (GB)

(54) **ADJUSTABLE PERSON SUPPORT SYSTEM WITH EXPANSION WINGS DRIVEN BY DUAL LEADSCREWS AND CENTER MOUNTED MOTORS**

(57) A bed comprises a deck section having a width and left and right outboard deck edges. Left side and right side wings are movably coupled to the deck section. The bed also includes a left leadscrew receiver mounted on the left wing, a right leadscrew receiver mounted on the right wing, and left and right motor assemblies both mounted on the deck section. A left leadscrew is coupled to the left motor assembly and to the left leadscrew receiver. A right leadscrew is coupled to the right motor assembly and to the right leadscrew receiver. Motor operation is capable of moving the wing to which it is coupled between a deployed position in which the lateral extremity of the wing is outboard of the respective outboard edge of the deck section and a stored position in which the lateral extremity of the wing is inboard of its deployed position.

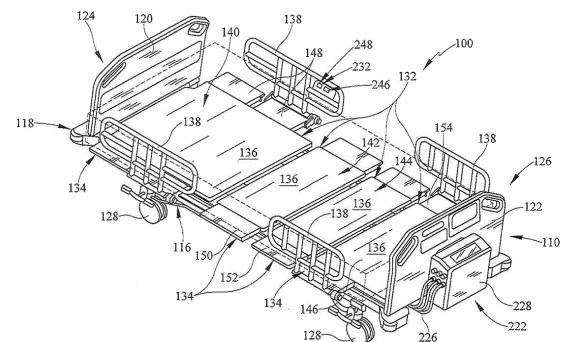


FIG. 1

Description

[0001] This disclosure relates to adjustable person support systems. More particularly, but not exclusively, one contemplated embodiment relates to a person support apparatus and mattress configurable to increase and decrease in length and/or width to accommodate a person supported thereon. While various length and/or width adjusting person support systems have been developed, there is still room for improvement. Thus, a need persists for further contributions in this area of technology.

[0002] One contemplated embodiment includes a control system, comprising: a first controller configured to control a function of a person support apparatus, the first controller receiving a first input corresponding to a function of the person support apparatus via a first user interface; and a second controller configured to control a function of a person support surface, the second controller receiving a second input corresponding to a function of the person support surface via a second user interface, wherein at least one input function on the second user interface is disabled when first controller and the second controller are in electrical communication with one another and the first user interface is configured to receive input signals corresponding to functions of the person support surface and person support apparatus.

[0003] Another contemplated embodiment includes a person support system, comprising: a person support apparatus including at least one of a width and length extension assembly; a person support surface configured to be supported on the person support apparatus and including at least one of a length and width extension assembly; a controller configured to cause at least one of the width and length extension assembly of the person support apparatus and the person support surface to move in response to an input from a user, wherein the at least one of the length and width extension assembly for the person support surface will remain in a retracted position unless the corresponding one of the at least one of the width and length extension assembly of the person support apparatus is positioned in one of a fully retracted position and a fully extended position.

[0004] Another contemplated embodiment includes a person support system, comprising: a person support apparatus including a first size adjusting assembly; a person support surface configured to be supported on the person support apparatus and including a second size adjusting assembly; a controller configured to cause at least one of the first size adjusting assembly of the person support apparatus and the second size adjusting assembly of the person support surface to change the size thereof in response to an input from a user, wherein the size adjusting assembly for the person support surface will remain in a retracted position unless the corresponding size adjusting assembly of the person support apparatus is in one of a fully retracted position and a fully extended position.

[0005] The invention will now be further described by

way of example with reference to the accompanying drawings, in which:

FIG. 1 is a perspective view of an adjustable width person support system, constructed according to one or more of the principles disclosed herein;

FIG. 2 is a perspective view of the upper frame base, deck sections, and deck extensions as seen by an observer looking from beneath the upper frame;

FIGS. 3A and 3B are perspective views showing a side of the upper body deck section with a head deck section extension in its deployed or extended state (FIG. 3A) and in its stored or retracted state (FIG. 3B) as seen by an observer looking from above the segment. A deck panel which rests atop the deck framework is absent from the illustration in order to expose to view components that would otherwise be obscured;

FIG. 4 is a perspective bottom view of the upper body deck section showing the power extension/retraction system and manual release assembly;

FIG. 5 is an exploded view of the manual release assembly according to one contemplated embodiment;

FIG. 6 is a perspective bottom view of the clasps in an engaged position where the clasps engage the lead screw and allow for powered extension/retraction of the deck extension;

FIG. 7 is a perspective bottom view of the clasps in a disengaged position where one of the clasps doesn't engage the lead screw and the deck extension is movable independent of the lead screw;

FIG. 8 is a perspective top view of the manual release assembly;

FIG. 9 is a side perspective view of a mattress and fluid supply system configured to be supported on the person support apparatus;

FIG. 10 is a schematic plan view of the mattress configured to be used with changeable width person support apparatus, constructed according to one or more of the principles disclosed herein;

FIG. 11 is a block diagram of one embodiment of a system configured to change width of a person support apparatus, constructed according to one or more of the principles disclosed herein;

FIG. 12 is a block diagram of another embodiment of a system configured to change width of a person

support apparatus, constructed according to one or more of the principles disclosed herein;

FIG. 13 is a view of a control interface having a retract button and an extend button that a user uses to reduce or expand respectively the width of the person support apparatus;

FIGS. 14A and 14B are schematic views of deck extensions staggered according to one or more principles disclosed, wherein the upper body deck extension lags the lower body deck extensions when the deck extensions are extended (FIG. 14A) and leads the lower body deck extensions when the deck extensions are retracted (FIG. 14B);

FIG. 15 is a flow chart of a method of monitoring a connection between a bed controller and a mattress controller.

FIGS. 16-17 show a flowchart showing a first method of changing width of a person support apparatus, constructed according to one or more of the principles disclosed herein; and

FIGS. 18, 18B, 19 and 19B are flowcharts showing a second method of changing the width of a person support apparatus.

FIG. 20 is a view showing an upper body deck section framework as seen from underneath, the section comprised of laterally extending supports configured as C-channels and longitudinally extending beams, and also showing portions of a deck extension comprised of spars which nest within the C-channels.

FIG. 21 is view similar to that of FIG. 20 but slightly rotated.

FIG. 22 is a schematic view of a motor assembly.

FIG. 23 is a view of a leadscrew.

FIG. 24 is a schematic plan view of a bed architecture having four deck sections each of which includes a left side motor assembly, a left wing or deck extension driven by the left motor assembly by way of a left leadscrew, a right side motor assembly, and a right wing or deck extension driven by the right motor assembly by way of a right leadscrew.

FIG. 25 is a schematic plan view of a bed architecture having four deck sections and shared left and right motor assemblies mounted on one of the sections such that left and right deck width extensions of that section are directly driven by the respective left and right motor assemblies and such that left and right width extensions of adjacent deck sections are indi-

rectly driven by the motor assemblies as a result of links connecting the directly driven extensions to the indirectly driven extensions.

FIG. 26 is a schematic plan view of a bed architecture having four deck sections and shared left and right motor assemblies mounted on one of the sections such that left and right deck width extensions of that section are directly driven by the respective left and right motor assemblies and such that left and right proximate width extensions are indirectly driven by the motor assemblies as a result of links connecting the directly driven extensions to the proximate indirectly driven extensions and such that left and right remote width extensions are indirectly driven by the motor assemblies as a result of links connecting the remote extensions to the proximate extensions.

[0006] A variable width person support system 100 according to one contemplated embodiment is shown in FIGS. 1-19. U.S. patent applications 11/774847, 11/775083, 13/468424, and 14/168538 disclose variable width person support apparatus, related systems and methods of use. The person support system 100 includes an adjustable width person support apparatus 110, an adjustable width person support surface or mattress 112 configured to be supported on the person support apparatus 110, and a control system 114 configured to control the adjustment of the width of the person support apparatus 110 and mattress 112. One contemplated embodiment of the person support apparatus 110 is shown in FIG. 1 as a bed frame, however, in other embodiments the person support apparatus 110 may be a wheelchair, stretcher or any other apparatus configured to support a person thereon. In another contemplated embodiment, the length of the person support apparatus 110 and mattress 112 can be adjusted. In one example, the length of the person support apparatus 110 and mattress 112 can be adjusted using the Flexafoot™ feature sold by Hill-Rom.

[0007] The person support apparatus 110 comprises a lower frame 116, an upper frame 118 movably supported above a lower frame 116 by supports (not shown) coupled to the lower frame 116, a head board 120 at the head end 124 of the person support apparatus 110, and a foot board 122 at the foot end 126 of the person support apparatus 110 as shown in FIGS. 1 & 2. The supports are configured to raise and lower at least a portion of the upper frame 118 with respect to the lower frame 116. The lower frame 116 rests on at least one caster wheel 128 in this embodiment, allowing the person supported apparatus 110 to be transported. The upper frame 118 includes an upper frame base 130 coupled to the supports, a plurality of deck sections 132, a plurality of deck extensions 134, a plurality of deck panels 136 supported on the deck sections 132 and deck extensions 134, and siderails 138. The siderails 138 are coupled to the deck extensions 134 and cooperate to define a portion of the

perimeter of the person support apparatus 110.

[0008] The deck sections 132 are movably coupled to the upper frame base 130 and are configured to be articulated with respect to one another and the upper frame base 130 between a number of configurations including a substantially co-planar configuration, a reclined configuration, a chair configuration, and various other configurations. The deck sections 132 include an upper body deck section 140, seat deck section 142, thigh deck section 144 and foot deck section 146 as shown in FIGS. 1 & 2. Each of the deck sections 132 includes a corresponding extension 134 (an upper body deck extension 148, seat deck extension 150, thigh deck extension 152 and foot deck extension 154) that can be extended and retracted from the deck sections 132 to increase and decrease the width of the person support apparatus 110. In this embodiment, the seat, thigh, and foot deck extensions 150, 152, and 154 are connected to one another and configured to be extended and retracted together; however, in other embodiments the seat, thigh, and foot deck extensions 150, 152, and 154 can be extended/retracted independently.

[0009] In one contemplated embodiment, a user can choose to extend/retract the deck extensions 134 using a powered extension/retraction system 156 by providing an input to the control system 114 or to manually extend/retract the deck extensions 134 by actuating a manual release assembly 158 to disengage the deck extension 134 from the powered extension/retraction system 156. The powered extension/retraction system 156 includes lead screws 160 rotatably coupled to the deck sections 132 and configured to be rotated by motors 162. In one contemplated embodiment, the seat, thigh, and foot deck extensions 150, 152, and 154 are connected together and a single motor 162 and lead screw 160 are used to extend/retract them as shown in FIGS. 14A & 14B. In one example, a motor 162 is coupled to the upper body deck section 140 and rotates a lead screw 160 when activated by the control system 114 in response to an input from a user to extend/retract the upper body deck extension 148.

[0010] The manual release assembly 158 includes a separable threaded clasp 164, a clasp separator 166, a cable 168, and a handle 170 as shown in FIGS. 4-8. In some contemplated embodiments, the clasp 164 is not threaded and is configured to engage and retain a carrier that includes a threaded bore configured to engage the lead screw 160. The threaded clasp 164 includes a first clasp member 172 and a second clasp member 174 that are aligned substantially perpendicular to the lead screw 160 and are configured to engage the lead screw 160 in an engaged position (FIG. 6) when adjacent to one another, and configured to disengage the lead screw 160 in a disengaged position (FIG. 7) when separated from one another. The clasp 164 is moved from the engaged position to the disengaged position by the clasp separator 166 upon actuation of the manual release handle 170 and allows the deck extension 134 to be manually ex-

tended/retracted independent of the motion of the lead screw 160. The first clasp member 172 includes a main body portion 176, a first guide 178 protruding from the bottom of the body 176, a second guide 180 protruding from the top of the body 176, a lead screw engaging portion 182, and a guide shaft 184. The first guide 178 is configured to move along a guide slot 186A in the deck extension frame 188 as the first clasp member 172 is moved with respect to the second clasp member 174. In some contemplated embodiments, the first clasp member 172 moves along a path that is substantially perpendicular to the rotational axis of the lead screw 160. The first guide 178 cooperates with the slot 186A to maintain alignment of the first and second clasp members 172 and 174. The second guide 180 is configured to move within a guide slot 190 in the second clasp member 174 and is configured to cooperate with the second clasp guide slot 190 to maintain alignment of the first and second clasp members 172 and 174. The lead screw engaging portion 182 extends from the main body portion 176 and includes a curved end 192 with threads cut therein that are configured to engage the threads on the lead screw 160. The guide shaft 184 extends opposite the threaded body portion 182 and is configured to move within a bore 194 in the deck extension frame 188 as the first clasp member 172 is moved between the engaged position and the disengaged position. A spring 196 is disposed around the guide shaft 184 and is configured to bias the first clasp member 172 toward the engaged position where the first clasp member 172 and second clasp member 174 engage the lead screw 160. When the manual release assembly 158 is actuated, the first clasp member 172 is moved away from the second clasp member 174 toward the disengaged position which causes the spring 196 to compress between the main body portion 176 and the deck extension frame 188. When the manual release assembly is no longer being actuated, the spring 196 expands and biases the first clasp member 172 to move toward the second clasp member 174 and re-engage the lead screw 160.

[0011] The second clasp member 174 is secured to the deck extension 134 and includes a main body portion 198, a first guide 200 protruding from the bottom of the main body portion 198, a guide slot 190 recessed along the top of the main body portion 198, and a receiving portion 202 as shown in FIGS. 5-7. Similar to the first guide 178, the first guide 200 cooperates with slot 186B to maintain alignment of the first and second clasp members 172 and 174. The receiving portion 202 is U-shaped and defines a slot 204 with a non-threaded base 206 recessed into the main body portion 198. The base 206 is not threaded like end 192 of the first clasp member 172 because the second clasp member 174, in this embodiment, is secured to the deck extension 134 and the lead screw 160 remains positioned adjacent to the base 206. Since the lead screw 160 remains positioned adjacent to the base 206, it must be able to rotate freely with respect to the second clasp member 174 when the first

clasp member **172** is disengaged from the lead screw **160**. The lead screw engaging portion **182** is positioned in the slot **204**, the second guide **180** is positioned in the guide slot **190**, and end **192** and base **206** engage the lead screw **160** when the first and second clasp members **172** and **174** are in the engaged position. In some contemplated embodiments, the first and second clasp members **172** and **174** can both move with respect to the deck extension frame **188** and, in that embodiment, the base **206** could be threaded to engage the lead screw **160**.

[0012] The clasp separator **166** is rotatably coupled to the deck extension frame **188** and is configured to move the first clasp member **172** with respect to the deck extension frame **188** and the second clasp member **174** as the clasp separator **166** is rotated as shown in FIGS. 4-8. In one contemplated embodiment, the clasp separator **166** and the threaded clasp **164** are coupled to opposite sides of the deck extension frame **188** (i.e., top and bottom). The clasp separator **166** in this embodiment is semi disc-shaped and includes an curved guide **208** that a follower **210** (such as a fastener coupled to the first guide **178**) travels along as the clasp separator **166** rotates and the first clasp member **172** moves with respect to the deck extension frame **188**. In some contemplated embodiments, the clasp separator **166** is disc shaped and includes two curved guides that engage followers coupled to the first clasp member **172** and the second clasp member **174** and cause the first and second clasp members **172** and **174** to both move with respect to the deck extension frame **188** and disengage the lead screw **160**. A spring **212** is coupled between the clasp separator **166** and a portion of the deck extension frame **188** and configured to help return the clasp separator **166** to the engaged position (where the first clasp portion **172** engages the lead screw **160**) from a disengaged position (where the first clasp portion **172** is disengaged from the lead screw **160**) when the manual release assembly **158** is no longer being actuated.

[0013] The handle **170** is pivotably coupled to the deck extension frame **188** such that it can be easily accessed by a user as shown in FIGS. 4-8. The cable **168** is connected to the handle **170** and to a side of the clasp separator **166** and is configured to cause the clasp separator **166** to rotate with respect to the deck extension frame **188** by creating a rotational moment about the rotational axis of the clasp separator **166** when the handle **170** is pulled by a user. When the user releases the handle **170**, the rotational moment caused by the cable **168** is relieved and spring **196** expands (and spring **212** contracts), creating a reverse rotational moment about the rotational axis of the clasp separator **166** and moving the first clasp member **172** into engagement with the lead screw **160**. In some contemplated embodiments, the cable **168** could be connected directly to the first clasp member **172** and configured to move it with respect to the deck extension frame **188**.

[0014] The mattress **112** includes a mattress core **214** and mattress side bolsters **216** on either side of the mat-

tress core **214**, and a cover **218** enclosing the mattress core **214** and side bolsters **216** as shown in FIGS. 9 and 10. In some contemplated embodiments, the mattress **112** also includes length bolsters at the foot end of the mattress **112** (such as those used with the Flexa-foot™ feature sold by Hill-Rom). In some contemplated embodiments, the mattress **112** is part of a mattress replacement system (MRS system). One example of a mattress replacement system is the Envision® E700 Low-Air Loss Therapy Surface sold by Hill-Rom. In one contemplated embodiment, the mattress core **214** includes a combination of static components (i.e., static fluid bladders or foam) and dynamic components (i.e., inflatable fluid bladders **220**), and the mattress side bolsters **216** include at least one inflatable fluid bladder **220** or chamber.

[0015] The fluid bladders **220** are in fluid communication with a fluid supply system **222** configured to supply fluid to inflate the bladders **220**, or create a vacuum to deflate the bladders **220**. In one contemplated embodiment, the fluid supply system **222** is configured to inflate/deflate the fluid bladders **220** in the mattress side bolsters **216** in response to the control system **114** sensing an increase/decrease in the width of the person support apparatus **110** or receiving an input from a user indicating a desire for the width of the person support apparatus **110** or the mattress **112** to be increased/decreased. The fluid supply system **222** includes a fluid supply or gas blower **224** that is connected to the fluid bladders **220** by hoses **226**. In some contemplated embodiments, the fluid supply **224** may be a compressor or a pump. The fluid supply **224** is contained within a mattress control box **228** that is hung from the footboard **122**.

[0016] The control system **114** shown in FIGS. 11-13 is configured to control operation of the powered extension/retraction system **156** and fluid supply system **222** in response to an input from the user corresponding to a desired change in width of the person support structure **100** in order to extend/retract the deck extensions **134** and inflate/deflate the side bolsters **220**, respectively. In some contemplated embodiments, other functions of the person support apparatus **110** and/or the mattress **114** may be controlled by the control system **114**, such as, for example, articulation and height adjustment, therapies and alarms. The control system **114** includes a person support apparatus controller or bed controller **230**, a person support apparatus control interface or bed control interface **232**, person support apparatus sensors or bed sensors **234**, a mattress controller **236**, mattress control interface **238**, and mattress sensors **240**. The bed controller **230** is configured to control at least one function of the person support apparatus **110** in response to a user input received via the bed control interface **232** or in response to manual operation to alter the width of a deck section **134** (e.g., a person actuating the manual release assembly **158** and pushing or pulling on the deck extension **134** or the siderail **138** to extend/retract the deck extension **134** manually). The bed controller **230**

includes a bed controller processor **242** and a bed controller memory **244**. The bed control interface **232** is in communication with the bed controller processor **242** which is configured to receive a signal indicative of selection of the button **248**. The bed controller memory **244** is configured to store procedures to be executed by the bed controller processor **242** and information regarding the status of the person support apparatus **110**, including the position of at least one of the deck extensions **134**, threshold values of position which would indicate full extension or retraction, and information received from the bed sensors **234** and bed control interface **232**. In one contemplated embodiment, when the deck extension **134** is fully retracted or extended it hits a mechanical stop causing a surge in electric current to the motor **162** which is recorded by the bed controller **230** and used to determine whether the deck extensions **134** are completely extended or retracted.

[0017] The bed sensors **234** are configured to sense characteristics of the bed components, such as, the position of the deck extensions **134** (fully extended/retracted), the position of the siderail **138** (deployed/storage), and the orientation of the deck sections **132**. The bed sensors **234** can include potentiometers, limit switches, hall-effect sensors, or other similar sensing devices and techniques. The bed sensors **234** can be coupled to the extensions **134** and/or the motors **162** or sense the position of the deck extensions **134** with respect to the deck sections **132**. In one contemplated embodiment, potentiometers are mounted on the shafts of the motors **162** to sense the motion of the deck extensions **134** and allow the bed controller **230** to track the position of the extensions **134**. In some contemplated embodiments, the sensors **234** also include force sensors, pressure sensors, and other sensors configured to sense characteristics and statuses of other systems and components of the person support apparatus **110**.

[0018] The bed control interface **232** shown in FIGS. **1** and **11-13** is removably mounted on the siderail **138** in one contemplated embodiment. The bed control interface **232** includes a display **246** configured to display alerts and visual messages to a viewer, and at least one button **248** to control the extension and retraction of at least one deck extension **134**. The display **246** in one embodiment is a Liquid Crystal Display (LCD) screen although any other technology could be used in other embodiments. The button **248** is a physical push button while in another embodiment the display **246** is a touch sensitive screen and button **248** is displayed on the touch sensitive screen. The bed control interface **232** shown in FIG. **13** may employ a button **248** for commanding both extension and retraction while in other embodiments the bed control interface **232** may comprise one button for commanding extension **248E** and a separate button for commanding retraction **248R**. The control interface **232** also has indicator lights **250E** and **250R**. When the extensions **134** are fully extended, light **250E** glows steady green and light **250R** is off. When the extensions **134** are

fully retracted, light **250R** glows steady green and light **250E** is off. When the extensions **134** are in an intermediate state (neither fully extended nor fully retracted) one or both of the lights **250E** and **250R** flashes amber.

[0019] The mattress control interface **238**, as shown in FIGS. **11** & **12**, is coupled to the mattress control box **228** and is configured to display alerts and visual messages to a viewer. In some contemplated embodiments, the alerts and visual messages provide information about the status of the mattress **112**, the fluid supply **224**, and therapies being provided by the mattress **112**. In one contemplated embodiment, the mattress control interface **238** is constructed like the bed control interface **232** above and includes a display **256** and at least one button **258** to control the extension and retraction of the side bolsters **216**. The mattress control interface **238** can also include buttons for controlling other functions of the mattress **112**, including, activating/deactivating therapies and increasing/decreasing pressure within the fluid bladders **220**.

[0020] The mattress controller **236** is configured to control the fluid supply system **222** in response to a user input provided via the mattress control interface **238** (or via the bed control interface **232** when the mattress controller **236** and the bed controller **230** are in communication with one another). The mattress controller **236** includes a mattress controller processor **252** and mattress controller memory **254** as shown in FIGS. **11** & **12**. The mattress controller memory **254** is configured to store procedures that may be executed by processor **252** and information regarding the status of the mattress **112**, including the pressure within the side bolsters **216**, threshold values of pressure which would indicate full inflation or deflation of the side bolsters **216**, and information received from the mattress sensors **240** or mattress control interface **238**. The mattress controller **236** is enclosed in the mattress control box **228** and is electrically coupled to the fluid supply **224**, the mattress control interface **238**, and the mattress sensors **240**. In some contemplated embodiments where the mattress **112** is integrated with the person support apparatus **110**, the mattress controller **236** may be located with the bed controller **230**, or combined with the bed controller **230** such that the bed controller **230** may be used to control functions of both the person support apparatus **110** and the mattress **112**.

[0021] The mattress sensors **240** are configured to sense various characteristics of the mattress components, such as, the fluid pressure within the side bolsters **216** (fully extended/retracted), and to provide the sensed information to the mattress controller **236**. In one contemplated embodiment, the mattress sensors **240** include pressure transducers that are configured to provide a signal indicative of the pressure inside the side bolsters **216** so that the mattress controller **236** can determine the inflation level of the side bolsters **216** (i.e., when they are fully deflated or fully inflated or partially inflated). In other contemplated embodiments, the mattress sensors **240** include temperature sensors, moisture sensors,

force sensors, and other sensors, coupled to the mattress **112** to sense characteristics of the mattress **112**, the fluid bladders **220**, and/or the person positioned on the mattress **112**. When the deck extensions **134** are retracted manually, the side rails **138** apply pressure on the side bolsters **216** as a user pushes the siderail **138** against the mattress **112**, which causes a signal from the pressure transducer **240** to indicate a spike in pressure. If the mattress controller **236** determines that the spike is greater than a predetermined threshold, then the mattress controller **236** causes the fluid supply **224** to initiate deflation of the side bolsters **216**.

[0022] The mattress controller **236** and the bed controller **230** are configured to communicate with one another to affect the extension/retraction of the deck extensions **134** and side bolsters **216**. In some contemplated embodiments, the mattress controller **236** is configured to use the bed controller **230** as a communication hub to communicate information about the mattress **112** to caregivers via nurse call systems, to electronic medical record systems, and to other devices and systems. In the case of a mattress replacement system, the mattress controller **236** is in electrical communication with the bed controller **230** via a wired or wireless connection. In one contemplated embodiment, the mattress controller **236** communicates alarm signals to the bed controller **230** so that, instead of an alarm on the control box **228** being activated to alert people in or near the patient's room, a remote caregiver can be notified by the nurse call system of the alert. In other contemplated embodiments, the mattress controller **236** can communicate patient position information, therapy history (which can be used for compliance tracking), cushion pressures (which can indicate a fluid supply **32** issue or a leak), and/or other information about the mattress **16** or patient positioned thereon to a caregiver over a nurse call system or other caregiver alert system, an electronic medical record system, or the person support apparatus **110** or other medical devices in communication with the person support apparatus **110**.

[0023] In one contemplated embodiment, when the mattress controller **236** is in electrical communication with the bed controller **230**, the mattress control interface **238** on the control box **228** is disabled and the bed control interface **232** is used to control the functions of both the person support apparatus **210** and the mattress **112**. In some contemplated embodiments, the mattress control interface **238** on the control box **228** does not display any information when it is deactivated. In another contemplated embodiment, the mattress control interface **238** can display information and/or errors, but control functions are locked out so that the user cannot control the operation of the mattress **112** from it. In some contemplated embodiments, the bed control interface **232** could be locked out instead of the mattress control interface **238**. In some contemplated embodiments, the controls for inflating/deflating the side bolsters **216** from the bed control interface **232** and the mattress control interface **238** are disabled since the function is controlled as part

of the width adjustment algorithm.

[0024] The mattress controller **236** and bed controller **230** periodically exchange a status signal to determine if they are connected. When communication between the bed controller **230** and the mattress controller **236** is interrupted, the mattress control interface **238** on the control box **228** is enabled (or re-activated) and allows the user to control the operation of the mattress **112**. In some contemplated embodiments, visual and/or audible indicators are used to indicate when communication between the bed controller **230** and the mattress controller **236** is lost or interrupted; the loss of communication is sensed as an event, not a status. In another contemplated embodiment, when communication between the bed controller **230** and the mattress controller **236** is interrupted, the side bolsters **216** are deflated and retracted. A user may, subsequently, extend the side bolsters **216** to a desired position by pressing the corresponding button **258** on the mattress control interface **238**. In another contemplated embodiment when communication between the bed controller **230** and the mattress controller **236** is lost, the deck extension/retraction function is locked out to prevent the user from using the powered extension/retraction system **156** to retract the deck section **134** and the mattress controller **236** maintains the mattress **112** in the state it was in prior to the mattress controller **236** losing communication with the bed controller **230**.

[0025] In operation, the bed controller **230** and mattress controller **236** determine whether they are connected and, if so, the mattress controller **236** disables the mattress control interface **238** and routes all mattress control functions to the bed control interface **232**. When the bed control interface **232** receives input indicative of a user's desire to increase or decrease the width of the person support apparatus **110** and mattress **112**, the bed controller **230** activates the powered extension/retraction system **156** on the person support apparatus **110** to move the deck extensions **134** in the desired manner, and provides the mattress controller **236** with the information corresponding to the user's desired action. The mattress controller **236** uses the information from the bed controller **230** to control the operation of the fluid supply **224** to inflate/deflate the side bolsters **216**. If the user does not fully extend or retract the deck extensions **134**, the bed controller **230** sends a signal to the mattress controller **236** and the mattress controller **236** causes the side bolsters **216** to deflate and retract (or to maintain the fully retracted position). The user can manually override the deflation/retraction of the side bolsters **216** by controlling the mattress **112** directly through the mattress control interface **238**. In some contemplated embodiments, if communication between the controllers is interrupted at any time, the side bolsters **216** are deflated and retracted.

[0026] A flow chart **260** of a method of monitoring the connection between the bed controller **230** and the mattress controller **236** according to one contemplated embodiment is shown in FIG. **15**. In one contemplated em-

bodiment, the procedure for monitoring the connection between the bed controller **230** and mattress controller **236** loops continuously. At operation **262**, a determination is made the bed controller **230** and mattress controller **236** as to whether the controllers are in communication with one another. This can be accomplished when either controller fails to receive a periodic status signal from the other controller. If the controllers are in communication, then the mattress **112** is controlled through the mattress control interface **238** and the person support apparatus **110** is controlled through the bed interface **232** at step **264**. The controllers return to monitoring the status of the connection between them at operation **262**.

[0027] If the controllers are in communication, then the mattress control interface **238** is disabled (or at least the function control buttons are deactivated while information and alerts are still able to be displayed) and the mattress **112** is controlled through the bed control interface **232** at step **266**. The controllers return to monitoring the status of the connection between them in operation **268** to determine if communications between the controllers is interrupted. If the communication between the controllers is not interrupted, the mattress control interface **238** remains disabled and the mattress **112** continues to be controlled through the bed control interface **232** at step **270**, and the controllers return to monitoring the status of the communication connection at operation **268**. In one contemplated embodiment, if the communication is interrupted, then a visual and/or audible alert is generated to indicate that communications have been interrupted between the controllers at operation **272**, the mattress controller **238** maintains the status of the mattress **112** just prior to communication between the controllers being interrupted, and the bed controller **230** disables the powered width expansion function at operation **274** before proceeding to operation **264**. In another contemplated embodiment, if communication is interrupted, a visual and/or audible alert is generated to indicate that communications have been interrupted between the controllers and the mattress controller **236** retracts the side bolsters **216** by deflating them before proceeding to operation **264**.

[0028] A flowchart **276** of a method of decreasing and increasing the width of a person support apparatus **110** according to one contemplated embodiment is shown in FIGS. 16 and 17, respectively. At operation **278**, a determination is made by the bed controller **230** as to whether the deck extensions **134** are completely extended. If the deck extensions **134** are completely extended, the bed controller **230** senses selection of the retraction button **248R** in operation **280** after which the system waits for a predetermined time, in one embodiment 2 seconds, in other embodiments, any amount of time in operation **282**. The bed controller **230** sends a signal to the mattress controller **236** to deflate the mattress side bolsters **216** in operation **284**. Mattress controller **236** monitors deflation of the mattress side bolsters **216** in operation **286**. Mattress controller **236** determines if the mattress side

bolsters **216** are completely deflated in operation **288**. In one embodiment the mattress controller **236** makes this determination by comparing a pressure derived from the signal supplied by pressure transducer **240** with a predetermined threshold which in one embodiment may be defined by a user through control interface **232**. In another embodiment the mattress controller **236** determines if the mattress side bolsters **216** are completely deflated by tracking the time spent deflating the mattress side bolsters **216**. If the mattress controller **236** determines that the mattress side bolsters **216** are not completely deflated it sends a corresponding signal to the bed controller **230** at operation **290**. The bed controller **230** sends the signal to the control interface **232** through which an audio indication and / or a visual indication on display **246** of ongoing mattress side bolster **216** deflation is communicated. If mattress controller **236** determines that deflation is complete at block **290** it communicates with the bed controller **230**. The bed controller **230** sends a signal to the control interface **232** through which an audio indication and / or a visual indication on display **246** of completion of mattress side bolster **216** deflation is communicated in operation **292**. The bed controller **230** now checks to determine whether retraction button **248R** is selected at operation **294**. If not, the bed controller **230** communicates a signal to the control interface **232** to display a message indicating that the mattress side bolsters **216** are deflated. If the bed controller **230** determines that the retraction button **248R** is selected, it sends a signal to motors **162** coupled to the upper body deck section **140** and the lower body deck sections **142**, **144**, and **146** to begin retracting the deck extensions **134**; the bed controller **230** monitors actuation of the deck extensions **134** in operation **296**. In one contemplated embodiment, the deck extensions **134** are prevented from retracting if the deck sections **132** are in an articulated configuration. In another contemplated embodiment, articulation of the deck sections **132** is disabled while the extensions **134** are being extended/retracted. In another contemplated embodiment, extension/retraction of the deck extensions **134** and inflation/deflation of the side bolsters **216** are performed substantially simultaneously.

[0029] During actuation of the deck extensions **134**, the bed controller **230** determines whether the deck extensions **134** are staggered in operation **298**. In one contemplated embodiment, the bed controller **230** can determine whether the deck extensions **134** are staggered based on information sensed by the bed sensors **234** (for example, in one embodiment the bed sensors **234** include limit switches, while in another embodiment the bed sensor **234** include a potentiometer coupled to the motors **162** which the controller **230** can use to calculate the positions of the extensions **134**). In another contemplated embodiment, the bed controller **230** can determine whether the deck extensions **134** are staggered by examining whether the motors **162** are synchronized where actuation of one extension **134** was delayed when compared the other extension **134**. Staggering of the deck

sections **134** can be achieved a number of ways. In one contemplated embodiment, the upper body deck extension **148** is retracted at faster speed than the lower body deck sections **150**, **152**, and **154**, and extended at a slower speed than the lower body deck sections **150**, **152**, and **154** to stagger the extensions **134** such that the siderails **138** coupled thereto are not co-planar until the extensions **134** are fully extended. In another contemplated embodiment, the lower body deck extension **150**, **152**, and **154** and the upper body deck extension **148** are extended/retracted at substantially the same speed, but retraction of the lower body deck extensions **150**, **152**, and **154** are started a predetermined amount of time after retraction of the upper body deck extension **148**, and extension of the lower body deck extensions **150**, **152**, and **154** are started at a predetermined time before extension of the upper body deck extension **148**. Staggering the movement of the deck sections **134** helps to prevent potential interferences between the siderails **138** coupled to the deck sections **134** when the person support apparatus **110** is articulated.

[0030] The bed controller **230** monitors whether the end of travel indicative of complete retraction of deck extensions **134** has been reached based on signals from the potentiometer and/or current readings from the motors **162** in operation **300**. In one contemplated embodiment, each extension **134** is extended/retracted to its limit irrespective of the staggering of the extensions **134**. In another contemplated embodiment, the extensions **134** are extended/retracted until the first extension **134** reaches its limit, which maintains the extensions **134** in a staggered state. If the bed controller **230** determines complete extension/retraction of the deck extensions **134** has been reached, the bed controller **230** sends a signal to the motors **162** to stop actuation. If the bed controller **230** determines that the deck extensions **134** have not been completely extended/retracted upon the occurrence of a condition, the bed controller **230** can cause the person support apparatus **110** or mattress **112** to perform or lock out various functions. In one contemplated embodiment, the conditions include the user releasing the button **248** prior to the extensions **134** being fully extended/retracted, a bed power cord being unplugged, or the person support apparatus **110** being powered by a battery system (in one contemplated embodiment, the mattress controller **236** and fluid supply **224** are not powered by the person support apparatus **110** battery and the side bolsters **216** cannot be deflated or inflated when the person support apparatus **110** is running on the battery). When one of the aforementioned conditions occur it can cause the bed controller **230** to lock out articulation of the deck sections **132**, generate an audible alarm, and/or flash an amber colored light **250** on the bed control interface **232**. The bed controller **230** is also configured to generate fault codes for display on the bed control interface **232** or using diagnostic LEDs when, for example, the extension and retraction limits are not reached within a predetermined time, movement of the extension

134 is not sensed after the bed controller **230** sends a signal to the motor **162** to extend/retract the extension **134**, the motor **162** is disconnected from the circuit, the bed sensors **234** or mattress sensors **240** signals are outside of an expected range, or the extend and retract limits are simultaneously met. When the fault codes are generated, the bed controller **230** can lock out the width expansion function and/or generate an audible alert or flash the light **250** to alert the user. In some contemplated embodiments, the sensors **234** and **240** are monitored real time and the position of each extension **134** is calculated at all times whether moving or stationary. In this embodiment, if the deck extensions **134** are not extended/retracted completely, the control system **114** determines whether the extensions **134** are substantially aligned. If they are not, then articulation of the deck sections **132** is prevented (specifically raising the upper body deck section **140** is prevented).

[0031] At operation **302**, a determination is made by the bed controller **230** as to whether the deck extensions **134** are completely retracted. In one contemplated embodiment, if the deck extensions **134** are not completely extended or retracted, then the bed controller **230** generates an audible and/or visual alert and disables articulation of the deck sections **132**. In this embodiment, raising the upper body deck section **140** can be disabled while lowering the upper body deck section **140** can still be enabled. In another contemplated embodiment, if the deck extensions **134** are not completely extended or retracted, then the bed controller **230** sends a signal to the mattress controller **236** to cause the side bolsters **216** to retract. If the deck extensions **134** are completely retracted, the bed controller **230** checks to determine whether extension button **248E** is selected at operation **306**. If the bed controller **230** determines that the extension button **248E** is selected, it sends a signal to upper body deck width motor **162** and lower body deck width motor **162** to begin extending the deck extensions **134**; the bed controller **230** monitors actuation of the deck extensions **134** in operation **308**. During actuation of the deck extensions **134**, the bed controller **230** determines whether the deck extensions **134** are staggered in operation **310**. If the bed controller **230** determines that the deck extensions **134** are not staggered, it sends a signal to the control interface **232** to display an error message. In some contemplated embodiments, the controller **230** can modify the speed at which the motors **162** are extending or retracting the extensions **134** to generate the desired stagger. If the bed controller **230** determines that the deck extensions **134** are staggered, the bed controller **230** monitors whether the end of travel indicative of complete extension has been reached based on signals from the potentiometer **234** and/or current readings from the motors **162** in operation **144**. If the bed controller **230** determines that complete extension of each deck extension **134** has been reached, the bed controller **230** sends a signal to the motors **162** to stop actuation. If the bed controller **230** determines that the deck extensions **134** have not been

completely extended, the bed controller **230** continues to monitor whether the motors **162** are staggered in step **310**.

[0032] In operation **312** if it is determined by the bed controller **230** that the deck extensions **134** are completely extended, the bed controller senses selection of the extension button **248E** in operation **314** after which the system waits for a predetermined time, in one embodiment 2 seconds, in other embodiments, any amount of time in operation **316**. The bed controller **230** sends a signal to the mattress controller **236** to inflate the mattress side bolsters **216** in operation **318**. Mattress controller **236** monitors inflation of the mattress side bolsters **216** in operation **320**. Mattress controller **236** determines if the mattress side bolsters **216** are completely inflated in operation **322**. In one embodiment the mattress controller **236** makes this determination by comparing a pressure derived from the signal supplied by pressure transducer **240** with a predetermined threshold which in one embodiment may be defined by a user through control interface **232**. In another embodiment the mattress controller **236** determines if the mattress side bolsters **216** are completely inflated by tracking the time spent inflating the mattress side bolsters **216**. In operation **322** if the mattress controller **236** determines the mattress side bolsters **216** are not completely inflated, it sends a corresponding signal to the bed controller **230**. The bed controller **230** sends a signal to the control interface **232** through which an audio indication and / or a visual indication on display **246** of ongoing mattress side bolster **216** inflation is communicated in operation **324**. If mattress controller **236** determines that inflation is complete it communicates with the bed controller **230**. The bed controller **230** sends a signal to the control interface **232** through which an audio indication and / or a visual indication on display **246** of completion of mattress side bolster **216** inflation is communicated in operation **326**.

[0033] In this embodiment the mattress side bolsters **216** are configured to toggle between a fully inflated state and a fully deflated state. In one embodiment the pressure indicative of full inflation is variable based on weight of the patient supported by the mattress **112** to a predetermined pressure relief set point. In another embodiment the pressure indicative of full inflation may be input by a user via the control interface **232**. In another contemplated embodiment, pressure indicative of full inflation is a function of the position of the extension **134**.

[0034] FIGS. **18** and **19** are block diagrams **328** showing a second method of altering the width of the bed **110** according to another contemplated embodiment. In FIG. **18**, block **330** tests whether or not the bed controller **230** senses that retract button **248R** is being pressed. If not the method proceeds to block **358** of FIG. **19** and tests whether or not the bed controller **230** senses that extend button **248E** is being pressed. However if the test at block **202** reveals that the retract button **248R** is being pressed the method proceeds to block **332**. Pressing either button **248R** or **248E** generates a command to alter the width

of the bed **110**. The commands are of opposite polarity, i.e. one is to retract, the other is to extend.

[0035] Block **332** tests whether or not the deck extensions **134** are at their limit of retraction. If so, the method stops except for continuing the tests of blocks **330** (FIG. **18**) and **358** (FIG. **19**). If the deck extensions **134** are not at their limit of retraction the method proceeds along paths **334A** and **334B** to blocks **352** (FIG. **18B**) and **336** (FIG. **18**) respectively. First considering path **334A**, at block **352** the bed controller **230** monitors whether the deck extensions **134** (which are being moved as a result of a user continuing to press the retract button **248R**) are staggered. If not the method proceeds to block **356** and changes the motors **162** speed to stagger the deck sections **134**. If so the method branches to block **350** (FIG. **18**). Now considering path **334B**, at block **336** the method pauses or delays for a brief time interval (a second or two) while continuing to monitor whether or not the retract button **248R** is still being pressed. If the user has continued to apply pressure to the retract button **248R** throughout the pause interval, the method proceeds to block **338**. However if user pressure on the retract button **248R** is discontinued during the pause interval the method does not proceed to block **338**. The pause interval enables the method to distinguish between a genuine user command and a brief inadvertent touch of the retract button **248R**.

[0036] Block **338** tests whether or not deflation of the side bolsters **216** has begun. If not the bed controller **230** issues a "deflate" command to the mattress controller **236** at block **340**. The mattress controller **236** responds by beginning deflation of the side bolsters **216**. At block **342** the mattress controller **236** monitors deflation progress and proceeds to block **344**. At block **344** the method tests whether or not deflation is complete either as a result of the actions at blocks **340** and **342** or as a result of having arrived directly at block **344** from block **338**. If the test at block **344** reveals that deflation is not complete the method continues the deflation process and sends a visual and/or aural indication of the ongoing deflation. One example of a visual indication is the flashing yellow illumination of one of lights **250E** and **250R** as described above. If the test at block **344** reveals that deflation is complete the method proceeds to block **348** where the mattress controller **236** signals the bed controller **230** that deflation is complete and sends a visual and/or aural indication of the fact that deflation is complete. One example of a visual indication is the steady green illumination of light **250R** as described above.

[0037] Irrespective of whether the method has followed path **334A** through blocks **352** and **354** or has followed path **334B** through the appropriate blocks beyond block **336**, the method arrives at block **350** where it tests whether or not the deck extensions **134** are at their limit of retraction. If not, the method returns to block **330**. If so, the method stops, except for continuing to monitor for whether or not the extend and retract buttons **248E** and **248R** are being pressed.

[0038] The portion of the method outlined in FIG. **19** is

similar to the portion of the method disclosed in FIG. 18 but shows how the method responds to user pressure applied to the extend button 248E. In FIG. 19, block 358 tests whether or not the bed controller 230 senses that extend button 248E is being pressed. If not the method stops, although the test of block 358 (and of block 330 in FIG. 18) continues to be made. However if the test at block 358 reveals that the extend 248E button is being pressed the method proceeds to block 360.

[0039] Block 360 tests whether or not the deck extensions 134 are at their limit of extension. If so, the method stops except for continuing the tests of blocks 330 and 358. If the deck extensions 134 are not at their limit of retraction the method proceeds along paths 362A and 362B to blocks 380 (FIG. 19B) and 364 (FIG. 19) respectively. First considering path 362A, at block 380 the bed controller 230 monitors whether the deck extensions 134 (which are being moved as a result of a user continuing to press the extend button 248E) are staggered. If not the method proceeds to block 384 and changes the speed of the motors 162 to stagger the deck sections 134. If so the method branches to block 378 (FIG. 19). Now considering path 362B, at block 364 the method pauses or delays for a brief time interval (a second or two) while continuing to monitor whether or not the extend button 248E is still being pressed. If the user has continued to apply pressure to the extend button 248E throughout the pause interval, the method proceeds to block 366. However if user pressure on the extend button 248E is discontinued during the pause interval the method does not proceed to block 366. The pause interval enables the method to distinguish between a genuine user command and a brief inadvertent touch of the retract button 248E.

[0040] Block 366 tests whether or not inflation of the side bolsters 216 has begun. If not the bed controller 230 issues a "inflate" command to the mattress controller 236 at block 368. The mattress controller 236 responds by beginning inflation of the side bolsters 216. At block 370 the mattress controller 236 monitors inflation progress and proceeds to block 372. At block 372 the method tests whether or not inflation is complete either as a result of the actions at blocks 368 and 370 or as a result of having arrived directly at block 372 from block 366. If the test at block 372 reveals that inflation is not complete the method continues the inflation process and sends a visual and/or aural indication of the ongoing inflation. One example of a visual indication is the flashing yellow illumination of one of lights 250E and 250R as described above. If the test at block 372 reveals that inflation is complete the method proceeds to block 376 where the mattress controller 236 signals the bed controller 230 that inflation is complete and sends a visual and/or aural indication of the fact that inflation is complete. One example of a visual indication is the steady green illumination of light 250E as described above.

[0041] Irrespective of whether the method has followed path 362A through blocks 380 and 382 or has followed path 362B through the appropriate blocks beyond block

364, the method arrives at block 378 where it tests whether or not the deck extensions 134 are at their limit of extension. If not, the method returns to block 358. If so, the method stops, except for continuing to monitor for whether or not the extend and retract buttons 248E and 248R are being pressed.

[0042] As previously noted the deck extensions 134 can be extended and retracted manually. In the case of manual operation the step of determining whether or not the extend or retract buttons 248E or 248R are pressed (blocks 330 and 358) will not yield a "yes" answer. However the bed controller 230 is still able to monitor current readings or potentiometer 240 signals to track the position of the deck extension 134, including whether or not the deck extension 134 is at its extend limit or retract limit. As a result the method for manual operation is the same except that instead of being initiated by the bed controller 230 sensing whether or not the retract or extend button 248E or 248R is being pressed (blocks 330, 358) it is initiated by changes in the current readings or potentiometer signals. Similar to the case of push-button operation, manual operation generates a width alteration command. If a user pushes on the deck extensions 134 (or a component attached to the deck extensions 134) to cause the deck extensions 134 to retract, the command is a retract command. If a user pulls on the deck extensions 134 (or a component attached to the deck extensions 134) to cause the deck extensions 134 to extend, the command is an extend command. The retract and extend commands are of opposite polarity.

[0043] The foregoing description and associated FIGS. 18 and 19 address retraction and extension explicitly. More generally the method monitors for a command to alter the width of the deck and determines the polarity of the command (blocks 330, 358). The method ensures that the deck extension 134 is not at a limit inconsistent with the polarity of the command (blocks 330, 358), operates powered extension/retraction system 156 to move the deck extension 134 in a direction consistent with the polarity of the command (implicit in blocks 352, 380) and issues a fluid supply control signal (not explicitly shown, but a consequence of blocks 340, 368) to operate the fluid supply 224 in a manner consistent with the polarity of the command. The fluid supply control signal is issued in response to a mattress control signal (output of blocks 340, 368). The mattress control signal is generated in response to the command.

[0044] The method monitors response of the mattress 112 to operation of the fluid supply 224 at blocks 342, 370. The method of curtails operation of powered extension/retraction system 156 in response to the deck extension 134 reaching a limit consistent with the polarity of the command. The issuing step is conditioned on continued presence of the command during a pause interval (blocks 336, 364). The method also includes the step of providing an indication distinguishing between completion and incompleteness of width adjustment (blocks 346, 374).

[0045] Referring principally to FIGS. 5 and 8, an embodiment of upper body section deck extension 148, also referred to as a wing, includes laterally extending spars 402 and a laterally outboard, longitudinally extending rail 404. A bridge 406 spans between the two longitudinally innermost spars 402B, 402C. As already described clasp 164 and clasp separator 166 are mounted to the wing.

[0046] Referring to FIGS. 4-8 and 20-23 an embodiment of the upper frame 118 of a person support apparatus includes an upper body deck section 140 having a framework which includes laterally extending supports configured as C-channels 410. One of each of the wing spars 402A, 402B, 402C, 402D nests within a corresponding C-channel 410A, 410B, 410C, 410D so that the spars are laterally translatable with respect to the channels. The illustrated embodiment includes four wing spars and four C-channels, however other quantities of spars and channels in a one to one correspondence may be used depending on design requirements. Friction reducing elements such as rollers (not visible in the illustrations) are used to reduce friction between the spars and the C-channels. The upper body deck section framework also includes longitudinally extending beams 412. Beam 412C coincides with deck section centerline 416 and may be referred to as a center beam.

[0047] A bearing block 418 projects upwardly from each of the beams except for the center beam. Two bearing blocks 418B, 418D are partially visible in FIG. 20, one extending from a flange portion of beam 412B, the other extending from a flange portion of beam 412D. Two additional bearing blocks, 418A, 418E, are partially visible in FIG. 21, one extending from beam 412A, the other extending from beam 412E. A hole, not visible, extends through each bearing block such that the hole axis is parallel to the leadscrew axis which is shown in FIG. 23. A bushing, also not visible, resides in each bearing block hole. One or more motor mount brackets 422 supports left and right motor assemblies 424L, 424R from the center beam (left and right are taken from the vantage point of a person lying face up on the person support system with his head nearer to the head end of the person support system and his feet nearer the foot end of the person support system).

[0048] Due to symmetry it will suffice to describe only one representative motor assembly (the right motor assembly) and the elements associated with it. Accordingly, the suffixes L and R will be appended to the reference numerals only as needed in the remainder of this description. Referring to FIG. 22 representative motor assembly 424 includes a motor 162 with an output shaft 426 and a worm gear 428 at the end of the shaft. The shaft and worm are rotatable about a motor axis 432 which extends substantially parallel to centerline 416. The motor assembly also includes a pinion 434 engaged with the worm and having a pinion shaft 436 rotatable about a pinion shaft rotational axis 438. Taken together the worm and pinion define a gear train.

[0049] Referring to FIG. 23 an inboard end of lead-

screw 160 includes a spline 450. The leadscrew also includes a drive thread 452 interrupted by inboard and outboard unthreaded segments 454, 456. The terms "inboard" and "outboard" refer to locations laterally closer to or laterally more distant from centerline 416. The spline is engaged with the pinion shaft 436. The leadscrew extends away from the motor assembly and through a clasp 164 on the same lateral side of the bed so that drive threads 452 engage the threads on threaded end 192 of clasp member 172 (FIG. 5). The leadscrew also extends through the bushings in the two bearing blocks 418 on the same lateral side of the bed.

[0050] As seen best in FIG. 20 an inboard ring 464 circumscribes the inboard unthreaded segment 454 of the leadscrew. An outboard ring 466 circumscribes the outboard unthreaded segment 456 of the leadscrew. The unthreaded segments, and therefore the rings, are located on the leadscrew so that outboard ring 466 resides immediately inboard of an outboard bearing block such as bearing block 418A (visible in FIG. 21) or 418E, and so that inboard ring 464 resides immediately outboard of an inboard bearing block such as bearing block 418B or 418D as seen in FIG. 20. The diameter of each ring is large enough that the ring will not pass through the bushing in the adjacent bearing block. As a result the rings prevent the leadscrew from moving parallel to its own axis 420.

[0051] When clasp 164 is engaged as seen in FIG. 6, the clasp acts as a leadscrew receiver. Operation of a motor in a first or forward rotational direction moves the corresponding clasp, and therefore the wing to which the clasp is secured, in a laterally outboard direction. Operation of the motor in a second or reverse rotational direction, opposite that of the first rotational direction, moves the corresponding clasp and wing in a laterally inboard direction. The terms "forward" and "reverse" are used merely to distinguish between opposite rotational senses.

[0052] FIG. 24 is a schematic representation of an architecture having four deck sections, an upper body section 140, a seat section 142 a thigh section 144 and a foot section 146, all four of which are rendered width adjustable by corresponding extension wings 148, 150, 152, 154. Each deck section has a width W and an outboard edge 472. The architecture includes eight motor assemblies 424, two mounted on each of the four deck sections. Two motor assemblies are associated with and dedicated to one and only one of the four sections such that one of the two motor assemblies drives the left leadscrew and the left wing of the section and the other of the two motor assemblies drives the right leadscrew and the right wing of that same section. In general, in a bed having at least two deck sections, and in which at least two of those sections are width adjustable sections, each section is serviced by its own pair of motor assemblies. Each motor can move its corresponding wing between a deployed position in which the lateral extremity 470 of the wing is outboard of the outboard edge 472 of the

corresponding deck section and a stored position in which the lateral extremity **470** is inboard of its deployed position as shown in phantom in FIG. **24** for one of the foot section extensions **154**. When the wing is stored its outboard extremity **470** may be outboard of, inboard of, or substantially laterally aligned with outboard edge **472** of the corresponding deck section.

[0053] FIG. **25** shows an alternative in which the wings of at least two of the deck sections are movable by a common or shared motor assembly. For example, a right motor assembly **424R** is connected to thigh deck segment **144**. Wing **152R** of section **144** is a directly driven wing because it is driven directly by the motor assembly. Wing **150R** of the seat section is an indirectly driven wing connected to the directly driven wing **152R** by a link **474** which conveys the lateral motion of the directly driven wing **152R** to the indirectly driven wing **150R**. Wing **154R** of the foot section is similarly an indirectly driven wing. Motor assembly **424R** of section **144** is considered to be a shared motor assembly because its driving energy is shared by at least two wings, the directly driven wing **152R** and the indirectly driven wings **150R** and/or **154R**. Wings **150R**, **154R** are also considered to be proximate indirectly driven wings because they are immediately adjacent to a directly driven wing. Section **144** may be referred to as a directly driven section. Section **140** may also be referred to as a directly driven section, and its wings **148** as directly driven wings even though wings **148** are not connected to longitudinally adjacent wings such as wings **150**. Sections **142**, **146** may be referred to as indirectly driven sections or as indirectly driven proximate sections.

[0054] FIG. **26** shows another alternative in which the wings of at least two of the width adjustable segments are movable by a common or shared motor assembly. A motor assembly **424R** is mounted on seat deck segment **142**. Wing **150R** of section **142** is a directly driven wing because it is driven directly by motor assembly **424R**. Wing **152R** of the thigh section is an indirectly driven wing connected to directly driven wing **150R** by a link **474** which conveys the lateral motion of the directly driven wing **150R** to the indirectly driven wing **152R**. Wing **154R** of the foot section is also an indirectly driven wing, but because it is adjacent to another indirectly driven wing (wing **152R**) rather than adjacent to a directly driven wing (wing **150R**) wing **154R** is considered to be a remote indirectly driven wing. Section **142** may be referred to as a directly driven section. Section **140** may also be referred to as a directly driven section, and its wings **148** as directly driven wings even though wings **148** are not connected to longitudinally adjacent wings such as wings **150**. Section **144** may be referred to as an indirectly driven section or as an indirectly driven proximate section to distinguish it from section **146**. Wings **152** may similarly be referred to as indirectly driven wings or, to distinguish them from wings **154**, as indirectly driven proximate wings. Section **146** may be referred to as an indirectly driven section or, in order to distinguish it from section

144, as an indirectly driven remote section.

[0055] Embodiments of the invention can be described with reference to the following numbered clauses, with preferred features laid out in the dependent clauses:

1. A bed comprising:

a deck section having a width and left and right outboard deck edges;
a left side wing and a right side wing, both movably coupled to the deck section and each having a laterally outboard extremity;
a left leadscrew receiver mounted on the left wing and a right leadscrew receiver mounted on the right wing;
a left motor assembly and a right motor assembly both mounted on the deck section;
a left leadscrew coupled to the left motor assembly and to the left leadscrew receiver, and a right leadscrew coupled to the right motor assembly and to the right leadscrew receiver;
wherein motor operation is capable of moving the wing to which it is coupled between a deployed position in which the lateral extremity of the wing is outboard of the respective outboard edge of the deck section and a stored position in which the lateral extremity of the wing is inboard of its deployed position.

2. The bed of clause 1 in which when the wing is in its stored position the lateral extremity thereof is outboard of the outboard edge.

3. The bed of clause 1 in which when the wing is in its stored position the lateral extremity thereof is substantially aligned with the outboard edge.

4. The bed of clause 1 in which when the wing is in its stored position the lateral extremity thereof is inboard of the outboard edge.

5. The bed of clause 1 wherein the deck section includes a framework comprised of longitudinally spaced apart channels, and each wing comprises longitudinally spaced apart spars in a one to one correspondence with the channels, each spar and corresponding channel being in a nested relationship with each other, the spars being translatable in a lateral direction relative to the channels.

6. The bed of clause 1 wherein the motor assembly includes a gear train.

7. The bed of clause 1 wherein the wings of the deck section are directly driven wings and the bed comprises at least one adjacent deck section having left and right indirectly driven wings coupled to the directly driven wings such that lateral translation of the directly driven wings causes lateral translation of the indirectly driven wings.

8. The bed of clause 1 wherein the deck section is a directly driven section and the wings of the directly driven deck section are directly driven wings, and

the bed comprises:

at least one proximate deck section adjacent to the directly driven deck section, the proximate section having left and right indirectly driven proximate wings coupled to the directly driven wings such that lateral translation of the directly driven wings causes lateral translation of the indirectly driven proximate wings, and at least one remote deck section non-adjacent to the directly driven deck section and adjacent to the indirectly driven proximate section, the remote section having left and right indirectly driven remote wings coupled to the indirectly driven proximate wings such that lateral translation of the directly driven wings causes lateral translation of the indirectly driven proximate wings and of the indirectly driven remote wings.

9. The bed of clause **1** wherein the leadscrew receiver is a clasp which can be engaged with and disengaged from the leadscrew.

10. The bed of clause **1** comprising:

an extension wing movement mechanism; and a release unit including a clasp comprising a first clasp portion movably coupled to the wing and a second clasp portion fixedly coupled to the wing, the release unit configured to transition between:

- a) an engaged state in which the release unit engages a portion of the movement mechanism and is moved by the movement mechanism to cause the wing to translate relative to the deck section; and
- b) a disengaged state in which the release unit is disengaged from the portion of the movement mechanism.

11. The bed of clause **10** wherein disengagement of the release unit from the portion of the movement mechanism renders the wing translatable independently of the wing movement mechanism.

12. The bed of clause **10** wherein the movement mechanism comprises a leadscrew having a rotational axis and a leadscrew driver coupled to the leadscrew for rotating the leadscrew about its axis.

13. The bed of clause **10** wherein the first clasp portion includes a threaded end that engages a thread of the leadscrew in the engaged state and is disengaged from the leadscrew thread in the disengaged state.

14. The bed of clause **10** wherein the second clasp portion includes a non-threaded slot configured to engage the lead screw.

15. The bed of clause **10** wherein the release unit includes a clasp separator rotatably coupled to the

wing and configured to move the first clasp portion with respect to the second clasp portion as the clasp separator rotates with respect to the extension wing.

16. The bed of clause **15**, wherein the clasp separator includes at least one guide slot.

17. The system of clause **15**, wherein the clasp separator includes two guide slots and is configured to move both clasp portions with respect to the extension wing.

18. The bed of clause **10** comprising a control system configured to determine engagement status of the release unit and trigger a response as a function of the engagement status.

19. The bed of clause **18**, wherein the response includes alerting a user as to the engagement status of the release unit.

20. The bed of clause **1** comprising a control system configured to sense the position of the wing and alert a user when the wing is in a deployed position in which a lateral extremity of the wing is outboard of the outboard edge and a stored position in which the lateral extremity is inboard of its deployed position.

21. The bed of clause **1** including a control system which includes limit switches configured to sense when the wing is in one of the deployed position and the stored position.

22. The bed of clause **1** comprising:

- a first controller configured to control a function of a person support apparatus, the first controller configured to receive a first input corresponding to a function of the person support apparatus via a first user interface; and
- a second controller configured to control a function of a person support surface, the second controller configured to:

- a) receive a second input corresponding to a function of the person support surface via a second user interface when the first controller is not in communication with the second controller, and to

- b) receive a third input corresponding to a function of the person support surface via the first controller when the first controller is in communication with the second controller, wherein the second controller is configured to control a function of the person support surface in accordance with the third input when the first controller is in communication with the second controller.

23. The bed of clause **22**, wherein the first controller is configured to receive a fourth input corresponding to a function of the person support surface via a first user interface when the first controller is in communication with the second controller.

24. The bed of clause **22**, wherein the second user

interface is disabled when the first controller is in communication with the second controller.

25. The bed of clause **22**, wherein the second user interface is enabled when communication between the first controller and the second controller is interrupted.

26. The bed of clause **22**, wherein the second user interface is configured to display information when the first controller is in communication with the second controller.

27. The bed of clause **22**, wherein the second user interface is configured to lock out function controls when the first controller is in communication with the second controller.

28. The bed of clause **22**, wherein the first user interface does not include function controls for the person support surface.

29. The bed of clause **22**, wherein at least one of the first user interface and the second user interface displays an error when the first controller is not in communication with the second controller.

30. The bed of clause **1** wherein the deck section and its left and right wings are elements of a person support apparatus and the bed comprises a person support surface configured to be supported on the person support apparatus and including a width extension assembly; and

a controller configured to control the width extension wing and the width extension assembly in response to an input from a user, such that the width extension assembly of the person support surface remains in a retracted position unless the corresponding width extension wing of the person support apparatus is positioned in one of a fully retracted position and a fully extended position.

31. The bed of clause **30** wherein:

the person support apparatus includes an apparatus length extension assembly;
the person support surface includes a surface length extension assembly; and wherein:

the controller is configured to cause at least one of the width extension wing and the apparatus length extension assembly and at least one of the width extension assembly and the surface length extension assembly to move in response to an input from a user, wherein the at least one of the surface length extension assembly and the width extension assembly of the support surface remains in a retracted position unless the corresponding one of the at least one of the width extension wing and apparatus length extension assembly of the support apparatus is positioned in one of a fully retracted position and a fully extended position.

32. The bed of clause **30** wherein an alarm is generated if the width extension assembly is not in one of a fully extended position or a fully retracted position.

33. A system for changing width of a person support apparatus, comprising:

a bed controller configured to receive a command signal indicative of a command for width alteration;

a first motor configured to be controlled by the bed controller, the first motor configured to alter the width of at least a portion of a first deck section of the support apparatus;

a second motor configured to be controlled by the bed controller, the second motor configured to alter the width of at least a portion of a second deck section of the support apparatus, wherein:

the bed controller controls the first motor and the second motor in a manner that causes the first deck section to reach a width alteration limit at a first time and the second deck section to reach a width alteration limit at a second time, wherein the first time and the second time are not equal.

34. The system of clause **33**, wherein the first motor and the second motor are controlled to operate at different speeds.

35. The system of clause **33** wherein the first motor is controlled to alter the width of at least a portion of the first deck section at a first time and the second motor is controlled to alter the width of at least a portion of the second deck section at a second time after the first time.

36. The system clause **33** wherein the bed controller activates the first motor, waits a predetermined amount of time, and then activates the second motor.

37. The system of clause **33** wherein the first deck section and the second deck section are prevented from being articulated until both the at least a portion of the first deck section and the at least a portion of the second deck section reach respective width alteration limits.

38. The system of clause **37** wherein the width alteration limit is defined by a deck extension wing in the fully extended position or the fully retracted position.

39. The system of clause **37** wherein the width alteration limit includes the at least a portion of a first deck section being in a fully extended position or a fully retracted position.

40. The system of clause **37** wherein the bed controller generates an alarm if a distal end of a first deck extension wing and a distal end of a second deck section are not staggered such that the distal ends of the respective extension wings reach their respective width alteration limits at different times.

41. The system of clause **33** comprising
a mattress controller configured to communicate
with the bed controller;
a fluid supply device configured to be controlled by
the mattress controller; and
a mattress configured to be supported by the deck
sections, the mattress comprising at least one cham-
ber fluidly connected to the fluid supply device and
configured to be inflated by the fluid supply device
upon the fluid supply device receiving a fluid supply
control signal from the mattress controller.
42. The system of clause **41** wherein the bed con-
troller further comprises a bed controller processor.
43. The system of clause **42** wherein the mattress
controller further comprises a mattress controller
processor configured to communicate with the bed
controller processor.
44. The system of clause **41** wherein the bed con-
troller sends a motor control signal to a motor to stop
actuation of at least one deck section extension wing
based on a signal representative of pressure inside
the chamber.
45. The system of clause **41** wherein the mattress
controller issues the fluid supply control signal to the
fluid supply device in response to the mattress con-
troller receiving a mattress control signal from the
bed controller.
46. The system of clause **33** wherein the command
signal is generated in response to manual operation
to alter the width of the at least a portion of a deck
section.

Claims

1. A bed comprising:

a deck section having a width and left and right
outboard deck edges;
a left side wing and a right side wing, both mov-
ably coupled to the deck section and each hav-
ing a laterally outboard extremity;
a left leadscrew receiver mounted on the left
wing and a right leadscrew receiver mounted on
the right wing;
a left motor assembly and a right motor assem-
bly both mounted on the deck section;
a left leadscrew coupled to the left motor assem-
bly and to the left leadscrew receiver, and a right
leadscrew coupled to the right motor assembly
and to the right leadscrew receiver;
wherein motor operation is capable of moving
the wing to which it is coupled between a de-
ployed position in which the lateral extremity of
the wing is outboard of the respective outboard
edge of the deck section and a stored position
in which the lateral extremity of the wing is in-
board of its deployed position.

2. The bed of claim **1** in which when the wing is in its
stored position the lateral extremity thereof is out-
board of the outboard edge, or the lateral extremity
thereof is substantially aligned with the outboard
edge, or the lateral extremity thereof is inboard of
the outboard edge.
3. The bed of either claim **1** or claim **2** wherein the motor
assembly includes a gear train.
4. The bed of any preceding claim wherein the wings
of the deck section are directly driven wings and the
bed comprises at least one adjacent deck section
having left and right indirectly driven wings coupled
to the directly driven wings such that lateral transla-
tion of the directly driven wings causes lateral trans-
lation of the indirectly driven wings.
5. The bed of any preceding claim wherein the deck
section is a directly driven section and the wings of
the directly driven deck section are directly driven
wings, and the bed comprises:

at least one proximate deck section adjacent to
the directly driven deck section, the proximate
section having left and right indirectly driven
proximate wings coupled to the directly driven
wings such that lateral translation of the directly
driven wings causes lateral translation of the in-
directly driven proximate wings, and
at least one remote deck section non-adjacent
to the directly driven deck section and adjacent
to the indirectly driven proximate section, the re-
mote section having left and right indirectly driv-
en remote wings coupled to the indirectly driven
proximate wings such that lateral translation of
the directly driven wings causes lateral transla-
tion of the indirectly driven proximate wings and
of the indirectly driven remote wings.

6. The bed of any preceding claim wherein the lead-
screw receiver is a clasp which can be engaged with
and disengaged from the leadscrew.

7. The bed of any preceding claim comprising:

an extension wing movement mechanism; and
a release unit including a clasp comprising a first
clasp portion movably coupled to the wing and
a second clasp portion fixedly coupled to the
wing, the release unit configured to transition
between:

- a) an engaged state in which the release
unit engages a portion of the movement
mechanism and is moved by the movement
mechanism to cause the wing to translate
relative to the deck section; and

- b) a disengaged state in which the release unit is disengaged from the portion of the movement mechanism.
8. The bed of any preceding claim comprising a control system configured to sense the position of the wing and alert a user when the wing is in a deployed position in which a lateral extremity of the wing is outboard of the outboard edge and a stored position in which the lateral extremity is inboard of its deployed position.
 9. The bed of any preceding claim comprising:
 - a first controller configured to control a function of a person support apparatus, the first controller configured to receive a first input corresponding to a function of the person support apparatus via a first user interface; and
 - a second controller configured to control a function of a person support surface, the second controller configured to:
 - a) receive a second input corresponding to a function of the person support surface via a second user interface when the first controller is not in communication with the second controller, and to
 - b) receive a third input corresponding to a function of the person support surface via the first controller when the first controller is in communication with the second controller, wherein the second controller is configured to control a function of the person support surface in accordance with the third input when the first controller is in communication with the second controller.
 10. The bed of claim 9, wherein the first controller is configured to receive a fourth input corresponding to a function of the person support surface via a first user interface when the first controller is in communication with the second controller.
 11. The bed of either claim 9 or claim 10, wherein the second user interface is disabled when the first controller is in communication with the second controller and/or wherein the second user interface is enabled when communication between the first controller and the second controller is interrupted.
 12. The bed of any one of claims 9 to 11, wherein the second user interface is configured to display information when the first controller is in communication with the second controller.
 13. The bed of any one of claims 7 to 12, wherein the second user interface is configured to lock out function controls when the first controller is in communication with the second controller.
 14. The bed of any one of claims 7 to 13, wherein the first user interface does not include function controls for the person support surface.
 15. The bed of any one of claims 7 to 14, wherein at least one of the first user interface and the second user interface displays an error when the first controller is not in communication with the second controller.
 16. The bed of any preceding claim wherein the deck section and its left and right wings are elements of a person support apparatus and the bed comprises a person support surface configured to be supported on the person support apparatus and including a width extension assembly; and a controller configured to control the width extension wing and the width extension assembly in response to an input from a user, such that the width extension assembly of the person support surface remains in a retracted position unless the corresponding width extension wing of the person support apparatus is positioned in one of a fully retracted position and a fully extended position.
 17. The bed of claim 16 wherein:
 - the person support apparatus includes an apparatus length extension assembly;
 - the person support surface includes a surface length extension assembly; and wherein:
 - the controller is configured to cause at least one of the width extension wing and the apparatus length extension assembly and at least one of the width extension assembly and the surface length extension assembly to move in response to an input from a user, wherein the at least one of the surface length extension assembly and the width extension assembly of the support surface remains in a retracted position unless the corresponding one of the at least one of the width extension wing and apparatus length extension assembly of the support apparatus is positioned in one of a fully retracted position and a fully extended position.
 18. The bed of either claim 16 or claim 17 wherein an alarm is generated if the width extension assembly is not in one of a fully extended position or a fully retracted position.

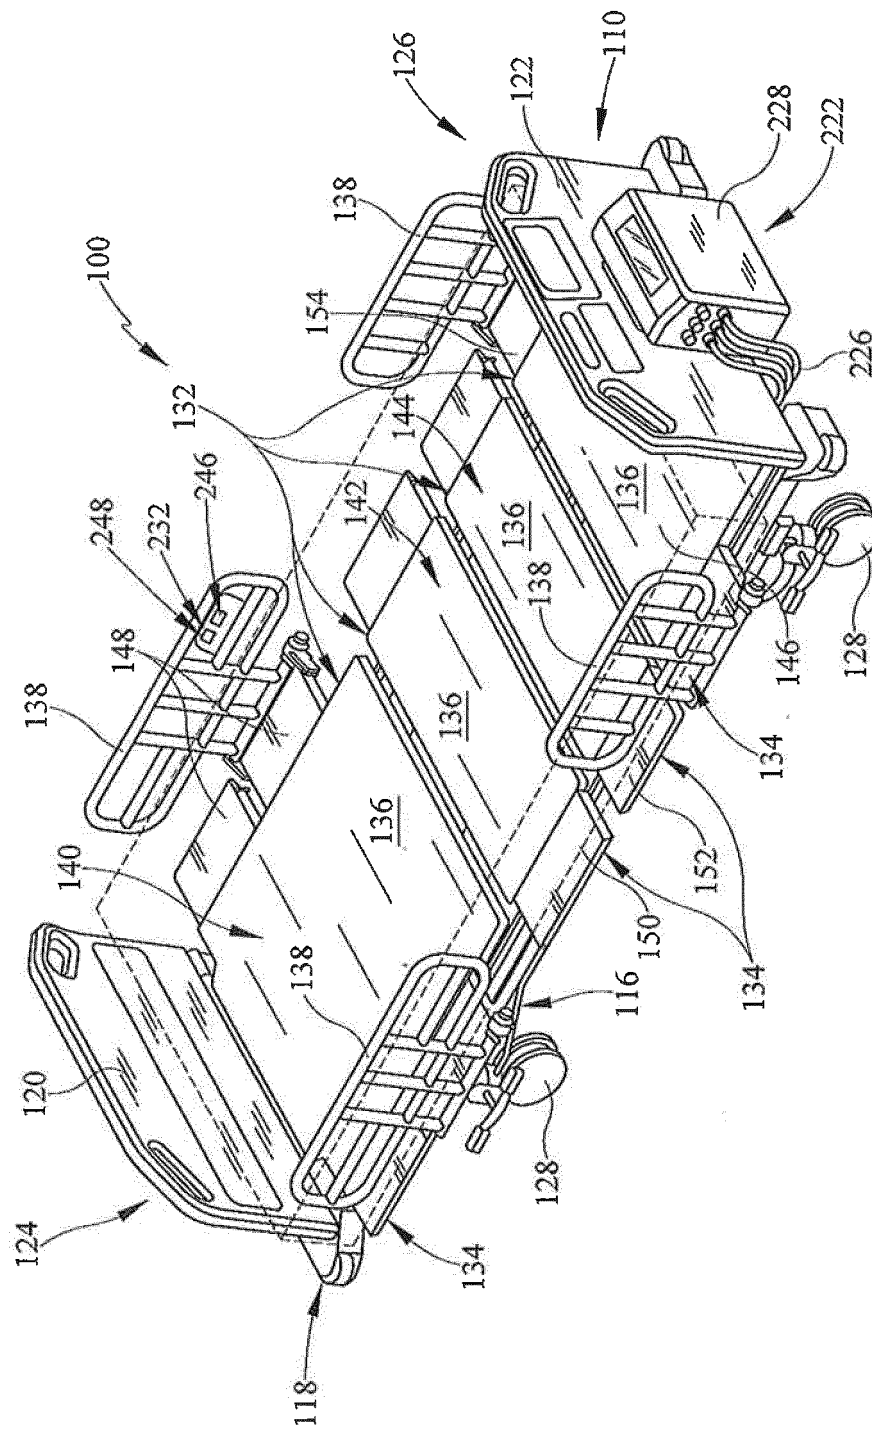


FIG. 1

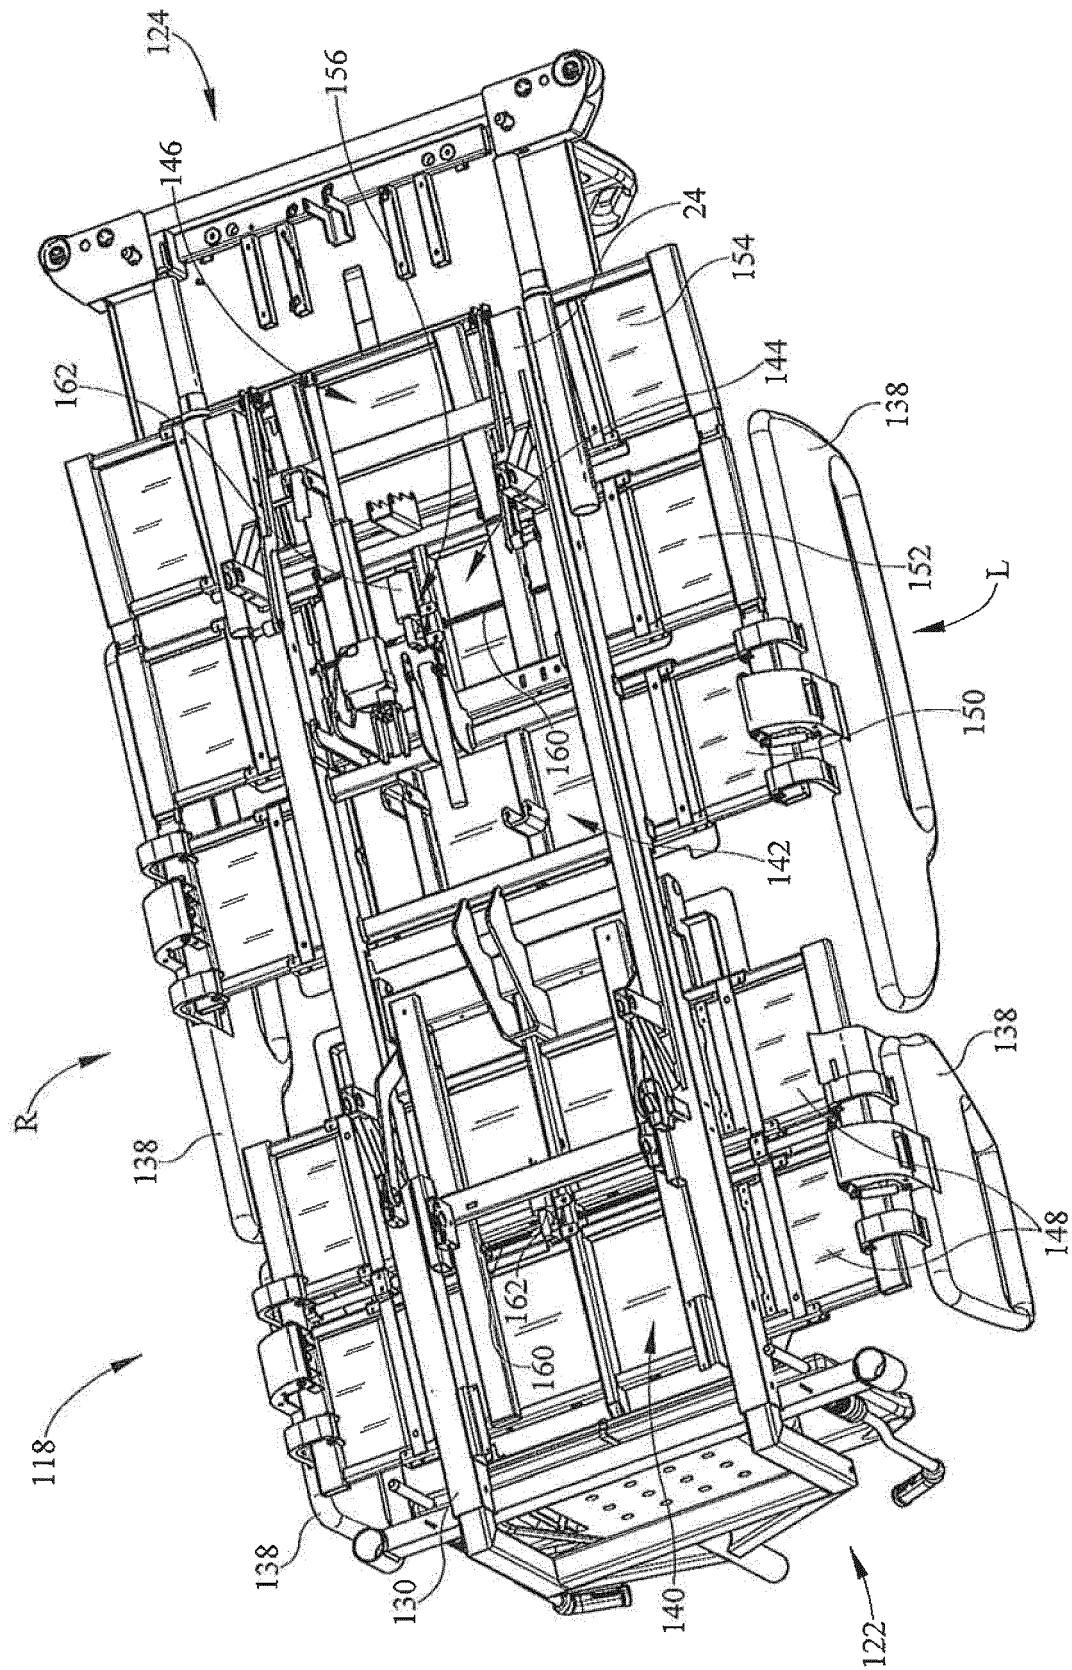


FIG. 2

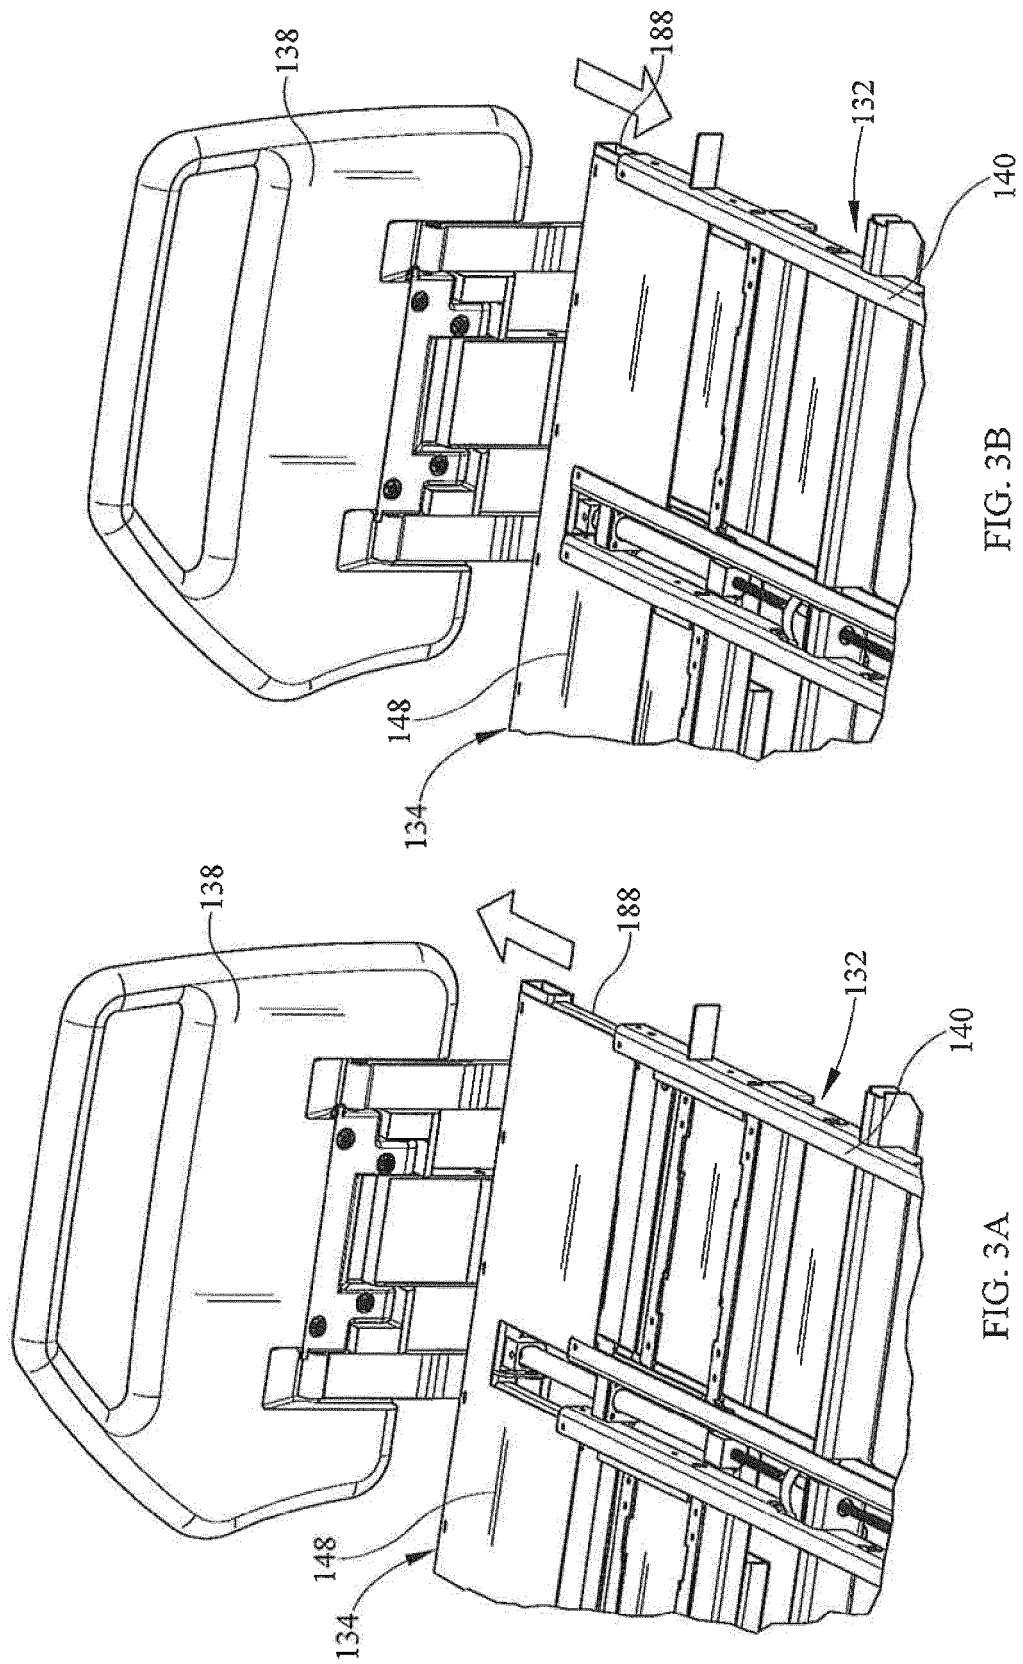


FIG. 3B

FIG. 3A

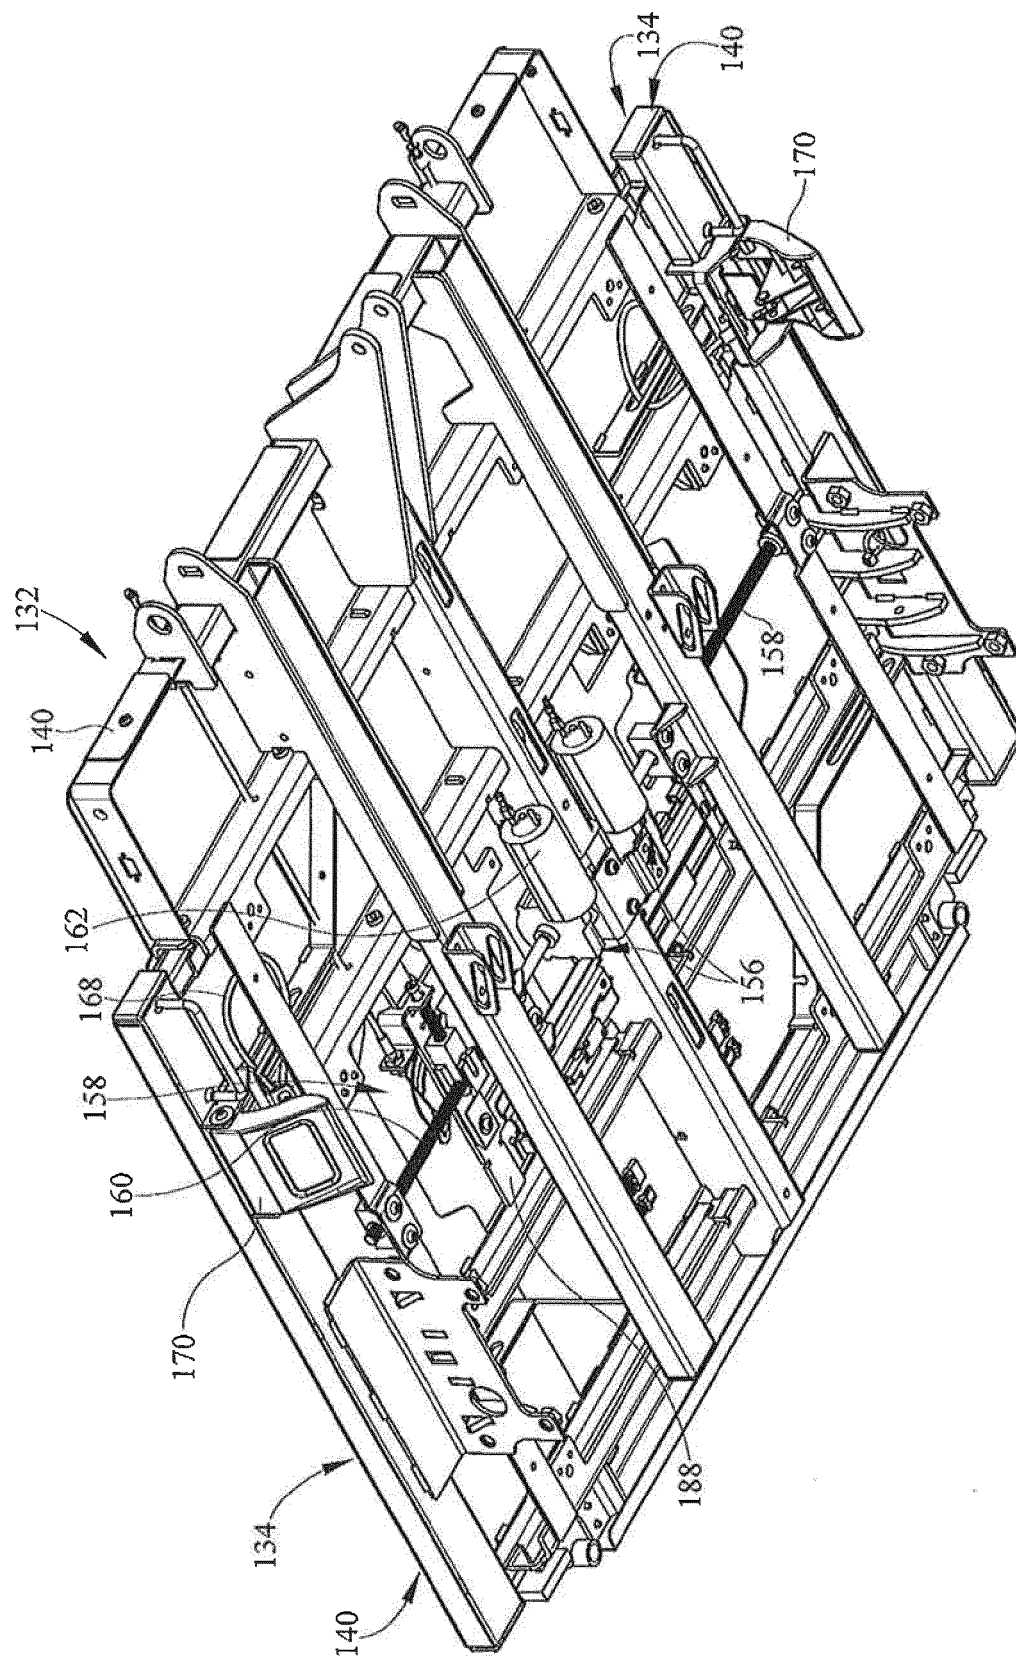


FIG. 4

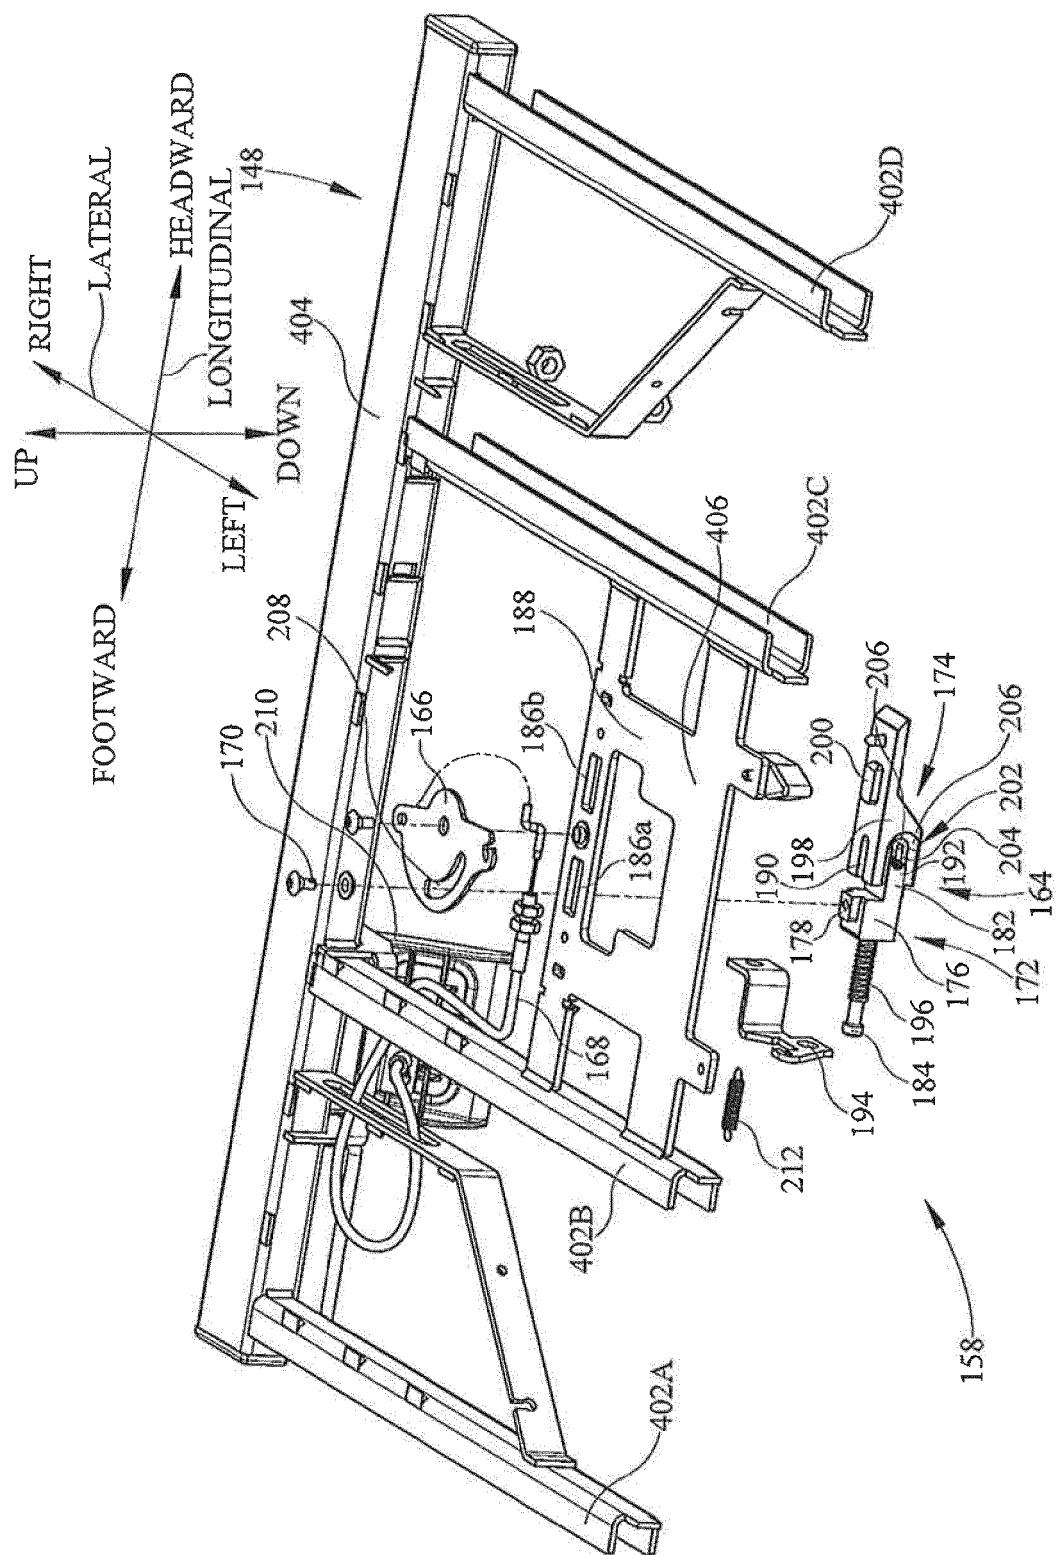


FIG. 5

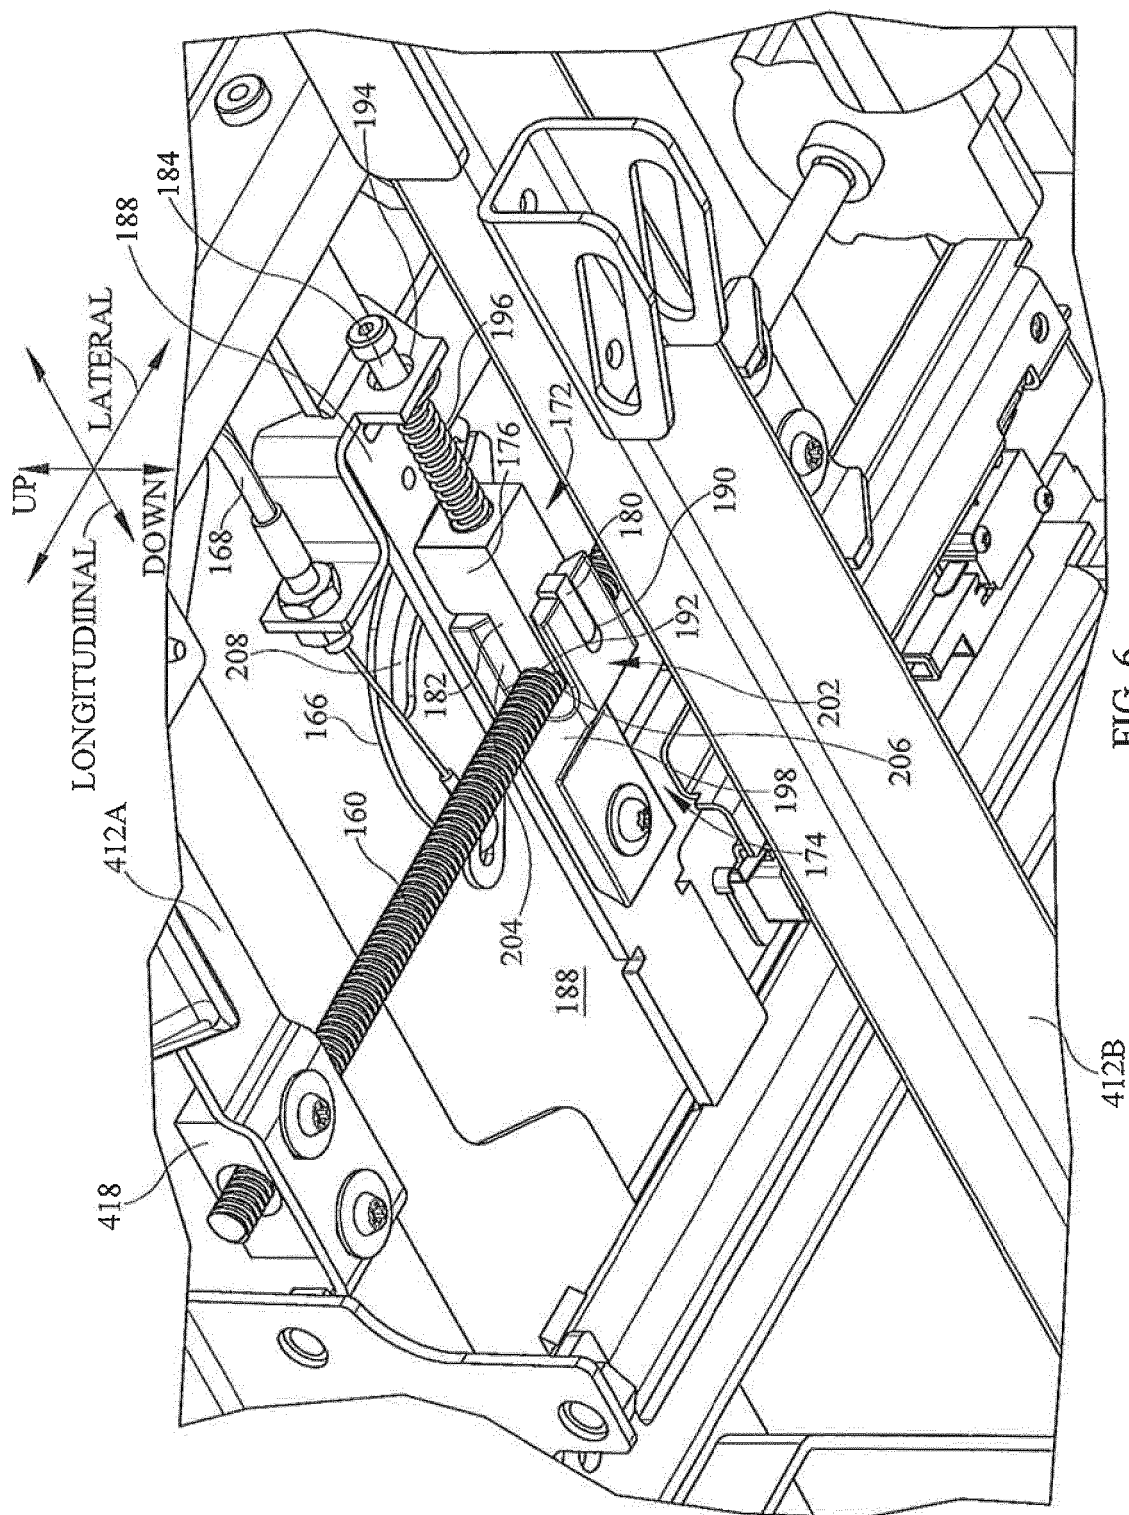


FIG. 6

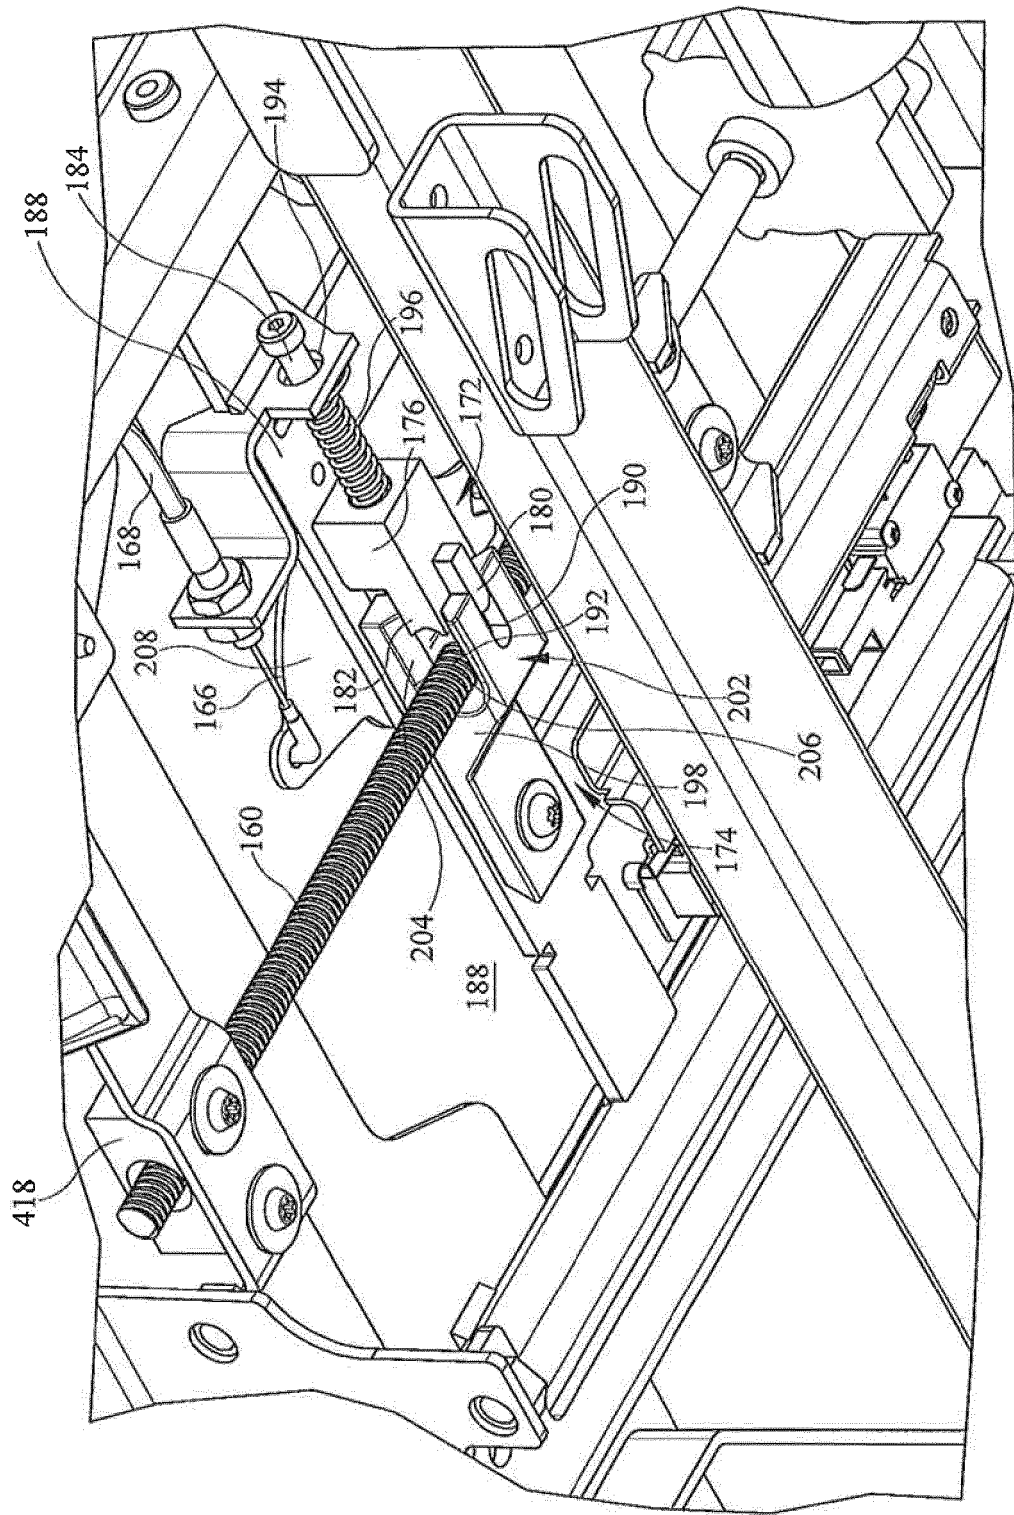


FIG. 7

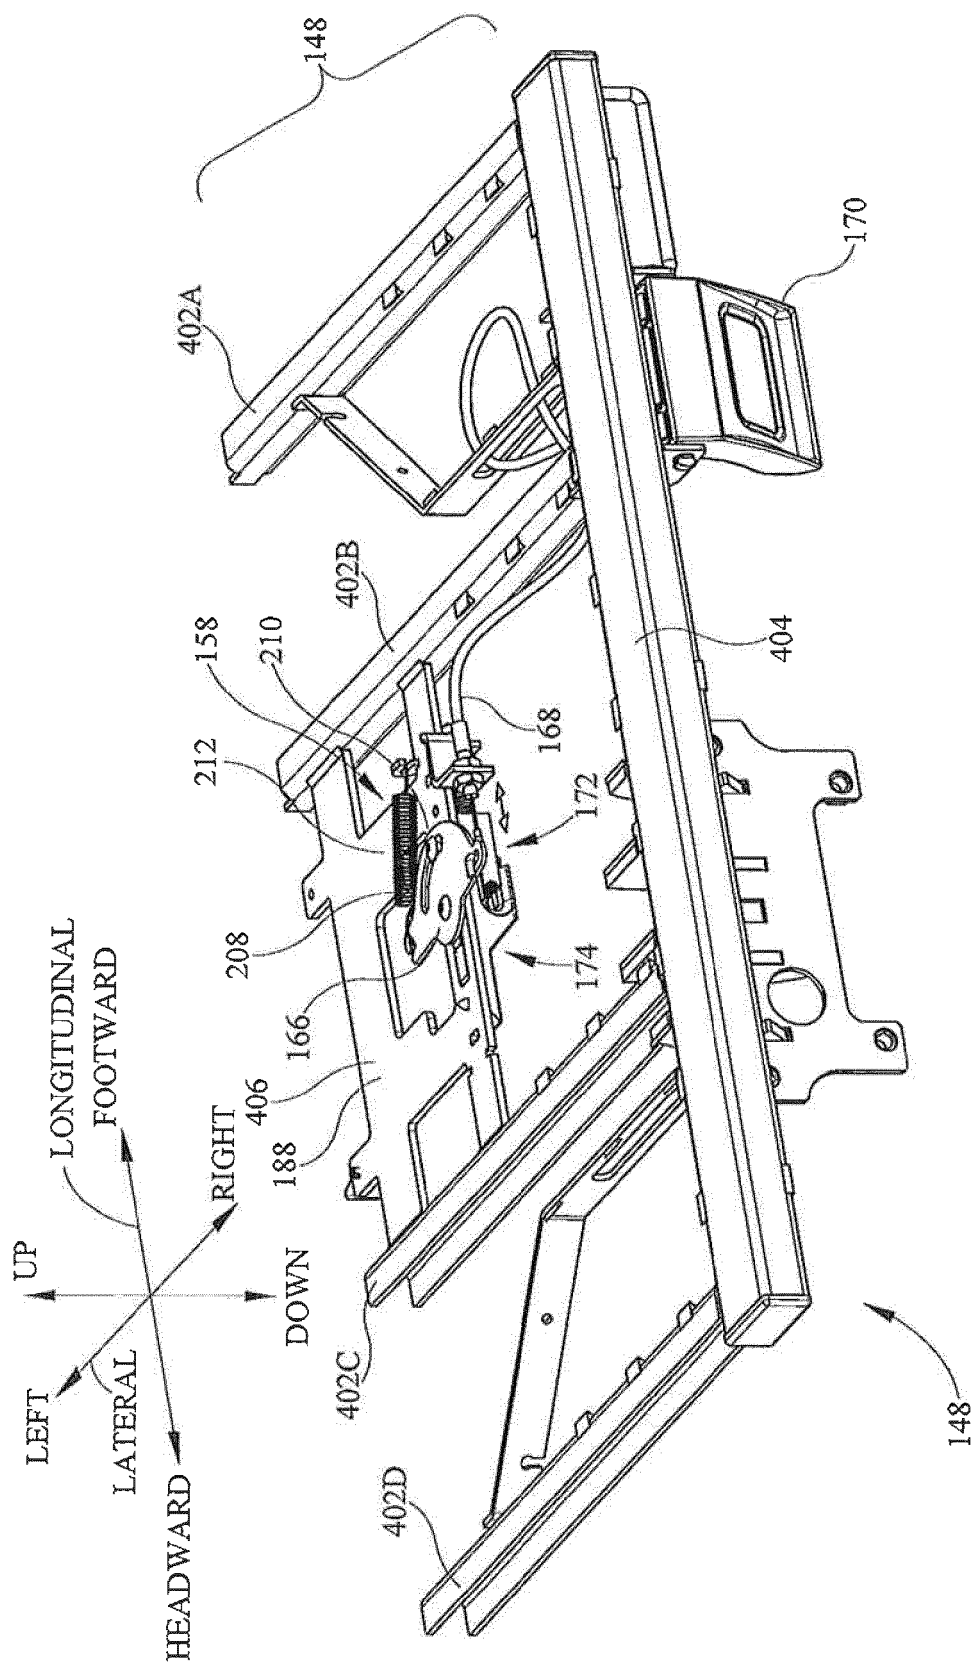


FIG. 8

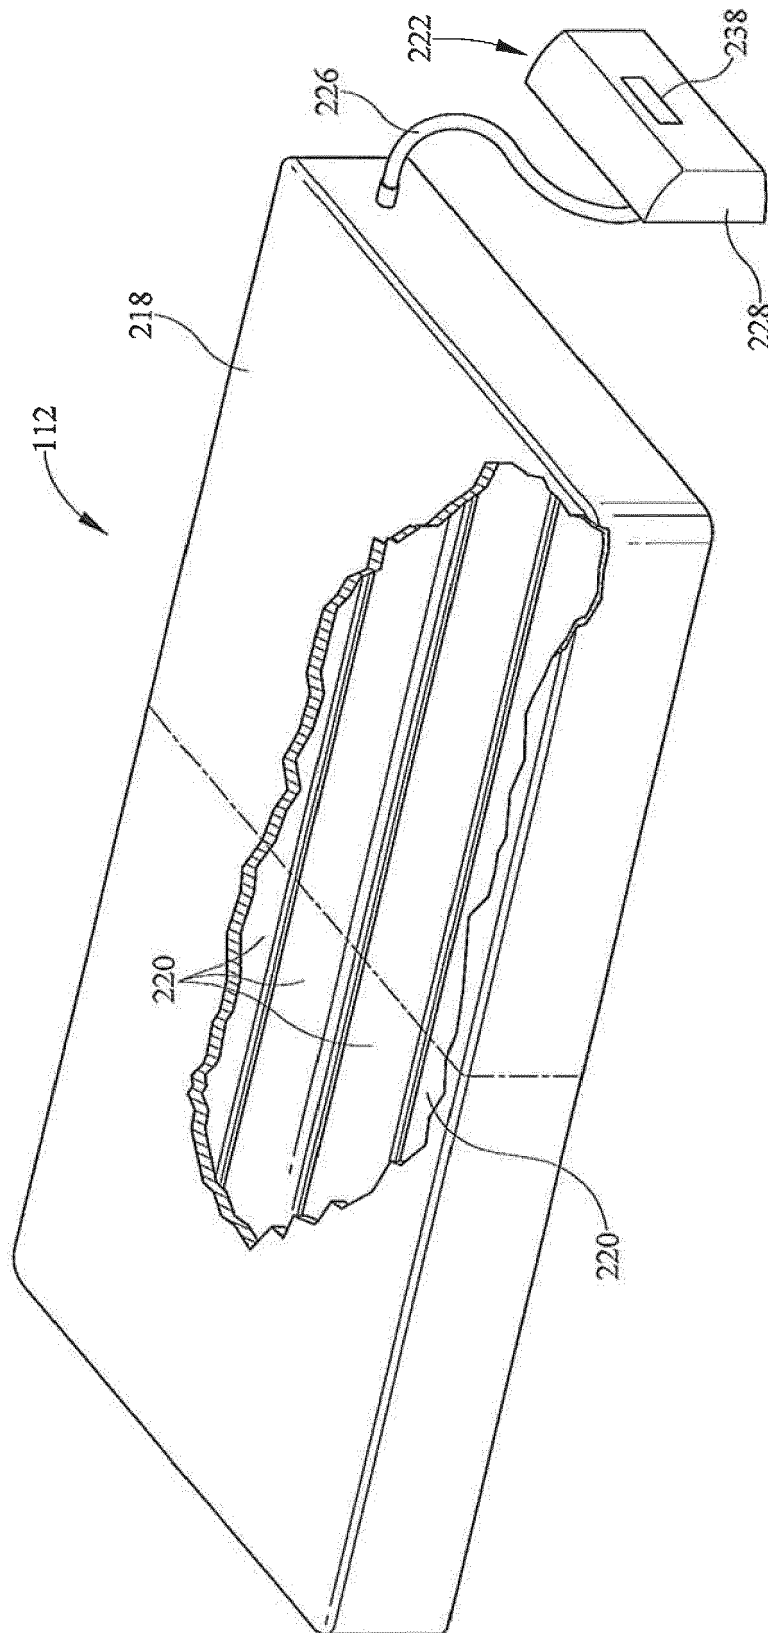


FIG. 9

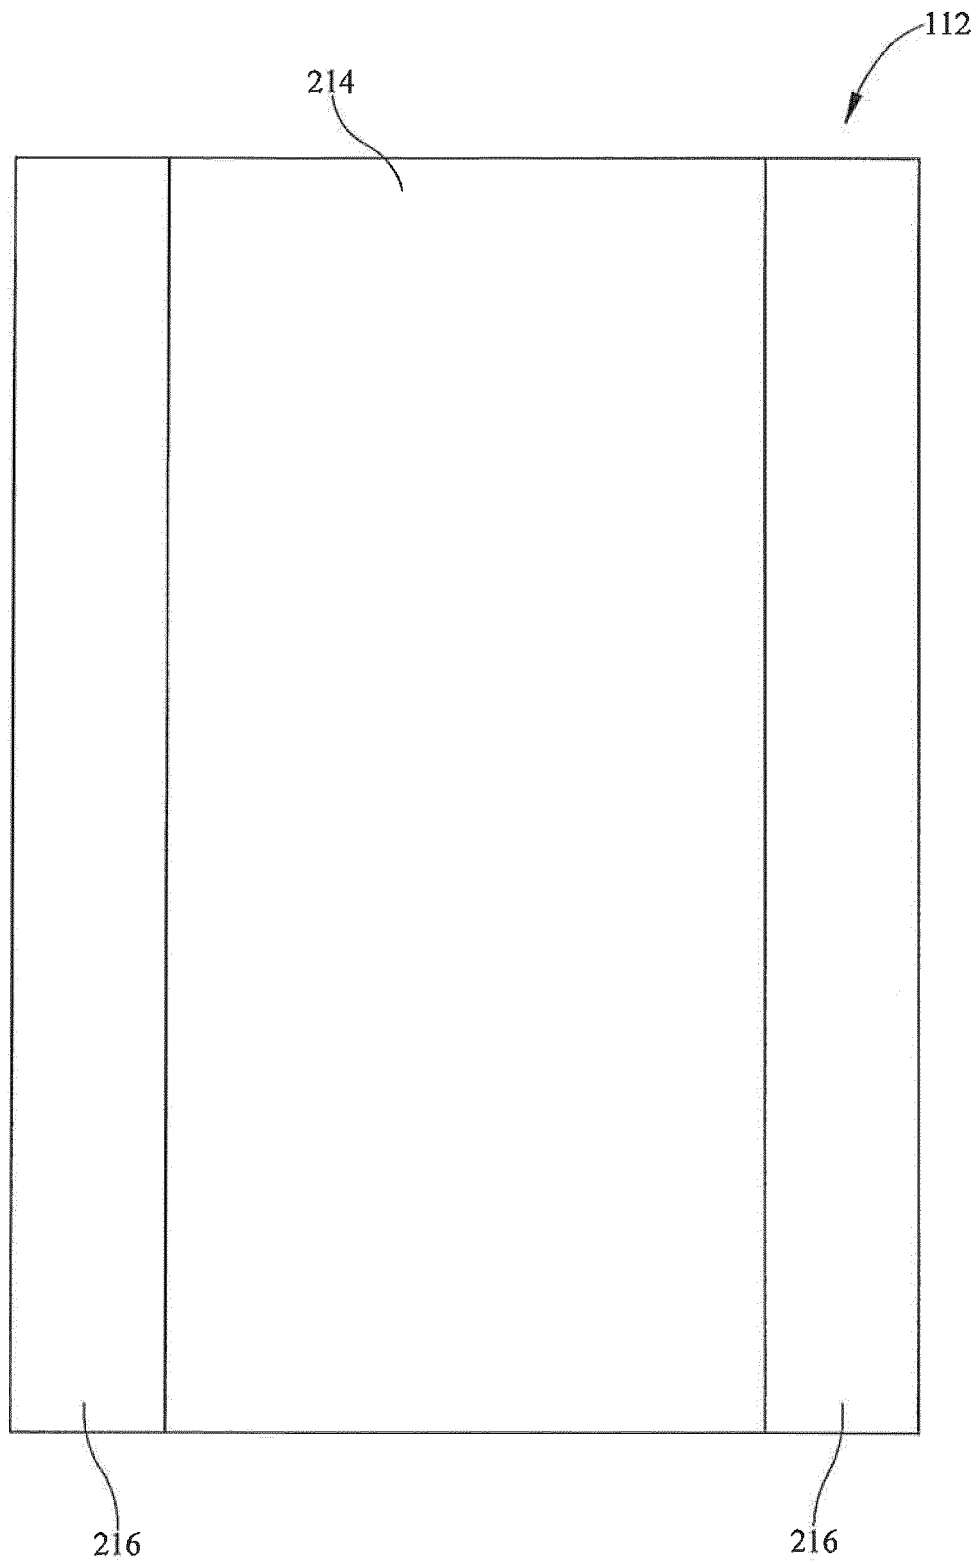


FIG. 10

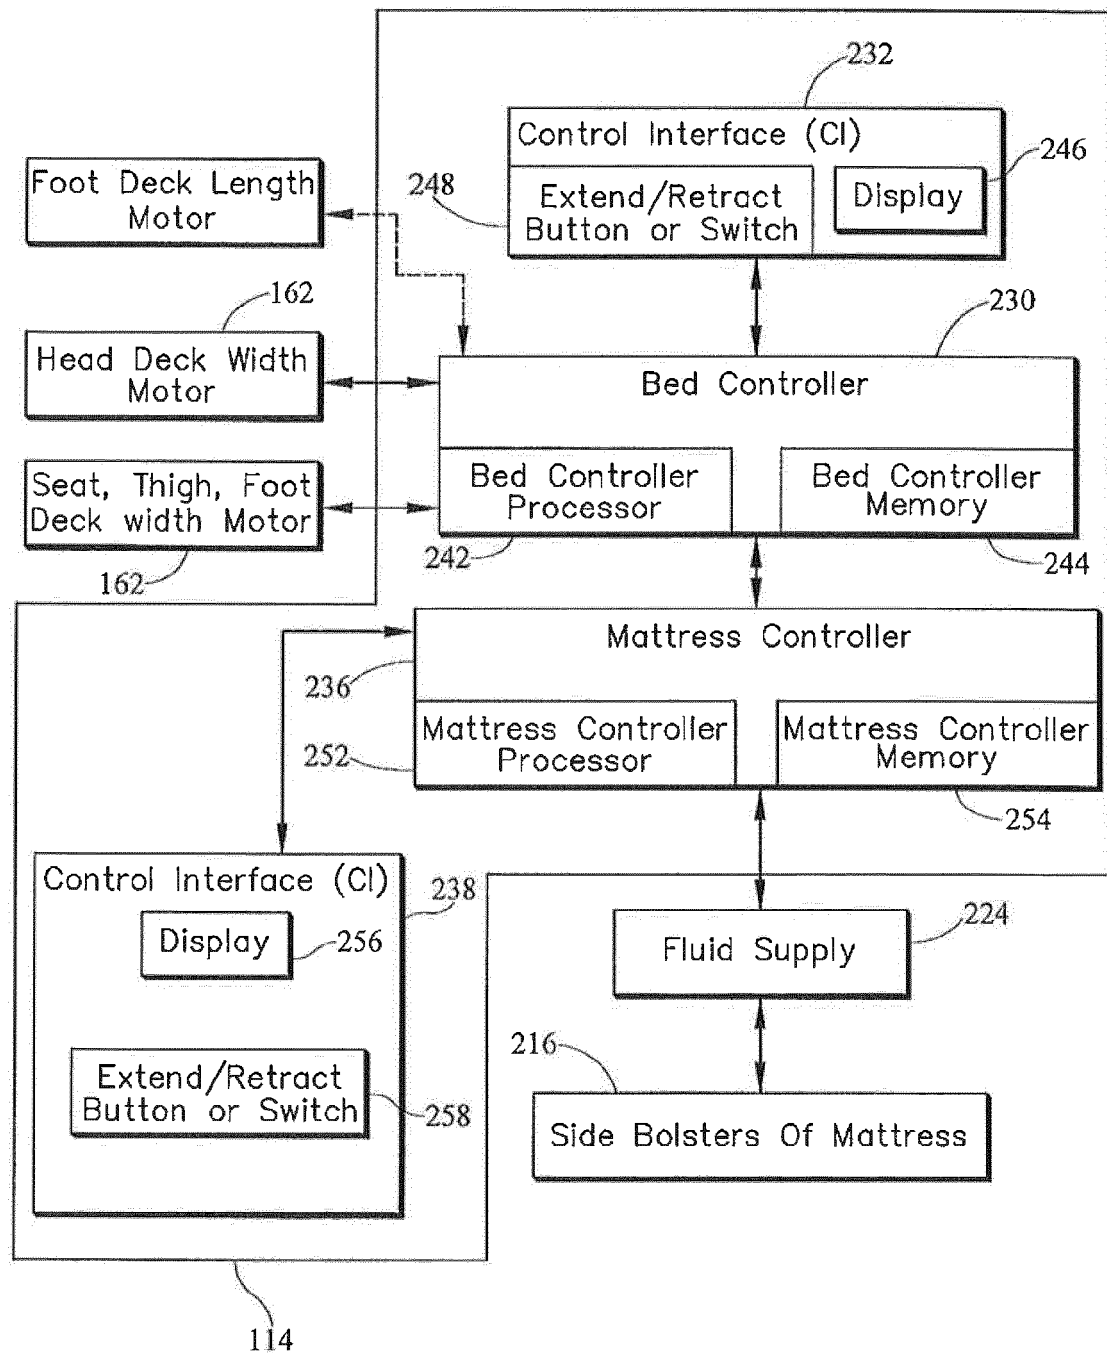


FIG. 11

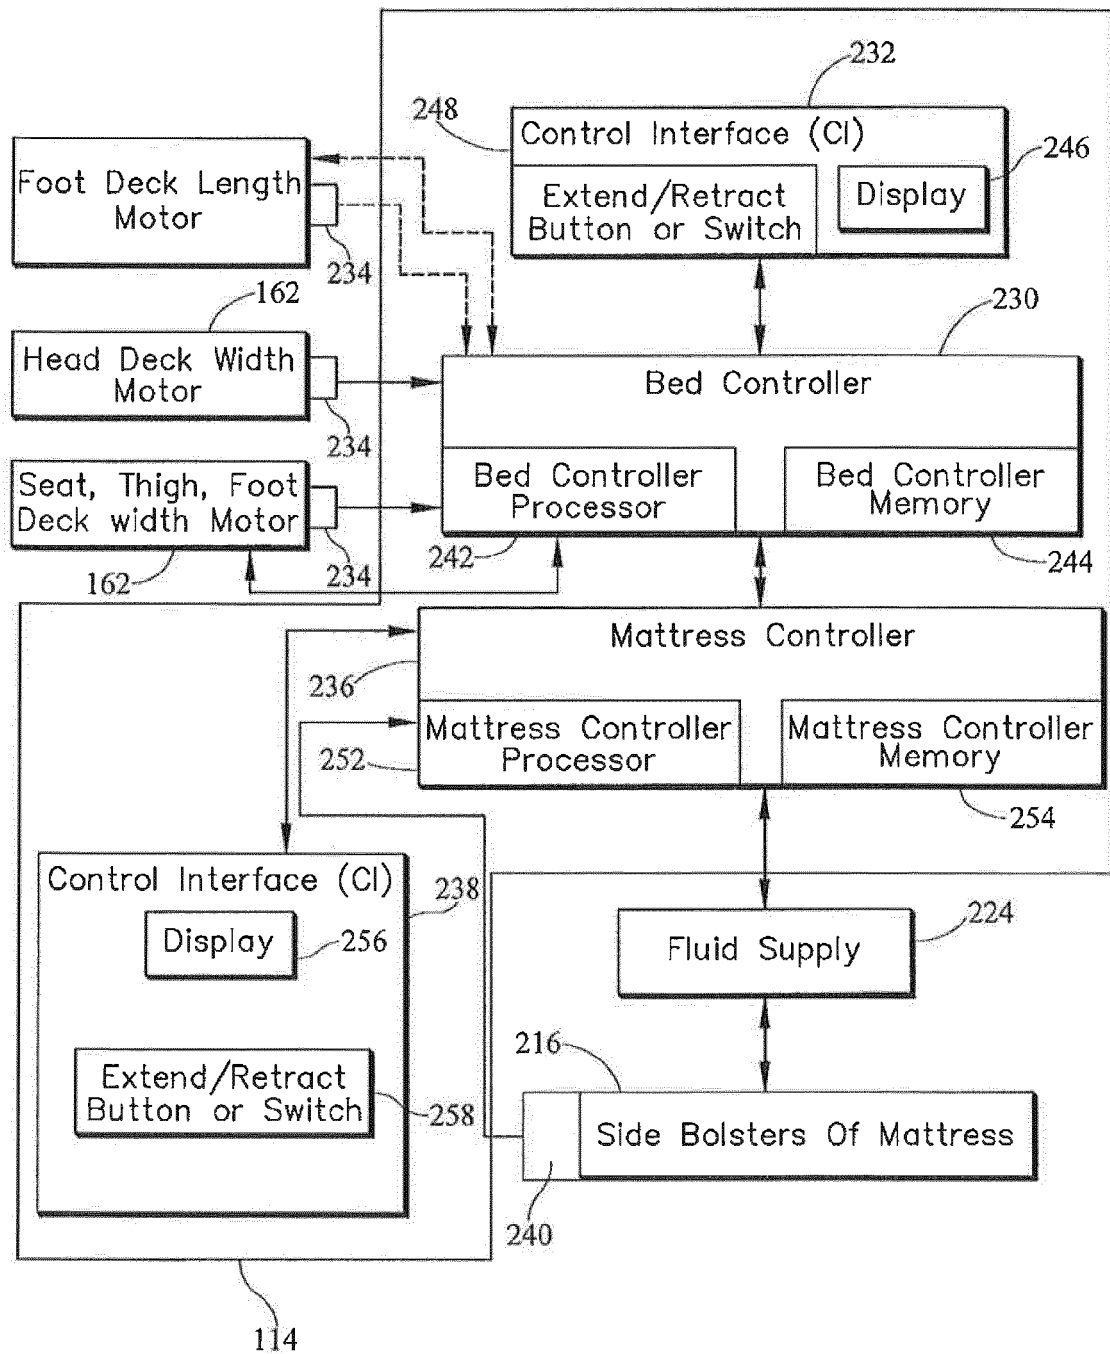


FIG. 12

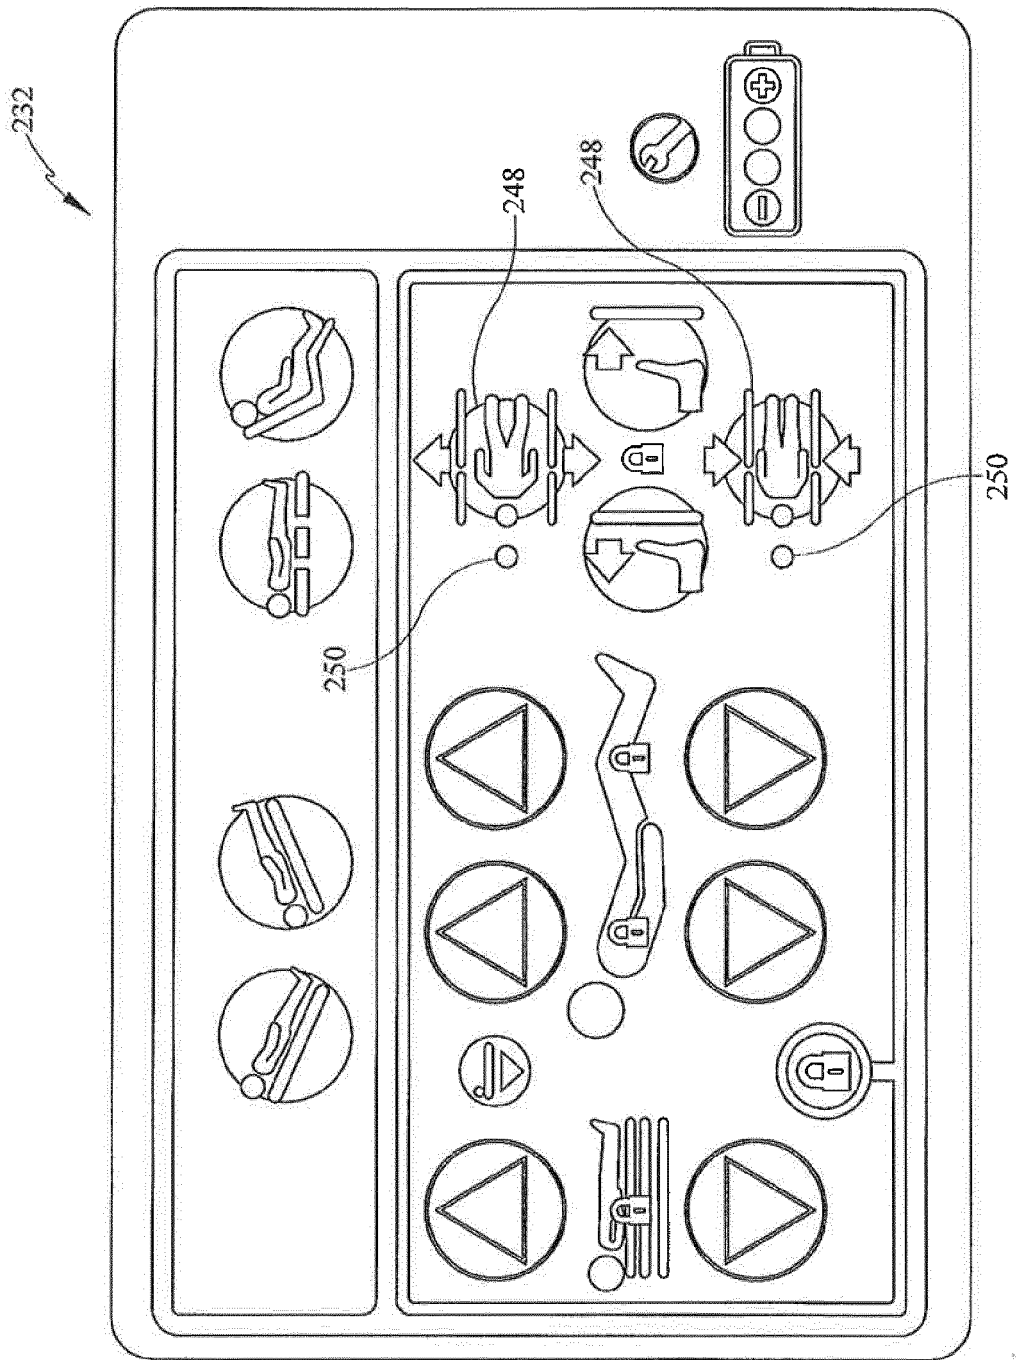
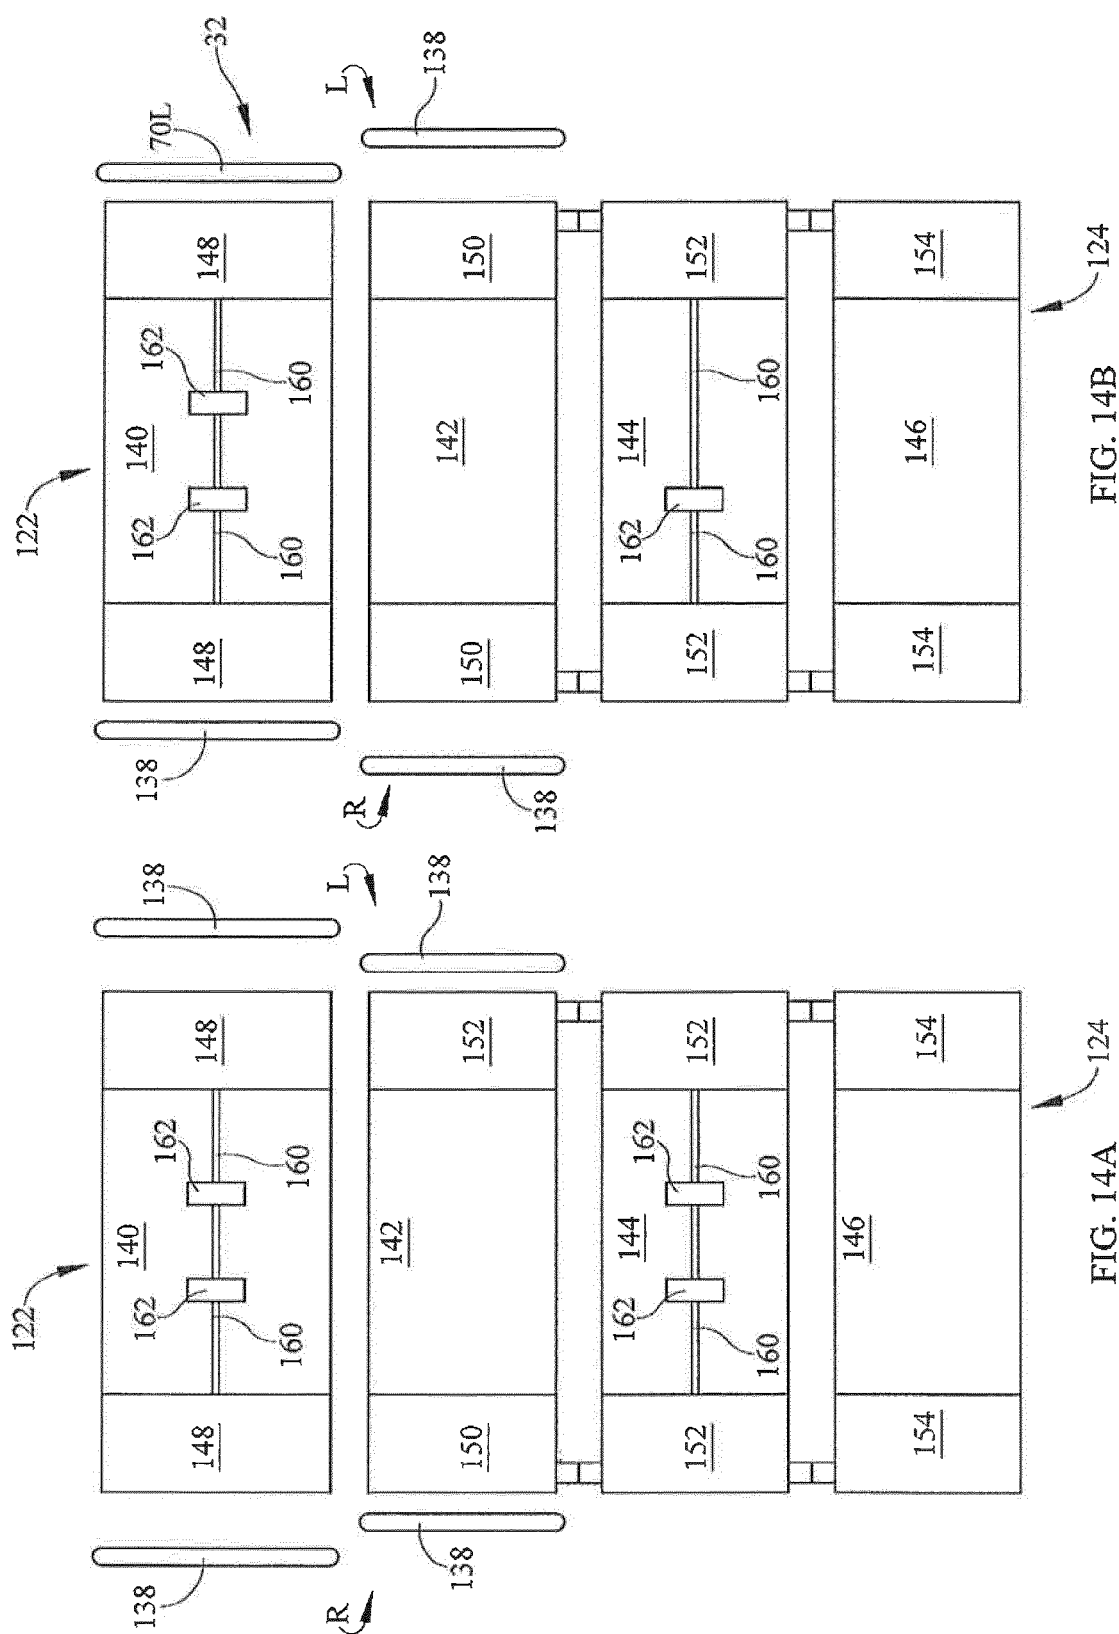


FIG. 13



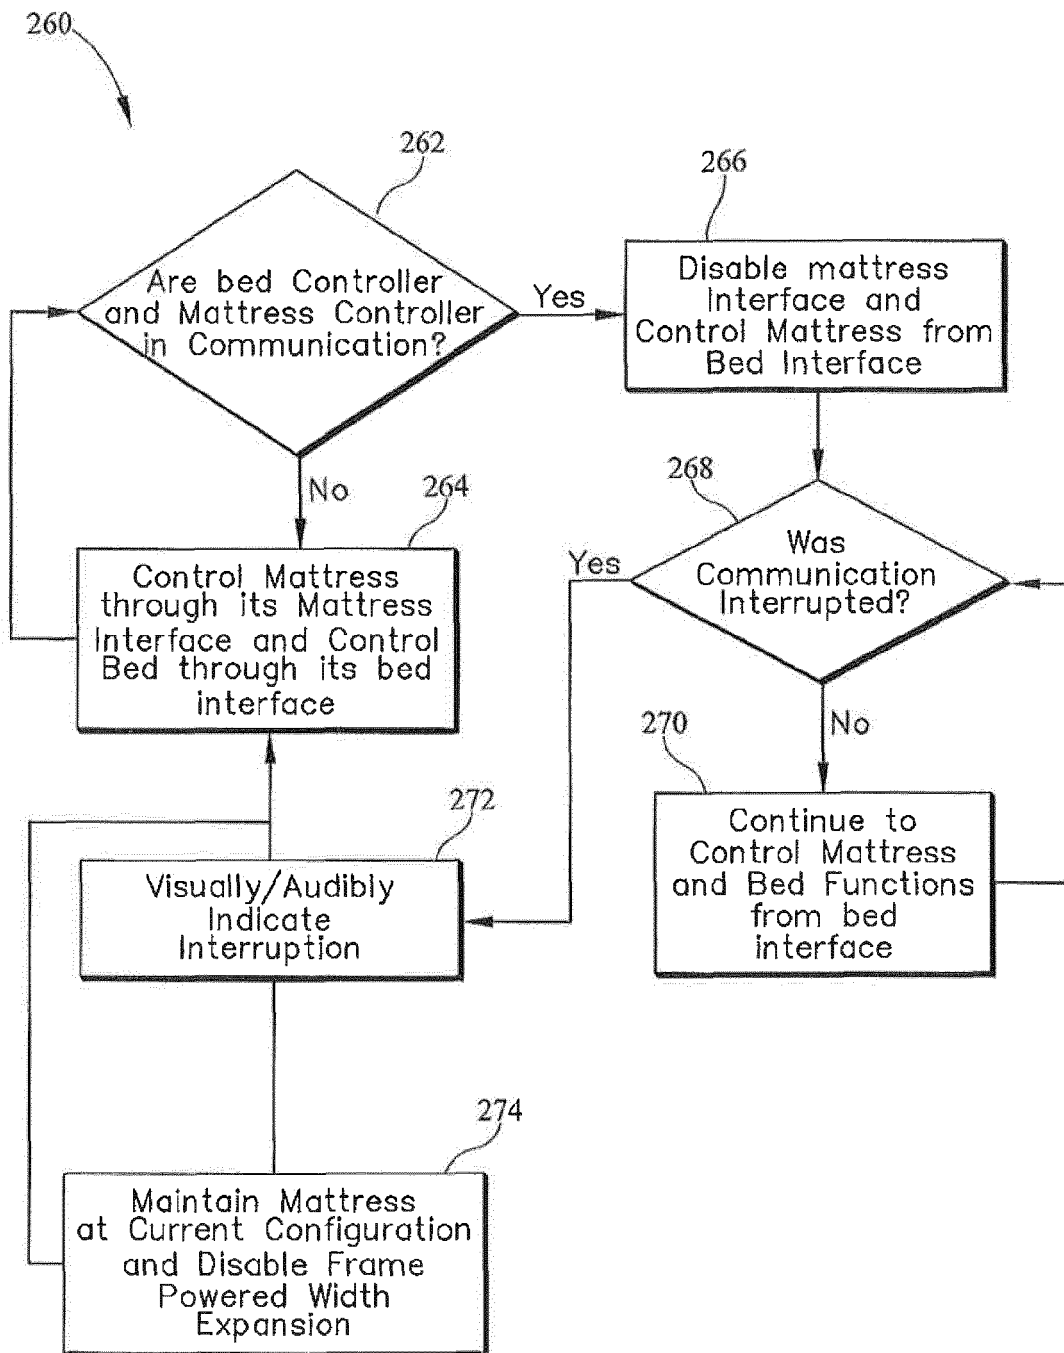


FIG. 15

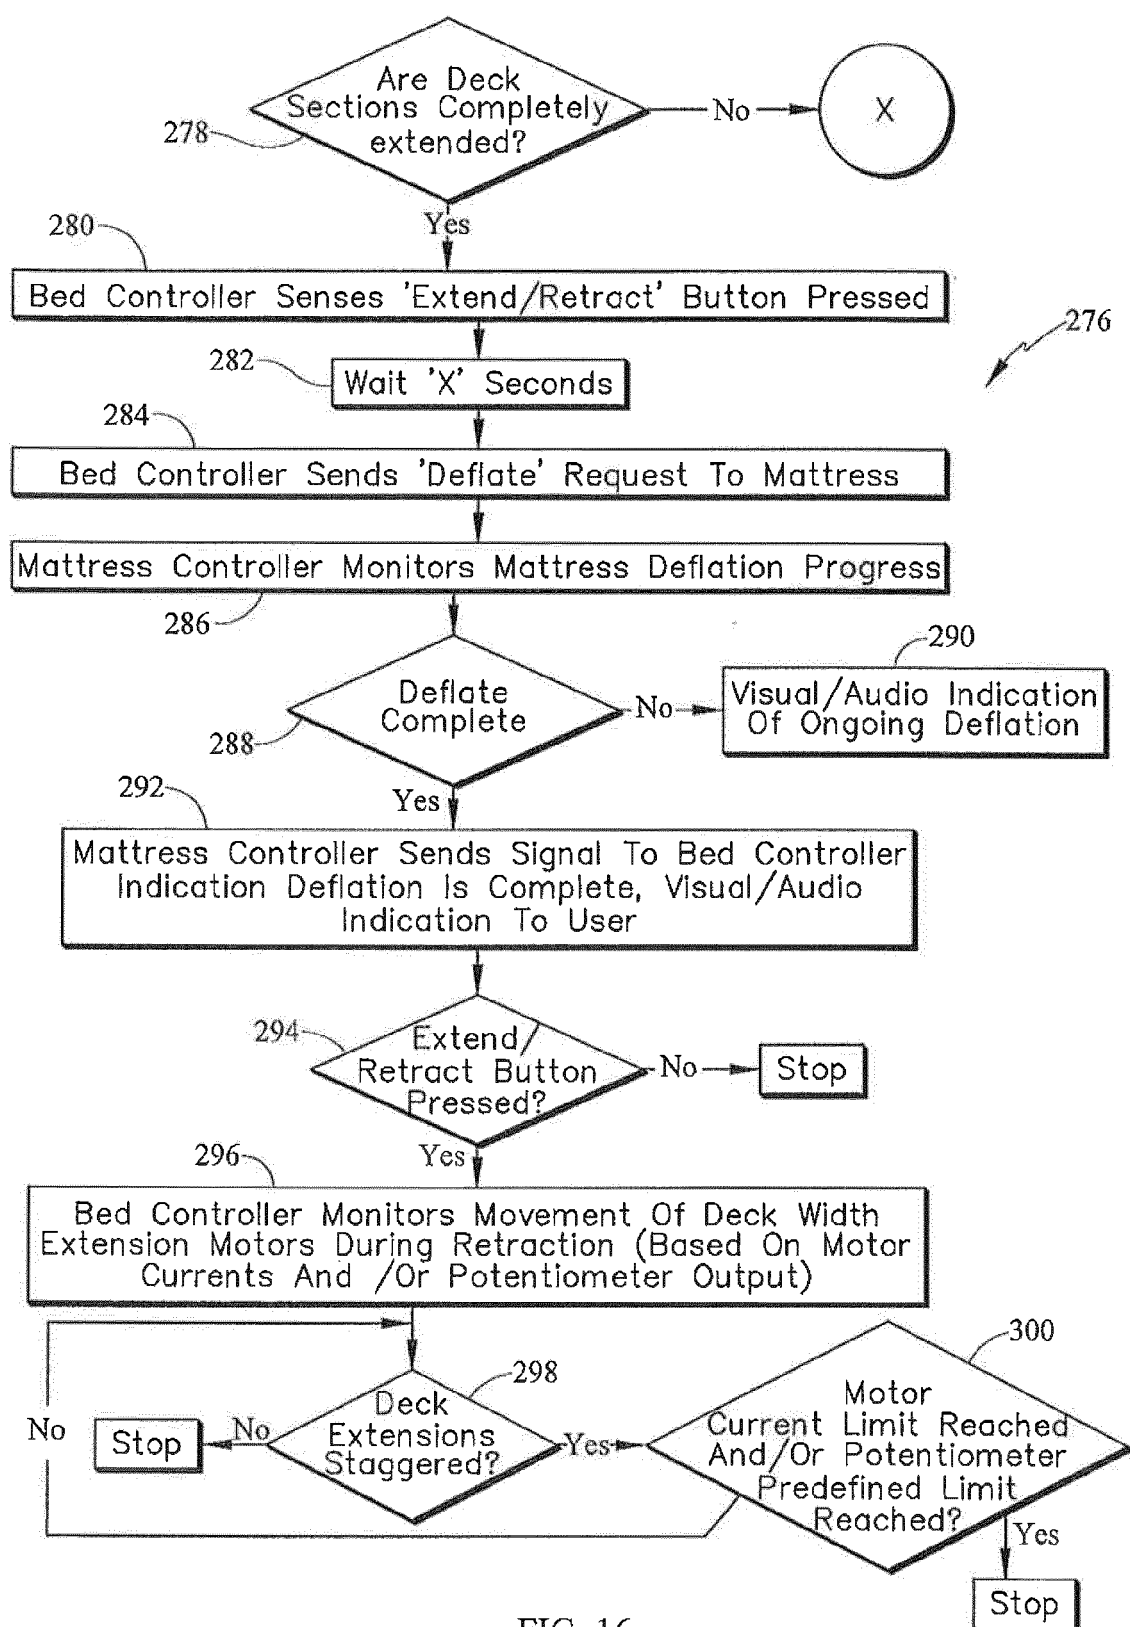


FIG. 16

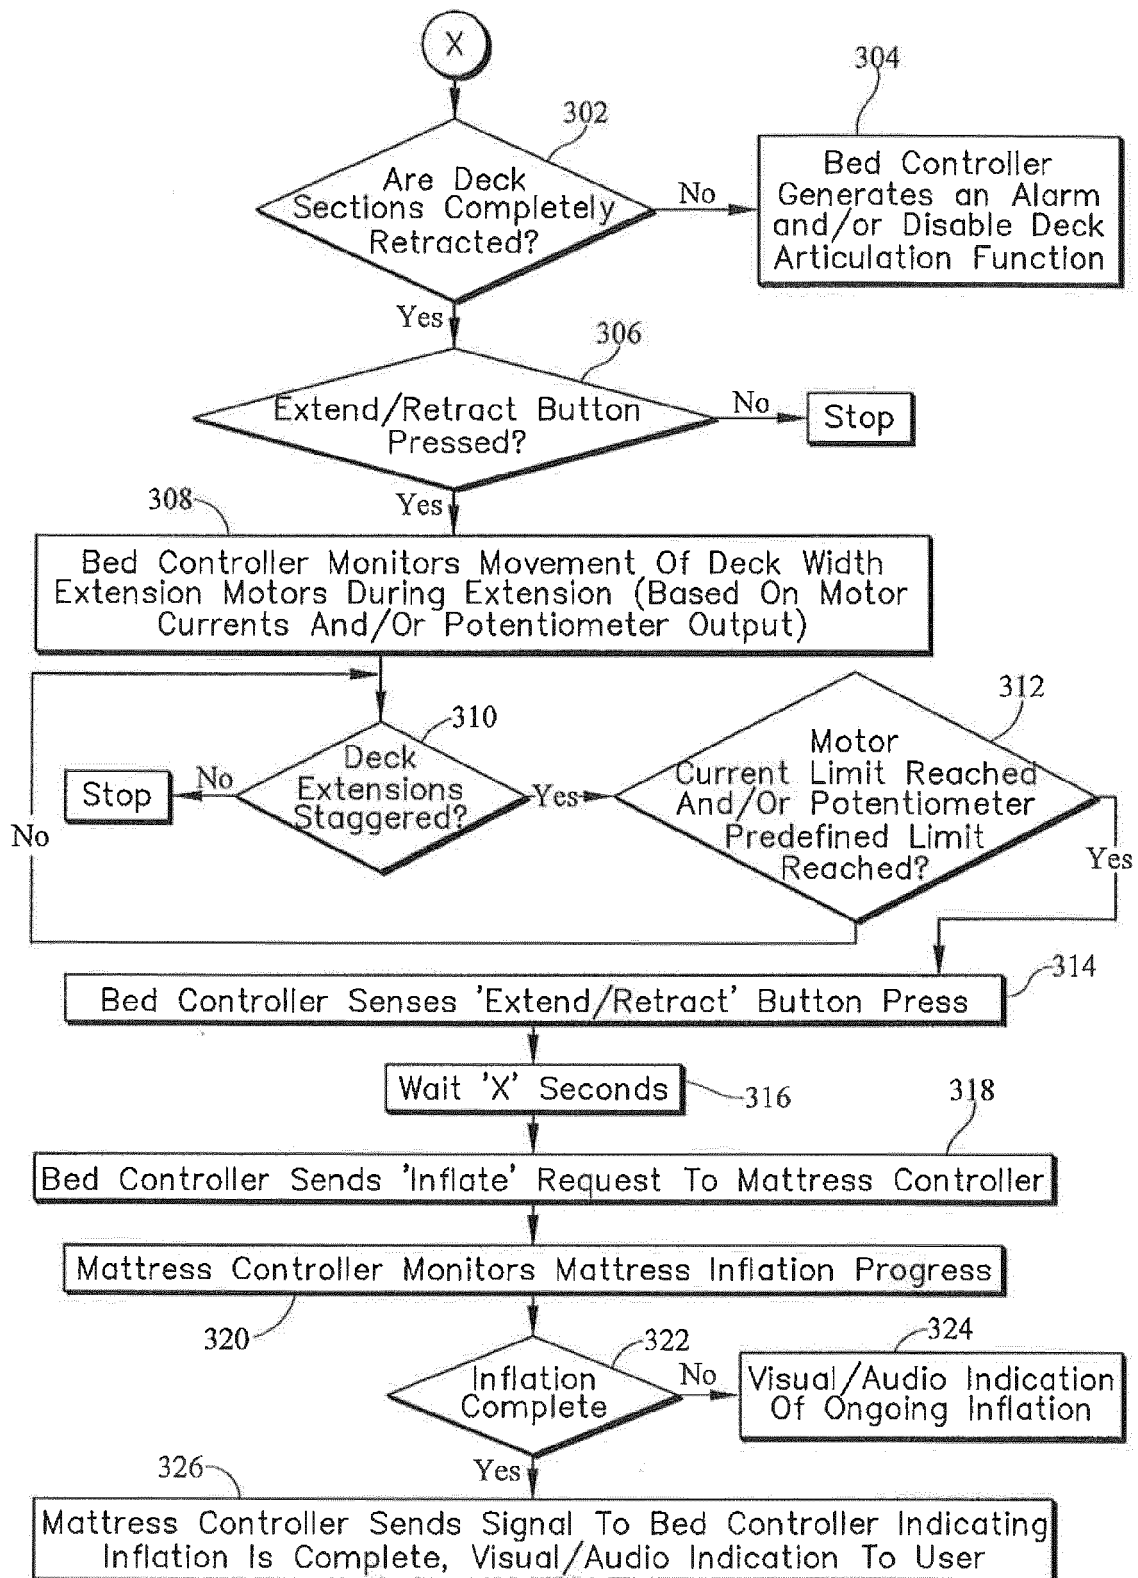


FIG. 17

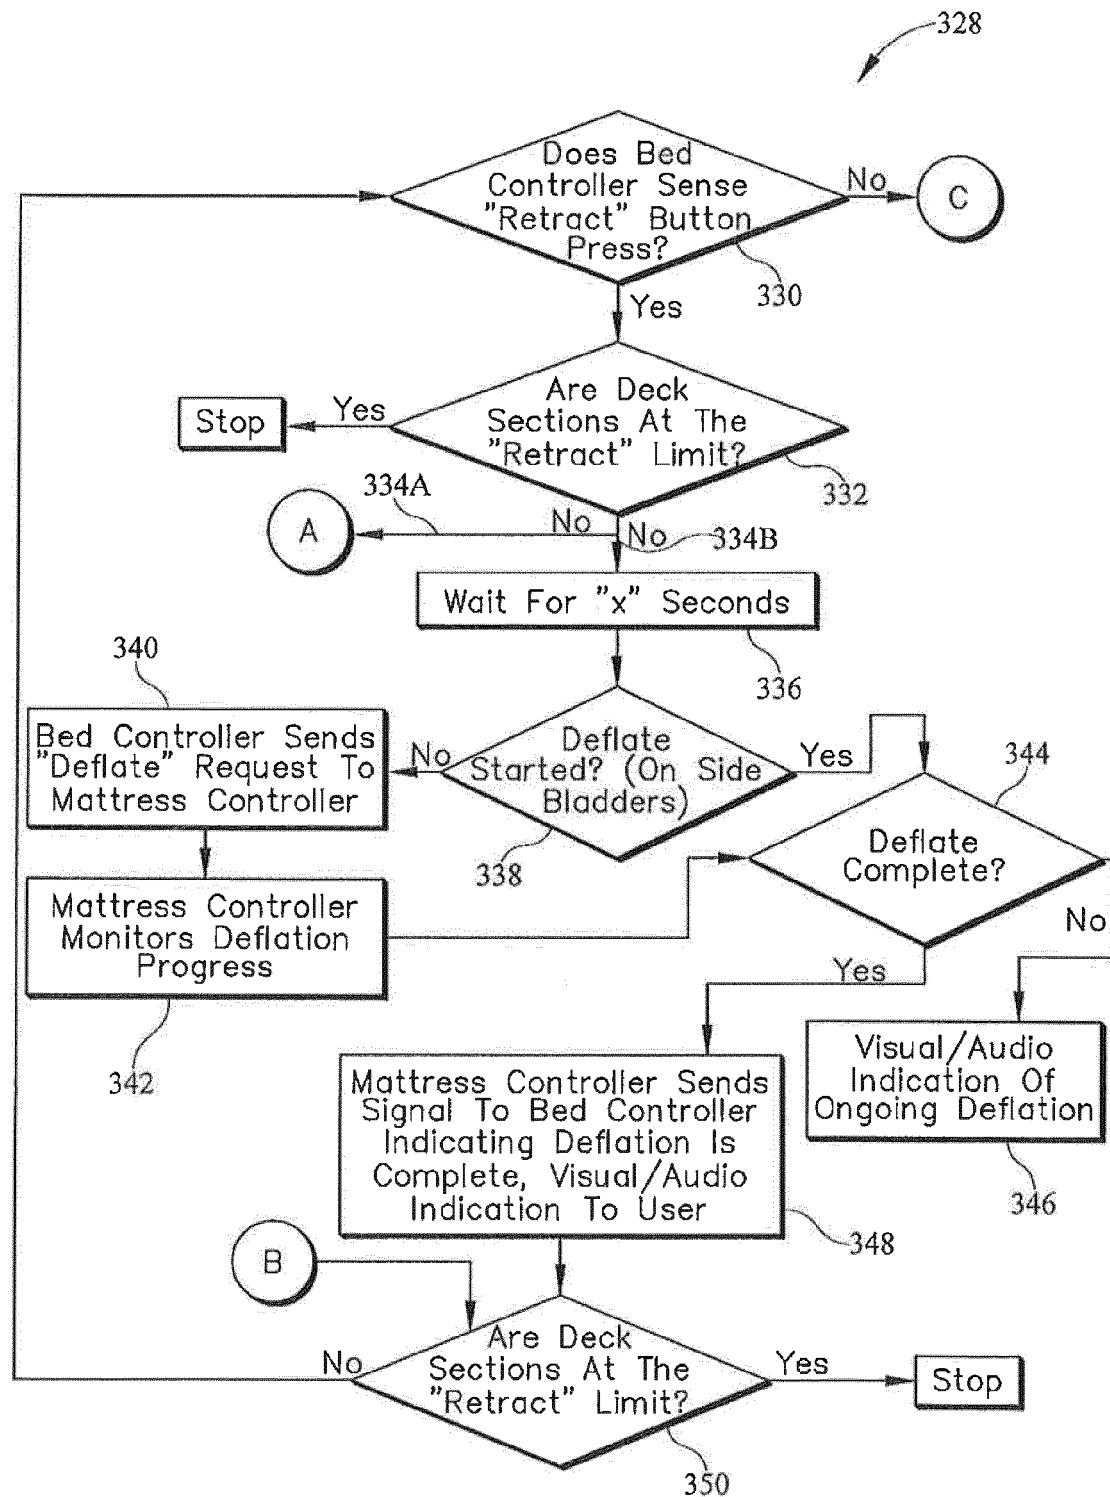


FIG. 18

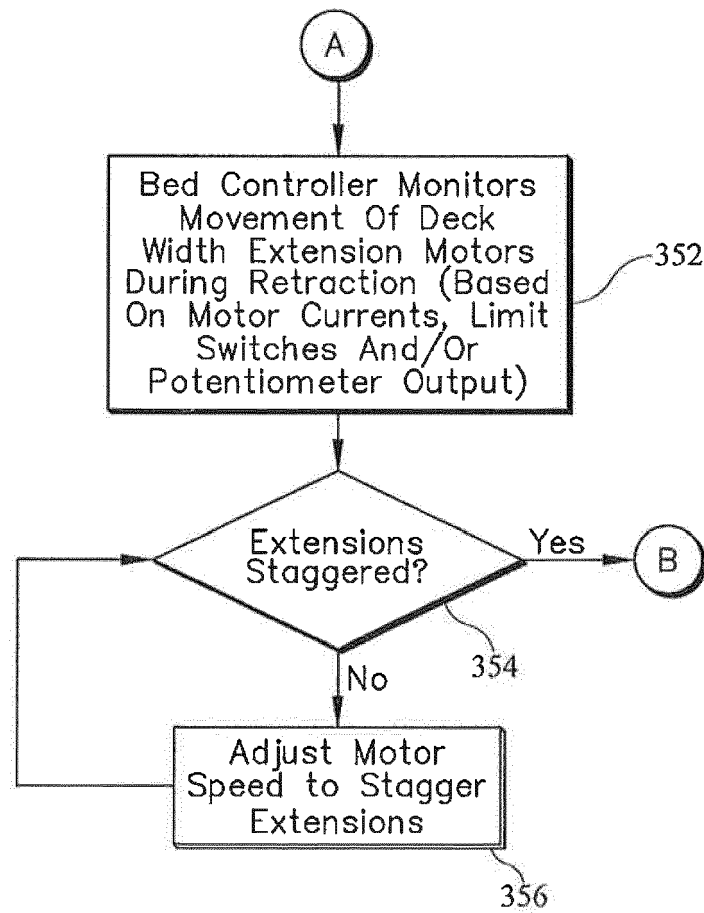


FIG. 18B

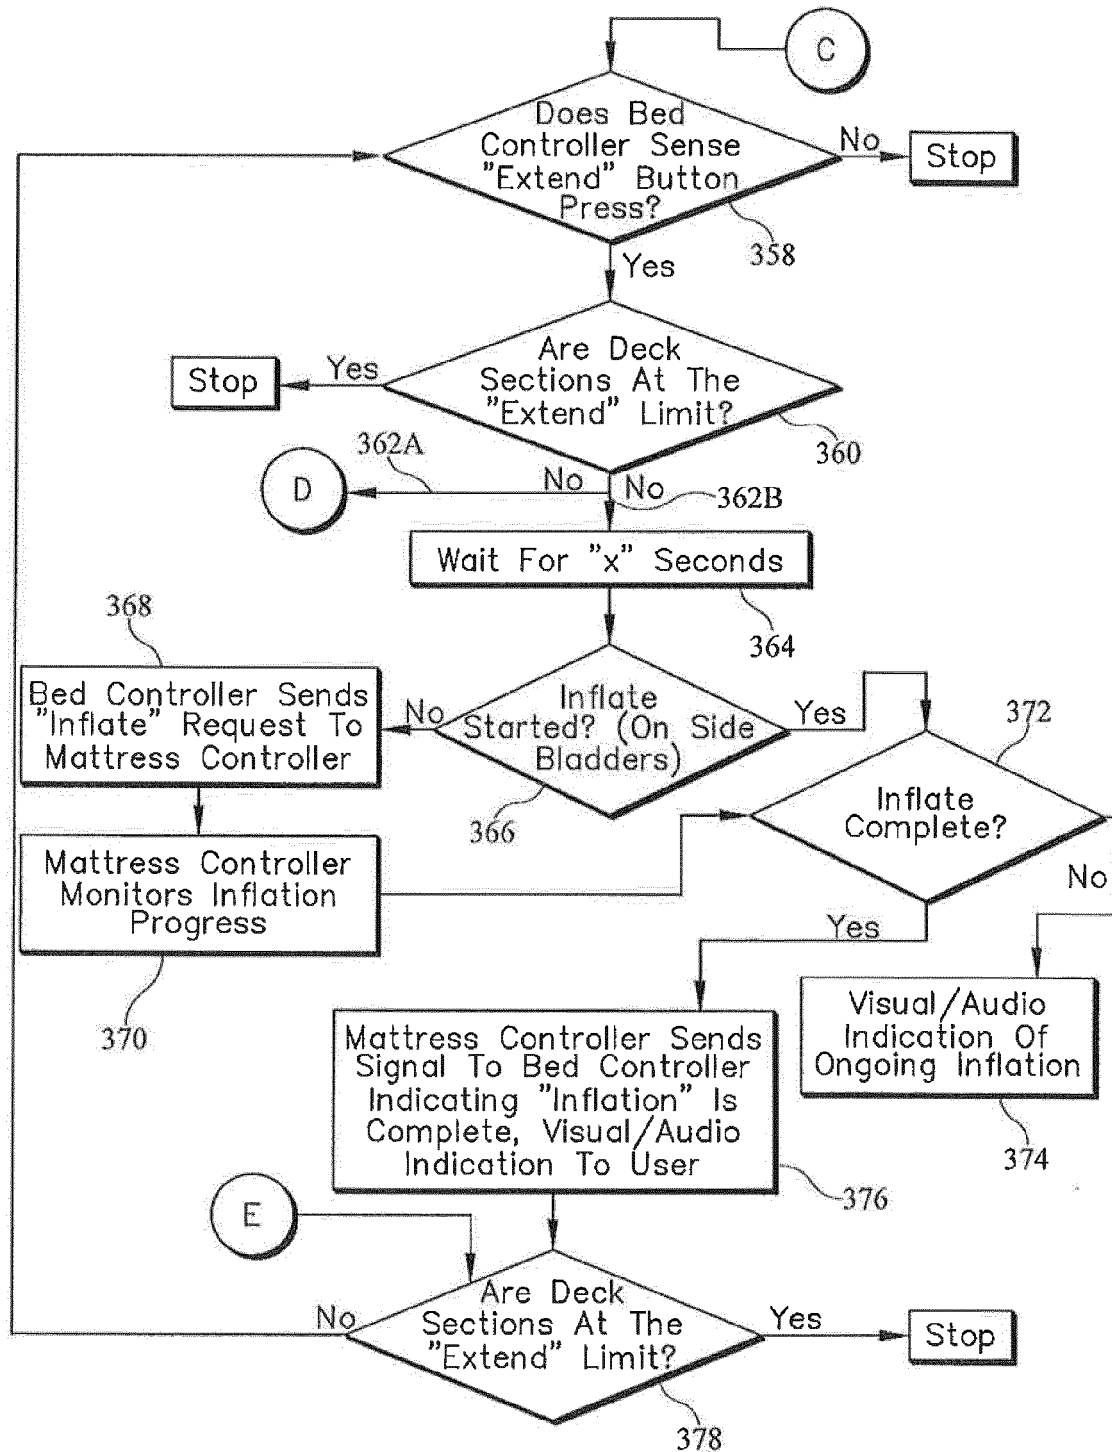


FIG. 19

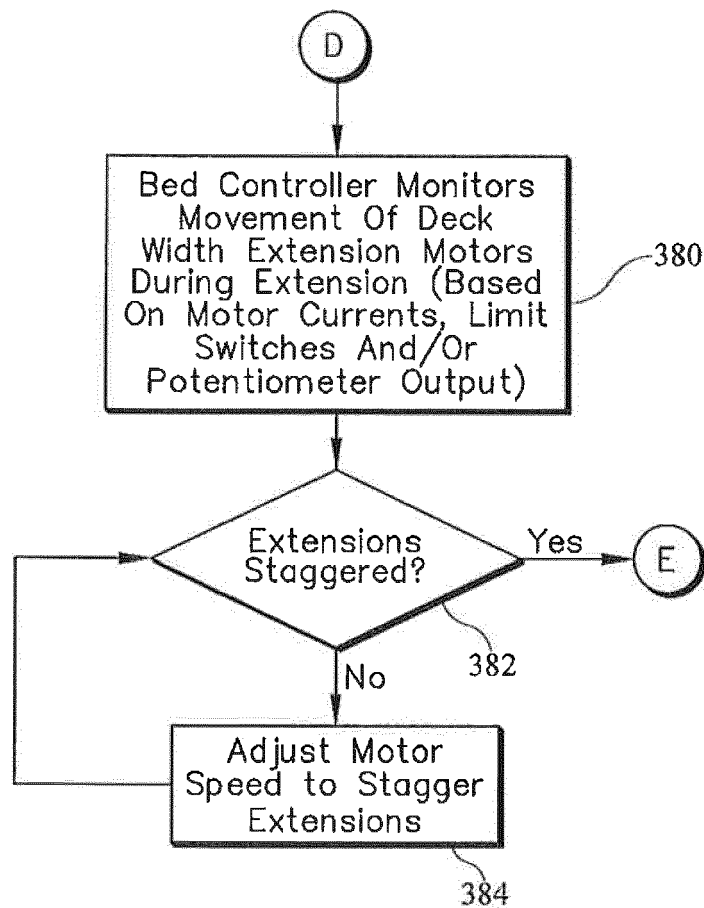
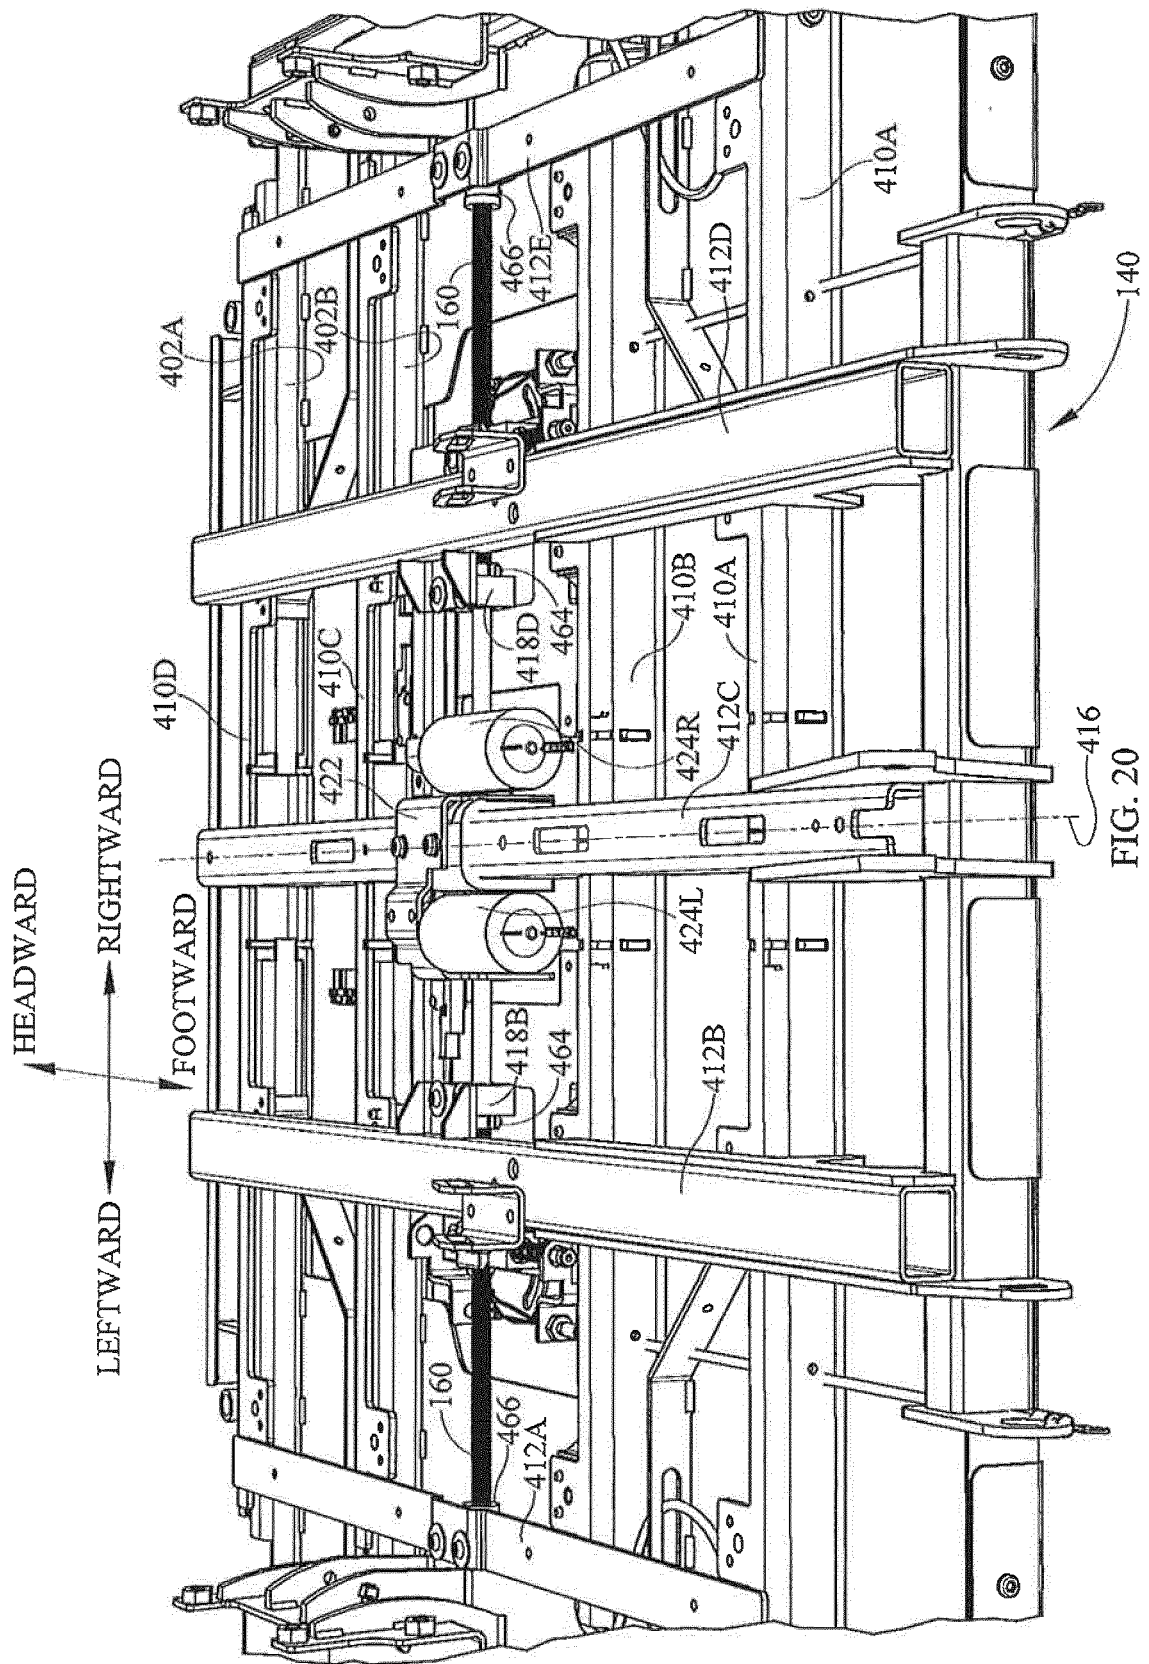
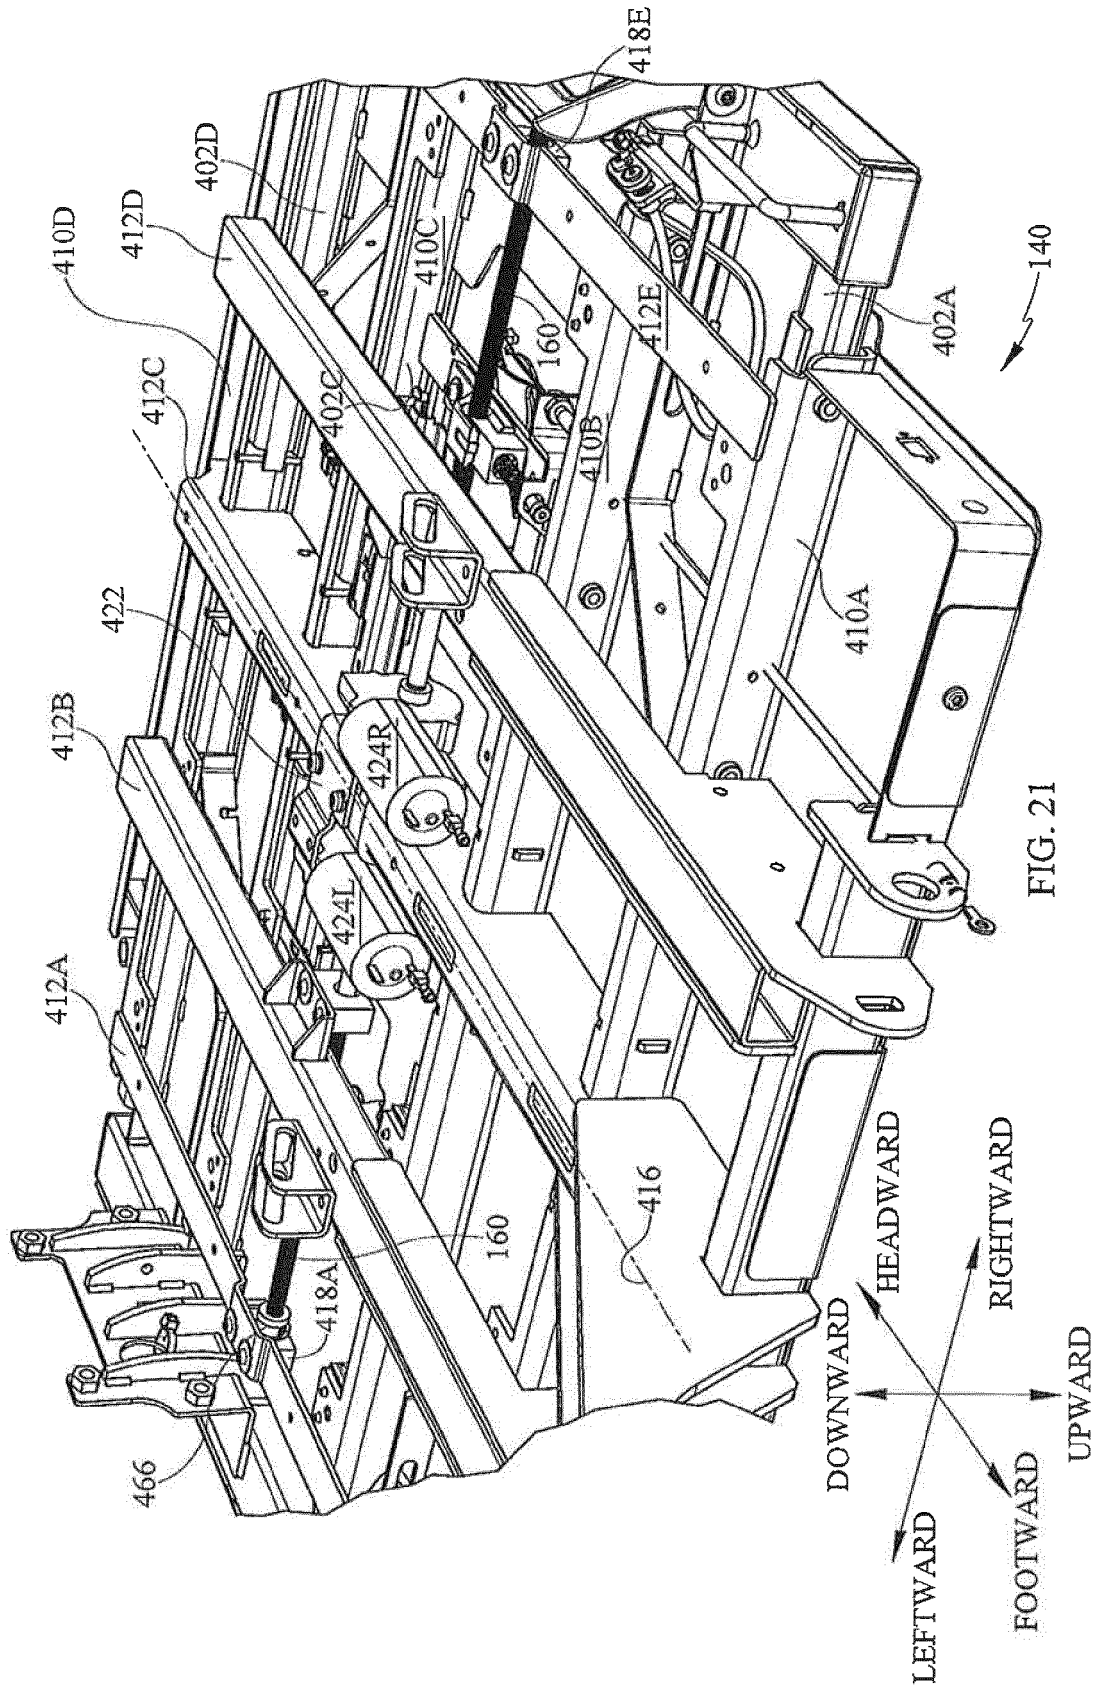


FIG. 19B





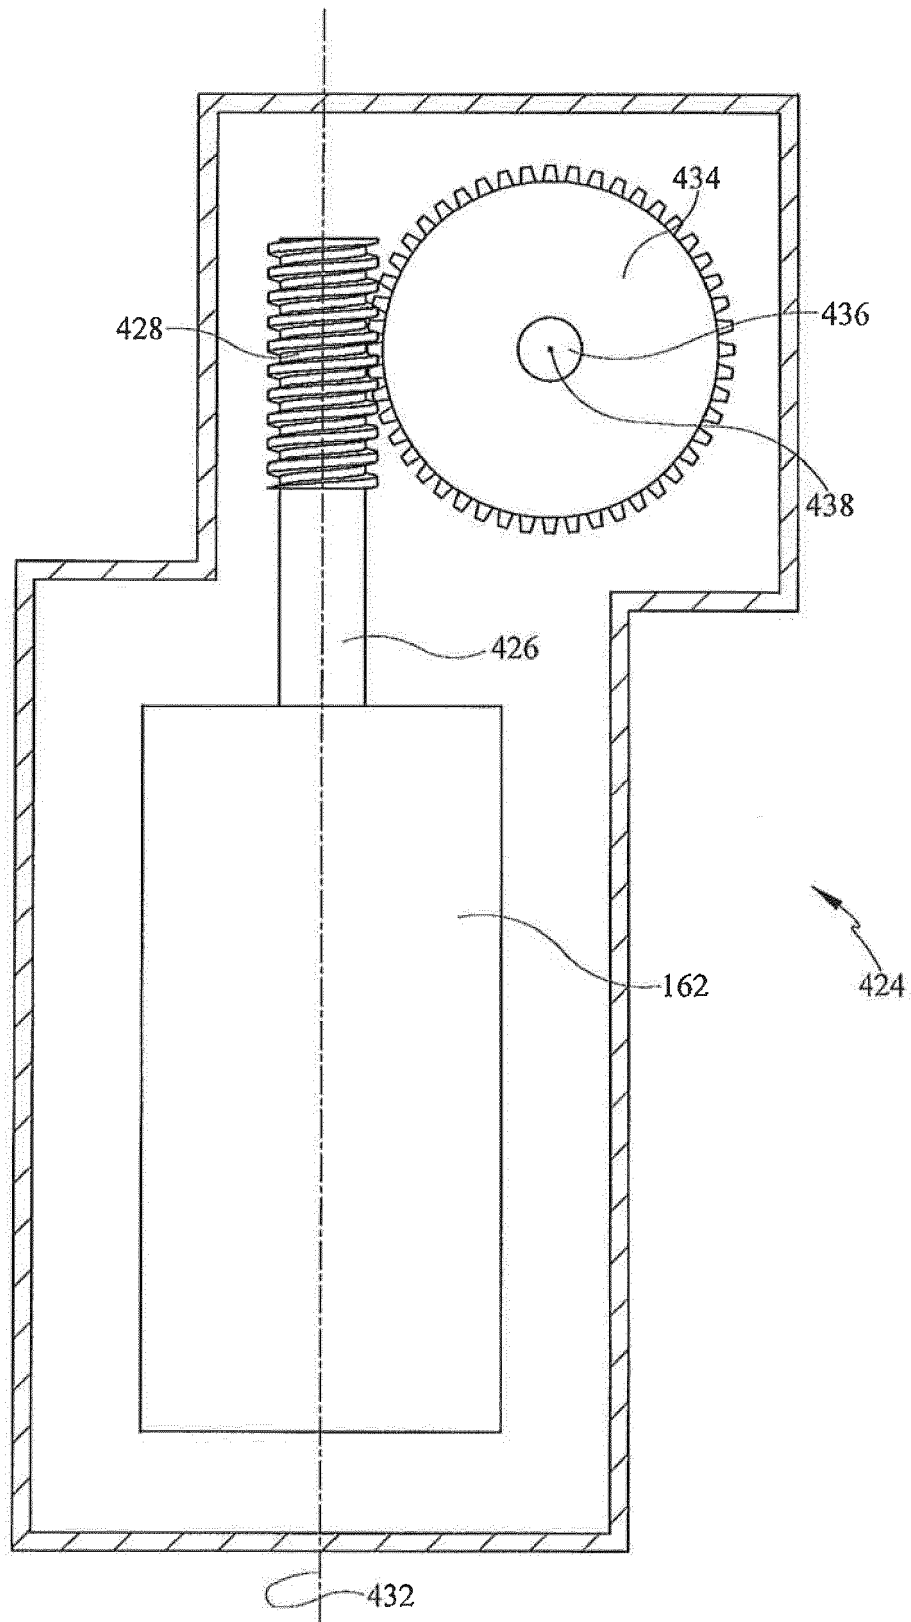


FIG. 22

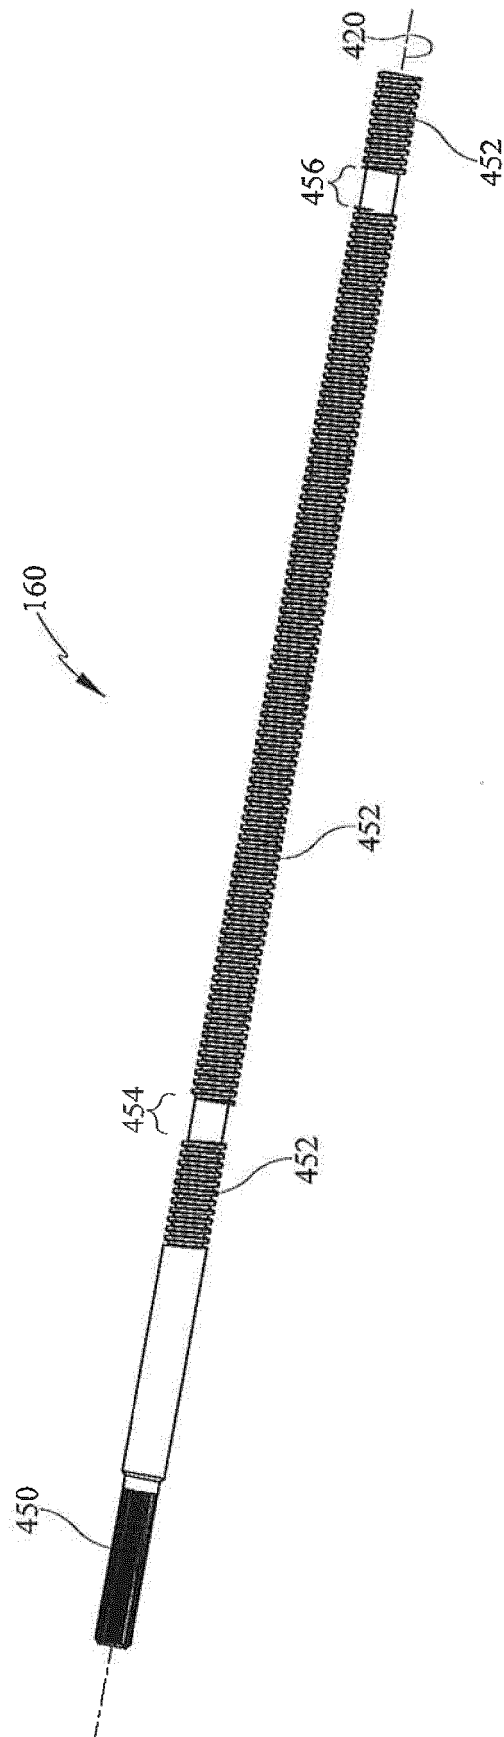


FIG. 23

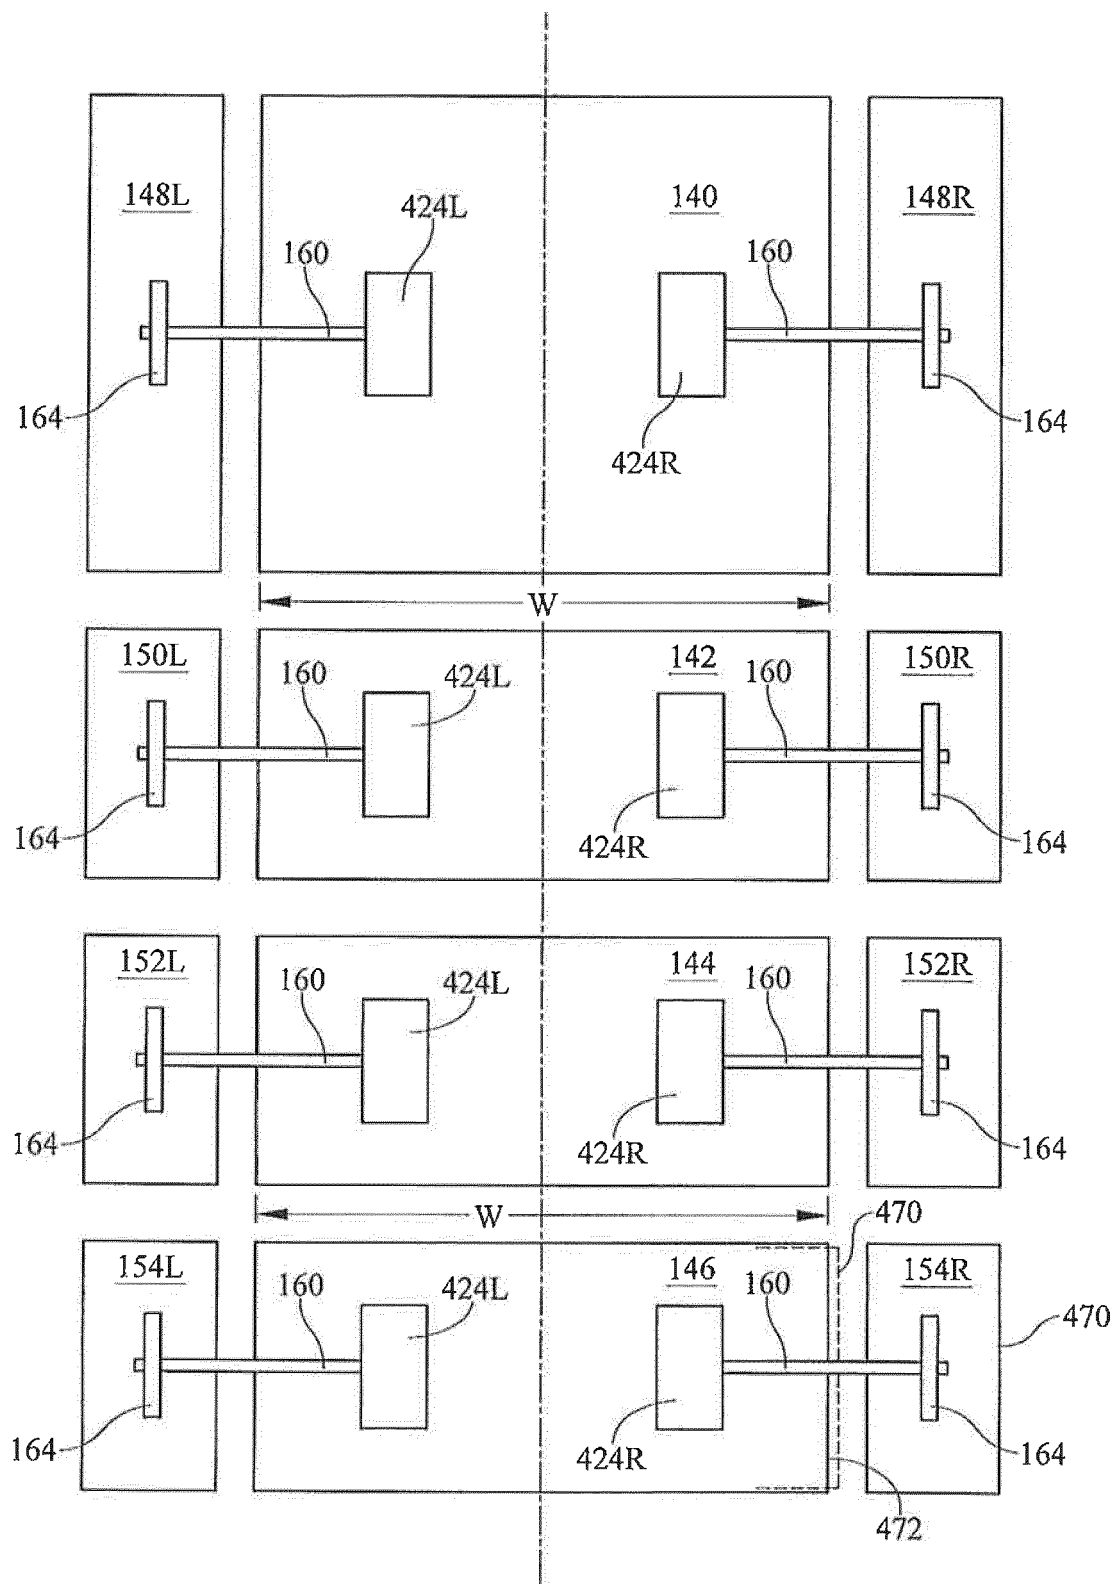


FIG. 24

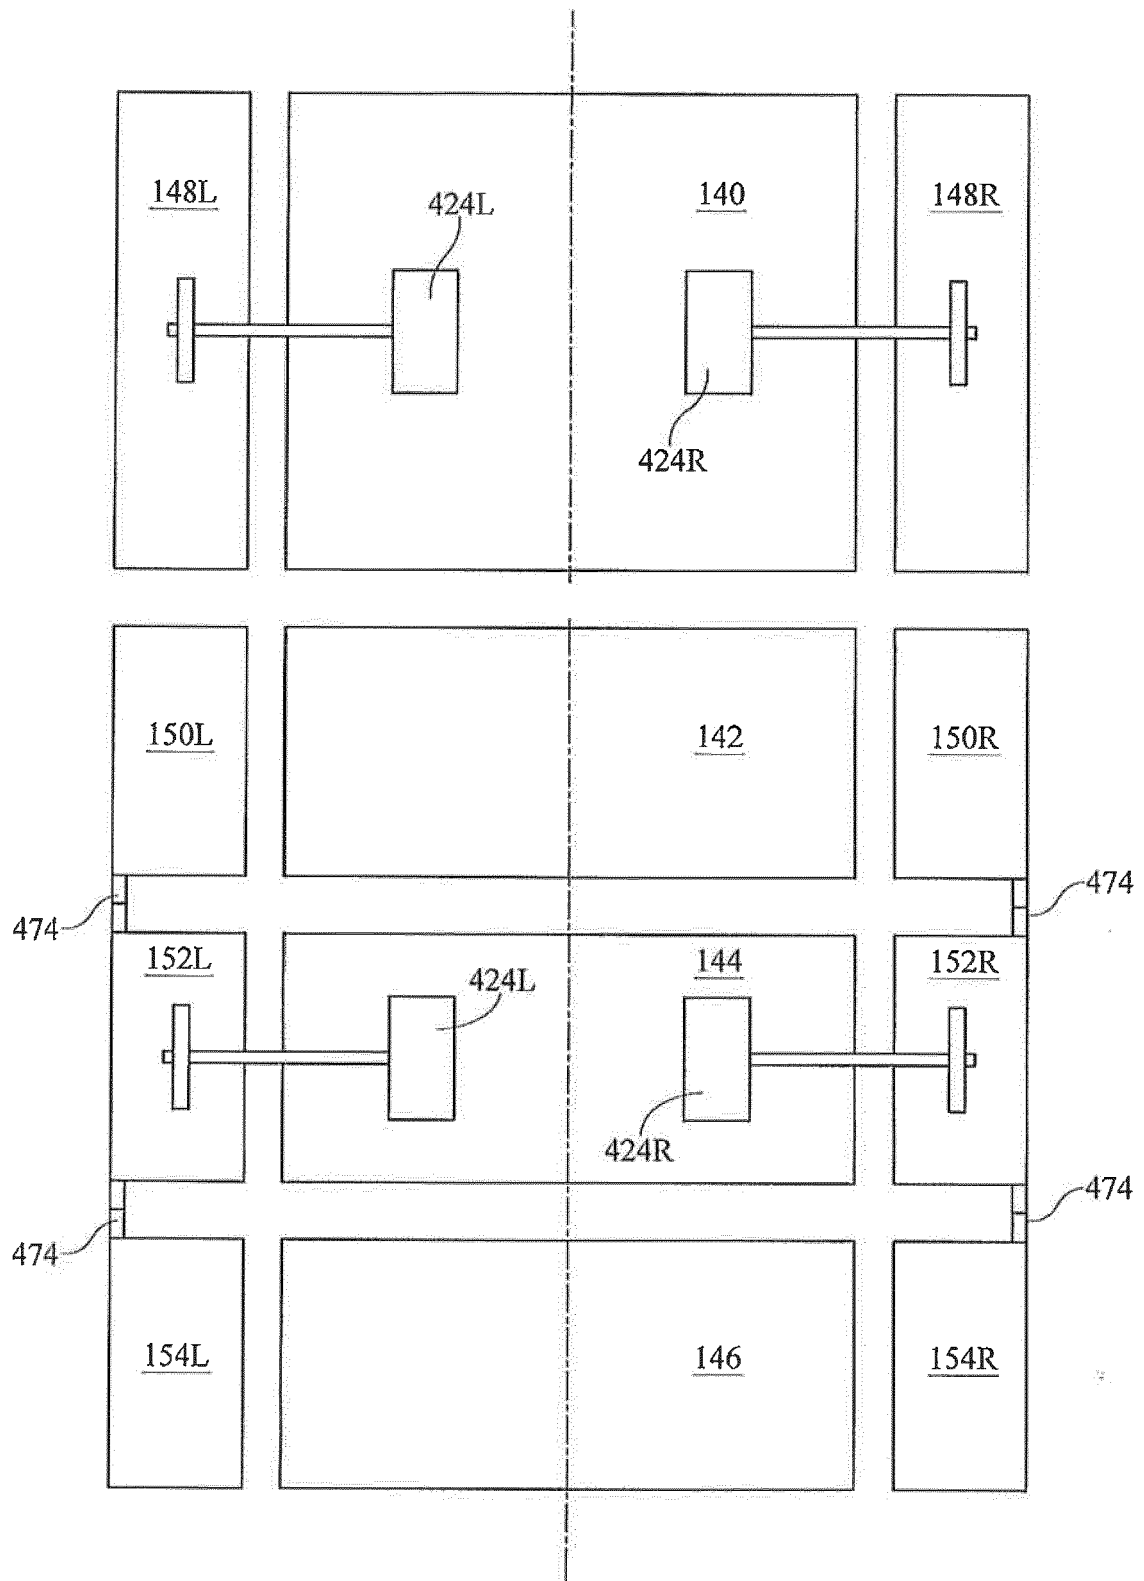


FIG. 25

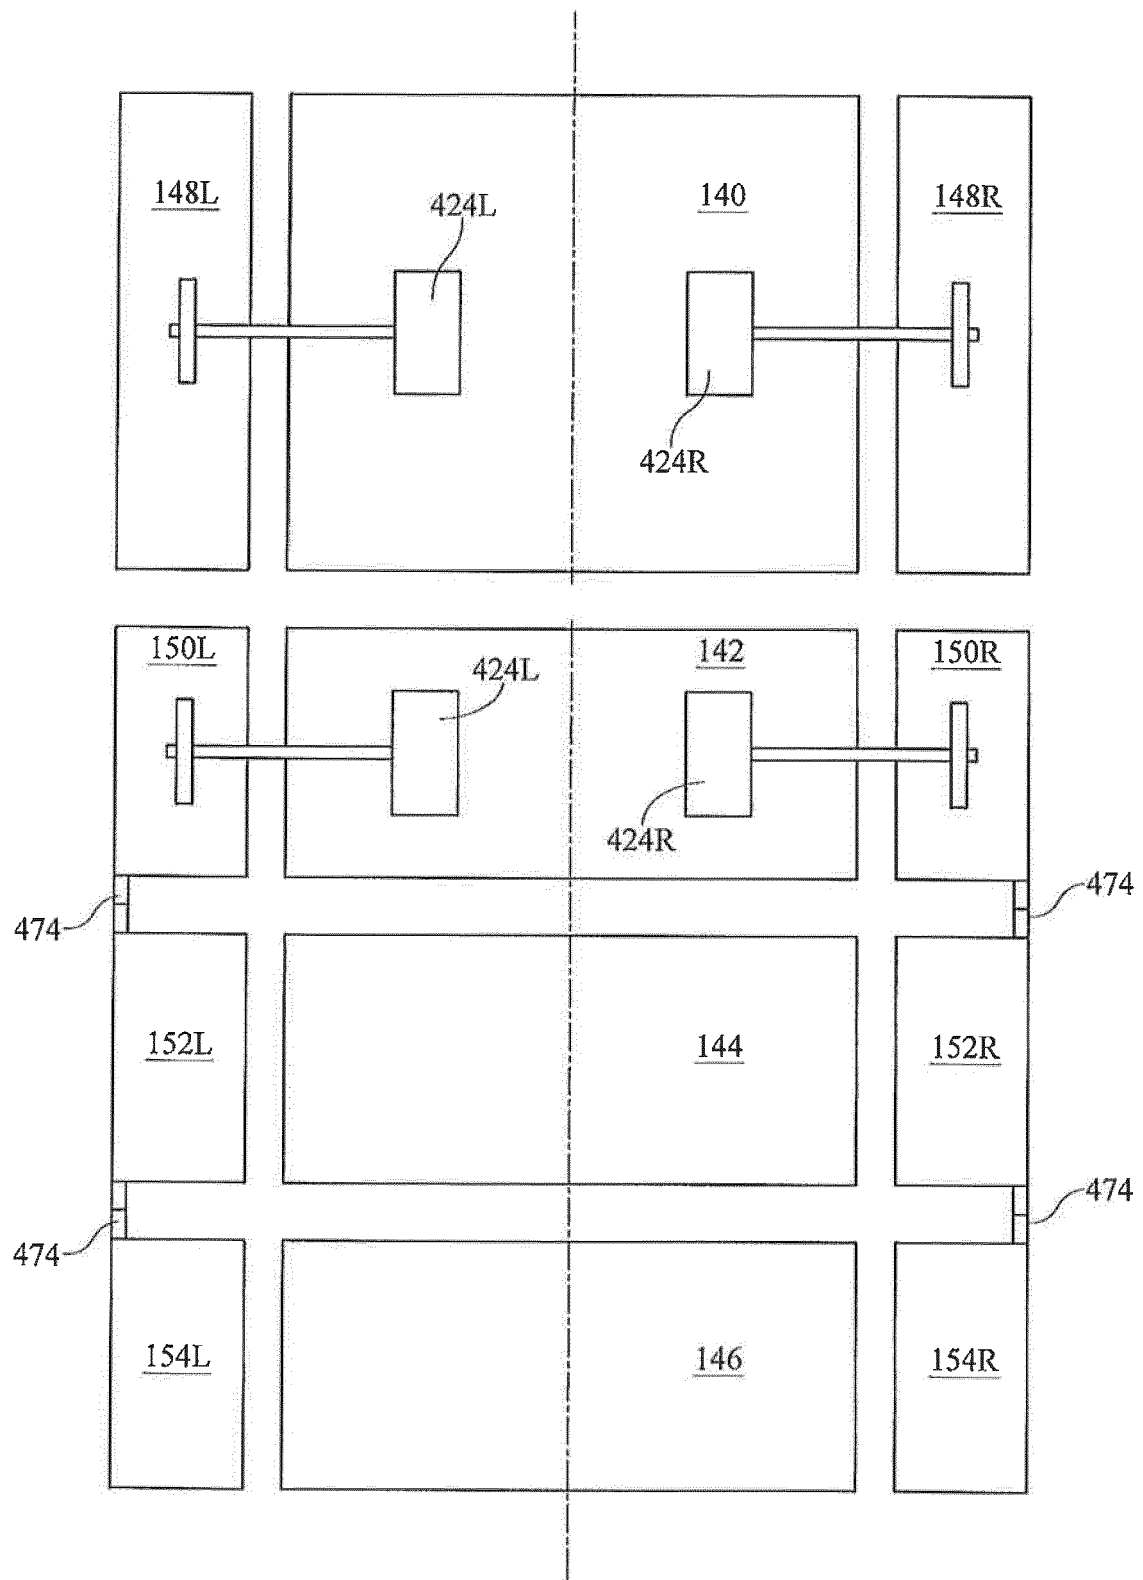


FIG. 26



EUROPEAN SEARCH REPORT

 Application Number
EP 15 17 0984

DOCUMENTS CONSIDERED TO BE RELEVANT			
Category	Citation of document with indication, where appropriate, of relevant passages	Relevant to claim	CLASSIFICATION OF THE APPLICATION (IPC)
X,D	US 2013/298331 A1 (BOSSINGHAM ROBERT [US] ET AL) 14 November 2013 (2013-11-14) * the whole document *	1-18	INV. A61G7/002 A61G7/015 A61G7/018
A	US 2008/000028 A1 (LEMIRE GUY [CA] ET AL) 3 January 2008 (2008-01-03) * paragraph [0081]; figures 18,19 *	1-18	
A,P	WO 2014/144593 A1 (KAP MEDICAL INC [US]) 18 September 2014 (2014-09-18) * paragraphs [0117] - [0124]; figures 16,23,24,32-36 *	1-18	
A,P	EP 2 762 122 A2 (HILL ROM SERVICES INC [US]) 6 August 2014 (2014-08-06)	1-18	
A,D,P	& US 2014/215717 A1 (RIGSBY MARK TYLER [US] ET AL) 7 August 2014 (2014-08-07) * the whole document *	1-18	
			TECHNICAL FIELDS SEARCHED (IPC)
			A61G
The present search report has been drawn up for all claims			
Place of search		Date of completion of the search	Examiner
The Hague		22 October 2015	Mammeri, Damya
CATEGORY OF CITED DOCUMENTS X : particularly relevant if taken alone Y : particularly relevant if combined with another document of the same category A : technological background O : non-written disclosure P : intermediate document T : theory or principle underlying the invention E : earlier patent document, but published on, or after the filing date D : document cited in the application L : document cited for other reasons & : member of the same patent family, corresponding document			

EPO FORM 1503 03.82 (P04C01)

**ANNEX TO THE EUROPEAN SEARCH REPORT
ON EUROPEAN PATENT APPLICATION NO.**

EP 15 17 0984

This annex lists the patent family members relating to the patent documents cited in the above-mentioned European search report.
The members are as contained in the European Patent Office EDP file on
The European Patent Office is in no way liable for these particulars which are merely given for the purpose of information.

22-10-2015

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
US 2013298331 A1	14-11-2013	EP 2662062 A2	13-11-2013
		US 2013298331 A1	14-11-2013

US 2008000028 A1	03-01-2008	EP 2046259 A2	15-04-2009
		US 2008000028 A1	03-01-2008
		WO 2008003027 A2	03-01-2008

WO 2014144593 A1	18-09-2014	CA 2906158 A1	18-09-2014
		US 2014259413 A1	18-09-2014
		WO 2014144593 A1	18-09-2014

EP 2762122 A2	06-08-2014	EP 2762122 A2	06-08-2014
		US 2014215717 A1	07-08-2014

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- US 774847 A [0006]
- US 11775083 A [0006]
- US 13468424 A [0006]
- US 14168538 A [0006]