

(19)



(11)

EP 3 056 277 A1

(12)

EUROPEAN PATENT APPLICATION

(43) Date of publication:
17.08.2016 Bulletin 2016/33

(51) Int Cl.:
B01L 7/04 (2010.01) **B01L 7/00** (2006.01)
B01L 9/06 (2006.01) **B01L 9/00** (2006.01)

(21) Application number: **15000420.8**

(22) Date of filing: **12.02.2015**

(84) Designated Contracting States:
**AL AT BE BG CH CY CZ DE DK EE ES FI FR GB
GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO
PL PT RO RS SE SI SK SM TR**
Designated Extension States:
BA ME

(72) Inventors:
• **Kling, Stephan**
78054 Schwenningen (DE)
• **Bruch, Christian**
78244 Gottmadingen (DE)

(71) Applicant: **QIAGEN Lake Constance GmbH**
78333 Stockach (DE)

(74) Representative: **Raible Deissler Lehmann**
Patentanwälte
Bolzstraße 3
70173 Stuttgart (DE)

(54) **Tempering clamp**

(57) The invention refers to a tempering clamp and a method for using this tempering clamp. The tempering clamp comprises first and second tempering elements associated to first and second clamping jaws.

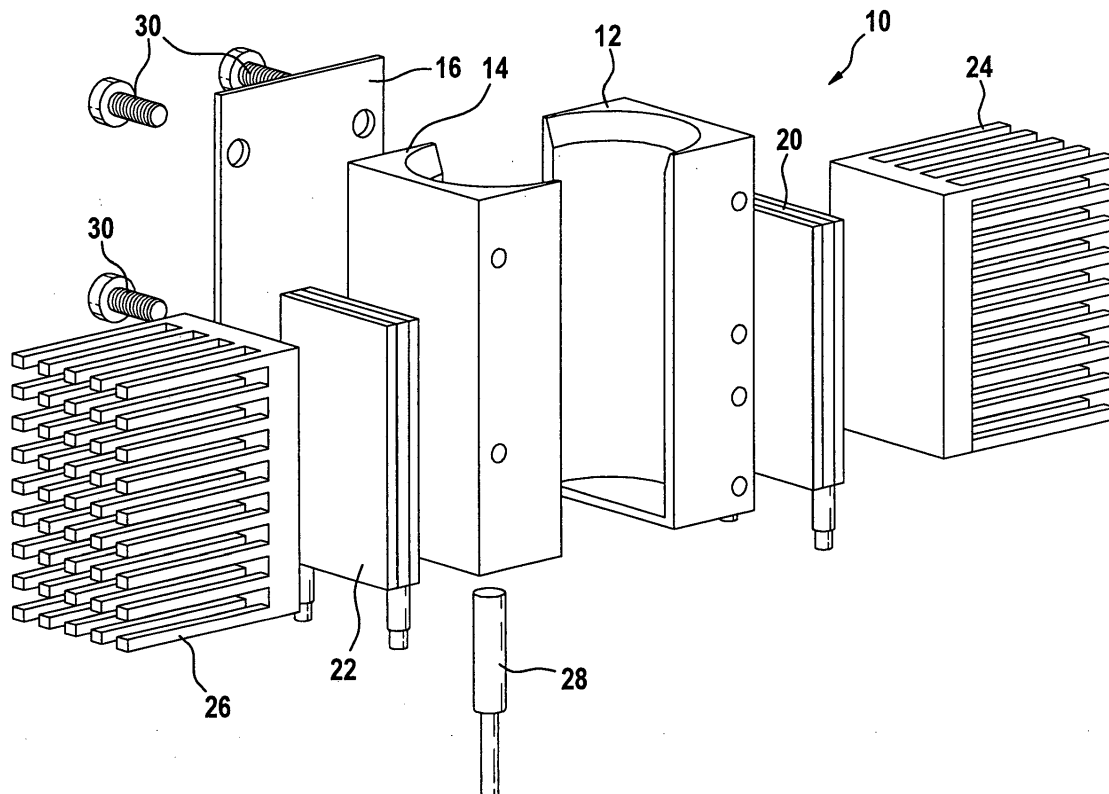


Fig. 1

EP 3 056 277 A1

Description

Field of the invention

[0001] The present invention relates to a tempering clamp for a sample container used for holding the container and heating or cooling the sample contained within the container.

Description of the related art

[0002] Generally, sample holders known in the art are rigid and inflexible and therefore, hardly suitable for providing tolerance compensation of different sample holders or sample tubes.

[0003] It is known in the art to use sample holders together with tempering elements in the domain of chemistry and medical science in order to temper, i.e. to heat or to cool, the sample contained within the sample holder.

[0004] Using conical or conical/cylindrical formed sample tubes a close contact can be achieved by pressing against the conical part of the heating element by pressure from above. For this, an additional corresponding device is necessary allowing for axial force transmission, for example, by a pressing lid. During tempering, the sample tube is not accessible at all even not from above. Therefore, no sample tubes can be used which form part of a microfluidic environment as a microfluidic chip.

Summary of the invention

[0005] In contrast thereto, the invention proposes a tempering clamp according to claim 1, for holding a sample container and for tempering a sample contained within the sample container. The tempering clamp comprises first and second clamping jaws movably, especially manually movably, connected by a spring element, and first and second tempering elements. The first tempering element is associated, e.g. connected or attached, to the first clamping jaw and the second tempering element is associated, e.g. connected or attached, to the second clamping jaw.

[0006] In one embodiment, a first heat insulator is attached to the first tempering element and a second heat insulator is attached to the second tempering element.

[0007] Furthermore, the first and second heat insulators can be cooling elements.

[0008] In another embodiment, the first and second tempering elements are adapted for heating and/or cooling the sample. Peltier elements can be used as tempering elements.

[0009] In one embodiment, an element is provided for effecting contact pressure in axial direction.

[0010] Furthermore, the spring element comprises a spring steel sheet.

[0011] For monitoring and controlling the tempering process a temperature sensor can be provided. Further sensors, e.g. for pH-value, oxygen partial pressure, etc.,

can be provided.

[0012] In one embodiment, the spring element is biased. Furthermore, outer surfaces of the tempering clamp can constitute an inwardly directed V-form. This can be achieved, for example, by biasing the spring element.

[0013] Moreover, the tempering clamp can be adapted to receive a microfluidic chip.

[0014] A method for holding a sample container and tempering a sample contained within the sample container uses a tempering clamp according to one of claims 1 to 12.

[0015] In one embodiment, the tempering process is monitored by a sensor inserted into the sample container from above.

[0016] The present application proposes a clamp serving as a heating element which is suitable for holding a sample tube serving as a sample container to be tempered and holding the sample holder with a radial pressure. In one embodiment, the clamp comprises two half shells reproducing the three-dimensional structure of the sample tube. However, the cavity between the half shells can be slightly smaller than the volume of the sample tube. The two half shells are connected by a flat spring which will be extended during insertion of the sample tube into the cavity between the half shells automatically building a radial contact pressure onto the outside surface of the sample tube.

[0017] Further features and embodiments of the invention will become apparent from the description and the accompanying drawings.

[0018] It will be understood that the features mentioned above and those described hereinafter can be used not only in the combination specified but also in other combinations or on their own, without departing from the scope of the present invention.

[0019] The invention is diagrammatically illustrated in the drawings by means of an embodiment by way of example and is hereinafter explained in detail with reference to the drawings. It is understood that the description is in no way limiting on the scope of the present invention and is merely an illustration of a preferred embodiment of the invention.

Brief description of the Drawings

[0020] In the drawings,

Figure 1 is an overall view of a tempering clamp according to the invention in exploded view,

Figure 2 is an overall view of the tempering clamp shown in figure 1 in assembled condition,

Figure 3 is a rear view of the tempering clamp,

Figure 4 is an overall view of the tempering clamp and a sample view inserted into the tempering clamp,

Figure 5 is a view of a detail in figure 4.

Detailed Description

[0021] The figures are described cohesively and in overlapping fashion, the same reference numerals denoting identical parts.

[0022] Figure 1 shows an embodiment of the tempering clamp in exploded view generally denoted with reference number 10. The tempering clamp 10 shown comprises a first clamping jaw 12 and a second clamping jaw 14 connected by a spring steel sheet 16. Furthermore, the drawing shows a first peltier element 20, a second peltier element 22, a first cooling element 24, a second cooling element 26, a temperature sensor 28, and a number of fastening elements 30.

[0023] The spring steel sheet 16 is the spring element connecting the two clamping jaws forming the half shells of the tempering clamp 10. In the shown embodiment the peltier elements 20, 22 are the tempering elements being able to heat and to cool. The cooling elements 24, 26 serve as insulating elements. These cooling elements 24, 26 are constructed as blocks having cooling fins.

[0024] Figure 2 illustrates the tempering clamp 10 assembled in front view. The drawing shows the first clamping jaw 12, the second clamping jaw 14 connected and pressed together by the spring steel sheet 16, the first peltier element 20, the second peltier element 22, the first cooling element 24, the second cooling element 26, and the temperature sensor 28.

[0025] Figure 3 shows the tempering clamp 10 in rear view illustrating the rear side of the tempering clamp 10 with the spring steel sheet 16 connecting the first clamping jaw 24 and the second clamping jaw 26 at their rear edges fixed by the fastening elements 30.

[0026] Figure 4 shows the tempering clamp 10 together with a sample tube 50 inserted into the tempering clamp 10, especially in between the two clamping jaws 12 and 14 of the tempering clamp 10. Furthermore, a microfluidic chip is attached to the tempering clamp 10. The tempering clamp 10 serves as a lysis clamp the microfluidic chip is attached to.

[0027] Figure 5 shows a detail of figure 4 encircled and denoted with reference number 52. The drawing shows the sample tube 50 inserted in between the two clamping jaws 12, 14. The sample tube 50 is securely fixed in the cavity between the two clamping jaws 12, 14 by means of the contact pressure caused by the spring element connecting the two clamping jaws 12, 14. As the sample tube is slightly bigger than the cavity in the tempering clamp there is a gap 54 between the front edges 62, 64 of the two clamping jaws 12, 14.

[0028] The tempering clamp according to the invention can be used for sample tubes which are rigidly connected to a microfluidic chip and can be heated up to 60 °C. The sample contained in the sample tube can contain biological cells in suspension and a so-called lysis buffer. By influence of the buffer and the increased temperature,

the cells will be decomposed, that means lysed.

[0029] After completion of the lysis, the liquid overlap of the sample tube will be transferred into the microfluidic of the chips. Therefore, the lid on the sample tube must be manipulated.

[0030] In this case, the head room filled by air of the tube will be pressurized by pumping air so that liquid can rise through a riser pipe. It is also possible to work with negative pressure. In both cases, it must be accessible by corresponding pipes. On the chip, there are micro-mechanic valves which can be operated by external actors.

[0031] Furthermore, applications for the tempering clamp are in the field of a thermostating chamber for incubation, biochemical reactions as amplification reactions, kinetic measurements or similar applications needing a rapid heat transportation.

[0032] The application enables a fast heat transfer from a heating block to a sample tube containing a sample, in many cases a liquid sample.

[0033] For this purpose, the tempering clamp provides a close contact of the heating element by radial contact pressure onto the sample tube to compensate for tolerances of the heating element and the sample tube. The contact pressure should be automatically adjusted by insertion of the sample tube into the heating element.

[0034] Manual adjustment of the contact pressure or other measures and arrangements, as, for example, additional components or manipulation by the user, should be avoided.

[0035] To solve this problem, the invention provides in one embodiment a heatable sample tube holder in form of a clamp or bracket consisting of two half shells being connected by a flat spring element. The spring element causes a pressure being effective in radial direction by insertion of the sample tube by means of contact faces of the clamp onto the wall of the sample tube.

[0036] The two half shells form a cavity in between each other correspondig to the form of the sample tube. It is to be noted that the outer circumference or outer volume of the sample tube should be slightly bigger than the inner circumference or inner volume, respectively, of the clamp to cause the spring contact pressure.

[0037] In one embodiment, the sample tube is cylindrical. Accordingly, the two half shells as well form a cylindrical cavity. The outer surfaces of the clamp can be plane in order to attach the heating elements an the body of the flat spring. Thereby, in one embodiment, the result is a clamp having a rectangular or quadratic layout, projected alongside the cylindrical axis.

[0038] In another embodiment, the outer surfaces of the clamp the flat spring is attached to constitute a flat inwardly directed V-form. Thus, the flat spring is biased and having the same spring constant the contact caused by insertion of a sample tube is higher in comparison with a clamp having a rectangular layout.

[0039] The cavity in between the two half shells can be conical, conical/cylindrical in shape. The conical part

should be in the lower part of the cavity in case the sample tube is inserted top down.

[0040] The clamp according to the inventions provides for an optimal thermal contact between the heating element and the sample container to be tempered by radial pressing the heated contact faces without the need for using additional components or additional manual steps.

[0041] The contact pressure is defined to a certain extent by the spring constant and the difference in dimension between the inner volume of the cavity of the clamp and the outer volume of the sample tube. In case fastening faces being in V-form to each other the pressure is additionally defined by the bias force and the structure of the layout of the tempering clamp for the flat spring.

[0042] Furthermore, the sample tube remains accessible from above during tempering. Therefore, a fluidic functional part, for example a microfluidic chip, can be connected to the sample tube by means of a suitable adapter as a thread, bayonet, plug or clip connection. In this manner fluidic processes can be performed with the fluid contained within the sample tube.

[0043] Alternatively, the processes within the tempered sample tube can be monitored by means of an optical aperture or corresponding optical detection and supervising devices. The tempering procedure can be supervised by detectors or sensors inserted from above (temperature, pH-value, oxygen partial pressure, etc.). Furthermore, the sample tube can be charged or discharged from above. Moreover, the pressure in the region above the liquid can be increased or decreased.

Claims

1. Tempering clamp for holding a sample container and for tempering a sample contained within the sample container, wherein the tempering clamp comprises first and second clamping jaws movably connected by a spring element, and first and second tempering elements, wherein the first tempering element is associated to the first clamping jaw and the second tempering element is associated to the second clamping jaw.
2. Tempering clamp according to claim 1, wherein a first heat insulator is attached to the first tempering element and a second heat insulator is attached to the second tempering element.
3. Tempering clamp according to claim 2, wherein the first and second heat insulators are cooling elements.
4. Tempering clamp according to one of claims 1 to 3, wherein the first and second tempering elements are adapted for heating the sample.
5. Tempering clamp according to one of claims 1 to 4,

wherein the first and second tempering elements are adapted for cooling the sample.

6. Tempering clamp according to one of claims 1 to 5, wherein peltier elements are used as tempering elements.
7. Tempering clamp according to one of claims 1 to 6, wherein an element is provided for effecting contact pressure in axial direction.
8. Tempering clamp according to one of claims 1 to 7, wherein the spring element comprises a spring steel sheet.
9. Tempering clamp according to one of claims 1 to 8, further comprising a temperature sensor.
10. Tempering clamp according to one of claims 1 to 9, wherein the spring element is biased.
11. Tempering clamp according to one of claims 1 to 10, wherein outer surfaces of the tampering clamp constitute an inwardly directed V-form.
12. Tempering clamp according to one of claims 1 to 11, wherein the tempering is adapted to receive a microfluidic chip.
13. Method for holding a sample container and tempering a sample contained within the sample container, using a tempering clamp according to one of claims 1 to 12.
14. Method according to claim 13, wherein the tempering process is monitored by a sensor inserted into the sample container from above.

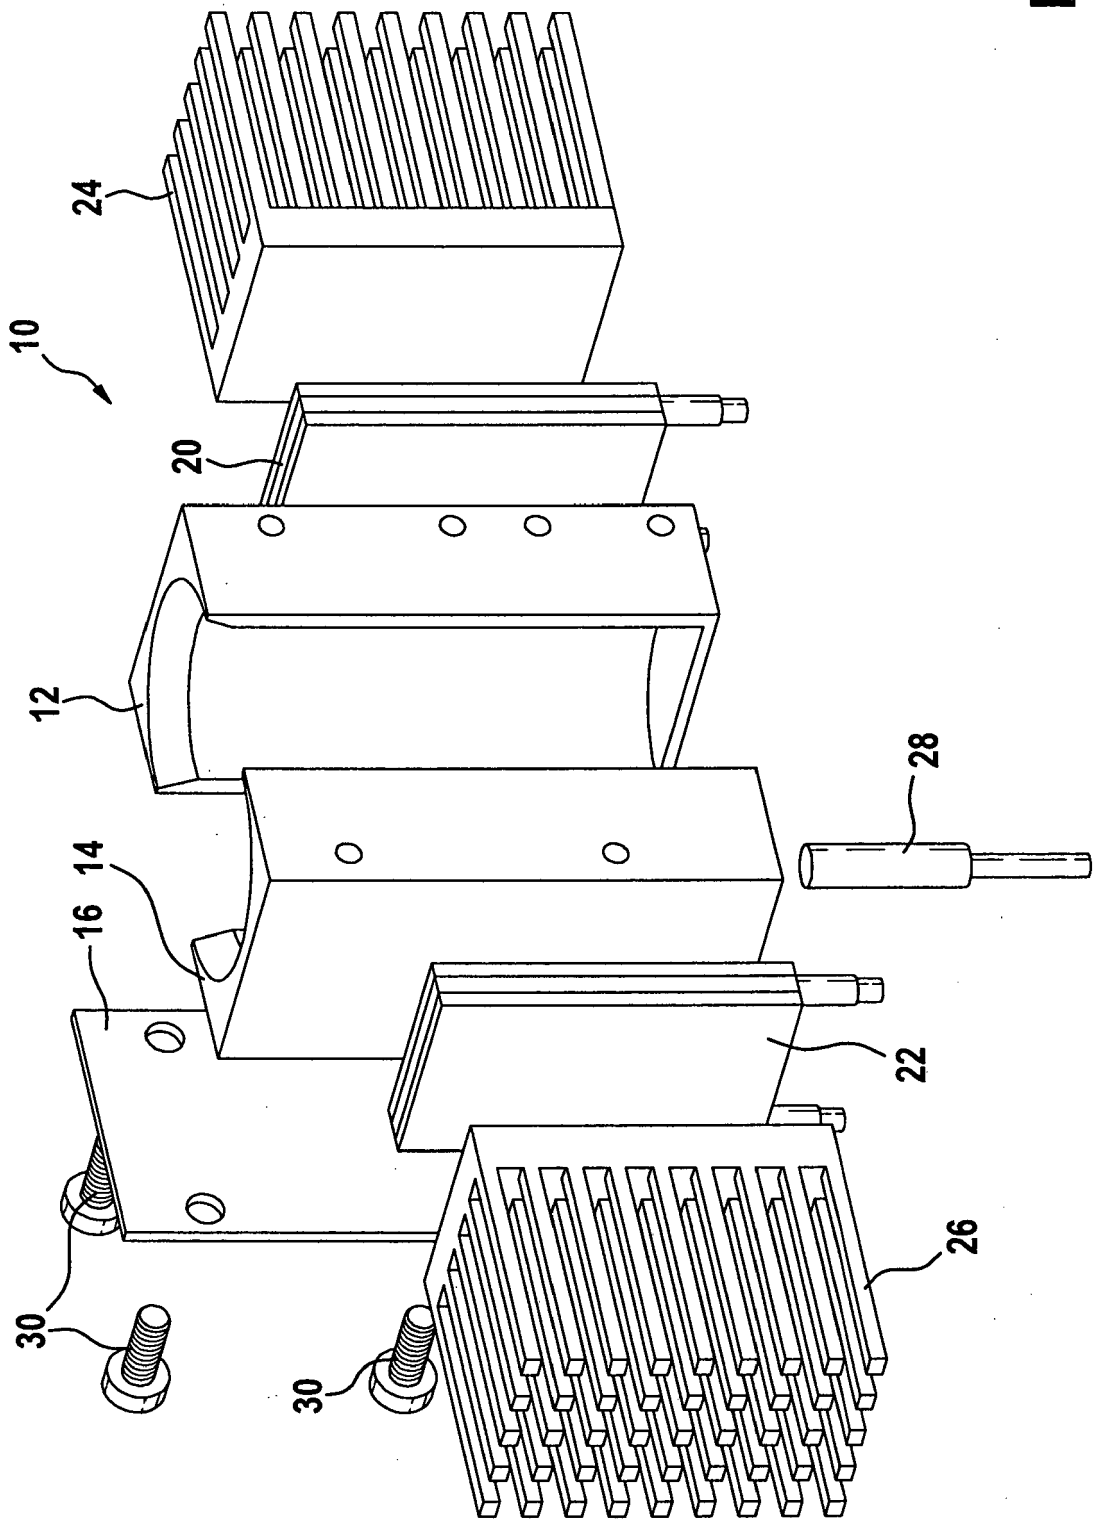


Fig. 1

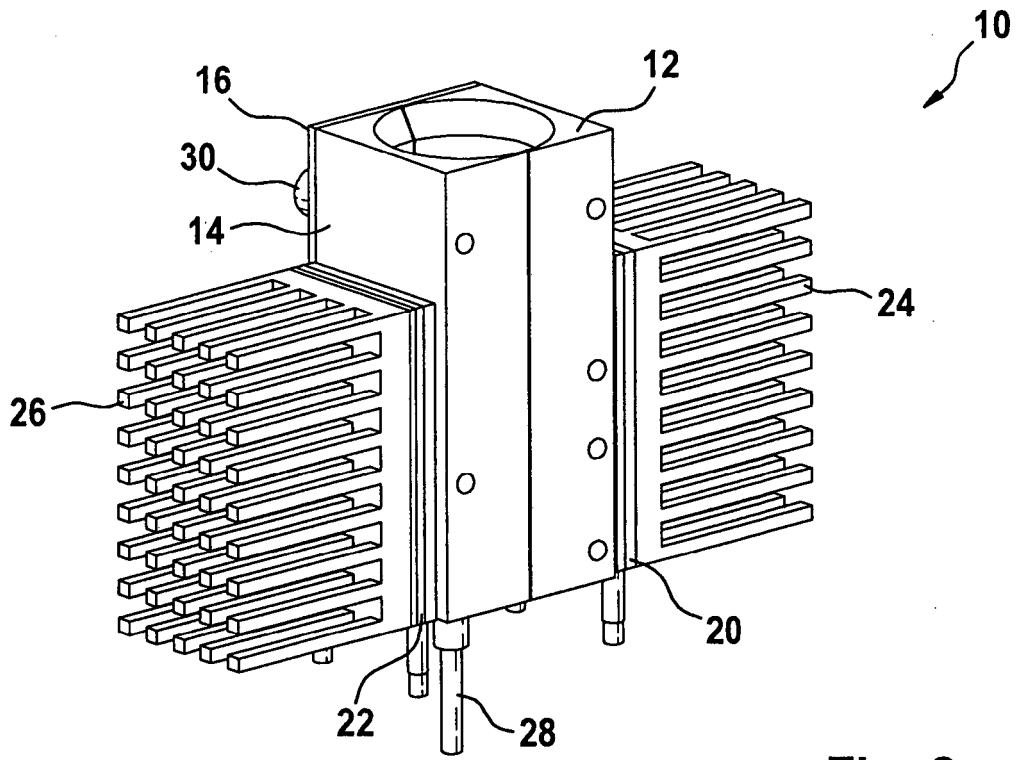


Fig. 2



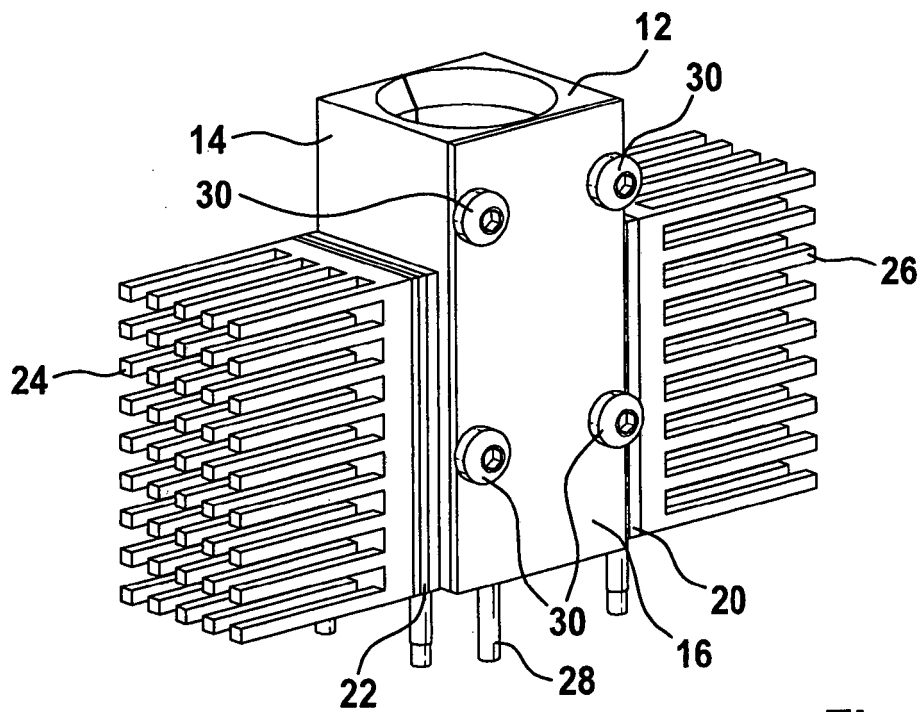


Fig. 3

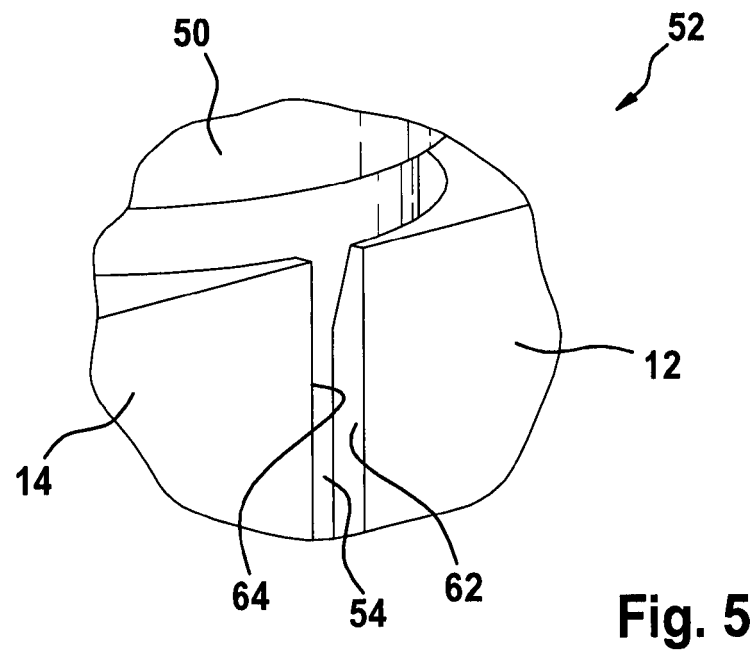

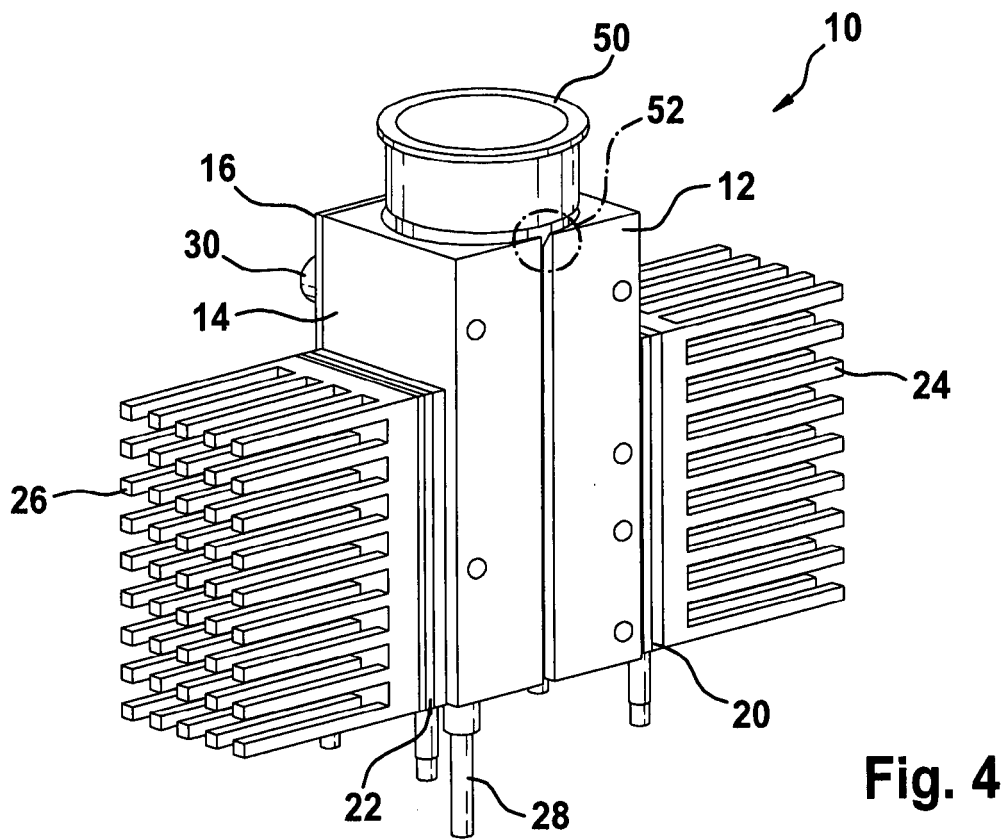

EUROPEAN SEARCH REPORT

 Application Number
EP 15 00 0420

5

10

15

20

25

30

35

40

45

50

55

DOCUMENTS CONSIDERED TO BE RELEVANT			
Category	Citation of document with indication, where appropriate, of relevant passages	Relevant to claim	CLASSIFICATION OF THE APPLICATION (IPC)
X	US 5 795 547 A (MOSER ROLF [CH] ET AL) 18 August 1998 (1998-08-18) * column 3, lines 30-36, 47-53 * * column 4, lines 4-7, 26-36, 39-59 * * column 6, line 21 - line 27 * * column 6, line 66 - column 7, line 11 * * figures 1-6 *	1-14	INV. B01L7/04 B01L7/00 B01L9/06 B01L9/00
A	US 2012/244047 A1 (TENG PING-HUA [TW] ET AL) 27 September 2012 (2012-09-27) * the whole document *	1-14	
			TECHNICAL FIELDS SEARCHED (IPC)
			B01L
The present search report has been drawn up for all claims			
Place of search The Hague		Date of completion of the search 28 July 2015	Examiner Bischoff, Laura
CATEGORY OF CITED DOCUMENTS X : particularly relevant if taken alone Y : particularly relevant if combined with another document of the same category A : technological background O : non-written disclosure P : intermediate document T : theory or principle underlying the invention E : earlier patent document, but published on, or after the filing date D : document cited in the application L : document cited for other reasons & : member of the same patent family, corresponding document			

 2
EPO FORM 1503 03.82 (P04C01)

**ANNEX TO THE EUROPEAN SEARCH REPORT
ON EUROPEAN PATENT APPLICATION NO.**

EP 15 00 0420

5 This annex lists the patent family members relating to the patent documents cited in the above-mentioned European search report.
The members are as contained in the European Patent Office EDP file on
The European Patent Office is in no way liable for these particulars which are merely given for the purpose of information.

28-07-2015

10

Patent document
cited in search report

Publication
date

Patent family
member(s)

Publication
date

15

US 5795547 A 18-08-1998

AT 199222 T 15-03-2001

AT 211023 T 15-01-2002

AT 211024 T 15-01-2002

CA 2130013 A1 11-03-1995

DE 59409658 D1 29-03-2001

DE 59410020 D1 31-01-2002

DE 59410021 D1 31-01-2002

DK 0642831 T3 21-05-2001

EP 0642831 A1 15-03-1995

EP 0807467 A2 19-11-1997

EP 0807468 A2 19-11-1997

ES 2155456 T3 16-05-2001

ES 2169294 T3 01-07-2002

ES 2169295 T3 01-07-2002

GR 3035810 T3 31-07-2001

JP H07151764 A 16-06-1995

PT 642831 E 31-07-2001

US 5616301 A 01-04-1997

US 5795547 A 18-08-1998

20

25

30

US 2012244047 A1 27-09-2012

TW 201239089 A 01-10-2012

US 2012244047 A1 27-09-2012

35

40

45

50

55

ORM P0459