



(12) **CORRECTED EUROPEAN PATENT SPECIFICATION**

(15) Correction information:
Corrected version no 1 (W1 B1)
Corrections, see
Sequence listing
Remarks
Sequence listing replaced or added

(48) Corrigendum issued on:
27.09.2023 Bulletin 2023/39

(45) Date of publication and mention
of the grant of the patent:
07.06.2023 Bulletin 2023/23

(21) Application number: **17826643.3**

(22) Date of filing: **14.12.2017**

(51) International Patent Classification (IPC):
A61K 31/00 ^(2006.01) **A61K 9/00** ^(2006.01)
A61K 31/519 ^(2006.01) **A61P 35/00** ^(2006.01)
A61M 31/00 ^(2006.01)

(52) Cooperative Patent Classification (CPC):
A61K 31/519; A61K 9/4808; A61K 31/00;
A61P 35/00; A61K 9/08; A61K 9/10; A61M 31/00

(86) International application number:
PCT/US2017/066492

(87) International publication number:
WO 2018/112245 (21.06.2018 Gazette 2018/25)

(54) **TREATMENT OF A DISEASE OF THE GASTROINTESTINAL TRACT WITH A JAK INHIBITOR AND DEVICES**

BEHANDLUNG EINER ERKRANKUNG DES GASTROINTESTINALTRAKTES MIT EINEM
JAK-HEMMER UND VORRICHTUNGEN

TRAITEMENT D'UNE MALADIE DU TRACTUS GASTRO-INTESTINAL AVEC UN INHIBITEUR DE
JAK ET DISPOSITIFS ASSOCIÉS

(84) Designated Contracting States:
AL AT BE BG CH CY CZ DE DK EE ES FI FR GB
GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO
PL PT RO RS SE SI SK SM TR

(30) Priority: **14.12.2016 US 201662434374 P**
30.03.2017 US 201762478919 P
14.08.2017 US 201762545380 P
09.11.2017 US 201762583832 P

(43) Date of publication of application:
23.10.2019 Bulletin 2019/43

(60) Divisional application:
22209435.1 / 4 190 318

(73) Proprietor: **Biora Therapeutics, Inc.**
San Diego, CA 92122 (US)

(72) Inventors:
• **JONES, Mitchell Lawrence**
La Jolla, California 92037 (US)

- **SINGH, Sharat**
Rancho Santa Fe, California 92067 (US)
- **WAHL, Christopher Loren**
San Diego, CA 92103 (US)
- **STYLLI, Harry**
La Jolla, California 92037 (US)

(74) Representative: **Mewburn Ellis LLP**
Aurora Building
Counterslip
Bristol BS1 6BX (GB)

(56) References cited:
WO-A1-92/21307 WO-A1-2008/104968
WO-A1-2012/158648 WO-A1-2013/188783
WO-A1-2016/049602 WO-A1-2016/049602
WO-A1-2016/193964 WO-A2-01/45789
WO-A2-2004/066903 WO-A2-2008/053396
US-A1- 2013 129 675 US-A1- 2016 213 234

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

- PETER J. VAN DER SCHAAR ET AL: "A novel ingestible electronic drug delivery and monitoring device", GASTROINTESTINAL ENDOSCOPY, vol. 78, no. 3, 1 September 2013 (2013-09-01), pages 520-528, XP055349388, NL ISSN: 0016-5107, DOI: 10.1016/j.gie.2013.03.170
- BEATTIE DAVID T ET AL: "Intestinally-restricted Janus Kinase inhibition: a potential approach to maximize the therapeutic index in inflammatory bowel disease therapy", JOURNAL OF INFLAMMATION, BIOMED CENTRAL, LONDON, GB, [Online] vol. 14, no. 1: Article No.: 28, 6 December 2017 (2017-12-06), pages 1-11, XP009503913, ISSN: 1476-9255, DOI: 10.1186/S12950-017-0175-2 Retrieved from the Internet:
URL:<https://doi.org/10.1186/s12950-017-0175-2?nosfx=y>
- BOLAND BRIGID S ET AL: "Update on Janus kinase antagonists in inflammatory bowel disease", GASTROENTEROLOGY CLINICS OF NORTH AMERICA UNITED STATES SEP 2014, GASTROENTEROLOGY CLINICS OF NORTH AMERICA UNITED STATES SEP 2014, GASTROENTEROLOGY CLINICS OF NORTH AMERICA UNITED STATES SEP 2014, vol. 43, no. 3, 31 August 2014 (2014-08-31), pages 603-617, XP009503890, ISSN: 1558-1942, DOI: 10.1016/J.GTC.2014.05.011
- TIMMINS P ET AL: "Formulation technology can enable oral delivery of new generation medicines for inflammatory bowel disease", INDUSTRIAL PHARMACY / INTERNATIONAL PHARMACEUTICAL FEDERATION, INDUSTRIAL PHARMACISTS SECTION, EUROMED COMMUNICATIONS, HASLEMERE, SURREY, vol. 2016, no. 52, 1 December 2016 (2016-12-01), pages 4-18, XP009503912, ISSN: 1741-4911
- TSURUTA ET AL: "Liposome Encapsulated Doxorubicin Transfer to the Pelvic Lymph Nodes by Endoscopic Administration into the Bladder Wall: A Preliminary Report", JOURNAL OF UROL, LIPPINCOTT WILLIAMS & WILKINS, BALTIMORE, MD, US, vol. 157, no. 5, 1 May 1997 (1997-05-01), pages 1652-1654, XP005571906, ISSN: 0022-5347, DOI: 10.1016/S0022-5347(01)64822-5
- ASLAM M S & MAJEED F ED - ASLAM M S & MAJEED F: "Ingestible electronically controlled drug-capsule in the gut", J. DRUG DELIVERY & THERAPEUTICS,, vol. 2, no. 3, 11 May 2012 (2012-05-11), pages 1-3, XP002778207,
- SHIMIZU J ED - SHIMIZU J: "Smart pills for oral drug delivery", INTL. PHARM. INDUSTRY,, vol. 6, no. 3, 1 January 2014 (2014-01-01) , pages 72-74, XP002778208,
- VANDER SCHAAR P J ET AL: "A novel ingestible electronic drug delivery and monitoring device", GASTROINTEST. ENDOSC., vol. 78, no. 3, 1 January 2013 (2013-01-01), pages 520-528, XP002778209,
- BARTOLI R: "Efficacy of endoscopic placement of a drugeluting platform with infliximab for the treatment of mucosal lesions in a rat model of experimental colitis", UNITED EUROPEAN GASTROENTEROLOGY JOURNAL 20171001 SAGE PUBLICATIONS LTD NLD, vol. 5, no. 5, Supplement 1, 1 October 2017 (2017-10-01), XP009503969, ISSN: 2050-6414

Remarks:

The complete document including Reference Table(s) and the Sequence Listing(s) can be downloaded from the EPO website

Description**CROSS-REFERENCE TO RELATED APPLICATIONS**

[0001] This application claims the benefit of the following U.S. Provisional Applications: 62/434,374 filed December 14, 2016; 62/478,919 filed March 30, 2017; 62/545,380 filed August 14, 2017; and 62/583,832 filed November 9, 2017. This disclosure of the prior applications is considered part of (and is incorporated by reference in its entirety in) the disclosure of this application.

TECHNICAL FIELD

[0002] This disclosure features compositions for treating diseases of the gastrointestinal tract with a JAK inhibitor.

BACKGROUND

[0003] The Janus kinase (JAK) proteins are a family of non-receptor tyrosine kinases that possess a highly conserved kinase domain responsible for its enzymatic activity. Mammals have four members of this family, JAK1, JAK2, JAK3 and Tyrosine kinase 2 (TYK2). These kinases associate with the intracellular portion of cytokine or hormone receptors, and transduce signals through seven members of the STAT transcription factors - STAT1, STAT2, STAT3, STAT4, STAT5A, STAT5B, and STAT6 in various combinations. JAK1 promotes signaling of multiple cytokines (e.g., certain type I and type II cytokines), including pro-inflammatory cytokines involved in the pathogenesis of autoimmune diseases. Single-nucleotide polymorphisms within the JAK/STAT pathway that confer susceptibility to IBD have been identified (Jostins et al., Host-microbe interactions have shaped the genetic architecture of inflammatory bowel disease, *Nature* 491:119-124, 2012). Both in vivo and in vitro studies have confirmed the role of JAK/STAT signaling in regulating immune responses (O'Shea and Plenge, JAK and STAT signaling molecules in immunoregulation and immune-mediated disease, *Immunity* 36:542-550, 2012). Tofacitinib, selective oral JAK inhibitor (including JAK1 and JAK3) has been tested in clinical trials for both ulcerative colitis (Sandborn et al., Tofacitinib, an Oral Janus Kinase Inhibitor, in Active Ulcerative Colitis, *New England J. Med* 367:616-24, 2012; Panes et al., Randomized trial of tofacitinib in active ulcerative colitis: analysis of efficacy base on patient-reported outcomes, *BMC Gastroenterology* 15:14, doi: 10.1186/s12876-015-0239-9, 2015) and Crohn's disease. The gastrointestinal (GI) tract generally provides a therapeutic medium for an individual's body. At times, therapeutic drugs may need to be dispensed to specified locations within the small intestine or large intestine, which is more effective than oral administration of the therapeutic drugs to cure or alleviate the symptoms of some medical conditions. For example, therapeutic drugs dispensed directly within the small intestine would not be contaminated, digested or otherwise compromised in the stomach, and thus allow a higher dose to be delivered at a specific location within the small intestine. However, dispensing therapeutic drugs directly within the small intestine inside a human body (e.g., the cecum, the ascending colon) can be difficult, because a device or mechanism (e.g., special formulation) would be needed to transport a therapeutically effective dose of drug to a desired location within the small intestine and then automatically deliver the therapeutic drug at the desired location. Dispensing therapeutic drugs directly within other locations in the GI tract of the human body can be similarly difficult. Such a device or mechanism also would also need to be operated in a safe manner in that the device or mechanism needs to physically enter the human body. Ingestible devices for delivery of drugs in the gastrointestinal tract have been described in prior art (*J. Drug Delivery & Ther.* 2(3):1-8, 2012; *Intl. J. Pharm. Ind.* 6(3):72-74; *Gastrointest. Endosc.* 78(3):520-528; WO2016049602; WO2004/066903). However, none of these disclose the effective delivery of drugs in the cecum.

[0004] In sum, there remains a significant unmet medical need for improved treatment regimens for gastrointestinal diseases, such as inflammatory bowel disease (IBD), including a need for regimens which can dispense therapeutics to specific locations within the GI tract, thereby reducing or avoiding the drawbacks of oral or other forms of systemic administration.

SUMMARY

[0005] The invention is as defined in the appended claims. Any subject-matter falling outside the scope of the claims is provided for information purposes only. The references to methods of treatment in the summary and detailed description of the invention in this description are to be interpreted as references to the compounds, pharmaceutical compositions and medicaments of the present invention for use in a method for treatment of the human (or animal) body by therapy.

[0006] The technical teachings can be summarized as follows:

The present disclosure provides novel treatment paradigms for inflammatory conditions of the gastrointestinal tract. The methods and compositions described herein allow for the regio-specific release of therapeutic drugs in the cecum, wherein the site of disease is in the colon. By releasing a therapeutic drug locally instead of systemically, the bioavailability

of the drug can be increased at the site of injury and/or decreased in the systemic circulation, thereby resulting in improved overall safety and/or efficacy and fewer adverse side effects. Advantages may include one or more of increased drug engagement at the target, leading to new and more efficacious treatment regimens, and/or lower systemic drug levels, which can translate to reduced toxicity and reduced immunogenicity, e.g., in the case of biologics. In some instances,

releasing a therapeutic drug locally also provides for new modes of action that may be unique to local delivery in the cecum as opposed to systemic administration. For patients, clinicians and payors, this can mean an easier or simpler route of administration, fewer co-medicaments (e.g., immunomodulators), fewer side effects, and/or better outcomes.

[0007] Accordingly, described herein are methods for treating disorders of the gastrointestinal (GI) tract. The methods can include one or more of:

- diagnosing a GI disease in a subject; and/or
- mapping, sampling, and/or assessing the site, severity, pathology, and extent of a GI disease in the GI tract of a subject and/or mapping, sampling, and/or assessing a patient response to a therapeutic agent, e.g., in the patient's GI tract; and/or
- identifying, quantifying, and/or monitoring one or more markers of a GI disease in the GI tract of the subject and/or one or more markers of patient response to a therapeutic agent, e.g., in the patient's GI tract; and/or
- releasing a therapeutic agent in the cecum.

[0008] The present disclosure accordingly provides patients and physicians more personalized treatment options for GI disorders by facilitating regimens which can release a therapeutic agent according to desired (e.g., customized or optimized) dosage, timing, and/or location parameters. In some cases, the treatment methods can employ one or more ingestible devices to achieve the benefits disclosed herein.

[0009] Disclosed herein is a method of treating a disease of the gastrointestinal tract in a subject, comprising:

administering to the subject a pharmaceutical formulation that comprises an JAK inhibitor, wherein the pharmaceutical formulation is released in the cecum, wherein the site of disease is in the colon.

[0010] Provided herein the pharmaceutical formulation is administered in an ingestible device. In some disclosures, the pharmaceutical formulation is released from an ingestible device. In some disclosures, the ingestible device comprises a housing, a reservoir containing the pharmaceutical formulation, and a release mechanism for releasing the pharmaceutical formulation from the device, wherein the reservoir is releasably or permanently attached to the exterior of the housing or internal to the housing.

[0011] Provided herein is a method of treating a disease of the gastrointestinal tract in a subject, comprising:

administering to the subject an ingestible device comprising a housing, a reservoir containing a pharmaceutical formulation, and a release mechanism for releasing the pharmaceutical formulation from the device, wherein the reservoir is releasably or permanently attached to the exterior of the housing or internal to the housing; wherein the pharmaceutical formulation comprises an JAK inhibitor, and the ingestible device releases the pharmaceutical formulation in the cecum, wherein the site of disease is in the colon.

[0012] In some embodiments, the housing is non-biodegradable in the GI tract.

In some embodiments, the release of the formulation is triggered autonomously. In some embodiments, the location of one or more sites of disease is predetermined.

[0013] In some embodiments, the reservoir is made of a material that allows the formulation to leave the reservoir, such as a biodegradable material.

[0014] In some embodiments, the release of the formulation is triggered by a preprogrammed algorithm. In some embodiments, the release of the formulation is triggered by data from a sensor or detector to identify the location of the device. In some more particular embodiments, the data is not based solely on a physiological parameter (such as pH, temperature, and/or transit time).

[0015] In some embodiments, the device comprises a detector configured to detect light reflectance from an environment external to the housing. In some more particular embodiments, the release is triggered autonomously or based on the detected reflectance.

[0016] In some embodiments, the device releases the formulation at substantially the same time as one or more sites of disease are detected. In some embodiments, the one or more sites of disease are detected by the device (e.g., by imaging the GI tract).

[0017] In some embodiments, the release mechanism is an actuation system. In some embodiments, the release mechanism is a chemical actuation system. In some embodiments, the release mechanism is a mechanical actuation system. In some embodiments, the release mechanism is an electrical actuation system. In some embodiments, the

actuation system comprises a pump and releasing the formulation comprises pumping the formulation out of the reservoir. In some embodiments, the actuation system comprises a gas generating cell.

In some embodiments, the formulation comprises a therapeutically effective amount of the JAK inhibitor. In some embodiments, the formulation comprises a human equivalent dose (HED) of the JAK inhibitor.

[0018] In some embodiments, the device is a device capable of releasing a solid JAK inhibitor or a solid formulation comprising the JAK inhibitor. In some embodiments, the device is a device capable of releasing a liquid JAK inhibitor or a liquid formulation comprising the JAK inhibitor. Accordingly, in some embodiments, the pharmaceutical formulation released from the device is a solid formulation. In other embodiments, the pharmaceutical formulation release from the device is a liquid formulation.

[0019] The devices disclosed herein are capable of releasing a JAK inhibitor or a formulation comprising the JAK inhibitor irrespective of the particular type of JAK inhibitor. For example, the JAK inhibitor may be a small molecule, a biological, a nucleic acid, an antibody, a fusion protein, and so on.

[0020] Provided herein is a method of releasing an JAK inhibitor into the cecum of a subject for treating one or more sites of disease within the colon, the method comprising:

administering to the subject a therapeutically effective amount of the JAK inhibitor housed in an ingestible device, wherein the ingestible device comprises:

a detector configured to detect the presence of the one or more sites of disease, and
a controller or processor configured to trigger the release of the JAK inhibitor in the cecum in response to the detector detecting the presence of the one or more sites of disease.

[0021] Also provided herein is a method of releasing an JAK inhibitor into the cecum of a subject for treating one or more pre-determined sites of disease within the colon, the method comprising:

administering to the subject a therapeutically effective amount of the JAK inhibitor contained in an ingestible device, wherein the ingestible device comprises:

a detector configured to detect the location of the device within the gastrointestinal tract, and
a controller or processor configured to trigger the release of the JAK inhibitor in the cecum in response to the detector detecting a location of the device in the cecum.

[0022] Provided herein is a method of releasing a JAK inhibitor into the cecum of a subject for treating one or more sites of disease within the colon, the method comprising:

administering to the subject a therapeutically effective amount of the JAK inhibitor contained in an ingestible device;
receiving at an external receiver from the device a signal transmitting environmental data;
assessing the environmental data to confirm the presence of the one or more sites of disease; and
when the presence of the one or more sites of disease is confirmed, sending from an external transmitter to the device a signal triggering the release of the JAK inhibitor in the cecum.

[0023] Provided herein is a method of releasing an JAK inhibitor into the cecum of a subject for treating one or more sites of disease within the colon, the method comprising:

administering to the subject a therapeutically effective amount of the JAK inhibitor contained in an ingestible device;
receiving at an external receiver from the device a signal transmitting environmental or optical data;
assessing the environmental or optical data to confirm the location of the device within the gastrointestinal tract; and
when the location of the device is confirmed, sending from an external transmitter to the device a signal triggering the release of the JAK inhibitor.

[0024] Provided herein is a method of treating a disease of the gastrointestinal tract in a subject, comprising: delivering a JAK inhibitor to the cecum of the subject, wherein the method comprises administering to the subject a pharmaceutical composition comprising a therapeutically effective amount of the JAK inhibitor.

[0025] Provided herein is a method of treating a disease of the gastrointestinal tract in a subject, comprising: releasing a JAK inhibitor in the cecum of the subject, wherein the method comprises administering to the subject a pharmaceutical composition comprising a therapeutically effective amount of the JAK inhibitor.

[0026] Provided herein in one embodiment is a method of treating a disease of the gastrointestinal tract in a subject, comprising:

releasing a JAK inhibitor in the cecum of the subject wherein the method comprises administering to the subject a pharmaceutical composition comprising a therapeutically effective amount of the JAK inhibitor, wherein the pharmaceu-

tical composition is an ingestible device. and the method comprises administering orally to the subject the pharmaceutical composition.

[0027] Provided herein is a method of treating a disease of the gastrointestinal tract in a subject, comprising: releasing a JAK inhibitor in the cecum of the subject, wherein the method comprises administering to the subject a pharmaceutical composition comprising a therapeutically effective amount of the JAK inhibitor, wherein the method provides a concentration of the JAK inhibitor in the plasma of the subject that is less than 3 µg/ml.

[0028] In another aspect of the present invention, there is provided a JAK inhibitor for use in a method of treating a disease of the gastrointestinal tract in a subject according to claim 1.

[0029] In another aspect, the present disclosure provides a composition comprising or consisting of an ingestible device loaded with a therapeutically effective amount of a JAK inhibitor, for use in a method of treatment, wherein the method comprises orally administering the composition to the subject, wherein the JAK inhibitor is released by the device in the cecum.

[0030] In another aspect, the present disclosure provides an ingestible device loaded with a therapeutically effective amount of a JAK inhibitor, wherein the device is controllable to release the JAK inhibitor in the cecum of the subject. The device may be for use in a method of treatment of the human or animal body, for example, any method as described herein.

[0031] In still another aspect, the present disclosure provides an ingestible device for use in a method of treating a disease of the gastrointestinal tract in a subject, wherein the method comprises orally administering to the subject the ingestible device loaded with a therapeutically effective amount of a JAK inhibitor, wherein the JAK inhibitor is released by the device in the cecum of the subject.

[0032] An ingestible device as used in the present disclosure may comprise one or more mechanical and/or electrical mechanisms which actively control release of the JAK inhibitor. For example, in any of the above aspects and embodiments, the ingestible device as used in the present invention may comprise a release mechanism for release of the JAK inhibitor (e.g., from a reservoir comprising the JAK inhibitor) and an actuator controlling the release mechanism.

[0033] In one disclosure, the ingestible device comprises:

an ingestible housing comprising a reservoir having a therapeutically effective amount of the JAK inhibitor stored therein;

a release mechanism having a closed state which retains the JAK inhibitor in the reservoir and an open state which releases the JAK inhibitor from the reservoir to the exterior of the device; and

an actuator which changes the state of the release mechanism from the closed to the open state.

[0034] In one aspect of the disclosure, the ingestible device comprises

a housing defined by a first end, a second end substantially opposite from the first end;

a reservoir located within the housing and containing the JAK inhibitor wherein a first end of the reservoir is attached to the first end of the housing;

a mechanism for releasing the JAK inhibitor from the reservoir;

and

an exit valve configured to allow the JAK inhibitor to be released out of the housing from the reservoir.

[0035] Here, the exit valve can be considered as the release mechanism having a closed state which retains the JAK inhibitor in the reservoir and an open state which releases the JAK inhibitor from the reservoir to the exterior of the device, and the mechanism for releasing the JAK inhibitor from the reservoir can be considered as the actuator.

[0036] In some disclosures of methods of treatment as described herein, the one or more disease sites may have been pre-determined (e.g., determined in a step preceding the administration of the composition of the present disclosure). The disease site(s) may have been determined by imaging the gastrointestinal tract. For example, the disease site(s) may have been pre-determined by endoscopy (e.g., a step of colonoscopy, enteroscopy, or using a capsule endoscope).

[0037] In some embodiments, the location of the device in the gut may be detected by tracking the device. For example, the device may comprise a localization mechanism which may be a communication system for transmitting localization data, e.g., by radiofrequency transmission. The device may additionally or alternatively comprise a communication system for receiving a signal remotely triggering the actuator and thus causing release of the JAK inhibitor. The signal may be sent when it is determined that the device is in the correct location in the gut.

[0038] Thus, the ingestible device may comprise:

an ingestible housing comprising a reservoir having a therapeutically effective amount of the JAK inhibitor stored therein;

a release mechanism having a closed state which retains the JAK inhibitor in the reservoir and an open state which

releases the JAK inhibitor from the reservoir to the exterior of the device;
 a communication system for transmitting localization data to an external receiver and for receiving a signal from an external transmitter; and
 an actuator which changes the state of the release mechanism from the closed to the open state and which can be triggered by the signal.

[0039] In other embodiments, the ingestible device as used in the present invention may comprise an environmental sensor for detecting the location of the device in the gut. For example, the environment sensor may be an image sensor for obtaining images *in vivo*.

[0040] Where the ingestible device comprises an environmental sensor, actuation of the release mechanism may be triggered by a processor or controller communicably coupled to the environmental sensor. Thus, in some embodiments, the device may not require any external signal or control in order to release the drug.

[0041] The ingestible device comprises:

an ingestible housing comprising a reservoir having a therapeutically effective amount of the JAK inhibitor stored therein;
 a release mechanism having a closed state which retains the JAK inhibitor in the reservoir and an open state which releases the JAK inhibitor from the reservoir to the exterior of the device;
 an actuator which controls the transition of the release mechanism from the closed to the open state;
 a detector for detecting the location of the device in the gut and/or the presence of diseased tissue; and
 a processor or controller which is coupled to the detector and to the actuator and which triggers the actuator to cause the release mechanism to transition from its closed state to its open state to release the anti-JAK inhibitor in the cecum when it is determined that the device is in the cecum of the subject, wherein the site of disease is in the colon.

[0042] In another aspect of the disclosure, there is provided:

an ingestible housing comprising a reservoir having a therapeutically effective amount of the JAK inhibitor stored therein;
 a detector coupled to the ingestible housing, the detector configured to detect a transition of the ingestible device from the ileum to the cecum;
 a valve system in fluid communication with the reservoir system; and
 a controller communicably coupled to the valve system and the detector, the controller configured to cause the valve system to open in response to the detector detecting a transition of the ingestible device from the ileum to the cecum so as to release the therapeutically effective amount of the JAK inhibitor in the cecum.

[0043] As above, detection of a transition from the ileum to the cecum may be based on environmental data indicating the location of the device in the GI tract (and reference to a pre-determined disease site).

[0044] Additionally, or alternatively, the device may further comprise a communication system adapted to transmit the environment data to an external receiver (e.g., outside of the body). This data may be used, for example, for diagnostic purposes. The external receiver may comprise means for displaying the data.

[0045] These data may be analyzed externally to the device and used to determine when the drug should be released: an external signal may then be sent to the device to trigger release of the drug. Thus, the communication system may further be adapted to receive a signal remotely triggering the actuator and thus causing release of the JAK inhibitor. The signal may be sent from an external transmitter in response to receipt/analysis and/or assessment of the environmental data, e.g., data indicating that the device has reached the desired location of the gut (where the location of the diseased tissue has been pre-determined) and/or data indicating the presence of diseased tissue. "External" may be "outside of the body".

[0046] Thus, in another aspect of the disclosure, the ingestible device may comprise:

an ingestible housing comprising a reservoir having a therapeutically effective amount of the JAK inhibitor stored therein;
 a release mechanism having a closed state which retains the JAK inhibitor in the reservoir and an open state which releases the JAK inhibitor from the reservoir to the exterior of the device;
 an environmental detector for detecting environmental data indicating the location of the device in the gut and/or the presence of diseased tissue;
 a communication system for transmitting the environmental data to an external receiver and for receiving a signal from an external transmitter; and
 an actuator which controls the transition of the release mechanism from the closed to the open state in response

to the signal.

[0047] Disclosed herein is a system comprising:

an ingestible device loaded with a therapeutically effective amount of a JAK inhibitor, a release mechanism for release of the JAK inhibitor (e.g., from a reservoir comprising the JAK inhibitor), an actuator controlling the release mechanism, an environmental sensor for determining the location of the device in the gut and a communication system adapted to transmit the environment data and receive a signal triggering the actuator;
a receiver and display module for receiving and displaying outside of the body the environment data from the ingestible device;
a transmitter for sending to the ingestible device a signal triggering the actuator.

[0048] In any of the above disclosures, disease of the GI tract may be an inflammatory bowel disease.

[0049] In some embodiments, the disease of the GI tract is ulcerative colitis.

[0050] In some embodiments, the disease of the GI tract is Crohn's disease.

[0051] In general, apparatuses, compositions, and methods disclosed herein are useful in the treatment of diseases of the gastrointestinal tract. Exemplary gastrointestinal tract diseases that can be treated include, without limitation, inflammatory bowel disease (IBD), Crohn's disease (e.g., active Crohn's disease, refractory Crohn's disease, or fistulizing Crohn's disease), ulcerative colitis, indeterminate colitis, microscopic colitis, infectious colitis, drug or chemical-induced colitis, diverticulitis, and ischemic colitis, gastritis, peptic ulcers, stress ulcers, bleeding ulcers, gastric hyperacidity, dyspepsia, gastroparesis, Zollinger-Ellison syndrome, gastroesophageal reflux disease, short-bowel (anastomosis) syndrome, a hypersecretory state associated with systemic mastocytosis or basophilic leukemia or hyperhistaminemia, Celiac disease (e.g., nontropical Sprue), enteropathy associated with seronegative arthropathies, microscopic colitis, collagenous colitis, eosinophilic gastroenteritis, colitis associated with radiotherapy or chemotherapy, colitis associated with disorders of innate immunity as in leukocyte adhesion deficiency-1, chronic granulomatous disease, food allergies, gastritis, infectious gastritis or enterocolitis (e.g., *Helicobacter pylori*-infected chronic active gastritis), other forms of gastrointestinal inflammation caused by an infectious agent, pseudomembranous colitis, hemorrhagic colitis, hemolytic-uremic syndrome colitis, diversion colitis, irritable bowel syndrome, irritable colon syndrome, and pouchitis.

[0052] In some embodiments, apparatuses, compositions, and methods disclosed herein are for use to treat one gastrointestinal disease. In some embodiments, apparatuses, compositions, and methods disclosed herein are for use to treat more than one gastrointestinal disease. In some embodiments, apparatuses, compositions, and methods disclosed herein are for use to treat multiple gastrointestinal diseases that occur in the same area of the gastrointestinal tract (the colon, or any sub-region thereof). In some disclosures, apparatuses, compositions, and methods disclosed herein are used to treat multiple gastrointestinal diseases that occur in different areas of the gastrointestinal tract. In some disclosures, administration (e.g., local administration to the cecum) of JAK inhibitor is useful in the treatment of gastrointestinal diseases including, but not limited to, inflammatory bowel disease (IBD), ulcerative colitis, Crohn's disease, or any of the other gastrointestinal diseases described herein.

[0053] In some aspects of the disclosures, administration (e.g., local administration to the gastrointestinal tract) of JAK inhibitor is useful in the treatment of gastrointestinal diseases including, but not limited to, inflammatory bowel disease (IBD), ulcerative colitis, Crohn's disease, or any of the other gastrointestinal diseases described herein.

[0054] The features described herein are intended to be freely combinable. For example, any details described herein for methods of treatment apply equally to a JAK inhibitor, composition or ingestible device for use in said treatment. Any details described for a device apply equally to methods of treatment using the device, or to a JAK inhibitor or composition for use in a method of treatment involving the device.

BRIEF DESCRIPTION OF THE DRAWINGS

[0055]

FIG. 1 is a view of an example ingestible device, in accordance with some parts of the disclosure;
FIG. 2 is an exploded view of the ingestible device of FIG. 1, in accordance with some parts of the disclosure;
FIG. 3 is a diagram of an ingestible device during an example transit through a GI tract, in accordance with some parts of the disclosure;
FIG. 4 is a diagram of an ingestible device during an example transit through a jejunum, in accordance with some parts of the disclosure;
FIG. 5 is a flowchart of illustrative steps for determining a location of an ingestible device as it transits through a GI tract, in accordance with some parts of the disclosure;
FIG. 6 is a flowchart of illustrative steps for detecting transitions from a stomach to a duodenum and from a duodenum

back to a stomach, which may be used when determining a location of an ingestible device as it transits through a GI tract, in accordance with some parts of the disclosure;

FIG. 7 is a plot illustrating data collected during an example operation of an ingestible device, which may be used when determining a location of an ingestible device as it transits through a GI tract, in accordance with some parts of the disclosure;

FIG. 8 is another plot illustrating data collected during an example operation of an ingestible device, which may be used when determining a location of an ingestible device as it transits through a GI tract, in accordance with some parts of the disclosure;

FIG. 9 is a flowchart of illustrative steps for detecting a transition from a duodenum to a jejunum, which may be used when determining a location of an ingestible device as it transits through a GI tract, in accordance with some parts of the disclosure;

FIG. 10 is a plot illustrating data collected during an example operation of an ingestible device, which may be used when detecting a transition from a duodenum to a jejunum, in accordance with some parts of the disclosure;

FIG. 11 is a plot illustrating muscle contractions detected by an ingestible device over time, which may be used when determining a location of an ingestible device as it transits through a GI tract, in accordance with some parts of the disclosure;

FIG. 12 is a flowchart of illustrative steps for detecting a transition from a jejunum to an ileum, which may be used when determining a location of an ingestible device as it transits through a GI tract, in accordance with some parts of the disclosure;

FIG. 13 is a flowchart of illustrative steps for detecting a transition from a jejunum to an ileum, which may be used when determining a location of an ingestible device as it transits through a GI tract, in accordance with some parts of the disclosure;

FIG. 14 is a flowchart of illustrative steps for detecting a transition from an ileum to a cecum, which may be used when determining a location of an ingestible device as it transits through a GI tract, in accordance with some parts of the disclosure;

FIG. 15 is a flowchart of illustrative steps for detecting a transition from a cecum to a colon, which may be used when determining a location of an ingestible device as it transits through a GI tract, in accordance with some parts of the disclosure;

FIG. 16 illustrates an ingestible device for delivering a substance in the GI tract;

FIG. 17 illustrates aspects of a mechanism for an ingestible device with a gas generating cell configured to generate a gas to dispense a substance;

FIG. 18 illustrates an ingestible device having a piston to push for drug delivery;

FIG. 19 illustrates an ingestible device having a bellows structure for a storage reservoir of dispensable substances;

FIG. 20 illustrates an ingestible device having a flexible diaphragm to deform for drug delivery;

FIG. 21 shows an illustrative part of an ingestible device with multiple openings in the housing;

FIG. 22 shows a highly cross-section of an ingestible device including a valve system and a sampling system;

FIG. 23 illustrates a valve system;

FIGs. 24A and 24B illustrate a portion of a two-stage valve system in its first and second stages, respectively;

FIGs. 25A and 25B illustrate a portion of a two-stage valve system in its first and second stages, respectively;

FIGs. 26A and 26B illustrate a portion of a two-stage valve system in its first and second stages, respectively;

FIG. 27 illustrates a more detailed view of an ingestible device including a valve system and a sampling system;

FIG. 28 illustrates a portion of an ingestible device including a sampling system and a two-stage valve system in its second stage; and

FIG. 29 is a highly schematic illustrate of an ingestible device.

FIG. 30 is a graph showing the percentage (%) change in body weight at day 14 (\pm SEM) for DSS mice treated with anti-IL-12 p40 antibody intraperitoneally (10 mg/kg) every third day (Q3D) or intracecally (10 mg/kg or 1 mg/kg) daily (QD), when compared to mice treated with anti-IL-12 p40 antibody intraperitoneally (10 mg/kg) every third day (Q3D) and vehicle control (Vehicle). Mann-Whitney's U-test and Student's t-test were used for statistical analysis on non-Gaussian and Gaussian data respectively. A value of $p < 0.05$ was considered significant (Graph Pad Software, Inc.).

FIG. 31 is a graph showing the concentration of anti-IL-12 p40 rat IgG2A (μ g/mL) in plasma of anti-IL-12 p40 intraperitoneally (10 mg/kg) and intracecally (10 mg/kg and 1 mg/kg) administered treatment groups given daily (QD) or every third day (Q3D) when compared to vehicle control (Vehicle) and when IP is compared to IC. ELISA analysis was used to determine the concentration of anti-IL-12 p40 (IgG2A). Data presented as mean \pm SEM. Mann-Whitney's U-test and Student's t-test were used for statistical analysis on non-Gaussian and Gaussian data respectively. A value of $p < 0.05$ was considered significant (Graph Pad Software, Inc.).

FIG. 32 is a graph showing the concentration of anti-IL-12 p40 antibody (IgG2A) (μ g/mL) in the cecum and colon content of anti-IL-12 p40 antibody intraperitoneally (10 mg/kg) and intracecally (10 mg/kg and 1 mg/kg) administered treatment groups given daily (QD) or every third day (Q3D), when compared to vehicle control (Vehicle) and when

IP is compared to IC. ELISA analysis was used to determine the concentration of rat IgG2A. Data presented as mean \pm SEM. Mann-Whitney's U- test and Student's t-test were used for statistical analysis on non-Gaussian and Gaussian data respectively. A value of $p < 0.05$ was considered significant (Graph Pad Software, Inc.).

FIG. 33 is a graph showing the mean overall tissue immunolabel scores (intensity and extent) in acute DSS colitis mouse colon of anti-IL-12 p40 antibody intracecally-treated versus vehicle control-treated DSS mice. Data presented as mean \pm SEM.

FIG. 34 is a graph showing the mean location-specific immunolabel scores in acute DSS colitis mouse colon of anti-IL-12 p40 intracecally-treated versus vehicle control-treated DSS mice. Data presented as mean \pm SEM. Mann-Whitney's U- test and Student's t-test were used for statistical analysis on non-Gaussian and Gaussian data respectively. A value of $p < 0.05$ was considered significant (Graph Pad Software, Inc.).

FIG. 35 is a graph showing the ratio of anti-IL-12 p40 antibody in the colon tissue to the plasma concentration of the anti-IL-12 p40 antibody in mice treated with the anti-IL-12 p40 antibody on day 0 (Q0) or day 3 (Q3D) of the study, when measured at the same time point after the initial dosing. An outlier animal was removed from Group 5.

FIG. 36 is a graph showing the concentration of IL-1 β ($\mu\text{g/mL}$) in colon tissue lysate of acute DSS colitis mice treated with anti-IL-12 p40 intraperitoneally (10 mg/kg) every third day (Q3D) or intracecally (10 mg/kg or 1 mg/kg) administered daily (QD), when compared to vehicle control (Vehicle). Data presented as mean \pm SEM. Mann-Whitney's U- test and Student's t-test were used for statistical analysis on non-Gaussian and Gaussian data respectively. A value of $p < 0.05$ was considered significant (Graph Pad Software, Inc.).

FIG. 37 is a graph showing the concentration of IL-6 ($\mu\text{g/mL}$) in colon tissue lysate of acute DSS colitis mice treated with anti-IL-12 p40 intraperitoneally (10 mg/kg) every third day (Q3D) or intracecally (10 mg/kg or 1 mg/kg) administered daily (QD), when compared to vehicle control (Vehicle). Data presented as mean \pm SEM. Mann-Whitney's U- test and Student's t-test were used for statistical analysis on non-Gaussian and Gaussian data respectively. A value of $p < 0.05$ was considered significant (Graph Pad Software, Inc.).

FIG. 38 is a graph showing the concentration of IL-17A ($\mu\text{g/mL}$) in colon tissue lysate of acute DSS colitis mice treated with anti-IL-12 p40 intraperitoneally (10 mg/kg) every third day (Q3D) or intracecally (10 mg/kg and 1 mg/kg) administered daily (QD), when compared to vehicle control (Vehicle). Data presented as mean \pm SEM. Mann-Whitney's U- test and Student's t-test were used for statistical analysis on non-Gaussian and Gaussian data respectively. A value of $p < 0.05$ was considered significant (Graph Pad Software, Inc.).

FIG. 39 is a graph showing the percentage (%) change in body weight at day 14 (\pm SEM) for DSS mice treated with DATK32 (anti- $\alpha 4\beta 7$ antibody intraperitoneally (25 mg/kg) every third day (Q3D) or intracecally (25 mg/kg or 5 mg/kg) administered daily (QD), when compared to vehicle control (Vehicle) and when IC is compared to IP. Data presented as mean \pm SEM. Mann-Whitney's U- test and Student's t-test were used for statistical analysis on non-Gaussian and Gaussian data respectively. A value of $p < 0.05$ was considered significant (Graph Pad Software, Inc.).

FIG. 40 is a graph showing the plasma concentration of DATK32 rat IgG2A ($\mu\text{g/mL}$) of intraperitoneally (25mg/kg) and intracecally (25 mg/kg and 5 mg/kg) administered treatment groups given daily (QD) or every third day (Q3D), where IP is compared to IC. Data presented as mean \pm SEM. Mann-Whitney's U- test and Student's t-test were used for statistical analysis on non-Gaussian and Gaussian data respectively. A value of $p < 0.05$ was considered significant (Graph Pad Software, Inc.).

FIG. 41 is a graph showing the concentration of DATK32 rat IgG2A antibody ($\mu\text{g/mL}$) in cecum and colon content of intraperitoneally (25mg/kg) or intracecally (25 mg/kg and 5 mg/kg) administered treatment groups given daily (QD) or every third day (Q3D), where IP is compared to IC. Data presented as mean \pm SEM. Mann-Whitney's U- test and Student's t-test were used for statistical analysis on non-Gaussian and Gaussian data respectively. A value of $p < 0.05$ was considered significant (Graph Pad Software, Inc.).

FIG. 42 is a graph showing the concentration of DATK32 rat IgG2A ($\mu\text{g/mL}$) in the colon content of intraperitoneally (25mg/kg) or intracecally (25 mg/kg and 5 mg/kg) administered treatment groups given daily (QD), and concentration over time (1, 2, 4, 24, and 48 hours), where IP is compared to IC. Data presented as mean \pm SEM. Mann-Whitney's U- test and Student's t-test were used for statistical analysis on non-Gaussian and Gaussian data respectively. A value of $p < 0.05$ was considered significant (Graph Pad Software, Inc.).

FIG. 43 is a graph showing the concentration of DATK32 rat IgG2A ($\mu\text{g/g}$) in colon tissue of intraperitoneally (25mg/kg) or intracecally (25 mg/kg and 5 mg/kg) administered treatment groups given daily (QD) or every third day (Q3D), where IP is compared to IC. Data presented as mean \pm SEM. Mann-Whitney's U- test and Student's t-test were used for statistical analysis on non-Gaussian and Gaussian data respectively. A value of $p < 0.05$ was considered significant (Graph Pad Software, Inc.).

FIG. 44 is a graph showing the concentration of DATK32 rat IgG2A ($\mu\text{g/g}$) in the colon tissue of intraperitoneally (25mg/kg) or intracecally (25 mg/kg and 5 mg/kg) administered treatment groups given daily (QD), and the concentration over time (1, 2, 4, 24, and 48 hours) was determined, where IP is compared to IC. Data presented as mean \pm SEM. Mann-Whitney's U- test and Student's t-test were used for statistical analysis on non-Gaussian and Gaussian data respectively. A value of $p < 0.05$ was considered significant (Graph Pad Software, Inc.).

FIG. 45 is a graph showing the mean overall tissue immunolabel scores (intensity and extent) in acute DSS colitis mouse colon of DATK32 (anti- $\alpha 4\beta 7$ antibody treated versus vehicle control (Vehicle) treated DSS mice. The data are presented as mean \pm SEM.

FIG. 46 is a graph showing the mean location-specific immunolabel scores in acute DSS colitis mouse colon of DATK32 (anti- $\alpha 4\beta 7$ antibody-treated versus vehicle control (Vehicle)-treated DSS mice. Data presented as mean \pm SEM. Mann-Whitney's U- test and Student's t-test were used for statistical analysis on non-Gaussian and Gaussian data respectively. A value of $p < 0.05$ was considered significant (Graph Pad Software, Inc.).

FIG. 47 is a graph showing the ratio of the DATK-32 antibody in the colon tissue to the plasma concentration of the DATK-32 antibody in mice treated with the DATK-32 antibody on day 0 (Q0) or day 3 (Q3D) of the study (Groups 9-12), when measured after initial dosing.

FIG. 48 is a graph showing the mean percentage of Th memory cells (mean \pm SEM) in blood for DATK32 (anti- $\alpha 4\beta 7$ antibody intraperitoneally (25mg/kg) or intracecally (25 mg/kg or 5 mg/kg) administered treatment groups given daily (QD) or every third day (Q3D), when compared to vehicle control (Vehicle) and when IP is compared to IC. Mean percentage Th memory cells were measured using FACS analysis. Data presented as mean \pm SEM. Mann-Whitney's U- test and Student's t-test were used for statistical analysis on non-Gaussian and Gaussian data respectively. A value of $p < 0.05$ was considered significant (Graph Pad Software, Inc.).

FIG. 49 is an exemplary image of a histological section of a distal transverse colon of Animal 1501 showing no significant lesions (i.e., normal colon).

FIG. 50 is an exemplary image of a histological section of a distal transverse colon of Animal 2501 (treated with TNBS) showing areas of necrosis and inflammation.

FIG. 51 is a representative graph of plasma adalimumab concentrations over time following a single subcutaneous (SQ) or topical administration of adalimumab. The plasma concentrations of adalimumab were determined 6, 12, 24, and 48 hours after administration of adalimumab. N/D = not detectable.

FIG. 52 is a representative table of the plasma adalimumab concentrations ($\mu\text{g/mL}$) as shown in FIG. 4.6.

FIG. 53 is a graph showing the concentration of $\text{TNF}\alpha$ (pg/mL per mg of total protein) in non-inflamed and inflamed colon tissue after intracecal administration of adalimumab, as measured 6, 12, 24, and 24 hours after the initial dosing.

FIG. 54 is a graph showing the concentration of $\text{TNF}\alpha$ (pg/mL per mg of total protein) in colon tissue after subcutaneous or intracecal (topical) administration of adalimumab, as measured 48 hours after the initial dosing.

FIG. 55 is a graph showing the percentage (%) change in body weight at day 14 (\pm SEM) in acute DSS colitis mice treated with cyclosporine A orally (10 mg/kg) every third day (Q3D) or intracecally (10 mg/kg or 3 mg/kg) daily (QD), when compared to vehicle control (Vehicle). Data presented as mean \pm SEM. Mann-Whitney's U- test and Student's t-test were used for statistical analysis on non-Gaussian and Gaussian data respectively. A value of $p < 0.05$ was considered significant (Graph Pad Software, Inc.).

FIG. 56 is a graph showing the plasma cyclosporine A (CsA) (ng/mL) concentration over time (1 h, 2 h, 4 h, and 24 h) in acute DSS colitis mice treated daily (QD) with orally (PO) (10 mg/kg) or intracecally (IC) (10 mg/kg or 3 mg/kg) administered CsA. Data presented as mean \pm SEM.

FIG. 57 is a graph showing the colon tissue cyclosporine A (CsA) (ng/g) concentration over time (1 h, 2 h, 4 h and 24 h) in acute DSS colitis mice treated daily (QD) with orally (PO) (10 mg/kg) or intracecally (IC) (10 mg/kg or 3 mg/kg) administered CsA. Data presented as mean \pm SEM.

FIG. 58 is a graph showing the peak colon tissue cyclosporine A (CsA) (ng/g) concentration in acute DSS colitis mice treated daily (QD) with orally (PO) (10 mg/kg) or intracecally (IC) (10 mg/kg or 3 mg/kg) administered CsA. Data presented as mean \pm SEM.

FIG. 59 is a graph showing the trough tissue concentration of cyclosporine (CsA) (ng/g) in colon of acute DSS colitis mice treated daily (QD) with orally (PO) (10 mg/kg) or intracecally (IC) (10 mg/kg or 3 mg/kg) administered CsA. Data presented as mean \pm SEM.

FIG. 60 is a graph showing the interleukin-2 (IL-2) concentration ($\mu\text{g/mL}$) in colon tissue of acute DSS colitis mice treated daily (QD) with orally (PO) (10 mg/kg) or intracecally (IC) (10 mg/kg or 3 mg/kg) administered CsA, where PO is compared to IC. Data presented as mean \pm SEM. Mann-Whitney's U- test and Student's t-test were used for statistical analysis on non-Gaussian and Gaussian data respectively. A value of $p < 0.05$ was considered significant (Graph Pad Software, Inc.).

FIG. 61 is a graph showing the interleukin-6 (IL-6) concentration ($\mu\text{g/mL}$) in colon tissue of acute DSS colitis mice treated daily (QD) with orally (PO) (10 mg/kg) or intracecally (IC) (10 mg/kg or 3 mg/kg) administered CsA. Data presented as mean \pm SEM.

FIG. 62 illustrates a nonlimiting example of a system for collecting, communicating and/or analyzing data about a subject, using an ingestible device.

FIGs. 63A-F are graphs showing rat IgG2A concentration as measured in (A) colon homogenate, (B) mLN homogenate, (C) small intestine homogenate, (D) cecum contents, (E) colon contents, and (F) plasma by ELISA. Standards were prepared with plasma matrix. Samples were diluted 1:50 before analysis. Sample 20 was removed from cecum

contents analysis graph (outlier). * $p < 0.05$; ** $p < 0.01$; **** $p < 0.001$ were determined using the unpaired t test.

FIG. 64 illustrates a tapered silicon bellows.

FIG. 65 illustrates a tapered silicone bellows in the simulated device jig.

FIG. 66 illustrates a smooth PVC bellows.

FIG. 67 illustrates a smooth PVC bellows in the simulated device jig.

FIG. 68 demonstrates a principle of a competition assay performed in an experiment.

FIG. 69 shows AlphaLISA data.

FIG. 70 shows AlphaLISA data.

FIG. 71 shows AlphaLISA data.

FIG. 72 is a flowchart of illustrative steps of a clinical protocol, in accordance with some parts of the disclosure.

FIG. 73 is a graph showing the level of FAM-SMAD7-AS oligonucleotide in the cecum tissue of DSS-induced colitis mice at 12-hours. The bars represent from left to right, Groups 2 through 5 in the experiment described in Example 9.

FIG. 74 is a graph showing the level of FAM-SMAD7-AS oligonucleotide in the colon tissue of DSS-induced colitis mice at 12-hours. The bars represent from left to right, Groups 2 through 5 in the experiment described in Example 9.

FIG. 75 is a graph showing the level of FAM-SMAD7-AS oligonucleotide in the cecum contents of DSS-induced colitis mice at 12-hours. The bars represent from left to right, Groups 2 through 5 in the experiment described in Example 9.

FIG. 76 is a graph showing the mean concentration of tacrolimus in the cecum tissue and the proximal colon tissue 12 hours after intra-cecal or oral administration of tacrolimus to swine as described in Example 10.

DETAILED DESCRIPTION

[0056] The present disclosure is directed to various methods and formulations for treating diseases of the gastrointestinal tract with a JAK inhibitor. For example, a method of treating a disease of the gastrointestinal tract in a subject comprises administering to the subject a pharmaceutical formulation comprising a JAK inhibitor wherein the pharmaceutical formulation is released in the subject's cecum. For example, the pharmaceutical formulation comprises a therapeutically effective amount of a JAK inhibitor. The formulation is contained in an ingestible device, and the device releases the formulation in the cecum. The location of the site of disease may be predetermined. The release of the formulation may be triggered autonomously, as further described herein.

[0057] The following disclosure illustrates aspects of the formulations and methods embodied in the claims.

Formulations, including Pharmaceutical Formulations

[0058] As used herein, a "formulation" of a JAK inhibitor may refer to either the JAK inhibitor in pure form, such as, for example, a lyophilized JAK inhibitor, or a mixture of the JAK inhibitor with one or more physiologically acceptable carriers, excipients or stabilizers. Thus, therapeutic formulations or medicaments can be prepared by mixing the JAK inhibitor having the desired degree of purity with optional physiologically acceptable carriers, excipients or stabilizers (Remington's Pharmaceutical Sciences 16th edition, Osol, A. Ed. (1980)), in the form of lyophilized formulations or aqueous solutions. Acceptable carriers, excipients, or stabilizers are nontoxic to recipients at the dosages and concentrations employed, and include buffers such as phosphate, citrate, and other organic acids; antioxidants including ascorbic acid and methionine; preservatives (such as octadecyldimethylbenzyl ammonium chloride; hexamethonium chloride; benzalkonium chloride, benzethonium chloride; phenol, butyl or benzyl alcohol; alkyl parabens such as methyl or propyl paraben; catechol; resorcinol; cyclohexanol; 3-pentanol; and m-cresol); low molecular weight (less than about 10 residues) antibody; proteins, such as serum albumin, gelatin, or immunoglobulins; hydrophilic polymers such as polyvinylpyrrolidone; amino acids such as glycine, glutamine, asparagine, histidine, arginine, or lysine; monosaccharides, disaccharides, and other carbohydrates including glucose, mannose, or dextrans; chelating agents such as EDTA; sugars such as sucrose, mannitol, trehalose or sorbitol; salt-forming counter-ions such as sodium; metal complexes (e.g., Zn-protein complexes); and/or nonionic surfactants such as TWEEN™, PLURONICS™ or polyethylene glycol (PEG). Exemplary pharmaceutically acceptable carriers herein further include interstitial drug dispersion agents such as soluble neutral-active hyaluronidase glycoproteins (sHASEGP), for example, human soluble PH-20 hyaluronidase glycoproteins, such as rHuPH20 (HYLENEX®), Baxter International, Inc.). Certain exemplary sHASEGPs and methods of use, including rHuPH20, are described in US Patent Publication Nos. 2005/0260186 and 2006/0104968. In one aspect, a sHASEGP is combined with one or more additional glycosaminoglycanases such as chondroitinases. Exemplary lyophilized formulations are described in US Patent No. 6,267,958. Aqueous formulations include those described in US Patent No. 6,171,586 and WO2006/044908, the latter formulations including a histidine-acetate buffer.

[0059] A formulation of a JAK inhibitor as disclosed herein, e.g., sustained-release formulations, can further include a mucoadhesive agent, e.g., one or more of polyvinyl pyrrolidone, methyl cellulose, sodium carboxyl methyl cellulose, hydroxyl propyl cellulose, carbopol, a polyacrylate, chitosan, a eudragit analogue, a polymer, and a thiomers. Additional

examples of mucoadhesive agents that can be included in a formulation with a JAK inhibitor are described in, e.g., Peppas et al., *Biomaterials* 17(16): 1553-1561, 1996; Kharenko et al., *Pharmaceutical Chemistry J.* 43(4):200-208, 2009; Salamat-Miller et al., *Adv. Drug Deliv. Reviews* 57(11):1666-1691, 2005; Bernkop-Schnurch, *Adv. Drug Deliv. Rev.* 57(11):1569-1582, 2005; and Harding et al., *Biotechnol. Genet. Eng. News* 16(1):41-86, 1999.

[0060] In some embodiments, components of a formulation may include any one of the following components, or any combination thereof:

Acacia, Alginate, Alginic Acid, Aluminum Acetate, an antiseptic, Benzyl Alcohol, Butyl Paraben, Butylated Hydroxy Toluene, an antioxidant, Citric acid, Calcium carbonate, Candelilla wax, a binder, Croscarmellose sodium, Confectioner sugar, Colloidal silicone dioxide, Cellulose, Carnuba wax, Corn starch, Carboxymethylcellulose calcium, Calcium stearate, Calcium disodium EDTA, Chelation agents, Copolyvidone, Castor oil hydrogenated, Calcium hydrogen phosphate dehydrate, Cetylpyridine chloride, Cysteine HCl, Crosspovidone, Dibasic Calcium Phosphate, Disodium hydrogen phosphate, Dimethicone, Erythrosine Sodium, Ethyl Cellulose, Gelatin, Glyceryl monooleate, Glycerin, Glycine, Glyceryl monostearate, Glyceryl behenate, Hydroxy propyl cellulose, Hydroxyl propyl methyl cellulose, Hypromellose, HPMC Pthalate, Iron oxides or ferric oxide, Iron oxide yellow, Iron oxide red or ferric oxide, Lactose (hydrous or anhydrous or monohydrate or spray dried), Magnesium stearate, Microcrystalline cellulose, Mannitol, Methyl cellulose, Magnesium carbonate, Mineral oil, Methacrylic acid copolymer, Magnesium oxide, Methyl paraben, PEG, Polysorbate 80, Propylene glycol, Polyethylene oxide, Propylene paraben, Polaxamer 407 or 188 or plain, Potassium bicarbonate, Potassium sorbate, Potato starch, Phosphoric acid, Polyoxy140 stearate, Sodium starch glycolate, Starch pregelatinized, Sodium crossmellose, Sodium lauryl sulfate, Starch, Silicon dioxide, Sodium benzoate, Stearic acid, Sucrose base for medicated confectionery, a granulating agent, Sorbic acid, Sodium carbonate, Saccharin sodium, Sodium alginate, Silica gel, Sorbiton monooleate, Sodium stearyl fumarate, Sodium chloride, Sodium metabisulfite, Sodium citrate dehydrate, Sodium starch, Sodium carboxy methyl cellulose, Succinic acid, Sodium propionate, Titanium dioxide, Talc, Triacetin, Triethyl citrate.

[0061] Accordingly, in some examples of the method of treating a disease, the method comprises administering to the subject a pharmaceutical composition that is a formulation as disclosed herein. In some cases the formulation is a dosage form, which may be, as an example, a solid form such as, for example, a capsule, a tablet, a sachet, or a lozenge; or which may be, as an example, a liquid form such as, for example, a solution, a suspension, an emulsion, or a syrup.

[0062] In some embodiments, the formulation is comprised in an ingestible device as defined in claim 1. In some embodiments, the formulation may be suitable for oral administration. The formulation may be, for example, a solid dosage form or a liquid dosage form as disclosed herein. In some embodiments the formulation is suitable for introduction and optionally for storage in the device. In some embodiments the formulation is suitable for introduction and optionally for storage in a reservoir comprised in the device. In some embodiments the formulation is suitable for introduction and optionally for storage in a reservoir comprised in the device. Thus, provided herein is a reservoir comprising a therapeutically effective amount of a JAK inhibitor, wherein the reservoir is configured to fit into an ingestible device. In some disclosures, the reservoir comprising a therapeutically effective amount of an JAK inhibitor is attachable to an ingestible device. In some cases the formulation is suitable for introduction in a spray catheter, as disclosed herein.

[0063] The formulation herein may also contain more than one active compound as necessary for the particular indication being treated, for example, those with complementary activities that do not adversely affect each other. For instance, the formulation may further comprise another JAK inhibitor or a chemotherapeutic agent. Such molecules are suitably present in combination in amounts that are effective for the purpose intended.

[0064] The active ingredients may also be entrapped in microcapsules prepared, for example, by coacervation techniques or by interfacial polymerization, for example, hydroxymethylcellulose or gelatin-microcapsule and poly-(methylmethacrylate) microcapsule, respectively, in colloidal drug delivery systems (for example, liposomes, albumin microspheres, microemulsions, nano-particles and nanocapsules) or in macroemulsions. Such techniques are disclosed in Remington's *Pharmaceutical Sciences* 16th edition, Osol, A. Ed. (1980). The formulations to be used for in vivo administration must be sterile. This is readily accomplished by filtration through sterile filtration membranes. Sustained-release preparations may be prepared. Suitable examples of sustained-release preparations include semipermeable matrices of solid hydrophobic polymers containing the JAK inhibitor, which matrices are in the form of shaped articles, e.g., films, or microcapsule. Examples of sustained-release matrices include polyesters, hydrogels (for example, poly(2-hydroxyethylmethacrylate), or poly(vinylalcohol)), polylactides (U.S. Pat. No. 3,773,919), copolymers of L-glutamic acid and γ ethyl-L-glutamate, non-degradable ethylene-vinyl acetate, degradable lactic acid-glycolic acid copolymers such as the LUPRON DEPOT[™] (injectable microspheres composed of lactic acid-glycolic acid copolymer and leuprolide acetate), and poly-D-(-)-3-hydroxybutyric acid. While polymers such as ethylene-vinyl acetate and lactic acid-glycolic acid enable release of molecules for over 100 days, certain hydrogels release proteins for shorter time periods. When encapsulated JAK inhibitors remain in the body for a long time, they may denature or aggregate as a result of exposure to moisture at 37°C, resulting in a loss of biological activity and possible changes in immunogenicity. Rational strategies can be devised for stabilization depending on the mechanism involved. For example, if the aggregation mechanism is discovered to be intermolecular S-S bond formation through thio-disulfide interchange, stabilization may be achieved by modifying

sulfhydryl residues, lyophilizing from acidic solutions, controlling moisture content, using appropriate additives, and developing specific polymer matrix compositions.

[0065] Pharmaceutical formulations may contain one or more JAK inhibitors. The pharmaceutical formulations may be formulated in any manner known in the art. In some cases the formulations include one or more of the following components: a sterile diluent (e.g., sterile water or saline), a fixed oil, polyethylene glycol, glycerin, propylene glycol, or other synthetic solvents, antibacterial or antifungal agents, such as benzyl alcohol or methyl parabens, chlorobutanol, phenol, ascorbic acid, thimerosal, and the like, antioxidants, such as ascorbic acid or sodium bisulfite, chelating agents, such as ethylenediaminetetraacetic acid, buffers, such as acetates, citrates, or phosphates, and isotonic agents, such as sugars (e.g., dextrose), polyalcohols (e.g., mannitol or sorbitol), or salts (e.g., sodium chloride), or any combination thereof. Liposomal suspensions can also be used as pharmaceutically acceptable carriers (see, e.g., U.S. Patent No. 4,522,811). The formulations can be formulated and enclosed in ampules, disposable syringes, or multiple dose vials. Where required, proper fluidity can be maintained by, for example, the use of a coating, such as lecithin, or a surfactant. Controlled release of the JAK inhibitor can be achieved by implants and microencapsulated delivery systems, which can include biodegradable, biocompatible polymers (e.g., ethylene vinyl acetate, polyanhydrides, polyglycolic acid, collagen, polyorthoesters, and polylactic acid; Alza Corporation and Nova Pharmaceutical, Inc.).

[0066] In some embodiments, the JAK inhibitor is present in a pharmaceutical formulation within the device.

[0067] In some embodiments, the JAK inhibitor is present in solution within the device.

[0068] In some embodiments, the JAK inhibitor is present in a suspension in a liquid medium within the device.

[0069] In some embodiments, the JAK inhibitor is present as a pure, powder (e.g., lyophilized) form of the JAK inhibitor.

Definitions:

[0070] By "ingestible", it is meant that the device can be swallowed whole.

[0071] "Gastrointestinal inflammatory disorders" are a group of chronic disorders that cause inflammation and/or ulceration in the mucous membrane. These disorders include, for example, inflammatory bowel disease (e.g., Crohn's disease, ulcerative colitis, indeterminate colitis and infectious colitis), mucositis (e.g., oral mucositis, gastrointestinal mucositis, nasal mucositis and proctitis), necrotizing enterocolitis and esophagitis. "Inflammatory Bowel Disease" or "IBD" is a chronic inflammatory autoimmune condition of the gastrointestinal (GI) tract. The GI tract can be divided into four main different sections, the oesophagus, stomach, small intestine and large intestine or colon. The small intestine possesses three main subcompartments: the duodenum, jejunum and ileum. Similarly, the large intestine consists of six sections: the cecum, ascending colon, transverse colon, ascending colon, sigmoid colon, and the rectum. The small intestine is about 6 m long, its diameter is 2.5 to 3 cm and the transit time through it is typically 3 hours. The duodenum has a C-shape, and is 30 cm long. Due to its direct connection with the stomach, it is physically more stable than the jejunum and ileum, which are sections that can freely move. The jejunum is 2.4 m in length and the ileum is 3.6 m in length and their surface areas are 180 m² and 280 m² respectively. The large intestine is 1.5 m long, its diameter is between 6.3 and 6.5 cm, the transit time through this section is 20 hours and has a reduced surface area of approximately 150 m². The higher surface area of the small intestine enhances its capacity for systemic drug absorption. The etiology of IBD is complex, and many aspects of the pathogenesis remain unclear. The treatment of moderate to severe IBD poses significant challenges to treating physicians, because conventional therapy with corticosteroids and immunomodulator therapy (e.g., azathioprine, 6 mercaptopurine, and methotrexate administered via traditional routes such as tablet form, oral suspension, or intravenously) is associated with side effects and intolerance and has not shown proven benefit in maintenance therapy (steroids). Monoclonal antibodies targeting tumor necrosis factor alpha (TNF- α), such as infliximab (a chimeric antibody) and adalimumab (a fully human antibody), are currently used in the management of CD. Infliximab has also shown efficacy and has been approved for use in UC. However, approximately 10%-20% of patients with CD are primary nonresponders to anti TNF therapy, and another -20%-30% of CD patients lose response over time (Schnitzler et al., Gut 58:492-500 (2009)). Other adverse events (AEs) associated with anti TNFs include elevated rates of bacterial infection, including tuberculosis, and, more rarely, lymphoma and demyelination (Chang et al., Nat Clin Pract Gastroenterol Hepatology 3:220 (2006); Hoentjen et al., World J. Gastroenterol. 15(17):2067 (2009)). No currently available therapy achieves sustained remission in more than 20%-30% of IBD patients with chronic disease (Hanauer et al, Lancet 359: 1541-49 (2002); Sandborn et al, N Engl J Med 353: 1912-25 (2005)). In addition, most patients do not achieve sustained steroid-free remission and mucosal healing, clinical outcomes that correlate with true disease modification.

[0072] Although the cause of IBD remains unknown, several factors such as genetic, infectious and immunologic susceptibility have been implicated. IBD is much more common in Caucasians, especially those of Jewish descent. The chronic inflammatory nature of the condition has prompted an intense search for a possible infectious cause. Although agents have been found which stimulate acute inflammation, none has been found to cause the chronic inflammation associated with IBD. The hypothesis that IBD is an autoimmune disease is supported by the previously mentioned extraintestinal manifestation of IBD as joint arthritis, and the known positive response to IBD by treatment with therapeutic

agents such as adrenal glucocorticoids, cyclosporine and azathioprine, which are known to suppress immune response. In addition, the GI tract, more than any other organ of the body, is continuously exposed to potential antigenic substances such as proteins from food, bacterial byproducts (LPS), etc.

[0073] A chronic inflammatory autoimmune condition of the gastrointestinal (GI) tract presents clinically as either ulcerative colitis (UC) or Crohn's disease (CD). Both IBD conditions are associated with an increased risk for malignancy of the GI tract.

[0074] "Crohn's disease" ("CD") is a chronic transmural inflammatory disease with the potential to affect any part of the entire GI tract, and UC is a mucosal inflammation of the colon. Both conditions are characterized clinically by frequent bowel motions, malnutrition, and dehydration, with disruption in the activities of daily living. CD is frequently complicated by the development of malabsorption, strictures, and fistulae and may require repeated surgery. UC, less frequently, may be complicated by severe bloody diarrhea and toxic megacolon, also requiring surgery. The most prominent feature Crohn's disease is the granular, reddish-purple edematous thickening of the bowel wall. With the development of inflammation, these granulomas often lose their circumscribed borders and integrate with the surrounding tissue. Diarrhea and obstruction of the bowel are the predominant clinical features. As with ulcerative colitis, the course of Crohn's disease may be continuous or relapsing, mild or severe, but unlike ulcerative colitis, Crohn's disease is not curable by resection of the involved segment of bowel. Most patients with Crohn's disease require surgery at some point, but subsequent relapse is common and continuous medical treatment is usual. Crohn's disease may involve any part of the alimentary tract from the mouth to the anus, although typically it appears in the ileocolic, small-intestinal or colonic-anorectal regions. Histopathologically, the disease manifests by discontinuous granulomatous, crypt abscesses, fissures and aphthous ulcers. The inflammatory infiltrate is mixed, consisting of lymphocytes (both T and B cells), plasma cells, macrophages, and neutrophils. There is a disproportionate increase in IgM- and IgG-secreting plasma cells, macrophages and neutrophils. To date, the primary outcome measure in Crohn's Disease clinical trials is the Crohn's Disease Activity Index (CDAI), which has served as the basis for approval of multiple drug treatments, including for example, vedolizumab and natalizumab. The CDAI was developed by regressing clinician global assessment of disease activity on eighteen potential items representing patient reported outcomes (PROs) (i.e. abdominal pain, pain awakening patient from sleep, appetite), physical signs (i.e. average daily temperature, abdominal mass), medication use (i.e. loperamide or opiate use for diarrhea) and a laboratory test (i.e. hematocrit). Backward stepwise regression analysis identified eight independent predictors which are the number of liquid or soft stools, severity of abdominal pain, general well-being, occurrence of extra-intestinal symptoms, need for anti diarrheal drugs, presence of an abdominal mass, hematocrit, and body weight. The final score is a composite of these eight items, adjusted using regression coefficients and standardization to construct an overall CDAI score, ranging from 0 to 600 with higher score indicating greater disease activity. Widely used benchmarks are: CDAI <150 is defined as clinical remission, 150 to 219 is defined as mildly active disease, 220 to 450 is defined as moderately active disease, and above 450 is defined as very severe disease (Best WR, et al., *Gastroenterology* 77:843-6, 1979). Vedolizumab and natalizumab have been approved on the basis of demonstrated clinical remission, i.e. CDAI < 150.

[0075] Although the CDAI has been in use for over 40 years, and has served as the basis for drug approval, it has several limitations as an outcome measure for clinical trials. For example, most of the overall score comes from the patient diary card items (pain, number of liquid bowel movements, and general well-being), which are vaguely defined and not standardized terms (Sandler et al., *J. Clin. Epidemiol* 41 :451-8, 1988; Thia et al., *Inflamm Bowel Dis* 17: 105-11, 2011). In addition, measurement of pain is based on a four- point scale rather than an updated seven-point scale. The remaining 5 index items contribute very little to identifying an efficacy signal and may be a source of measurement noise. Furthermore, concerns have been raised about poor criterion validity for the CDAI, a reported lack of correlation between the CDAI and endoscopic measures of inflammation (which may render the CDAI as a poor discriminator of active CD and irritable bowel syndrome) and high reported placebo rates (Korzenik et al., *N Engl J Med.* 352:2193-201, 2005; Sandborn WJ, et al., *N Engl J Med* 353 : 1912-25, 2005; Sandborn WJ, et al., *Ann Intern* 19; 146:829-38, 2007, Epub 2007 Apr 30; Kim et al., *Gastroenterology* 146: (5 supplement 1) S-368, 2014). It is, thus, generally recognized that additional or alternative measures of CD symptoms are needed, such as new PRO tools or adaptations of the CDAI to derive a new PRO. The PRO2 and PRO3 tools are such adaptations of the CDAI and have been recently described in Khanna et al., *Aliment Pharmacol. Ther.* 41: 77-86, 2015. The PRO2 evaluates the frequency of loose/liquid stools and abdominal pain {Id}. These items are derived and weighted accordingly from the CDAI and are the CDAI diary card items, along with general well-being, that contribute most to the observed clinical benefit measured by CDAI (Sandler et al., *J. Clin. Epidemiol* 41 :451-8, 1988; Thia et al., *Inflamm Bowel Dis* 17: 105-11, 2011; Kim et al., *Gastroenterology* 146: (5 supplement 1) S-368, 2014). The remission score of < 11 is the CDAI-weighted sum of the average stool frequency and pain scores in a 7-day period, which yielded optimum sensitivity and specificity for identification of CDAI remission (score of < 150) in a retrospective data analysis of ustekinumab induction treatment for moderate to severe CD in a Phase II clinical study (Gasink C, et al., abstract, ACG Annual Meeting 2014). The PRO2 was shown to be sensitive and responsive when used as a continuous outcome measure in a retrospective data analysis of MTX treatment in active CD (Khanna R, et al., *Inflamm Bowel Dis* 20: 1850-61, 2014) measured by CDAI. Additional outcome measures include

the Mayo Clinic Score, the Crohn disease endoscopic index of severity (CDEIS), and the Ulcerative colitis endoscopic index of severity (UCEIS). Additional outcome measures include Clinical remission, Mucosal healing, Histological healing (transmural), MRI or ultrasound for measurement or evaluation of bowel wall thickness, abscesses, fistula and histology.

[0076] An additional means of assessing the extent and severity of Crohn's Disease is endoscopy. Endoscopic lesions typical of Crohn's disease have been described in numerous studies and include, e.g., aphthoid ulcerations, "punched-out ulcers," cobblestoning and stenosis. Endoscopic evaluation of such lesions was used to develop the first validated endoscopic score, the Crohn's Disease Endoscopic Index of Severity (CDEIS) (Mary et al., Gut 39:983-9, 1989). More recently, because the CDEIS is time-consuming, complicated and impractical for routine use, a Simplified Endoscopic Activity Score for Crohn's Disease (SES- CD) was developed and validated (Daperno et al., Gastrointest. Endosc. 60(4):505-12, 2004). The SES-CD consists of four endoscopic variables (size of ulcers, proportion of surface covered by ulcers, proportion of surface with any other lesions (e.g., inflammation), and presence of narrowings[stenosis]) that are scored in five ileocolonic segments, with each variable, or assessment, rated from 0 to 3.

[0077] To date, there is no cure for CD. Accordingly, the current treatment goals for CD are to induce and maintain symptom improvement, induce mucosal healing, avoid surgery, and improve quality of life (Lichtenstein GR, et al., Am J Gastroenterol 104:465-83, 2009; Van Assche G, et al., J Crohns Colitis. 4:63-101, 2010). The current therapy of IBD usually involves the administration of antiinflammatory or immunosuppressive agents, such as sulfasalazine, corticosteroids, 6- mercaptopurine/azathioprine, or cyclosporine, all of which are not typically delivered by localized release of a drug at the site or location of disease. More recently, biologics like TNF-alpha inhibitors and IL-12/IL-23 blockers, are used to treat IBD. If anti-inflammatory/immunosuppressive/biologic therapies fail, colectomies are the last line of defense. The typical operation for CD not involving the rectum is resection (removal of a diseased segment of bowel) and anastomosis (reconnection) without an ostomy. Sections of the small or large intestine may be removed. About 30% of CD patients will need surgery within the first year after diagnosis. In the subsequent years, the rate is about 5% per year. Unfortunately, CD is characterized by a high rate of recurrence; about 5% of patients need a second surgery each year after initial surgery.

[0078] Refining a diagnosis of inflammatory bowel disease involves evaluating the progression status of the diseases using standard classification criteria. The classification systems used in IBD include the Truelove and Witts Index (Truelove S. C. and Witts, L.J. Br Med J. 1955;2: 1041-1048), which classifies colitis as mild, moderate, or severe, as well as Lennard- Jones. (Lennard-Jones JE. Scand J Gastroenterol Suppl 1989; 170:2-6) and the simple clinical colitis activity index (SCCAI). (Walmsley et. al. Gut. 1998;43:29-32) These systems track such variables as daily bowel movements, rectal bleeding, temperature, heart rate, hemoglobin levels, erythrocyte sedimentation rate, weight, hematocrit score, and the level of serum albumin.

[0079] There is sufficient overlap in the diagnostic criteria for UC and CD that it is sometimes impossible to say which a given patient has; however, the type of lesion typically seen is different, as is the localization. UC mostly appears in the colon, proximal to the rectum, and the characteristic lesion is a superficial ulcer of the mucosa; CD can appear anywhere in the bowel, with occasional involvement of stomach, esophagus and duodenum, and the lesions are usually described as extensive linear fissures.

[0080] In approximately 10-15% of cases, a definitive diagnosis of ulcerative colitis or Crohn's disease cannot be made and such cases are often referred to as "indeterminate colitis." Two antibody detection tests are available that can help the diagnosis, each of which assays for antibodies in the blood. The antibodies are "perinuclear anti-neutrophil antibody" (pANCA) and "anti-Saccharomyces cerevisiae antibody" (ASCA). Most patients with ulcerative colitis have the pANCA antibody but not the ASCA antibody, while most patients with Crohn's disease have the ASCA antibody but not the pANCA antibody. However, these two tests have shortcomings as some patients have neither antibody and some Crohn's disease patients may have only the pANCA antibody. A third test, which measures the presence and accumulation of circulating anti-microbial antibodies - particularly flagellin antibodies, has proven to be useful for detecting susceptibility to Crohn's Disease before disease development. See Choung, R. S., et al. "Serologic microbial associated markers can predict Crohn's disease behaviour years before disease diagnosis." Alimentary pharmacology & therapeutics 43.12 (2016): 1300-1310.

[0081] "Ulcerative colitis (UC)" afflicts the large intestine. The course of the disease may be continuous or relapsing, mild or severe. The earliest lesion is an inflammatory infiltration with abscess formation at the base of the crypts of Lieberkuhn. Coalescence of these distended and ruptured crypts tends to separate the overlying mucosa from its blood supply, leading to ulceration. Symptoms of the disease include cramping, lower abdominal pain, rectal bleeding, and frequent, loose discharges consisting mainly of blood, pus and mucus with scanty fecal particles. A total colectomy may be required for acute, severe or chronic, unremitting ulcerative colitis.

[0082] The clinical features of UC are highly variable, and the onset may be insidious or abrupt, and may include diarrhea, tenesmus and relapsing rectal bleeding. With fulminant involvement of the entire colon, toxic megacolon, a life-threatening emergency, may occur. Extraintestinal manifestations include arthritis, pyoderma gangrenosum, uveitis, and erythema nodosum.

[0083] The terms "antibody" and "immunoglobulin" are used interchangeably in the broadest sense and include mon-

oclonal antibodies (for example, full length or intact monoclonal antibodies), polyclonal antibodies, multivalent antibodies, multispecific antibodies (e.g., bispecific, trispecific etc. antibodies so long as they exhibit the desired biological activity) and may also include certain antibody fragments (as described in greater detail herein). An antibody can be human, humanized and/or affinity matured.

[0084] "Antibody fragments" comprise only a portion of an intact antibody, where in certain embodiments, the portion retains at least one, and typically most or all, of the functions normally associated with that portion when present in an intact antibody. In one embodiment, an antibody fragment comprises an antigen binding site of the intact antibody and thus retains the ability to bind antigen. In another embodiment, an antibody fragment, for example one that comprises the Fc region, retains at least one of the biological functions normally associated with the Fc region when present in an intact antibody, such as FcRn binding, antibody half-life modulation, ADCC function and complement binding. In one embodiment, an antibody fragment is a monovalent antibody that has an in vivo half-life substantially similar to an intact antibody. For example, such an antibody fragment may comprise an antigen binding arm linked to an Fc sequence capable of conferring in vivo stability to the fragment.

[0085] The term "monoclonal antibody" as used herein refers to an antibody obtained from a population of substantially homogeneous antibodies, i.e., the individual antibodies comprising the population are identical except for possible naturally occurring mutations that may be present in minor amounts. Monoclonal antibodies are highly specific, being directed against a single antigen. Furthermore, in contrast to polyclonal antibody preparations that typically include different antibodies directed against different determinants (epitopes), each monoclonal antibody is directed against a single determinant on the antigen.

[0086] The monoclonal antibodies herein specifically include "chimeric" antibodies in which a portion of the heavy and/or light chain is identical with or homologous to corresponding sequences in antibodies derived from a particular species or belonging to a particular antibody class or subclass, while the remainder of the chain(s) is identical with or homologous to corresponding sequences in antibodies derived from another species or belonging to another antibody class or subclass, as well as fragments of such antibodies, so long as they exhibit the desired biological activity (U.S. Patent No. 4,816,567; and Morrison et al, Proc. Natl. Acad. Sci. USA 81 :6851-6855 (1984)).

[0087] "Treatment regimen" refers to a combination of dosage, frequency of administration, or duration of treatment, with or without addition of a second medication.

[0088] "Effective treatment regimen" refers to a treatment regimen that will offer beneficial response to a patient receiving the treatment.

[0089] "Effective amount" refers to an amount of drug that offers beneficial response to a patient receiving the treatment. For example, an effective amount may be a Human Equivalent Dose (HED).

[0090] "Dispensable", with reference to any substance, refers to any substance that may be released from an ingestible device as disclosed herein, or from a component of the device such as a reservoir. For example, a dispensable substance may be an JAK inhibitor, and/or a formulation comprising an JAK inhibitor.

[0091] "Patient response" or "patient responsiveness" can be assessed using any endpoint indicating a benefit to the patient, including, without limitation, (1) inhibition, to some extent, of disease progression, including slowing down and complete arrest; (2) reduction in the number of disease episodes and/or symptoms; (3) reduction in lesional size; (4) inhibition (i.e., reduction, slowing down or complete stopping) of disease cell infiltration into adjacent peripheral organs and/or tissues; (5) inhibition (i.e., reduction, slowing down or complete stopping) of disease spread; (6) decrease of auto-immune response, which may, but does not have to, result in the regression or ablation of the disease lesion; (7) relief, to some extent, of one or more symptoms associated with the disorder; (8) increase in the length of disease-free presentation following treatment; and/or (9) decreased mortality at a given point of time following treatment. The term "responsiveness" refers to a measurable response, including complete response (CR) and partial response (PR).

[0092] As used herein, "complete response" or "CR" means the disappearance of all signs of inflammation or remission in response to treatment. This does not necessarily mean the disease has been cured.

[0093] "Partial response" or "PR" refers to a decrease of at least 50% in the severity of inflammation, in response to treatment.

[0094] A "beneficial response" of a patient to treatment with a therapeutic agent and similar wording refers to the clinical or therapeutic benefit imparted to a patient at risk for or suffering from a gastrointestinal inflammatory disorder from or as a result of the treatment with the agent. Such benefit includes cellular or biological responses, a complete response, a partial response, a stable disease (without progression or relapse), or a response with a later relapse of the patient from or as a result of the treatment with the agent.

[0095] As used herein, "non-response" or "lack of response" or similar wording means an absence of a complete response, a partial response, or a beneficial response to treatment with a therapeutic agent.

[0096] "A patient maintains responsiveness to a treatment" when the patient's responsiveness does not decrease with time during the course of a treatment.

[0097] A "symptom" of a disease or disorder (e.g., inflammatory bowel disease, e.g., ulcerative colitis or Crohn's disease) is any morbid phenomenon or departure from the normal in structure, function, or sensation, experienced by

a subject and indicative of disease.

Inhibitory Agents of Janus Kinase (JAK) Activity and/or Expression

[0098] The term "JAK inhibitor" refers to an agent which decreases the expression of Janus kinase 1 (JAK1), JAK2, JAK3, or non-receptor protein tyrosine kinase 2 (TYK-2) and/or the kinase activity of at least one of JAK1, JAK2, JAK3, and TYK-2. In some embodiments, the JAK inhibitor decreases the expression of JAK1. In some embodiments, the JAK inhibitor decreases the expression of JAK2. In some embodiments, the JAK inhibitor decreases the expression of JAK3. In some embodiments, the JAK inhibitor decreases the expression of TYK-2.

[0099] In some embodiments, the JAK inhibitor decreases the kinase activity of JAK1. In some embodiments, the JAK inhibitor decreases the kinase activity of JAK2. In some embodiments, the JAK inhibitor decreases the kinase activity of JAK3. In some embodiments, the JAK inhibitor decreases the kinase activity of TYK-2. In some embodiments, the JAK inhibitor decreases the kinase activity of JAK1, JAK2, JAK3, and TYK2. In some embodiments, the JAK inhibitor decreases the kinase activity of two or more (e.g., 3 or 4) of: JAK1, JAK2, JAK3 and TYK2. In some embodiments, the JAK inhibitor decreases the kinase activity of a single JAK isoform (e.g., JAK1, JAK2, JAK3, or TYK2).

[0100] In some embodiments, the JAK inhibitor decreases the kinase activity of JAK1 and JAK2. In some embodiments, the JAK inhibitor decreases the kinase activity of JAK1 and JAK3. In some embodiments, the JAK inhibitor decreases the kinase activity of JAK2 and JAK3. In some embodiments, the JAK inhibitor decreases the kinase activity of JAK1, JAK2 and JAK3.

[0101] In some embodiments, a JAK inhibitory agent is an inhibitory nucleic acid or a small molecule. In some embodiments, the inhibitory nucleic acid is an antisense nucleic acid, a ribozyme, a small interfering RNA, a small hairpin RNA, or a microRNA. Examples of aspects of these different inhibitory nucleic acids are described below. Any of the examples of inhibitory nucleic acids that can decrease expression of a JAK1, JAK2, JAK3, or TYK2 mRNA in a mammalian cell can be synthesized in vitro.

[0102] Inhibitory nucleic acids that can decrease the expression of JAK1, JAK2, JAK3, or TYK2 mRNA expression in a mammalian cell include antisense nucleic acid molecules, i.e., nucleic acid molecules whose nucleotide sequence is complementary to all or part of a JAK1, JAK2, JAK3, or TYK2 mRNA (e.g., complementary to all or a part of any one of SEQ ID NOs: 1-15).

Human JAK1 mRNA Variant 1 (SEQ ID NO: 1)

[0103]

1 ggggccccgac gggaggcggt gcgtcgctga gcgcaggccg cggcggccgc ggagtatcct
 61 ggagctgcag acagtgcggg cctgcgcca gtcccggctg tctcgccgc gacccctct
 121 cagccctggg cgcgcgcacg ctggggcccc gcggggctgg ccgcctagcg agcctgccgg
 181 tcgaccccag ccagcgcagc gacggggcgc tgcctggccc aggcgcacac ggaagtgcgc
 241 ttctctgaag tagctttgga aagtagagaa gaaaatccag ttgcttctt ggagaacact
 301 ggacagctga ataatgcag tatctaaata taaaagagga ctgcaatgcc atggcttct
 361 gtgctaaaat gaggagctcc aagaagactg aggtgaacct ggaggcccct gagccagggg
 421 tggaaagtga ctctatctg tcggacaggg agcccctccg gctgggcagt ggagagtaca
 481 cagcagagga actgtgcac agggctgcac aggcattgcc tatctctct ctttgcaca
 541 acctcttgc cctgtatgac gagaacacca agctctgga tgctccaaat cgcaccatca
 601 ccgttgatga caagatgcc ctccggctcc actaccgat gaggttctat ttaccaatt
 661 ggcatggaac caacgacaat gacagtcag tgtggcgtca ttctcaaag aagcagaaaa
 721 atggctacga gaaaaaaaaag attccagatg caaccctct cttgatgcc agctcactgg
 781 agtatctgtt tgctcaggga cagtatgatt tggtgaaatg cctggctcct atcgagacc
 841 ccaagaccga gcaggatgga catgatattg agaacgagtg tctagggatg gctgtcctgg
 901 ccatctcaca ctatgccatg atgaagaaga tgcagttgcc agaactgccc aaggacatca
 961 gctacaagcg atatattcca gaaacattga ataagtccat cagacagagg aaccttctca
 1021 ccaggatgag gataaataat gtttcaagg atttctaaa ggaatttaac aacaagacca
 1081 tttgtgacag cagcgtgtcc acgcatgacc tgaagggtgaa atacttggct accttgaaa
 1141 ctttgacaaa acattacggg gctgaaatat ttgagacttc catgttactg attcatcag
 1201 aaaatgagat gaattggtt cattcgaatg acggtggaaa cgttctctac tacgaagtga
 1261 tggtgactgg gaatcttga atccagtga ggcataaacc aaatgttgt tctgttga
 1321 aggaaaaaaaa taaactgaag cggaaaaaac tggaaaataa acacaagaag gatgaggaga
 1381 aaaacaagat ccgggaagag tggacaatt ttcttactt cctgaaatc actcacattg
 1441 taataaagga gtctgtggtc agcataaca agcaggacaa caagaaaatg gaactgaagc

1501 tctcttccca cgaggaggcc ttgtccttg tgtccctggt agatggctac ttccggctca
 1561 cagcagatgc ccatcattac ctctgcaccg acgtggcccc cccgttgatc gtccacaaca
 1621 tacagaatgg ctgtcatggt ccaatctgta cagaatacgc catcaataaa ttgcggcaag
 5 1681 aaggaagcga ggaggggatg tacgtgctga ggtggagctg caccgacttt gacaacatcc
 1741 tcatgaccgt cacctgcttt gagaagtctg agcagggtgca ggggtgccag aagcagttca
 1801 agaactttca gatcgagggtg cagaagggcc gctacagtct gcacgggtcg gaccgcagct
 1861 tccccagctt gggagacctc atgagccacc tcaagaagca gatcctgcgc acggataaca
 10 1921 tcagcttcat gctaaaacgc tgctgccagc ccaagccccc agaaatctcc aacctgctgg
 1981 tggctactaa gaaagcccag gagtggcagc ccgtctacc catgagccag ctgagtttcg
 2041 atcggatcct caagaaggat ctggtgcagg gcgagcacct tgggagaggc acgagaacac
 2101 acatctattc tgggacctg atggattaca aggatgacga aggaacttct gaagagaaga
 15 2161 agataaaagt gatctcaaa gtcttagacc ccagccacag ggatatttcc ctggccttct
 2221 tcgaggcagc cagcatgatg agacaggctc ccacaaaaca catcgtgtac ctctatggcg
 2281 tctgtgtccg cgacgtggag aatatcatgg tgggaagagt tgtggaaggg ggtcctctgg
 2341 atcttctcat gcaccgaaa agcgtgtcc ttaccacacc atggaaattc aaagtgcca
 20 2401 aacagctggc cagtgccttg agtacttgg aggataaaga cctggtccat ggaaatgtgt
 2461 gtactaaaaa cctcctcctg gcccgtagg gcacgcacag tgagtgtggc ccattcatca
 2521 agctcagtga ccccggcac cccattacgg tgctgtctag gcaagaatgc attgaacgaa
 2581 tcccatggat tgctcctgag tgtgtgagg actccaagaa cctgagtgtg gctgctgaca
 2641 agtggagctt tgggaaccacg ctctgggaaa tctgtacaa tggcgagatc cccttgaaag
 2701 acaagacgct gattgagaaa gagagattct atgaaagccg gtgcaggcca gtgacaccat
 2761 catgtaagga gctggctgac ctcatgacc gctgcatgaa ctatgacccc aatcagaggc
 2821 ctttctccg agccatcatg agagacatta ataagctga agagcagaat ccagatattg
 30 2881 tttcagaaaa aaaaccagca actgaagtgg accccacaca tttgaaaag cgcttcttaa
 2941 agaggatccg tgacttggga gagggccact ttgggaaggt tgagctctgc aggtatgacc
 3001 ccgaagggga caatacaggg gagcagggtg ctgttaaate tctgaagcct gagagtggag
 3061 gtaaccacat agctgatctg aaaaaggaaa tcgagatctt aaggaacctc tatcatgaga
 3121 acattgtgaa gtacaaagga atctgcacag aagacggagg aatgggtatt aagctcatca
 3181 tgggaattct gccttcggga agccttaagg aatatctcc aaagaataag aacaaaataa
 3241 acctcaaaac gcagctaaaa tatgccgttc agatttgtaa ggggatggac tatttgggtt
 3301 ctcggaataa cgttcaccgg gacttggcag caagaaatgt ccttgtgag agtgaacacc
 3361 aagtgaataa tggagacttc ggtttaacca aagcaattga aaccgataag gagtattaca
 3421 ccgtcaagga tgaccgggac agccctgtgt ttggtatgc tccagaatgt ttaatgcaat
 3481 ctaaatttta tattgcctct gacgtctggt ctttggagt cactctgcat gagctgctga
 3541 cttactgtga ttcatgattc agtccatgg ctttctcct gaaaatgata ggcccaaccc
 3601 atggccagat gacagtcaca agacttgtga atacgttaa agaaggaaaa cgcctgccgt
 3661 gccaccta ctgtccagat gaggtttatc aacttatgag gaaatgctgg gaattccaac
 3721 catccaatcg gacaagcttt cagaacctta tgaaggatt tgaagcactt taaaataag
 3781 aagcatgaat aacatttaaa ttccacagat tatcaagtc ttctctgca acaaatgcc
 3841 aagtcatttt taaaaattt ctaatgaaag aagtttgtgt tctgtccaa aagtcactga
 3901 actcactatt cagtacatat acatgtataa ggcacactgt agtgctta atgtgtaagg
 3961 acttctctt taaatttgg accagtaact tagtgacaca taatgacaac caaatattt
 4021 gaaagcactt aagcactcct cttgtggaa agaataacc accatttcat ctggctagt
 4081 caccatcaca actgcattac caaaagggga ttttgaana cgaggagt accaaaataa

EP 3 554 485 B9

4141 tatctgaaga tgattgcttt tccctgctgc cagctgatct gaaatgtttt gctggcacat
4201 taatcataga taaagaaaga ttgatggact tagccctcaa atttcagtat ctatacagta
4261 ctagaccatg cattcttaaa atattagata ccaggtagta tatattgttt ctgtacaaaa
5 4321 atgactgtat tctctacca gtaggactta aactttgttt ctccagtggc ttagctcctg
4381 ttctttggg tgatcactag caccatttt tgagaaagct ggttctacat ggggggatag
4441 ctgtggaata gataattgc tgcattgtaa ttctcaagaa ctaagcctgt gccagtgcct
10 4501 tctaagcag tataccttta atcagaactc attcccagaa cctggatgct attacacatg
4561 ctttaagaa acgtcaatgt atatectttt ataactctac cactttgggg caagctatct
4621 cagcactggg tttgaatgct gtatgcaacc agtctgaata ccacatacgc tgcactgttc
4681 ttagagggtt tccatactta ccaccgatct acaagggttg atccctgttt ttaccatcaa
15 4741 tcatcacct gtggtgcaac acttgaaaga cccggctaga ggcactatgg acttcaggat
4801 ccactagaca gtttcagtt tgcttgagg tagctgggta atcaaaaatg ttagtcatt
4861 gattcaatgt gaacgattac ggtctttatg accaagagtc tgaaaatctt tttgttatgc
4921 tgtttagtat tcgttgata ttgttacttt tcacctgttg agcccaaatt caggattggt
20 4981 tcagtggcag caatgaagtt gccattaaa ttgttcata gcctacatca ccaaggtctc
5041 tgtgtcaaac ctgtggccac tctatatgca cttgtttac tctttatata aataaatata
5101 ctaaagactt tacatgca

25 Human JAK1 mRNA Variant 2 (SEQ ID NO: 2)

[0104]

30

35

40

45

50

55

1 agaagcggag cgtatacggg ggaggcggga tgcatttctg catcgagcgc acaaagttat
 61 ctaaaacagt tcatgctgct gaaaacctcc ttctggcag atgtccctca accetactgg
 121 tgcctggctt ctgagacaca cgcttctctg aagtagcttt ggaaagtaga gaagaaaatc
 181 cagtttgctt ctgggagAAC actggacagc tgaataaatg cagtatctaa atataaaaga
 241 ggactgcaat gccatggctt tctgtgctaa aatgaggagc tccaagaaga ctgaggtgaa
 301 cctggaggcc cctgagccag gggtggaagt gatcttctat ctgtcggaca gggagcccct
 361 ccgctgggc agtgagagat acacagcaga ggaactgtgc atcagggctg cacaggcatg
 421 ccgtatctct cctcttctg acaacctctt tgcctgtat gacgagaaca ccaagctctg
 481 gtatgtcca aatcgcacca tcaccgtga tgacaagatg tccctccggc tccactaccg
 541 gatgaggttc tatttcacca attggcatgg aaccaacgac aatgagcagt cagtgtggcg
 601 tcatttcca aagaagcaga aaaatggcta cgagaaaaaa aagattccag atgcaacccc
 661 tctccttgat gccagctcac tggagtatct gtttgcctag ggacagtatg atttggtgaa
 721 atgcctggct cctattcgag accccaagac cgagcaggat ggacatgata ttgagaacga
 781 gtgtctaggg atggctgtcc tggccatctc aactatgcc atgatgaaga agatgcagtt
 841 gccagaactg cccaaggaca tcagctacaa gcgatatatt ccagaaacat tgaataagtc
 901 catcagacag aggaaccttc tcaccaggat gcggataaat aatgtttca aggatttctt
 961 aaaggaattt aacaacaaga ccatttgtga cagcagcgtg tccacgcatg acctgaaggt
 1021 gaaatacttg gctaccttgg aaactttgac aaaacattac ggtgctgaaa tatttgagac
 1081 ttccatgtta ctgatttcat cagaaaatga gatgaattgg ttcatcga atgacgggtg
 1141 aaacgttctc tactacgaag tgatgggtgac tgggaatctt ggaatccagt ggaggcataa
 1201 accaaatgtt gtttctgtg aaaaggaaaa aaataaactg aagcggaaaa aactggaaaa
 1261 taaacacaag aaggatgagg agaaaaacaa gatccgggaa gagtggaaca attttctta
 1321 cttccctgaa atcactcaca ttgtaataaa ggagtctgtg gtcagcatta acaagcagga
 1381 caacaagaaa atggaactga agctctcttc ccacgaggag gccttgctct ttgtgtccct
 1441 ggtagatggc tacttccggc tcacagcaga tgcccatcat tacctctgca ccgacgtggc

1501 cccccgttg atcgccaca acatacagaa tggctgtcat ggtccaatct gtacagaata
 1561 cgccatcaat aaattgcggc aagaaggaag cgaggagggg atgtacgtgc tgaggtggag
 1621 ctgcaccgac ttgacaaca tctcatgac cgtcacctgc ttgagaagt ctgagcaggt
 5 1681 gcagggtgcc cagaagcagt tcaagaactt tcagatcgag gtgcagaagg gccgctacag
 1741 tctgcacggt tggaccgca gttccccag cttgggagac ctcagagacc acctcaagaa
 1801 gcagatcctg cgcacggata acatcagctt catgctaaaa cgtgctgcc agcccaagcc
 1861 ccgagaaatc tccaacctgc tgggtggctac taagaaagcc caggagtggc agcccgtcta
 10 1921 ccccatgagc cagctgagtt tcatcggtat cctcaagaag gatctggtgc agggcgagca
 1981 cttggggaga ggcacgagaa cacacatcta ttctgggacc ctgatggatt acaaggatga
 2041 cgaaggaact tctgaagaga agaagataaa agtgatcctc aaagtcttag accccagcca
 2101 caggatatt tccctggcct tcttcgaggc agccagcatg atgagacagg tctcccaca
 15 2161 acacatcgtg tacctctatg gcgtctgtgt ccgcgacgtg gagaatatca tgggtgaaga
 2221 gtttgggaa gggggctcct tggatctctt catgcaccgg aaaagcgtg tcttaccac
 2281 accatggaaa ttcaaagttg ccaaacagct ggccagtgcc ctgagctact tggaggataa
 2341 agacctggc catggaaatg tgtgtactaa aaacctctc ctggcccggt agggcatcga
 20 2401 cagtgagtgt ggccattca tcaagtcag tgaccccggt atccccatta cgggtctgtc
 2461 taggcaagaa tgcattgaac gaatcccatg gattgctctt gagtgtgtt aggactccaa
 2521 gaacctgagt gtggctgctg acaagtggag ctttgaacc acgctctggg aaatctgcta
 2581 caatggcgag atcccctga aagacaagac gctgattgag aaagagagat tctatgaaag
 2641 ccggtgcagg ccagtgcacac catcatgtaa ggagctggct gacctcatga cccgctgcat
 2701 gaactatgac ccaatcaga ggccttctt ccgagccatc atgagagaca ttaataagct
 2761 tgaagagcag aatccagata ttgttcaga aaaaaacca gcaactgaag tggacccac
 2821 acatttgaa aagcgtctc taaagaggat ccgtgacttg ggagagggcc actttgggaa
 30 2881 ggttgagctc tgcaggtatg accccgaagg ggacaatata ggggagcagg tggctgttaa
 2941 atctctgaag cctgagagtg gaggtaacca catagctgat ctgaaaaagg aaatcgagat
 3001 ctaaggaac ctctatcatg agaacattgt gaagtacaaa ggaatctgca cagaagacgg
 3061 aggaaatgg attaaactca tcatggaatt tctgccttcg ggaagccta aggaatatct
 35 3121 tcaaagaat aagaacaaa taaacctcaa acagcagcta aaatatgccg ttcagatttg
 3181 taaggggatg gactatttgg gttctcggca atacgttcac cgggacttgg cagcaagaaa
 3241 tgccttgtt gagagtgaac accaagtga aattggagac ttcggttaa ccaaagcaat
 40 3301 tgaaccgat aaggagtatt acaccgtcaa ggatgaccgg gacagccctg tgttttgta
 3361 tgcctcagaa tgttaaatgc aatctaaatt ttatattgcc tctgacgtc ggtcttttg
 3421 agtcaactct catgagctgc tgacttactg tgattcagat tctagtcca tggctttgtt
 3481 cctgaaaatg ataggcccaa cccatggcca gatgacagtc acaagacttg tgaatacgtt
 45 3541 aaaagaagga aaacgcctgc cgtgccacc taactgtcca gatgaggtt atcaacttat
 3601 gaggaatgc tgggaattcc aaccatcaa tcggacaagc ttcagaacc ttattgaagg
 3661 attgaagca cttttaaata aagaagcatg aataacattt aaattccaca gattatcaag
 3721 tcttctctt gcaacaaatg ccaagtcatt ttttaaaaa ttctaataga aagaagttg
 50 3781 tgttctgtc aaaaagtcac tgaactcata cttcagtaca tatacatgta taaggcacac
 3841 ttagtgctt aatatgtga aggacttctt ctttaattt ggtaccagta acttagtgac
 3901 acataatgac aacaaaata ttgaaagca ctaagcact cctccttctg gaaagaatat
 3961 accaccattt catctggcta gttcaccatc acaactgcat taccaaaagg ggattttga
 55 4021 aaacgaggag ttgacaaaaa taatatctga agatgattgc tttccctgc tgccagctga
 4081 tctgaaatgt ttgctggca cattaatcat agataaagaa agattgatgg acttagccct

EP 3 554 485 B9

4141 caaatccag tatctataca gtactagacc atgcattctt aaaatattag ataccaggta
4201 gtatatattg ttctgtaca aaaatgactg tattctctca ccagtaggac ttaaactttg
4261 ttctccagt ggcttagctc ctgttcttt gggtgatcac tagcacccat ttgtagaaa
5 4321 gctgggtcta catgggggga tagctgtgga atagataatt tgctgcatgt taattctcaa
4381 gaactaagcc tgtgccagtg ctttctaag cagtatacct ttaatcagaa ctcattccca
4441 gaacctggat gctattacac atgcttttaa gaaacgtcaa tgtatatect ttataactc
4501 taccactttg gggcaagcta ttccagcact gggtttgaat gctgtatgca accagtctga
10 4561 ataccacata cgctgcactg ttcttagagg gttccatac ttaccaccga tctacaaggg
4621 ttgatccctg ttttaccat caatcatcac cctgtggtgc aacacttgaa agaccggct
4681 agaggcacta tggacttcag gatccactag acagtttca gtttgcttgg aggtagctgg
15 4741 gtaatcaaaa atgttagtc attgattcaa tgtgaacgat tacggtcttt atgaccaaga
4801 gtctgaaaat cttttgtta tgctgttag tattcgttg atattgttac tttcacctg
4861 ttgagcccaa attcaggatt gggtcagtgg cagcaatgaa gttgccattt aaatttggtc
4921 atagcctaca tcaccaaggt ctctgtgtca aacctgtggc cactctatat gcacttgtt
20 4981 tactctttat acaataaat atactaaaga ctttacatgc a

Human JAK1 mRNA Variant 3 (SEQ ID NO: 3)

[0105]

25

30

35

40

45

50

55

1 atctatcaca tggcagagat agaataaaaa cagaaaaatg gcgacgggtca cgttgtggcg
 61 agccttgctg cgtcattaga taatcctcat gcaaatagcg ggaagaacaa aggaagggga
 121 gcccgggacc cccgggggcg cagcgcttct ctgaagtagc ttggaaagt agagaagaaa
 5 181 atccagtttg cttcttggaag aacactggac agctgaataa atgcagtatc taaatataaa
 241 agaggactgc aatgcatggt ctttctgtgc taaaatgagg agctccaaga agactgaggt
 301 gaacctggag gccctgagc caggggtgga agtgatcttc tatctgtcgg acagggagcc
 10 361 cctccggctg ggcagtggag agtacacagc agaggaactg tgcacaggg ctgcacaggc
 421 atgccgtatc tctctcttt gtcacaacct ctttgcctg tatgacgaga acaccaagct
 481 ctggtatgct ccaaactgca ccatcacctg tgatgacaag atgtccctcc ggctccacta
 541 ccggatgagg ttctatttca ccaattggca tggaaccaac gacaatgagc agtcagtgtg
 15 601 gcgtattct ccaaagaagc agaaaaatgg ctacgagaaa aaaaagattc cagatgcaac
 661 ccctctcctt gatgccagct cactggagta tctgtttgct cagggacagt atgatttgg
 721 gaaatgctg gtcctattc gagaccccaa gaccgagcag gatggacatg atattgagaa
 781 cgagtgtcta gggatggctg tcttgccat ctcacactat gccatgatga agaagatgca
 20 841 gttgccagaa ctgccaagg acatcagcta caagcgatat attccagaaa cattgaataa
 901 gtccatcaga cagaggaacc ttctaccag gatgcggata aataatgttt tcaaggattt
 961 cctaaaggaa ttaacaaca agaccatttg tgacagcagc gtgtccacgc atgacctgaa
 1021 ggtgaaatac ttggctacct tggaacttt gacaaaacat tacggtgctg aaatatttga
 25 1081 gactccatg ttactgattt catcagaaaa tgagatgaat tggtttcatt cgaatgacgg
 1141 tggaacggt cttactacg aagtgatggt gactgggaat cttggaatcc agtggaggca
 1201 taaaccaaat gttgtttctg ttgaaaagga aaaaaataaa ctgaagcggg aaaaactgga
 1261 aaataaacac aagaaggatg aggagaaaaa caagatccgg gaagagtgga acaattttc
 30 1321 ttacttcctt gaaatcactc acattgtaat aaaggagtct gtggtcagca ttaacaagca
 1381 ggacaacaag aaaatggaac tgaagctctc ttcccacgag gaggccttgt ctttgtgtc
 1441 cctggtagat ggctacttcc ggctcacagc agatgcccac cattacctct gcaccgacgt
 35 1501 ggcccccccg ttgatcgtec acaacataca gaatggctgt catggtccaa tctgtacaga
 1561 atacgccatc aataaattgc ggcaagaagg aagcgaggag gggatgtacg tgctgaggtg

1621 gagctgcacc gactttgaca acatcctcat gaccgtcacc tgctttgaga agtctgagca
 1681 ggtgcagggg gcccgaaagc agttcaagaa ctttcagatc gaggtgcaga agggccgcta
 1741 cagtctgcac gggtcggacc gcagcttccc cagcttggga gacctcatga gccacctcaa
 5 1801 gaagcagatc ctgcgcacgg ataacatcag cttcatgcta aaacgctgct gccagcccaa
 1861 gccccgagaa atctccaacc tgctggtggc tactaagaaa gcccaggagt ggcagcccgt
 1921 ctaccccatg agccagctga gtttcgatcg gatacctcaag aaggatctgg tgagggcgga
 1981 gcaccttggg agaggcacga gaacacacat ctattctggg accctgatgg attacaagga
 10 2041 tgacgaagga acttctgaag agaagaagat aaaagtgate ctcaaagtct tagacccag
 2101 ccacagggat atttccctgg cttcttcga ggcagccagc atgatgagac aggtctcca
 2161 caaacacatc gtgtacctct atggcgtctg tgcgcgcgac gtggagaata tcatggtgga
 2221 agagtttgag gaagggggc ctctggatct cttcatgcac cggaaaagcg atgtcctac
 15 2281 cacaccatgg aaattcaag ttgccaaaca gctggccagt gccctgagct acttgaggga
 2341 taaagacctg gtccatggaa atgtgtgtac taaaaacctc ctctggccc gtgagggcat
 2401 cgacagttag tggggccat tcatcaagct cagtgacccc ggcatcccca ttacgggtgct
 2461 gtctaggcaa gaatgcattg aacgaatccc atggattgct cctgagtgtg ttgaggactc
 20 2521 caagaacctg agtgtggctg ctgacaagtg gagctttgga accacgctct gggaaatctg
 2581 ctacaatggc gagatcccct tgaagacaa gacgctgatt gagaaagaga gattctatga
 2641 aagccggtgc aggccagtga caccatcatg taaggagctg gctgacctca tgaccgctg
 2701 catgaactat gacccaatc agaggccttt ctccgagcc atcatgagag acattaataa
 25 2761 gcttgaagag cagaatccag atattgtttc agaaaaaaaa ccagcaactg aagtggaccc
 2821 cacacatttt gaaaagcgtc tcctaaagag gatccgtgac ttgggagagg gccactttgg
 2881 gaaggttgag ctctgcaggt atgacccga aggggacaa acaggggagc aggtggctgt
 2941 taaatctctg aagcctgaga gtggaggtaa ccacatagct gatctgaaaa aggaaatcga
 30 3001 gatcttaagg aacctctatc atgagaacat tgtgaagtac aaaggaatct gcacagaaga
 3061 cggaggaaat ggtattaagc tcatcatgga atttctgcct tcgggaagcc ttaaggaata
 3121 tcttccaaag aataagaaca aaataaacct caaacagcag ctaaaatatg ccgttcagat
 3181 ttgtaagggg atggactatt tgggttctcg gcaatacgtt caccgggact tggcagcaag
 35 3241 aaatgtcctt gttgagagt aacaccaagt gaaaattgga gacttcggtt taaccaaaagc
 3301 aattgaaacc gataaggagt attacaccgt caaggatgac cgggacagcc ctgtgtttg
 3361 gtatgtcca gaatgtttaa tgcaatctaa attttatatt gcctctgacg tctggtcttt
 3421 tggagtact ctgcatgagc tgctgactta ctgtgattca gattctagtc ccatggcttt
 40 3481 gttcctgaaa atgataggcc caacccatgg ccagatgaca gtcacaagac ttgtgaatac
 3541 gttaaaagaa ggaaaacgcc tgccgtgccc acctactgt ccagatgagg ttatcaact
 3601 tatgaggaaa tgctgggaat tccaaccatc caatcggaca agcttcaga acctattga
 45 3661 aggatttgaa gcacttttaa aataagaagc atgaataaca tttaaattcc acagattatc
 3721 aagtccttct cctgcaacaa atgcccagt catttttaa aaatttctaa tgaaagaagt
 3781 ttgtgttctg tccaaaaagt cactgaactc atacttcagt acatatacat gtataaggca
 3841 cactgtagtg cttaatatgt gtaaggactt cctctttaa ttggtacca gtaacttagt
 50 3901 gacacataat gacaacaaa atattgaaa gcacttaagc actcctcctt gtggaaagaa
 3961 tataccacca ttcatctgg ctagtacc atcacaactg cattacaaa aggggatttt
 4021 tgaaaacgag gattgacca aaataatc tgaagatgat tgctttccc tgctgccagc
 4081 tgatctgaaa tgtttgctg gcacattaat catagataaa gaaagattga tggacttagc
 55 4141 cctcaaattt cagtatctat acagtactag accatgcatt cttaaaatat tagataccag
 4201 gtagtatata ttgttctgt acaaaaatga ctgtattctc tcaccagtag gacttaaac

EP 3 554 485 B9

5 4261 ttgtttctcc agtggettag ctctgttcc ttgggtgat cactagcacc cattttgag
4321 aaagctgggt ctacatgggg ggatagctgt ggaatagata atttgctgca tgtaattct
4381 caagaactaa gcctgtgcca gtgcttcct aagcagtata ctttaatca gaactcattc
4441 ccagaacctg gatgctatta cacatgcttt taagaaacgt caatgtatat cttttataa
4501 ctctaccact ttggggcaag ctattccagc actggtttg aatgctgtat gcaaccagtc
4561 tgaataccac atacgctgca ctgttcttag agggtttcca tacttaccac cgatctacaa
10 4621 ggggtgatcc ctgtttttac catcaatcat caccctgtgg tgcaaacatt gaaagaccgc
4681 gctagaggca ctatggactt caggatccac tagacagttt tcagtttgct tggaggttagc
4741 tgggtaatca aaaatgttta gtcattgatt caatgtgaac gattacggtc tttatgacca
4801 agagtctgaa aatctttttg ttatgctgtt tagtattcgt ttgatattgt tactttcac
15 4861 ctgttgagcc caaattcagg attggttcag tggcagcaat gaagttgcca tttaaatttg
4921 ttcatagcct acatcaccaa ggtctctgtg tcaaacctgt ggccactcta tatgcacttt
4981 gtttactctt tatacaaata aatatactaa agactttaca tgca

20 Human JAK1 mRNA Variant 4 (SEQ ID NO: 4)

[0106]

25

30

35

40

45

50

55

1 atctatcaca tggcagagat agaataaaaa cagaaaaatg gcgacggtca cgttggtggcg
 61 agccttgctg cgtcattaga taatcctcat gcaaatagcg ggaagaacaa aggaagggga
 121 gccccgggacc cccggggggcg caggatccgg cgggaggagt ctaagaggag gaggcggcgg
 181 tgccggagga ggaggaggag ggaggagaga gagaggaaga ccggagtccc cgcggcggcg
 241 gcggtccgga gagagggcga gccccgcgcg gcgccgggga ccgggcgcta ccacaggcc
 301 gggacgctgg agtctgggtt atctaaaaca gttcatgctg ctgaaaacct ctttctggc
 361 agatgtccct caaccctact ggtgcctggc ttctgagaca cacgttctc tgaagtagct
 421 ttggaaagta gagaagaaaa tccagtttgc ttctggaga aactggaca gctgaataaa
 481 tgcagtatct aatataaaa gaggactgca atgccatggc ttctgtgct aaaatgagga
 541 gctccaagaa gactgaggtg aacctggagg cccctgagcc aggggtggaa gtgatcttct
 601 atctgtcgga caggagagccc ctccggctgg gcagtggaga gtacacagca gaggaactgt
 661 gcatcagggc tgcacaggca tgccgtatct ctctctttg tcacaacctc ttgcctgt
 721 atgacgagaa caccaagctc tggtatgctc caaatcgac catcaccgtt gatgacaaga
 781 tgccctccg gctccactac cggatgaggt tctatttca caattggcat ggaaccaacg
 841 acaatgagca gtcagtgtgg cgtcattctc caaagaagca gaaaaatggc tacgagaaaa
 901 aaaagattcc agatgcaacc cctctcctg atgccagctc actggagtat ctgtttgctc
 961 agggacagta tgatttggg aaatgcctgg ctctattcg agacccaag accgagcagg
 1021 atggacatga tattgagaac gagtgtctag ggatggctgt cctggccatc tcacactatg
 1081 ccatgatgaa gaagatgcag ttgccagaac tgccaagga catcagctac aagcgatata
 1141 ttccagaaac attgaataag tccatcagac agaggaacct tctaccagg atgcggataa
 1201 ataattgttt caaggatttc ctaaaggaat ttaacaacaa gaccatttgt gacagcagcg
 1261 tgccacgca tgacctgaag gtgaaatact tggctacctt ggaaactttg aaaaaacatt
 1321 acggtgctga aatatttgag acttccatgt tactgattc atcagaaaat gagatgaatt
 1381 ggtttcattc gaatgacggt ggaaacgttc tctactacga agtgatggg actgggaatc
 1441 ttggaatcca gtggaggcat aaacaaatg ttgtttctgt tgaaaaggaa aaaaataaac
 1501 tgaagcggaa aaaactggaa aataaacaca agaaggatga ggagaaaaac aagatccggg
 1561 aagagtggaa caattttct tacttcctg aaatcactca cattgtaata aaggagtctg
 1621 tggtcagcat taacaagcag gacaacaaga aaatggaact gaagctctct tcccacgagg
 1681 aggccttgct ctttgtgtcc ctggtagatg gctacttccg gctcacagca gatgcccatc

1741 attacctctg caccgacgtg gccccccgt tgatcgtcca caacatacag aatggctgtc
 1801 atggtccaat ctgtacagaa tacgccatca ataaattgcg gcaagaagga agcgaggagg
 1861 ggatgtacgt gctgaggtgg agctgcaccg actttgacaa catcctcatg accgtcacct
 5 1921 gctttgagaa gtctgagcag gtgcaggggtg cccagaagca gttcaagaac ttcagatcg
 1981 aggtgcagaa gggccgctac agtctgcacg gtteggaccg cagcttcccc agcttgggag
 2041 acctcatgag ccacctcaag aagcagatcc tgccgcacgga taacatcagc ttcattgctaa
 2101 aacgctgctg ccagcccaag ccccgagaaa tctccaacct gctgggtggct actaagaaag
 10 2161 cccaggagtg gcagcccgtc taccccatga gccagctgag ttcgatcgg atcctcaaga
 2221 aggatctggt gcagggcgag caccttggga gaggcacgag aacacacatc tattctggga
 2281 ccctgatgga ttacaaggat gacgaaggaa cttctgaaga gaagaagata aaagtgatcc
 2341 tcaaagctt agacccacgc cacagggata tttccctggc ctcttcgag gcagccagca
 15 2401 tgatgagaca ggtctccac aaacacatcg tgtacctta tggcgtctgt gtccgcgacg
 2461 tggagaatat catggtggaa gatttggg aaggggtcc tctggatctc ttcattgcacc
 2521 ggaaaagcga tgtccttacc acaccatgga aattcaaatg tgccaaacag ctggccagtg
 2581 ccctgagcta cttggaggat aaagacctgg tccatggaaa tgtgtgtact aaaaacctcc
 20 2641 tctggcccg tgagggcac gacagtgaat gtggccatt catcaagctc agtgaccccg
 2701 gcaccccat tacggtgctg tctaggcaag aatgcattga acgaatcca tggattgctc
 2761 ctgagtgtgt tgaggactcc aagaacctga gtgtggctgc tgacaagtgg agctttggaa
 2821 ccacgctctg ggaaatctgc tacaatggcg agatcccctt gaaagacaag acgctgattg
 25 2881 agaaagagag attctatgaa agccggtgca ggccagtgc accatcatgt aaggagctg
 2941 ctgacctcat gaccgctgc atgaactatg acccaatca gaggccttc tccgagcca
 3001 tcatgagaga cattaataag cttgaagagc agaatccaga tattgtttca gaaaaaaac
 3061 cagcaactga agtggaaccc acacatttg aaaagcgctt ctaaaagagg atccgtgact
 30 3121 tgggagaggg ccactttggg aaggttgagc tctgcaggta tgaccccgaa ggggacaata
 3181 caggggagca ggtggctgtt aaatctctga agcctgagag tggaggtaac cacatagctg
 3241 atctgaaaaa ggaaatcgag atcttaagga acctctatca tgagaacatt gtgaagtaca
 3301 aaggaatctg cacagaagac ggaggaaatg gtattaagct catcatggaa tttctgcctt
 35 3361 cggggaagcct taaggaatat ctccaaaga ataagaacaa aataaacctc aaacagcagc
 3421 taaaatatgc cgttcagatt tgtaagggga tggactattt gggttctcgg caatacgttc
 3481 accgggactt ggcagcaaga aatgtccttg ttgagagtga acaccaagtg aaaattggag
 40 3541 acttcggtt aaccaaagca attgaaaccg ataaggagta ttacaccgtc aaggatgacc
 3601 gggacagccc tgtgttttg tatgtccag aatgttaat gcaatctaaa ttttatattg
 3661 cctctgacgt ctggtcttt ggagtcactc tgcattgagct gctgacttac tgtattcag
 3721 attctagtcc catggcttg ttctgaaaa tgataggccc aacctatggc cagatgacag
 45 3781 tcacaagact tgtgaatagc taaaagaag gaaaacgcct gccgtgccc cctaactgtc
 3841 cagatgaggt ttatcaact atgaggaaat gctgggaatt ccaaccatcc aatcggacaa
 3901 gctttcagaa ccttattgaa ggattgaag cacttttaa ataagaagca tgaataacat
 3961 ttaaattcca cagattatca agtccttctc ctgcaacaaa tgcccaagtc attttttaa
 50 4021 aatttcta at gaaagaagt tgtgttctgt ccaaaaagtc actgaactca tacttcagta
 4081 catatacatg tataaggcac actgtagtgc ttaatatgtg taaggacttc ctctttaa
 4141 ttggtaccag taacttagtg acacataatg acaacaaaaa tatttgaaag cacttaagca
 4201 ctctccttg tggaaagaat ataccacat tcatctggc tagttacca tcacaactgc
 55 4261 attacaaaaa ggggattttt gaaacgagg agtgacca aataatatct gaagatgatt
 4321 gctttccct gctgccagct gatctgaaat gtttgctgg cacattaatc atagataaag

EP 3 554 485 B9

5 4381 aaagattgat ggacttagcc ctcaaatttc agtatctata cagtactaga ccatgcattc
4441 ttaaaatatt agataccagg tagtatatat tgtttctgta caaaaatgac tgtattctct
4501 caccagtagg acttaaactt tgtttctcca gtggcttagc tcctgttcct ttgggtgac
4561 actagcacc attttgaga aagctgggtc tacatggggg gatagctgtg gaatagataa
4621 tttgtgcat gttaattctc aagaactaag cctgtgccag tgcttccta agcagtatac
4681 cttaatcag aactcattcc cagaacctgg atgctattac acatgctttt aagaaacgc
10 4741 aatgtatata cttttataac tctaccactt tggggcaagc tattccagca ctggttttga
4801 atgctgtatg caaccagtct gaataccaca tacgctgcac tgttctaga gggtttccat
4861 acttaccacc gatctacaag ggttgatccc tgttttacc atcaatcacc accctgtggt
4921 gcaacacttg aaagaccggg ctagaggcac tatggacttc aggatccact agacagttt
15 4981 cagtttgctt ggaggtagct gggtaatcaa aaatgttag tcattgattc aatgtgaacg
5041 attacggtct ttatgaccaa gagtctgaaa atcttttgt tatgctgttt agtatcggt
5101 tgatattgtt acttttcacc tgttgagccc aaattcagga ttggttcagt ggcagcaatg
5161 aagttgcat ttaaattgt tcatagccta catcaccaag gtctctgtgt caaacctgtg
20 5221 gccactctat atgcacttg tttactctt atacaaataa atatactaaa gactttacat
5281 gca

Human JAK1 mRNA Variant 5 (SEQ ID NO: 5)

[0107]

1 atctatcaca tggcagagat agaataaaaa cagaaaaatg gcgacgggtca cgttggtggcg
 61 agccttgctg cgtcattaga taatcctcat gcaaatagcg ggaagaacaa aggaagggga
 5 121 gcccgggacc cccgggggcg caggatccgg cgggaggagt ctaagaggag gaggcggcgg
 181 tgccggagga ggaggaggag ggaggagagaa gagaggaaga ccggagtccc cgcggcggcg
 241 gcggtccgga gagagggcga gccccgcgcg gcgccgggga ccgggcgcta ccacgaggcc
 301 gggacgctgg agtctgggcg cttctctgaa gtagctttgg aaagtagaga agaaaatcca
 10 361 gtttgcttct tggagaacac tggacagctg aataaatgca gtatctaat ataaaagagg
 421 actgcaatgc catggcttct tgtgctaaaa tgaggagctc caagaagact gaggtgaacc
 481 tggaggcccc tgagccaggg gtggaagtga tcttctatct gtcggacagg gagccccctc
 541 ggctgggcag tggagagtac acagcagagg aactgtgcat cagggtgca caggcatgcc
 15 601 gtatctctcc tcttgctac aacctcttg cctgtatga cgagaacacc aagctctggt
 661 atgctccaaa tcgcaccatc accgttgatg acaagatgct cctccggctc cactaccgga
 721 tgaggttcta tttaccaat tggcatggaa ccaacgacaa tgagcagtca gtgtggcgct
 781 atttccaaa gaagcagaaa aatggctacg agaaaaaaaa gattccagat gcaaccctc
 20 841 tccttgatgc cagctcactg gagtatctgt ttgctcaggg acagtatgat ttggtgaaat
 901 gcctggctcc tattegagac cccaagaccg agcaggatgg acatgatatt gagaacgagt
 961 gtctagggat ggctgtcctg gccatctcac actatgccat gatgaagaag atgcagttgc
 25 1021 cagaactgcc caaggacatc agctacaagc gatatatcc agaaacattg aataagtcca
 1081 tcagacagag gaacctctc accaggatgc ggataaataa tgtttcaag gatttctaa
 1141 aggaatttaa caacaagacc atttgtaga gcagcgtgct cacgcatgac ctgaaggatga
 1201 aatactggc taccttgga actttgacaa aacattacgg tgctgaaata ttgagactt
 30 1261 ccatgttact gatttcatca gaaaatgaga tgaattggtt tcattcgaat gacggtggaa
 1321 acgttctcta ctacgaagtg atggtgactg ggaatcttgg aatccagtgagggcataaac
 1381 caaatgttgt ttctgtgaa aaggaaaaaa ataaactgaa gcggaaaaaa ctggaaaata

1441 aacacaagaa ggatgaggag aaaaacaaga tccgggaaga gtggaacaat tttcttact
 1501 tccctgaaat cactcacatt gtaataaagg agtctgtggt cagcattaac aagcaggaca
 1561 acaagaaaat ggaactgaag ctctctccc acgaggaggc ctgtccttt gtgtccctgg
 5 1621 tagatggcta ctccgggctc acagcagatg cccatcatta cctctgcacc gacgtggccc
 1681 ccccggtgat cgtccacaac atacagaatg gctgtcatgg tccaatctgt acagaatacg
 1741 ccatcaataa attgcggaac gaaggaagcg aggaggggat gtacgtgctg aggtggagct
 1801 gcaccgactt tgacaacatc ctcatgaccg tcacctgctt tgagaagtct gagcaggtgc
 10 1861 aggggtgccc gaagcagttc aagaacttc agatcgaggt gcagaagggc cgctacagtc
 1921 tgcacggttc ggaccgcagc tccccagct tgggagacct catgagccac ctaagaagc
 1981 agatcctgcg cacggataac atcagcttca tgctaaaacg ctgctgccag cccaagcccc
 2041 gagaaatctc caacctgctg gtggctacta agaaagccc gaagtggcag cccgtctacc
 15 2101 ccatgagcca gctgagtttc gatcggtacc tcaagaagga tctggtgcag ggcgagcacc
 2161 ttgggagagg cagagaaca cacatctatt ctgggacct gatggattac aaggatgacg
 2221 aaggaacttc tgaagagaag aagataaaa tgatcctcaa agtcttagac cccagccaca
 2281 gggatatttc cctggccttc ttcgaggcag ccagcatgat gagacaggtc tcccacaaac
 20 2341 acatcgtgta cctctatggc gtctgtgtcc gcgacgtgga gaatatcatg gtggaagagt
 2401 ttgtggaagg gggctctctg gatctcttca tgcaccggaa aagcagatgc cttaccacac
 2461 catggaaatt caaagtggcc aaacagctgg ccagtgcctt gagctacttg gaggataaag
 2521 acctggcca tggaaatgtg tgtactaaaa acctcctcct ggcccgtgag ggcatcgaca
 25 2581 gtgagtgtgg cccattcatc aagctcagtg accccggcat cccattacg gtgctgtcta
 2641 ggcaagaatg cattgaacga atcccatgga ttgctcctga gtgtgtgag gactccaaga
 2701 acctgagtgt ggctgctgac aagtggagct ttggaaccac gctctgggaa atctgctaca
 2761 atggcgagat ccccttgaaa gacaagacgc tgattgagaa agagagattc tatgaaagcc
 30 2821 ggtgcaggcc agtgacacca tcatgtaagg agctggctga cctcatgacc cgctgcatga
 2881 actatgacc caatcagagg ctttcttcc gagccatcat gagagacatt aataagctg
 2941 aagagcagaa tccagatatt gtttcagaaa aaaaaccagc aactgaagtg gacccacac
 3001 attttgaaaa gcgcttcta aagaggatcc gtgacttggg agagggccac ttgggaagg
 35 3061 ttgagctctg caggtatgac cccgaagggg acaatacagg ggagcaggtg gctgttaaat
 3121 ctctgaagcc tgagagtga ggtaaccaca tagctgatct gaaaaaggaa atcgagatct
 3181 taaggaacct ctatcatgag aacattgtga agtacaaagg aatctgcaca gaagacggag
 3241 gaaatggtat taagtcac atggaatttc tgccttcggg aagcettaag gaatatcttc
 40 3301 caaagaataa gaacaaaata aacctcaaac agcagctaaa atatgccgtt cagatttga
 3361 aggggatgga ctatttgggt tctcggaat acgttcaccg ggacttggca gcaagaaatg
 3421 tccttgttga gagtgaacac caagtgaaaa ttggagactt cgggttaacc aaagcaattg
 45 3481 aaaccgataa ggagtattac accgtcaagg atgaccggga cagccctgtg ttttggatg
 3541 ctccagaatg ttaatgcaa tctaaattt atattgcctc tgacgtctgg tcttttggag
 3601 tctcttgca tgagctgctg acttactgtg attcagattc tagtccatg gctttgtcc
 3661 tgaaaatgat aggcccaacc catggccaga tgacagtcac aagacttgg aatacgttaa
 50 3721 aagaaggaaa acgctgccc tgccaccta actgtccaga tgaggttat caacttatga
 3781 ggaaatgctg ggaattcaa ccatccaatc ggacaagctt tcagaacctt attgaaggat
 3841 ttgaagcact tttaaaataa gaagcatgaa taacatttaa attccacaga ttatcaagtc
 3901 ctctcctgc acaaatgcc caagtcattt ttaaaaatt tctaatgaaa gaagtttgtg
 55 3961 ttctgtccaa aaagtcaact aactcatact tcagtacata tacatgtata aggcacactg
 4021 tagtgcttaa tatgtgaag gacttctct ttaatttgg taccagtaac ttagtgacac

4081 ataatgacaa ccaaaatatt tgaaagcact taagcactcc tccttggtga aagaatatac
 4141 caccatttca tctggctagt tcaccatcac aactgcatta ccaaaagggg attttgaaa
 5 4201 acgaggagtt gacaaaaata atatctgaag atgattgctt tccctgctg ccagctgac
 4261 tgaaatgttt tgctggcaca ttaatcatag ataaagaaag attgatggac ttagccctca
 4321 aatttcagta tctatacagt actagacat gcattcttaa aatattagat accaggtagt
 4381 atatattggt tctgtacaaa aatgactgta ttctctcacc agtaggactt aaactttgtt
 10 4441 tctccagtgg cttagctcct gtctcttgg gtgatcacta gcaccattt ttgagaaagc
 4501 tggttctaca tgggggggata gctgtggaat agataattg ctgcatgtta attctcaaga
 4561 actaagcctg tgccagtgc ttcctaagca gtatacctt aatcagaact cattcccaga
 4621 acctggatgc tattacacat gctttaaga aacgtcaatg tatatcctt tataactcta
 15 4681 ccactttggg gcaagctatt ccagcactgg tttgaatgc tgatgcaac cagtctgaat
 4741 accacatacg ctgcactgtt cttagagggt ttccatactt accaccgac tacaagggtt
 4801 gatccctgtt ttaccatca atcatcacc tgtggtgcaa cacttgaaag acccggctag
 4861 aggcactatg gacttcagga tccactagac agtttctagt ttgcttgag gtagctgggt
 20 4921 aatcaaaaat gtttagtcat tgattcaatg tgaacgatta cggctttat gaccaagagt
 4981 ctgaaaatct tttgttatg ctgttagta ttcgttgat attgttactt ttcactgtt
 5041 gagcccaaat tcaggattgg ttcagtggca gcaatgaagt tgccatttaa attgttcat
 5101 agcctacatc accaaggtct ctgtgtcaa cctgtggcca ctctatatgc actttgttta
 25 5161 ctctttatac aaataaatat actaaagact ttacatgca

Human JAK1 mRNA Variant 6 (SEQ ID NO: 6)

30 [0108]

35

40

45

50

55

1 ggggccccgac gggaggcggg gcgtcgctga gcgcaggccg cggcggccgc ggagtatcct
 61 ggagctgcag acagtgcggg cctgcgcca gtccggctg tctcgccgc gacctcct
 121 cagccctggg cgcgcgcacg ctggggcccc gcggggctgg ccgcctagcg agcctgccgg
 181 tcgacccag ccagcgcagc gacggggcgc tgctggccc aggcgcacac ggaagtgtta
 241 tctaaaacag tcatgctgc tgaaacctc ctcttgga gatgtccctc aacctactg
 301 gtgcctggct tctgagacac acgttctct gaagtagctt tggaaagtag agaagaaaat
 361 ccagtttgc tctggagaa cactggacag ctgaataat gcagtatcta aatataaaag
 421 aggactgcaa tgccatggct ttctgtgcta aaataggag ctccaagaag actgaggtga
 481 acctggaggc cctgagcca ggggtggaag tgatcttcta tctgtcggac agggagcccc
 541 tccggctggg cagtggagag tacacagcag aggaactgtg catcagggtc gcacaggcat
 601 gccgtatctc tctctttgt cacaacctc ttgccctgta tgacgagaac accaagctc
 661 ggtatgtcc aaatgcacc atcaccgtg atgacaagat gtcctccgg ctccactacc
 721 ggatgaggtt ctattcacc aattggcatg gaaccaacga caatgagcag tcaagtgtgc
 781 gtcattctcc aaagaagcag aaaaatggct acgagaaaaa aaagattcca gatgcaacc
 841 ctctcttga tgccagctca ctggagtatc tgttgctca gggacagtat gatttggtga
 901 aatgcctggc tctattcga gacccaaga ccgagcagga tggacatgat attgagaacg
 961 agtgtctagg gatggctgc ctggccatct cacactatgc catgatgaag aagatgcagt
 1021 tgccagaact gccaaggac atcagctaca agcgatatat tccagaaaca tgaataagt
 1081 ccatcagaca gaggaacctt ctcaccagga tgcggataaa taatgtttc aaggatttcc
 1141 taaaggaatt taacaacaag accatttgatg acagcagcgt gtccacgcat gacctgaagg
 1201 tgaaatactt ggctacctg gaaacttga caaacatta cgggtgctgaa atatttgaga
 1261 ctccatggt actgatttca tcagaaaatg agatgaattg gtttcattcg aatgacggtg
 1321 gaaacgttct ctactacgaa gtgatggtga ctgggaatct tggaatccag tggaggcata

1381 aaccaaagtgt tgtttctgtt gaaaaggaaa aaaataaact gaagcggaaa aaactggaaa
 1441 ataaacacaa gaaggatgag gagaaaaaca agatccggga agagtggaaac aattttctt
 1501 acttcctga aatcactcac attgtaataa aggagtctgt ggtcagcatt aacaagcagg
 5 1561 acaacaagaa aatggaactg aagctctctt cccacgagga ggcttgtcc tttgtgtccc
 1621 tggtagatgg ctacttccgg ctcacagcag atgcccata ttacctctgc accgacgtgg
 1681 cccccccgtt gatcgtccac aacatacaga atggctgtca tggccaate tgtacagaat
 1741 acgccatcaa taaattgcgg caagaaggaa gcgaggaggg gatgtacgtg ctgaggtgga
 10 1801 gctgcaccga ctttgacaac atctcatga cgtcacctg ctttgagaag tctgagcagg
 1861 tgcagggtgc ccagaagcag ttcaagaact ttcagatcga ggtgcagaag ggccgctaca
 1921 gtctgcacgg ttcggaccgc agcttcccca gcttgggaga cctcatgagc cacctcaaga
 1981 agcagatcct gcgcacggat aacatcagct tcatgctaaa acgtgctgc cagcccaagc
 15 2041 cccgagaaat ctccaacctg ctggtggcta ctaagaaagc ccaggagtgg cagcccgtct
 2101 acccatgag ccagctgagt ttcgatcga tcctcaagaa ggatctggtg cagggcgagc
 2161 accttgggag aggcacgaga acacacatct attctgggac cctgatggat tacaaggatg
 2221 acgaaggaa ttctgaagag aagaagataa aagtatcct caaagtctta gacccagcc
 20 2281 acagggatat ttccctggcc ttcttcgagg cagccagcat gatgagacag gtctcccaca
 2341 aacacatcgt gtacctctat ggctgtgtg tccgcgacgt ggagaatata atggtggaag
 2401 agtttgtgga aggggggtct ctggatctct tcatgcaccg gaaaagcgat gtccttacca
 2461 caccatggaa attcaaagt gccaacacgc tggccagtgc cctgagctac ttggaggata
 25 2521 aagacctggt ccattggaat gtgtgtacta aaaacctct cctggcccgt gagggcatcg
 2581 acagtgagtg tggccattc atcaagctca gtgaccccg catcccatc acggtgctgt
 2641 ctaggcaaga atgcattgaa cgaatccat ggattgctcc tgagtgtgtt gaggactcca
 2701 agaacctgag tgtggctgt gacaagtga gcttggaa cagctctgg gaaatctgt
 30 2761 acaatggcga gatcccctg aaagacaaga cgctgattga gaaagagaga ttctatgaaa
 2821 gccggtgcag gccagtga ccatcatgta aggagctggc tgacctcatg accgctgca
 2881 tgaactatga cccaatcag aggccttct tccgagccat catgagagac attaataagc
 2941 ttgaagagca gaatccagat attgttcag aaaaaaac agcaactgaa gtggaccca
 35 3001 cacatttga aaagcgctc cttaaagagga tccgtgactt gggagagggc cacttggga
 3061 aggttgagct ctgcaggtat gacccgaag gggacaatac aggggagcag gtggctgta
 3121 aatctctgaa gcctgagagt ggaggtaacc acatagctga tctgaaaaag gaaatcgaga
 3181 tcttaaggaa cctctatcat gagaacattg tgaagtacaa agaatctgc acagaagacg
 40 3241 gaggaatgg tattaagctc atcatggaat ttctgccttc gggaagcctt aaggaatata
 3301 ttcaaagaa taagaacaaa ataaacctca aacagcagct aaaatatgcc gttcagattt
 3361 gtaaggggat ggactatttg ggttctcggc aatacgttca ccgggacttg gcagcaagaa
 45 3421 atgtccttgt tgagagtga caccaagtga aaattggaga cttcggtta accaaagcaa
 3481 ttgaaaccga taaggatgat tacaccgtca aggatgaccg ggacagccct gtgttttgg
 3541 atgtccaga atgttaatg caatctaaat tttatattgc ctctgacgtc tggcttttg
 3601 gagtactct gcatgagctg ctgacttact gtgattcaga tttagtccc atggcttgt
 50 3661 tctgaaaat gataggecca acccatggcc agatgacagt cacaagactt gtgaatacgt
 3721 taaaagaagg aaaacgctg ccgtgccac ctaactgtcc agatgaggtt tatcaacta
 3781 tgaggaaatg ctgggaattc caaccatcca atcgacaag ctttcagaac cttattgaag
 3841 gatttgaagc acttttaaaa taagaagcat gaataacatt taaattccac agattatcaa
 55 3901 gtcttctec tgcaacaaat gcccaagtca tttttaaaa atttetaatg aaagaagttt
 3961 gtgttctgc caaaaagtc ctgaactcat acttcagtac atatacatgt ataaggcaca

4021 ctgtagtgt taatatgtgt aaggacttcc tctttaaatt tggtagcagt aacttagtga
 4081 cacataatga caacaaaaat atttgaaagc acttaagcac tcctccttgt ggaaagaata
 4141 taccaccatt tcatctggct agttcacat cacaactgca ttacaaaag gggattttg
 5 4201 aaaacgagga gttgacaaa ataatatctg aagatgattg ctttccttg ctgccagctg
 4261 atctgaaatg tttgctggc acattaatca tagataaaga aagattgatg gacttagccc
 4321 tcaaatttca gtatctatac agtactagac catgcattct taaaatatta gataccaggt
 4381 agtatatatt gtttctgtac aaaaatgact gtattctctc accagtagga cttaaacttt
 10 4441 gtttctccag tggcttagct cctgttcctt tgggtgatca ctagcaccca ttttgagaa
 4501 agctgggtct acatgggggg atagctgtgg aatagataat ttgctgcatg ttaatttca
 4561 agaactaagc ctgtgccagt gcttcctaa gcagtatacc ttaatcaga actcattccc
 15 4621 agaacctgga tgctattaca catgcttta agaaacgtca atgtatatcc tttataact
 4681 ctaccacttt ggggcaagct attccagcac tggtttgaa tgctgtatgc aaccagtctg
 4741 aataccacat acgctgcact gttcttagag ggtttccata cttaccaccg atctacaagg
 4801 gttgatccct gttttacca tcaatcatca ccctgtgggtg caacacttga aagacccggc
 20 4861 tagaggcact atggacttca ggatccacta gacagtttc agtttgctg gaggtagctg
 4921 ggtaatcaaa aatgtttagt cattgattca atgtgaacga ttacgggtct tatgaccaag
 4981 agtctgaaaa tcttttgtt atgctgttta gtattcgtt gatattgtta ctttcacct
 5041 gttgagccca aattcaggat tgggtcagtg gcagcaatga agttgccatt taaatttgt
 25 5101 catagcctac atcaccaagg tctctgtgtc aaacctgtgg ccactctata tgcactttgt
 5161 ttactcttta taaaataaa tatactaaag actttacatg ea

Human JAK1 mRNA Variant 7 (SEQ ID NO: 7)

[0109]

1 agaagcggag cgtatacggg ggagggcggga tgcatttctg catcgagcgc acaaagcgt
 61 tctctgaagt agctttggaa agtagagaag aaaatccagt ttgcttctg gagaacctg
 5 121 gacagctgaa taaatgcagt atctaaatat aaaagaggac tgcaatgccca tggcttctg
 181 tgctaaaatg aggagctcca agaagactga ggtgaacctg gagggccctg agccaggggt
 241 ggaagtgatc ttctatctgt cggacaggga gccctccgg ctgggcagtg gagagtacac
 301 agcagaggaa ctgtgcatca gggctgcaca ggcatgccgt atctctctc tttgcacaa
 10 361 cctctttgcc ctgtatgacg agaacaccaa gctctggtat gctccaaatc gcaccatcac
 421 cgttgatgac aagatgtccc tccggctcca ctaccggatg aggttctatt tcaccaattg
 481 gcatggaacc aacgacaatg agcagtcagt gtggcgtcat tctccaaaga agcagaaaaa
 541 tggctacgag aaaaaaaga ttccagatgc aacctctc ctgatgccca gctcactgga
 15 601 gtatctgttt gctcaggga agtatgattt ggtgaaatgc ctggctccta ttcgagacct
 661 caagaccgag caggatggac atgatattga gaacgagtgt ctagggatgg ctgtcttggc
 721 catctcacac tatgcatga tgaagaagat gcagttgccca gaactgcccaggacatcag
 781 ctacaagcga tatattccag aaacattgaa taagtccatc agacagagga acctctcac
 20 841 caggatgcgg ataaataatg tttcaagga tttcctaaag gaatttaaca acaagaccat
 901 ttgtgacagc agcgtgtcca cgcagacat gaaggtgaaa tacttggtta ccttggaac
 961 ttgacaaaa cattacgggtg ctgaaatatt tgagacttcc atgttactga tttcatcaga
 1021 aatgagatg aattggttc attcgaatga cgggtggaac gttcttact acgaagtgat
 25 1081 ggtgactggg aatcttgga tccagtggag gcataaacca aatgttgtt ctgttgaaaa
 1141 ggaaaaaat aaactgaagc ggaaaaaact ggaaaaataa cacaagaagg atgaggagaa
 1201 aaacaagatc cgggaagagt ggaacaattt ttcttactt cctgaaatca ctcacattgt
 30 1261 aataaaggag tctgtgttca gcattaacaa gcaggacaac aagaaaatgg aactgaagct

35

40

45

50

55

1321 ctcttccac gaggaggcct tgcctttgt gtccttgga gatggctact tccggctcac
 1381 agcagatgcc catcattacc tctgcaccga cgtggccccc cgttgatcg tccacaacat
 1441 acagaatggc tgtcatggc caatctgtac agaatacgcc atcaataaat tgcggcaaga
 5 1501 aggaagcggag gagggggatgt acgtgctgag gtggagctgc accgactttg acaacatcct
 1561 catgaccgtc acctgctttg agaagtctga gcaggtgcag ggtgccaga agcagttcaa
 1621 gaactttcag atcgaggtgc agaagggccg ctacagtctg cacggttcgg accgcagctt
 1681 cccagcttg ggagacctca tgagccacct caagaagcag atcctgcgca cggataacat
 10 1741 cagcttcattg ctaaaacgct gctgccagcc caagccccga gaaatctcca acctgctggt
 1801 ggctactaag aaagcccagg agtggcagcc cgtctacccc atgagccagc tgagtttca
 1861 tcggatctc aagaaggatc tgggtgcaggg cgagcacctt gggagaggca cgagaacaca
 1921 catctattct gggacctga tggattacaa ggaatgacgaa ggaacttctg aagagaagaa
 15 1981 gataaaagtg atcctcaaag tcttagacct cagccacagg gatatttccc tggccttctt
 2041 cgaggcagcc agcatgatga gacaggtctc ccacaaacac atcgtgtacc tctatggcgt
 2101 ctgtgtccgc gacgtggaga atatcatggt ggaagagttt gtggaagggg gtcctctgga
 2161 tctcttcattg caccggaaaa gcatgtcct taccacacca tggaaattca aagttgcaa
 20 2221 acagctggcc agtgcctga gctacttga ggataaagac ctggtccatg gaaatgtgtg
 2281 tactaaaaac ctctcctgg cccgtgaggg catcgacagt gagtgtggcc cattcatcaa
 2341 gctcagtgac cccggcatcc ccattacggt gctgtctagg caagaatgca ttgaacgaat
 2401 cccatggatt gctcctgagt gtgtgagga ctccaagaac ctgagtgtgg ctgctgacaa
 25 2461 gtggagcttt ggaaccacgc tctgggaaat ctgctacaat ggcgagatcc ccttgaaaga
 2521 caagacgtg attgagaaag agagattcta tgaaagccgg tgcaggccag tgacaccatc
 2581 atgtaaggag ctggctgacc tcatgacccg ctgcatgaac tatgaccca atcagaggcc
 2641 tttctccga gccatcatga gagacattaa taagctgaa gacgagaatc cagatattgt
 30 2701 ttcagaaaaa aaaccagcaa ctgaagtga cccacacat ttgaaaagc gcttctaaa
 2761 gaggatccgt gacttgggag agggccactt tgggaagggt gagctctgca ggtatgacct
 2821 cgaaggggac aatacagggg agcaggtggc tgttaaatct ctgaagcctg agagtggagg
 35 2881 taaccacata gctgatctga aaaaggaaat cgagatctta aggaacctct atcatgagaa
 2941 cattgtgaag taaaaggaa tctgcacaga agacggagga aatggtatta agctcatcat
 3001 ggaatttctg ccttcgggaa gccttaagga atatctcca aagaataaga acaaaataaa
 3061 cctcaaacag cagctaaaat atgccgttca gatttgaag gggatggact atttgggtc
 40 3121 tggcaatac gttcaccggg acttggcagc aagaaatgtc cttgttgaga gtgaacacca
 3181 agtgaaaatt ggagacttcg gttaaccaa agcaattgaa accgataagg agtattacac
 3241 cgtcaaggat gaccgggaca gccctgtgtt ttggtatgct ccagaatgtt taatgcaatc
 3301 taaattttat attgcctctg acgtctggc ttttgagtc actctgcatg agctgctgac
 45 3361 ttactgtgat tcagattcta gtccatggc tttgttctg aaaatgatag gcccaacca
 3421 tggccagatg acagtcacaa gacttgtgaa tacgttaaaa gaaggaaaac gcctgccgtg
 3481 cccacctaac tgtccagatg aggtttatca acttatgagg aatgctggg aattccaacc
 3541 atccaatcgg acaagcttc agaaccttat tgaaggattt gaagcactt taaaataaga
 50 3601 agcatgaata acatttaaat tccacagatt atcaagtcct tctcctgcaa caaatgccc
 3661 agtcattttt taaaatttc taatgaaga agtttgtgtt ctgtcaaaa agtcactgaa
 3721 ctcatcttc agtacatata catgtataag gcacactgta gtgcttaata tgtgtaagga
 3781 ctctctctt aaatttggta ccagtaactt agtgacacat aatgacaacc aaaatatttg
 55 3841 aaagcactta agcactctc cttgtggaaa gaatatacca ccatttcac tggctagttc
 3901 accatcacia ctgcattacc aaaaggggat tttgaaaac gaggagttga ccaaataat

3961 atctgaagat gattgctttt ccctgctgcc agctgatctg aaatgttttg ctggcacatt
 4021 aatcatagat aaagaaagat tgatggactt agccctcaaa ttccagtatc tatacagtac
 5 4081 tagaccatgc attcttaaaa tattagatac caggtagtat atattgttc tgtacaaaaa
 4141 tgactgtatt ctctcaccag taggacttaa actttgttc tccagtggct tagctcctgt
 4201 tcctttgggt gatcactagc acccatttt gagaaagctg gttctacatg gggggatagc
 4261 tgtggaatag ataattgct gcatgttaat tctcaagaac taagcctgtg ccagtgcctt
 10 4321 cctaagcagt atacctttaa tcagaactca ttcccagaac ctggatgcta ttacacatgc
 4381 ttttaagaaa cgtcaatgta tatecttta taactctacc actttggggc aagctattcc
 4441 agcactgggt ttgaatgctg tatgcaacca gtctgaatac cacatacgtc gcactgttct
 4501 tagagggttt ccatacttac caccgatcta caagggttga tccctgtttt taccatcaat
 15 4561 catcacccctg tgggtgaaca cttgaaagac ccggctagag gcactatgga cttcaggatc
 4621 cactagacag tttcagttt gcttgagggt agctgggtaa tcaaaaatgt ttagtcattg
 4681 attcaatgtg aacgattacg gtctttatga ccaagagtct gaaaatcttt ttgttatgct
 4741 gtttagtatt cgtttgatat tgttactttt cacctgttga gcccaaattc aggattgggt
 20 4801 cagtggcagc aatgaagttg ccatttaaatt ttgttcacag cctacatcac caaggtctct
 4861 gtgtcaaacc tgtggccact ctatatgcac ttgtttact ctttatacaa ataaatatac
 4921 taaagacttt acatgca

25 **Human JAK1 mRNA Variant 8 (SEQ ID NO: 8)**

[0110]

30

35

40

45

50

55

1 ggggccccgac gggaggcggt gcgctcgctga ggcgaggccg cggcgggccgc ggagtatcct
 61 ggagctgcag acagtgcggg cctgcgcccc gtcccggctg tctcgccgc gacccctcct
 121 cagccctggg cgcgcgcacg ctggggcccc gcggggctgg ccgcctagcg agcctgccgg
 181 tcgaccccag ccagcgcagc gacggggcgc tgccctggccc aggcgcacac ggaagtgcgc
 241 ttctctgaag tagctttgga aagtagagaa gaaaatccag ttgcttctt ggagaacact
 301 ggacagctga ataatgcag tatctaaata taaaagagga ctgcaatgcc atggcttct
 361 gtgctaaaat gaggagctcc aagaagactg aggtgaacct ggaggcccct gagccagggg
 421 tggaaagtga ctctatctg tcggacaggg agcccctccg gctgggcagt ggagagtaca
 481 cagcagagga actgtgcac agggctgcac aggcattgcc tatctctcct ctttgcaca
 541 acctcttgc cctgtatgac gagaacacca agctctggtg tgctccaaat cgcaccatca
 601 ccgttgatga caagatgcc ctccggctcc actaccgat gaggttctat ttaccaatt
 661 ggcatggaac caacgacaat gacagtcag tgggctgca ttctccaaag aagcagaaaa
 721 atggctacga gaaaaaaaaag attccagatg caaccctct cttgatgcc agctcactgg
 781 agtatctgtt tgctcaggga cagtatgatt tggtgaaatg cctggctcct atcgagacc
 841 ccaagaccga gcaggatgga catgatattg agaacgagtg tctagggatg gctgtcctgg
 901 ccatctcaca ctatgccatg atgaagaaga tgcagtgcc agaactgccc aaggacatca
 961 gctacaagcg atatattcca gaaacattga ataagtccat cagacagagg aaccttctca
 1021 ccaggatgag gataaataat gtttcaagg atttctaaa ggaatttaac aacaagacca
 1081 ttttgacag cagcgtgtcc acgcatgacc tgaagggtgaa atacttggct acctggaaa
 1141 ctttgacaaa acattacggg gctgaaatat ttgagacttc catgttactg attcatcag
 1201 aaaatgagat gaattggtt cattcgaatg acggtggaaa cgttctctac tacgaagtga
 1261 tggtgactgg gaatcttggg atccagtggg ggcataaacc aaatgttgtt tctgttgaag
 1321 aggaaaaaaaa taaactgaag cggaaaaaac tggaaaataa acacaagaag gatgaggaga
 1381 aaaacaagat ccgggaagag tggacaattt ttcttactt cctgaaatc actcacattg
 1441 taataaagga gtctgtggtc agcattaaca agcaggacaa caagaaaatg gaactgaagc

1501 tctcttccca cgaggaggcc ttgtccttg tgccctggg agatggctac ttccggctca
 1561 cagcagatgc ccatcattac ctctgcaccg acgtggcccc cccgttgatc gtccacaaca
 1621 tacagaatgg ctgtcatggg ccaatctgta cagaatacgc catcaataaa ttgcggcaag
 5 1681 aaggaagcga ggaggggatg tacgtgctga ggtggagctg caccgacttt gacaacatcc
 1741 tcatgaccgt cacctgcttt gagaagtctg aggtgcaggg tgcccagaag cagttaaga
 1801 actttcagat cgaggtgcag aagggccgct acagtctgca cggttcggac cgcagcttc
 1861 ccagcttggg agacctcatg agccacctca agaagcagat cctgcgcacg gataacatca
 10 1921 gcttcatgct aaaacgctgc tgccagccca agccccgaga aatctccaac ctgctgggtg
 1981 ctactaagaa agcccaggag tggcagcccg tctacccat gagccagctg agtttcgac
 2041 ggatcctcaa gaaggatctg gtgcagggcg agcaccttgg gagaggcacg agaacacaca
 2101 tctattctgg gacctgatg gattacaagg atgacgaagg aacttctgaa gagaagaaga
 15 2161 taaaagtgat cctcaaagtc ttagaccca gccacaggga tatttccctg gccttcttcg
 2221 aggcagccag catgatgaga caggtctccc acaaacacat cgtgtacctc tatggcgtct
 2281 gtgtccgcga cgtggagaat atcatgggtg aagagtttgt ggaagggggg cctctggatc
 2341 tcttcatgca ccgaaaagc gatgtcctta ccacaccatg gaaattcaaa gttgccaac
 20 2401 agctggccag tgccctgagc tacttggagg ataaagacct ggtccatgga aatgtgtgta
 2461 ctaaaaacct cctctggcc cgtgagggca tcgacagtga gtgtggccca ttcatcaagc
 2521 tcagtgacc cggcatcccc attacgggtc tgtctaggca agaatgcatt gaacgaatcc
 2581 catggattgc tctgagtgt gttgaggact ccaagaacct gagtgtggct gctgacaagt
 25 2641 ggagctttgg aaccacgctc tgggaaatct gctacaatgg cgagatcccc ttgaaagaca
 2701 agacgtgat tgagaaagag agattctatg aaagccggtg caggccagtg acaccatcat
 2761 gtaaggagct ggctgacctc atgacccgct gcatgaacta tgaccccaat cagaggcctt
 2821 tcttccgagc catcatgaga gacattaata agcttgaaga gcagaatcca gatattgttt
 30 2881 cagaaaaaaa accagcaact gaagtggacc ccacacattt tgaagcgc ttctaaaga
 2941 ggatccgtga ctgggagag ggccacttgg ggaagggtga gctctgcagg tatgaccccg
 3001 aaggggacaa tacaggggag caggtggctg taaatctct gaagcctgag agtggaggta
 3061 accacatagc tgatctgaaa aaggaaatcg agatcttaag gaacctctat catgagaaca
 35 3121 ttgtgaagta caaaggaatc tgcacagaag acggaggaaa tggatattaag ctcatcatgg
 3181 aatttctgcc ttcggaagc ctaaggaat atcttccaaa gaataagaac aaaataaacc
 3241 tcaaacagca gctaaaatat gccgttcaga ttgtaaggg gatggactat ttgggttctc
 3301 ggcaatacgt tcacgggac ttggcagcaa gaaatgtcct tgttgagagt gaacaccaag
 40 3361 tgaagattgg agacttcggt ttaaccaag caattgaaac cgataaggag tattacaccg
 3421 tcaaggatga ccgggacagc cctgtgtttt ggtatgctcc agaattgtta atgcaatcta
 3481 aattttatat tgcctctgac gtctggtctt ttggagtcac tctgcatgag ctgctgactt
 45 3541 actgtgattc agattctagt cccatggctt ttttctgaa aatgataggc ccaacctatg
 3601 gccagatgac agtcacaaga ctgtgaata cgtaaaaga aggaaaacgc ctgccgtgcc
 3661 cacctaactg tccagatgag gtttatcaac ttatgaggaa atgctgggaa ttccaacct
 3721 ccaatcggac aagcttcag aacctattg aaggattga agcacttta aaataagaag
 50 3781 catgaataac atttaaattc cacagattat caagtcttc tctgcaaca aatgcccag
 3841 tcattttta aaaatttcta atgaaagaag tttgtgtt gtccaaaaag tactgaact
 3901 catacttcag tacatataca tgtataaggc acactgtagt gcttaatatg tgtaaggact
 3961 tctctttaa atttggatc agtaacttag tgacacataa tgacaacaa aatatttgaa
 55 4021 agcacttaag cactctcct tgtggaaaga atataccacc atttcatctg gctagttcac
 4081 catcacaact gcattacaa aaggggattt tgaaaacga ggagttgacc aaaataatat

4141 ctgaagatga ttgcttttcc ctgctgccag ctgatctgaa atgttttgct ggcacattaa
 4201 tcatagataa agaaagattg atggacttag ccctcaaatt tcagtatcta tacagtacta
 5 4261 gaccatgcat tcttaaaata ttagatacca ggtagtatat attgtttctg tacaaaaatg
 4321 actgtattct ctcaccagta ggacttaaac ttgtttctc cagtggctta gctcctgttc
 4381 ctttgggtga tcactagcac ccatttttga gaaagctggt tctacatggg gggatagctg
 4441 tggaatagat aatttgctgc atgttaattc tcaagaacta agcctgtgcc agtgctttcc
 10 4501 taagcagtat acctttaatc agaactcatt ccagaaacct ggatgctatt acacatgctt
 4561 ttaagaaacg tcaatgtata tcctttata actctaccac ttgggggcaa gctattccag
 4621 cactggtttt gaatgctgta tgcaaccagt ctgaatacca catacgtgc actgtttcta
 4681 gagggtttcc atacttacca ccgatctaca agggttgatc cctgtttta ccatcaatca
 15 4741 tcacctgtg gtgcaacact tgaaagaccc ggctagaggc actatggact tcaggatcca
 4801 ctagacagtt ttcagtttgc ttggaggtag ctgggtaatc aaaaatgttt agtcattgat
 4861 tcaatgtgaa cgattacggc ctttatgacc aagagtctga aaatctttt gttatgctgt
 20 4921 ttagtattcg ttgatattg ttacttttca cctgttgagc ccaaattcag gattggttca
 4981 gtggcagcaa tgaagtgcc atttaaattt gttcatagcc tacatcacca aggtctctgt
 5041 gtcaaacctg tggccactct atatgcactt tgtttactct ttatacaat aaatatacta
 5101 aagactttac atgca

25 **Human JAK2 mRNA Variant 1 (SEQ ID NO: 9)**

[0111]

30

35

40

45

50

55

1 ctgcaggaag gagagaggaa gaggagcaga agggggcagc agcggacgcc gctaacggcc
 61 tcctcggcg ctgacaggct gggccggcgc ccggctcgt tgggtgttcg cgtcgccact
 121 tcggcttctc ggccggtcgg gcccctcggc ccgggcttgc ggcgcgcgtc ggggctgagg
 181 gctgctgcgg cgcagggaga ggcctggtcc tcgctgccga gggatgtgag tgggagctga
 241 gcccacactg gagggcccc gagggcccag cctggaggtc gttcagagcc gtgcccgtcc
 301 cggggcttcg cagacctga cccgccgggt aggagccgcc cctgcgggct cgagggcgcg
 361 ctctggtcgc ccgatctgtg tagccggtt cagaagcagg caacaggaac aagatgtgaa
 421 ctgtttctct tctgcagaaa aagaggctct tctctctct cccgcgacgg caaatgttct
 481 gaaaaagact ctgcatggga atggcctgcc ttacgatgac agaaatggag ggaacatcca
 541 cctttctat atatacagaat ggtgatatt ctggaaatgc caattctatg aagcaaatag
 601 atccagttct tcaggtgtat cttaccatt ccctgggaa atctgaggca gattatctga
 661 ctttccatc tggggagtat gttcagaag aaatctgtat tgctgcttct aaagcttgtg
 721 gtatcacacc tgttatcat aatatgtttg cttaatatg tgaaacagaa aggatctggt
 781 atccaccaa ccatgtctc catatagatg agtcaaccag gcataatgta ctctacagaa
 841 taagatttta ctttctcgt tggattgca gtggcagcaa cagagcctat cggcatggaa
 901 tatctcagg tgctgaagct cctctcttg atgactttgt catgtcttac ctctttgctc
 961 agtggcggca tgattttgtg cacggatgga taaaagtacc tgtgactcat gaaacacagg
 1021 aagaatgtct tgggatggca gtgttagata tgatgagaat agccaaagaa aacgatcaaa
 1081 cccactggc catctataac tctatcagct acaagacatt cttacaaaaa tgtattcgag
 1141 caaagatcca agactatcat atttgacaa ggaagcgaat aaggtaga tttcgcat
 1201 ttattcagca attcagcaa tgcaaagcca ctgccagaaa ctgaaactt aagtatctta
 1261 taaatctgga aactctgcag tctgccttct acacagagaa atttgaagta aaagaacctg
 1321 gaagtgggcc ttcaggtgag gagattttg caaccattat aataactgga aacgggtggaa
 1381 ttcagtggc aagagggaaa cataaagaaa gtgagacact gacagaacag gatttacagt
 1441 tatattgcga ttttctaatt attattgatg tcagtattaa gcaagcaaac caagagggtt

1501 caaatgaaag ccgagttgta actatccata agcaagatgg taaaaatctg gaaattgaac
 1561 ttgctcatt aagggaagct ttgtcttcg tgcattaat tgatggatat tatagattaa
 1621 ctgcagatgc acatcattac ctctgtaaag aagtagcacc tccagccgtg ctgaaaata
 5 1681 tacaagcaa ctgtcatggc ccaatttcga tggatttgc cattagtaa ctgaagaaag
 1741 caggaatca gactggactg tatgtacttc gatgcagtc taaggacttt aataaatatt
 1801 tttgacttt tgctgtcgag cgagaaaatg tcattgaata taaacactgt ttgattacaa
 1861 aaaatgagaa tgaagagtac aacctcagt ggacaaagaa gaacttcagc agtcttaaag
 10 1921 atcttttgaa ttgtaccag atggaaactg ttcgctcaga caatataatt ttccagtta
 1981 ctaaatgctg tccccaaag ccaaagata aatcaaact tctagtcttc agaacgaatg
 2041 gtgtttctga tgtaccaacc tcaccaacat tacagaggcc tactcatatg aaccaaatgg
 2101 gtttcacaa aatcagaaat gaagatttga tatttaatga aagccttggc caaggcactt
 15 2161 ttacaaagat tttaaaggc gtacgaagag aagtaggaga ctacggtcaa ctgcatgaaa
 2221 cagaagtct tttaaaagt ctggataaag cacacagaaa ctattcagag tcttctttg
 2281 aagcagcaag tatgatgagc aagcttctc acaagcattt ggttttaa attgagat
 2341 gtgtctgtgg agacgagaat attctggtc aggagttgt aaaatttga tctactagata
 20 2401 catatctgaa aaagaataaa aattgtataa atatattatg gaaacttgaa gtgctaaac
 2461 agtggcatg ggccatgcat ttctagaag aaaacaccct tattcatggg aatgtatgtg
 2521 caaaaaatat tctgcttacc agagaagaag acaggaagac aggaaatcct ccttcatca
 2581 aacttagtga tctggcatt agtattacag tttgccaaa ggacattct caggagagaa
 25 2641 taccatgggt accacctgaa tgcattgaaa atcctaaaaa tttaaattg gcaacagaca
 2701 aatggagttt tggtagcact ttgtgggaaa tctgcagtgg aggagataaa cctctaagt
 2761 ctctggattc tcaaagaaag ctacaattt atgaagatag gcatcagctt cctgcaccaa
 2821 agtgggcaga attagcaaac cttataaata attgtatgga ttatgaacca gatttcaggc
 30 2881 cttcttcag agccatcata cgagatctta acagtttgt tactccagat tatgaactat
 2941 taacagaaaa tgacatgta ccaaatatga ggataggtgc cctggggtt tctggtgcct
 3001 ttgaagaccg ggatcctaca cagtttgaag agagacattt gaaatttcta cagcaactg
 3061 gcaagggtaa tttgggagt gtggagatgt gccggtatga cctctacag gacaactg
 35 3121 gggaggtggt cgctgtaaaa aagcttcagc atagtactga agagcaccta agagacttg
 3181 aaagggaat tgaatcctg aaatccctac agcatgaca cattgtaaag tacaaggag
 3241 tgtgtacag tgctggtcgg cgtaattctaa aattaattat ggaatatta ccatatggaa
 3301 gtttacgaga ctatctcaa aaacataaag aacggataga tcacataaaa ctctgcagt
 3361 acacatctca gatatgcaag ggtatggagt atcttggtac aaaaaggat atccacagg
 3421 atctggcaac gagaaatata ttggtggaga acgagaacag agttaaatt ggagatttg
 3481 ggtaaccaa agtcttgcca caagacaaag aatactataa agtaaaagaa cctggtgaaa
 3541 gtcccatatt ctggtatgct ccagaatcac tgacagagag caagtttct gtggcctcag
 3601 atgttggag cttggagtg gtctgtatg aactttcac atacattgag aagagtaaaa
 3661 gtccaccagc ggaatttatg cgtatgattg gcaatgaca acaaggacag atgatcgtg
 3721 tccatttgat agaactttg aagaataatg gaagattacc aagaccagat ggatgccag
 3781 atgagatcta tatgatcatg acagaatgct ggaacaataa tgtaaatcaa cgccctct
 3841 ttagggatct agctctcga gtggatcaaa taagggataa catggctgga tgaagaaat
 3901 gaccttcatt ctgagaccaa agtagattta cagaacaaag ttttatatt cacattgctg
 3961 tggactatta ttacatatat cattattata taaatcatga tgctagccag caaagatgtg
 4021 aaaatatctg ctcaaaact tcaaagtta gtaagtttt cttcatgagg ccaccagtaa
 55 4081 aagacattaa tgagaattcc ttagcaagga tttgtaaga agtttctaa acattgtcag

4141 ttaacatcac tcttgtctgg caaaagaaaa aaaatagact tttcaactc agcttttga
4201 gacctgaaaa aattattatg taaattttgc aatgttaaag atgcacagaa tatgtatgta
5 4261 tagtttttac cacagtggat gtataatacc ttggcatctt gtgtgatgtt ttacacacat
4321 gagggctggg gttcattaat actgttttct aatttttcca tagttaatct ataattaatt
4381 acttcactat acaaacaaat taagatgttc agataattga ataagtacct ttgtgtcctt
4441 gttcatttat atcgctggcc agcattataa gcaggtgtat acttttagct ttagttcca
10 4501 tgtactgtaa atattttca cataaagga acaaatgtct agttttattt gtataggaaa
4561 ttccctgac cctaaataat acattttgaa atgaaacaag cttacaaaga tataatctat
4621 ttattatgg ttccctgt atctatttgc ggtgaatgtg tttttaaat ggaactatct
4681 ccaaatttt ctaagactac tatgaacagt tttctttaa aatttgaga ttaagaatgc
15 4741 caggaatatt gtcaccttt gagctgctga ctgccaataa cattcttcga tctctgggat
4801 ttatgctcat gaactaaatt taagcttaag ccataaaata gattagattg tttttaaaa
4861 atggatagct cattaagaag tgcagcaggt taagaatttt ttctaaaga ctgtatattt
4921 gaggggttc agaattttgc attgcagtca tagaagagat ttatttcctt tttagagggg
20 4981 aaatgaggta aataagtaaa aaagtatgct tgtaatttt attcaagaat gccagtagaa
5041 aattcataac gtgtatcttt aagaaaaatg agcatacatc ttaaacttt tcaattaagt
5101 ataaggggtt gtgcgttgtt gtcatttgtt atagtgtac tccactttag acaccatagc
5161 taaaataaaa tatggtgggt tttgtgtgtg tgtgtgtgtg tgtgtgtgtg tgtgtgtgtg
25 5221 tgttatttat aaaaactta aaatacttgc tgttttgatt aaaaagaaaa tagtttctta
5281 cttta

Human JAK2 mRNA Variant 2 (SEQ ID NO: 10)

[0112]

1 attcggggag actgcaggcc aaccgggagg ctgagttcga agctagcagg gcggcgaagc
 61 cagtgtcgcc cgcggcgttg agaagacggg gtggccccgg agagggtgga gacaactgtg
 121 acggggcttc cggctgcccg aagtgggagt ggtgtggggc tgcaggaagg agagaggaag
 181 aggagcagaa gggggcagca gcggacgccg ctaacggcct ccctcggcgc tgacaggctg
 241 ggccggcgcc cggctcgctt ggggtgtcgc gtcgccactt cggcttctcg gccggtcggg
 301 cccctcggcc cgggcttgcg gcgcgcgctg gggctgaggg ctgctgcggc gcagggagag
 361 gcctggtcct cgctgccgag ggatgtgagt gggagctgag ccacactgg agggcccccg
 421 agggcccagc ctggaggtcg ttcagagccg tgcccgtccc ggggcttcgc agacctgac
 481 ccgccgggtt tcagaagcag gcaacaggaa caagatgtga actgtttctc ttctgcagaa
 541 aaagaggctc ttctctcc tcccgcgac gcaaatgtt tgaaaaagac tctgcatggg
 601 aatggcctgc cttacgatga cagaaatgga gggaacatcc acctctcta tatatcagaa
 661 tggatgatt tctggaaatg ccaattctat gaagcaaata gatccagttc ttcaggtgta
 721 tctttaccat tcccttgga aatctgaggc agattatctg accttccat ctggggagta
 781 tgttgagaa gaaatctgta ttgctgctc taaagcttgt ggtatcacac ctgtgtatca
 841 taatatgtt gctttaatga gtgaaacaga aaggatctgg tatccacca accatgtctt
 901 ccatatagat gagtcaacca ggcataatgt actctacaga ataagattt actttcctcg
 961 ttgtattgc agtggcagca acagagccta tcggcatgga atatctcgag gtgctgaagc
 1021 tctcttctt gatgactttg tcatgtctta cctctttgct cagtggcggc atgattttgt
 1081 gcacggatgg ataaaagtac ctgtgactca tgaaacacag gaagaatgtc ttgggatggc
 1141 agtgtagat atgatgagaa tagccaaaga aaacgatcaa accccactgg ccatctataa
 1201 ctctatcagc tacaagacat tcttaccaaa atgtattcga gcaaagatcc aagactatca
 1261 tattttgaca aggaagcgaa taaggtagag atttcgcaga ttattcagc aattcagcca

1321 atgcaaagcc actgccagaa acttgaaact taagtatctt ataaatctgg aaactctgca
 1381 gtctgccttc tacacagaga aatttgaagt aaaagaacct ggaagtgggc cttcaggtga
 1441 ggagattttt gcaaccatta taataactgg aaacgggtgga attcagtggt caagagggaa
 5 1501 acataaagaa agtgagacac tgacagaaca ggatttacag ttatattgcg attttctaa
 1561 tattattgat gtcagtatta agcaagcaaa ccaagagggt tcaaatgaaa gccgagttgt
 1621 aactatccat aagcaagatg gtaaaaatct ggaaattgaa ctagctcat taagggaagc
 1681 tttgtcttc gtgtcattaa ttgatggata ttatagatta actgcagatg cacatcatta
 10 1741 cctctgtaaa gaagtagcac ctccagccgt gcttgaaaat atacaaagca actgtcatgg
 1801 cccaatttcg atggatttg ccattagtaa actgaagaaa gcaggtaatc agactggact
 1861 gtatgtactt cgatgcagtc ctaaggactt taataaatat ttttgactt ttgctgtcga
 1921 gcgagaaaa gtcatgaaat ataaacactg ttgattaca aaaaatgaga atgaagagta
 15 1981 caacctcagt gggacaaaaga agaacttcag cagtcttaa gatctttga attgttacca
 2041 gatggaaact gttcgctcag acaatataat ttccagttt actaatgct gtccccaaa
 2101 gccaaaagat aaatcaaacc ttctagtctt cagaacgaat ggtgttctg atgtaccaac
 2161 ctaccaaca ttacagaggc ctactcatat gaaccaaag gtgttcaca aaatcagaaa
 20 2221 tgaagatttg atatttaag aaagccttgg ccaaggcact ttacaaaga ttttaaagg
 2281 cgtacgaaga gaagtaggag actacggta actgcatgaa acagaagttc tttaaaagt
 2341 tctggataaa gcacacagaa actattcaga gtcttctt gaagcagcaa gtatgatgag
 2401 caagcttct cacaagcatt tggtttaaa ttatggagta tgtgtctgt gagacgagaa
 25 2461 tattctggtt caggagttg taaaatttgg atcactagat acatatctga aaaagaataa
 2521 aaattgtata aatatattat ggaaacttga agttgctaaa cagttggcat gggccatgca
 2581 tttctagaa gaaaacaccc ttattcatgg gaatgtatgt gccaaaaata ttctgcttat
 2641 cagagaagaa gacaggaaga caggaaatcc tctttcatc aaacttagtg atcctggcat
 30 2701 tagtattaca gttttgcaa aggacattct tcaggagaga ataccatggg taccaccta
 2761 atgcattgaa aatcctaaaa atttaattt ggcaacagac aaatggagtt ttggtaccac
 2821 tttgtgggaa atctgcagtg gaggagataa acctctaagt gctctggatt ctcaaagaaa
 35 2881 gctacaattt tatgaagata ggcatcagct tctgcacca aagtgggcag aattagcaaa
 2941 ccttataaat aattgtatgg attatgaacc agatttcagg ccttcttca gagccatcat
 3001 acgagatctt aacagtttgt ttactccaga ttatgaacta ttaacagaaa atgacatgtt
 3061 accaaatatg aggataggtg ccctgggggt ttctggtgcc ttgaagacc gggatcctac
 40 3121 acagtttgaa gagagacatt tgaatttct acagcaactt ggcaagggtg attttgggag
 3181 tgtggagatg tgccggtatg accctctaca ggacaacact ggggaggtgg tcgctgtaaa
 3241 aaagcttcag catagtactg aagagcacct aagagactt gaaagggaaa ttgaaatct
 3301 gaaatcccta cagcatgaca acattgtaaa gtacaaggga gtgtgctaca gtgctggtcg
 45 3361 gcgtaatcta aaattaatta tggaatattt accatatgga agtttacgag actatctca
 3421 aaaacataaa gaacggatag atcacataaa acttctgcag tacacatctc agatatgcaa
 3481 gggatatggag tatcttggtg caaaaaggta tatccacagg gatctggcaa cgagaaatat
 3541 attggtggag aacgagaaca gagttaaata ttgagattt gggtaacca aagtcttggc
 50 3601 acaagacaaa gaatactata aagtaaaaga acctggtgaa agtcccatat tctggtatgc
 3661 tccagaatca ctgacagaga gcaagtttct tgggctca gatgtttgga gctttggagt
 3721 ggttctgtat gaactttca catacattga gaagagtaaa agtccaccag cggaatttat
 3781 gcgtatgatt ggcaatgaca aacaaggaca gatgatcgtg ttccatttga tagaacttt
 55 3841 gaagaataat ggaagattac caagaccaga ttgatgccc gatgagatct atatgatcat
 3901 gacagaatgc tggaacaata atgtaaatca acgcccctcc tttagggatc tagctctcg

3961 agtggatcaa ataagggata acatggctgg atgaaagaaa tgaccttcat tctgagacca
 4021 aagtagattt acagaacaaa gttttatatt tcacattgct gtggactatt attacatata
 5 4081 tcattattat ataaatcatg atgctagcca gcaaagatgt gaaaatatct gctcaaaact
 4141 ttcaaagttt agtaagtttt tcttcatgag gccaccagta aaagacatta atgagaattc
 4201 cttagcaagg attttgtaag aagtttctta aacattgtca gttaacatca ctctgtctg
 4261 gcaaaagaaa aaaaatagac ttttcaact cagcttttg agacctgaaa aaattattat
 10 4321 gtaaatttg caatgttaaa gatgcacaga atatgtatgt atagtttta ccacagtgga
 4381 tgtataatac ctggcatct tgtgtatgt ttacacaca tgagggtgg tgttcattaa
 4441 tactgtttt taattttcc atagttaatc tataattaat tacttcta tacaacaaa
 4501 ttaagatgtt cagataattg aataagtacc tttgtgtcct tgttcattta tatcgctggc
 15 4561 cagcattata agcaggtgta tacttttagc ttgtagtcc atgtactgta aatattttc
 4621 acataaaggg acaaatgtc tagttttatt tgtataggaa attccctga ccctaaataa
 4681 tacatttga aatgaaacaa gcttacaaag atataatcta tttattatg gttcccttg
 4741 tatctatttg tggatgaatgt gtttttaaa tggaactatc tccaaattt tctaagacta
 20 4801 ctatgaacag tttctttta aaatttgag attaagaatg ccaggaatat tgtcatcctt
 4861 tgagctgctg actgccaata acattctcg atctctggga tttatgctca tgaactaaat
 4921 ttaagcttaa gccataaaat agattagatt gtttttaaa aatggatagc tcattaagaa
 25 4981 gtgcagcagg ttaagaattt tttcctaaag actgtatatt tgagggggtt cagaatttg
 5041 cattgcagtc atagaagaga ttatttcct ttttagaggg gaaatgaggt aaataagtaa
 5101 aaaagtatgc ttgttaattt tattcaagaa tgccagtaga aaattcataa cgtgtatctt
 5161 taagaaaaat gagcatacat cttaaactt ttcaattaag tataaggggt tgttcgttgt
 30 5221 tgtcatttgt tatagtgcta ctccactta gacaccatag ctaaaataaa atatggtggg
 5281 tttgtgtgt gtgtgtgtgt gtgtgtgtgt gtgtgtgtgt gtgttattta taaaaaactt
 5341 aaaatacttg ctgtttgat taaaagaaa atagtttctt acttta

35 **Human JAK2 mRNA Variant 3 (SEQ ID NO: 11)**

[0113]

40

45

50

55

1 attcggggag actgcaggcc aaccgggagg ctgagttcga agctagcagg gcggcgaagc
61 cagtgtcgcc cgcggcgttg agaagacggc aaatgttctg aaaaagactc tgcattggaa
5 121 tggcctgcct tacgatgaca gaaatggagg gaacatccac ctcttctata taccagaatg
181 gtgatatttc tggaaatgcc aattctatga agcaaataga tccagttctt caggtgtatc
241 ttaccattc cttgggaaa tctgaggcag attatctgac cttccatct ggggagtatg
301 ttgcagaaga aatctgtatt gctgcttcta aagcttggg taccacacct gtgtatcata
10 361 atatgtttgc ttaattgagt gaaacagaaa ggatctggta tccaccaac catgtcttcc
421 atatagatga gtcaaccagg cataatgtac tctacagaat aagattttac ttctctggt
481 ggtattgcag tggcagcaac agagcctatc ggcatggaat atctcgaggt gctgaagctc
541 ctcttctga tgactttgtc atgtcttacc tcttgctca gtggcggcat gattttgtgc
15 601 acggatggat aaaagtacct gtgactcatg aaacacagga agaattgtctt gggatggcag
661 tggtagatat gatgagaata gccaaagaaa acgatcaaac cccactggcc atctataact
721 ctatcagcta caagacattc ttacaaaat gtattcgagc aaagatccaa gactatcata
781 tttgacaag gaagcgaata aggtacagat ttgcagatt tattcagcaa ttacccaat
20 841 gcaaagccac tgccagaaac ttgaaactta agtatcttat aaatctggaa actctgcagt
901 ctgccttcta cacagagaaa ttgaagtaa aagaacctgg aagtggctct tcaggtgagg
961 agattttgc aaccattata ataactggaa acggtggaat tcagtggta agagggaac
25 1021 ataaagaaag tgagacactg acagaacagg atttacagt atattgcgat ttcttaata

30

35

40

45

50

55

1081 ttattgatgt cagtattaag caagcaaacc aagaggggttc aaatgaaagc cgagttgtaa
 1141 ctatccataa gcaagatggg aaaaatctgg aaattgaact tagctcatta agggaagctt
 1201 tgtctttcgt gtcattaatt gatggatatt atagattaac tgcagatgca catcattacc
 5 1261 tctgtaaaga agtagcacct ccagccgtgc ttgaaaatat acaaagcaac tgtcatggcc
 1321 caatttcgat ggattttgcc attagtaaac tgaagaaagc aggtaatcag actggactgt
 1381 atgtacttcg atgcagtctc aaggacttta ataaatattt ttgactttt gctgtcgagc
 1441 gagaaaatgt cattgaatat aaacactgtt tgattacaaa aaatgagaat gaagagtaca
 10 1501 acctcagtgg gacaaagaag aacttcagca gtcttaaaga tcttttgaat tgttaccaga
 1561 tggaaactgt tcgtcagac aatataattt tccagttac taaatgctgt cccccaagc
 1621 caaaagataa atcaaacctt ctagtcttca gaacgaatgg tgtttctgat gtaccaacct
 1681 caccaacatt acagaggcct actcatatga accaaatggg gttcacaaa atcagaaatg
 15 1741 aagatttgat atttaatgaa agccttggcc aaggcacttt tacaaagatt ttaaaggcg
 1801 tacgaagaga agtaggagac tacggtcaac tgcagaaac agaagttctt taaaagtgc
 1861 tggataaagc acacagaaac tattcagagt ctttcttga agcagcaagt atgatgagca
 1921 agctttctca caagcatttg gtttaaatt atggagtatg tgtctgtgga gacgagaata
 20 1981 ttctggttca ggagtttga aaatttggat cactagatac atatctgaaa agaataaaa
 2041 attgtataaa tatattatgg aaacttgaag ttgctaaaca gttggcatgg gccatgcatt
 2101 ttctagaaga aaacaccctt attcatggga atgtatgtgc caaaaatatt ctgcttatca
 2161 gagaagaaga caggaagaca ggaaatctc ctttcatcaa acttagtgat cctggcatta
 25 2221 gtattacagt ttgccaag gacattctc aggagagaat accatgggta ccacctgaat
 2281 gcattgaaaa tcctaaaaat ttaatttgg caacagacaa atggagtttt ggtaccatt
 2341 tgtgggaaat ctgcagtgga ggagataaac ctctaagtgc tctggattct caaagaaagc
 2401 tacaatttta tgaagatagg catcagctc ctgcaccaa gtgggcagaa ttagcaaac
 30 2461 ttataaataa ttgtatggat tatgaaccag atttcaggcc ttcttcaga gccatcatac
 2521 gagatcttaa cagtttgtt actccagatt atgaactatt aacagaaaat gacatgtac
 2581 caaatatgag gataggtgcc ctggggtttt ctggtgcctt tgaagaccgg gatcctacac
 35 2641 agtttgaaga gagacatttg aaatttctac agcaactgg caagggtaat ttgggagtg
 2701 tggagatgtg ccggtatgac cctctacagg acaacactgg ggaggtggtc gctgtaaaaa
 2761 agcttcagca tagtactgaa gagcacctaa gagacttga aagggaatt gaaatcctga
 2821 aatccctaca gcatgacaac attgtaaagt acaaggagtg gtgctacagt gctggtcggc
 40 2881 gtaatctaaa attaattatg gaattttac catatggaag ttacgagac tatcttcaa
 2941 aacataaaga acggatagat cacataaac ttctgcagta cacatctcag atatgcaagg
 3001 gtatggagta tcttggtaca aaaaggata tccacaggga tctggcaacg agaaatatat
 3061 tgggtggagaa cgagaacaga gttaaaattg gagattttgg gttaaccaa gtcttgcac
 45 3121 aagacaaaga atactataaa gtaaaagaac ctggtgaaag tcccatattc tggtagctc
 3181 cagaatcact gacagagagc aagttttctg tggcctcaga tgtttggagc ttggagtg
 3241 ttctgtatga acttttcaca tacattgaga agagtaaaag tccaccagcg gaatttatgc
 3301 gtatgattgg caatgacaaa caaggacaga tgatcgtgtt ccatttgata gaactttga
 50 3361 agaataatgg aagattacca agaccagatg gatgccaga tgagatctat atgatcatga
 3421 cagaatgctg gaacaataat gtaaatcaac gccctcctt tagggatcta gctctcgag
 3481 tggatcaaat aagggataac atggctggat gaaagaaatg accttcattc tgagaccaa
 3541 gtagatttac agaacaaagt ttatatttc acattgctgt ggactattat tacatatatc
 55 3601 attattatat aaatcatgat gctagccagc aaagatgtga aaatatctgc tcaaaacttt
 3661 caaagtttag taagttttc tcatgaggc caccagtaaa agacattaat gagaatctc

3721 tagcaaggat tttgtaagaa gtttcttaaa cattgtcagt taacatcact cttgtctggc
 3781 aaaagaaaaa aaatagactt ttcaactca gcttttgag acctgaaaaa attattatgt
 3841 aaattttgca atgttaaaga tgcacagaat atgtatgtat agtttttacc acagtggatg
 3901 tataatacct tggcatcttg tgtgatgttt tacacacatg agggctggtg ttcattaata
 3961 ctgttttcta attttccat agttaatcta taattaatta cttcactata caaacaatt
 4021 aagatgttca gataattgaa taagtacctt tgtgtccttg ttcatttata tcgctggcca
 4081 gcattataag caggtgtata ctttagctt gtagttccat gtactgtaaa tatttttcac
 4141 ataaaggga caaatgtcta gttttatttg tataggaaat ttcctgacc ctaaataata
 4201 cattttgaaa tgaaacaagc ttacaaagat ataacttatt ttattatggt ttccttgta
 4261 tctatttgtg gtgaatgtgt ttttaaatg gaactatctc caaattttc taagactact
 4321 atgaacagtt ttcttttaaa attttgagat taagaatgcc aggaatattg tcatccttg
 4381 agctgctgac tgccaataac attcttcgat ctctgggatt tatgctcatg aactaaattt
 4441 aagcttaagc cataaaatag attagattgt ttttaaaaaa tggatagctc attaagaagt
 4501 gcagcaggtt aagaattttt tcctaaagac tgtatatttg aggggtttca gaattttgca
 4561 ttgcagtcac agaagagatt ttttccttt ttagaggga aatgaggtaa ataagtaaaa
 4621 aagtatgctt gttaatttta ttcaagaatg ccagtagaaa attcataacg tgtatcttta
 4681 agaaaaatga gcatacatct taaatctttt caattaagta taaggggttg ttcgtgttg
 4741 tcatttgta tagtgctact ccactttaga caccatagct aaaataaaat atggtgggtt
 4801 ttgtgtgtgt gtgtgtgtgt gtgtgtgtgt gtgtgtgtgt gttatttata caaaacttaa
 4861 aatacttgct gtttgatta aaaagaaaat agtttcttac tta

Human JAK2 mRNA Variant 4 (SEQ ID NO: 12)

[0114]

1 gggagtgggtg tggggctgca ggaaggagag aggaagagga gcagaagggg gcagcagcgg
 61 acgccgctaa cggcctccct cggcgtgac aggctgggcc ggcgcccggc tcgcttgggt
 121 gttcgcgtcg ccacttcggc ttctggccg gtcgggcccc tcggcccggg cttgcggcgc
 181 gcgtcggggc tgagggtgc tgcggcgcag ggagaggcct ggtcctcgt gccgagggat
 241 gtgagtggga gctgagccca cactggaggg cccccagggg ccagcctgg aggtcgttca
 301 gagccgtgcc cgtcccgggg cttgcagac cttgaccgc cgggtaggag ccgccctgc
 361 gggctcgagg gcgcgtctg gtcggccgat ctgtgtagcc ggcaaagt ttgaaaaaga
 421 ctctcatgg gaatggcctg cctacgatg acagaaatgg agggaaatc cacctctt
 481 atatatcaga atggtgat ttctggaaat gccaattcta tgaagcaat agatccagt
 541 cttcaggtgt atctttacca ttccctggg aaatctgagg cagattatc gaccttcca
 601 tctggggagt atgttcaga agaaatctgt attgctgctt cttaaagctg tggatcaca
 661 cctgtgtatc ataatatgt tgctttaat agtgaaacag aaaggatctg gtatccacc
 721 aaccatgtct tccatataga tgagtcaacc aggcataatg tactctacag aataagatt
 781 tactttctc gttggtattg cagtggcagc aacagagcct atcggcatgg aatatctga
 841 ggtgctgaag ctctcttct tgatgactt gtcagtctt acctcttgc tcagtggcgg
 901 catgatttg tgcacggatg gataaaagta cctgtgactc atgaaacaca ggaagaatgt
 961 ctgggatgg cagtgttaga tatgatgaga atagccaaag aaaacgatca aacccactg
 1021 gccatctata actctatcag ctacaagaca ttcttacc aaatgtattc agcaaagatc
 1081 caagactatc atatttgac aaggaagcga ataaggtaca gatttcgcag attattcag
 1141 caattcagcc aatgcaaagc cactgccaga aacttgaaac ttaagtatc tataaatctg
 1201 gaaactctgc agtctgcctt ctacacagag aaattgaag taaaagaacc tggaagtgt

1261 ccttcaggtg aggagatttt tgcaaccatt ataataactg gaaacggtgg aattcagtg
 1321 tcaagaggga aacataaaga aagtgagaca ctgacagaac aggatttaca gttatattgc
 1381 gattttccta atattattga tgcagtatt aagcaagcaa accaagaggg ttcaaatgaa
 5 1441 agccgagttg taactatcca taagcaagat ggtaaaaaatc tggaaattga acttagctca
 1501 ttaagggag ctttgtcttt cgtgtcatta attgatggat attatagatt aactgcagat
 1561 gcacatcatt acctctgtaa agaagtagca cctccagccg tgcttgaaaa tatacaaaagc
 1621 aactgtcatg gcccatttc gatggatttt gccattagta aactgaagaa agcaggtaat
 10 1681 cagactggac tgtatgtact tcgatgcagt cctaaggact ttaataaata tttttgact
 1741 tttgtgtcg agcgagaaaa tgcattgaa tataaacact gtttgattac aaaaaatgag
 1801 aatgaagagt acaacctcag tgggacaaag aagaacttca gcagtcttaa agatctttg
 1861 aattgttacc agatggaaac tgttcgtca gacaataaa tttccagt tactaaatgc
 15 1921 tgtcccccac agccaaaaga taaatcaaac cttctagtct tcagaacgaa tgggtttct
 1981 gatgtaccaa cctcaccaac attacagagg cctactcata tgaaccaa ggtgtttcac
 2041 aaaatcagaa atgaagattt gatatttaat gaaagccttg gccaaaggcac tttacaaag
 2101 attttaaaag gcgtacgaag agaagtagga gactacggc aactgcatga aacagaagtt
 20 2161 cttttaaag tctggataa agcacacaga aactattcag agtctttct tgaagcagca
 2221 agtatgatga gcaagcttc tcacaagcat ttggtttta attatggagt atgtgtctgt
 2281 ggagacgaga atattctggc tcaggagttt gtaaaatttg gatcactaga tacatatctg
 2341 aaaaagaata aaaattgtat aaatatatta tggaaacttg aagttgctaa acagttggca
 25 2401 tgggccatgc attttctaga agaaaacacc cttattcatg ggaatgtatg tgccaaaaat
 2461 attctgctta tcagagaaga agacaggag acaggaaatc ctcctttcat caaacttagt
 2521 gatcctggca ttagtattac agttttgcca aaggacattc ttcaggagag aataccatgg
 2581 gtaccacctg aatgcattga aaatcctaaa aatttaaatt tggcaacaga caaatggagt
 30 2641 tttgtacca ctttgtggga aatctgcagt ggaggagata aacctctaag tgctctggat
 2701 tctcaaagaa agctacaatt ttatgaagat aggcacagc ttctgcacc aaagtgggca
 2761 gaattagcaa acctataaa taattgtatg gattatgaac cagatttcag gccttcttc
 2821 agagccatca tacgagatct taacagttt tttactccag attatgaact attaacagaa
 35 2881 aatgacatgt taccaaatat gaggataggt gccctggggt tttctggtgc cttgaagac
 2941 cgggaccta cacagtttga agagagacat ttgaaattc tacagcaact tggcaagggt
 3001 aattttggga gtgtggagat gtgccggtat gaccctctac aggacaacac tggggaggtg
 3061 gtcgtgttaa aaaagcttca gcatagtact gaagagcacc taagagactt tgaagggaa
 40 3121 attgaaatcc tgaatccct acagcatgac aacattgtaa agtacaaggg agtgtgctac
 3181 agtgcgtggt ggcgtaatct aaaattaatt atggaatatt taccatatgg aagtttacga
 3241 gactatcttc aaaaacataa agaacggata gatcacataa aacttctgca gtacacatct
 3301 cagatatgca agggatgga gtatcttggc aaaaaaggt atatccacag ggatctggca
 45 3361 acgagaaata tattggtgga gaacgagaac agagttaaaa ttggagattt tgggttaacc
 3421 aaagtcttg cacaagacaa agaatactat aaagtaaaag aacctggtga aagtcacata
 3481 ttctggtatg ctccagaatc actgacagag agcaagttt ctgtggcctc agatgtttgg
 50 3541 agctttggag tggttctgta tgaactttc acatacattg agaagagtaa aagtcacca
 3601 gcggaattta tgcgtatgat tggcaatgac aaacaaggac agatgatcgt gttccattg
 3661 atagaacttt tgaagaataa tgggaagatta ccaagaccag atggatgcc agatgagatc
 3721 tatatgatca tgacagaatg ctggaacaat aatgtaaate aacgcccctc ctttagggat
 55 3781 ctagctcttc gaggatgca aataaggat aacatggctg gatgaaagaa atgaccttca
 3841 ttctgagacc aaagtagatt tacagaacaa agttttatat ttcacattgc tgtggactat

3901 tattacatat atcattatta tataaatcat gatgctagcc agcaaagatg tgaaaatc
 3961 tgctcaaaac ttcaaaagt tagtaagtt ttctcatga ggccaccagt aaaagacatt
 5 4021 aatgagaatt ccttagcaag gattttgtaa gaagtttctt aaacattgtc agttaacatc
 4081 actcttgtct ggcaaaagaa aaaaaataga cttttcaac tcagctttt gagacctgaa
 4141 aaaattatta tgtaaatttt gcaatgttaa agatgcacag aatatgtatg tatagtttt
 4201 accacagtgg atgtataata cctggcatc ttgtgtgatg tttacacac atgagggtg
 10 4261 gtgttcatta atactgttt ctaattttc catagttaat ctataattaa ttacttact
 4321 atacaacaa attaagatgt tcagataatt gaataagtac ctttgtgcc ttgttcatt
 4381 atatcgctgg ccagcattat aagcaggtgt atacttttag ctgtagtgc catgtactgt
 4441 aaatatttt cacataaagg gaacaaatgt ctagttttat ttgtatagga aatttcctg
 15 4501 accctaaata atacattttg aaatgaaaca agcttacaaa gatataatct attttattat
 4561 ggtttccct gtatctatt gtggtgaatg tgtttttaa atggaactat ctccaaatt
 4621 ttctaagact actatgaaca gttttcttt aaaattttga gattaagaat gccaggaata
 4681 ttgtcatcct ttgagctgct gactgccaat aacattcttc gatctctggg atttatgctc
 20 4741 atgaactaaa ttaagctta agccataaaa tagattagat tgtttttaa aaatggatag
 4801 ctcatgaaga agtgcagcag gttaagaatt tttcctaaa gactgtatat ttgaggggtt
 4861 tcagaatttt gcattgcagt catagaagag atttatttcc ttttagagg ggaaatgagg
 4921 taaataagta aaaaagtatg ctgttaatt ttattcaaga atgccagtag aaaattcata
 25 4981 acgtgtatct ttaagaaaaa tgagcataca tcttaaatct ttcaattaa gtataagggg
 5041 ttgtcgttg ttgtcattg ttatagtgt actccactt agacaccata gctaaaataa
 5101 aatatgggtg gttttgtgtg tgtgtgtgtg tgtgtgtgtg tgtgtgtgtg tgtgttatt
 30 5161 atacaaaact taaaatactt gctgtttga ttaaaaagaa aatagtttct tacttta

Human JAK3 mRNA (SEQ ID NO: 13)

[0115]

35

40

45

50

55

1 cacacaggaa ggagccgagt gggactttcc tctcgtgcc tcccggctct gcccgccctt
 61 cgaaagtcca gggtcctgc ccgctaggca agttgcactc atggcacctc caagtgaaga
 121 gacgcccctg atccctcagc gttcatgcag cctcttgcc acggaggctg gtgccctgca
 181 tgtgctgctg cccgctcggg gccccgggccc ccccccagcgc ctatctttct cctttgggga
 241 ccacttggct gaggacctgt gcgtgcaggc tgccaaggcc agcggcatcc tgcctgtgta
 301 ccactccctc ttgctctgg ccacggagga cctgtctgc tggttcccc cgagccacat
 361 cttctccgtg gaggatgcca gcaccaagt cctgctgtac aggatctgct ttacttccc
 421 caattggtt gggctggaga agtgccaccg ctccgggcta cgcaaggatt tggccagtgc
 481 tatecttgac ctgccagtcc tggagcacct cttgcccag caccgcagtg acctggtgag
 541 tgggcgcctc cccgtgggccc tcagtctcaa ggagcagggt gagtgtctca gcctggccgt
 601 gttggacctg gcccggatgg cgcgagagca ggcccagcgg ccgggagagc tgctgaagac
 661 tgtagctac aaggcctgcc taccaccaag cctgcgcgac ctgatccagg gcctgagctt
 721 cgtgacgcgg aggcgtattc ggaggacggt gcgcagagcc ctgcgccgcg tggccgcctg
 781 ccaggcagac cggcactcgc tcatggccaa gtacatcatg gacctggagc ggctggatcc
 841 agccggggccc gccgagacct tcacgtggg cctccctggg gcccttggtg gccacgacgg
 901 gctggggctg ctccgcgtgg ctggtgacgg cggcatcgcc tggaccagg gagaacagga
 961 ggtcctccag cccttctgcg actttccaga aatcgtagac attagcatca agcaggcccc
 1021 gcgcgttggc ccggccggag agcaccgct ggtcactgtt accaggacag acaaccagat
 1081 ttagaggcc gagttcccag ggctgcccga ggctctgtcg ttcgtggcgc tcgtggacgg

1141 ctacttccgg ctgaccacgg actcccagca cttcttctgc aaggagggtgg caccgccgag
 1201 gctgctggag gaagtggccg agcagtgcc aagccccatc actctggact ttgccatcaa
 1261 caagctcaag actgggggct cacgtcctgg ctctatgtt ctccgccga gccccagga
 5 1321 ctttgacagc ttctectca ctgtctgtgt ccagaacccc ctgggtcctg attataaggg
 1381 ctgctcctc cggegcagcc ccacaggaac ctctctctg gttggcctca gccgacccca
 1441 cagcagtctt cgagagctcc tggcaacctg ctgggatggg gggctgcacg tagatggggg
 1501 ggagtgacc ctacttctt gctgtatccc cagacccaaa gaaaagtcca acctgatcgt
 10 1561 ggtccagaga ggtcacagcc caccacatc atccttggtt cagccccaat cccaatacca
 1621 gctgagtcag atgacattc acaagatccc tgctgacagc ctggagtggc atgagaacct
 1681 gggccatggg tccttcacca agattaccg gggctgtcgc catgaggtgg tggatgggga
 1741 ggcccgaaag acagaggtgc tctgaagggt catggatgcc aagcacaaga actgcatgga
 15 1801 gtcattcctg gaagcagcga gcttgatgag ccaagtgtcg taccggcctc tctgtctgct
 1861 ccacggcgtg tgcagggctg gagacagcac catggtgcag gaattgtac acctgggggc
 1921 catagacatg tatctgcgaa aacgtggcca cctgggtgcca gccagctgga agctgcaggt
 1981 ggtcaaacag ctggcctacg cctcaacta tctggaggac aaaggcctgc ccatggcaa
 20 2041 tgtctctgcc cggaaggtgc tctgggtcgc ggagggggct gatgggagcc cgcccttcat
 2101 caagctgagt gacctgggg tgagccccgc tgtgttaagc ctggagatgc tcaccgacag
 2161 gateccctgg gtggcccccg agtgtctcgc ggaggcgcag acacttagct tggaaactga
 2221 caagtggggc ttggcgcca cgtctggga agtgtttagt ggcgtacca tgcccatcag
 25 2281 tgccctggat cctgctaaga aactccaatt ttataggac cggcagcagc tgccggcccc
 2341 caagtggaca gagctggccc tctgattca acagtgcag gcctatgagc cggtcagag
 2401 gccctcctc cgagccgtca tctgtacct caatagcctc atctctcag actatgagct
 2461 cctctcagac ccacacctg gtgccctggc acctcgtgat gggctgtgga atgtgacca
 30 2521 gctctatgcc tgccaagacc ccacgatctt cgaggagaga cacctcaagt acatctcaca
 2581 gctgggcaag ggcaacttg gcagcgtgga gctgtgccgc tatgaccgc taggcgacaa
 2641 tacaggtgcc ctggtggccg tgaacagct gcagcacagc gggccagacc agcagaggga
 35 2701 cttcagcgg gagattcaga tctcaaagc actgcacagt gatttcattg tcaagtatc
 2761 tgggtgcagc tatggcccg gccgccagag cctgcggctg gtcattggagt acctgcccag
 2821 cggtgcttg cgcgacttc tcagcggca ccgcgcgcgc ctgatgcca gccgcctct
 2881 tctctatcc tcgagatct gcaagggcct ggagtacct ggctccgcc gctgcgtgca
 30 2941 ccgcgacctg gccgccgaa acatctcgt ggagagcag gcacacgtca agatcgtga
 3001 cttcggccta gctaagctgc tgccgctga caaagactac tacgtggtcc gcgagccagg
 3061 ccagagcccc atttctggt atgccccga atccctctc gacaacatct tctctgcca
 3121 gtcagacgtc tggagcttc gggctgtcct gtacgagctc ttacctact gcgacaaaag
 45 3181 ctgcagcccc tggccgagt tctgaggat gatgggatgt gagcgggatg tccccgcct
 3241 ctgccgcctc ttggaactgc tggaggagg ccagaggctg ccggcgctc ctgctgccc
 3301 tgctgaggtt cagagctca tgaagctgt ctgggcccct agcccacagg accggcctc
 3361 attcagcgc ctgggcccc agctggacat gctgtggagc ggaagccggg ggtgtgagac
 50 3421 tcatgcctc actgctacc cagagggcaa acaccactc ctgtccttt catagctct
 3481 gcccgcagac ctctggatta ggtctctgt gactggctgt gtgacctag gcccgagct
 3541 gccctctct gggcctcaga ggccttatga gggctctc cttcaggaac accccatga
 3601 cattgcattt gggggggctc ccgtggcctg tagaatagcc tgtggccttt gcaatttgt
 55 3661 aaggttaag acagatgggc atatgtgtca gtgggctct ctgagctctg gcccagaag
 3721 gcaaggaacc aaatttaaga ctctgcctc tcccaacc ctaagccct ggccccctga

3781 gtttcctttt ctgtctctct cttttattt tttttattt tttttattt tttgagacag
 3841 agcctcgtctc tgttaccag ggtggagtgc agtgggtgca tctcggctca gtgcaacctc
 3901 tgcttcccag gttcaagcga ttctcctgcc tcagcctccc gagtagctgg gattacaggt
 3961 gtgcaccacc acacccggct aattttttt attttaata gagatgaggt ttcacatga
 4021 tggccaggct gatctcgaa ccttaacctc aagtgtcct cccacctcag cctcccaaag
 4081 tgttgaata ataggcatga gccactgcac ccaggctttt tttttttaa atttattatt
 4141 attatttta agagacagga tcttgctacg ttgccaggc tggcttgaa ctcctgggct
 4201 acagtgtcc tctgcctta tctcctaaa tagctgggac tacagcacct agtttgagt
 4261 ttctgtctt atttcaatg gggacattca ttagctttt tttttttt ttttttgag
 4321 acggagtctc gctctgtcgc ccaggctgga gtacagtggc gcaatctagg ctcactgcaa
 4381 gctccgcctc ctgggttcac accattctct cgcctcagcc tccaagtag ctgggactac
 4441 aggcgccccg caccacaccc ggctaattt ttgtatttt agtagagacg gggtttcacc
 4501 ttgttagcca ggatggttc catctcctga cctcgtgatc tgcccgtctc ggcctccaa
 4561 agtgctggga ttacaggcat gagccactgc gcccgccct catgtagctt taaatgtatg
 4621 atctgacttc tgctccccga tctctgttc tctggaggaa gccaaggaca agagcagttg
 4681 ctgtggctgg gactctgct ttaggggag cccgtgtatc tcttgggat cctgaaaggg
 4741 ggcaggaaa gctggggctc cagtcaccc taatggtatc tgagtgtcct agggcttcag
 4801 tttccacc tgccaatgg gacccttct gtctcacc tacaaggggc acaaaggat
 4861 gacaccaaac ctggcaggaa ctttcacgc aatcaaggga aggaaaggca ttctggcag
 4921 agggaaacag atgccaagcg tgagaaggct cagagtaagg aggttaagag cccaagtatt
 4981 ggagcctaca gtttgcccc tccatgcag tgtgacagtg ggcaagtcc ttccctctc
 5041 tgggtctcag ttctgtccc tgcaaatgg tcagagctta ccccttggt gtgcagggtc
 5101 aactttctga ctggtgagag ggattctcat gcaggttaag cttctgtgc tctcctcac
 5161 ctgcaaagct tttctgccac tttgcctcc ttggaaaact cttatccatc tctcaaaact
 5221 ccagctacca catccttga gcctccctc atatacccc actactactg tagcctgtc
 5281 ctccctcca gcccactct ggccctgggg ctgggggaagt gtctgtgtcc agctgtctcc
 5341 cctgacctca ggggtcctg ggggctgggc tgaggcctca gtacagaggg ggctctggaa
 5401 atgtttgtg actgaataaa ggaattcagt ggaaaaaaaa aaaaaaaaaa

Human JAK3 mRNA (SEQ ID NO: 14)

[0116]

EP 3 554 485 B9

1 ccctetgacc aggactgagg ggcttttct ctctgtgcc caggcaagt gcactcatta
61 tgggaattccg gcggcccgt aggcaagtg cactcatggc acctccaagt gaagagacgc
121 ccctgatecc tcagcgttca tgcagcctct tgtccacgga ggctggtgcc ctgcatgtgc
5 181 tgctgcccgc tcgggccccg gggcccccc agcgcctatc ttctcctt ggggaccact
241 tggctgagga cctgtgcgtg caggctgcca aggccagcgg catcctgcct gtgtaccact
301 ccctctttgc tctggccacg gaggacctgt cctgctgggt cccccgagc cacatcttct
10 361 ccgtggagga tgccagcacc caagtctgc tgtacaggat tcgctttac ttcccaatt
421 ggtttgggct ggagaagtgc caccgcttcg ggctacgcaa ggatttgcc agtgctatec
481 ttgacctgc agtctggag cactctttg ccagcaccg cagtgcctg gtgagtgggc
541 gcctccccgt gggcctcagt ctcaaggagc agggtgagtg ttcagcctg gccgtgttg
15 601 acctggcccg gatggcgca gagcaggccc agcggccggg agagctgctg aagactgtca
661 gctacaaggc ctgcctacc ccaagctgc gcgacctg ccagggcctg agcttcgtga
721 cgcggagggc tctcggagg acggtgcga gagccctgcc gcgcgtggcc gcctgccagg
20 781 cagaccggca ctgcctcatg gccaaagta tcatggacct ggagcggctg gatccagccg

20

25

30

35

40

45

50

55

841 gggccgccga gaccttcac gtgggctcc ctggggccct tggggccac gacgggctgg
 901 ggctgctccg cgtggctggt gacggcgga tcgctggac ccaggagaa caggaggtcc
 961 tccagccctt ctgcacttt ccagaaatcg tagacattag catcaagcag gccccgcgcg
 5 1021 ttggcccggc cggagagcac cgcctggtca ctgtaccag gacagacaac cagattttag
 1081 aggccgagtt cccagggtg cccgaggctc tgtcgttcgt ggcgctcgtg gacggctact
 1141 tccggctgac cacggactcc cagcacttct tctgcaagga ggtggcaccg ccgaggctgc
 1201 tggaggaagt ggccgagcag tgccacggcc ccactactct ggactttgcc atcaacaagc
 10 1261 tcaagactgg gggctcacgt cctggctcct atgttctccg ccgcagcccc caggactttg
 1321 acagcttctt cctactgtc tgtgtccaga accccttgg tctgattat aagggtgccc
 1381 tcatccggcg cagccccaca ggaaccttcc ttctggttgg cctcagccga cccacagca
 1441 gtcttcgaga gctcctggca acctgctggg atggggggct gcacgtagat ggggtggcag
 15 1501 tgacctcac ttctgctgt atccccagac ccaaagaaaa gtccaacctg atcgtggtcc
 1561 agagaggtca cagcccacc acatcactct tggttcagcc ccaatccaa taccagctga
 1621 gtcagatgac attcacaag atccctgctg acagcctgga gtggcatgag aacctgggccc
 1681 atgggtcctt caccaagatt taccggggct gtcgcatga ggtggtggat ggggaggccc
 20 1741 gaaagacaga ggtgctgctg aaggtcatgg atgccaagca caagaactgc atggagtcat
 1801 tcttgaagc agcgagcttg atgagccaag tgtcgtaccg gcactcgtg ctgtccacg
 1861 gcgtgtgcat ggctggagac agcacatgg tgcaggaatt tgtacacctg ggggccatag
 1921 acatgtatct gcgaaaacgt ggccacctgg tgccagccag ctggaagctg caggtggtca
 25 1981 aacagctggc ctacgccctc aactatctgg aggacaaagg cctgccccat ggcaatgtct
 2041 ctgcccggaa ggtgctcctg gctcgggagg gggctgatgg gagcccgccc ttcatcaagc
 2101 tgagtgacct tggggtcagc cccgctgtgt taagcctgga gatgtcacc gacaggatcc
 2161 cctgggtggc ccccgagtgt ctcgggagg cgcagacact tagcttgga gctgacaagt
 30 2221 ggggcttcgg cgcacggctc tgggaagtgt ttagtggcgt caccatgccc atcagtcccc
 2281 tggatcctgc taagaaactc caattttatg aggaccggca gcagctgccg gccccaaagt
 2341 ggacagagct ggccctgctg attcaacagt gcatggccta tgagccggtc cagaggccct
 2401 cttccgagc cgtcattcgt gacctcaata gctcactc ttacagactat gagtctctt
 35 2461 cagacccac acctggtgcc ctggcacctc gtgatgggct gtggaatggt gccagctct
 2521 atgctgcca agacccacg atcttcgagg agagacacct caagtacatc tcacagctgg
 2581 gcaagggcaa ctttggcagc gtggagctgt gccgctatga cccgctagcc cacaatacag
 2641 gtgccctggt ggccgtgaaa cagctgcagc acagcgggcc agaccagcag agggactttc
 40 2701 agcgggagat tcagatctc aaagcactgc acagtgattt cattgtcaag tctcgtggtg
 2761 tcagctatgg cccgggcccgg ccagagctgc ggctggtcat ggagtacctg ccagcggct
 2821 gcttgcgca cttctgcag cggcaccgcg cgcgctcga tgccagccgc ctccttctt
 45 2881 attctcgca gatctgcaag ggcatggagt acctgggctc ccgccgctgc gtgcaccgcg
 2941 acctggccgc ccgaaacatc ctctgggaga gcgaggcaca cgtcaagatc gctgacttcg
 3001 gcctagctaa gctgctgccg cttgacaaag actactacgt ggtccgag ccaggccaga
 3061 gccccatttt ctggtatgcc cccgaatccc tctcggaca catcttctt cgcagtcag
 50 3121 acgtctggag cttcggggtc gtctgtacg agctcttca ctactgcgac aaaagctgca
 3181 gcccctcggc cgagttcctg cgcatgatgg gatgtgagcg ggatgtccc gccctctgcc
 3241 gcctcttga actgctggag gagggccaga ggctgccg gcctctgcc tgcctgctg
 3301 aggttcacga gctcatgaag ctgtgctggg ccctagccc acaggaccgg ccactattca
 55 3361 gcgccctggg ccccgagctg gacatgtgt ggagcggag ccgggggtgt gagactcatg
 3421 cttcactgc taccagag ggcaaacacc actccctgtc ctttcatag ctctgcccg

EP 3 554 485 B9

3481 cagacctctg gattaggtct ctgttgactg gctgtgtgac cttaggcccg gagctgcccc
3541 tctctgggcc tcagaggcct tatgagggtc ctctacttca ggaacacccc catgacattg
5 3601 catttggggg ggctcccgtg gcctgtagaa tagcctgtgg ccttgcaat ttgttaaggt
3661 tcaagacaga tgggcatatg tgcagtggg gctctctgag tcctggccca aagaagcaag
3721 gaaccaaatt taagactctc gcattctccc aacccttaa gccctggccc cctgagtttc
3781 cttttctcgt ctctctcttt ttatTTTTT tatttttatt ttatTTTTg agacagagcc
10 3841 tcgctcgta cccagggtgg agtgcagtgg tagcgatctc ggctcacagt gcaacctctg
3901 ctcccaggt tcaagcgatt ctctgcctc agcctccga gtagctggga ttacaggtgt
3961 gcaccaccac acccggctaa ttttttat ttttaataga gatgaggttt caccatgatg
4021 gccaggctga tctcgaactc ctaacctcaa gtgacctcc cacc

Human TYK2 mRNA (SEQ ID NO: 15)

[0117]

20

25

30

35

40

45

50

55

1 aagcagtagc tacccgcggg agcggggagg ggtccgggtt cgagcttggtg tcccccgga
 61 aggggtgagtc tggacgcggg cgcggaaggga gcgcggccgg aggtcctcag gaagaagccg
 121 cggggactgg ctgcgttga caggctgcac ttggatggga gcacctggtg cctcgggact
 181 gctccgatgc cggggtctgt gctgaatgtg taatatgcgg aactatattg aacattaca
 241 accatctttt gatggcaaca ccctgaggac ctccctttc cagatgggga aactgaggcc
 301 cagaattgct aagtggcttg cttgagttga cacagggagc tccaggactc accctcagct
 361 gagccacctg ccgggagcat gcctctgcgc cactggggga tggccagggg cagtaagccc
 421 gttggggatg gagcccagcc catggctgcc atgggaggcc tgaaggtgct tctgactgg
 481 gctggtccag gcggcgggga gccctgggtc actttcagtg agtcacgct gacagctgag
 541 gaagtctgca tccacattgc acataaagtt ggtatcactc ctcttgctt caatctctt
 601 gccctcttcg atgctcaggc ccaagtctgg ttgccccaa accacatcct agagatcccc
 661 agagatgcaa gcctgatgct atattccgc ataagtttt attccggaa ctggcatggc
 721 atgaatcctc gggaaccggc tgtgtaccgt tgtgggcccc caggaaccga ggcacctca
 781 gatcagacag cacaggggat gcaactcctg gaccagcct catttgagta cctctttgag
 841 cagggcaagc atgagttgt gaatgacgtg gcatcactgt gggagctgtc gaccgaggag
 901 gagatccacc actttaagaa tgagagcctg ggcatggcct ttctgcacct ctgtcacctc
 961 gctctccgcc atggcatccc cctggaggag gtggccaaga agaccagctt caaggactgc
 1021 atcccgct cttccggcg gcataccgg cagcacagcg ccctgaccg gctgcgcctt
 1081 cggaaactct tccgagggt cctgcgggac ttccagccgg gccgactctc ccagcagatg
 1141 gtcatggtca aatacctagc cacactcgag cggctggcac cccgcttcgg cacagagcgt
 1201 gtgcccgtgt gccacctgag gctgctggcc caggccgagg gggagccctg ctacatccgg
 1261 gacagtgggg tggcccctac agaccctggc cctgagctg ctgctgggcc cccaaccac
 1321 gaggtgctgg tgacaggcac tgggtggcatc cagtgggtgc cagtagagga ggaggtgaac
 1381 aaggaggagg gttctagtgg cagcagtggc aggaaccccc aagccagcct gtttgggaag
 1441 aaggccaagg ctacaaggc agtcggccag ccggcagaca ggccgcggga gccactgtgg
 1501 gcctacttct gtgacttccg ggacatcacc cacgtggtgc tgaaagagca ctgtgtcagc
 1561 atccaccggc aggacaacaa gtgcctggag ctgagcttgc cttcccgggc tgcggcgctg
 1621 tccttcgtgt cgctggtgga cggctattc cgcctgacgg ccgactccag ccactacctg
 1681 tgccacgagg tggctcccc acggctggtg atgagcatcc gggatgggat ccacggacc
 1741 ctgctggagc catttgca ggccaagctg cggcccagg acggcctgta cctcattcac
 1801 tggagcacca gccacccta ccgcctgac ctcacagtgg ccagcgtag ccaggcacca
 1861 gacggcatgc agagcttgcg gtcggaag tccccattg agcagcagga cggggccttc

1921 gtgctggagg gctggggccg gtccttcccc agcgttcggg aacttggggc tgccttgacg
 1981 ggctgcttgc tgagggccgg ggatgactgc ttctctctgc gtcgctgttg cctgccccaa
 2041 ccaggagaaa cctccaatct catcatcatg cgggggggctc gggccagccc caggacactc
 5 2101 aacctcagcc agctcagctt ccaccgggtt gaccagaagg agatcaccca gctgtccac
 2161 ttgggccagg gcacaaggac caacgtgtat gagggccgcc tgcgagtga gggcagcggg
 2221 gaccctgagg agggcaagat ggatgacgag gacccctcg tgcctggcag ggaccgtggg
 2281 caggagctac gagtgggtct caaagtgtcg gaccctagtc accatgacat cgccttgccc
 10 2341 ttctacgaga cagccagcct catgagccag gtctcccaca cgcacctggc ctctgtgcat
 2401 ggctgtctgt tgcgcggccc tgaaaatgc atggtgacag agtacgtgga gcacggaccc
 2461 ctggatgtgt ggctgaggag ggagcggggc catgtgcca tggcttgaa gatggtggtg
 15 2521 gccagcagc tggccagcgc cctcagctac ctggagaaca agaacctggt tcatggtaat
 2581 gtgtgtggcc ggaacatcct gctggcccg ctggggttg cagagggcac cagcccttc
 2641 atcaagctga gtgacctg cgtgggctg ggcgccctct ccaggaggga gcgggtggag
 2701 aggateccct ggctggcccc cgaatgccta ccaggtgggg ccaacagcct aagcaccgcc
 20 2761 atggacaagt ggggggttgg cgccacctc ctggagatct gcttgacgg agaggccct
 2821 ctgcagagcc gcagtcctc cgagaaggag cattctacc agaggcagca ccggtgccc
 2881 gagccctct gccacagct ggccacactc accagccagt gtctgacctc tgagccaacc
 2941 cagaggccat cattccgcac catcctgctg gacctaccc ggctgcagcc ccacaatctt
 25 3001 gctgacgtct tgactgtgaa cccggactca ccggcgtcg accctacggt ttccacaag
 3061 cgctatttga aaaagatccg agatctgggc gaggggtact tcggcaagggt cagctgtac
 3121 tgctacgac cgaccaacga cggcactggc gagatggtg cggtgaaagc cctcaaggca
 3181 gactgcggcc ccagcaccg ctggggtgg aagcaggaga ttgacattct gcgcacgtc
 30 3241 taccacgagc acatcatcaa gtacaagggc tgctgcgagg accaaggcga gaatgcgtg
 3301 cagctggtca tggagtacgt gccctgggc agcctccgag actacctgcc ccggcacagc
 3361 atcgggtgg cccagctgct gctctcgc cagcagatct gcgaggcat ggcctatctg
 3421 cacgcgagc actacatcca ccgagacctc gccgcgcga acgtgctgct ggacaacgac
 35 3481 aggtggtca agatcgggga ctttggccta gccaaggccg tgcccgaagg ccacgagtac
 3541 taccgctgc gcgaggatgg ggacagcccc gtgttctggt atgcccaga gtgctgaag
 3601 gagtataagt tctactatgc gtcagatgc tggctcttc gggtgacct gtatgagctg
 40 3661 ctgacgcact gtgactccag ccagagcccc cccacgaaat tcttgagct cataggcatt
 3721 gctcagggtc agatgacagt tctgagactc actgagttgc tggaacgagg ggagaggctg
 3781 ccacggcccc acaaatgtcc ctgtgagtc tatcatctca tgaagaactg ctgggagaca
 3841 gaggcgtct ttcgccaac ctgcgagac ctcataccca ttctgaagac agtccatgag
 45 3901 aagtaccaag gccagcccc tcagtgttc agcgtgtgct gaggcacaaat ggcagccctg
 3961 cctgggagga ctggaccagg cagtggctgc agagggagcc tctgctccc tgctccagga
 4021 tgaaaccaag agggggatgt cagcctcacc cacaccgtgt gccttactcc tgtctagaga
 4081 cccacctct gtgaacttat tttctttct tggccgtgag cctaaccatg atcttgagg
 50 4141 acccaacatt ttaggggca ctaatccagc ccttaaatcc cccagctcc aaacttgagg
 4201 cccaccatct ccaccatctg gtaataaact catgtttct ctgctggaaa aaaaaaaaaa
 4261 aa

Inhibitory Nucleic Acids

[0118] An antisense nucleic acid molecule can be complementary to all or part of a non-coding region of the coding strand of a nucleotide sequence encoding a JAK1, JAK2, JAK3, or TYK2 protein. Non-coding regions (5' and 3' untrans-

lated regions) are the 5' and 3' sequences that flank the coding region in a gene and are not translated into amino acids.

[0119] Based upon the sequences disclosed herein, one of skill in the art can easily choose and synthesize any of a number of appropriate antisense nucleic acids to target a nucleic acid encoding a JAK1, JAK2, JAK3, or TYK2 protein described herein. Antisense nucleic acids targeting a nucleic acid encoding a JAK1, JAK2, JAK3, or TYK2 protein can

be designed using the software available at the Integrated DNA Technologies website.

[0120] An antisense nucleic acid can be, for example, about 5, 10, 15, 20, 25, 30, 35, 40, 45, or 50 nucleotides or more in length. An antisense oligonucleotide can be constructed using chemical synthesis and enzymatic ligation reactions using procedures known in the art. For example, an antisense nucleic acid can be chemically synthesized using naturally occurring nucleotides or variously modified nucleotides designed to increase the biological stability of the molecules or to increase the physical stability of the duplex formed between the antisense and sense nucleic acids, e.g., phosphorothioate derivatives and acridine substituted nucleotides can be used.

[0121] Examples of modified nucleotides which can be used to generate an antisense nucleic acid include 5-fluorouracil, 5-bromouracil, 5-chlorouracil, 5-iodouracil, hypoxanthine, xanthine, 4-acetylcytosine, 5-(carboxyhydroxymethyl) uracil, 5-carboxymethylaminomethyl-2-thiouridine, 5-carboxymethylaminomethyluracil, dihydrouracil, beta-D-galactosylqueosine, inosine, N6-isopentenyladenine, 1-methylguanine, 1-methylinosine, 2,2-dimethylguanine, 2-methyladenine, 2-methylguanine, 3-methylcytosine, 5-methylcytosine, N6-adenine, 7-methylguanine, 5-methylaminomethyluracil, 5-methoxyaminomethyl-2-thiouracil, beta-D-mannosylqueosine, 5'-methoxycarboxymethyluracil, 5-methoxyuracil, 2-methylthio-N6-isopentenyladenine, uracil-5-oxyacetic acid (v), wybutosine, pseudouracil, queosine, 2-thiocytosine, 5-methyl-2-thiouracil, 2-thiouracil, 4-thiouracil, 5-methyluracil, uracil-5-oxyacetic acid methylester, uracil-5-oxyacetic acid (v), 5-methyl-2-thiouracil, 3-(3-amino-3-N-2-carboxypropyl) uracil, (acp3)w, and 2,6-diaminopurine. Alternatively, the antisense nucleic acid can be produced biologically using an expression vector into which a nucleic acid has been subcloned in an antisense orientation (i.e., RNA transcribed from the inserted nucleic acid will be of an antisense orientation to a target nucleic acid of interest).

[0122] The antisense nucleic acid molecules described herein can be prepared in vitro and administered to a mammal, e.g., a human. Alternatively, they can be generated in situ such that they hybridize with or bind to cellular mRNA and/or genomic DNA encoding a JAK1, JAK2, JAK3, or TYK2 protein to thereby inhibit expression, e.g., by inhibiting transcription and/or translation. The hybridization can be by conventional nucleotide complementarities to form a stable duplex, or, for example, in the case of an antisense nucleic acid molecule that binds to DNA duplexes, through specific interactions in the major groove of the double helix. The antisense nucleic acid molecules can be delivered to a mammalian cell using a vector (e.g., a lentivirus, a retrovirus, or an adenovirus vector).

[0123] An antisense nucleic acid can be an α -anomeric nucleic acid molecule. An α -anomeric nucleic acid molecule forms specific double-stranded hybrids with complementary RNA in which, contrary to the usual, β -units, the strands run parallel to each other (Gaultier et al., *Nucleic Acids Res.* 15:6625-6641, 1987). The antisense nucleic acid can also comprise a 2'-O-methylribonucleotide (Inoue et al., *Nucleic Acids Res.* 15:6131-6148, 1987) or a chimeric RNA-DNA analog (Inoue et al., *FEBS Lett.* 215:327-330, 1987).

[0124] Another example of an inhibitory nucleic acid is a ribozyme that has specificity for a nucleic acid encoding a JAK1, JAK2, JAK3, or TYK2 protein (e.g., specificity for a JAK1, JAK2, JAK3, or TYK2 mRNA, e.g., specificity for any one of SEQ ID NOs: 1-15). Ribozymes are catalytic RNA molecules with ribonuclease activity that are capable of cleaving a single-stranded nucleic acid, such as an mRNA, to which they have a complementary region. Thus, ribozymes (e.g., hammerhead ribozymes (described in Haselhoff and Gerlach, *Nature* 334:585-591, 1988)) can be used to catalytically cleave mRNA transcripts to thereby inhibit translation of the protein encoded by the mRNA. A ribozyme having specificity for a JAK1, JAK2, JAK3, or TYK2 mRNA can be designed based upon the nucleotide sequence of any of the JAK1, JAK2, JAK3, or TYK2 mRNA sequences disclosed herein. For example, a derivative of a *Tetrahymena* L-19 IVS RNA can be constructed in which the nucleotide sequence of the active site is complementary to the nucleotide sequence to be cleaved in a JAK1, JAK2, JAK3, or TYK2 mRNA (see, e.g., U.S. Patent Nos. 4,987,071 and 5,116,742). Alternatively, a JAK1, JAK2, JAK3, or TYK2 mRNA can be used to select a catalytic RNA having a specific ribonuclease activity from a pool of RNA molecules. See, e.g., Bartel et al., *Science* 261:1411-1418, 1993.

[0125] An inhibitory nucleic acid can also be a nucleic acid molecule that forms triple helical structures. For example, expression of a JAK1, JAK2, JAK3, or JAK4 polypeptide can be inhibited by targeting nucleotide sequences complementary to the regulatory region of the gene encoding the JAK1, JAK2, JAK3, or TYK2 polypeptide (e.g., the promoter and/or enhancer, e.g., a sequence that is at least 1 kb, 2 kb, 3 kb, 4 kb, or 5 kb upstream of the transcription initiation start state) to form triple helical structures that prevent transcription of the gene in target cells. See generally Helene, *Anticancer Drug Des.* 6(6):569-84, 1991; Helene, *Ann. N.Y. Acad. Sci.* 660:27-36, 1992; and Maher, *Bioassays* 14(12):807-15, 1992.

[0126] In various aspects of the disclosure, inhibitory nucleic acids can be modified at the base moiety, sugar moiety, or phosphate backbone to improve, e.g., the stability, hybridization, or solubility of the molecule. For example, the deoxyribose phosphate backbone of the nucleic acids can be modified to generate peptide nucleic acids (see, e.g., Hyrup et al., *Bioorganic Medicinal Chem.* 4(1):5-23, 1996). Peptide nucleic acids (PNAs) are nucleic acid mimics, e.g.,

DNA mimics, in which the deoxyribose phosphate backbone is replaced by a pseudopeptide backbone and only the four natural nucleobases are retained. The neutral backbone of PNAs allows for specific hybridization to DNA and RNA under conditions of low ionic strength. The synthesis of PNA oligomers can be performed using standard solid phase peptide synthesis protocols (see, e.g., Perry-O'Keefe et al., *Proc. Natl. Acad. Sci. U.S.A.* 93:14670-675, 1996). PNAs can be

used as antisense or antigene agents for sequence-specific modulation of gene expression by, e.g., inducing transcription or translation arrest or inhibiting replication.

[0127] PNAs can be modified, e.g., to enhance their stability or cellular uptake, by attaching lipophilic or other helper groups to PNA, by the formation of PNA-DNA chimeras, or by the use of liposomes or other techniques of drug delivery known in the art. For example, PNA-DNA chimeras can be generated which may combine the advantageous properties of PNA and DNA. Such chimeras allow DNA recognition enzymes, e.g., RNase H and DNA polymerases, to interact with the DNA portion while the PNA portion would provide high binding affinity and specificity. PNA-DNA chimeras can be linked using linkers of appropriate lengths selected in terms of base stacking, number of bonds between the nucleobases, and orientation.

[0128] The synthesis of PNA-DNA chimeras can be performed as described in Finn et al., *Nucleic Acids Res.* 24:3357-63, 1996. For example, a DNA chain can be synthesized on a solid support using standard phosphoramidite coupling chemistry and modified nucleoside analogs. Compounds such as 5'-(4-methoxytrityl)amino-5'-deoxy-thymidine phosphoramidite can be used as a link between the PNA and the 5' end of DNA (Mag et al., *Nucleic Acids Res.* 17:5973-88, 1989). PNA monomers are then coupled in a stepwise manner to produce a chimeric molecule with a 5' PNA segment and a 3' DNA segment (Finn et al., *Nucleic Acids Res.* 24:3357-63, 1996). Alternatively, chimeric molecules can be synthesized with a 5' DNA segment and a 3' PNA segment (Peterser et al., *Bioorganic Med. Chem. Lett.* 5:1119-1124, 1975).

[0129] In some cases, the inhibitory nucleic acids can include other appended groups such as peptides, or agents facilitating transport across the cell membrane (see, Letsinger et al., *Proc. Natl. Acad. Sci. U.S.A.* 86:6553-6556, 1989; Lemaitre et al., *Proc. Natl. Acad. Sci. U.S.A.* 84:648-652, 1989; and WO 88/09810). In addition, the inhibitory nucleic acids can be modified with hybridization-triggered cleavage agents (see, e.g., Krol et al., *Bio/Techniques* 6:958-976, 1988) or intercalating agents (see, e.g., Zon, *Pharm. Res.* 5:539-549, 1988). To this end, the oligonucleotide may be conjugated to another molecule, e.g., a peptide, hybridization triggered cross-linking agent, transport agent, hybridization-triggered cleavage agent, etc.

[0130] Another means by which expression of a JAK1, JAK2, JAK3, or TYK2 mRNA can be decreased in a mammalian cell is by RNA interference (RNAi). RNAi is a process in which mRNA is degraded in host cells. To inhibit an mRNA, double-stranded RNA (dsRNA) corresponding to a portion of the gene to be silenced (e.g., a gene encoding a JAK1, JAK2, JAK3, or TYK2 polypeptide) is introduced into a mammalian cell. The dsRNA is digested into 21-23 nucleotide-long duplexes called short interfering RNAs (or siRNAs), which bind to a nuclease complex to form what is known as the RNA-induced silencing complex (or RISC). The RISC targets the homologous transcript by base pairing interactions between one of the siRNA strands and the endogenous mRNA. It then cleaves the mRNA about 12 nucleotides from the 3' terminus of the siRNA (see Sharp et al., *Genes Dev.* 15:485-490, 2001, and Hammond et al., *Nature Rev. Gen.* 2:110-119, 2001). RNA-mediated gene silencing can be induced in a mammalian cell in many ways, e.g., by enforcing endogenous expression of RNA hairpins (see, Paddison et al., *Proc. Natl. Acad. Sci. U.S.A.* 99: 1443-1448, 2002) or, as noted above, by transfection of small (21-23 nt) dsRNA (reviewed in Caplen, *Trends Biotech.* 20:49-51, 2002). Methods for modulating gene expression with RNAi are described, e.g., in U.S. Patent No. 6,506,559 and US 2003/0056235A1.

[0131] Standard molecular biology techniques can be used to generate siRNAs. Short interfering RNAs can be chemically synthesized, recombinantly produced, e.g., by expressing RNA from a template DNA, such as a plasmid, or obtained from commercial vendors, such as Dharmacon. The RNA used to mediate RNAi can include synthetic or modified nucleotides, such as phosphorothioate nucleotides. Methods of transfecting cells with siRNA or with plasmids engineered to make siRNA are routine in the art.

[0132] The siRNA molecules used to decrease expression of a JAK1, JAK2, JAK3, or TYK2 mRNA can vary in a number of ways. For example, they can include a 3' hydroxyl group and strands of 21, 22, or 23 consecutive nucleotides. They can be blunt ended or include an overhanging end at either the 3' end, the 5' end, or both ends. For example, at least one strand of the RNA molecule can have a 3' overhang from about 1 to about 6 nucleotides (e.g., 1-5, 1-3, 2-4, or 3-5 nucleotides (whether pyrimidine or purine nucleotides) in length. Where both strands include an overhang, the length of the overhangs may be the same or different for each strand. To further enhance the stability of the RNA duplexes, the 3' overhangs can be stabilized against degradation (by, e.g., including purine nucleotides, such as adenosine or guanosine nucleotides or replacing pyrimidine nucleotides by modified analogues (e.g., substitution of uridine 2'-nucleotide 3' overhangs by 2'-deoxythymidine is tolerated and does not affect the efficiency of RNAi). Any siRNA can be used in the methods of decreasing a JAK1, JAK2, JAK3, or TYK2 mRNA, provided it has sufficient homology to the target of interest (e.g., a sequence present in any one of SEQ ID NOs: 1-15, e.g., a target sequence encompassing the translation start site or the first exon of the mRNA). There is no upper limit on the length of the siRNA that can be used (e.g., the siRNA can range from about 21 base pairs of the gene to the full length of the gene or more (e.g., about 20 to

about 30 base pairs, about 50 to about 60 base pairs, about 60 to about 70 base pairs, about 70 to about 80 base pairs, about 80 to about 90 base pairs, or about 90 to about 100 base pairs).

[0133] Non-limiting examples of JAK inhibitors that are short interfering RNAs (siRNAs) are described in Cook et al., Blood 123:2826-2837, 2014. Non-limiting examples of JAK inhibitors that are short hairpin RNAs (shRNAs) are described in Koppikar et al., Nature 489(7414): 155-159, 2012).

[0134] In some disclosures, a therapeutically effective amount of an inhibitory nucleic acid targeting a nucleic acid encoding a JAK1, JAK2, JAK3, or TYK2 protein can be administered to a subject (e.g., a human subject) in need thereof. In some cases, the inhibitory nucleic acid can be about 10 nucleotides to about 40 nucleotides (e.g., about 10 to about 30 nucleotides, about 10 to about 25 nucleotides, about 10 to about 20 nucleotides, about 10 to about 15 nucleotides, 10 nucleotides, 11 nucleotides, 12 nucleotides, 13 nucleotides, 14 nucleotides, 15 nucleotides, 16 nucleotides, 17 nucleotides, 18 nucleotides, 19 nucleotides, 20 nucleotides, 21 nucleotides, 22 nucleotides, 23 nucleotides, 24 nucleotides, 25 nucleotides, 26 nucleotides, 27 nucleotides, 28 nucleotides, 29 nucleotides, 30 nucleotides, 31 nucleotides, 32 nucleotides, 33 nucleotides, 34 nucleotides, 35 nucleotides, 36 nucleotides, 37 nucleotides, 38 nucleotides, 39 nucleotides, or 40 nucleotides) in length. One skilled in the art will appreciate that inhibitory nucleic acids may comprise at least one modified nucleic acid at either the 5' or 3' end of DNA or RNA.

[0135] As is known in the art, the term "thermal melting point (T_m)" refers to the temperature, under defined ionic strength, pH, and inhibitory nucleic acid concentration, at which 50% of the inhibitory nucleic acids complementary to the target sequence hybridize to the target sequence at equilibrium. In some cases, an inhibitory nucleic acid can bind specifically to a target nucleic acid under stringent conditions, e.g., those in which the salt concentration is at least about 0.01 to 1.0 M Na ion concentration (or other salts) at pH 7.0 to 8.3 and the temperature is at least about 30 °C. for short oligonucleotides (e.g., 10 to 50 nucleotide). Stringent conditions can also be achieved with the addition of destabilizing agents such as formamide.

[0136] In some cases of the inhibitory nucleic acids described herein, the inhibitory nucleic acid binds to a target nucleic acid (e.g., a nucleic acid encoding JAK1, JAK2, JAK3, or TYK2) with a T_m of greater than 20 °C, greater than 22 °C, greater than 24 °C, greater than 26 °C, greater than 28 °C, greater than 30 °C, greater than 32 °C, greater than 34 °C, greater than 36 °C, greater than 38 °C, greater than 40 °C, greater than 42 °C, greater than 44 °C, greater than 46 °C, greater than 48 °C, greater than 50 °C, greater than 52 °C, greater than 54 °C, greater than 56 °C, greater than 58 °C, greater than 60 °C, greater than 62 °C, greater than 64 °C, greater than 66 °C, greater than 68 °C, greater than 70 °C, greater than 72 °C, greater than 74 °C, greater than 76 °C, greater than 78 °C, or greater than 80 °C, e.g., as measured in phosphate buffered saline using a UV spectrophotometer.

[0137] In some cases of the inhibitor nucleic acids described herein, the inhibitory nucleic acid binds to a target nucleic acid (e.g., a nucleic acid encoding a JAK1, JAK2, JAK3, or TYK2) with a T_m of about 20 °C to about 80 °C, about 78 °C, about 76 °C, about 74 °C, about 72 °C, about 70 °C, about 68 °C, about 66 °C, about 64 °C, about 62 °C, about 60 °C, about 58 °C, about 56 °C, about 54 °C, about 52 °C, about 50 °C, about 48 °C, about 46 °C, about 44 °C, about 42 °C, about 40 °C, about 38 °C, about 36 °C, about 34 °C, about 32 °C, about 30 °C, about 28 °C, about 26 °C, about 24 °C, or about 22 °C (inclusive); about 22 °C to about 80 °C, about 78 °C, about 76 °C, about 74 °C, about 72 °C, about 70 °C, about 68 °C, about 66 °C, about 64 °C, about 62 °C, about 60 °C, about 58 °C, about 56 °C, about 54 °C, about 52 °C, about 50 °C, about 48 °C, about 46 °C, about 44 °C, about 42 °C, about 40 °C, about 38 °C, about 36 °C, about 34 °C, about 32 °C, about 30 °C, about 28 °C, about 26 °C, or about 24 °C (inclusive); about 24 °C to about 80 °C, about 78 °C, about 76 °C, about 74 °C, about 72 °C, about 70 °C, about 68 °C, about 66 °C, about 64 °C, about 62 °C, about 60 °C, about 58 °C, about 56 °C, about 54 °C, about 52 °C, about 50 °C, about 48 °C, about 46 °C, about 44 °C, about 42 °C, about 40 °C, about 38 °C, about 36 °C, about 34 °C, about 32 °C, about 30 °C, about 28 °C, or about 26 °C (inclusive); about 26 °C to about 80 °C, about 78 °C, about 76 °C, about 74 °C, about 72 °C, about 70 °C, about 68 °C, about 66 °C, about 64 °C, about 62 °C, about 60 °C, about 58 °C, about 56 °C, about 54 °C, about 52 °C, about 50 °C, about 48 °C, about 46 °C, about 44 °C, about 42 °C, about 40 °C, about 38 °C, about 36 °C, about 34 °C, about 32 °C, about 30 °C, or about 28 °C (inclusive); about 28 °C to about 80 °C, about 78 °C, about 76 °C, about 74 °C, about 72 °C, about 70 °C, about 68 °C, about 66 °C, about 64 °C, about 62 °C, about 60 °C, about 58 °C, about 56 °C, about 54 °C, about 52 °C, about 50 °C, about 48 °C, about 46 °C, about 44 °C, about 42 °C, about 40 °C, about 38 °C, about 36 °C, about 34 °C, about 32 °C, or about 30 °C (inclusive); about 30 °C to about 80 °C, about 78 °C, about 76 °C, about 74 °C, about 72 °C, about 70 °C, about 68 °C, about 66 °C, about 64 °C, about 62 °C, about 60 °C, about 58 °C, about 56 °C, about 54 °C, about 52 °C, about 50 °C, about 48 °C, about 46 °C, about 44 °C, about 42 °C, about 40 °C, about 38 °C, about 36 °C, about 34 °C, or about 32 °C (inclusive); about 32 °C to about 80 °C, about 78 °C, about 76 °C, about 74 °C, about 72 °C, about 70 °C, about 68 °C, about 66 °C, about 64 °C, about 62 °C, about 60 °C, about 58 °C, about 56 °C, about 54 °C, about 52 °C, about 50 °C, about 48 °C, about 46 °C, about 44 °C, about 42 °C, about 40 °C, about 38 °C, about 36 °C, or about 34 °C (inclusive); about 34 °C to about 80 °C, about 78 °C, about 76 °C, about 74 °C, about 72 °C, about 70 °C, about 68 °C, about 66 °C, about 64 °C, about 62 °C, about 60 °C, about 58 °C, about 56 °C, about 54 °C, about 52 °C, about 50 °C, about 48 °C, about 46 °C, about 44 °C, about 42 °C, about 40 °C, about 38 °C, or about 36 °C (inclusive); about 36 °C to about 80 °C, about 78 °C, about 76 °C, about 74 °C, about 72 °C, about 70 °C,

about 68 °C, about 66 °C, about 64 °C, about 62 °C, about 60 °C, about 58 °C, about 56 °C, about 54 °C, about 52 °C, about 50 °C, about 48 °C, about 46 °C, about 44 °C, about 42 °C, about 40 °C, or about 38 °C (inclusive); about 38 °C to about 80 °C, about 78 °C, about 76 °C, about 74 °C, about 72 °C, about 70 °C, about 68 °C, about 66 °C, about 64 °C, about 62 °C, about 60 °C, about 58 °C, about 56 °C, about 54 °C, about 52 °C, about 50 °C, about 48 °C, about 46 °C, about 44 °C, about 42 °C, or about 40 °C (inclusive); about 40 °C to about 80 °C, about 78 °C, about 76 °C, about 74 °C, about 72 °C, about 70 °C, about 68 °C, about 66 °C, about 64 °C, about 62 °C, about 60 °C, about 58 °C, about 56 °C, about 54 °C, about 52 °C, about 50 °C, about 48 °C, about 46 °C, about 44 °C, or about 42 °C (inclusive); about 42 °C to about 80 °C, about 78 °C, about 76 °C, about 74 °C, about 72 °C, about 70 °C, about 68 °C, about 66 °C, about 64 °C, about 62 °C, about 60 °C, about 58 °C, about 56 °C, about 54 °C, about 52 °C, about 50 °C, about 48 °C, or about 46 °C (inclusive); about 44 °C to about 80 °C, about 78 °C, about 76 °C, about 74 °C, about 72 °C, about 70 °C, about 68 °C, about 66 °C, about 64 °C, about 62 °C, about 60 °C, about 58 °C, about 56 °C, about 54 °C, about 52 °C, about 50 °C, about 48 °C, or about 46 °C (inclusive); about 46 °C to about 80 °C, about 78 °C, about 76 °C, about 74 °C, about 72 °C, about 70 °C, about 68 °C, about 66 °C, about 64 °C, about 62 °C, about 60 °C, about 58 °C, about 56 °C, about 54 °C, about 52 °C, about 50 °C, or about 48 °C (inclusive); about 48 °C to about 80 °C, about 78 °C, about 76 °C, about 74 °C, about 72 °C, about 70 °C, about 68 °C, about 66 °C, about 64 °C, about 62 °C, about 60 °C, about 58 °C, about 56 °C, about 54 °C, about 52 °C, or about 50 °C (inclusive); about 50 °C to about 80 °C, about 78 °C, about 76 °C, about 74 °C, about 72 °C, about 70 °C, about 68 °C, about 66 °C, about 64 °C, about 62 °C, about 60 °C, about 58 °C, about 56 °C, or about 54 °C (inclusive); about 54 °C to about 80 °C, about 78 °C, about 76 °C, about 74 °C, about 72 °C, about 70 °C, about 68 °C, about 66 °C, about 64 °C, about 62 °C, about 60 °C, about 58 °C, about 56 °C, or about 56 °C (inclusive); about 56 °C to about 80 °C, about 78 °C, about 76 °C, about 74 °C, about 72 °C, about 70 °C, about 68 °C, about 66 °C, about 64 °C, about 62 °C, or about 60 °C (inclusive); about 60 °C to about 80 °C, about 78 °C, about 76 °C, about 74 °C, about 72 °C, about 70 °C, about 68 °C, about 66 °C, about 64 °C, or about 62 °C (inclusive); about 62 °C to about 80 °C, about 78 °C, about 76 °C, about 74 °C, about 72 °C, about 70 °C, about 68 °C, about 66 °C, or about 64 °C (inclusive); about 64 °C to about 80 °C, about 78 °C, about 76 °C, about 74 °C, about 72 °C, about 70 °C, about 68 °C, or about 66 °C (inclusive); about 66 °C to about 80 °C, about 78 °C, about 76 °C, about 74 °C, about 72 °C, about 70 °C, or about 68 °C (inclusive); about 68 °C to about 80 °C, about 78 °C, about 76 °C, about 74 °C, or about 72 °C (inclusive); about 70 °C to about 80 °C, about 78 °C, about 76 °C, or about 74 °C (inclusive); about 72 °C to about 80 °C, about 78 °C, about 76 °C, or about 74 °C (inclusive); about 74 °C to about 80 °C, about 78 °C, or about 76 °C (inclusive); about 76 °C to about 80 °C or about 78 °C (inclusive); or about 78 °C to about 80 °C (inclusive),

[0138] In some cases, the inhibitory nucleic acid can be formulated in a nanoparticle (e.g., a nanoparticle including one or more synthetic polymers, e.g., Patil et al., *Pharmaceutical Nanotechnol.* 367:195-203, 2009; Yang et al., *ACS Appl. Mater. Interfaces*, doi: 10.1021/acsami.6b16556, 2017; Perepelyuk et al., *Mol. Ther. Nucleic Acids* 6:259-268, 2017). In some cases, the nanoparticle can be a mucoadhesive particle (e.g., nanoparticles having a positively-charged exterior surface) (Andersen et al., *Methods Mol. Biol.* 555:77-86, 2009). In some cases, the nanoparticle can have a neutrally-charged exterior surface.

[0139] In some cases, the inhibitory nucleic acid can be formulated, e.g., as a liposome (Buyens et al., *J. Control Release* 158(3): 362-370, 2012; Scarabel et al., *Expert Opin. Drug Deliv.* 17:1-14, 2017), a micelle (e.g., a mixed micelle) (Tangsangasakri et al., *BioMacromolecules* 17:246-255, 2016; Wu et al., *Nanotechnology*, doi: 10.1088/1361-6528/aa6519, 2017), a microemulsion (WO 11/004395), a nanoemulsion, or a solid lipid nanoparticle (Sahay et al., *Nature Biotechnol.* 31:653-658, 2013; and Lin et al., *Nanomedicine* 9(1):105-120, 2014). Additional exemplary structural features of inhibitory nucleic acids and formulations of inhibitory nucleic acids are described in US 2016/0090598.

[0140] In some embodiments, a pharmaceutical composition can include a sterile saline solution and one or more inhibitory nucleic acid (e.g., any of the inhibitory nucleic acids described herein). In some examples, a pharmaceutical composition consists of a sterile saline solution and one or more inhibitory nucleic acid (e.g., any of the inhibitory nucleic acids described herein). In certain embodiments, the sterile saline is a pharmaceutical grade saline. In certain embodiments, a pharmaceutical composition can include one or more inhibitory nucleic acid (e.g., any of the inhibitory nucleic acids described herein) and sterile water. In certain embodiments, a pharmaceutical composition consists of one or more inhibitory nucleic acid (e.g., any of the inhibitory nucleic acids described herein) and sterile water. In certain embodiments, a pharmaceutical composition includes one or more inhibitory nucleic acid (e.g., any of the inhibitory nucleic acids described herein) and phosphate-buffered saline (PBS). In certain embodiments, a pharmaceutical composition consists of one or more inhibitory nucleic acids (e.g., any of the inhibitory nucleic acids described herein) and sterile phosphate-buffered saline (PBS). In some examples, the sterile saline is a pharmaceutical grade PBS.

[0141] In certain cases, one or more inhibitory nucleic acids (e.g., any of the inhibitory nucleic acids described herein)

may be admixed with pharmaceutically acceptable active and/or inert substances for the preparation of pharmaceutical compositions or formulations. Compositions and methods for the formulation of pharmaceutical compositions depend on a number of criteria, including, but not limited to, route of administration, extent of disease, or dose to be administered.

[0142] Pharmaceutical compositions including one or more inhibitory nucleic acids encompass any pharmaceutically acceptable salts, esters, or salts of such esters. Non-limiting examples of pharmaceutical compositions include pharmaceutically acceptable salts of inhibitory nucleic acids. Suitable pharmaceutically acceptable salts include, but are not limited to, sodium and potassium salts.

[0143] Also provided herein are prodrugs that can include additional nucleosides at one or both ends of an inhibitory nucleic acid which are cleaved by endogenous nucleases within the body, to form the active inhibitory nucleic acid.

[0144] Lipid moieties can be used to formulate an inhibitory nucleic acid. In certain such methods, the inhibitory nucleic acid is introduced into preformed liposomes or lipoplexes made of mixtures of cationic lipids and neutral lipids. In certain methods, inhibitory nucleic acid complexes with mono- or poly-cationic lipids are formed without the presence of a neutral lipid. In certain cases, a lipid moiety is selected to increase distribution of an inhibitory nucleic acid to a particular cell or tissue in a mammal. In some examples, a lipid moiety is selected to increase distribution of an inhibitory nucleic acid to fat tissue in a mammal. In certain cases, a lipid moiety is selected to increase distribution of an inhibitory nucleic acid to muscle tissue.

[0145] In certain cases, pharmaceutical compositions provided herein comprise one or more inhibitory nucleic acid and one or more excipients. In certain such cases, excipients are selected from water, salt solutions, alcohol, polyethylene glycols, gelatin, lactose, amylase, magnesium stearate, talc, silicic acid, viscous paraffin, hydroxymethylcellulose and polyvinylpyrrolidone.

[0146] In some examples, a pharmaceutical composition provided herein includes liposomes and emulsions. Liposomes and emulsions can be used to formulate hydrophobic compounds. In some examples, certain organic solvents such as dimethylsulfoxide are used.

[0147] In some examples, a pharmaceutical composition provided herein includes one or more tissue-specific delivery molecules designed to deliver one or more inhibitory nucleic acids to specific tissues or cell types in a mammal. For example, a pharmaceutical composition can include liposomes coated with a tissue-specific antibody.

[0148] In some embodiments, a pharmaceutical composition provided herein can include a co-solvent system. Examples of such co-solvent systems include benzyl alcohol, a nonpolar surfactant, a water-miscible organic polymer, and an aqueous phase. A non-limiting example of such a co-solvent system is the VPD co-solvent system, which is a solution of absolute ethanol comprising 3% w/v benzyl alcohol, 8% w/v of the nonpolar surfactant Polysorbate 80™ and 65% w/v polyethylene glycol 300. As can be appreciated, other surfactants may be used instead of Polysorbate 80™; the fraction size of polyethylene glycol may be varied; other biocompatible polymers may replace polyethylene glycol, e.g., polyvinyl pyrrolidone; and other sugars or polysaccharides may substitute for dextrose.

[0149] In some examples, a pharmaceutical composition can be formulated for oral administration. In some examples, pharmaceutical compositions are formulated for buccal administration.

In some examples, a pharmaceutical composition is formulated for administration by injection (e.g., intravenous, subcutaneous, intramuscular, etc.). In some of these embodiments, a pharmaceutical composition includes a carrier and is formulated in aqueous solution, such as water or physiologically compatible buffers such as Hanks's solution, Ringer's solution, or physiological saline buffer. In some examples, other ingredients are included (e.g., ingredients that aid in solubility or serve as preservatives). In some examples, injectable suspensions are prepared using appropriate liquid carriers, suspending agents, and the like. Some pharmaceutical compositions for injection are formulated in unit dosage form, e.g., in ampoules or in multi-dose containers. Some pharmaceutical compositions for injection are suspensions, solutions, or emulsions in oily or aqueous vehicles, and may contain formulatory agents such as suspending, stabilizing, and/or dispersing agents. Solvents suitable for use in pharmaceutical compositions for injection include, but are not limited to, lipophilic solvents and fatty oils, such as sesame oil, synthetic fatty acid esters, such as ethyl oleate or triglycerides, and liposomes.

Small Molecules

[0150] In some cases, the JAK inhibitor is a small molecule. In some cases, the JAK inhibitory agent is a pan-JAK inhibitor (e.g., 3-O-methylthiespesilactam (Li et al., *Biochem. Pharmacol.* 86(10):1411-8, 2013)). In some embodiments, the JAK inhibitor is a JAK1 and JAK2 inhibitor. In some embodiments, the JAK1 and JAK2 inhibitor is ruxolitinib (Jakafi®, Jakavi®, INCB018424) (Harrison et al., *N Engl. J Med* 366:787-798, 2012; Pieri et al., *Am. J Hematol.* 92(2):187-195, 2017; Mackay-Wiggan et al., *JCI Insight* 1(15):e89790, 2016; Rudolph et al., *Leukemia* 30(10):2119-2123, 2016; Furqan et al., *Biomark Res.* 1(1):5, 2013), baricitinib (INCB028050, LY3009104) (Gras, *Drugs Today (Bare)* 52(10):543-550, 2016; Smolen et al., *Ann. Rheum. Dis.* 76(4):694-700, 2016; Kubo et al., *Expert. Rev. Clin. Immunol.* 12(9):911-919, 2016; Fridman et al., *J Immunol.* 184(9):5298-5307, 2010), AZD1480 (Guschin et al., *EMBO J* 14:1421-1429, 1995; Ioannidis et al., *J Med Chem.* 54: 262-276, 2011; Moisan et al., *Nat. Cell Biol.* 17(1):57-67, 2015; Qin et al., *J Neurosci.*

36(18):5144059, 2016; Jiang et al., *Biochem. Biophys. Res. Commun.* 458(4):908-912, 2015; Verstovsek et al., *Leuk. Res.* 39(2):157-163, 2015; Plimack et al., *Oncologist* 18(7): 819-820, 2013; Yan et al., *Oncotarget* 4(3):433-445, 2013), filgotinib (GLPG0634, G146034) (Vermeire et al., *Lancet* 389(10066):266-275, 2017; Menet et al., *J Med Chem.* 57(22):9323-9342, 2014; Van Rompaey et al., *J Immunol.* 191(7):3568-3577, 2013; Namour et al., *Clin. Pharmacokinet.* 54(8):859-874, 2015), momelotinib (GS-0387, CYT387) (Pardanani et al., *Leukemia* 23: 1441-1445, 2009; Gupta et al., *Haematologica* 102(1):94-102, 2017; Hu et al., *Mol. Pharm.* 13(2):689-697, 2016; Abubaker et al., *BMC Cancer* 14: 317, 2014; Durmus et al., *Pharmacol. Res.* 76:9-16, 2013; Pardanani et al., *Leukemia* 27(6): 1322-1327, 2013; Monaghan et al., *Leukemia* 25(12):1891-1899, 2011; Tyner et al., *Blood* 115(25):5232-5240, 2010).

[0151] In some embodiments, the JAK inhibitory agent is a JAK1 inhibitor (e.g., GSK2586184 (Kahl et al., *Lupus* 25(13): 1420-1430, 2016; Ludbrook et al., *Er. J Dermatol.* 174(5):985-995, 2016; van Vollenhoven et al., *Lupus* 24(6): 648-649, 2015), oclacitinib (PF03394197, Apoquel®) (Gonzales et al., *J Vet. Pharmacol. Ther.* 37(4):317-324, 2014; Collard et al., *J Vet. Pharmacol. Ther.* 37(3):279-285, 2014; Cosgrove et al., *Vet. Dermatol.* 24(6):587-597, 2013), upadacitinib (ABT494) (Kremer et al., *Arthritis Rheumatol.* 68(12):2867-2877, 2016; Mohamed et al., *Clin. Pharmacol.* 55(12): 1547-1558, 2016), GLG0778 (O'Shea et al., *Ann. Rev. Med* 66(1):311-28, 2015; Schwartz et al., *Nat. Rev. Rheum.* 12: 25-36, 2016), INCB039110 (Mascarenhas et al., *Haematologica* 102(2):327-335, 2017; Bissonnette et al., *J Dermatolog. Treat.* 27(4):332-338, 2016; Rosenthal et al., *Exp. Opin. Pharmacother.* 15(9):1265-1276, 2014), PF04965842 (Gadina et al., *Curr. Opin. Rheumatol.* 26(2):237-243, 2014; Degryset et al., *J Hematol. Oncol.* 8:91, 2015); SAR-20347 (Works et al., *J Immunol.* 193(7):3278-3287, 2014)).

[0152] In some embodiments, the JAK inhibitory agent is a JAK2 inhibitor (e.g., CEP-33779 (Dugan et al., *J Med Chem.* 55(11):5243-5254, 2012; Seavey et al., *Mol. Cancer Ther.* 11(4):984-993, 2012; Stump et al., *Arthritis Res. Ther.* 13(2):R68, 2011), fedratinib (TG101348, SAR302503) (Pardanani et al., *J Clin. Oncol.* 29:789-796, 2011; Jamieson et al., *J Transl. Med* 13:294, 2015; Zhang et al., *Oncotarget* 6(16): 14329-14343, 2015; Wemig et al., *Blood* 105:4508-4515, 2008); lestaurtinib (CEP-701) (Hexner et al., *Blood* 111:5663- 5671, 2008; Santos et al., *Blood* 115: 1131-1136, 2010; Smith et al., *Blood* 103: 3669-3676, 2004; Hexner et al., *Leuk. Lymphoma* 56(9):2543, 2015; Geyer et al., *Hematology* 117(Suppl):S129-132, 2012; Diaz et al., *PLoS One* 6(4):e18856, 2011; Mintum et al., *Cancer Chemother. Pharmacol.* 68(4): 1057-1065, 2011), AC-430 (O'Shea et al., *Immunity* 36(4):542-550, 2012; Patterson et al., *Clin. Exp. Immunol.* 176:1-10, 2014), pacritinib (SB1518) (Deeg et al., *J Clin. Oncol.* 29: Abstract 6515, 2011; Verstovsek et al., *J Hematol. Oncol.* 9(1):137, 2016; Chow et al., *Onco Targets. Ther.* 9:2655-2665, 2016; Komrokji et al., *Blood* 125(17):2649-2655, 2015; Jayaraman et al., *Drug Metab. Lett.* 9(1):28-47, 2015), BMS-911543 (Mace et al., *Oncotarget* 6(42):44509-44522, 2015; Wan et al., *ACS Med Chem. Lett.* 6(8):850-855, 2015; Purandare et al., *Leukemia* 26(2):280-288, 2012), XL019 (Verstovsek et al., *Leuk. Res.* 38(3):316-322, 2014; Forsyth et al., *Bioorg. Med Chem. Lett.* 22(24):7653-7658, 2012), INCB039110 (Mascarenhas et al., *Haematologica* 102(2):327-335, 2017; Bissonnette et al., *J Dermatol. Treat.* 27(4):332-338, 2016), gandotinib® (LY- 2784544) (Ma et al., *Blood Cancer J* 3:e109, 2013; Verstovsek et al., *Blood* 122: 665, 2013; Mitchell et al., *Org. Process Res. Dev.* 16(1):70-81, 2012); R723 (Shide et al., *Blood* 117(25): 6866-6875, 2011); Z3 (Sayyah et al., *Mol. Cancer. Ther.* 7(8):2308-2318, 2008)) or a variant thereof.

[0153] In some embodiments, the JAK inhibitory agent is a JAK3 inhibitor (e.g., decemotinib (VX-509) (Elwood et al., *J Pharmacol. Exp. Ther.* 2017; Genovese et al., *Ann Rheum Dis.* 75(11):1979-1983, 2016; Gadina et al., *Arthritis Rheumatol.* 68(1):31-34, 2016; Farmer et al., *J Med Chem.* 58(18):7195-7216, 2015; Fleischmann et al., *Arthritis Rheumatol.* 67(2):334-343, 2015; Mahajan et al., *J Pharmacol.* 353(2):405-414, 2015), R348 or a variant thereof (Velotta et al., *Transplantation* 87(5):653-659, 2009; Deuse et al., *Transplantation* 85(6):885-892, 2008)). In some embodiments, the small molecule is R256 or a variant thereof (Ashino et al., *J Allergy Clin. Immunol.* 133(4):1162-1174, 2014). In some embodiments, the small molecule is R333 or a variant thereof. In some embodiments, the small molecule is INCB047986 or a variant thereof (Norman, *Exp. Opin. Investig. Drugs* 23(8):1067-1077, 2014). In some embodiments, the small molecule is INCB 16562 or a variant thereof (Koppikar et al., *Blood* 115(4):2919-2927, 2010; Li et al., *Neoplasia* 12(1):28-38, 2010). In some embodiments, the small molecule is NVP-BSK805 or a variant thereof (Ringel et al., *Acta Haematol.* 132(1):75-86, 2014; Baffert et al., *Mol. Cancer. Ther.* 9(7):1945-1955, 2010). In some embodiments, the small molecule is peficitinib (ASP015K, JNJ-54781532) or a variant thereof (Genovese et al., *Arthritis Rheumatol.*, 2017; Ito et al., *J Pharmacol. Sci.* 133(1):25-33, 2017; Cao et al. (2016) *Clin. Pharmacol. Drug Dev.* 5(6):435- 449, 2016; Takeuchi et al., *Ann. Rheum. Dis.* 75(6):1057-1064, 2016). In some embodiments, the small molecule is tofacitinib (Xeljanz®, Jakvinus®, CP-690, 500) or a variant thereof (Ghoreschi et al., *J Immunol.* 186(7):4234-4243, 2011; Yoshida et al., *Biochem. Biophys. Res. Commun.* 418(2):234-240, 2012; Calama et al., *Pulm. Pharmacol. Ther.* S1094-5539(16):30060-30068, 2017; Cutolo et al., *J Inflamm. Res.* 6:129-137, 2013). In some embodiments, the small molecule is cucurbitacin I (JSI-124) or a variant thereof (Oi et al., *Int. J. Oncol.* 49(6):2275-2284, 2016; Qi et al., *Am. J. Chin. Med* 43(2):337-347, 2015; Seo et al., *Food Chem. Toxicol.* 64:217-224, 2014). In some embodiments, the small molecule is CHZ868 or a variant thereof (Wu et al., *Cancer Cell* 28(1):29-41, 2015; Meyer et al., *Cancer Cell* 28(1):15-28, 2015).

[0154] In some embodiments, the small molecule is a TYK2 inhibitor (e.g., Masse et al., *J Immunol.* 194(1):67, 2015; Menet, *Pharm. Pat. Anal.* 3(4):449-466, 2014; Liang et al., *Euro. J Med Chem.* 67: 175-187, 2013; Jang et al., *Bioorg. Med Chem. Lett.* 25(18):3947-3952, 2015); U.S. Patent Nos. 9,296,725 and 9,309,240; US 2013/0231340; and US

2016/0251376). In some embodiments, the TYK2 inhibitor is Ndi-031301 (Akahane et al., Blood 128:1596, 2016); BMS-986165 (Gillooly et al., 2016ACRIARHP Annual Meeting, Abstract 1 IL, 2016); SAR-20347 (Works et al., J Immunol. 193(7):3278-3287, 2014); tyrphostin A1 (Ishizaki et al., Int. Immunol. 26(5):257-267, 2014); a triazolopyridine (US 2013/0143915); or a variant thereof.

[0155] Additional examples of JAK inhibitors that are small molecules are described in, e.g., Furomoto et al., BioDrugs 27(5):431-438, 2013; O' Shea et al., Ann. Rheum. Dis. 72(2):ii11-ii115, 2013; Sonbol et al., Ther. Adv. Hematol. 4(1):15-35, 2013; and Tanaka et al. (2015) J Biochem. 158(3): 173-179, 2015.

[0156] In some embodiments, the JAK inhibitor is a pan-JAK inhibitor. As used herein, the term "pan-JAK inhibitor" is an agent that has an IC₅₀ of about 500 nM to 4 μ M (e.g., about 500 nM to about 2 μ M) for each of human JAK1, human JAK2, and human JAK3 isoforms, when the IC₅₀ is determined for each of wildtype human JAK1, wildtype human JAK2, and wildtype human JAK3 using similar assay conditions (e.g., the same assay conditions). In some embodiments, a pan-JAK inhibitor can be an agent that has an IC₅₀ for wildtype human JAK1, wildtype human JAK2, and wildtype human JAK3 that are within \pm 10% of each other, when each of the IC₅₀ values is assays under similar assay conditions (e.g., the same assay, e.g., the human wildtype JAK1, wildtype human JAK2, and wildtype human JAK3 assay described in Kim et al., J Med Chem. 58(18):7596-5602, 2015).

[0157] In some embodiments, the pan-JAK inhibitor is tofacitinib (Xeljanz[®], Jakvinus[®], tasocitinib, CP-690550; Yokoyama et al., J Clin. Immunol. 33(3):586-594, 2013; and Thoma et al., J Med Chem. 54(1):284-288, 2011); cerdulatinib (PRT2070; Coffey et al. (2014) J Pharmacol. Exp. Ther. 351(3):538-548, 2014; and Ma et al., Oncotarget 6(41):43881-43896, 2015); Pyridone 6 (P6; Nakagawa et al., J Immunol. 187(9): 4611-4620, 2011; and Pedranzini et al., Cancer Res. 66(19):9714-9721, 2006); PF-06263276 (Jones et al. "Design and Synthesis of a Pan-Janus Kinase Inhibitor Clinical Candidate (PF-06263276) Suitable for Inhaled and Topical Delivery for the Treatment of Inflammatory Diseases of the Lungs and Skin" J. Med. Chem., 2017, 60 (2), pp 767-786); JAK inhibitor 1 (CAS 457081-03-07; JAKI; Wang et al., Antimicrob. Agents Chemother. 60(5):2834-48, 2016; Bordonaro et al., PLoS One 9:e15068, 2014; and Osorio et al., PLoS Pathogens 10(6):e1004165, 2014); or baricitinib (Olumiant; LY3009104; INCB-28050; and Hsu and Armstrong, J Immunol. Res. Article ID 283617, 2014).

[0158] In some embodiments, the JAK inhibitor is a selective JAK1/JAK3 inhibitor. As used herein, the term "selective JAK1/JAK3 inhibitor" means an agent that has an IC₅₀ for wildtype human JAK1 and wildtype human JAK3, that are each at least 5-fold (e.g., at least 10-fold or at least 20-fold) lower than the IC₅₀ for wildtype human JAK2, when the IC₅₀ is determined for each of wild type human JAK1, wildtype human JAK2, and wildtype human JAK3 using similar assay conditions (e.g., the same assay, e.g., the human wildtype JAK1, wildtype human JAK2, and wildtype human JAK3 assay described in Kim et al., J Med Chem. 58(18):7596-5602, 2015).

[0159] In some embodiments, the JAK inhibitor is a selective JAK1 inhibitor. As used herein, the term "selective JAK1 inhibitor" means an agent that has an IC₅₀ for wildtype human JAK1 that is at least 10-fold (e.g., at least 20-fold) lower than each of the IC₅₀ for wildtype human JAK2 and the IC₅₀ for wildtype human JAK3 when measured using similar assay conditions (e.g., the same assay, e.g., the human wildtype JAK1, wildtype human JAK2, and wildtype human JAK3 assay described in Kim et al., J Med Chem. 58(18):7596- 5602, 2015). In some embodiments, the JAK1 inhibitor is (3S,4R)-3-ethyl-4-(3H-imidazol[1,2-a]pyrrolo[2,3-e]pyrazin-8-yl)-N-(2,2,2-trifluoroethyl)pyrrolidine-1-carboxamide as disclosed in international patent application PCT/US2014/062145, incorporated by reference herein in its entirety.

[0160] In some embodiments, the JAK inhibitor is a selective JAK3 inhibitor. As used herein, the term "selective JAK3 inhibitor" means an agent that has an IC₅₀ for wildtype human JAK3 that is at least 10-fold (e.g., at least 20-fold) lower than each of the IC₅₀ for wildtype human JAK2 and the IC₅₀ for wildtype human JAK1 when measured using similar assay conditions (e.g., the same assay, e.g., the human wildtype JAK1, wildtype human JAK2, and wildtype human JAK3 assay described in Kim et al., J Med Chem. 58(18):7596-5602, 2015).

[0161] In some embodiments, the JAK inhibitor is a JAK1 and JAK 3 inhibitor (e.g., a selective JAK1/JAK3 inhibitor). In some embodiments, the selective JAK1/JAK3 inhibitor is ZM 39923 (Brown et al., Bioorg. Med Chem. Lett. 10(6):575-579, 2000; and Lai et al., Chem. Biol. 15(9):969-978, 2008); or peficitinib (ASP015K; JNJ-54781532; Ito et al., J Pharmacol. Sci. 133(1):25-33, 2017; Cao et al., Clin. Pharmacol. Drug Dev. 5(6):435-449, 2016; Takeuchi et al., Ann. Rheum. Dis. 75(6): 1057-1064, 2016); and Papp et al., Er. J Dermatol. 173(3):767-776, 2015).

[0162] In some embodiments, the JAK inhibitor is PF-06700841. In some embodiments, the JAK inhibitor is PF-06651600.

[0163] In some embodiments, the inhibitor is one of the following:

Common Name	Brand name	Company
Tofacitinib	Xeljanz	Pfizer
peficitinib (ASP015K or JNJ-54781532)		JNJ
TD-1473		Theravance Biopharma

EP 3 554 485 B9

(continued)

Common Name	Brand name	Company
PF-06263276		Pfizer
Cerdulatinib (PRT-062070)		
upadacitinib (ABT494)		Abbvie
Baricitinib (INCB028050, LY3009104)	Olumiant	Incyte & Eli Lilly
Filgotinib (GLPG0634)	TBD	Gilead, Galapagos NV
Jakafi®, Jakavi®	ruxolitinib (INCB018424)	
AZD1480		AstraZeneca
momelotinib (GS-0387)		
GSK2586184		GSK
ocacitinib (PF03394197)	Apoquel®	Pfizer
ocacitinib (PF03394197)		Abbvie
GLG0778		
GLG0778		
fedratinib (TG101348, SAR302503)		
lestaurtinib (CEP-701)		
AC-430		
pacritinib (SB1518)		
XL019		
gandotinib® (LY-2784544)		
BMS-911543		BMS
NVP-BSK805		
INCB16562		
Decemotinib (VX509)		
cucurbitacin I (JSI-124)		
R333		
Ndi-031301		
SAR-20347		
tyrphostin AI		
triazolopyridine		
BMS-986165		
TOP-1288		Topivert Pharma Ltd
PF-06700841		Pfizer
PF-06651600		Pfizer
Inhibitory Nucleic Acids		

[0164] In some embodiments, the kinase inhibitor is TOP-1288 from TopiVert Pharma Ltd., which is described in "The Pharmacological Profile of TOP1288, a Narrow Spectrum Kinase Inhibitor (NSKI) in Clinical Development as an Antinflammatory Treatment for Ulcerative Colitis" Foster, Martyn et al. Gastroenterology, Volume 152, Issue 5, S766.

Ingestible Devices

[0165] As discussed herein, in some cases, a method of treating a disease of the gastrointestinal tract comprises administering to the subject a pharmaceutical formulation wherein the pharmaceutical formulation is delivered to the cecum by one of various methods. For example, the pharmaceutical formulation may be delivered via an ingestible device; the pharmaceutical formulation may be a solid dosage form, a liquid dosage form, a suppository or an enema for rectal administration with different types of release such as sustained or delayed release.

[0166] In one cases, the pharmaceutical formulation is delivered to the cecum by an ingestible device containing the pharmaceutical formulation.

[0167] The GI tract can be imaged using endoscopes, or more recently, by ingestible devices that are swallowed. Direct visualization of the GI mucosa is useful to detect subtle mucosal alterations, as in inflammatory bowel diseases, as well as any flat or sessile lesions.

[0168] As discussed herein, in some embodiments, the method of treating a disease of the gastrointestinal tract comprises administering to the subject a pharmaceutical formulation. In some cases, the pharmaceutical formulation is delivered to the cecum by one of various methods. For example, the pharmaceutical formulation may be delivered via a medical device such as an ingestible device; the pharmaceutical formulation may be a solid dosage form, a liquid dosage form, a suppository or an enema for rectal administration with different types of release such as sustained or delayed release. In one case, the pharmaceutical formulation is delivered to the cecum by an ingestible device containing the pharmaceutical formulation.

[0169] Ingestible devices are advantageous over spray catheters in that they are less invasive, thereby allowing for regular dosing more frequently than spray catheters. Another advantage of ingestible devices is the greater ease with which they can access, relative to a catheter, certain sections of the GI tract such as the ascending colon, the cecum, and all portions of the small intestine.

Methods and Mechanisms for Localization

[0170] In addition to, or as an alternative, to directly visualizing the GI tract, one or more different mechanisms can be used to determine the location of an ingestible device within the GI tract. Various implementations may be used for localization of ingestible devices within the GI tract.

[0171] For example, certain implementations can include one or more electromagnetic sensor coils, magnetic fields, electromagnetic waves, electric potential values, ultrasound positioning systems, gamma scintigraphy techniques or other radio-tracker technology have been described by others. Alternatively, imaging can be used to localize, for example, using anatomical landmarks or more complex algorithms for 3D reconstruction based on multiple images. Other technologies rely on radio frequency, which relies on sensors placed externally on the body to receive the strength of signals emitted by the capsule. Ingestible devices may also be localized based on reflected light in the medium surrounding the device; pH; temperature; time following ingestion; and/or acoustic signals.

[0172] The disclosure provides an ingestible device, as well as related systems and methods that provide for determining the position of the ingestible device within the GI tract of a subject with very high accuracy. In some embodiments, the ingestible device can autonomously determine its position within the GI tract of the subject.

[0173] Typically, the ingestible device includes one or more processing devices, and one more machine readable hardware storage devices. In some cases, the one or more machine readable hardware storage devices store instructions that are executable by the one or more processing devices to determine the location of the ingestible device in a portion of a GI tract of the subject. In certain cases, the one or more machine readable hardware storage devices store instructions that are executable by the one or more processing devices to transmit data to an external device (e.g., a base station external to the subject, such as a base station carried on an article worn by the subject) capable of implementing the data to determine the location of the device within the GI tract of the subject.

[0174] In some disclosures, the location of the ingestible device within the cecum of the subject can be determined to an accuracy of at least 85%, e.g., at least 90%, at least 95%, at least 97%, at least 98%, at least 99%, 100%. An exemplary and non-limiting disclosure is provided below in Example 13.

[0175] As used herein, the term "reflectance" refers to a value derived from light emitted by the device, reflected back to the device, and received by a detector in or on the device. For example, in some cases this refers to light emitted by the device, wherein a portion of the light is reflected by a surface external to the device, and the light is received by a detector located in or on the device.

[0176] As used herein, the term "illumination" refers to any electromagnetic emission. In some cases, an illumination may be within the range of Infrared Light (IR), the visible spectrum and ultraviolet light (UV), and an illumination may have a majority of its power centered at a particular wavelength in the range of 100nm to 1000nm. In some cases, it may be advantageous to use an illumination with a majority of its power limited to one of the infrared (750nm-1000nm), red (600nm-750nm), green (495nm-600nm), blue (400nm-495nm), or ultraviolet (100nm-400nm) spectrums. In some

cases a plurality of illuminations with different wavelengths may be used. One option is to use green or blue spectrums of light. However, it is understood that one may use any suitable light having a wavelength that is substantially or approximately within the green or blue spectra defined above, and the localization systems and methods described herein may use any suitable spectra of light.

[0177] Referring now to FIG. 1, shown therein is a view of an example of an ingestible device 100, which may be used to identify a location within a gastrointestinal (GI) tract. In some cases, the ingestible device 100 may be configured to autonomously determine whether it is located in the stomach, a particular portion of the small intestine such as a duodenum, jejunum, or ileum, or the large intestine by utilizing sensors operating with different wavelengths of light. Additionally, ingestible device 100 may be configured to autonomously determine whether it is located within certain portions of the small intestine or large intestine, such as the duodenum, the jejunum, the cecum, or the colon.

[0178] Ingestible device 100 may have a housing 102 shaped similar to a pill or capsule. The housing 102 of ingestible device 100 may have a first end portion 104, and a second end portion 106. The first end portion 104 may include a first wall portion 108, and second end portion 106 may include a second wall portion 110. In some cases, the first end portion 104 and second end portion 106 of ingestible device 100 may be manufactured separately, and may be affixed together by a connecting portion 112.

[0179] In some cases, the ingestible device 100 may include an optically transparent window 114. Optically transparent window 114 may be transparent to various types of illumination in the visible spectrum, infrared spectrum, or ultraviolet light spectrum, and ingestible device 100 may have various sensors and illuminators located within the housing 102, and behind the transparent window 114. This may allow ingestible device 100 to be configured to transmit illumination at different wavelengths through transparent window 114 to an environment external to housing 102 of ingestible device 100, and to detect a reflectance from a portion of the illumination that is reflected back through transparent window 114 from the environment external to housing 102. Ingestible device 100 may then use the detected level of reflectance in order to determine a location of ingestible device 100 within a GI tract. In some cases, the optically transparent window 114 may be of any shape and size, and may wrap around the circumference of ingestible device 100. In this case, ingestible device 100 may have multiple sets of sensors and illuminators positioned at different locations azimuthally behind window 114.

[0180] In some cases, the ingestible device 100 may optionally include an opening 116 in the second wall portion 110. In some cases, the second wall portion 110 may be configured to rotate around the longitudinal axis of ingestible device 100 (e.g., by means of a suitable motor or other actuator housed within ingestible device 100). This may allow ingestible device 100 to release a substance into the GI tract, through opening 116.

[0181] FIG. 2 shows an exploded view of ingestible device 100. In some cases, the ingestible device 100 may optionally include a rotation assembly 118. Optional rotation assembly 118 may include a motor 118-1 driven by a microcontroller (e.g., a microcontroller coupled to printed circuit board 120), a rotation position sensing ring 118-2, and a storage sub-unit 118-3 configured to fit snugly within the second end portion 104. In some cases, the rotation assembly 118 may cause second end portion 104, and opening 116, to rotate relative to the storage sub-unit 118-3. In some cases, there may be cavities on the side of storage sub-unit 118-3 that function as storage chambers. When the opening 116 is aligned with a cavity on the side of the storage sub-unit 118-3, the cavity on the side of the storage sub-unit 118-3 may be exposed to the environment external to the housing 102 of ingestible device 100. In some cases, the storage sub-unit 118-3 may be loaded with a medicament or other substance prior to the ingestible device 100 being administered to a subject. In this case, the medicament or other substance may be released from the ingestible device 100 by aligning opening 116 with the cavity within storage sub-unit 118-3. FIG. Other ingestible devices capable of releasing substances are discussed in commonly-assigned PCT Application WO/2013/120184 filed February 15, 2013, commonly-assigned U.S. Provisional publication US2018/0070857A1. It is understood that any suitable method of releasing substances may be incorporated into some of the examples of the ingestible devices disclosed herein, and that the systems and methods for determining a location of an ingestible device may be incorporated into any suitable type of ingestible device.

[0182] Ingestible device 100 may include a printed circuit board (PCB) 120, and a battery 128 configured to power PCB 120. PCB 120 may include a programmable microcontroller, and control and memory circuitry for holding and executing firmware or software for coordinating the operation of ingestible device 100, and the various components of ingestible device 100. For example, PCB 120 may include memory circuitry for storing data, such as data sets of measurements collected by sensing sub-unit 126, or instructions to be executed by control circuitry to implement a localization process, such as, for example, one or more of the processes, discussed herein, including those discussed below in connection with one or more of the associated flow charts. PCB 120 may include a detector 122 and an illuminator 124, which together form sensing sub-unit 126. In some cases, the control circuitry within PCB 120 may include processing units, communication circuitry, or any other suitable type of circuitry for operating ingestible device 100. For illustrative purposes, only a single detector 122 and a single illuminator 124 forming a single sensing sub-unit 126 are shown. However, it is understood that in some cases there may be multiple sensing sub-units, each with a separate illuminator and detector, within ingestible device 100. For example, there may be several sensing sub-units spaced azimuthally around the circumference of the PCB 120, which may enable ingestible device 100 to transmit illumination and detect

reflectances or ambient light in all directions around the circumference of the device. In some cases, the sensing sub-unit 126 may be configured to generate an illumination using illuminator 124, which is directed through the window 114 in a radial direction away from ingestible device 100. This illumination may reflect off of the environment external to ingestible device 100, and the reflected light coming back into ingestible device 100 through window 114 may be detected as a reflectance by detector 122.

[0183] In some cases, the window 114 may be of any suitable shape and size. For example, window 114 may extend around a full circumference of ingestible device 100. In some cases there may be a plurality of sensing sub-units (e.g., similar to sensing sub-unit 126) located at different positions behind the window. For example, three sensing sub-units may be positioned behind the window at the same longitudinal location, but spaced 120 degrees apart azimuthally. This may enable ingestible device 100 to transmit illuminations in all directions radially around ingestible device 100, and to measure each of the corresponding reflectances.

[0184] In some cases, the illuminator 124 may be capable of producing illumination at a variety of different wavelengths in the ultraviolet, infrared, or visible spectrum. For example, illuminator 124 may be implemented by using Red-Green-Blue Light-Emitting diode packages (RGB-LED). These types of RGB-LED packages are able to transmit red, blue, or green illumination, or combinations of red, blue, or green illumination. Similarly, detector 122 may be configured to sense reflected light of the same wavelengths as the illumination produced by illuminator 124. For example, if illuminator 124 is configured to produce red, blue, or green illumination, detector 122 may be configured to detect different reflectances produced by red, blue, or green illumination (e.g., through the use of an appropriately configured photodiode). These detected reflectances may be stored by ingestible device 100 (e.g., within memory circuitry of PCB 120), and may then be used by ingestible device 100 in determining a location of ingestible device 100 within the GI tract (e.g., through the use of process 500 (FIG. 5), process 600 (FIG. 6), or process 900 (FIG. 9)).

[0185] It is understood that ingestible device 100 is intended to be illustrative, and not limiting. It will be understood that modifications to the general shape and structure of the various devices and mechanisms described in relation to FIG. 1 and FIG. 2 may be made without significantly changing the functions and operations of the devices and mechanisms. For example, ingestible device 100 may have a housing formed from a single piece of molded plastic, rather than being divided into a first end portion 104 and a second end portion 106. As an alternate example, the location of window 114 within ingestible device 100 may be moved to some other location, such as the center of ingestible device 100, or to one of the ends of ingestible device 100. Moreover, the systems and methods discussed in relation to FIGS. 1-10 may be implemented on any suitable type of ingestible device, provided that the ingestible device is capable of detecting reflectances or levels of illumination in some capacity. For example, in some cases the ingestible device 100 may be modified to replace detector 122 with an image sensor, and the ingestible device may be configured to measure relative levels of red, blue, or green light by decomposing a recorded image into its individual spectral components. Other examples of ingestible devices with localization capabilities, which may be utilized in order to implement the systems and methods discussed in relation to FIG. 1-11, are discussed in co-owned PCT Application WO/2016/049602 filed on September 25, 2015.

[0186] FIG. 3 is a diagram of an ingestible device during an example transit through a gastrointestinal (GI) tract, in accordance with some aspects of the disclosure. Ingestible device 300 may include any portion of any other ingestible device discussed in this disclosure (e.g., ingestible device 100 (FIG. 1)), and may be any suitable type of ingestible device with localization capabilities. For example, ingestible device 300 may be one of an ingestible device 100 without the optional opening 116 (FIG. 1) or optional rotation assembly 118 (FIG. 2)). In some cases, the ingestible device 300 may be ingested by a subject, and as ingestible device 300 traverses the GI tract, ingestible device 300 may be configured to determine its location within the GI tract. For example, the movement of ingestible device 300 and the amount of light detected by ingestible device 300 (e.g., via detector 122 (FIG. 2)) may vary substantially depending on the location of ingestible device 300 within the GI tract, and ingestible device 300 may be configured to use this information to determine a location of ingestible device 300 within the GI tract. For instance, ingestible device 300 may detect ambient light from the surrounding environment, or reflectances based on illumination generated by ingestible device 300 (e.g., generated by illuminator 124 (FIG. 1)), and use this information to determine a location of ingestible device 300 through processes, such as described herein. The current location of ingestible device 300, and the time that ingestible device 300 detected each transition between the various portions of the GI tract, may then be stored by ingestible device 300 (e.g., in memory circuitry of PCB 120 (FIG. 2)), and may be used for any suitable purpose.

[0187] Shortly after ingestible device 300 is ingested, ingestible device will traverse the esophagus 302, which may connect the subject's mouth to a stomach 306. In some cases, the ingestible device 300 may be configured to determine that it has entered the esophagus portion GI tract by measuring the amount and type of light (e.g., via detector 122 (FIG. 2)) in the environment surrounding the ingestible device 300. For instance, ingestible device 300 may detect higher levels of light in the visible spectrum (e.g., via detector 122 (FIG. 2)) while outside the subject's body, as compared to the levels of light detected while within the GI tract. In some cases, the ingestible device 300 may have previously stored data (e.g., on memory circuitry of PCB 120 (FIG. 2)) indicating a typical level of light detected when outside of the body, and the ingestible device 300 may be configured to determine that entry to the body has occurred when a detected level

of light (e.g., detected via detector 122 (FIG. 2)) has been reduced beyond a threshold level (e.g., at least a 20-30% reduction) for a sufficient period of time (e.g., 5.0 seconds). In some cases, the ingestible device 100 may also be configured to monitor for one or more transitions. Such transitions can include an ileocecal transition from the ileum to the cecum, a transition from the cecum to the colon, or detect exit from the body (e.g., by measuring reflectances, temperature, or levels of ambient light).

[0188] FIG. 7 is a plot illustrating data collected during an example operation of an ingestible device (e.g., ingestible device 100, 300, or 400), which may be used when determining a location of an ingestible device as it transits through a gastrointestinal (GI) tract, in accordance with some aspects of the disclosure.

[0189] Although FIG. 7 may be described in connection with ingestible device 100 for illustrative purposes, this is not intended to be limiting, and plot 700 and data set 702 may be typical of data gathered by any device discussed in this application. Plot 700 depicts the ratios of the measured green reflectance levels to the measured blue reflectance levels over time. For example, ingestible device 100 may have computed the value for each point in the data set 702 by transmitting green and blue illumination at a given time (e.g., via illuminator 124 (FIG. 2)), measuring the resulting green and blue reflectances (e.g., via detector 122 (FIG. 2)), calculating the ratio of the resulting reflectances, and storing the ratio in the data set along with a timestamp indicating the time that the reflectances were gathered.

[0190] At 704, shortly after ingestible device 100 begins operation, ingestible device 100 determines that it has reached at least the stomach (e.g., as a result of making a determination similar to the determination discussed in relation to 506 in process 500 (FIG. 5)). Ingestible device 100 continues to gather additional measurements of green and blue reflectance levels, and at 706 ingestible device 100 determines that a pyloric transition has occurred from the stomach to the duodenum (e.g., as a result of making a determination similar to the determinations discussed in relation to 616-624 of process 600 (FIG. 6)). Notably, the values in data set 702 around 706 jump up precipitously, which is indicative of the higher ratios of measured green reflectance levels to measured blue reflectance levels typical of the duodenum.

[0191] The remainder of the data set 702 depicts the ratios of the measured green reflectance levels to the measured blue reflectance levels throughout the remainder of the GI tract. At 708, ingestible device 100 has reached the jejunum (e.g., as determined through measurements of muscle contractions, as discussed in relation to FIG. 9), and by 710, ingestible device 100 has reached the cecum. It is understood that, in some cases, the overall character and appearance of data set 702 changes within the small intestine (i.e., the duodenum, jejunum, and ileum) versus the cecum. Within the jejunum and ileum, there may typically be a wide variation in the ratios of the measured green reflectance levels to the measured blue reflectance levels, resulting in relatively noisy data with a high standard deviation. By comparison, within the cecum ingestible device 100 may measure a relatively stable ratio of the measured green reflectance levels to the measured blue reflectance levels. In some cases, the ingestible device 100 may be configured to determine transitions from the small intestine to the cecum based on these differences. For example, ingestible device 100 may compare recent windows of data to past windows of data, and detect a transition to the cecum in response to determining that the standard deviation of the ratios in the recent window of data is substantially less than the standard deviation of the ratios in the past window of data.

[0192] FIG. 8 is another plot illustrating data collected during an example operation of an ingestible device, which may be used when determining a location of an ingestible device as it transits through a gastrointestinal (GI) tract, in accordance with some aspects of the disclosure. Similar to FIG. 7, FIG. 8 may be described in connection with the ingestible device 100 for illustrative purposes. However, this is not intended to be limiting, and plot 800 and data set 802 may be typical of data gathered by any device discussed in this application.

[0193] At 804, shortly after ingestible device 100 begins operation, ingestible device 100 determines that it has reached at least the stomach (e.g., as a result of making a determination similar to the determination discussed in relation to 506 in process 500 (FIG. 5)). Ingestible device 100 continues to gather additional measurements of green and blue reflectance levels (e.g., via sensing sub-unit 126 (FIG. 2)), and at 806 ingestible device 100 determines that a pyloric transition has occurred from the stomach to the duodenum (e.g., as a result of making a determination similar to the determinations discussed in relation to 616-624 of process 600 (FIG. 6)). Notably, the values in data set 802 around 806 jump up precipitously, which is indicative of the higher ratios of measured green reflectance levels to measured blue reflectance levels typical of the duodenum, before falling shortly thereafter. As a result of the reduced values in data set 802, ingestible device 100 determines that a reverse pyloric transition has occurred from the duodenum back to the stomach at 808 (e.g., as a result of making a determination similar to the determinations discussed in relation to 610-612 of process 600 (FIG. 6)). At 810, as a result of the values in data set 802 increasing again, ingestible device 100 determines that another pyloric transition has occurred from the stomach to the duodenum, and shortly thereafter ingestible device 100 proceeds onwards to the jejunum, ileum, and cecum.

[0194] The remainder of the data set 802 depicts the ratios of the measured green reflectance levels to the measured blue reflectance levels throughout the remainder of the GI tract. Notably, at 812, ingestible device reaches the transition point between the ileum and the cecum. As discussed above in relation to FIG. 7, the transition to the cecum is marked by a reduced standard deviation in the ratios of measured green reflectances and measured blue reflectances over time, and ingestible device 100 may be configured to detect a transition to the cecum based on determining that the standard

deviation of a recent set of measurements is substantially smaller than the standard deviation of past measurements taken from the jejunum or ileum.

[0195] In some cases, the ingestible device (e.g., ingestible device 100, 300, or 400) may be configured to deliver a dispensable substance that is pre-stored within the ingestible device from the ingestible device into the cecum in response to identifying the change in the location of the ingestible device. For example, ingestible device 100 may have a dispensable substance pre-stored within the ingestible device 100 (e.g., within a storage chamber or cavity on optional storage sub-unit 118-3 (FIG. 2)), and ingestible device 100 may be configured to dispense the substance into the cecum (e.g., through the use of optional opening 116 and optional rotating assembly 118 (FIG. 2)) when the ingestible device 100 detects that the ingestible device 100 is located within the cecum.

[0196] In some cases, the ingestible device (e.g., ingestible device 100, 300, or 400) may be configured to perform an action based on the total number of detected muscle contractions. For example, ingestible device 100 may be configured to retrieve data indicative of the total number of muscle contractions (e.g., from memory circuitry of PCB 120 (FIG. 2)), and compare that to an expected number of muscle contractions in a healthy individual. In response, the ingestible device may dispense a substance into the cecum (e.g., through the use of optional opening 116 and optional rotating assembly 118 (FIG. 2)) As an example, ingestible device 100 may be configured to deliver a substance into the cecum (such as a medicament), in response to determining that the detected muscle contractions are inconsistent with a functioning GI tract in a healthy individual.

[0197] It will be understood that the steps and descriptions of the flowcharts of this disclosure, , are merely illustrative. Any of the steps and descriptions of the flowcharts, , may be modified, omitted, rearranged, performed in alternate orders or in parallel, two or more of the steps may be combined, or any additional steps may be added, without departing from the scope of the present disclosure. For example, the ingestible device 100 may calculate the mean and the standard deviation of multiple data sets in parallel (e.g., multiple data sets, each one corresponding to a different wavelength of reflectance or different sensing sub-unit used to detect the reflectance) in order to speed up the overall computation time.

[0198] FIG. 11 is a plot illustrating muscle contractions detected by an ingestible device over time, which may be used when determining a location of an ingestible device as it transits through a gastrointestinal (GI) tract, in accordance with some aspects of the disclosure. In some cases, the ingestible device 100 may be configured to detect muscle contractions, and store data indicative of when each muscle contraction is. Plot 1100 depicts the detected muscle contractions 1106 over time, with each muscle contraction being represented by a vertical line reaching from "0" to "1" on the y-axis.

[0199] At 1102, around the 10-minute mark, ingestible device 100 first enters the duodenum. Shortly thereafter, at 1108, ingestible device 100 begins to detect several muscle contractions 1106 in quick succession, which may be indicative of the strong peristaltic waves that form in the jejunum (e.g., jejunum 314 (FIG. 3)). Later, around 1110, ingestible device 100 continues to detect intermittent muscle contractions, which may be consistent with an ingestible device 100 within the ileum. Finally, at 1104, ingestible device 100 transitions out of the small intestine, and into the cecum. Notably, ingestible device 100 detects more frequent muscle contractions in the jejunum portion of the small intestine as compared to the ileum portion of the small intestine, and ingestible device 100 does not measure any muscle contractions after having exited the small intestine. In some cases, the ingestible device 100 may incorporate this information into a localization process. For example, ingestible device 100 may be configured to detect a transition from a jejunum to an ileum in response to determining that a frequency of detected muscle contractions (e.g., the number of muscle contractions measured in a given 10-minute window) has fallen below a threshold number.

[0200] As another example, ingestible device 100 may be configured to detect a transition from an ileum to a cecum in response to determining that no muscle contractions have been detected for a threshold period of time. It is understood that these examples are intended to be illustrative, and not limiting, and that measurements of muscle contractions may be combined with any of the other processes, systems, or methods discussed in this disclosure. FIG 14 is a flowchart 1400 for an exemplary process for determining a transition of the device from the ileum to the cecum. In general, the process involves detecting changes in the reflected optical signal (e.g., red light, blue light, green light, ratio of red light to green light, ratio of red light to blue light, and/or ratio of green light to blue light). In some cases, the process includes detecting changes in the ratio of reflected red light to reflected green light, and also detecting changes in the ratio of reflected green light to reflected blue light. Generally, in the process 1400, the sliding window analysis (first and second windows) discussed with respect to process 600 is continued.

[0201] Step 1410 includes setting a first threshold in a detected signal, e.g., ratio of detected red light to detected green light, and setting a second threshold for the coefficient of variation for a detected signal, e.g., the coefficient of variation for the ratio of detected green light to detected blue light. The first threshold can be set to a fraction (e.g., from 0.5 to 0.9, from 0.6 to 0.8) of the average signal (e.g., ratio of detected red light to detected green light) in the first window, or a fraction (e.g., from 0.4 to 0.8, from 0.5 to 0.7) of the mean difference between the detected signal (e.g., ratio of detected red light to detected green light) in the two windows. The second threshold can be set to 0.1 (e.g., 0.05, 0.02).

[0202] Step 1420 includes detecting the signals in the first and second windows that are to be used for comparing to the first and second thresholds.

[0203] Step 1430 includes comparing the detected signals to the first and second thresholds. If the corresponding

value is not below the first threshold or the corresponding value is not below the second threshold, then it is determined that the device has not left the ileum and entered the cecum, and the process returns to step 1420. If the corresponding value is below the first threshold and the corresponding value is below the second threshold, then it is determined that the device has left the ileum and entered the cecum, and the process proceeds to step 1440.

[0204] Step 1450 includes determining whether it is the first time that the device was determined to leave the ileum and enter the cecum. If it is the first time that the device was determined to leave the ileum and enter the cecum, then the process proceeds to step 1460. If it is not the first time that the device has left the ileum and entered the cecum, then the process proceeds to step 1470.

[0205] Step 1460 includes setting a reference signal. In this step the optical signal (e.g., ratio of detected red light to detected green light) as a reference signal.

[0206] Step 1470 includes determining whether the device may have left the cecum and returned to the ileum. The device is determined to have left the cecum and returned to the ileum if the corresponding detected signal (e.g., ratio of detected red light to detected green light) is statistically comparable to the reference signal (determined in step 1460) and the coefficient of variation for the corresponding detected signal (e.g., ratio of detected green light to detected blue light) exceeds the second threshold. If it is determined that the device may have left the cecum and returned to the ileum, the process proceeds to step 1480.

[0207] Step 1480 includes continuing to detect the relevant optical signals for a period of time (e.g., at least one minute, from five minutes to 15 minutes).

[0208] Step 1490 includes determining whether the signals determined in step 1480 indicate (using the methodology discussed in step 1470) that the device re-entered the ileum. If the signals indicate that the device re-entered the ileum, the process proceeds to step 1420. If the signals indicate that the device is in the cecum, the process proceeds to step 1492.

[0209] Step 1492 includes continuing to monitor the relevant optical signals for a period of time (e.g., at least 30 minutes, at least one hour, at least two hours).

[0210] Step 1494 includes determining whether the signals determined in step 1492 indicate (using the methodology discussed in step 1470) that the device re-entered the ileum. If the signals indicate that the device re-entered the ileum, the process proceeds to step 1420. If the signals indicate that the device is in the cecum, the process proceeds to step 1496.

[0211] At step 1496, the process determines that the device is in the cecum.

[0212] For illustrative purposes the disclosure focuses primarily on a number of different examples of an ingestible device, and methods for determining a location of an ingestible device within a GI tract. However, the possible ingestible devices that may be constructed are not limited to these examples, and variations in the shape and design may be made without significantly changing the functions and operations of the device. Similarly, the possible procedures for determining a location of the ingestible device within the GI tract are not limited to the specific procedures and disclosed (e.g., process 1400 (FIG. 14)) At least some of the elements of the ingestible device described herein which are implemented via software (e.g., software executed by control circuitry within PCB 120 (FIG. 2)) may be written in a high-level procedural language such as object oriented programming, a scripting language or both. Accordingly, the program code may be written in C, C++ or any other suitable programming language and may comprise modules or classes, as is known to those skilled in object oriented programming. Alternatively, or in addition, at least some of the elements of the of the ingestible device described herein that are implemented via software may be written in assembly language, machine language or firmware as needed. In either case, the language may be a compiled or an interpreted language.

[0213] At least some of the program code used to implement the ingestible device can be stored on a storage media or on a computer readable medium that is readable by a general or special purpose programmable computing device having a processor, an operating system and the associated hardware and software that is necessary to implement the functionality of at least one of the elements described herein. The program code, when read by the computing device, configures the computing device to operate in a new, specific and predefined manner in order to perform at least one of the methods described herein.

[0214] Furthermore, at least some of the programs associated with the systems, devices, and methods described herein are capable of being distributed in a computer program product comprising a computer readable medium that bears computer usable instructions for one or more processors. The medium may be provided in various forms, including non-transitory forms such as, but not limited to, one or more diskettes, compact disks, tapes, chips, and magnetic and electronic storage. In some cases, the medium may be transitory in nature such as, but not limited to, wire-line transmissions, satellite transmissions, internet transmissions (e.g. downloads), media, digital and analog signals, and the like. The computer useable instructions may also be in various formats, including compiled and non-compiled code.

[0215] The techniques described above can be implemented using software for execution on a computer. For instance, the software forms procedures in one or more computer programs that execute on one or more programmed or programmable computer systems (which may be of various architectures such as distributed, client/server, or grid) each including at least one processor, at least one data storage system (including volatile and non-volatile memory and/or

storage elements), at least one input device or port, and at least one output device or port.

[0216] The software may be provided on a storage medium, such as a CD-ROM, readable by a general or special purpose programmable computer or delivered (encoded in a propagated signal) over a communication medium of a network to the computer where it is executed. All of the functions may be performed on a special purpose computer, or using special-purpose hardware, such as coprocessors. The software may be implemented in a distributed manner in which different parts of the computation specified by the software are performed by different computers. Each such computer program is preferably stored on or downloaded to a storage media or device (e.g., solid state memory or media, or magnetic or optical media) readable by a general or special purpose programmable computer, for configuring and operating the computer when the storage media or device is read by the computer system to perform the procedures described herein. The inventive system may also be considered to be implemented as a computer-readable storage medium, configured with a computer program, where the storage medium so configured causes a computer system to operate in a specific and predefined manner to perform the functions described herein.

Methods and Mechanisms of Delivery

[0217] FIG. 16 provides an example mock-up diagram illustrating aspects of a structure of an ingestible device 1600 for delivering a dispensable substance, such as a formulation of a therapeutic agent described herein, according to some cases described herein. In some cases, the ingestible device 1600 may generally be in the shape of a capsule, a pill or any swallowable form that may be orally consumed by an individual. In this way, the ingestible device 1600 may be ingested by a patient and may be prescribed by healthcare practitioners and patients.

[0218] The ingestible device 1600 includes a housing 1601 that may take a shape similar to a capsule, a pill, and/or the like, which may include two ends 1602a-b. The housing 1601 may be designed to withstand the chemical and mechanical environment of the GI tract (e.g., effects of muscle contractile forces and concentrated hydrochloric acid in the stomach). A broad range of materials that may be used for the housing 1601. Examples of these materials include, but are not limited to, thermoplastics, fluoropolymers, elastomers, stainless steel and glass complying with ISO 10993 and USP Class VI specifications for biocompatibility; and any other suitable materials and combinations thereof.

[0219] In some cases, the wall of the housing 1601 may have a thickness of 0.5mm-1mm, which is sufficient to sustain an internal explosion (e.g., caused by hydrogen ignition or over pressure inside the housing).

[0220] The housing 1601 may or may not have a pH-sensitive enteric coating to detect or otherwise be sensitive to a pH level of the environment external to the ingestible device. As discussed elsewhere in the application in more detail, the ingestible device 1600 may additionally or alternatively include one more sensors, e.g., temperature sensor, optical sense.

[0221] The housing 1601 may be formed by coupling two enclosure portions together. The ingestible device 1600 may include an electronic component within the housing 1600. The electronic component may be placed proximally to an end 1602b of the housing, and includes a printed circuit board (PCB), a battery, an optical sensing unit, and/or the like.

[0222] The ingestible device 1600 further includes a gas generating cell 1603 that is configured to generate gas and thus cause an internal pressure within the housing 1601. In some cases, the gas generating cell may include or be connected to a separate channel or valve of the ingestible device such that gas may be release through the channel or valve to create a motion to alter the position of the ingestible device within the GI tract. Such gas release can also be used to position the ingestible device relative to the intestinal lining. In another cases, gas may be released through the separate channel or valve to alter the surface orientation of the intestinal tissue prior to delivery of the dispensable substance.

[0223] A traveling plunger 1604 may be placed on top of the gas generating cell 1603 within the housing 1601. The traveling plunger 1604 is a membrane that separates the gas generating cell 1603 and a storage reservoir that stores the dispensable substance 1605. In some cases, the traveling plunger 1604 may be a movable piston. In some cases, the traveling plunger 1604 may instead be a flexible membrane such as but not limited to a diaphragm. In some cases, the traveling plunger 1604, which may have the form of a flexible diaphragm, may be placed along an axial direction of the housing 1601, instead of being placed on top of the gas generating cell 1603. The traveling plunger or the membrane 1604 may move (when the membrane 1604 is a piston) or deform (when the membrane 1604 is a diaphragm) towards a direction of the end 1602a of the housing, when the gas generating cell 1603 generates gas to create an internal pressure that pushes the membrane 1604. In this way, the membrane or traveling plunger 1604 may push the dispensable substance 1605 out of the housing via a dispensing outlet 1607.

[0224] The housing 1601 may include a storage reservoir storing one or more dispensable substances 1605 adjacent to the traveling plunger 1604. The dispensable substance 1605 may be a therapeutic or medical agent that may take a form of a powder, a compressed powder, a fluid, a semi-liquid gel, or any other dispensable or deliverable form. The delivery of the dispensable substance 1605 may take a form such as but not limited to bolus, semi-bolus, continuous, burst drug delivery, and/or the like. In some cases, a single bolus is delivered to the cecum. In some cases, more than one bolus is released to the cecum. In some cases the release of more than one bolus is triggered according to a pre-

programmed algorithm. In some cases the release profile is continuous. In some cases the release profile is time-based. In some disclosures the release profile is location-based. In some cases, the amount delivered is based on the severity and/or extent of the disease in the following manner. In some embodiments, the JAK inhibitor is ustekinumab. In some embodiments, the JAK inhibitor is briakinumab. In some embodiments, the JAK inhibitor is guselkumab. In some em-
 5 bodiments, the JAK inhibitor is tildrakizumab. In some embodiments, the JAK inhibitor is brazikumab. In some embodiments, the JAK inhibitor is ustekinumab.

[0225] In some cases the dispensable substance is a small molecule therapeutic that is released in the cecum. Small molecules that are administered by typical oral routes are primarily absorbed in the small intestine, with much lower absorption taking place in the large intestine (outside of the rectum). Accordingly, an ingestible device that is capable
 10 of releasing a small molecule selectively in the cecum with resulting low systemic levels (even when high doses are used) is attractive for subjects with inflammatory bowel disease in the large intestine.

[0226] In some cases, the storage reservoir may include multiple chambers, and each chamber stores a different dispensable substance. For example, the different dispensable substances can be released at the same time via the dispensing outlet 1607. Alternatively, the multiple chambers may take a form of different layers within the storage reservoir
 15 such that the different dispensable substance from each chamber is delivered sequentially in an order. In one example, each of the multiple chambers is controlled by a separate traveling plunger, which may be propelled by gas generation. The electronic component may control the gas generating cell 1603 to generate gas to propel a specific traveling plunger, e.g., via a separate gas generation chamber, etc., to deliver the respective substance. In some cases, the content of the multiple chambers may be mixed or combined prior to release, for example, to activate the drug.

[0227] The ingestible device 1600 may include a dispensing outlet 1607 at one end 1602a of the housing 1601 to direct the dispensable substance 105 out of the housing. The dispensing outlet 1607 may include an exit valve, a slit or a hole, a jet injection nozzle with a syringe, and/or the like. When the traveling plunger 1604 moves towards the end
 20 1602a of the housing 1601, an internal pressure within the storage reservoir may increase and push the dispensing outlet to be open to let the dispensable substance 1605 be released out of the housing 1601.

[0228] In some cases, a pressure relief device 1606 may be placed within the housing 1601, e.g., at the end 1602a of the housing 1601.

[0229] In some cases, the housing 1601 may include small holes (e.g., with a diameter smaller than 2 mm), e.g., on the side of the housing 1601, or at the end 1602a to facilitate loading the dispensable substance into the storage reservoir.

[0230] In some cases, a feedback control circuit (e.g., a feedback resistor, etc.) may be added to send feedback from the gas generating cell 1603 to the electronic component such that when the internal pressure reaches a threshold level,
 30 the electronic component may control the gas generating cell 1603 to turn off gas generation, or to activate other safety mechanism (e.g., feedback-controlled release valve, etc.). For example, an internal pressure sensor may be used to measure the internal pressure within the ingestible device and generate feedback to the feedback control circuit.

[0231] FIG. 17 provides an example diagram illustrating aspects of a mechanism for a gas generating cell 1603 configured to generate a gas to dispense a substance, according to some cases described herein. As shown in FIG.
 35 17, the gas generating cell 1603 generates a gas 1611 which can propel the dispensable substance 1605 out of the dispensing outlet 1607. A variable resistor 1608 may be connected to a circuit with the gas generating cell 1603 such that the variable resistor 1608 may be used to control an intensity and/or an amount of gas 1611 (e.g., hydrogen) generated by the cell 1603. Specifically, the gas generating cell 1603 may be a battery form factor cell that is capable
 40 of generating hydrogen when a resistor is applied. In this way, as the gas generating cell 1603 only needs the use of a resistor only without any active power requirements, the gas generating cell 1603 may be integrated into an ingestible device such as a capsule with limited energy/power available. For example, the gas generating cell 1603 may be compatible with a capsule at a size of 26mm x 13mm or smaller.

[0232] In some cases, based on the elution rate of gas from the cell, and an internal volume of the ingestible device,
 45 it may take time to generate sufficient gas 1611 to deliver the substance 1605, and the time required may be 30 seconds or longer. For example, the time to generate a volume of hydrogen equivalent to 500 μ L of fluid would be approximately 5 minutes. A longer period of time may be needed based upon non-ideal conditions within the ingestible device, such as friction, etc. Thus, given that the production of gas (e.g., hydrogen) may take time, gas generation may need to start prior to the ingestible device arriving at the site of delivery to build pressure up within the device. The ingestible device
 50 may then need to know when it is approaching the site of delivery. For example, the device may start producing gas on an "entry transition," which is determined by temperature, so as to produce enough gas to be close to the pressure high enough to deliver the dispensable substance. The ingestible device may then only start producing gas again when it arrives at the site of delivery, which will cause the internal pressure within the ingestible device to reach a level required by the dispensing outlet to release the dispensable substance. Also, for regio- specific delivery, the ingestible device
 55 may estimate the time it takes to build up enough pressure to deliver the dispensable substance before the ingestible device arrives at a specific location, to activate gas generation.

[0233] The gas 1611 that may be generated for a continuous delivery of drug (e.g., 1cc H₂ in 4 hours, 16 breaths per minute at 0.5L tidal volume) may equate to 1 cc hydrogen in approximately 2000L of exhaled air, or approximately 0.5

ppm H₂, which is below physiologic values of exhaled hydrogen. Reducing this time to 10 minutes equates to approximately 13 ppm hydrogen. Thus, due to the length of intestine that may be covered during this time period, the ingestible device may possess a higher localized value than physiologic.

[0234] FIGs. 18 and 19, disclosed in US patent publication US2018/0070857A1, illustrates an example of an ingestible device for localized delivery of pharmaceutical compositions disclosed herein, in accordance with particular implementations. The ingestible device 1600 includes a piston or drive element 1634 to push for drug delivery, in accordance with particular implementations described herein. The ingestible device 1600 may have one or more batteries 1631 placed at one end 1602a of a housing 1601 to provide power for the ingestible device 1600. A printed circuit board (PCB) 1632 may be placed adjacent to a battery or other power source 1631, and a gas generating cell 1603 may be mounted on or above the PCB 1632. The gas generating cell 1603 may be sealed from the bottom chamber (e.g., space including 1631 and 1632) of the ingestible device 1600. A movable piston 1634 may be placed adjacent to the gas generating cell 1603. In this way, gas generation from the gas generating cell 1603 may propel a piston 1634 to move towards another end 1602b of the housing 1601 such that the dispensable substance in a reservoir compartment 1635 can be pushed out of the housing through a dispensing outlet 1607, e.g., the movement is shown at 1636, with the piston 1634 at a position after dispensing the substance. The dispensing outlet 1607 may comprise a plug. The reservoir compartment 1635 can store the dispensable substance (e.g., drug substance), or alternatively the reservoir compartment can house a storage reservoir 1661 which comprises the dispensable substance. The reservoir compartment 1635 or storage reservoir 1661 may have a volume of approximately 600 μ L or even more dispensable substance, which may be dispensed in a single bolus, or gradually over a period of time.

[0235] The battery cells 1631 may have a height of 1.65 mm each, and one to three batteries may be used. The height of the piston may be reduced with custom molded part for around 1.5mm to save space. If the gas generating cell 1603 is integrated with the piston 1634, the overall height of the PCB, batteries and gas generating cell in total can be reduced to around 5 mm, thus providing more space for drug storage. For example, for an ingestible device of 7.8 mm in length (e.g., from end 1602a to the other end 1602b), a reservoir compartment 1635 or a storage reservoir 1661 of approximately 600 μ L may be used for drug delivery. For another example, for an ingestible device of 17.5 mm in length, a reservoir compartment 1635 or a storage reservoir 1661 of approximately 1300 μ L may be used for drug release.

[0236] In some implementations, the reservoir 1635 or 1661 for storing a therapeutically effective amount of the JAK inhibitor forms at least a portion of the device housing 1601. The therapeutically effective amount of the JAK inhibitor can be stored in the reservoir 1635 or 1661 at a particular pressure, for example, determined to be higher than a pressure inside the GI tract so that once the reservoir 1635 or 1661 is in fluid communication with the GI tract, the JAK inhibitor is automatically released. In certain implementations, the reservoir compartment 1635 includes a plurality of chambers, and each of the plurality of the chambers stores a different dispensable substance or a different storage reservoir 1661.

[0237] In certain cases, the storage reservoir 1661 is a compressible component or has compressible side walls. In particular cases, the compressible component can be composed, at least in part, or coated (e.g., internally) with polyvinyl chloride (PVC), silicone, DEHP (di-2-ethylhexyl phthalate), Tyvek, polyester film, polyolefin, polyethylene, polyurethane, or other materials that inhibit the JAK inhibitor from sticking to the reservoir and provide a sterile reservoir environment for the JAK inhibitor. The storage reservoir 1661 can be hermetically sealed. The reservoir compartment 1635 or storage reservoir 1661 can be configured to store JAK inhibitor in quantities in the range of 0.01 mL - 2 mL, such as 0.05 mL - 2 mL, such as 0.05 mL - 2 mL, such as 0.6mL - 2 mL. In some disclosures, the storage reservoir 1661 is attachable to the device housing 1601, for example, in the reservoir compartment. Accordingly, the storage reservoir 1635 can be loaded with the JAK inhibitor prior to being positioned in and/or coupled to the ingestible device housing 1601. The ingestible device housing 1601 includes one or more openings configured as a loading port to load the dispensable substance into the reservoir compartment. In another case, the ingestible device housing 1601 includes one or more openings configured as a vent.

[0238] As noted above, in some cases, a storage reservoir (optionally, containing a JAK inhibitor, such as a therapeutically effective amount of JAK inhibitor) is attachable to an ingestible device. In general, in such cases the storage reservoir and ingestible device can be designed in any appropriate fashion so that the storage reservoir can attach to the ingestible device when desired. Examples of designs include a storage reservoir that fits entirely within the ingestible device (e.g., in the ingestible device so that the storage reservoir is sealed within the device at the time the device is ingested by a subject), a storage reservoir that fits partially within the ingestible device, and a storage reservoir that is carried by the housing of the device. In some cases, the storage reservoir snap fits with the ingestible device. In certain cases, the storage reservoir is friction fit with the ingestible device. In some cases, the storage reservoir is held together with the ingestible device via a biasing mechanism, such as one or more springs, one or more latches, one or more hooks, one or more magnets, and/or electromagnetic radiation. In certain cases, the storage reservoir can be a piercable member. In some cases, the ingestible device has a sleeve into which the storage reservoir securely fits. In some cases, the storage reservoir is disposed in/on a slidable track/groove so that it can move onto a piercing needle when delivery of the therapeutic agent is desired. In certain cases, the storage reservoir is made of a soft plastic coating, which is contacted with a needle at any orientation to deliver the therapeutic agent when desired. Generally, the storage reservoir

can be made of one or more appropriate materials, such as, for example, one or more plastics and/or one or more metals or alloys. Exemplary materials include silicone, polyvinyl chloride, polycarbonate and stainless steel. Optionally, the design may be such that the storage reservoir carries some or all of the electrical componentry to be used by the ingestible device. Although the foregoing discussion relates to one storage reservoir, it is to be understood that an ingestible device

5 can be designed to carry any desired number (e.g., two, three, four, five) storage reservoirs. Different storage reservoirs can have the same or different designs. In some cases, the ingestible device (when fully assembled and packaged) satisfies the regulatory requirements for marketing a medical device in one or more jurisdictions selected from the United States of America, the European Union or any member state thereof, Japan, China, Brazil, Canada, Mexico, Colombia,

10 Argentina, Chile, Peru, Russia, the UK, Switzerland, Norway, Turkey, Israel, any member state of the Gulf Cooperative Council, South Africa, India, Australia, New Zealand, South Korea, Singapore, Thailand, the Philippines, Malaysia, Viet Nam, Indonesia, Taiwan and Hong Kong.

[0239] In certain cases, the ingestible device housing 1601 includes one or more actuation systems (e.g., gas generating cell 1603) for pumping the JAK inhibitor from the reservoir 1635. In some cases, the actuation system can include a mechanical, electrical, electromechanical, hydraulic, and/or fluid actuation system. For example, a chemical actuation

15 means may use chemical reaction of mixing one or more reagents to generate a sufficient volume of gas to propel the piston or drive element 1634 for drug release. The actuation system can be integrated into the reservoir compartment 1635 or can be an auxiliary system acting on or outside of the reservoir compartment 1635. For example, the actuation system can include pumping system for pushing/pulling the JAK inhibitor out of the reservoir compartment 1635 or the actuation system can be configured to cause the reservoir compartment 1635 to change structurally so that the volume

20 inside of the reservoir compartment 1635 changes, thereby dispensing the JAK inhibitor from the reservoir compartment 1635. The actuation system can include an energy storage component such as a battery or a capacitor for powering the actuation system. The actuation system can be actuated via gas pressure or a system storing potential energy, such as energy from an elastic reservoir component being expanded during loading of the reservoir and after being positioned in the ingestible device housing 1601 being subsequently released from the expanded state when the ingestible device

25 housing is at the location for release within the cecum. In certain cases, the reservoir compartment 1635 can include a membrane portion, whereby the JAK inhibitor is dispensed from the reservoir compartment 1635 or storage reservoir 1661 via osmotic pressure.

[0240] In particular cases the storage reservoir 1661 is in a form of a bellow that is configured to be compressed via a pressure from the gas generating cell. The JAK inhibitor may be loaded into the bellow, which may be compressed

30 by gas generation from the gas generating cell or other actuation means to dispense the dispensable substance through the dispensing outlet 1607 and out of the housing 1601. In some cases, the ingestible device includes a capillary plate placed between the gas generating cell and the first end of the housing, and a wax seal between the gas generating cell and the reservoir, wherein the wax seal is configured to melt and the dispensable substance is pushed through the capillary plate by a pressure from the gas generating cell. The shape of the bellow may aid in controlled delivery. The

35 reservoir compartment 1635 includes a dispensing outlet, such as a valve or dome slit 1662 extending out of an end of the housing 1601, in accordance with particular implementations. Thus when the bellow is being compressed, the dispensable substance may be propelled out of the bellow through the valve or the dome slit.

[0241] In certain cases, the reservoir compartment 1635 includes one or more valves (e.g. a valve in the dispensing outlet 1607) that are configured to move or open to fluidly couple the reservoir compartment 1635 to the GI tract. In

40 certain cases, a housing wall of the housing 1601 can form a portion of the reservoir compartment 1635. In certain cases, the housing walls of the reservoir serve as a gasket. One or more of the one or more valves are positioned in the housing wall of the device housing 1601, in accordance with particular implementations. One or more conduits may extend from the reservoir 1635 to the one or more valves, in certain implementations.

[0242] In certain cases, a housing wall of the housing 1601 can be formed of a material that is configured to dissolve, for example, in response to contact at the disease site. In certain cases, a housing wall of the housing 1601 can be

45 configured to dissolve in response to a chemical reaction or an electrical signal. The one or more valves and/or the signals for causing the housing wall of the housing 1601 to dissolve or dissipate can be controlled by one or more processors or controllers positioned on PCB 1632 in the device housing 1601. The controller is communicably coupled to one or more sensors or detectors configured to determine when the device housing 1601 is in the cecum. The sensors

50 or detectors comprise a plurality of electrodes comprising a coating, in certain implementations. Releasing of the JAK inhibitor from the reservoir compartment 1635 is triggered by an electric signal from the electrodes resulting from the interaction of the coating with the one or more sites of disease site. The one or more sensors can include a chemical sensor, an electrical sensor, an optical sensor, an electromagnetic sensor, a light sensor, and/or a radiofrequency sensor.

[0243] In particular cases, the device housing 1601 can include one or more pumps configured to pump the therapeutically effective amount of the JAK inhibitor from the reservoir compartment 1635. The pump is communicably coupled

55 to the one or more controllers. The controller is configured to activate the pump in response to detection by the one or more detectors of the disease site and activation of the valves to allow the reservoir 1635 to be in fluid communication with the GI tract. The pump can include a fluid actuated pump, an electrical pump, or a mechanical pump.

[0244] FIG. 20 provides an example structural diagram having a flexible diaphragm 1665 that may deform towards the dispensing outlet 1607 when the gas generating cell 1603 generates gas. The dispensable substance may then be propelled by the deformed diaphragm out of the housing through the dispensing outlet 1607. The dispensing outlet 1607 shown at FIG. 20 is in the form of a ring valve, however, any outlet design can be applied.

[0245] In some cases, an ingestible device can have an umbrella-shaped exit valve structure as a dispensing outlet of the ingestible device. Optionally, an ingestible device can have a flexible diaphragm to deform for drug delivery, and/or an integrated piston and gas generating cell such that the gas generating cell is movable with the piston to push for drug delivery.

[0246] In some cases, when the gas generating cell generates gas to propel the piston to move towards the nozzle such that the dispensable substance can be pushed under the pressure to break a burst disc to be injected via the nozzle.

[0247] In some cases, an ingestible device has a jet delivery mechanism with enhanced usable volume of dispensable substance. For example, the nozzle may be placed at the center of the ingestible device, and gas channels may be placed longitudinally along the wall of the ingestible device to transport gas from the gas generating cell to propel the piston, which is placed at an end of the ingestible device. In certain embodiments, the reservoir is attachable to an ingestible device. In certain embodiments, the ingestible device comprises a housing and the reservoir is attachable to the housing.

[0248] Accordingly, in certain cases, provided herein is a JAK inhibitor for use in a method of treating a disease of the gastrointestinal tract as disclosed herein, wherein the JAK inhibitor is contained in a reservoir suitable for attachment to a device housing, and wherein the method comprises attaching the reservoir to the device housing to form the ingestible device, prior to orally administering the ingestible device to the subject.

[0249] In certain cases, provided herein is an attachable reservoir containing a JAK inhibitor for use in a method of treating a disease of the gastrointestinal tract, wherein the method comprises attaching the reservoir to a device housing to form an ingestible device and orally administering the ingestible device to a subject, wherein the JAK inhibitor is released by the device in the cecum of the subject wherein the site of disease is in the colon.

[0250] In certain cases, provided herein is an attachable reservoir containing a JAK inhibitor, wherein the reservoir is attachable to a device housing to form an ingestible device that is suitable for oral administration to a subject and that is capable of releasing the JAK inhibitor in the cecum of the subject wherein the site of disease is in the colon.

[0251] In particular implementation the ingestible device includes cameras (e.g., video cameras) that affords inspection of the entire GI tract without discomfort or the need for sedation, thus avoiding many of the potential risks of conventional endoscopy. Video imaging can be used to help determine one or more characteristics of the GI tract, including the location of disease (e.g., presence or location of inflamed tissue and/or lesions associated with inflammatory bowel disease). In some cases, the ingestible device 101 may comprise a camera for generating video imaging data of the GI tract which can be used to determine, among other things, the location of the device. Examples of video imaging capsules include Medtronic's PillCam™, Olympus' Endocapsule®, and IntroMedic's MicroCam™. For a review of imaging capsules, see Basar et al. "Ingestible Wireless Capsule Technology: A Review of Development and Future Indication" International Journal of Antennas and Propagation (2012); 1-14). Other imaging technologies implemented with the device 101 can include thermal imaging cameras, and those that employ ultrasound or Doppler principles to generate different images (see Chinese patent application CN104473611: "Capsule endoscope system having ultrasonic positioning function").

[0252] Ingestible devices can be equipped with sources for generating reflected light, including light in the Ultraviolet, Visible, Near-infrared and/or Mid-infrared spectrum, and the corresponding detectors for spectroscopy and hyperspectral imaging. Likewise, autofluorescence may be used to characterize GI tissue (e.g., subsurface vessel information), or low-dose radiation (see Check-Cap™) can be used to obtain 3D reconstructed images.

Device Components

[0253] An ingestible device may comprise a component made of a non-digestible material and contain the JAK inhibitor. In some embodiments, the material is plastic.

[0254] It is envisaged that the device is single-use. The device is loaded with a drug prior to the time of administration. In some embodiments, it may be preferred that there is provided a medicinal product comprising the device pre-filled with the drug.

Locomotion components

[0255] Ingestible devices can be active or passive, depending on whether they have controlled or non-controlled locomotion. Passive (non-controlled) locomotion is more commonly used among ingestible devices given the challenges of implementing a locomotion module. Active (controlled) locomotion is more common in endoscopic ingestible capsules. For example, a capsule may comprise a miniaturized locomotion system (internal locomotion). Internal locomotion mechanisms may employ independent miniaturized propellers actuated by DC brushed motors, or the use of water jets.

As an example, a mechanism may comprise flagellar or flap-based swimming mechanisms. As an example, a mechanism may comprise cyclic compression/extension shape-memory alloy (SMA) spring actuators and anchoring systems based on directional micro-needles. As an example, a mechanism may comprise six SMA actuated units, each provided with two SMA actuators for enabling bidirectional motion. As an example, a mechanism may comprise a motor adapted to electrically stimulating the GI muscles to generate a temporary restriction in the bowel.

[0256] As an example, a capsule may comprise a magnet and motion of the capsule is caused by an external magnetic field. For example, a locomotion system may comprise an ingestible capsule and an external magnetic field source. For example, the system may comprise an ingestible capsule and magnetic guidance equipment such as, for example, magnetic resonance imaging and computer tomography, coupled to a dedicated control interface.

In some cases drug release mechanisms may also be triggered by an external condition, such as temperature, pH, movement, acoustics, or combinations thereof.

[0257] An ingestible device can include an outlet port connected to the volume within housing of the ingestible device. The outlet port may provide a path for the gas to exit the ingestible device and be released into the environment surrounding the ingestible device. This may prevent pressure from building up within the housing of the ingestible device.

In some cases, an ingestible device does not include an outlet port, and the gas stays inside the volume of the ingestible device. In some cases, the outlet port may contain a gas permeable membrane, a one-way valve, a hydrophobic channel, or some other mechanism to avoid unwanted material, (e.g., fluids and solid particulates from within the GI tract), from entering the ingestible device through the outlet port.

Communication systems

[0258] An ingestible device may be equipped with a communication system adapted to transmit and/or receive data, including imaging and/or localization data. As an example, a communication system may employ radiofrequency transmission. Ingestible devices using radiofrequency communication are attractive because of their efficient transmission through the layers of the skin. This is especially true for low frequency transmission (UHF-433 ISM and lower, including the Medical Device Radio Communication Service band (MDRS) band 402-406MHz). In another possibility, acoustics are used for communications, including the transmission of data. For example, an ingestible capsule may be able to transmit information by applying one or more base voltages to an electromechanical transducer or piezoelectric (e.g., PZT, PVDF, etc.) device to cause the piezoelectric device to ring at particular frequencies, resulting in an acoustic transmission. A multi-sensor array for receiving the acoustic transmission may include a plurality of acoustic transducers that receive the acoustic transmission from a movable device such as an ingestible capsule as described in US Patent US8615284B2 filed September 6, 2007.

[0259] As an example, a communication system may employ human body communication technology. Human body communication technology uses the human body as a conductive medium, which generally requires a large number of sensor electrodes on the skin. As an example, a communication system may integrate a data storage system.

Environmental Sensors

[0260] In some cases the device may comprise environmental sensors to measure pH, temperature, transit times, or combinations thereof. Other examples of environmental sensors include, but are not limited to a capacitance sensor, an impedance sensor, a heart rate sensor, acoustic sensor such as a microphone or hydrophone, image sensor, and/or a movement sensor. In one aspect, the ingestible device comprises a plurality of different environmental sensors for generating different kinds of environmental data.

[0261] In order to avoid the problem of capsule retention, a thorough past medical and surgical history should be undertaken. In addition, several other steps have been proposed, including performing investigations such as barium follow-through. In cases where it is suspected that there is a high risk of retention, the patient is given a patency capsule a few days before swallowing an ingestible device. Any dissolvable non-endoscopic capsule may be used to determine the patency of the GI tract. The patency capsule is usually the same size as the ingestible device and can be made of cellophane. In some cases, the patency capsule contains a mixture of barium and lactose, which allows visualization by x-ray. The patency capsule may also include a radiotag or other label, which allows for it to be detected by radio-scanner externally. The patency capsule may comprise wax plugs, which allow for intestinal fluid to enter and dissolve the content, thereby dividing the capsule into small particles.

[0262] Accordingly, in some cases, the methods herein comprise (a) identifying a subject having a disease of the gastrointestinal tract and (b) evaluating the subject for suitability to treatment. In some cases, the methods herein comprise evaluating for suitability to treatment a subject identified as having a disease of the gastrointestinal tract. In some cases, evaluating the subject for suitability to treatment comprises determining the patency of the subject's GI tract.

[0263] In some cases, the ingestible device contains an electric energy emitting means, a radio signal transmitting means, a medicament storage means and a remote actuatable medicament releasing means. The capsule signals a

remote receiver as it progresses through the alimentary tract in a previously mapped route and upon reaching the cecum is remotely triggered to release a dosage of medicament. Accordingly, in some cases, releasing the JAK inhibitor is triggered by a remote electromagnetic signal.

[0264] In some cases, the ingestible device includes a housing introducible into a body cavity and of a material insoluble in the body cavity fluids, but formed with an opening covered by a material which is soluble in body cavity fluids. A diaphragm divides the interior of the housing into a medication chamber including the opening, and a control chamber. An electrolytic cell in the control chamber generates a gas when electrical current is passed therethrough to deliver medication from the medication chamber through the opening into the body cavity at a rate controlled by the electrical current. Accordingly, in some cases, releasing the JAK inhibitor is triggered by generation in the composition of a gas in an amount sufficient to expel the JAK inhibitor.

[0265] In some cases, the ingestible device includes an oral drug delivery device having a housing with walls of water permeable material and having at least two chambers separated by a displaceable membrane. The first chamber receives drug and has an orifice through which the drug is expelled under pressure. The second chamber contains at least one of two spaced apart electrodes forming part of an electric circuit which is closed by the ingress of an aqueous ionic solution into the second chamber. When current flows through the circuit, gas is generated and acts on the displaceable membrane to compress the first chamber and expel the active ingredient through the orifice for progressive delivery to the gastrointestinal tract.

[0266] In some cases, the ingestible device includes an ingestible device for delivering a substance to a chosen location in the GI tract of a mammal includes a receiver of electromagnetic radiation for powering an openable part of the device to an opened position for dispensing of the substance. The receiver includes a coiled wire that couples the energy field, the wire having an air or ferrite core. Also disclosed is an apparatus for generating the electromagnetic radiation, the apparatus including one or more pairs of field coils supported in a housing. The device optionally includes a latch defined by a heating resistor and a fusible restraint. The device may also include a flexible member that may serve one or both the functions of activating a transmitter circuit to indicate dispensing of the substance; and restraining of a piston used for expelling the substance.

[0267] In some cases, the ingestible device includes an ingestible device for delivering a substance to the cecum of a mammal includes a receiver of electromagnetic radiation for powering an openable part of the device to an opened position for dispensing of the substance. The receiver includes a coiled wire that couples the energy field, the wire having an air or ferrite core. A further aspect of the disclosure includes an apparatus for generating the electromagnetic radiation, the apparatus including one or more pairs of field coils supported in a housing. The device optionally includes a latch defined by a heating resistor and a fusible restraint. The device may also include a flexible member that may serve one or both the functions of activating a transmitter circuit to indicate dispensing of the substance; and restraining of a piston used for expelling the substance.

[0268] In some cases, the ingestible device is a device a swallowable capsule. A sensing module is disposed in the capsule. A bioactive substance dispenser is disposed in the capsule. A memory and logic component is disposed in the capsule and in communication with the sensing module and the dispenser.

In some cases, the ingestible device includes electronic control means for dispensing the drug substantially to the cecum, according to a pre-determined drug release profile obtained prior to administration from the specific mammal. Accordingly, in some cases, releasing the JAK inhibitor is triggered by an electromagnetic signal generated within the device. The releasing may occur according to a pre-determined drug release profile.

[0269] In some cases, the ingestible device can include at least one guide tube, one or more tissue penetrating members positioned in the guide tube, a delivery member, an actuating mechanism and a release element. The release element degrades upon exposure to various conditions in the intestine so as to release and actuate the actuating mechanism. These are particularly useful for the delivery of drugs which are poorly absorbed, tolerated and/or degraded within the GI tract.

[0270] In some cases, the ingestible device includes an electronic pill comprising at least one reservoir with a solid powder or granulate medicament or formulation, a discharge opening and an actuator responsive to control circuitry for displacing medicine from the reservoir to the discharge opening. The medicament or formulation comprises a dispersion of one or more active ingredients--e.g., solids in powder or granulate form--in an inert carrier matrix. Optionally, the active ingredients are dispersed using intestinal moisture absorbed into the pill via a semipermeable wall section.

[0271] In some cases, the ingestible device includes a sensor comprising a plurality of electrodes having a miniature size and a lower power consumption and a coating exterior to the electrodes, wherein the coating interacts with a target condition thereby producing a change in an electrical property of the electrodes, wherein the change is transduced into an electrical signal by the electrodes. Accordingly, in some cases, releasing the JAK inhibitor is triggered by an electric signal by the electrodes resulting from the interaction of the coating with the one or more sites of disease. Further provided herein is a system for medication delivery comprising such sensor and a pill.

[0272] In some cases, the ingestible device includes an electronic pill comprising a plurality of reservoirs, each of the reservoirs comprising a discharge opening covered by a removable cover. The pill comprises at least one actuator

responsive to control circuitry for removing the cover from the discharge opening. The actuator can for example be a spring loaded piston breaking a foil cover when dispensing the medicament. Alternatively, the cover can be a rotatable disk or cylinder with an opening which can be brought in line with the discharge opening of a reservoir under the action of the actuator.

[0273] In some cases, the ingestible device includes an electronically and remotely controlled pill or medicament delivery system. The pill includes a housing; a reservoir for storing a medicament; an electronically controlled release valve or hatch for dispensing one or more medicaments stored in the reservoir while traversing the gastrointestinal tract; control and timing circuitry for opening and closing the valve; and a battery. The control and timing circuitry opens and closes the valve throughout a dispensing time period in accordance with a preset dispensing timing pattern which is programmed within the control and timing circuitry. RF communication circuitry receives control signals for remotely overriding the preset dispensing timing pattern, reprogramming the control and timing circuitry or terminating the dispensing of the medicament within the body. The pill includes an RFID tag for tracking, identification, inventory and other purposes.

[0274] In some cases, the ingestible device includes an electronic capsule which has a discrete drive element comprising: a housing, electronics for making the electronic capsule operable, a pumping mechanism for dosing and displacing a substance, a power source for powering the electronic capsule and enabling the electronics and the pumping mechanism to operate, and a locking mechanism; and a discrete payload element comprising: a housing, a reservoir for storing the substance, one or more openings in the housing for releasing the substance from the reservoir and a locking mechanism for engaging the drive element locking mechanism. Engagement of the drive element locking mechanism with the payload element locking mechanism secures the drive element to the payload element, thereby making the electronic capsule operable and specific. In some cases, the ingestible device may be a mucoadhesive device configured for release of an active agent, i.e. an anti-JAK inhibitor.

[0275] In one aspect of the disclosure the ingestible device may also include one or more environmental sensors. Environmental sensor may be used to generate environmental data for the environment external to device in the gastrointestinal (GI) tract of the subject. In some cases, environmental data is generated at or near the location within the GI tract of the subject where a drug is delivered. Examples of environmental sensor include, but are not limited to a capacitance sensor, a temperature sensor, an impedance sensor, a pH sensor, a heart rate sensor, acoustic sensor, image sensor (e.g., a hydrophone), and/or a movement sensor (e.g., an accelerometer). In one cases, the ingestible device comprises a plurality of different environmental sensors for generating different kinds of environmental data.

[0276] In one cases, the image sensor is a video camera suitable for obtaining images *in vivo* of the tissues forming the GI tract of the subject. In one cases, the environmental data is used to help determine one or more characteristics of the GI tract, including the location of disease (e.g., presence or location of inflamed tissue and/or lesions associated with inflammatory bowel disease). In some cases, the ingestible device may comprise a camera for generating video imaging data of the GI tract which can be used to determine, among other things, the location of the device.

[0277] In another cases, the ingestible device described herein may be localized using a gamma scintigraphy technique or other radio-tracker technology as employed by Phaeton Research's Enterion™ capsule (See Teng, Renli, and Juan Maya. "Absolute bioavailability and regional absorption of ticagrelor in healthy volunteers." *Journal of Drug Assessment* 3.1 (2014): 43-50), or monitoring the magnetic field strength of permanent magnet in the ingestible device (see T. D. Than, et al., "A review of localization systems for robotic endoscopic capsules," *IEEE Trans. Biomed. Eng.*, vol. 59, no. 9, pp. 2387-2399, Sep. 2012).

[0278] In one cases, the one or more environmental sensors measure pH, temperature, transit times, or combinations thereof.

[0279] In some cases, releasing the JAK inhibitor is dependent on the pH at or in the vicinity of the location.

[0280] In some cases, releasing the JAK inhibitor is not dependent on the pH at or in the vicinity of the location. In some disclosures, releasing the JAK inhibitor is triggered by degradation of a release component located in the capsule. In some cases, the JAK inhibitor is not triggered by degradation of a release component located in the capsule. In some disclosures, wherein releasing the JAK inhibitor is not dependent on enzymatic activity at or in the vicinity of the location. In some cases, releasing the JAK inhibitor is not dependent on bacterial activity at or in the vicinity of the location.

[0281] In any ingestible device disclosed herein, the JAK inhibitor is present in a therapeutically effective amount.

Locations of treatment

[0282] The JAK inhibitor is delivered at a location in the cecum of the subject. In some embodiments, the location is in the proximal portion of the cecum. In some embodiments, the location is in the distal portion of the cecum.

[0283] The JAK inhibitor is delivered at a location in the cecum of the subject and is not delivered at other locations in the gastrointestinal tract. In some embodiments, the JAK inhibitor is delivered at a location in the distal portion of the cecum of the subject and is not delivered at other locations in the gastrointestinal tract, wherein a site of disease is in the cecum and/or ascending colon, and no site of disease is present at other locations in the gastrointestinal tract.

[0284] The site of disease is in the colon and the JAK inhibitor is released in the cecum. In some cases, a site of disease is in the ascending colon and the JAK inhibitor is released in the cecum.

[0285] In some cases the subject is diagnosed with colitis throughout the colon and the JAK inhibitor is released (a) in the cecum. In some cases, the JAK inhibitor is delivered 150 cm or less from the one or more sites of disease. In some cases, the JAK inhibitor is delivered 125 cm or less from the one or more sites of disease. In some cases the JAK inhibitor is delivered 100 cm or less from the one or more sites of disease. In some cases, the JAK inhibitor is delivered 50 cm or less from the one or more sites of disease. In some cases, the JAK inhibitor is delivered 40 cm or less from the one or more sites of disease. In some cases, the JAK inhibitor is delivered 30 cm or less from the one or more sites of disease. In some cases, the JAK inhibitor is delivered 20 cm or less from the one or more sites of disease. In some cases, the JAK inhibitor is delivered 10 cm or less from the one or more sites of disease. In some cases, the JAK inhibitor is delivered 5 cm or less from the one or more sites of disease. In some cases, the JAK inhibitor is delivered 2 cm or less from the one or more sites of disease. In some cases, the method further comprises using an ingestible device to deliver the JAK inhibitor and using localization methods disclosed herein (e.g., such as discussed in Example 13 below) to determine the location of the ingestible device within the GI tract (e.g., relative to the site of disease). In some cases, the method further comprises using an ingestible device to deliver the JAK inhibitor and determining the period of time since the ingestible device was ingested to determine the location of the ingestible device within the GI tract (e.g., relative to the site of disease). In some cases, the method further comprises identifying the one or more sites of disease by a method comprising imaging of the gastrointestinal tract. In some cases, imaging of the gastrointestinal tract comprises video imaging. In some cases, imaging of the gastrointestinal tract comprises thermal imaging. In some cases, imaging of the gastrointestinal tract comprises ultrasound imaging. In some cases, imaging of the gastrointestinal tract comprises Doppler imaging. In some cases, the at least 80%, at least 90%, at least 95%, at least 96%, at least 97%, or at least 98% of the JAK inhibitor is delivered 150 cm or less from the one or more sites of disease. In some cases, the at least 80%, at least 90%, at least 95%, at least 96%, at least 97%, or at least 98% of the JAK inhibitor is delivered 125 cm or less from the one or more sites of disease. In some cases, the at least 80%, at least 90%, at least 95%, at least 96%, at least 97%, or at least 98% of the JAK inhibitor is delivered 100 cm or less from the one or more sites of disease. In some cases, the at least 80%, at least 90%, at least 95%, at least 96%, at least 97%, or at least 98% of the JAK inhibitor is delivered 50 cm or less from the one or more sites of disease. In some cases, the at least 80%, at least 90%, at least 95%, at least 96%, at least 97%, or at least 98% of the JAK inhibitor is delivered 40 cm or less from the one or more sites of disease. In some cases, the at least 80%, at least 90%, at least 95%, at least 96%, at least 97%, or at least 98% of the JAK inhibitor is delivered 30 cm or less from the one or more sites of disease. In some cases, the at least 80%, at least 90%, at least 95%, at least 96%, at least 97%, or at least 98% of the JAK inhibitor is delivered 20 cm or less from the one or more sites of disease. In some cases, the at least 80%, at least 90%, at least 95%, at least 96%, at least 97%, or at least 98% of the JAK inhibitor is delivered 10 cm or less from the one or more sites of disease. In some cases, the at least 80%, at least 90%, at least 95%, at least 96%, at least 97%, or at least 98% of the JAK inhibitor is delivered 5 cm or less from the one or more sites of disease. In some cases, the at least 80%, at least 90%, at least 95%, at least 96%, at least 97%, or at least 98% of the JAK inhibitor is delivered 2 cm or less from the one or more sites of disease. In some cases, the method further comprises using an ingestible device to deliver the JAK inhibitor and using localization methods disclosed herein (e.g., such as discussed in Example 13 below) to determine the location of the ingestible device within the GI tract (e.g., relative to the site of disease). In some cases, the amount of JAK inhibitor that is delivered is a Human Equivalent Dose. In some cases, the JAK inhibitor is delivered to the location by mucosal contact.

[0286] In some examples where the JAK inhibitor is an antibody or an antigen-binding fragment thereof (e.g., any of the antibodies or antigen-binding antibody fragments described herein) are administered to a subject using any of the compositions or devices described herein, the antibody or antigen-binding antibody fragment can penetrate the GI tissue of the subject. As used herein, "GI tissue" refers to tissue in the gastrointestinal (GI) tract, such as tissue in one or more of duodenum, jejunum, ileum, cecum, ascending colon, transverse colon, descending colon, sigmoid colon, and rectum. In one particular cases, GI tissue refers to tissue in the proximal portion of one or more of duodenum, jejunum, ileum, cecum, ascending colon, transverse colon, descending colon, and sigmoid colon. In one particular cases, GI tissue refers to tissue in the distal portion of one or more of duodenum, jejunum, ileum, cecum, ascending colon, transverse colon, descending colon, and sigmoid colon. The GI tissue may be, for example, GI tissue proximate to one or more sites of disease. In some cases the antibody or antigen-binding antibody fragment can penetrate the cecum tissue proximate to one or more sites of disease. For example, an antibody or antigen-binding fragment thereof (e.g., a F(ab')₂, a Fv, or a scFv) can penetrate one or more (e.g., two, three, or four) of the lumen/superficial mucosa, the lamina propria, the submucosa, and the tunica muscularis/serosa. In some disclosures, any of the devices or compositions described herein can release a recombinant antibody (e.g., a humanized or fully human antibody, e.g., human or humanized IgG1, human or humanized IgG2, human or humanized IgG3, human or humanized IgG4, human or humanized IgA1, human or humanized IgA2, human or humanized IgD, human or humanized IgE, or human or humanized IgM), which is degraded into an antigen-binding antibody fragment (e.g., a Fab, a Fv, or a F(ab')₂), which in turn is able to penetrate GI tissue (e.g., one or more (e.g., two, three, or four) of the lumen/superficial mucosa, the lamina propria, the submucosa, and

the tunica muscularis/serosa) of the subject. In some cases, the device releases an antigen-binding antibody fragment (e.g., any of the antigen-binding antibody fragments described herein).

[0287] In some examples, administration of an antibody or an antigen-binding fragment thereof using any of the compositions or devices described herein results in penetration (e.g., a detectable level of penetration) of GI tissue (e.g., one or more (e.g., two, three, or four) of the lumen/superficial mucosa, the lamina propria, the submucosa, and the tunica muscularis/serosa) within a time period of about 10 minutes to about 10 hours. Penetration of GI tissue by an antibody or an antigen-binding antibody fragment can be detected by administering a labeled antibody or labeled antigen-binding antibody fragment, and performing imaging on the subject (e.g., ultrasound, computed tomography, or magnetic resonance imaging). For example, the label can be a radioisotope, a heavy metal, a fluorophore, or a luminescent agent (e.g., any suitable radioisotopes, heavy metals, fluorophores, or luminescent agents used for imaging known in the art).

[0288] While not wishing to be bound to a particular theory, the inventors contemplate that at or near the site of release a concentration gradient of the JAK inhibitor is generated in the mucosa, and that administration of an JAK inhibitor using a device as described herein advantageously results in a "reverse" concentration gradient when compared to the concentration gradient resulting from systemic administration. In such "reverse" concentration gradient, the drug concentration is highest from superficial to deep with respect to the mucosal surface. Systemic administration instead typically results in concentrations of the drug being highest from deep to superficial. A "reverse" concentration gradient as described above aligns more favorably with the pathophysiology of IBD.

[0289] In some cases, administration of an antibody or an antigen-binding antibody fragment can provide for treatment (e.g., a reduction in the number, severity, and/or duration of one or more symptoms of any of the disorders described herein in a subject) for a time period of between about 1 hour to about 30 days in a subject following first administration of an antibody or antigen-binding antibody fragment using any of the compositions or devices described herein. Non-limiting examples of symptoms of a disease described herein are described below. For example, treatment can result in a decrease (e.g., about 1% to about 99% decrease) in one or more (e.g., two, three, four, five, six, seven, eight, or nine) of: the level of interferon- γ in GI tissue, the level of IL-1 β in GI tissue, the level of IL-6 in GI tissue, the level of IL-22 in GI tissue, the level of IL-17A in the GI tissue, the level of TNF α in GI tissue, the level of IL-2 in GI tissue, and endoscopy score in a subject (e.g., as compared to the level in the subject prior to treatment or compared to a subject or population of subjects having a similar disease but receiving a placebo or a different treatment) (e.g., for a time period of between about 1 hour to about 30 days (e.g., or any of the subranges herein) following the first administration of an antibody or antigen-binding antibody fragment using any of the compositions or devices described herein. Exemplary methods for determining the endoscopy score are described herein and other methods for determining the endoscopy score are known in the art. Exemplary methods for determining the levels of interferon- γ , IL-1, IL-6, IL-22, IL-17A, TNF α , and IL-2 are described herein. Additional methods for determining the levels of these cytokines are known in the art. In some examples, treatment can result in an increase (e.g., about 1% to about 500% increase) in one or both of stool consistency score and weight of a subject (e.g., as compared to the level in the subject prior to treatment or compared to a subject or population of subjects having a similar disease but receiving a placebo or a different treatment) (e.g., for a time period of between about 1 hour to about 30 days (e.g., or any of the subranges herein) following the first administration of an antibody or antigen-binding antibody fragment using any of the compositions or devices described herein. Exemplary methods for determining stool consistency score are described herein. Additional methods for determining a stool consistency score are known in the art.

[0290] In some examples, administration of an antibody or an antigen-binding antibody fragment using any of the devices or compositions described herein can result in a ratio of GI tissue concentration of the antibody or the antigen-binding antibody fragment to the blood, serum, or plasma concentration of the antibody or the antigen-binding antibody fragment of, e.g., about 2.8 to about 6.0.

[0291] Some examples of any of the methods described herein can, e.g., result in a selective suppression of a local inflammatory response (e.g., an inflammatory response in local GI tissue), while maintaining the systemic immune response (e.g., blood). The GI tissue may be, for example, GI tissue proximate to one or more sites of disease. As used herein, "GI content" refers to the content of the gastrointestinal (GI) tract, such as the content of one or more of duodenum, jejunum, ileum, cecum, ascending colon, transverse colon, descending colon, sigmoid colon, and rectum, more particularly of the proximal portion of one or more of duodenum, jejunum, ileum, cecum, ascending colon, transverse colon, descending colon, and sigmoid colon, or of the distal portion of one or more of duodenum, jejunum, ileum, cecum, ascending colon, transverse colon, descending colon, and sigmoid colon. Accordingly, in some cases, the methods described herein can result in a selective suppression of the inflammatory response in the duodenum tissue proximate to one or more sites of disease, while maintaining the systemic immune response. In some cases, the methods described herein can result in a selective suppression of the inflammatory response in the jejunum tissue proximate to one or more sites of disease, while maintaining the systemic immune response. In some cases, the methods described herein can result in a selective suppression of the inflammatory response in the ileum tissue proximate to one or more sites of disease, while maintaining the systemic immune response. In some cases, the methods described herein can result in a selective suppression of the inflammatory response in the cecum tissue proximate to one or more sites of disease,

while maintaining the systemic immune response. In some cases, the methods described herein can result in a selective suppression of the inflammatory response in the ascending colon tissue proximate to one or more sites of disease, while maintaining the systemic immune response. In some cases, the methods described herein can result in a selective suppression of the inflammatory response in the transverse colon tissue proximate to one or more sites of disease, while maintaining the systemic immune response. In some cases, the methods described herein can result in a selective suppression of the inflammatory response in the descending colon tissue proximate to one or more sites of disease, while maintaining the systemic immune response. In some cases, the methods described herein can result in a selective suppression of the inflammatory response in the sigmoid colon tissue proximate to one or more sites of disease, while maintaining the systemic immune response. In some examples, the methods described herein can result in a 1% increase to 500% in one or more (e.g., two, three, four, five, six, seven, eight, nine, or ten) of: the plasma, serum, or blood level of IL-6; the plasma, serum, or blood level of IL-2; the plasma, serum, or blood level of IL-1 β ; the plasma, serum, or blood level of TNF α ; the plasma, serum, or blood level of IL-17A; the plasma, serum, or blood level of IL-22; the plasma, serum, or blood level of interferon- γ ; the level of blood Th memory cells (CD44⁺CD45RB-CD4⁺ cells); and the level of α 4 β 7 expression in blood cells; e.g., each as compared to the corresponding level in a subject systemically administered the same dose of the same JAK inhibitor. Methods for determining the plasma, serum, or blood level of IL-6; the plasma, serum, or blood level of IL-2; the plasma, serum, or blood level of IL-1 β ; the plasma, serum, or blood level of TNF α ; the plasma, serum, or blood level of IL-17A; the plasma, serum, or blood level of IL-22; the plasma, serum, or blood level of interferon-K; the level of blood Th memory cells (CD44⁺CD45RB-CD4⁺ cells); and the level of α 4 β 7 expression in blood cells are known in the art.

[0292] In some examples of any of the methods described herein can result, e.g., in a 1% to 99% decrease (or any of the subranges of this range described herein) in one or more (e.g., two, three, four, five, six, or seven) of: the level of interferon- γ in GI tissue or GI content; the level of IL-1 β in GI tissue or GI content; the level of IL-6 in GI tissue or GI content; the level of IL-22 in GI tissue or GI content; the level of IL-17A in GI tissue or GI content; the level of TNF α in GI tissue or GI content; and the level of IL-2 in GI tissue or GI content, e.g., as compared to the corresponding level in a subject not administered a treatment, or not administered a JAK inhibitor locally as disclosed herein. Accordingly, in some cases, the methods described herein can result, e.g., in a 1% to 99% decrease (or any of the subranges of this range described herein) in one or more (e.g., two, three, four, five, six, or seven) of the level of interferon- γ ; the level of IL-1 β ; the level of IL-6; the level of IL-22; the level of IL-17A; the level of TNF α ; and the level of IL-2, in the duodenum tissue proximate to one or more sites of disease. Accordingly, in some cases, the methods described herein can result, e.g., in a 1% to 99% decrease (or any of the subranges of this range described herein) in one or more (e.g., two, three, four, five, six, or seven) of the level of interferon- γ ; the level of IL-1 β ; the level of IL-6; the level of IL-22; the level of IL-17A; the level of TNF α ; and the level of IL-2, in the ileum tissue proximate to one or more sites of disease. Accordingly, in some cases, the methods described herein can result, e.g., in a 1% to 99% decrease (or any of the subranges of this range described herein) in one or more (e.g., two, three, four, five, six, or seven) of the level of interferon- γ ; the level of IL-1 β ; the level of IL-6; the level of IL-22; the level of IL-17A; the level of TNF α ; and the level of IL-2, in the jejunum tissue proximate to one or more sites of disease. Accordingly, in some cases, the methods described herein can result, e.g., in a 1% to 99% decrease (or any of the subranges of this range described herein) in one or more (e.g., two, three, four, five, six, or seven) of the level of interferon- γ ; the level of IL-1 β ; the level of IL-6; the level of IL-22; the level of IL-17A; the level of TNF α ; and the level of IL-2, in the cecum tissue proximate to one or more sites of disease. Accordingly, in some cases, the methods described herein can result, e.g., in a 1% to 99% decrease (or any of the subranges of this range described herein) in one or more (e.g., two, three, four, five, six, or seven) of the level of interferon- γ ; the level of IL-1 β ; the level of IL-6; the level of IL-22; the level of IL-17A; the level of TNF α ; and the level of IL-2, in the ascending colon tissue proximate to one or more sites of disease. Accordingly, in some cases, the methods described herein can result, e.g., in a 1% to 99% decrease (or any of the subranges of this range described herein) in one or more (e.g., two, three, four, five, six, or seven) of the level of interferon- γ ; the level of IL-1 β ; the level of IL-6; the level of IL-22; the level of IL-17A; the level of TNF α ; and the level of IL-2, in the transverse colon tissue proximate to one or more sites of disease. Accordingly, in some cases, the methods described herein can result, e.g., in a 1% to 99% decrease (or any of the subranges of this range described herein) in one or more (e.g., two, three, four, five, six, or seven) of the level of interferon- γ ; the level of IL-1 β ; the level of IL-6; the level of IL-22; the level of IL-17A; the level of TNF α ; and the level of IL-2, in the descending colon tissue proximate to one or more sites of disease. Accordingly, in some cases, the methods described herein can result, e.g., in a 1% to 99% decrease (or any of the subranges of this range described herein) in one or more (e.g., two, three, four, five, six, or seven) of the level of interferon- γ ; the level of IL-1 β ; the level of IL-6; the level of IL-22; the level of IL-17A; the level of TNF α ; and the level of IL-2, in the sigmoid colon tissue proximate to one or more sites of disease.

[0293] In some cases, the amount of the JAK inhibitor that is administered is from about 1 mg to about 500 mg. In some embodiments, the amount of the JAK inhibitor that is administered is from about 1 mg to about 100 mg. In some cases, the amount of the JAK inhibitor that is administered is from about 10 mg to about 300 mg. In some cases, the amount of the JAK inhibitor that is administered is from about 5 mg to about 50 mg. In some cases, the amount of the

JAK inhibitor that is administered from about 10 mg to about 50 mg. In some cases, the amount of the JAK inhibitor that is administered is from about 5 mg to about 40 mg.

[0294] In some cases, the amount of the JAK inhibitor that is administered is less than an amount that is effective when the JAK inhibitor is delivered systemically.

[0295] In some cases, the amount of the JAK inhibitor that is administered is an induction dose. In some cases, such induction dose is effective to induce remission of the TNF and cytokine storm and healing of acute inflammation and lesions. In some cases, the induction dose is administered once a day. In some cases, the induction dose is administered once every three days. In some cases, the induction dose is administered once a week. In some cases, the induction dose is administered once a day, once every three days, or once a week, over a period of about 6-8 weeks.

[0296] In some cases, the method comprises administering (i) an amount of the JAK inhibitor that is an induction dose, and (ii) an amount of the JAK inhibitor that is a maintenance dose, in this order. In some cases, step (ii) is repeated one or more times. In some cases, the induction dose is equal to the maintenance dose. In some cases, the induction dose is greater than the maintenance dose. In some cases, the induction dose is five times greater than the maintenance dose. In some cases, the induction dose is two times greater than the maintenance dose.

[0297] In some cases, the induction dose is the same as or higher than an induction dose administered systemically for treatment of the same disorder to a subject. In more particular cases, the induction dose is the same as or higher than an induction dose administered systemically for treatment of the same disorder to a subject, and the maintenance dose is lower than the maintenance dose administered systemically for treatment of the same disorder to a subject. In some cases, the induction dose is the same as or higher than an induction dose administered systemically for treatment of the same disorder to a subject, and the maintenance dose is higher than the maintenance dose administered systemically for treatment of the same disorder to a subject.

[0298] In some cases an induction dose of JAK inhibitor and a maintenance dose JAK inhibitor are each administered to the subject by administering a pharmaceutical composition comprising a therapeutically effective amount of the JAK inhibitor inhibitor, wherein the pharmaceutical composition is a device. In some cases an induction dose of JAK inhibitor is administered to the subject in a different manner from the maintenance dose. As an example, the induction dose may be administered systemically. In some cases, the induction dose may be administered other than orally. As an example, the induction dose may be administered rectally. As an example, the induction dose may be administered intravenously. As an example, the induction dose may be administered subcutaneously. In some cases, the induction dose may be administered by spray catheter.

[0299] In some cases, the concentration of the JAK inhibitor delivered at the location in the gastrointestinal tract is 10%, 25%, 50%, 75%, 100%, 200%, 300%, 400%, 500%, 1000%, 2000% greater than the concentration of JAK inhibitor in plasma.

[0300] In some cases, the method provides a concentration of the JAK inhibitor at a location that is a site of disease or proximate to a site of disease that is 2-100 times greater than at a location that is not a site of disease or proximate to a site of disease.

[0301] In some cases, the method comprises delivering the JAK inhibitor at the location in the gastrointestinal tract as a single bolus.

[0302] In some cases, the method comprises delivering the JAK inhibitor at the location in the gastrointestinal tract as more than one bolus.

[0303] In some cases, the method comprises delivering the JAK inhibitor at the location in the gastrointestinal tract in a continuous manner.

[0304] In some cases, the method comprises delivering the JAK inhibitor at the location in the gastrointestinal tract over a time period of 20 or more minutes.

[0305] In some cases, the method provides a concentration of the JAK inhibitor in the plasma of the subject that is less than 10 $\mu\text{g/ml}$. In some cases, the method provides a concentration of the JAK inhibitor in the plasma of the subject that is less than 3 $\mu\text{g/ml}$. In some cases, the method provides a concentration of the JAK inhibitor in the plasma of the subject that is less than 1 $\mu\text{g/ml}$. In some cases, the method provides a concentration of the JAK inhibitor in the plasma of the subject that is less than 0.3 $\mu\text{g/ml}$. In some cases, the method provides a concentration of the JAK inhibitor in the plasma of the subject that is less than 0.1 $\mu\text{g/ml}$. In some cases, the method provides a concentration of the JAK inhibitor in the plasma of the subject that is less than 0.01 $\mu\text{g/ml}$. In some cases, the values of the concentration of the JAK inhibitor in the plasma of the subject provided herein refer to C_{trough} , that is, the lowest value of the concentration prior to administration of the next dose.

[0306] In some cases, the method provides a concentration C_{max} of the JAK inhibitor in the plasma of the subject that is less than 10 $\mu\text{g/ml}$. In some disclosures, the method provides a concentration C_{max} of the JAK inhibitor in the plasma of the subject that is less than 3 $\mu\text{g/ml}$. In some cases, the method provides a concentration C_{max} of the JAK inhibitor in the plasma of the subject that is less than 1 $\mu\text{g/ml}$. In some cases, the method provides a concentration C_{max} of the JAK inhibitor in the plasma of the subject that is less than 0.3 $\mu\text{g/ml}$. In some cases, the method provides a concentration C_{max} of the JAK inhibitor in the plasma of the subject that is less than 0.1 $\mu\text{g/ml}$. In some cases, the method provides

a concentration C_{\max} of the JAK inhibitor in the plasma of the subject that is less than 0.01 $\mu\text{g/ml}$.

[0307] In some cases, the methods disclosed herein comprise producing a therapeutically effective degradation product of the JAK inhibitor in the gastrointestinal tract. In some cases, the degradation product is a therapeutic antibody fragment. In some cases, a therapeutically effective amount of the degradation product is produced.

[0308] In some cases, the antibody can be a humanized antibody, a chimeric antibody, a multivalent antibody, or a fragment thereof. In some cases, an antibody can be a scFv-Fc (Sokolowska-Wedzina et al., Mol. Cancer Res. 15(8):1040-1050, 2017), a VHH domain (Li et al., Immunol. Lett. 188:89-95, 2017), a VNAR domain (Hasler et al., Mol. Immunol. 75:28-37, 2016), a (scFv)₂, a minibody (Kim et al., PLoS One 10(1):e113442, 2014), or a BiTE. In some cases, an antibody can be a DVD-Ig (Wu et al., Nat. Biotechnol. 25(11):1290-1297, 2007; WO 08/024188; WO 07/024715), and a dual-affinity re-targeting antibody (DART) (Tsai et al., Mol. Ther. Oncolytics 3:15024, 2016), a triomab (Chelius et al., MAbs 2(3):309-319, 2010), kih IgG with a common LC (Kontermann et al., Drug Discovery Today 20(7):838-847, 2015), a crossmab (Regula et al., EMBO Mol. Med. 9(7):985, 2017), an ortho-Fab IgG (Kontermann et al., Drug Discovery Today 20(7):838-847, 2015), a 2-in-1-IgG (Kontermann et al., Drug Discovery Today 20(7):838-847, 2015), IgG-scFv (Cheal et al., Mol. Cancer Ther. 13(7): 1803-1812, 2014), scFv2-Fc (Natsume et al., J. Biochem. 140(3):359-368, 2006), a bi-nanobody (Kontermann et al., Drug Discovery Today 20(7):838-847, 2015), tandem antibody (Kontermann et al., Drug Discovery Today 20(7):838-847, 2015), a DART-Fc (Kontermann et al., Drug Discovery Today 20(7):838-847, 2015), a scFv-HSA-scFv (Kontermann et al., Drug Discovery Today 20(7):838-847, 2015), DNL-Fab3 (Kontermann et al., Drug Discovery Today 20(7):838-847, 2015), DAF (two-in-one or four-in-one), DutaMab, DT-IgG, knobs-in-holes common LC, knobs-in-holes assembly, charge pair antibody, Fab-arm exchange antibody, SEEDbody, Triomab, LUZ-Y, Fcab, $\kappa\lambda$ -body, orthogonal Fab, DVD-IgG, IgG(H)-scFv, scFv(H)-IgG, IgG(L)-scFv, scFv(L)-IgG, IgG (L,H)-Fc, IgG(H)-V, V(H)-IgG, IgG(L)-V, V(L)-IgG, KIH IgG-scFab, 2scFv-IgG, IgG-2scFv, scFv4-Ig, Zyboby, DVI-IgG, nanobody (e.g., antibodies derived from *Camelus bactriamus*, *Camelus dromaderius*, or *Lama paccos*) (U.S. Patent No. 5,759,808; Stijlemans et al., J. Biol. Chem. 279:1256-1261, 2004; Dumoulin et al., Nature 424:783-788, 2003; and Pleschberger et al., Bioconjugate Chem. 14:440-448, 2003), nanobody-HSA, a diabody (e.g., Poljak, Structure 2(12):1121-1123, 1994; Hudson et al., J. Immunol. Methods 23(1-2):177-189, 1999), a TandAb (Reusch et al., mAbs 6(3):727-738, 2014), scDiabody (Cuesta et al., Trends in Biotechnol. 28(7):355-362, 2010), scDiabody-CH3 (Sanz et al., Trends in Immunol. 25(2):85-91, 2004), Diabody-CH3 (Guo et al., Triple Body, miniantibody, minibody, TriBi minibody, scFv-CH3 KIH, Fab-scFv, scFv-CH-CL-scFv, F(ab')₂-scFv2, scFv-KIH, Fab-scFv-Fc, tetravalent HCAB, scDiabody-Fc, diabody-Fc, tandem scFv-Fc, intrabody (Huston et al., Human Antibodies 10(3-4):127-142, 2001; Wheeler et al., Mol. Ther. 8(3):355-366, 2003; Stocks, DrugDiscov. Today 9(22):960-966, 2004), dock and lock bispecific antibody, ImmTAC, HSABody, scDiabody-HSA, tandem scFv, IgG-IgG, Cov-X-Body, and scFv1-PEG-scFv2.

[0309] Non-limiting examples of an antigen-binding fragment of an antibody include an Fv fragment, a Fab fragment, a F(ab')₂ fragment, and a Fab' fragment. Additional examples of an antigen-binding fragment of an antibody is an antigen-binding fragment of an IgG (e.g., an antigen-binding fragment of IgG1, IgG2, IgG3, or IgG4) (e.g., an antigen-binding fragment of a human or humanized IgG, e.g., human or humanized IgG1, IgG2, IgG3, or IgG4); an antigen-binding fragment of an IgA (e.g., an antigen-binding fragment of IgA1 or IgA2) (e.g., an antigen-binding fragment of a human or humanized IgA, e.g., a human or humanized IgA1 or IgA2); an antigen-binding fragment of an IgD (e.g., an antigen-binding fragment of a human or humanized IgD); an antigen-binding fragment of an IgE (e.g., an antigen-binding fragment of a human or humanized IgE); or an antigen-binding fragment of an IgM (e.g., an antigen-binding fragment of a human or humanized IgM).

[0310] In some cases, an antibody can be an IgNAR, a bispecific antibody (Milstein and Cuello, Nature 305:537-539, 1983; Suresh et al., Methods in Enzymology 121:210, 1986; WO 96/27011; Brennan et al., Science 229:81, 1985; Shalaby et al., J. Exp. Med. 175:217-225, 1992; Kolstelnly et al., J. Immunol. 148(5):1547-1553, 1992; Hollinger et al., Proc. Natl. Acad. Sci. U.S.A. 90:6444-6448, 1993; Gruber et al., J. Immunol. 152:5368, 1994; Tutt et al., J. Immunol. 147:60, 1991), a bispecific diabody, a triabody (Schoonooghe et al., BMC Biotechnol. 9:70, 2009), a tetrabody, scFv-Fc knobs-into-holes, a scFv-Fc-scFv, a (Fab'scFv)₂, a V-IgG, a IvG-V, a dual V domain IgG, a heavy chain immunoglobulin or a camelid (Holt et al., Trends Biotechnol. 21(11):484-490, 2003), an intrabody, a monoclonal antibody (e.g., a human or humanized monoclonal antibody), a heteroconjugate antibody (e.g., U.S. Patent No. 4,676,980), a linear antibody (Zapata et al., Protein Eng. 8(10):1057-1062, 1995), a trispecific antibody (Tutt et al., J. Immunol. 147:60, 1991), a Fabs-in-Tandem immunoglobulin (WO 15/103072), or a humanized camelid antibody.

[0311] In some cases, the methods comprising administering the JAK inhibitor in the manner disclosed herein result in a reduced immunosuppressive properties relative to methods of administration of the JAK inhibitor systemically.

[0312] In some cases, the methods comprising administering the JAK inhibitor in the manner disclosed herein result in reduced immunogenicity relative to methods of administration of the JAK inhibitor systemically.

[0313] In some cases, data obtained from cell culture assays and animal studies can be used in formulating an appropriate dosage of any given JAK inhibitor. The effectiveness and dosing of any JAK inhibitor can be determined by a health care professional or veterinary professional using methods known in the art, as well as by the observation of one or more disease symptoms in a subject (e.g., a human). Certain factors may influence the dosage and timing required

to effectively treat a subject (e.g., the severity of the disease or disorder, previous treatments, the general health and/or age of the subject, and the presence of other diseases).

[0314] In some cases, the subject is further administered an additional therapeutic agent (e.g., any of the additional therapeutic agents described herein). The additional therapeutic agent can be administered to the subject at substantially the same time as the JAK inhibitor or pharmaceutical composition comprising it is administered and/or at one or more other time points. In some cases, the additional therapeutic agent is formulated together with the JAK inhibitor (e.g., using any of the examples of formulations described herein).

[0315] In some cases, the subject is administered a dose of the JAK inhibitor at least once a month (e.g., at least twice a month, at least three times a month, at least four times a month, at least once a week, at least twice a week, three times a week, once a day, or twice a day). The JAK inhibitor may be administered to a subject chronically. Chronic treatments include any form of repeated administration for an extended period of time, such as repeated administrations for one or more months, between a month and a year, one or more years, more than five years, more than 10 years, more than 15 years, more than 20 years, more than 25 years, more than 30 years, more than 35 years, more than 40 years, more than 45 years, or longer. Alternatively, or in addition, chronic treatments may be administered. Chronic treatments can involve regular administrations, for example one or more times a day, one or more times a week, or one or more times a month. For example, chronic treatment can include administration (e.g., intravenous administration) about every two weeks (e.g., between about every 10 to 18 days).

[0316] A suitable dose may be the amount that is the lowest dose effective to produce a desired therapeutic effect. Such an effective dose will generally depend upon the factors described herein. If desired, an effective daily dose of JAK inhibitor can be administered as two, three, four, five, or six or more sub-doses administered separately at appropriate intervals throughout the day, optionally, in unit dosage forms.

[0317] In some examples, administration of a JAK inhibitor using any of the compositions or devices described herein can result in the onset of treatment (e.g., a reduction in the number, severity, or duration of one or more symptoms and/or markers of any of the diseases described herein) or drug-target engagement in a subject within a time period of about 10 minutes to about 10 hours of administration of a dose of an JAK inhibitor using any of the devices or compositions described herein. Drug-target engagement may be determined, for example, as disclosed in Simon GM, Niphakis MJ, Cravatt BF, *Nature chemical biology*. 2013;9(4):200-205.

[0318] In some cases, administration of an JAK inhibitor using any of the devices or compositions described herein can provide for treatment (e.g., a reduction in the number, severity, and/or duration of one or more symptoms and/or markers of any of the disorders described herein in a subject) for a time period of between about 1 hour to about 30 days in a subject following first administration of an JAK inhibitor using any of the compositions or devices described herein. Non-limiting examples of symptoms and/or markers of a disease described herein are described below. For example, treatment can result in a decrease (e.g., about 1% to about 99% decrease) in one or more (e.g., two, three, four, five, six, seven, eight, or nine) of: the level of interferon- γ in GI tissue, the level of IL-1 β in GI tissue, the level of IL-6 in GI tissue, the level of IL-22 in GI tissue, the level of IL-17A in the GI tissue, the level of TNF α in GI tissue, the level of IL-2 in GI tissue, and endoscopy score in a subject (e.g., as compared to the level in the subject prior to treatment or compared to a subject or population of subjects having a similar disease but receiving a placebo or a different treatment) (e.g., for a time period of between about 1 hour to about 30 days (e.g., or any of the subranges herein) following the first administration of an JAK inhibitor using any of the compositions or devices described herein. As used herein, "GI tissue" refers to tissue in the gastrointestinal (GI) tract, such as tissue in one or more of duodenum, jejunum, ileum, cecum, ascending colon, transverse colon, descending colon, sigmoid colon, and rectum, more particularly in the proximal portion of one or more of duodenum, jejunum, ileum, cecum, ascending colon, transverse colon, descending colon, and sigmoid colon, or in the distal portion of one or more of duodenum, jejunum, ileum, cecum, ascending colon, transverse colon, descending colon, and sigmoid colon. The GI tissue may be, for example, GI tissue proximate to one or more sites of disease. Exemplary methods for determining the endoscopy score are described herein and other methods for determining the endoscopy score are known in the art. Exemplary methods for determining the levels of interferon- γ , IL-1 β , IL-6, IL-22, IL-17A, TNF α , and IL-2 are described herein. Additional methods for determining the levels of these cytokines are known in the art. In some examples, treatment can result in an increase (e.g., about 1% to about 500% increase) in one or both of stool consistency score and weight of a subject (e.g., as compared to the level in the subject prior to treatment or compared to a subject or population of subjects having a similar disease but receiving a placebo or a different treatment) (e.g., for a time period of between about 1 hour to about 30 days (e.g., or any of the subranges herein) following the first administration of an JAK inhibitor using any of the compositions or devices described herein. Exemplary methods for determining stool consistency score are described herein. Additional methods for determining a stool consistency score are known in the art.

Combination therapy

[0319] The JAK inhibitor inhibitors disclosed herein may be optionally be used with additional agents in the treatment

of the diseases disclosed herein. Nonlimiting examples of such agents for treating or preventing inflammatory bowel disease in such adjunct therapy (e.g., Crohn's disease, ulcerative colitis) include substances that suppress cytokine production, down-regulate or suppress self-antigen expression, or mask the MHC antigens. Examples of such agents include 2-amino-6-aryl-5-substituted pyrimidines (see U.S. Patent No. 4,665,077); non-steroidal antiinflammatory drugs (NSAIDs); ganciclovir; tacrolimus; glucocorticoids such as Cortisol or aldosterone; anti-inflammatory agents such as a cyclooxygenase inhibitor; a 5-lipoxygenase inhibitor; or a leukotriene receptor antagonist; purine antagonists such as azathioprine or mycophenolate mofetil (MMF); alkylating agents such as cyclophosphamide; bromocryptine; danazol; dapsone; glutaraldehyde (which masks the MHC antigens, as described in U.S. Patent No. 4,120,649); anti-idiotypic antibodies for MHC antigens and MHC fragments; cyclosporine; 6-mercaptopurine; steroids such as corticosteroids or glucocorticosteroids or glucocorticoid analogs, e.g., prednisone, methylprednisolone, including SOLU-MEDROL®, methylprednisolone sodium succinate, and dexamethasone; dihydrofolate reductase inhibitors such as methotrexate (oral or subcutaneous); anti-malarial agents such as chloroquine and hydroxychloroquine; sulfasalazine; leflunomide; cytokine or cytokine receptor antibodies or antagonists including anti-interferon-alpha, -beta, or -gamma antibodies, anti-tumor necrosis factor(TNF)-alpha antibodies (infliximab (REMICADE®) or adalimumab), anti-TNF- alpha immunoadhesin (etanercept), anti-TNF-beta antibodies, anti-interleukin-2 (IL-2) antibodies and anti-IL-2 receptor antibodies, and anti-interleukin-6 (IL-6) receptor antibodies and antagonists; anti-LFA-1 antibodies, including anti-CD 1 la and anti-CD 18 antibodies; anti- L3T4 antibodies; heterologous anti-lymphocyte globulin; pan-T antibodies, anti-CD3 or anti- CD4/CD4a antibodies; soluble peptide containing a LFA-3 binding domain (WO 90/08187 published Jul. 26, 1990); streptokinase; transforming growth factor-beta (TGF-beta); streptodornase; RNA or DNA from the host; FK506; RS-61443; chlorambucil; deoxyspergualin; rapamycin; T-cell receptor (Cohen et al, U.S. Patent No. 5,114,721); T-cell receptor fragments (Offner et al, Science, 251 : 430-432 (1991); WO 90/11294; Ianeway, Nature, 341 : 482 (1989); and WO 91/01133); BAFF antagonists such as BAFF or BR3 antibodies or immunoadhesins and zTNF4 antagonists (for review, see Mackay and Mackay, Trends Immunol, 23: 113-5 (2002) and see also definition below); biologic agents that interfere with T cell helper signals, such as anti-CD40 receptor or anti-CD40 ligand (CD 154), including blocking antibodies to CD40-CD40 ligand.(e.g., Durie et al, Science, 261 : 1328-30 (1993); Mohan et al, J. Immunol, 154: 1470-80 (1995)) and CTLA4-Ig (Finck et al, Science, 265: 1225-7 (1994)); and T-cell receptor antibodies (EP 340,109) such as T10B9. Non-limiting examples of adjunct agents also include the following: budesonide; epidermal growth factor; aminosaliclates; metronidazole; mesalamine; olsalazine; balsalazide; antioxidants; thromboxane inhibitors; IL-1 receptor antagonists; anti-IL-1 monoclonal antibodies; growth factors; elastase inhibitors; pyridinyl-imidazole compounds; TNF antagonists; IL-4, IL-10, IL-13 and/or TGFβ cytokines or agonists thereof (e.g., agonist antibodies); IL-11; glucuronide- or dextran-conjugated prodrugs of prednisolone, dexamethasone or budesonide; ICAM-I antisense phosphorothioate oligodeoxynucleotides (ISIS 2302; Isis Pharmaceuticals, Inc.); soluble complement receptor 1 (TPIO; T Cell Sciences, Inc.); slow-release mesalazine; antagonists of platelet activating factor (PAF); ciprofloxacin; and lignocaine. Examples of agents for UC are sulfasalazine and related salicylate-containing drugs for mild cases and corticosteroid drugs in severe cases. Topical administration of either salicylates or corticosteroids is sometimes effective, particularly when the disease is limited to the distal bowel, and is associated with decreased side effects compared with systemic use. Supportive measures such as administration of iron and antidiarrheal agents are sometimes indicated. Azathioprine, 6-mercaptopurine and methotrexate are sometimes also prescribed for use in refractory corticosteroid-dependent cases.

[0320] In other embodiments, a JAK inhibitor as described herein may be administered with one or more of: a CHST15 inhibitor, a IL-6 receptor inhibitor, a TNF inhibitor, an integrin inhibitor a JAK inhibitor, a SMAD7 inhibitor, a IL-13 inhibitor, an IL-1 receptor inhibitor, a TLR agonist, an immunosuppressant, a live biotherapeutic such as a stem cell, IL-10 or an IL-10 agonist, copaxone, a CD40 inhibitor, an S1P-inhibitor, or a chemokine/chemokine receptor inhibitor. In other embodiments, a JAK inhibitor as described herein may be administered with a vitamin C infusion, one or more corticosteroids, and optionally thiamine.

Examples of particular combinations include the following. Unless otherwise specified, the first component (component (1)) is administered in an ingestible device, while the second component (component (2)) is administered either in an ingestible device, which may be the same or different ingestible device as the first component, or by another form of administration.

(1) JAK inhibitor; (2) TNF inhibitor.

(1) JAK inhibitor; (2) TNF inhibitor in an ingestible device.

(1) JAK inhibitor; (2) TNF inhibitor intravenously or subcutaneously.

(1) TNF inhibitor; (2) JAK inhibitor

(1) TNF inhibitor; (2) JAK inhibitor in an ingestible device.

(1) TNF inhibitor; (2) JAK inhibitor orally.

(1) Neoregulin-4; (2) JAK inhibitor.

(1) Neoregulin-4; (2) JAK inhibitor in an ingestible device.

(1) Neoregulin-4; (2) JAK inhibitor intravenously or subcutaneously.

[0321] In some disclosures, the methods disclosed herein comprise administering (i) the JAK inhibitor as disclosed herein, and (ii) a second agent orally, intravenously or subcutaneously, wherein the second agent in (ii) is the same JAK inhibitor in (i); a different JAK inhibitor; or an agent having a different biological target from the JAK inhibitor.

[0322] In some cases, the methods disclosed herein comprise administering (i) the JAK inhibitor in the manner disclosed herein, and (ii) a second agent orally, intravenously or subcutaneously, wherein the second agent in (ii) is an agent suitable for treating an inflammatory bowel disease.

[0323] In some cases, the JAK inhibitor is administered prior to the second agent. In some cases, the JAK inhibitor is administered after the second agent. In some cases, the JAK inhibitor and the second agent are administered substantially at the same time. In some cases, the JAK inhibitor is delivered prior to the second agent. In some cases, the JAK inhibitor is delivered after the second agent. In some cases, the JAK inhibitor and the second agent are delivered substantially at the same time.

[0324] In some cases, the second agent is an agent suitable for the treatment of a disease of the gastrointestinal tract. In some cases, the second agent is an agent suitable for the treatment of an inflammatory bowel disease. In some cases, the second agent is administered intravenously. In some cases, the second agent is administered subcutaneously. In some cases, the second agent is methotrexate.

[0325] In some cases, delivery of the JAK inhibitor to the cecum, such as delivery to the cecum by mucosal contact, results in systemic immunogenicity levels at or below systemic immunogenicity levels resulting from administration of the JAK inhibitor systemically. In some cases comprising administering the JAK inhibitor in the manner disclosed herein and a second agent systemically, delivery of the JAK inhibitor to the cecum, such as delivery to the cecum by mucosal contact, results in systemic immunogenicity levels at or below systemic immunogenicity levels resulting from administration of the JAK inhibitor systemically and the second agent systemically. In some disclosures, the method comprises administering the JAK inhibitor in the manner disclosed herein and a second agent, wherein the amount of the second agent is less than the amount of the second agent when the JAK inhibitor and the second agent are both administered systemically. In some aspects of these cases, the second agent is a JAK inhibitor.

[0326] In some cases, the method comprises administering the JAK inhibitor in the manner disclosed herein and does not comprise administering a second agent.

Example 1 - Preclinical Murine Colitis Model

Experimental Induction of Colitis

[0327] Colitis is experimentally induced to mice via the dextran sulfate sodium (DSS) induced colitis model. This model is widely used because of its simplicity and many similarities with human ulcerative colitis. Briefly, mice are subjected to DSS via cecal catheterization, which is thought to be directly toxic to colonic epithelial cells of the basal crypts, for several days until colitis is induced.

Groups

[0328] Mice are allocated to one of seven cohorts, depending on the agent that is administered:

1. Control (no agent)
2. Adalimumab (2.5 mg/kg)
3. Adalimumab (5 mg/kg)
4. Adalimumab (10 mg/kg)

[0329] The control or agent is applied to a damaged mucosal surface of the bowel via administration through a cecal catheter at the dose levels described above.

[0330] Additionally, for each cohort, the animals are separated into two groups. One group receives a single dose of the control or agent on day 10 or 12. The other group receives daily (or similar) dosing of the control or agent.

Analysis

[0331] For each animal, efficacy is determined (e.g., by endoscopy, histology, etc.), and cytotoxic T-cell levels are determined in blood, feces, and tissue (tissue levels are determined after animal sacrifice). For tissue samples, levels HER2 are additionally determined, and the level of cytotoxic T cells is normalized to the level of HER2. Additionally, other cytokine levels are determined in tissue (e.g., phospho STAT 1, STAT 3 and STAT 5), in plasma (e.g., VEGF, VCAM, ICAM, IL-6), or both.

[0332] Pharmacokinetics are determined both systemically (e.g., in the plasma) and locally (e.g., in colon tissue). For

systemic pharmacokinetic analysis, blood and/or feces is collected from the animals at one or more timepoints after administration (e.g., plasma samples are collected at 15 minutes, 30 minutes, 1 hour, 2 hours, 4 hours, and/or 8 hours after administration). Local/colon tissue samples are collected once after animal sacrifice.

Example 2a - Development of Preclinical Porcine Colitis Model

Experimental Induction of Colitis

[0333] Female swine weighing approximately 35 to 45 kg at study start are fasted at least 24 hours prior to intra-rectal administration of trinitrobenzene sulfonic acid (TNBS). Animals are lightly anesthetized during the dosing and endoscopy procedure. An enema to clean the colon is used, if necessary. One animal is administered 40 ml of 100% EtOH mixed with 5 grams of TNBS diluted in 10 ml of water via an enema using a ball-tipped catheter. The enema is deposited in the proximal portion of the descending colon just past the bend of the transverse colon. The TNBS is retained at the dose site for 12 minutes by use of two Foley catheters with 60-ml balloons placed in the mid-section of the descending colon below the dose site. A second animal is similarly treated, but with a solution containing 10 grams of TNBS. An Endoscope is employed to positively identify the dose site in both animals prior to TNBS administration. Dosing and endoscopy are performed by a veterinary surgeon

[0334] Seven (7) days after TNBS administration, after light anesthesia, the dose site and mucosal tissues above and below the dose site are evaluated by the veterinary surgeon using an endoscope. Pinch Biopsies are obtained necessary, as determined by the surgeon. Based on the endoscopy findings, the animals may be euthanized for tissue collection on that day, or may proceed on study pending the results of subsequent endoscopy exams for 1 to 4 more days. Macroscopic and microscopic alterations of colonic architecture, possible necrosis, thickening of the colon, and substantial histologic changes are observed at the proper TNBS dose.

[0335] Clinical signs (e.g., ill health, behavioral changes, etc.) are recorded at least daily during acclimation and throughout the study. Additional pen-side observations are conducted twice daily (once-daily on weekends). Body weight is measured for both animals Days 1 and 7 (and on the day of euthanasia if after Day 7).

[0336] On the day of necropsy, the animals are euthanized via injection of a veterinarian-approved euthanasia solution. Immediately after euthanasia in order to avoid autolytic changes, colon tissues are collected, opened, rinsed with saline, and a detailed macroscopic examination of the colon is performed to identify macroscopic findings related to TNBS-damage. Photos are taken. Tissue samples are taken from the proximal, mid, and distal transverse colon; the dose site; the distal colon; the rectum; and the anal canal. Samples are placed into NBF and evaluated by a board certified veterinary pathologist.

Example 2b - Pharmacokinetic/Pharmacodynamic and Bioavailability of Adalimumab After Topical Application

Groups

[0337] Sixteen (16) swine (approximately 35 to 45 kg at study start) are allocated to one of five groups:

1. Vehicle Control: (3.2 mL saline); intra-rectal; (n=2)
2. Treated Control: Adalimumab (40mg in 3.2mL saline); subcutaneous; (n=2)
3. Adalimumab (low): Adalimumab (40mg in 3.2mL saline); intra-rectal; (n=4)
4. Adalimumab (med): Adalimumab (80mg in 3.2 mL saline); intra-rectal; (n=4)
5. Adalimumab (high): Adalimumab (160mg in 3.2 mL saline); intra-rectal; (n=4)

[0338] On Day 0, the test article is applied to a damaged mucosal surface of the bowel via intra-rectal administration or subcutaneous injection by a veterinary surgeon at the dose levels and volume described above.

Clinical Observations and Body Weight

[0339] Clinical observations are conducted at least once daily. Clinical signs (e.g., ill health, behavioral changes, etc.) are recorded on all appropriate animals at least daily prior to the initiation of experiment and throughout the study until termination. Additional clinical observations may be performed if deemed necessary. Animals whose health condition warrants further evaluation are examined by a Clinical Veterinarian. Body weight is measured for all animals Days -6, 0, and after the last blood collections.

Samples*Blood:*

5 **[0340]** Blood is collected (cephalic, jugular, and/or catheter) into EDTA tubes during acclimation on Day-7, just prior to dose on Day 0, and 0.5, 1, 2, 4, 6, 8, 12, 24, and 48 hours post-dose. The EDTA samples are split into two aliquots and one is centrifuged for pharmacokinetic plasma and either analyzed immediately, or stored frozen (-80°C) for later pharmacokinetic analyses. The remaining sample of whole blood is used for pharmacodynamic analyses.

10 *Feces:*

[0341] Feces is collected Day -7, 0 and 0.5, 1, 2, 4, 6, 8, 12, 24 and 48 hours post-dose, and either analyzed immediately, or flash-frozen on liquid nitrogen and stored frozen at -70°C pending later analysis of drug levels and inflammatory cytokines.

15 *Tissue:*

20 **[0342]** Immediately after euthanasia in order to avoid autolytic changes, colon tissues are collected, opened, rinsed with saline, and a detailed macroscopic examination of the colon is performed to identify macroscopic findings related to TNBS-damage. Triplicate samples of normal and damaged tissues are either analyzed immediately, or are flash-frozen on liquid nitrogen and stored frozen at -70°C pending later analysis of drug concentration, inflammatory cytokines and histology.

[0343] Samples are analyzed for adalimumab levels (local mucosal tissue levels and systemic circulation levels), and for levels of inflammatory cytokines including TNF-alpha.

25 Terminal Procedures

30 **[0344]** Animals are euthanized as per the schedule in Table AA, where one animal each of Vehicle and Treated Control groups is euthanized at 6 and 48 hours post-dose, and one animal of each the adalimumab groups are euthanized at 6, 12, 24 and 48 hours post-dose. Animals are discarded after the last blood collection unless retained for a subsequent study.

Table AA

35					Days								Hours											
					-7	-6	-5	-4	-3	-2	-1	0	0.5	1	2	4	6	8	12	24	48			
	General	Sample size	Dose	Route																				
	Fast				•																			
	Food/Water		ad libidum	oral		•	•	•	•	•	•	•	•	•	•	•	•	•	•	•	•	•	•	•
40	Observations																							
	clinical observations				•	•	•	•	•	•	•	•										•	•	
	body weight				•							•										•	•	
	Treatments (groups)																							
	TNBS (all animals)			intra rectal		•																		
	1. Vehicle control	n=2	1.6mL saline (vehicle)	intra rectal								•												
	euthanized																n=1						n=1	
45	2. Treated control	n=2	40mg in 1.6mL saline	sub-cutaneous																				
	euthanized																n=1						n=1	
	3. Adalimumab (low)	n=4	40mg in 1.6mL saline	intra rectal								•												
	euthanized																n=1			n=1	n=1	n=1		
50	4. Adalimumab (med)	n=4	80mg in 1.6mL saline	intra rectal								•												
	euthanized																n=1			n=1	n=1	n=1		
	5. Adalimumab (high)	n=4	160mg in 1.6mL saline	intra rectal								•												
	euthanized																n=1			n=1	n=1	n=1		
	Adalimumab (required)		1200																					
55	Samples																							
	Blood			cephalic, jugular or catheter	•							•	•	•	•	•	•	•	•	•	•	•	•	•
	Fecal			rectal	•							•	•	•	•	•	•	•	•	•	•	•	•	•
	Tissue			necropsy	•												•		•	•	•	•	•	•

Example 2c - Pharmacokinetic/Pharmacodynamic and Bioavailability of Adalimumab After Topical ApplicationGroups

[0345] DSS-induced colitis Yorkshire-Cross Farm Swine (approximately 5-10 kg at study start) are allocated to one of five groups:

1. Vehicle Control: (saline); intra-rectal;
2. Treated Control: Adalimumab (13 mg in saline); subcutaneous;
3. Adalimumab: Adalimumab (13 mg in saline); intra-rectal;

[0346] At $t = 0$, the test article is applied to a damaged mucosal surface of the bowel via intra-rectal administration or subcutaneous injection by a veterinary surgeon at the dose levels and volume described above.

Clinical Observations

[0347] Clinical signs (e.g., ill health, behavioral changes, etc.) are recorded on all appropriate animals at least daily prior to the initiation of experiment and throughout the study until termination. Additional clinical observations may be performed if deemed necessary. Animals whose health condition warrants further evaluation are examined by a Clinical Veterinarian.

Samples*Blood:*

[0348] Blood is collected (cephalic, jugular, and/or catheter) into EDTA tubes during acclimation on Day-7, just prior to dose on Day 0, and 12 hours post-dose. The EDTA samples are split into two aliquots and one is centrifuged for pharmacokinetic plasma and either analyzed immediately, or stored frozen (-80°C) for later pharmacokinetic analyses. The remaining sample of whole blood is used for pharmacodynamic analyses.

Feces:

[0349] Feces is collected Day -7, 0 and 12 hours post-dose, and either analyzed immediately, or flash-frozen on liquid nitrogen and stored frozen at -70°C pending later analysis of drug levels and inflammatory cytokines.

Tissue:

[0350] Immediately after euthanasia (12 hours after dosing) in order to avoid autolytic changes, colon tissues are collected, opened, rinsed with saline, and a detailed macroscopic examination of the colon is performed to identify macroscopic findings related to DSS-damage. Triplicate samples of normal and damaged tissues are either analyzed immediately, or are flash-frozen on liquid nitrogen and stored frozen at -70°C pending later analysis of drug concentration, inflammatory cytokines and histology.

[0351] Samples are analyzed for adalimumab levels (local mucosal tissue levels and systemic circulation levels), and for levels of inflammatory cytokines including TNF-alpha.

Terminal Procedures

[0352] Animals are euthanized at 12 hours post-dose.

Example 3. Comparison of Systemic versus Intracecal Delivery of an Anti-IL-12 Antibody

[0353] The objective of this study was to compare the efficacy of an IL-12 inhibitor (anti-IL-12 p40; anti-p40 mAb; BioXCell (Cat#: BE0051)), when dosed systemically versus intracecally, to the treat dextran sulfate sodium salt (DSS)-induced colitis in male C57B1/6 mice.

Materials and Methods

Mice

[0354] Normal male C57B1/6 mice between the ages of 6-8 weeks old, weighing 20-24 g, were obtained from Charles River Laboratories. The mice were randomized into thirteen groups of twelve animals and two groups of eight animals, and housed in groups of 6-8 per cage, and acclimatized for at least three days prior to entering the study. Animal rooms were set to maintain a minimum of 12 to 15 air changes per hour, with an automatic timer for a light/dark cycle of 12 hours on/off, and fed with Labdiet 5053 sterile rodent chow, with water administered *ad libitum*.

Cecal Cannulation

[0355] Animals were placed under isoflurane anesthesia, with the cecum exposed via a midline incision in the abdomen. A small point incision was made in the distal cecum where 1-2 cm of the cannula was inserted. The incision was closed with a purse string suture using 5-0 silk. An incision was then made in the left abdominal wall through which the distal end of the cannula was inserted and pushed subcutaneously to the dorsal aspect of the back. The site was then washed copiously with warmed saline prior to closing the abdominal wall. A small incision was also made in the skin of the back between the shoulder blades, exposing the tip of the cannula. The cannula was secured in place using suture, wound clips, and tissue glue. All animals received 1 mL of warm sterile saline (subcutaneous injection) and were monitored closely until recovery before returning to their cage. All animals received 0.6 mg/kg BID buprenorphine for the first 3 days, and Baytril® at 10mg/Kg every day for the first 5 days post surgery.

Induction of Colitis

[0356] Colitis was induced in male C57B1/6 mice by exposure to 3% DSS drinking water (MP Biomedicals #0260110) from Day 0 to Day 5. Fresh DSS/water solutions were made again on Day 3 and any of the remaining original DSS solution will be discarded.

Assessment of Colitis

[0357] All animals were weighed daily and visually assessed for the presence of diarrhea and/or bloody stool at the time of dosing. The mice underwent two video endoscopies, one on day 10 and one on day 14, to assess colitis severity. Images were captured from each animal at the most severe region of disease identified during the endoscopy, and assessed using the rubric demonstrated in Table 1.1. Additionally, stool consistency was scored during the endoscopy using this rubric (Table 1.2) (0 = Normal, well-formed pellet, 1 = Loose stool, soft, staying in shape, 2 = Loose stool, abnormal form with excess moisture, 3 = Watery or diarrhea, 4 = Bloody diarrhea). At necropsy, intestinal contents, peripheral blood, and tissue, and cecum/colon contents were collected for analysis.

Table 1.1. Endoscopy Scoring

Score	Description of Endoscopy Score
0	Normal
1	Loss of vascularity
2	Loss of vascularity and friability
3	Friability and erosions
4	Ulcerations and bleeding

Table 1.2. Stool Consistency Score

Score	Description of Stool Consistency
0	Normal, well-formed pellet
1	Loose stool, soft, staying in shape
2	Loose stool, abnormal form with excess moisture

(continued)

Score	Description of Stool Consistency
3	Watery or diarrhea
4	Bloody diarrhea

Treatment of Colitis

[0358] Mice were treated with anti-IL-12 p40 during the acute phase of colitis due to its efficacy in the treatment of DSS-induced colitis. The test article was dosed at a volume of 0.1 mL/20 g from days 0 to 14. Anti-IL-12 p40 was administered intraperitoneally at a dose of 10 mg/kg every 3 days, and intracecally at a dose of 10 mg/kg, either every 3 days or every day. There was also a lower dose of 1 mg/kg given every day intracecally. The control groups were not administered drugs, and the vehicles (sterile PBS) were administered the placebo drug intraperitoneally and intracecally every day. These drugs were given from days 5-14, which is 9 days of administration. A more detailed explanation of dosing and groups can be seen in Table 1.3.

Table 1.3. Groups of Animals

Group #	# of Animals	DSS	Cecal Cannula	Treatment	Dose(mg/ kg)	Route	Dosing Schedule
1	8 males	---	NO	---	---	---	---
2	8 males	---	YES	---	---	---	---
3	12 males	3% DSS (day 0-5)	NO	Vehicle	---	PO	QD day 0-14
4	12 males	3% DSS (day 0-5)	YES	Vehicle	---	IC	QD day 0-14
5	12 males	3% DSS (day 0-5)	NO	Anti-p40	10	IP	Q3 0,3,6,9,12
6	12 males	3% DSS (day 0-5)	YES	Anti-p40	10	IC	Q3 0,3,6,9,12
7	12 males	3% DSS (day 0-5)	YES	Anti-p40	10	IC	QD day 0-14
8	12 males	3% DSS (day 0-5)	YES	Anti-p40	1	IC	QD day 0-14

Sample Collection

[0359] Intestinal contents, peripheral blood, and tissue were collected at sacrifice on day 14, as follows: at the end of each study period, mice were euthanized by CO₂ inhalation immediately following endoscopy on day 14. The blood was collected via cardiac puncture into K₂EDTA-coated tubes and centrifuged at 4000 x g for 10 minutes. The blood cell pellet was retained and snapped frozen. The resulting plasma was then split into two separate cryotubes, with 100 µL in one tube and the remainder in the second. Plasma and cell pellet were also collected, flash frozen, and stored at -80 degrees Celsius.

[0360] The cecum and colon were removed from each animal and contents were collected, weighed, and snap frozen in separate cryovials. The colon was excised, rinsed, measured, weighed, and then trimmed to 6 cm in length and divided into 5 pieces. The most proximal 1 cm of colon was snapped frozen for subsequent bioanalysis of test article levels. Of the remaining 5 cm of colon, the most distal and proximal 1.5-cm sections was placed in formalin for 24 hours then transferred to 70% ethanol for subsequent histological evaluation. The middle 2-cm portion was bisected longitudinally and placed into two separate cryotubes, weighed, and snap frozen in liquid nitrogen.

Results

[0361] The data in Figure 30 show that the DSS mice that were intracecally administered an anti-IL-12 p40 (IgG2A) antibody had decreased weight loss as compared to DSS mice that were intraperitoneally administered the anti-IL-12 p40 antibody.

[0362] The data in Figure 31 show that the plasma concentration of the anti-IL-12 p40 antibody was decreased in DSS mice that were intracecally administered the anti-IL-12 p40 antibody as compared to DSS mice that were intraperitoneally administered the anti-IL-12 p40 antibody. The data in Figure 32 show that the cecum and colon concentration of the anti-IL-12 p40 antibody is increased in DSS mice that were intracecally administered the anti-IL-12 p40 antibody as compared to the DSS mice that were intraperitoneally administered the anti-IL-12 p40 antibody.

[0363] The data in Figures 33 and 34 show that the anti-IL-12 p40 antibody is able to penetrate colon tissues (the lumen superficial, lamina propria, submucosa, and tunica muscularis/serosa) in DSS mice intracecally administered the anti-IL-12 p40 antibody, while the anti-IL-12 p40 antibody did not detectably penetrate the colon tissues of DSS mice intraperitoneally administered the anti-IL-12 p40 antibody. The data in Figure 35 also show that the ratio of the concentration of anti-IL-12 p40 antibody in colon tissue to the concentration of the anti-IL-12 p40 antibody in plasma is increased in DSS mice intracecally administered the anti-IL-12 p40 antibody as compared to the ratio in DSS mice intraperitoneally administered the anti-IL-12 p40 antibody.

[0364] The data in Figure 36 show that the concentration of IL-1 β in colon tissue is decreased in DSS mice intracecally administered the anti-IL-12 p40 antibody as compared to the concentration of IL-1 β in colon tissue in DSS mice intraperitoneally administered the anti-IL-12 p40 antibody. The data in Figure 37 show that the concentration of IL-6 in colon tissue is decreased in DSS mice intracecally administered the anti-IL-12 p40 antibody as compared to the concentration of IL-6 in colon tissue in DSS mice intraperitoneally administered the anti-IL-12 p40 antibody. The data in Figure 38 show that the concentration of IL-17A in colon tissue is decreased in DSS mice intracecally administered the anti-IL-12 p40 antibody as compared to the concentration of IL-17A in colon tissue in DSS mice intraperitoneally administered the anti-IL-12 p40 antibody.

[0365] No significant differences in clinical observations or gastrointestinal-specific adverse effects, including stool consistency and/or bloody stool, were observed due to cannulation or intra-cecal treatments when compared with vehicle. No toxicity resulting from the treatments was reported. A significant reduction in body weight-loss (AUC) was found in groups treated with anti-IL-12 p40 antibody (10 mg/kg and 1mg/kg, QD) via intra-cecal delivery when compared with vehicle control and intraperitoneal delivery (10 mg/kg, Q3D). The immunohistochemistry staining in anti-IL-12 p40 antibody (10 mg/kg, QD) treatment groups showed penetration of the antibody in all layers of colon tissue, including lumen mucosa, lamina propria, submucosa, tunica muscularis, via intra-cecal delivery. The distribution of anti-IL-12 p40 antibody was found in all segments of the colon, however, higher levels were detected in the proximal region. A significantly higher mean concentration of anti-IL-12 p40 antibody was found in the gastrointestinal contents and colon tissues when delivered via intra-cecal administration (Anti-p40: 10 mg/kg and 1mg/kg, QD) compared with intraperitoneal administration (anti-p40: 10 mg/kg, Q3D). The blood level of anti-IL-12 p40 antibody was significantly higher when delivered via intraperitoneal administration (Q3D) as compared to intra-cecal administration (Q3D & QD). The concentrations of inflammatory cytokines, including IL-1 β , IL-6, and IL-17, were significantly reduced by anti-IL-12 p40 antibody (10 mg/kg, QD) treatment when delivered via intra-cecal administration as compared to vehicle controls.

[0366] In sum, these data show that the compositions and devices provided herein can suppress the local immune response in the intestine, while having less of a suppressive effect on the systemic immune response of an animal. These data also suggest that the presently claimed compositions and devices will provide for treatment of colitis and other pro-inflammatory disorders of the intestine.

Example 4. Comparison of Systemic versus Intracecal Delivery of an Anti-Integrin α 4 β 7 Antibody

[0367] The objective of this study was to compare the efficacy of an integrin inhibitor (anti-integrin α 4 β 7; anti-LPAM1; DATK-32 mAb; BioXCell (Cat#: BE0034)) when dosed systemically versus intracecally for treating dextran sulfate sodium salt (DSS)-induced colitis in male C57B1/6 mice.

Materials and Methods

Mice

[0368] Normal male C57B1/6 mice between the ages of 6-8 weeks old, weighing 20-24 g, were obtained from Charles River Laboratories. The mice were randomized into thirteen groups of twelve animals and two groups of eight animals, and housed in groups of 6-8 per cage, and acclimatized for at least three days prior to entering the study. Animal rooms were set to maintain a minimum of 12 to 15 air changes per hour, with an automatic timer for a light/dark cycle of 12 hours on/off, and fed with Labdiet 5053 sterile rodent chow, with water administered *ad libitum*.

Cecal Cannulation

[0369] The animals were placed under isoflurane anesthesia, with the cecum exposed via a midline incision in the abdomen. A small point incision was made in the distal cecum where 1-2 cm of the cannula was inserted. The incision was closed with a purse string suture using 5-0 silk. An incision was then made in the left abdominal wall through which the distal end of the cannula was inserted and pushed subcutaneously to the dorsal aspect of the back. The site was then washed copiously with warmed saline prior to closing the abdominal wall. A small incision was also made in the skin of the back between the shoulder blades, exposing the tip of the cannula. The cannula was secured in place using

EP 3 554 485 B9

suture, wound clips, and tissue glue. All animals received 1 mL of warm sterile saline (subcutaneous injection) and were monitored closely until recovery before returning to their cage. All animals received 0.6 mg/kg BID buprenorphine for the first 3 days, and Baytril® at 10mg/Kg every day for the first 5 days post-surgery.

Induction of Colitis

[0370] Colitis was induced in male C57B1/6 mice by exposure to 3% DSS drinking water (MP Biomedicals #0260110) from day 0 to day 5. Fresh DSS/water solutions were made again on day 3 and any of the remaining original DSS solution will be discarded.

Assessment of Colitis

[0371] All animals were weighed daily and visually assessed for the presence of diarrhea and/or bloody stool at the time of dosing. Mice underwent two video endoscopies, one on day 10 and one on day 14, to assess colitis severity. Images were captured from each animal at the most severe region of disease identified during the endoscopy, and assessed using the rubric demonstrated in Table 2.1. Additionally, stool consistency was scored during the endoscopy using this rubric (Table 2.2) (0 = Normal, well-formed pellet, 1= Loose stool, soft, staying in shape, 2 = Loose stool, abnormal form with excess moisture, 3 = Watery or diarrhea, 4 = Bloody diarrhea). At necropsy, intestinal contents, peripheral blood and tissue, and cecum/colon contents were collected for analysis.

Table 2.1. Endoscopy Score

Score	Description of Endoscopy Score
0	Normal
1	Loss of vascularity
2	Loss of vascularity and friability
3	Friability and erosions
4	Ulcerations and bleeding

Table 2.2. Stool Consistency Score

Score	Description of Stool Consistency
0	Normal, well-formed pellet
1	Loose stool, soft, staying in shape
2	Loose stool, abnormal form with excess moisture
3	Watery or diarrhea
4	Bloody diarrhea

Treatment of Colitis

[0372] Mice were treated with DATK32 during the acute phase of colitis due to its efficacy in the treatment of DSS-induced colitis. The test article was dosed at a volume of 0.1 mL/20 g from days 0 to 14. DATK32 was administered intraperitoneally at a dose of 25 mg/kg every 3 days, and intracecally at a dose of 25 mg/kg, either every 3 days or every day. There was also a lower dose of 5 mg/kg given every day intracecally. The control groups were not administered drugs, and the vehicle (sterile PBS) was administered as the placebo drug intraperitoneally and intracecally every day. These drugs were given from days 5-14, which is 9 days of administration. A more detailed explanation of dosing and groups can be seen in Table 2.3.

Table 2.3. Groups of Mice

Group #	# of Animals	DSS	Cecal Cannula	Treatment	Dose(mg/ kg)	Route	Dosing Schedule
1	8 males	---	NO	---	---	---	---

(continued)

Group #	# of Animals	DSS	Cecal Cannula	Treatment	Dose(mg/ kg)	Route	Dosing Schedule
2	8 males	---	YES	---	---	---	---
3	12 males	3% DSS (day 0-5)	NO	Vehicle	---	PO	QD day 0-14
4	12 males	3% DSS (day 0-5)	YES	Vehicle	---	IC	QD day 0-14
9	12 males	3% DSS (day 0-5)	NO	DATK32	25	IP	Q3 0,3,6,9,12
10	12 males	3% DSS (day 0-5)	YES	DATK32	25	IC	Q3 0,3,6,9,12
11	12 males	3% DSS (day 0-5)	YES	DATK32	25	IC	QD day 0-14
12	12 males	3% DSS (day 0-5)	YES	DATK32	5	IC	QD day 0-14

Sample Collection

[0373] Intestinal contents, peripheral blood, and tissue were collected at sacrifice on day 14, as follows: at the end of each study period, mice were euthanized by CO₂ inhalation immediately following endoscopy on day 14. The blood was collected via cardiac puncture into K₂EDTA-coated tubes and centrifuged at 4000 x g for 10 minutes. The blood cell pellet was retained and snapped frozen. The resulting plasma was then split into two separate cryotubes, with 100 µL in one tube and the remainder in the second. Plasma and the cell pellet were also collected, flash frozen, and stored at -80 degrees Celsius. An ELISA was used to determine the level of rat IgG2A.

[0374] The cecum and colon were removed from each animal and contents were collected, weighed, and snap frozen in separate cryovials. The colon was excised, rinsed, measured, weighed, and then trimmed to 6 cm in length and divided into 5 pieces. The most proximal 1 cm of colon was snapped frozen for subsequent bioanalysis of anti-DATK32 levels. Of the remaining 5 cm of colon, the most distal and proximal 1.5-cm sections was placed in formalin for 24 hours then transferred to 70% ethanol for subsequent histological evaluation. The middle 2-cm portion was bisected longitudinally and placed into two separate cryotubes, weighed, and snap frozen in liquid nitrogen.

[0375] There was an additional collection of 100 µL of whole blood from all animals and processed for FACS analysis of α4 and β7 expression on T-helper memory cells. Tissue and blood were immediately placed in FACS buffer (1x PBS containing 2.5% fetal calf serum) and analyzed using the following antibody panel (Table 2.4).

Table 2.4. Fluorophore Labelled Antibodies Used in FACS Analysis

Antibody Target	Fluorochrome	Purpose
CD4	APC-Vio770	Defines T-Helper Cells
CD44	VioBlue	Memory/Naive Discrimination
CD45RB	FITC	Memory/Naive Discrimination
α4	APC	Defines T-helper memory subset of interest
β7	PE	Defines T-helper memory subset of interest
CD 16/32	-	Fc Block

Results

[0376] The data in Figure 39 show decreased weight loss in DSS mice intracecally administered DATK antibody as compared to DSS mice that were intraperitoneally administered the DATK antibody. The data in Figure 40 show that DSS mice intracecally administered DATK antibody have a decreased plasma concentration of DATK antibody as compared to DSS mice that were intraperitoneally administered DATK antibody. The data in Figures 41 and 42 show that DSS mice intracecally administered DATK antibody have an increased concentration of DATK antibody in the cecum and colon content as compared to DSS mice intraperitoneally administered DATK antibody. The data in Figures 43 and 44 show that DSS mice intracecally administered DATK antibody have an increased concentration of DATK antibody in colon tissue as compared to DSS mice intraperitoneally administered DATK antibody. The data in Figures 45 and 46 show an increased level of penetration of DATK antibody into colon tissue in DSS mice intracecally administered the DATK antibody as compared to an intracecal vehicle control (PBS). The data in Figure 47 show that DSS mice intracecally administered DATK antibody have an increased ratio of the concentration of DATK antibody in colon tissue to the plasma

concentration of the DATK antibody, as compared to the same ratio in DSS mice intraperitoneally administered the DATK antibody.

[0377] The data in Figure 48 show that DSS mice intracecally administered the DATK antibody have an increased percentage of blood Th memory cells as compared to DSS mice intraperitoneally administered the DATK antibody.

[0378] No significant differences in clinical observations or gastrointestinal-specific adverse effects, including stool consistency and/or bloody stool, were observed due to cannulation or intra-cecal treatments when compared with vehicle. No toxicity resulting from the treatments was reported. A significant reduction in body weight-loss was also found with DATK32 (5 mg/kg, QD) treatment (IC) when compared to vehicle control at the endpoint (day 14). The immunohistochemistry staining in DATK32 (25 mg/kg, QD) treatment groups showed penetration of DATK32 in all layers of colon tissue, including lumen mucosa, lamina propria, submucosa, tunica muscularis, via intra-cecal delivery. The distribution of DATK32 was found in all segments of the colon, however, higher levels were detected in the proximal region. A significantly higher mean concentration of DATK32 was found in gastrointestinal contents and colon tissues when delivered via intra-cecal administration (DATK32: 25 mg/kg and 5 mg/kg, QD) as compared to intraperitoneal administration (DATK32: 25 mg/kg, Q3D). The blood level of DATK32 was significantly higher when delivered via intraperitoneal administration (Q3D) as compared to intra-cecal administration (Q3D & QD). The pharmacokinetics of DATK32 (25 mg/kg, QD) showed significantly higher mean concentrations of DATK32 when delivered via intra-cecal administration at 1, 2, and 4 h post-dose in the gastrointestinal contents, and 1, 2, 4 and 24 h in colon tissue as compared with the mean concentrations of DATK32 following intraperitoneal administration. The mean number of gut-homing T cells (Th memory cells) was significantly higher in the blood of groups treated with DATK32 via intra-cecal administration (QD 25 mg/kg and QD 5 mg/kg) as compared to the groups treated with DATK32 via intraperitoneal administration (Q3D 25 mg/kg). The mean number of Th memory cells was significantly lower in the Peyer's Patches of groups treated with DATK32 via intra-cecal administration (QD 25 mg/kg and 5 mg/kg) as compared to the groups treated with DATK32 via intraperitoneal administration (Q3D 25 mg/kg). The mean number of Th memory cells in mesenteric lymph nodes (MLN) was significantly lower in groups treated with DATK32 via intra-cecal administration (QD and Q3D 25 mg/kg and QD 5 mg/kg) as compared to the groups treated with DATK32 via intraperitoneal administration (Q3D 25 mg/kg).

[0379] In sum, these data show that the compositions and devices provided herein can suppress the local immune response in the intestine, while having less of a suppressive effect on the systemic immune response of an animal. These data also show that the release of DATK-32 antibody in the colon can result in a suppression of leukocyte recruitment and may provide for the treatment of colitis and other pro-inflammatory diseases of the intestine.

Example 5. An Assessment of DATK32 Bio-Distribution Following Intracecal Administration in Male C57B 1/6 Mice

[0380] The objective of this study is to assess DATK32 bio-distribution when dosed intracecally in male C57B1/6 mice. A minimum of 10 days prior to the start of the experiment a cohort of animals will undergo surgical implantation of a cecal cannula. A sufficient number of animals will undergo implantation to allow for 24 cannulated animals to be enrolled in the main study (e.g., 31 animals). Animals were dosed with vehicle or test article via intracecal injection (IC) on Day 0 as indicated in Table 3. Animals from all groups were sacrificed for terminal sample collection three hours following test article administration.

Materials and Methods

Mice

[0381] Normal male C57B1/6 mice between the ages of 6-8 weeks old, weighing 20-24 g, were obtained from Charles River Laboratories. The mice were randomized into two groups of twelve animals, and housed in groups of 12 per cage, and acclimatized for at least three days prior to entering the study. Animal rooms were set to maintain a minimum of 12 to 15 air changes per hour, with an automatic timer for a light/dark cycle of 12 hours on/off, and fed with Labdiet 5053 sterile rodent chow, with water administered *ad libitum*.

Cecal Cannulation

[0382] The animals were placed under isoflurane anesthesia, with the cecum exposed via a midline incision in the abdomen. A small point incision was made in the distal cecum where 1-2 cm of the cannula was inserted. The incision was closed with a purse string suture using 5-0 silk. An incision was then made in the left abdominal wall through which the distal end of the cannula was inserted and pushed subcutaneously to the dorsal aspect of the back. The site was then washed copiously with warmed saline prior to closing the abdominal wall. A small incision was also made in the skin of the back between the shoulder blades, exposing the tip of the cannula. The cannula was secured in place using suture, wound clips, and tissue glue. All animals received 1 mL of warm sterile saline (subcutaneous injection) and were

EP 3 554 485 B9

monitored closely until recovery before returning to their cage. All animals received 0.6 mg/kg BID buprenorphine for the first 3 days, and Baytril® at 10mg/Kg every day for the first 5 days post-surgery.

Dosing

[0383] Animals were dosed IC at a volume of 0.075 mL/animal on Days 0 as indicated in Table 3.

Sacrifice

[0384] All animals were euthanized by CO₂ inhalation three hours after dosing on Day 0.

Sample Collection

[0385] Terminal blood was collected and prepared for plasma using K₂EDTA as the anti-coagulant. The plasma will be split into two cryotubes, with 50 µL in one tube (PK analysis) and the remainder in another (other). Both samples were flash-frozen in liquid nitrogen. Plasma was stored at -80°C for downstream analysis. Mesenteric lymph nodes (mLN) were collected, weighed, and flash-frozen in liquid nitrogen. Mesenteric lymph nodes were stored at -80°C for downstream analysis. The small intestine was excised and rinsed, and the most distal 1 cm of ileum was dissected, weighed, and flash-frozen in liquid nitrogen. The samples were stored at -80°C for downstream analysis. The cecum and colon were removed from each animal and contents collected, weighed, and snap frozen in separate cryovials. The samples were stored at -80°C for downstream analysis. The colon was rinsed, and the most proximal 1 cm of colon was weighed and flash-frozen in liquid nitrogen. The snap frozen tissues were stored at -80 °C.

Table 3. Study Design

Group	N° Animals	Treatment	Route	Schedule	Terminal Collections Day 0
1	12	Vehicle (PBS)	IC	Day 0 **	Blood (plasma) Small intestine mLN
2	12	DATK32			
		(625 µg)*			Colon Colon Contents Cecum Contents
*Per mouse. TA was administered in 0.075 mL/animal. DATK32 was delivered in sterile PBS.					
**Animals were dosed on Day 0 and collections were performed 3 hours later.					

Results

[0386] The data in FIGs. 63A-F show no significant differences in clinical observations. No gastrointestinal-specific or adverse effects were found in the group administered DATK32 via intra-cecal administration as compared to the group administered a vehicle control. No toxicity resulting from the treatments was reported. The level of DATK32 in the group intra-cecally administered DATK32 was significantly higher in cecum and colon content, and colon tissue compared to the group administered a vehicle control at 3h post-dose. A small amount of DATK32 was also detected in plasma, small intestine, and mesenteric lymph node in the group intra-cecally administered DATK32.

Example 6. Pharmacokinetics/Pharmacodynamics and Bioavailability of Adalimumab When Applied to a TNBS-damaged Mucosal Surface (Induced Colitis) in Swine

[0387] The purpose of this non-Good Laboratory Practice (GLP) study was to explore the PK/PD, and bioavailability of adalimumab when applied to a TNBS-damaged mucosal surface (induced colitis) in Yorkshire-Cross farm swine, and to determine an appropriate dose and frequency for studies where a drug will be delivered by the ingestible device system. The ingestible device system will be capable of delivering a TNF inhibitor (adalimumab) topically and locally to damaged mucosa in human patients with inflammatory bowel disease (IBD). The TNBS-induced colitis model was validated when a single administration on Day 1 of 40 mL of 100% ethanol (EtOH) mixed with 5 grams of TNBS diluted in 10 mL of water via an enema using a rubber catheter resulted in the intended reproducible induction of damaged mucosal surface (induced colitis) in Yorkshire-Cross farm swine.

[0388] This study investigated whether topical delivery of adalimumab would result in increased local mucosal tissue levels with limited drug reaching systemic circulation, as compared to subcutaneous administration; whether local mu-

cosal tissue levels of drug would be greater in damaged tissues when compared to normal tissues; whether increasing the dose of drug would result in increased mucosal tissue levels in local and distal TNBS-damaged tissues; and whether topical delivery of adalimumab would result in reductions in inflammatory cytokines such as TNF- α in damaged tissues, feces, and possibly blood.

[0389] All animals were subjected to intra-rectal administration of trinitrobenzene sulfonic acid (TNBS) to induce chronic colitis on day -2. All animals were fasted prior to colitis induction. Bedding was removed and replaced with rubber mats on day -3 to prevent ingestion of straw bedding material. The dose was 40 mL of 100% EtOH mixed with 5 grams of TNBS diluted in 10 mL of water, then instilled into the colon intra-rectally using a flexible gavage tube by a veterinary surgeon (deposited in a 10-cm portion of the distal colon and proximal rectum, and retained for 12 minutes by use of two Foley catheters with 60-mL balloons). Approximately 3 days after induction, macroscopic and microscopic alterations of colonic architecture were apparent: some necrosis, thickening of the colon, and substantial histologic changes were observed (Figures 49 and 50). The study employed 15 female swine (approximately 35 to 45 kg at study start) allocated to one of five groups. Group 1 employed three animals that were the treated controls. Each animal in Group 1 was administered adalimumab by subcutaneous injection at 40 mg in 0.8 mL saline. Groups 2, 3, 4, and 5 employed 3 animals in each group. Animals in these groups were administered intra-rectal adalimumab at 40 mg in 0.8 mL saline. The test drug (adalimumab) was administered to all groups on study day 1. The intra-rectal administrations (Groups 2-5) were applied to damaged mucosal surface of the bowel via intra-rectal administration by a veterinary surgeon. Blood (EDTA) was collected from all animals (cephalic, jugular, or catheter) on day -3 (n=15), -1 (n=15), and 6 (n=15), 12 (n=12), 24 (n=9), and 48 (n=6) hours post-dose (87 bleeds total). The EDTA samples were split into two aliquots, and one was centrifuged for PK plasma, and stored frozen (-80°C) for PK analyses and reporting. Fecal samples were collected for the same time-points (87 fecal collections). Fecal samples were flash-frozen in liquid nitrogen and then stored at -80°C for analysis of drug levels and inflammatory cytokines. Groups 2, 3, 4, and 5 were euthanized and subjected to gross necropsy and tissue collection 6, 12, 24, and 48 hours post-dose, respectively. Group 1 was similarly euthanized and necropsied 48 hours post-dose. The animals were euthanized via injection of a veterinarian-approved euthanasia solution as per the schedule. Immediately after euthanasia in order to avoid autolytic changes, colon tissues were collected, opened, rinsed with saline, and a detailed macroscopic examination of the colon were performed to identify macroscopic findings related to TNBS-damage. Tissue samples were taken from the proximal, mid, and distal transverse colon; the dose site; and the distal colon. Each tissue sample was divided into two approximate halves; one tissue section was placed into 10% neutral buffered formalin (NBF) and evaluated by a Board certified veterinary pathologist, and the remaining tissue section was flash frozen in liquid nitrogen and stored frozen at -80 °C. Clinical signs (ill health, behavioral changes, etc.) were recorded daily beginning on day -3. Additional pen-side observations were conducted once or twice daily. Animals observed to be in ill health were examined by a veterinarian. Body weight was measured for all animals on day -3, and prior to scheduled euthanasia. Table 4.1, depicted below, shows the study design.

Materials and Methods

Test Article

[0390] Adalimumab (EXEMPTIA™) is a Tumour Necrosis Factor (TNF) inhibitor. A single dose was pre-filled in a syringe (40 mg in a volume of 0.8 mL).

Table 4.1. Study Design Table

General	Sample size	Dose	Route	Days					Hours								
				-3	-2	-1	1	0.5	1	2	4	6	8	12	24	48	
Fast				•													
Food/Water		ad libidum	oral		•	•	•	•	•	•	•	•	•	•	•	•	•
Observations																	
clinical observations				•	•	•	•								•	•	•
body weight				•			•								•	•	•
Treatments (groups)																	
TNBS (all animals)			intra rectal		•												
1. Treated control	n=3	40mg in 0.8mL saline	sub-cutaneous				•										n=3
euthanized																	
2. Adalimumab	n=3	40mg in 0.8mL saline	intra rectal				•										
euthanized													n=3				
3. Adalimumab	n=3	40mg in 0.8mL saline	intra rectal				•										
euthanized																	
4. Adalimumab	n=3	40mg in 0.8mL saline	intra rectal				•										
euthanized																	
5. Adalimumab	n=3	40mg in 0.8mL saline	intra rectal				•								n=3		
euthanized																	n=3
Adalimumab (required)		600															
Samples																	
PBMCs			cephalic, jugular or catheter				•					•		•	•	•	•
Serum			cephalic, jugular or catheter	•		•	•					•		•	•	•	•
Fecal			rectal	•		•	•					•		•	•	•	•
Tissue			necropsy									•		•	•	•	•

(continued)

						Days				Hours									
						-3	-2	-1	1	0.5	1	2	4	6	8	12	24	48	
General		Sample size	Dose		Route														
Analysis																			
Histopathology		1 location	4 locations																
inflamed		45	180		H&E														
normal		45	180		H&E														
Blood																			
adalimumab		57			pbl				15					15		12	9	6	6
TNF α		87			pbl	15	15	15	15					15		12	9	6	6
Feces																			
adalimumab		57			pbl				15					15		12	9	6	6
TNF α		87			pbl	15	15	15	15					15		12	9	6	6
Tissue																			
Inflamed																			
adalimumab		45	180		pbl									3		3	3	6	6
TNF α		45	180		pbl									3		3	3	6	6
HER2		45	180		pbl									3		3	3	6	6
Normal																			
adalimumab		45	180		pbl									3		3	3	6	6
TNF α		45	180		pbl									3		3	3	6	6
HER2		45	180		pbl									3		3	3	6	6

Results

[0391] While subcutaneously administered adalimumab was detected at all times points tested in plasma, topically administered adalimumab was barely detectable in plasma (Figures 51 and 52). Both topical delivery and subcutaneous delivery of adalimumab resulted in reduced levels of TNF- α in colon tissue of TNBS-induced colitis animals, yet topical delivery of adalimumab was able to achieve a greater reduction in TNF- α levels (Figures 53 and 54).

[0392] Either subcutaneous or intra-rectal administration of adalimumab was well tolerated and did not result in death, morbidity, adverse clinical observations, or body weight changes. A decreased level of total TNBS-related inflammatory response was observed by adalimumab treatment via intra-rectal administration when applied to the damaged mucosal surface of the bowel when compared to subcutaneous delivery. A significantly higher concentration of adalimumab was measured in blood following subcutaneous delivery as compared to the blood concentration following intra-rectal administration. Intra-rectal administration of adalimumab decreased the total and normalized TNF α concentration over time (6~48h) and was more effective at reducing TNF α at the endpoint (48h) as compared to groups administered adalimumab subcutaneously.

[0393] In sum, these data show that the compositions and devices provided herein can suppress the local immune response in the intestine, while having less of a suppressive effect on the systemic immune response of an animal. For example, these data show that intracecal administration of adalimumab using a device as described herein can provide for local delivery of adalimumab to the site of disease, without suppressing the systemic immune response. These data also show that local administration of adalimumab using a device as described herein can result in a significant reduction of the levels of TNF α in diseases animals.

Example 7. Comparison of Systemic Versus Intracecal Delivery of Cyclosporine A

[0394] The objective of this study was to compare the efficacy of an immunosuppressant agent (cyclosporine A; CsA) when dosed systemically versus intracecally to treat dextran sulfate sodium salt (DSS)-induced colitis in male C57Bl/6 mice.

Experimental Design

[0395] A minimum of 10 days prior to the start of the experiment a cohort of animals underwent surgical implantation of a cecal cannula. A sufficient number of animals underwent implantation to allow for 44 cannulated animals to be enrolled in the main study (e.g., 76 animals). Colitis was induced in 60 male C57Bl/6 mice by exposure to 3% DSS-treated drinking water from day 0 to day 5. Two groups of eight additional animals (cannulated and non-cannulated) served as no-disease controls (Groups 1 and 2). Animals were dosed with cyclosporine A via intraperitoneal injection (IP), oral gavage (PO), or intracecal injection (IC) from day 0 to 14 as indicated in Table 5.1. All animals were weighed daily and assessed visually for the presence of diarrhea and/or bloody stool at the time of dosing. Mice underwent video endoscopy on days 10 and 14 to assess colitis severity. Images were captured from each animal at the most severe region of disease identified during endoscopy. Additionally, stool consistency was scored during endoscopy using the parameters defined in Table 5.2. Following endoscopy on day 14, animals from all groups were sacrificed and underwent terminal sample collection.

[0396] Specifically, animals in all treatment groups dosed on day 14 were sacrificed at a pre-dosing time point, or 1, 2, and 4 hours after dosing (n=3 / group / time point). Terminal blood was collected via cardiac puncture and prepared for plasma using K₂EDTA as the anti-coagulant. The blood cell pellet was retained and snap frozen while the resulting plasma was split into two separate cryotubes, with 100 μ L in one tube and the remainder in the second. Additionally, the cecum and colon were removed from all animals; the contents were collected, weighed, and snap frozen in separate cryovials. The colon was then rinsed, measured, weighed, and then trimmed to 6 cm in length and divided into five pieces. The most proximal 1 cm of colon was snap frozen for subsequent bioanalysis of cyclosporine A levels. Of the remaining 5 cm of colon, the most distal and proximal 1.5-cm sections were each placed in formalin for 24 hours, then transferred to 70% ethanol for subsequent histological evaluation. The middle 2-cm portion was bisected longitudinally and placed into two separate cryotubes, weighed, and snap frozen in liquid nitrogen. All plasma and frozen colon tissue were stored at -80 °C for selected end point analysis. For all control animals in Groups 1-4, there was an additional collection of 100 μ L of whole blood from all animals which was then processed for FACS analysis of α 4 and β 7 expression on T_H memory cells. The details of the study are shown in Table 5.1.

Table 5.1. Study Design

Group Number	1	2	3	4	13	14	15
Number of Animals	8	8	12	12	12	12	12

(continued)

Cecal Cannula	NO	YES	NO	YES	NO	YES	YES
DSS	N/A	N/A	3% DSS on Day 0 to Day 5				
Treatment	none	none	vehicle	vehicle	CsA	CsA	CsA
Dose (mg/kg)	N/A	N/A	N/A	N/A	10	10	3
Route	N/A	N/A	N/A	N/A	PO	IC	IC
Dosing Schedule	N/A	N/A	QD: Day 0 to 14	QD: Day 0 to 14	QD: Day 0 to 14	QD: Day 0 to 14	QD: Day 0 to 14
Endoscopy Schedule*	Days 10 and 14						
Endpoints Day 14	Endoscopy, Colon weight/ length, stool score Terminal Collection (all groups): Cecal contents, colon contents,						
	plasma, and colon tissue FACS analysis collection of Groups 1-4: Whole blood for the following FACS panel: CD4, CD44, CD45RB, α4, β7, CD 16/32						
PK Sacrifice (Day 14)	N=3/ time points At pre-dose and 1, 2, and 4 hours post-dosing						
*Animals were dosed once (QD) on Day 14 and plasma collected (K2EDTA) at pre-dosing, 1, 2, and 4 hours post-dosing from n=3/group/time point. Each collection was terminal.							

Experimental Procedures*Cecal Cannulation*

[0397] Animals were placed under isoflurane anesthesia, and the cecum exposed via a mid-line incision in the abdomen. A small point incision was made in the distal cecum through which 1-2 cm of the cannula was inserted. The incision was closed with a purse-string suture using 5-0 silk. An incision was made in the left abdominal wall through which the distal end of the cannula was inserted and pushed subcutaneously to the dorsal aspect of the back. The site was washed copiously with warmed saline prior to closing the abdominal wall. A small incision was made in the skin of the back between the shoulder blades, exposing the tip of the cannula. The cannula was secured in place using suture, wound clips, and tissue glue. All animals received 1 mL of warm sterile saline (subcutaneous injection) and were monitored closely until fully recovered before returning to the cage. All animals received buprenorphine at 0.6 mg/kg BID for the first 3 days, and Baytril® at 10 mg/kg QD for the first 5 days following surgery.

Disease Induction

[0398] Colitis was induced on day 0 via addition of 3% DSS (MP Biomedicals, Cat #0260110) to the drinking water. Fresh DSS/water solutions were made on day 3 and any of the remaining original DSS solution was discarded.

Dosing

[0399] Animals were dosed by oral gavage (PO), intraperitoneal injection (IP), or intracecal injection (IC) at a volume of 0.1 mL/20 g on days 0 to 14 as indicated in Table 5.1.

Body Weight and Survival

[0400] Animals were observed daily (weight, morbidity, survival, presence of diarrhea, and/or bloody stool) in order to assess possible differences among treatment groups and/or possible toxicity resulting from the treatments.

Animals Found Dead or Moribund

[0401] Animals were monitored on a daily basis and those exhibiting weight loss greater than 30% were euthanized, and samples were not collected from these animals.

Endoscopy

[0402] Each mouse underwent video endoscopy on days 10 and 14 using a small animal endoscope (Karl Storz Endoskope, Germany) under isoflurane anesthesia. During each endoscopic procedure still images as well as video were recorded to evaluate the extent of colitis and the response to treatment. Additionally, we attempted to capture an image from each animal at the most severe region of disease identified during endoscopy. Colitis severity was scored using a 0-4 scale (0 = normal; 1 = loss of vascularity; 2 = loss of vascularity and friability; 3 = friability and erosions; 4 = ulcerations and bleeding). Additionally, stool consistency was scored during endoscopy using the parameters defined in Table 5.2.

Table 5.2. Stool Consistency

Score	Description
0	Normal, well-formed pellet
1	Loose stool, soft, staying in shape
2	Loose stool, abnormal form with excess moisture
3	Watery or diarrhea
4	Bloody diarrhea

Tissue/Blood for FACS

[0403] Tissue and blood were immediately placed in FACS buffer (1x phosphate-buffered saline (PBS) containing 2.5% fetal calf serum (FCS)) and analyzed using the antibody panel in Table 5.3.

Table 5.3. FACS Antibody Panel

Antibody Target	Fluorochrome	Purpose
CD4	APC-Vio770	Defines T _H cells
CD44	VioBlue	Memory/ Naive discrimination
CD45RB	FITC	Memory/ Naive discrimination
$\alpha 4$	APC	Defines T _H -memory subset of interest
$\beta 7$	PE	Defines T _H -memory subset of interest
CD 16/32	-	Fc block

Results

[0404] The data in Figure 55 show a decrease in weight loss is observed in DSS mice intracably administered cyclosporine A as compared to DSS mice orally administered cyclosporine A. The data in Figure 56 show a decrease in plasma concentration of cyclosporine A in DSS mice intracably administered cyclosporine A as compared to DSS mice orally administered cyclosporine A. The data in Figures 57-59 show an increased concentration of cyclosporine A in the colon tissue of DSS mice intracably administered cyclosporine A as compared to the concentration of cyclosporine A in the colon tissue of DSS mice orally administered cyclosporine A.

[0405] The data in Figure 60 show that DSS mice intracably administered cyclosporine A have an increased concentration of IL-2 in colon tissue as compared to DSS mice orally administered cyclosporine A. The data in Figure 61 show that DSS mice intracably administered cyclosporine A have a decreased concentration of IL-6 in colon tissue as compared to DSS mice orally administered cyclosporine A.

[0406] In sum, these data show that the compositions and devices provided herein can suppress the local immune response in the intestine, while having less of a suppressive effect on the systemic immune response of an animal. For

example, these data demonstrate that the present compositions and devices can be used to release cyclosporine A to the intestine and that this results in a selective immune suppression in the colon, while having less of an effect on the immune system outside of the intestine. These data also suggest that the present compositions and devices will provide for the treatment of colitis and other pro-inflammatory disorders of the intestine.

Example 8. Bellows Testing: Drug Stability Bench Test

[0407] Experiments were run to evaluate the effects that bellows material would have on the function of a drug used as the dispensable substance. The experiments also evaluated the effects on drug function due to shelf life in the bellows.

[0408] The adalimumab was loaded into simulated device jigs containing either tapered silicone bellows or smooth PVC bellows and allowed to incubate for 4, 24, or 336 hours at room temperature while protected from light. FIG. 64 illustrates the tapered silicone bellows, and FIG. 65 illustrates the tapered silicone bellows in the simulated device jig. FIG. 66 illustrates the smooth PVC bellows, and FIG. 67 illustrates the smooth PVC in the simulated device jig.

[0409] The drug was subsequently extracted using the respective dispensing systems and tested by a competitive inhibition assay. The test method has been developed from the literature (Velayudhan et al., "Demonstration of functional similarity of proposed biosimilar ABP501 to adalimumab" BioDrugs 30:339-351 (2016) and Barbeau et al., "Application Note: Screening for inhibitors of TNF α /s TNFR1 Binding using AlphaScreen™ Technology". PerkinElmer Technical Note ASC-016. (2002)), as well as pre-testing development work using control drug and experiments using the provided AlphaLISA test kits. FIG. 68 demonstrates the principle of the competition assay performed in the experiment.

[0410] The bellows were loaded as follows: aseptically wiped the dispensing port of the simulated ingestible device jig with 70% ethanol; allowed to air dry for one minute; used an adalimumab delivery syringe to load each set of bellows with 200 μ L of drug; took a photo of the loaded device; gently rotated the device such that the drug is allowed to come in contact with all bellows surfaces; protected the bellows from light; and incubate at room temperature for the predetermined time period to allow full contact of the drug with all bellows' surfaces.

[0411] The drug was extracted as follows: after completion of the incubation period; the device jig was inverted such that the dispensing port was positioned over a sterile collection microfuge tube and petri dish below; five cubic centimeters of air was drawn into an appropriate syringe; the lure lock was attached to the device jig; the syringe was used to gently apply positive pressure to the bellow with air such that the drug was recovered in the collection microfuge tube; where possible, a video of drug dispensing was taken; samples were collected from each bellows type; a control drug sample was collected by directly dispensing 200 μ L of drug from the commercial dispensing syringe into a sterile microfuge tube; the control drug-free sample was collected by directly dispensing 200 μ L of PBS using a sterile pipette into a sterile microfuge tube; the collected drug was protected from light; and the drug was diluted over the following dilution range (250, 125, 25, 2.5, 0.25, 0.025, 0.0125, 0.0025 μ g) in sterile PBS to determine the IC₅₀ range of the drug.

[0412] To determine any effects storage conditions may have on drug efficacy in the device, the drug (stored either in the syringe, silicon bellows, PVC bellows) was stored at room temperature while protected from light for 24 hours and 72 hours. Samples were then extracted and the steps in the preceding paragraph were repeated. The AlphaLISA (LOCI™) test method was used. Human TNF α standard dilution ranges were prepared as described in Table 6.

Table 6

Tube	Vol. of human TNF α (μ L)	Vol. of diluent (μ L) *	[human TNF α] in standard curve	
			(g/mL in 5 μ L)	(pg/mL in 5 μ L)
A	10 μ L of reconstituted human TNF α	90	1E-07	100 000
B	60 μ L of tube A	140	3E-08	30 000
C	60 μ L of tube B	120	1E-08	10 000
D	60 μ L of tube C	140	3E-09	3 000
E	60 μ L of tube D	120	1E-09	1 000
F	60 μ L of tube E	140	3E-10	300
G	60 μ L of tube F	120	1E-10	100
H	60 μ L of tube G	140	3E-11	30
I	60 μ L of tube H	120	1E-11	10
J	60 μ L of tube I	140	3E-12	3
K	60 μ L of tube J	120	1E-12	1

(continued)

Tube	Vol. of human TNF α (μ L)	Vol. of diluent (μ L) *	[human TNF α] in standard curve	
			(g/mL in 5 μ L)	(pg/mL in 5 μ L)
L	60 μ L of tube K	140	3E-13	0.3
M ** (background)	0	100	0	0
N ** (background)	0	100	0	0
O ** (background)	0	100	0	0
P ** (background)	0	100	0	0

[0413] The test was performed as follows: the above standard dilution ranges were in a separate 96-well plate; to ensure consistent mixing, samples were mixed up and down gently with a pipette five times; a 384-well test plate was prepared according to the test layout diagram depicted Table 7; five microliters of 10,000 pg/mL TNF α standard from the previously made dilution plate was added to each corresponding concentration as shown in Table 6; five microliters of recovered drug (directly from the commercial syringe (A), from the silicone bellows (B Si), from the PVC bellows (B PVC), or from the PBS control (C) was added into the corresponding wells described in Table 5; the test plate was incubated for one hour at room temperature while protected from light; 10 microliters of acceptor beads were added to each previously accessed well; the wells were incubated for 30 minutes at room temperature while protected from light; 10 μ L of biotinylated antibody was added to each previously accessed well; the wells were incubated for 15 minutes at room temperature, while protected from light; the room lights were darkened and 25 microliters of streptavidin (SA) donor beads were added to each previously accessed well; the wells were incubated for 30 minutes at room temperature while protected from light; the plate was read in Alpha Mode; and the results were recorded. Upon addition of reagent(s) in the various steps, each well was pipetted up and down three times to achieve good mixing.

Table 7

	1	2	3	4	5	6	7	8	9	10	11	12	13	14	15	16	17	18	19	20	21	22	23
A	STD2 1.00E+05		STD10 10	250 A	250 A	250 A	250 A	250 A	250 B Si	250 B Si	250 B Si	250 B Si	250 B Si	250 B PVC	250 B PVC	250 B PVC	250 B PVC	250 B PVC	250 C	250 C	250 C	250 C	250 C
B																							
C	STD3 30000		STD11 3	125 A	125 A	125 A	125 A	125 A	125 B Si	125 B Si	125 B Si	125 B Si	125 B Si	125 B PVC	125 B PVC	125 B PVC	125 B PVC	125 B PVC	125 C	125 C	125 C	125 C	125 C
D																							
E	STD4 10000		STD12 1	25 A	25 A	25 A	25 A	25 A	25 B Si	25 B Si	25 B Si	25 B Si	25 B Si	25 B PVC	25 B PVC	25 B PVC	25 B PVC	25 B PVC	25 C	25 C	25 C	25 C	25 C
F																							
G	STD5 3000		STD13 0.333	2.5 A	2.5 A	2.5 A	2.5 A	2.5 A	2.5 B Si	2.5 B Si	2.5 B Si	2.5 B Si	2.5 B Si	2.5 B PVC	2.5 B PVC	2.5 B PVC	2.5 B PVC	2.5 B PVC	2.5 C	2.5 C	2.5 C	2.5 C	2.5 C
H																							
I	STD6 1000		Blank 0	0.25 A	0.25 A	0.25 A	0.25 A	0.25 A	0.25 B Si	0.25 B Si	0.25 B Si	0.25 B Si	0.25 B Si	0.25 B PVC	0.25 B PVC	0.25 B PVC	0.25 B PVC	0.25 B PVC	0.25 C	0.25 C	0.25 C	0.25 C	0.25 C
J																							
K	STD7 300		Blank 0	0.025 A	0.025 A	0.025 A	0.025 A	0.025 A	0.025 B Si	0.025 B Si	0.025 B Si	0.025 B Si	0.025 B Si	0.025 B PVC	0.025 B PVC	0.025 B PVC	0.025 B PVC	0.025 B PVC	0.025 C	0.025 C	0.025 C	0.025 C	0.025 C
L																							
M	STD8 100		Blank 0	0.013 A	0.013 A	0.013 A	0.013 A	0.013 A	0.013 B Si	0.013 B Si	0.013 B Si	0.013 B Si	0.013 B Si	0.013 B PVC	0.013 B PVC	0.013 B PVC	0.013 B PVC	0.013 B PVC	0.013 C	0.013 C	0.013 C	0.013 C	0.013 C
N																							
O	STD9 30		Blank 0	0.003 A	0.003 A	0.003 A	0.003 A	0.003 A	0.003 B Si	0.003 B Si	0.003 B Si	0.003 B Si	0.003 B Si	0.003 B PVC	0.003 B PVC	0.003 B PVC	0.003 B PVC	0.003 B PVC	0.003 C	0.003 C	0.003 C	0.003 C	0.003 C
P																							

[0414] The data are shown in FIGs. 69-71. The data demonstrate that the bellows do not negatively impact the drug function after shelf lives of 4 hours, 24 hours, or 336 hours. The IC₅₀ values of the drug dispensed from the bellows were comparable to the IC₅₀ values of the standard dispensation method (Table 6). A slight right shift was noted in the bellows curves after 24 hours (FIG. 70), but this shift was well within the error bars of the curves. Tables 8-11 represent data of FIGs. 69-71, respectively. Of note, when comparing mean (n=5) RFU data between test articles over the concentration ranges significant differences (p<0.05) were discerned. However, these significant differences did not favor

EP 3 554 485 B9

either test article over time, suggesting that they were not related to the performance of the material in response to the drug (FIGs. 69-71).

Table 8

	Needle control (A)	Silicone Bellows (B)	PVC Bellows (C)
4 Hours	0.0174	0.0169	0.0172
24 Hours	0.0180	0.0180	0.0180
336 Hours	0.0144	0.0159	0.0163

Table 9

Statistics (Student's T-test, 2 tailed, non-pair-wise, for significance $p < 0.05$)			
Drug (micrograms)	Needle control (A) vs. Silicone (B)	Needle control (A) vs. PVC	Silicone vs. PVC
0.0001	0.911	0.008*	0.268
0.0025	0.138	0.390	0.822
0.0125	0.122	0.118	0.771
0.025	0.143	0.465	0.020*
0.25	0.591	0.984	0.350
2.5	0.243	0.124	0.169
125	0.867	0.688	0.182
250	0.681	0.184	0.108
* $p < 0.5$ data set			

Table 10

Statistics (Student's T-test, 2 tailed, non-pair-wise, for significance $p < 0.05$)			
Drug (micrograms)	Needle control (A) vs. Silicone (B)	Needle control (A) vs. PVC	Silicone vs. PVC
0.0001	0.132	0.038*	0.292
0.0025	0.003*	0.076	0.575
0.0125	0.161	0.022*	0.783
0.025	0.058	0.078	0.538
0.25	0.974	0.384	0.198
2.5	0.714	0.080	0.017*
125	0.873	0.731	0.269
250	0.798	0.956	0.903
* $p < 0.5$ data set			

Table 11

Statistics (Student's T-test, 2 tailed, non-pair-wise, for significance $p < 0.05$)			
Drug (micrograms)	Needle control (A) vs. Silicone (B)	Needle control (A) vs. PVC	Silicone vs. PVC
0.0001	0.858449	0.036847*	0.026444 *
0.0025	0.087379	0.280302	0.046767*

(continued)

Statistics (Student's T-test, 2 tailed, non-pair-wise, for significance $p < 0.05$)			
Drug (micrograms)	Needle control (A) vs. Silicone (B)	Needle control (A) vs. PVC	Silicone vs. PVC
0.0125	0.469282	0.057232	0.117194
0.025	0.02758*	0.078234	0.373419
0.25	0.411548	0.258928	0.400498
2.5	0.368959	0.156574	0.006719*
125	0.948649	0.246702	0.463735
250	0.485046	0.128993	0.705543
* $p < 0.5$ data set			

Example 9. A Comparison Study of Systemic vs Intracecal Delivery of SMAD7 Bio-Distribution in DSS-Induced Colitis in Male C57Bl/6 Mice

[0415] The objective of this study was to compare the efficacy of novel test articles, e.g., fluorescent SMAD7 antisense oligonucleotides (SMAD7 AS), when dosed systemically versus intracecally in the treatment of DSS-induced colitis, in male C57Bl/6 mice.

Experimental Design

[0416] A minimum of 10 days prior to the start of the experiment a cohort of animals underwent surgical implantation of a cecal cannula. A sufficient number of animals underwent implantation to allow for 12 cannulated animals to be enrolled in the main study (i.e., 16 animals).

[0417] Colitis was induced in 12 male C57Bl/6 mice (Groups 4-5) by exposure to 3% DSS-treated drinking water from Day 0 to Day 5. Three groups of six additional animals per group ($n = 6$ cannulated; $n = 12$ non-cannulated; Groups 1-3) served as no-disease controls (Groups 1-3). All animals were weighed daily and assessed visually for the presence of diarrhea and/or bloody stool during this time.

[0418] Animals were dosed with test-article via oral gavage (PO) or intracecal injection (IC) once on Day 9 as indicated in Table 12. The animals in Group 0 were not dosed. The animals in Groups 2 and 4 were dosed PO with SMAD7 antisense. The animals in Groups 3 and 5 were dosed IC with SMAD7 antisense.

[0419] All animals were euthanized by CO₂ inhalation 12 hours after dosing, on Day 10. Terminal blood was collected into two K₂EDTA tubes and processed for plasma. Both plasma and pellet samples were snap-frozen in liquid nitrogen and stored at -80 °C. Cecum contents were removed and the contents were split into two aliquots. Both aliquots were weighed and snap frozen in separate cryovials in liquid nitrogen. The cecum was excised and bisected longitudinally; each piece is separately weighed and flash-frozen in liquid nitrogen. The colon contents were removed and the contents were split into two aliquots. Both aliquots were weighed and snap frozen in separate cryovials in liquid nitrogen. The colon was then rinsed, and the most proximal 2 cm of colon was collected. This 2-cm portion was bisected longitudinally; each piece was separately weighed and flash-frozen in liquid nitrogen. Snap-frozen blood pellet, cecum/colon contents, and tissue samples were used for downstream fluoremetry or RP-HPLC. The details of the study design are shown in Table 12.

Table 12: Study design

Group	No Animals	Cecal Cannula	Colitis Induction	Treatment	Route	Schedule	Terminal Collections Day 10
-------	------------	---------------	-------------------	-----------	-------	----------	-----------------------------

(continued)

Group	No Animals	Cecal Cannula	Colitis Induction	Treatment	Route	Schedule	Terminal Collections Day 10
1	6	NO	--	--	--	--	Whole blood, plasma, cecal contents, colon contents, cecal tissue, colon tissue
2	6	NO		Fluorescently labeled SMAD7 antisense 50 μ g*	PO	QD Day 9**	
3	6	YES			IC		
4	6	NO	PO				
5	6	YES	3% DSS Days 0-5		IC		

*Per mouse. TA is administered in 0.075 mL/animal.

**Animals are dosed on Day 9 and collections are performed 12 hours later.

Materials and Methods

Mice

[0420] Normal male C57Bl/6 mice between the ages of 6-8 weeks old, weighing 20-24 g, were obtained from Charles River Laboratories. The mice were randomized into five groups of six mice each, and housed in groups of 8-15 per cage, and acclimatized for at least three days prior to entering the study. Animal rooms were set to maintain a minimum of 12 to 15 air changes per hour, with an automatic timer for a light/dark cycle of 12 hours on/off, and fed with Labdiet 5053 sterile rodent chow, with water administered *ad libitum*.

Cecal Cannulation

[0421] The animals were placed under isoflurane anesthesia, with the cecum exposed via a midline incision in the abdomen. A small point incision was made in the distal cecum, where 1-2 cm of the cannula was inserted. The incision was closed with a purse string suture using 5-0 silk. An incision was then made in the left abdominal wall through which the distal end of the cannula was inserted and pushed subcutaneously to the dorsal aspect of the back. The site was then washed copiously with warmed saline prior to closing the abdominal wall. A small incision was also made in the skin of the back between the shoulder blades, exposing the tip of the cannula. The cannula was secured in place using suture, wound clips, and tissue glue. All animals were administered 1 mL of warm sterile saline (subcutaneous injection) and were monitored closely until recovery before returning to their cage. All animals were administered 0.6 mg/kg BID buprenorphine for the first 3 days, and Baytril® at 10mg/Kg every day for the first 5 days post-surgery.

Disease Induction

[0422] Colitis was induced on Day 0 via addition of 3% DSS (MP Biomedicals, Cat #0260110) to the drinking water. Fresh DSS/water solutions was provided on Day 3 and any of the remaining original DSS solution is discarded.

Body Weight and Survival

[0423] Animals were observed daily (weight, morbidity, survival, presence of diarrhea and/or bloody stool) in order to assess possible differences among treatment groups and/or possible toxicity resulting from the treatments.

Animals Found Dead or Moribund

[0424] Animals were monitored on a daily basis. Animals exhibiting weight loss greater than 30% were euthanized, and samples were not collected from these animals.

Dosing

[0425] Animals were dosed with test-article via oral gavage (PO) or intracecal injection (IC) once on Day 9 as indicated in Table 12. Animals in Group 0 were not dosed. Animals in Groups 2 and 4 were dosed PO with SMAD7 antisense. Animals in Groups 3 and 5 were dosed IC with SMAD7 antisense.

Sacrifice

[0426] All animals were euthanized by CO₂ inhalation 12 hours after dosing, on Day 10.

Sample Collection

[0427] Intestinal contents, peripheral blood and tissue were collected at sacrifice on Day 10, as follows:

Blood/Plasma

[0428] Terminal blood was collected into two K₂EDTA tubes and processed for plasma. The approximate volume of each blood sample was recorded prior to centrifugation. Both plasma and pellet samples were snap-frozen in liquid nitrogen and stored at -80 °C. The first pellet sample (sample 1) was used for fluorometry. The second pellet sample (sample 2) was used for RP-HPLC.

Cecum Contents

[0429] Cecum contents was removed and contents were split into two aliquots. Both aliquots were weighed and snap frozen in separate cryovials in liquid nitrogen. The first sample (sample 1) was used for fluorometry. The second sample (sample 2) was used for RP-HPLC.

Cecum

[0430] The cecum was excised and bisected longitudinally; each piece was separately weighed and snap-frozen. The first sample (sample 1) was used for fluorometry. The second sample (sample 2) was used for RP-HPLC.

Colon Contents

[0431] Colon contents were removed and contents were split into two aliquots. Both aliquots were weighed and snap frozen in separate cryovials in liquid nitrogen. The first sample (sample 1) was used for fluorometry. The second sample (sample 2) was used for RP-HPLC.

Colon

[0432] The colon was rinsed, and the most proximal 2 cm of colon was collected and bisected longitudinally. Each piece was separately weighed and flash-frozen in liquid nitrogen. The first sample (sample 1) was used for fluorometry. The second sample (sample 2) was used for RP-HPLC.

SMAD7 Antisense Bioanalysis

[0433] Samples flash-frozen for fluoremetry were homogenized in 0.5 mL buffer RLT+ (Qiagen). Homogenate was centrifuged (4000 × g; 10 minutes), and supernatant was collected. Forty microliters of the sample was diluted 1:6 in 200 µL of bicarbonate solution and 100 µL of diluted supernatant was analyzed on a fluorescent plate reader (485 excitation; 535 emission) in duplicate.

[0434] Prior to the above, assay development was performed as follows. Samples (as indicated in *Sample Collection*) were harvested from a naive animal and flash-frozen. Samples were then homogenized in 0.5 mL buffer RLT+, homogenate was centrifuged (4000 × g; 10 minutes) and supernatant was collected and diluted 1:6 with bicarbonate solution (i.e., 0.5 mL supernatant was added to 2.5 mL of PBS). An aliquot (0.200 mL (90 µL for each duplicate) of each diluted sample was pipetted into 15 (14 dilution of FAM-AS-SAMD7+ blank control) Eppendorf tubes. One tube was set-aside to be used as a blank sample. Ten microliters of fluorescently-labeled SMAD7 antisense was then spiked into all other sample to achieve final concentrations of 50 µg/mL, 16.67 µg/mL, 5.56 µg/mL, 1.85 µg/mL, 0.62 µg/mL, 0.21 µg/mL, 0.069 µg/mL, 0.023 µg/mL, 7.6 ng/mL, 2.5 ng/mL, 0.847 ng/mL, 0.282 ng/mL, 0.094 ng/mL, and 0.024 ng/mL respectively. The fluorescently-labeled SMAD7 antisense was prepared and serially diluted such that the volume added to each organ homogenate sample was the same for each of the above concentrations. These samples were analyzed on a fluorescent plate reader (485 excitation; 535 emission) in duplicate.

Processing for RP-HPLC

[0435] Samples flash-frozen for RP-HPLC were homogenized in buffer RLT+ (Qiagen). Homogenate was centrifuged (4000 x g; 10 minutes), and supernatant was used to perform RP-HPLC analysis.

Results

[0436] The data in Figures 73 and 74 show that significantly more SMAD7 antisense oligonucleotide was present in cecum tissue and colon tissue for mice with or without DSS treatment that were intra-cecally administered the SMAD7 antisense oligonucleotide as compared to mice with or without DSS treatment that were orally administered the SMAD7 antisense oligonucleotide. The data in Figure 75 show that there is about the same level of SMAD7 antisense oligonucleotide in the cecum contents of mice with or without DSS treatment that were orally or intra-cecally administered the SMAD7 antisense oligonucleotide. No SMAD7 antisense oligonucleotide was found in the plasma or white blood cell pellet of SMAD7 antisense oligonucleotide treated mice.

Example 10. Comparison of the Tissue, Plasma, and GI Content Pharmacokinetics of Tacrolimus through Oral vs. Intra-Cecal Ingestible Device Delivery in Yorkshire-Cross Farm Swine

[0437] The primary objective of this study was to compare the tissue, plasma, rectal sample, and GI content pharmacokinetics of tacrolimus through oral versus intra-cecal ingestible device delivery in normal Yorkshire-Cross farm swine.

[0438] This study compares the effects of administration of: a single intra-cecal administration of an ingestible device containing 0.8 mL sterile vehicle solution (80% alcohol, 20% castor oil (HCO-60)); a single oral dose of tacrolimus at 4 mg/0.8 mL (in sterile vehicle solution); and a single intra-cecal administration of an ingestible device containing either 1 mg/0.8 mL (in sterile vehicle solution), 2 mg/0.8 mL (in sterile vehicle solution), or 4 mg/0.8 mL (in sterile vehicle solution).

[0439] This study employed five groups of three female swine weighing approximately 45 to 50 kg at study start. Swine were randomly placed into animal rooms/pens as they are transferred from the delivery vehicle without regard to group. Group numbers were assigned to the rooms in order of room number. No further randomization procedure was employed. The study design is provided in Table 13.

Table 13. Study Design Table

				Days Pre-Dose							Hours Post-dose						
				-11	-10	-5	-1	1			0.5	1	2	3	4	6	12
General	Group size	Dose	Route														
Fast Food/Water		ad libitum	
Observations																	
clinical observations		Day -10~-5 & Day 1	
body weight*			
Treatments (Groups)																	
1. Vehicle control	n=3	0.8 mL (20% HCO-60, 80% EtOH)	IC														
Surgical placement of IC port** Euthanized		(1 Ingestible Device)		.													n=3
2. Tacrolimus (PO)	n=3	4 mg in 0.8 mL 0.08mg/kg (solution)	Oral		.			.									n=3
Surgical placement of IC port** Euthanized				.													
3. Tacrolimus (IC)	n=3	1 mg in 0.8 mL 0.02 mg/kg (1 Ingestible Device)	IC		.			.									n=3
Surgical placement of IC port** Euthanized				.													
4. Tacrolimus (IC)	n=3	2 mg in 0.8 mL 0.04 mg/kg (1 Ingestible Device)	IC		.			.									n=3
Surgical placement of IC port** Euthanized				.													
5. Tacrolimus (IC)	n=3	4 mg in 0.8 mL 0.08 mg/kg (1 Ingestible Device)	IC		.			.									n=3
Surgical placement of IC port** Euthanized				.													

(continued)

	General	Group size	Dose	Route	Days Pre-Dose							Hours Post-dose						
					-11	-10	-5	-1	1			0.5	1	2	3	4	6	12
Tacrolimus (required)			20 mg															
Samples****																		
Plasma																		
Rectal contents																		
Tissue***		x5		cephalic, jugular or catheter rectal necropsy														
Luminal contents		x5		necropsy														
Analysis (Agrilux Charles River)		Total Samples																
Plasma																		
[Tacrolimus]		105																
Rectal contents																		
[Tacrolimus]		60																
Tissue (intact)***																		
[Tacrolimus]		105																105
Luminal contents																		
[Tacrolimus]		75																75
Tissue after removing luminal content																		
[Tacrolimus]		75																75
Notes: *Animal weight was ~45-50 kg for drug doses proposed. **Surgical placement of IC port in all animals to control. ***Tissue samples [drug] (five GI section cecum (CAC); proximal colon (PCN); transverse colon (TCN); distal colon (DCN); rectum (RTM), plus mesenteric lymph nodes and Peyer's Patch). ****Luminal contents (cecum (CAC); proximal colon (PCN); transverse colon (TCN); distal colon (DCN); rectum (RTM)).																		

[0440] Animals in Group 1 received an ingestible device containing 0.8 mL of vehicle solution (80% alcohol, 20% HCO-60). Animals in Group 2 received orally 4 mL liquid formulation of tacrolimus at 4 mg/0.8 mL per animal (Prograf: 5 mg/mL). Animals in Group 3 received intra-cecally an ingestible device containing tacrolimus at 1 mg in 0.8 mL per ingestible device. Animals in Group 4 received intra-cecally an ingestible device containing tacrolimus at 2 mg in 0.8 mL per ingestible device. Animals in Group 5 received intra-cecally an ingestible device containing tacrolimus at 4 mg in 0.8 mL per ingestible device. To control for potential confounding effects of the surgery, all groups fast on Day -11 at least 24 hr before being subjected to anesthesia followed by surgical placements of a cecal port by a veterinary surgeon at Day -10. All animals were fasted for at least 12 hr prior to dosing on Day 1. Animals were dosed via either intra-cecal dosing (IC) or oral dosing (PO) at Day 1 (between 6-8 p.m.). All animals resumed feeding at approximately 4 hours after dose (11-12 p.m. after dosing).

[0441] Animals in Group 1 (Vehicle Control) were administered a single intra-cecal ingestible device containing 0.8 mL Vehicle solution (80% alcohol, 20% castor oil (HCO-60) on Day 1. On Day -10 the animals were anesthetized, and a veterinary surgeon surgically placed an intra-cecal port in each animal. On Day 1, each animal was placed into a sling then a single intra-cecal ingestible device containing 0.8 mL vehicle solution (80% alcohol, 20% castor oil (HCO-60)) is introduced by the veterinary surgeon into the cecum via the cecal port in each animal. Following ingestible device placement, the animals were removed from the slings and placed back into their pens with water. All animals resumed feeding at approximately 4 hours after dose. Samples of rectal contents were collected for pharmacokinetic analyses from each animal at each of 1, 3, 6, and 12 hours post-ingestible device placement using a fecal swab (rectal swab). A total of 60 samples were collected.

[0442] Approximately 200-400 mg of rectal content were collected, if available, with a fecal swab (Copan Diagnostics Nylon Flocked Dry Swabs, 502CS01). The fecal swab was pre-weighed and weighed after collection in the collection tube (Sterile Tube and Cap No Media, PFFM913S), and the sample weight was recorded. The fecal swab was broken via the breakpoint, and was stored in the collection tube, and immediately frozen at -70 °C. Whole blood (2 mL) was collected into K₂EDTA coated tubes for pharmacokinetics at each time-point of pre-dose and 1, 2, 3, 4, 6 and 12 hours post-dose. Immediately following euthanasia, tissue was collected. A total of 105 samples were collected.

[0443] For tissue necropsy, small intestine fluid and cecal fluid were collected separately from all the animals into two separate square plastic bottles, and stored at -20 °C. The length and diameter of the cecum and the colon was measured from one animal in each group and recorded for reference. Tissues were collected for pharmacokinetic analyses and include mesenteric lymph nodes, a Peyer's Patch, and five gastrointestinal sections, including cecum, proximal colon, transverse colon, distal colon, and rectum. All samples were weighed, and the tissue sample weights were recorded. In each of the five gastrointestinal sections, tissue samples were collected in three different areas where the mucosal surface was visible and not covered by luminal content by using an 8.0-mm punch biopsy tool. Around 3 grams of the total punched sample were collected into a pre-weighed 15-mL conical tube, and the tissue weight was recorded. Three mesenteric lymph nodes were collected from different areas and weighed. At least one Peyer's Patch was collected and weighed. Tissues were snap-frozen in liquid nitrogen and stored frozen at approximately -70 °C or below (total of 105 samples).

[0444] Luminal contents were collected for pharmacokinetic analyses from the surface of the tissue from each of five gastrointestinal sections: cecum, proximal colon, transverse colon, distal colon, and rectum (total of 75). The contents were collected in pre-weighed 15-mL conical tubes and the sample weights were recorded. Samples were snap-frozen in liquid nitrogen stored frozen at approximately -70 °C or below.

[0445] After removing the luminal content, another set of tissue samples from 3 different areas were collected via an 8.0-mm punch biopsy in each section of the five tissue gastrointestinal sections described above. Around 3 grams of the total punched sample were collected into a pre-weighed 15-mL conical tube, and the tissue weight was recorded (total of 75). Tissues were snap-frozen in liquid nitrogen and stored frozen at approximately -70 °C or below.

[0446] A 30-cm length of jejunum (separated into two 15 cm lengths), and the remaining distal and transverse colon tissue sample (after tissue and luminal content were collected for PK) were collected in one animal in each group of treatment, snap-frozen in liquid nitrogen and stored frozen at approximately -70 °C or below. All samples for pharmacokinetic analyses were stored on dry ice before analyses.

[0447] Group 2 animals were administered a single oral dose of tacrolimus at 1 mg/0.8 mL (in the vehicle solution) on Day 1. Plasma, rectal content sample, tissue collection, GI content collection and related procedures/storage/shipments was the same as those employed in Group 1.

[0448] Group 3 animals were administered a single intra-cecal ingestible device containing tacrolimus at 0.5 mg/0.8 mL (in the vehicle solution) on Day 1 by a veterinary surgeon. Plasma, rectal content sample, tissue collection, GI content collection and related procedures/storage/shipments was the same as those employed in Group 1. All samples were analyzed for tacrolimus.

[0449] Group 4 animals were administered a single intra-cecal ingestible device of tacrolimus at 2 mg/0.8 mL (in sterile vehicle solution) on Day 1 by a veterinary surgeon. Plasma, rectal content sample, tissue collection, GI content collection and related procedures/storage/shipments were the same as those employed in Group 1. All samples were analyzed

for tacrolimus.

[0450] Group 5 animals are administered a single intra-cecal ingestible device containing tacrolimus at 4 mg /0.8 mL (in the vehicle solution) on Day 1 by a veterinary surgeon. Plasma, rectal content sample, tissue collection, GI content collection and related procedures/storage/shipments were the same as those employed in Group 1. All samples were analyzed for tacrolimus.

[0451] Detailed clinical observations were conducted daily from Day -10 to -5, and on Day 1. Additional pen-side observations were conducted at least once each day. The animals remained under constant clinical observation for the entire 12 hours from dose until euthanasia. Body weights were collected on Day -10, Day -5, and pre-dose on Day 1. Animals were euthanized via injection of a veterinarian-approved euthanasia.

Test Article and Formulation

1. Vehicle solution, 20 mL

[0452]

Description: 80% alcohol, 20% PEG-60 castor oil

Physical characteristics: clear liquid solution.

2. Prograf (tacrolimus injection), 10 ampules

[0453] Description: A sterile solution containing the equivalent of 5 mg anhydrous tacrolimus in 1 mL. Tacrolimus is macrolide immunosuppressant and the active ingredient of Prograf. 0.8 mL of Prograf (5 mg/mL) was administered through oral gavage per animal in group 2. Prograf (5 mg/mL) was diluted 2x folds (2.5 mg/mL) and 4x folds (1.25 mg/mL) by using vehicle solution. 0.8 mL of each concentration, 1.25 mg/mL, 2.5 mg/mL, and 5 mg/mL of Prograf, was injected into a DDS ingestible device for group 3, 4, and 5.

[0454] Formulation: Each mL contained polyoxyl 60 hydrogenated castor oil (HCO-60), 200 mg, and dehydrated alcohol, USP, 80.0% v/v.

[0455] Physical characteristics: clear liquid solution.

3. DDS ingestible device containing Tacrolimus

[0456] Description: Three (3) DDS ingestible devices containing vehicle solution for Group 1, three (3) DDS ingestible devices containing 1 mg tacrolimus for Group 3, three (3) DDS ingestible devices containing 2 mg tacrolimus for Group 4, and three (3) DDS ingestible devices containing 4 mg tacrolimus for Group 5.

Acclimation

[0457] Animals were acclimated prior to study initiation for at least 7 days. Animals in obvious poor health were not placed on study.

Concurrent Medication

[0458] Other than veterinary-approved anesthetics and medications used during surgery to install the ileocecal ports, or for vehicle or test article administration, and analgesia and antibiotics post-surgery, no further medications were employed.

Feed

[0459] All swine were fasted at least 24 hours before being anesthetized and properly medicated for surgery or overnight before dosing. Otherwise, animals were fed ad-libitum. Tap water was pressure-reduced and passed through a particulate filter, then a carbon filter prior to supply to an automatic watering system. Water was supplied ad libitum. There were no known contaminants in the feed or water that would be expected to interfere with this study.

Results

[0460] The data in Figure 76 show that the mean concentration of tacrolimus in the cecum tissue and the proximate colon tissue were higher in swine that were intra-cecally administered tacrolimus as compared to swine that were orally

administered tacrolimus.

[0461] These data suggest that intra-cecal administration of tacrolimus is able to locally deliver tacrolimus to the tissues in the GI tract of a mammal, while not decreasing the systemic immune system of a mammal.

5 Example 11. Comparison of the Tissue, Plasma, and GI Content Pharmacokinetics of Adalimumab through SC vs. Intra-Cecal Ingestible Device Delivery in Yorkshire-Cross Farm Swine in DSS-induced Colitis

[0462] The purpose of this non-Good Laboratory Practice (GLP) study is to explore the PK/PD and bioavailability of adalimumab when applied to DSS-induced colitis in Yorkshire-cross farm swine. All animals are randomized into groups of three. Animals are dosed once with adalimumab via subcutaneous (SC), perirectal (PR), or intracecal (IC) administration.

[0463] The concentration of adalimumab and $\text{TNF}\alpha$ is measured in plasma at 1, 2, 3, 4, 6, and 12 hours post-dose. The concentration of adalimumab is measured in rectal contents at 1, 3, 6, and 12 hours post-dose and in luminal content at 12 hours post-dose. Concentration of adalimumab and $\text{TNF}\alpha$, HER2, and total protein is measured in gastrointestinal tissue, e.g., cecum sample (CAC), proximal colon sample (PCN), transverse colon sample (TCN), distal colon sample (DCNi) inflamed, distal colon non-inflamed sample (DCNn), and rectum sample (RTM), at 12 hours post-dose.

Example 12. Human Clinical Trial of Treatment of Ulcerative Colitis using Adalimumab

20 **[0464]** As a proof of concept, the patient population of this study is patients that (1) have moderate to severe ulcerative colitis, regardless of extent, and (2) have had an insufficient response to a previous treatment, e.g., a conventional therapy (e.g., 5-ASA, corticosteroid, and/or immunosuppressant) or a FDA-approved treatment. In this placebo-controlled eight-week study, patients are randomized. All patient undergo a colonoscopy at the start of the study (baseline) and at week 8. Patients enrolled in the study are assessed for clinical status of disease by stool frequency, rectal bleeding, abdominal pain, physician's global assessment, and biomarker levels such as fecal calprotectin and hsCRP. The primary endpoint is a shift in endoscopy scores from Baseline to Week 8. Secondary and exploratory endpoints include safety and tolerability, change in rectal bleeding score, change in abdominal pain score, change in stool frequency, change in partial Mayo score, change in Mayo score, proportion of subjects achieving endoscopy remission, proportion of subjects achieving clinical remission, change in histology score, change in biomarkers of disease such as fecal calprotectin and hsCRP, level of adalimumab in the blood/tissue/stool, change in cytokine levels (e.g., $\text{TNF}\alpha$, IL-6) in the blood and tissue.

30 **[0465]** Figure 72 describes an exemplary process of what would occur in clinical practice, and when, where, and how the ingestible device will be used. Briefly, a patient displays symptoms of ulcerative colitis, including but not limited to: diarrhea, bloody stool, abdominal pain, high c-reactive protein (CRP), and/or high fecal calprotectin. A patient may or may not have undergone a colonoscopy with diagnosis of ulcerative colitis at this time. The patient's primary care physician refers the patient. The patient undergoes a colonoscopy with a biopsy, CT scan, and/or MRI. Based on this testing, the patient is diagnosed with ulcerative colitis. Most patients are diagnosed with ulcerative colitis by colonoscopy with biopsy. The severity based on clinical symptoms and endoscopic appearance, and the extent, based on the area of involvement on colonoscopy with or without CT/MRI is documented. Treatment is determined based on diagnosis, severity and extent.

40 **[0466]** For example, treatment for a patient that is diagnosed with ulcerative colitis is an ingestible device programmed to release a single bolus of a therapeutic agent, e.g., 40 mg adalimumab, in the cecum. Prior to administration of the treatment, the patient is fasted overnight and is allowed to drink clear fluids. Four hours after swallowing the ingestible device, the patient can resume a normal diet. An ingestible device is swallowed at the same time each day. The ingestible device is not recovered.

45 **[0467]** In some cases, there may be two different ingestible devices: one including an induction dose (first 8 to 12 weeks) and a different ingestible device including a different dose or a different dosing interval.

[0468] In some examples, the ingestible device can include a mapping tool, which can be used after 8 to 12 weeks of induction therapy, to assess the response status (e.g., based on one or more of the following: drug level, drug antibody level, biomarker level, and mucosal healing status). Depending on the response status determined by the mapping tool, a subject may continue to receive an induction regimen or maintenance regimen of adalimumab.

EXAMPLE 13

55 **[0469]** An ingestible medical device according to the disclosure ("TLC1") was tested on 20 subjects to investigate its localization ability. TLC1 was a biocompatible polycarbonate ingestible device that contained a power supply, electronics and software. An onboard software algorithm used time, temperature and reflected light spectral data to determine the location of the ingestible device as it traveled the GI tract. The ingestible device is 0.51 x 1.22 inches which is larger than a vitamin pill which is 0.4 x 0.85 inches. The subjects fasted overnight before participating in the study. Computerized

tomography ("CT") were used as a basis for determining the accuracy of the localization data collected with TLC1. One of the 20 subjects did not follow the fasting rule. CT data was lacking for another one of the 20 subjects. Thus, these two subjects were excluded from further analysis. TLC1 sampled RGB data (radially transmitted) every 15 seconds for the first 14 hours after it entered the subject's stomach, and then samples every five minutes after that until battery dies. TLC1 did not start to record optical data until it reached the subject's stomach. Thus, there was no RGB-based data for the mouth-esophagus transition for any of the subjects.

[0470] In addition, a PillCam® SB (Given Imaging) device was tested on 57 subjects. The subjects fasted overnight before joining the study. PillCam videos were recorded within each subject. The sampling frequency of PillCam is velocity dependent. The faster PillCam travels, the faster it would sample data. Each video is about seven to eight hours long, starting from when the ingestible device was administrated into the subject's mouth. RGB optical data were recorded in a table. A physician provided notes on where stomach-duodenum transition and ileum-cecum transition occurred in each video. Computerized tomography ("CT") was used as a basis for determining the accuracy of the localization data collected with PillCam.

Esophagus-Stomach Transition

[0471] For TLC1, it was assumed that this transition occurred one minute after the patient ingested the device. For PillCam, the algorithm was as follows:

1. Start mouth-esophagus transition detection after ingestible device is activated/administrated
2. Check whether Green < 102.3 and Blue < 94.6
 - a. If yes, mark as mouth-esophagus transition
 - b. If no, continue to scan the data
3. After detecting mouth-esophagus transition, continue to monitor Green and Blue signals for another 30 seconds, in case of location reversal
 - a. If either Green > 110.1 or Blue > 105.5, mark it as mouth-esophagus location reversal
 - b. Reset the mouth-esophagus flag and loop through step 2 and 3 until the confirmed mouth-esophagus transition detected
4. Add one minute to the confirmed mouth-esophagus transition and mark it as esophagus-stomach transition

[0472] For one of the PillCam subjects, there was not a clear cut difference between the esophagus and stomach, so this subject was excluded from future analysis of stomach localization. Among the 56 valid subjects, 54 of them have correct esophagus-stomach transition localization. The total agreement is 54/56=96%. Each of the two failed cases had prolonged esophageal of greater than one minute. Thus, adding one minute to mouth-esophagus transition was not enough to cover the transition in esophagus for these two subjects.

Stomach-Duodenum

[0473] For both TLC1 and PillCam, a sliding window analysis was used. The algorithm used a dumbbell shape two-sliding-window approach with a two-minute gap between the front (first) and back (second) windows. The two-minute gap was designed, at least in part, to skip the rapid transition from stomach to small intestine and capture the small intestine signal after ingestible device settles down in small intestine. The algorithm was as follows:

1. Start to check for stomach-duodenum transition after ingestible device enters stomach
2. Setup the two windows (front and back)
 - a. Time length of each window: 3 minutes for TLC1; 30 seconds for PillCam
 - b. Time gap between two windows: 2 minutes for both devices
 - c. Window sliding step size: 0.5 minute for both devices
3. Compare signals in the two sliding windows
 - a. If difference in mean is higher than 3 times the standard deviation of Green/Blue signal in the back window

- i. If this is the first time ever, record the mean and standard deviation of signals in the back window as stomach reference
- ii. If mean signal in the front window is higher than stomach reference signal by a certain threshold (0.3 for TLC1 and 0.18 for PillCam), mark this as a possible stomach-duodenum transition

b. If a possible pyloric transition is detected, continue to scan for another 10 minutes in case of false positive flag

- i. If within this 10 minutes, location reversal is detected, the previous pyloric transition flag is a false positive flag. Clear the flag and continue to check
- ii. If no location reversal has been identified within 10 minutes following the possible pyloric transition flag, mark it as a confirmed pyloric transition

c. Continue monitoring Green/Blue data for another 2 hours after the confirmed pyloric transition, in case of location reversal

- i. If a location reversal is identified, flag the timestamp when reversal happened and then repeat steps a-c to look for the next pyloric transition
- ii. If the ingestible device has not gone back to stomach 2 hours after previously confirmed pyloric transition, stops location reversal monitoring and assume the ingestible device would stay in intestinal area

[0474] For TLC1, one of the 18 subjects had too few samples (<3 minutes) taken in the stomach due to the delayed esophagus-stomach transition identification by previously developed localization algorithm. Thus, this subject was excluded from the stomach-duodenum transition algorithm test. For the rest of the TLC1 subjects, CT images confirmed that the detected pyloric transitions for all the subjects were located somewhere between stomach and jejunum. Two out of the 17 subjects showed that the ingestible device went back to stomach after first the first stomach-duodenum transition. The total agreement between the TLC1 algorithm detection and CT scans was $17/17 = 100\%$.

[0475] For one of the PillCam subjects, the ingestible device stayed in the subject's stomach all the time before the video ended. For another two of the PillCam subjects, too few samples were taken in the stomach to run the localization algorithm. These three PillCam subjects were excluded from the stomach-duodenum transition localization algorithm performance test. The performance summary of pyloric transition localization algorithm for PillCam was as follows:

1. Good cases (48 subjects):

- a. For 25 subjects, our detection matches exactly with the physician's notes
- b. For 19 subjects, the difference between the two detections is less than five minutes
- c. For four subjects, the difference between the two detections is less than 10 minutes (The full transition could take up to 10 minutes before the G/B signal settled)

2. Failed cases (6 subjects):

- a. Four subjects had high standard deviation of Green/Blue signal in the stomach
- b. One subject had bile in the stomach, which greatly affected Green/Blue in stomach
- c. One subject had no Green/Blue change at pyloric transition

[0476] The total agreement for the PillCam stomach-duodenum transition localization algorithm detection and physician's notes was $48/54 = 89\%$.

Duodenum-Jejenum Transition

[0477] For TLC1, it was assumed that the device left the duodenum and entered the jejunum three minutes after it was determined that the device entered the duodenum. Of the 17 subjects noted above with respect to the TLC1 investigation of the stomach-duodenum transition, 16 of the subjects mentioned had CT images that confirmed that the duodenum-jejenum transition was located somewhere between stomach and jejunum. One of the 17 subjects had a prolonged transit time in duodenum. The total agreement between algorithm detection and CT scans was $16/17 = 94\%$.

[0478] For PillCam, the duodenum-jejenum transition was not determined.

Jejunum-Ileum Transition

[0479] It is to be noted that the jejunum is redder and more vascular than ileum, and that the jejunum has a thicker intestine wall with more mesentery fat. These differences can cause various optical responses between jejunum and ileum, particularly for the reflected red light signal. For both TLC1 and PillCam, two different approaches were explored to track the change of red signal at the jejunum-ileum transition. The first approach was a single-sliding-window analysis, where the window is 10 minutes long, and the mean signal was compared with a threshold value while the window was moving along. The second approach was a two-sliding-window analysis, where each window was 10 minutes long with a 20 minute spacing between the two windows. The algorithm for the jejunum-ileum transition localization was as follows:

1. Obtain 20 minutes of Red signal after the duodenum-jejunum transition, average the data and record it as the jejunum reference signal
2. Start to check the jejunum-ileum transition 20 minutes after the device enters the jejunum

- a. Normalize the newly received data by the jejunum reference signal
- b. Two approaches:

- i. Single-sliding-window analysis

- Set the transition flag if the mean of reflected red signal is less than 0.8

- ii. Two-sliding-window analysis:

- Set the transition flag if the mean difference in reflected red is higher than 2X the standard deviation of the reflected red signal in the front window

[0480] For TLC1, 16 of the 18 subjects had CT images that confirmed that the detected jejunum-ileum transition fell between jejunum and cecum. The total agreement between algorithm and CT scans was $16/18 = 89\%$. This was true for both the single-sliding-window and double-sliding-window approaches, and the same two subjects failed in both approaches.

[0481] The performance summary of the jejunum-ileum transition detection for PillCam is listed below:

1. Single-sliding-window analysis:

- a. 11 cases having jejunum-ileum transition detected somewhere between jejunum and cecum
- b. 24 cases having jejunum-ileum transition detected after cecum
- c. 19 cases having no jejunum-ileum transition detected
- d. Total agreement: $11/54 = 20\%$

2. Two-sliding-window analysis:

- a. 30 cases having jejunum-ileum transition detected somewhere between jejunum and cecum
- b. 24 cases having jejunum-ileum transition detected after cecum
- c. Total agreement: $30/54 = 56\%$

Ileum-Cecum Transition

[0482] Data demonstrated that, for TLC1, mean signal of reflected red/green provided the most statistical difference before and after the ileum-cecum transition. Data also demonstrated that, for TLC1, the coefficient of variation of reflected green/blue provided the most statistical contrast at ileum-cecum transition. The analysis based on PillCam videos showed very similar statistical trends to those results obtained with TLC1 device. Thus, the algorithm utilized changes in mean value of reflected red/green and the coefficient of variation of reflected green/blue. The algorithm was as follows:

1. Start to monitor ileum-cecum transition after the ingestible device enters the stomach
2. Setup the two windows (front (first) and back (second))

- a. Use a five-minute time length for each window
- b. Use a 10-minute gap between the two windows

c. Use a one-minute window sliding step size

3. Compare signals in the two sliding windows

- 5 a. Set ileum-cecum transition flag if
 - i. Reflected red/green has a significant change or is lower than a threshold
 - ii. Coefficient of variation of reflected green/blue is lower than a threshold
- 10 b. If this is the first ileum-cecum transition detected, record average reflected red/green signal in small intestine as small intestine reference signal
- c. Mark location reversal (i.e. ingestible device returns to terminal ileum) if
 - 15 i. Reflected red/green is statistically comparable with small intestine reference signal
 - ii. Coefficient of variation of reflected green/blue is higher than a threshold
- d. If a possible ileum-cecum transition is detected, continue to scan for another 10 minutes for TLC1 (15 minutes for PillCam) in case of false positive flag
- 20 i. If within this time frame (10 minutes for TLC1, 15 minutes for PillCam), location reversal is detected, the previous ileum-cecum transition flag is a false positive flag. Clear the flag and continue to check
- ii. If no location reversal has been identified within this time frame (10 minutes for TLC1, 15 minutes for PillCam) following the possible ileum-cecum transition flag, mark it as a confirmed ileum-cecum transition
- 25 e. Continue monitoring data for another 2 hours after the confirmed ileum-cecum transition, in case of location reversal
 - i. If a location reversal is identified, flag the timestamp when reversal happened and then repeat steps a-d to look for the next ileum-cecum transition
 - 30 ii. If the ingestible device has not gone back to small intestine 2 hours after previously confirmed ileum-cecum transition, stop location reversal monitoring and assume the ingestible device would stay in large intestinal area

[0483] The flag setting and location reversal criteria particularly designed for TLC1 device were as follows:

- 35 1. Set ileum-cecum transition flag if
 - a. The average reflected red/Green in the front window is less than 0.7 or mean difference between the two windows is higher than 0.6
 - 40 b. And the coefficient of variation of reflected green/blue is less than 0.02
2. Define as location reversal if
 - a. The average reflected red/green in the front window is higher than small intestine reference signal
 - 45 b. And the coefficient of variation of reflected green/blue is higher than 0.086

[0484] For TLC1, 16 of the 18 subjects had CT images that confirmed that the detected ileum-cecum transition fell between terminal ileum and colon. The total agreement between algorithm and CT scans was $16/18 = 89\%$. Regarding those two subject where the ileum-cecum transition localization algorithm failed, for one subject the ileum-cecum transition was detected while TLC1 was still in the subject's terminal ileum, and for the other subject the ileum-cecum transition was detected when the device was in the colon.

[0485] Among the 57 available PillCam endoscopy videos, for three subjects the endoscopy video ended before PillCam reached cecum, and another two subjects had only very limited video data (less than five minutes) in the large intestine. These five subjects were excluded from ileum-cecum transition localization algorithm performance test. The performance summary of ileum-cecum transition detection for PillCam is listed below:

1. Good cases (39 subjects):

- a. For 31 subjects, the difference between the PillCam detection and the physician's notes was less than five minutes
- b. For 3 subjects, the difference between the PillCam detection and the physician's notes was less than 10 minutes
- c. For 5 subjects, the difference between the PillCam detection and the physician's notes was less than 20 minutes (the full transition can take up to 20 minutes before the signal settles)

2. Marginal/bad cases (13 subjects):

a. Marginal cases (9 subjects)

- i. The PillCam ileum-cecum transition detection appeared in the terminal ileum or colon, but the difference between the two detections was within one hour

b. Failed cases (4 subjects)

i. Reasons of failure:

- 1. The signal already stabilized in the terminal ileum
- 2. The signal was highly variable from the entrance to exit
- 3. There was no statistically significant change in reflected red/green at ileum-cecum transition

[0486] The total agreement between ileocecal transition localization algorithm detection and the physician's notes is $39/52 = 75\%$ if considering good cases only. Total agreement including possibly acceptable cases is $48/52 = 92.3\%$

Cecum-Colon Transition

[0487] Data demonstrated that, for TLC1, mean signal of reflected red/green provided the most statistical difference before and after the cecum-colon transition. Data also demonstrated that, for TLC1, the coefficient of variation of reflected blue provided the most statistical contrast at cecum-colon transition. The same signals were used for PillCam. The cecum-colon transition localization algorithm was as follows:

- 1. Obtain 10 minutes of reflected red/green and reflected blue signals after ileum-cecum transition, average the data and record it as the cecum reference signals
- 2. Start to check cecum-colon transition after ingestible device enters cecum (The cecum-colon transition algorithm is dependent on the ileum-cecum transition flag)

a. Normalize the newly received data by the cecum reference signals

b. Two-sliding-window analysis:

- i. Use two adjacent 10 minute windows
- ii. Set the transition flag if any of the following criteria were met
 - The mean difference in reflected red/green was more than 4X the standard deviation of reflected red/green in the back (second) window
 - The mean of reflected red/green in the front (first) window was higher than 1.03
 - The coefficient of variation of reflected blue signal in the front (first) window was greater than 0.23

[0488] The threshold values above were chosen based on a statistical analysis of data taken by TLC1.

[0489] For TLC1, 15 of the 18 subjects had the cecum-colon transition detected somewhere between cecum and colon. One of the subjects had the cecum-colon transition detected while TLC1 was still in cecum. The other two subjects had both wrong ileum-cecum transition detection and wrong cecum-colon transition detection. The total agreement between algorithm and CT scans was $15/18 = 83\%$.

[0490] For PillCam, for three subjects the endoscopy video ended before PillCam reached cecum, and for another two subjects there was very limited video data (less than five minutes) in the large intestine. These five subjects were excluded from cecum-colon transition localization algorithm performance test. The performance summary of cecum-colon transition detection for PillCam is listed below:

1. 27 cases had the cecum-colon transition detected somewhere between the cecum and the colon
2. one case had the cecum-colon transition detected in the ileum
3. 24 cases had no cecum-colon transition localized

[0491] The total agreement: $27/52 = 52\%$.

[0492] The following table summarizes the localization accuracy results.

Transition	TLC1	PillCam
Stomach-Duodenum	100% (17/17)	89% (48/54)
Duodenum-Jejunum	94% (16/17)	N/A
Ileum-Cecum	89% (16/18)	75% (39/52)
Ileum-terminal ileum/cecum/colon	100% (18/18)	92% (48/52)

Claims

1. A JAK inhibitor for use in a method of treating ulcerative colitis in a subject, the method comprising administering to the subject the JAK inhibitor in an ingestible device, wherein the ingestible device comprises:

an ingestible housing comprising a reservoir having a therapeutically effective amount of the JAK inhibitor stored therein;

a release mechanism having a closed state which retains the JAK inhibitor in the reservoir and an open state which allows for the release of the JAK inhibitor from the reservoir to the exterior of the device;

an actuator which controls the transition of the release mechanism from the closed to the open state;

a detector for detecting the location of the ingestible device in the subject's gastrointestinal tract; and

a processor which is coupled to the detector and to the actuator and which triggers the actuator to cause the release mechanism to transition from its closed state to its open state to release the JAK inhibitor in the cecum when it is determined that the ingestible device is in the cecum of the subject, wherein the site of disease is in the colon, wherein determining the location of the ingestible device in the gastrointestinal tract comprises detecting a transition of the ingestible device from the ileum to the cecum.

2. The JAK inhibitor for use according to claim 1, wherein the reservoir is configured to attach to the housing of the ingestible device, optionally wherein the reservoir is configured to friction fit with the ingestible device.

3. The JAK inhibitor for use according to any of the preceding claims, wherein the ingestible device autonomously determines that it is located at the cecum.

4. The JAK inhibitor for use according to any of the preceding claims, wherein the ingestible device comprises a gas generating cell located within the housing, wherein the ingestible device is configured so that, when the gas generating cell generates a gas, the gas creates an internal pressure that forces a release mechanism from a closed state, which retains the JAK inhibitor in the reservoir, to an open state, thereby allowing for the release of the JAK inhibitor from the reservoir to the exterior of the device.

5. The JAK inhibitor for use according to any of the preceding claims, wherein the ingestible device comprises a safety device placed within or attached to the housing, wherein the safety device is configured to relieve an internal pressure within the housing when the internal pressure exceeds a threshold level.

6. The JAK inhibitor for use according to any one of the preceding claims, wherein the ingestible device comprises an optical sensing unit supported by the housing, wherein the optical sensing unit is configured to detect a reflectance from an environment external to the housing.

7. The JAK inhibitor for use according to any one of the preceding claims, wherein the location of the ingestible device within the gastrointestinal tract of the subject is determined to an accuracy of at least 85%.

8. The JAK inhibitor for use according to any of the preceding claims, wherein the method of treatment provides a level

of JAK inhibitor in plasma in the subject at a time point following administration of the device that is lower than the level of the JAK inhibitor in plasma in a subject at substantially the same time point following systemic administration of an equal amount of the JAK inhibitor.

9. The JAK inhibitor for use according to claim 1 or 2, wherein the method comprises oral administration of the ingestible device.
10. The JAK inhibitor for use according to any of the preceding claims, wherein the method of treatment comprises delivering the JAK inhibitor at the location in the gastrointestinal tract as a bolus.
11. The JAK inhibitor for use according to any of the preceding claims, wherein the JAK inhibitor is selected from tofacitinib, filgotinib, upadacitinib, TD-1473, ruxolitinib optionally, wherein the JAK inhibitor is tofacitinib.

Patentansprüche

1. JAK-Inhibitor zur Verwendung in einem Verfahren zur Behandlung von Colitis ulcerosa bei einem Individuum, wobei das Verfahren die Verabreichung des JAK-Inhibitors in einer einnehmbaren Vorrichtung an das Individuum umfasst, wobei die einnehmbare Vorrichtung Folgendes umfasst:

ein einnehmbares Gehäuse, das ein Reservoir mit einer therapeutisch wirksamen Menge des JAK-Inhibitors darin untergebracht umfasst;
einen Freisetzungsmechanismus, der einen geschlossenen Zustand, der den JAK-Inhibitor im Reservoir zurückhält, und einem offenen Zustand, der die Freisetzung des JAK-Inhibitors aus dem Reservoir außerhalb der Vorrichtung ermöglicht, aufweist;
einen Aktuator, der den Übergang des Freisetzungsmechanismus aus dem geschlossenen in den offenen Zustand steuert;
einen Detektor zum Detektieren der Position der einnehmbaren Vorrichtung im Magen-Darm-Trakt des Individuums; und
einen Prozessor, der an den Detektor und den Aktuator gekoppelt ist und auslöst, dass der Aktuator den Freisetzungsmechanismus veranlasst, von seinem geschlossenen Zustand in seinen offenen Zustand überzugehen, um den JAK-Inhibitor im Zäkum freizusetzen, wenn festgestellt wird, dass sich die einnehmbare Vorrichtung im Zäkum des Individuums befindet, wobei die Erkrankungsstelle im Kolon ist, wobei die Bestimmung der Position der einnehmbaren Vorrichtung im Magen-Darm-Trakt das Detektieren eines Übergangs der einnehmbaren Vorrichtung aus dem Ileum in das Zäkum umfasst.

2. JAK-Inhibitor zur Verwendung nach Anspruch 1, wobei das Reservoir dazu ausgelegt ist, sich an das Gehäuse der einnehmbaren Vorrichtung anzuhängen, wobei das Reservoir gegebenenfalls dazu ausgelegt ist, sich mit der einnehmbaren Vorrichtung reibschlüssig zu verbinden.
3. JAK-Inhibitor zur Verwendung nach einem der vorangegangenen Ansprüche, wobei die einnehmbare Vorrichtung selbstständig bestimmt, dass sie sich im Zäkum befindet.
4. JAK-Inhibitor zur Verwendung nach einem der vorangegangenen Ansprüche, wobei die einnehmbare Vorrichtung eine gaserzeugende Zelle umfasst, die sich im Gehäuse befindet, wobei die einnehmbare Vorrichtung so ausgelegt ist, dass, wenn die gaserzeugende Zelle ein Gas erzeugt, das Gas einen Innendruck erzeugt, der einen Freisetzungsmechanismus aus einem geschlossenen Zustand, in dem der JAK-Inhibitor im Reservoir gehalten wird, in einen offenen Zustand zwingt, wodurch die Freisetzung des JAK-Inhibitors aus dem Reservoir aus der Vorrichtung hinaus ermöglicht wird.
5. JAK-Inhibitor zur Verwendung nach einem der vorangegangenen Ansprüche, wobei die einnehmbare Vorrichtung eine Sicherheitsvorrichtung umfasst, die innerhalb des Gehäuses angeordnet oder daran befestigt ist, wobei die Sicherheitsvorrichtung dazu ausgelegt ist, einen Innendruck innerhalb des Gehäuses abzulassen, wenn der Innendruck einen Schwellenwert überschreitet.
6. JAK-Inhibitor zur Verwendung nach einem der vorangegangenen Ansprüche, wobei die einnehmbare Vorrichtung eine vom Gehäuse getragene optische Sensoreinheit umfasst, wobei die optische Sensoreinheit dazu ausgelegt ist, ein Reflexionsvermögen aus der Umgebung außerhalb des Gehäuses zu detektieren.

7. JAK-Inhibitor zur Verwendung nach einem der vorangegangenen Ansprüche, wobei die Position der einnehmbaren Vorrichtung im Magen-Darm-Trakt des Individuums mit einer Genauigkeit von zumindest 85 % bestimmt wird.
8. JAK-Inhibitor zur Verwendung nach einem der vorangegangenen Ansprüche, wobei das Behandlungsverfahren zu einem Zeitpunkt nach der Verabreichung der Vorrichtung eine Menge an JAK-Inhibitor im Plasma in dem Individuum bereitstellt, die niedriger ist als die Menge des JAK-Inhibitors im Plasma eines Individuums zum im Wesentlichen gleichen Zeitpunkt nach einer systemischen Verabreichung einer gleichen Menge des JAK-Inhibitors.
9. JAK-Inhibitor zur Verwendung nach Anspruch 1 oder 2, wobei das Verfahren die orale Verabreichung der einnehmbaren Vorrichtung umfasst.
10. JAK-Inhibitor zur Verwendung nach einem der vorangegangenen Ansprüche, wobei das Behandlungsverfahren die Zufuhr des JAK-Inhibitors an die Position im Magen-Darm-Trakt als Bolus umfasst.
11. JAK-Inhibitor zur Verwendung nach einem der vorangegangenen Ansprüche, wobei der JAK-Inhibitor aus Tofacitinib, Filgotinib, Upadacitinib, TD-1473 und Ruxolitinib ausgewählt ist, wobei der JAK-Inhibitor gegebenenfalls Tofacitinib ist.

Revendications

1. Inhibiteur de JAK à utiliser dans un procédé de traitement de la rectocolite hémorragique chez un sujet, le procédé comprenant l'administration au sujet de l'inhibiteur de JAK dans un dispositif pouvant être ingéré, dans lequel le dispositif pouvant être ingéré comprend :
 - un logement pouvant être ingéré comprenant un réservoir dans lequel est stockée une quantité thérapeutiquement efficace de l'inhibiteur de JAK ;
 - un mécanisme de libération présentant un état fermé qui retient l'inhibiteur de JAK dans le réservoir et un état ouvert qui permet la libération de l'inhibiteur de JAK à partir du réservoir vers l'extérieur du dispositif ;
 - un actionneur qui commande la transition du mécanisme de libération de l'état fermé à l'état ouvert ;
 - un détecteur pour détecter l'emplacement du dispositif pouvant être ingéré dans le tractus gastro-intestinal du sujet ; et
 - un processeur qui est couplé au détecteur et à l'actionneur et qui déclenche l'actionneur pour amener le mécanisme de libération à passer de son état fermé à son état ouvert afin de libérer l'inhibiteur de JAK dans le cæcum lorsqu'il est déterminé que le dispositif pouvant être ingéré est dans le cæcum du sujet, dans lequel le site de la maladie est dans le côlon, dans lequel la détermination de l'emplacement du dispositif pouvant être ingéré dans le tractus gastro-intestinal comprend une détection d'une transition du dispositif pouvant être ingéré de l'iléon au cæcum.
2. Inhibiteur de JAK à utiliser selon la revendication 1, dans lequel le réservoir est configuré pour se fixer au logement du dispositif pouvant être ingéré, facultativement dans lequel le réservoir est configuré pour être ajusté par friction avec le dispositif pouvant être ingéré.
3. Inhibiteur de JAK à utiliser selon l'une quelconque des revendications précédentes, dans lequel le dispositif pouvant être ingéré détermine de manière autonome qu'il est situé au niveau du cæcum.
4. Inhibiteur de JAK à utiliser selon l'une quelconque des revendications précédentes, dans lequel le dispositif pouvant être ingéré comprend une cellule génératrice de gaz située à l'intérieur du logement, dans lequel le dispositif pouvant être ingéré est configuré de telle sorte que, lorsque la cellule génératrice de gaz génère un gaz, le gaz crée une pression interne qui force un mécanisme de libération d'un état fermé, qui retient l'inhibiteur de JAK dans le réservoir, à un état ouvert, en permettant ainsi la libération de l'inhibiteur de JAK à partir du réservoir vers l'extérieur du dispositif.
5. Inhibiteur de JAK à utiliser selon l'une quelconque des revendications précédentes, dans lequel le dispositif pouvant être ingéré comprend un dispositif de sécurité placé à l'intérieur du logement ou fixé à celui-ci, dans lequel le dispositif de sécurité est configuré pour relâcher une pression interne à l'intérieur du logement lorsque la pression interne dépasse un niveau de seuil.
6. Inhibiteur de JAK à utiliser selon l'une quelconque des revendications précédentes, dans lequel le dispositif pouvant

être ingéré comprend une unité de détection optique supportée par le logement, dans lequel l'unité de détection optique est configurée pour détecter une réflectance à partir d'un environnement externe au logement.

- 5 **7.** Inhibiteur de JAK à utiliser selon l'une quelconque des revendications précédentes, dans lequel l'emplacement du dispositif pouvant être ingéré à l'intérieur du tractus gastro-intestinal du sujet est déterminé à une précision d'au moins 85 %.
- 10 **8.** Inhibiteur de JAK à utiliser selon l'une quelconque des revendications précédentes, dans lequel le procédé de traitement fournit un niveau d'inhibiteur de JAK dans le plasma chez le sujet à un instant suivant l'administration du dispositif qui est inférieur au niveau de l'inhibiteur de JAK dans le plasma chez un sujet sensiblement au même instant suivant une administration systémique d'une quantité égale de l'inhibiteur de JAK.
- 15 **9.** Inhibiteur de JAK à utiliser selon la revendication 1 ou 2, dans lequel le procédé comprend une administration orale du dispositif pouvant être ingéré.
- 20 **10.** Inhibiteur de JAK à utiliser selon l'une quelconque des revendications précédentes, dans lequel le procédé de traitement comprend l'administration de l'inhibiteur de JAK au niveau de l'emplacement dans le tractus gastro-intestinal sous la forme d'un bol.
- 25 **11.** Inhibiteur de JAK à utiliser selon l'une quelconque des revendications précédentes, dans lequel l'inhibiteur de JAK est choisi parmi tofacitinib, filgotinib, upadacitinib, TD-1473, ruxolitinib, facultativement dans lequel l'inhibiteur de JAK est le tofacitinib.

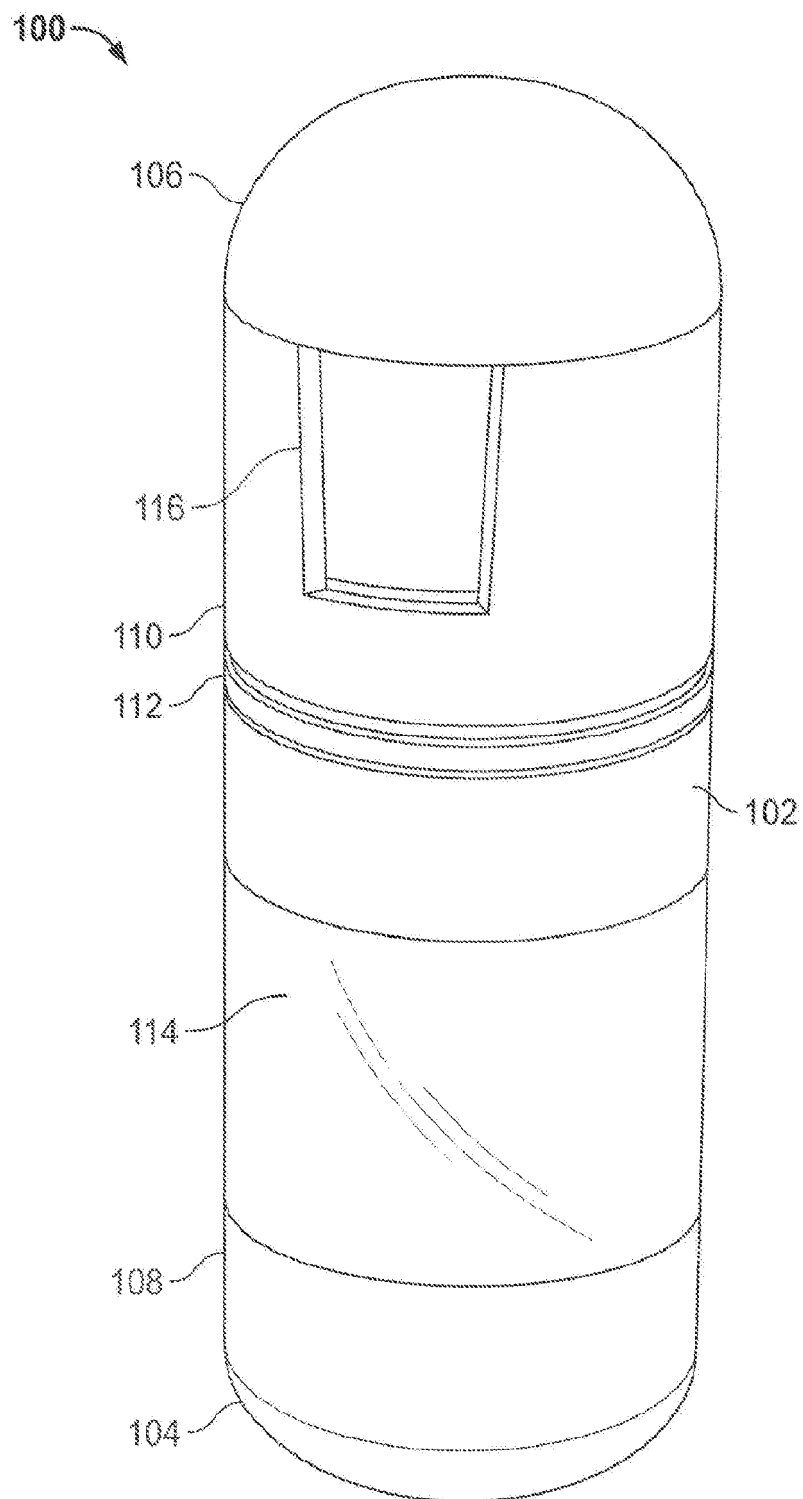


FIG. 1

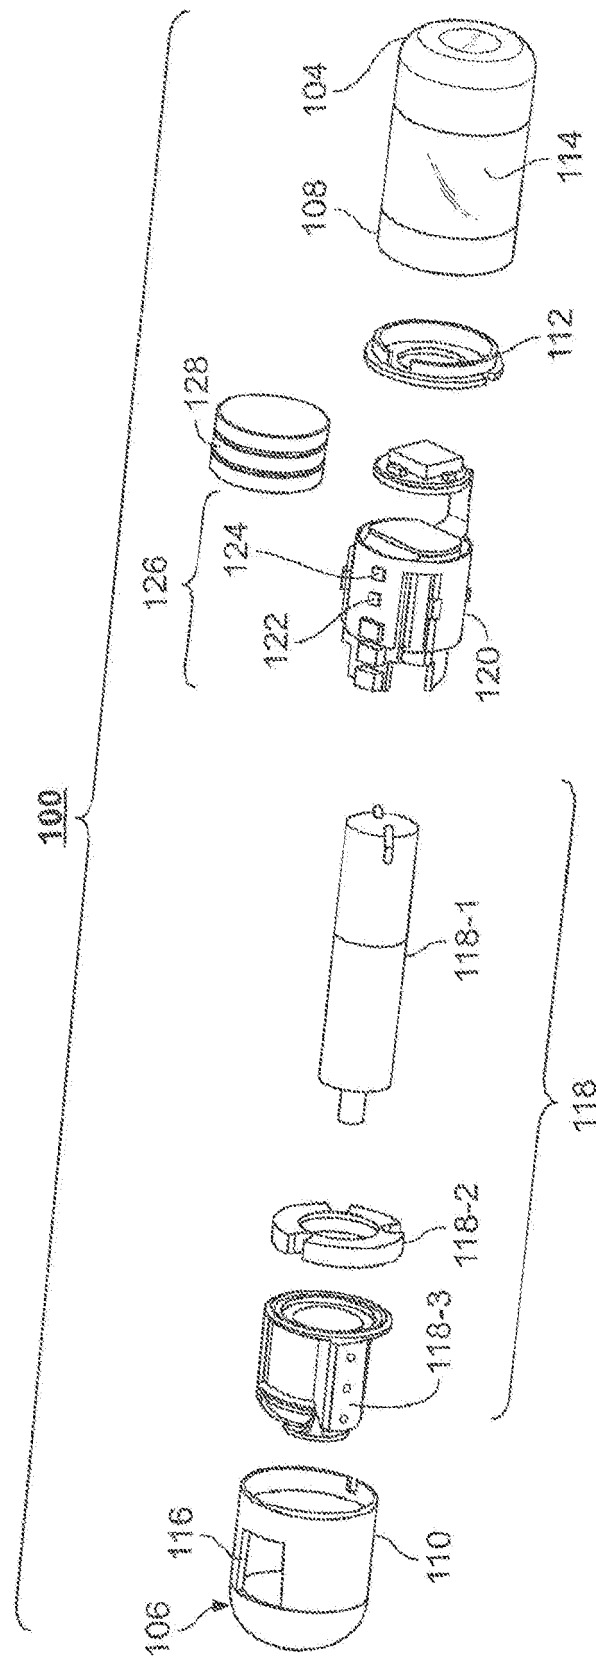


FIG. 2

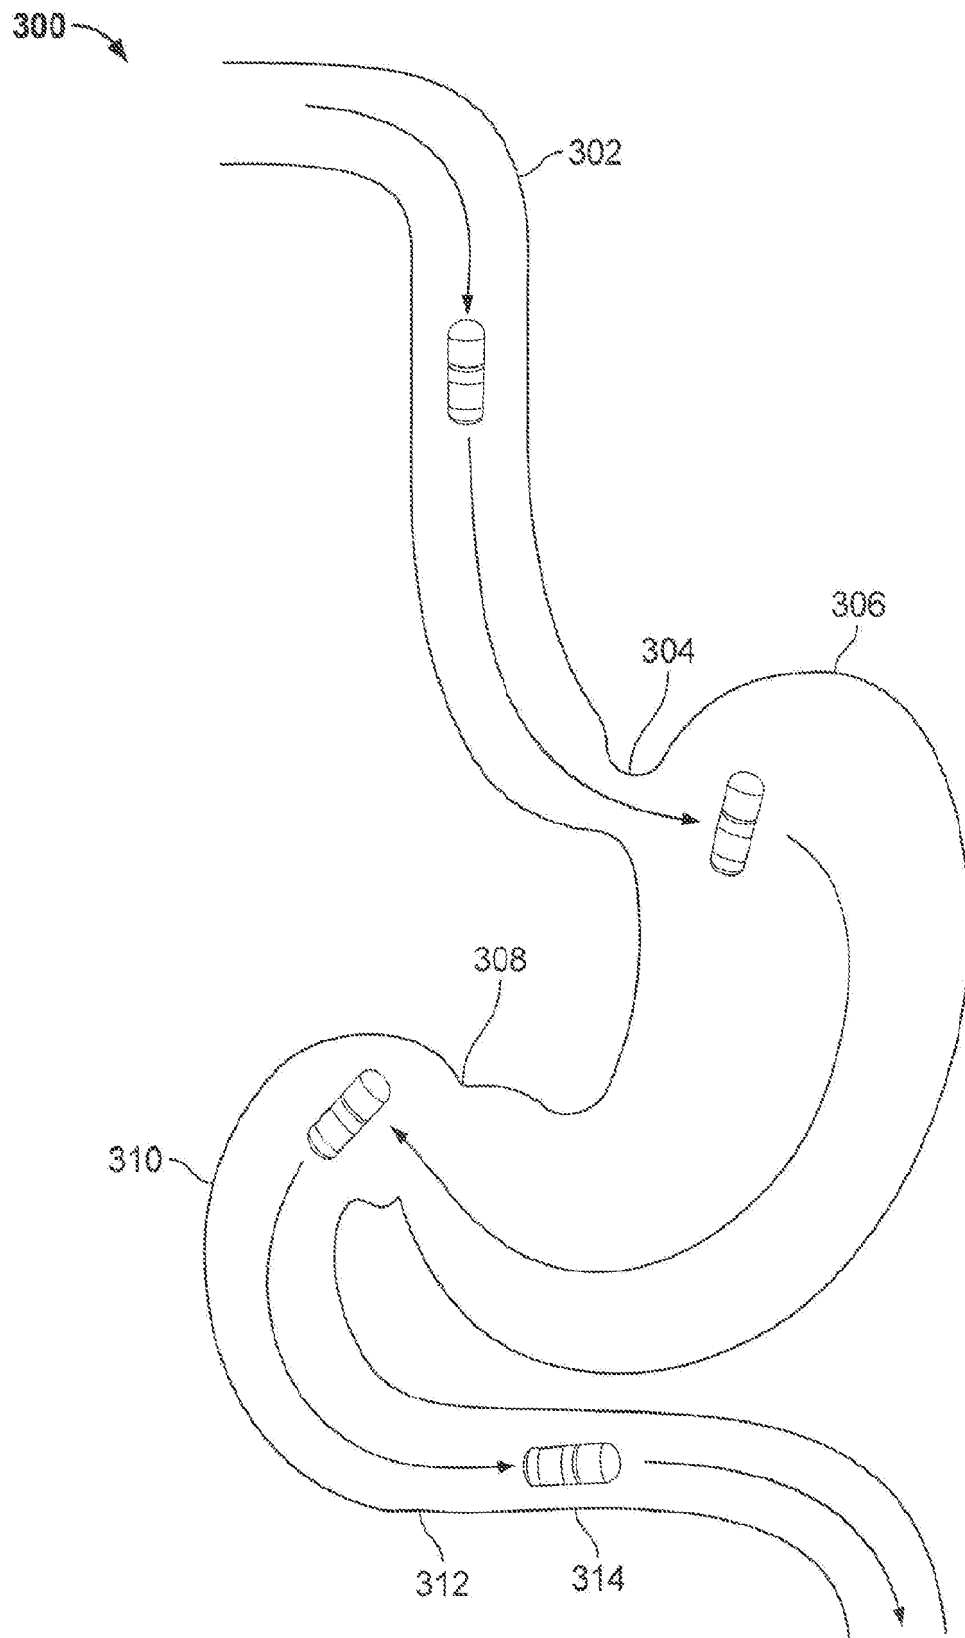


FIG. 3

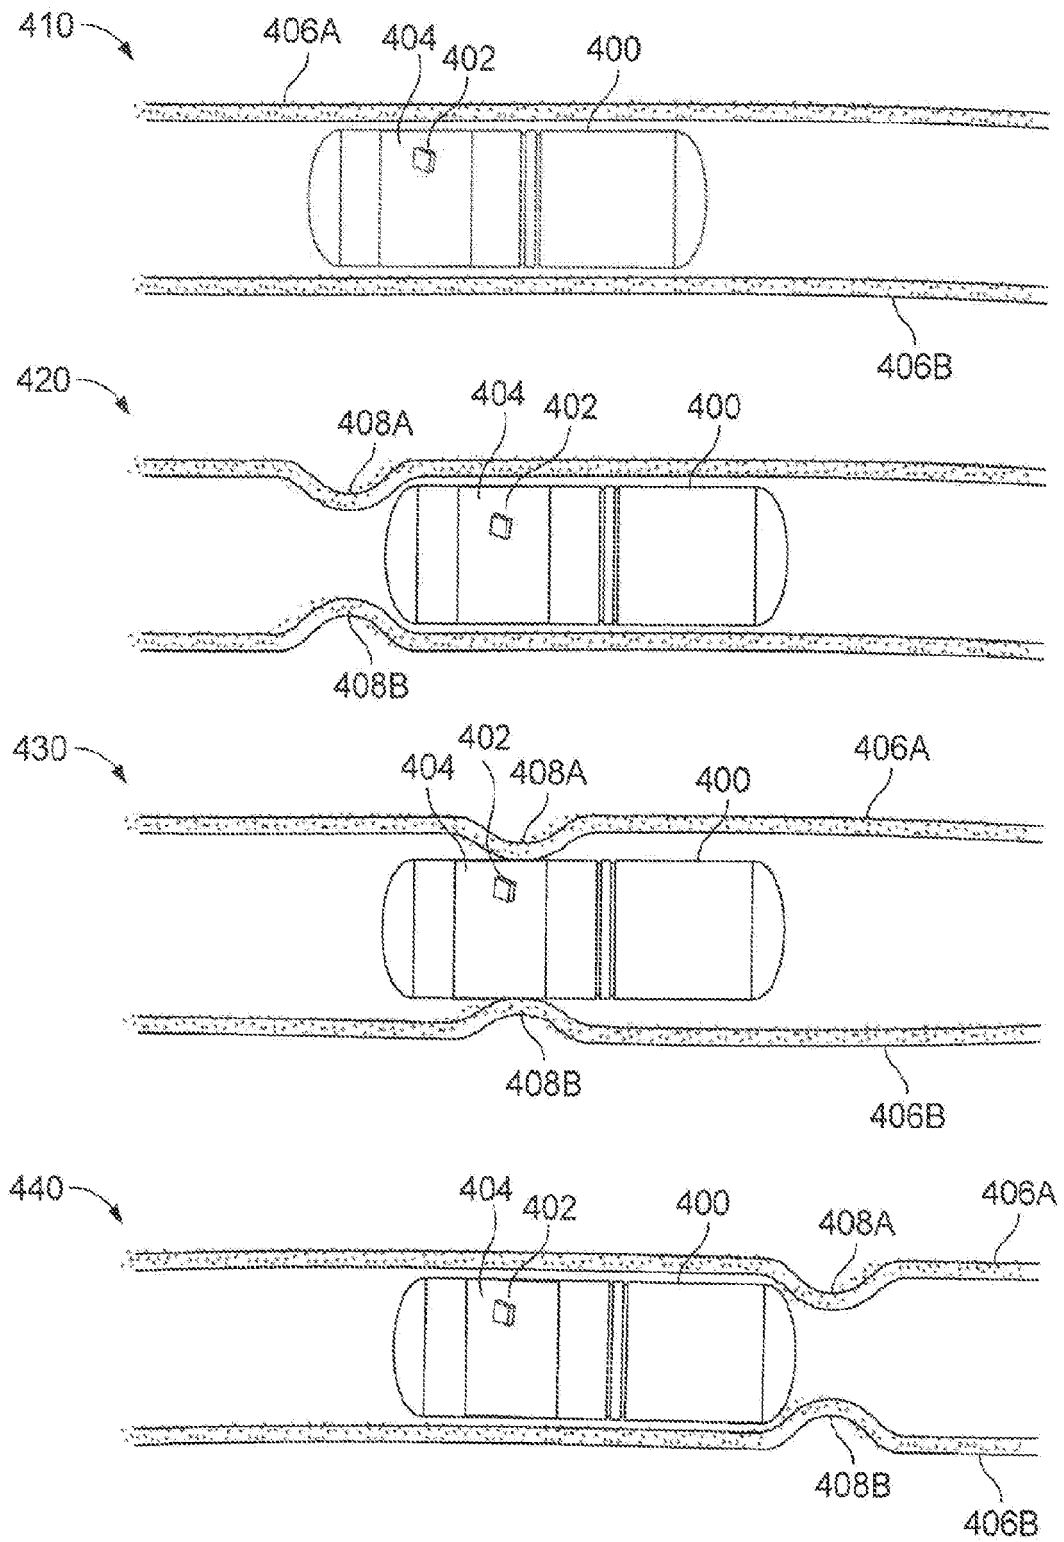


FIG. 4

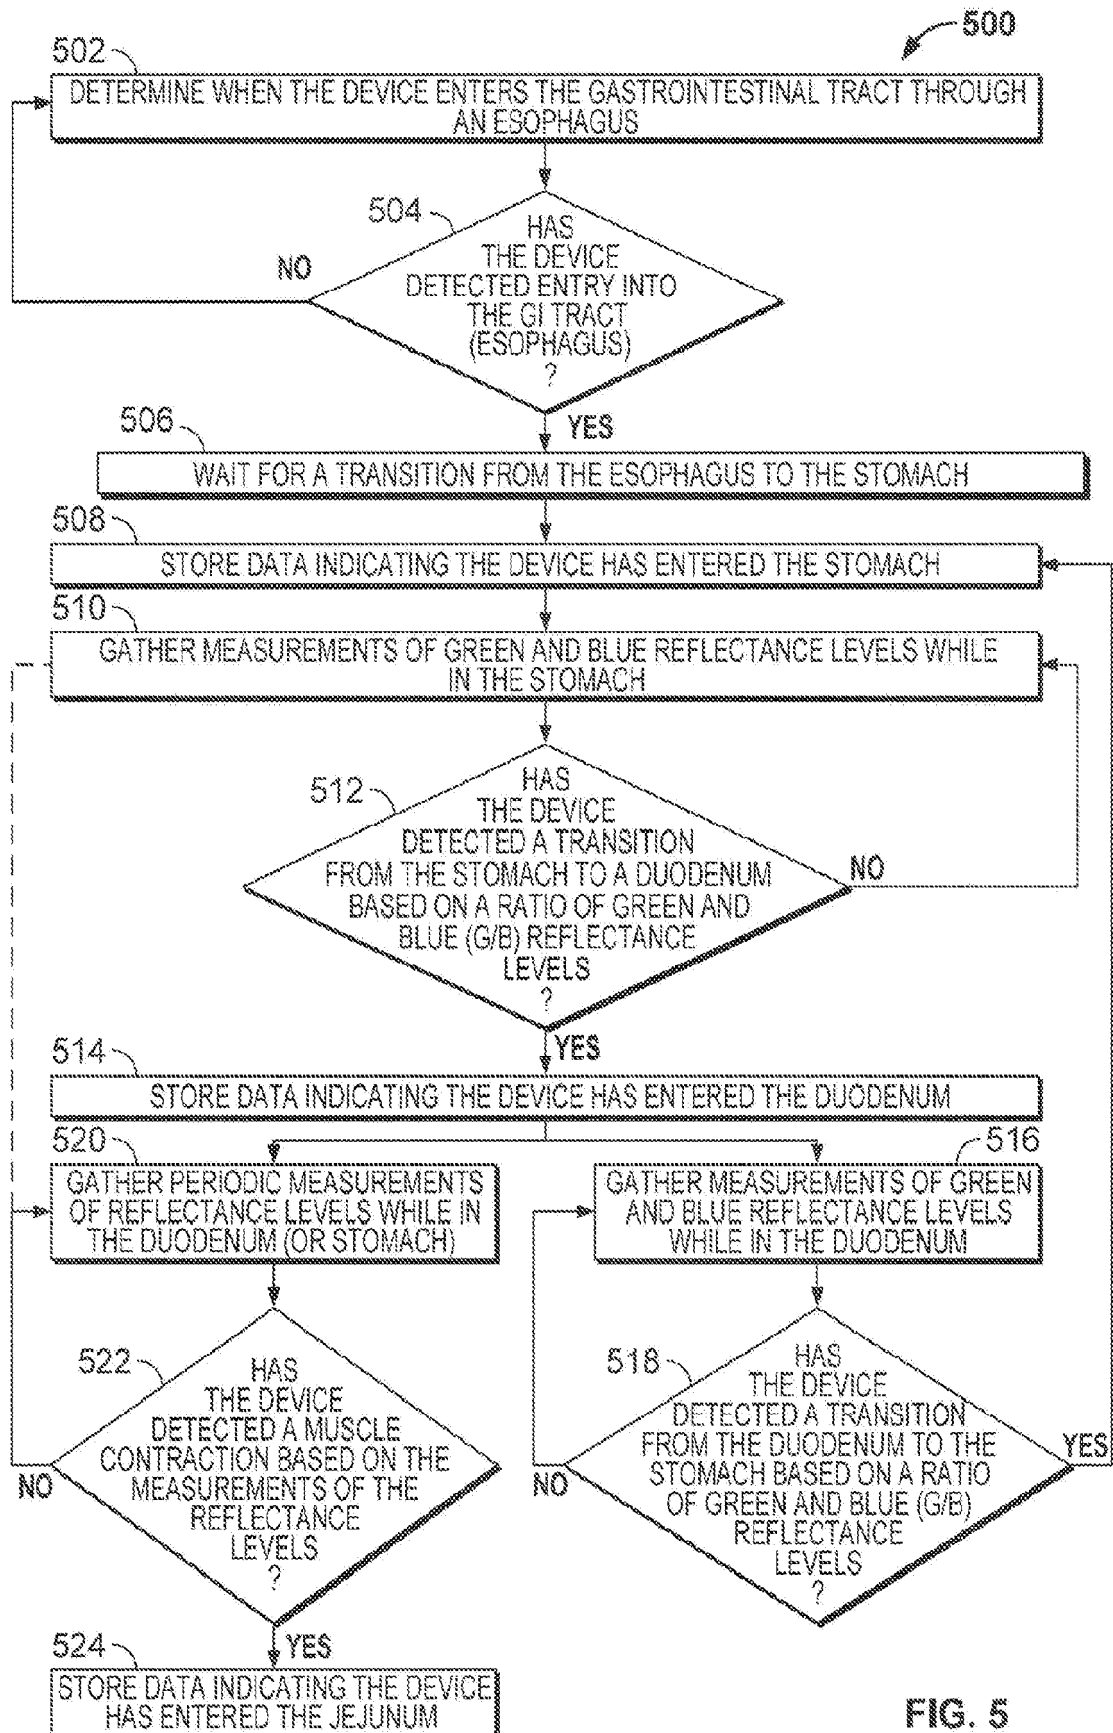


FIG. 5

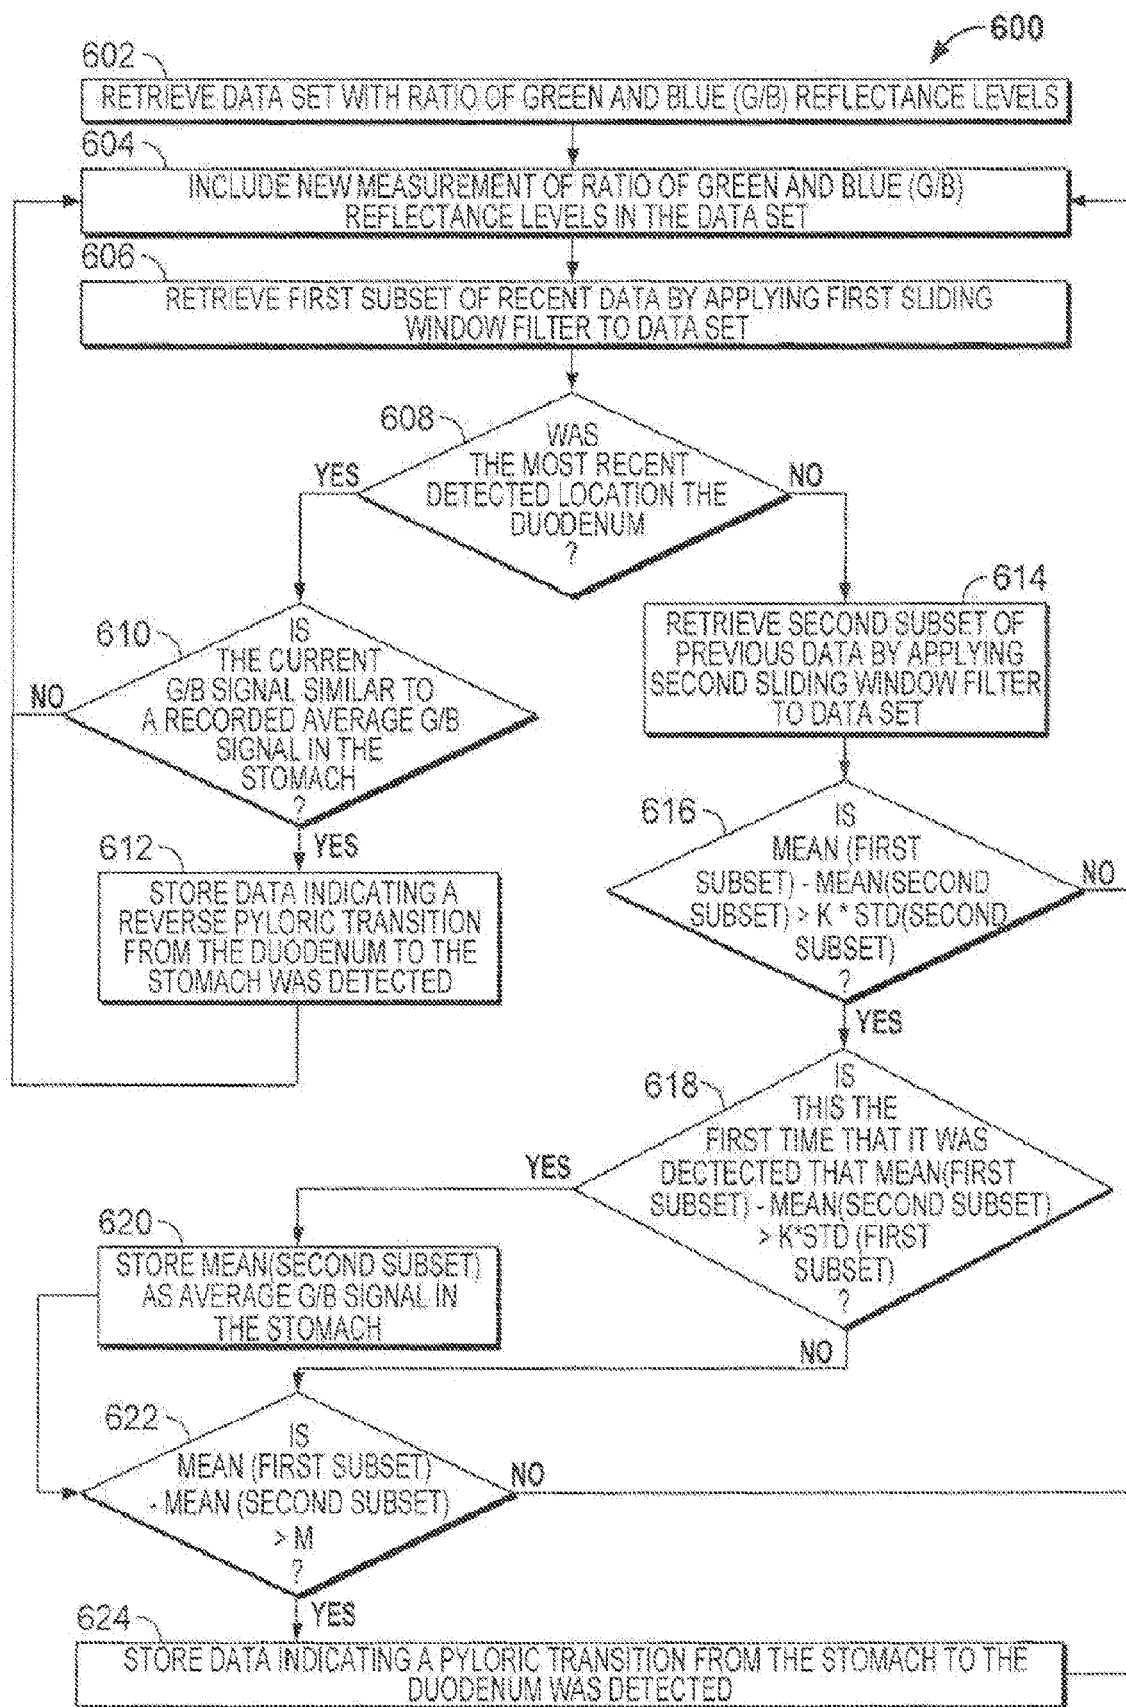


FIG. 6

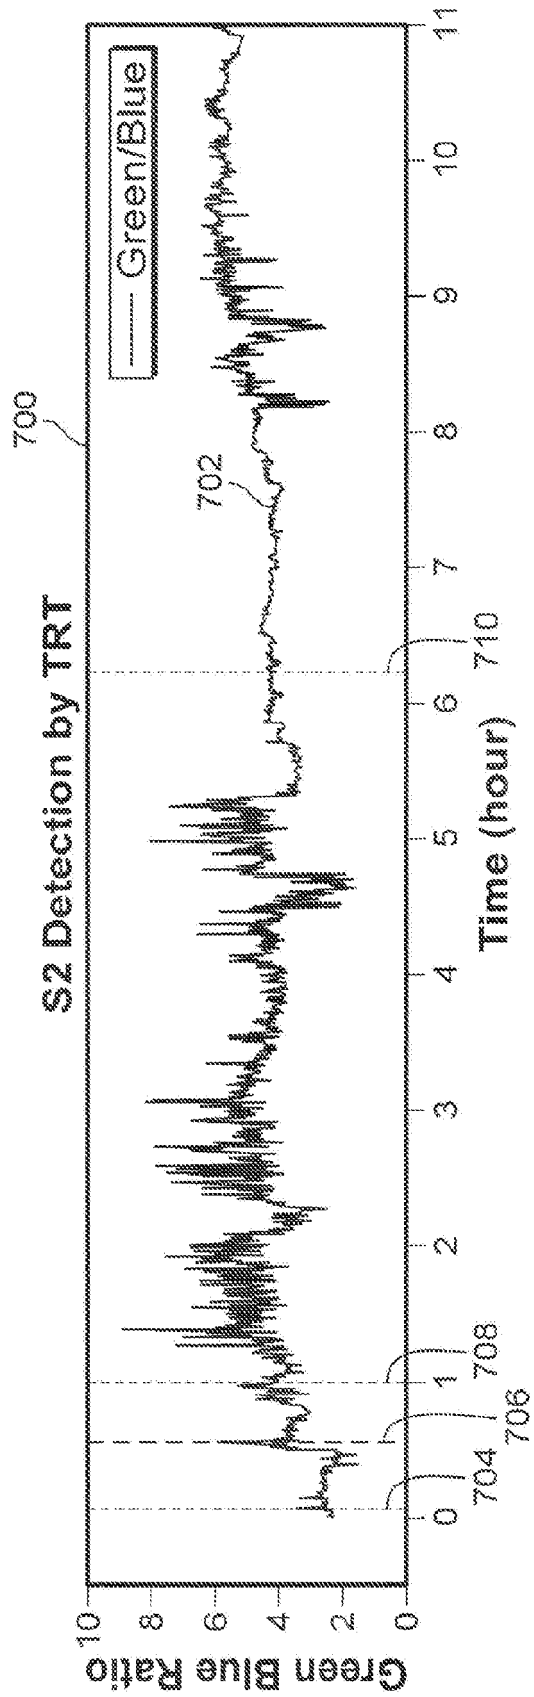


FIG. 7

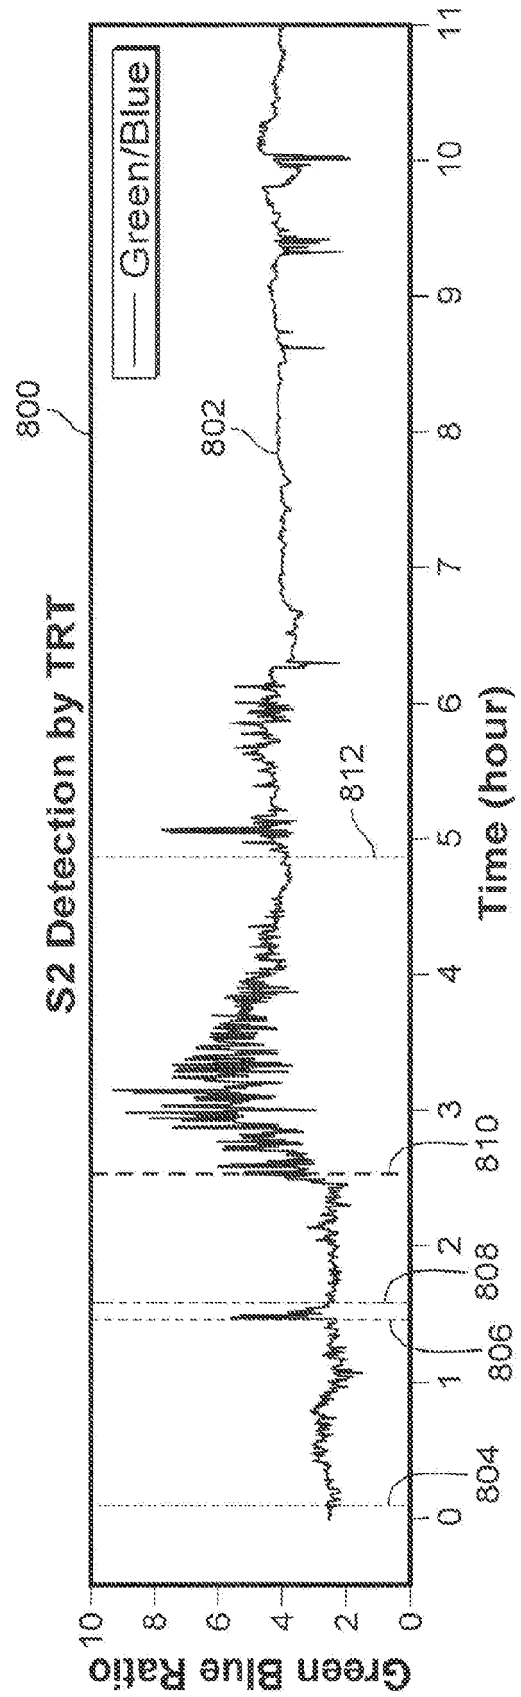


FIG. 8

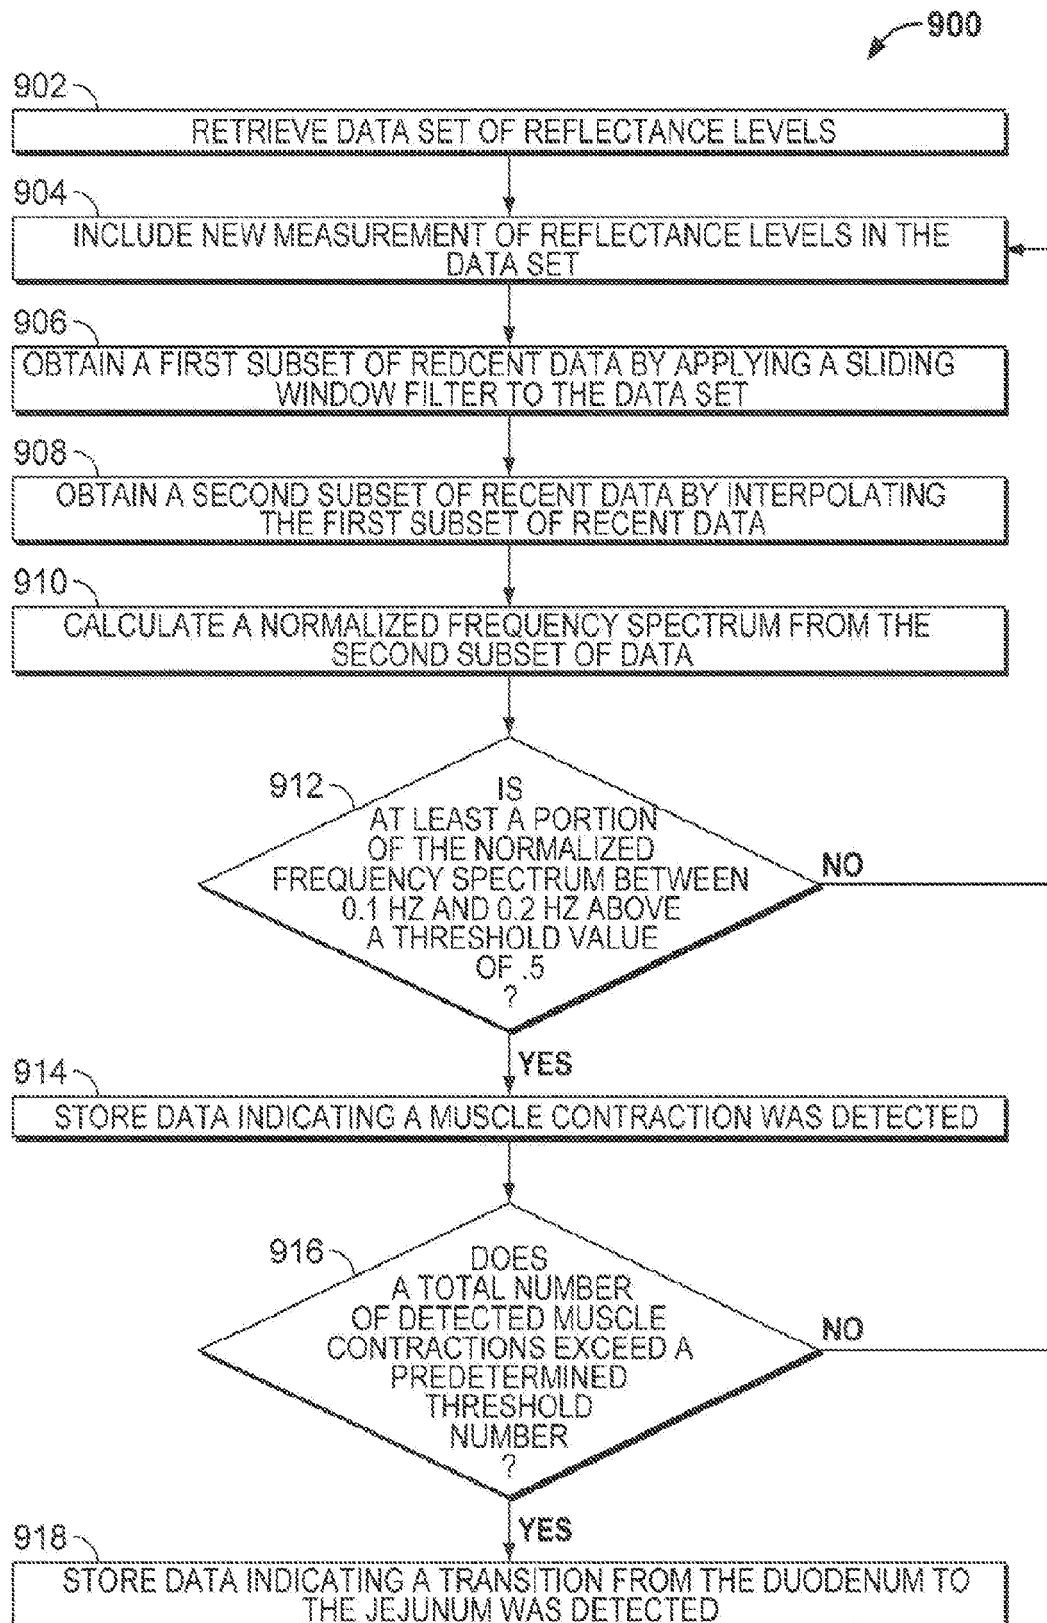


FIG. 9

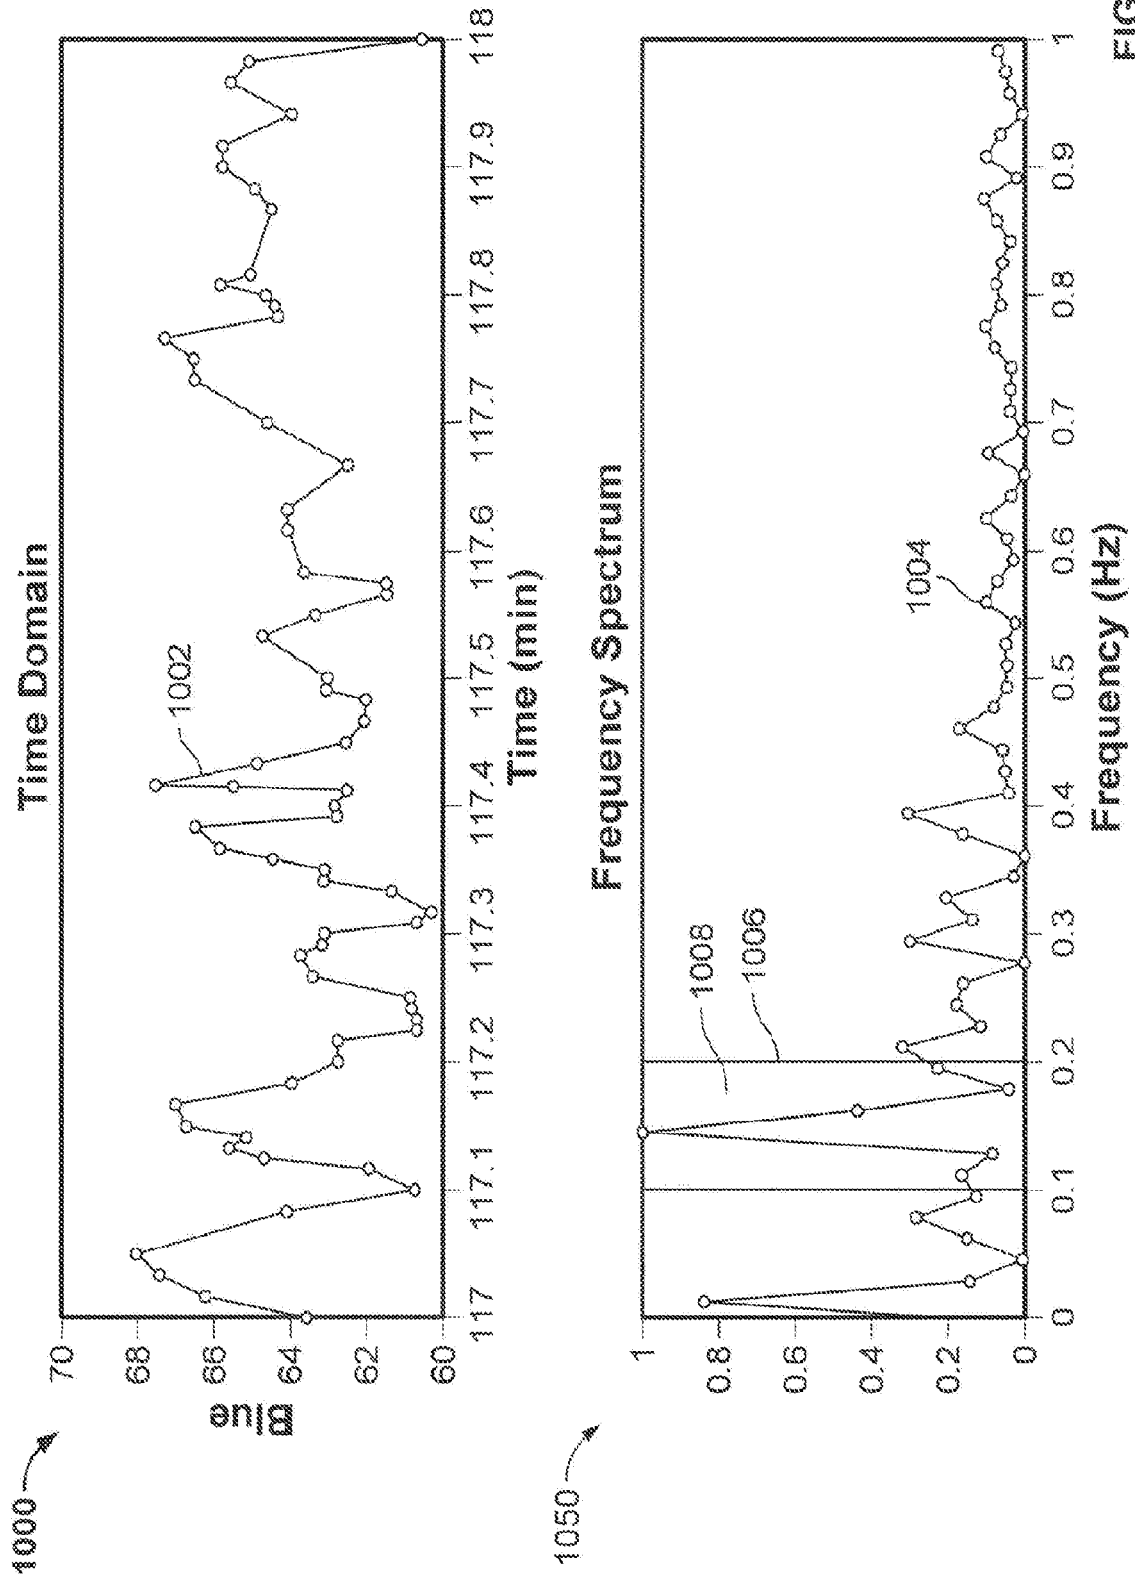
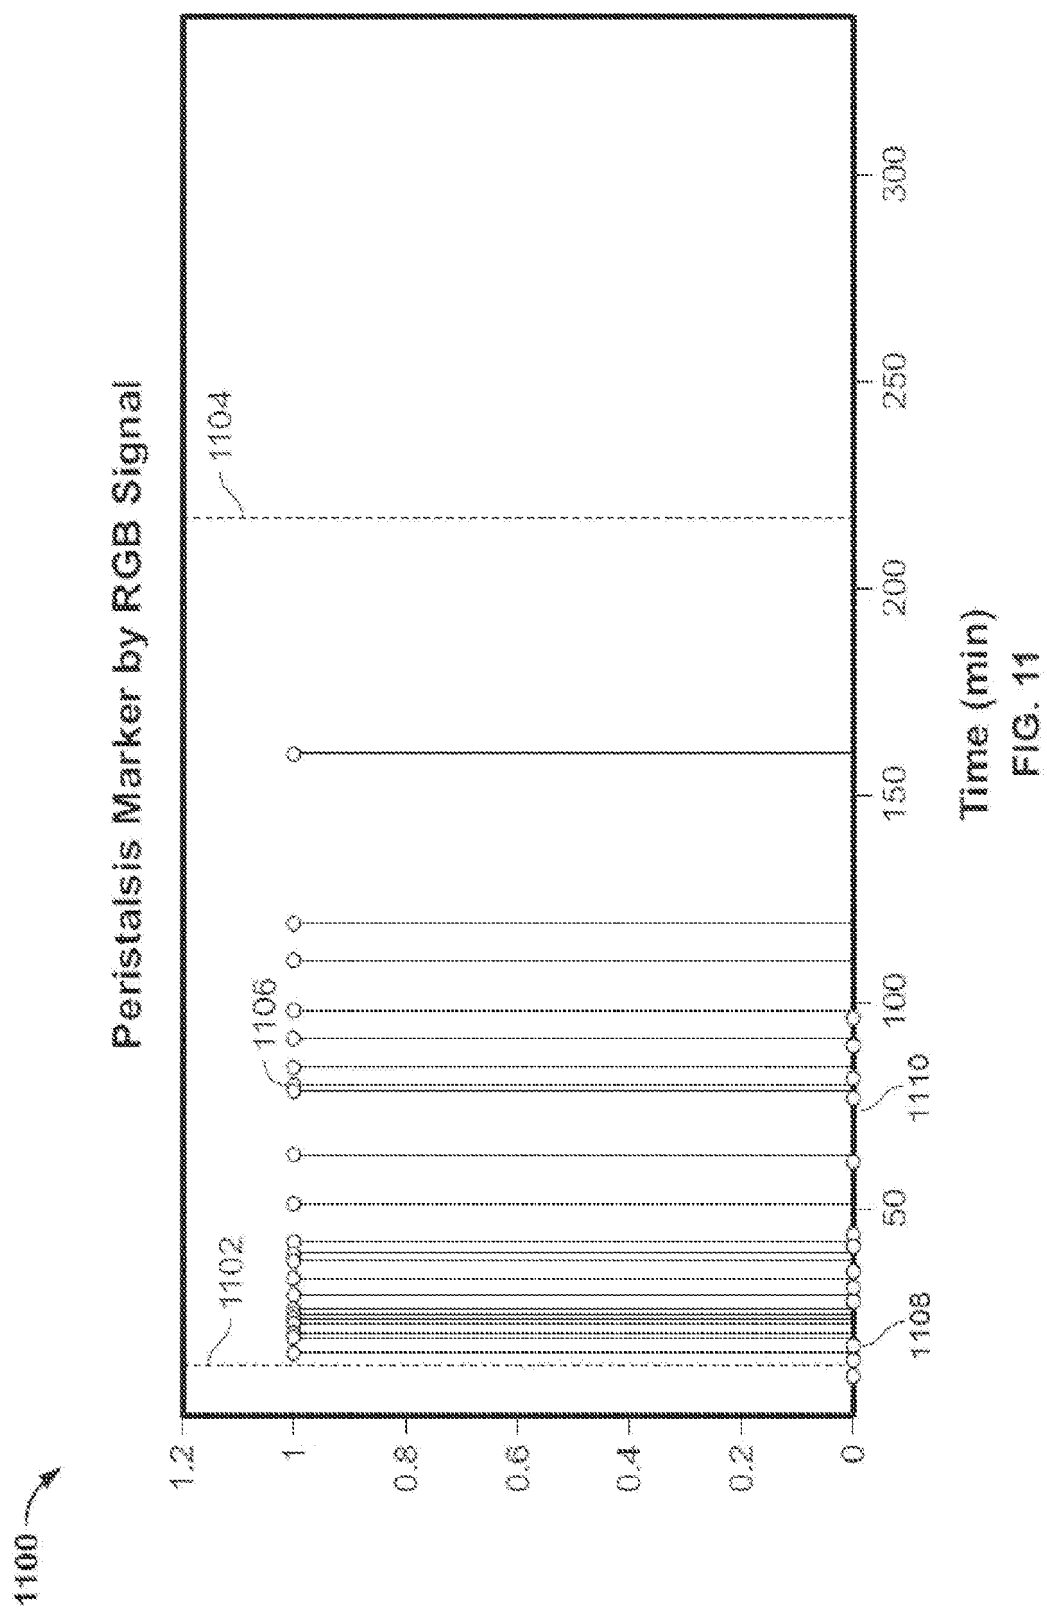


FIG. 10



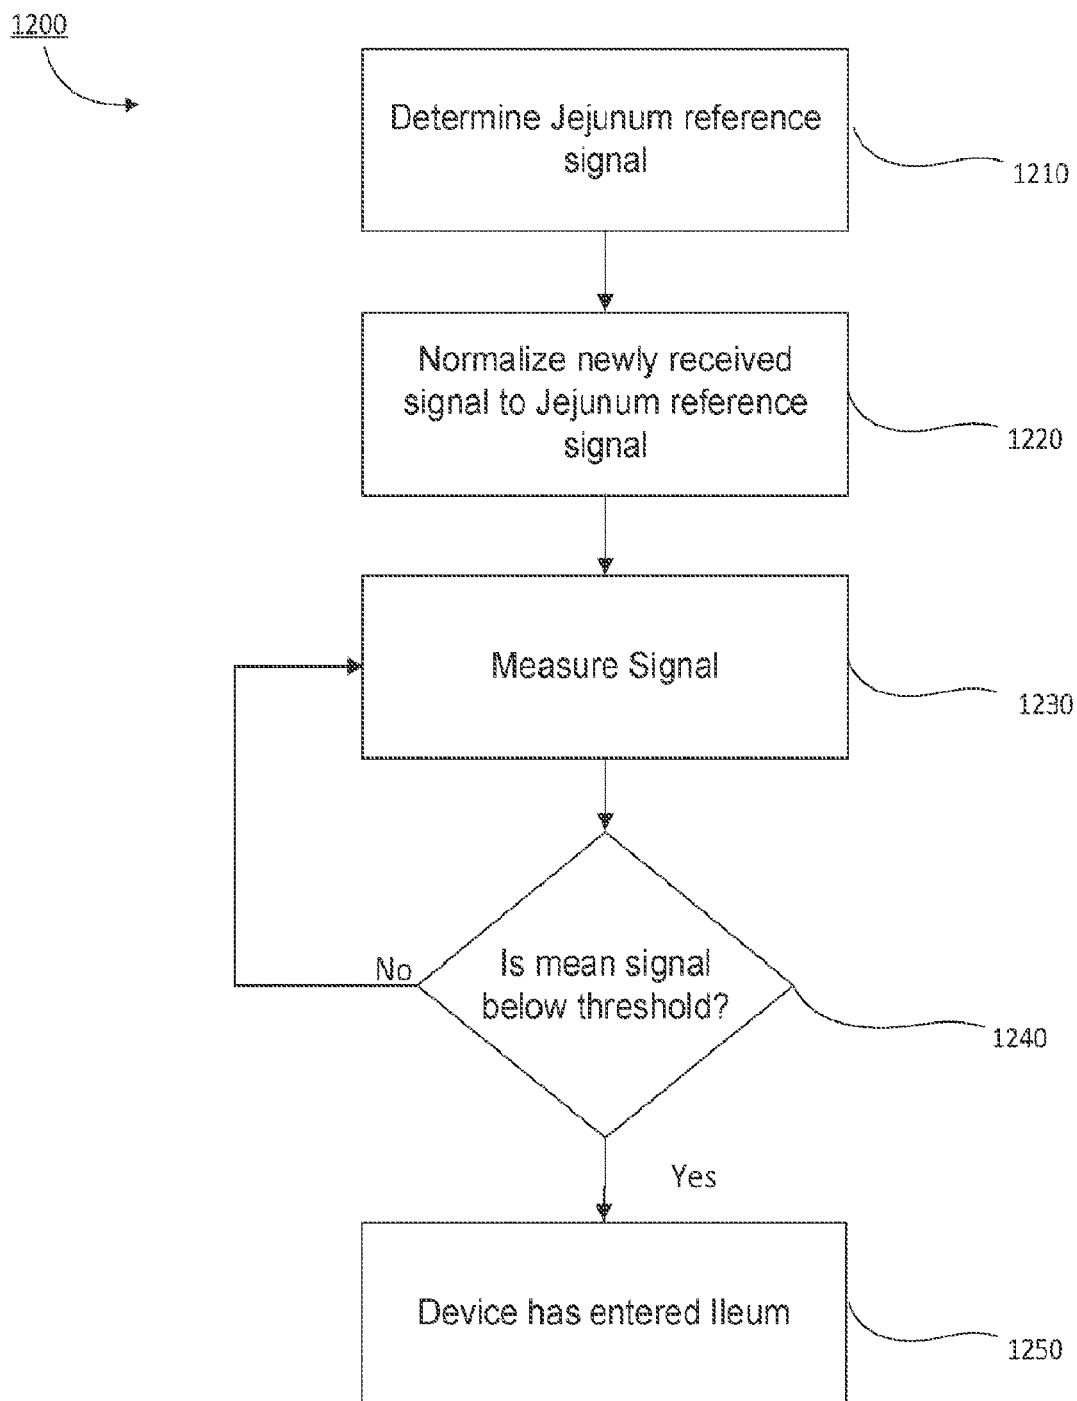


FIG. 12

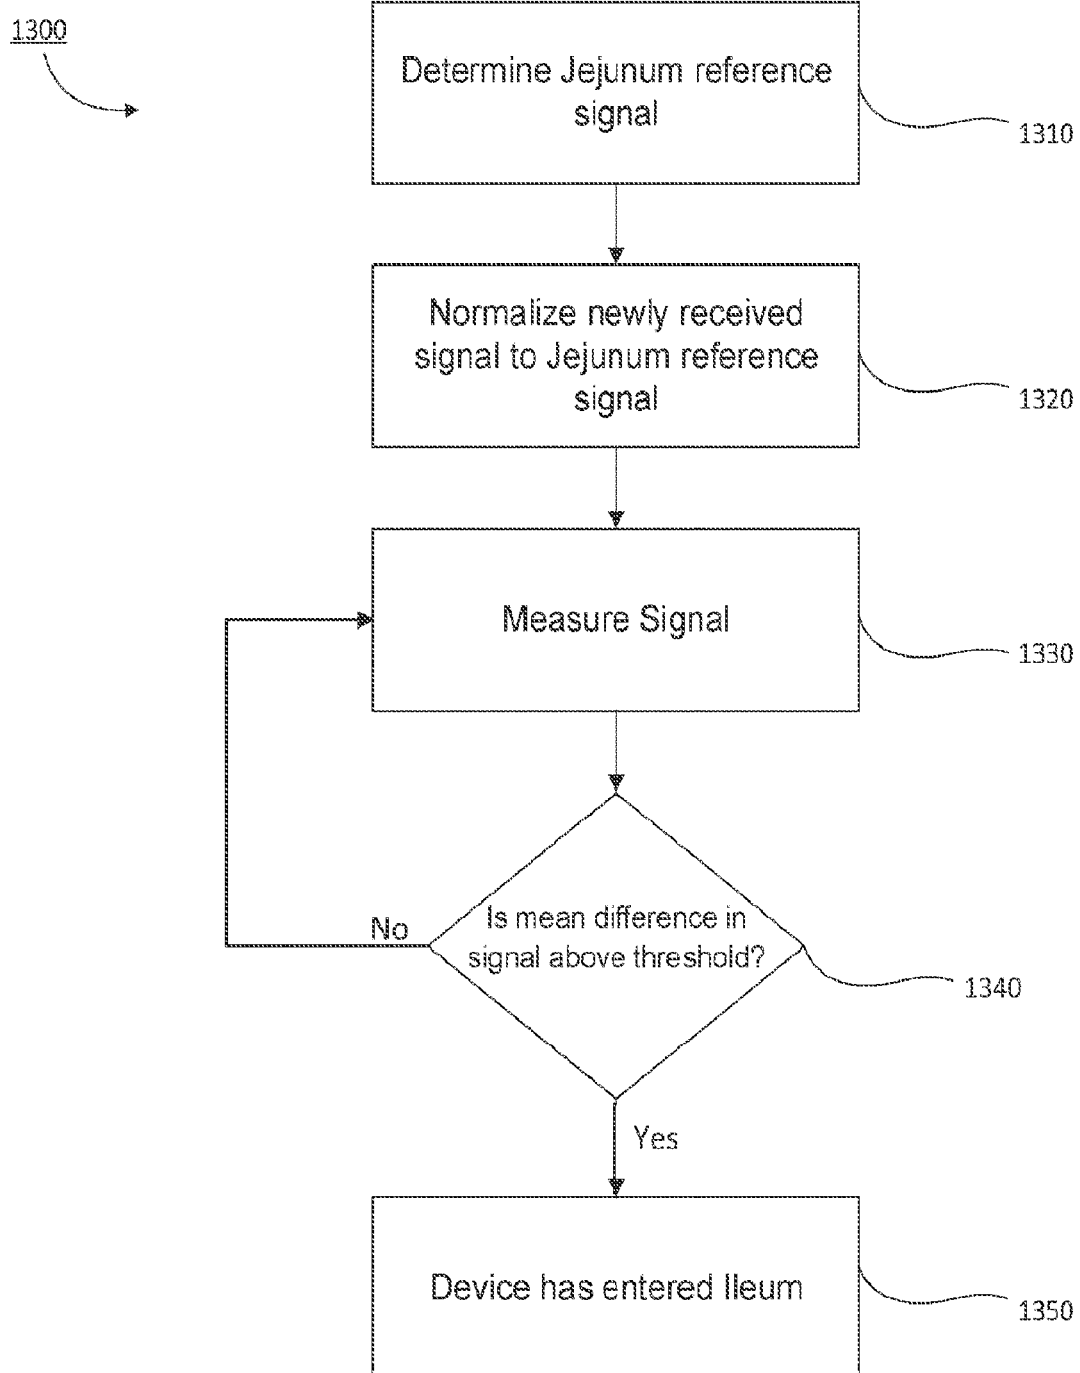


FIG. 13

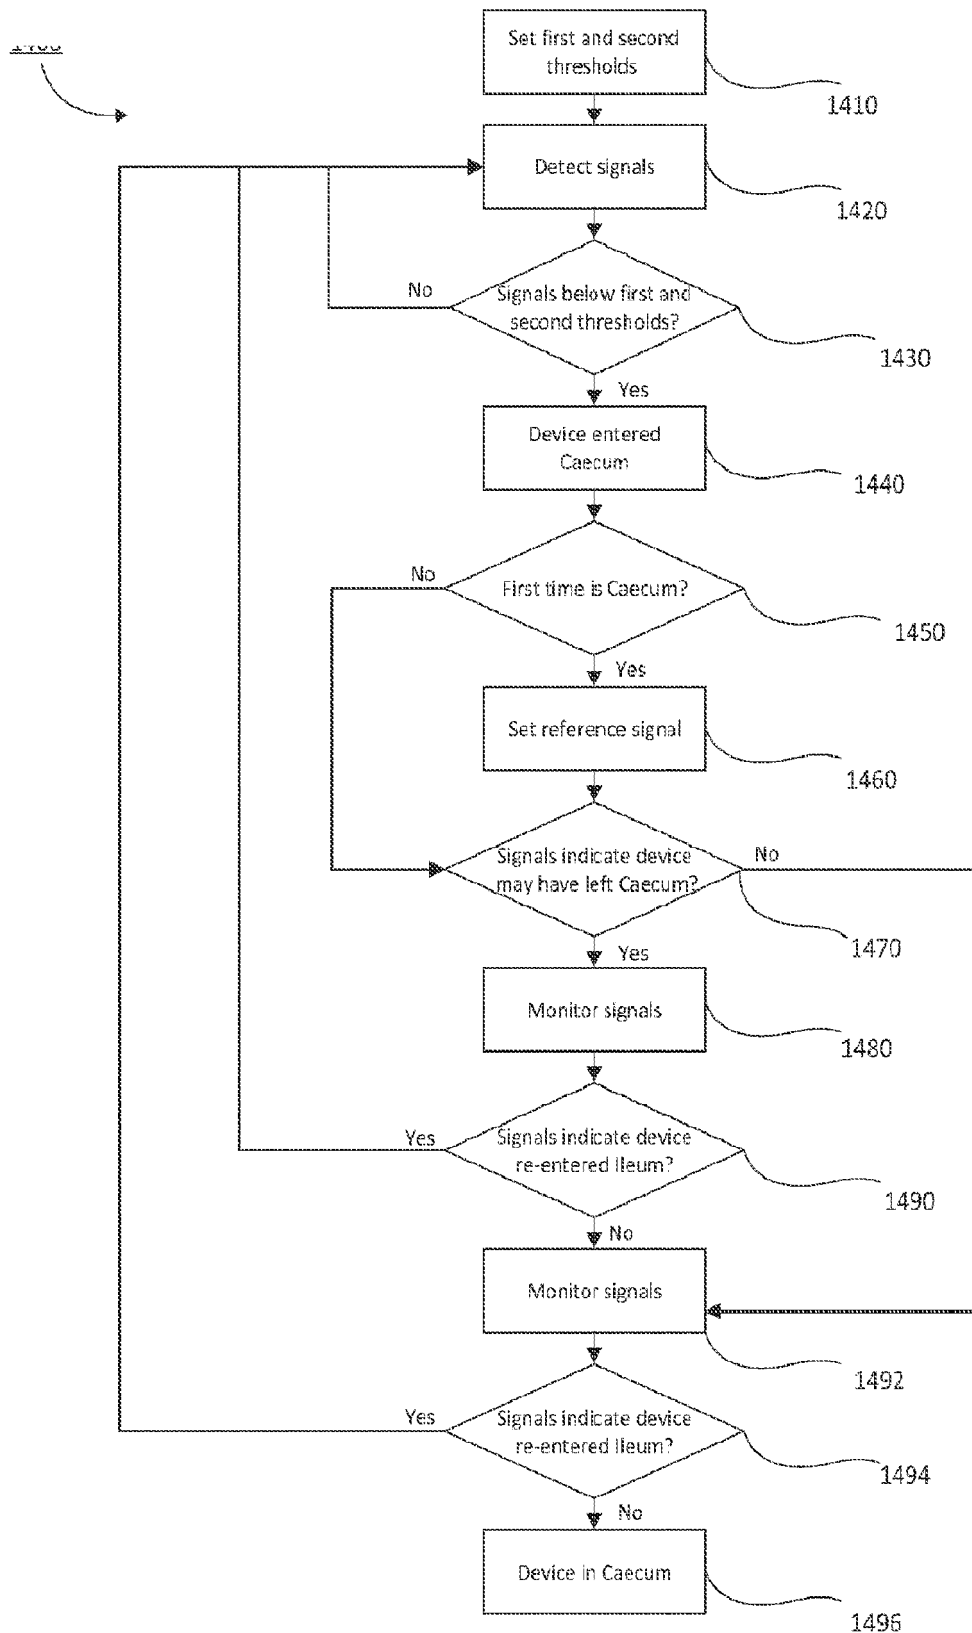


FIG. 14

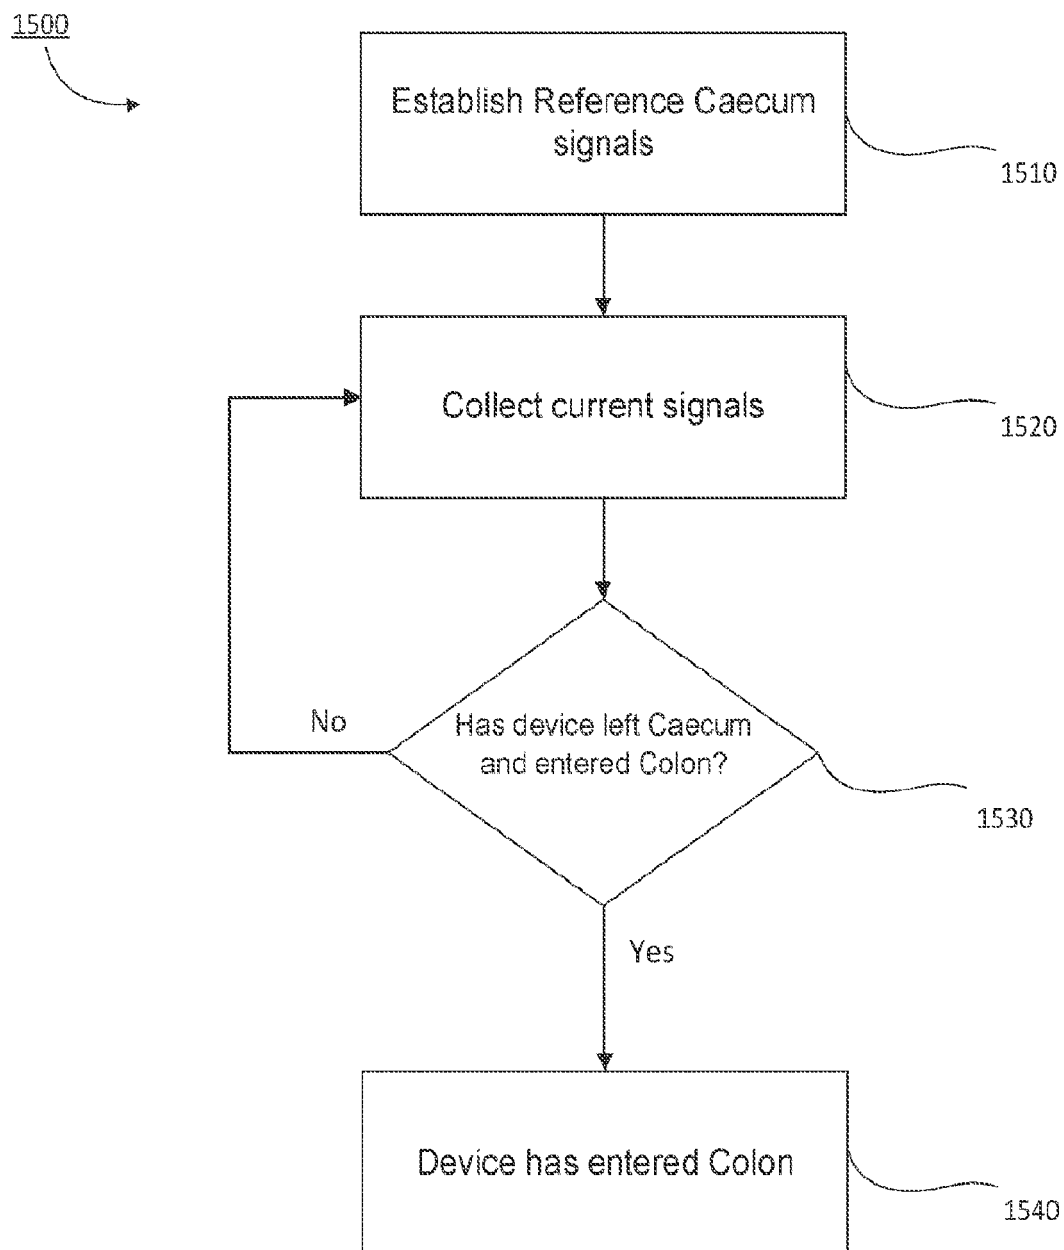


FIG. 15

1600

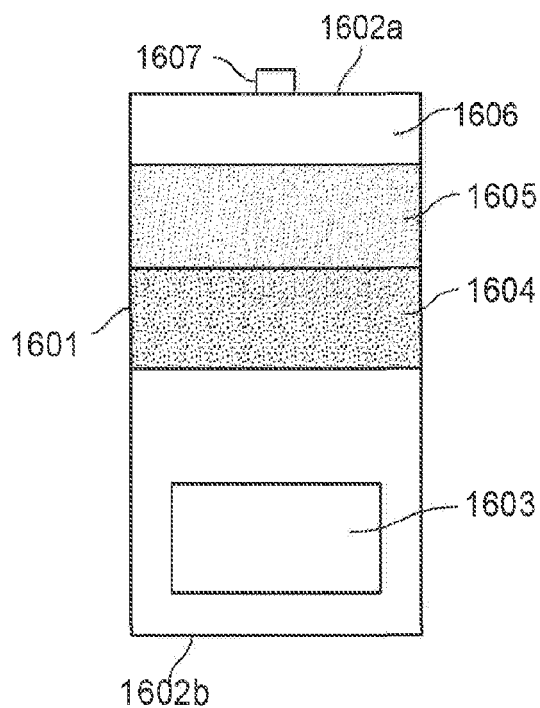


FIG. 16

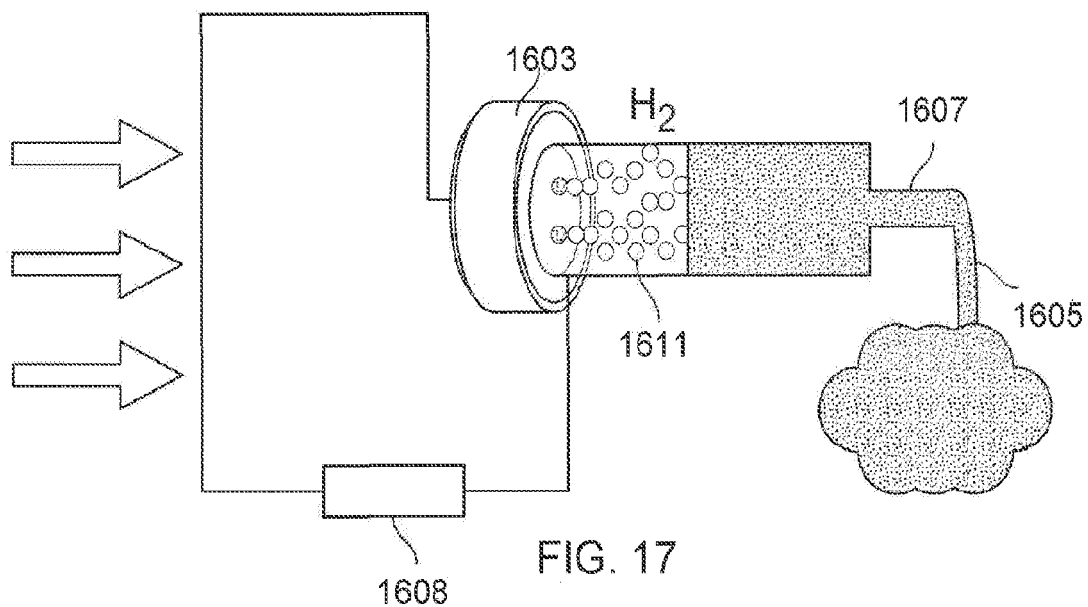


FIG. 17

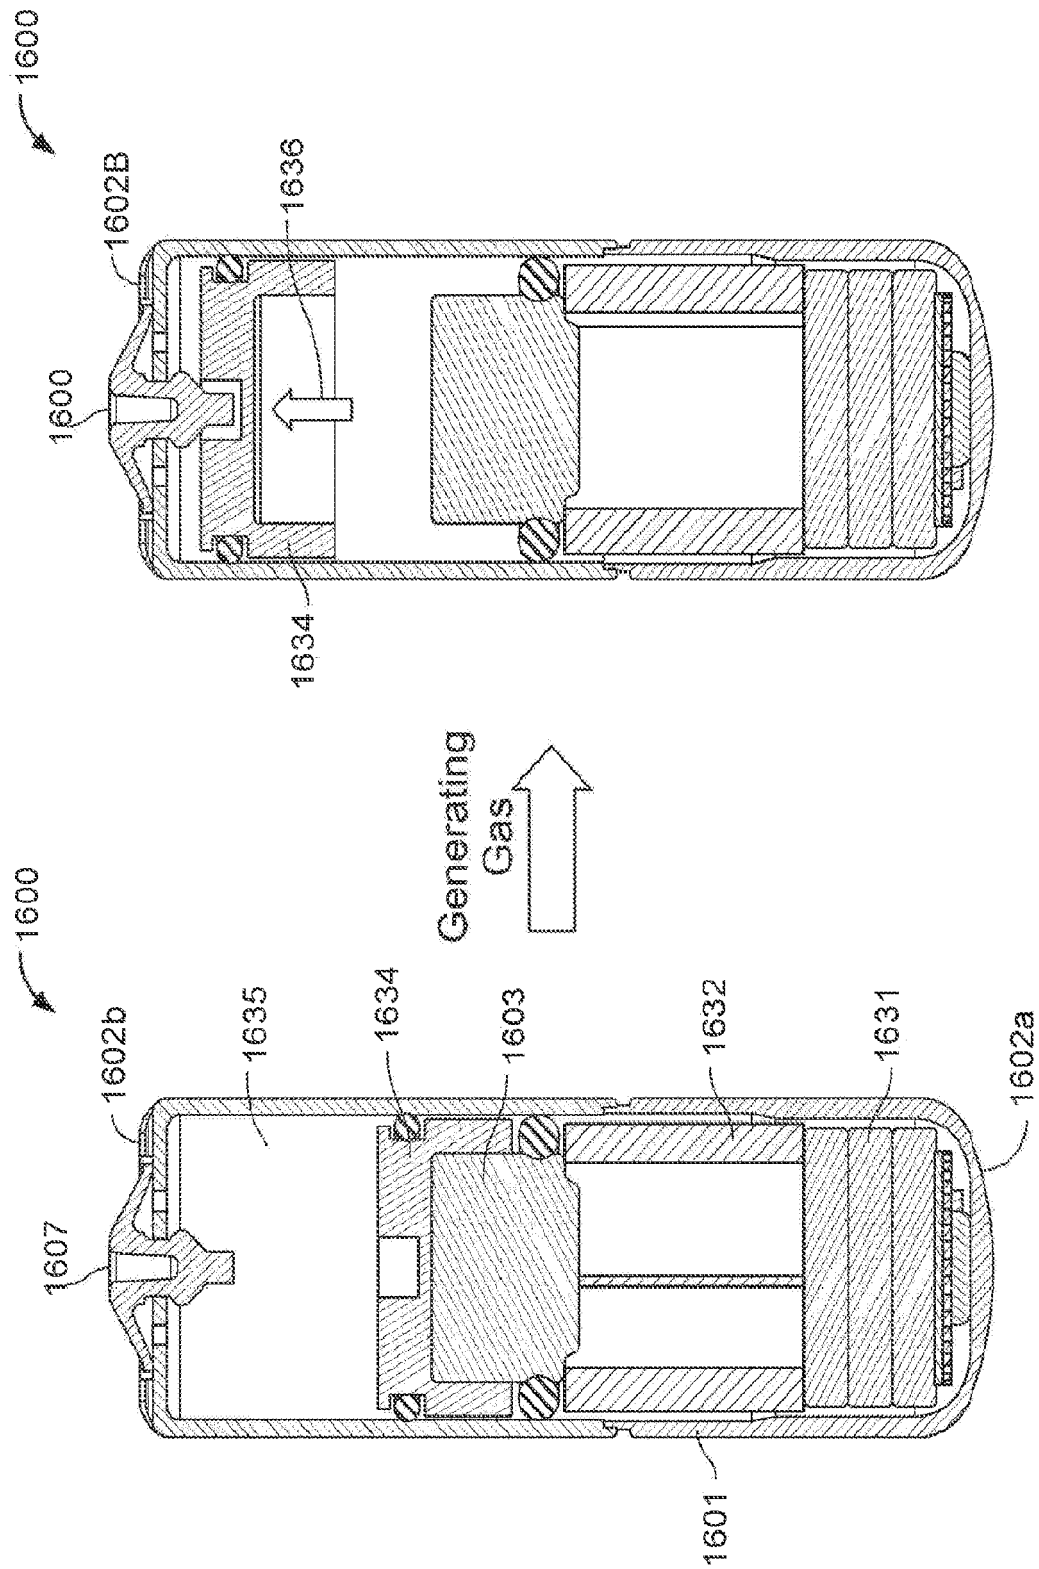


FIG. 18

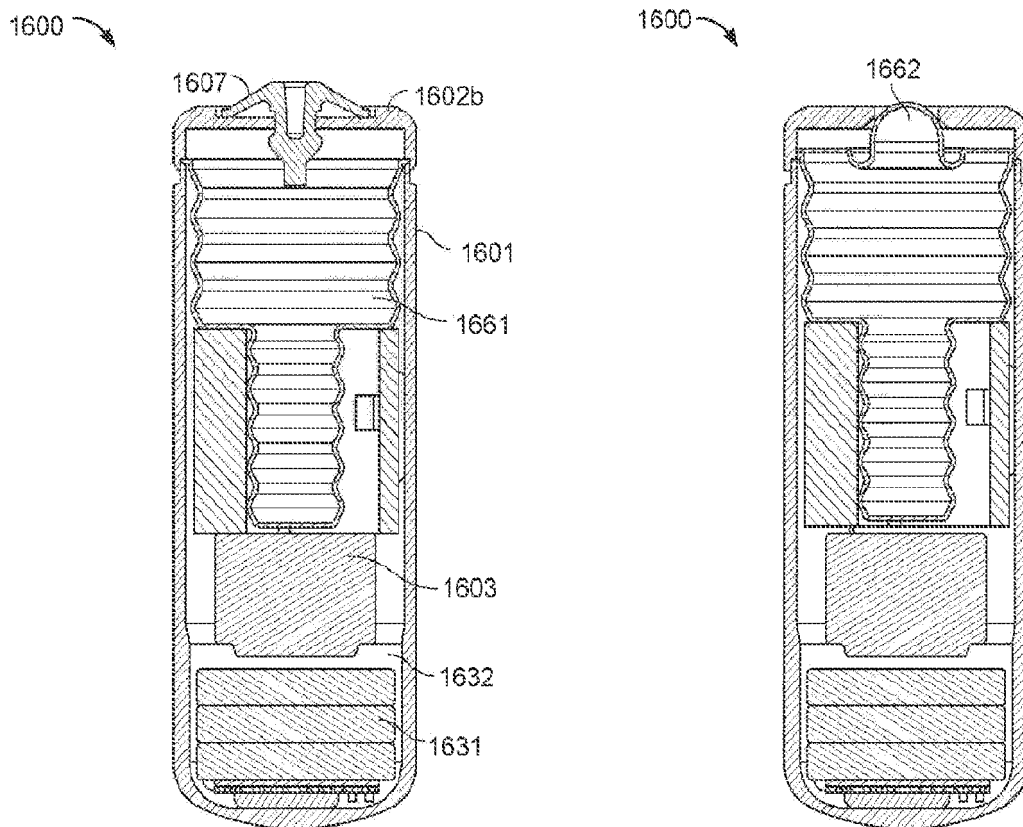


FIG. 19

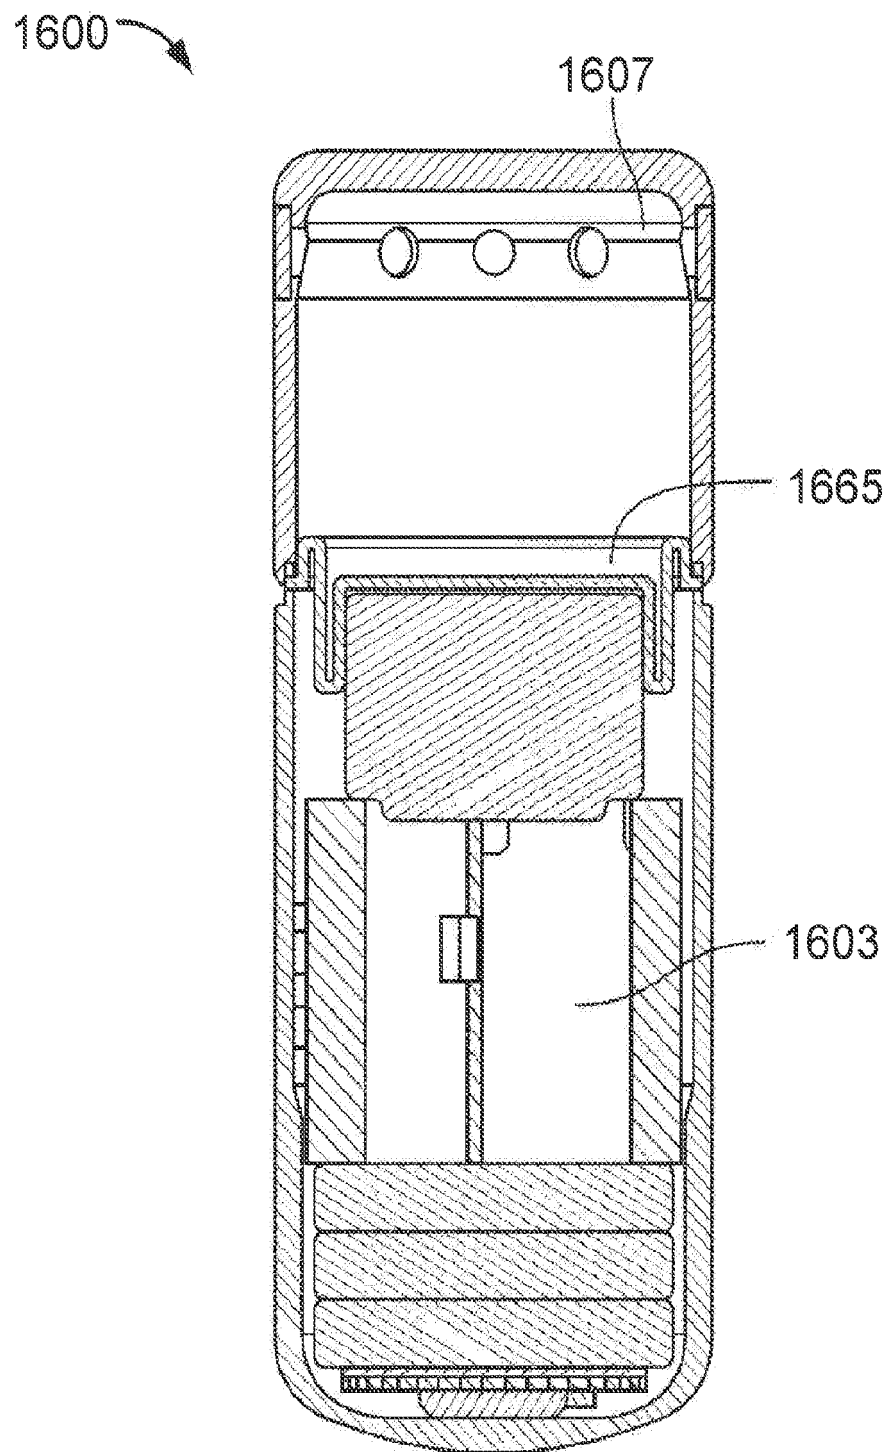


FIG. 20

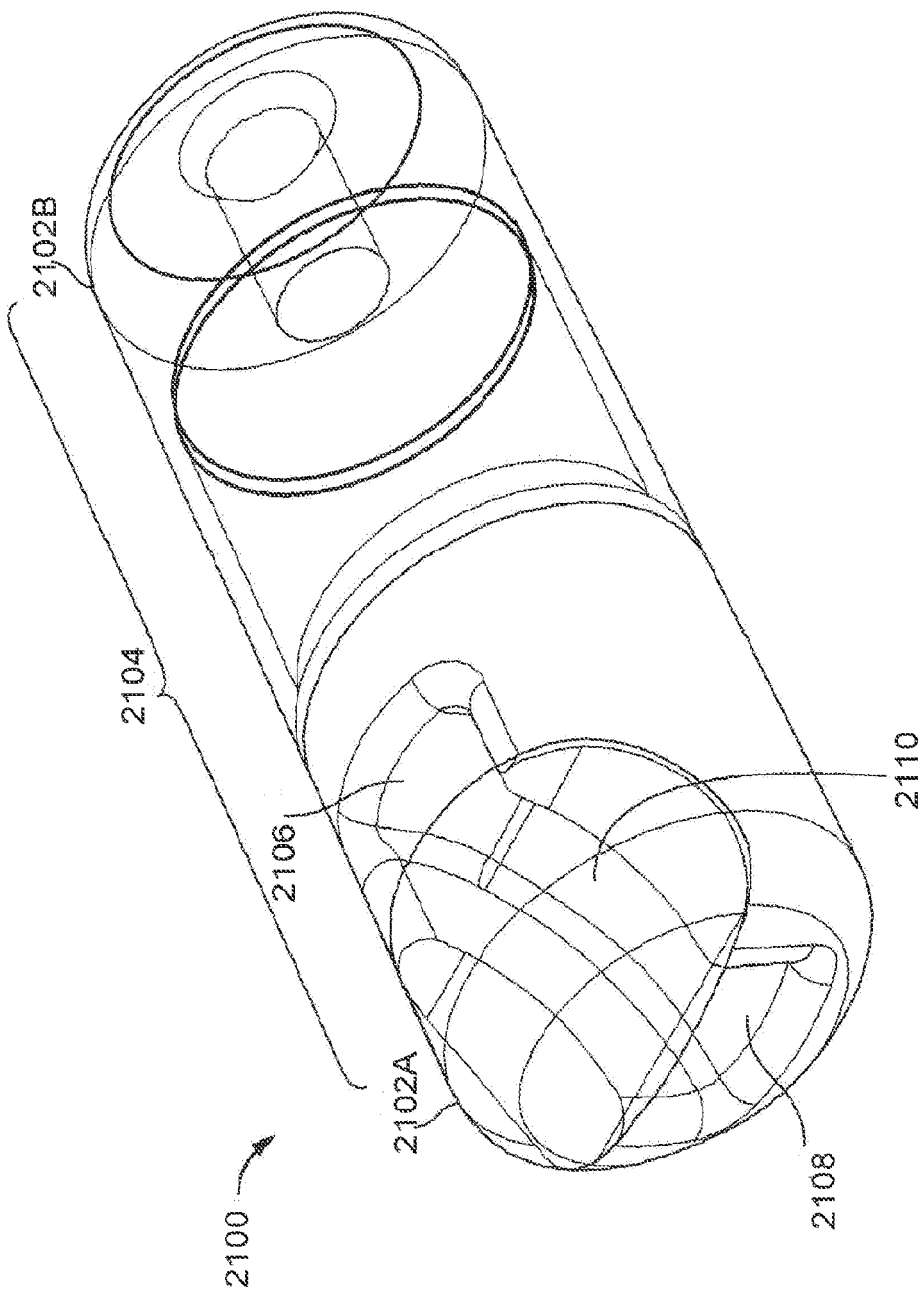


FIG. 21

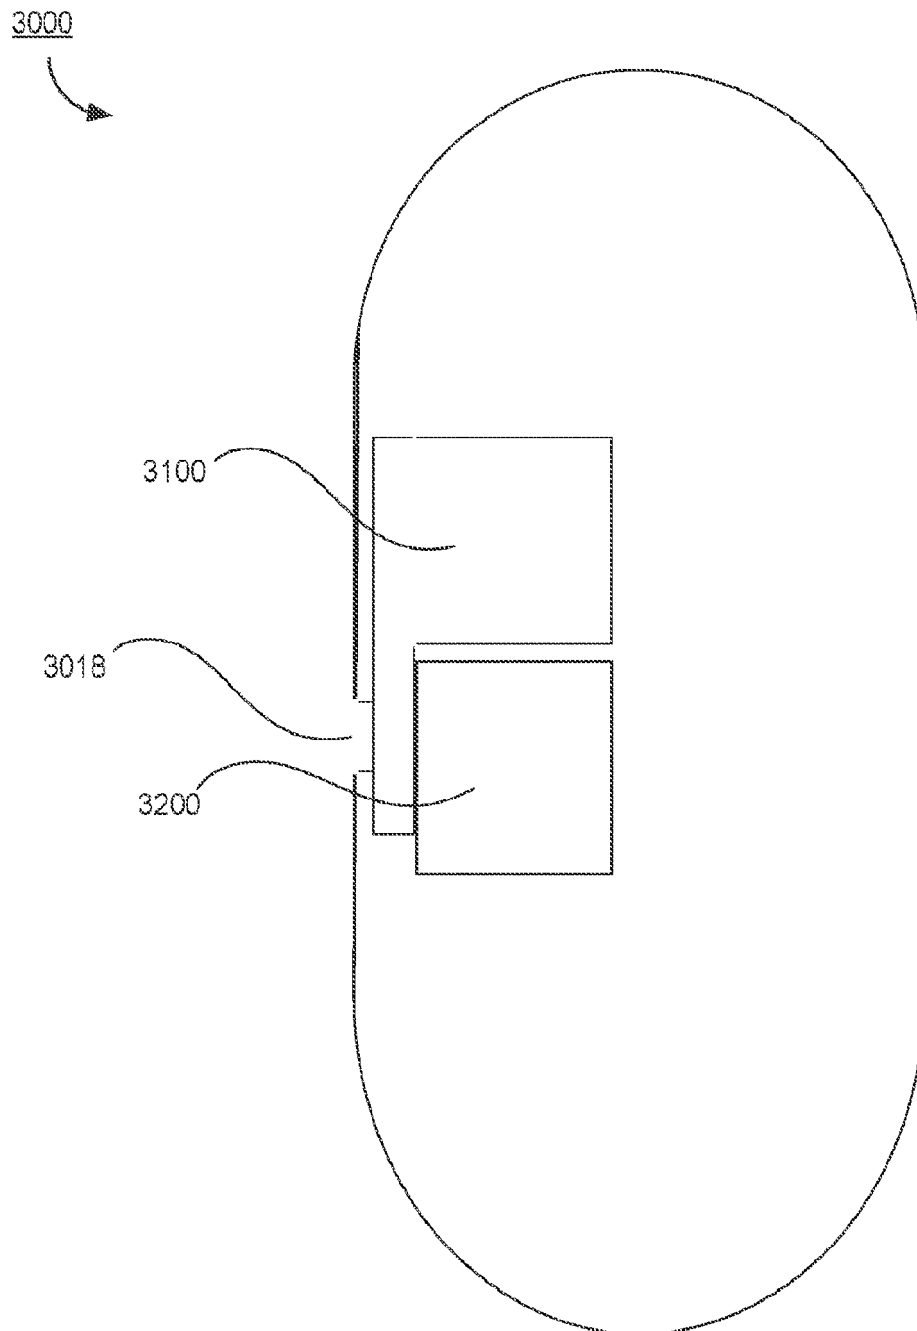


FIG. 22

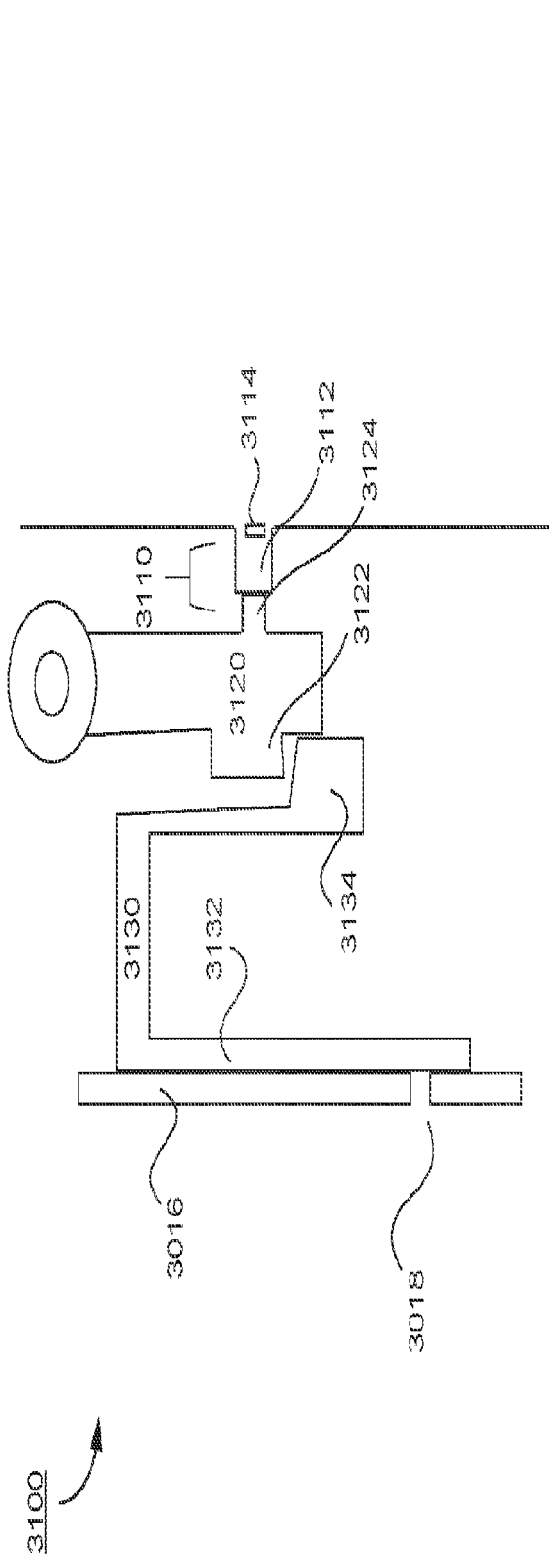


FIG. 23

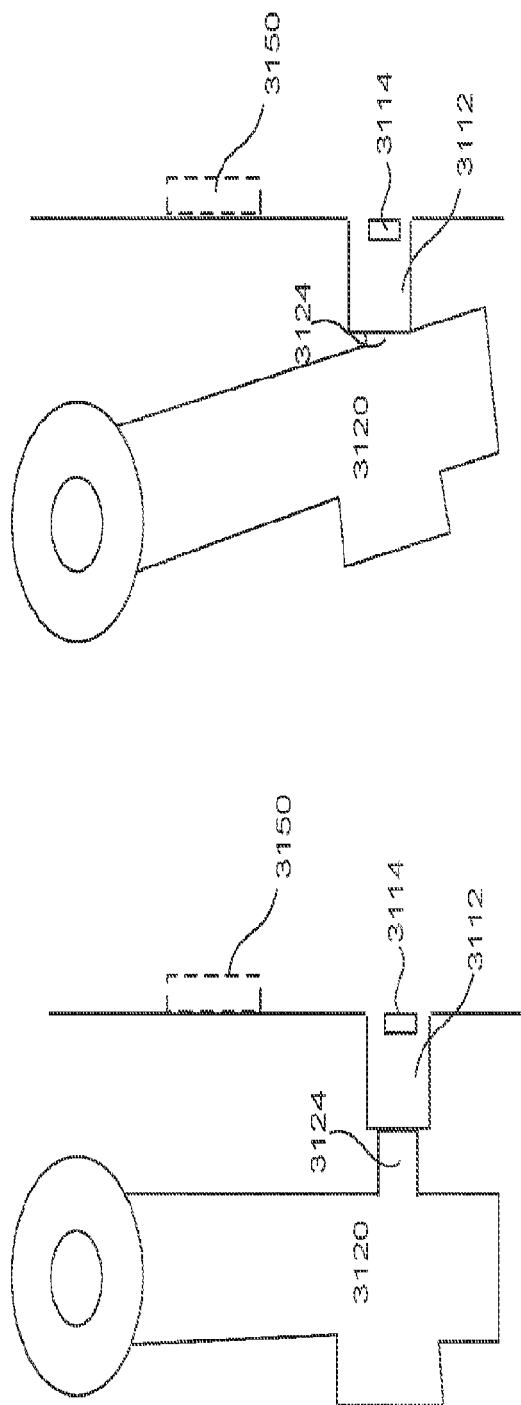


FIG. 24A

FIG. 24B

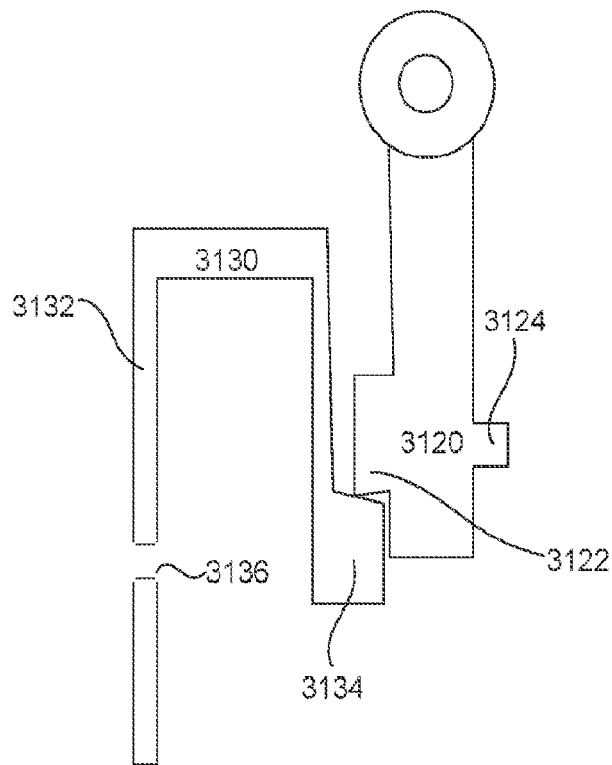


FIG. 25A

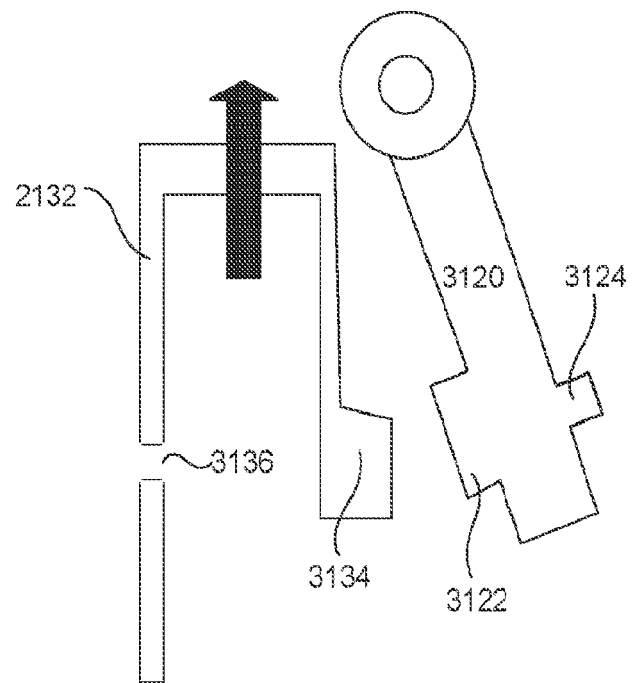


FIG. 25B

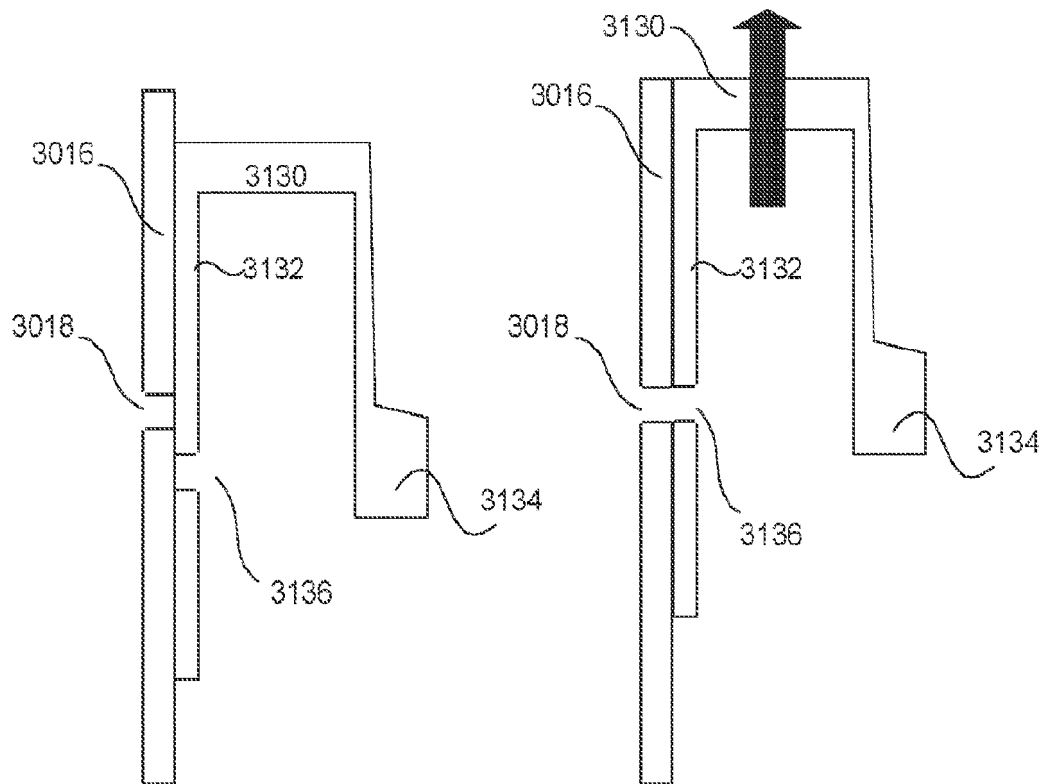


FIG. 26A

FIG. 26B

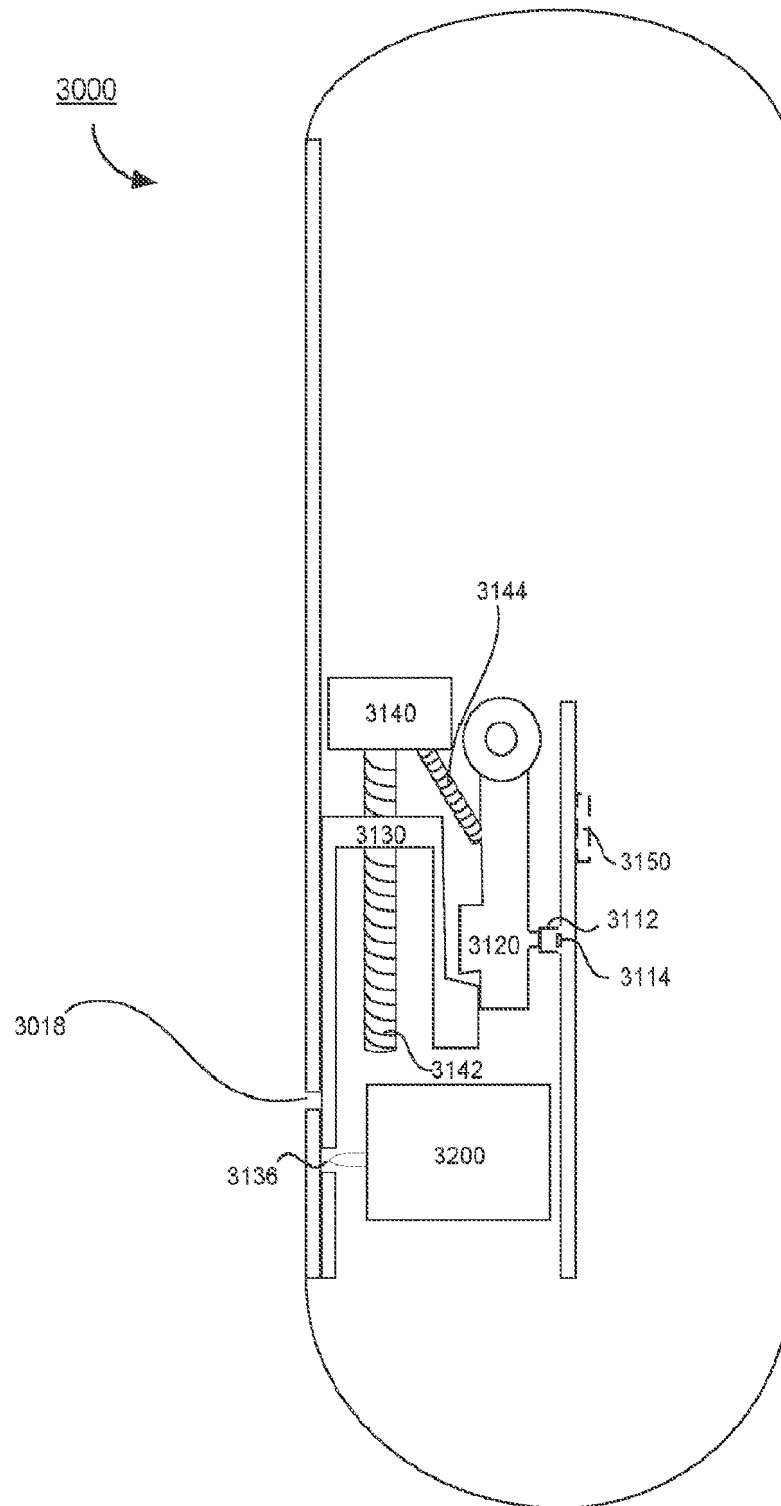


FIG. 27

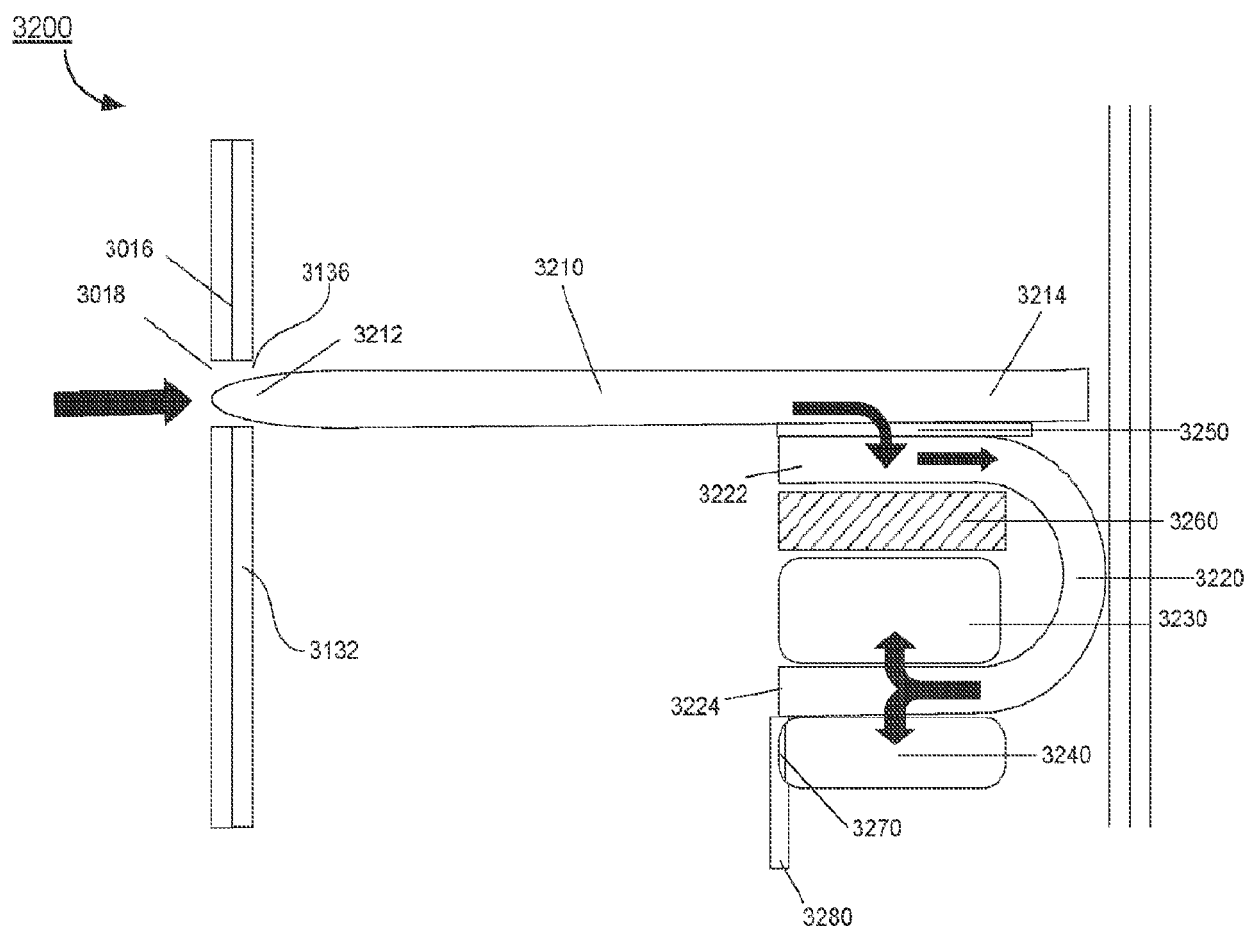


FIG. 28

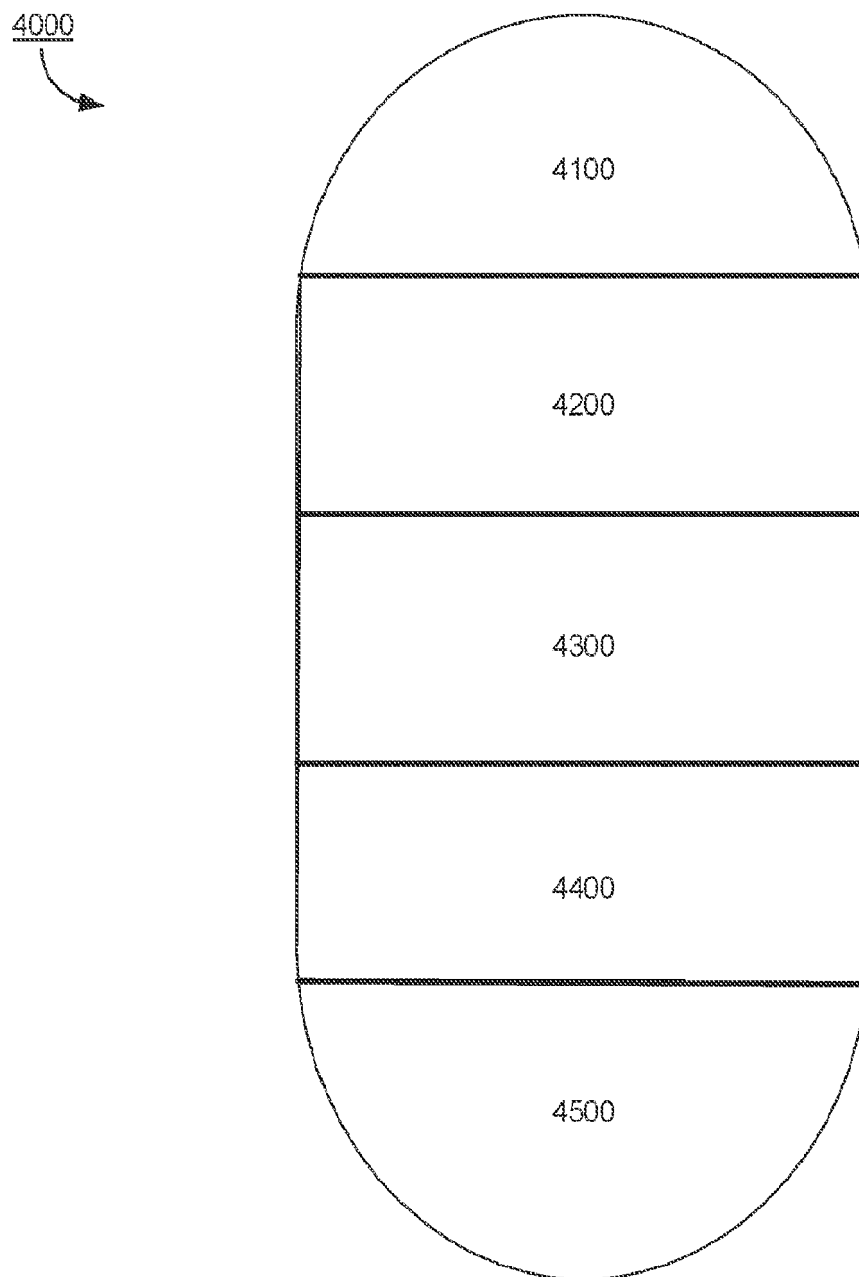


FIG. 29

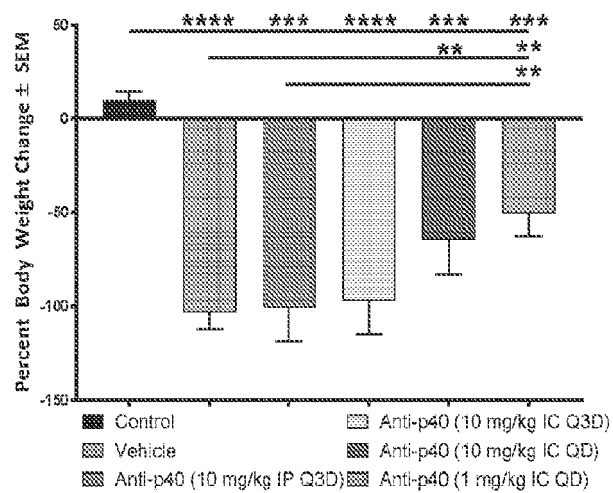


FIG. 30

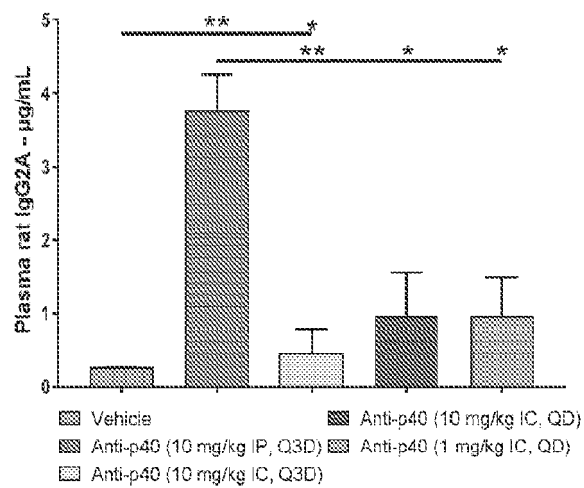


FIG. 31

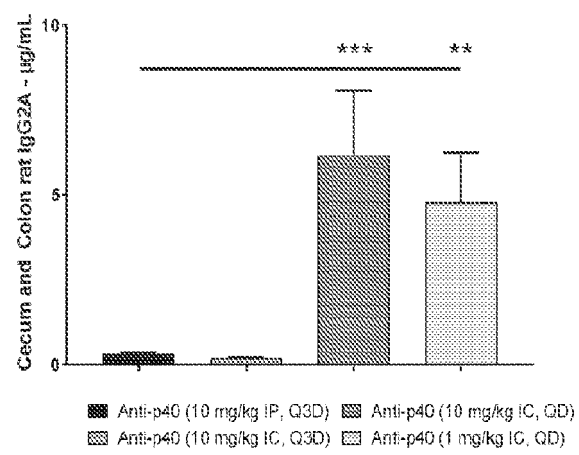


FIG. 32

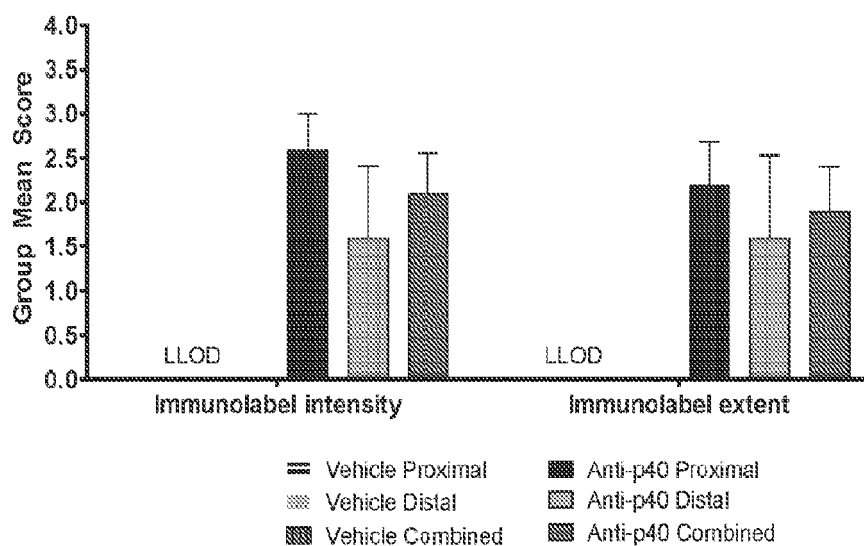


FIG. 33


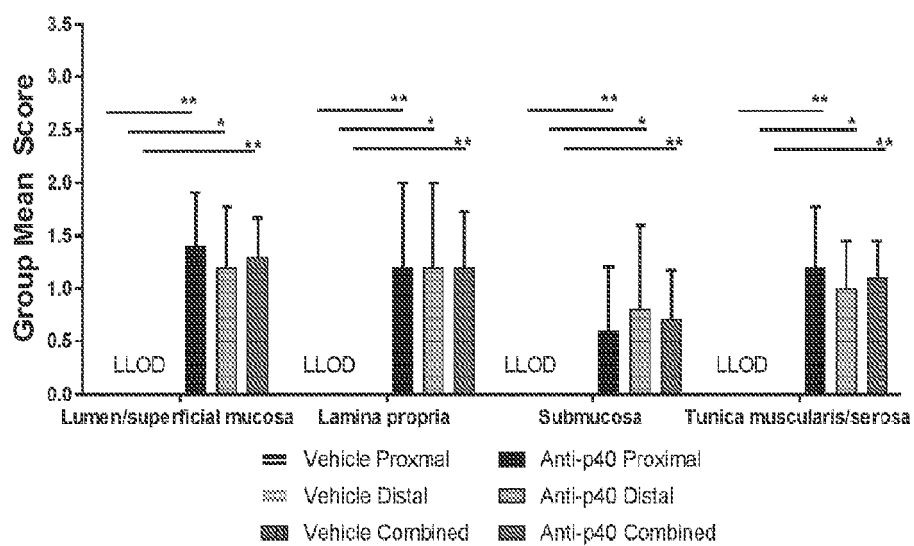


FIG. 34

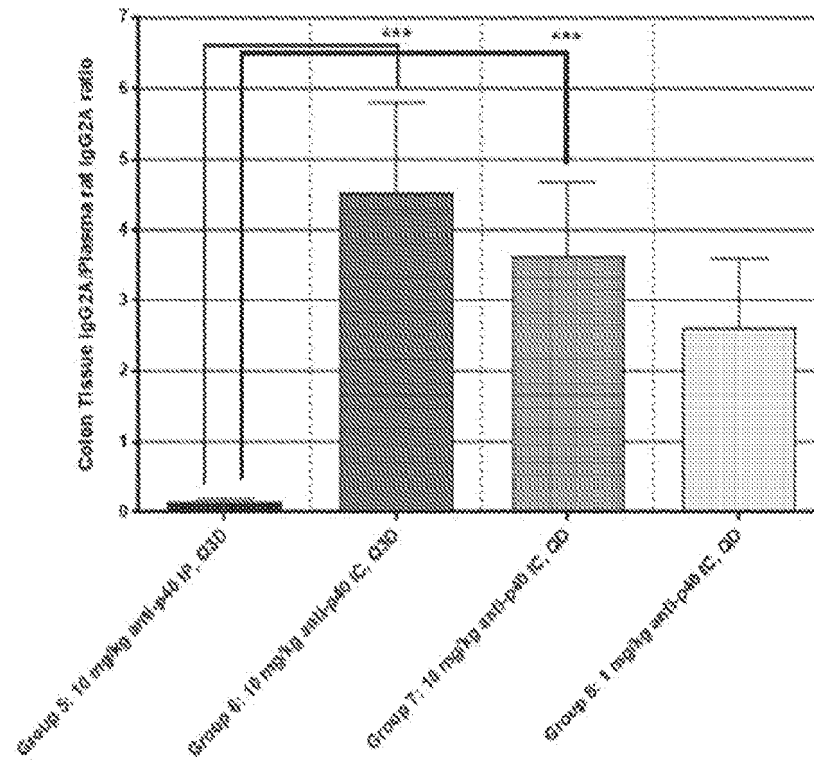

^Outlier removed from Group 5

FIG. 35

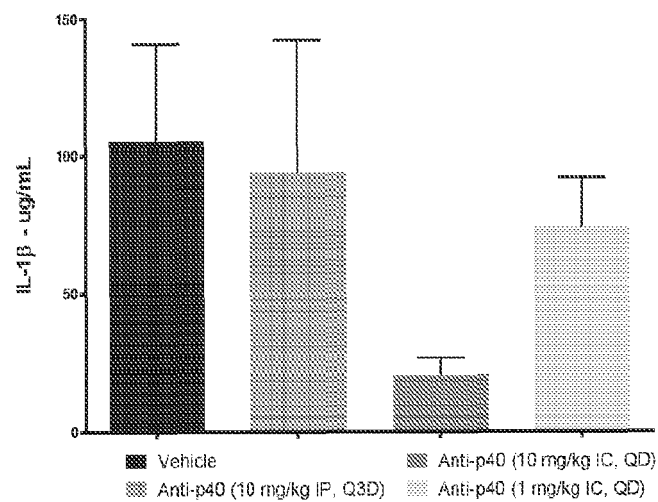


FIG. 36

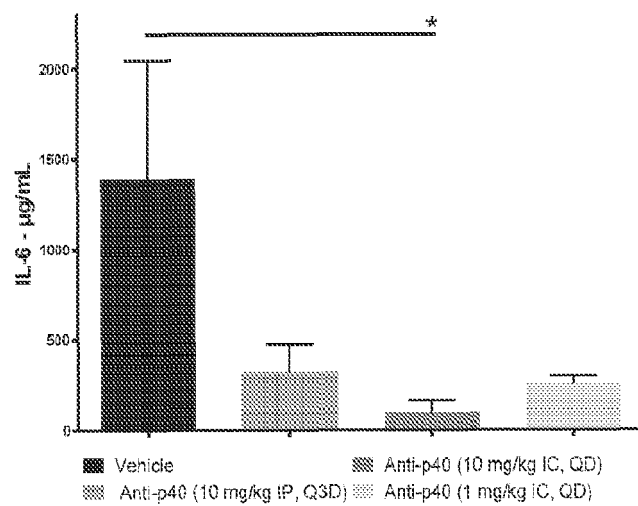
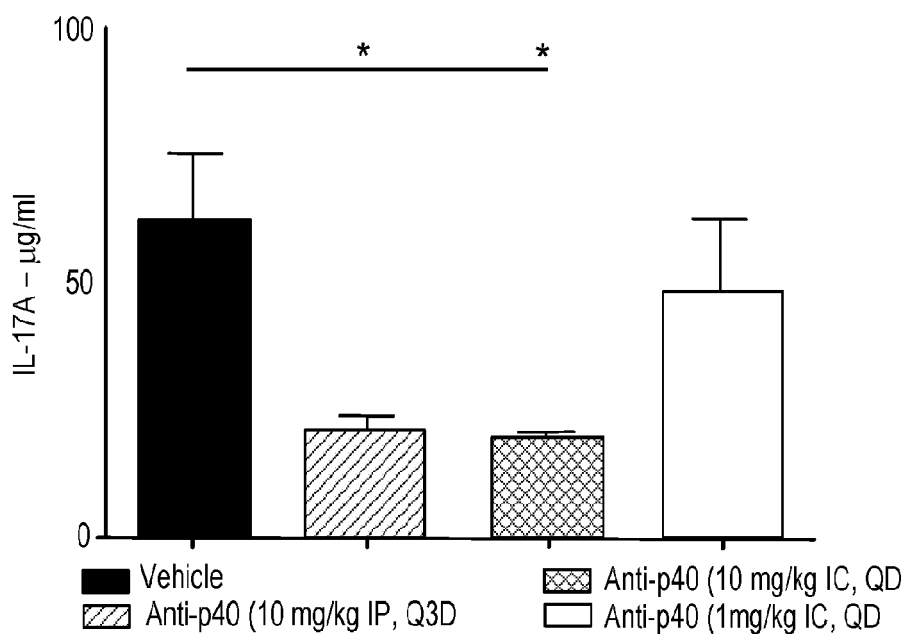
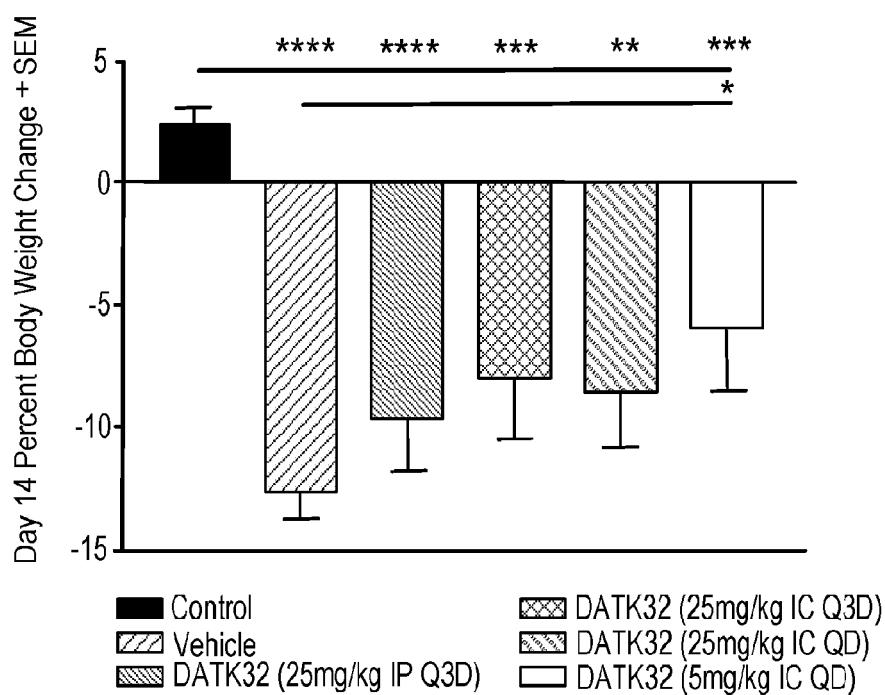


FIG. 37

**FIG. 38****FIG. 39**

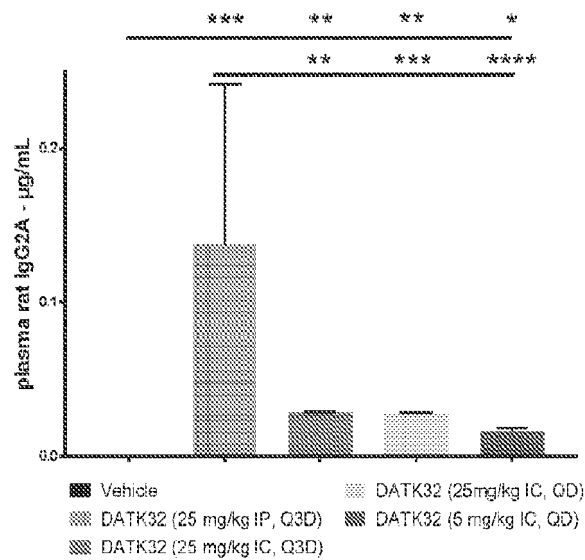


FIG. 40

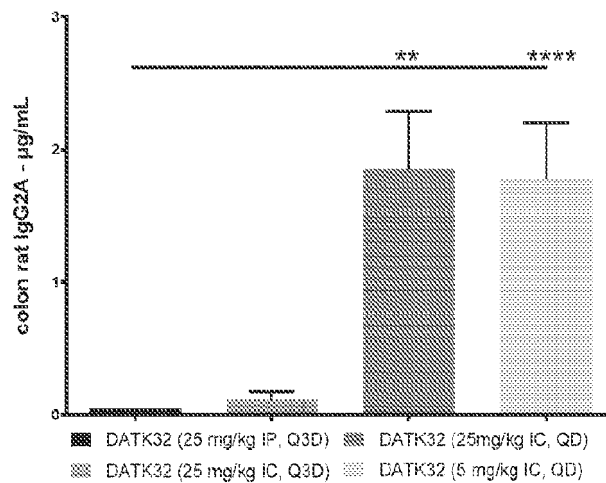


FIG. 41

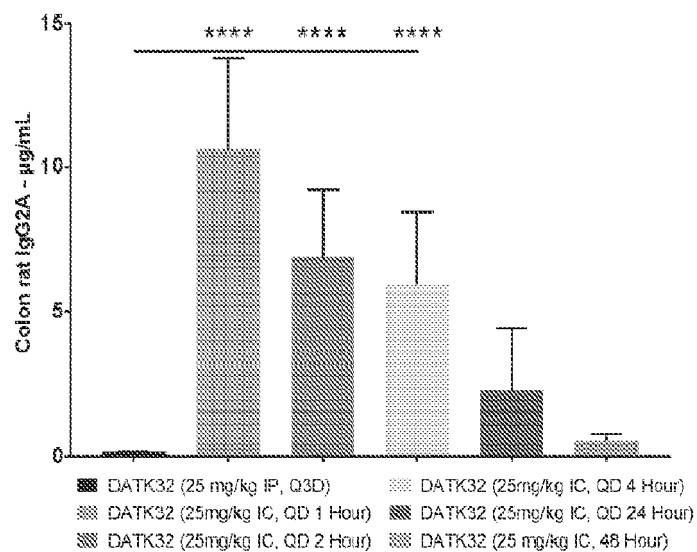


FIG. 42

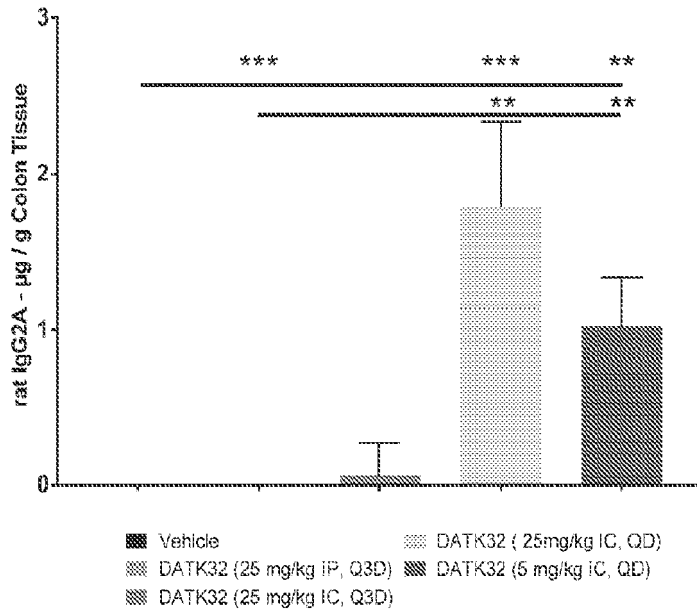


FIG. 43

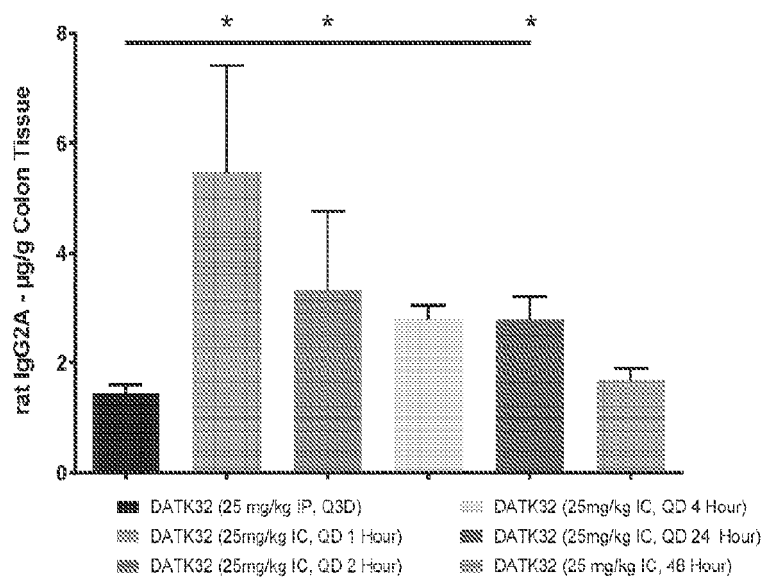


FIG. 44

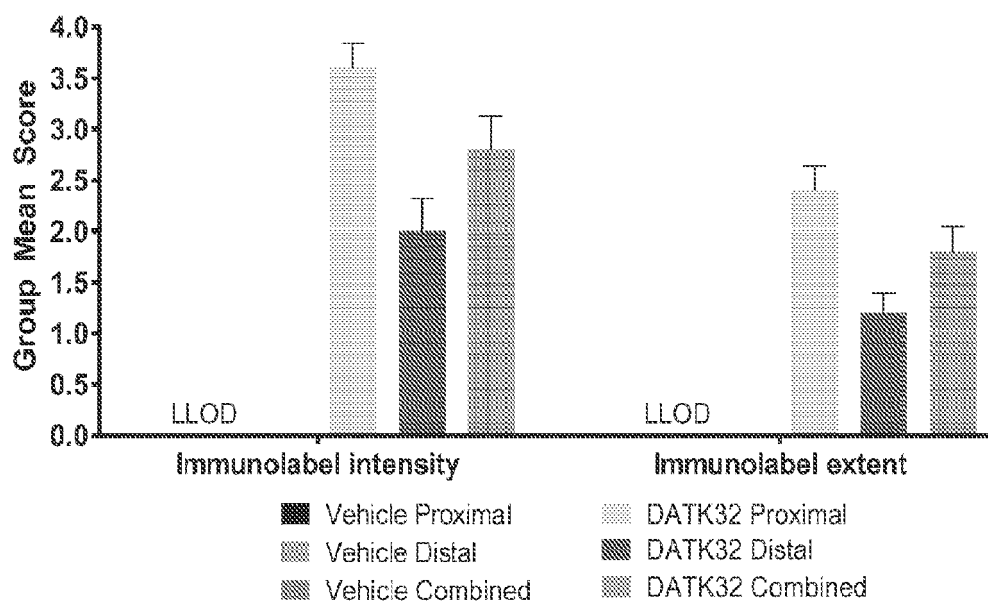


FIG. 45

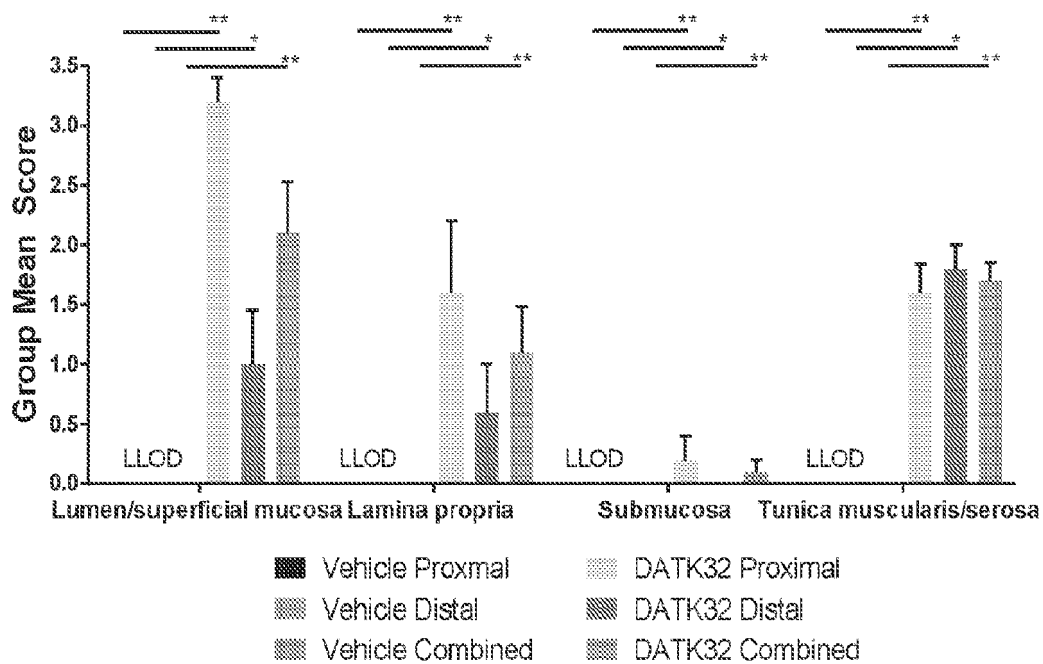


FIG. 46

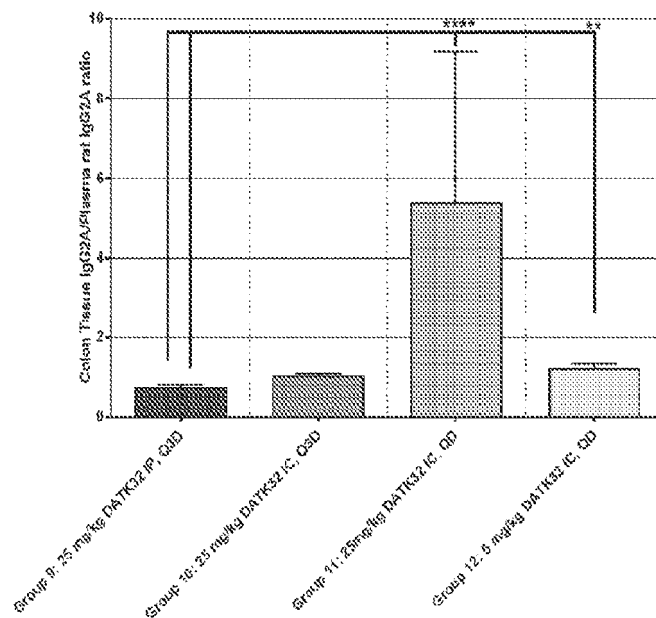


FIG. 47

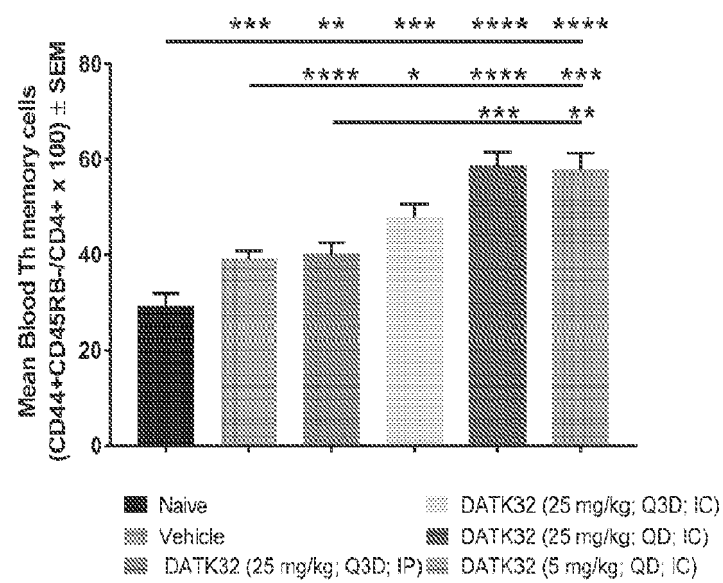


FIG. 48

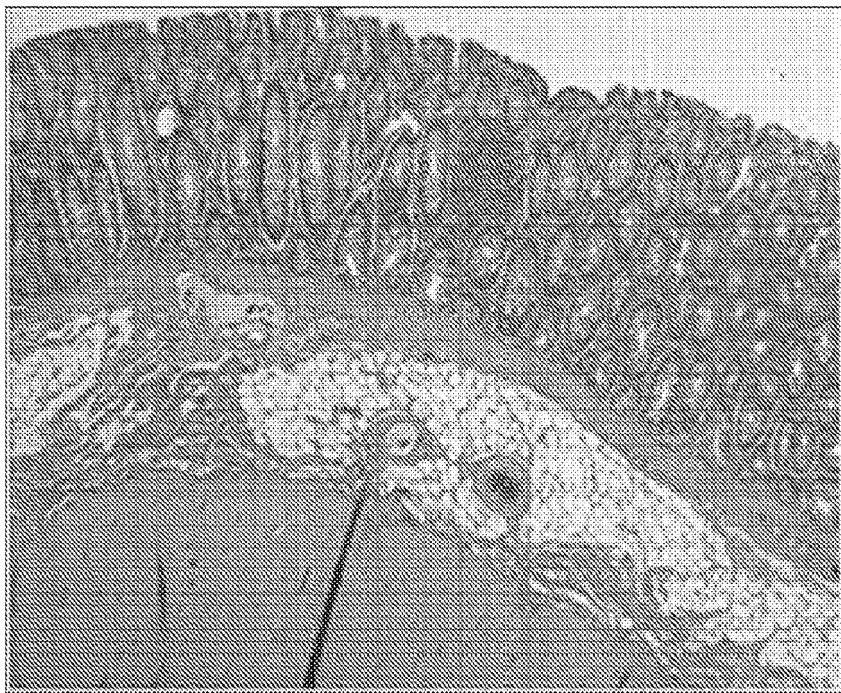


FIG. 49



FIG. 50

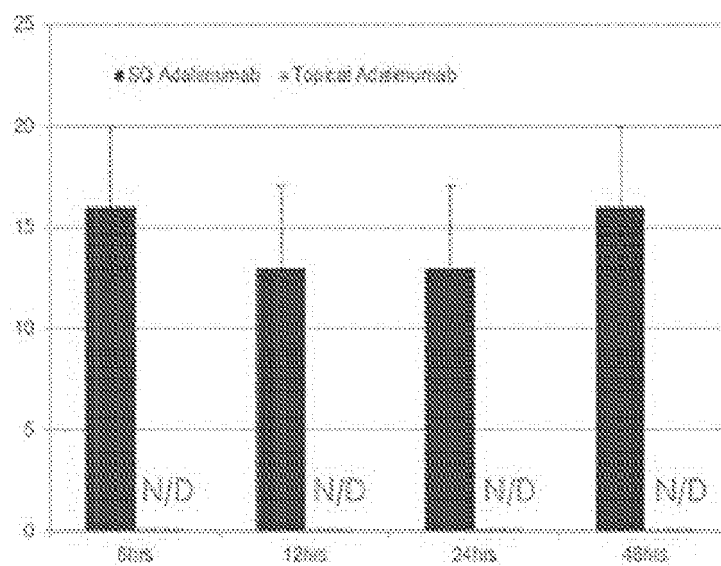


FIG. 51

Time	SQ Adalimumab Plasma concentration $\mu\text{g}/\text{ml}$	Topical Adalimumab Plasma concentration $\mu\text{g}/\text{ml}$
6hrs	16 \pm 8	0.01
12hrs	13 \pm 4	0.01
24hrs	13 \pm 3	0.01
48hrs	16 \pm 5	0.01

FIG. 52

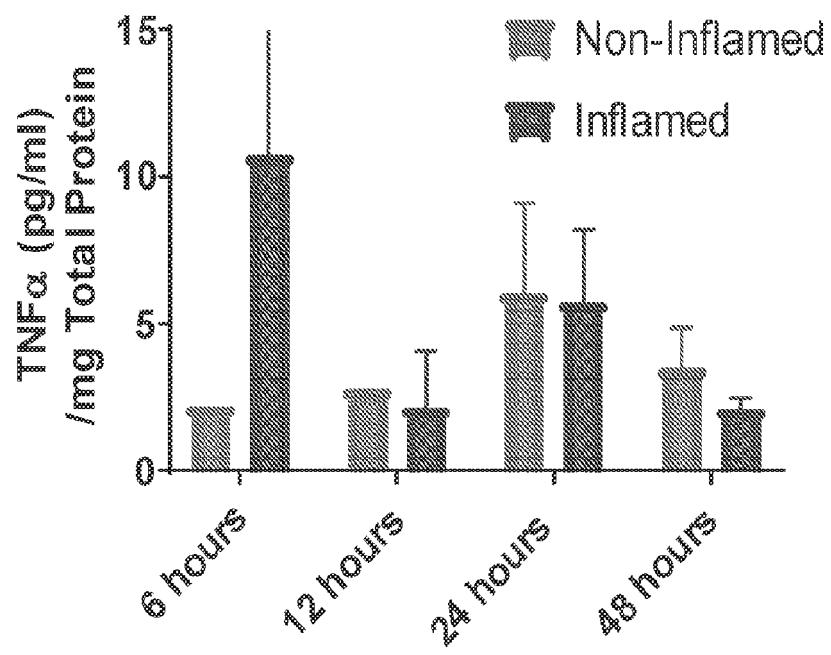


FIG. 53

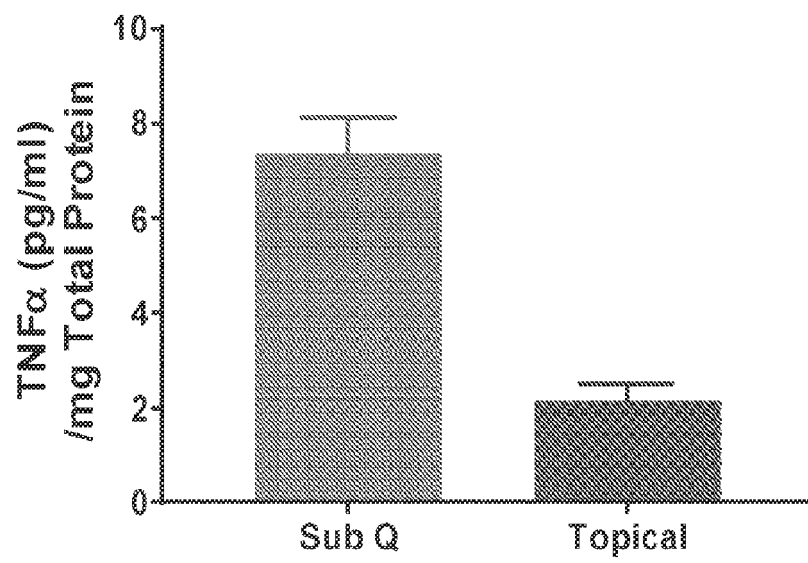


Fig. 54

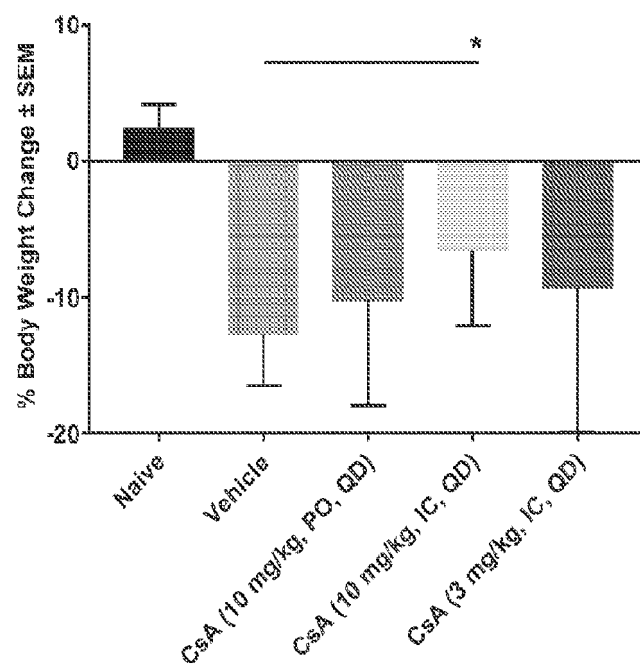


FIG. 55

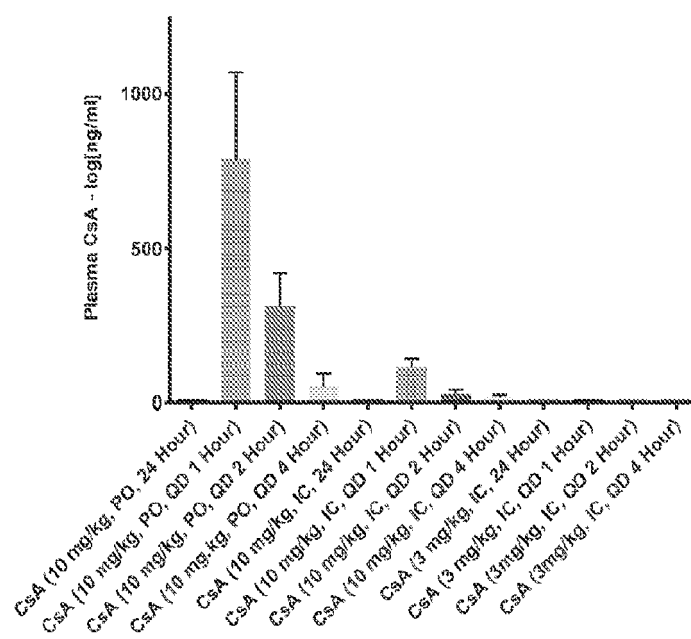


FIG. 56

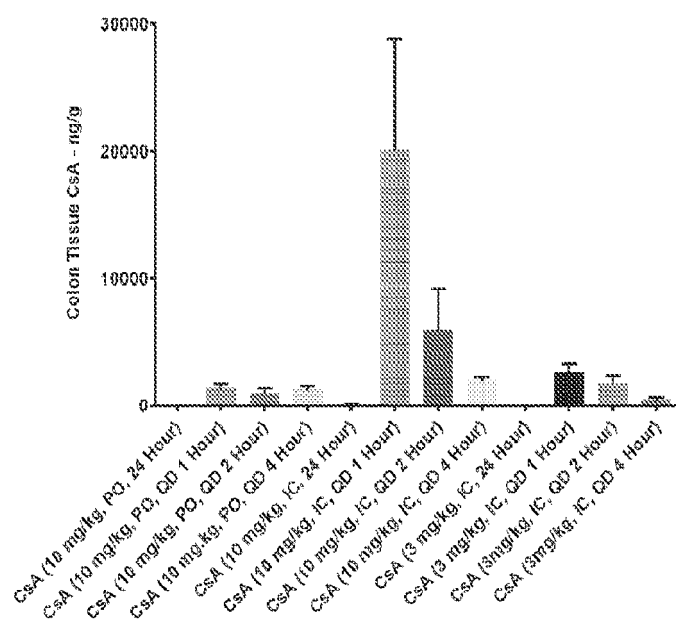


FIG. 57

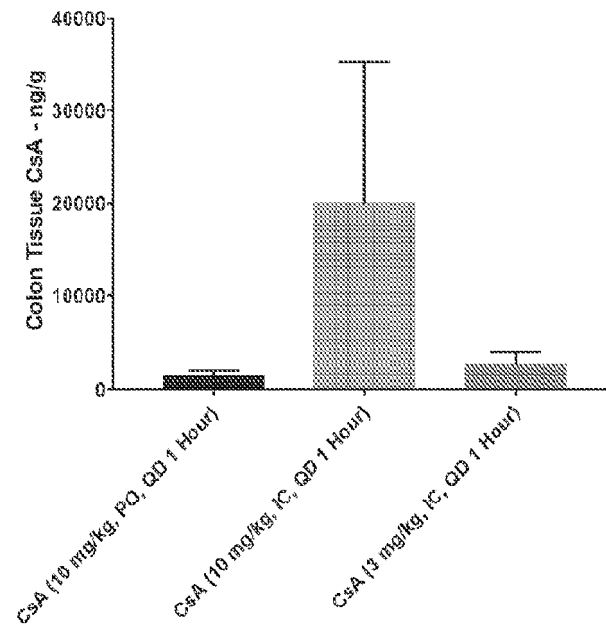


FIG. 58

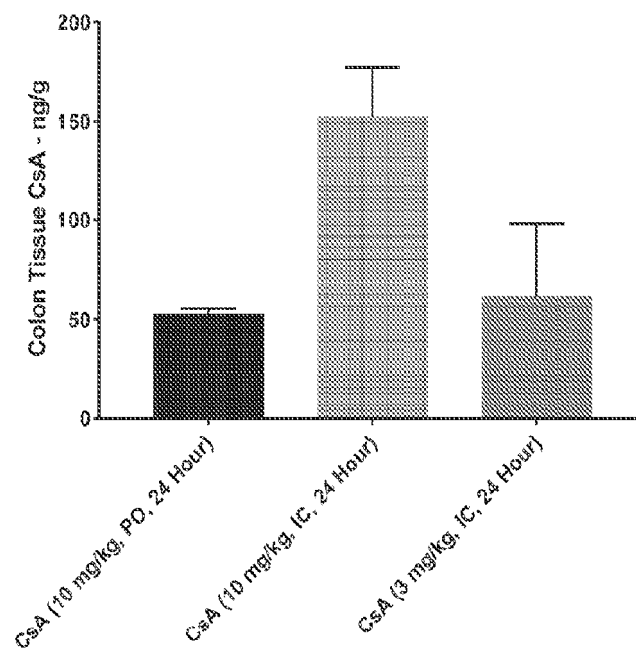


FIG. 59

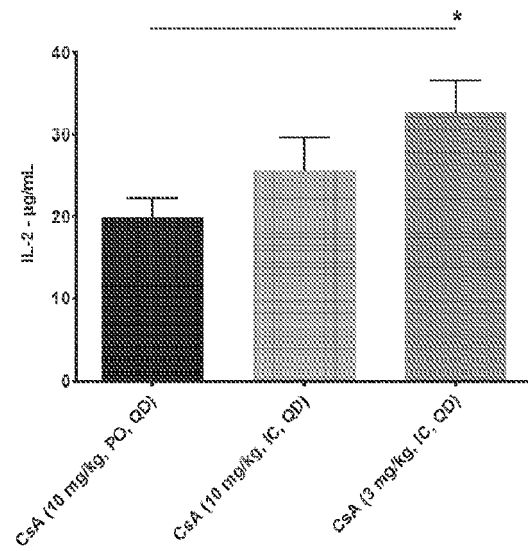


FIG. 60

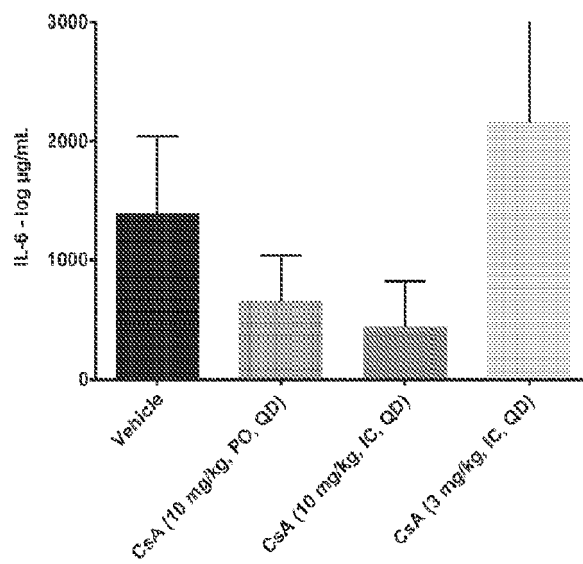


FIG. 61

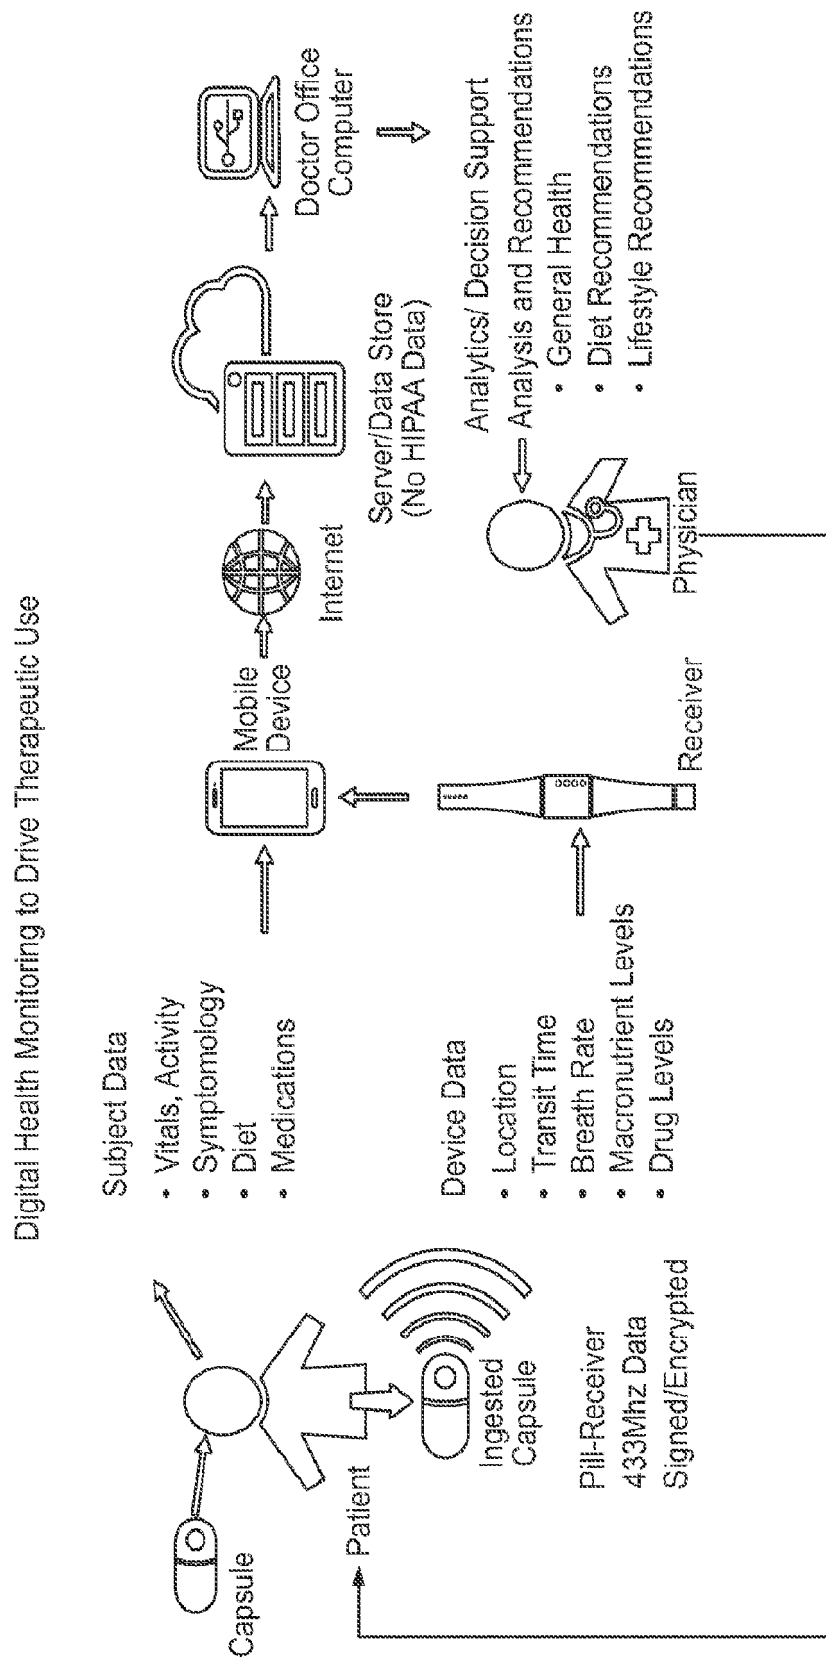
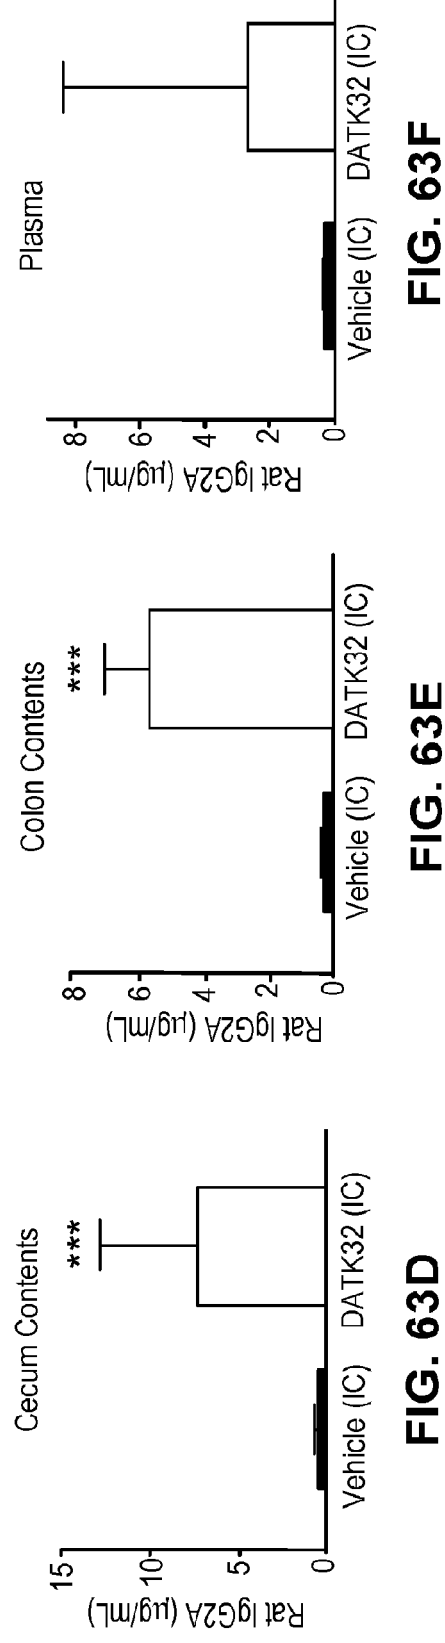
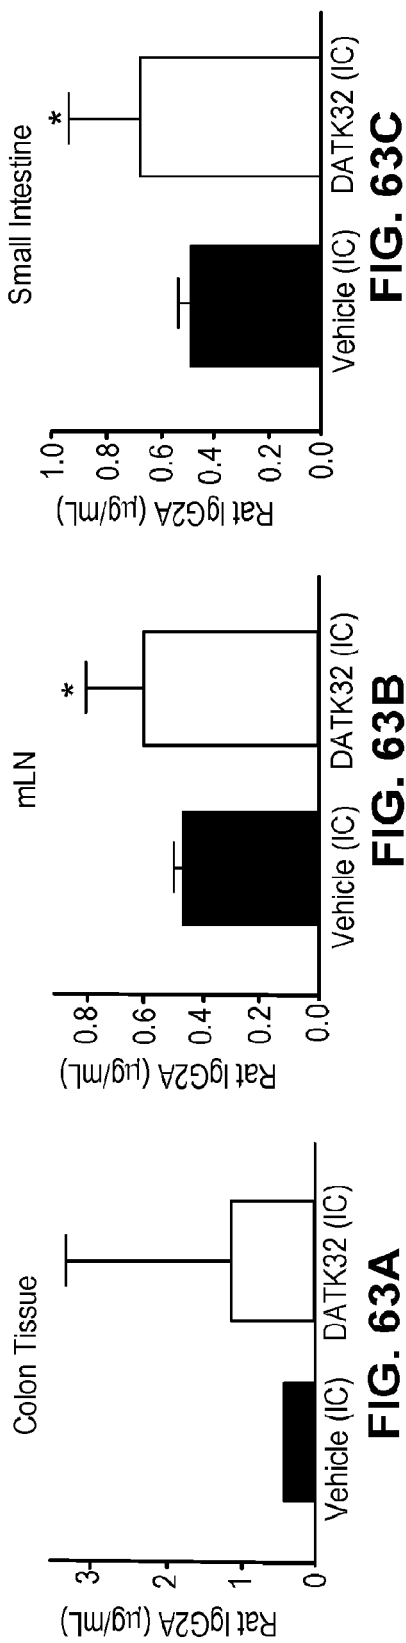


FIG.62



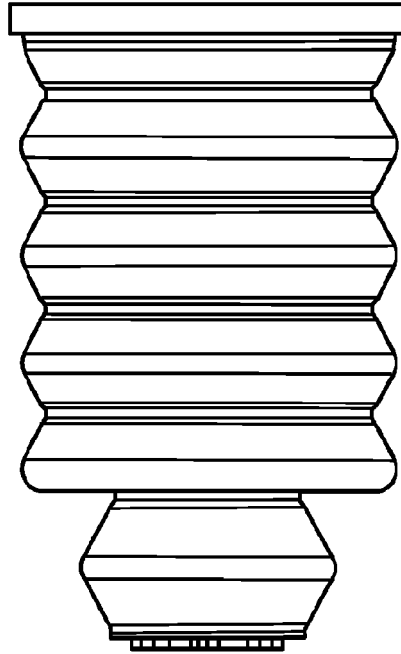


FIG. 64

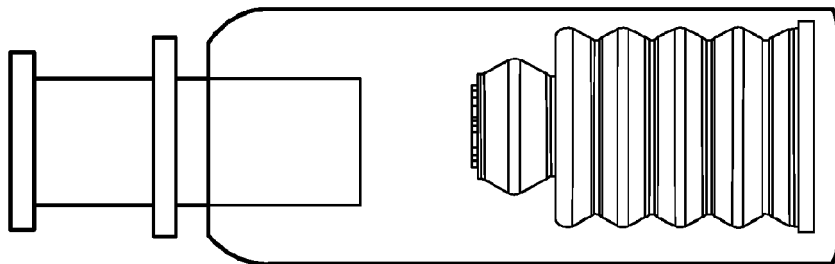


FIG. 65

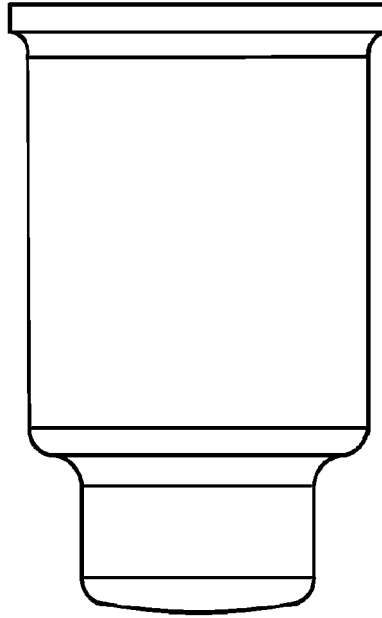


FIG. 66

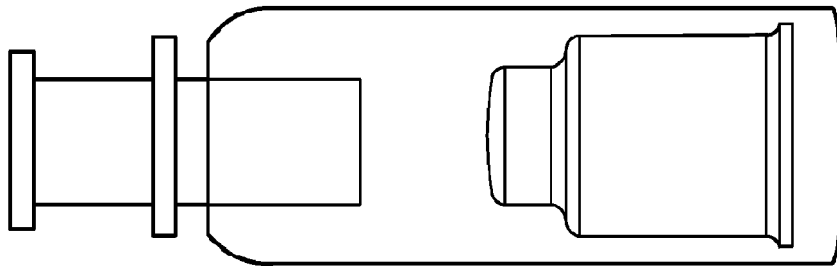


FIG. 67

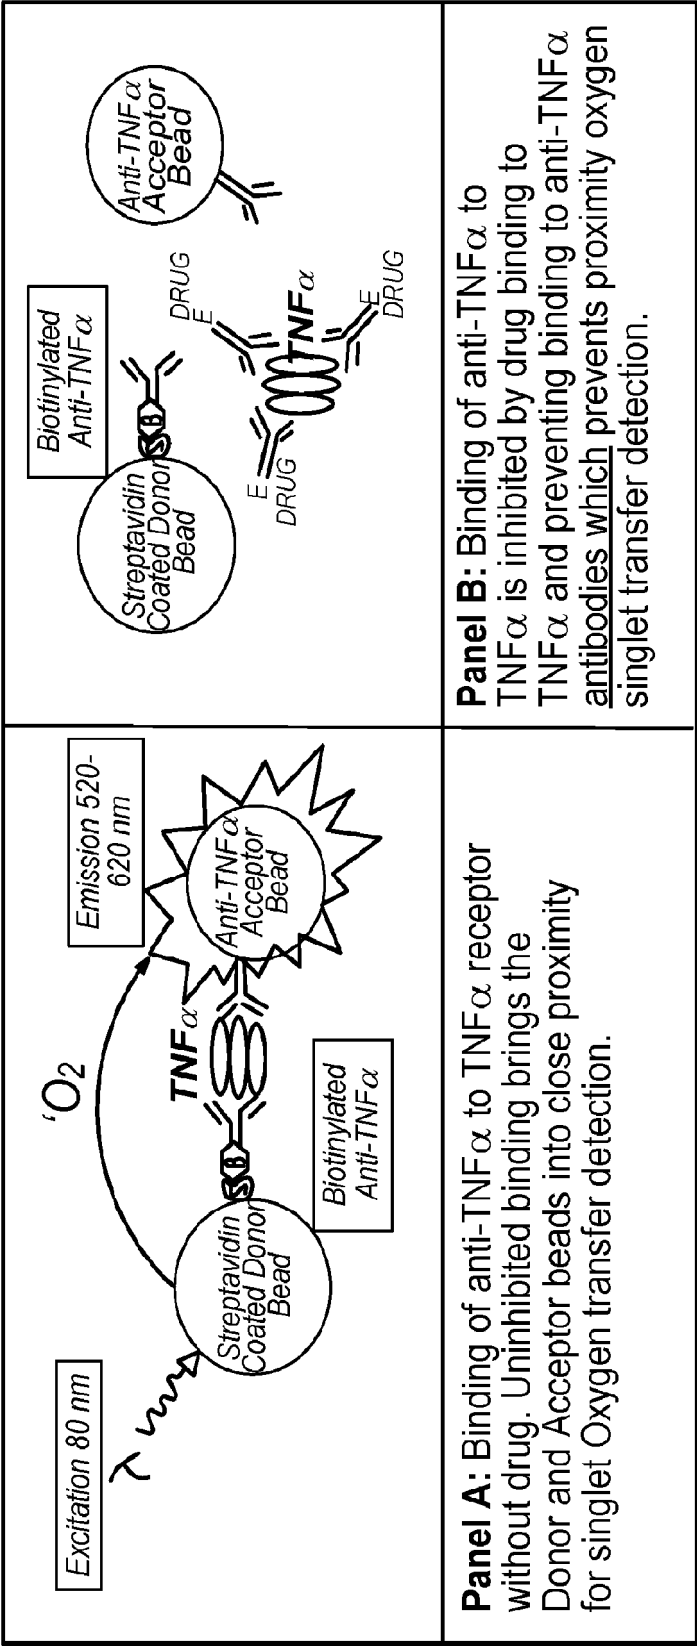


FIG. 68

Dose response curves Exemptia binding to TNFa (10,000 pg) of Exemptia dispensed from standard injector, Si bellows or PVC bellows.
Error bars = standard deviation. Saline control n-1.

4 hour exposure

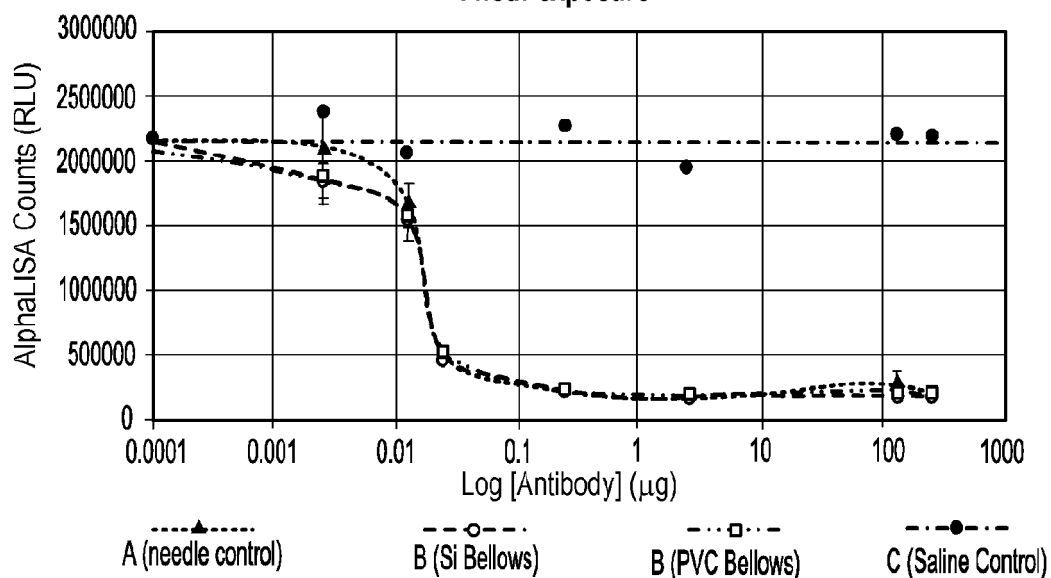


FIG. 69

Dose response curves Exemptia binding to TNFa (10,000 pg) of Exemptia dispensed from standard injector, Si bellows or PVC bellows.
Error bars = standard deviation. Saline control n-1.

24 hour exposure

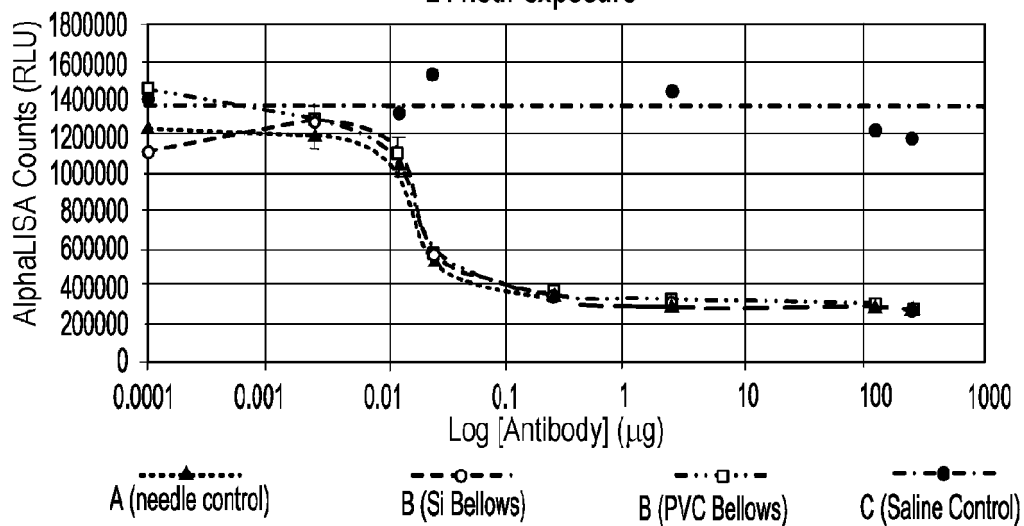


FIG. 70

Dose response curves Exemptia binding to TNFa (10,000 pg) of Exemptia dispensed from standard injector, Si bellows or PVC bellows.

Error bars = standard deviation. Saline control n-1.

336 hour exposure

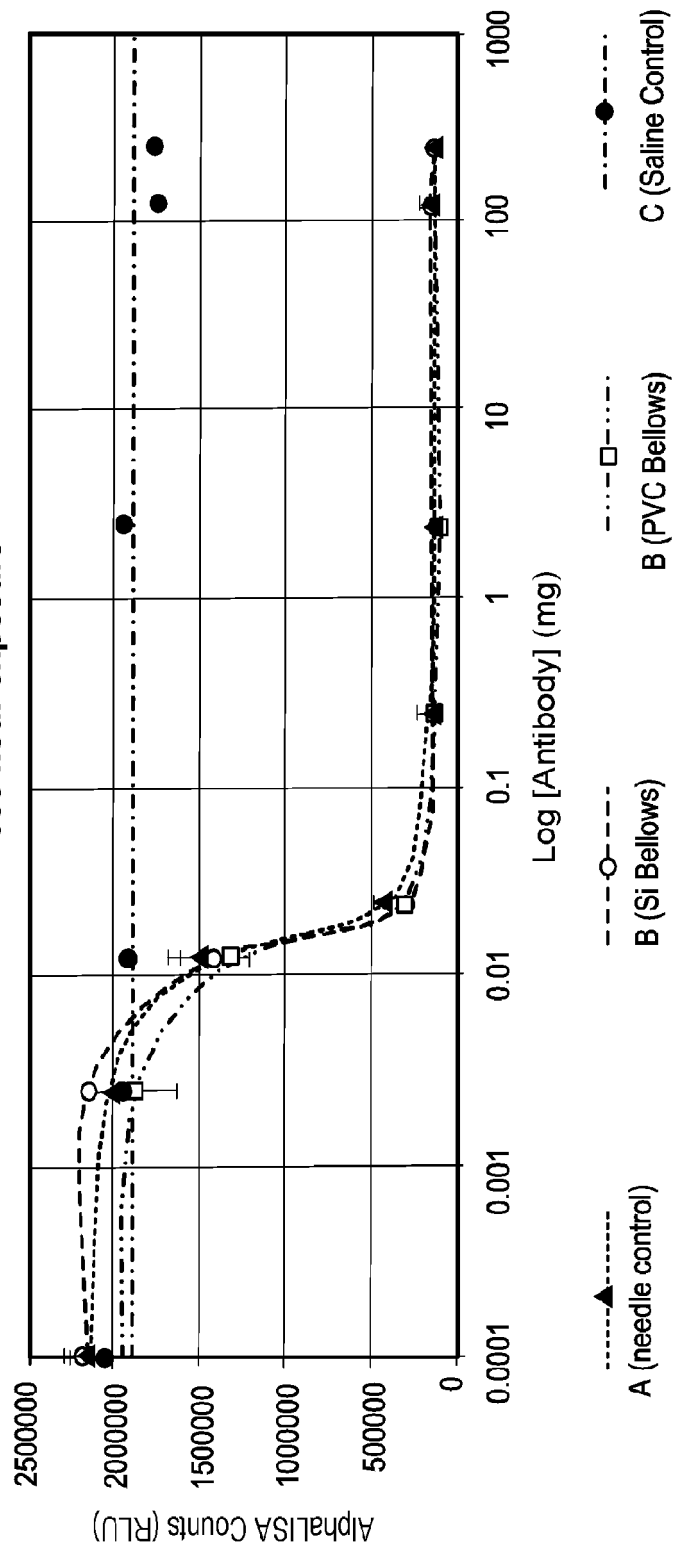


FIG. 71

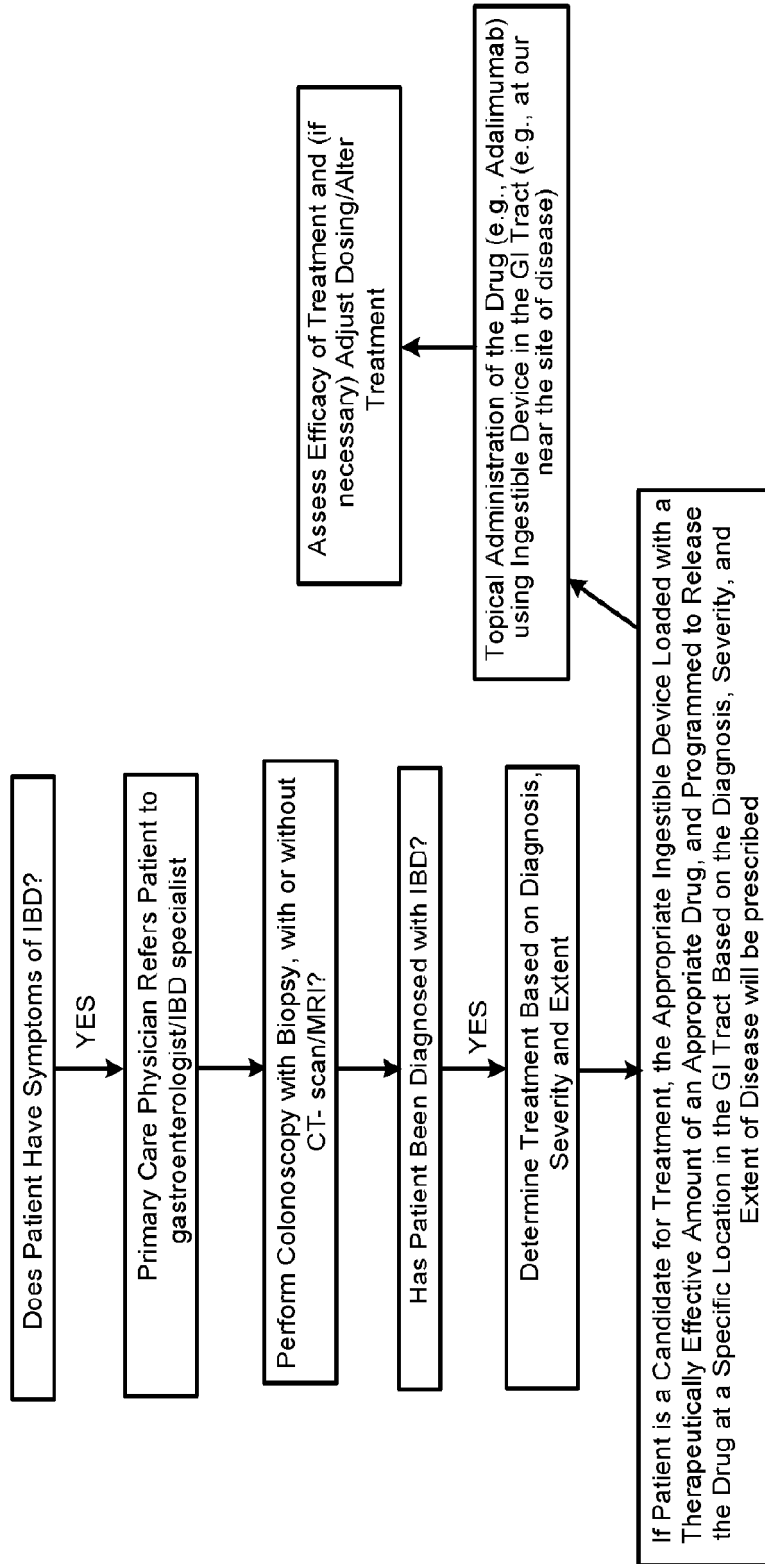


FIG. 72

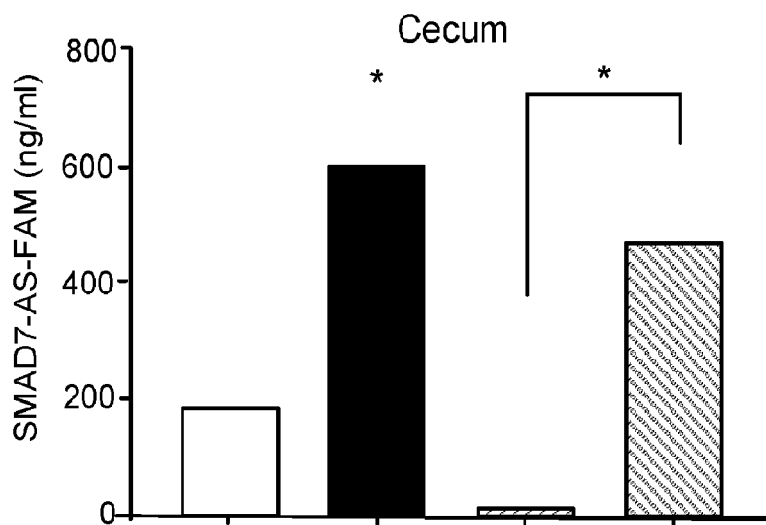


FIG. 73

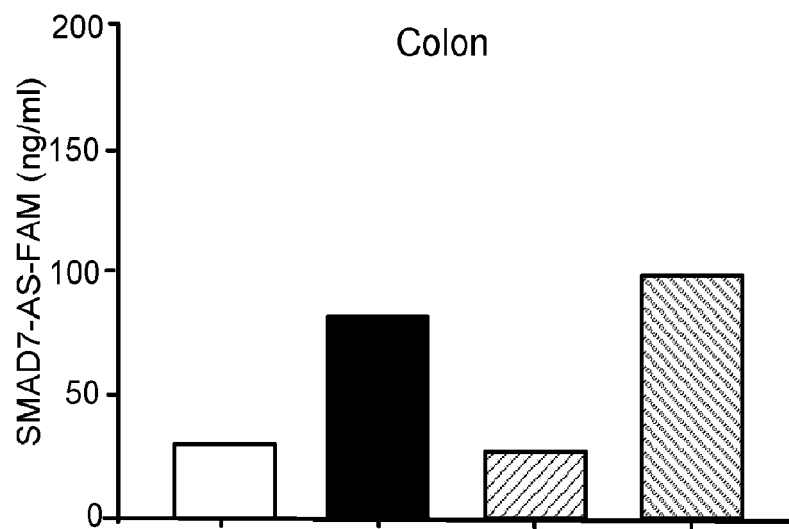


FIG. 74

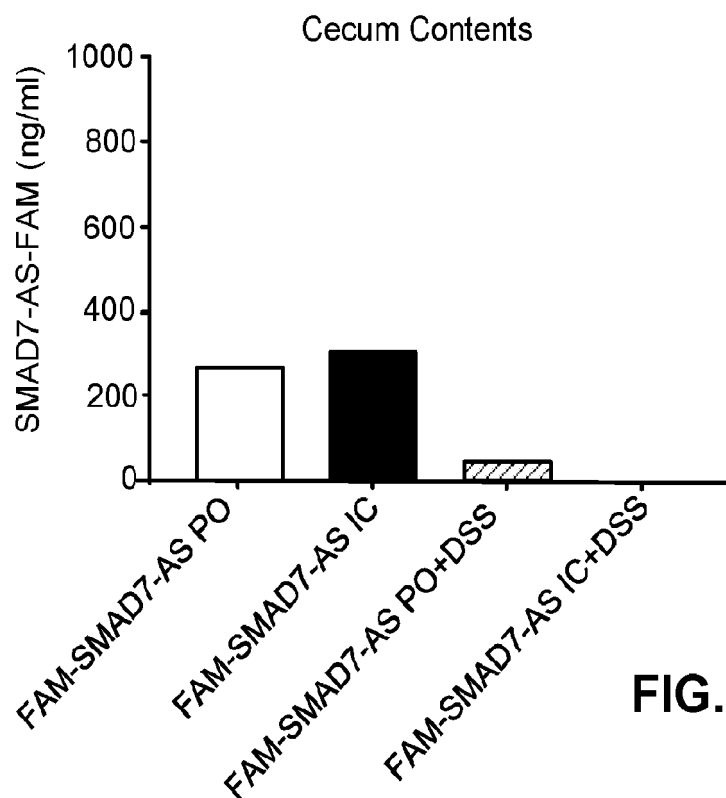


FIG. 75

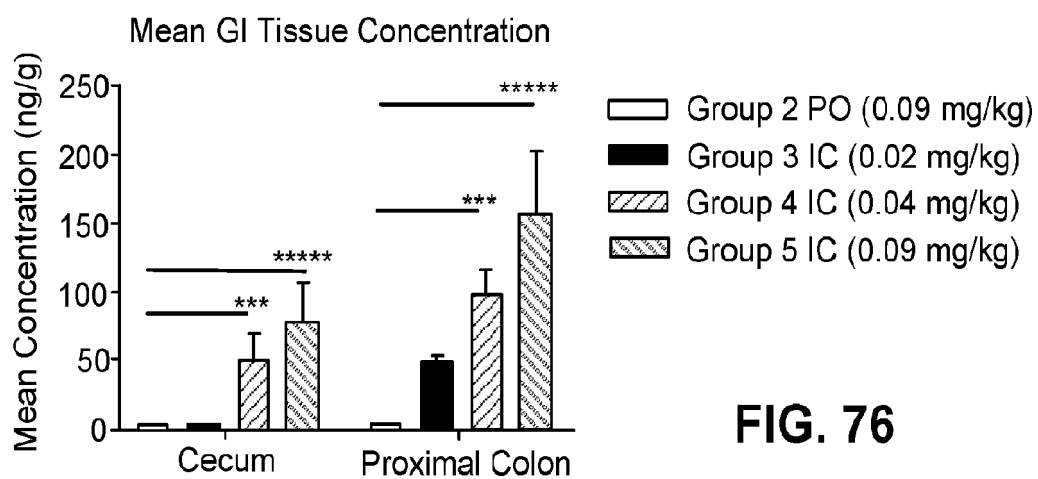


FIG. 76

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- US 62434374 [0001]
- US 62478919 B [0001]
- US 62545380 B [0001]
- US 62583832 B [0001]
- WO 2016049602 A [0003] [0185]
- WO 2004066903 A [0003]
- US 20050260186 A [0058]
- US 20060104968 A [0058]
- US 6267958 B [0058]
- US 6171586 B [0058]
- WO 2006044908 A [0058]
- US 3773919 A [0064]
- US 4522811 A [0065]
- US 4816567 A [0086]
- US 4987071 A [0124]
- US 5116742 A [0124]
- WO 8809810 A [0129]
- US 6506559 B [0130]
- US 20030056235 A1 [0130]
- WO 11004395 A [0139]
- US 20160090598 A [0139]
- US 9296725 B [0154]
- US 9309240 B [0154]
- US 20130231340 A [0154]
- US 20160251376 A [0154]
- US 20130143915 A [0154]
- US 2014062145 W [0159]
- WO 2013120184 A [0181]
- US 20180070857 A1 [0181] [0234]
- CN 104473611 [0251]
- US 8615284 B2 [0258]
- WO 08024188 A [0308]
- WO 07024715 A [0308]
- US 5759808 A [0308]
- WO 9627011 A [0310]
- US 4676980 A [0310]
- WO 15103072 A [0310]
- US 4665077 A [0319]
- US 4120649 A [0319]
- WO 9008187 A [0319]
- US 5114721 A, Cohen [0319]
- WO 9011294 A [0319]
- WO 9101133 A [0319]
- EP 340109 A [0319]

Non-patent literature cited in the description

- **JOSTINS et al.** Host-microbe interactions have shaped the genetic architecture of inflammatory bowel disease. *Nature*, 2012, vol. 491, 119-124 [0003]
- **O'SHEA ; PLENGE.** JAK and STAT signaling molecules in immunoregulation and immune-mediated disease. *Immunity*, 2012, vol. 36, 542-550 [0003]
- **SANDBORN et al.** Tofacitinib, an Oral Janus Kinase Inhibitor, in Active Ulcerative Colitis. *New England J. Med*, 2012, vol. 367, 616-24 [0003]
- **PANES et al.** Randomized trial of tofacitinib in active ulcerative colitis: analysis of efficacy base on patient-reported outcomes. *BMC Gastroenterology*, 2015, vol. 15, 14 [0003]
- *J. Drug Delivery & Ther.*, 2012, vol. 2 (3), 1-8 [0003]
- *Intl. J. Pharm. Ind.*, vol. 6 (3), 72-74 [0003]
- *Gastrointest. Endosc.*, vol. 78 (3), 520-528 [0003]
- Remington's Pharmaceutical Sciences. 1980 [0058] [0064]
- **PEPPAS et al.** *Biomaterials*, 1996, vol. 17 (16), 1553-1561 [0059]
- **KHARENKO et al.** *Pharmaceutical Chemistry J.*, 2009, vol. 43 (4), 200-208 [0059]
- **SALAMAT-MILLER et al.** *Adv. Drug Deliv. Reviews*, 2005, vol. 57 (11), 1666-1691 [0059]
- **BERNKOP-SCHNURCH.** *Adv. Drug Deliv. Rev.*, 2005, vol. 57 (11), 1569-1582 [0059]
- **HARDING et al.** *Biotechnol. Genet. Eng. News*, 1999, vol. 16 (1), 41-86 [0059]
- **SCHNITZLER et al.** *Gut*, 2009, vol. 58, 492-500 [0071]
- **CHANG et al.** *Nat Clin Pract Gastroenterol Hepatology*, 2006, vol. 3, 220 [0071]
- **HOENTJEN et al.** *World J. Gastroenterol.*, 2009, vol. 15 (17), 2067 [0071]
- **HANAUER et al.** *Lancet*, 2002, vol. 359, 1541-49 [0071]
- **SANDBORN et al.** *N Engl J Med*, 2005, vol. 353, 1912-25 [0071]
- **BEST WR et al.** *Gastroenterology*, 1979, vol. 77, 843-6 [0074]
- **SANDLER et al.** *J. Clin. Epidemiol*, 1988, vol. 41, 451-8 [0075]
- **THIA et al.** *Inflamm Bowel Dis*, 2011, vol. 17, 105-11 [0075]

- **KORZENIK et al.** *N Engl J Med.*, 2005, vol. 352, 2193-201 [0075]
- **SANDBORN WJ et al.** *N Engl J Med*, 2005, vol. 353, 1912-25 [0075]
- **SANDBORN WJ et al.** *Ann Intern*, 30 April 2007, vol. 19 (146), 829-38 [0075]
- **KIM et al.** *Gastroenterology*, 2014, vol. 146 (5), S-368 [0075]
- **KHANNA et al.** *Aliment Pharmacol. Ther.*, 2015, vol. 41, 77-86 [0075]
- **GASINK C et al.** *ACG Annual Meeting*, 2014 [0075]
- **KHANNA R et al.** *Inflamm Bowel Dis*, 2014, vol. 20, 1850-61 [0075]
- **MARY et al.** *Gut*, 1989, vol. 39, 983-9 [0076]
- **DAPERNO et al.** *Gastrointest. Endosc.*, 2004, vol. 60 (4), 505-12 [0076]
- **LICHTENSTEIN GR et al.** *Am J Gastroenterol*, 2009, vol. 104, 465-83 [0077]
- **VAN ASSCHE G et al.** *J Crohns Colitis*, 2010, vol. 4, 63-101 [0077]
- **TRUELOVE S. C. ; WITTS, L.J.** *Br Med J.*, 1955, vol. 2, 1041-1048 [0078]
- **LENNARD-JONES JE.** *Scand J Gastroenterol Suppl*, 1989, vol. 170, 2-6 [0078]
- **WALMSLEY.** *Gut.*, 1998, vol. 43, 29-32 [0078]
- **CHOUNG, R. S. et al.** Serologic microbial associated markers can predict Crohn's disease behaviour years before disease diagnosis. *Alimentary pharmacology & therapeutics*, 2016, vol. 43 (12), 1300-1310 [0080]
- **MORRISON et al.** *Proc. Natl. Acad. Sci. USA*, 1984, vol. 81, 6851-6855 [0086]
- **GAULTIER et al.** *Nucleic Acids Res.*, 1987, vol. 15, 6625-6641 [0123]
- **INOUE et al.** *Nucleic Acids Res.*, 1987, vol. 15, 6131-6148 [0123]
- **INOUE et al.** *FEBS Lett.*, 1987, vol. 215, 327-330 [0123]
- **HASELHOFF ; GERLACH.** *Nature*, 1988, vol. 334, 585-591 [0124]
- **BARTEL et al.** *Science*, 1993, vol. 261, 1411-1418 [0124]
- **HELENE.** *Anticancer Drug Des.*, 1991, vol. 6 (6), 569-84 [0125]
- **HELENE.** *Ann. N.Y. Acad. Sci.*, 1992, vol. 660, 27-36 [0125]
- **MAHER.** *Bioassays*, 1992, vol. 14 (12), 807-15 [0125]
- **HYRUP et al.** *Bioorganic Medicinal Chem.*, 1996, vol. 4 (1), 5-23 [0126]
- **PERRY-O'KEEFE et al.** *Proc. Natl. Acad. Sci. U.S.A.*, 1996, vol. 93, 14670-675 [0126]
- **FINN et al.** *Nucleic Acids Res.*, 1996, vol. 24, 3357-63 [0128]
- **MAG et al.** *Nucleic Acids Res.*, 1989, vol. 17, 5973-88 [0128]
- **PETERSER et al.** *Bioorganic Med. Chem. Lett.*, 1975, vol. 5, 1119-11124 [0128]
- **LETSINGER et al.** *Proc. Natl. Acad. Sci. U.S.A.*, 1989, vol. 86, 6553-6556 [0129]
- **LEMAITRE et al.** *Proc. Natl. Acad. Sci. U.S.A.*, 1989, vol. 84, 648-652 [0129]
- **KROL et al.** *Bio/Techniques*, 1988, vol. 6, 958-976 [0129]
- **ZON.** *Pharm. Res.*, 1988, vol. 5, 539-549 [0129]
- **SHARP et al.** *Genes Dev.*, 2001, vol. 15, 485-490 [0130]
- **HAMMOND et al.** *Nature Rev. Gen.*, 2001, vol. 2, 110-119 [0130]
- **PADDISON et al.** *Proc. Natl. Acad. Sci. U.S.A.*, 2002, vol. 99, 1443-1448 [0130]
- **CAPLEN.** *Trends Biotech.*, 2002, vol. 20, 49-51 [0130]
- **COOK et al.** *Blood*, 2014, vol. 123, 2826-2837 [0133]
- **KOPPIKAR et al.** *Nature*, 2012, vol. 489 (7414), 155-159 [0133]
- **PATIL et al.** *Pharmaceutical Nanotechnol.*, 2009, vol. 367, 195-203 [0138]
- **YANG et al.** *ACS Appl. Mater. Interfaces*, 2017 [0138]
- **PEREPELYUK et al.** *Mol. Ther. Nucleic Acids*, 2017, vol. 6, 259-268 [0138]
- **ANDERSEN et al.** *Methods Mol. Biol.*, 2009, vol. 555, 77-86 [0138]
- **BUYENS et al.** *J. Control Release*, 2012, vol. 158 (3), 362-370 [0139]
- **SCARABEL et al.** *Expert Opin. Drug Deliv.*, 2017, vol. 17, 1-14 [0139]
- **TANGSANGASAKSRI et al.** *BioMacromolecules*, 2016, vol. 17, 246-255 [0139]
- **WU et al.** *Nanotechnology*, 2017 [0139]
- **SAHAY et al.** *Nature Biotechnol.*, 2013, vol. 31, 653-658 [0139]
- **LIN et al.** *Nanomedicine*, 2014, vol. 9 (1), 105-120 [0139]
- **LI et al.** *Biochem. Pharmacol.*, 2013, vol. 86 (10), 1411-8 [0150]
- **HARRISON et al.** *N Engl. J Med*, 2012, vol. 366, 787-798 [0150]
- **PIERI et al.** *Am. J Hematol.*, 2017, vol. 92 (2), 187-195 [0150]
- **MACKAY-WIGGAN et al.** *JCI Insight*, 2016, vol. 1 (15), e89790 [0150]
- **RUDOLPH et al.** *Leukemia*, 2016, vol. 30 (10), 2119-2123 [0150]
- **FURQAN et al.** *Biomark Res.*, 2013, vol. 1 (1), 5 [0150]
- **GRAS.** *Drugs Today (Bare)*, 2016, vol. 52 (10), 543-550 [0150]
- **SMOLEN et al.** *Ann. Rheum. Dis.*, 2016, vol. 76 (4), 694-700 [0150]
- **KUBO et al.** *Expert. Rev. Clin. Immunol.*, 2016, vol. 12 (9), 911-919 [0150]
- **FRIDMAN et al.** *J Immunol.*, 2010, vol. 84 (9), 5298-5307 [0150]

- GUSCHIN et al. *EMBO J*, 1995, vol. 14, 1421-1429 [0150]
- IOANNIDIS et al. *J Med Chem.*, 2011, vol. 54, 262-276 [0150]
- MOISAN et al. *Nat. Cell Biol.*, 2015, vol. 17 (1), 57-67 [0150]
- QIN et al. *J Neurosci.*, 2016, vol. 36 (18), 5144-5149 [0150]
- JIANG et al. *Biochem. Biophys. Res. Commun.*, 2015, vol. 458 (4), 908-912 [0150]
- VERSTOVSEK et al. *Leuk. Res.*, 2015, vol. 39 (2), 157-163 [0150]
- PLIMACK et al. *Oncologist*, 2013, vol. 18 (7), 819-820 [0150]
- YAN et al. *Oncotarget*, 2013, vol. 4 (3), 433-445 [0150]
- VERMEIRE et al. *Lancet*, 2017, vol. 389 (10066), 266-275 [0150]
- MENET et al. *J Med Chem.*, 2014, vol. 57 (22), 9323-9342 [0150]
- VAN ROMPAEY et al. *J Immunol.*, 2013, vol. 191 (7), 3568-3577 [0150]
- NAMOUR et al. *Clin. Pharmacokinet.*, 2015, vol. 54 (8), 859-874 [0150]
- PARDANANI et al. *Leukemia*, 2009, vol. 23, 1441-1445 [0150]
- GUPTA et al. *Haematologica*, 2017, vol. 102 (1), 94-102 [0150]
- HU et al. *Mol. Pharm.*, 2016, vol. 13 (2), 689-697 [0150]
- ABUBAKER et al. *BMC Cancer*, 2014, vol. 14, 317 [0150]
- DURMUS et al. *Pharmacol. Res.*, 2013, vol. 76, 9-16 [0150]
- PARDANANI et al. *Leukemia*, 2013, vol. 27 (6), 1322-1327 [0150]
- MONAGHAN et al. *Leukemia*, 2011, vol. 25 (12), 1891-1899 [0150]
- TYNER et al. *Blood*, 2010, vol. 115 (25), 5232-5240 [0150]
- KAHL et al. *Lupus*, 2016, vol. 25 (13), 1420-1430 [0151]
- LUDBROOK et al. *Er. J Dermatol.*, 2016, vol. 174 (5), 985-995 [0151]
- VAN Vollenhoven et al. *Lupus*, 2015, vol. 24 (6), 648-649 [0151]
- GONZALES et al. *J Vet. Pharmacol. Ther.*, 2014, vol. 37 (4), 317-324 [0151]
- COLLARD et al. *J Vet. Pharmacol. Ther.*, 2014, vol. 37 (3), 279-285 [0151]
- COSGROVE et al. *Vet. Dermatol.*, 2013, vol. 24 (6), 587-597 [0151]
- KREMER et al. *Arthritis Rheumatol.*, 2016, vol. 68 (12), 2867-2877 [0151]
- MOHAMED et al. *Clin. Pharmacol.*, 2016, vol. 55 (12), 1547-1558 [0151]
- O'SHEA et al. *Ann. Rev. Med.*, 2015, vol. 66 (1), 311-28 [0151]
- SCHWARTZ et al. *Nat. Rev. Rheum.*, 2016, vol. 12, 25-36 [0151]
- MASCARENHAS et al. *Haematologica*, 2017, vol. 102 (2), 327-335 [0151] [0152]
- BISSONNETTE et al. *J Dermatolog. Treat.*, 2016, vol. 27 (4), 332-338 [0151]
- ROSENTHAL et al. *Exp. Opin. Pharmacother.*, 2014, vol. 15 (9), 1265-1276 [0151]
- GADINA et al. *Curr. Opin. Rheumatol.*, 2014, vol. 26 (2), 237-243 [0151]
- DEGRYSET et al. *J Hematol. Oncol.*, 2015, vol. 8, 91 [0151]
- WORKS et al. *J Immunol.*, 2014, vol. 193 (7), 3278-3287 [0151] [0154]
- DUGAN et al. *J Med Chem.*, 2012, vol. 55 (11), 5243-5254 [0152]
- SEAVEY et al. *Mol. Cancer Ther.*, 2012, vol. 11 (4), 984-993 [0152]
- STUMP et al. *Arthritis Res. Ther.*, 2011, vol. 13 (2), R68 [0152]
- PARDANANI et al. *J Clin. Oncol.*, 2011, vol. 29, 789-796 [0152]
- JAMIESON et al. *J Transl. Med.*, 2015, vol. 13, 294 [0152]
- ZHANG et al. *Oncotarget*, 2015, vol. 6 (16), 14329-14343 [0152]
- WEMIG et al. *Blood*, 2008, vol. 105, 4508-4515 [0152]
- HEXNET et al. *Blood*, 2008, vol. 111, 5663-5671 [0152]
- SANTOS et al. *Blood*, 2010, vol. 115, 1131-1136 [0152]
- SMITH et al. *Blood*, 2004, vol. 103, 3669-3676 [0152]
- HEXNER et al. *Leuk. Lymphoma.*, 2015, vol. 56 (9), 2543 [0152]
- GEYER et al. *Hematology*, 2012, vol. 117, S129-132 [0152]
- DIAZ et al. *PLoS One*, 2011, vol. 6 (4), e18856 [0152]
- MINTURN et al. *Cancer Chemother. Pharmacol.*, 2011, vol. 68 (4), 1057-1065 [0152]
- O'SHEA et al. *Immunity*, 2012, vol. 36 (4), 542-550 [0152]
- PATTERSON et al. *Clin. Exp. Immunol.*, 2014, vol. 176, 1-10 [0152]
- DEEG et al. *J Clin. Oncol.*, 2011, vol. 29 [0152]
- VERSTOVSEK et al. *J Hematol. Oncol.*, 2016, vol. 9 (1), 137 [0152]
- CHOW et al. *Onco Targets. Ther.*, 2016, vol. 9, 2655-2665 [0152]
- KOMROKJI et al. *Blood*, 2015, vol. 125 (17), 2649-2655 [0152]
- JAYARAMAN et al. *Drug Metab. Lett.*, 2015, vol. 9 (1), 28-47 [0152]
- MACE et al. *Oncotarget*, 2015, vol. 6 (42), 44509-44522 [0152]
- WAN et al. *ACS Med Chem. Lett.*, 2015, vol. 6 (8), 850-855 [0152]

- **PURANDARE et al.** *Leukemia*, 2012, vol. 26 (2), 280-288 [0152]
- **VERSTOVSEK et al.** *Leuk. Res.*, 2014, vol. 38 (3), 316-322 [0152]
- **FORSYTH et al.** *Bioorg. Med Chem. Lett.*, 2012, vol. 22 (24), 7653-7658 [0152]
- **BISSONNETTE et al.** *J Dermatol. Treat.*, 2016, vol. 27 (4), 332-338 [0152]
- **MA et al.** *Blood Cancer J*, 2013, vol. 3, e109 [0152]
- **VERSTOVSEK et al.** *Blood*, 2013, vol. 122, 665 [0152]
- **MITCHELL et al.** *Org. Process Res. Dev.*, 2012, vol. 16 (1), 70-81 [0152]
- **SHIDE et al.** *Blood*, 2011, vol. 117 (25), 6866-6875 [0152]
- **SAYYAH et al.** *Mol. Cancer. Ther.*, 2008, vol. 7 (8), 2308-2318 [0152]
- **ELWOOD et al.** *J Pharmacol. Exp. Ther.*, 2017 [0153]
- **GENOVESE et al.** *Ann Rheum Dis.*, 2016, vol. 75 (11), 1979-1983 [0153]
- **GADINA et al.** *Arthritis Rheumatol.*, 2016, vol. 68 (1), 31-34 [0153]
- **FARMER et al.** *J Med Chem.*, 2015, vol. 58 (18), 7195-7216 [0153]
- **FLEISCHMANN et al.** *Arthritis Rheumatol.*, 2015, vol. 67 (2), 334-343 [0153]
- **MAHAJAN et al.** *J Pharmacol.*, 2015, vol. 353 (2), 405-414 [0153]
- **VELOTTA et al.** *Transplantation*, 2009, vol. 87 (5), 653-659 [0153]
- **DEUSE et al.** *Transplantation*, 2008, vol. 85 (6), 885-892 [0153]
- **ASHINO et al.** *J Allergy Clin. Immunol.*, 2014, vol. 133 (4), 1162-1174 [0153]
- **NORMAN.** *Exp. Opin. Investig. Drugs*, 2014, vol. 23 (8), 1067-1077 [0153]
- **KOPPIKAR et al.** *Blood*, 2010, vol. 115 (4), 2919-2927 [0153]
- **LI et al.** *Neoplasia*, 2010, vol. 12 (1), 28-38 [0153]
- **RINGEL et al.** *Acta Haematol.*, 2014, vol. 132 (1), 75-86 [0153]
- **BAFFERT et al.** *Mol. Cancer. Ther.*, 2010, vol. 9 (7), 1945-1955 [0153]
- **GENOVESE et al.** *Arthritis Rheumatol.*, 2017 [0153]
- **ITO et al.** *J Pharmacol. Sci.*, 2017, vol. 133 (1), 25-33 [0153] [0161]
- **CAO et al.** *Clin. Pharmacol. Drug Dev.*, 2016, vol. 5 (6), 435-449 [0153]
- **TAKEUCHI et al.** *Ann. Rheum. Dis.*, 2016, vol. 75 (6), 1057-1064 [0153] [0161]
- **GHORESCHI et al.** *J Immunol.*, 2011, vol. 186 (7), 4234-4243 [0153]
- **YOSHIDA et al.** *Biochem. Biophys. Res. Commun.*, 2012, vol. 418 (2), 234-240 [0153]
- **CALAMA et al.** *Pulm. Pharmacol. Ther.*, 2017 [0153]
- **CUTOLO et al.** *J Inflamm. Res.*, 2013, vol. 6, 129-137 [0153]
- **OI et al.** *Int. J. Oneal.*, 2016, vol. 49 (6), 2275-2284 [0153]
- **QI et al.** *Am. J. Chin. Med.*, 2015, vol. 43 (2), 337-347 [0153]
- **SEO et al.** *Food Chem. Toxicol.*, 2014, vol. 64, 217-224 [0153]
- **WU et al.** *Cancer Cell*, 2015, vol. 28 (1), 29-41 [0153]
- **MEYER et al.** *Cancer Cell*, 2015, vol. 28 (1), 15-28 [0153]
- **MASSE et al.** *J Immunol.*, 2015, vol. 194 (1), 67 [0154]
- **MENET.** *Pharm. Pat. Anal.*, 2014, vol. 3 (4), 449-466 [0154]
- **LIANG et al.** *Euro. J Med Chem.*, 2013, vol. 67, 175-187 [0154]
- **JANG et al.** *Bioorg. Med Chem. Lett.*, 2015, vol. 25 (18), 3947-3952 [0154]
- **AKAHANE et al.** *Blood*, 2016, vol. 128, 1596 [0154]
- **GILLOOLY et al.** *2016ACRIARHP Annual Meeting*, 2016 [0154]
- **ISHIZAKI et al.** *Int. Immunol.*, 2014, vol. 26 (5), 257-267 [0154]
- **FUROMOTO et al.** *BioDrugs*, 2013, vol. 27 (5), 431-438 [0155]
- **O' SHEA et al.** *Ann. Rheum. Dis.*, 2013, vol. 72 (2), ii 111-ii-115 [0155]
- **SONBOL et al.** *Ther. Adv. Hematol.*, 2013, vol. 4 (1), 15-35 [0155]
- **TANAKA et al.** *J Biochem.*, 2015, vol. 158 (3), 173-179 [0155]
- **KIM et al.** *J Med Chem.*, 2015, vol. 58 (18), 7596-5602 [0156] [0158] [0160]
- **YOKOYAMA et al.** *J Clin. Immunol.*, 2013, vol. 33 (3), 586-594 [0157]
- **THOMA et al.** *J Med Chem.*, 2011, vol. 54 (1), 284-288 [0157]
- **COFFEY et al.** *J Pharmacol. Exp. Ther.*, 2014, vol. 351 (3), 538-548 [0157]
- **MA et al.** *Oncotarget*, 2015, vol. 6 (41), 43881-43896 [0157]
- **NAKAGAWA et al.** *J Immunol.*, 2011, vol. 187 (9), 4611-4620 [0157]
- **PEDRANZINI et al.** *Cancer Res.*, 2006, vol. 66 (19), 9714-9721 [0157]
- **JONES et al.** Design and Synthesis of a Pan-Janus Kinase Inhibitor Clinical Candidate (PF-06263276) Suitable for Inhaled and Topical Delivery for the Treatment of Inflammatory Diseases of the Lungs and Skin. *J. Med. Chem.*, 2017, vol. 60 (2), 767-786 [0157]
- **CHEMICAL ABSTRACTS**, 457081-03-07 [0157]
- **WANG et al.** *Antimicrob. Agents Chemother.*, 2016, vol. 60 (5), 2834-48 [0157]
- **BORDONARO et al.** *PLoS One*, 2014, vol. 9, e115068 [0157]
- **OSORIO et al.** *PLoS Pathogens*, 2014, vol. 10 (6), e1004165 [0157]
- **HSU ; ARMSTRONG.** *J Immunol. Res.*, 2014 [0157]

- **KIM et al.** *J Med Chem.*, 2015, vol. 58 (18), 7596-5602 [0159]
- **BROWN et al.** *Bioorg. Med Chem. Lett.*, 2000, vol. 10 (6), 575-579 [0161]
- **LAI et al.** *Chem. Biol.*, 2008, vol. 15 (9), 969-978 [0161]
- **CAO et al.** *Clin. Pharmacol. Drug Dev.*, 2016, vol. 5 (6), 435-449 [0161]
- **PAPP et al.** *Er. J Dermatol.*, 2015, vol. 173 (3), 767-776 [0161]
- **FOSTER, MARTYN et al.** The Pharmacological Profile of TOP1288, a Narrow Spectrum Kinase Inhibitor (NSKI) in Clinical Development as an AntiInflammatory Treatment for Ulcerative Colitis. *Gastroenterology*, vol. 152 (5), S766 [0164]
- **BASAR et al.** Ingestible Wireless Capsule Technology: A Review of Development and Future Indication. *International Journal of Antennas and Propagation*, 2012, 1-14 [0251]
- **TENG, RENLI ; JUAN MAYA.** Absolute bioavailability and regional absorption of ticagrelor in healthy volunteers. *Journal of Drug Assessment*, 2014, vol. 3 (1), 43-50 [0277]
- **T. D. THAN et al.** A review of localization systems for robotic endoscopic capsules. *IEEE Trans. Biomed. Eng.*, September 2012, vol. 59 (9), 2387-2399 [0277]
- **SOKOLOWSKA-WEDZINA et al.** *Mol. Cancer Res.*, 2017, vol. 15 (8), 1040-1050 [0308]
- **LI et al.** *Immunol. Lett.*, 2017, vol. 188, 89-95 [0308]
- **HASLER et al.** *Mol. Immunol.*, 2016, vol. 75, 28-37 [0308]
- **KIM et al.** *PLoS One*, 2014, vol. 10 (1), e113442 [0308]
- **WU et al.** *Nat. Biotechnol.*, 2007, vol. 25 (11), 1290-1297 [0308]
- **TSAI et al.** *Mol. Ther. Oncolytics*, 2016, vol. 3, 15024 [0308]
- **CHELIUS et al.** *MAbs*, 2010, vol. 2 (3), 309-319 [0308]
- **KONTERMANN et al.** *Drug Discovery Today*, 2015, vol. 20 (7), 838-847 [0308]
- **REGULA et al.** *EMBO Mol. Med.*, 2017, vol. 9 (7), 985 [0308]
- **CHEAL et al.** *Mol. Cancer Ther.*, 2014, vol. 13 (7), 1803-1812 [0308]
- **NATSUME et al.** *J. Biochem.*, 2006, vol. 140 (3), 359-368 [0308]
- **STIJLEMANS et al.** *J. Biol. Chem.*, 2004, vol. 279, 1256-1261 [0308]
- **DUMOULIN et al.** *Nature*, 2003, vol. 424, 783-788 [0308]
- **PLESCHBERGER et al.** *Bioconjugate Chem.*, 2003, vol. 14, 440-448 [0308]
- **POLJAK.** *Structure*, 1994, vol. 2 (12), 1121-1123 [0308]
- **HUDSON et al.** *J. Immunol. Methods*, 1999, vol. 23 (1-2), 177-189 [0308]
- **REUSCH et al.** *mAbs*, 2014, vol. 6 (3), 727-738 [0308]
- **CUESTA et al.** *Trends in Biotechnol.*, 2010, vol. 28 (7), 355-362 [0308]
- **SANZ et al.** *Trends in Immunol.*, 2004, vol. 25 (2), 85-91 [0308]
- **HUSTON et al.** *Human Antibodies*, 2001, vol. 10 (3-4), 127-142 [0308]
- **WHEELER et al.** *Mol. Ther.*, 2003, vol. 8 (3), 355-366 [0308]
- **STOCKS.** *DrugDiscov. Today*, 2004, vol. 9 (22), 960-966 [0308]
- **MILSTEIN ; CUELLO.** *Nature*, 1983, vol. 305, 537-539 [0310]
- **SURESH et al.** *Methods in Enzymology*, 1986, vol. 121, 210 [0310]
- **BRENNAN et al.** *Science*, 1985, vol. 229, 81 [0310]
- **SHALABY et al.** *J. Exp. Med.*, 1992, vol. 175, 217-225 [0310]
- **KOLSTELNY et al.** *J. Immunol.*, 1992, vol. 148 (5), 1547-1553 [0310]
- **HOLLINGER et al.** *Proc. Natl. Acad. Sci. U.S.A.*, 1993, vol. 90, 6444-6448 [0310]
- **GRUBER et al.** *J. Immunol.*, 1994, vol. 152, 5368 [0310]
- **TUTT et al.** *J. Immunol.*, 1991, vol. 147, 60 [0310]
- **SCHOONOOGHE et al.** *BMC Biotechnol.*, 2009, vol. 9, 70 [0310]
- **HOLT et al.** *Trends Biotechnol.*, 2003, vol. 21 (11), 484-490 [0310]
- **ZAPATA et al.** *Protein Eng.*, 1995, vol. 8 (10), 1057-1062 [0310]
- **SIMON GM ; NIPHAKIS MJ ; CRAVATT BF.** *Nature chemical biology*, 2013, vol. 9 (4), 200-205 [0317]
- **OFFNER et al.** *Science*, 1991, vol. 251, 430-432 [0319]
- **IANEWAY.** *Nature*, 1989, vol. 341, 482 [0319]
- **MACKAY ; MACKAY.** *Trends Immunol*, 2002, vol. 23, 113-5 [0319]
- **DURIE et al.** *Science*, 1993, vol. 261, 1328-30 [0319]
- **MOHAN et al.** *J. Immunol*, 1995, vol. 154, 1470-80 [0319]
- **FINCK et al.** *Science*, 1994, vol. 265, 1225-7 [0319]
- **VELAYUDHAN et al.** Demonstration of functional similarity of proposed biosimilar ABP501 to adalimumab. *BioDrugs*, 2016, vol. 30, 339-351 [0409]
- **BARBEAUET et al.** Application Note: Screening for inhibitors of TNF α /s TNFR1 Binding using AlphaScreen™ Technology. *PerkinElmer Technical Note ASC-016*, 2002 [0409]