



(12) **EUROPEAN PATENT APPLICATION**

(43) Date of publication:
09.12.2020 Bulletin 2020/50

(51) Int Cl.:
B65H 54/58 (2006.01) B65H 54/62 (2006.01)

(21) Application number: **19179055.9**

(22) Date of filing: **07.06.2019**

(84) Designated Contracting States:
**AL AT BE BG CH CY CZ DE DK EE ES FI FR GB
GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO
PL PT RO RS SE SI SK SM TR**
Designated Extension States:
BA ME
Designated Validation States:
KH MA MD TN

(72) Inventors:
• **Ibrahimovic, Hazret**
2074 Marin (CH)
• **Jacquot, Philippe**
25300 Pontarlier (FR)
• **Ritter, Roger**
2502 Bienne (CH)

(71) Applicant: **Mikron SA**
2017 Boudry (CH)

(74) Representative: **P&TS SA (AG, Ltd.)**
Avenue J.-J. Rousseau 4
P.O. Box 2848
2001 Neuchâtel (CH)

(54) **EQUIPMENT FOR WINDING MEDICAL TUBING**

(57) The present invention discloses an equipment for winding medical tubing, employing automated, sequentially-arranged workstations (1,5,7) capable of operating simultaneously, comprising one or more conveying units (2), one or more bending units (3) for arranging

medical tubing (10) in a U shape, one or more loading units (4), one or more winding stations (5) for winding medical tubing (10), one or more unloading units (6) and, optionally, one or more packaging units (7).

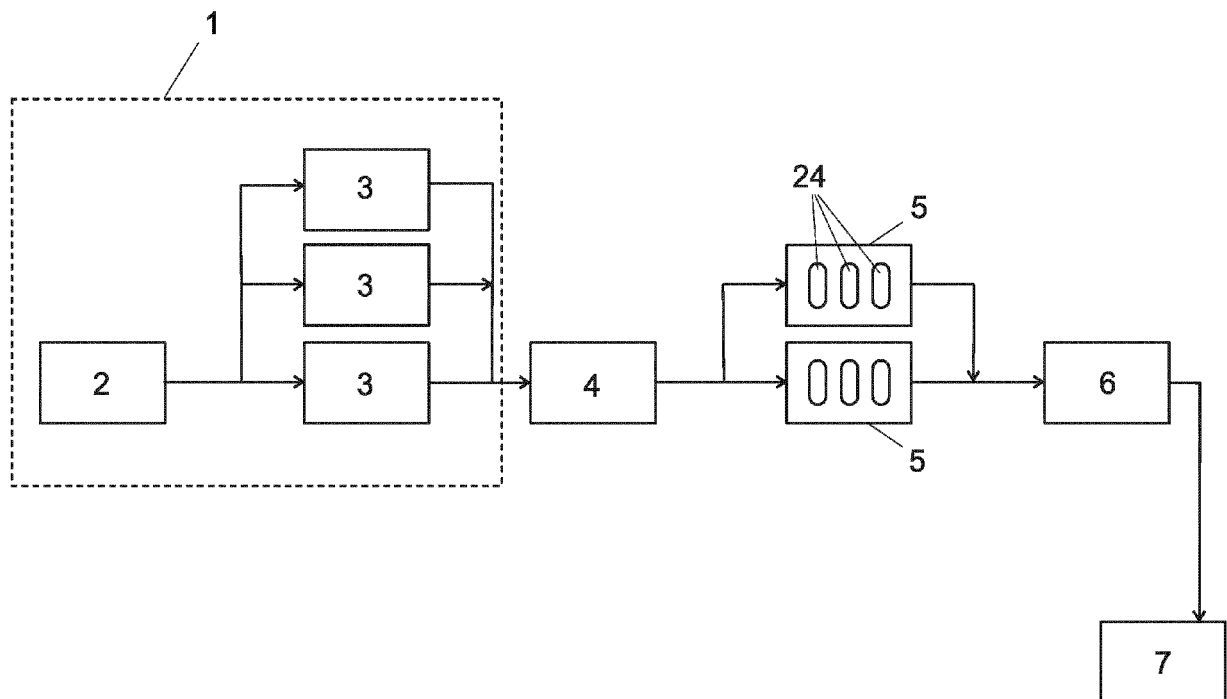


Fig. 1

Description

Technical Domain

[0001] The present invention discloses an equipment for winding medical tubing employing automated and sequentially-arranged workstations, which can be operated simultaneously.

State of the art

[0002] Flexible plastic tubing is produced for a variety of sectors, ranging from engineering (automotive, aerospace), agriculture, horticulture and water management, plumbing, hydraulics, oil and gas, as well as the medical and healthcare. The specifications of the tubing, such as dimensions, material and its chemical and physical properties, are adapted to its specific use, whereby a coiled or wound assembly of the tubing generally eases the packaging, transport, use and manipulation of the tubing. To this end, different types of coiling machines, mostly employing motorised rotating reels, have been developed for industrial tubing and are available on the market today.

[0003] Yet, for the medical sector large-scale automated winding of medical tubing remains an unmet need, with medical tubing still primarily being wound by hand. Apart from the limitations in processing speed and the increased risk of contamination which come with the manual handling of the tubing, inconsistencies in winding and waste of material due to mis-manipulation of the tubing are more likely to occur when compared to an automated process.

[0004] Many medical devices include plastic tubing for fluid or gas transfer. Such medical tubing must comply with international norms and display adequate quality requirements concerning its sterility, performance, ingredients, etc.

[0005] In its practical application medical tubing is handled by medically-trained professionals, but also by untrained patients. For both user groups a simple and safe manipulation of the medical tubing without the risk of causing damage or entanglement of the tubing, is adamant. In order to mitigate these risks, it is critical to provide the tubing in a suitably organised state, such as a wound or coiled state.

[0006] To this end, several solutions for winding medical tubing have been developed employing desk top equipment, by way of example: <http://www.medicalsyst-forindustry.com/custom%20tube%20coilers.html>. However, these solutions are extremely limited in their processing rate and are therefore primarily useful for individual laboratories, but not suited for large-scale industrial operations.

[0007] Document CN108313424 describes an automatic winding and bagging mechanism for a medical catheter. The automatic winding and bagging mechanism comprises a rack, a catheter winding mechanism

and a bagging grinding device, and the catheter winding mechanism and the bagging grinding device are sequentially arranged on the rack. The throughput of this mechanism is limited.

[0008] Document US2018008798 discloses a device for holding coils of medical tubing to simplify packaging and handling thus making it easier for patient to manipulate each coil of tubing and reducing the probability of entanglement. This solution is particularly suited to organise medical tubing conveying medical fluid in connection with dialysis machines, as it simplifies the handling of the tubing in a clinical or in a domestic setting. However, this method does not provide a solution for winding large volumes of medical tubing at industrial scale.

[0009] The advantage of providing medical tubing organised in a wound state is further emphasised in document US2013/0006226 describing a compact catheter assembly, whereby the wound state of the catheter enhances its safe use, thus preventing hygiene-related medical issues.

[0010] None of the approaches provided today provides a satisfactory solution for safe, industrial-scale winding of medical tubing at a high and adjustable processing rate.

Brief summary of the invention

[0011] One objective of the present invention is to provide an equipment for winding medical tubing which is adapted for industrial-scale manufacturing, thereby increasing efficiency of winding medical tubing.

[0012] Another objective is to propose an equipment for winding medical tubing which is capable of operating in a controlled environment, thereby reducing the risk of contamination.

[0013] According to one aspect, those objectives are achieved by providing an equipment for winding medical tubing, employing a plurality distinct operational units performing automated tasks and which are capable of operating simultaneously comprising:

(i) one or more conveying units arranged for conveying medical tubing to one or more bending units;

(ii) one or more said bending units arranged for bending medical tubing in a U shape;

(iii) one or more loading units adapted for individually picking and transporting each medical tubing after its bending from the bending unit to the winding unit;

(iv) one or more winding units for winding medical tubing, comprising a winding nest arranged for receiving medical tubing from said loading unit, and a winding module adapted for winding medical tubing after its deposition into said winding nest;

[0014] The equipment for winding medical tubing may

furthermore comprise:

(i) one or more unloading units adapted for individually picking and transporting each medical tubing after its winding from said winding unit to a packaging unit;

(ii) one or more packaging units for packaging each tubing after its winding, said packaging units capable of receiving the wound medical tubing from said unloading unit and employing a sliding cover plate for maintaining medical tubing in its wound state.

[0015] According to another aspect, said one or more operational units can be arranged and combined with other operational units in sequentially arranged and simultaneously operating working stations, including

(i) one or more preparation stations each comprising said conveying unit(s) said bending unit(s); and/or

(ii) one or more winding stations for winding medical tubing, each comprising said winding unit(s) arranged on a winding station plate;

[0016] This equipment effectively solves the above-mentioned problems of the prior art with automated, sequentially-arranged units and sequentially arranged workstations which can operate simultaneously and are adapted for industrial-scale manufacturing to match a specific production line speed, thereby increasing efficiency and safety of winding and packaging medical tubing.

[0017] Each workstation can comprise a plurality of units in parallel and/or serial arrangement.

[0018] The number of units of each type might be increased to improve the throughput.

[0019] The number of workstations of each type might be increased to improve the throughput.

[0020] The number of units and/or workstations of different types might be different. For example, the number of slow units with a low throughput might be higher than the number of fast units with a higher throughput.

[0021] Different units and/or units of the same type might be mounted in parallel. For example, the equipment might comprise a plurality of bending units in parallel, and/or a plurality of winding units and/or winding stations in parallel.

[0022] Workstation of the same type may be mounted in parallel arrangement. Workstation of different types may be mounted in serial arrangement.

[0023] Optionally, the equipment may further comprise one or more said packaging units for packaging each tubing after its winding, said packaging units.

[0024] The arrangement of the units permits the equipment to operate efficiently and at a high and adjustable throughput rate due to the following favourable aspects:

- (i) The process is fully automated, and
- (ii) a plurality of each workstation as well as a plurality of each unit can be employed, and
- (iii) the units of the workstations are capable of operating simultaneously
- (iv) the processing speed of each unit and the number of each unit and workstation can be optimised to achieve a favourable throughput rate.

[0025] Advantageously, in the bending unit the medical tubing is arranged in a "U"-shape with optimal dimensions for the winding process in the winding unit.

[0026] As a further advantage, the ratio between the number of bending units, the number of loading units and the number of winding stations can be optimised to achieve efficient and smooth operations as well as a favourable throughput rate.

[0027] Furthermore, this advantageous "U"-shape is maintained by the loading unit throughout the transfer of the medical tubing to the winding unit. The disposition of the medical tubing in said "U" shape which is adjusted to the dimension of the winding unit permits consistent and rapid winding without straining or damaging the medical tubing.

[0028] Advantageously, the distal end of the tubing is received below the plate of the winding station by rotatable jaws, which are connected to and rotating with the winding module, permitting winding of the medical tubing around the vertical axis of the winding module, thus facilitating a favourable compact arrangement of several winding units.

[0029] As an additional advantage, the rotatable jaws are operated by fixed jaw grippers which are actuated by an independent motor, thus permitting the rotatable jaws an unlimited range of freedom.

[0030] The rotatable jaws favourably perform a rotating movement along the vertical axis of the winding module together with the rotating winding core, which is actuated by a motor.

[0031] For the duration of the automated winding of the medical tubing around the axis, tube jaws favourably keep the tube positioned within the winding nest and below the level of the winding station plate.

[0032] The wound medical tubing is advantageously raised along the vertical axis to the level of the winding station plate in a controlled movement preventing the tubing from being compressed or damaged and presented to the grippers of the unloading unit which optionally transfer the medical tubing to the packaging unit.

[0033] Advantageously, the ratio between the number of winding stations, which may contain a plurality of winding units, and the number of the unloading units can be optimised to achieve efficient and coordinated operations as well as a favourable throughput rate.

[0034] Once the medical tubing has been placed in the packaging container a cover plate is advantageously positioned over it in an automated gliding movement, which prevents the unwinding of the wound medical tubing.

Brief description of the figures

[0035] Examples of the practical implementation of the invention are disclosed in the description and illustrated by the attached figures of which:

- Figure 1 is a schematic representation of the modular organisation of the operational units and workstations.
- Figure 2A is a schematic representation of the preparation station;
- Figure 2B is a perspective view of the bending unit lever indicating the direction of its automated movement;
- Figure 3 is a top view of the preparation station, identifying the conveying unit and the bending unit;
- Figure 4 is a schematic representation of the winding station;
- Figure 5 is a perspective view of a winding unit from above the winding station plate, comprising the winding nest and the winding module;
- Figure 6 is a perspective view of the winding unit from below the winding station plate;
- Figure 7A is a side view of the winding module
- Figure 7B is a top view of the winding module
- Figure 7C is a perspective view of the winding module

Detailed Description of the Invention

[0036] The present invention describes an equipment for automated winding of medical tubing employing sequentially arranged operational units and workstations, comprising a plurality of units. A first workstation 1, called preparation station, comprises at least one conveying unit 2 and at least one bending unit 3. A second workstation 5, called winding station, comprises at least one, but preferably a plurality of winding units 24. One or more loading units 4 connect the operational processes of the preparation station 1 to the winding station 5. One or more unloading units 6 connect the operational processes of the winding station 5 to a packaging unit 7.

[0037] The equipment of the present invention is configured to wind different type of medical tubing 10, such as but not limited to catheters, dialysis tubing, fluid management (drainage), respiratory equipment, biopharmaceutical equipment and others.

[0038] Figure 1 exemplifies an arrangement of the equipment comprising a preparation station 1, a loading

unit 4, two winding stations 5, an unloading unit 6 and a packaging unit 7. The preparation station 1 comprises a conveying unit 2 configured to dispose medical tubing 10 (Figure 2) into three bending units 3. The medical tubing 10 (Figure 2) might be transferred by the loading unit 4 servicing two separate winding stations 5 comprising each three of winding units 24, each comprising a winding nest 16 (Figure 4) and three winding modules 17 (Figure 4). The unloading unit 6 might be configured to alternately remove medical tubing 10 (Figure 2) from two winding stations 5 and transfer it to the packaging unit 7. The above-mentioned numbers of workstations and different units are intended to be an example and can be varied according to specific needs.

[0039] Optionally, the loading unit 4 and the unloading unit 6 might be equipped with sensors able to detect, if a receiving cavity, such as the winding nest 16 (Figure 4) or the packaging container, is unloaded before the deposition of the medical tubing 10 (Figure 4) in either the receiving cavity, thus enabling the equipment to operate in a highly coordinated and efficient manner.

[0040] Optionally, the winding station 5 might be moved from proximity of the preparation station 1 to proximity of the packaging unit 7 during the winding process in order to minimise the transfer distances of the medical tubing 10 and to increase efficiency of the process.

[0041] Figure 2A illustrates the possible composition of a preparation station comprising a conveying unit 2 and three sequentially arranged bending units 3 and parts of the loading unit 4 with its tube grippers 12. Figure 2B illustrates the binding unit lever 13 in two possible positions, wherein its rotating movement performed to stretch the bent medical tubing 10 is indicated by arrows.

[0042] As shown in Figures 2A and 2B, the ends of the medical tubing 10 are fastened by end grippers 8 of the bending unit 3 and arranged in a "U" shape with the aid of two open end grippers 14 located next to the end grippers 8 and a lever 13, which moves the middle section of the medical tubing 10 in the opposite direction of its ends. The distance between the end grippers 8 configured to fasten the medical tubing 10 and the lever 13 can be adapted to suit the length of the medical tubing.

[0043] Figure 3 illustrates the preparation station 1, in which the medical tubing 10 is delivered to the binding unit 3 by the conveying unit 2, which employs end grippers 8 (Figure 2A) to fasten the ends of the medical tubing 10.

[0044] The medical tubing 10 is received in its "U" shape by the loading unit 4 (Figure 1), which comprises a plurality of grippers to transfer and subsequently dispose the medical tubing 10 in its maintained "U" shape in the winding nest 16 of the winding station 5, which is depicted in Figure 4. For each piece of medical tubing 10, the loading unit 4 (Figure 2A) employs two end grippers grasping the ends of the medical tubing and one tube gripper 12 (Figure 2A) grasping the middle section of the medical tubing. The plurality of grippers is adjusted to suit the plurality of bending units 3 and the plurality of

winding stations 5. The loading unit 4 (Figure 1) can transfer medical tubing 10 to a plurality of winding stations 5 (Figure 1) in an alternating manner.

[0045] The medical tubing 10 is configured to be positioned in the winding nest 16, shown in Figure 4, which is milled into a winding station plate 15, whereby the distal end of the medical tubing is lowered into a descending groove 20 as shown in in Figures 7A to C. The ends of the medical tubing are fastened by a fixed gripper 22 at the level of the winding station plate 15 and by rotatable jaws 18 (Figure 5), which are actuated by fixed jaw grippers 23 (Figure 5) and positioned below the winding station plate 15.

[0046] In a subsequent step, the medical tubing 10 is wound vertically around the winding core 19 of the winding module as shown in Figures 7 A to C, whereby the rotatable jaws 18 clasp one end of the medical tubing are attached to and perform the rotating movement with the winding module 17.

[0047] The winding of the medical tubing 10 around the vertical axis of the winding core 19, as opposed to horizontal coiling in a disc-like shape, facilitates a compact arrangement with several winding units 24 in parallel, as shown in Figure 4.

[0048] During the automated winding of the medical tubing around the winding core 19, tube jaws 21 (Figure 5), which are connected to the winding station plate 15 and can be moved into close proximity of the winding core 19 and away from it in a rotating movement, keeping the medical tubing positioned within the winding nest 16 and below the level of the winding station plate 15.

[0049] The wound medical tubing is raised to the level of the winding station plate 15 (Figure 5) and received by the unloading unit 6 (Figure 1), which employs a plurality of grippers suited to the number of medical tubing to be transferred. The unloading unit 6 subsequently transfers the medical tubing to the packaging unit 7 (Figure 1).

[0050] Upon release and deposition of the medical tubing in the packaging container, a sliding cover plate is moved onto the packaging container in a gliding movement in order to prevent the wound medical tubing from unwinding.

Reference numbers used in the figures

[0051]

- 1 Preparation station
- 2 Conveying unit
- 3 Bending unit
- 4 Loading unit
- 5 Winding station
- 6 Unloading unit
- 7 Packaging unit
- 8 End grippers
- 9 Bending station plate
- 10 Medical tubing

- 11 Alternative lever position adjusted to length of tubing
- 12 Tube gripper
- 13 Lever
- 5 14 Open end grippers
- 15 Winding station plate
- 16 Winding nest
- 17 Winding module
- 18 Rotatable jaws
- 10 19 Winding core
- 20 Descending groove
- 21 Tube jaws
- 22 Fixed grippers
- 23 Fixed jaw grippers
- 15 24 Winding unit

Claims

- 20 1. An equipment for winding medical tubing, comprising:
 - (i) one or more conveying units (2) arranged for conveying medical tubing to one or more bending units (3);
 - (ii) one or more said bending units (3) arranged for bending medical tubing (10) in a U shape;
 - (iii) one or more loading units (4) adapted for individually picking and transporting each medical tubing (10) after its bending;
 - (iv) one or more winding units (24) for winding medical tubing (10), comprising a winding nest (16) arranged for receiving medical tubing (10) from said loading unit (4), and a winding module (17) adapted for winding medical tubing (10) after its deposition into said winding nest (16).
- 25 2. The equipment of claim 1, further comprising:
 - 30 (i) one or more unloading units (6) adapted for individually picking and transporting each medical tubing (10) after its winding;
 - 35 (ii) one or more packaging units (7) for packaging each tubing after its winding, said packaging units (7) employing a sliding cover plate for maintaining medical tubing (10) in its wound state.
- 40 3. An equipment according to any of claim 1 to 2, comprising a plurality of said bending units (3) in parallel.
- 45 4. An equipment according to claim 1 to 3, comprising a plurality of said winding units (24) in parallel.
- 50 5. The equipment of claims 1 to 4, wherein one or a plurality of distinct operational units are organised into automated, sequentially arranged workstations capable of operating simultaneously, including:

- (i) one or more preparation stations (1) comprising said conveying unit(s) (2) and said bending unit(s) (3); and
(ii) one or more winding stations (5) comprising said winding unit(s) (24).
- 5
6. The equipment of any of claim 1 to 5, said conveying unit (2) comprising end grippers (8) arranged for fastening proximal and distal ends of the medical tubing (10) and open end grippers (14) for positioning the medical tubing, and said bending unit (3) comprising a lever (13) arranged for pulling a middle section of the medical tubing in the direction opposite the end grippers (8), so as to arrange the medical tubing (10) in a "U" shape.
- 10
7. The equipment of any of claims 1 to 6, said loading unit (4) comprising for each piece of medical tubing (10) two end grippers (8) capable of grasping the ends of the medical tube piece and one tube gripper (12) capable of grasping the middle section of the medical tubing and transferring the piece of medical tubing to said winding unit (24).
- 15
8. An equipment according to any of claims 1 to 7, wherein said winding units (24) comprise:
- 20
- (i) said winding nest (16), which is cut into the winding station plate (15), comprises a descending groove (20) and which is adapted for receiving the U-shaped medical tubing from the loading unit (4);
- 25
- (ii) two tube jaws (21) capable of keeping the medical tubing positioned within said winding nest (16) and below the surface of said plate (15), a descending groove adapted for presenting the distal end of the medical tubing to rotatable jaws (18); and
- 30
- (iii) a rotatable winding core (19) powered by a fixed motor;
- 35
- (iv) a fixed gripper (22) capable of fastening the proximal end of the medical tubing; and
- 40
- (v) a fixed jaw gripper (23) capable of actuating said rotatable jaws (18).
- 45
9. An equipment according to claim 8, furthermore comprising a fixed motor for actuating said fixed jaw gripper (23), wherein the rotatable jaws (18) and the fixed jaw gripper (23) are located below said winding station plate (15).
- 50
10. An equipment according to any of the claims 1 to 9, comprising an unloading unit (6) equipped with grippers capable of grasping, transferring, and releasing the wound medical tubing.
- 55
11. An equipment according to any of the claims 2 to 10, said packaging unit (7) being equipped with packaging containers capable of receiving the wound medical tubing from said unloading unit (6), said sliding cover plate being capable of being placed onto the packaging container in a gliding movement.
12. An equipment according to claim 11, comprising a plurality of said packaging containers and said sliding cover plates.
13. A method employing an equipment according to any of the claims 1 to 12, to wind medical tubing in an automated process, comprising the steps of:
- i) conveying the medical tubing (10) with said conveying unit (2);
- ii) arranging the medical tubing (10) in a U shape in said bending unit (3);
- iii) individually picking each tubing (10) and placing it onto said winding unit (5);
- iv) receiving said tubing from said loading unit (4) in said winding nest (16) of said winding unit (24);
- v) winding the medical tubing (10) after its deposition into said winding nest (16).
14. A method according to claim 13, wherein the medical tubing (10) is moved into position in said winding nest (16) by said loading unit (4), and wherein the proximal end is fastened by a fixed gripper (22) at the level of said winding station plate (15) and wherein the distal end of the medical tubing (10) is lowered into said descending groove (20) of said winding station and fastened by said rotatable jaws (18), which are actuated by said motorised fixed jaw gripper (22) located below said winding station plate (15) and which perform a rotating movement together with said winding core (19), which is actuated by a motor.

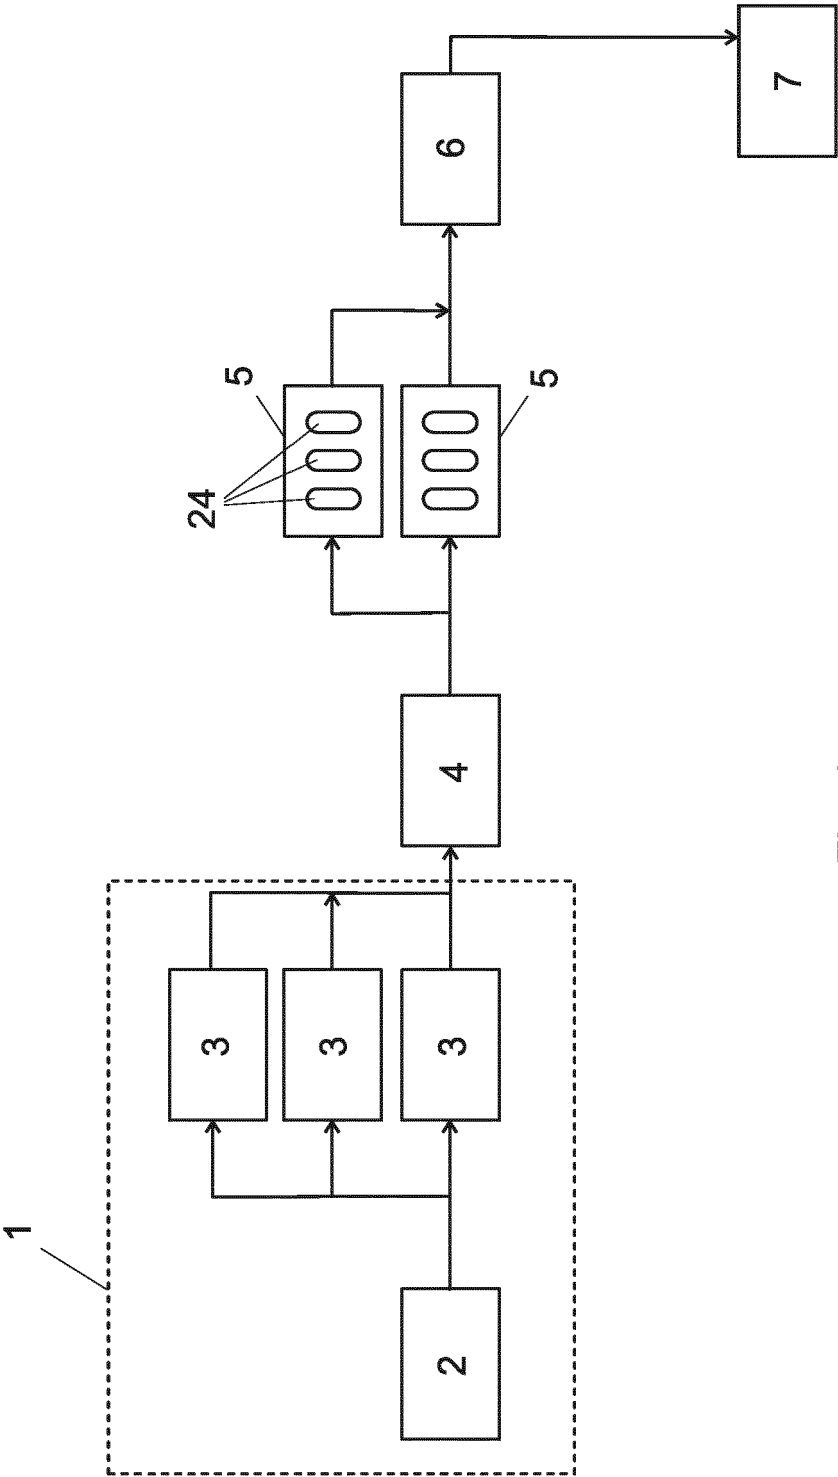


Fig. 1

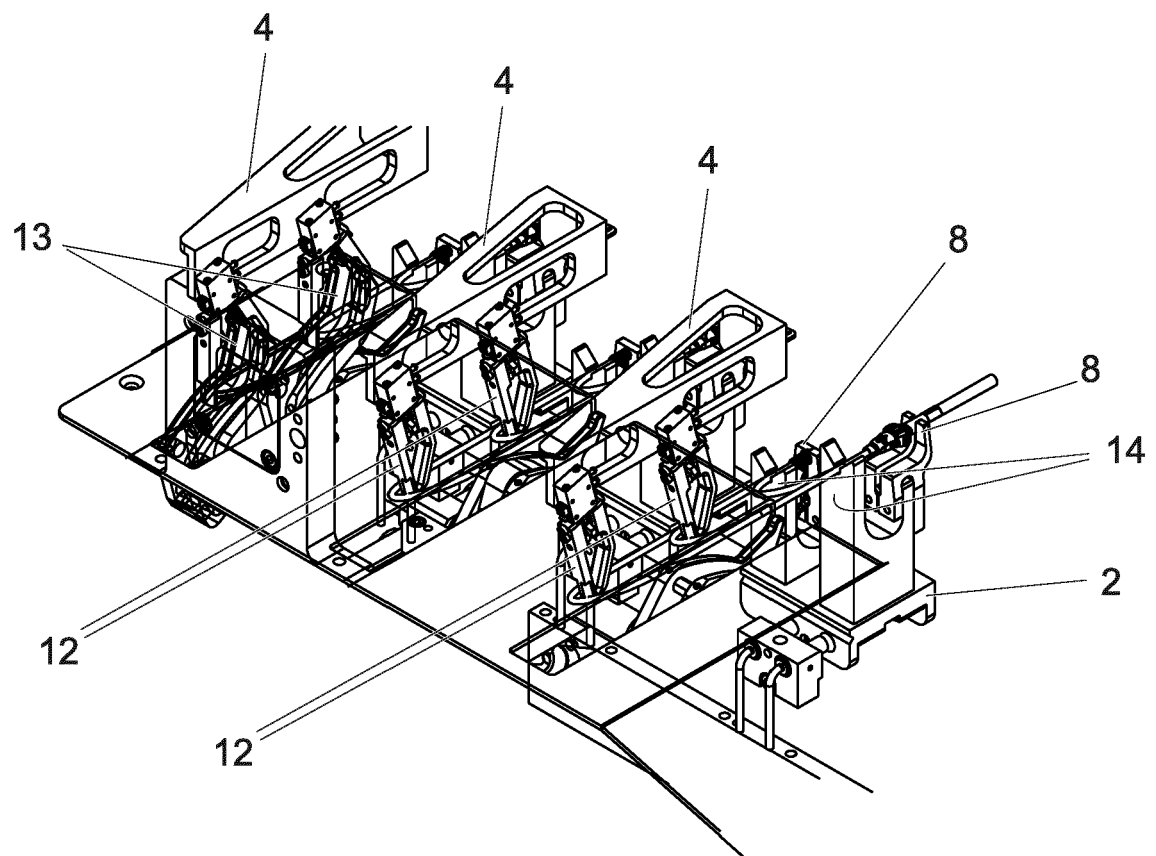


Fig.2a

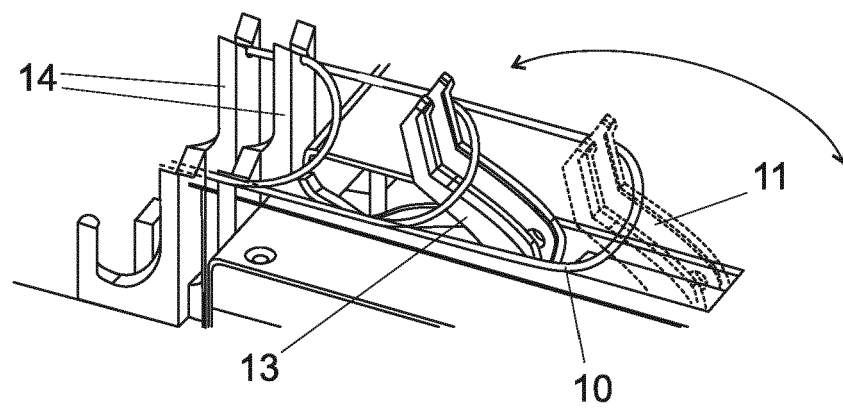
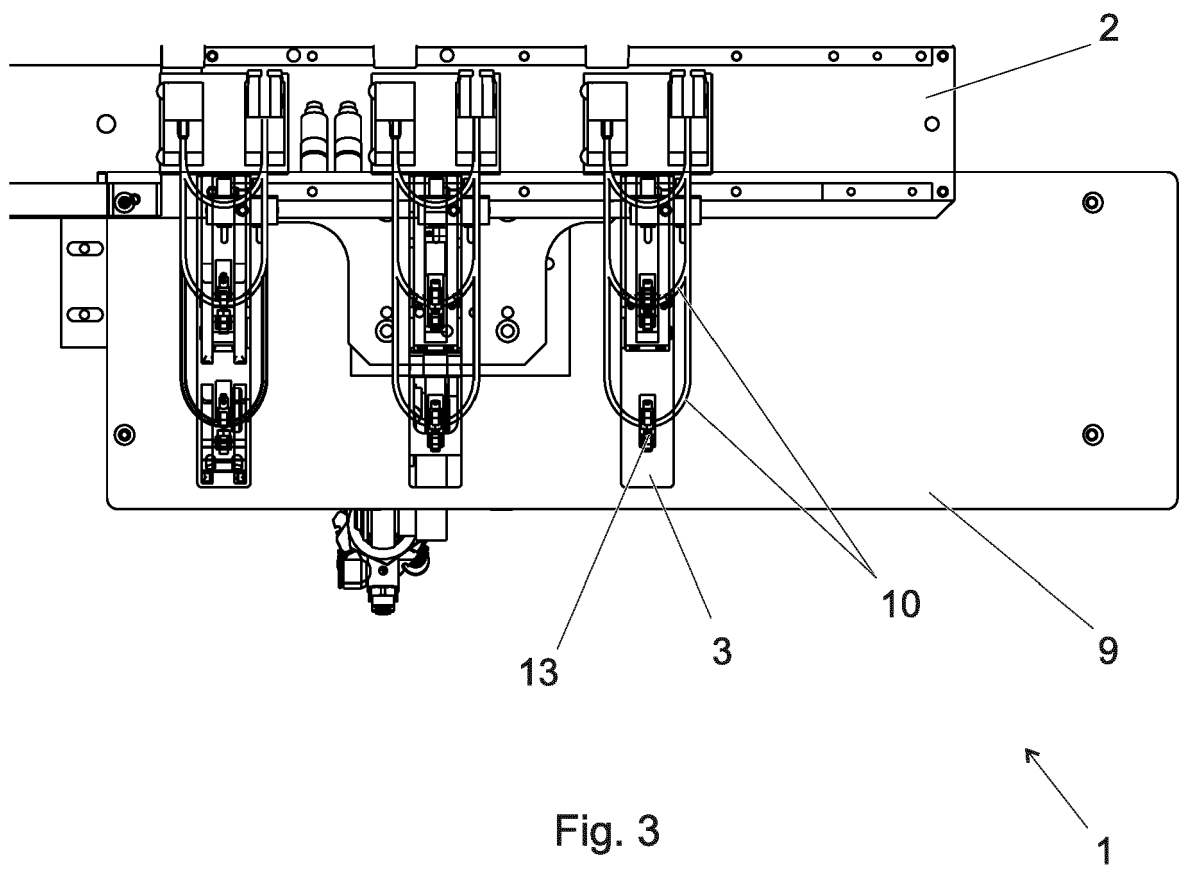


Fig. 2b



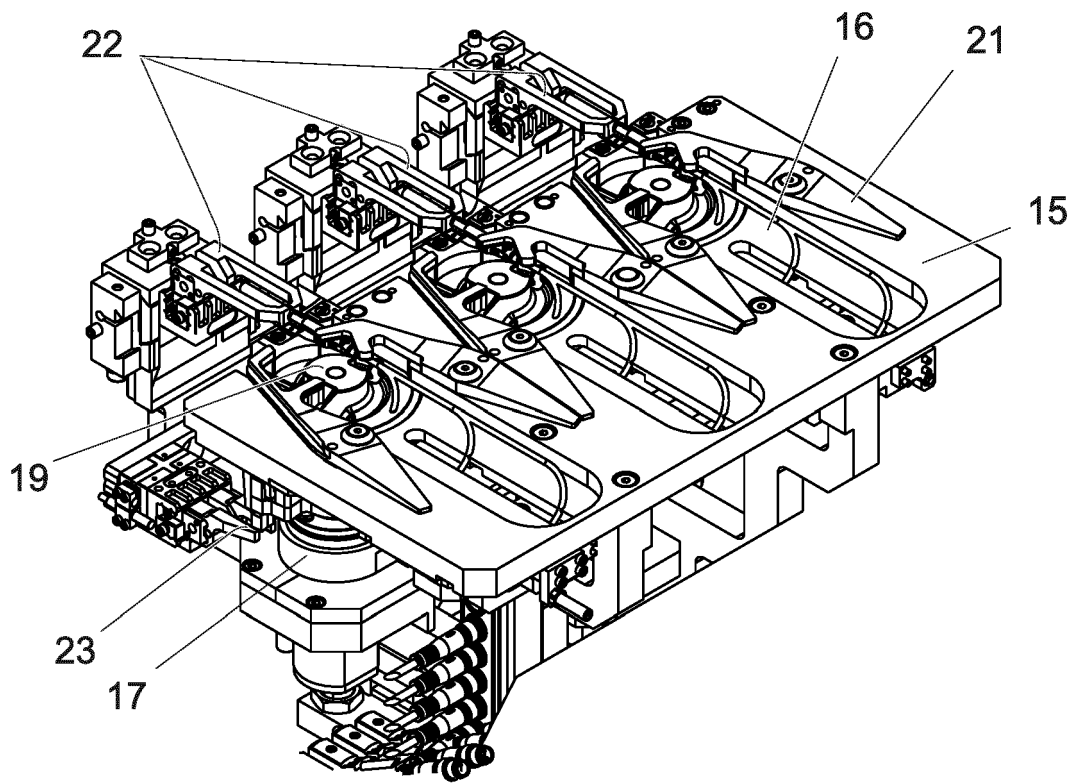


Fig. 4

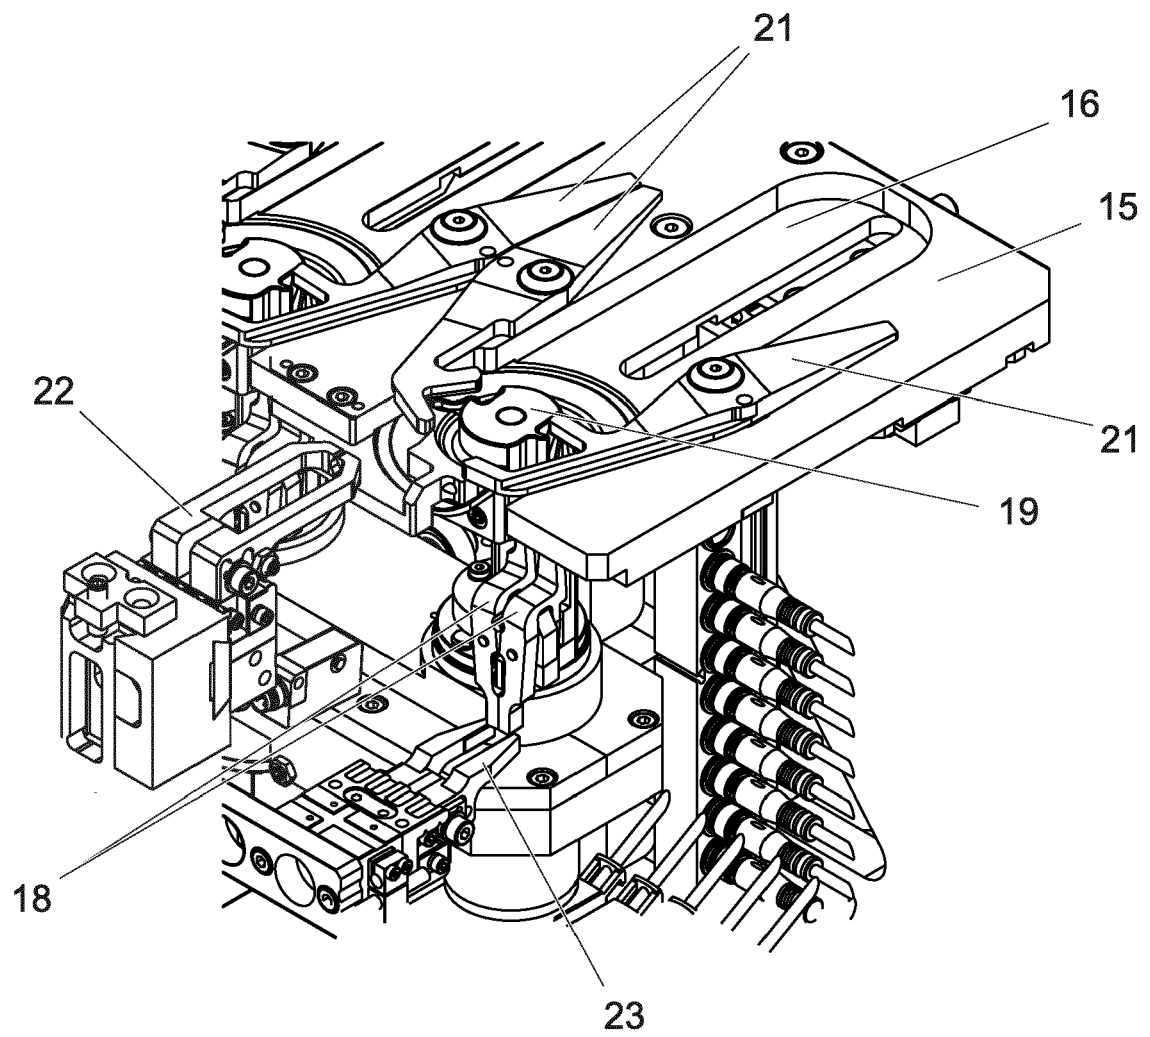


Fig. 5

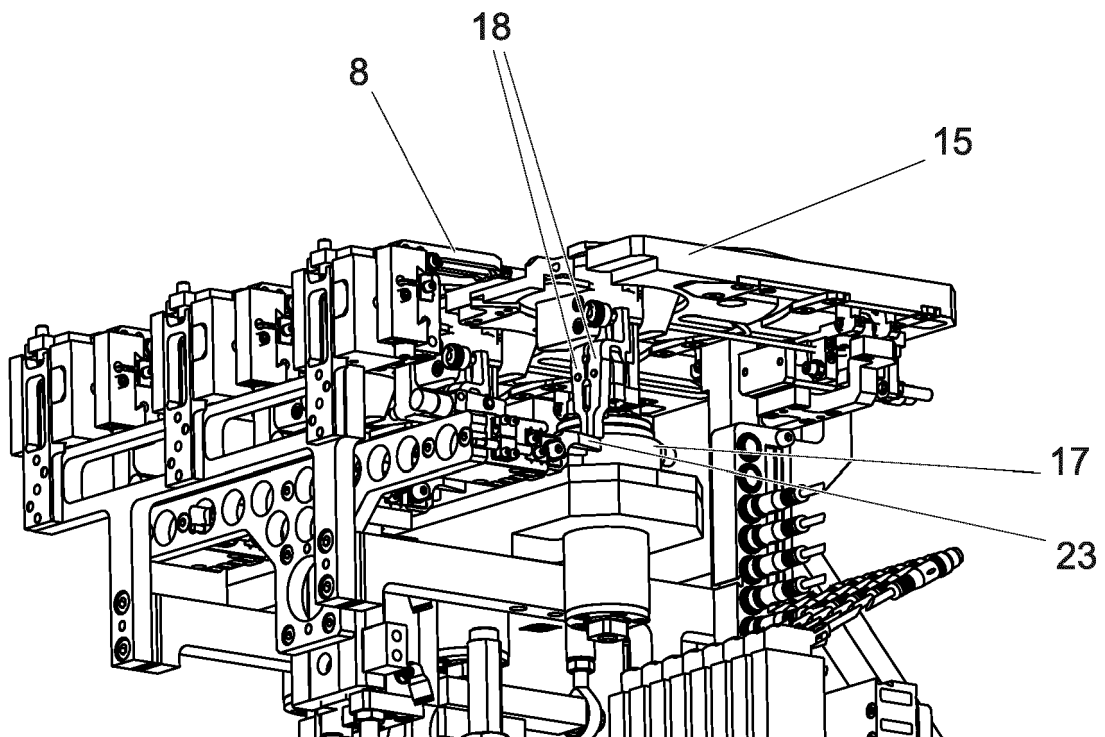


Fig. 6

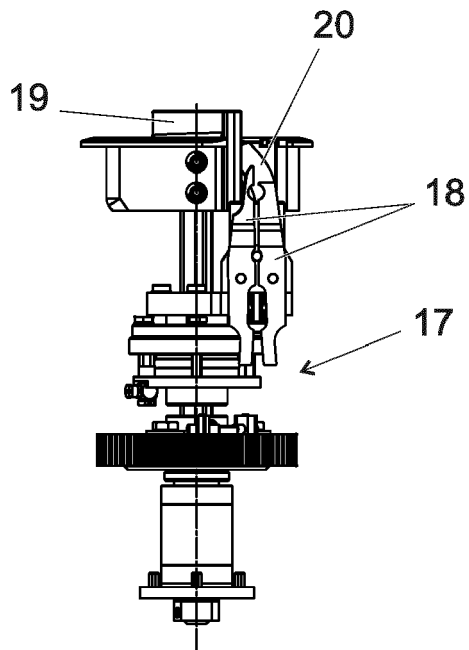


Fig. 7a

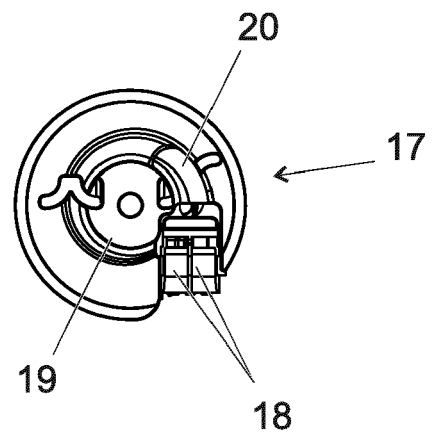


Fig. 7b

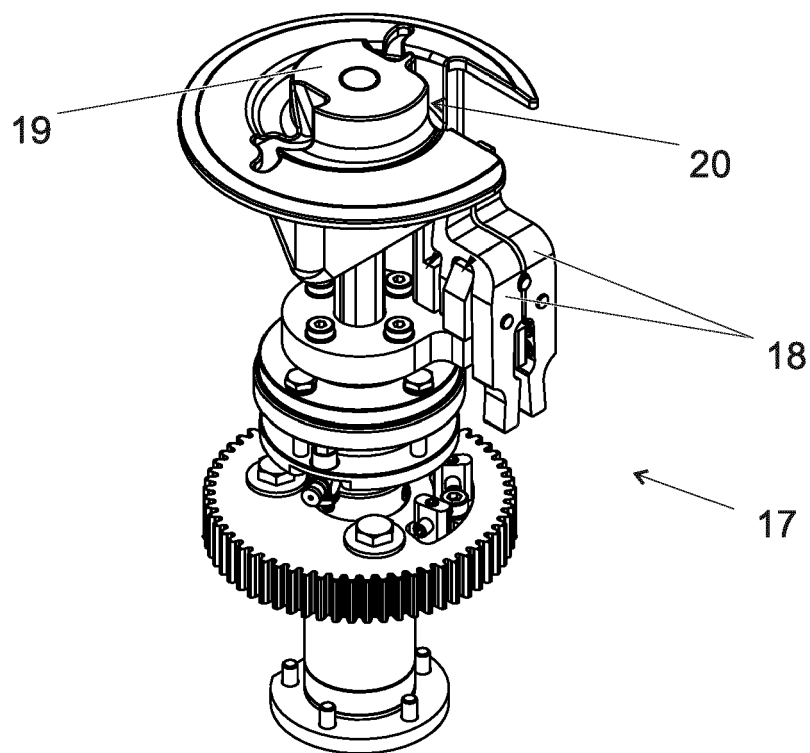


Fig. 7c



EUROPEAN SEARCH REPORT

Application Number
EP 19 17 9055

5

10

15

20

25

30

35

40

45

50

55

DOCUMENTS CONSIDERED TO BE RELEVANT			
Category	Citation of document with indication, where appropriate, of relevant passages	Relevant to claim	CLASSIFICATION OF THE APPLICATION (IPC)
A,D	CN 108 313 424 A (XIAO LIUYUE) 24 July 2018 (2018-07-24) * abstract; figure 1 *	1-14	INV. B65H54/58 B65H54/62
A	DE 35 23 848 A1 (SORTIMAT CREUZ & CO GMBH [DE]) 8 January 1987 (1987-01-08) * claim 1; figures 1A-1C *	1-14	
A	CN 103 523 560 B (TAIZHOU MAIDER MEDICAL INDUSTRY EQUIPMENT CO LTD) 30 September 2015 (2015-09-30) * figures 1,8 *	1-14	
A	EP 1 452 474 A1 (BERNHARD SCHAEFER WERKZEUG UND [DE]) 1 September 2004 (2004-09-01) * paragraphs [0002] - [0005]; figures 1-8 *	1-14	
A	US 6 135 164 A (CELOUDOUX JEAN-PAUL [FR] ET AL) 24 October 2000 (2000-10-24) * claim 1; figures 3-12 *	1,3,5,6	TECHNICAL FIELDS SEARCHED (IPC) B65H
The present search report has been drawn up for all claims			
Place of search The Hague		Date of completion of the search 14 November 2019	Examiner Pussemier, Bart
CATEGORY OF CITED DOCUMENTS X : particularly relevant if taken alone Y : particularly relevant if combined with another document of the same category A : technological background O : non-written disclosure P : intermediate document		T : theory or principle underlying the invention E : earlier patent document, but published on, or after the filing date D : document cited in the application L : document cited for other reasons & : member of the same patent family, corresponding document	

EPO FORM 1503 03.82 (P04C01)

**ANNEX TO THE EUROPEAN SEARCH REPORT
ON EUROPEAN PATENT APPLICATION NO.**

EP 19 17 9055

5 This annex lists the patent family members relating to the patent documents cited in the above-mentioned European search report.
The members are as contained in the European Patent Office EDP file on
The European Patent Office is in no way liable for these particulars which are merely given for the purpose of information.

14-11-2019

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
CN 108313424 A	24-07-2018	NONE	
DE 3523848 A1	08-01-1987	NONE	
CN 103523560 B	30-09-2015	NONE	
EP 1452474 A1	01-09-2004	AT 344776 T DE 10308432 A1 EP 1452474 A1 ES 2274156 T3 JP 4204962 B2 JP 2004256300 A	15-11-2006 23-09-2004 01-09-2004 16-05-2007 07-01-2009 16-09-2004
US 6135164 A	24-10-2000	DE 19844416 A1 GB 2330545 A US 6135164 A	01-04-1999 28-04-1999 24-10-2000

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- CN 108313424 [0007]
- US 2018008798 A [0008]
- US 20130006226 A [0009]