



(12) **EUROPEAN PATENT APPLICATION**

(43) Date of publication:
31.03.2021 Bulletin 2021/13

(51) Int Cl.:
A61B 5/00 (2006.01) A61B 5/145 (2006.01)

(21) Application number: **20204860.9**

(22) Date of filing: **10.12.2014**

(84) Designated Contracting States:
AL AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO PL PT RO RS SE SI SK SM TR

(30) Priority: **10.01.2014 US 201461926215 P**

(62) Document number(s) of the earlier application(s) in accordance with Art. 76 EPC:
14821031.3 / 3 091 893

(71) Applicant: **Ascensia Diabetes Care Holdings AG 4052 Basel (CH)**

(72) Inventors:
• **GOFMAN, Igor**
Crouton-on-Hudson, NY 10520 (US)

• **DIONISIO, Christopher**
Millington, NJ 07946 (US)

(74) Representative: **Cohausz & Florack**
Patent- & Rechtsanwälte
Partnerschaftsgesellschaft mbB
Bleichstraße 14
40211 Düsseldorf (DE)

Remarks:

This application was filed on 30-10-2020 as a divisional application to the application mentioned under INID code 62.

(54) **SETUP SYNCHRONIZATION APPARATUS AND METHODS FOR END USER MEDICAL DEVICES**

(57) Embodiments of the present invention enable setup synchronization of an end user medical device such as a blood glucose meter. The invention includes a controller including a memory; a transceiver operatively coupled to the controller; and a host computer interface operative to couple the controller to a host computer, wherein the memory is operative to store instructions ex-

ecutable on the controller. The instructions are adapted to cause the controller to scan for an advertising medical device using the transceiver, establish a communications connection with a medical device advertising for synchronization, and transmit synchronization data to a medical device once a communication connection has been established. Numerous other aspects are disclosed.

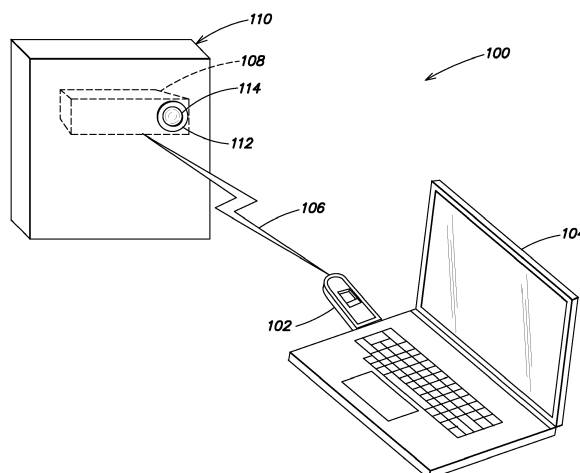


FIG. 1

Description

RELATED APPLICATIONS

[0001] The present application claims priority to U.S. Provisional Patent Application Serial No. 61/926,215, filed January 10, 2014 and entitled "SETUP SYNCHRONIZATION APPARATUS AND METHODS FOR END USER MEDICAL DEVICES", (Attorney Docket No. BHC134020(BHDD/045/L)), which is hereby incorporated herein by reference in its entirety for all purposes.

FIELD

[0002] The present invention relates to medical devices, and more specifically to apparatus, systems, and methods for setup synchronization of medical devices.

BACKGROUND

[0003] Conventional end user medical devices such as blood glucose meters (BGMs) are typically packaged by manufacturers with an initial configuration that may not always be optimal for the intended application or patient. Thus, frequently, a healthcare provider (HCP) must adjust the configuration of the meter. Accordingly, systems, apparatus, and methods for facilitating setup of such devices are needed.

SUMMARY

[0004] In some aspects, embodiments of the present invention provide an apparatus for setup synchronization of a medical device such as a blood glucose meter. The apparatus includes a controller including a memory; a transceiver operatively coupled to the controller; and a host computer interface operative to couple the controller to a host computer, wherein the memory is operative to store instructions executable on the controller, the instructions adapted to cause the controller to scan for an advertising medical device using the transceiver, establish a communications connection with a medical device advertising for synchronization, and transmit synchronization data to a medical device once a communication connection has been established.

[0005] In other aspects, embodiments of the present invention provide a system for setup synchronization of a medical device such as a blood glucose meter. The system includes an end user medical device including an activation function for putting the medical device in an advertising mode for requesting synchronization; and a setup synchronization apparatus including a controller including a memory; a transceiver operatively coupled to the controller; and a host computer interface operative to couple the controller to a host computer. The memory is operative to store instructions executable on the controller, the instructions adapted to cause the controller to scan for an advertising medical device using the trans-

ceiver.

[0006] In yet other aspects, embodiments of the present invention provide a method for setup synchronization of a medical device such as a blood glucose meter.

5 The method includes scanning for an end user medical device advertising for synchronization using a setup synchronization apparatus; discovering an end user medical device advertising for synchronization; establishing a communication connection with a discovered end user medical device; and synchronizing the connected end user medical device.

10 [0007] Numerous other aspects are provided in accordance with these and other embodiments of the invention. Other features and aspects of embodiments of the present invention will become more fully apparent from the following detailed description, the appended claims, and the accompanying drawings.

BRIEF DESCRIPTION OF THE DRAWINGS

[0008]

FIG. 1 illustrates a perspective view of an example setup synchronization system according to some embodiments of the present invention.

FIG. 2 illustrates a perspective view of an example setup synchronization apparatus according to some embodiments of the present invention.

FIG. 3 illustrates a schematic block drawing of a circuit for a setup synchronization apparatus according to some embodiments of the present invention.

FIG. 4 illustrates a block diagram representation of a system initiation process according to some embodiments of the present invention.

FIG. 5 illustrates a block diagram representation of a synchronization process according to some embodiments of the present invention.

FIG. 6 is a flowchart depicting a method of synchronizing a medical device according to some embodiments of the present invention.

DETAILED DESCRIPTION

[0009] End user medical devices such as, for example, blood glucose meters (BGMs) are typically provided to patients by a healthcare provider (HCP). The HCP can stock a number of devices as packaged by the manufacturer and provide the devices to patients as needed. Such devices can include a real-time clock (RTC) that conventionally is set by the manufacturer before the devices are packaged. This ensures that the end user receives a device with an accurately set RTC so that medical data can be correctly time indexed. Thus, the RTC is typically running while the device is in storage. Since the storage time for such devices can be as long as fifteen months or more, a significant amount of battery power consumption can occur during this period. In addition, the HCP can be located in a different time zone than the manufacturer

and thus, correctly setting the RTC can be further complicated.

[0010] Conventionally, manufacturers solve these problems by using a more expensive battery with sufficient power to last the maximum storage duration. Manufacturers also set the RTC based upon the location to which the devices are to be used. Both of these solutions however, require additional manufacturing expense and increase the cost of the medical devices to the end users. Accordingly, improved methods and apparatus are needed to perform setup synchronization of such devices. Further, there are a variety of other configuration options that HCPs can setup on end user medical devices (e.g., BGMs) such as the units used (e.g., mg/dL vs. mmol/L), high/low limits, reminder alarms, etc.

[0011] Embodiments of the present invention provide a setup synchronization apparatus that addresses all of these issues. A setup synchronization apparatus according to embodiments of the present invention can be adapted to wirelessly and automatically set an RTC and other parameters of an end user medical device. Such a setup synchronization apparatus can include a controller (e.g., a programmable microcontroller); a memory for storage of a host computer application; a transceiver (e.g., a transmitter/receiver) that enables wireless communication with the end user medical devices; and a computer interface I/O port such as a universal serial bus (USB) interface for communication with a host computer and to allow uploading/installation of the host computer application to the host computer.

[0012] Turning to FIG. 1, in some embodiments, the system 100 of the present invention includes a setup synchronization apparatus 102 that is adapted to be connected to a host computer 104 operated by a HCP. The setup synchronization apparatus 102 is also adapted to wirelessly communicate 106 with an end user medical device 108 (e.g., a BGM) while the end user medical device 108 is still contained within the packaging 110 from the manufacturer. In some embodiments, the packaging 110 can include an access hole 112 that allows a HCP to trigger an activation function (e.g., press an activation button 114) on the end user medical device 108 while the device 108 is still contained within the packaging 110.

[0013] In operation, the setup synchronization apparatus 102 is initially connected to the host computer 104, for example, via a USB port in the host computer 104. In some embodiments, upon connection to the host computer 104, an application executing on the setup synchronization apparatus 102 checks to see if the host computer 104 has the host computer application installed. If not, the host computer application can be automatically (or with HCP authorization) installed on the host computer 104.

[0014] Once the installation of the host computer application is complete, the host computer application will run in the background of the host computer 104, waiting for a setup synchronization apparatus 102 to request the

time and setup parameters. As long as the setup synchronization apparatus 102 is connected to the host computer 104, the setup synchronization apparatus 102 will scan for end user medical devices 108 to synchronize.

5 The host application is operative to provide a user interface to the HCP for configuring parameters of the medical device. The host application can include any number of graphical user interface (GUI) controls to allow the HCP to select parameter values such as time zone, units of measure, warning alarms, target zone levels, operating modes, sampling rates, glucose measurement data, patient information, etc.

10 **[0015]** In some embodiments, the end user medical device 108 can be shipped in a low power consumption mode (e.g., in a "deep sleep" mode) or in an "off" state. In either case, the RTC within the end user medical device 108 is not running. Pressing the activation button 114 through the packaging access hole 112 triggers an activation function which switches end user medical device 108 to an active mode and/or powers up the device 108 to an "on" state. The end user medical device 108 initializes and begins "advertising" by broadcasting a wireless signal that both uniquely identifies the device 108 and requests synchronization data from any setup synchronization apparatus 102 within the broadcast range. If a setup synchronization apparatus 102 coupled to a host computer 104 is within range, the setup synchronization apparatus 102 and the device 108 establish a wireless connection 106.

20 **[0016]** Once the end user medical device 108 and the setup synchronization apparatus 102 connect, the apparatus 102 receives the correct time and setup parameters from the host application running on the host computer 104 via the wireless connection 106 between the apparatus 102 and the device 108. The host computer 104 thereby synchronizes with the end user medical device 108. In some embodiments, once synchronization has completed, a message or other indicia can be displayed on the host computer 104 and/or on a display of the end user medical device 108. In some embodiments, indicator lights or other indicia can be included on the setup synchronization apparatus 102 and/or the end user medical device 108 to indicate the wireless connection status and/or the synchronization status. Upon completion of synchronization, the end user medical device 108 can automatically disconnect from the setup synchronization apparatus 102 and return to a lower power consumption state but with the RTC now running (e.g., a "shallow sleep" mode). The setup synchronization apparatus 102 can return to a scanning state so that a next end user medical device 108 can be synchronized.

30 **[0017]** Turning now to FIGs. 2 and 3, details of the setup synchronization apparatus 102 are illustrated and described. FIG. 2 depicts a magnified perspective view of an example embodiment of a setup synchronization apparatus 102. The example embodiment includes a housing 202 that encloses and protects a circuit (not visible in FIG. 2 but see FIG. 3). The example setup synchroni-

zation apparatus 102 depicted in FIG. 2 also includes configuration switches 204 (e.g., dual in-line package (DIP) switches) for setting certain parameters of the apparatus 102 and an indicator 206 (e.g., a tri-color LED light) that can indicate the status of the setup synchronization apparatus 102.

[0018] For example, in some embodiments, the configuration switches 204 can be used to set values for parameters such as time zone, units of measurement, reminder alarms enabled/disabled, etc. that will be passed to end user medical device 108. In some embodiments, the indicator 206 can display different colors to reflect, for example, that the setup synchronization apparatus 102 is (1) scanning for an end user medical device 108 to synchronize, (2) wirelessly connected to an end user medical device 108, or (3) completed synchronizing an end user medical device 108. The example setup synchronization apparatus 102 depicted in FIG. 2 also includes a connector 208 (e.g., a USB connector) for coupling the setup synchronization apparatus 102 to the host computer 104.

[0019] FIG. 3 is a block diagram illustrating an example embodiment of a circuit 102' for the setup synchronization apparatus 102. The circuit 102' can include a controller 302 (e.g., a programmed microcontroller) operatively coupled to memory 304 (e.g., non-volatile random access memory (NVRAM)) adapted to store instructions for execution by the controller 302 as well as a host computer application. The controller 302 can also be operatively coupled to a transceiver 306 (e.g., a Bluetooth® transceiver, a near field communication (NFC) transceiver, etc.) including an appropriate antennae 308 for wireless communication with end user medical devices 108. Additionally, the circuit 102' can include a host computer interface 208' (e.g., a USB interface) operatively coupled to the controller 302 to enable communication between the setup synchronization apparatus 102 and the host computer 104.

[0020] Turning now to FIG. 4, the details of an example embodiment of initial communication between the setup synchronization apparatus 102 and the host computer 104 are illustrated in a block diagram 400. The setup synchronization apparatus 102 is initially connected to the host computer 104 (402) and the setup synchronization apparatus 102 checks the host computer 104 to determine if the host computer application has been installed on the host computer 104 (404). The host computer 104 receives the request and responds (406). If the application has not been installed, the setup synchronization apparatus 102 uploads the application to the host computer 104 (408) and the host computer installs the application (410). Now that the application has been installed, the setup synchronization apparatus 102 begins scanning for an end user medical device 108 to synchronize (412) and the host computer 104 runs the application as a background process (414).

[0021] FIG. 5 illustrates an example embodiment of the details of a synchronization process over time. The

example depicts the activities of the setup synchronization apparatus 102, the HCP operating the host computer 104 (with a setup synchronization apparatus 102 and associated application installed), and the end user medical device 108 relative to each other as three concurrent interrelated horizontal process flows occurring over time in block diagram 500. Initially, the setup synchronization apparatus 102 is scanning for an end user medical device 108 to synchronize (502) and the end user medical device 108 is in a low power consumption (e.g., deep sleep) mode with the RTC not running (504). Upon the HCP pressing the activation button 114 on the end user medical device 108 (506), the end user medical device 108 begins "advertising" (508) and the setup synchronization apparatus 102 discovers the end user medical device 108 (510). Once a communication connection 106 is established, the setup synchronization apparatus 102 synchronizes with the end user medical device 108 (512) and the end user medical device 108 synchronizes with the setup synchronization apparatus 102 (514). Once the synchronization is complete, the HCP receives a message indicating the completion status (516). The setup synchronization apparatus 102 returns to scanning for another device 108 to synchronize (518) and the end user medical device 108 switches to a low power consumption (e.g., shallow sleep) mode but with the RTC running (520).

[0022] Turning now to FIG. 6, an example method 600 of embodiments of the present invention is depicted in a flowchart. Initially, the setup synchronization apparatus 102 is scanning for an end user medical device 108 to synchronize (602) and the end user medical device 108 is in a low power consumption (e.g., deep sleep) mode with the RTC not running (604). Upon the HCP pressing the activation button 114 on the end user medical device 108 (606), the end user medical device 108 begins "advertising" (608) and the setup synchronization apparatus 102 discovers the end user medical device 108 (610). Once a communication connection 106 is established (612), the setup synchronization apparatus 102 synchronizes with the end user medical device 108 (614). Once the synchronization is complete, the HCP receives a message indicating the completion status (616). The setup synchronization apparatus 102 returns to scanning for another device 108 to synchronize (618) and the end user medical device 108 switches to a low power consumption (e.g., shallow sleep) mode but with the RTC running (620).

[0023] The following numbered embodiments describe features in accordance with embodiments of the disclosure.

Embodiment 1. An apparatus comprising: a controller including a memory; a transceiver operatively coupled to the controller; and a host computer interface operative to couple the controller to a host computer, wherein the memory is operative to store instructions executable on the controller, the instruc-

tions adapted to cause the controller to: scan for an advertising medical device using the transceiver, establish a communications connection with a medical device advertising for synchronization, and transmit synchronization data to a medical device once a communication connection has been established. 5

Embodiment 2. The apparatus of embodiment 1 wherein the memory is further operative to store a host application for installation and execution on a host computer via the host computer interface. 10

Embodiment 3. The apparatus of embodiment 2 wherein the instructions are further adapted to cause the controller to determine if the host application is installed on the host computer. 15

Embodiment 4. The apparatus of embodiment 1 wherein the instructions are further adapted to cause the controller to synchronize a real-time clock running in the medical device receiving the synchronization data. 20

Embodiment 5. The apparatus of embodiment 4 wherein the instructions are further adapted to cause the controller to transmit configuration parameter values to the medical device and to configure the medical device based on the configuration parameter values. 25

Embodiment 6. The apparatus of embodiment 4 wherein the instructions are further adapted to cause the controller to cause a connected host computer to display a synchronization complete indication once the medical device has been synchronized. 30 35

Embodiment 7. The apparatus of embodiment 4 wherein the instructions are further adapted to cause the controller to return to a scanning mode once the medical device has been synchronized. 40

Embodiment 8. A system comprising an end user medical device including an activation function for putting the medical device in an advertising mode for requesting synchronization; and a setup synchronization apparatus including a controller including a memory; a transceiver operatively coupled to the controller; and a host computer interface operative to couple the controller to a host computer, wherein the memory is operative to store instructions executable on the controller, the instructions adapted to cause the controller to scan for an advertising medical device using the transceiver. 45 50

Embodiment 9. The system of embodiment 8 further comprising a host computer executing a host application adapted to allow a health care provider to configure the end user medical device. 55

Embodiment 10. The system of embodiment 8 wherein the instructions are further adapted to cause the controller to establish a communications connection with the medical device once the medical device is advertising for synchronization, and to transmit synchronization data to the medical device once a communication connection has been established.

Embodiment 11. The system of embodiment 10 wherein the memory is further operative to store a host application for installation and execution on a host computer via the host computer interface.

Embodiment 12. The system of embodiment 11 wherein the instructions are further adapted to cause the controller to determine if the host application is installed on the host computer.

Embodiment 13. The system of embodiment 10 wherein the instructions are further adapted to cause the controller to synchronize a real-time clock running in the medical device receiving the synchronization data.

Embodiment 14. The system of embodiment 13 wherein the instructions are further adapted to cause the controller to transmit configuration parameter values to the medical device and to configure the medical device based on the configuration parameter values. 30

Embodiment 15. The system of embodiment 13 wherein the instructions are further adapted to cause the controller to cause a connected host computer to display a synchronization complete indication once the medical device has been synchronized.

Embodiment 16. The system of embodiment 13 wherein the instructions are further adapted to cause the controller to return to a scanning mode once the medical device has been synchronized.

Embodiment 17. A method comprising: scanning for an end user medical device advertising for synchronization using a setup synchronization apparatus; discovering an end user medical device advertising for synchronization; establishing a communication connection with a discovered end user medical device; and synchronizing the connected end user medical device.

Embodiment 18. The method of embodiment 17 further comprising displaying an indication that the end user medical device has been synchronized.

Embodiment 19. The method of embodiment 17 further comprising returning to scanning for another end user medical device advertising for synchronization.

Embodiment 20. The method of embodiment 17 further comprising determining if a host computer connected to the setup synchronization apparatus has a host application installed.

Embodiment 21. The method of embodiment 17 wherein synchronizing the connected end user medical device includes configuring the connected end user medical device with configuration parameter values.

[0024] The foregoing description discloses only example embodiments of the invention. Modifications of the above-disclosed apparatus, systems and methods which fall within the scope of the invention will be readily apparent to those of ordinary skill in the art. Accordingly, while the present invention has been disclosed in connection with example embodiments, it should be understood that other embodiments may fall within the scope of the invention, as defined by the following claims.

Claims

1. An end user medical device comprising:

a manually-operated actuator to cause the controller to perform an activation function;
a real-time clock, the real-time clock not running prior to the end user medical device being in an advertising mode for requesting synchronization;
a wireless transceiver for transmitting a synchronization request and for receiving synchronization data;
a battery to power the controller, wireless transceiver, and real-time clock once running; and
a controller and a memory operative to store instructions executable on the controller, the controller and memory operative to:

perform the activation function to put the end user medical device in the advertising mode for requesting synchronization,
establish a communications connection with a setup synchronization apparatus, receive synchronization data from the setup synchronization apparatus once a communication connection has been established, synchronize the end user medical device in accordance with received synchronization data including setting the real-time clock to the correct time, and determine and store medical data of a user.

2. The end user medical device of claim 1 further comprising packaging sized to contain the end user medical device therein.

3. The end user medical device of claim 2 wherein the packaging has an access hole aligned with the manually-operated actuator to provide access to the manually-operated actuator.

4. The end user medical device of claim 1 wherein the manually-operated actuator is an activation button that can be pressed to cause the controller to perform the activation function.

5. The end user medical device of claim 1 wherein the synchronization data further comprises at least one of time zone, units of measure, operating modes, sampling rates, patient information, and medical data target zones.

6. The end user medical device of claim 1 further comprising a display configured to display a message or other indicia indicating that synchronization has completed.

7. The end user medical device of claim 1 wherein the controller is further operative to disconnect from the setup synchronization apparatus upon completion of synchronization.

8. The end user medical device of claim 1 wherein, upon completion of synchronization, the end user medical device switches to a low power consumption mode with the real-time clock running.

9. The end user medical device of claim 1 wherein the end user medical device comprises a blood glucose meter.

10. A method of synchronizing an end user medical device, the method comprising:

performing an activation function in the end user medical device to put the end user medical device in an advertising mode for requesting synchronization;
advertising for synchronization via the end user medical device in the advertising mode, the end user medical device having a real-time clock, the real-time clock not running prior to the advertising for synchronization;
establishing a communication connection between the end user medical device and synchronization apparatus; and
synchronizing the end user medical device in accordance with synchronization data received from the synchronization apparatus, the synchronizing comprising setting the real-time clock to the correct time.

11. The method of claim 10 further comprising displaying an indication at the end user medical device that the

end user medical device has been synchronized.

12. The method of claim 10 wherein the synchronizing further comprises configuring the end user medical device with at least one of a time zone, units of measure, operating modes, sampling rates, patient information, and medical data target zones. 5
13. The method of claim 10 wherein the performing, the advertising, the establishing, and the synchronizing are performed while the end user medical device is contained within packaging from the manufacturer. 10
14. The method of claim 10 further comprising shipping from the manufacturer the end user medical device in a low power consumption mode with the real-time clock not running. 15
15. The method of claim 10 further comprising switching the end user medical device to a low power consumption mode with the real-time clock running upon completion of synchronization. 20

25

30


35

40

45

50

55

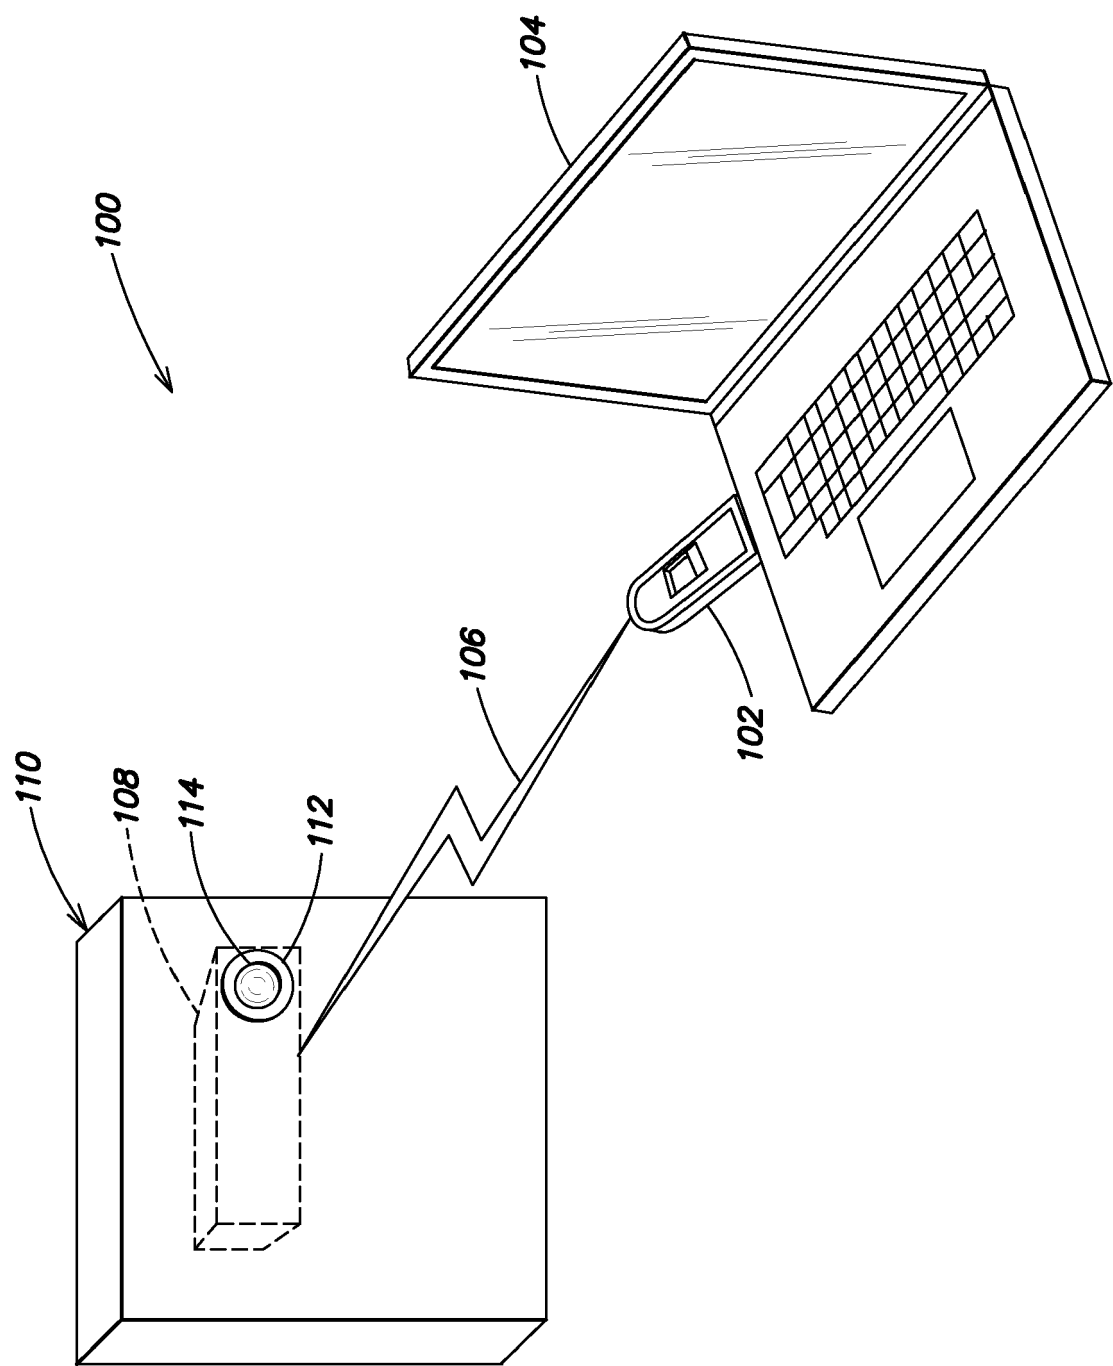

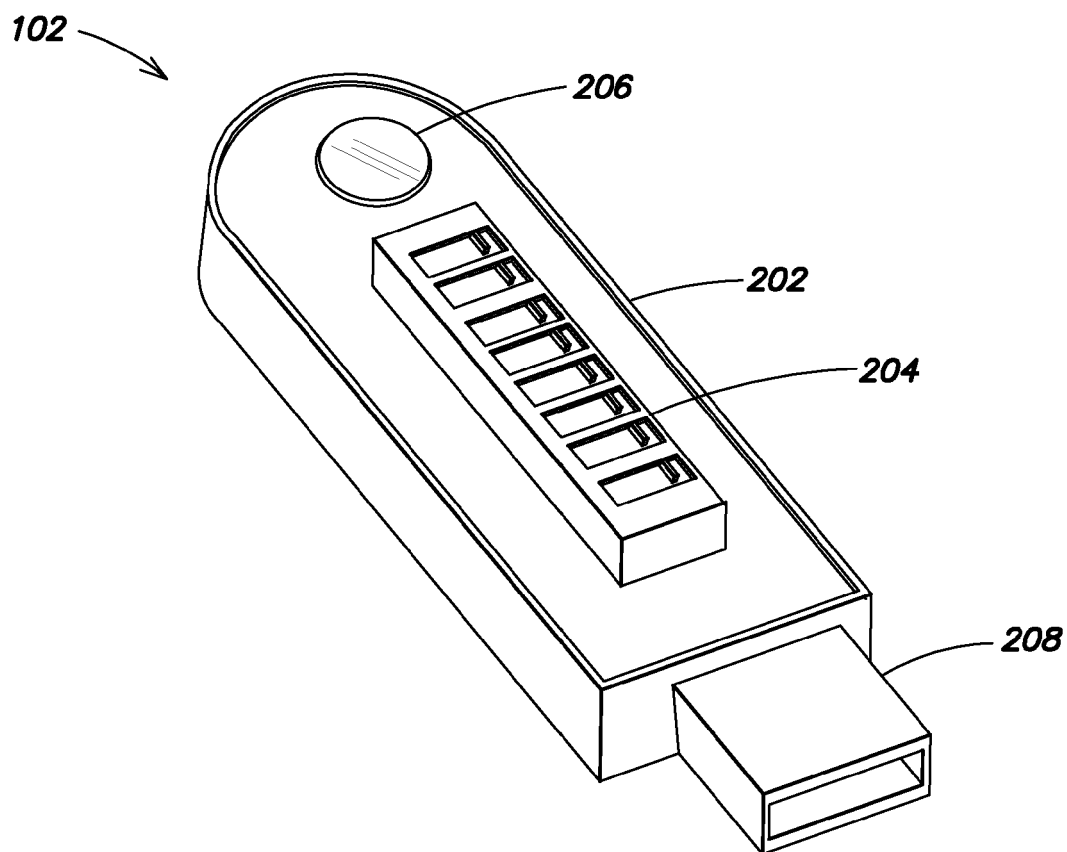


FIG. 2

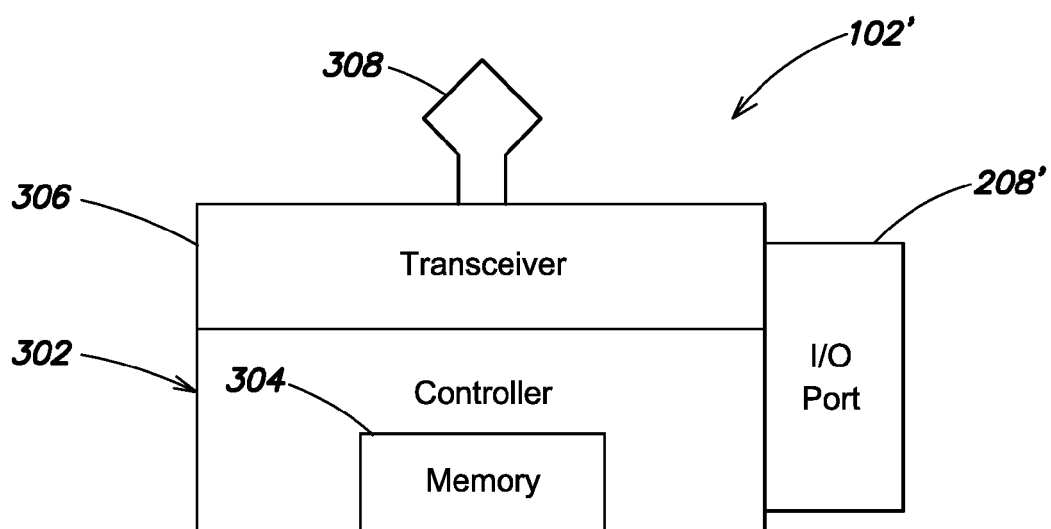


FIG. 3

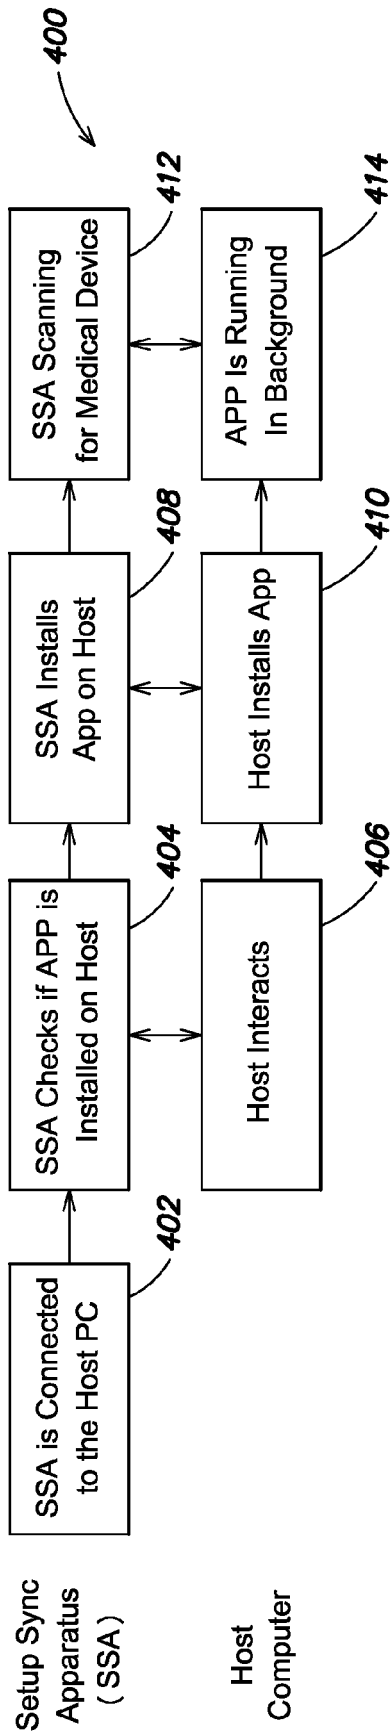


FIG. 4


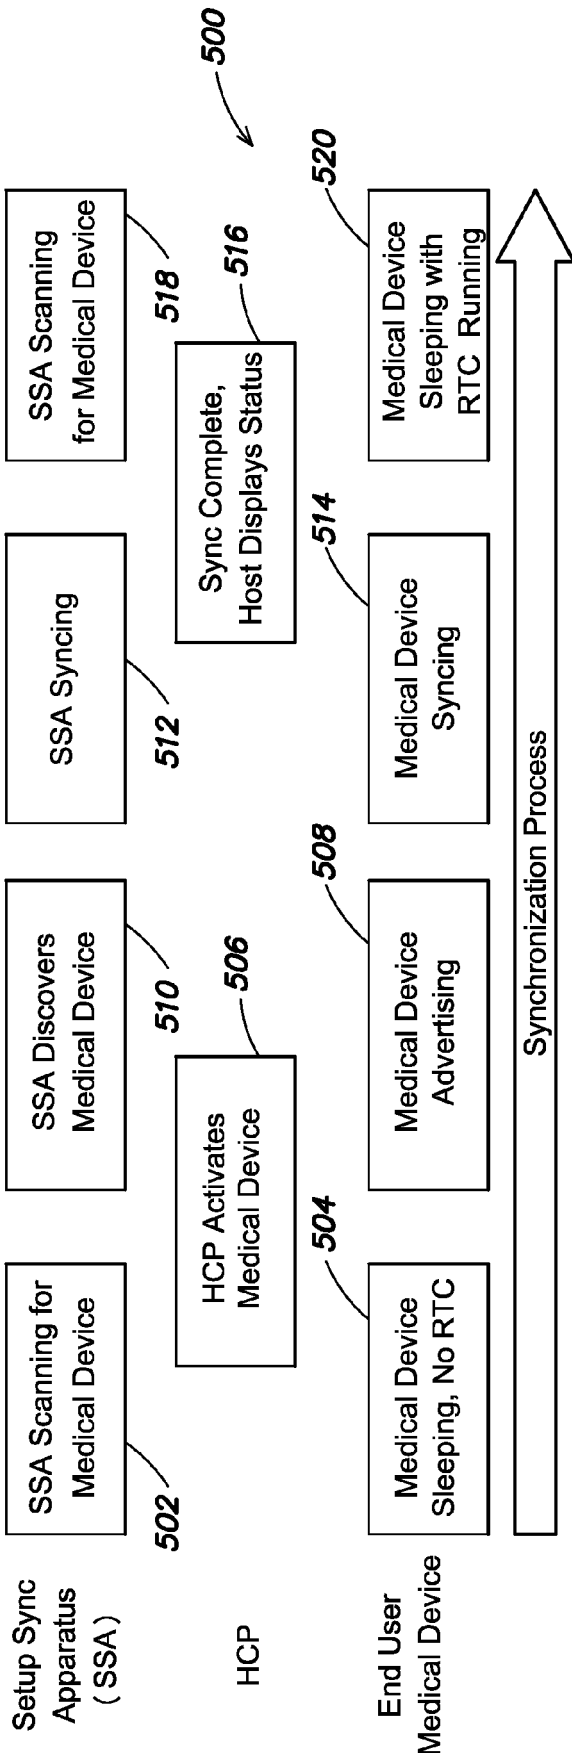


FIG. 5

**FIG. 6**

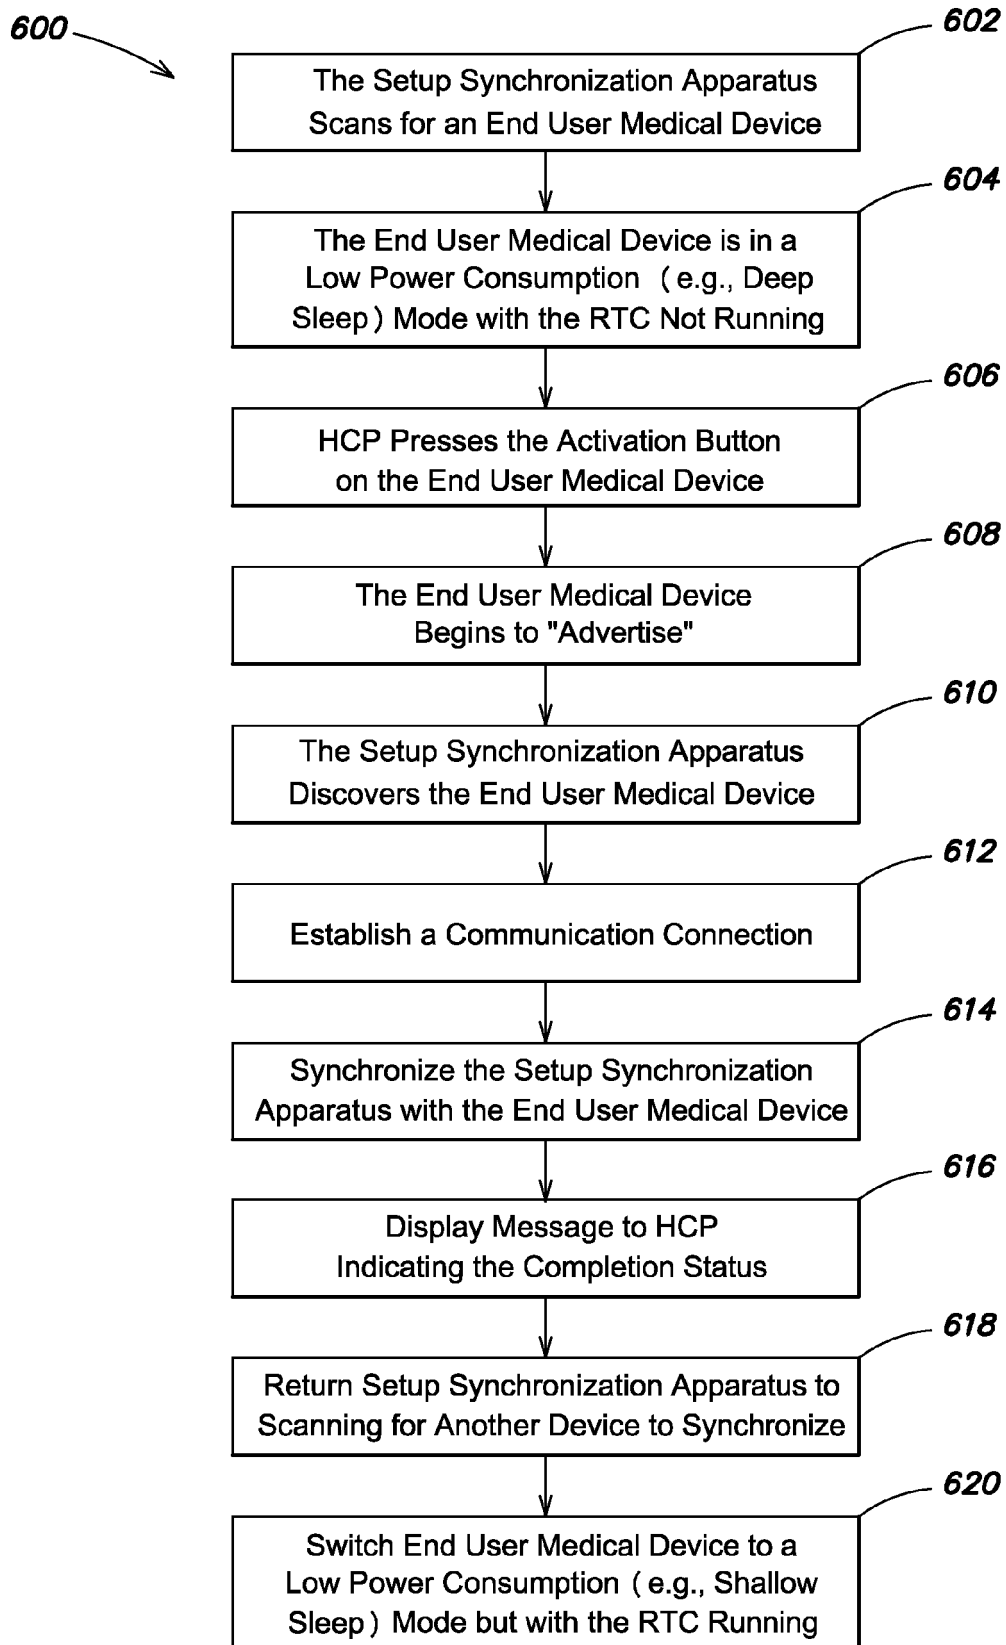

EUROPEAN SEARCH REPORT

Application Number
EP 20 20 4860

5

10

15

20

25

30

35

40

45

50

55

DOCUMENTS CONSIDERED TO BE RELEVANT			
Category	Citation of document with indication, where appropriate, of relevant passages	Relevant to claim	CLASSIFICATION OF THE APPLICATION (IPC)
A	US 2006/106433 A1 (MAZAR SCOTT T [US] ET AL MAZAR SCOTT THOMAS [US] ET AL) 18 May 2006 (2006-05-18) * paragraphs [0040], [0044]; figures 2,3 *	1-15	INV. A61B5/00 A61B5/145
A	US 2011/256024 A1 (COLE JEAN-PIERRE [US] ET AL) 20 October 2011 (2011-10-20) * paragraph [0100] *	1-15	
A	US 6 674 821 B1 (MEJYR SVEN [SE]) 6 January 2004 (2004-01-06) * abstract *	1,10	
			TECHNICAL FIELDS SEARCHED (IPC)
			A61B G06F
The present search report has been drawn up for all claims			
Place of search Berlin		Date of completion of the search 18 February 2021	Examiner Clevorn, Jens
CATEGORY OF CITED DOCUMENTS X : particularly relevant if taken alone Y : particularly relevant if combined with another document of the same category A : technological background O : non-written disclosure P : intermediate document T : theory or principle underlying the invention E : earlier patent document, but published on, or after the filing date D : document cited in the application L : document cited for other reasons & : member of the same patent family, corresponding document			

EPO FORM 1503 03.82 (P04C01)

**ANNEX TO THE EUROPEAN SEARCH REPORT
ON EUROPEAN PATENT APPLICATION NO.**

EP 20 20 4860

5

This annex lists the patent family members relating to the patent documents cited in the above-mentioned European search report.
The members are as contained in the European Patent Office EDP file on
The European Patent Office is in no way liable for these particulars which are merely given for the purpose of information.

18-02-2021

10

15

20

25

30

35

40

45

50

55

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
US 2006106433 A1	18-05-2006	AU 2003299967 A1	29-07-2004
		EP 1578261 A2	28-09-2005
		JP 2006512165 A	13-04-2006
		US 2004127958 A1	01-07-2004
		US 2006106433 A1	18-05-2006
		WO 2004060043 A2	22-07-2004

US 2011256024 A1	20-10-2011	NONE	

US 6674821 B1	06-01-2004	AU 2138200 A	24-07-2000
		CN 1348558 A	08-05-2002
		DE 19983862 T1	28-02-2002
		JP 2002534731 A	15-10-2002
		US 6674821 B1	06-01-2004
		WO 0041057 A2	13-07-2000

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- US 61926215 [0001]