



(12) **EUROPEAN PATENT APPLICATION**

(43) Date of publication:
27.03.2024 Bulletin 2024/13

(51) International Patent Classification (IPC):
A61J 3/00^(2006.01)

(21) Application number: **24156596.9**

(52) Cooperative Patent Classification (CPC):
A61J 3/002; A61J 1/2089

(22) Date of filing: **23.03.2018**

(84) Designated Contracting States:
AL AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO PL PT RO RS SE SI SK SM TR

- **FRAUSTO, Tomas**
Walnut, 91789 (US)
- **FERDAWS, Dereck S.**
Corona, 92883 (US)

(30) Priority: **24.03.2017 US 201762476692 P**

(74) Representative: **Epping - Hermann - Fischer**
Patentanwalts-gesellschaft mbH
Schloßschmidstraße 5
80639 München (DE)

(62) Document number(s) of the earlier application(s) in accordance with Art. 76 EPC:
18716850.5 / 3 600 212

(71) Applicant: **Carefusion 303 Inc.**
San Diego, California 92130 (US)

Remarks:

This application was filed on 08.02.2024 as a divisional application to the application mentioned under INID code 62.

(72) Inventors:
• **ODA, Todd**
Torrance, 90504 (US)

(54) **DRY DISCONNECT CARTRIDGE AND DUAL LUMEN NEEDLE FOR AUTOMATIC DRUG COMPOUNDER**

(57) Various aspects of the subject disclosure relate to a compounder system having a cartridge that includes fluid pathways controllable by valves of the cartridge. A pump component within the cartridge is actuable to move fluid through the controllable fluid pathways. The cartridge includes a needle extending from a cartridge body and fluidly coupled to at least one of the controllable fluid pathways. The cartridge includes a vacuum bellows that surrounds the needle when the bellows is in an extended configuration. The vacuum bellows is compressible to expose the needle and generates a vacuum condition within the bellows when the bellows is extended from a compressed configuration to the extended configuration. The needle may be a dual-lumen plastic needle.

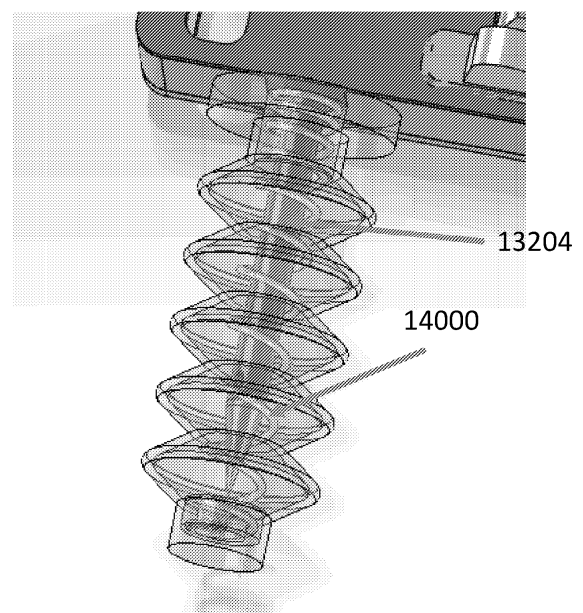


FIG. 40

Description

CROSS-REFERENCE TO RELATED APPLICATIONS

[0001] The present application claims priority to U.S. Provisional Patent Application Serial No. 62/476,692 entitled "Automatic Drug Compounder," filed on March 24, 2017, the disclosure of which is hereby incorporated by reference in its entirety for all purposes.

TECHNICAL FIELD

[0002] The present disclosure generally relates to an apparatus that reconstitutes, mixes, and delivers a drug from a vial to a receiving container. Specifically, the present disclosure relates to dry disconnect features of a closed system automatic drug compounder.

BACKGROUND

[0003] Pharmaceutical compounding is the practice of creating a specific pharmaceutical product to fit the unique need of a patient. In practice, compounding is typically performed by a pharmacist, tech or a nurse who combines the appropriate ingredients using various tools. One common form of compounding comprises the combination of a powdered drug formulation with a specific diluent to create a suspended pharmaceutical composition. These types of compositions are commonly used in intravenous/parenteral medications. It is vital that the pharmaceuticals and diluents are maintained in a sterile state during the compounding process, and there exists a need for automating the process while maintaining the proper mixing characteristics (i.e., certain pharmaceuticals must be agitated in specific ways so that the pharmaceutical is properly mixed into solution but the solution is not frothed and air bubbles are not created). There exists a need for a compounding system that is easy to use, may be used frequently, efficiently, is reliable, and reduces user error.

SUMMARY

[0004] A compounder system may pump diluent from a diluent container to a vial containing a drug, and then pump the reconstituted drug to a receiving container. In order to ensure each medication is correctly and safely reconstituted and moved to the receiving container without mixing of medications or leakage, a disposable cartridge is provided that couples the diluent container and the receiving container to the vial and includes fluid pathways controllable by valves of the cartridge for pumping fluids to and from the vial and the container. A pump component within the cartridge is actuable to move fluid through the controllable fluid pathways.

[0005] In order to fluidly couple the one or more of the controllable fluid pathways to the vial, the cartridge includes a needle extending from a cartridge body and flu-

idly coupled to at least one of the controllable fluid pathways. To help ensure a dry disconnect, the cartridge includes a bellows that surrounds needle. The bellows is compressible to expose the needle for insertion into the vial and generates a vacuum condition within the bellows when the bellows is extended from a compressed configuration to an extended configuration. The needle may be a dual-lumen plastic needle.

[0006] In accordance with various aspects of the disclosure, a compounder system is provided that includes a cartridge having a plurality of controllable fluid pathways fluidly coupled to at least one diluent port and a receiving container port, a pump component actuable to pump a fluid within the plurality of controllable fluid pathways, and a needle configured to couple the plurality of controllable fluid pathways to a vial containing a drug. The cartridge also includes a bellows configured to surround the needle in an extended configuration and to be compressed to allow the needle to extend from the bellows into the vial.

[0007] In accordance with other aspects of the disclosure, a compounder system is provided that includes a cartridge having a plurality of controllable fluid pathways fluidly coupled to at least one diluent port and a receiving container port, a pump member actuable to pump a fluid within the plurality of controllable fluid pathways, and a needle configured to couple the plurality of controllable fluid pathways to a vial containing a drug, wherein the needle comprises a dual-lumen plastic needle.

[0008] In accordance with other aspects of the disclosure, a method is provided that includes coupling a cartridge to a pump head of a compounder system, the cartridge having a body enclosing a plurality of fluid pathways, a needle extending from the body and having a lumen fluidly coupled to at least one of the fluid pathways, and a bellows forming a cavity within which the needle is disposed; and extending the needle into a vial by compressing the bellows with the vial.

BRIEF DESCRIPTION OF THE DRAWINGS

[0009] The accompanying drawings, which are included to provide further understanding and are incorporated in and constitute a part of this specification, illustrate disclosed embodiments and together with the description serve to explain the principles of the disclosed embodiments. In the drawings:

FIG. 1 illustrates a front perspective view of an example of an exemplary embodiment of a compounding system in accordance with aspects of the present disclosure.

FIG. 2 illustrates a front perspective view of the compounding system of FIG. 1 with a transparent housing in accordance with aspects of the present disclosure.

FIG. 3 illustrates a side view of the compounding system of FIG. 1 with the housing removed in accordance with aspects of the present disclosure.

FIG. 4 illustrates a perspective view of an exemplary embodiment of a pump drive mechanism in accordance with aspects of the present disclosure. 5

FIG. 5 illustrates an exploded view of the pump drive mechanism of FIG. 4 in accordance with aspects of the present disclosure. 10

FIG. 6 illustrates a perspective view of a pump head assembly with an exemplary embodiment of a gripping system and vial puck in accordance with aspects of the present disclosure. 15

FIG. 7 illustrates a perspective view of the pump head assembly, gripping system and vial puck of FIG. 6 in accordance with aspects of the present disclosure. 20

FIG. 8 is a flow chart illustrating an exemplary embodiment of the steps of a process in accordance with aspects of the present disclosure. 25

FIG. 9 illustrates a perspective view of an exemplary embodiment of a cartridge in accordance with aspects of the present disclosure. 30

FIG. 10 illustrates a perspective view of an exemplary embodiment of a carousel with a cover in accordance with aspects of the present disclosure.

FIG. 11 illustrates a front perspective view of another exemplary embodiment of a compounding system in accordance with aspects of the present disclosure. 35

FIG. 12 illustrates a front perspective view of the compounding system of FIG. 11 with portions of the housing removed in accordance with aspects of the present disclosure. 40

FIG. 13 illustrates a rear perspective view of the compounding system of FIG. 11 with portions of the housing removed in accordance with aspects of the present disclosure. 45

FIG. 14 illustrates a perspective view of the compounding system of FIG. 11 with various components shown in enlarged views for clarity in accordance with aspects of the present disclosure. 50

FIG. 15 illustrates a perspective view of the cartridge of FIG. 9 in accordance with aspects of the present disclosure. 55

FIG. 16 illustrates a perspective view of the cartridge

of FIG. 9 with a transparent bezel in accordance with aspects of the present disclosure.

FIG. 17 illustrates a perspective view of an exemplary embodiment of a cartridge with a backpack attachment in accordance with aspects of the present disclosure.

FIG. 18 illustrates a perspective view of the cartridge of FIG. 17 with a transparent backpack attachment in accordance with aspects of the present disclosure.

FIG. 19 illustrates an exploded perspective view of another embodiment of a pump cartridge in accordance with aspects of the present disclosure.

FIG. 20A illustrates a rear plan view of the cartridge of FIG. 19 in accordance with aspects of the present disclosure.

FIG. 20B illustrates a front plan view of the cartridge of FIG. 19 in accordance with aspects of the present disclosure.

FIG. 21 illustrates a cross-sectional perspective view of the cartridge of FIG. 19 with an attached backpack in accordance with aspects of the present disclosure.

FIG. 22 illustrates a cross-sectional side view of the cartridge of FIG. 19 in accordance with aspects of the present disclosure.

FIG. 23 illustrates the cartridge of FIG. 19 showing the valves and fluid flow paths in accordance with aspects of the present disclosure.

FIG. 24 illustrates the cartridge of FIG. 19 showing a valve configuration for a diluent to receiving container fluid path in accordance with aspects of the present disclosure.

FIG. 25 illustrates the cartridge of FIG. 19 showing a valve configuration for a reconstitution fluid path through in accordance with aspects of the present disclosure.

FIG. 26 illustrates the cartridge of FIG. 19 showing a valve configuration for a compounding fluid path from in accordance with aspects of the present disclosure.

FIG. 27 illustrates the cartridge of FIG. 19 showing a valve configuration for an air removal fluid path in accordance with aspects of the present disclosure.

FIG. 28 is a chart showing the positioning of certain valves in accordance with aspects of the present disclosure.

FIG. 29A illustrates a cross-sectional side view of the cartridge of FIG. 19 showing a plurality of ports in accordance with aspects of the present disclosure.

FIG. 29B illustrates a cross-sectional side view of a portion of a diluent manifold having a needle that may interface with one of the ports of FIG. 29A in accordance with aspects of the present disclosure.

FIG. 29C illustrates a cross-sectional side view of a portion of the cartridge of FIG. 19 showing port seals formed by a plurality of sealing members in accordance with aspects of the present disclosure.

FIG. 29D illustrates a cross-sectional side view of the portion of the manifold of FIG. 29B compressed against the portion of the cartridge of FIG. 29C in accordance with aspects of the present disclosure.

FIG. 30 illustrates a cross-sectional perspective view of the cartridge disposed adjacent a vial in accordance with aspects of the present disclosure.

FIG. 31 illustrates a cross-sectional side view of a portion of the cartridge of FIG. 19 in the vicinity of a dual lumen needle in accordance with aspects of the present disclosure.

FIG. 32 illustrates a cross-sectional side view of a vial puck having a hydroscopic member in accordance with aspects of the present disclosure.

FIG. 33 illustrates another cross-sectional side view of a vial puck having a hydroscopic member in accordance with aspects of the present disclosure.

FIG. 34 illustrates a partially transparent side view of a vial puck having a hydroscopic member in accordance with aspects of the present disclosure.

FIGS. 35A and 35B illustrate cross-sectional perspective views of a vial puck having a hydroscopic member in accordance with aspects of the present disclosure.

FIG. 36 illustrates another cross-sectional side view of a vial puck having a hydroscopic member in accordance with aspects of the present disclosure.

FIG. 37 illustrates another cross-sectional side view of a vial puck having a hydroscopic member in accordance with aspects of the present disclosure.

FIG. 38 illustrates a perspective view of a cartridge having a bellows in accordance with aspects of the present disclosure.

FIG. 39 illustrates a partially transparent side view

of a portion of a cartridge having a bellows in accordance with aspects of the present disclosure.

FIG. 40 illustrates a partially transparent perspective view of a portion of a cartridge having a bellows in accordance with aspects of the present disclosure.

FIG. 41 illustrates a perspective view of a portion of a cartridge having a bellows in accordance with aspects of the present disclosure.

FIG. 42 illustrates a cross-sectional side view of a portion of a cartridge having a bellows in accordance with aspects of the present disclosure.

FIG. 43 illustrates another cross-sectional side view of a portion of a cartridge having a bellows in accordance with aspects of the present disclosure.

FIG. 44 illustrates a partially transparent side view of a portion of dual-lumen needle having a vertically separated fluid pathway and vent pathway in accordance with aspects of the present disclosure.

FIG. 45 illustrates a cross-sectional side view of the needle of FIG. 44 in accordance with aspects of the present disclosure.

FIG. 46 illustrates a cross-sectional perspective view of the needle of FIG. 44 in accordance with aspects of the present disclosure.

FIG. 47 illustrates a perspective view of the needle of FIG. 44 in accordance with aspects of the present disclosure.

FIG. 48 illustrates another perspective view of the needle of FIG. 44 in accordance with aspects of the present disclosure.

FIG. 49 illustrates another perspective view of the needle of FIG. 44 in accordance with aspects of the present disclosure.

FIG. 50 illustrates a top view of the needle of FIG. 44 in accordance with aspects of the present disclosure.

FIG. 51 illustrates a side view of portion of a compounder system including a vial puck having a cannula in accordance with aspects of the present disclosure.

FIG. 52 illustrates a perspective view of the portion of the compounder system of FIG. 51 in accordance with aspects of the present disclosure.

FIGS. 53 and 54 illustrate side and cross-sectional

side views of a cannula of a vial puck in accordance with aspects of the present disclosure.

FIG. 55 illustrates a partially transparent view of a vial puck, attached to a vial, and having a cannula in accordance with aspects of the present disclosure.

FIG. 56 illustrates a partially transparent view of the vial puck of FIG. 55 with the cannula extended in accordance with aspects of the present disclosure.

FIG. 57 illustrates a perspective view of the vial puck of FIG. 55 in accordance with aspects of the present disclosure.

FIG. 58 illustrates a perspective view of the vial puck of FIG. 56 in accordance with aspects of the present disclosure.

FIG. 59 illustrates a partially transparent side view of portion of a compounder system including a vial puck having a cannula in accordance with aspects of the present disclosure.

FIG. 60 illustrates a partially transparent side view of portion of a compounder system including a cartridge coupled to a vial puck having a cannula in accordance with aspects of the present disclosure.

FIG. 61 illustrates a side view of portion of a compounder system including a cartridge having a protrusion, a needleless fluid port, and a needleless vent port in accordance with aspects of the present disclosure.

FIG. 62 illustrates a side view of portion of a compounder system including a vial puck having a cannula and a vent in accordance with aspects of the present disclosure.

FIG. 63 illustrates a side view of portion of a compounder system including a vial puck having a cannula and a check valve in accordance with aspects of the present disclosure.

FIG. 64 illustrates a perspective view of a dry disconnect shuttle valve in accordance with aspects of the present disclosure.

FIG. 65 illustrates a cross-sectional view of the dry disconnect shuttle valve of FIG. 64 in accordance with aspects of the present disclosure.

FIG. 66 illustrates another cross-sectional view of the dry disconnect shuttle valve of FIG. 64 in accordance with aspects of the present disclosure.

FIG. 67 illustrates a cross-sectional view of the dry

disconnect shuttle valve of FIG. 64 in a fluidly coupled configuration in accordance with aspects of the present disclosure.

FIG. 68 illustrates another cross-sectional view of the dry disconnect shuttle valve of FIG. 64 in accordance with aspects of the present disclosure.

FIG. 69 illustrates a partially transparent perspective view of a connector having an inline filter in accordance with aspects of the present disclosure.

FIG. 70 illustrates a perspective view of a connector having an inline filter in accordance with aspects of the present disclosure.

FIG. 71 illustrates a perspective view of a portion of a syringe pump in accordance with aspects of the present disclosure.

FIG. 72 illustrates another perspective view of a portion of a syringe pump in accordance with aspects of the present disclosure.

DETAILED DESCRIPTION

[0010] The detailed description set forth below describes various configurations of the subject technology and is not intended to represent the only configurations in which the subject technology may be practiced. The detailed description includes specific details for the purpose of providing a thorough understanding of the subject technology. Accordingly, dimensions may be provided in regard to certain aspects as non-limiting examples. However, it will be apparent to those skilled in the art that the subject technology may be practiced without these specific details. In some instances, well-known structures and components are shown in block diagram form in order to avoid obscuring the concepts of the subject technology.

[0011] It is to be understood that the present disclosure includes examples of the subject technology and does not limit the scope of the appended claims. Various aspects of the subject technology will now be disclosed according to particular but non-limiting examples. Various embodiments described in the present disclosure may be carried out in different ways and variations, and in accordance with a desired application or implementation.

[0012] The present system comprises multiple features and technologies that in conjunction form a compounding system that can efficiently reconstitute pharmaceuticals in a sterile environment and deliver the compounded pharmaceutical to a delivery bag for use on a patient.

[0013] Figure 1 illustrates a compounder system 10 according to an embodiment. Figure 2 illustrates the system 10 with a transparent outer housing 12 and Figure

3 illustrates the system with the housing removed. The system comprises a carousel assembly 14 that contains up to 10 individual cartridges 16. The carousel 14 can hold more or less cartridges 16 if desired. The cartridges 16 are disposable and provide unique fluid paths between a vial 18 containing a powdered drug (or concentrated liquid drug), multiple diluents, and a receiving container. The cartridges 16 may, if desired, also provide a fluid path to a vapor waste container. However, in other embodiments, filtered or unfiltered non-toxic waste may be vented from the compounder to the environment reducing or eliminating the need for a waste port. Each cartridge contains a piston pump and valves that control the fluid intake, outtake, and fluid path selection during the steps of the compounding process as the fluid moves through the cartridge and into a receiving container.

[0014] The carousel assembly 14 is mounted on the apparatus such that it can rotate to bring different cartridges 16 into alignment with the pump drive mechanism 20. The carousel 14 is typically enclosed within a housing 12 that can be opened in order to replace the carousel 14 with a new carousel 14 after removing a used one. As illustrated, the carousel 14 can contain up to 10 cartridges 16, allowing a particular carousel to be used up to 10 times. In this configuration, each carousel assembly can support, for example, 10 to 100 receiving containers, depending on the type of compounding to be performed. For example, for hazardous drug compounding, a carousel assembly can support compounding to ten receiving containers. In another example, for non-hazardous drug compounding such as antibiotic or pain medication compounding, a carousel assembly can support compounding to 100 receiving containers. The housing 12 also includes a star wheel 22 positioned underneath the carousel 14. The star wheel 22 rotates vials 18 of pharmaceuticals into position either in concert with, or separate from, the specific cartridges 16 on the carousel 14. The housing 12 may also include an opening 24 for loading the vials 18 into position on the star wheel 22.

[0015] Each one of the cartridges 16 in the carousel 14 is a disposable unit that includes multiple pathways for the diluent and vapor waste. These pathways will be described in detail with reference to, for example, Figures 39 et seq. Each cartridge 16 is a small, single disposable unit that may also include a "backpack" in which a tube for connection to the receiving container (e.g., an IV bag, a syringe, or an elastomeric bag) may be maintained. Each cartridge 16 also may include a pumping mechanism such as a piston pump for moving fluid and vapor through the cartridge 16 as well as a dual lumen needle in a housing that can pierce a vial puck 26 on top of a vial 18 once the vial 18 has been moved into position by the pump drive mechanism 20. For example, the needle may pierce the vial puck 26 via the compressive action of the vial puck 26, which is moved towards the needle. Each cartridge 16 also includes a plurality of ports designed to match up with the needles of a plurality of diluent manifolds. Each cartridge 16 also includes openings to

receive mounting posts and a locking bayonet from the pump head assembly 28. Although a locking bayonet is described herein as an example, other locking mechanisms may be used to retrieve and lock a cartridge to the pump head (e.g., grippers, clamps, or the like may extend from the pump head). Each cartridge 16 also includes openings allowing valve actuators from the pump motor mechanism to interact with the valves on each cartridge 16.

[0016] Adjacent the housing 12 that holds the vials 18 and the carousel 14 is an apparatus 30 for holding at least one container 32, such as an IV bag 32 as shown in the figures. The IV bag 32 typically has two ports such as ports 34 and 36. For example, in one implementation, port 34 is an intake port 34 and port 36 is an outlet port 36. Although this implementation is sometimes discussed herein as an example, either of ports 34 and 36 may be implemented as an input and/or outlet port for container 32. For example, in another implementation, an inlet 34 for receiving a connector at the end of tubing 38 may be provided on the outlet port 36. In the embodiment shown, the IV bag 32 hangs from the holding apparatus 30, which, in one embodiment is a post with a hook as illustrated in FIGS. 1-3. As discussed in further detail hereinafter, one or more of the hooks for hanging containers such as diluent containers, receiving containers, or waste containers may be provided with a weight sensor such as a load cell that detects and monitors the weight of a hung container. The holding apparatus 30 can take any other form necessary to position the IV bag 32 or other pharmaceutical container. Once the IV bag 32 is positioned on the holding apparatus 30, a first tube 38 (a portion of which is shown in FIG. 1) is connected from a cartridge 16 on the carousel 14 to the inlet 34 of the IV bag 32. For example, the first tube may be housed in a backpack attached to the cartridge and extended from within the backpack (e.g., by an operator or automatically) to reach the IV bag 32. A connector 37 such as a Texium® connector may be provided on the end of tube 38 for connecting to inlet 34 of receiving container 32.

[0017] On the opposite side of the compounder 10 is an array of holding apparatuses 40 for holding multiple IV bags 32 or other containers. In the illustrated version of the compounder 10, five IV bags 42, 44 are pictured. Three of these bags 42 may contain diluents, such as saline, D5W or sterile water, although any diluent known in the art may be utilized. An additional bag in the array may be an empty vapor waste bag 44 for collecting waste such as potentially hazardous or toxic vapor waste from the mixing process. An additional bag 44 may be a liquid waste bag. The liquid waste bag may be configured to receive non-toxic liquid waste such as saline from a receiving container. As discussed in further detail hereinafter, liquid waste may be pumped to the waste bag via dedicated tubing using a mechanical pump. In operation, diluent lines and a vapor waste line from the corresponding containers 42 and 44 may each be connected to a

cartridge 16 through a disposable manifold.

[0018] The compounding system 10 also includes a specialized vial puck 26 designed to attach to multiple types of vials 18. In operation, the vial puck 26 is placed on top of the vial 18 containing the drug in need of re-constitution. Once the vial puck 26 is in place, the vial 18 is loaded into the star wheel 22 of the compounder 10. Mating features on the vial puck 26 provide proper alignment both while the vial puck 26 is in the star wheel 22 and when the vial puck 26 is later rotated into position so that the compounder 10 can remove it from the star wheel 22 for further processing.

[0019] The pump drive mechanism 20 is illustrated in Figure 4, and in an exploded view in Figure 5, according to an embodiment. In the embodiment shown in FIGS. 4 and 5, the pump drive mechanism 20 comprises a multitude of sections. At one end of the pump drive mechanism 20 is the rotation housing 46, which holds the drive electronics and includes locking flanges 94 on its housing 96 for flexible tubing 50 which may run from one or more diluent containers and/or waste containers to one or more corresponding manifolds. The rotation housing 46 is capable of rotating around its axis to rotate the rest of the pump drive mechanism 20. The rotation housing 46 includes bearing ribs 52 on its ends, which allow it to rotate. For example, the pump drive mechanism may be configured to rotate through any suitable angle such as up to and including 180°, or more than 180°.

[0020] The compounder system also includes a diluent magazine that mounts in a slot 60 located on the side of the pump drive mechanism. The diluent magazine may be a disposable piece configured to receive any number of individual diluent manifolds operable as diluent ports. The diluent manifolds may be modular so they can easily and removably connect to each other, the magazine, and/or connect to the pump drive mechanism 20.

[0021] Pump drive mechanism 20 also includes pump head assembly 28. The pump head assembly 28 includes the vial grasping arms 76, the vial lift 78, the pump cartridge grasp 80, the pump piston eccentric drive shaft 82 with drive pin 222, the valve actuation mechanisms 84, as well as the motors that allow the pump drive mechanism 20 to move forward and back and to rotate in order to mix the pharmaceutical in the vial 18 once the diluent has been added to it. The compounder 10 may also include an input screen 86 such as a touch screen 86 as shown in the figures to provide data entry by the user and notifications, instructions, and feedback to the user.

[0022] The operation of the compounder system 10 will now be generally described in the flowchart illustrated at Figure 8, according to an embodiment. In the first step 88, a user inserts a new diluent manifold magazine having a plurality of manifolds (e.g., diluent manifolds and waste manifolds) into the slot 60 on the side of the pump head assembly 28. Manifolds may be loaded into the magazine before or after installing the magazine in the slot 60. The manifolds maintain needles inside the housing of the manifold until the cartridge 16 is later locked in

place. The magazine may contain any number of diluent manifolds and vapor waste manifolds. In one illustrative system, there may be three diluent manifolds and one vapor waste manifold. In the next step 92, diluent tubing is connected to corresponding diluent bags. The tubes may be routed through locking flanges on a surface (e.g., the front surface) of the compounder frame to hold them in place. For example, in the illustrated embodiment of FIG. 11, the tubes are held in place with locking flanges 2402 on the frame of the compounder. Alternatively, other types of clips or locking mechanisms known in the art may be used to hold the tubes securely in place. In the illustrated embodiment of FIG. 4, the additional flanges 94 positioned on the outside housing 96 of the pump drive mechanism 20 are provided for securing internal wiring of the compounder. In the next step 98, waste tubing may be connected to the vapor waste bag 44. In other embodiments, tubing may be pre-coupled between the manifolds and associated containers such as diluent containers and/or waste containers and the operations of steps 92 and 98 may be omitted.

[0023] If desired, in the next step 100, a new carousel 14 may be loaded into a carousel mounting station such as a carousel hub of the compounder system. The carousel 14 may contain any number of disposable cartridges 16 arranged in a generally circular array. In the next step 110, a vial puck 26 is attached to the top of a vial 18 of a powdered or liquid pharmaceutical for reconstitution and the vial 18 is loaded into the star wheel 22 under the carousel 14 in the next step 112. Step 110 may include loading multiple vials 18 into multiple vial puck recesses in star wheel 22. After one or more vials are loaded into the star wheel, the vials are rotated into position to enable and initiate scanning of the vial label of each vial. In one embodiment, the user will be allowed to load vials into the star wheel until all vial slots are occupied with vials before the scanning is initiated. A sensor may be provided that detects the loading of each vial after which a next vial puck recess is rotated into the loading position for the user. Allowing the user to load all vials into the star wheel prior to scanning of the vial labels helps increase the efficiency of compounding. However, in other implementations, scanning of vial labels may be performed after each vial is loaded or after a subset of vials is loaded. Following these setup steps, the next step 114 is for a user to select the appropriate dosage on the input screen.

[0024] After the selection on the input screen 86, the compounder 10 begins operation 116. The star wheel 22 rotates the vial into alignment 118 with the vial grasping calipers 76 of the pump head assembly 28. The vial puck 26 includes, for example, gears that interface with gears coupled to a rotational motor that allow the vial 18 to rotate 120 so that a scanner (e.g., a bar code scanner or one or more cameras) can scan 122 a label on the vial 18. The scanner or camera (and associated processing circuitry) may determine a lot number and an expiration date for the vial. The lot number and expiration date may

be compared with other information such as the current date and/or recall or other instructions associated with the lot number. Once the vial 18 is scanned and aligned, in the next step 124 the pump drive mechanism 20 moves forward into position to grip the vial 18 with the calipers 76. The forward movement also brings the mounting posts 130 and locking bayonet 128 on the front of the pump head assembly 28 into matching alignment with corresponding openings on a cartridge 16. In the next step 126 the cartridge 16 is locked in place on the pump head assembly 28 with the locking bayonet 128 and the calipers 76 grip 132 the vial puck 26 on the top of the vial 18. The calipers 76 then remove 132 the vial 18 from the star wheel 22 by moving backward, while at the same time pulling 134 the cartridge 16 off of the carousel 14.

[0025] In some embodiments, the cartridge 16 includes a backpack that includes a coiled tube. In this embodiment, in step 136 the pump drive mechanism 20 tilts the cartridge 16 toward the user to expose the end of the tube and prompts 138 the user to pull the tube out of the backpack and connect it to the receiving bag 32. In an alternative embodiment, the tube 38 is exposed on the side of the carousel 14 once the cartridge 16 is pulled away from the carousel 14. In another alternative embodiment, the tube 38 is automatically pushed out (e.g., out of the backpack) thus allowing the user to grab onto the connector located at the end of the tube and connect to the receiving container. The system prompts 138 the user to pull the tube out from the carousel 14 and connect it to the input 34 of the IV bag 32. Once the tube 38 is connected, in step 140 the user may notify the compounding 10 to continue the compounding process by interacting with the input screen 86.

[0026] At step 142, the vial 18 is pulled up towards the cartridge 16 so that one or more needles such as a coaxial dual lumen needle of the cartridge 16 pierce the top of the vial puck 26 and enter the interior of the vial 18. Although the example of FIG. 8 shows engagement of the needle with the vial puck after the user attaches the tube from the cartridge to the receiving container, this is merely illustrative. In another embodiment, steps 138 and 140 may be performed after step 142 such that engagement of the needle with the vial puck occurs before the user attaches the tube from the cartridge to the receiving container.

[0027] Diluent is pumped at step 144 into the vial 18 through the cartridge 16 and a first needle in the proper dosage. If necessary, a second or third diluent may be added to the vial 18 via a second or third diluent manifold attached to the cartridge 16. Simultaneously, vapor waste is pumped 144 out of the vial 18, through a second needle, through the cartridge 16 and the vapor waste manifold, and into the vapor waste bag 44. The valve actuators 84 on the pump head assembly 28 open and close the valves of the cartridge 16 in order to change the fluid flow paths as necessary during the process. Once the diluent is pumped into the vial 18, the pump drive mechanism 20 agitates the vial 18 in the next step

146 by rotating the vial lift 78 up to, for example 180 degrees such that the vial 18 is rotated between right-side-up and upside-down positions. The agitation process may be repeated for as long as necessary, depending on the type of pharmaceutical that is being reconstituted. Moreover, different agitation patterns may be used depending on the type of drugs being reconstituted. For example, for some drugs, rather than rotating by 180 degrees, a combination of forward-backward, and left-right motion of the pump head may be performed to generate a swirling agitation of the vial. A plurality of default agitation patterns for specific drugs or other medical fluids may be included in the drug library stored in (and/or accessible by) the compounding control circuitry. Once the agitation step is complete, the pump drive mechanism rotates the vial to an upside down position or other suitable position and holds it in place. In some embodiments, a fluid such as a diluent already in the receiving container 32 may be pumped (e.g., through the cartridge or via a separate path) into a liquid waste container to allow room in the receiving container for receiving the reconstituted medicine.

[0028] In the next step 148, the valve actuators 84 reorient the valves of the cartridge and the pumping mechanism of the cartridge 16 is activated to pump 150 the reconstituted drug into the receiving bag 32 through the attached tube. Once the drug is pumped into the receiving bag 32, in the next step 152 the pump drive mechanism 20 clears the tube 38 by either pumping filtered air or more diluent through the tube 38 into the receiving bag 32 after another valve adjustment to ensure that all of the reconstituted drug is provided to the receiving bag 32. In some scenarios, a syringe may be used as a receiving container 32. In scenarios in which a syringe is used as the receiving container 32, following delivery of the reconstituted drug to the syringe, a vacuum may be generated in tube 38 by pump drive mechanism 20 to remove any air or other vapors that may have been pushed into the syringe so that, when the syringe is removed from tube 38, the reconstituted drug is ready for delivery to a patient and no air or other unwanted gasses are present in the syringe.

[0029] The system then prompts 154 the user to remove the tube 38 from the receiving container 32. The user may then insert the connector (e.g., a Texium® or SmartSite® connector) into its slot in the backpack or carousel and an optical sensor in the pump head may sense the presence of the connector and automatically retract the tube into either the carousel or the backpack. The tube is pulled back into either the carousel 14 or the backpack, depending on which type of system is in use. In the next step 156, the compounding 10 rotates the vial 18 back into alignment with the star wheel 22 and releases it. The used cartridge 16 may also be replaced on the carousel 14. The used cartridge may be released when a sensor in the pump drive determines that the tube has been replaced in the cartridge (e.g., by sensing the presence of a connector such as a Texium® connector at the

end of the tube in the backpack of the cartridge through a window of the cartridge). The carousel 14 and/or star wheel 22 then may rotate 158 to a new unused cartridge 16 and/or a new unused vial 18 and the process may be replicated for a new drug. In some circumstances (e.g., multiple reconstitutions of the same drug), a single cartridge may be used more than once with more than one vial.

[0030] The cartridges 16 are designed to be disposable, allowing a user to utilize all the cartridges 16 in a given carousel 14 before replacing the carousel 14. After a cartridge 16 is used, the carousel 14 rotates to the next cartridge 16, and the system software updates to note that the cartridge 16 has been used, thus preventing cross-contamination from other reconstituted drugs. Each cartridge 16 is designed to contain all the necessary flow paths, valves, filters and pumps to reconstitute a drug with multiple diluents if necessary, pump the reconstituted drug into the receiving container, pump vapor waste out of the system into a waste container, and perform a final QS step in order to make sure that the proper amount of drug and diluent is present in the receiving container. This complete package is made possible by the specific and unique construction of the cartridge 16, its flow paths, and its valve construction.

[0031] An embodiment of a cartridge 16 is illustrated in Figure 9. As shown in FIG. 9, cartridge 16 may include a cartridge frame 160, a cartridge bezel 164, as well as a piston pump 166, a needle housing 168 and a needle assembly 170. The cartridge frame 160 provides the main support for each cartridge 16 and includes diluent chambers, a vapor waste chamber, a pumping chamber, a hydrophobic vent, an exit port, and/or other features as described hereinafter that can be connected to a tube that connects to the receiving container 32.

[0032] The frame 160 of the cartridge 16 also includes locating features that allow each cartridge 16 to be removably mounted to the pump head assembly 28. These features include, for example, three openings 198 to receive mounting posts 130 from the pump head assembly 28, and a keyhole 210 that allows a locking bayonet 128 to be inserted therein and turned to lock the cartridge 16 to the pump head assembly 28 for removal from the carousel 14. An outlet port extension 220 may be present in some embodiments. The piston pump 166 is mounted within a chamber with a rod 194 positioned within a silicone piston boot. Furthermore, the bezel 164 includes openings 228 in which the valves 190 of the sealing membrane are located and be accessed by the valve actuators 84. Moreover, the bezel 164 includes openings 230 that allow a fluid manifold to be connected to the diluent and vapor waste chambers in the cartridge 16. As discussed in further detail hereinafter, bezel 164 may also include an opening that facilitates the detection of a connector (e.g., a Texium® or SmartSite® connector) when the user inserts the connector into the provided slot when compounding is complete. In operation, the needles of the fluid manifold enter through the openings 230 in the bezel

164 and pierce the sealing membrane to gain fluidic access to the diluent and vapor waste chambers defined in the cartridge 16 between the sealing membrane and the cartridge frame 160. Further details of various embodiments of the cartridge 16 will be discussed hereinafter.

[0033] Referring to Figure 10, an exemplary embodiment of a carousel 14 removed from the compounder 10 is illustrated, according to an embodiment. The carousel 14 of FIG. 10 includes an array of ten cartridges 16 in this embodiment, but it should be understood that more or fewer cartridges 16 can be present on the carousel 14, leaving some of the carousel 14 pockets 500 empty, or the frame 510 of the carousel can be designed to have more or fewer cartridge pockets 500. In some implementations, the carousel 14 may also, optionally, include a cover 511 that prevents a user from accessing the tubes coupled to each of the cartridges 16 directly. In these implementations, the cover 511 may be removed if necessary to access the backs of the cartridges 16. In the example implementation of FIG. 10, a connector such as a Texium® attachment 548 is disposed adjacent each cartridge 16, the attachment 548 being attached to the tube 38 that runs from the extension 220 on each cartridge 16.

[0034] FIGS. 11-14 show the compounder 10 according to another embodiment. As shown in FIG. 11, holding apparatus 40 may be implemented as an extended arm providing support for mounting devices for each of containers 42 and 44. Holding apparatus 40 and holding apparatus 30 may each include one or more sensors such as weight sensors configured to provide weight measurements for determining whether an appropriate amount of fluid has been added to or removed from a container or to confirm that fluid is being transferred to and/or from the appropriate container (e.g., that the appropriate diluent is being dispensed). A scanner 2404 may be provided with which each diluent container and/or the receiving container can be scanned before and/or after attachment to compounder 10. As shown in FIG. 11, a carousel cover 2400 and tube management structures 2402 may also be provided on compounder 10 in various embodiments. For example, tubes connected between containers 42 and/or 44 and corresponding manifolds can each be mounted in a groove of tube management structure 2402 to prevent tangling or catching of the tubes during operation of compounder 10.

[0035] An opening may be provided by which vials 18 can be installed in the star wheel. Additionally, an exterior pump 2500 may be provided for pumping non-toxic liquid waste from, for example, receiving container 32 to a waste container 44 (e.g., for pumping a desired amount of saline out of receiving container 32 quickly and without passing the liquid waste through a cartridge and/or other portions of the compounder).

[0036] A fluidics module 2504 may be provided that includes several container mounts which may be used for hanging diluent and waste containers and may include sensor circuitry for sensing when a container has been

hung and/or sensing the weight of the container. In this way, the operation of compounder 10 can be monitored to ensure that the correct diluent contain has been scanned and hung in the correct location and that the waste is being provided in an expected amount to the appropriate waste container.

[0037] As shown in FIG. 12, pump 2500 and display 86 may be mounted to a chassis 2600. Pump drive 20 may be mounted partially within the chassis 2600 with pump head assembly 28 extending from the chassis to a position which allows the pump head assembly to rotate (e.g., to turn over or agitate a vial). Carousel 14 is also shown in FIG. 12 without any cartridges mounted therein so that cartridge mounting recesses 500 can be seen.

[0038] Star wheel 22 (sometimes referred to herein as a vial tray) is shown in FIG. 12 with several empty vial puck recesses 2604. Vial tray 22 may be rotated and an actuating door 2608 may be opened to facilitate loading of vials 18 into the vial puck recesses 2604 in vial tray 22. In some embodiments, door 2608 may be closed before rotation of vial tray 22 to ensure that the operator's fingers are not in danger of injury from the rotating tray. However, this is merely illustrative. In other embodiments a sensor such as sensor 2650 (e.g., a light curtain) may be provided instead of (or in addition to) door 2608 to sense the presence of an operator in the vicinity of tray 22 and prevent rotation of the tray if the operator or any other obstruction is detected.

[0039] Similarly, a lid may be provided for carousel 14 to prevent contamination of cartridges 16 loaded therein, and to prevent injury to an operator due to rotation of the carousel. A lid sensor (not shown) may also be provided to detect the position (e.g., an open position or a closed position) of the lid. Rotation of carousel 14 may be prevented if the lid is not detected in a closed position by the lid sensor.

[0040] Each vial 18 that is inserted may be detected using a sensor such as sensor 2652 (e.g., a load sensor or an optical sensor) when placed in a vial puck recess 2604. When detected, the inserted vial may be moved to a scanning position by rotating vial tray 22 and then the inserted vial 18 may be rotated within its position in vial tray 22 using a vial rotation motor 2602 to allow the vial label to be scanned.

[0041] A reverse perspective view of compounder 10 is shown in FIG. 13 in which scanning components can be seen. In particular, a camera 2700 is mounted in an opening in chassis 2600 and configured to view a vial 18 in a scanning position. Motor 2602 may rotate vial 18 through one or more full rotations so that camera 2700 can capture images of the vial label. In some embodiments, an illumination device 2702 (e.g., a light-emitting diode or other light source) may be provided that illuminates vial 18 for imaging with camera 2700.

[0042] As shown in FIG. 13 one or more gears 2704 coupled to motor 2602 may be provided that engage corresponding gears on a vial puck 26 to which a vial 18 is attached at the scanning position. The vial tray 22 may

be rotated so that the vial puck gears engage the rotation motor gears so that when the motor 2602 is operated the vial 18 is rotated.

[0043] FIG. 13 also shows how a magazine 2706 containing one or more manifolds may be mounted in a recess in pump head assembly 28. A magazine slot in magazine 2706 for the vapor waste manifold may be keyed to prevent accidental connection of a diluent manifold in that slot (or a waste manifold in a diluent slot in the magazine). Other diluent slots in magazine 2706 may have a common geometry and thus any diluent manifold can fit in the magazine diluent slots. One or more manifold sensors such as manifold sensor 2750 (e.g., an optical sensor) may be provided in the manifold recess in pump head assembly 28. Manifold sensor 2750 may be configured to detect the presence (or absence) of a manifold in a manifold recess (slot) in magazine 2706 to ensure that an appropriate manifold (e.g., a diluent manifold or waste manifold) is loaded at the expected position for compounding operations. In this way, the pump head may detect a manifold presence. The pump head and/or manifold sensors may communicate with the diluent load sensors to ensure proper positioning of the diluent manifolds. Various operational components 2708 such as valve actuators, needle actuators, mounting posts, a locking bayonet, and a drive pin can also be seen extended from pump head assembly 28 which are configured to secure and operate a pump cartridge 16.

[0044] Compounder 10 may include additional components such as a chassis base and chassis housing, and an internal electronics assembly. Pump drive 20 may be seated in an opening in the chassis housing that allows pump head assembly 28 to protrude from the chassis housing. Processing circuitry for managing operations of compounder system 10 may be included in the electronics assembly.

[0045] Carousel 14 may be placed onto a carousel hub and rotated by a vial tray and carousel drive assembly operating to rotate the hub to move a selected cartridge in the carousel into position to be retrieved and operated by pump drive 20. The vial tray and carousel drive assembly may include separate drive assemblies for the vial tray and for the carousel such that vial tray 22 and carousel 14 may be rotated independently.

[0046] FIG. 14 shows another perspective view of compounder 10 highlighting the locations of various particular components such as the carousel 14 with cartridges 16 mounted therein, a cartridge 16 having a backpack 2900, a vial puck 26 for mounting vials 18, and pump head assembly 28 with a diluent magazine 2706 containing a plurality of manifolds 2906 in accordance with an embodiment. Further features of compounder 10 will be described hereinafter in connection with FIGS. 15-73 in accordance with various embodiments.

[0047] The cartridges 16 are designed to be disposable, allowing a user to utilize all the cartridges 16 in a given carousel 14 before replacing the carousel 14. After a cartridge 16 is used, the carousel 14 rotates to the next

cartridge 16, and the system software updates to note that the cartridge 16 has been used, thus preventing cross-contamination from other reconstituted drugs. Each cartridge 16 is designed to contain all the necessary flow paths, valves, filters, pistons, and pumps to reconstitute a drug with multiple diluents if necessary, pump the reconstituted drug into the receiving container, pump vapor waste out of the system into a waste container, and perform a final QS step in order to make sure that the proper amount of drug and diluent is present in the receiving container. The amount of diluent pumped into vials for reconstitution and the amount of medication pumped out of vials to the receiving container are controlled by the volumetric piston pump in the cartridge which can be compared against weights obtained by the gravimetric scales (e.g., one or more diluent load cells and a receiving container load cell) of the compounder for quality control. This complete package is made possible by the specific and unique construction of the cartridge 16, its flow paths, and its valve construction.

[0048] Various embodiments of a cartridge 16 are illustrated in FIG. 15-20B. A fully constructed cartridge 16 is shown in Figures 15 and 16 in one embodiment. A cartridge 16 having a tube management structure implemented as a backpack for the cartridge is shown in FIGS. 17 and 18. An exploded version of a cartridge 16 is illustrated in Figure 19 and shows three main portions of the cartridge 16: the cartridge frame 160, the cartridge sealing membrane 162, the cartridge bezel 164, as well as the piston pump 166, the needle housing 168 and the needle assembly 170 according to an embodiment. A fully constructed cartridge 16 is shown in Figures 20A and 20B in one embodiment. Various features of the cartridge of FIGS. 19, 20A, and 20B are shown in FIGS. 21-31.

[0049] As shown in FIG. 15, a front view of the cartridge 16 is illustrated. Cartridge frame 160 provides the main support for each cartridge 16. Piston pump 166 and a cartridge needle housing 168 to hold the needle assembly 170 are provided that can be operated to move liquids and waste vapor to and from vial 18 during reconstitution and filling of receiving container 32. Valves 190 are positioned with respect to various internal flow paths within cartridge 16 for diluents, vapor waste, filtered air, and reconstituted drugs and are operable to modify and control the internal flow paths when desired.

[0050] Frame 160 of the cartridge 16 also includes locating features that allow each cartridge 16 to be removably mounted to the pump head assembly 28. These features include three openings 198 to receive mounting posts 130 from the pump head assembly 28, and a keyhole 210 that allows a locking bayonet 128 to be inserted therein and turned to lock the cartridge 16 to the pump head assembly 28 for removal from the carousel 14.

[0051] The cartridge needle housing 168 extends from the bottom of the cartridge frame 160 and may be designed to be removable by snapping a pair of locking flanges 214 on the needle housing 168 into flange open-

ings 216 in the cartridge frame 160. The cartridge needle housing 168 is designed to prevent accidental user contact with the needle assembly 170 and to maintain the sterility of one or more needles of the needle assembly (see, e.g., needles 316 and 318 of FIG. 31). The needle housing 168 also receives the vial puck 26 in a position to allow the needles to pierce the vial puck 26.

[0052] A sealing membrane may be disposed between frame 160 and bezel 164 to form sealed internal flow paths in cartridge 16 in cooperation with internal features of frame 160 and bezel 164 as described in further detail hereinafter.

[0053] Before describing the various fluid flow paths in the cartridge 16, the operation of the pumping and valve mechanisms will be described with reference to Figures 3, 4, 6 and 7. A piston pump such as piston pump 166 acts as a positive displacement pump that has significant advantages over a traditional peristaltic pump mechanism. First, it has the best rate accuracy and flow continuity regardless of the pump's orientation or environmental conditions. Second, it is able to push an excess of 50 psi into elastomeric pumps. The piston pump 166 may be positioned within the cartridge 16 in a silicone piston pump boot. The pump mechanism is driven by a motor in the pump motor mechanism 20 which rotates an eccentric drive shaft 82 and drive pin 222 on the pump head assembly 28 which controls the movement of the piston 166 as well as the valve actuators 84. In operation, the cartridge 16 is placed on the cartridge grasp 80 on the locating posts 130 and locked in place by the locking bayonet 128. This aligns the valves disposed in openings 228 of bezel 164 with the valve actuators 84 and the eccentric drive shaft 82 and pin 222 with the piston pump 166. The piston 166 is driven by the eccentric drive pin 222. The pin 222 is parallel to but offset from the rotational axis of the drive shaft, which produces sinusoidal motion that is converted to an axial movement of the piston 166.

[0054] The valve actuators 84 are illustrated in Figures 6 and 7, which show the pump head assembly 28 removed from the rest of the pump motor mechanism 20. Each one of the valves in openings 228 has a corresponding valve actuator 84 that is controlled by a geared cam to cause axial movement of the valve actuator 84 into contact with the valve to close the valve and away from the valve to open the valve. In one embodiment, eight valve actuators 84 are provided, one for each valve, and they are aligned with the positions of the valves so they can extend through the openings 228 in the bezel 164 of the cartridge 16 and contact the valves. The valve actuators 84 are software controlled so that they can automatically cause the valves to open and close depending on which internal flow paths within cartridge 16 are to be opened and closed.

[0055] The valve actuators 84 are operated at different times in the pumping cycle depending on the required fluid flow path. The fill portion of the piston 166 starts as the piston rod 194 moves, and the inlet valve is opened and the outlet valve is closed. Other valves will be opened

and closed depending on the necessary fluid flow paths. At the end of the fill portion of the cycle when the piston 166 is at the bottom dead center position, the valve actuation changes to close the inlet and open the outlet valves. At this point, the delivery portion of the cycle starts and the piston 166 moves in the opposite direction. The delivery portion of the cycle ends when the piston 166 reaches the top dead center location, which is the home location. When the piston 166 reaches this position, a new cycle is started.

[0056] The movement of the eccentric drive shaft 82 can be in a clockwise direction under normal conditions when delivering fluid and counter clockwise when pulling fluid. The pump mechanism can be made to pump backwards depending on the required flow path. The drive may be prevented from being inadvertently back driven in either direction by the effects of pressure in the disposable line up to 50 psi.

[0057] An alternative embodiment of the cartridge 16 utilizing a "backpack" to coil the flexible tubing 38 is illustrated in Figures 17 and 18. The backpack 298 is attached to the back of the cartridge frame 160 and one end of the flexible tube 38 is attached to an outlet port on the back of the cartridge frame 16. The backpack 298 comprises a housing 310 and may include a tube control mechanism defined in a chamber that can rotate or otherwise operate to coil the flexible tubing 38. At the opposite end of the tubing from the outlet port is a connector 300 (e.g., an ISO Luer connector such as a Texium® attachment) that a user can pull out of the backpack 298 and attach to the receiving bag 32. In some embodiments, the tubing attached to the connector 300 may be automatically extended from within backpack 298 to facilitate attachment by the user. Upon completion of the filling of the bag 32, the tube control mechanism can draw the flexible tubing 38 back into the backpack 298 and out of the way so that the next cartridge 16 in the carousel 14 can be utilized. Retraction of the flexible tubing may be automatic once the ISO Luer is placed into the opening in the backpack.

[0058] Turning now to FIG. 19, an exploded perspective view of another embodiment of cartridge 16 shows three main portions of the cartridge 16: the cartridge frame 160, the cartridge sealing membrane 162, the cartridge bezel 164, as well as the piston pump 166, the needle housing 168 and the needle assembly 170. In the example of FIG. 19, cartridge bezel 164 includes an additional opening 3022 to provide access to a pressure dome formed on membrane 162 to allow sensing of pressure in the fluid pathways of cartridge 16. An air-in-line sensor fitment 3000 is also provided that is configured to mate with an air-in-line (AIL) sensor in the compound-

[0059] In order to control the flow of gasses such as vapor waste and sterile air within the cartridge, cartridge 16 may be provided with gas flow control structures such as an air filter 3006 and one or more check valve discs 3004 that mount to frame 160 with a check valve cover 3002. Air filter 3006, check valve discs 3004, and check

valve cover 3002 may cooperate to allow vapor waste to flow in only one direction from the vial to the waste port and to allow sterile (filtered) air to flow in only one direction into the cartridge from a vent adjacent the air filter to the vial. In this way, unwanted vapor waste may be prevented from flowing out of the pump cartridge and may be instead guided to a vapor waste container.

[0060] As shown in FIG. 19, piston 166 may include a piston boot 3007 that, for example, provides one or more moveable seals (e.g., two moveable seals) for controlling the volume of a pump chamber when piston 166 is actuated. FIG. 19 also shows various structures for control of another embodiment of needle housing 168 in which needle assembly 170 includes a dual lumen needle with a first needle overmold 317A, a second needle overmold 317B, a needle spring 3014, and a needle membrane 3008. An opening 3020 in bezel 164 may be provided that aligns with a corresponding opening 3021 in frame 160 to allow a view through cartridge 16 (e.g., by a sensor of the pump drive mechanism) into a backpack that is mounted to cartridge 16 as will be described in further detail hereinafter. A protrusion 3016 formed on a top side of cartridge frame 160 may be provided as a mounting structure for the backpack.

[0061] FIGS. 20A and 20B show assembled views of the cartridge embodiment shown in FIG. 67 from the bezel side and frame side respectively in which an opening 3120 (formed by openings 3020 and 3021 of FIG. 19) that allows a view completely through cartridge 16 can be seen. As shown in FIG. 20A, in some embodiments, cartridge 16 may include four diluent and waste ports 3100 and a pressure dome 3101. For example, three of the ports 3100 may be configured as diluent ports and one of the ports 3100 may be configured as a waste port. A pressure sensor in the pump head assembly 28 may determine pressure within the fluid pathways in cartridge 16 by contacting pressure dome 3101. Each of the ports 3100 may be formed from an opening in bezel 164 and a chamber located behind a portion of membrane 162 in frame 160.

[0062] FIG. 21 is a cross-sectional perspective side view of an assembled cartridge 16 having a backpack 3202 (e.g., an implementation of backpack 2900 of FIG. 14) attached thereto to form a cartridge and backpack assembly 3203. As shown in FIG. 21, protrusion 3016 may extend into an opening 3201 in the backpack 3202 to latch the backpack to cartridge 16 at the top side. Additional latching structures at the bottom side will be described in further detail hereinafter. An additional structure 3200 may be disposed between backpack 3202 and cartridge 16. Structure 3200 may be substantially planar and may be shaped and positioned to latch cartridge and backpack assembly 3203 to carousel 14. For example, protrusions 3206 that extend from the top of the backpack 3202 may be actuatable to facilitate installation and removal of the cartridge and backpack assembly into and out of the carousel. For example, ramp structures on the carousel may compress protrusions 3206 when cartridge

and backpack assembly 3203 is pushed into the carousel until protrusions 3206 snap up into a locked position to secure the cartridge and backpack assembly in the carousel. To remove cartridge and backpack assembly 3203 from the carousel for compounding operations, a bayonet 128 that extends into opening 210 may be turned to lower protrusions 3206 to release the cartridge and backpack assembly from the carousel. Further features of the coupling of cartridge and backpack assembly 3203 to the carousel will be described hereinafter.

[0063] Tubing (e.g., flexible tubing 38) for fluidly coupling cartridge 16 to a receiving container 32 may be housed within backpack 3202. For example, the tubing may be coupled at an output port 180 (e.g., a receiving container port - see, e.g., FIG. 20B) to cartridge 16, coiled within an internal cavity of backpack 3202, and extend through opening 3210 so that an end of the tubing can be pulled by an operator to extend the tubing for coupling to the receiving container. An additional opening 3204 may be provided within which a connector such as a Texium® connector coupled to the end of the tubing can be stored when the cartridge and backpack assembly is not in use. When instructed (e.g., by onscreen instructions on display 86) an operator may remove the connector from opening 3204, pull the tubing from within backpack 3202, and connect to the connector to a receiving container. For example, processing circuitry of the compounder system may provide instructions, using the display, to (a) remove a connector that is coupled to the tubing from an additional opening in the backpack, (b) pull the tubing from the backpack, and (c) connect the connector to the receiving container. In another embodiment, extension of the flexible tubing is automatic (e.g., software determines the precise moment the flexible tube should be extended, the pump head operates screw mechanism to extend the tubing, and a signal to the user to pull the ISO Luer out of the backpack opening is provided). Compounder 10 may include a sensor such as an optical sensor that determines whether the connector is present within opening 3204 (e.g., by viewing the connector through opening 3120).

[0064] Compounder 10 may determine, based on whether the connector is within opening 3204, whether and when to release the cartridge and backpack assembly from the pump head assembly. For example, following compounding operations, an operator may be instructed to remove the connector from the receiving container and return the connector into opening 3204. Backpack 3202 may include features and components for facilitating the storage and extraction of the tubing from within the internal cavity. When the connector is detected in opening 3204, the pump drive mechanism 20 may operate one or more coiling mechanisms within backpack 3202 to pull the extended tubing back into the backpack and may turn the bayonet to lower protrusions 3206 so that the cartridge and backpack assembly can be returned to the carousel.

[0065] FIG. 21 also shows an enlarged view of a portion

of cartridge 16 with the crosssection taken through two of valves 190 within openings 228 in bezel 164. As shown in the enlarged view, each valve 190 may be formed from a raised portion 6908 of sealing membrane 162 that extends from a planar portion 6906 of sealing membrane 162 into a corresponding opening 228 in cartridge bezel 164. In the example shown in, for example, FIGS. 19-21, raised portion 6908 is a pyramid-shaped dome formed in opening 228. In a portion of the fluid path 6900 formed between sealing membrane 162 and frame 160 adjacent each valve 190, frame 160 may include a rib 6902 in spaced opposition to the raised portion 6908 of the sealing membrane for that valve. When raised portion 6908 is in a raised position, fluid and/or vapor can flow over rib 6902 through the open valve. In operation, a valve actuator 84 that extends from and is operable by pump head assembly 28 can extend through opening 228 to compress raised portion 6908 against rib 6902 to close the valve and prevent fluid from flowing therethrough.

[0066] FIG. 22 is a cross-sectional side view of the cartridge showing piston pump 166. As shown in FIG. 22, piston pump 166 may include a silicon boot 7100 having first and second seals 7102 and 7104. Forward seal 7104 may form a moving boundary of a pump chamber 6106. Rearward seal 7102 may prevent dust or other contaminants from contacting forward seal 7104. Pump chamber 7106 may be formed adjacent one or more valves 190 (e.g., a pair of valves may be disposed on opposing sides of the pump chamber to control fluid flow into and out of the pump chamber).

[0067] In FIG. 23, for purposes of discussion herein, valves 190 are labeled in three valve groups V1, V2, and V3. Valve group V1 may be a diluent valve group having three valves P1, P2, and P3. Valve group V2 may be a reconstitution valve group having three valves P1, P2, and P3. Piston pump valves P1 and P2 of valve group V3 (e.g., a piston pump valve group) may be operated alternately in cooperation with piston pump 166. For example, during a forward stroke of piston pump 166, valve V3/P1 may be closed and valve V3/P2 may be open and during a backward stroke of piston pump 166, valve V3/P1 may be open and valve V3/P2 may be closed to pump fluid in a first direction within the fluid pathways of cartridge 16. In another example, to pump fluid in an opposite, second direction within the fluid pathways of cartridge 16, during a forward stroke of piston pump 166, valve V3/P1 may be open and valve V3/P2 may be closed and during a backward stroke of piston pump 166, valve V3/P1 may be closed and valve V3/P2 may be open.

[0068] FIGS. 24-27 show various examples of valve configurations for pumping fluids through cartridge 16 for various portions of a compounding operation using the valve labels shown in FIG. 23 for reference. In the example of FIG. 24, the valves of valve groups V1 and V2 are configured for pumping diluent from a diluent container directly to a receiving container (e.g., valves P1 and P3 of group V1 are closed, valve P2 of group V1 is open, valves P1 and P2 of group V2 are closed, and valve P3

of group V2 is open to form a fluid path 7300 from one of diluent ports 3100 to receiving container port 7302).

[0069] In the example of FIG. 25, the valves of valve groups V1 and V2 are configured for pumping diluent from a diluent container to a vial for reconstitution operations (e.g., valves P1 and P3 of group V1 are closed, valve P2 of group V1 is open, valves P2 and P3 of group V2 are closed, and valve P1 of group V2 is open to form a fluid path 7400 from one of diluent ports 3100 to vial port 7402). As shown, during reconstitution operations, a hazardous vapor path 7404 may be formed from a vial waste port 7406 to waste port 3100 to be provided to waste container 44. In some embodiments, a non-hazardous waste path 7408 may be provided from a non-hazardous vial waste port 7405 to air filter port 7410. However, this is merely illustrative. In some embodiments, air filter port 7410 may be associated with air filter check valve structures 3004, 3004, and 3006 that prevent flow of any vapor waste along path 7408 and ensure that all vapor waste from vial 18 is moved along path 7404 through waste port 3100.

[0070] In the example of FIG. 26, the valves of valve groups V1 and V2 are configured for pumping a reconstituted drug from a vial to a receiving container for compounding operations (e.g., valves P1 and P2 of group V1 are closed, valve P3 of group V1 is open, valves P1 and P1 of group V2 are closed, and valve P3 of group V2 is open to form a fluid path 7500 from vial port 7402 to receiving container port 7302). As shown, during compounding operations, a path 7502 may be formed from air filter port 7410 to non-hazardous vapor vial port 7405 to provide filtered, sterile air from outside cartridge 16 into the vial to prevent a vacuum from being generated when the drug is pumped from the vial.

[0071] Although the receiving container 32 is shown in, for example, FIGS. 1, 3, and 11, as an IV bag, in some scenarios, the receiving container 32 may be implemented as a syringe. For example, a Texium® connector coupled by tubing to an output port such as receiving container port 7302 may be connected to a needle free valve connector such as a SmartSite® connector, the SmartSite® connector being coupled by additional tubing to another needle free valve connector (e.g., another SmartSite® connector) that is connected to a syringe for receiving a reconstituted drug. In scenarios in which the receiving container is a syringe, it may be desirable, after pumping the drug from the vial into the syringe, to remove air or other vapors from the syringe.

[0072] In the example of FIG. 27, the valves of valve groups V1 and V2 are configured for pumping air from a receiving container such as a syringe (e.g., valves P1 and P3 of group V1 are closed, valve P2 of group V1 is open, valves P2 and P3 of group V2 are closed, and valve P1 of group V2 is open to form a fluid path 7600 from receiving container port 4302 to waste port 3100). In some configurations, the valves P1 and P2 of group V3 may be alternately opened and closed in cooperation with the motion of piston pump 166 to move the desired fluid

or vapor along the fluid pathways defined by valves 190.

[0073] FIG. 28 is a chart showing the position and operation of the valves 190 as labeled in FIG. 23 during various portions of a reconstitution/compounding process as described above in connection with FIGS. 24-27.

[0074] FIG. 29A is a cross-sectional side view of cartridge 16 with the cross section take through diluent ports 3100D, waste port 3100W, and receiving container port 7302. As shown in the example of FIG. 29A, each diluent port 3100D may be formed by a portion of membrane 162 that is formed within an opening in bezel 164 and adjacent to a diluent chamber 8200D. Waste port 3100W may be formed by a portion of membrane 162 that is formed within an opening in bezel 164 and adjacent to a vapor waste chamber 8200W. Receiving container port 7302 may be formed from an opening that leads to a receiving container chamber 8202 in which tubing that extends into backpack 3202 may be disposed to form a fluid path to the receiving container from cartridge 16.

[0075] When compressed by a sealing manifold membrane such as sealing manifold membrane 8252 of manifold 8250 of FIG. 29B, the portion of sealing membrane 162 that forms diluent and/or waste ports 3100 creates a drip-free connection between the manifold 8250 and the cartridge. A manifold needle 8254 of a selected diluent manifold 8250 and a manifold needle of a waste manifold can extend through the corresponding manifold membrane 8252 and the sealing membrane 162 in the respective diluent and waste port to form fluid paths through sealing membrane 162 (e.g., through opening 8256, central bore 8257, and opening 8258 of needle 8254) for diluents and waste vapors for reconstitution and compounding operations.

[0076] However, the example of FIG. 29A, in which the seal of ports 3100D and 3100W are formed solely by a portion of membrane 162 that extends into an opening in bezel 164 is merely illustrative. In some embodiments, in order to provide an improved drip-free seal, the seal of each of ports 3100D and port 3100W may be formed by a plurality of sealing members. In one example, three sealing members may be provided to form a port seal for cartridge 16.

[0077] FIG. 29C shows a cross-sectional view of a port of cartridge 16 in an implementation with three sealing members. As shown in FIG. 29C, a port 3100 (e.g., one of diluent port 3100D or waste port 3100W) may be formed from a portion of membrane 162 that is disposed between an outer sealing member 8262 (formed in an opening 8260 in bezel 164) and an inner sealing member 8264. Inner sealing member 8264 may be disposed between membrane 162 and chamber 8200.

[0078] As shown in FIG. 29C, outer sealing member 8262 may include a portion that extends through opening 8260 and may also include a recess 8268 on an interior surface adjacent to membrane 162. Membrane 162 may also include a recess 8266 on an interior surface adjacent to inner sealing member 8264. Providing a port 3100 with multiple sealing members such as the three sealing

members (i.e., member 8262, member 8264, and the portion of membrane 162 formed between members 8262 and 8264) may provide an enhanced wiping of needle 8254 to provide an improved dry disconnect in comparison with implementations with a single sealing member. However, this is merely illustrative. In various embodiments, one, two, three, or more than three sealing members for each port may be provided. Similarly, interstitial spaces formed from recesses 8266 and 8268 may further increase the efficiency of the wiping of needle 8254, however, in various embodiments, sealing members may be provided with or without recesses 8266 and/or 8268.

[0079] FIG. 29D shows the manifold 8250 with manifold sealing member 8252 compressed against outer sealing member 8262 of port 3100. As shown in FIG. 29D, needle 8254 is extended from manifold 8250 through sealing members 8252 and 8262, through interstitial space 8268, through membrane 162, through interstitial space 8266, and through inner sealing member 8264 such that openings 8256 and 8258 and central bore 8257 form a fluid pathway between cartridge 16 and manifold 8250.

[0080] In the example of FIG. 29A, the portion of membrane 162 that extends into the openings in bezel 164 in ports 3100 may be compressed (e.g., compressed by 10% radially) to cause a wiping effect on the diluent needles that are extended therethrough and withdrawn therefrom so that when the diluent needles are retracted into the manifold, no liquid is left on the diluent needle or one the outer surfaces of the cartridge or the membrane.

[0081] In the example of FIGS. 29C and 29D, the portion of sealing member 8262 that extends into the openings in bezel 164 in ports 3100 may be compressed (e.g., compressed by 10% radially) to cause a wiping effect on the diluent needles that are extended therethrough and withdrawn therefrom so that when the diluent needles are retracted into the manifold, no liquid is left on the diluent needle or one the outer surfaces of the cartridge or the membrane. The multiple sealing members of FIGS. 29C and 29D may be arranged to each provide a wiping effect on needle 8254 that complements the wiping effect of the other sealing members (e.g., by providing, with each member, a peak wiping force on the needle at locations angularly spaced with respect to the peak wiping force of other members).

[0082] FIG. 30 is cross-sectional perspective side view of cartridge and backpack assembly 3203 in which protrusion 3016 and protrusion 3304 of cartridge frame 160 can be seen cooperating to couple cartridge 16 to backpack 3202 to form cartridge and backpack assembly 3203. To install backpack 3202 onto cartridge 16, opening 3201 of backpack 3202 can be positioned over protrusion 3016 and backpack 3202 can be rotated (e.g., in a direction 3401) to push latching features 3302 of backpack 3202 against latching protrusion 3304 until latching protrusion 3304 snaps into position between latching features 3302. As shown, protrusion 3016 may be formed on an additional latching structure of cartridge 16 such

as a flexible arm 3400. Flexible arm 3400 may allow backpack 3202 to be pulled downward by a small distance when backpack 3202 is rotated to press latching feature 3302 onto protrusion 3304. Flexible arm 3400 may be resilient to maintain an upward force the holds latching features 3302 in a latched position against protrusion 3304.

[0083] In the example of FIG. 30, a vial 18 and vial puck 26 are positioned adjacent to cartridge and backpack assembly 3203 with needle assembly 170 extended into the vial through sealing member 3402 of cartridge 16 and sealing member 3404 of vial puck 26 which may provide a drip free seal and allow fluid to be provided into and/or removed from vial 18. Sealing member 3402 may be, for example, an implementation of sealing member 3008. As shown, when the needle assembly 170 is extended into the vial, portions of the vial puck 26 may be located adjacent to latching features 3302 of backpack 3202.

[0084] FIG. 31 shows a cross-sectional view of a portion of cartridge 16 along with an enlarged view of a portion of needle assembly 170. As shown in FIG. 31, needle housing 186 may include a sealing membrane 3402 formed within an annular housing member 8404 that is attached to cartridge frame 160 via one or more housing arms 8408. A spring 8410 may be provided that extends from needle housing 317B into needle housing 186 such that compression of spring 8410 is necessary to extend needles 316 and 318 through sealing membrane 3402. In this way, a user handling cartridge 16 is prevented from being injured by access to needle assembly 170. In operation, a vial puck may be pressed against annular housing member 8404 to compress spring 8410 such that needle assembly 170 extends through sealing membrane 3402 and through a sealing membrane of the vial puck into the vial.

[0085] Dual lumen needles 316 and 318 may be respectively provided with openings 8400 and 8402 that provide fluid access to central bores of the needles. Needle 316 may, for example, be a 24 gauge needle held in cartridge frame 160 by a high density polyethylene (HDPE) overmold 317A, the needle having an opening 8400 for venting the drug vial. Opening 8400 may be formed using a slot cut as shown to reduce coring of the sealing membranes as the needle is inserted and retracted. Needle 318 may, for example, be an 18 gauge needle held in cartridge frame by a high density polyethylene (HDPE) overmold 317B with one or more openings 8402 for fluid flow into and/or out of the vial. Openings 8402 may include two drilled holes configured to reduce coring and to allow up to, for example, 60 mL/min of fluid flow.

[0086] In this way, during reconstitution operations, diluent may be provided into the vial via openings 8402 of needle 318 and vapor waste may be simultaneously extracted from the vial via opening 8400 in needle 316. During compounding operations, a reconstituted drug may be pulled from the vial via openings 8402 of needle 318 and sterile air may be provided into the vial via open-

ing 8400 of needle 316.

[0087] Various aspects of a dry disconnect are described (e.g., a dry disconnect between cartridge 16 and vial 18 via vial puck 26). For example, a dry disconnect can be achieved when the needle of cartridge 16 is wiped or "squeegeed" clean as it retracts through sealing membranes of puck 26 and cartridge 16. However, compounder 10 is a closed system transfer device (CSTD) that requires certain processes to happen out of "first air." One of the processes that is performed out of first air is inserting cartridge needle into vial 18. This requires protecting the vial needle from "outside" air while also allowing a leak free disconnect when the vial is removed from the cartridge needle. Accordingly, in various implementations, additional features may be provided to help ensure a dry disconnect.

[0088] For example, FIGS. 32-35 show an exemplary implementation of a vial puck 13202 (e.g., an implementation of vial puck 26) that includes a hydroscopic member 13210 in addition to a sealing membrane 13200 (e.g., an implementation of sealing membrane 3402).

[0089] In the example of FIGS. 32-35B, a single lumen needle 13204 is shown, however this is merely illustrative and a puck having a hydroscopic medium and a sealing membrane may be adapted to any needle configuration. In the example of FIGS. 32-35B, vial septum 13208 of vial cap 13206 works in conjunction with vial puck membrane 13200 to "squeegee" any fluid from the outside of the needle. Additionally, as shown in the cross-sectional view of FIG. 32, located between vial puck membrane 13200 and vial septum 13208 is a hydroscopic material 13210 (e.g., a sponge) that is "feature flexible," allowing hydroscopic material 13210 to absorb fluid in hard to reach areas of needle 13204 such as corners and fluid passage openings.

[0090] For example, FIG. 33 shows a cross-sectional view of a configuration in which opening 13334 of needle 13204 is disposed within hydroscopic material 13210 during retraction of the needle from vial cap 13206 while sealing membrane 13200 wipes a portion of the needle at interface 13300 and vial septum 13208 wipes another portion of needle 13204 at interface 13336. Absorbing fluid in hard to reach areas as shown in FIG. 33 allows a greater chance of a good dry disconnect as the vial needle is retracted.

[0091] FIG. 34 shows a partially transparent view of puck 13202 and vial cap 13206 in which the exterior side of puck 13202 and a portion of vial puck membrane 13200 are visible (within the housing of puck 13202 shown in partial transparency to allow viewing of hydroscopic material 13210) with a needle having a bevel cut 13402 passing through vial puck membrane 13200, hydroscopic material 13210 and vial septum 13208.

[0092] FIG. 35A shows a perspective cross-sectional view of the needle passing through a hydroscopic medium adjacent to a vial septum, in which the hydroscopic medium is provided with a plurality of radial slits 13500. FIG. 35B shows an exemplary implementation in which

a stack 13502 of hydroscopic media with slits can be provided spaced apart from the puck sealing membrane.

[0093] Having hydroscopic material 13210 sandwiched between vial puck membrane 13200 and vial septum 13208 allows a successful dry disconnect to be made with various vial needle configurations and sizes. For example, coaxial needles 316 and 318 described herein (see, e.g., FIG. 31) can include an abrupt step between the main needle and the air bleed needle, making it difficult to clear that area of fluid. However, feature conforming hydroscopic material 13210 allows the needle interface step area to be cleared of fluid prior to needle extraction.

[0094] In addition to providing hydroscopic material 13210 in puck 13202, in some implementations, prior to pulling needle 13204 completely from vial septum 13208, a slight vacuum may be constantly pulled on the fluid needle 13204 (as indicated by arrow 13600 of FIG. 36) to clear the needle's internal fluid passages (which may also clear the vent needle passage of fluid in a dual lumen needle configuration). Clearing the needle fluid passage may reduce or eliminate the possibility of any fluid wicking onto the outside of any of the dry disconnect surfaces once the needle starts to separate from the vial puck dry disconnect. In addition, pulling a constant vacuum as the port of the needle is being pulled through the various membranes, helps remove any fluid remaining between needle 13204 and the membrane passages

[0095] For example, as shown in FIG. 37, fluid 13708 that may be disposed between needle 13204 and puck sealing membrane 13200 may be pulled into needle 13204 by a vacuum as the side port 13334 of needle 13204 travels through membrane 13200, so that the surface 13702 of needle 13204 is dry. In implementations in which a vacuum is applied to during retraction of needle 13204, needle 13204 may be provided with openings configured to facilitate the vacuum features (e.g., needle 130204 may be provided without two holes of the same size located vertically from each other on the needle to prevent, during the vacuum process, only the top opening being cleared of fluid with the bottom opening not being cleared of fluid and causing a dry disconnect failure).

[0096] In addition to, or instead of providing vial puck 26/13202 with a hydroscopic medium and/or an internal vacuum pressure, to help ensure a dry disconnect, cartridge 160 may be provided a bellows that surrounds needle 13204 (or needles 316/318). FIGS. 38-43 show various views of a needle assembly that includes a bellows. FIG. 38 shows a perspective view of an exemplary implementation of cartridge 16 having a needle assembly 170 with bellows 13800 that surrounds the needle (and having dial valves instead of membrane valves). FIG. 39 shows bellows 13800 in partial transparency so that the position of needle 13204 within bellows 13800 can be seen. Needle 13204 in the examples of FIGS. 38-43 may be implemented as a dual lumen needle formed from metal or plastic.

[0097] FIG. 40 shows bellows 13800 again in partial

transparency and shows how an internal extension spring 14000 within bellows 13800 and around needle 13204 may be provided to bias bellows 13800 in an extended configuration in which needle 13204 is completely surrounded by (and sealed within) bellows 13800 (e.g., in the absence of an external force that overcomes the tension of spring 14000). As shown in FIG. 41, bellows 13800 may be bonded to a lower surface 14102 (e.g., a lower surface of cartridge frame 160) to form an airtight seal with lower surface 14102.

[0098] Bellows 13800 may be formed from silicone or other flexible materials. Bellows 13800 may also include a dry disconnect mating area 14104 configured to mate with a vial or vial puck dry disconnect feature. As shown in FIG. 42, dry disconnect mating area 14104 may include a seal 14200 configured to be pierced by needle 13204 when vial lift 78 lifts a vial/vial puck assembly toward cartridge 16 (e.g., in direction 14202) to compress bellows 13800 while needle 13204 remains fixed. In the configuration shown in FIG. 42, seal 14200 maintains a sealed cavity within bellows 13800.

[0099] As a vial/vial puck assembly is pulled towards cartridge 16, bellows 13800 compresses until eventually needle 13204 protrudes through all of the dry disconnects. Later, as the vial/vial puck assembly is retracted (e.g., in direction 14300 of FIG. 43) and needle 13204 is extracted, bellows 13800 begins to expand and create a slight vacuum within cavity 14204 of bellows 13800. This vacuum helps pull in any remaining fluid between needle 13204 and the dry disconnect membranes. Removing any excess fluid, helps promote a better dry disconnect between the two membrane surfaces.

[0100] As previously noted, in some implementations, needle 13204 may be a dual-lumen plastic needle. FIGS. 44-50 show various views of an exemplary implementation of a dual-lumen plastic needle for cartridge 16. As shown in the partial transparency side view of FIG. 44, needle 13204 may be provided with an upper fluid port 14400, a lower fluid port 14404, an upper vent port 14402, and a lower vent port 14406. FIG. 45 shows a cross-sectional view of needle 13204 in which divider 14500 can be seen separating the fluid side (fluid pathway) from the vent side (vent pathway) of the needle. As shown in FIG. 46, one or more internal features such as a ledge 14600 may be provided as guide to aid in installation of divider 14500. As shown in FIG. 47, needle 13204 may be provided with energy directors 14700 on the upper fluid and vent ports for ultrasonic welding of the ports to corresponding fluid and vent paths within cartridge 16. As shown in FIG. 48, needle 13204 may be provided with a smooth needle tip 14800 to prevent coring of sealing membranes. FIG. 49 shows a top-side perspective view of needle 13204 with divider 14500. Divider 14500 may be solvent bonded to the main body of the needle or may be integrally formed with the main body. As shown in FIG. 50, additional channel definition members such as

dual-lumen needle. Channel definition members such as channel definition member 15000 may be integrally formed with the main body of the needle or may be separate members.

[0101] In the example of FIGS. 44-50, cartridge 16 interacts with a vial 18 containing a drug using a dual lumen vial/vent plastic needle 13204. Needle 13204 has a fluid passage large enough to handle a wide range of fluid viscosities and also a passage to allow the vial to be vented to prevent pressure or vacuum buildup in the vial. In addition, needle 13204 includes features that prevent coring of the vial and dry disconnect membranes. For example, instead of fluid passages that exit towards the tip of the needle, needle 13204 in the examples of FIGS. 44-50 includes fluid port 14404 and vent port 14406 located on the sides of the needle rather than the tip of the needle, reducing the sharp edges that can sometimes cause coring

[0102] In various implementations, needle 13204 may be a two piece plastic needle that is composed of the main body and a divider (e.g., divider 14500) that separates the fluid passage from the air vent passage. The two pieces are either welded or solvent bonded together to form a permanent assembly. The fluid and air ports 14404 and 14406 exit the side of the needle rather than the tip of the needle. This helps to prevent coring of the vial and dry disconnect membranes. The ports 14404 and 14406 may also be located 180 degrees to each other for moldability (see, e.g., FIG. 44).

[0103] Although various implementations have been described in which a needle for coupling cartridge 16 to vial 18 through vial puck 26 is disposed in the cartridge, it should be appreciated that, in other implementations, the needle or a cannula may be disposed in vial puck 26 for coupling vial 18 to cartridge 16. FIGS. 51-63 show various views of an exemplary implementation in which a dual-lumen cannula is disposed in puck 26. For example, FIGS. 51 and 52 respectively show side and perspective views of vial puck 26 with an incorporated cannula (not visible in FIGS. 51 and 52; see FIGS. 53 and 54) and two dry disconnect valves 15102 and 15104 used to make the mate between vial 18 and cartridge 16. Since the material of the vial stopper is typically chosen by the pharmaceutical companies and may be variable from vial to vial, providing the cannula as part of vial puck 26 may reduce the risks of coring the vial stopper, as the vial is only accessed by this cannula a single time.

[0104] Additionally, in the initial state shown in FIGS. 51 and 52, the cannula is in a retracted position that allows the puck to be attached to the vial without piercing the stopper. When the cartridge is first mated to vial puck 26, a protrusion 15100 on cartridge 16 advances the cannula into vial 18.

[0105] This configuration may increase the usable life of the drug from beginning when the puck is attached, to when it is first mated to a cartridge, allowing the pucks to be installed many hours or even days prior to when the drug is needed. The puck also incorporates two dry

disconnect valves 15102 and 15104 that allow for a need-
less fluid transfer to and from vial 18. The connection is
achieved by a ridged plastic face coming together with a
compliant plastic face. As shown, the compliant face is
attached to a bellows and as it compresses, a port on
the ridged component is exposed and allows for fluid
transfer. Since fluid is not transferred across the two fac-
es, when the connection is terminated, the faces will re-
main dry. By placing two of these connections on the cap,
fluid and waste air are able to be independently trans-
ferred from the vial.

[0106] When adding/removing fluid from vial 18, it is
desirable for an equal amount of air to be evacuated/in-
troduced to the vial to equalize the pressure in the vial.
In the example of FIGS. 51-63, when fluid is added to
vial 18 from cartridge 16, this air is displaced through the
aforementioned dry disconnect valve. When fluid is re-
moved from vial 18, ambient air is introduced to vial 18
through a check valve/filter combination.

[0107] Having the cannula incorporated into the vial
puck significantly reduces the risks of the vial stopper
coring, thus reducing the possibility of fragments entering
the cartridge and ultimately, entering the patient. The
ability to install the puck and have the needle/plastic can-
nula pierce the vial at a later time, also increases the
amount of time the drug/puck combination can be used
for after the cap is installed. The inclusion of the dry dis-
connect valves, as in the example of FIGS. 51-63, may
also eliminate the use of a needle in cartridge 16 and
allow for a wider range of flow rates while maintaining a
leak-free seal at disconnection.

[0108] FIG. 53 shows a side view of an exemplary im-
plementation of a dual-lumen plastic cannula 15400 that
may be provided within puck 26 to be actuated by pro-
trusion 15100. FIG. 54 shows a cross-sectional view of
cannula 15400 in which a fluid path 15402 and an air/vent
path 15404 are visible. FIG. 55 shows a partially trans-
parent side view of puck 26 attached to vial 18 in which
cannula 15400 is completely disposed within puck 26
and vial 18 has not yet been accessed. FIG. 56 shows a
partially transparent side view of puck 26 attached to vial
18 in which cannula 15400 has been extended into vial
18 by protrusion 15100 on puck 26. FIG. 57 shows a
bottom side perspective view of puck 26 in which cannula
15400 is completely disposed within opening 15500 of
puck 26. FIG. 58 shows a bottom side perspective view
of puck in which cannula 15400 has been extended into
recess 15600 of puck 26, recess 15600 being configured
to attach to the top of a vial 18.

[0109] The retracted state of FIGS. 55 and 57 allows
puck 26 to be attached without puncturing the vial. This
advances the usable life of the drug from beginning when
the puck is attached, to when it is first mated to a cartridge,
allowing the pucks to be installed many hours or even
days prior to when the drug in the vial is needed. Since
the material of the vial stopper is chosen by the pharma-
ceutical companies and can be difficult to control, pro-
viding puck 26 with a needle or cannula 15400 incorpo-

rated into vial puck 26, can help reduce the risks of coring
the vial stopper as the vial is only accessed by the nee-
dle/cannula a single time.

[0110] FIG. 59 shows cartridge 16 and vial puck 26
aligned for coupling. As shown in FIG. 60, bellows 16000
of each of the dry disconnect valves compresses on in-
sertion and seals against the face of puck 26 to allow a
conduit 16002 of each of the dry disconnect valves to be
exposed to create the desired fluid and/or vent pathways
between vial 18 and cartridge 16 (e.g., via pathways
15402 and 15404 of the cannula). FIG. 61 shows a side
view of a portion of cartridge 16 in which bellows 16000
protect and surround the conduits of each dry disconnect
valve. As shown in the side views of puck 26 in FIGS. 62
and 63, in the example of FIGS. 51-63, puck 26 may be
provided with an ambient air filter 16200 that filters in-
coming ambient air and a check valve 16204 that ensures
that waste air cannot escape the system.

[0111] As described above in connection with, for ex-
ample, FIGS. 29A, cartridge 16 may be provided with
one or more diluent ports 3100D and/or one or more
waste ports. One or more manifolds, each having a nee-
dle may be coupled to a respective diluent container or
waste container. The needle of each manifold may be
extended by the pump head into a corresponding port
3100 to couple the diluent or waste container to cartridge
16. However, in some implementations, ports 3100 and
the associated magazines can be implemented with a
dry disconnecting interface that does not include a nee-
dle. FIGS. 64-68 show an exemplary implementation of
a dry disconnecting interface using a face seal and a side
ported shuttle valve that can be used to couple, for ex-
ample, containers 42 or 44 to cartridge 16.

[0112] The dry disconnecting interface of FIGS. 64-68
allows for a dry disconnection between the compounder
manifold and cartridge diluent ports. A face seal keeps
fluid from leaking into the environment while a shuttling
valve is used to enable and disable flow. Having a face
seal and a shuttling valve eliminates the use of a needle
and allows for a wider range of flow rates while main-
taining a leak-free seal at disconnection. FIG. 64 shows a
male portion 16402 and a female portion 16400 of a dry
disconnect shuttle valve. For example, male portion
16402 may be connected to a diluent container via tubing
and female portion 16400 may be an implementation of
one of diluent ports 3100D of cartridge 16.

[0113] FIG. 65 shows male side 16402 and female side
16400 in cross section, spaced apart by a gap 16500 and
disconnected. FIG. 66 shows male side 16402 and fe-
male side 16400 in cross section, in contact at interface
16600, with the fluid path between male side 16402 and
female side 16400 still closed. FIG. 67 shows male side
16402 and female side 16400 in cross section, connected
with shuttle valve 16702 of male side 16402 extended
into female side 16400 such that a side port 16704 pro-
vides a fluid path 16700 from male side 16402 to female
side 16400. FIG. 68 shows a broader view of male side
16402 and female side 16400 in cross section with the

fluid path closed.

[0114] In some implementations of compounder 10, one or more filters may be provided in the fluid flow path between cartridge 16 and receiving container 32 (e.g., to prevent any coring material of the vial septum or any foreign matter left within the cartridge from flowing into the receiving container). A compounded drug is transferred between cartridge 16 and receiving container 32 via tubing such as "pigtail" tubing in some embodiments. For example, a filter and/or screen may be provided within the cartridge or an in-line fluid filter located at the end of the pigtail prior to the receiving container may be provided. FIGS. 69 and 70 show exemplary implementations of a connector (e.g., a Texium® connector) for coupling to receiving container input 34 in which a filter 16900 is provided at the interface between the connector and tubing for coupled to cartridge 16. In the example of FIG. 69, the connector is shown in partial transparency so that filter 16900 within the connector is visible. In the example of FIG. 70, a separate filter/screen element 17000 is disposed between the connector and the tubing.

[0115] Although various implementations of cartridge 16 have been described in which an oscillating piston pump (see, e.g., piston 166 of FIG. 21) is operated to move fluid and/or gasses through cartridge 16 and from diluent containers and to a receiving container, in other implementations, a syringe pump may be used instead of or in addition to an oscillating piston pump. FIG. 71 shows an exemplary implementation of a syringe piston 17103 and an associated grasping mechanism 17101 (e.g., for grasping and actuating the syringe piston). In the example of FIG. 71, syringe piston 17103 includes a tapered grab handle 17102 and one or more seals such as o-rings 17100. O-rings 17100 may be provided to seal the plunger to the bore of the syringe pump (not shown) instead of, for example, a rubber "boot" that fits over the end of the plunger tip (e.g., which can, in some circumstances allow for volumetric inaccuracies if the rubber boot flexes fore and aft as the plunger changes directions as it is being pulled or pushed). O-rings 17100 can therefore be particularly helpful in micro-dosing scenarios.

[0116] Grasping mechanism 17101 may be a claw with arms that can be actuated to grasp grasping handle 17102. Grasping mechanism 17101 may be actuatable to slowly move syringe piston 17103 to pump fluid and/or gas. In order to help ensure the volumetric accuracy of fluids and/or gasses pumped by slowly actuating syringe piston 17103, as shown in FIG. 71, grasping mechanism 17101 may include tapered surfaces 17200 that are complementary to the tapered shape of grasping handle 17102. Providing a tapered claw 17101 may reduce or eliminate backlash when mating grasping mechanism 17101 and tapered grasping handle 17102 of syringe plunger 17103 (e.g., by reducing or eliminating clearances between mating parts). For example, the tapered end 17102 of syringe plunger 17103 may be slid into the tapered groove of a syringe activation device such as claw 17101. Syringe plunger 17103 may be securely held by

approximately 180 degrees of contact by the syringe activation device.

[0117] The claw portion of grasping mechanism 17101 may be spring loaded or mechanically actuated. In other implementations, grasping mechanism 17101 may be a claw having a pitchfork design without moving parts.

[0118] The present disclosure is provided to enable any person skilled in the art to practice the various aspects described herein. The disclosure provides various examples of the subject technology, and the subject technology is not limited to these examples. Various modifications to these aspects will be readily apparent to those skilled in the art, and the generic principles defined herein may be applied to other aspects.

[0119] The subject technology is illustrated, for example, according to various aspects described above. Various examples of these aspects are described as numbered concepts or clauses (1, 2, 3, etc.) for convenience. These concepts or clauses are provided as examples and do not limit the subject technology. It is noted that any of the dependent concepts may be combined in any combination with each other or one or more other independent concepts, to form an independent concept. The following is a non-limiting summary of some concepts presented herein:

Concept 1. A compounder system, comprising:
a cartridge having:

a plurality of controllable fluid pathways fluidly coupled to at least one diluent port and a receiving container port,
a pump component actuatable to pump a fluid within the plurality of controllable fluid pathways, and
a needle configured to couple the plurality of controllable fluid pathways to a vial containing a drug; and
a bellows configured to surround the needle in an extended configuration and to be compressed to allow the needle to extend from the bellows into the vial.

Concept 2. The compounder system of Concept 1 or any other Concept, wherein the bellows forms a cavity around the needle and is configured to generate a vacuum pressure within the cavity when the bellows extends upon retraction of the needle from the vial.

Concept 3. The compounder system of Concept 2 or any other Concept, wherein the cartridge further comprises a spring configured to bias the bellows in the extended configuration.

Concept 4. The compounder system of Concept 3 or any other Concept, wherein the bellows comprises a dry disconnect seal.

Concept 5. The compounder system of Concept 4 or any other Concept, wherein the dry disconnect seal forms a distalmost boundary of the cavity, and wherein the needle is entirely disposed within the cavity when the bellows is in the extended configuration. 5

Concept 6. The compounder system of Concept 5 or any other Concept, wherein a portion of the needle extends through the dry disconnect seal when the bellows is in a compressed configuration. 10

Concept 7. The compounder system of Concept 6 or any other Concept, wherein the dry disconnect seal is configured to sealingly slide along an outer surface of the needle as the bellows is compressed from the extended configuration to the compressed configuration and when the bellows extends from the compressed configuration to the extended configuration. 15 20

Concept 8. The compounder system of Concept 3 or any other Concept, wherein the spring is a coil spring that wraps around at least a portion of the needle within the cavity. 25

Concept 9. A compounder system, comprising:
a cartridge having:

a plurality of controllable fluid pathways fluidly coupled to at least one diluent port and a receiving container port,
a pump member actuatable to pump a fluid within the plurality of controllable fluid pathways, and
a needle configured to couple the plurality of controllable fluid pathways to a vial containing a drug, wherein the needle comprises a dual-lumen plastic needle. 30 35

Concept 10. The compounder system of Concept 9 or any other Concept, wherein the dual-lumen plastic needle comprises: 40

a fluid pathway having upper and lower fluid ports;
a gas pathway having upper and lower gas ports; and
a tip, wherein the lower fluid port and the lower gas port are located away from the tip. 45 50

Concept 11. The compounder system of Concept 10 or any other Concept, wherein the dual-lumen plastic needle further comprises a vertical divider between the fluid pathway and the gas pathway, wherein the lower fluid port and the lower gas port are horizontally spaced apart, and wherein the lower fluid port is larger than the lower gas port. 55

Concept 12. The compounder system of Concept 11 or any other Concept, wherein the vertical divider extends along a length of the needle from a base of the needle to the tip.

Concept 13. The compounder system of Concept 12 or any other Concept, wherein the dual-lumen plastic needle further comprises an interior ledge configured to guide the vertical divider for assembly of the dual-lumen plastic needle.

Concept 14. The compounder system of Concept 9 or any other Concept, wherein cartridge comprises a body within which the plurality of controllable fluid pathways and the pump member are disposed, and wherein the dual-lumen plastic needle extends from an outer surface of the body of the cartridge.

Concept 15. The compounder system of Concept 9 or any other Concept, wherein the cartridge further comprises a compressible vacuum bellows configured to surround at least a portion of the needle.

Concept 16. A method, comprising:

coupling a cartridge to a pump head of a compounder system, the cartridge having a body enclosing a plurality of fluid pathways, a needle extending from the body and having a lumen fluidly coupled to at least one of the fluid pathways, and a bellows forming a cavity within which the needle is disposed; and
extending the needle into a vial by compressing the bellows with the vial.

Concept 17. The method of Concept 16 or any other Concept, wherein extending the needle into the vial by compressing the bellows with the vial comprises moving the vial toward the cartridge such that a tip of the needle extends through a dry disconnect seal of the bellows. Concept 18. The method of Concept 17 or any other Concept, wherein moving the vial comprises actuating a vial lift of the compounder system to remove the vial from a vial tray and to compress the bellows by pressing a vial puck attached to the vial against the bellows.

Concept 19. The method of Concept 16 or any other Concept, further comprising extending the bellows while removing the needle from the vial such that extension of the bellows generates a vacuum within the bellows.

Concept 20. The method of Concept 19 or any other Concept, wherein extending the bellows comprises sealingly sliding a dry disconnect seal of the bellows along an outer surface of the needle.

[0120] One or more aspects or features of the subject matter described herein may be realized in digital electronic circuitry, integrated circuitry, specially designed ASICs (application specific integrated circuits), computer hardware, firmware, software, and/or combinations thereof. For example, infusion pump systems disclosed herein may include an electronic system with one or more processors embedded therein or coupled thereto. Such an electronic system may include various types of computer readable media and interfaces for various other types of computer readable media. Electronic system may include a bus, processing unit(s), a system memory, a read-only memory (ROM), a permanent storage device, an input device interface, an output device interface, and a network interface, for example.

[0121] Bus may collectively represent all system, peripheral, and chipset buses that communicatively connect the numerous internal devices of electronic system of an infusion pump system. For instance, bus may communicatively connect processing unit(s) with ROM, system memory, and permanent storage device. From these various memory units, processing unit(s) may retrieve instructions to execute and data to process in order to execute various processes. The processing unit(s) can be a single processor or a multi-core processor in different implementations.

[0122] A reference to an element in the singular is not intended to mean "one and only one" unless specifically so stated, but rather "one or more." Unless specifically stated otherwise, the term "some" refers to one or more. Pronouns in the masculine (e.g., his) include the feminine and neuter gender (e.g., her and its) and vice versa. Headings and subheadings, if any, are used for convenience only and do not limit the invention.

[0123] The word "exemplary" is used herein to mean "serving as an example or illustration." Any aspect or design described herein as "exemplary" is not necessarily to be construed as preferred or advantageous over other aspects or designs. In one aspect, various alternative configurations and operations described herein may be considered to be at least equivalent.

[0124] As used herein, the phrase "at least one of" preceding a series of items, with the term "or" to separate any of the items, modifies the list as a whole, rather than each item of the list. The phrase "at least one of" does not require selection of at least one item; rather, the phrase allows a meaning that includes at least one of any one of the items, and/or at least one of any combination of the items, and/or at least one of each of the items. By way of example, the phrase "at least one of A, B, or C" may refer to: only A, only B, or only C; or any combination of A, B, and C.

[0125] A phrase such as an "aspect" does not imply that such aspect is essential to the subject technology or that such aspect applies to all configurations of the subject technology. A disclosure relating to an aspect may apply to all configurations, or one or more configurations. An aspect may provide one or more examples. A phrase

such as an aspect may refer to one or more aspects and vice versa. A phrase such as an "embodiment" does not imply that such embodiment is essential to the subject technology or that such embodiment applies to all configurations of the subject technology. A disclosure relating to an embodiment may apply to all embodiments, or one or more embodiments. An embodiment may provide one or more examples. A phrase such an embodiment may refer to one or more embodiments and vice versa. A phrase such as a "configuration" does not imply that such configuration is essential to the subject technology or that such configuration applies to all configurations of the subject technology. A disclosure relating to a configuration may apply to all configurations, or one or more configurations. A configuration may provide one or more examples. A phrase such a configuration may refer to one or more configurations and vice versa.

[0126] In one aspect, unless otherwise stated, all measurements, values, ratings, positions, magnitudes, sizes, and other specifications that are set forth in this specification, including in the claims that follow, are approximate, not exact. In one aspect, they are intended to have a reasonable range that is consistent with the functions to which they relate and with what is customary in the art to which they pertain.

[0127] It is understood that the specific order or hierarchy of steps, or operations in the processes or methods disclosed are illustrations of exemplary approaches. Based upon implementation preferences or scenarios, it is understood that the specific order or hierarchy of steps, operations or processes may be rearranged. Some of the steps, operations or processes may be performed simultaneously. In some implementation preferences or scenarios, certain operations may or may not be performed. Some or all of the steps, operations, or processes may be performed automatically, without the intervention of a user. The accompanying method Concepts present elements of the various steps, operations or processes in a sample order, and are not meant to be limited to the specific order or hierarchy presented.

[0128] All structural and functional equivalents to the elements of the various aspects described throughout this disclosure that are known or later come to be known to those of ordinary skill in the art are expressly incorporated herein by reference and are intended to be encompassed by the Concepts. Moreover, nothing disclosed herein is intended to be dedicated to the public regardless of whether such disclosure is explicitly recited in the Concepts. No Concepts element is to be construed under the provisions of 35 U.S.C. §112 (f) unless the element is expressly recited using the phrase "means for" or, in the case of a method Concepts, the element is recited using the phrase "step for." Furthermore, to the extent that the term "include," "have," or the like is used, such term is intended to be inclusive in a manner similar to the term "comprise" as "comprise" is interpreted when employed as a transitional word in a Concepts.

[0129] The Title, Background, Summary, Brief De-

scription of the Drawings and Abstract of the disclosure are hereby incorporated into the disclosure and are provided as illustrative examples of the disclosure, not as restrictive descriptions. It is submitted with the understanding that they will not be used to limit the scope or meaning of the Concepts. In addition, in the Detailed Description, it can be seen that the description provides illustrative examples and the various features are grouped together in various embodiments for the purpose of streamlining the disclosure. This method of disclosure is not to be interpreted as reflecting an intention that the claimed subject matter requires more features than are expressly recited in each Concepts. Rather, as the following Concepts reflect, inventive subject matter lies in less than all features of a single disclosed configuration or operation. The following Concepts are hereby incorporated into the Detailed Description, with each Concept standing on its own as a separately disclosed subject matter.

[0130] The Concepts are not intended to be limited to the aspects described herein, but are to be accorded the full scope consistent with the language Concepts and to encompass all legal equivalents. Notwithstanding, none of the Concepts are intended to embrace subject matter that fails to satisfy the requirement of 35 U.S.C. § 101, 102, or 103, nor should they be interpreted in such a way.

Claims

1. A compounder system (10), comprising:

a cassette cartridge (16) comprising:

a plurality of controllable fluid pathways fluidly coupled to at least one diluent port (3100) and a receiving container port (7302);
a pump member actuable to pump a fluid within the plurality of controllable fluid pathways; and

a needle (13204) configured to couple the plurality of controllable fluid pathways to a vial containing a drug, wherein the needle (13204) comprises a dual-lumen needle (13204) comprising:

a fluid pathway having upper and lower fluid ports (14400, 14404);
a gas pathway having upper and lower gas ports (14402, 14406);
a vertical divider (14500) between the fluid pathway and the gas pathway;
a first channel definition member (15000) disposed on a fluid pathway side of the vertical divider (14500) and configured to shape and size a fluid lumen comprising the fluid pathway;

a second channel definition member (15000) disposed on a gas pathway side of the vertical divider (14500) and configured to shape and size a vent lumen comprising the gas pathway; and
a tip (14800).

2. The compounder system (10) of claim 1, wherein one of:

the lower fluid port (14404) is larger than the lower gas port (14406);
the lower fluid port (14404) and the lower gas port (14406) are located away from the tip (14800); and
the lower fluid port (14404) and the lower gas port (14406) are horizontally spaced apart 180 degrees.

3. The compounder system (10) of either of claim 1 or claim 2, wherein the vertical divider (14500) extends along a length of the dual-lumen needle (13204) from a base of the dual-lumen needle (13204) to the tip (14800), and wherein the dual-lumen needle (13204) further comprises an interior ledge (14600) configured to guide the vertical divider (14500) for assembly of the dual-lumen needle (13204).

4. The compounder system (10) of any of claim 1 to claim 3, wherein the cartridge (16) comprises a body within which the plurality of controllable fluid pathways and the pump member are disposed, and wherein the dual-lumen needle (13204) extends from an outer surface of the body of the cartridge (16).

5. The compounder system (10) of any of claim 1 to claim 4, wherein the cartridge (16) further comprises a compressible vacuum bellows (13800) configured to surround at least a portion of the dual-lumen needle (13204).

6. The compounder system (10) of any of claim 1 to claim 4, further comprising a bellows (13800) configured to surround the dual-lumen needle (13204) in an extended configuration and to be compressed to allow the dual-lumen needle (13204) to extend from the bellows (13800) into the vial.

7. The compounder system (10) of claim 6, wherein the cartridge (16) further comprises one of:

a spring (14000) configured to bias the bellows (13800) in the extended configuration; and
a coil spring (14000) that wraps around at least a portion of the dual-lumen needle (13204) within a cavity formed by the bellows (13800).

8. The compounder system (10) of claim 6, wherein the bellows (13800) forms a cavity around the dual-lumen needle (13204) and is configured to generate a vacuum pressure within the cavity when the bellows (13800) extends upon retraction of the dual-lumen needle (13204) from the vial. 5
9. The compounder system (10) of claim 8, wherein the bellows (13800) comprises a dry disconnect seal (14200). 10
10. The compounder system (10) of claim 9, wherein one of:
- the dry disconnect seal (14200) forms a distal-most boundary of the cavity, and wherein the dual-lumen needle (13204) is entirely disposed within the cavity when the bellows (13800) is in the extended configuration; 15
- a portion of the dual-lumen needle (13204) extends through the dry disconnect seal (14200) when the bellows (13800) is in a compressed configuration; and 20
- the dry disconnect seal (14200) is configured to sealingly slide along an outer surface of the dual-lumen needle (13204) as the bellows (13800) is compressed from the extended configuration to the compressed configuration and when the bellows (13800) extends from the compressed configuration to the extended configuration. 25 30
11. The compounder system (10) of any of the preceding claims, further comprising a first energy director (14700) disposed on the upper fluid port (14400) and a second energy director (14700) disposed on the upper gas port (14402), the first and second energy directors (14700) configured for ultrasonic welding of the upper fluid port (14400) and upper gas port (14402) to corresponding fluid and vent paths of the plurality of controllable fluid pathways within the cartridge (16). 35 40
12. The compounder system (10) of any of the preceding claims, wherein the lower gas port (14406) is a slot cut opening and the lower fluid port (14404) is two adjacent holes. 45
13. A method, comprising:
- coupling a cartridge (16) to a pump head of a compounder system, the cartridge (16) having a body enclosing a plurality of fluid pathways, a dual-lumen needle (13204) extending from the body and having a first lumen having upper and lower fluid ports (14400, 14404) and fluidly coupled to at least one of the fluid pathways, a second lumen having upper and lower gas ports (14402, 14406) and fluidly coupled to a gas path-

way, a vertical divider (14500) between the first lumen and the second lumen, a first channel definition member (15000) disposed on a first lumen side of the vertical divider (14500) and configured to shape and size the first lumen, and a second channel definition member (15000) disposed on a second lumen side of the vertical divider (14500) and configured to shape and size the second lumen, wherein the lower fluid port (14404) and the lower gas port (14406) are horizontally spaced apart 180 degrees and a bellows (13800) forming a cavity within which the dual-lumen needle (13204) is disposed; and extending the dual-lumen needle (13204) into a vial (18) by compressing the bellows (13800) with the vial (18), comprising moving the vial (18) toward the cartridge (16) such that a tip (14800) of the dual-lumen needle (13204) extends into the vial (18).

14. The method of claim 13, wherein moving the vial (18) comprises actuating a vial lift (78) of the compounder system to remove the vial (18) from a vial tray (22) and to compress the bellows (13800) by pressing a vial puck (26) attached to the vial (18) against the bellows (13800).
15. The method of claim 13, further comprising extending the bellows (13800) while removing the dual-lumen needle (13204) from the vial (18) such that extension of the bellows (13800) generates a vacuum within the bellows (13800), wherein extending the bellows (13800) comprises sealingly sliding a dry disconnect seal (14200) of the bellows (13800) along an outer surface of the needle (13204).

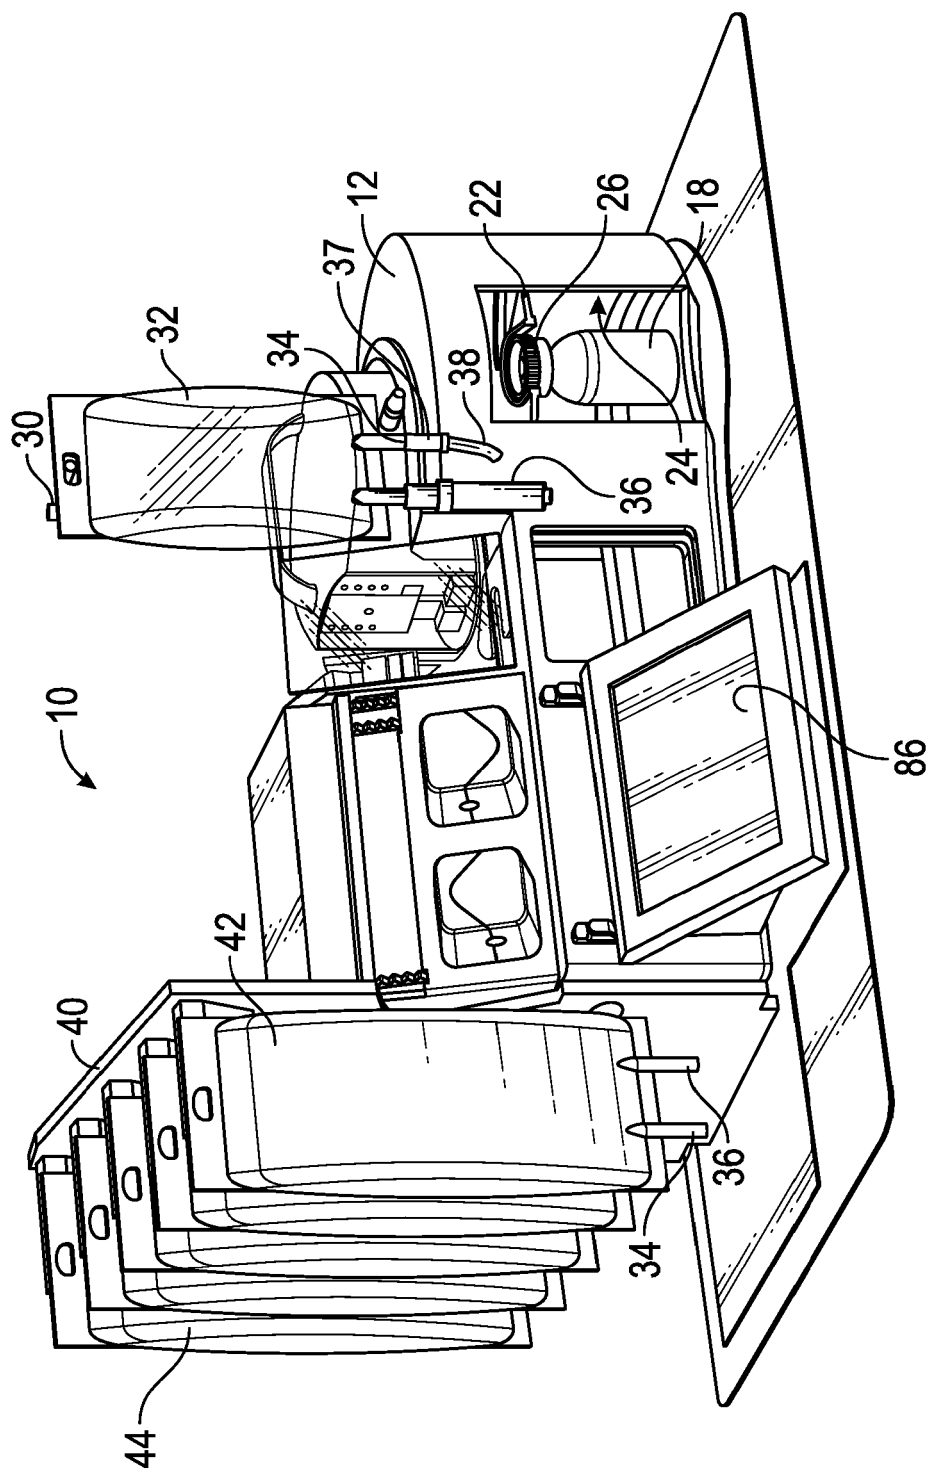


FIG. 1

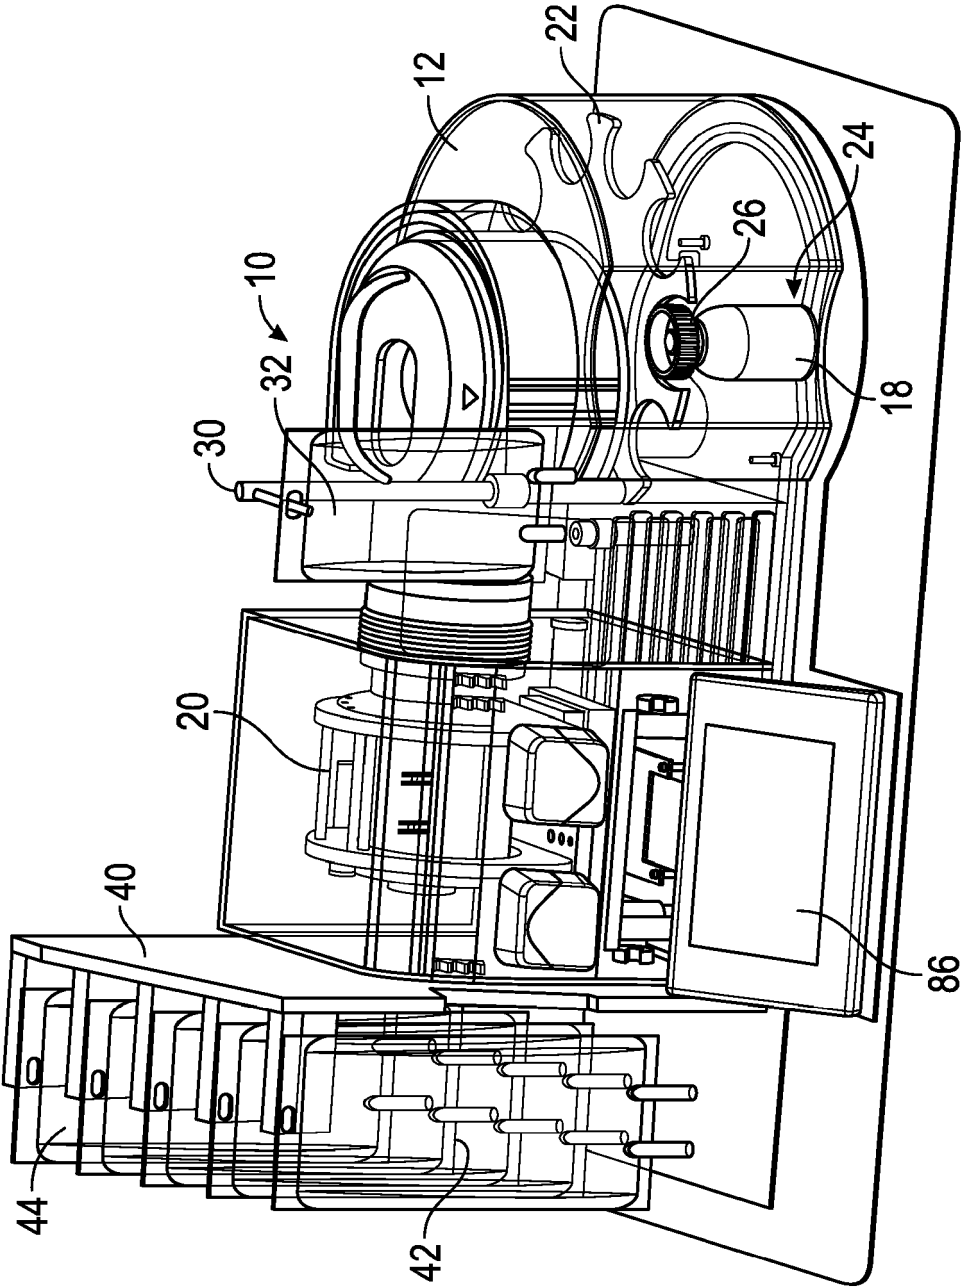


FIG. 2

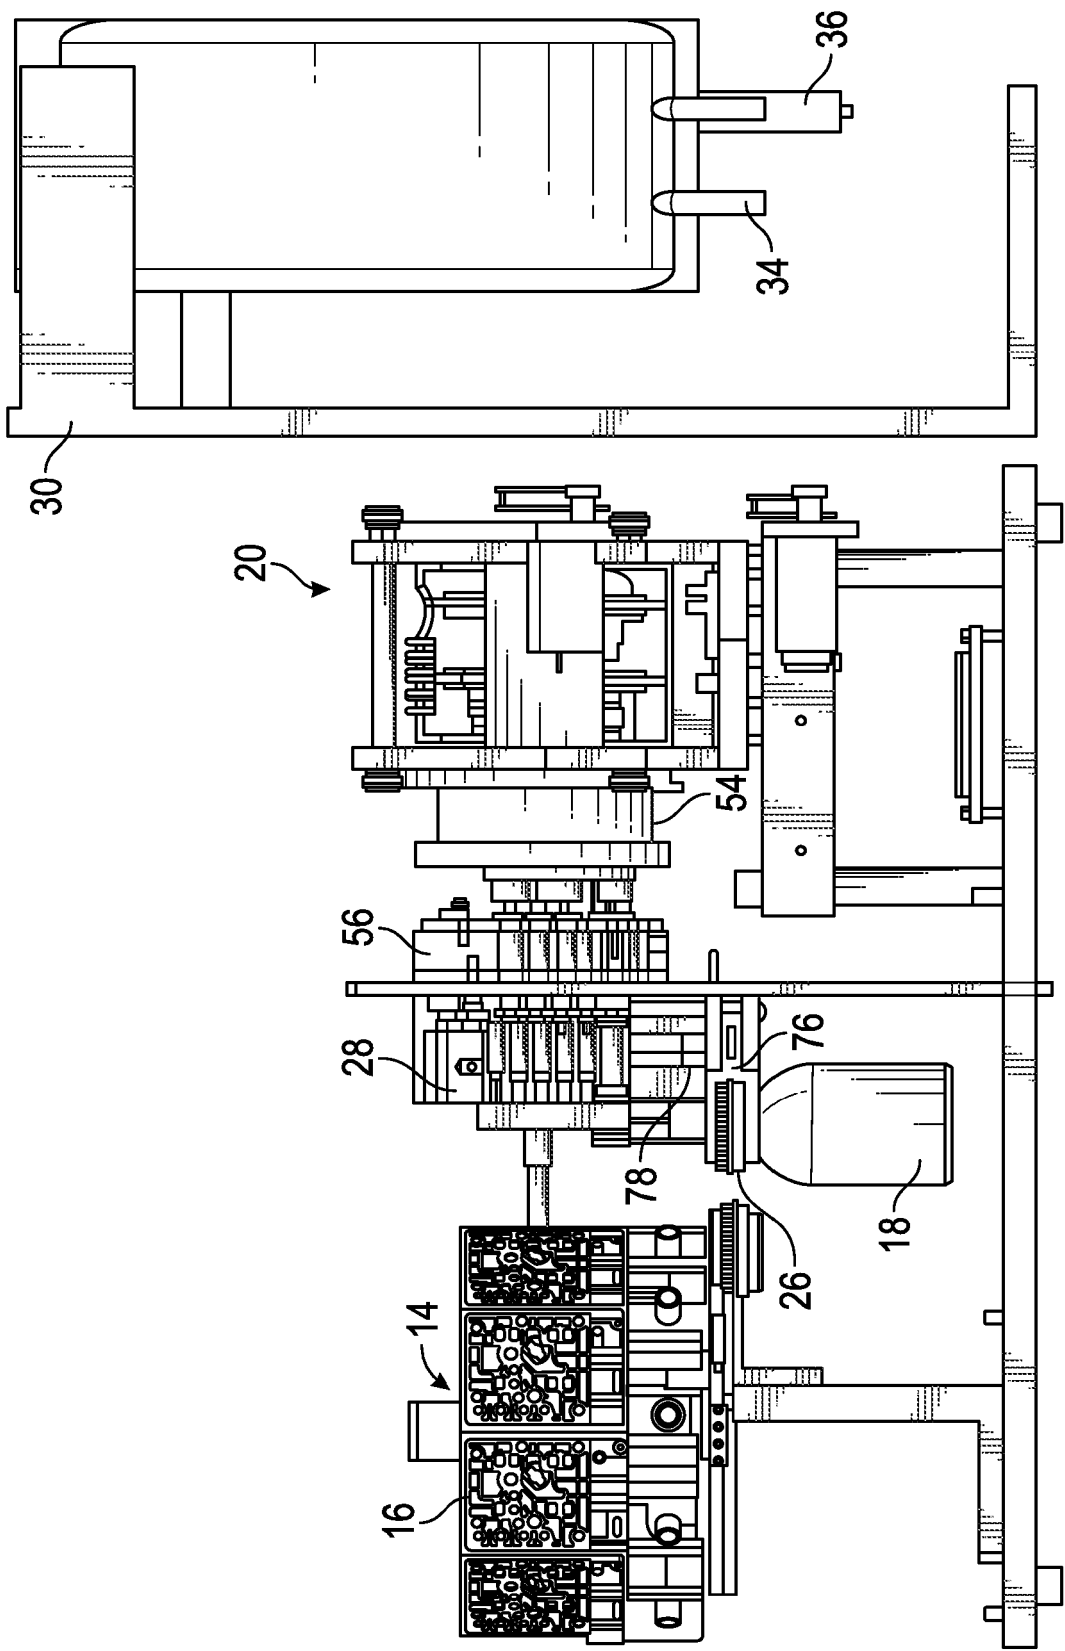


FIG. 3

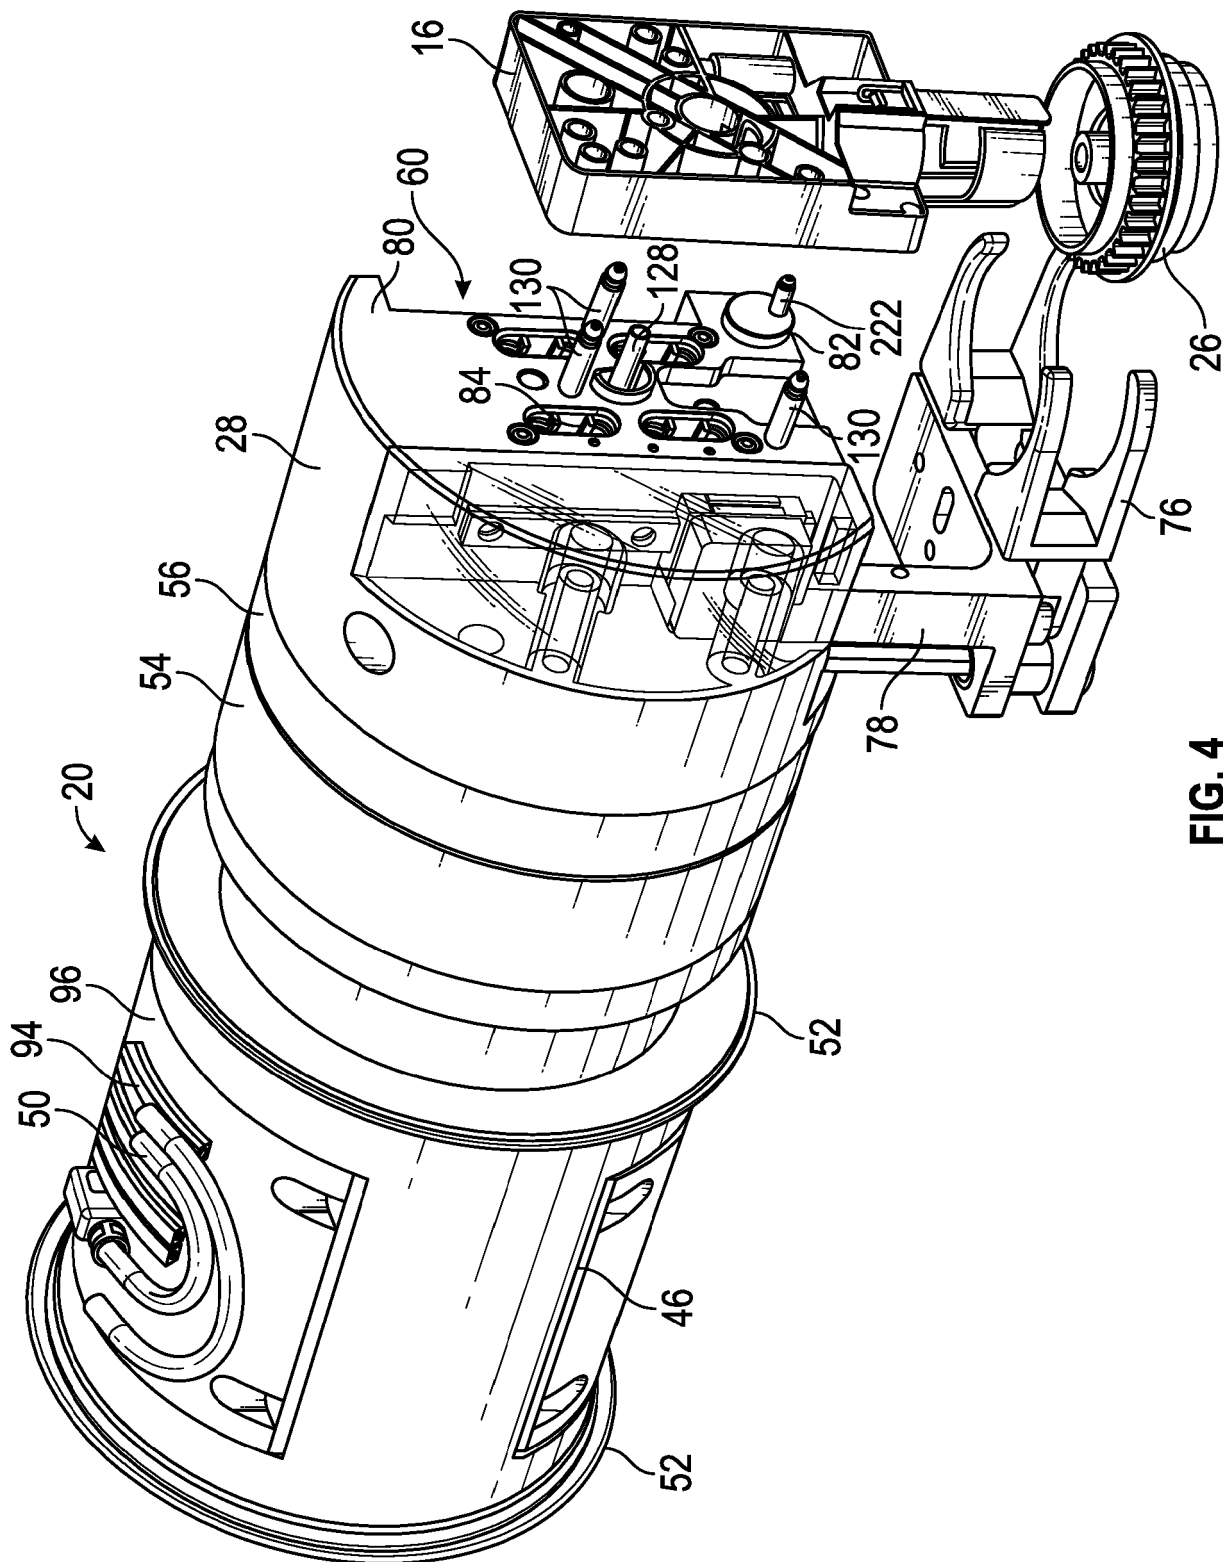


FIG. 4

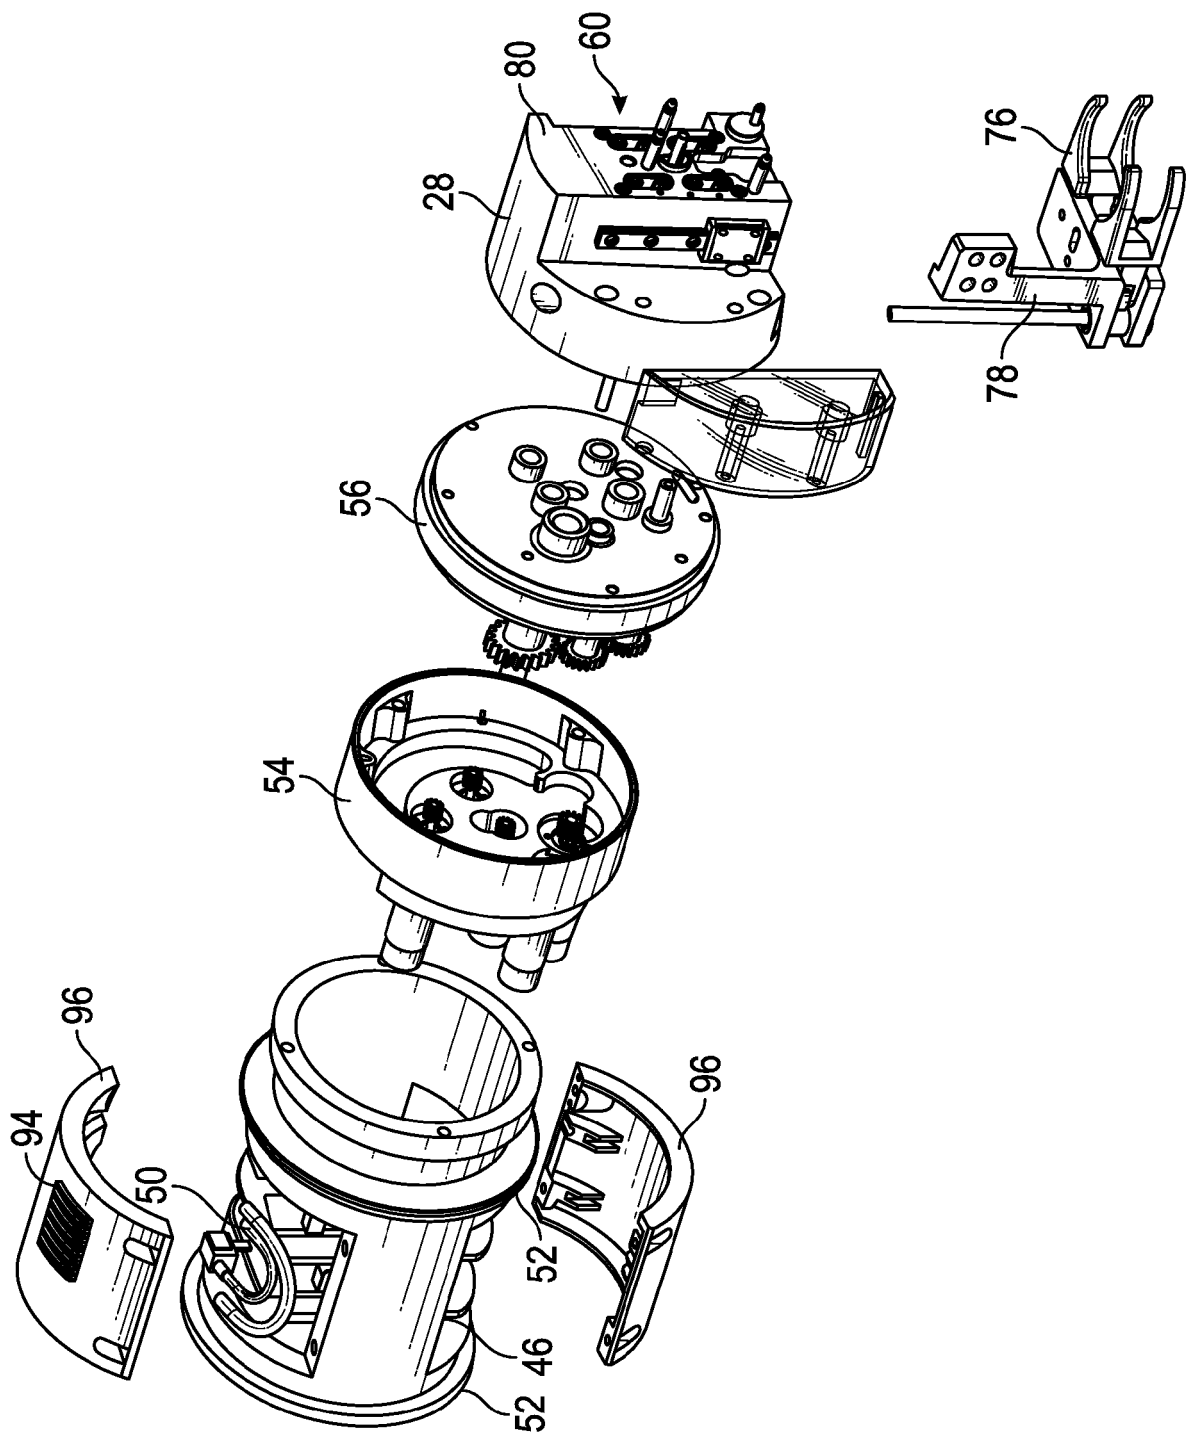


FIG. 5

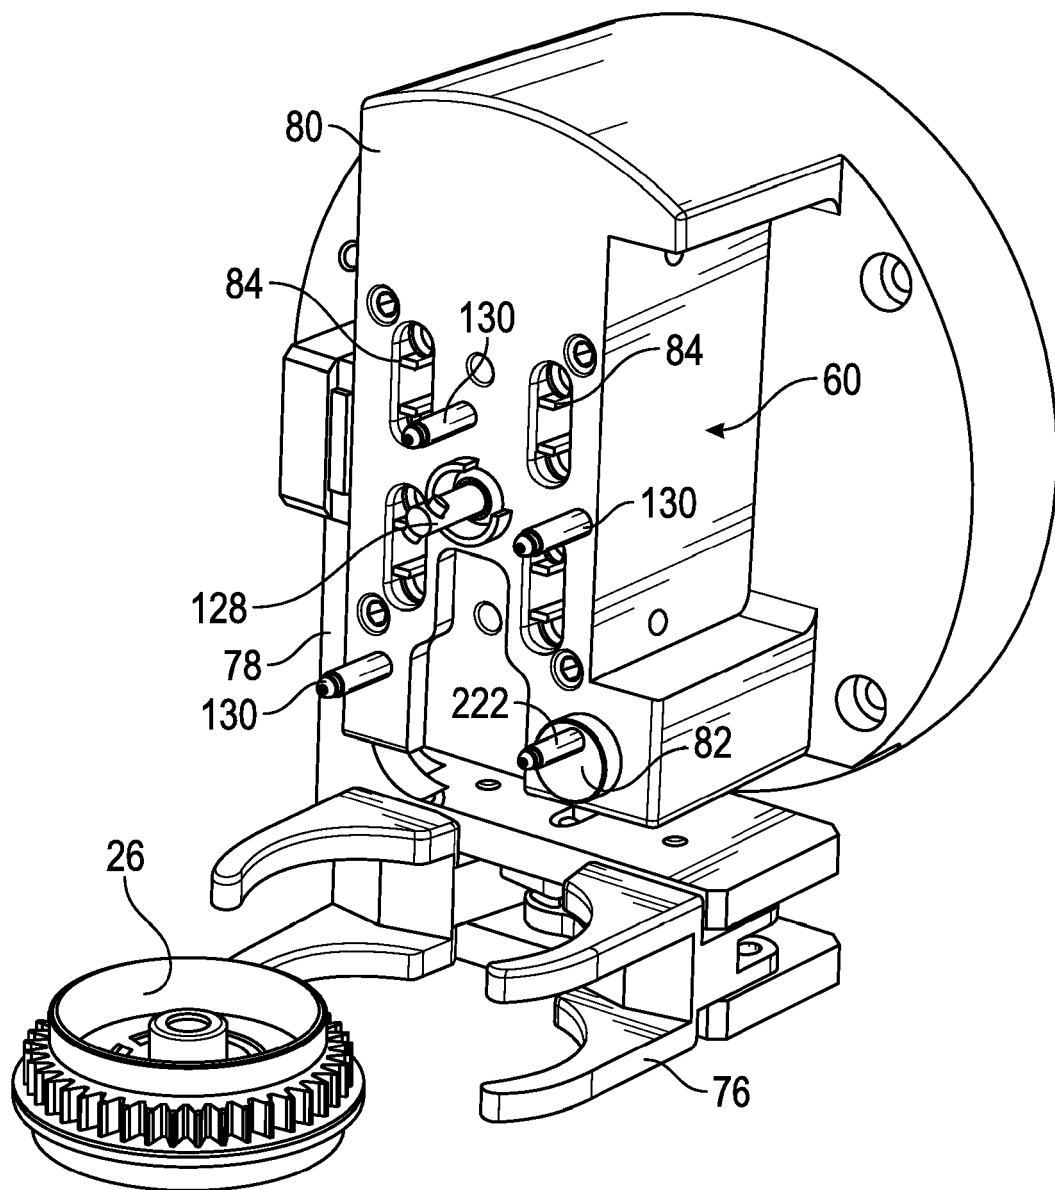


FIG. 6

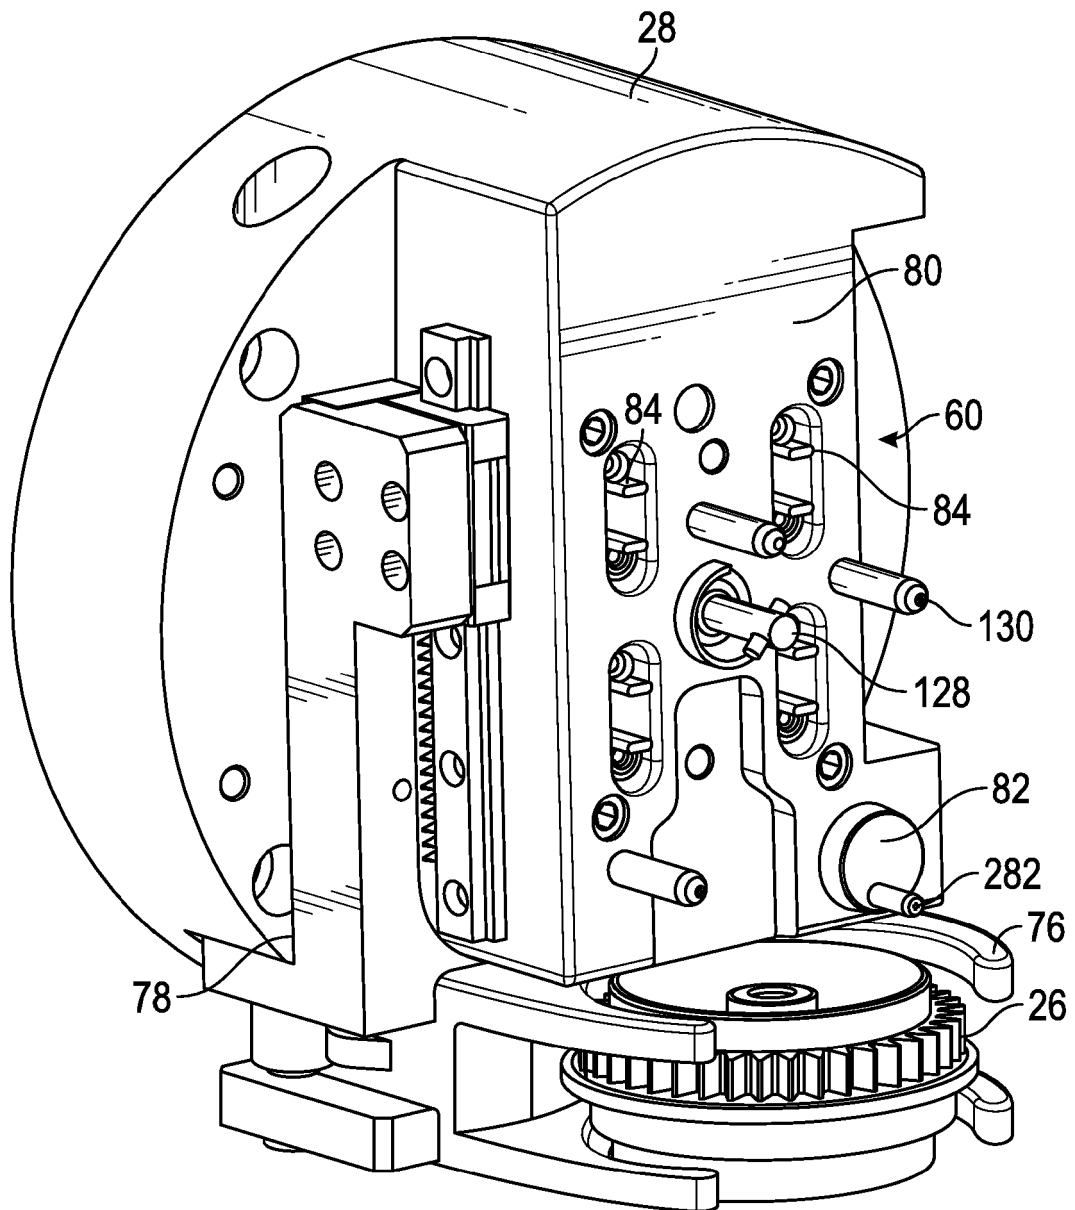


FIG. 7

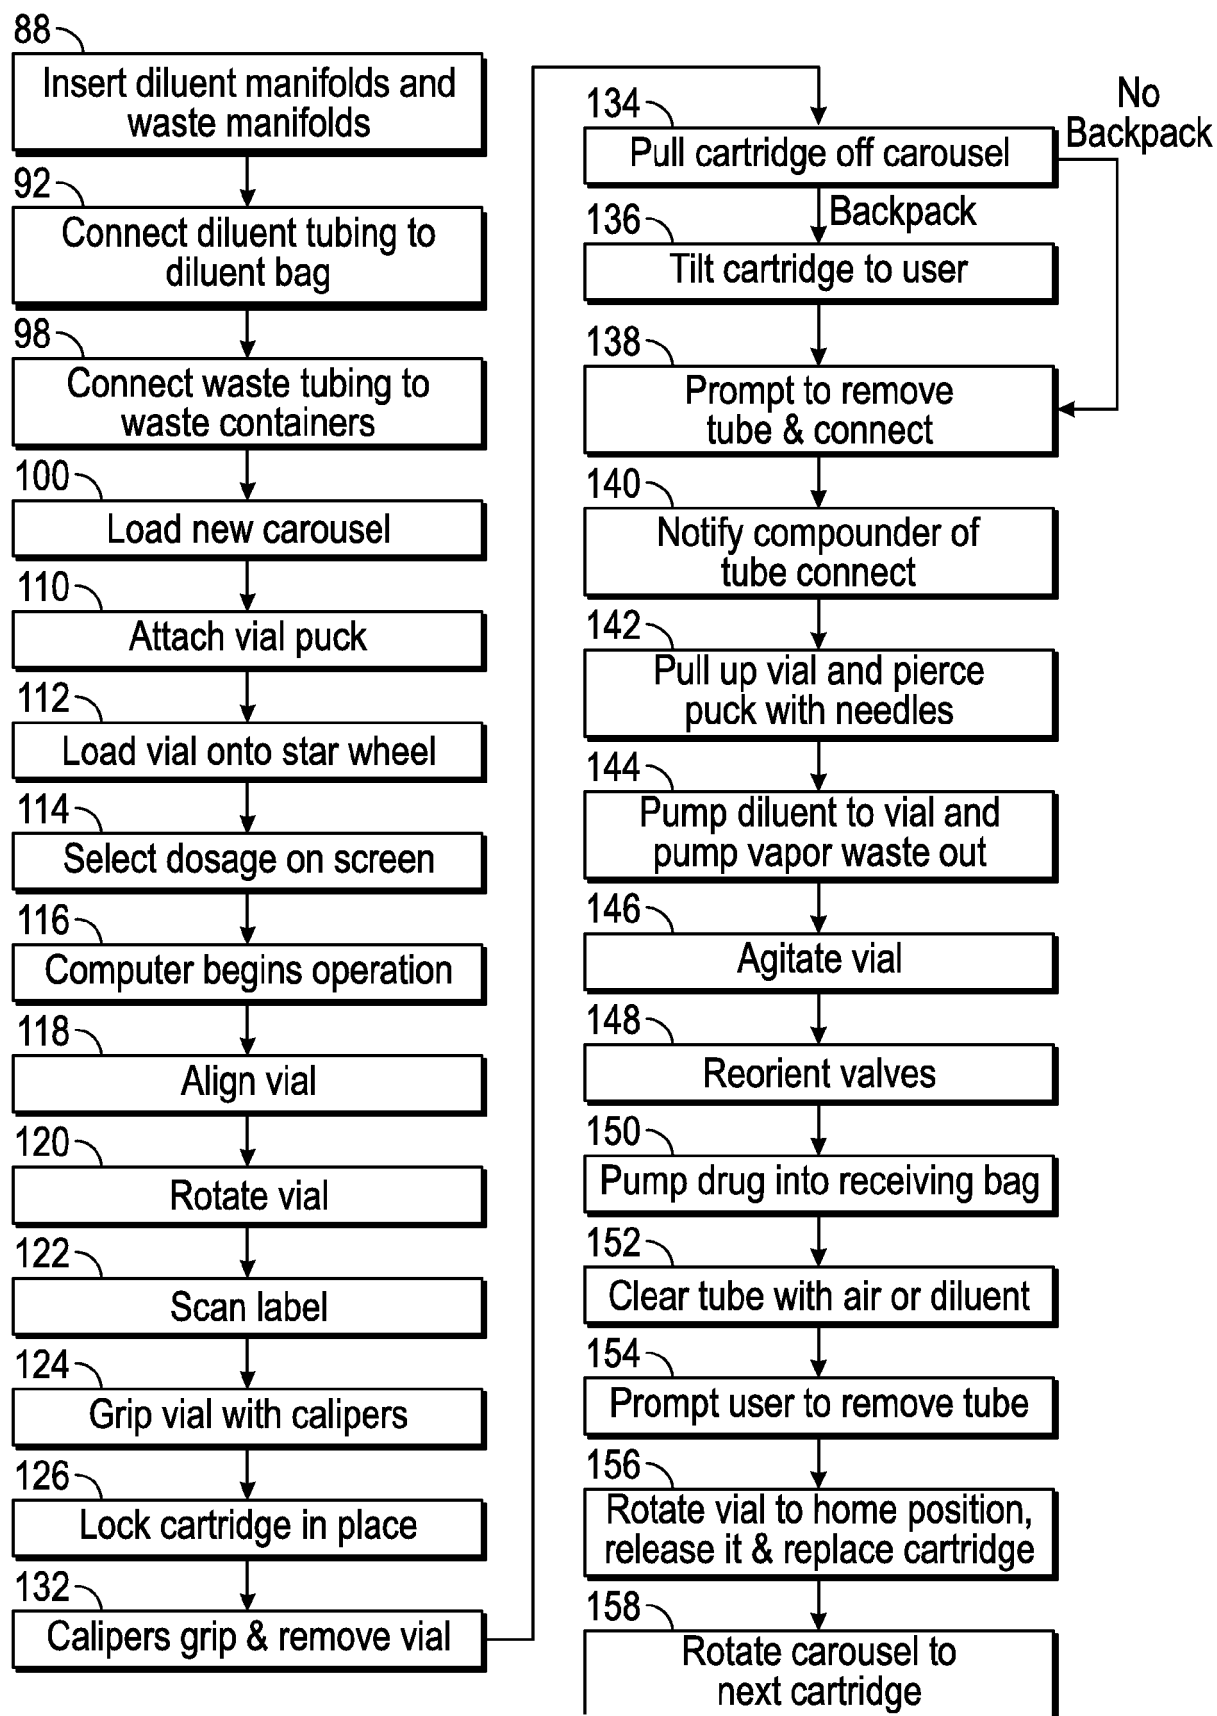


FIG. 8

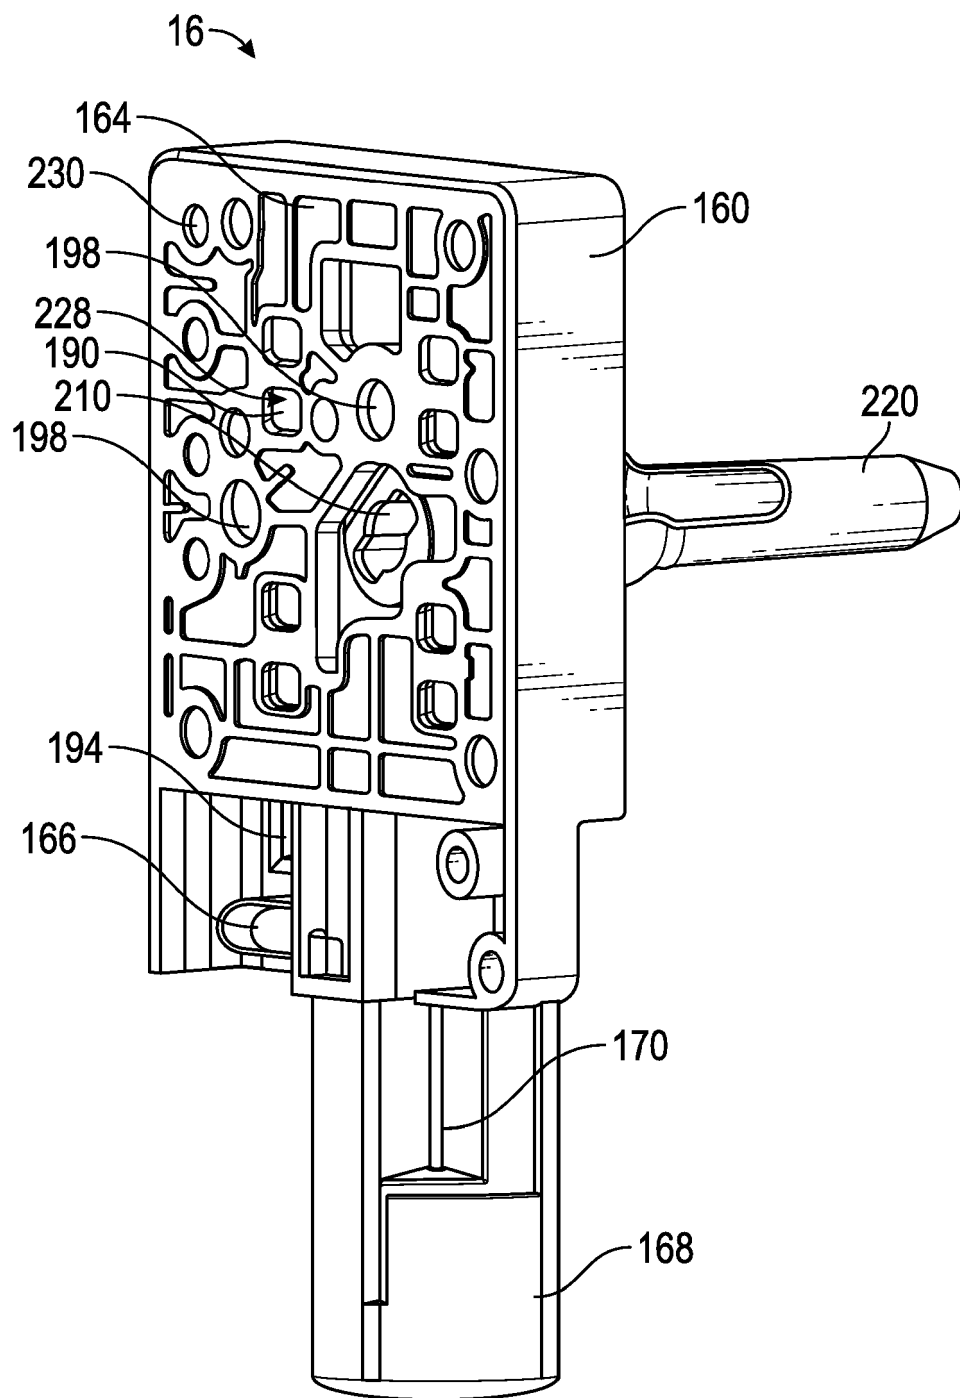


FIG. 9

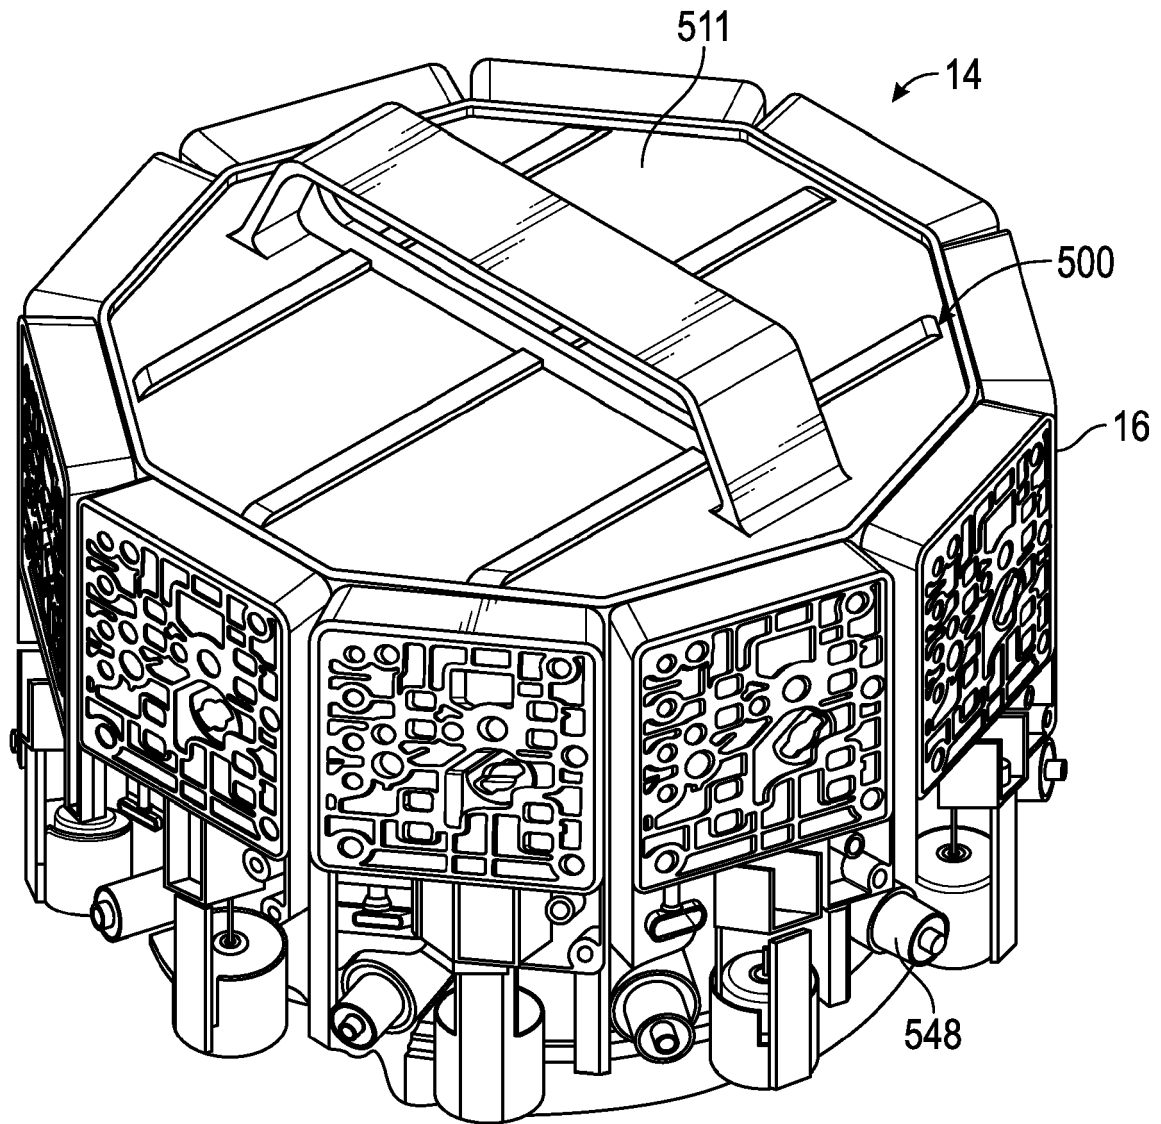


FIG. 10

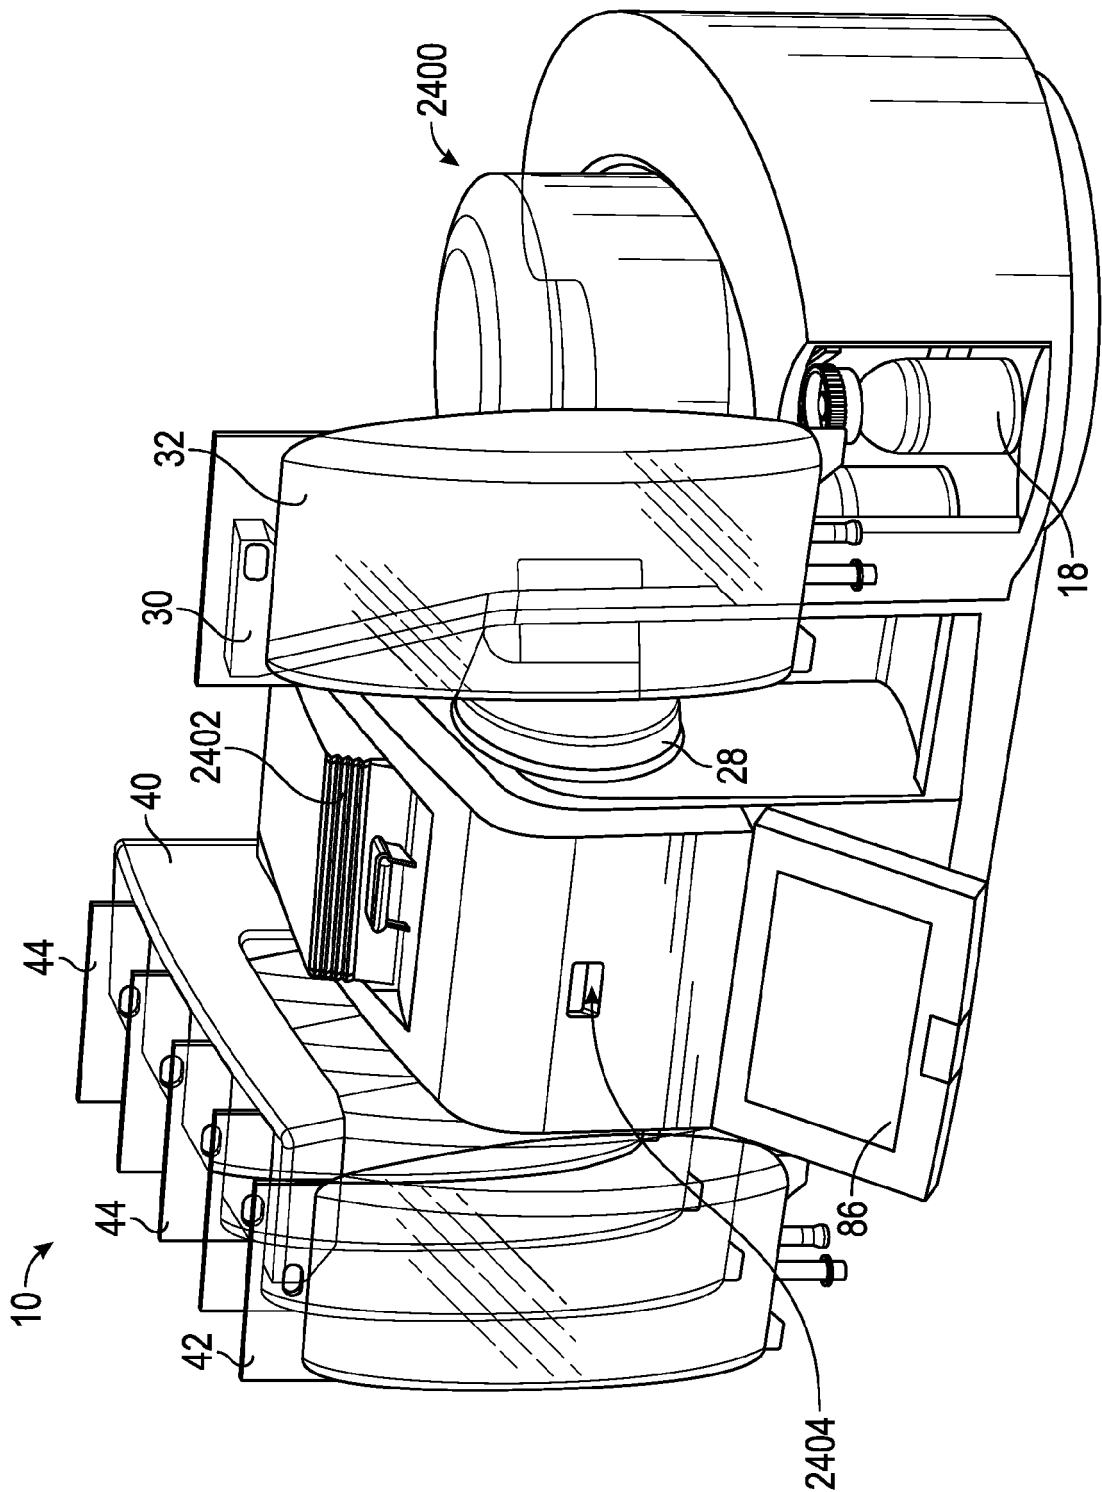


FIG. 11

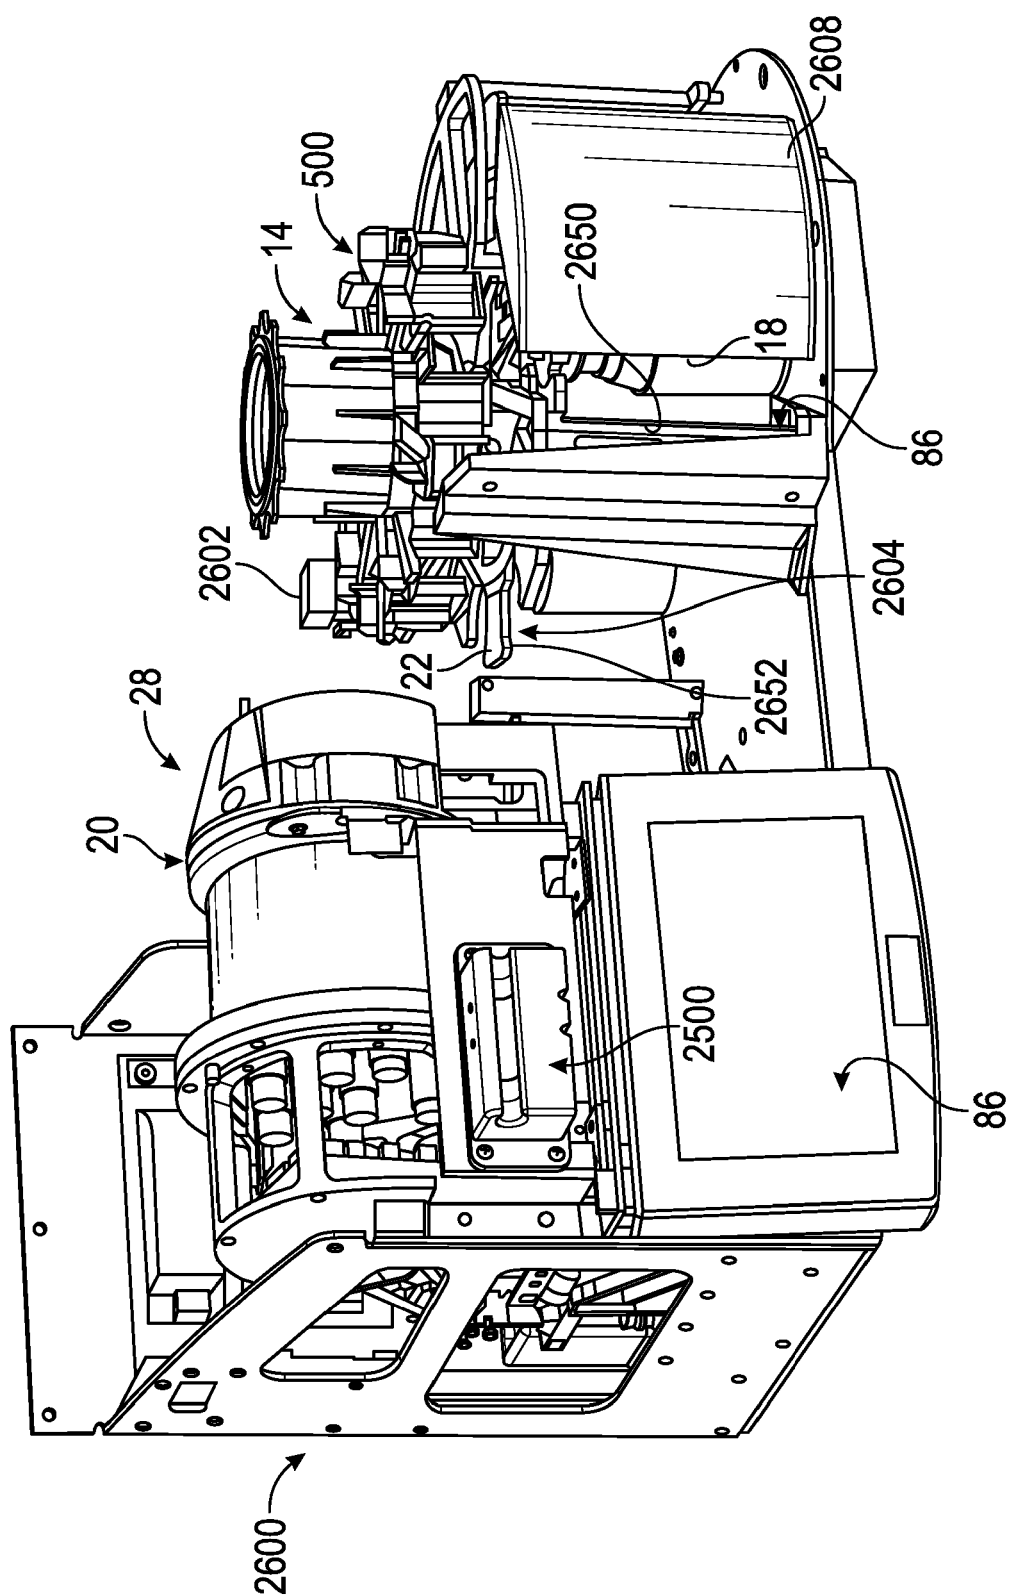


FIG. 12

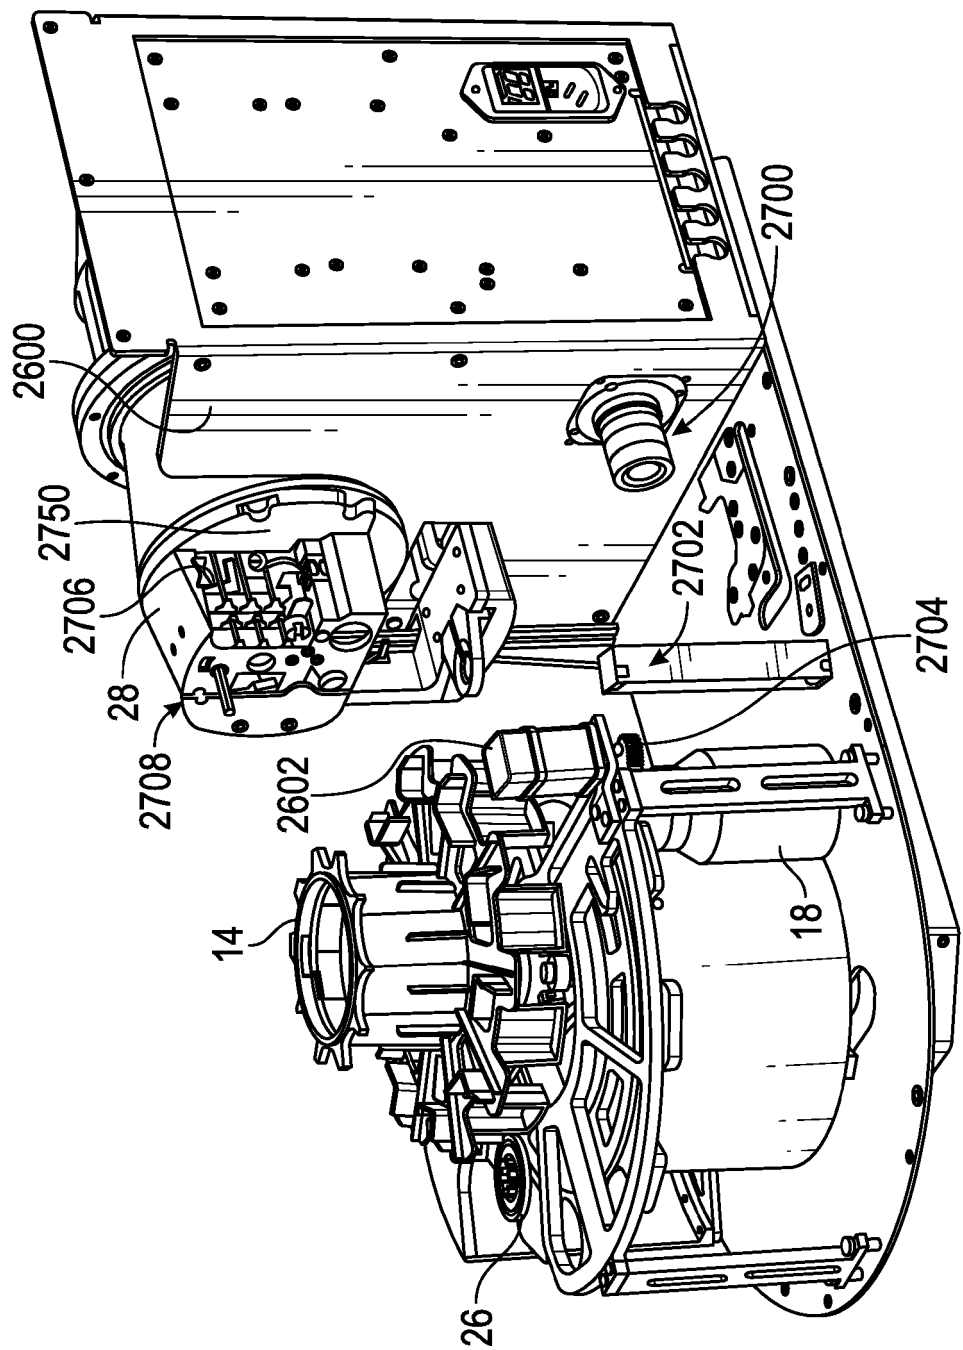


FIG. 13

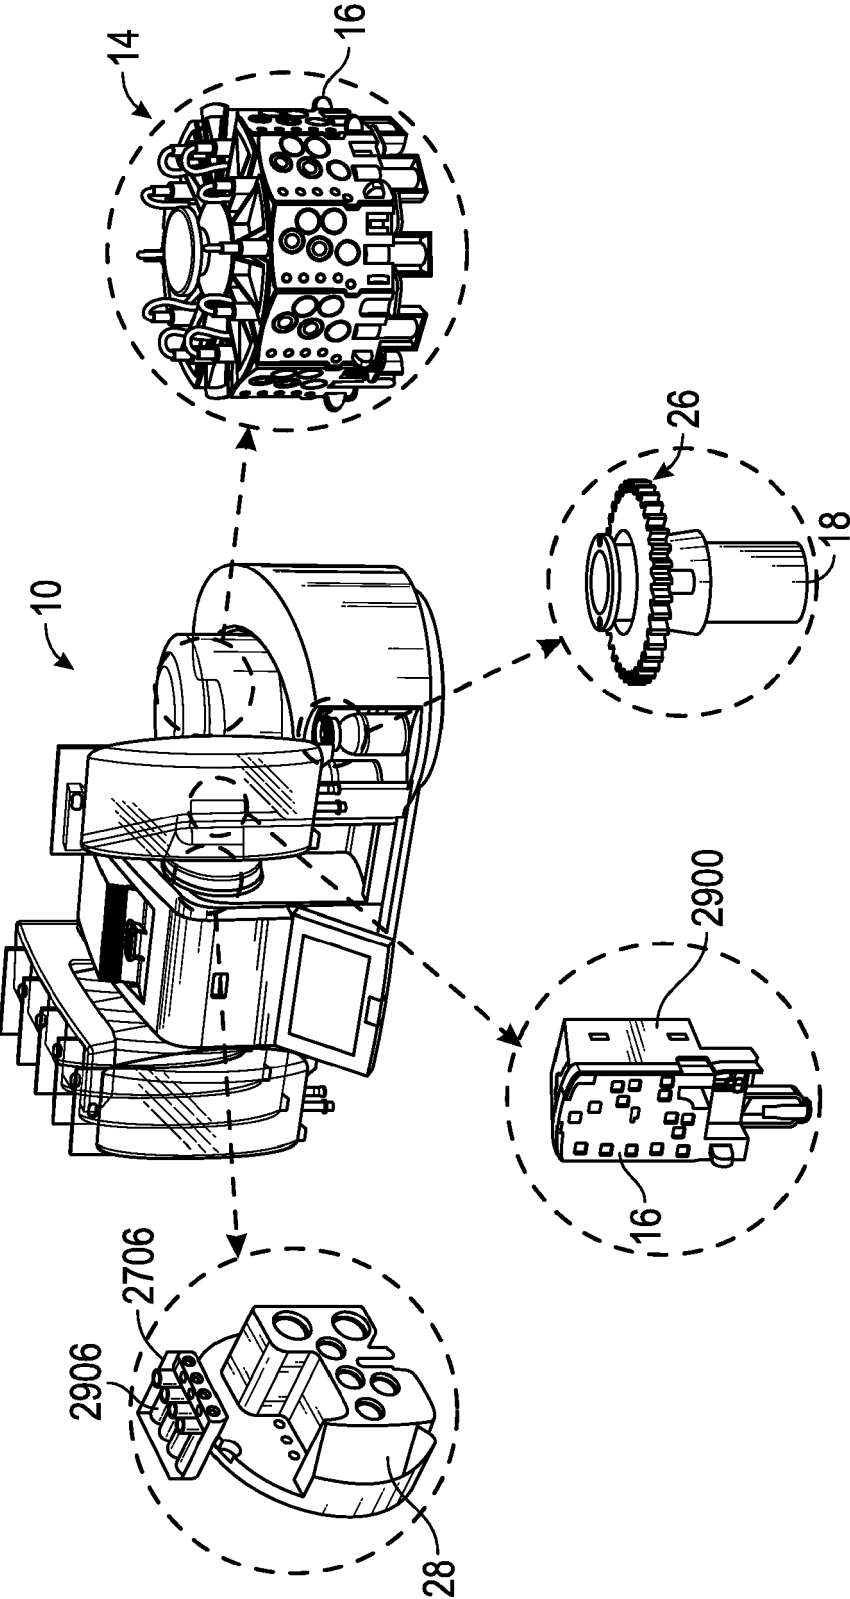


FIG. 14

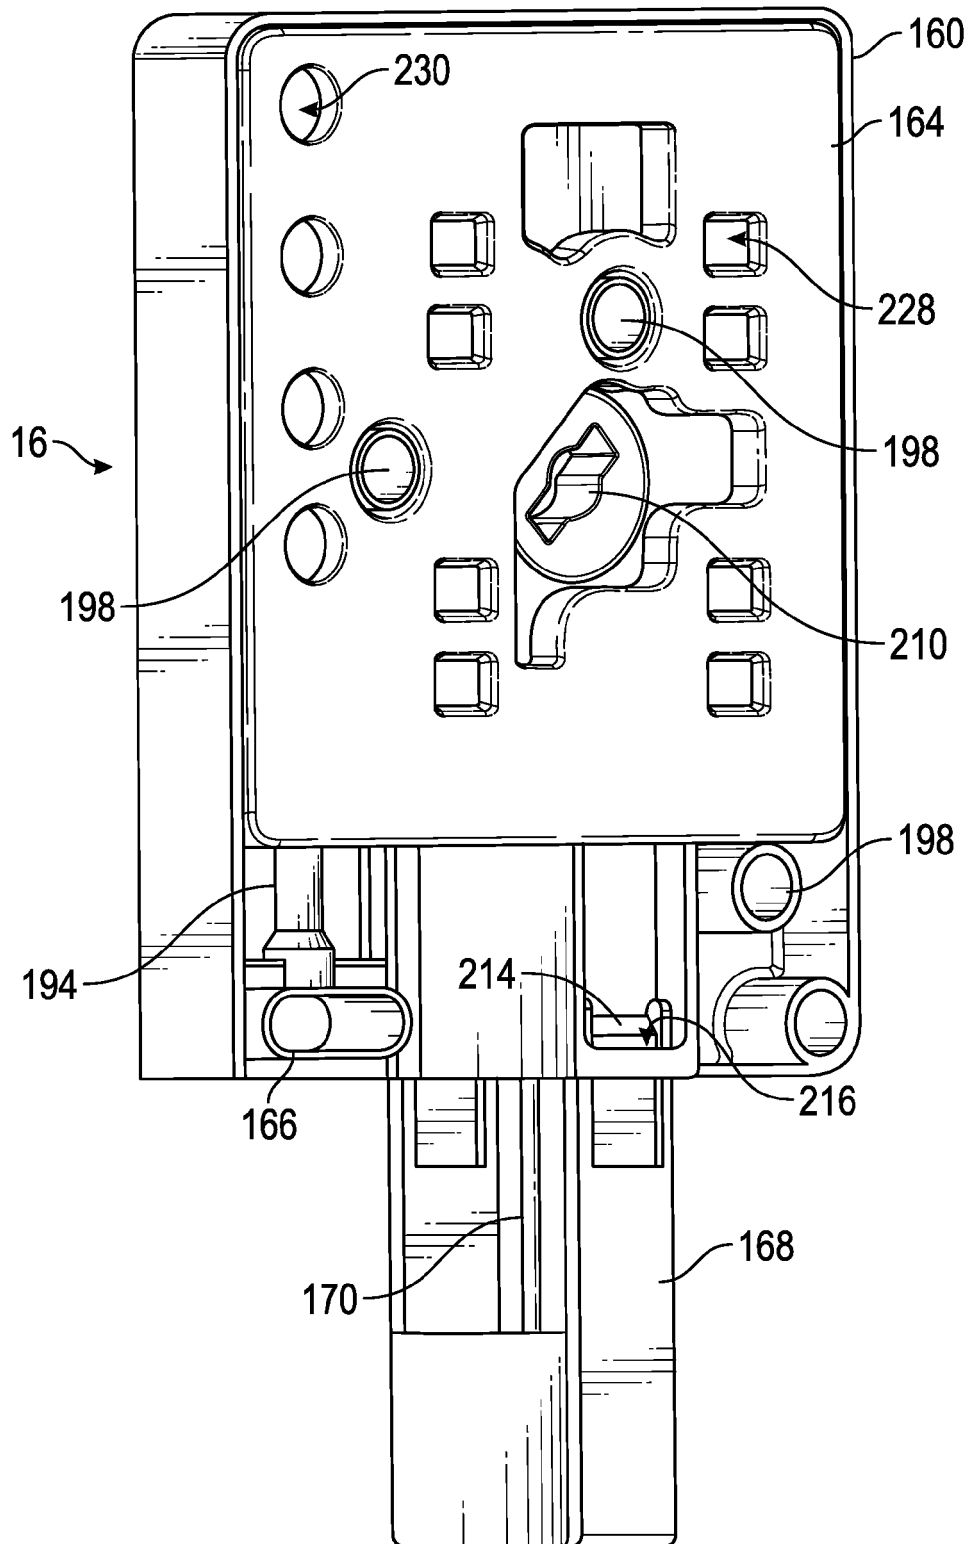


FIG. 15

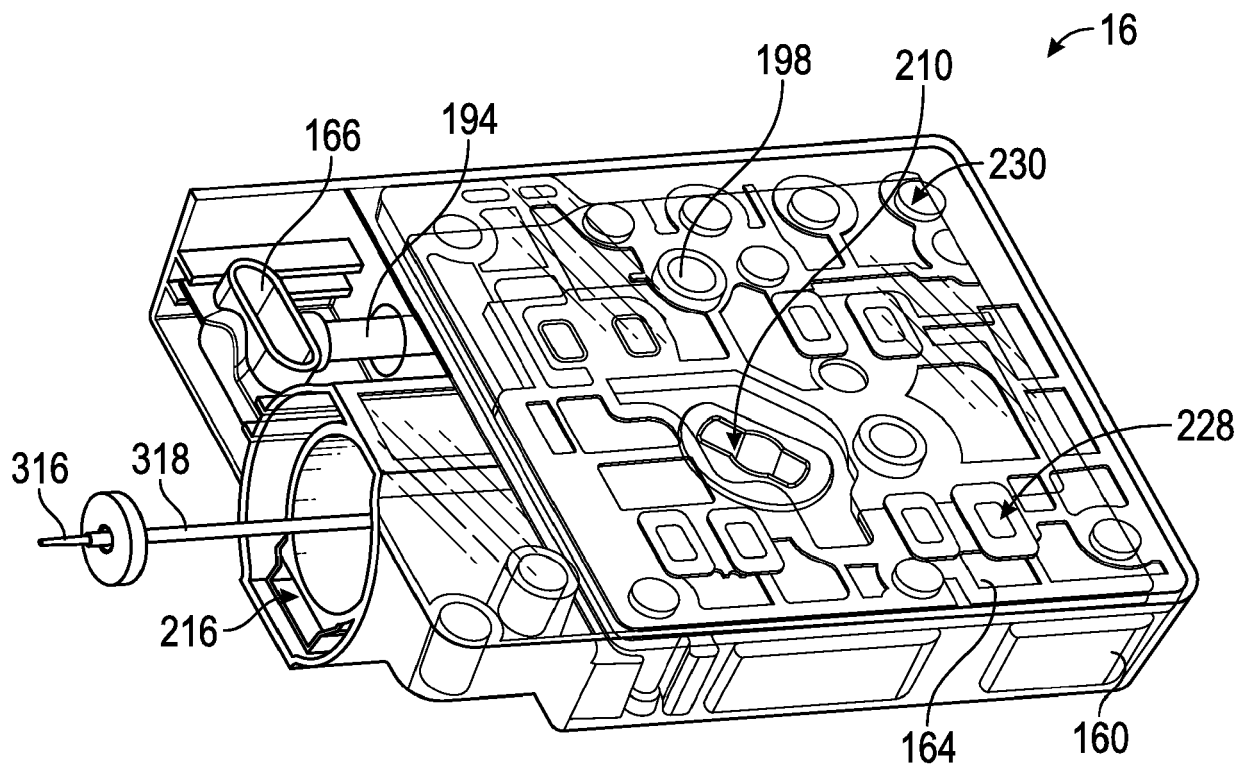


FIG. 16

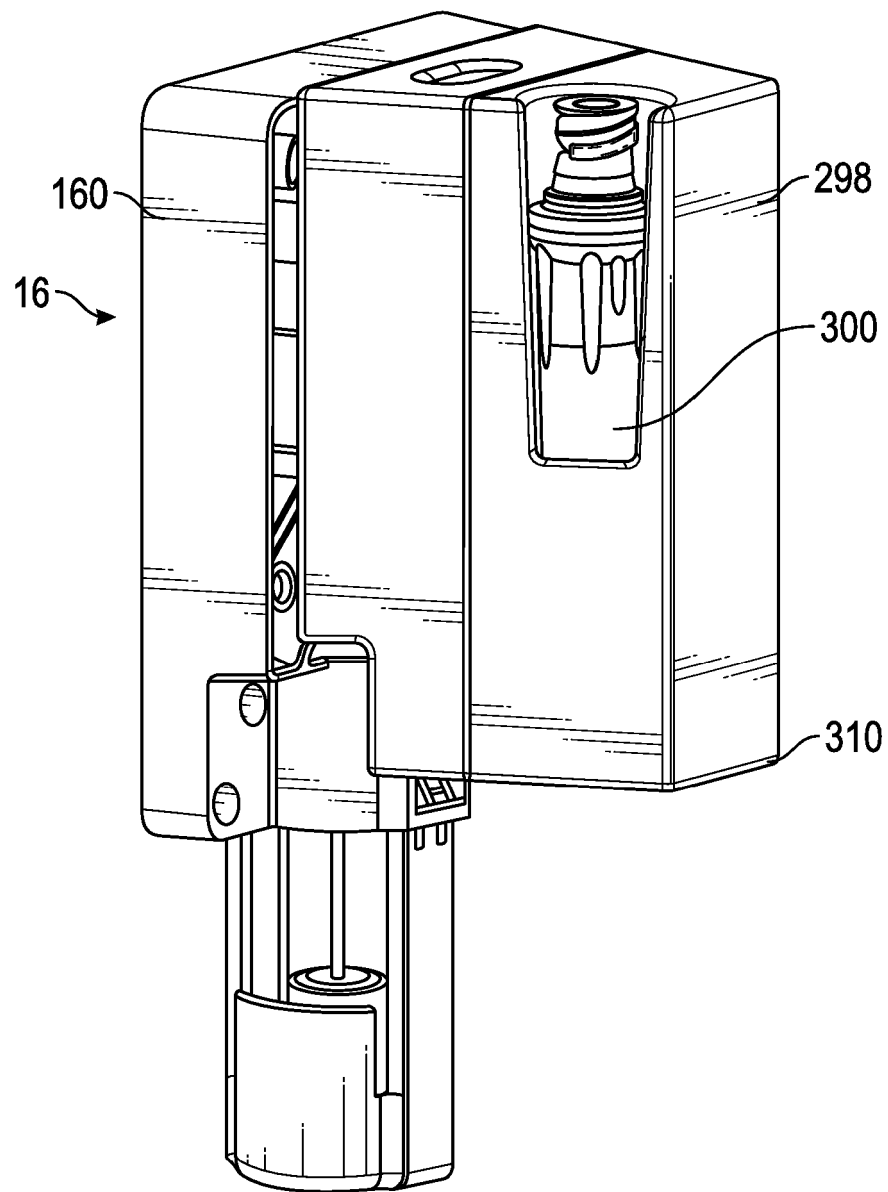


FIG. 17

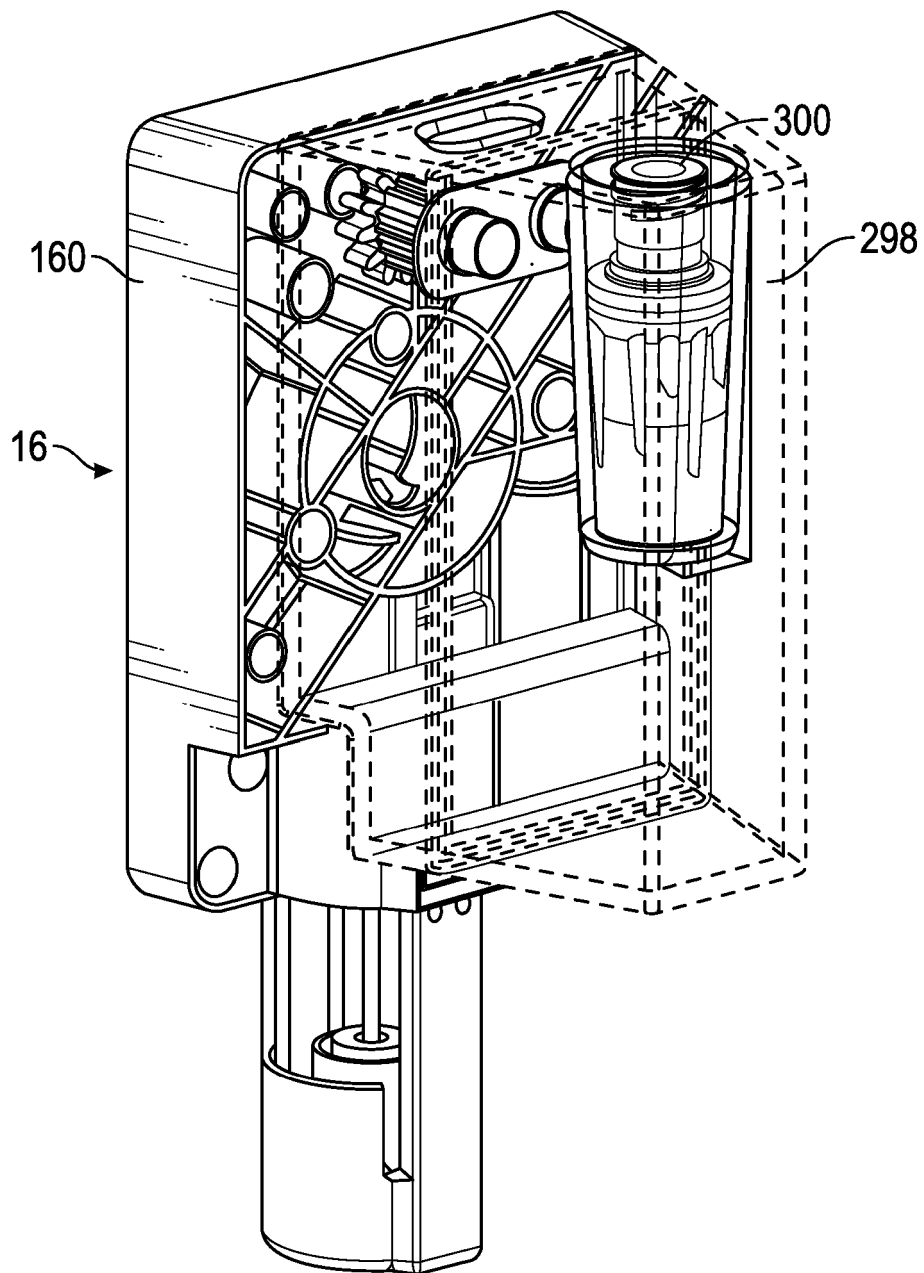


FIG. 18

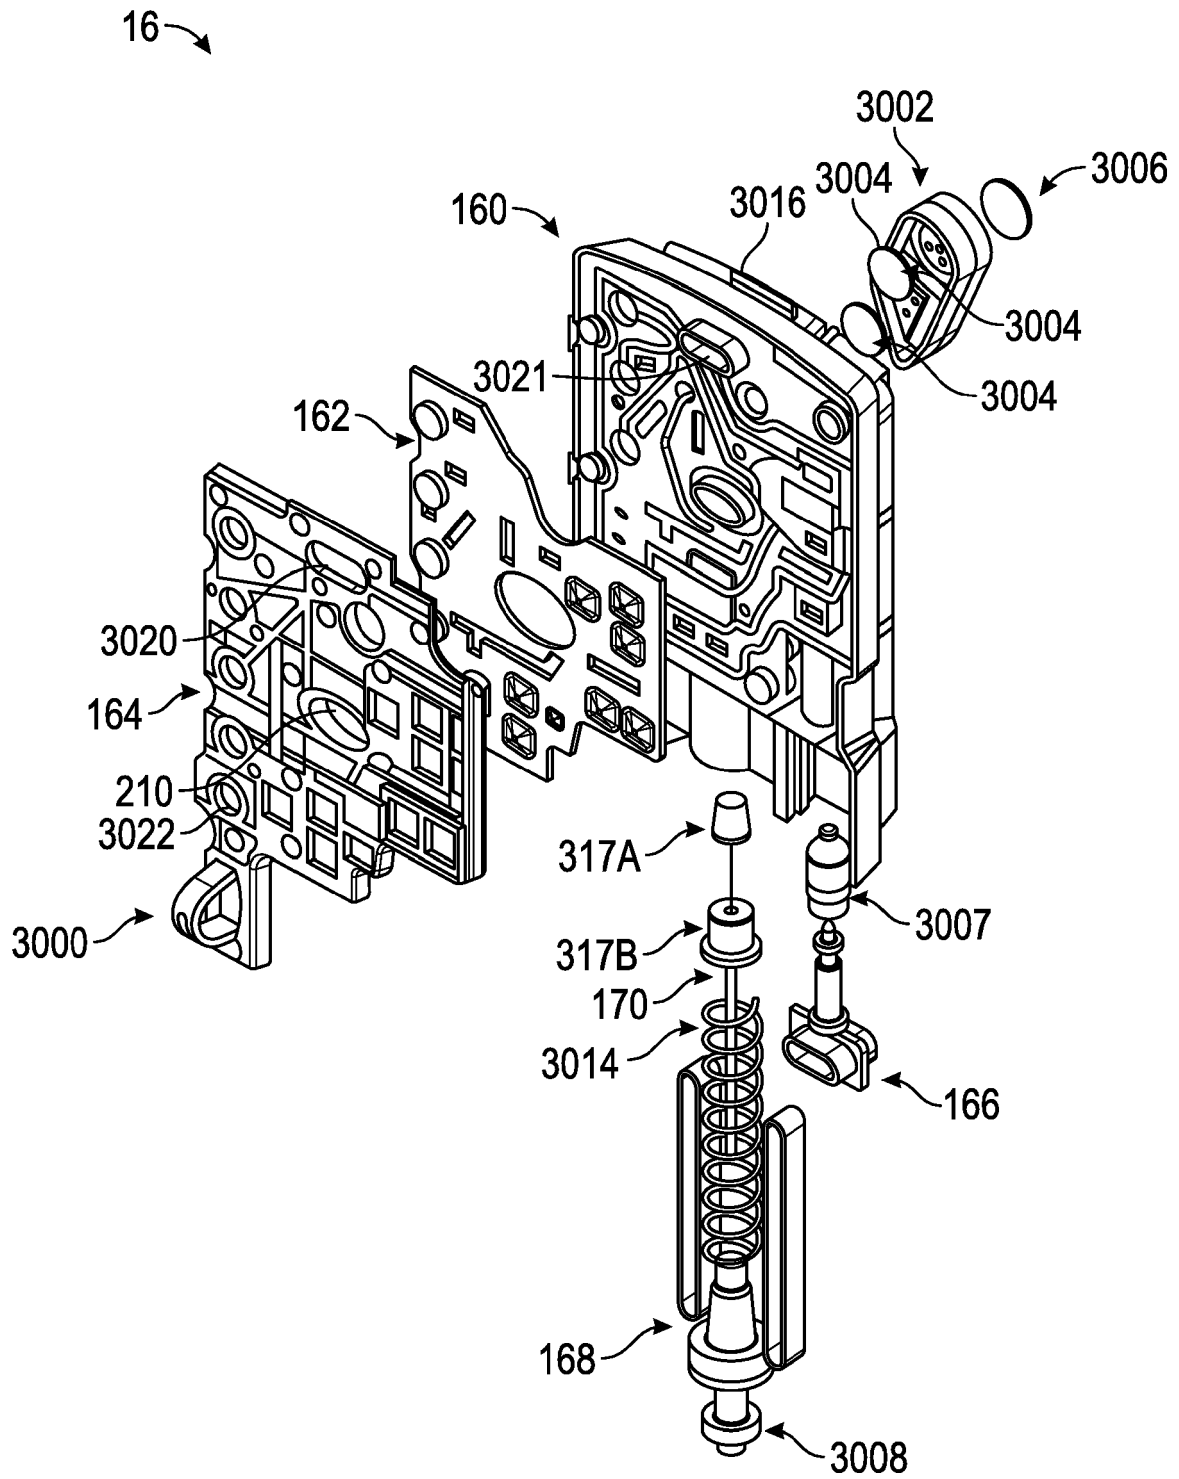


FIG. 19

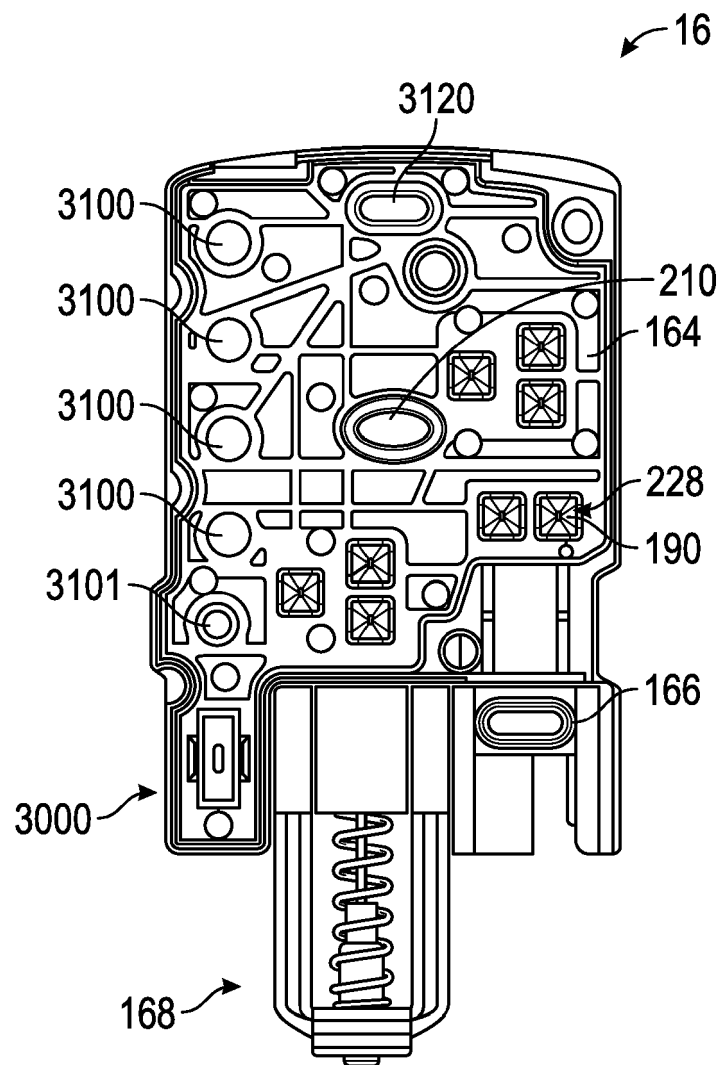


FIG. 20A

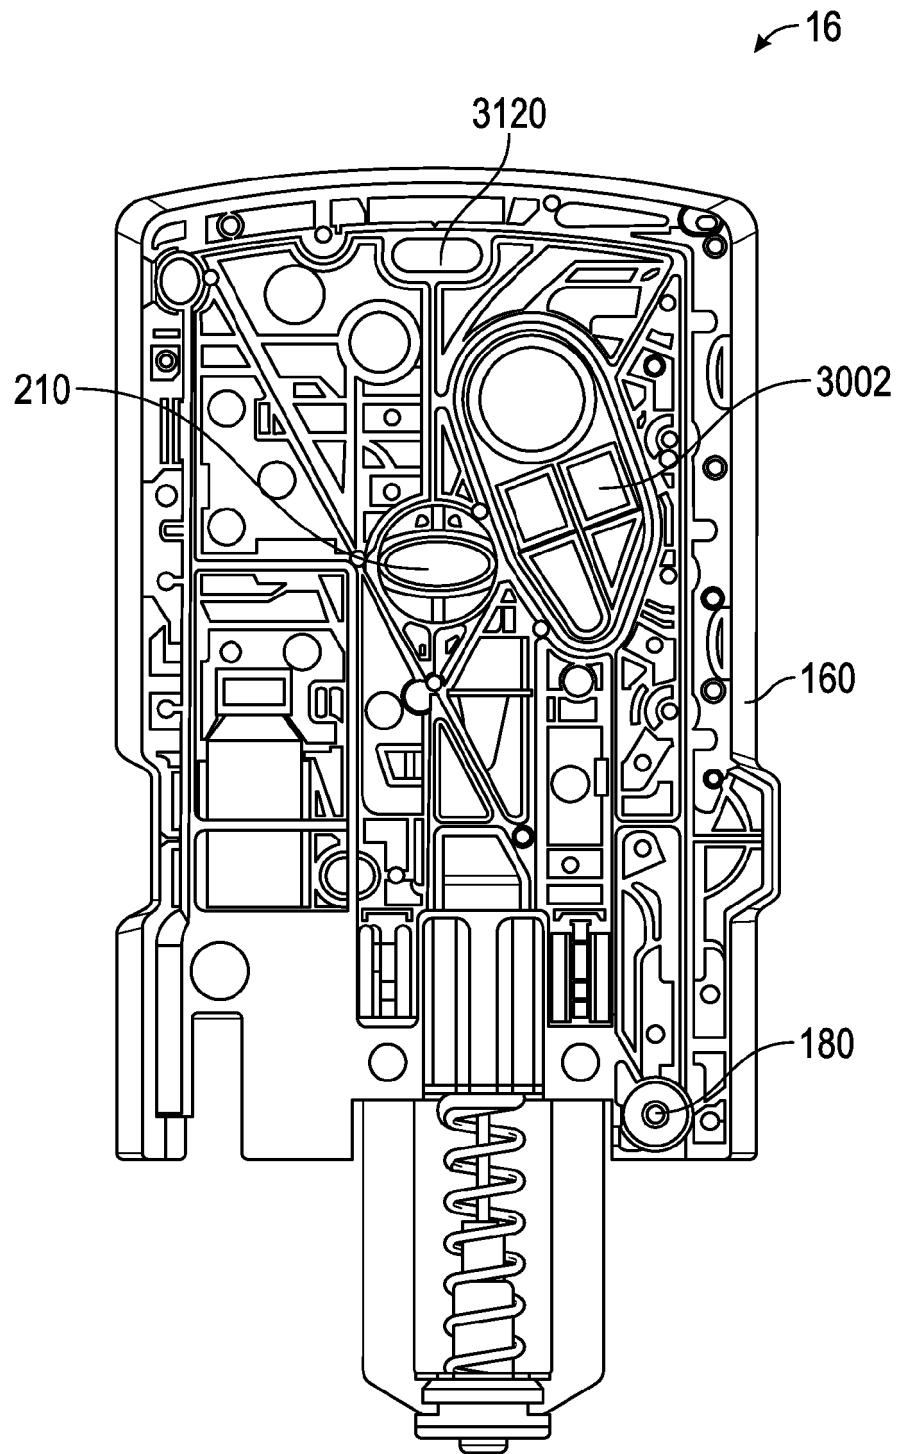
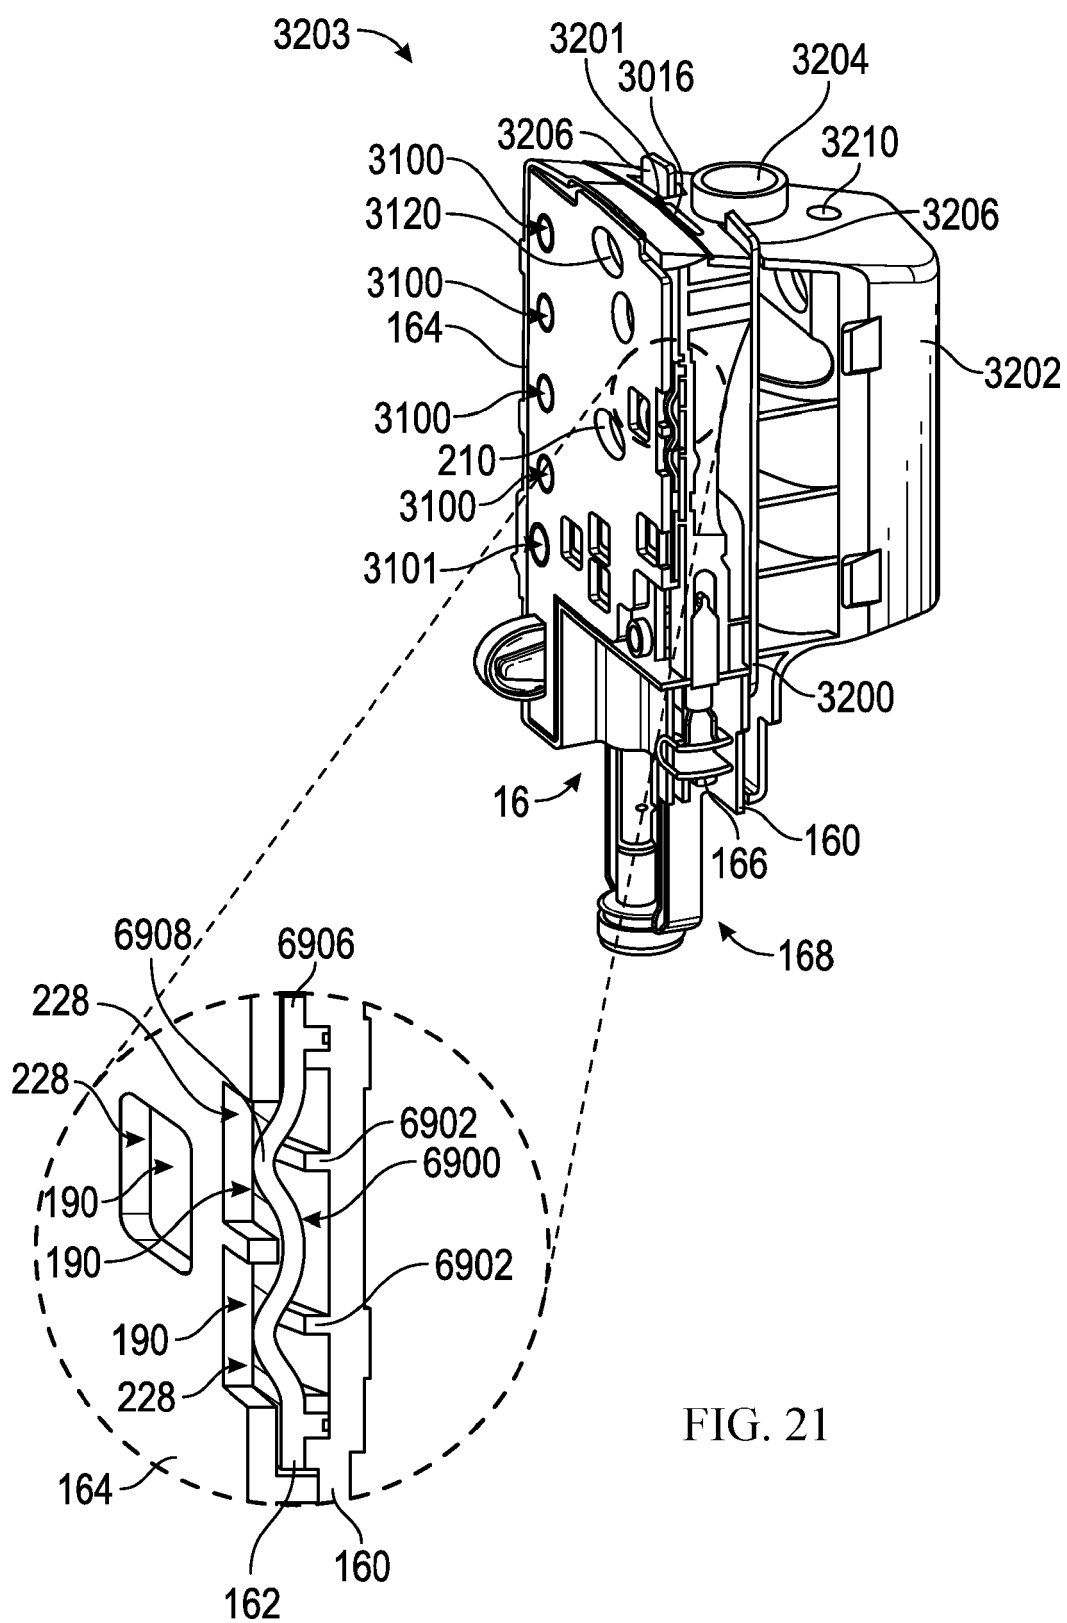


FIG. 20B



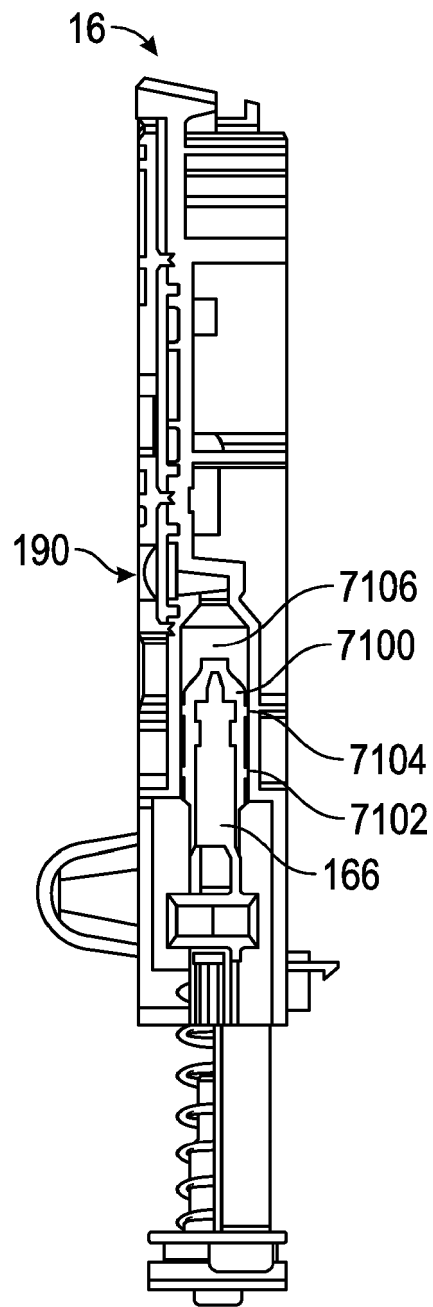


FIG. 22

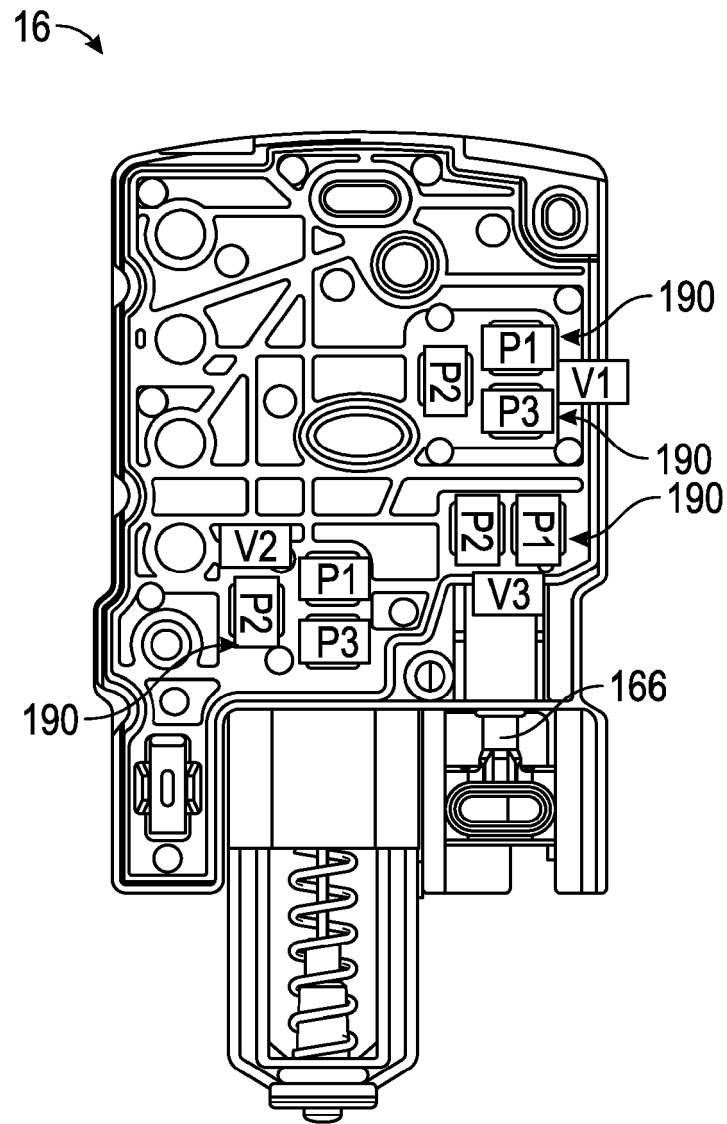


FIG. 23

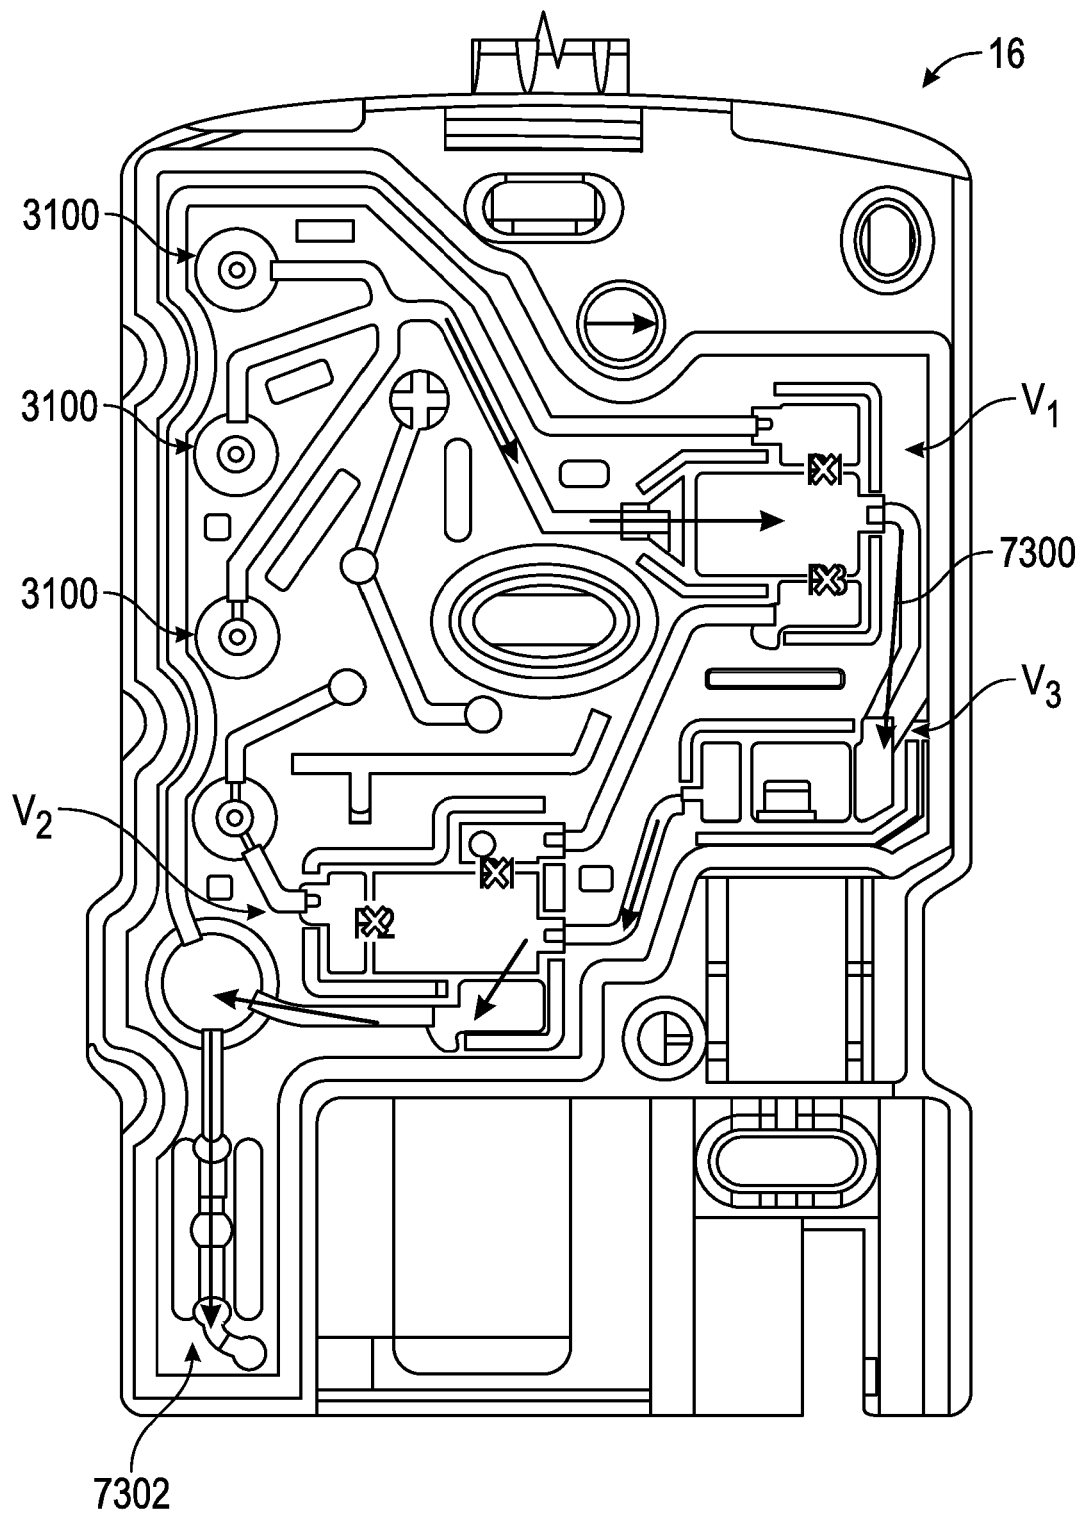


FIG. 24

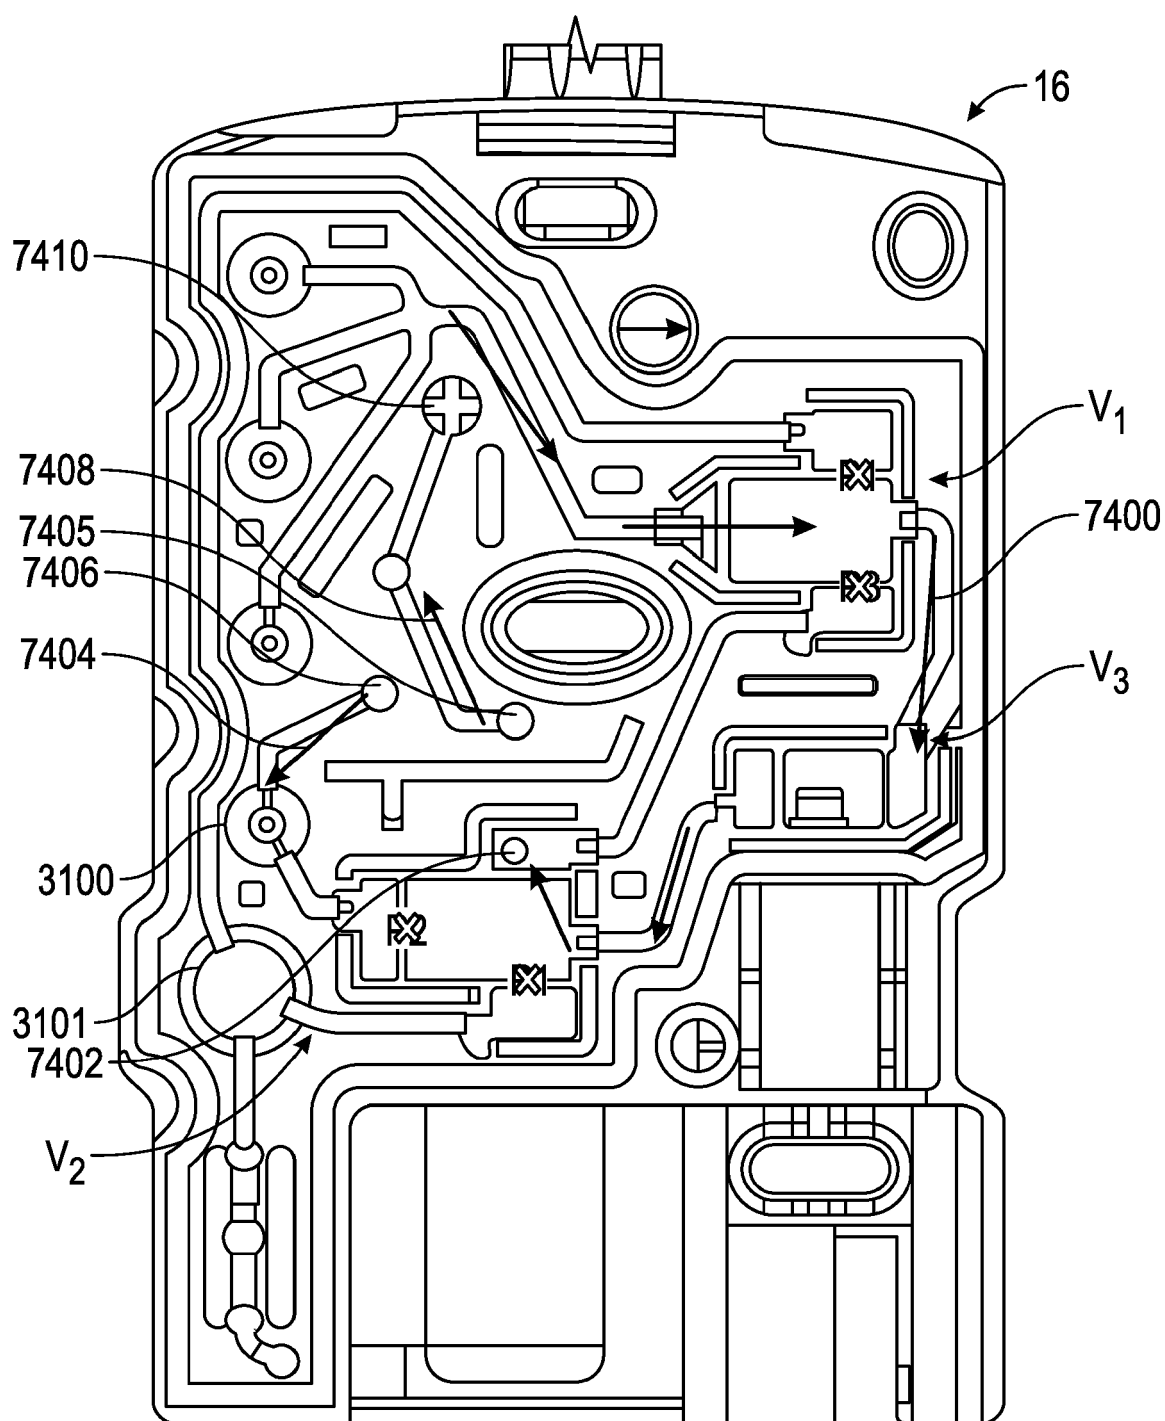


FIG. 25

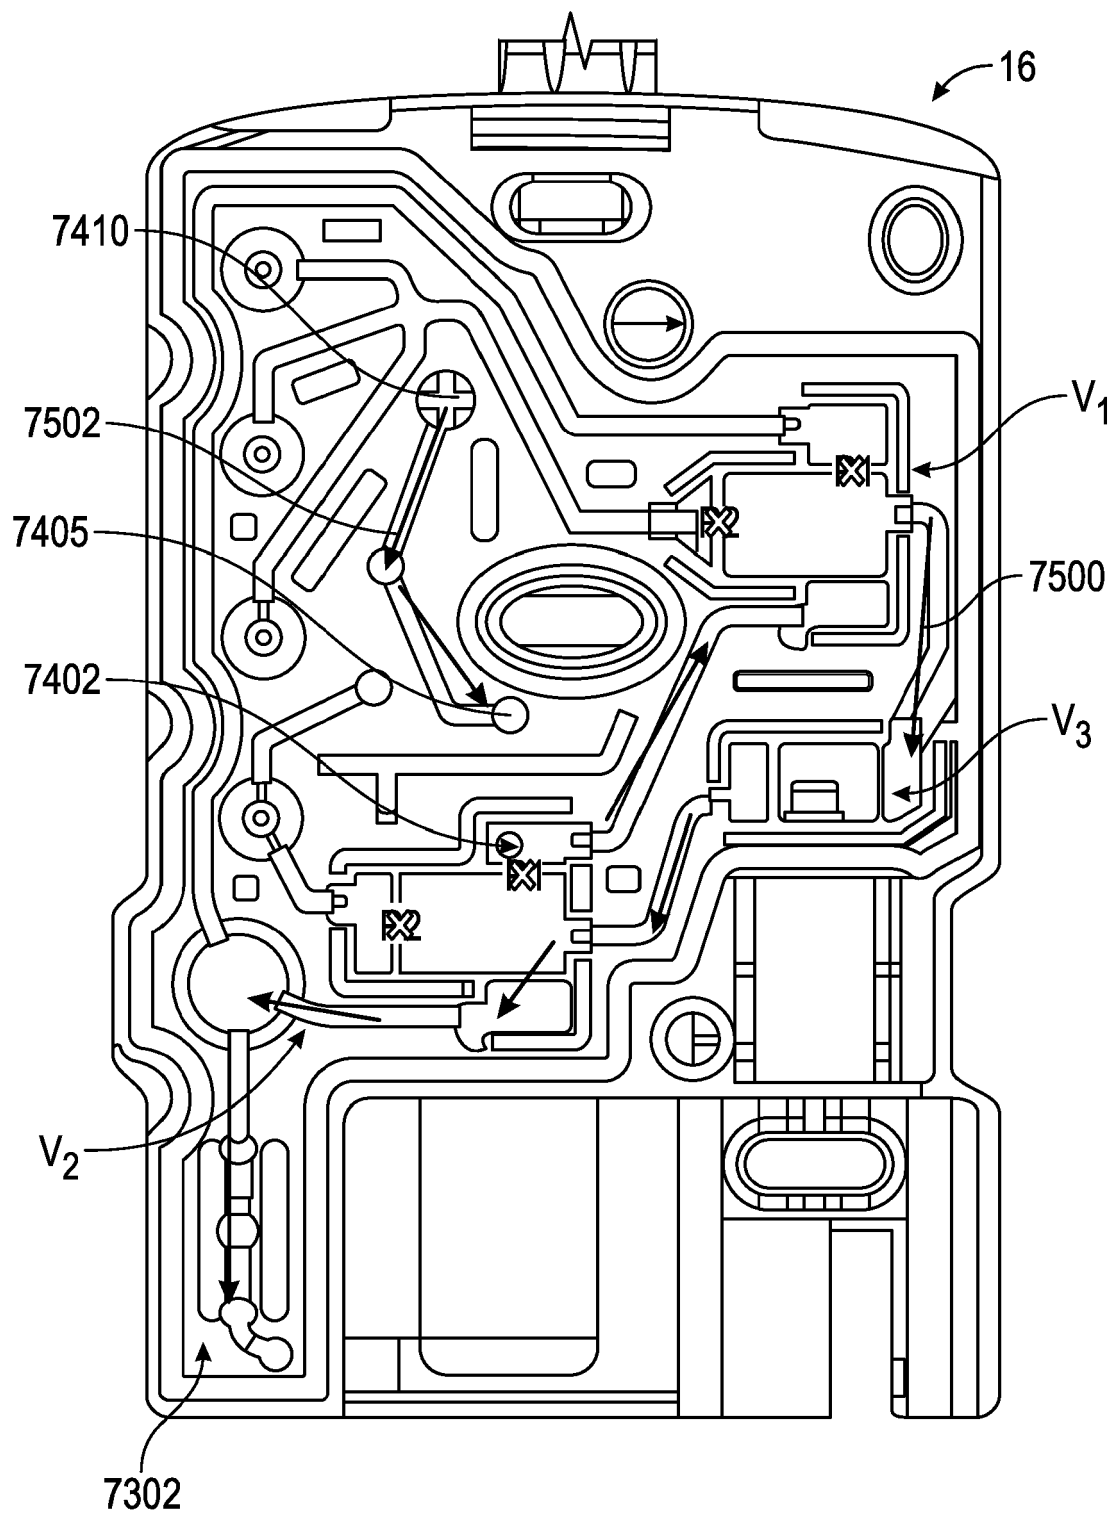


FIG. 26

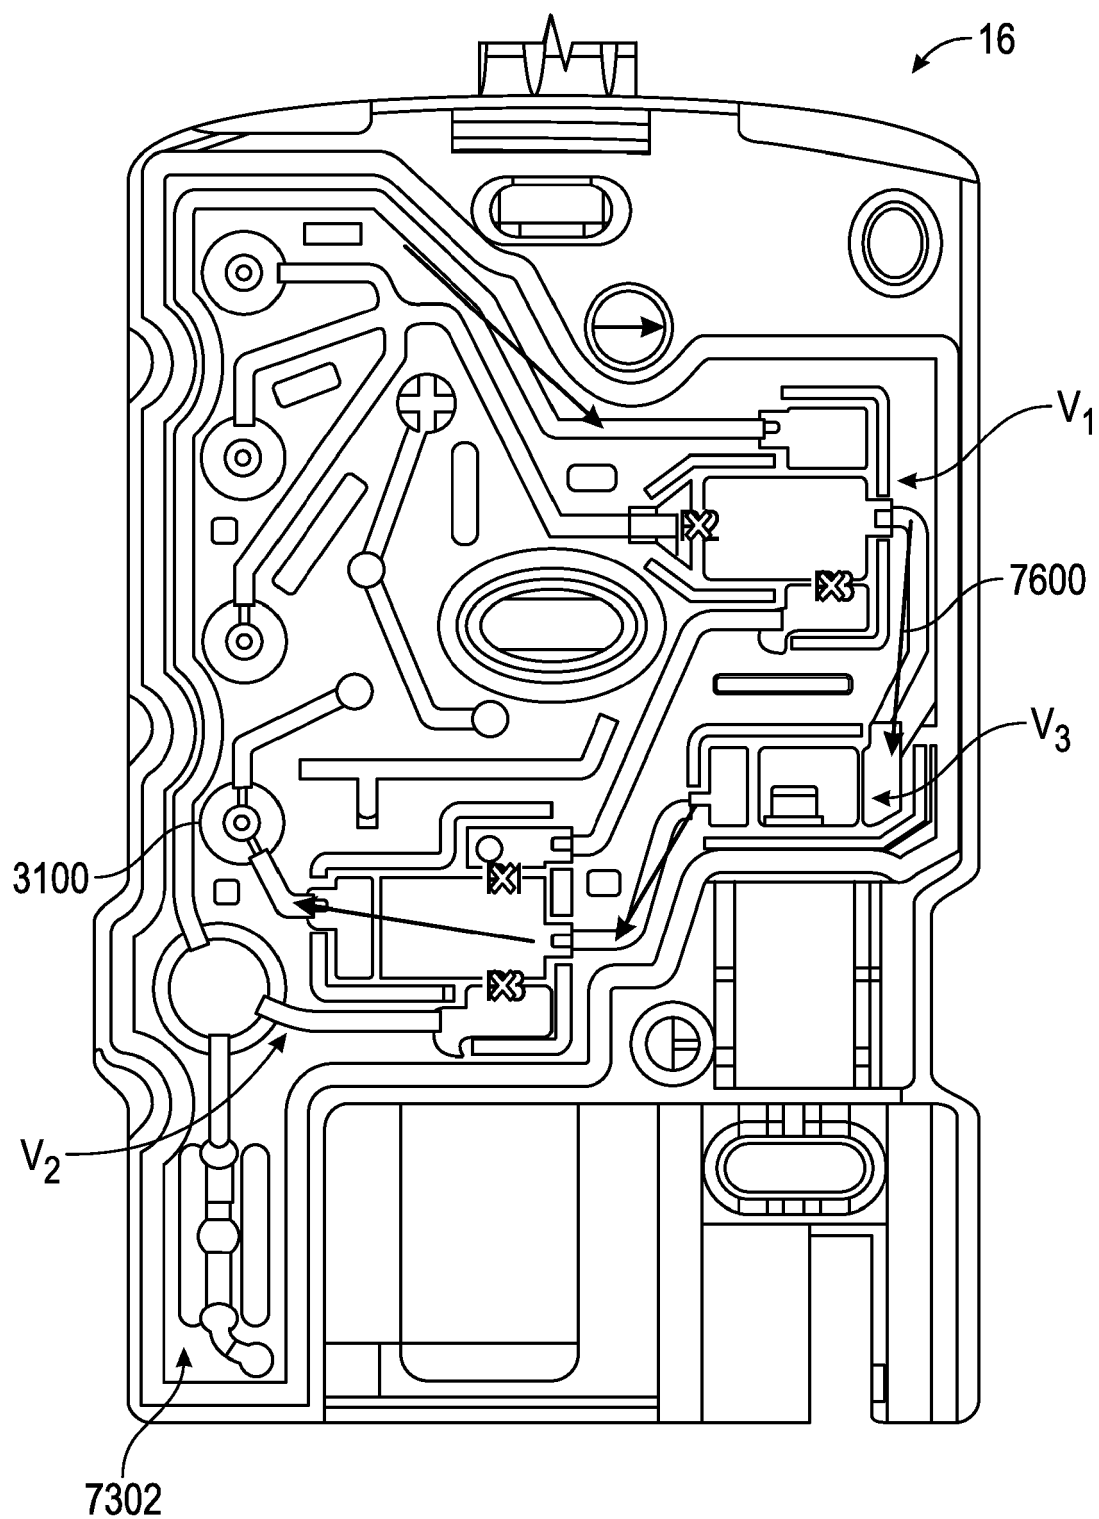


FIG. 27

Operation	Valve 1 Diluent			Valve 2 RC		
	P1	P2	P3	P1	P2	P3
Diluent to Receiving Container	Closed	Open	Closed	Closed	Closed	Open
Diluent to Vial	Closed	Open	Closed	Open	Closed	Closed
Vial to Receiving Container	Closed	Closed	Open	Closed	Closed	Open
Pull Air Back from Receiving Container	Open	Closed	Closed	Closed	Open	Closed

FIG. 28

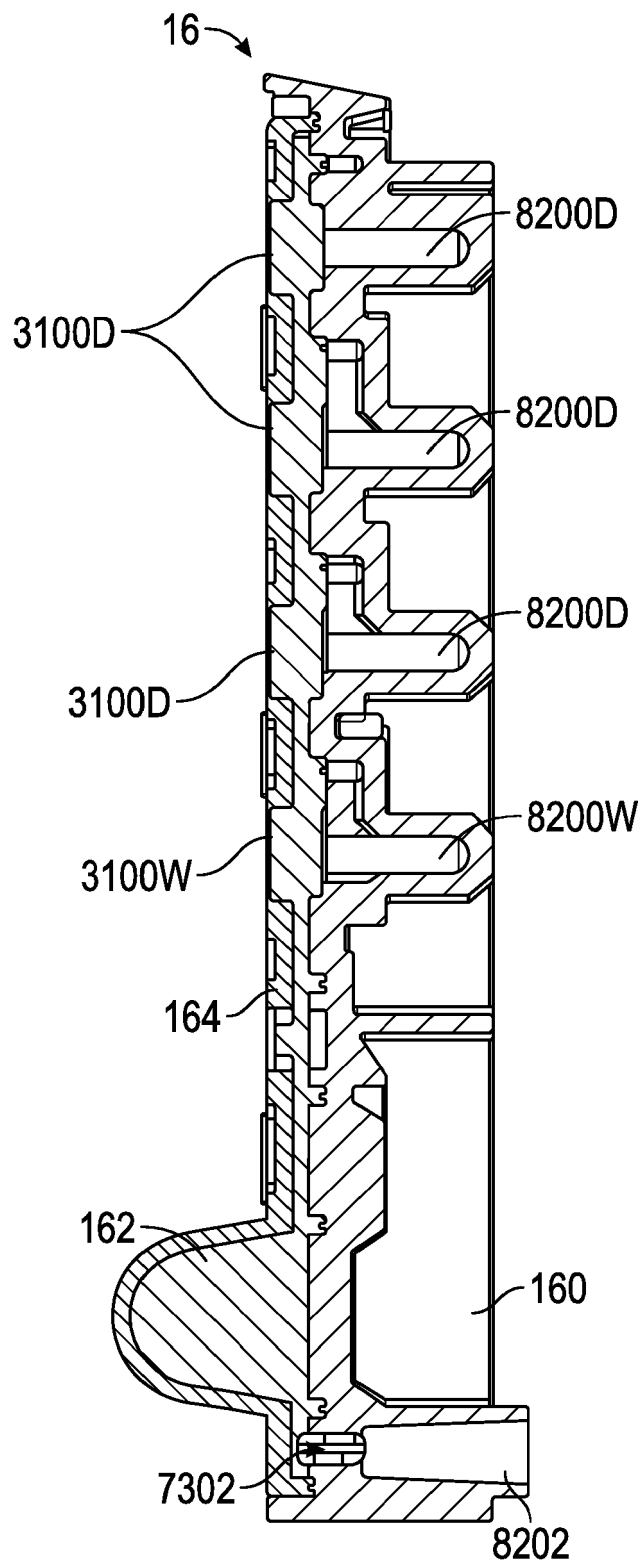


FIG. 29A

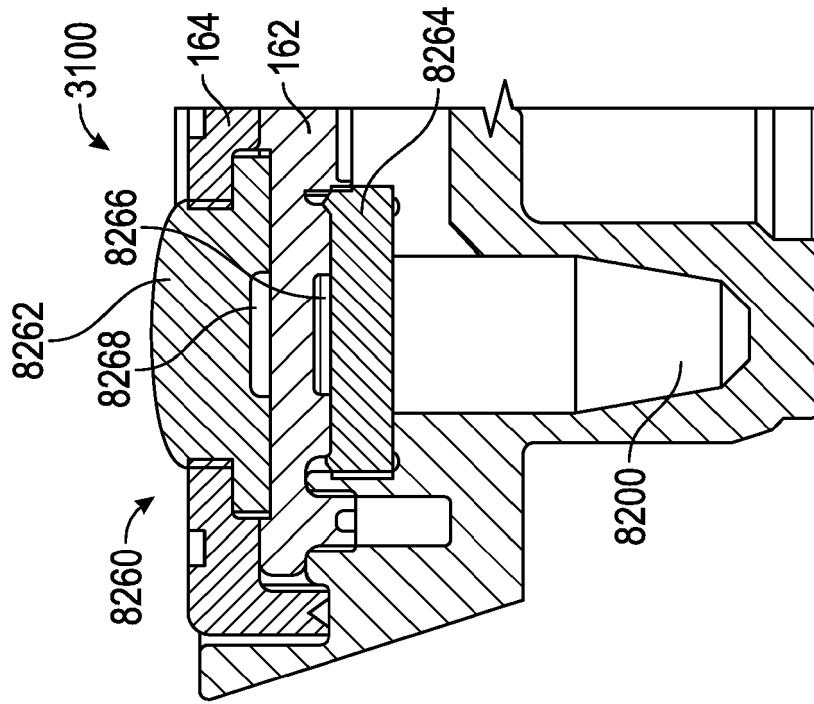


FIG. 29C

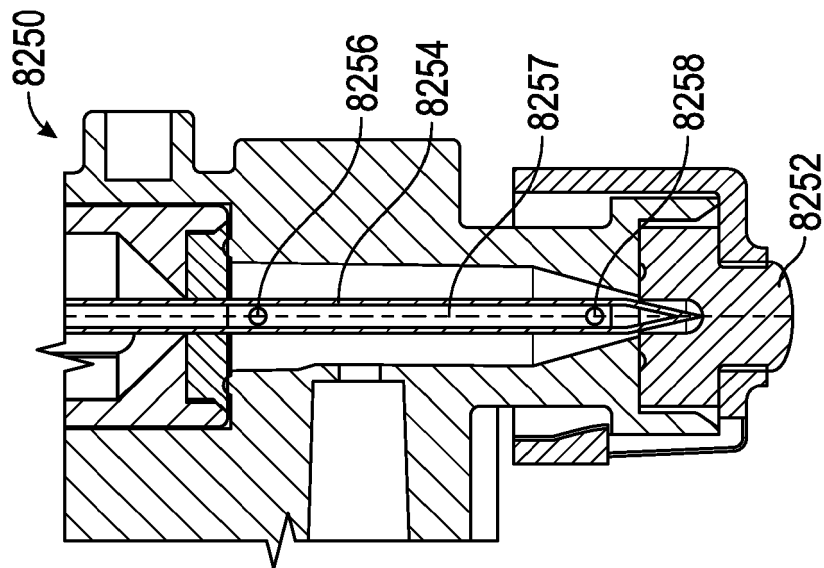


FIG. 29B

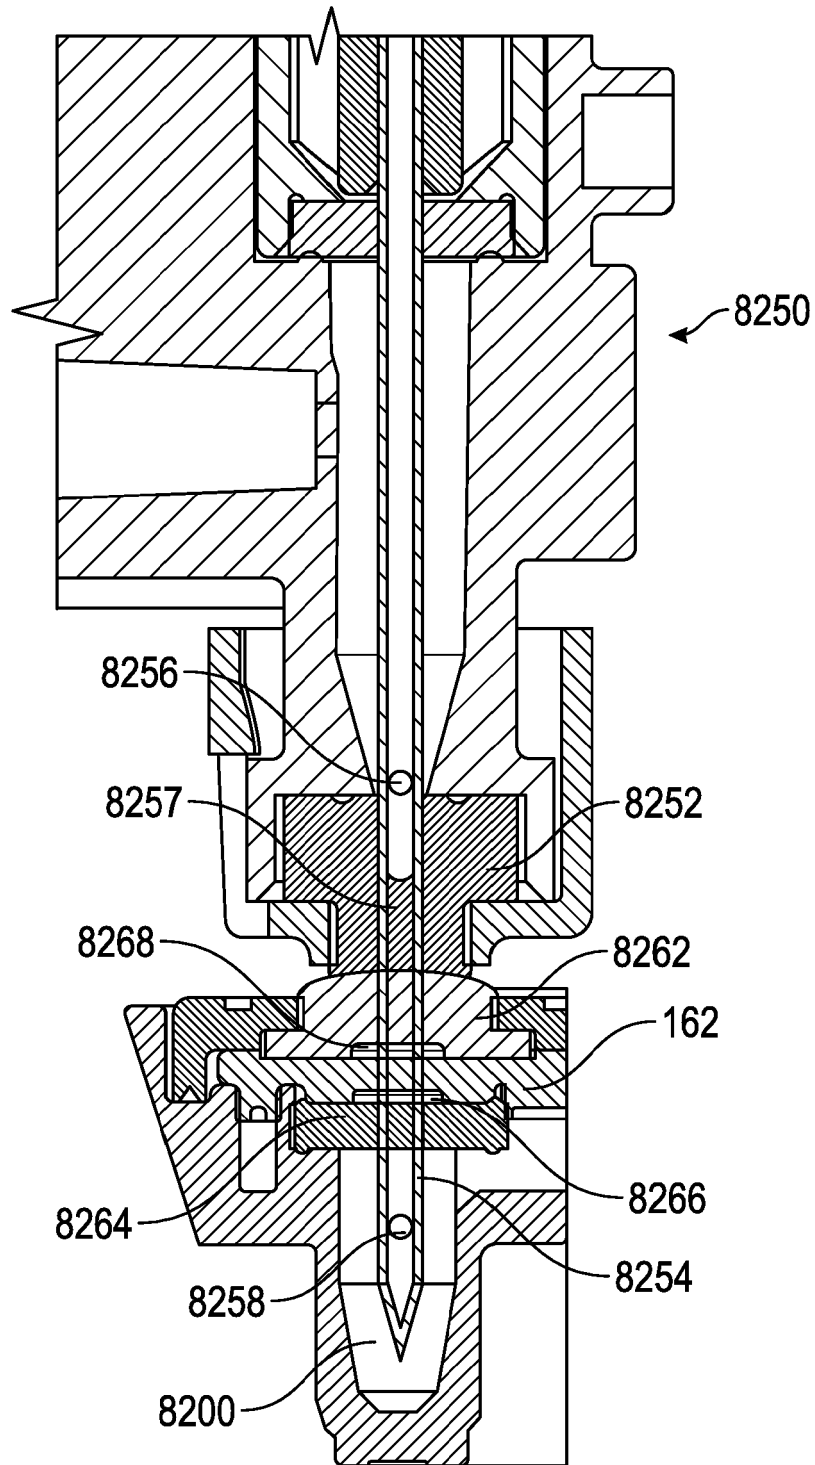


FIG. 29D

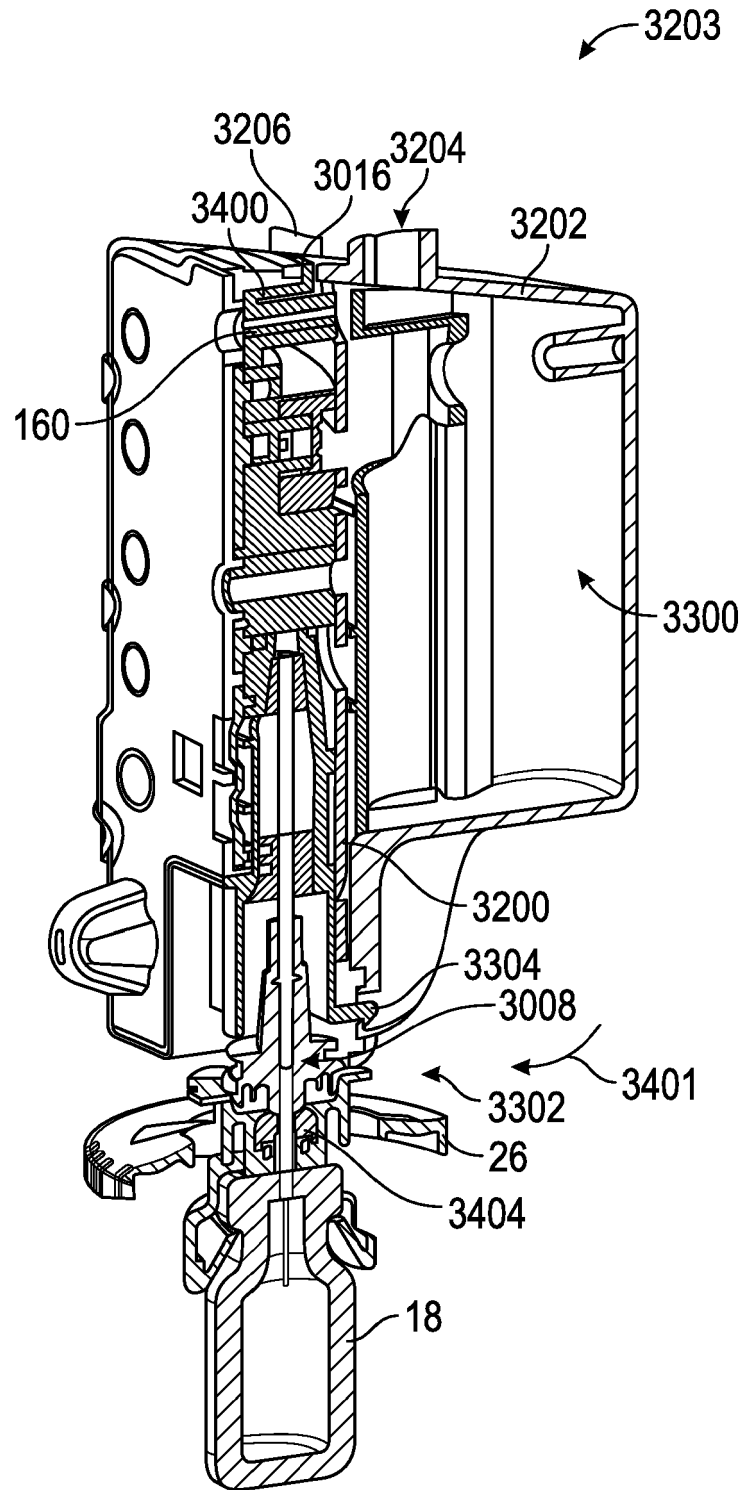


FIG. 30

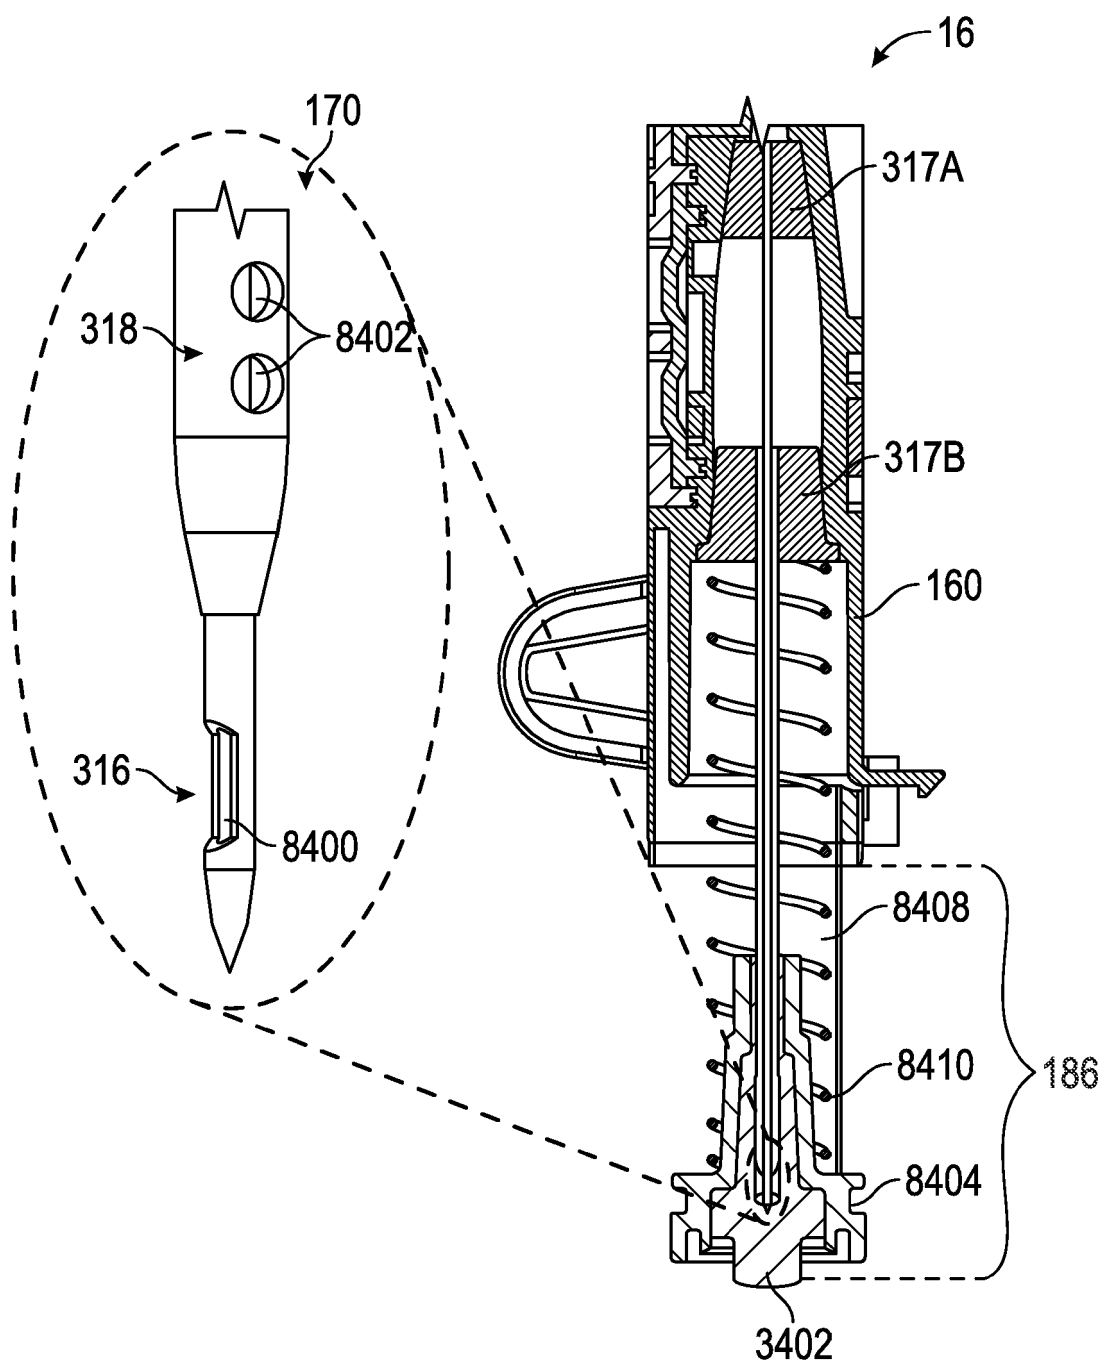


FIG. 31

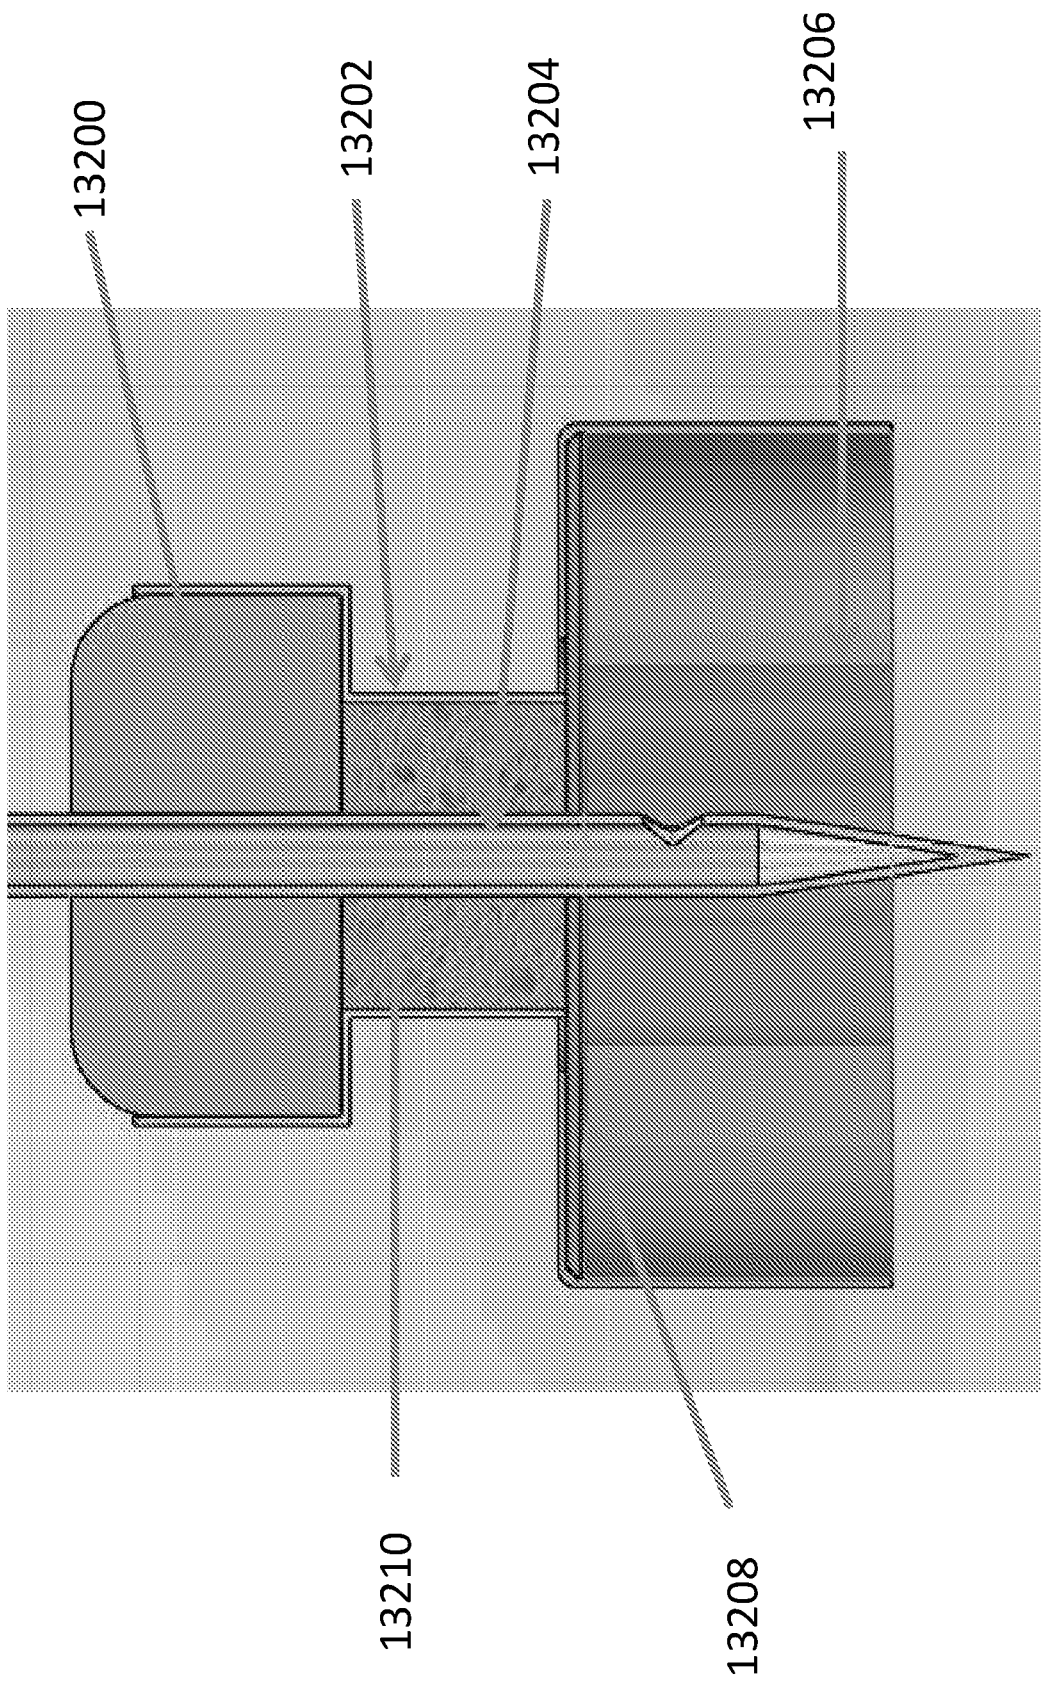


FIG. 32

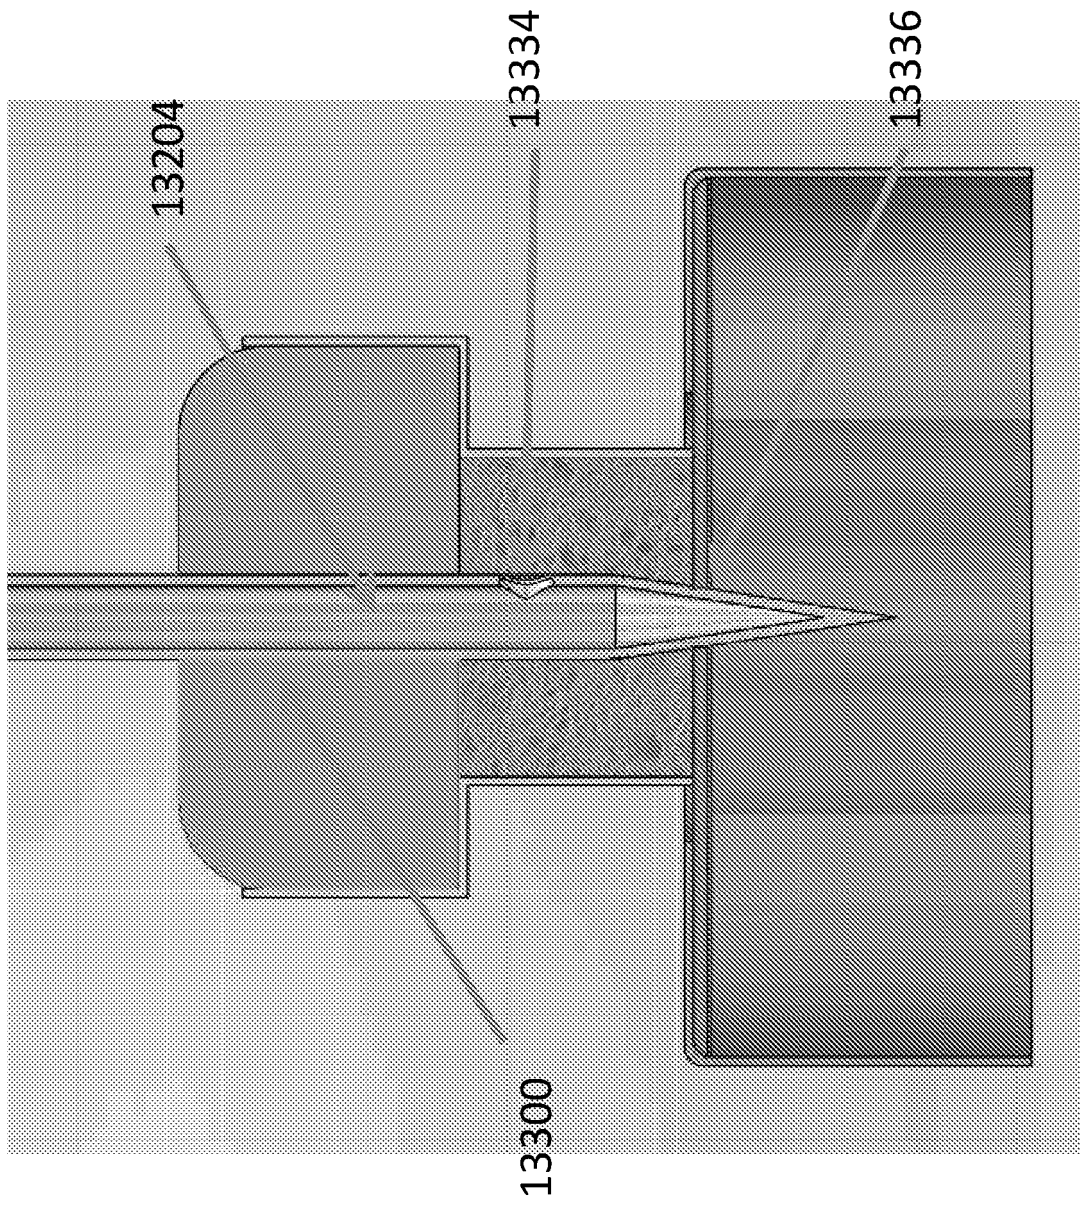


FIG. 33

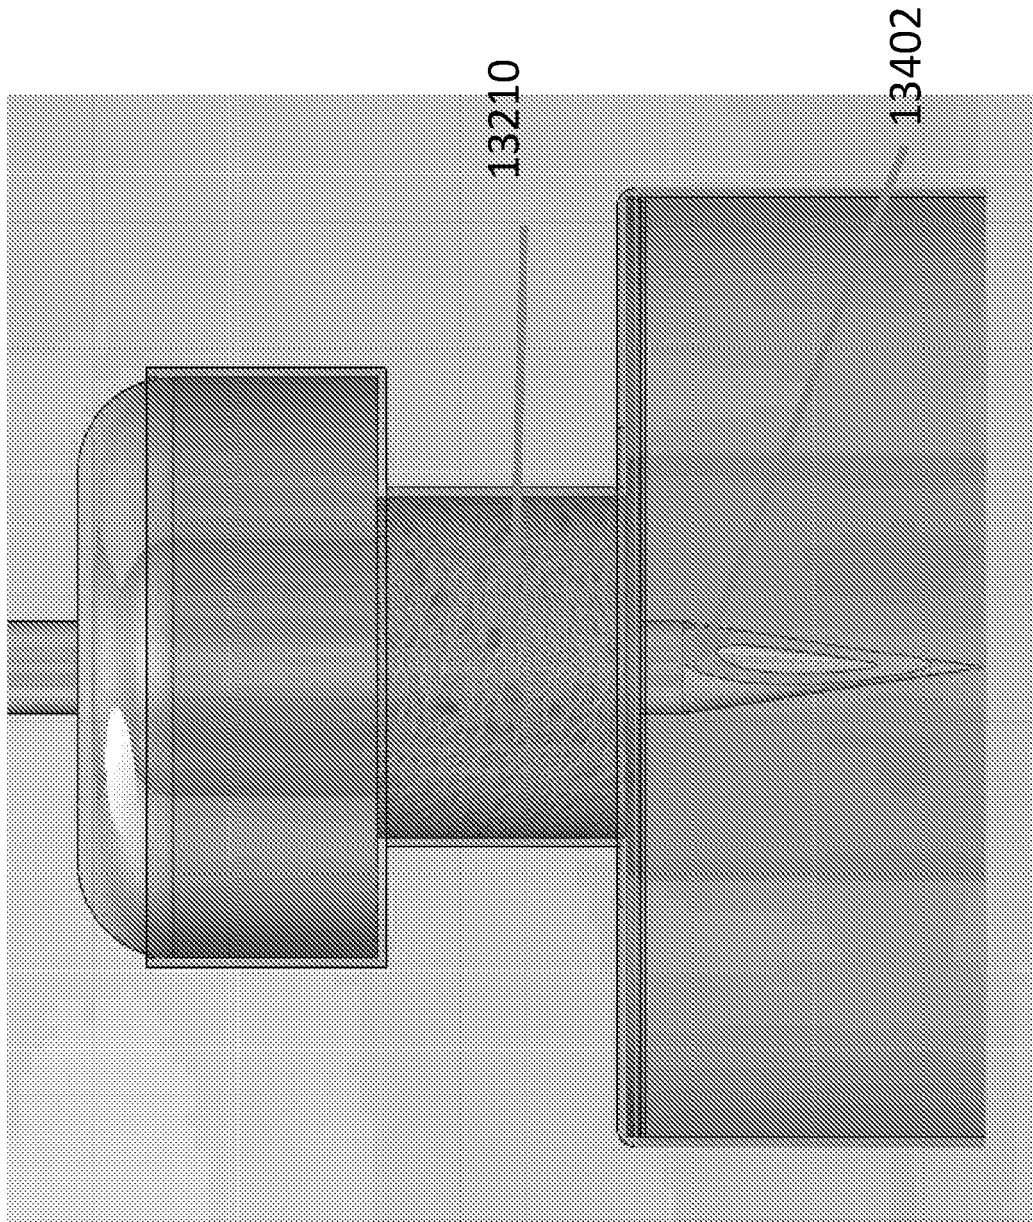


FIG. 34

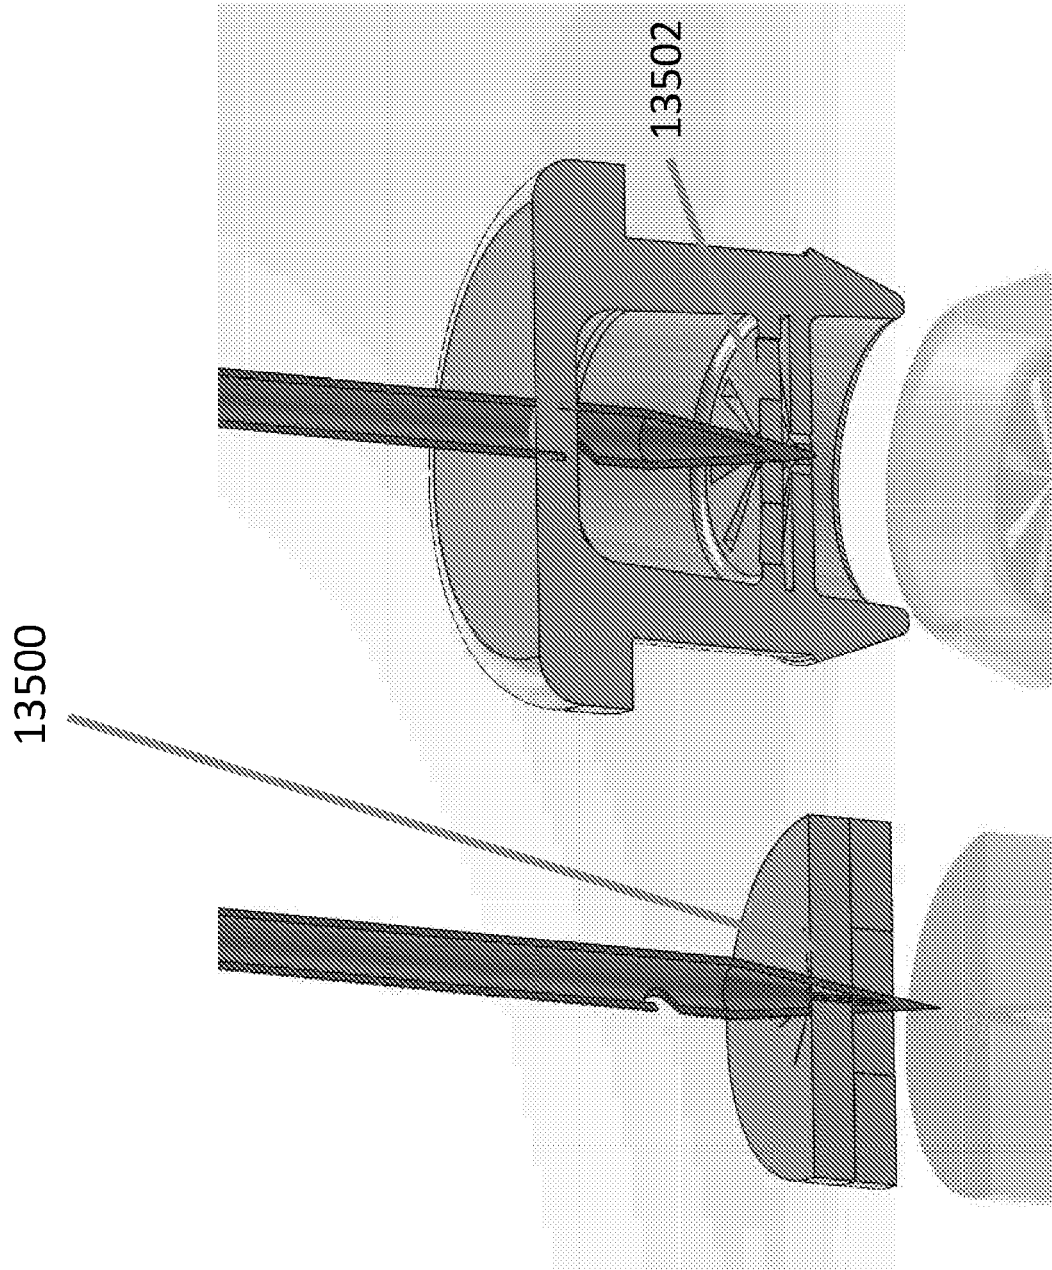


FIG. 35B

FIG. 35A

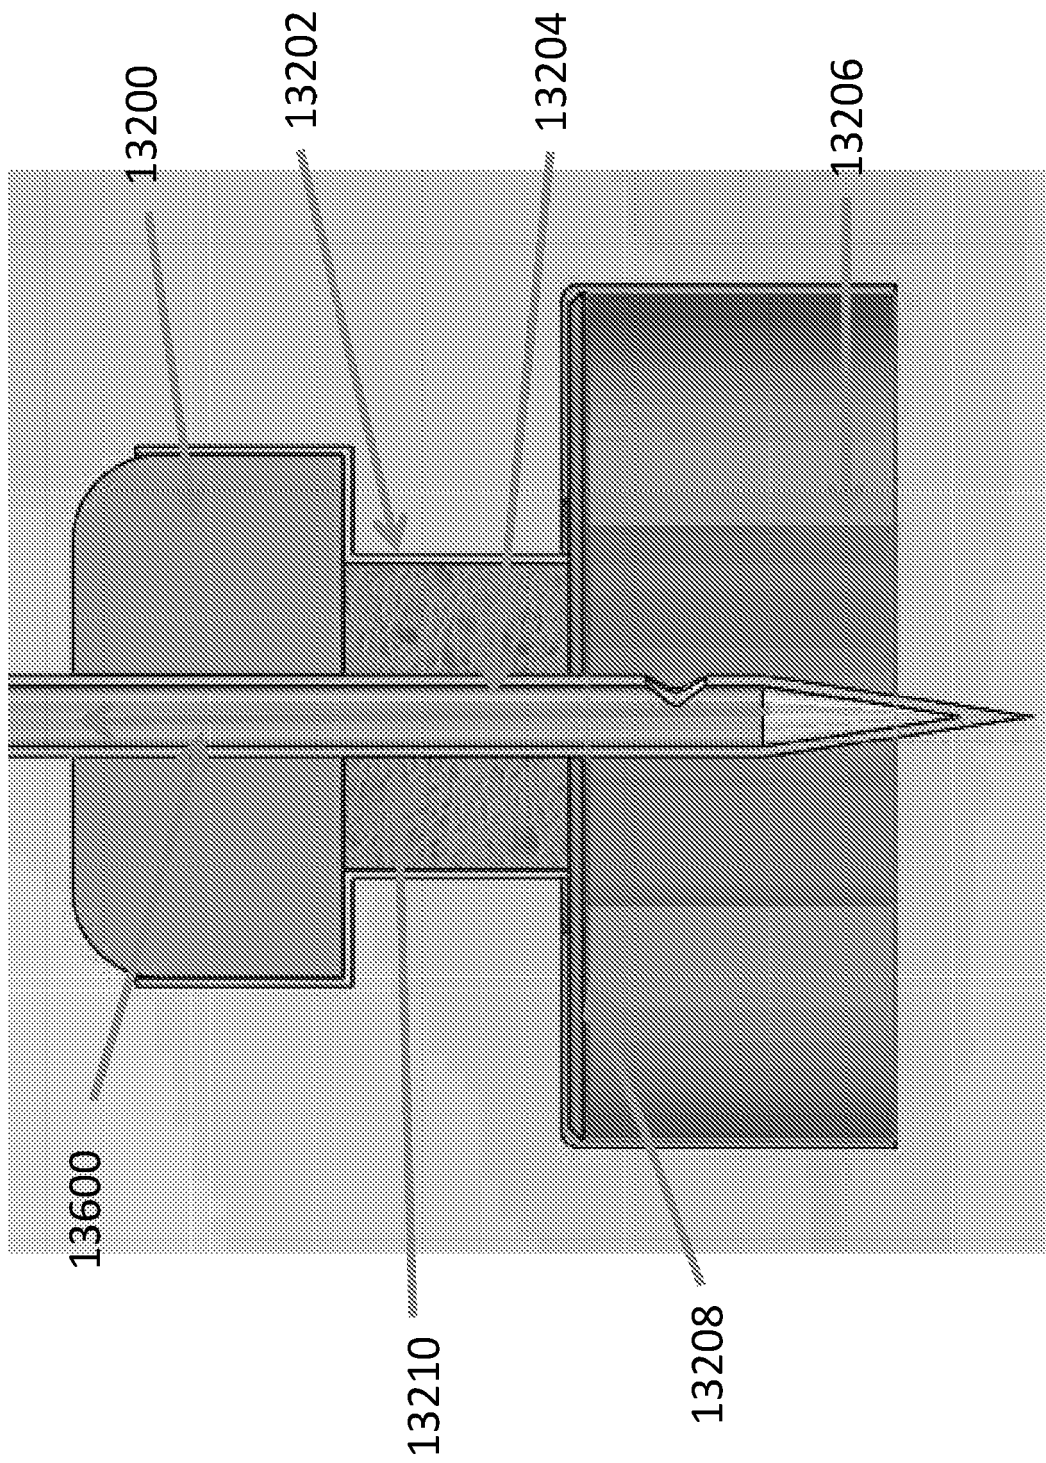


FIG. 36

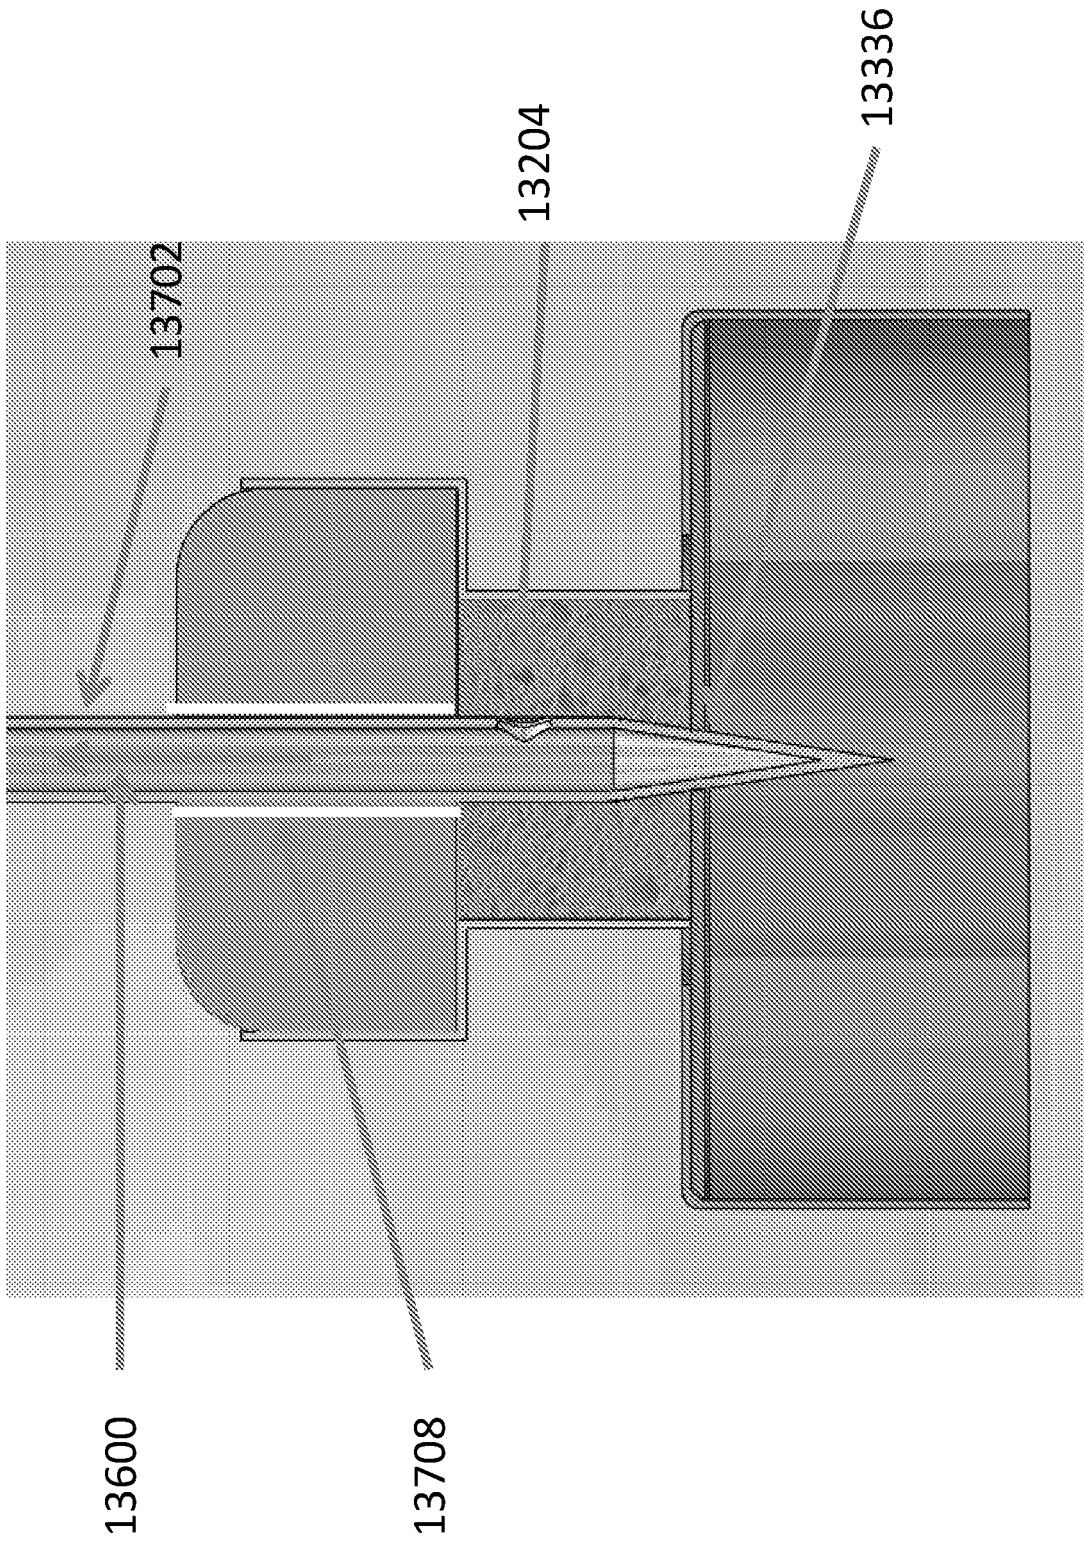


FIG. 37

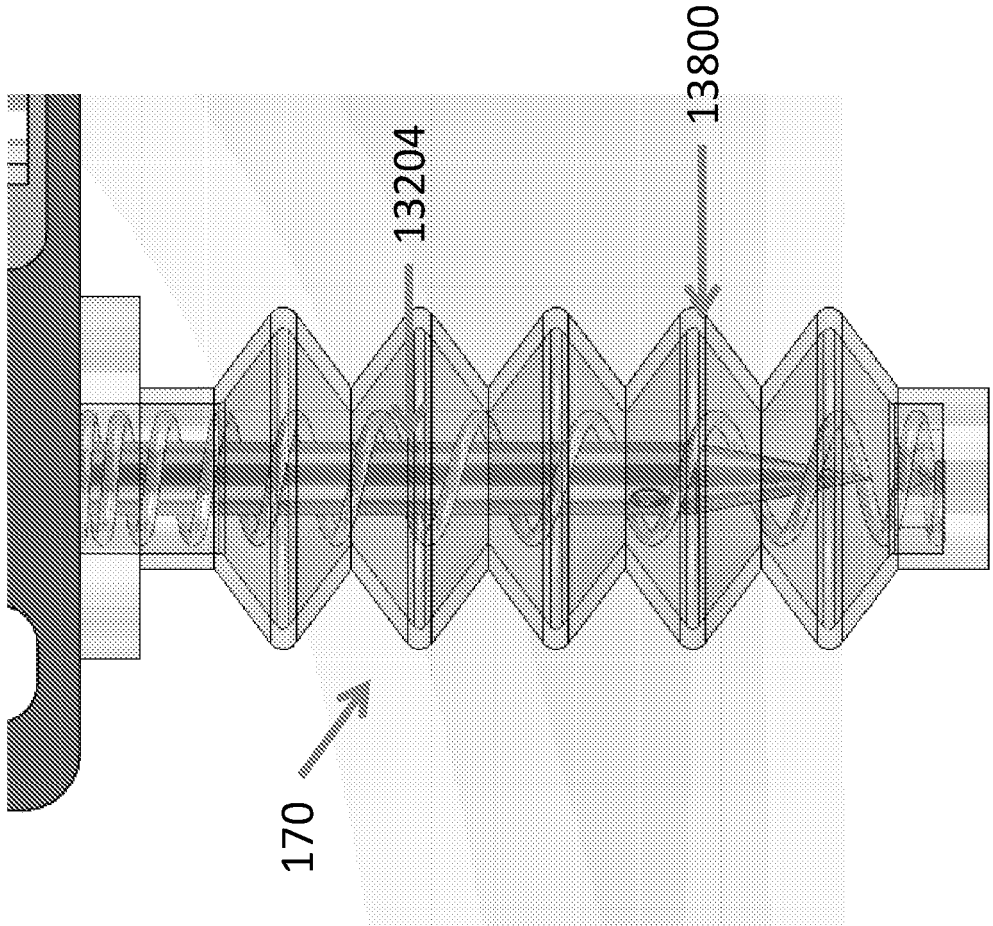


FIG. 39

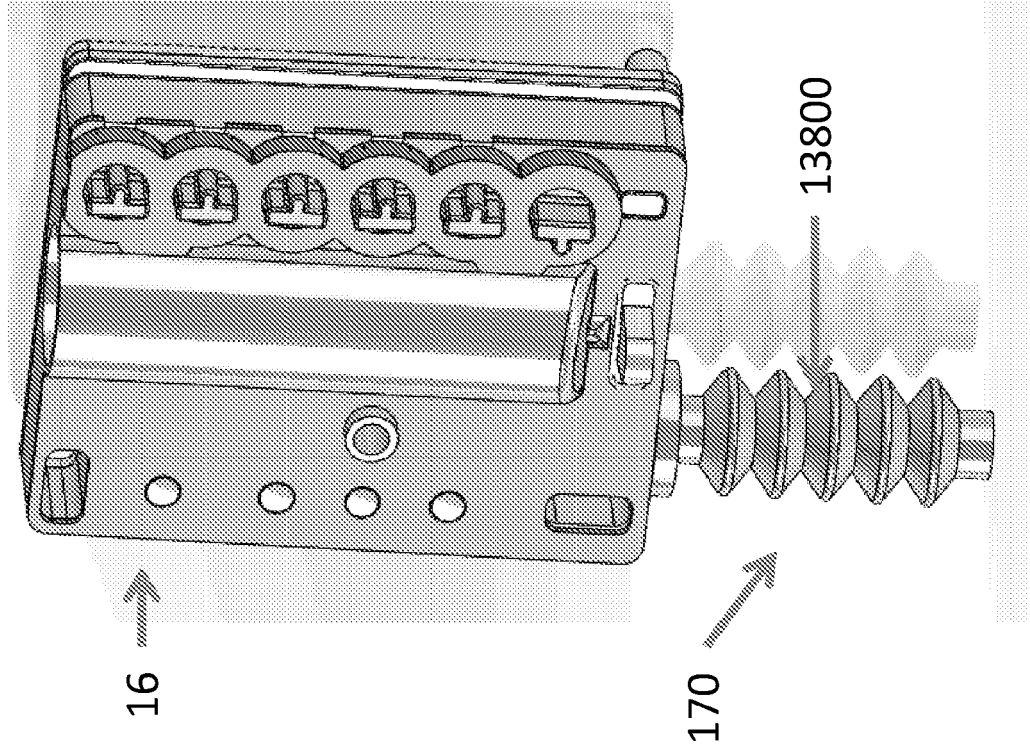


FIG. 38

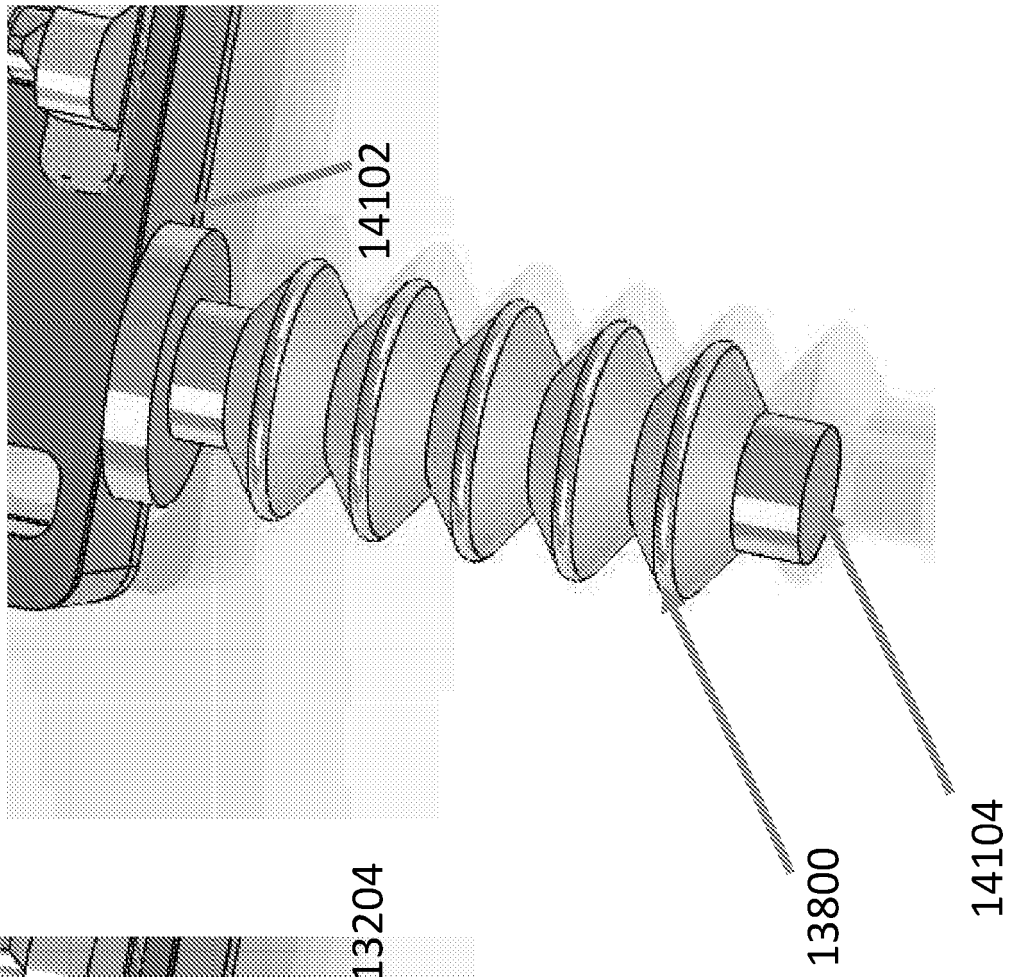


FIG. 41

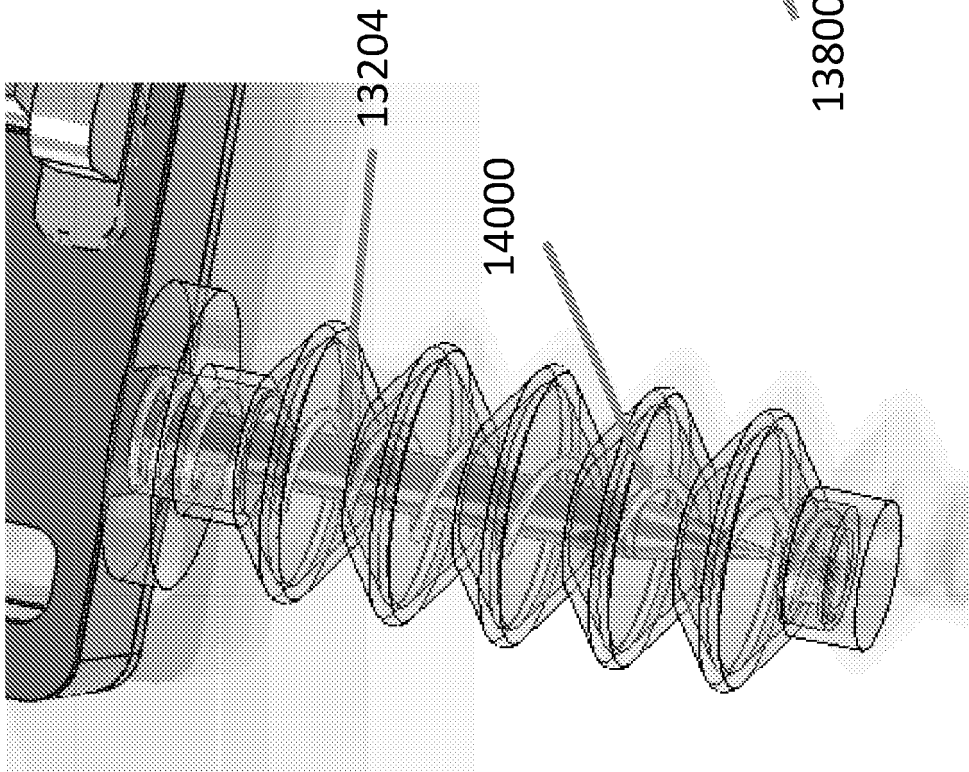


FIG. 40

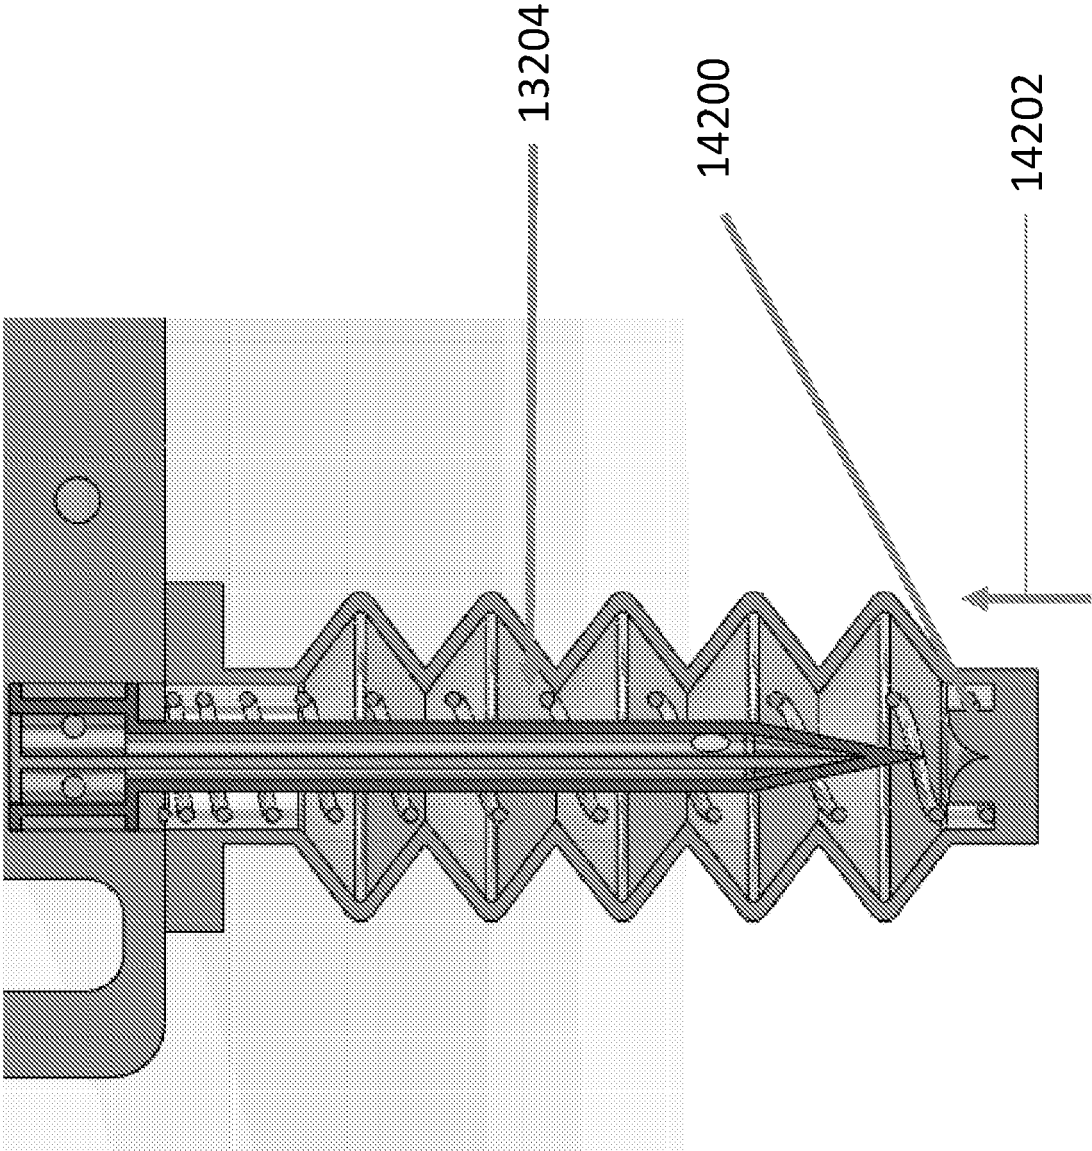


FIG. 42

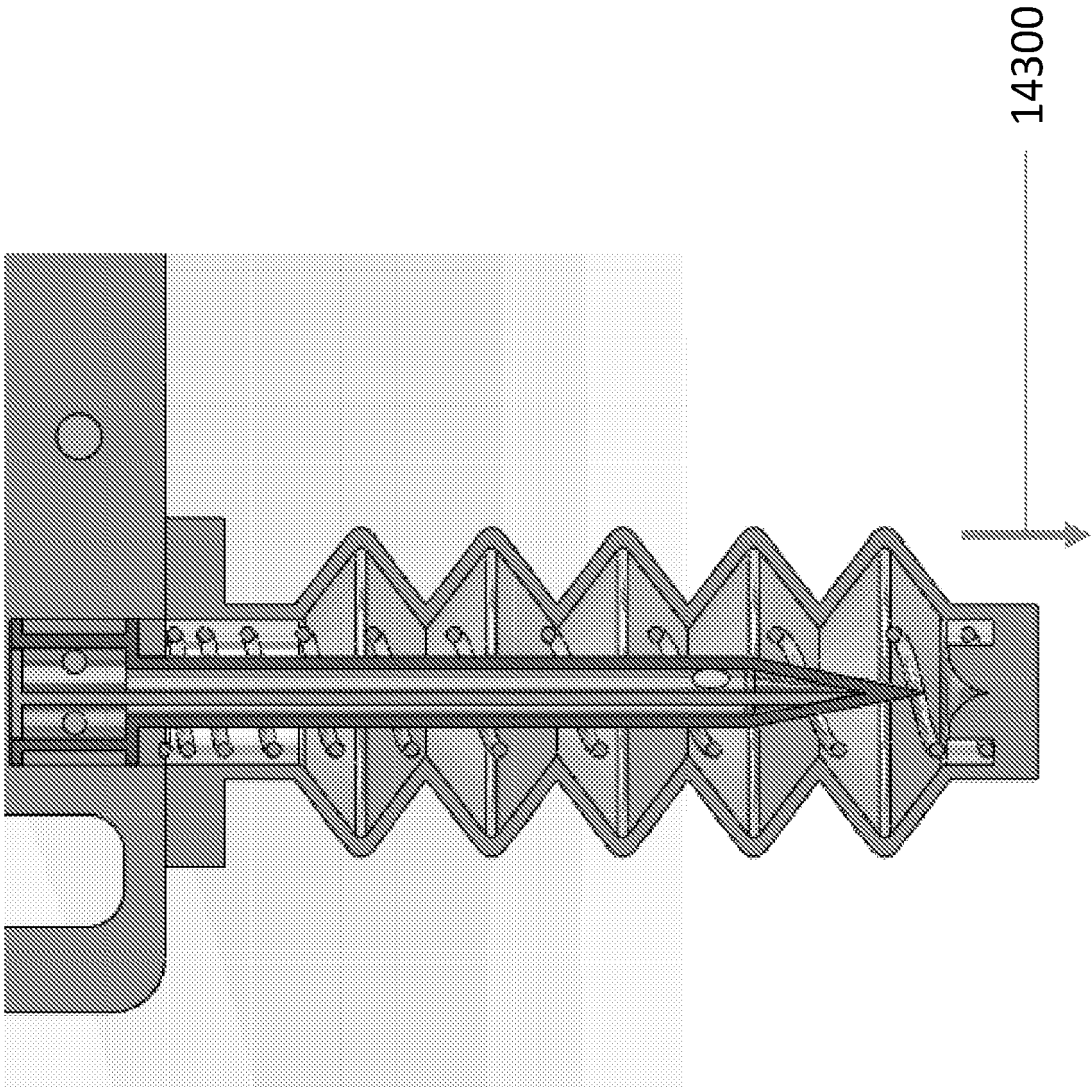


FIG. 43

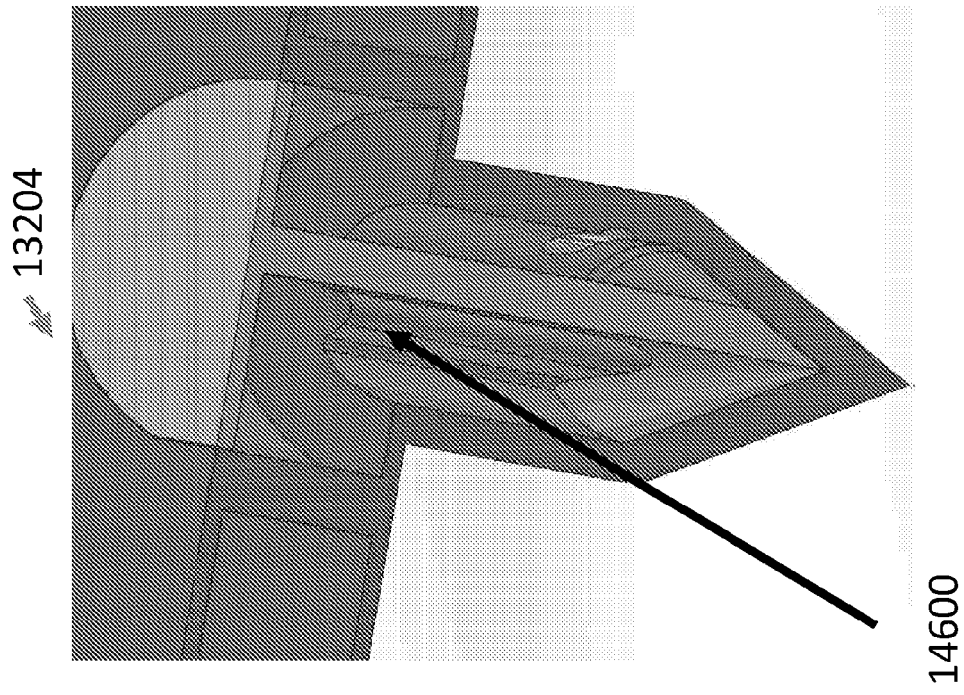


FIG. 46

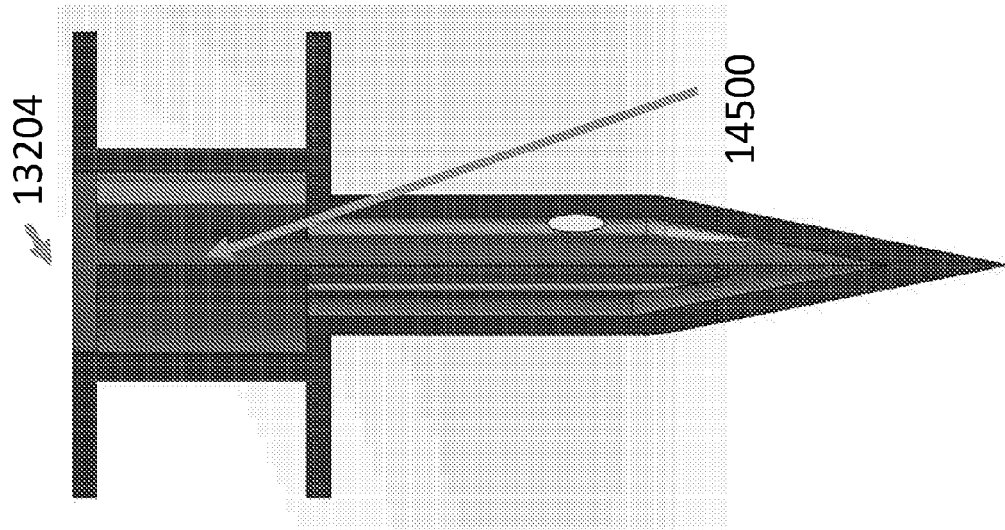


FIG. 45

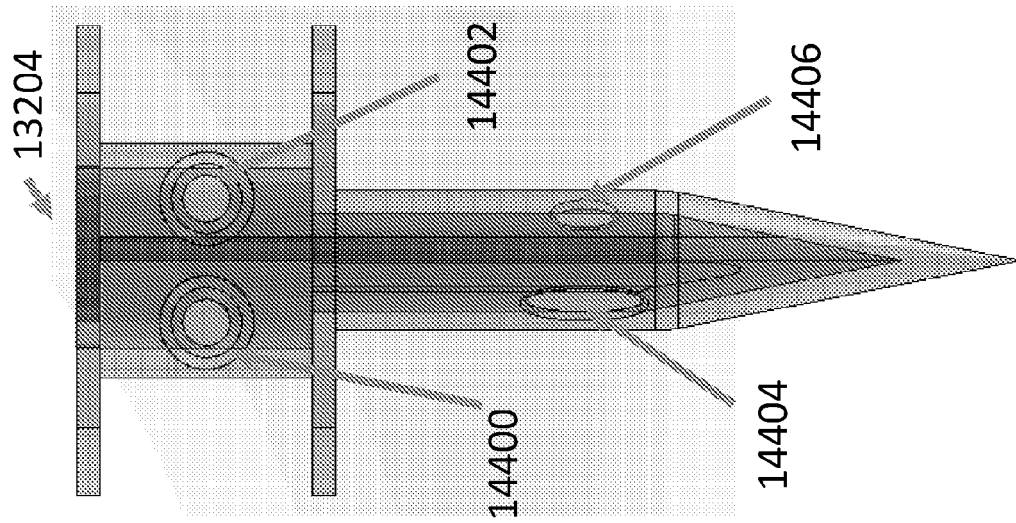


FIG. 44

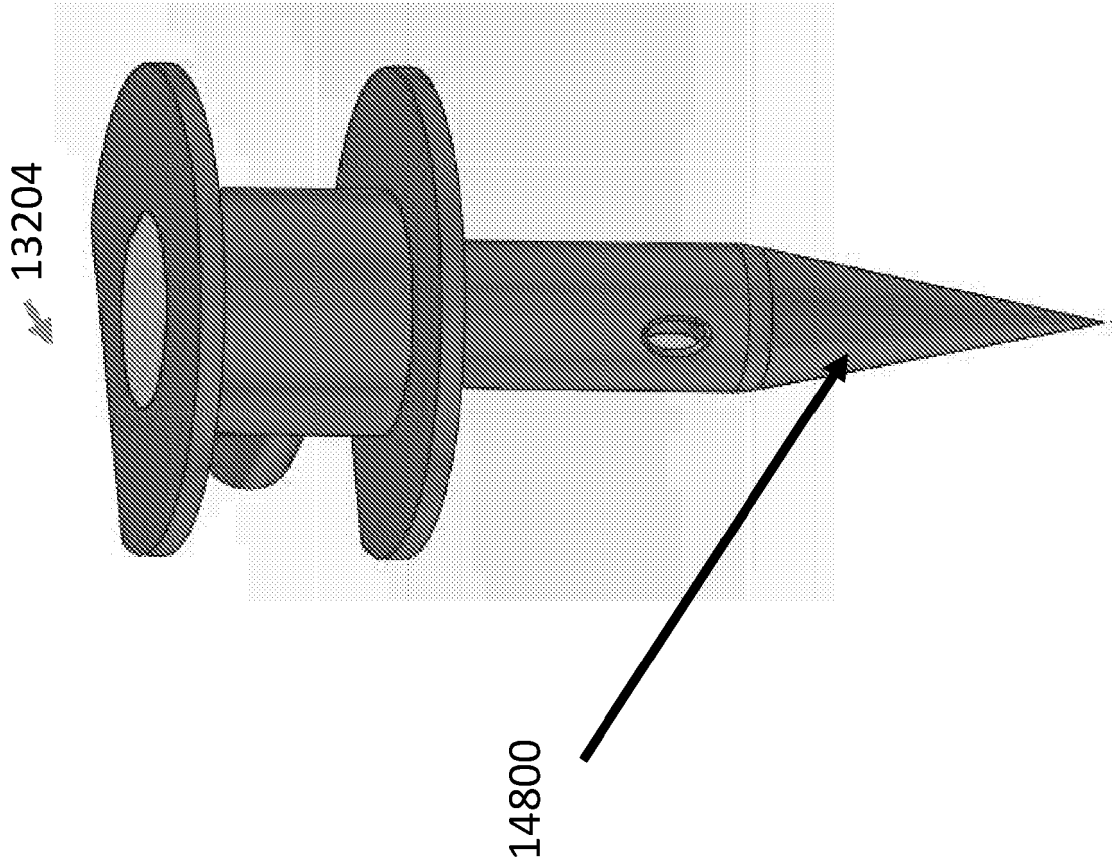


FIG. 48

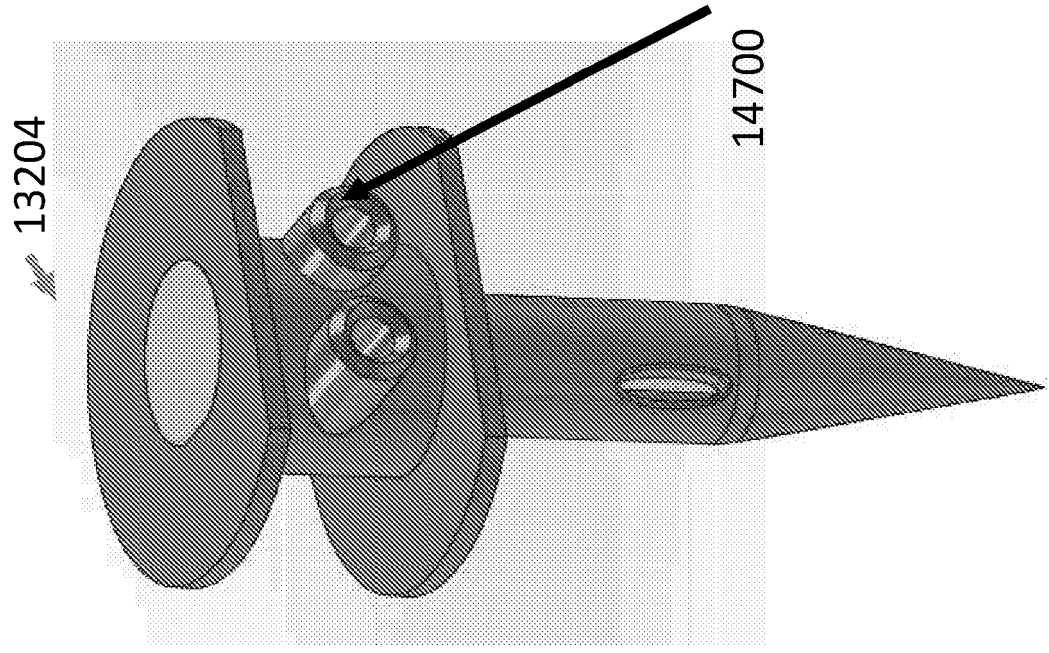


FIG. 47

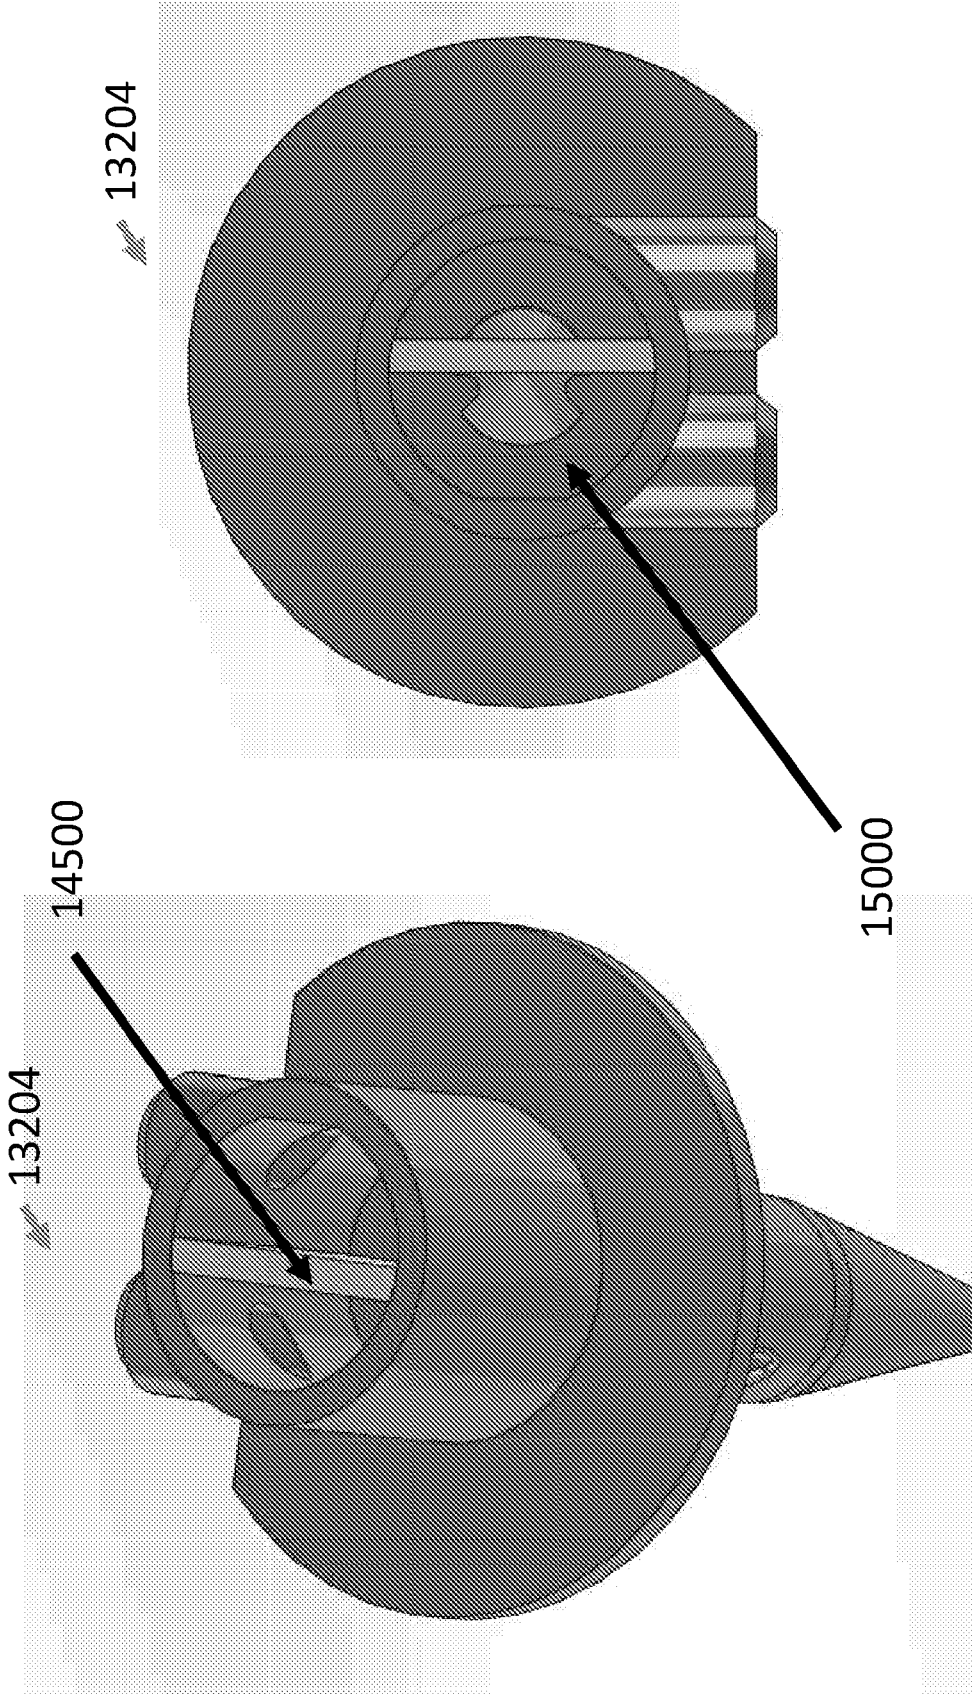


FIG. 50

FIG. 49

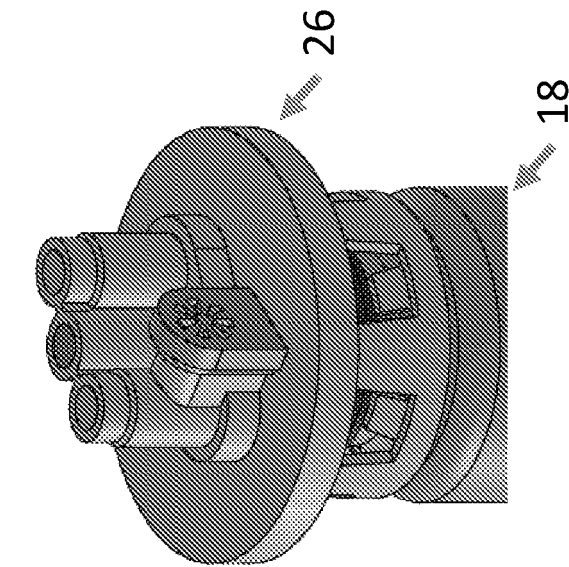
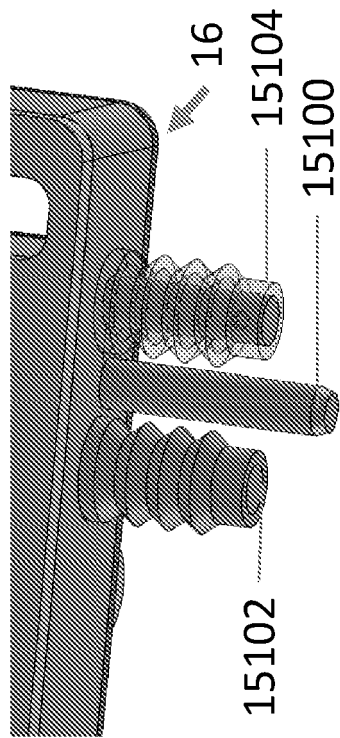


FIG. 52

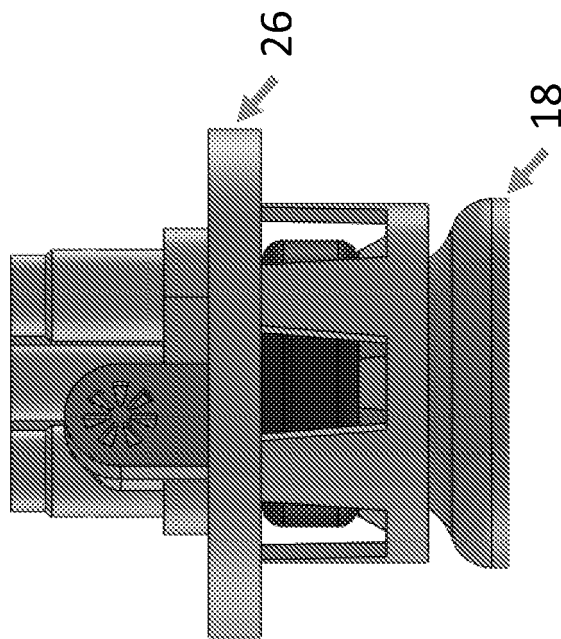
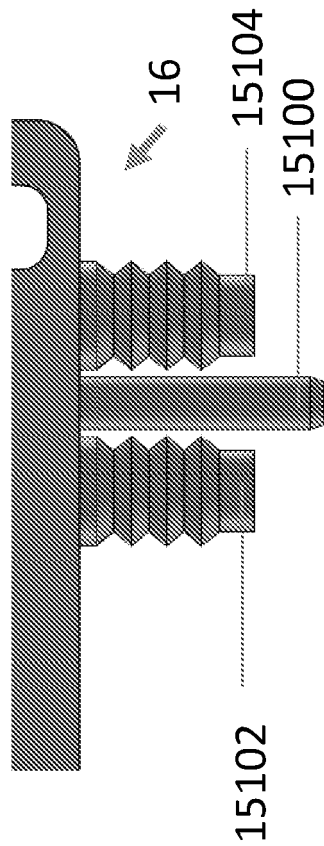


FIG. 51

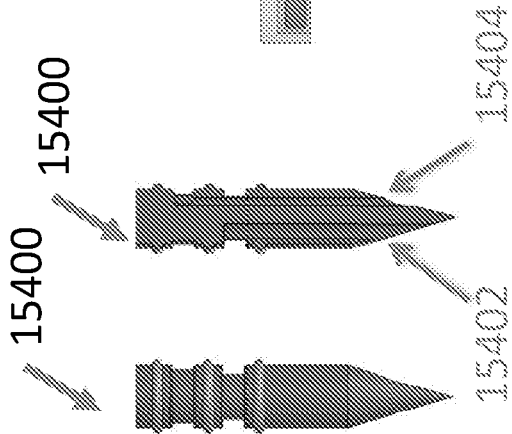


FIG. 53

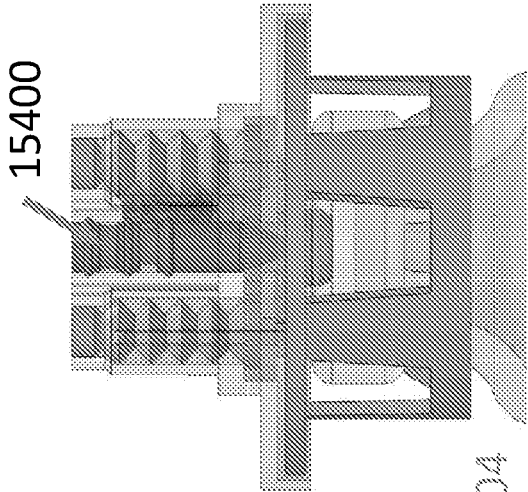


FIG. 54

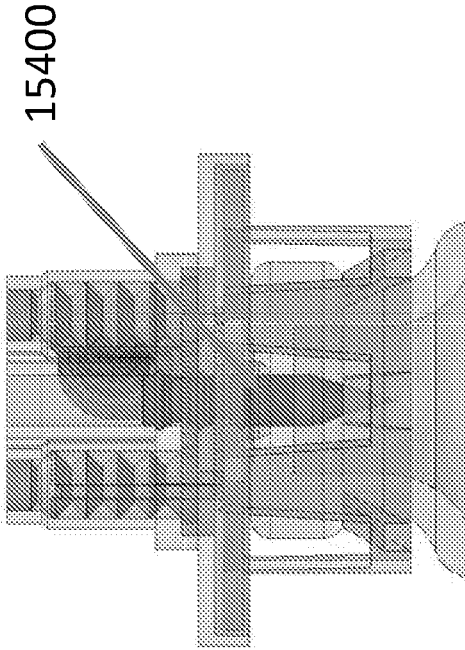


FIG. 55

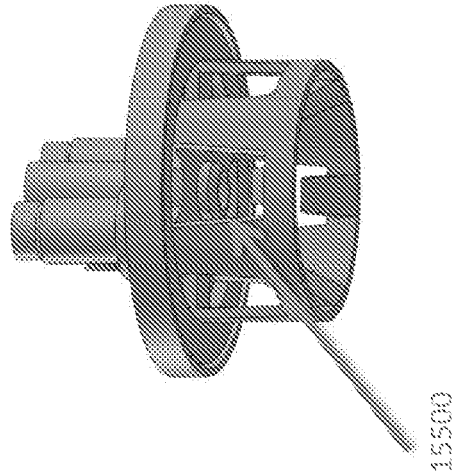


FIG. 56

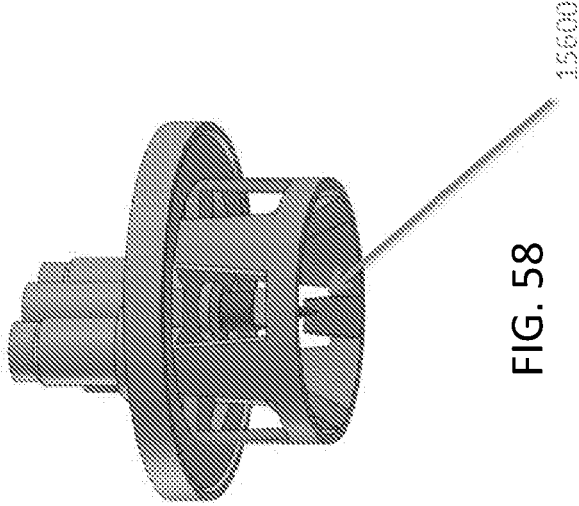


FIG. 57

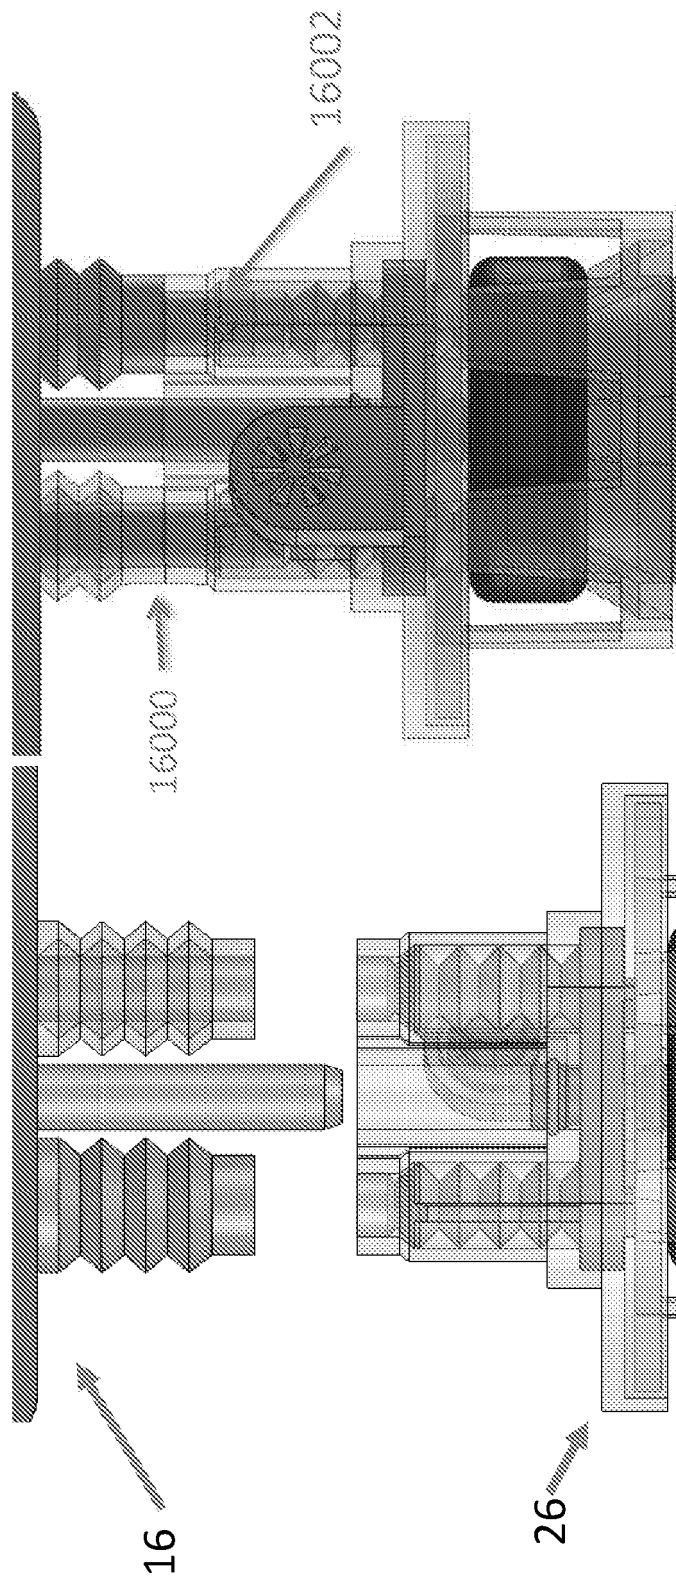


FIG. 59

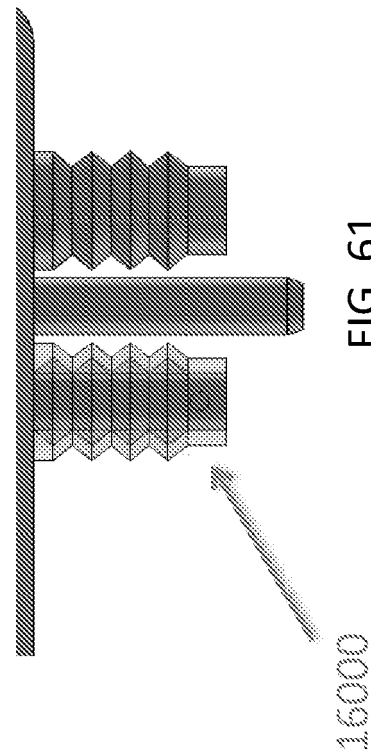


FIG. 60

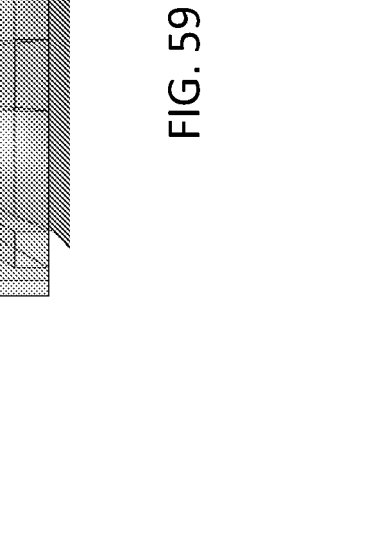


FIG. 61

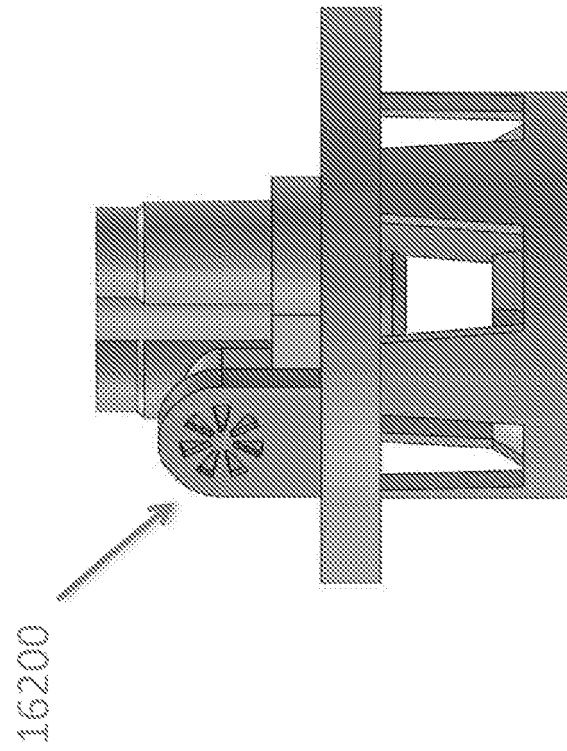


FIG. 62

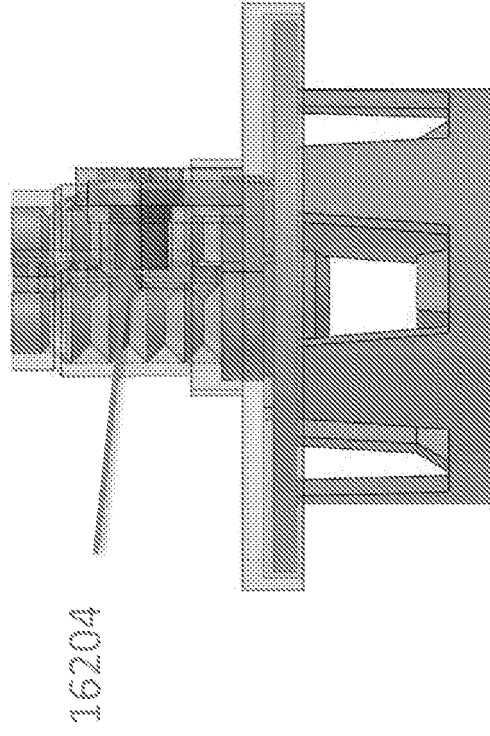
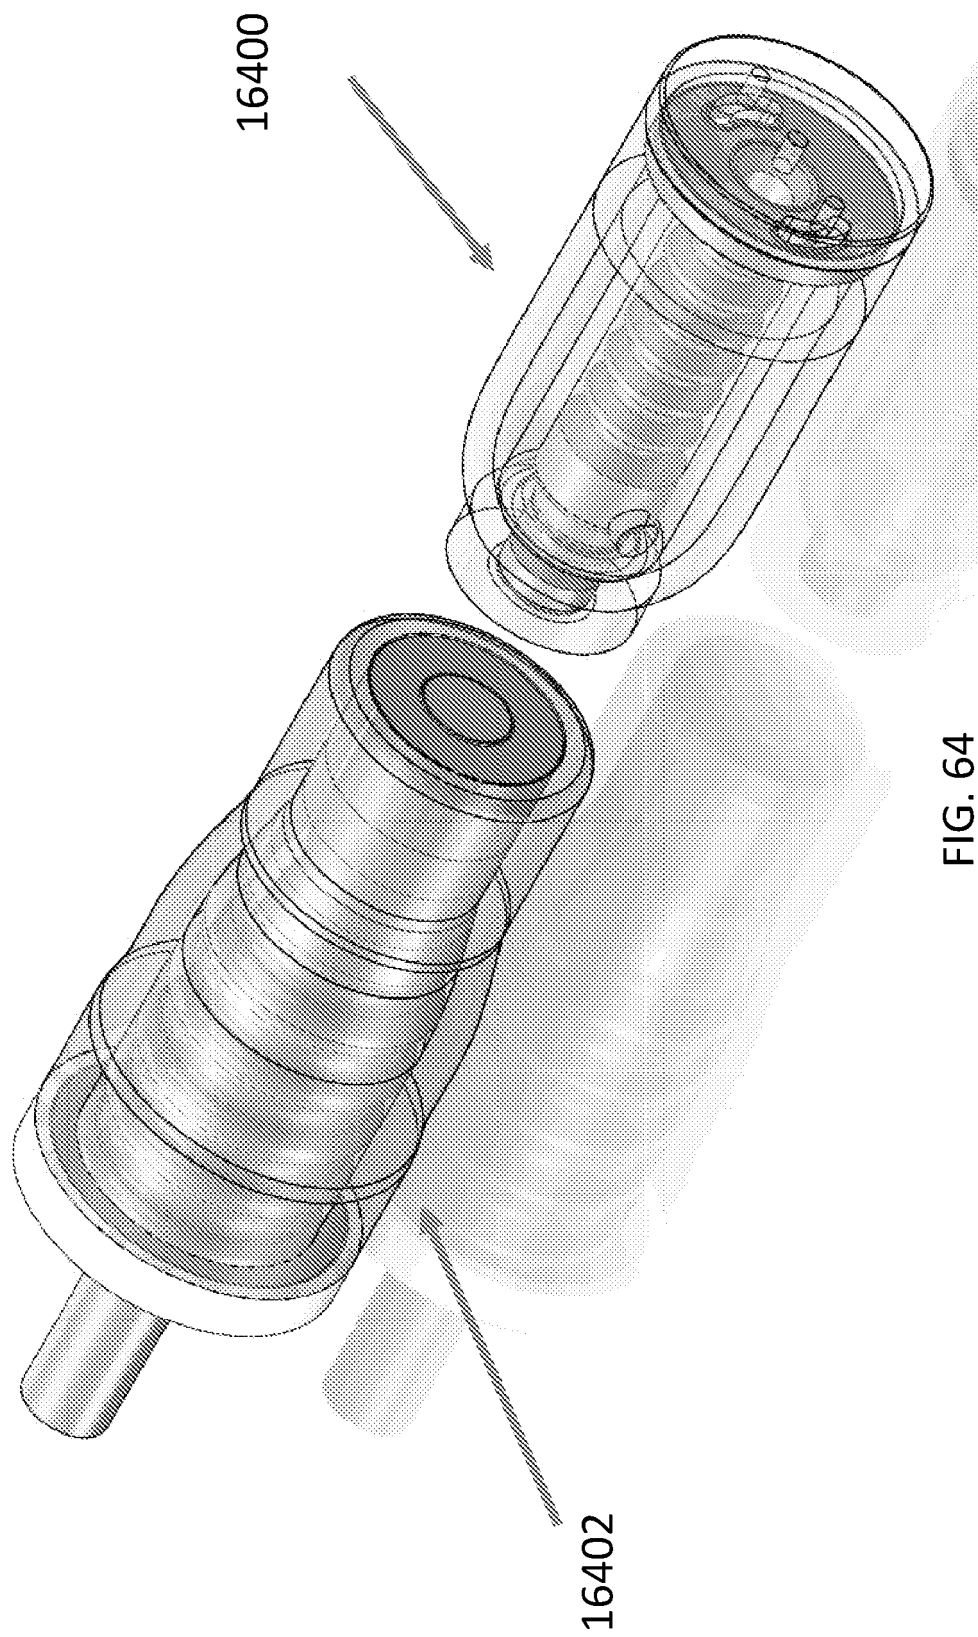
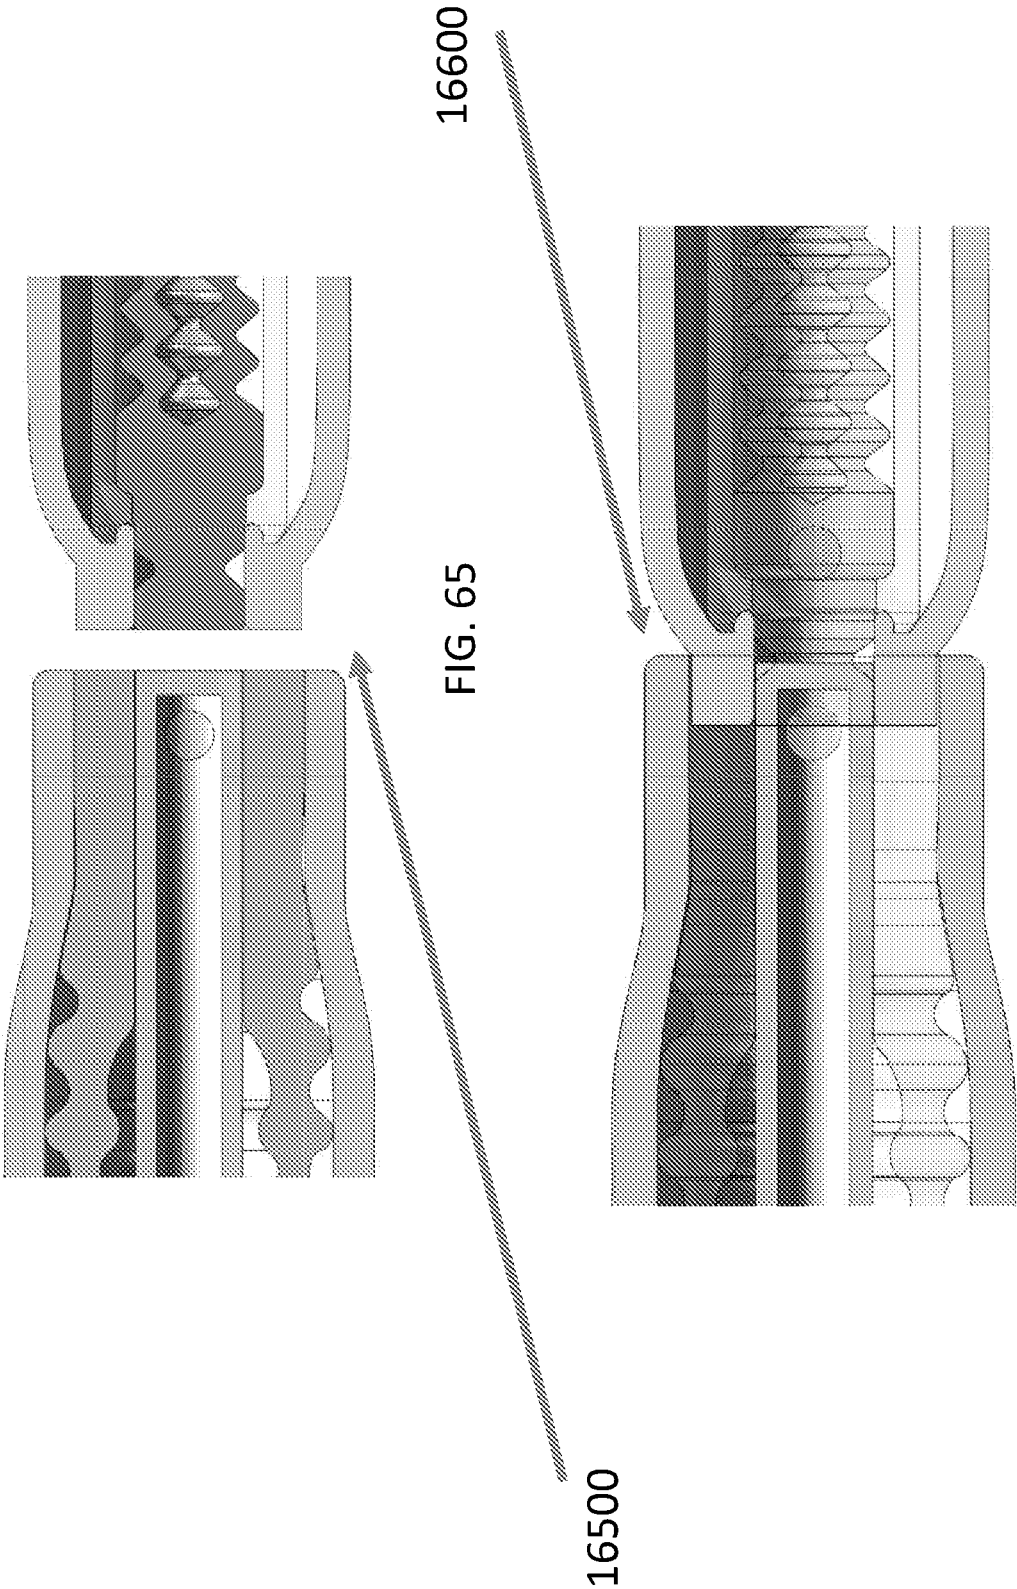
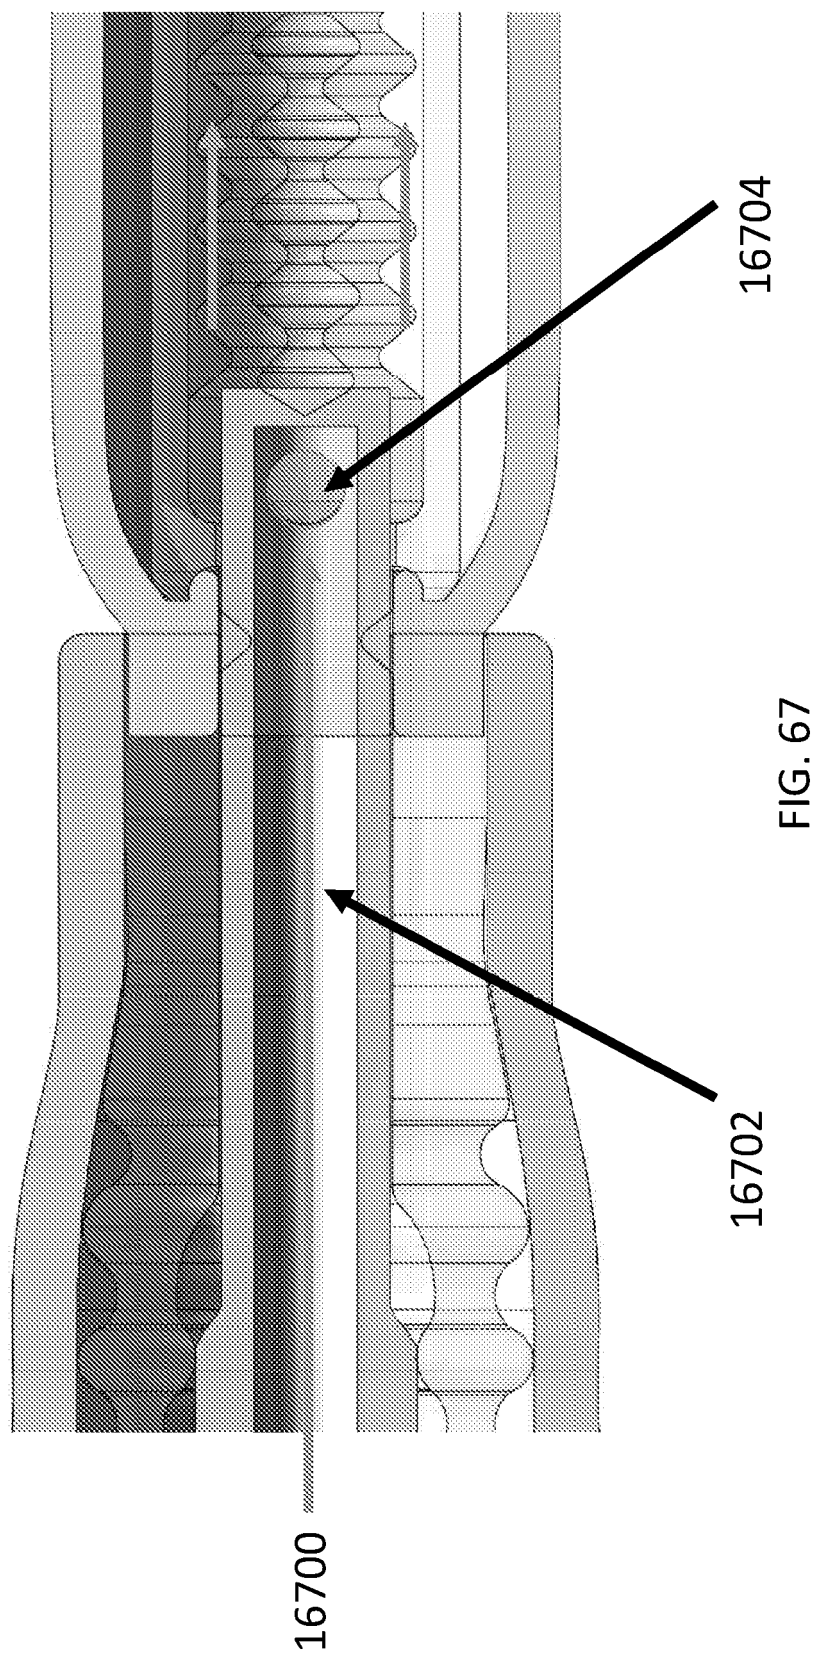


FIG. 63







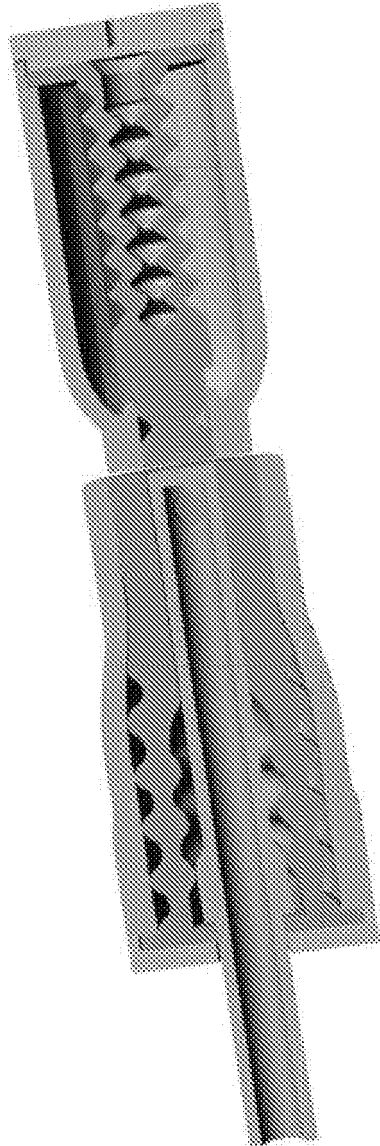
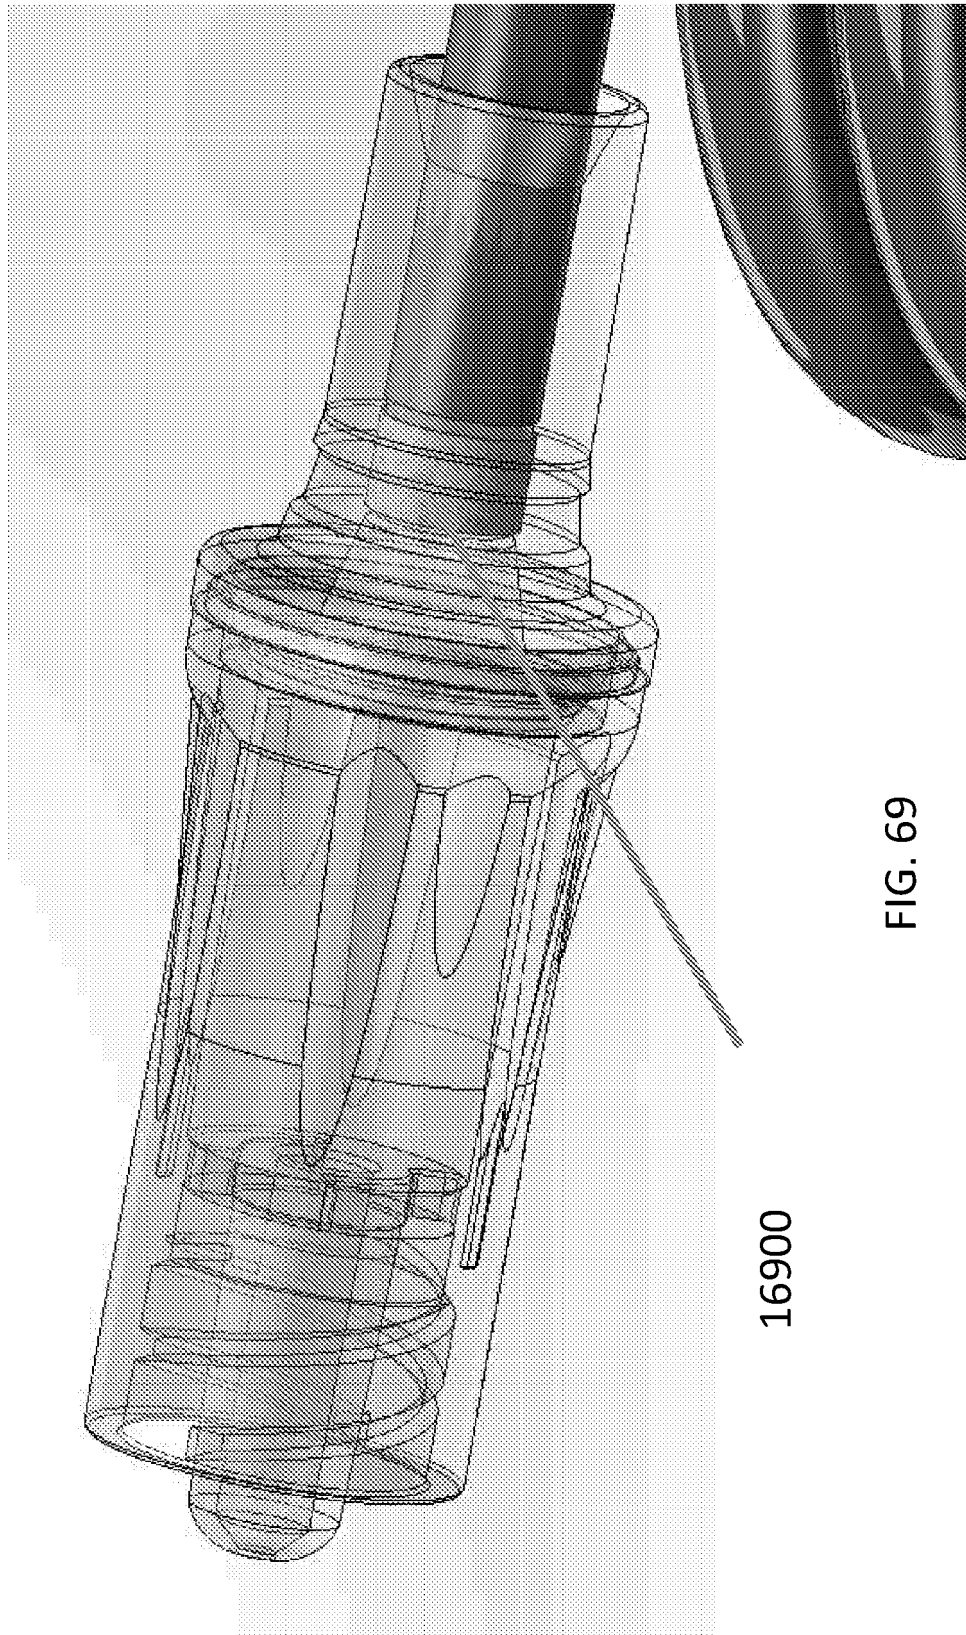
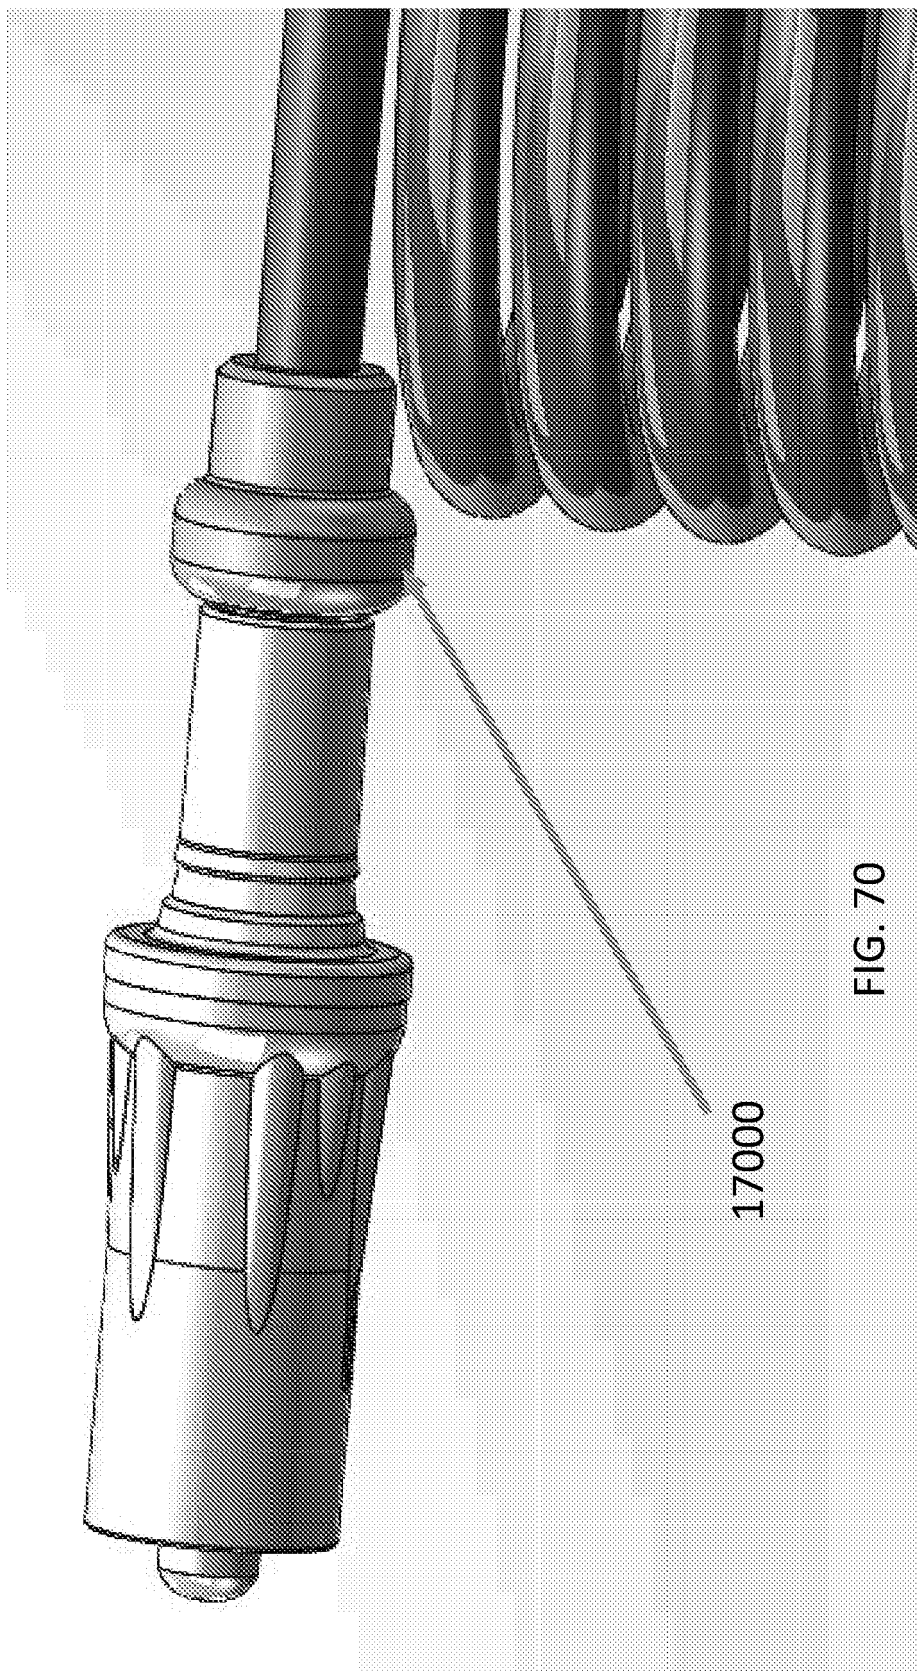


FIG. 68





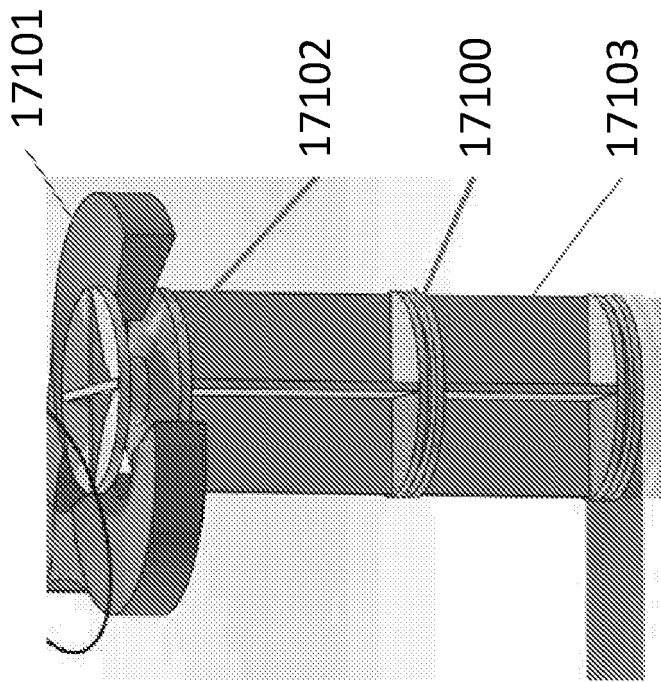


FIG. 71

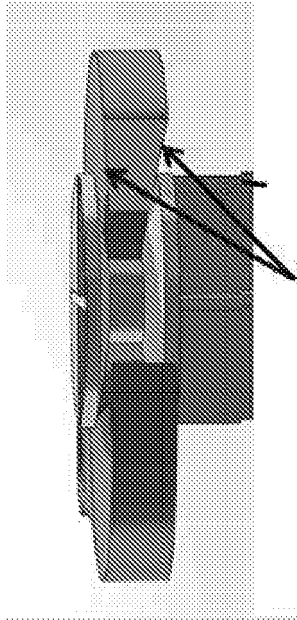


FIG. 72

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- US 62476692 [0001]